



Validation of spectroscopic gas analyzer accuracy using gravimetric standard gas mixtures: impact of background gas composition on CO₂ quantitation by cavity ring-down spectroscopy

Jeong Sik Lim, Miyeon Park, Jinbok Lee, and Jeongsoo Lee

Center for Gas Analysis, Chemical and Medical Metrology Division, Korea Research Institute of Standards and Science (KRISS), Gajeong-ro 267, Yuseong-gu, Daejeon 34113, Republic of Korea

Correspondence to: Jeongsoo Lee (leejs@kriss.re.kr)

Received: 23 February 2017 – Discussion started: 24 May 2017

Revised: 11 August 2017 – Accepted: 16 September 2017 – Published: 1 December 2017

Abstract. The effect of background gas composition on the measurement of CO₂ levels was investigated by wavelength-scanned cavity ring-down spectrometry (WS-CRDS) employing a spectral line centered at the $R(1)$ of the $(3\ 0^0\ 1)_{III} \leftarrow (0\ 0\ 0)$ band. For this purpose, eight cylinders with various gas compositions were gravimetrically and volumetrically prepared within $2\sigma = 0.1\%$, and these gas mixtures were introduced into the WS-CRDS analyzer calibrated against standards of ambient air composition. Depending on the gas composition, deviations between CRDS-determined and gravimetrically (or volumetrically) assigned CO₂ concentrations ranged from -9.77 to $5.36\ \mu\text{mol mol}^{-1}$, e.g., excess N₂ exhibited a negative deviation, whereas excess Ar showed a positive one. The total pressure broadening coefficients (TPBCs) obtained from the composition of N₂, O₂, and Ar thoroughly corrected the deviations up to -0.5 to $0.6\ \mu\text{mol mol}^{-1}$, while these values were -0.43 to $1.43\ \mu\text{mol mol}^{-1}$ considering PBCs induced by only N₂. The use of TPBC enhanced deviations to be corrected to $\sim 0.15\%$.

Furthermore, the above correction linearly shifted CRDS responses for a large extent of TPBCs ranging from 0.065 to $0.081\ \text{cm}^{-1}\ \text{atm}^{-1}$. Thus, accurate measurements using optical intensity-based techniques such as WS-CRDS require TPBC-based instrument calibration or use standards prepared in the same background composition of ambient air.

1 Introduction

Emission of carbon dioxide (CO₂), the most important greenhouse gas, has been reported to increase, resulting in global climate change (Messerschmidt et al., 2011; Solomon et al., 2007). According to the IPCC Fourth Assessment Report (Solomon et al., 2007), CO₂ is the major contributor to global warming, with a 62.9% share of the total radiative force caused by long-lived greenhouse gases. Although it is not yet feasible to quantify all its sources and sinks within small uncertainties (Conway et al., 1988; Schulze et al., 2009), all countries have agreed to consistently control CO₂ emissions, necessitating accurate measurements of atmospheric CO₂ mole fractions. Gas chromatography coupled with flame ionization detection (GC-FID) (van der Laan et al., 2009), nondispersive infrared spectroscopy (NDIR) at $4.26\ \mu\text{m}$ (Lee et al., 2006; Min et al., 2009; Crawley, 2008; Tohjima et al., 2009), Fourier transform infrared (FTIR) spectroscopy (Griffith et al., 2012), tunable diode laser absorption spectroscopy (TDLAS) (Durry et al., 2010), wavelength-scanned cavity ring-down spectroscopy (WS-CRDS) (Crosson, 2008), and other cavity-enhanced absorption spectroscopies (O'Shea et al., 2013) are well-known techniques for quantifying atmospheric CO₂. Despite exhibiting the advantage of high measurement precision, GC-FID suffers from long acquisition time due to delayed CO₂ retention in the separation column (typically several tens of minutes). NDIR shows better performance than GC-FID in real-time measurements due to using filtered spectral fingerprints of CO₂ instead of relying on analyte separation. However, frequent calibrations are required to correct NDIR response drifts. Recently, WS-CRDS

has attracted attention because of its high precision and low drift. In contrast to intensity-based techniques such as NDIR and TDLAS, CRDS is immune to laser shot noise and detector electric noise due to employing the ring-down count method. Furthermore, the increased path length offered by the resonant optical cavity provides excellent sensitivity, i.e., signal-to-noise ratio, and high precision. Since a CO₂ inter-laboratory compatibility of $\pm 0.1 \mu\text{mol mol}^{-1}$ in the Northern Hemisphere was set as a goal by the World Meteorological Organization (WMO), WS-CRDS is viewed as a competitive technique for measuring atmospheric greenhouse gas levels (Rella et al., 2013).

Accurate measurements of atmospheric CO₂ levels by WS-CRDS require the removal of water vapor, which causes spectral interference, and an empirical cubic polynomial model for correcting the water background has been developed (Rella et al., 2013). Nevertheless, CO₂ mole fraction measurements can be adversely affected by spectral line broadening if calibration gas mixtures whose background composition is different from the natural N₂:O₂:Ar ratio in the atmosphere are used (Nara et al., 2012). In this study, standard gas mixtures containing ambient levels of CO₂ in synthetic air (N₂ + O₂ + Ar) were gravimetrically prepared for utilization as calibration standards and measuring targets for investigating the impact of background gas composition on WS-CRDS responses, owing to the excellent uncertainty of gravimetric gas mixtures. Furthermore, an empirical equation for correcting the “matrix effect” was derived in terms of total pressure broadening. The good agreement achieved between CO₂ mole fractions of the calibration standards and synthetic samples of arbitrary composition validated the measurement accuracy of matrix-effect-corrected WS-CRDS.

2 Materials and methods

2.1 Preparation of standard gas mixtures

Gas mixtures were prepared using gravimetric and volumetric methods, based on ISO 6142-1 (2015) and ISO 6144 (2003), respectively. The gravimetric method featured filling pure CO₂ (MG industries, USA) and N₂ (Deokyang Energen, South Korea) gases into a clean aluminum cylinder. Subsequently, pure O₂ (Praxair Co., South Korea) and Ar (Deokyang Energen, South Korea) gases were added to the obtained CO₂/N₂ mixture to obtain an ambient level of CO₂ in a matrix of synthetic air. The amounts of filled gases were determined based on their weight, which was obtained by weighing the aluminum cylinder before and after filling. The weights used for calibrating the weighing balance (Mettler Toledo, XP 26003L, USA) were calibrated against the national kilogram standard to ensure measurement traceability. For high weighing precision, an automatic weighing machine patented by KRISS was used to control the loading po-

sition on the weighing pan of the top loading balance, resulting in a typical weighing uncertainty of less than 0.005 %. A circular turntable was used to support tare and sample cylinders. During weighing, the drift of the weighing balance and the buoyancy effect exerted by the cylinders were effectively corrected or canceled out by using the following bracketing sequence: tare – cylinder A – tare – cylinder B – tare – cylinder C. The preparation of standard gas mixtures based on this technique has been reported in detail elsewhere (Wessel, 2008). The CO₂ mole fraction in the resulting mixture can be computed as follows:

$$y_j = \frac{\sum_{A=1}^P \left(\frac{x_{j,A} \cdot m_A}{\sum_{i=1}^n x_{i,A} \cdot M_i} \right)}{\sum_{A=1}^P \left(\frac{m_A}{\sum_{i=1}^n x_{i,A} \cdot M_i} \right)}. \quad (1)$$

Here, y_j is the mole fraction of component j in the gas mixture, P is the total number of parent gases, n is the total number of components in the final mixture, m_A is the measured mass of parent gas A , M_i is the molar mass of component i , and $x_{i,A}$ or $x_{j,A}$ is the mole fraction of component i or j in parent gas A . Therefore, quantification of impurities present in pure parent gases is needed to determine the composition of each parent gas. Hence, impurities in N₂, O₂, Ar, and CO₂ were analyzed by gas chromatography employing various detection methods, e.g., thermal conductivity detection (TCD), pulsed discharge detection (PDD), FID, and atomic emission detection (AED), with detector assignments for all impurities given in Table 1. Purity, namely the mole fraction of the dominant component in “pure” parent gas (x_{pure}), was determined as follows:

$$x_{\text{pure}} = 1 - \sum_{i=1}^N x_i, \quad (2)$$

where N is the number of impurities likely to be present in the final mixture. For selecting target impurities, the source and its purification process were considered. If the expected impurity was not detected, its mole fraction was set to half of the limit of detection (LOD/2), and the associated standard uncertainty was defined as the assigned mole fraction divided by $\sqrt{3}$, e.g., $\text{LOD}/(2 \cdot \sqrt{3})$, as expected for a uniform probability density function ranging from 0 to LOD (ISO 6142-1, 2015). In particular, it was very important to accurately analyze the mole fractions of target components (N₂, O₂, Ar, and CO₂) in the respective raw gases, since the weighed target component amount in the obtained mixture could be biased by the presence of the same component in other raw gases as an impurity. For instance, the mole fractions of CO₂ in pure N₂, O₂, and Ar gases were determined as 0.002, 0.195, and $< 0.002 \mu\text{mol mol}^{-1}$, respectively. Thus, the amounts of CO₂ in pure N₂ and Ar gases were negligible

Table 1. Purities of raw carbon dioxide and background gases (N₂, O₂, and Ar).

Impurity component	Mole fraction (μmol mol ⁻¹)				Detectors ^a
	CO ₂	N ₂	O ₂	Ar	
H ₂	< 0.1	< 0.1	< 0.1	< 0.1	PDD ^b
O ₂	< 0.1	0.003 ± 0.003	–	0.003 ± 0.002	PDD
Ar	< 0.1	21.6 ± 4.32	< 1.0	–	TCD ^c
N ₂	12.8 ± 2.56	–	3.1 ± 0.62	2.4 ± 0.48	PDD
CO	0.3 ± 0.06	< 0.005	0.08 ± 0.016	< 0.005	PDD and FID ^d
CH ₄	2.6 ± 0.52	< 0.005	< 0.005	< 0.005	PDD and FID
CO ₂	–	0.002 ± 0.001	0.195 ± 0.039	< 0.002	PDD and FID
H ₂ O	4.5 ± 2.25	1.6 ± 0.8	1.1 ± 0.55	0.9 ± 0.45	Dew point meter
C ₂	2.8 ± 0.56	–	–	–	AED ^e
C ₃ –C ₅	0.7 ± 0.35	–	–	–	AED
Purity (%) (<i>k</i> = 2)	99.9976 ± 0.0007	99.9976 ± 0.0009	99.9995 ± 0.0002	99.9996 ± 0.0001	

^a Tabulated detectors were coupled to the main body of the gas chromatograph (Agilent 6890A). ^b Pulsed discharge detector. ^c Thermal conductivity detector. ^d Flame ionization detector. ^e Atomic emission detector.

and did not impact final mixtures with CO₂ fractions above 300 μmol mol⁻¹. However, the large amount of CO₂ in pure O₂ led to a bias of 0.04 μmol mol⁻¹, which was comparable to the uncertainty level of the final mixture. Table 1 summarizes the reference values and associated uncertainties of major impurities in raw gases.

For CO₂, a verification test was representatively performed to determine the potential systematic error of the gravimetric procedure described above, relying on comparing the detection sensitivity of CO₂ in different gas mixtures using GC-FID coupled with an MS-5A (molecular sieve 5A, 4 m) separation column. The column oven was kept at 30 °C, and high-purity N₂ (99.999 %, Deokyang Energen) was used as a carrier gas. Sample gas flows were carefully controlled to ensure that the same amount of gas was introduced into the sample loop regardless of its composition; for this purpose, mass flow controllers (MFCs) were calibrated using a flow meter (digital flow calibrator, cat no. 20123, Restek Inc., USA). Therefore, the CO₂ mole fraction uncertainty of prepared mixtures included uncertainties associated with the weighing process, raw gas purities, and verification tests, resulting in a gravimetric preparation uncertainty of less than 0.1 μmol mol⁻¹ (1σ).

The standard gas mixture denoted as EBXXXXXXX (Table 2) was prepared by the static volumetric method (ISO 6144, 2003; Waldén, 2009). Ambient air was collected with a pressurizing pump through a chemical moisture trap containing Mg(ClO₄)₂ in order to yield the complementary gas, namely dry air. The amount of N₂ was then varied by diluting the dry air with high-purity N₂ (> 99.999 %), which eventually led to a variation in the mole fractions of the major components, N₂, O₂, Ar, and CO₂. In this way, the mole fractions of the background gas composition can be easily predicted by using the measured pressure ratio of the filled

Table 2. Mole fractions of gas mixtures.

Cylinder no.	Gas composition (cmol mol ⁻¹)				Preparation method
	CO ₂ [*]	N ₂	O ₂	Ar	
DF4560	400.61 (0.05 %)	99.96	–	–	gravimetry
EB0011591	351.78 (0.10 %)	83.45	16.48	0.04	volumetry
EB0011528	353.08 (0.10 %)	80.97	18.19	0.81	volumetry
ME5590	386.94 (0.05 %)	78.33	21.63	–	gravimetry
EB0006391	406.40 (0.10 %)	78.16	20.87	0.93	volumetry
ME0434	402.25 (0.05 %)	78.07	21.03	0.87	gravimetry
ME5502	384.35 (0.05 %)	77.57	20.53	1.86	gravimetry
ME5537	385.35 (0.05 %)	70.98	18.85	10.12	gravimetry


* Numbers denote the mole fraction (μmol mol⁻¹) of CO₂ and its relative preparation uncertainty.

gas. In the case of the CO₂ mole fraction, three volumetric cylinders (EBXXXXXXX) were calibrated against the gravimetric standards (Table 2) because the mixing ratio of atmospheric CO₂ varies each day. Eventually, the compositions of EB0006391 and ME0434 closely reflected the atmospheric ratio of the major components. Notably, all prepared gas mixtures were maintained under very dry conditions, with the mole fraction of H₂O being less than 5 μmol mol⁻¹.

The ¹²C/¹³C ratio of CO₂ raw gas for the gravimetric standards was similar to the atmospheric level of approximately –11 ‰, which suggests similar isotope ratios would occur across the prepared cylinders as determined by gravimetry and volumetry. Nevertheless, isotope effects biasing the CRDS response seemed to be hardly discernable in this study because verification (calibration) of the CO₂ mole fractions in the prepared gravimetric (volumetric) standards was carried out by GC-FID, which measured the total carbon isotopes.


Table 3. Summary of CRDS calibration results.

Cylinder no.	CO ₂ mole fraction ($\mu\text{mol mol}^{-1}$)			Difference	
	Gravimetrically assigned value (A)	Before CRDS calibration	After CRDS calibration (B)	(B – A) ($\mu\text{mol mol}^{-1}$)	(B – A)/A \times 100 (%)
ME0424	371.22	371.18	371.29	0.07	0.0193
ME0485	380.31	380.23	380.28	–0.03	–0.0088
ME5552	384.76	384.66	384.67	–0.09	–0.0222
ME0434	402.25	402.41	402.30	0.05	0.0117

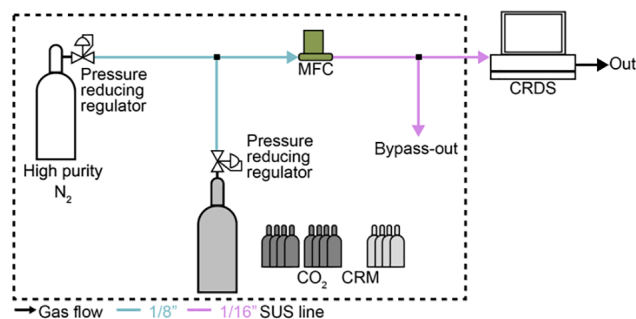**Figure 1.** Schematic diagram depicting the gas supply to the WS-CRDS analyzer. The acronym SUS represents the stainless steel.

2.2 Cavity ring-down spectroscopy

CRDS is an ultrasensitive technique introduced by O’Keefe and Deacon in 1988 (Chen et al., 2010; Rothman et al., 2005). In principle, the leakage rate of the trapped laser source in the optical cavity can be fitted by monoexponential decay, and absorbance at wavelength λ can then be calculated from the difference of ring-down signal decay rates in the presence and absence of the target gas. Alternatively, the absorbance at λ can be determined from the ring-down time at the non-absorbing wavelength λ_0 in the presence of the target gas. In this study, a commercial WS-CRDS (G-1301, Picarro, USA) was employed. Since the WS-CRDS system has been described elsewhere (Chen et al., 2010; Nara et al., 2012), only a brief description is provided here. The WS-CRDS analyzer, operating at a wavelength of $1.603 \mu\text{m}$ that corresponds to $R(1)$ of the $(3\ 0^0\ 1)_{\text{III}} \leftarrow (0\ 0\ 0)$ band, is comprised of diode lasers, a high-precision wavelength monitor, a high-finesse cavity defined by three high-reflectivity mirrors ($< 99.995\%$), a photodiode detector, and a data acquisition computer. Laser light confined in the cavity traveled along the triangular optical axis, exhibiting an effective path length of 15–20 km. Ambient air or gas from a pressure-regulated tank was supplied to the optical cavity backed by a built-in diaphragm pump, which was conditioned to a highly controlled pressure and temperature of 140 ± 0.05 Torr and 40 ± 0.01 °C, respectively.

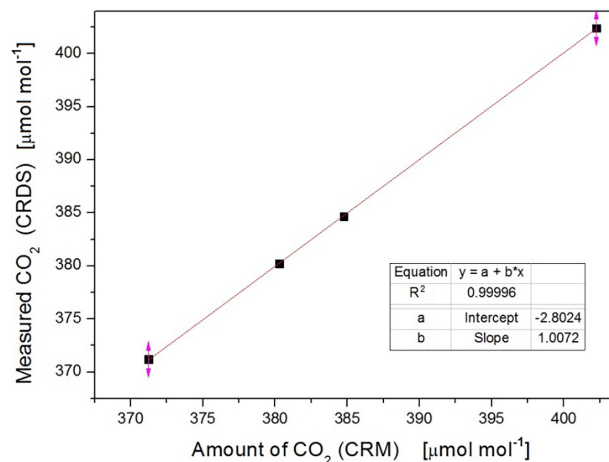**Figure 2.** Result of WS-CRDS calibration using gravimetric standards (ambient air background composition, see main text for details). Good agreement between gravimetric and CRDS-determined CO₂ concentrations was observed.

For this study, a gas flow rate of 400 mL min^{-1} and a pig-tailed bypass-out were combined to achieve a steady gas flow undisturbed by laboratory pressure fluctuation, yielding a constant pressure in the CRDS cavity (Fig. 1). The outer diameters of stainless steel tubes connecting highly pressurized cylinders to the MFC (5850E, Brooks Inc., USA) inlet and the MFC to the spectrometer equaled 0.125 and 0.0625 in., respectively. High-purity nitrogen was used for flushing the gas lines and CRDS analyzer between switching cylinders.

The measured spectral line consisting of ~ 10 points was fitted by the Galatry profile to obtain quantitative information, based on the assumption that the CRDS read-out was influenced only by variations in the CO₂ concentration of tested samples and not by variations of background gas composition (Chen et al., 2010). This assumption implies that the peak height of the fitted profile was regarded as a CRDS read-out instead of the corresponding integrated area (Nara et al., 2012). As described in Table 3, CRDS responses were calibrated against gravimetric standards, in which N₂, O₂, and Ar ratios are close to that in the atmosphere ratio, with CO₂ concentrations very similar to those of ambient air (between 360 and $410 \mu\text{mol mol}^{-1}$). Absorbance was found to be linearly

Table 4. CO₂ concentrations determined by gravimetry and measured by well-calibrated CRDS, together with the correction due to N₂-induced pressure broadening (PBC(N₂)) and total pressure broadening coefficient (TPBC). Differences between the measured (corrected) and assigned concentrations are also listed.

Cylinder no.	CO ₂ mole fraction (μmol mol ⁻¹)				Difference			
	Gravimetrically assigned value (A)	CRDS measured value (B)	PBC (N ₂) corrected (C)	TPBC corrected (D)	$D_{\text{STD-CRDS}}$ (B - A) (μmol mol ⁻¹)	(B - A)/A × 100 (%)	(C - A)/A × 100 (%)	(D - A)/A × 100 (%)
DF4560	400.61	390.84	401.09	400.82	-9.77	-2.44	0.12	0.05
EB0011591	351.78	349.62	351.79	351.97	-2.16	-0.61	0.00	0.05
EB0011528	353.08	352.05	353.00	353.15	-1.03	-0.29	-0.02	0.02
ME5590	386.94	386.51	386.17	386.47	-0.43	-0.11	-0.20	-0.12
EB0006391	406.40	406.39	405.97	406.15	-0.01	0.00	-0.11	-0.06
ME0434	402.25	402.34	401.87	402.09	0.09	0.02	-0.09	-0.04
ME5502	384.35	384.80	384.09	384.17	0.45	0.12	-0.07	-0.05
ME5537	385.35	390.71	386.78	385.95	5.36	1.39	0.37	0.16

proportional to the concentration of light-absorbing gas, as indicated by the straight-line fit of CRDS responses with $R^2 \sim 0.9999$ (Fig. 2 and Table 3), supporting the validity of the attempted calibration and the hypothesis proposed in this study. In other words, deviations from expected sensitivity (i.e., CRDS response divided by the gravimetric concentration of CO₂) were due to deviations in the composition of background gas from that of ambient air, namely the extent of alien gas line broadening or narrowing.

3 Results and discussion

To investigate the effect of background gas composition on CRDS responses, gas mixtures were analyzed against ambient-air-like standards using a well-calibrated CRDS (Table 4).

Deviations of CO₂ concentrations determined by CRDS from those assigned by gravimetry (or volumetry) ranged from -2.44 to 1.39 %. CRDS responses of EB0006391 and ME0434 were in good agreement with the assigned CO₂ concentrations, showing deviations of less than 0.1 μmol mol⁻¹, whereas extreme deviations of greater than 1 % were observed for cylinders DF4560 and ME5537. In particular, the CO₂ concentration of DF4560 (CO₂ in pure N₂) showed a deviation of -9.77 μmol mol⁻¹. Therefore, it can be conjectured that N₂-induced broadening is more important than that induced by other background gases, O₂ and Ar. Since the optical cavity was kept at constant pressure and temperature, Doppler broadening was not considered. Instead, collision-induced broadening (or narrowing) was invoked in the case of variable composition. The collisional half-width, i.e., the total pressure broadening coefficient (γ_{TPB}), can be expressed as follows:

$$\gamma_{\text{TPB}} = \sum_{i=1}^n \gamma_i \cdot p_i, \quad (3)$$

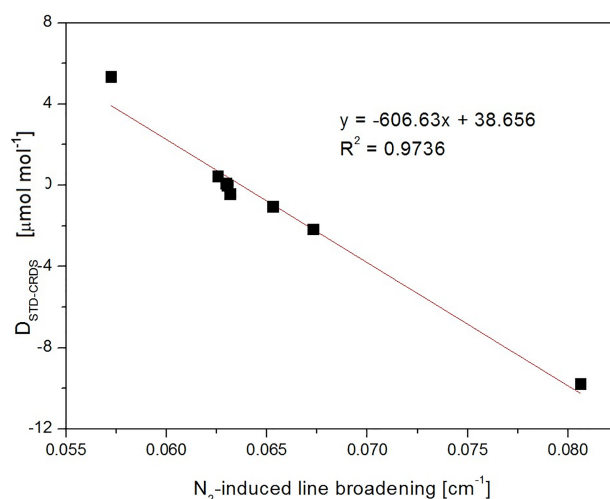


Figure 3. N₂-induced line broadening (x axis) vs. difference between CRDS-measured and assigned CO₂ levels of standard gas mixtures (y axis).

where γ_i is the pressure broadening coefficient (PBC) of component i , and p_i is the partial pressure of component i , e.g., its molar fraction multiplied by the cavity pressure of 18 kPa. The maximum peak height of the Galatry profile at a given background gas composition, $G(\gamma)$, can be assumed to be linearly proportional to the PBC for a sufficiently narrow interval of p_i , Δp_i (Varghese and Hanson, 1984). In view of the dominance of N₂-induced pressure broadening, the difference between CRDS-determined and gravimetrically (volumetrically) assigned CO₂ concentrations of the measured sample, $D_{\text{STD-CRDS}}$, can be determined as follows:

$$D_{\text{STD-CRDS}} \propto G(\gamma) \propto \gamma_{\text{N}_2} \cdot p_{\text{N}_2}. \quad (4)$$

As shown in Fig. 3, a linear relationship between $D_{\text{STD-CRDS}}$ and N₂-induced line broadening was found at given partial pressures (i.e., mole fractions multiplied by cavity pressure) in the optical cavity.

Table 5. Summary of N₂-, O₂-, and Ar-related pressure broadening coefficients in cm⁻¹ atm⁻¹. All parameters were taken by using the Voigt function.

	Pouchet et al. (2004)	Nakamichi et al. (2006)	HITRAN 2004
γ_{N_2}	0.0721	0.08064	0.0778
γ_{O_2}	0.0660	0.06695	0.0702
γ_{Ar}	–	0.06312	–
γ_{air}	–	–	0.0758

The PBC of N₂ was set to 0.08064 cm⁻¹ atm⁻¹, as reported by Nakamichi et al. (2006). Since N₂ showed the largest PBC among those of other background components, positive (or negative) deviations between CRDS-determined and assigned CO₂ concentrations of tested cylinders, i.e., the lower (or higher) extent of pressure broadening, were observed at N₂ concentrations below (or above) the ambient value of 78 cmol mol⁻¹ corresponding to ME5590 (Table 4). Thus, the CO₂ concentration could be corrected based on the following linear fit:

$$y_{corrected} = y_{CRDS} - (-606.63 \cdot \gamma_{N_2} \cdot p_{N_2} + 38.656), \quad (5)$$

where $\gamma_{N_2} \cdot p_{N_2}$ is the N₂-induced pressure broadening, y_{CRDS} is the value obtained by WS-CRDS, and $y_{corrected}$ is the CO₂ concentration corrected for N₂-induced pressure broadening. Corrected CO₂ concentrations exhibited good agreement (within 0.4 %) with the regression fit ($R^2 \sim 0.9736$). This correction error significantly exceeded the instrumental precision (reported as 0.01 % (1 σ); Nara et al., 2012), strongly suggesting the presence of other error sources.

The pressure broadening correction of ME5537 showed the highest deviation of 0.4 %. The background gas composition of ME5537 (70.98 % N₂, 18.85 % O₂, and 10.13 % Ar) implied that the Ar content should be taken into account for the correction. Since CO₂ self-broadening is negligible due to the low concentration of CO₂ compared to that of other components (N₂, O₂, and Ar) in the investigated gas mixtures, the total pressure broadening coefficient (TPBC) could be expressed as a function of alien gas PBCs and the partial pressures of the corresponding components:

$$\gamma_{TPBC} = \gamma_{N_2} p_{N_2} + \gamma_{O_2} p_{O_2} + \gamma_{Ar} p_{Ar}. \quad (6)$$

Table 5 shows the reported PBCs for N₂, O₂, and Ar, and Table 6 shows TPBCs of all cylinders, with (a), (b), and (c) denoting results obtained independently by Pouchet et al. (2004), Nakamichi et al. (2006), and HITRAN2004 (Rothman et al., 2005), respectively.

Since the coefficients of Ar have not been reported by Pouchet et al. (2004) and HITRAN2004, the corresponding TPBCs include only N₂- and O₂-related pressure broadening

Table 6. Pressure broadening for investigated gas mixtures based on pressure broadening coefficients from different sources.

Cylinder no.	Pouchet et al. (2004)*	Nakamichi et al. (2006)	HITRAN 2004*
DF4560	0.0721	0.08061	0.0778
EB0011591	0.0710	0.07835	0.0765
EB0011528	0.0704	0.07798	0.0758
ME5590	0.0708	0.07765	0.0761
EB0006391	0.0701	0.07759	0.0755
ME0434	0.0702	0.07758	0.0755
ME5502	0.0695	0.07747	0.0748
ME5537	0.0636	0.07625	0.0685

* Pressure broadenings were estimated without Ar due to the absence of a broadening coefficient in the corresponding studies.

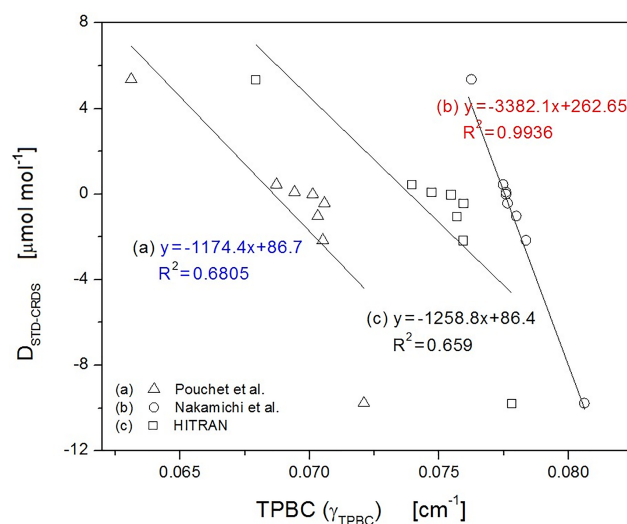


Figure 4. Total pressure broadening coefficient vs. difference between CRDS-measured and assigned CO₂ levels of standard gas mixtures. Due to the lack of γ_{Ar} , correlations (a) and (c) exhibit poor fits.

(Table 6). Therefore, the TPBCs in (a) and (c) were underestimated in comparison to those in (b). For instance, TPBCs of 0.0636 and 0.0685 were obtained for cylinder ME5537 in the cases of (a) and (c), respectively, with the value for (b) equaling 0.07625. As shown in Table 6, the TPBC of ME5537 exhibited the largest deviation of 20 %, originating mainly from the Ar mole fraction. Figure 4 shows $D_{STD-CRDS}$ values (taken from fourth column in Table 4) as a function of calculated TPBCs (taken from Table 6).

TPBC values reported by Nakamichi et al. (2006) exhibited a linear correlation with CRDS responses within the investigated background composition interval. In practice, Huang and Yung (2004) reported that the Lorentzian width is inversely proportional to the peak value of the Voigt function for a fixed Gaussian width. The results shown in Fig. 4 reveal that $D_{STD-CRDS}$ values decreased with increasing TPBCs, in

agreement with previous reports (Huang and Yung, 2004). Only the result of (b) exhibited a fairly linear behavior; however, nonlinearity was observed when the broadening coefficients of O₂ or Ar were not taken into account. The following equation was derived for correcting CRDS-determined concentrations:

$$y_{\text{corr.TPBC}} = y_{\text{CRDS}} - (-3382.1 \cdot \gamma_{\text{TPBC}} + 262.65). \quad (7)$$

Here, y_{CRDS} is the CRDS-measured value of the standard gas mixture, and $y_{\text{corr.TPBC}}$ is the corresponding corrected CRDS response computed using the relation in (b) (Fig. 4). Table 4 summarizes the results obtained after correction using Eq. (7), showing that the correction was improved from 0.68 (N₂ PBC) to 0.33 $\mu\text{mol mol}^{-1}$ (TPBC) in terms of standard deviations (1σ) of differences (corrected minus gravimetry-assigned). Furthermore, R^2 was improved to 0.99 when pressure broadening related to three main components of air (N₂, O₂, and Ar) was taken into account. For every cylinder, excellent agreement was observed after implementing the TPBC corresponding to the assigned values. In particular, even cylinders DF4560, ME5590, and ME5537, whose background gas compositions were significantly different from that of ambient air, exhibited good correlation of CO₂ concentrations determined by CRDS with those assigned by gravimetry or volumetry. It is worth noting that the quality of the TPBC correction can be improved further by using quality standards with lower background composition uncertainties, including ¹³CO₂ isotopologues and precisely measured broadening coefficients that are deduced from advanced line-shape functions such as Galatry and Rautian profiles.

4 Conclusions

In this study, we investigated the impact of background gas composition on spectroscopic quantitation of CO₂ at ambient concentration. Standard gas mixtures with various background compositions were prepared by gravimetry or volumetry for use as calibration standards and test samples. Purity analysis and gravimetric weighing showed high accuracy and precision. For purity analysis, analytical techniques such as GC-PDD, TCD, FID, AED, and dew point metering were used. Raw gas (N₂, O₂, Ar, and CO₂) purities were obtained within uncertainties of less than 0.001 % (1σ). Moreover, biasing impurities in N₂, O₂, and CO₂ were accurately cross-checked. With a weighing precision of 0.007 %, the preparation uncertainties of gravimetric and volumetric mixing were demonstrated to be lower than 0.05 and 0.1 % (2σ), respectively, after performing verification tests. The preparation uncertainty of volumetry was slightly higher than that of gravimetry, still being sufficiently satisfactory to distinguish error sources for “matrix effect” correction. Based on the composition accuracy of the prepared gas mixtures, CO₂ levels were determined by WS-CRDS for eight standard gas mixtures with different background compositions. An injec-

tion unit with a bypass-out was used to ensure a precise and moderate gas inflow from a highly pressurized cylinder to the WS-CRDS, which was calibrated against well-certified standard gas mixtures of air composition with CO₂ levels of 360–410 $\mu\text{mol mol}^{-1}$. Among the eight cylinders, the CRDS responses of EB0006391 and ME0434 were well matched to the corresponding preparative values, whereas the values obtained for other cylinders exhibited large deviations between +5.36 and −9.77 $\mu\text{mol mol}^{-1}$. For a N₂-enriched mixture (DF4560), the CRDS-determined CO₂ concentration was 2.44 % lower than the preparative value. Since CRDS calibration was performed using standards with ambient air composition, the fact that CRDS responses tended to be negative for N₂-enriched and positive for Ar-enriched mixtures was in good agreement with the results obtained in earlier experimental (Nara et al., 2012; Zhao et al., 1997) and theoretical studies (Huang and Yung, 2004), reflecting the dependence of line broadening on alien gas composition.

Therefore, a linear shift of CRDS responses was observed for TPBCs above 0.05 $\text{cm}^{-1} \text{atm}^{-1}$, which covers 20 % N₂-enriched and 10 % Ar-enriched gas mixtures. TPBC-corrected CRDS responses were in good agreement with the gravimetric (or volumetric) concentration of the investigated gas mixtures within 0.15 % ($\pm 0.6 \mu\text{mol mol}^{-1}$). Considering the instrumental uncertainty of 0.01 % (1σ), the improved PBC uncertainties should lead to lower discrepancies of corrected CRDS responses. The correction presented in Eq. (7) works only for the designated vibrational transition, i.e., $R(1)$ of the $(3\ 0^0\ 1)_{\text{III}} \leftarrow (0\ 0\ 0)$ band at 1.603 μm , and referred PBCs, but a similar calibration strategy can be used for determining gas mixing ratios by other intensity-based optical measurement techniques.

Data availability. No data sets were used in this article.

Author contributions. JiL prepared the certified reference materials, JSL and MP performed measurements and analysis. JeL designed experiments, and JSL prepared the manuscript with contributions from other co-authors.

Competing interests. The authors declare that they have no conflict of interest.

Acknowledgements. This work was funded by the Korea Meteorological Administration Research and Development Program under grant no. KMIPA 2015-2032.

Edited by: Christian Brümmer
Reviewed by: Zoe Loh and Jooil Kim

References

- Chen, H., Winderlich, J., Gerbig, C., Hofer, A., Rella, C. W., Crosson, E. R., Van Pelt, A. D., Steinbach, J., Kolle, O., Beck, V., Daube, B. C., Gottlieb, E. W., Chow, V. Y., Santoni, G. W., and Wofsy, S. C.: High-accuracy continuous airborne measurements of greenhouse gases (CO₂ and CH₄) using the cavity ring-down spectroscopy (CRDS) technique, *Atmos. Meas. Tech.*, 3, 375–386, <https://doi.org/10.5194/amt-3-375-2010>, 2010.
- Conway, T. J., Tans, P., Waterman, L. S., Thoning, K. W., Masarie, K. A., and Gammon, R. H.: Atmospheric carbon dioxide measurements in the remote global troposphere 1981–1984, *Tellus B*, 40, 81–115, <https://doi.org/10.1111/j.1600-0889.1988.tb00214.x>, 1998.
- Crawley, L. H.: Application of non-dispersive infrared (NDIR) spectroscopy to the measurement of atmospheric trace gases, MSc Thesis, University of Canterbury, Christchurch, New Zealand, 2008.
- Crosson E. R.: A cavity ring-down analyzer for measuring atmospheric levels of methane, carbon dioxide, and water vapor, *Appl. Phys. B*, 92, 403–408, <https://doi.org/10.1007/s00340-008-3135-y>, 2008.
- Durry, G., Li, J. S., Vinogradov, I., Titov, A., Joly, L., Cousin, J., Decarpenterie, T., Amarouche, N., Liu, X., Parvitte, B., Korablev, B., Gerasimov, M., and Zéninari, V.: Near infrared diode laser spectroscopy of C₂H₂, H₂O, CO₂ and their isotopologues and the application to TDLAS, a tunable diode laser spectrometer for the Martian PHOBOS-GRUNT space mission, *Appl. Phys. B*, 99, 339–351, <https://doi.org/10.1007/s00340-010-3924-y>, 2010.
- Griffith, D. W. T., Deutscher, N. M., Caldow, C., Kettlewell, G., Riggensbach, M., and Hammer, S.: A Fourier transform infrared trace gas and isotope analyser for atmospheric applications, *Atmos. Meas. Tech.*, 5, 2481–2498, <https://doi.org/10.5194/amt-5-2481-2012>, 2012.
- Huang, X. and Yung, Y. L.: A common misunderstanding about the Voigt line profile, *J. Atmos. Sci.*, 61, 1630–1632, [https://doi.org/10.1175/1520-0469\(2004\)061<1630:ACMATV>2.0.CO;2](https://doi.org/10.1175/1520-0469(2004)061<1630:ACMATV>2.0.CO;2), 2004.
- ISO 6142-1: Gas analysis- Preparation of calibration gas mixture- Part 1: Gravimetric method for class 1 mixtures, available at: <https://www.iso.org/standard/59631.html>, last access: August 2015.
- ISO 6144: Gas analysis- Preparation of calibration gas mixture- Static volumetric method, available at: <https://www.iso.org/standard/24666.html>, last access: February 2003.
- Lee, J.-Y., Hee-Soo, Y., Marti, K., Moon, D. M., Lee, J. B., and Kim, J. S.: Effect of carbon isotopic variations on measured CO₂ abundances in reference gas mixtures, *J. Geophys. Res.*, 111, D053302, <https://doi.org/10.1029/2005JD006551>, 2006.
- Messerschmidt, J., Geibel, M. C., Blumenstock, T., Chen, H., Deutscher, N. M., Engel, A., Feist, D. G., Gerbig, C., Gisi, M., Hase, F., Katrynski, K., Kolle, O., Lavric, J. V., Notholt, J., Palm, M., Ramonet, M., Rettinger, M., Schmidt, M., Sussmann, R., Toon, G. C., Truong, F., Warneke, T., Wennberg, P. O., Wunch, D., and Xueref-Remy, I.: Calibration of TCCON column-averaged CO₂: the first aircraft campaign over European TCCON sites, *Atmos. Chem. Phys.*, 11, 10765–10777, <https://doi.org/10.5194/acp-11-10765-2011>, 2011.
- Min, D., Kang, N., Moon, D. M., Lee, J. B., Lee, D. S., and Kim, J. S.: Effect of variation in argon content of calibration gases on determination of atmospheric carbon dioxide, *Talanta*, 80, 422–427, <https://doi.org/10.1016/j.talanta.2009.03.019>, 2009.
- Nakamichi, S., Kawaguchi, Y., Fukuda, H., Enami, S., Hashimoto, S., Kawasaki, M., Umekawa, T., Morino, I., Suto, H., and Inoue, G.: Buffer-gas pressure broadening for the (3 0⁰ 1)_{III} ← (0 0 0) band of CO₂ measured with continuous-wave cavity ring-down spectroscopy, *Phys. Chem. Chem. Phys.*, 8, 364–368, <https://doi.org/10.1039/b511772k>, 2006.
- Nara, H., Tanimoto, H., Tohjima, Y., Mukai, H., Nojiri, Y., Katsumata, K., and Rella, C. W.: Effect of air composition (N₂, O₂, Ar, and H₂O) on CO₂ and CH₄ measurement by wavelength-scanned cavity ring-down spectroscopy: calibration and measurement strategy, *Atmos. Meas. Tech.*, 5, 2689–2701, <https://doi.org/10.5194/amt-5-2689-2012>, 2012.
- O’Shea, S. J., Bauguitte, S. J.-B., Gallagher, M. W., Lowry, D., and Percival, C. J.: Development of a cavity-enhanced absorption spectrometer for airborne measurements of CH₄ and CO₂, *Atmos. Meas. Tech.*, 6, 1095–1109, <https://doi.org/10.5194/amt-6-1095-2013>, 2013.
- Pouchet, I., Zéninari, V., Parvitte, B., and Durry, G.: Diode laser spectroscopy of CO₂ in the 1.6 μm region for the in situ sensing of the middle atmosphere, *J. Quant. Spectrosc. Ra.*, 83, 619–628, [https://doi.org/10.1016/S0022-4073\(03\)00108-0](https://doi.org/10.1016/S0022-4073(03)00108-0), 2004.
- Solomon, S., Qin, D., Manning, M., Chen, Z., Marquis, M., Averyt, K., Tignor, M. M. B., and Miller, H. L. (Eds.): *Climate Change 2007: The Physical Science Basis. Contribution of Working Group I to the Fourth Assessment Report of the Intergovernmental Panel on Climate Change*, Cambridge University Press, New York, N. Y., 2007.
- Rella, C. W., Chen, H., Andrews, A. E., Filges, A., Gerbig, C., Hatakka, J., Karion, A., Miles, N. L., Richardson, S. J., Steinbacher, M., Sweeney, C., Wastine, B., and Zellweger, C.: High accuracy measurements of dry mole fractions of carbon dioxide and methane in humid air, *Atmos. Meas. Tech.*, 6, 837–860, <https://doi.org/10.5194/amt-6-837-2013>, 2013.
- Rothman, L. S., Jacquemart, D., Barbe, A., Benner, D. C., Birk, M., Brown, L. R., Carleer, M. R., Chackerian Jr., C., Chance, K., Coudert, L. H., Dana, V., Devi, V. M., Flaud, J.-M., Gamache, R. R., Goldman, A., Hartmann, J.-M., Jucks, K. W., Maki, A. G., Mandin, J.-Y., Massie, S. T., Orphal, J., Perrin, A., Rinsland, C. P., Smith, M. A. H., Tennyson, J., Tolchenov, R. N., Toth, R. A., Vander Auwera, J., Varanasi, P., and Wagner, G.: The HITRAN 2004 molecular spectroscopic database, *J. Quant. Spectrosc. Ra.*, 96, 139–204, <https://doi.org/10.1016/j.jqsrt.2004.10.008>, 2005.
- Schulze, E. D., Luyssaert, S., Ciais, P., Freibauer, A., Janssens, I. A., Soussana, J. F., Smith, P., Grace, J., Levin, I., Thiruchittampalam, B., Heimann, M., Dolman, A. J., Valentini, R., Bousquet, P., Peylin, P., Peters, W., Rödenbeck, C., Etiope, G., Vuichard, N., Wattenbach, M., Nabuurs, G. J., Poussi, Z., Nieschulze, J., Gash, J. H., and the CarboEurope Team: Importance of methane and nitrous oxide for Europe’s terrestrial greenhouse-gas balance, *Nat. Geosci.*, 2, 842–850, <https://doi.org/10.1038/ngeo686>, 2009.
- Tohjima, Y., Katsumata, K., Morino, I., Mukai, H., Machida, T., Akama, I., Amari, Y., and Tsunogai, U.: Theoretical and experimental evaluation of the isotope effect of NDIR analyzer on atmospheric CO₂ measurement, *J. Geophys. Res.*, 114, D13302, <https://doi.org/10.1029/2009JD011734>, 2009.
- van der Laan, S., Neubert, R. E. M., and Meijer, H. A. J.: A single gas chromatograph for accurate atmospheric mixing ratio mea-

- surements of CO₂, CH₄, N₂O, SF₆ and CO, *Atmos. Meas. Tech.*, 2, 549–559, <https://doi.org/10.5194/amt-2-549-2009>, 2009.
- Varghese, P. L. and Hanson, R. K.: Collisional narrowing effects on spectral line shapes measured at high resolution, *Appl. Optics*, 23, 2376, <https://doi.org/10.1364/AO.23.002376>, 1984.
- Waldén, J. (Ed.): *Metrology of Gaseous Air Pollutants*, No. 79 (Finnish Meteorological Institute Contributions), Finnish Meteorological Institute, Finland, 2009.
- Wessel, R. M., van der Veen, A. M. H., Ziel, P. R., Steele, P., Langenfelds, R., van der Schoot, M., Smeulders, D., Besley, L., da Cunha, V. S., Zhou, Z., Qiao, H., Heine, H. J., Martin, B., Macé, T. P., Gupta, K., di Meane, E. A., Sega, M., Rolle, F., Maruyama, M., Kato, K., Matsumoto, N., Kim, J. S., Moon, D. M., Lee, J. B., Murillo, F. R., Nambo, C. R., Caballero, V. M. S., de Jesús Avila Salas, M., Castorena, A. P., Konopelko, L. A., Kustikov, Y. A., Kolobova, A. V., Pankratov, V. V., Efremova, O. V., Musil, S., Chromek, F., Valkova, M., Milton, M. J. T., Vargha, G., Guenther, F., Miller, W. R., Botha, A., Tshilongo, J., Mokgoro, I. S., and Leshabane, N.: International comparison CCQM-K52: Carbon dioxide in synthetic air, *Metrologia*, 45, 08011, <https://doi.org/10.1088/0026-1394/45/1A/08011>, 2008.
- Zhao, C. L., Tans, P. P., and Thoning, K. W.: A high precision manometric system for absolute calibrations of CO₂ in dry air, *J. Geophys. Res.*, 102, 5885–5894, <https://doi.org/10.1029/96JD03764>, 1997.