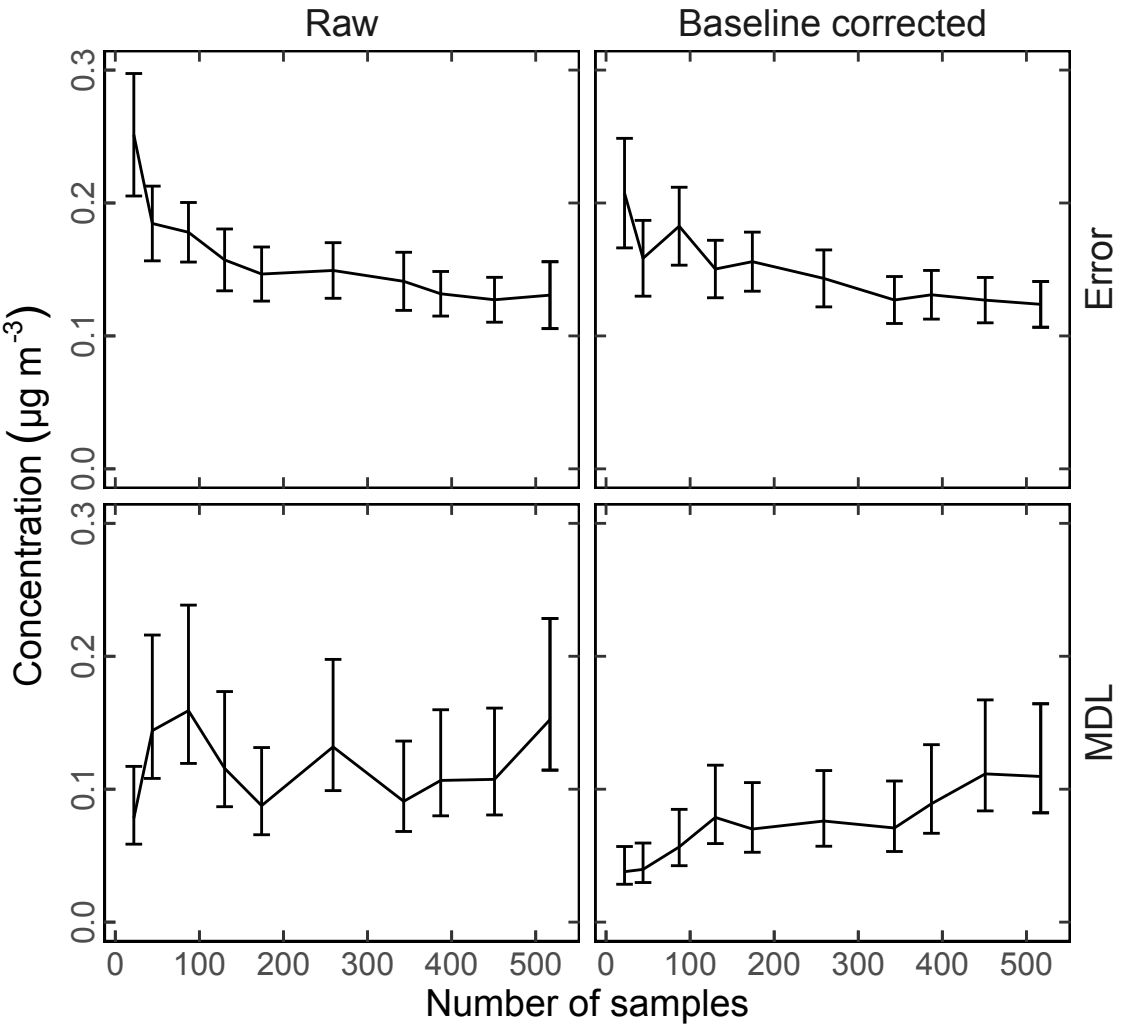
Raw
Baseline corrected
Error
MDL
Concentration (μg m-3)
0.0
0.1
0.2
0.3
0
100
200
300
400
500
Number of samples