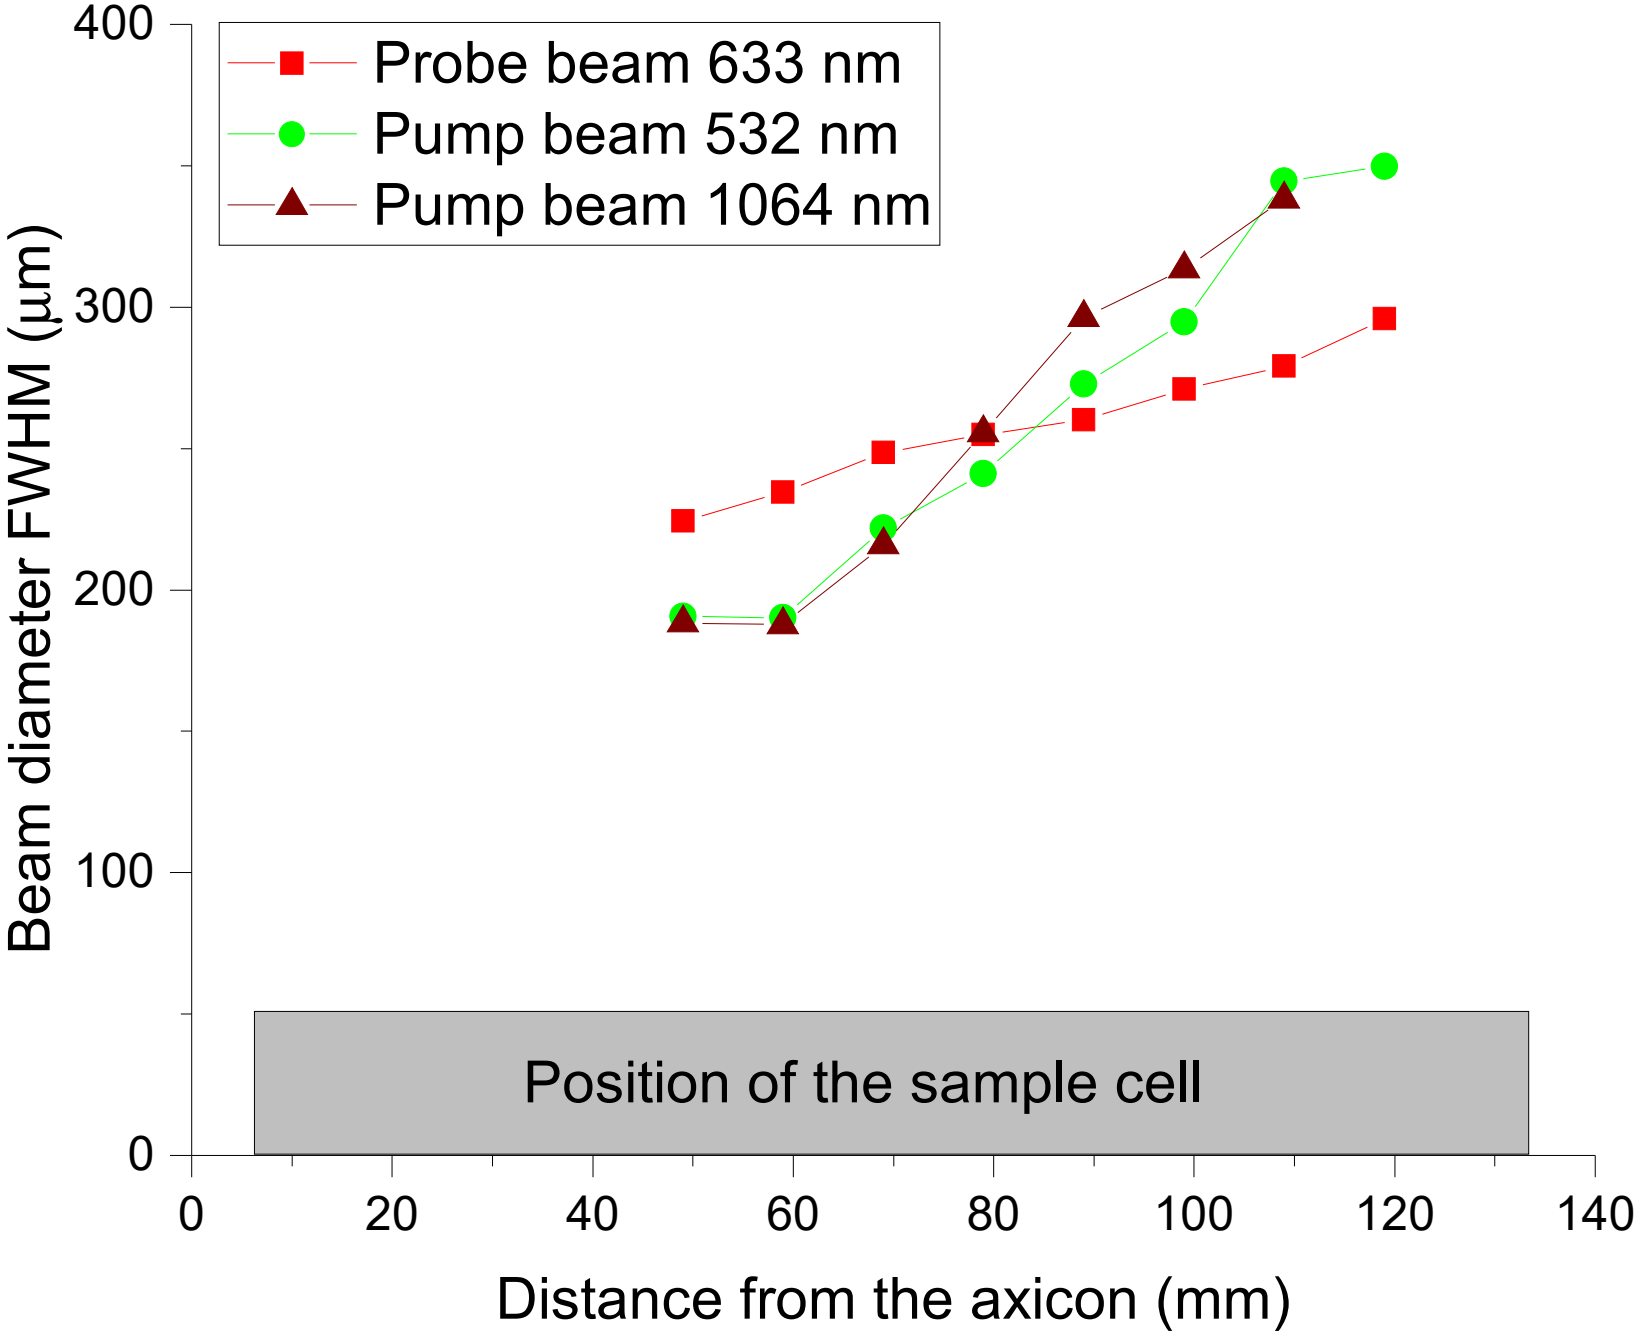
Probe beam 633 nm
Pump beam 532 nm
Pump beam 1064 nm
Position of the sample cell
Beam diameter FWHM (µm)
Distance from the axicon (mm)
0
100
200
300
400
0
20
40
60
80
100
120
140