



Sensitivity of tunable infrared laser spectroscopic measurements of $\Delta^{17}\text{O}$ in CO_2 to analytical conditions

David Bajnai¹ and Vincent J. Hare^{2,3}

¹Department of Geochemistry and Isotope Geology, Geoscience Center, University of Göttingen, Göttingen, Germany

²Stable Light Isotope Laboratory, Department of Archaeology, University of Cape Town, Cape Town, South Africa

³Node for Isotope Biogeochemistry, BIOGRIP, University of Cape Town, Cape Town, South Africa

Correspondence: David Bajnai (david.bajnai@uni-goettingen.de)

Received: 25 June 2025 – Discussion started: 14 August 2025

Revised: 23 October 2025 – Accepted: 17 November 2025 – Published: 5 December 2025

Abstract. Triple oxygen isotope ($\Delta^{17}\text{O}$) measurements of CO_2 are increasingly used in atmospheric and paleoenvironmental research, supported by the rise of tunable infrared laser direct absorption spectroscopy (TILDAS) as a cost- and time-effective method for quantifying rare isotopologues in CO_2 . In this study we use data from two TILDAS instruments (University of Göttingen and University of Cape Town) to evaluate how the stability of analytical conditions, such as temperature, optical cell pressure, and the analyte's CO_2 concentration influences measurement repeatability. We identify the mismatch in CO_2 concentration between sample and working gas as the most significant factor affecting the repeatability of $\Delta^{17}\text{O}$ measurements. The resulting scale-offset effect can amount to several ppm per $\mu\text{mol mol}^{-1}$ mismatch, depending on instrumental configuration. Applying empirical corrections for such offsets significantly improves repeatability. We show that maintaining electronics temperature, cell temperature, and cell pressure stability within $\pm 0.1\text{ K}$, $\pm 1\text{ mK}$, and $\pm 10\text{ Pa}$, respectively, across the cycles of a replicate measurement is sufficient to avoid any resolvable impact on the internal error. Over multi-week timescales, drift in measured isotope ratios is primarily driven by variations in the temperature of electronic components, while fluctuations in cell temperature, pressure, and analyte concentration exert smaller but detectable influences. We conclude with practical recommendations for achieving high precision triple oxygen isotope measurements with TILDAS, emphasizing that continuous monitoring and reporting of analytical conditions is essential.

1 Introduction

Oxygen has three stable isotopes, with 99.7 % as ^{16}O , 0.2 % as ^{18}O , and only about 0.04 % as ^{17}O . Measurements of the $^{18}\text{O}/^{16}\text{O}$ ratio in solids, liquids, and gases has proved invaluable across nearly every field of Earth science. Additional measurements of the $^{17}\text{O}/^{16}\text{O}$ ratios, known as triple oxygen isotope analyses, provides additional information on fractionation mechanisms and the mixing and transport processes that drive variations in oxygen isotope ratios (Pack and Herwartz, 2014; Young et al., 2002).

Mass-dependent fractionation processes result in a correlation between the $\delta^{17}\text{O}$ and $\delta^{18}\text{O}$ values, following slopes of approximately 0.5 (Craig, 1957; Matsuhisa et al., 1978; Young et al., 2002). The exact slope of the correlation depends on the specific mass dependent fractionation process and temperature. The $\Delta^{17}\text{O}$ notation expresses deviations in the relative abundances of oxygen isotopes from a reference line:

$$\Delta^{17}\text{O} = \ln(\delta^{17}\text{O} + 1) - \lambda_{\text{RL}} \cdot \ln(\delta^{18}\text{O} + 1) - \gamma_{\text{RL}} \quad (1)$$

where λ_{RL} and γ_{RL} represent the slope and intercept of the reference line, respectively. Following common practice, we use $\lambda_{\text{RL}} = 0.528$ and $\gamma_{\text{RL}} = 0$ (Luz and Barkan, 2010; Miller et al., 2020).

Mass-independent isotope fractionation during photochemical reactions in the stratosphere produce CO_2 that is enriched in ^{17}O ($\Delta^{17}\text{O} \gg 0$) (cf., Boering et al., 2004; Thiemens et al., 1995). Carbon dioxide from high-temperature combustion processes inherits the ^{17}O -depleted signature of atmospheric O_2 ($\Delta^{17}\text{O} \ll 0$) (Horváth et

al., 2012). These ^{17}O -anomalies are largely reset to near-zero values in the troposphere through mass-dependent isotope exchange between CO_2 and water. The $\Delta^{17}\text{O}$ value of tropospheric CO_2 therefore provides information on the various natural and anthropogenic CO_2 sources and enables quantification of their respective fluxes. Because isotope exchange between CO_2 and water occurs predominantly through the terrestrial biosphere, the triple oxygen isotope approach also offers a means of estimating gross primary productivity (Adnew et al., 2025; Barkan and Luz, 2012; Hoag et al., 2005; Hofmann et al., 2017; Horváth et al., 2012; Koren et al., 2019; Liang et al., 2023; Steur et al., 2024; Thiemens et al., 2014). These applications, however, require analytical methods capable of providing high-precision $\Delta^{17}\text{O}$ measurements (≤ 10 ppm repeatability) rapidly and cost-effectively.

There is a methodological overlap between atmospheric and carbonate research, as both analyse CO_2 – in carbonate work, this is commonly obtained via phosphoric acid digestion. A sub-10 ppm repeatability of $\Delta^{17}\text{O}$ measurements in carbonates is also desirable, as such high-precision analyses are necessary to investigate near-equilibrium fractionation processes relevant to biomineralization and paleoenvironmental research (e.g., Affek et al., 2025; Bajnai et al., 2024; Hare et al., 2025; Kelson et al., 2022).

Stable carbon and oxygen isotope ratios ($\delta^{13}\text{C}$ and $\delta^{18}\text{O}$) in CO_2 are typically measured using isotope ratio mass spectrometry (McCrea, 1950). However, the isotopologue $^{16}\text{C}^{13}\text{C}^{16}\text{O}$ has the same nominal mass as the most abundant ^{17}O -containing isotopologue $^{16}\text{O}^{12}\text{C}^{17}\text{O}$. This mass interference not only prevents the direct measurement of $\delta^{17}\text{O}$ in CO_2 using conventional mass spectrometry but also necessitates corrections in these measurements to account for the ^{17}O signal (Brand et al., 2010; Saenger et al., 2021).

To generate $\Delta^{17}\text{O}$ data for CO_2 , alternative approaches have been developed, most of which produce O_2 as the analyte, thereby avoiding mass interference. These techniques include the fluorination of CO_2 (Wostbrock et al., 2020), the conversion of CO_2 to H_2O followed by the fluorination of H_2O using CoF_3 (Brenninkmeijer and Röckmann, 1998; Passey et al., 2014), the equilibration of CO_2 with O_2 using a Pt catalyst (Barkan and Luz, 2012; Mahata et al., 2013), and the equilibration of CO_2 with CeO_2 followed by fluorination (Hofmann and Pack, 2010; Mahata et al., 2012). High-resolution mass spectrometry has also been used to obtain precise $\Delta^{17}\text{O}$ data on CO_2 (Adnew et al., 2019). However, the above methods are generally too labor-intensive to be practical for routine monitoring of atmospheric CO_2 .

In recent years, laser spectroscopy has become a viable alternative to mass spectrometry for quantifying rare isotopologues in a range of trace gases, such as CO , CO_2 , N_2O , and CH_4 (Becker et al., 1992; Bergamaschi et al., 1994; Lee and Majkowski, 1986; McManus et al., 2006; Mohn et al., 2014; Nataraj et al., 2022; Nelson et al., 2008; Prokhorov et al., 2019; Sakai et al., 2017; Stoltmann et al., 2017; Tuz-

son et al., 2008; Wang et al., 2020; Yanay et al., 2022; Zhang et al., 2025). Laser spectroscopy determines isotopologue abundances based on the absorption of laser light at specific wavelengths that correspond to the unique vibrational and rotational energy levels of different isotopologues. Consequently, isotopologue ratios obtained through laser spectroscopy are inherently free from mass interference-related biases. For triple oxygen isotope measurements in CO_2 , two different spectroscopy techniques have been used, cavity ring-down spectroscopy (CRDS) (Chaillot et al., 2025; Stoltmann et al., 2017), and tunable infrared laser direct absorption spectroscopy (TILDAS) (Bajnai et al., 2023; Hare et al., 2022; Perdue et al., 2022; Steur et al., 2021). In this paper, we specifically focus on TILDAS. While some aspects of our discussion relate to the commercially available TILDAS instrument from Aerodyne Research Inc. (Billerica, MA, USA), which also has been used in several recent studies on CO_2 triple oxygen isotopes, most apply to the tunable laser absorption spectroscopy in general. Several studies have demonstrated that TILDAS can achieve a repeatability (standard error) of $\Delta^{17}\text{O}$ measurements of 10 ppm or better, at high speed, while maintaining relatively low analytical costs making it ideal for both air monitoring studies and analyses of carbonate-derived CO_2 (Bajnai et al., 2023; Hare et al., 2022; Perdue et al., 2022).

A typical TILDAS setup consists of a laser with a tunable output frequency, a multipass cell containing the analyte gas, and a detector (McManus et al., 2006, 2015; Nelson et al., 2008). The Beer–Lambert Law provides the foundation for calculating isotopologue abundances:

$$I_{(\nu)} = I_{0(\nu)} \exp \left[- \frac{N_A}{\ln(10)} S_{(T)} \phi_{(\nu,P,T)} L C \right] \quad (2)$$

where I and I_0 are the intensity of the transmitted and the incident light at frequency ν , respectively. N_A is Avogadro's number ($\text{molecules mol}^{-1}$), S denotes the line strength ($\text{cm}^{-1} (\text{molecule cm}^{-2})^{-1}$), which depends on temperature, ϕ the line-shape function (cm), L the absorption path length (cm), and C the concentration of the absorbing species (mol cm^{-3}). For CO_2 triple oxygen isotope measurements, the abundance of the isotopologues “628” ($^{16}\text{O}^{12}\text{C}^{18}\text{O}$), “627” ($^{16}\text{O}^{12}\text{C}^{17}\text{O}$), and “626” ($^{16}\text{O}^{12}\text{C}^{16}\text{O}$) are quantified based on respective, distinct absorption peaks in the spectral region around 2349 cm^{-1} (Fig. 1). These shorthand notations, commonly used in spectroscopy, identify isotopologues by the second digit of the atoms' atomic masses. The line shape function describes how the absorption of light is distributed around the central wavenumber of a spectral line. It is typically represented by Voigt profile and is derived empirically from the acquired absorption spectra, measurements of temperatures and pressure as well as spectroscopic fitting parameters retrieved from the high-resolution transmission molecular absorption database (HITRAN) (Gordon et al., 2022).

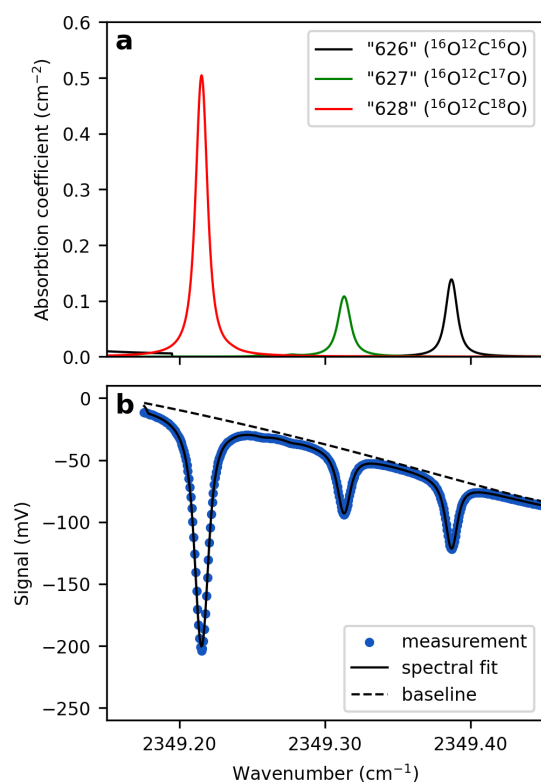


Figure 1. Modeled and measured CO_2 absorption spectra for $\Delta^{17}\text{O}$ analysis. **(a)** Absorption coefficients of the three CO_2 isotopologues used for triple oxygen isotope measurements, retrieved from the HITRAN database. The broadening coefficients reflect the experimental conditions below: $P = 41.335$ Torr, $T = 297.6$ K, and $p\text{CO}_2 = 420 \mu\text{mol mol}^{-1}$. **(b)** Measured spectrum of a CO_2 -in-air gas mixture obtained using TILDAS. Green dots represent individual data points, each corresponding to an average of 1538 spectra acquired at a rate of one spectrum per second. The TDLWintel software fits the spectrum to the data (blue line), accounting for several parameters, including the analyte's temperature and pressure, as well as spectroscopic information from the HITRAN database. Diluting a pure CO_2 analyte with a collision gas broadens the absorption peaks, allowing each peak to be represented by more data points.

While variations in the analytical conditions, such as temperature, optical cell pressure, and CO_2 concentration have been shown to influence the repeatability of $\Delta^{17}\text{O}$ measurements by TILDAS (Bajnai et al., 2023; Hare et al., 2022, 2025; Perdue et al., 2022; Steur et al., 2021), the extent to which they affect the measured values remain largely unexplored. Understanding the impacts of changing analytical conditions is becoming increasingly important as TILDAS is applied more widely, for example, in long-term atmospheric monitoring studies where analytical conditions are likely to vary (e.g., Steur et al., 2024). In this paper, we examine the sources of analytical uncertainties in two TILDAS setups, located at the University of Göttingen and the University of Cape Town, and evaluate how variations in analytical condi-

tions affect the repeatability of triple oxygen isotope ($\Delta^{17}\text{O}$) measurements of CO_2 .

2 Definitions of spectroscopic isotopologue ratios

TILDAS instruments report scaled isotopologue mole fractions, also referred to as mixing ratios (χ' , commonly expressed as $\mu\text{mol mol}^{-1}$ but Aerodyne Research Inc. instruments report nmol mol^{-1}):

$$\chi'_i = C_i R \frac{T}{P} \frac{1}{X_i} \quad (3)$$

where C is the concentration (mol m^{-3}) of the isotopologue i (e.g., "626", "627", "628"), R is the gas constant ($\text{m}^3 \text{Pa K}^{-1} \text{mol}^{-1}$), T and P denote the temperature (K) and pressure (Pa) of the analyte gas, respectively. X_i denotes the isotopologue abundance of the analyzed isotopologue, as defined in the HITRAN database: $X_{626} = 0.98420$, $X_{628} = 0.0039471$, and $X_{627} = 0.000734$ (De Bièvre et al., 1984; Gordon et al., 2022). Each isotopologue absorption feature is scaled by the corresponding line strength in the HITRAN database and the reference isotopic abundances. Consequently, the mixing ratios in Eq. (3) are effectively normalized to the total concentration of all isotopologues at natural abundance.

Expressing isotopologue abundances as mixing ratios facilitates the calculation of the δ values (cf., Griffith et al., 2012; Hare et al., 2022):

$$\delta^{17}\text{O}_{\text{meas}} = \frac{\chi'_{627,\text{meas}}}{\chi'_{626,\text{meas}}} - 1 \quad (4)$$

The scale of these measured δ values is based on the natural isotopologue abundances used in HITRAN and need to be corrected for instrumental drift. This is done similarly as in isotope ratio mass spectrometry, by repeated alternating measurements of sample ("smp") and a working gas ("wg"), and reporting δ values relative to the working gas (McKinney et al., 1950):

$$\delta^{17}\text{O}_{\text{meas}}^{\text{smp/wg}} = \frac{\delta^{17}\text{O}_{\text{meas}}^{\text{smp}} + 1}{\delta^{17}\text{O}_{\text{meas}}^{\text{wg}} + 1} - 1 \quad (5)$$

As in isotope-ratio mass spectrometry, instrumental drift is mitigated by bracketing each sample analysis with measurements of a working gas. This approach relies on the assumption that changes in analytical conditions affect both the sample and the working gas equally, and that sample and working gas have similar molecular composition (i.e. they are matrix-matched).

3 Analytical setups

University of Göttingen and the University of Cape Town are both equipped with TILDAS instruments from Aerodyne Re-

search Inc. (Billerica, MA, USA), each coupled with custom-built inlet systems. The design and operation of these systems are described in detail by Bajnai et al. (2023) and Hare et al. (2022). In both laboratories, a single replicate measurement consists of multiple sample cycles bracketed by measurements of a working gas (Eq. 5). However, differences in the inlet systems result in slightly differing analytical procedures.

In TILDAS, mixtures of CO_2 and a collision gas (e.g., CO_2 -free air or pure N_2) are used to create optimal spectral line shapes through collisional broadening at pressures between around 30 Torr and 40 Torr (Fig. 1). Matching the CO_2 concentration of the sample to that of the working gas, typically within $1 \mu\text{mol mol}^{-1}$ can be challenging. A key distinction between the setups at Göttingen and Cape Town lies in how the mismatch in CO_2 concentrations between the sample and working gas are handled. At Göttingen, the χ'_{626} of sample and working gas are kept within $\pm 1 \mu\text{mol mol}^{-1}$ of each other within a replicate (Fig. 2a), and subsequent replicate analyses are also kept within $\pm 1 \mu\text{mol mol}^{-1}$. This is achieved by mixing pure CO_2 analytes, for both reference and sample, with a collision gas to a predefined target prior to each respective measurement cycle. In contrast, at Cape Town, the reference gas is pre-mixed and taken from a 50 L high pressure cylinder of $421 \mu\text{mol mol}^{-1}$ CO_2 in Nitrogen 5.0, resulting in identical χ'_{626} values of the working gas across replicate analyses within $0.1 \mu\text{mol mol}^{-1}$ (1σ). The χ'_{626} of the sample, however, varies from sample to sample, depending on the amount of sample gas available for analysis (Fig. 2b).

Another difference between the two laboratories lies in the temperature control of the TILDAS. The optical cell and some electronic components of the Aerodyne TILDAS instruments are thermally stabilized by a recirculating liquid chiller. To prevent large and rapid room temperature fluctuations that the chiller cannot compensate for, the Göttingen instrument is housed in an insulated box with PID temperature control, maintaining the ambient temperature stable within ± 0.01 K. In Cape Town, the instrument is not custom-insulated but is housed in a laboratory with an exceptionally stable temperature, varying by only ± 0.1 K over the course of a one-hour measurement.

4 Dependence of the measured $\Delta^{17}\text{O}$ values on the analytical conditions

4.1 Concentration dependence due to scale-offset

The effect of mismatched CO_2 concentrations between sample and working gas have been shown to substantially affect the measured $\Delta^{17}\text{O}$ values and requires correction (Bajnai et al., 2023; Hare et al., 2022, 2025; Steur et al., 2021, 2024). According to Eqs. (2) and (3), the measured χ' values are a function of the area under the corresponding spec-

tral peaks [e.g., $\chi'_{626} \propto A(626)$]. The size of the absorption peaks varies with $p\text{CO}_2$. Under perfectly ideal instrumental conditions, the observed ratio of the peak areas would remain constant even with a change in $p\text{CO}_2$ ($\delta^{17}\text{O}_{\text{meas}} \propto a \times A(627)/A(626) + b$, with $a = 0$ and $b = 0$). However, under real world conditions changes in peak areas are not perfectly retrieved introducing concentration dependence of the ratios of the peak areas, which leads to a concentration dependence of the measured δ values ($\delta^{17}\text{O}_{\text{meas}} \propto a \times A(627)/A(626) + b$, with $a \neq 0$ and $b \neq 0$). The underlying causes of this effect are related to systematic errors in the measurement of mole fractions and likely include nonlinearities related to spectral retrievals and the infrared detector response.

Deviations in the measured χ' values from the “true” mole fractions of the analyte gas can be expressed as (cf., Griffith et al., 2012; Hare et al., 2022):

$$\chi'_{627,\text{meas}} = a_{627} \times \chi'_{627,\text{true}} + b_{627} \quad (6)$$

where a_{627} and b_{627} are scaling factors which relate the measured isotopologue mole fractions to the “true” isotopologue mole fractions of the analyte gas, either sample or working gas. Similar equations can be written for χ'_{626} and χ'_{628} . Using Eq. (6), we can describe a more accurate form of Eq. (4), adjusted for the offsets:

$$\delta^{17}\text{O}_{\text{meas}} = \frac{a_{627} \times \chi'_{627,\text{true}} + b_{627}}{a_{626} \times \chi'_{626,\text{true}} + b_{626}} - 1 \quad (7)$$

From Eqs. (6) and (7), the “true” δ values of sample or working gas can be expressed as follows (see Eq. 4 in Hare et al., 2022):

$$\begin{aligned} \delta^{17}\text{O}_{\text{true}} = & \frac{\chi'_{626,\text{meas}}}{\frac{a_{627}}{a_{626}} (\chi'_{626,\text{meas}} - b_{626})} \\ & \times \left(\delta^{17}\text{O}_{\text{meas}} + \frac{\frac{a_{627}}{a_{626}} \times b_{626} - b_{627}}{\chi'_{626,\text{meas}}} - \frac{a_{627}}{a_{626}} + 1 \right) \end{aligned} \quad (8)$$

Equation (8) implies that all δ values, and consequently $\Delta^{17}\text{O}$ values, measured by spectroscopy depend on the measured mole fraction of the most abundant CO_2 isotopologue, χ'_{626} . Therefore, variations in χ'_{626} across successive measurement cycles within a replicate or across individual replicate analyses affect measurement repeatability.

To correct for $p\text{CO}_2$ mismatch, the “true”, scale-offset-corrected δ values need to be determined. In practical terms, this means that the constants a and b in Eq. (7) need to be known. Instead of correcting the δ values, it is convenient to perform the correction on the measured $\Delta^{17}\text{O}$ values directly. By combining Eqs. (1), (5), (7), and (8) we can derive a correction scheme for “true” $\Delta^{17}\text{O}_{\text{smp/wg}}$ values relative to the working gas used for bracketing (see Appendix A):

$$\Delta^{17}\text{O}_{\text{true}}^{\text{smp/wg}} \simeq \Delta^{17}\text{O}_{\text{meas}}^{\text{smp/wg}} - m \times \left(\chi_{626,\text{meas}}^{\text{smp}} - \chi_{626,\text{meas}}^{\text{wg}} \right) \quad (9)$$

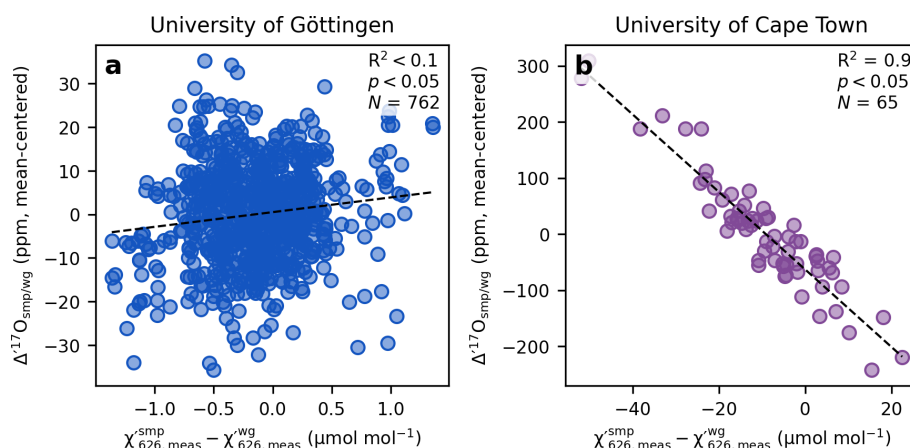


Figure 2. The effect of $p\text{CO}_2$ mismatch between sample and working gas on the measured $\Delta^{17}\text{O}$ values.

To determine the correction slope m empirically, we carried out a series of experiments. At Cape Town, 10 mg of IAEA-603 was reacted in 100 % phosphoric acid at 70 °C and then diluted with varying amounts of N_2 . This resulted in χ_{626}^{smp} ranging from 360 $\mu\text{mol mol}^{-1}$ to 435 $\mu\text{mol mol}^{-1}$, while the χ_{626}^{wg} was held constant at 421 $\mu\text{mol mol}^{-1}$. A similar experiment was done by diluting the working reference gas. A fit to this data – measured within the same analytical session (10–12 March 2025) – yields a slope of $m = -6$ ppm per $\mu\text{mol mol}^{-1}$ mismatch ($\chi_{626}^{\text{smp}} - \chi_{626}^{\text{wg}}$), both for IAEA-603 and for the zero-enrichment measurements (Fig. 3). A second set of experiments conducted during a separate analytical session (21 November–10 December 2024) yielded a slightly different slope for IAEA-603 of $m = -7$ ppm per $\mu\text{mol mol}^{-1}$ mismatch (Fig. 3).

At Göttingen, we used the internal light CO_2 and heavy CO_2 reference gases for similar dilution experiments. For the 2023 analytical session (15–19 March 2023), both analytes yielded a slope of $m = 6$ ppm per $\mu\text{mol mol}^{-1}$ mismatch. After the laser was replaced in 2025, the same dilution experiments (30 June–14 July 2025) produced a slope of $m = 15$ ppm per $\mu\text{mol mol}^{-1}$ mismatch (Fig. 3).

The observation that gases with different isotope compositions ($\Delta\delta^{18}\text{O}$ relative to the working gas ranging from -28‰ to $+48\text{‰}$) yield identical correction slopes m within the same analytical sessions suggests that m is largely independent of the isotopic composition of the sample analyte.

The opposite sign of m observed in Göttingen and Cape Town (Fig. 3) can be explained by differences in the sign of the expression a_{626}/b_{626} . This, together with the variation in the correction slopes across the analytical sessions, indicates that m , that is ultimately a_{626} and b_{626} , are instrument dependent and may vary in response to changing instrumental parameters, such as the laser tuning rate, the instrument purging rate, etc.

We apply the correction described by Eq. (9) to address the mismatch between the χ_{626}' of the sample and the working

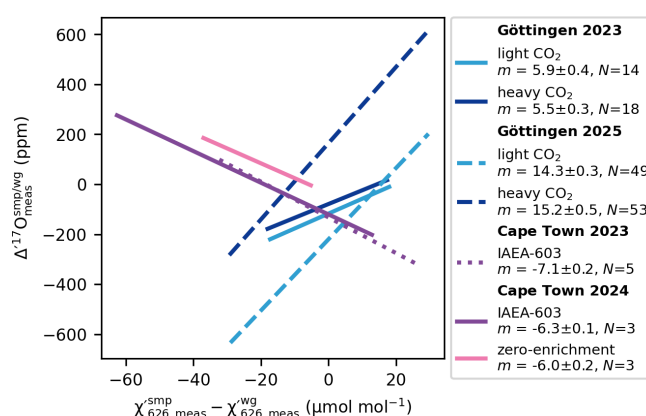


Figure 3. Concentration dependence of $\Delta^{17}\text{O}$. Linear trendlines showing the relationship between mismatches in the measured χ_{626}' mixing ratios of sample and working gas and corresponding $\Delta^{17}\text{O}$ values. The figure also highlights that the slopes vary not only between instruments but also among analytical sessions of the same instrument. The corresponding concentration dependence of the measured $\delta^{18}\text{O}$ values is smaller than $\pm 0.03\text{‰}$ per $\mu\text{mol mol}^{-1}$ mismatch in χ_{626}' .

gas in the Cape Town dataset. Before correction, the external 1 standard deviation of the Cape Town NBS-18 and IAEA-603 $\Delta^{17}\text{O}$ values is 110 and 98 ppm, respectively, over the entire measurement period (Fig. 4a). After applying apply a scale-offset correction to the entire dataset, these values improve significantly to 32 and 38 ppm (Fig. 4b). Applying a session-specific correction (i.e. with different m fitted to each analytical session), there is further improvement to 20 ppm for both NBS-18 and IAEA-603 (see details in Hare et al., 2025).

The correction scheme outlined above is only valid for small differences in χ_{626}' between sample and working gas. We estimate a $\pm 1\%$ error in the linear correction slope m , if χ_{626}^{smp} is within approximately 14 % of χ_{626}^{wg} , i.e. ± 58 ppm

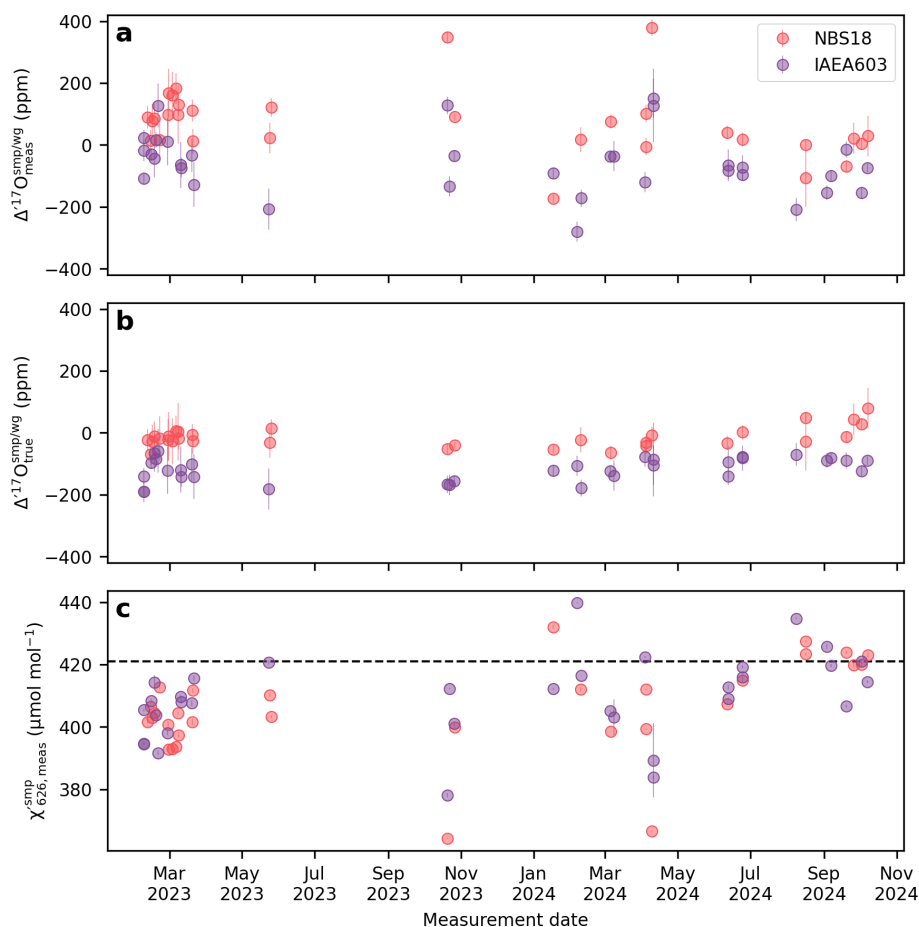


Figure 4. The effect of scale-offset correction of the Cape Town $\Delta^{17}\text{O}$ data. (a) Measured $\Delta^{17}\text{O}$ values, (b) “true” $\Delta^{17}\text{O}$ values after scale-offset correction, (c) Average χ'_{626} values of the sample gas within a replicate analysis. For the Cape Town setup the χ'_{626} value of the working gas is a constant $421 \mu\text{mol mol}^{-1}$, and within a replicate measurement the mismatch between subsequent χ'_{626} values stay within $\pm 1 \mu\text{mol mol}^{-1}$.

for a typical χ'^{wg}_{626} value of 420 ppm (see Appendix A). That is, if $m = 6 \text{ ppm per } \mu\text{mol mol}^{-1}$ mismatch, as observed at both laboratories, the error arising from the correction while correcting for a 58 ppm mismatch is about 3 ppm.

We briefly note that other techniques, e.g., CRDS, use pure CO_2 gas as analyte instead of gas mixtures (cf., Chaillot et al., 2025). According to Eq. (9), pure CO_2 implies that $\chi'^{\text{smp}}_{626} - \chi'^{\text{wg}}_{626} \simeq 0$, eliminating the need for a scale-offset correction.

4.2 Temperature dependence

Temperature variability could affect a laser spectroscopy system in multiple ways. Because the line shape function is empirically derived from the absorption spectra, the calculated concentrations are inherently subject to some inaccuracy (Eq. 2). The empirical fit may not fully capture subtle variations in thermal or collisional peak broadening, resulting in residual temperature and pressure dependencies in

the measured concentrations (Becker et al., 1992; Bergamaschi et al., 1994; Nelson et al., 2008). These biases can affect each spectral peak, and therefore each measured mixing ratio, differently, leading to uncorrelated changes in the measured δ values, and, ultimately, variations in the $\Delta^{17}\text{O}$ values.

The temperature sensitivity of the electronics components could also affect the measured isotope ratios. Temperature variations could affect the sensors, such as the infrared detector, or pressure sensor. The output power and wavelength of a laser are affected by temperature in two main ways: through the temperature of the laser itself and through the temperature sensitivity of the current driver, which influences the laser current (e.g., Hare et al., 2022; Nelson et al., 2008; Wavelength Electronics, 2020).

Figure 5 shows a 10 h measurement of a CO_2 -in-air mixture conducted at the University of Göttingen using TILDAS (cf. Fig. 3 in Bajnai et al., 2023). This uninsulated prototype setup was placed in an air-conditioned laboratory without a

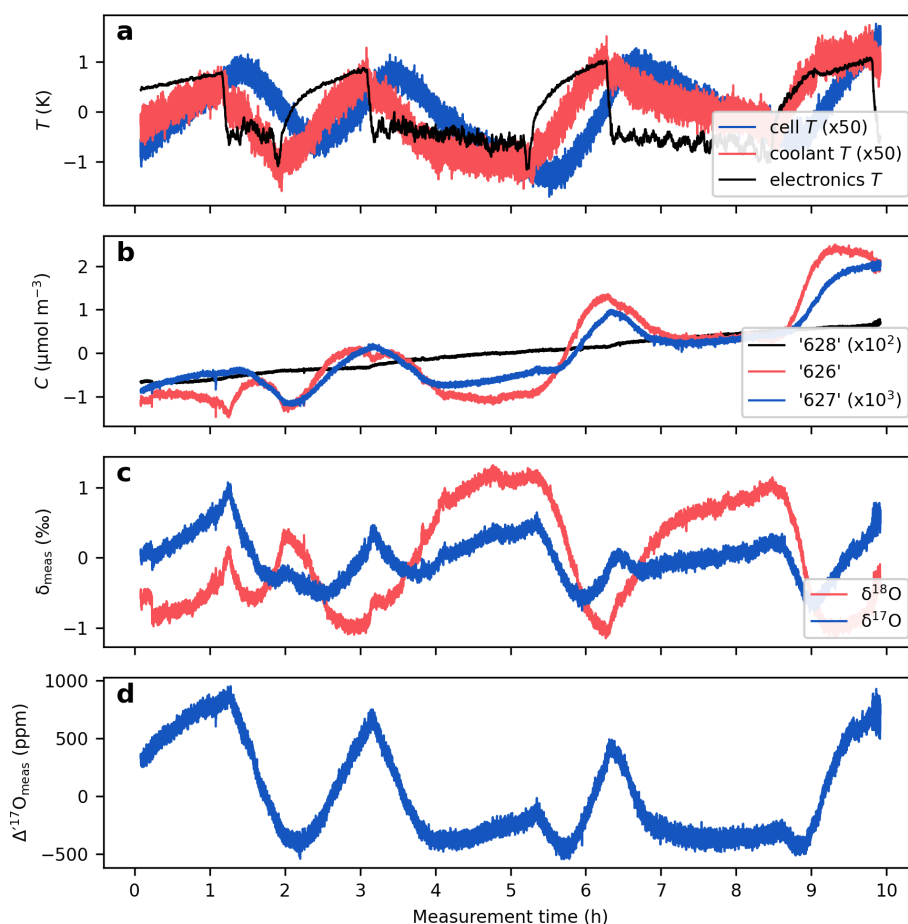


Figure 5. Temperature effects on the measured isotope ratios. The figure presents a continuous measurement of a CO_2 -in-air mixture at $420\ \mu\text{mol mol}^{-1}$. (a) Instrumental temperatures. Coolant temperature refers to the temperature of the circulating liquid entering the instrument. Electronics temperature represents the temperature measured adjacent to the electronics boards and the laser current driver. Note the approximately 20 min lag between the cell temperature and the electronics and coolant temperatures, which result from the thermal inertia of the metal cell. (b) Isotopologue concentrations calculated from mixing ratios, cell temperature and cell pressure (Eq. 3). (c) δ values; (d) $\Delta^{17}\text{O}$ values. All data are mean centered to highlight relative variations.

strict temperature control. Variations in room temperature are clearly reflected in both the electronics (by 2 K) and coolant temperatures (by 0.07 K). The cell temperature also closely tracks the fluctuations in the room temperature, albeit with a ca. 20 min delay and a reduced amplitude (by 0.07 K) due to the large metal mass of the cell and its active temperature control.

The temperature variations are broadly reflected in the measured concentrations of the “626”, “627”, and “628” isotopologues. However, these changes are not identically mirrored across the three isotopologue concentrations (Fig. 5b), leading to uncorrelated variations in the δ values (Fig. 5c) and resulting in a drift of about 1500 ppm in the measured $\Delta^{17}\text{O}$ values (Fig. 5d).

The alignment of the isotope ratio variations with the electronics temperature, rather than with the cell temperature, suggests that the temperature sensitivity of the $\Delta^{17}\text{O}$ measurements, in this case, is primarily linked to the tempera-

ture sensitivity of the electronic components rather than to the empirical fitting of the line shape function.

4.3 Gas purity

A major advantage of optical isotope ratio measurement techniques over mass spectrometry is that they are inherently free from isobaric interferences. However, optical measurements can still be affected by contaminants, particularly gases that exhibit overlapping absorption features or contribute to peak broadening.

In the spectral window used for triple oxygen isotope analyses of CO_2 , the three relevant CO_2 isotopologues produce distinct absorption peaks (Fig. 1), with no overlapping signals from water or other common contaminant gases such as N_2O , NO_2 , CO , or SO_2 (cf., Gordon et al., 2022). For completeness, we note that this advantage does not extend to Δ_{47} clumped isotope analyses, where N_2O exhibit peaks within

the relevant spectral window (Yanay et al., 2025). In such cases, a robust sample purification is required to remove interfering species.

The absence of direct spectral overlap does not imply that analyte purity is irrelevant. Variations in the gas composition – particularly the presence of water vapor – can lead to peak broadening effects, as well as isotopic exchange between CO_2 and water. Corresponding changes in the measured molar concentrations, in turn, contribute to variability in isotope ratios across replicate analyses. This effect has been well documented in atmospheric CO_2 monitoring studies (e.g., Paul et al., 2020; Tuzson et al., 2008), and may also be relevant for analyses of CO_2 produced by the acid digestion of carbonates. Although the water content of the released CO_2 analyte is typically low, it is not negligible and may vary depending on acid temperature and density (cf. Wacker et al., 2013).

An additional source of gas-purity-related error arises when the gas matrices of the sample and the working gas differ. For example, the spectroscopic fitting parameters used by the Aerodyne Research Inc. TDLWintel software are based on HITRAN data, which assume peak broadening due to collisions in a CO_2 -free air matrix. If the actual matrix deviates substantially from this assumption, spectral fits may degrade. This was observed by Bajnai et al. (2023), who noted to encounter fitting issues when using argon as a bathing gas without adjusting the fit parameters.

Changes in the gas matrix can also influence the scaling factors a and b in Eqs. (6)–(9). Gas matrix effects may become a significant source of uncertainty in air monitoring studies, particularly when the gas matrix of the working gas (e.g., CO_2 -in- N_2) differs from that of the sample (CO_2 -in-air with variable argon concentrations), since the resulting scale-offsets can differ and be difficult to correct. Matching the matrices of the working gas to that of the sample analyte as closely as possible helps prevent detrimental effects arising from variable scale-offsets.

A similar gas-matrix-related issue can arise when the matrix of the reference gas used for standardization differs from that of the sample gas. For example, consider a pre-mixed CO_2 -in- N_2 reference gas used to correct measurements of CO_2 -in-air. In such cases, even if the analytical conditions remain completely stable, gas matrix effects may be carried into the correction, ultimately biasing the data.

5 Internal error and long-term drift in the Göttingen and the Cape Town datasets

5.1 Internal error

Variations in the analytical conditions can introduce instrumental drift. Instrumental drift is mitigated by bracketing each sample analysis with measurements of a working gas (McKinney et al., 1950). This approach relies on the assumption

that changes in analytical conditions affect both the sample and the working gas equally. It also assumes that the changeover between cycles is fast enough for variations in analytical parameters to be approximated by a linear trend between two working gas cycles. The internal error of a single replicate analysis, i.e. the repeatability of approximately 10 sample cycles within a bracketing measurement, primarily depends on how constant the measurement conditions remain between cycles.

We assess the variability and stability of key analytical parameters – cell temperature, electronics temperature, cell pressure, and the mixing ratio of the most abundant CO_2 isotopologue (χ'_{626}) – using four indicators. First, we determined the mean value of each parameter separately for sample and reference cycles within each replicate. Second, we used the range of these parameter means across replicates as a measure of long-term drift in analytical conditions. Third, to quantify systematic deviations between sample and reference measurements, we calculated, for each sample cycle, the difference between its mean value and the mean of the reference cycles immediately before and after. The average of these differences (sample minus reference) is referred to as the mismatch parameter. A mismatch may not decrease the repeatability if, for example it is constant over the cycles of a replicate analysis. However, variations in mismatch values, both within a single replicate and across replicates, affects measurement repeatability. To assess the stability of the analytical conditions within a single replicate, we calculated the standard deviation of the mismatch values within a replicate.

Figure 6 shows the relationship between the stability of the mismatch in the mixing ratio of the most abundant CO_2 isotopologue (χ'_{626}), cell pressure, cell temperature, electronics temperature, and the internal error of individual replicate measurements (68 % confidence interval of the approximately 10 sample cycles bracketed by working gas analyses). At the University of Göttingen, the χ'_{626} mismatch across the cycles of a single replicate remains stable within $\pm 1 \mu\text{mol mol}^{-1}$ (Fig. 6a). The cell pressure mismatch stays stable within $\pm 0.8 \text{ Pa}$ (approximately $\pm 6 \text{ mTorr}$; Fig. 6c), and the cell temperature mismatch within $\pm 1 \text{ mK}$ (Fig. 6e). The electronics temperature stays stable within $\pm 0.10 \text{ K}$ (Fig. 6g). None of these parameters show a statistically significant correlation with the observed internal error, suggesting that these variables are kept stable enough during a replicate measurement to avoid influencing the results.

At the University of Cape Town, the across the cycles of a single replicate the mismatch in χ'_{626} , cell pressure, cell temperature and electronics temperature remain stable better than $\pm 12 \mu\text{mol mol}^{-1}$ (Fig. 6b), 34.7 Pa (approximately $\pm 260 \text{ mTorr}$; Fig. 6d), $\pm 3 \text{ mK}$ (Fig. 6f), and $\pm 0.14 \text{ K}$ (Fig. 6h), respectively. Weak correlations (up to $R^2 = 0.2$) between the mismatch stabilities and the internal error appear to be driven by outlier points. Overall, the lack of meaningful correlation between the stability of the mismatch parameters

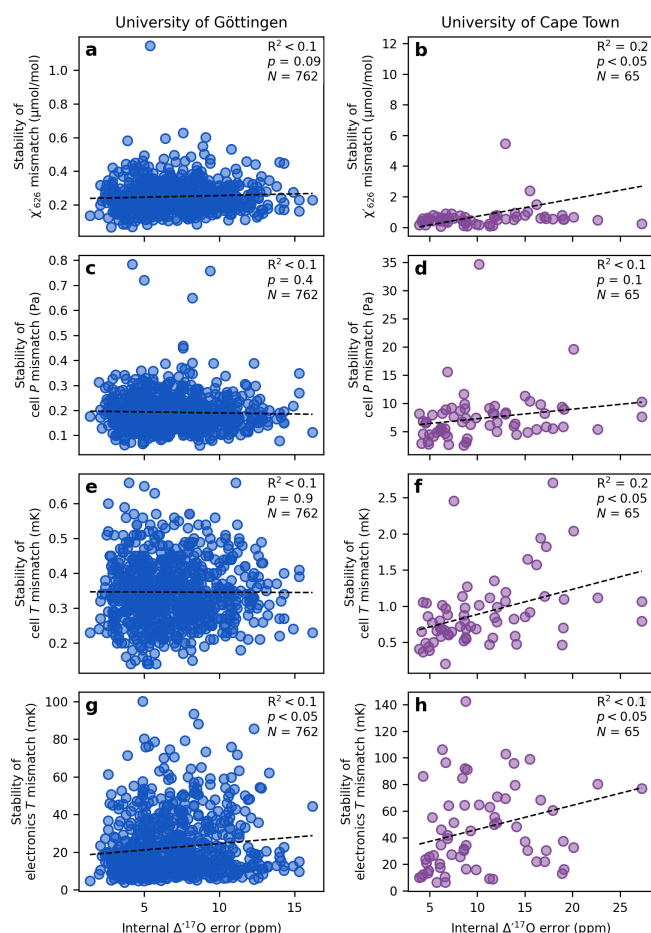


Figure 6. Effect of analytical variability on the internal error of a replicate $\Delta^{17}\text{O}$ measurement. The standard deviation of the mismatch parameters serves as a measure of variability in analytical conditions across cycles of individual replicate analyses. The internal error is reported as the 68 % confidence interval of the calculated $\Delta^{17}\text{O}$ values from approximately 10 sample cycles. The black dashed line and the corresponding correlation coefficients indicate the relationship between parameter stability and internal repeatability. In both laboratory setups, the analytical conditions are generally stable enough that they do not have a detectable effect on the internal reproducibility of the measurements.

and the internal error of the $\Delta^{17}\text{O}$ measurements suggests that the stability of the analytical parameters is sufficiently stable in both laboratories to prevent any systematic effect on internal error.

5.2 Long-term drift in the analytical parameters

The external repeatability – i.e. the consistency of results across multiple independent replicate analyses – primarily depends on the stability of measurement conditions. Rather than focusing on the drift of individual reference materials, we examine the difference in measured $\Delta^{17}\text{O}$ values between two reference materials. We refer to this difference as

scale compression, adopting terminology similar to that used in mass spectrometry. This approach offers two key advantages: it simplifies the identification of trends in the data and, more importantly, directly relates to the most common isotope standardization strategy, which relies on two-point calibration using reference materials measured within a defined period. In this context, drift in the scale compression within a measurement period directly affects the accuracy of the final $\Delta^{17}\text{O}$ values.

Figures 7 and 8 illustrate the long-term drift in the analytical parameters and the measured $\Delta^{17}\text{O}$ values of two reference materials and the corresponding scale compression in the Göttingen and Cape Town datasets. A LOESS fit is used to approximate temporal trends in each variable. To assess which variables most strongly influence the drift in the scale compression, we performed a multiple linear regression analysis, relating various combinations of analytical parameters to the scale compression (Fig. 9). Note that in the case of the Cape Town dataset χ'_{626} is not considered, as $\Delta^{17}\text{O}$ values have already been corrected to a constant χ'_{626} value of $421 \mu\text{mol mol}^{-1}$ (cf., Fig. 4). The R^2 values of the multiple linear regression analysis indicate that in Göttingen, variations in electronics temperature is the primary driver of the scale compression drift, while cell temperature, cell pressure, and χ'_{626} exert smaller yet still considerable effects (Fig. 9a). Considering only variations in χ'_{626} in the regression model does not explain the long-term drift in the scale compression. This result is consistent with expectations: given the χ'_{626} sensitivity of $\Delta^{17}\text{O}$ of 6 ppm per $\mu\text{mol mol}^{-1}$, the observed ca. $2.5 \mu\text{mol mol}^{-1}$ variation in χ'_{626} would lead to a maximum drift of about 15 ppm, that is comparable to the 1σ repeatability of measurements under ideal conditions. By contrast, the observed overall ~ 60 Pa variation in cell pressure and ~ 0.1 K variation in cell temperature produce more substantial effects on the scale compression. Variations in cell as well as electronics temperature and cell pressure are the dominant contributors to the scale compression drift in Cape Town (Fig. 9b). Figures 7f and 8e illustrate the combined parameter drift resulting from the analytical parameters combinations yielding the highest R^2 values in Fig. 9.

Figure 7a illustrates that the magnitude and direction of the drift in the $\Delta^{17}\text{O}$ values of the two standards used in the Göttingen laboratory are not identical. The $\delta^{18}\text{O}$ values of these two standards differ by ca. 80 ‰. As discussed above and shown in Fig. 5, the mixing ratios of the three CO_2 isotopologues respond in an uncorrelated fashion to variations in analytical conditions related to systematic errors in the measurement of mole fractions. It follows that the magnitude of the drift in the measured δ and $\Delta^{17}\text{O}$ values in response to changing analytical conditions, particularly temperature, depends on the isotopic composition of the analyte.

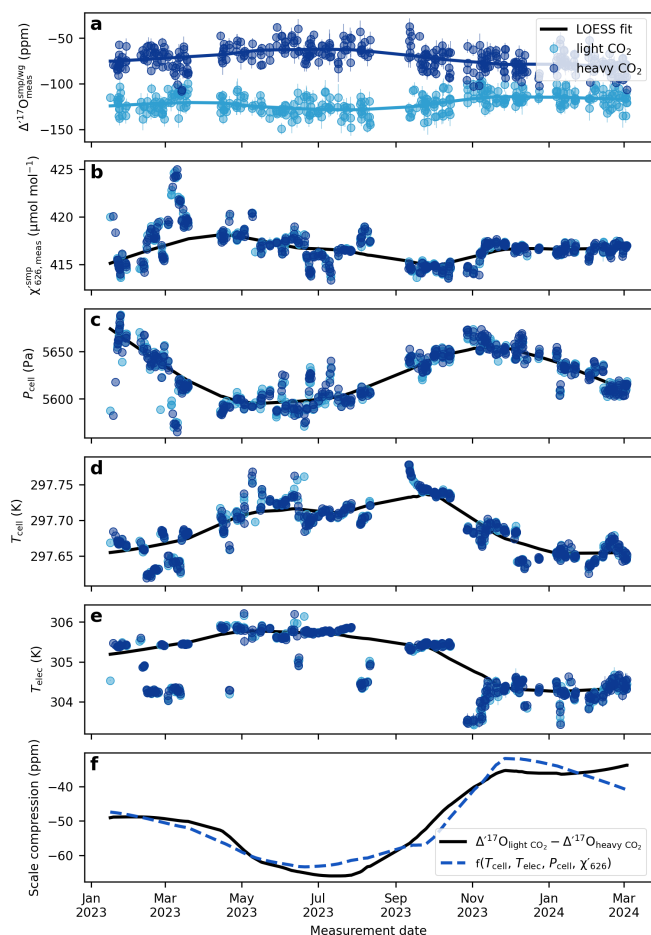


Figure 7. The drift of the compression of the Göttingen setup. (a) $\Delta^{17}\text{O}$ values for the two internal reference gases, light CO_2 and heavy CO_2 . (b) average χ'_{626} of the sample cycles within a replicate. For the Göttingen setup the χ'_{626} of the reference cycles are within $1 \mu\text{mol mol}^{-1}$ of the samples. (c) cell pressure, (d) cell temperature, (e) electronics temperature, (f) scale compression; defined as the difference between the $\Delta^{17}\text{O}$ values of the light CO_2 and heavy CO_2 . The solid lines depict LOESS fits to the data (smoothing: 0.4). The dashed blue line shows the multivariate linear regression model from the LOESS fits of the cell temperature, electronics temperature, cell pressure, and χ'_{626} .

6 Summary and recommendations

Variations in analytical conditions – such as cell temperature, electronics temperature, cell pressure, and the $p\text{CO}_2$ of the analytes – can influence the measured $\Delta^{17}\text{O}$ values. For instance, the sensitivity of $\Delta^{17}\text{O}$ to changes in analyte $p\text{CO}_2$ is on the order of $10 \text{ ppm per } \mu\text{mol mol}^{-1}$, depending on the instrumentation. This source of bias is particularly relevant for atmospheric monitoring studies, as atmospheric CO_2 concentrations can fluctuate by more than $100 \mu\text{mol mol}^{-1}$ over the course of a day, potentially causing a variability of

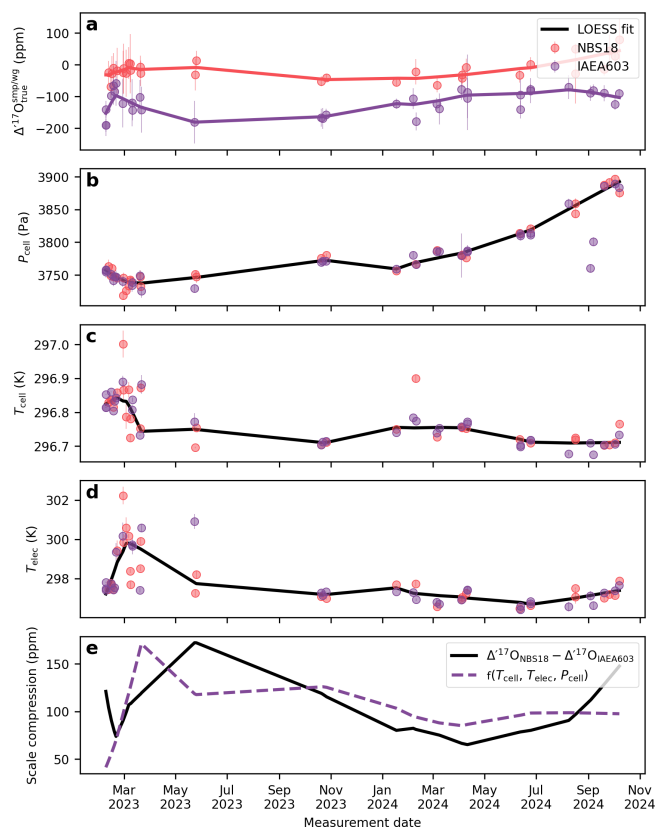


Figure 8. The drift of the compression of the Cape Town setup. (a) $\Delta^{17}\text{O}$ values for two commonly used reference materials, NBS-18 and IAEA-603 (b) cell pressure, (c) cell temperature, (d) electronics temperature, (e) scale compression; defined as the difference between the $\Delta^{17}\text{O}$ values of NBS-18 and IAEA-603. The dashed red line shows the multivariate linear regression model from the LOESS fits of the cell temperature, electronics temperature, and cell pressure.

1000 ppm in the measured $\Delta^{17}\text{O}$ values that needs to be corrected.

In addition to $p\text{CO}_2$, instability in cell temperature, electronics temperature, and cell pressure can compromise measurement repeatability (internal error). Data from the University of Göttingen and the University of Cape Town show that maintaining cell temperature and pressure stability within $\pm 1 \text{ mK}$ and $\pm 10 \text{ Pa}$, respectively, across the cycles of a replicate measurement is sufficient to avoid any resolvable impact on the internal error beyond $\pm 10 \text{ ppm}$ on $\Delta^{17}\text{O}$. The temperature sensitivity of the instrumental setup depends on the relative speed of the changeover measurements to the speed of the variation in the ambient temperature. To minimize the influence of ambient temperature fluctuations, TILDAS systems are typically placed in thermally insulated enclosures or operated in climate-controlled laboratories.

Long-term drift in the analytical conditions – such as a gradual changes in electronics temperature, cell temperature and pressure, and mixing ratios over the course several weeks

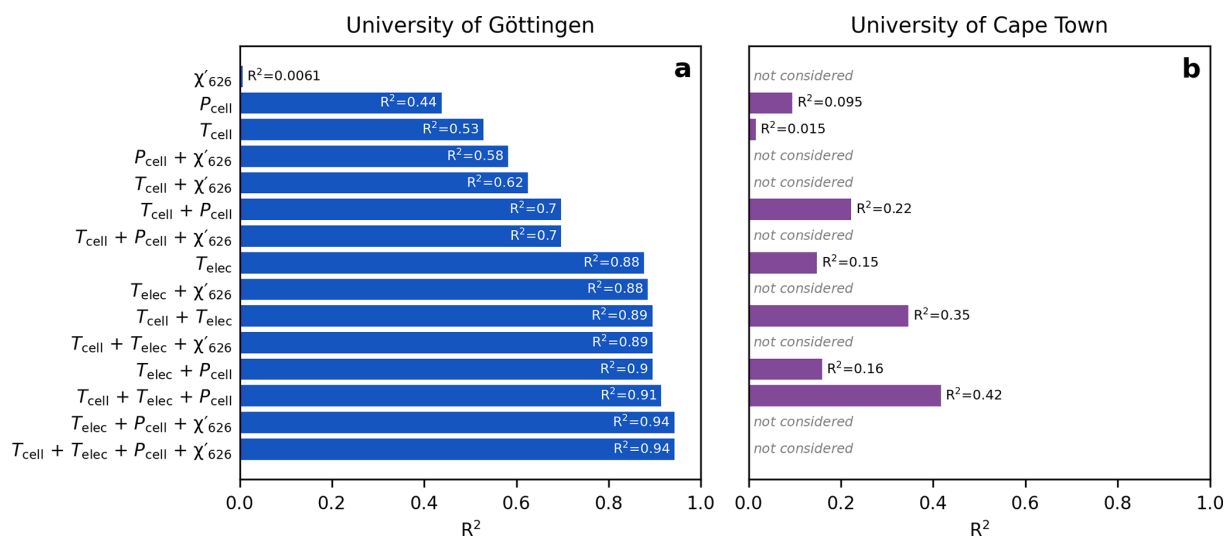


Figure 9. Correlation coefficients of multiple linear regression models between scale compression in $\Delta^{17}\text{O}$ and various combinations of cell and electronics temperature, cell pressure, and χ'_{626} . (a) University of Göttingen, (b) University of Cape Town. In this latter case, the models use only cell and electronics temperatures and cell pressure, as the $\Delta^{17}\text{O}$ values were already corrected for scale-offset and normalized to a χ'_{626} value of $421 \mu\text{mol mol}^{-1}$. The multiple linear regression models yielding the highest correlation coefficients are plotted on Figs. 7f and 8e. We speculate that the comparatively weaker correlation in the Cape Town dataset is due to the fewer data points used to compute the LOESS fits. All p values < 0.05 .

– can introduce drift in the measured $\Delta^{17}\text{O}$ values. As the magnitude of the drift in the measured $\Delta^{17}\text{O}$ values seemingly depend on the isotope composition of the analyte, the suitability of a polynomial fit based on reference materials for correcting drift in samples needs to be confirmed. If left unrecognized, these drifts may be misinterpreted as genuine seasonal variations in $\Delta^{17}\text{O}$ data. Continuous monitoring and reporting of the analytical conditions, along with periodical recalibration of temperature and pressure sensors, are therefore essential to ensure data integrity over extended timescales.

Finally, we demonstrated that changes in analytical conditions can impact the instrument's scaling, that is, the measured difference in $\Delta^{17}\text{O}$ between two reference materials used for data correction. To ensure accurate data correction, subsequent measurements should be grouped into measurements periods under which variations in the analytical conditions do not introduce a resolvable effect on the measured oxygen isotope values. The duration of the measurement periods and the required number of reference measurements necessary for a precise correction depends on the specific analytical setup.

Appendix A: Correction for concentration dependence

The following text outlines the derivation of Eq. (9). Equation (8) describes the concentration dependence of the δ values of sample and working gas. Substituting a_{627}/a_{626} with A_{627} , and a_{628}/a_{626} with A_{628} , following the nomenclature

of Hare et al. (2022), yields:

$$\delta^{17}\text{O}_{\text{true}} = \frac{\chi'_{626,\text{meas}}}{A_{627}(\chi'_{626,\text{meas}} - b_{626})} \times \left(\delta^{17}\text{O}_{\text{meas}} + \frac{A_{627} \times b_{626} - b_{627}}{\chi'_{626,\text{meas}}} - A_{627} + 1 \right) \quad (\text{A1})$$

The fitted coefficients in Hare et al. (2022) provide indicative numerical values of $A_{627} = 0.674$, $A_{628} = 0.632$, $b_{626} = -168$, $b_{627} = -1974$, $b_{628} = -4782$, when χ'_{626} is expressed in nmol mol^{-1} .

Assuming that $|\chi'_{626}| \gg |b_{626}|$, $|b_{626}| \gg |A_i|$, and $|b_i| \approx |b_{626}|$, with $i = 627, 628$, we can approximate Eq. (A1) as:

$$\delta^{17}\text{O}_{\text{true}} \simeq \frac{\chi'_{626,\text{meas}}}{A_{627}(\chi'_{626,\text{meas}} - b_{626})} \delta^{17}\text{O}_{\text{meas}} \quad (\text{A2})$$

This approximation preserves the concentration dependence. Evaluating the prefactor with the fitted coefficients above, yields a multiplier of approximately 1.48. This multiplier will be different on each system, depending on the value of χ'_{626} , as well as b_{626} and A_{627} (or A_{628} for $\delta^{18}\text{O}$).

From Eqs. (1) and (5) we have:

$$\Delta^{17}\text{O}_{\text{true}}^{\text{smp/wg}} = \Delta^{17}\text{O}_{\text{true}}^{\text{smp}} - \Delta^{17}\text{O}_{\text{true}}^{\text{wg}} \quad (\text{A3})$$

Under the assumptions outlined above, we can approximate that $\ln(\delta^{17}\text{O}_{\text{true}} + 1) \approx \ln[\delta^{17}\text{O}_{\text{true}} + \chi'_{626}/A_{627}(\chi'_{626} - b_{626})]$. With Eqs. (1), (5), and (7), and a separate form of

Eq. (A2) for sample and working gas, Eq. (A3) can be evaluated as:

$$\Delta^{17}\text{O}_{\text{true}}^{\text{smp/wg}} = \Delta^{17}\text{O}_{\text{meas}}^{\text{smp/wg}} + (1 - \lambda_{\text{RL}}) \ln \left[\frac{\chi_{626,\text{meas}}^{\text{smp}} (\chi_{626,\text{meas}}^{\text{wg}} - b_{626})}{\chi_{626,\text{meas}}^{\text{wg}} (\chi_{626,\text{meas}}^{\text{smp}} - b_{626})} \right] \quad (\text{A4})$$

Under the assumption that $|\chi_{626}'| \gg |b_{626}|$, a Taylor-series expansion of Eq. (A4) yields the following hyperbolic correction equation, to first order:

$$\Delta^{17}\text{O}_{\text{smp/wg}}^{\text{true}} \simeq \Delta^{17}\text{O}_{\text{smp/wg}}^{\text{meas}} + (1 - \lambda_{\text{RL}}) b_{626} \left[\frac{1}{\chi_{626,\text{meas}}^{\text{smp}}} - \frac{1}{\chi_{626,\text{meas}}^{\text{wg}}} \right] \quad (\text{A5})$$

From here, it is convenient to linearize the hyperbola Eq. (A5) for large values (i.e. $420\,000\text{ nmol mol}^{-1}$) of χ_{626}^{wg} and small differences between χ_{626}^{wg} and χ_{626}^{smp} :

$$\Delta^{17}\text{O}_{\text{smp/wg}}^{\text{true}} \simeq \Delta^{17}\text{O}_{\text{smp/wg}}^{\text{meas}} - (1 - \lambda_{\text{RL}}) \frac{b_{626}}{(\chi_{626,\text{meas}}^{\text{wg}})^2} (\chi_{626,\text{meas}}^{\text{smp}} - \chi_{626,\text{meas}}^{\text{wg}}) \quad (\text{A6})$$

From Eq. (A6) we get Eq. (9), with the correction slope m as $(1 - \lambda_{\text{RL}}) \cdot b_{626} / (\chi_{626}^{\text{wg}})^2$,

The condition for a maximum 1 % error in the linear approximation of the hyperbola (Eq. A6) is $(\chi_{626}^{\text{smp}} - \chi_{626}^{\text{wg}}) / (2(\chi_{626}^{\text{wg}})^2) \leq 0.01$, which implies that $|\chi_{626}^{\text{smp}} - \chi_{626}^{\text{wg}}| \leq 0.14 \chi_{626}^{\text{wg}}$. In other words, the concentration of the sample should be within 14 % of the working gas, to avoid errors of greater than 1 % in the correction. For example, if m is 6 ppm per $\mu\text{mol mol}^{-1}$, then at a mismatch of $58\mu\text{mol mol}^{-1}$, there will be an absolute error in corrected, “true” $\Delta^{17}\text{O}_{\text{smp/wg}}$ of approximately 3 ppm due to a deviation in linearity.

Code and data availability. All data and codes used in this manuscript are deposited at GitHub (https://github.com/davidbajnai/TILDAS_drift, last access: 2 December 2025) and Zenodo (<https://doi.org/10.5281/zenodo.15742110>) (Bajnai and Hare, 2025). The supplementary files include Table S1 (long-term replicate-level measurement data from the University of Göttingen), Table S2 (long-term replicate-level measurement data from the University of Cape Town), Table S3 (concentration experiments from the University of Cape Town), and Table S4 (concentration experiments from the University of Göttingen). We also provided the MATLAB and Python files used to process TILDAS output data (.STC and .STR files).

Author contributions. DB: conceptualization, formal analyses, investigation methodology, writing – original draft, visualization; VJH: conceptualization, formal analyses, investigation methodology, writing – original draft.

Competing interests. The contact author has declared that neither of the authors has any competing interests.

Disclaimer. Publisher’s note: Copernicus Publications remains neutral with regard to jurisdictional claims made in the text, published maps, institutional affiliations, or any other geographical representation in this paper. While Copernicus Publications makes every effort to include appropriate place names, the final responsibility lies with the authors. Views expressed in the text are those of the authors and do not necessarily reflect the views of the publisher.

Acknowledgements. David Bajnai gratefully acknowledges Prof. Andreas Pack, head of the stable isotope laboratory at the University of Göttingen, for his generous support and for providing the infrastructure that made this research possible. He also thanks Dennis Kohl, Thierry Wasselin, and Tommaso Di Rocco for their technical assistance. Vincent Hare gratefully acknowledges the laboratory assistance of Drake Yarian and Anna Kudriavtseva at the University of Cape Town.

Financial support. This research has been supported by the Department of Science and Innovation, South Africa (Biogeochemistry Research Infrastructure Platform (BIOGRIP)).

This open-access publication was funded by the University of Göttingen.

Review statement. This paper was edited by Christof Janssen and reviewed by David Nelson and Mathieu Daéron.

References

- Adnew, G. A., Hofmann, M. E. G., Paul, D., Laskar, A., Surma, J., Albrecht, N., Pack, A., Schwieters, J., Koren, G., Peters, W., and Röckmann, T.: Determination of the triple oxygen and carbon isotopic composition of CO_2 from atomic ion fragments formed in the ion source of the 253 Ultra high-resolution isotope ratio mass spectrometer, *Rapid Commun. Mass Spectrom.*, 33, 1363–1380, <https://doi.org/10.1002/rcm.8478>, 2019.
- Adnew, G. A., Koren, G., Mehendale, N., Gromov, S., Krol, M., and Röckmann, T.: Triple oxygen isotope composition of CO_2 in the upper troposphere and stratosphere, *Atmos. Meas. Tech.*, 18, 2701–2719, <https://doi.org/10.5194/amt-18-2701-2025>, 2025.
- Affek, H. P., Barkan, E., Tal, Y., Steidle, S. D., Wendt, K. A., Spötl, C., Edwards, R. L., Fishman, E., and Dublyansky, Y.: $^{17}\text{O}_{\text{excess}}$ in Devils Hole calcite: an indicator of equilibrium fractionation and paleo moisture sources, *Earth Planet. Sci. Lett.*, 667, 119528, <https://doi.org/10.1016/j.epsl.2025.119528>, 2025.
- Bajnai, D. and Hare, V. J.: Supplementary material for: Sensitivity of tunable infrared laser spectroscopic measurements of $\Delta^{17}\text{O}$ in CO_2 to analytical conditions, Zenodo [data set], <https://doi.org/10.5281/zenodo.15742110>, 2025.

- Bajnai, D., Pack, A., Arduin Rode, F., Seefeld, M., Surma, J., and Di Rocco, T.: A dual inlet system for laser spectroscopy of triple oxygen isotopes in carbonate-derived and air CO_2 , *Geochim. Geophys. Geosyst.*, 24, e2023GC010976, <https://doi.org/10.1029/2023GC010976>, 2023.
- Bajnai, D., Klipsch, S., Davies, A. J., Raddatz, J., Gischler, E., Rüggeberg, A., Pack, A., and Herwartz, D.: Correcting for vital effects in coral carbonate using triple oxygen isotopes, *Geochim. Persp. Lett.*, 31, 38–43, <https://doi.org/10.7185/geochemlet.2430>, 2024.
- Barkan, E. and Luz, B.: High-precision measurements of $^{17}\text{O}/^{16}\text{O}$ and $^{18}\text{O}/^{16}\text{O}$ ratios in CO_2 , *Rapid Commun. Mass Spectrom.*, 26, 2733–2738, <https://doi.org/10.1002/rcm.6400>, 2012.
- Becker, J. F., Sauke, T. B., and Loewenstein, M.: Stable isotope analysis using tunable diode laser spectroscopy, *Appl. Opt.*, 31, 1921, <https://doi.org/10.1364/AO.31.001921>, 1992.
- Bergamaschi, P., Schupp, M., and Harris, G. W.: High-precision direct measurements of $^{13}\text{CH}_4/^{12}\text{CH}_4$ and $^{12}\text{CH}_3\text{D}/^{12}\text{CH}_4$ ratios in atmospheric methane sources by means of a long-path tunable diode laser absorption spectrometer, *Appl. Opt.*, 33, 7704, <https://doi.org/10.1364/AO.33.007704>, 1994.
- Boering, K. A., Jackson, T., Hoag, K. J., Cole, A. S., Perri, M. J., Thiemens, M., and Atlas, E.: Observations of the anomalous oxygen isotopic composition of carbon dioxide in the lower stratosphere and the flux of the anomaly to the troposphere, *Geophys. Res. Lett.*, 31, 2003GL018451, <https://doi.org/10.1029/2003GL018451>, 2004.
- Brand, W. A., Assonov, S. S., and Coplen, T. B.: Correction for the ^{17}O interference in $\delta(^{13}\text{C})$ measurements when analyzing CO_2 with stable isotope mass spectrometry (IUPAC Technical Report), *Pure Appl. Chem.*, 82, 1719–1733, <https://doi.org/10.1351/pac-rep-09-01-05>, 2010.
- Brenninkmeijer, C. A. M. and Röckmann, T.: A rapid method for the preparation of O_2 from CO_2 for mass spectrometric measurement of $^{17}\text{O}/^{16}\text{O}$ ratios, *Rapid Commun. Mass Spectrom.*, 12, 479–483, [https://doi.org/10.1002/\(SICI\)1097-0231\(19980430\)12:8<479::AID-RCM184>3.0.CO;2-R](https://doi.org/10.1002/(SICI)1097-0231(19980430)12:8<479::AID-RCM184>3.0.CO;2-R), 1998.
- Chaillot, J., Kassi, S., Clauzel, T., Pesnin, M., Casado, M., Landais, A., and Daëron, M.: Linking the oxygen-17 compositions of water and carbonate reference materials using infrared absorption spectroscopy of carbon dioxide, *Chem. Geol.*, 673, 122450, <https://doi.org/10.1016/j.chemgeo.2024.122450>, 2025.
- Craig, H.: Isotopic standards for carbon and oxygen and correction factors for mass-spectrometric analysis of carbon dioxide, *Geochim. Cosmochim. Acta*, 12, 133–149, [https://doi.org/10.1016/0016-7037\(57\)90024-8](https://doi.org/10.1016/0016-7037(57)90024-8), 1957.
- De Bièvre, P., Gallet, M., Holden, N. E., and Barnes, I. L.: Isotopic abundances and atomic weights of the elements, *J. Phys. Chem. Ref. Data*, 13, 809–891, <https://doi.org/10.1063/1.555720>, 1984.
- Gordon, I. E., Rothman, L. S., Hargreaves, R. J., Hashemi, R., Karlovets, E. V., Skinner, F. M., Conway, E. K., Hill, C., Kochanov, R. V., Tan, Y., Wcisło, P., Finenko, A. A., Nelson, K., Bernath, P. F., Birk, M., Boudon, V., Campargue, A., Chance, K. V., Coustenis, A., Drouin, B. J., Flaud, J.-M., Gamache, R. R., Hodges, J. T., Jacquemart, D., Mlawer, E. J., Nikitin, A. V., Perevalov, V. I., Rotger, M., Tennyson, J., Toon, G. C., Tran, H., Tyuterev, V. G., Adkins, E. M., Baker, A., Barbe, A., Canè, E., Császár, A. G., Dudaryonok, A., Egorov, O., Fleisher, A. J., Fleurbaey, H., Foltynowicz, A., Furtenbacher, T., Harrison, J. J., Hartmann, J.-M., Horneman, V.-M., Huang, X., Karman, T., Karns, J., Kassi, S., Kleiner, I., Kofman, V., Kwabia-Tchana, F., Lavrentieva, N. N., Lee, T. J., Long, D. A., Lukashevskaya, A. A., Lyulin, O. M., Makhnev, V. Yu., Matt, W., Massie, S. T., Melosso, M., Mikhailenko, S. N., Mondelain, D., Müller, H. S. P., Naumenko, O. V., Perrin, A., Polyansky, O. L., Raddaoui, E., Raston, P. L., Reed, Z. D., Rey, M., Richard, C., Tóbiás, R., Sadiek, I., Schwenke, D. W., Starikova, E., Sung, K., Tamassia, F., Tashkun, S. A., Vander Auwera, J., Vasilenko, I. A., Vigasin, A. A., Villanueva, G. L., Vispoel, B., Wagner, G., Yachmenev, A., and Yurchenko, S. N.: The HITRAN2020 molecular spectroscopic database, *J. Quant. Spectrosc. Radiat. Transf.*, 277, 107949, <https://doi.org/10.1016/j.jqsrt.2021.107949>, 2022.
- Griffith, D. W. T., Deutscher, N. M., Caldwell, C., Kettlewell, G., Rigenbach, M., and Hammer, S.: A Fourier transform infrared trace gas and isotope analyser for atmospheric applications, *Atmos. Meas. Tech.*, 5, 2481–2498, <https://doi.org/10.5194/amt-5-2481-2012>, 2012.
- Hare, V. J., Dyroff, C., Nelson, D. D., and Yarian, D. A.: High-precision triple oxygen isotope analysis of carbon dioxide by tunable infrared laser absorption spectroscopy, *Anal. Chem.*, 94, 16023–16032, <https://doi.org/10.1021/acs.analchem.2c03005>, 2022.
- Hare, V. J., Yarian, D. A., Faith, J. T., Harris, C., Lee-Thorp, J. A., Passey, B. H., Sokolowski, K. G., and Ségalen, L.: Triple oxygen isotopes in eggshell carbonate as a proxy of late Cenozoic CO_2 and primary productivity, *Geochim. Cosmochim. Acta*, 399, 48–63, <https://doi.org/10.1016/j.gca.2025.04.002>, 2025.
- Hoag, K. J., Still, C. J., Fung, I. Y., and Boering, K. A.: Triple oxygen isotope composition of tropospheric carbon dioxide as a tracer of terrestrial gross carbon fluxes, *Geophys. Res. Lett.*, 32, L02802, <https://doi.org/10.1029/2004GL021011>, 2005.
- Hofmann, M. E. and Pack, A.: Technique for high-precision analysis of triple oxygen isotope ratios in carbon dioxide, *Anal. Chem.*, 82, 4357–61, <https://doi.org/10.1021/ac902731m>, 2010.
- Hofmann, M. E. G., Horváth, B., Schneider, L., Peters, W., Schützenmeister, K., and Pack, A.: Atmospheric measurements of $\Delta^{17}\text{O}$ in CO_2 in Göttingen, Germany reveal a seasonal cycle driven by biospheric uptake, *Geochim. Cosmochim. Acta*, 199, 143–163, <https://doi.org/10.1016/j.gca.2016.11.019>, 2017.
- Horváth, B., Hofmann, M. E. G., and Pack, A.: On the triple oxygen isotope composition of carbon dioxide from some combustion processes, *Geochim. Cosmochim. Acta*, 95, 160–168, <https://doi.org/10.1016/j.gca.2012.07.021>, 2012.
- Kelson, J. R., Petersen, S. V., Niemi, N. A., Passey, B. H., and Curley, A. N.: Looking upstream with clumped and triple oxygen isotopes of estuarine oyster shells in the early Eocene of California, USA, *Geology*, 50, 755–759, <https://doi.org/10.1130/G49634.1>, 2022.
- Koren, G., Schneider, L., Velde, I. R., Schaik, E., Gromov, S. S., Adnew, G. A., Mrozek Martino, D. J., Hofmann, M. E. G., Liang, M., Mahata, S., Bergamaschi, P., Laan-Luijkx, I. T., Krol, M. C., Röckmann, T., and Peters, W.: Global 3-D simulations of the triple oxygen isotope signature $\Delta^{17}\text{O}$ in atmospheric CO_2 , *J. Geophys. Res.-Atmos.*, 124, 8808–8836, <https://doi.org/10.1029/2019JD030387>, 2019.
- Lee, P. S. and Majkowski, R. F.: High resolution infrared diode laser spectroscopy for isotope analysis – Measurement of

- isotopic carbon monoxide, *Appl. Phys. Lett.*, 48, 619–621, <https://doi.org/10.1063/1.96722>, 1986.
- Liang, M.-C., Laskar, A. H., Barkan, E., Newman, S., Thiemens, M. H., and Rangarajan, R.: New constraints of terrestrial and oceanic global gross primary productions from the triple oxygen isotopic composition of atmospheric CO_2 and O_2 , *Sci. Rep.*, 13, 2162, <https://doi.org/10.1038/s41598-023-29389-z>, 2023.
- Luz, B. and Barkan, E.: Variations of $^{17}\text{O}/^{16}\text{O}$ and $^{18}\text{O}/^{16}\text{O}$ in meteoric waters, *Geochim. Cosmochim. Acta*, 74, 6276–6286, <https://doi.org/10.1016/j.gca.2010.08.016>, 2010.
- Mahata, S., Bhattacharya, S. K., Wang, C.-H., and Liang, M.-C.: An improved CeO_2 method for high-precision measurements of $^{17}\text{O}/^{16}\text{O}$ ratios for atmospheric carbon dioxide: High-precision triple-isotope measurements of CO_2 , *Rapid Commun. Mass Spectrom.*, 26, 1909–1922, <https://doi.org/10.1002/rcm.6296>, 2012.
- Mahata, S., Bhattacharya, S. K., Wang, C. H., and Liang, M. C.: Oxygen isotope exchange between O_2 and CO_2 over hot platinum: An innovative technique for measuring $\Delta^{17}\text{O}$ in CO_2 , *Anal. Chem.*, 85, 6894–6901, <https://doi.org/10.1021/ac4011777>, 2013.
- Matsuhisa, Y., Goldsmith, J. R., and Clayton, R. N.: Mechanisms of hydrothermal crystallization of quartz at 250 °C and 15 kbar, *Geochim. Cosmochim. Acta*, 42, 173–182, [https://doi.org/10.1016/0016-7037\(78\)90130-8](https://doi.org/10.1016/0016-7037(78)90130-8), 1978.
- McCrea, J. M.: On the isotopic chemistry of carbonates and a paleotemperature scale, *J. Chem. Phys.*, 18, 849–857, <https://doi.org/10.1063/1.1747785>, 1950.
- McKinney, C. R., McCrea, J. M., Epstein, S., Allen, H. A., and Urey, H. C.: Improvements in mass spectrometers for the measurement of small differences in isotope abundance ratios, *Rev. Sci. Instrum.*, 21, 724–730, <https://doi.org/10.1063/1.1745698>, 1950.
- McManus, J. B., Nelson, D. D., Shorter, J. H., Jimenez, R., Herndon, S., Saleska, S., and Zahniser, M.: A high precision pulsed quantum cascade laser spectrometer for measurements of stable isotopes of carbon dioxide, *J. Mod. Opt.*, 52, 2309–2321, <https://doi.org/10.1080/09500340500303710>, 2006.
- McManus, J. B., Zahniser, M. S., Nelson, D. D., Shorter, J. H., Herndon, S. C., Jarvis, D., Agnese, M., McGovern, R., Yacovitch, T. I., and Roscioli, J. R.: Recent progress in laser-based trace gas instruments: performance and noise analysis, *Appl. Phys. B*, 119, 203–218, <https://doi.org/10.1007/s00340-015-6033-0>, 2015.
- Miller, M. F., Pack, A., Bindeman, I. N., and Greenwood, R. C.: Standardizing the reporting of $\Delta^{17}\text{O}$ data from high precision oxygen triple-isotope ratio measurements of silicate rocks and minerals, *Chem. Geol.*, 532, 119332, <https://doi.org/10.1016/j.chemgeo.2019.119332>, 2020.
- Mohn, J., Wolf, B., Toyoda, S., Lin, C.-T., Liang, M.-C., Brüggemann, N., Wissel, H., Steiker, A. E., Dyckmans, J., Szewc, L., Ostrom, N. E., Casciotti, K. L., Forbes, M., Giesemann, A., Well, R., Doucet, R. R., Yarnes, C. T., Ridley, A. R., Kaiser, J., and Yoshida, N.: Interlaboratory assessment of nitrous oxide isotopomer analysis by isotope ratio mass spectrometry and laser spectroscopy: current status and perspectives: Interlaboratory assessment of nitrous oxide isotopomer analysis, *Rapid Commun. Mass Spectrom.*, 28, 1995–2007, <https://doi.org/10.1002/rcm.6982>, 2014.
- Nataraj, A., Gianella, M., Prokhorov, I., Tuzson, B., Bertrand, M., Mohn, J., Faist, J., and Emmenegger, L.: Quantum cascade laser absorption spectrometer with a low temperature multipass cell for precision clumped CO_2 measurement, *Opt. Express*, 30, 4631, <https://doi.org/10.1364/OE.447172>, 2022.
- Nelson, D. D., McManus, J. B., Herndon, S. C., Zahniser, M. S., Tuzson, B., and Emmenegger, L.: New method for isotopic ratio measurements of atmospheric carbon dioxide using a 4.3 μm pulsed quantum cascade laser, *Appl. Phys. B*, 90, 301–309, <https://doi.org/10.1007/s00340-007-2894-1>, 2008.
- Pack, A. and Herwartz, D.: The triple oxygen isotope composition of the Earth mantle and understanding $\Delta^{17}\text{O}$ variations in terrestrial rocks and minerals, *Earth Planet. Sci. Lett.*, 390, 138–145, <https://doi.org/10.1016/j.epsl.2014.01.017>, 2014.
- Passey, B. H., Hu, H., Ji, H., Montanari, S., Li, S., Henkes, G. A., and Levin, N. E.: Triple oxygen isotopes in biogenic and sedimentary carbonates, *Geochim. Cosmochim. Acta*, 141, 1–25, <https://doi.org/10.1016/j.gca.2014.06.006>, 2014.
- Paul, D., Scheeren, H. A., Jansen, H. G., Kers, B. A. M., Miller, J. B., Crotwell, A. M., Michel, S. E., Gatti, L. V., Domingues, L. G., Correia, C. S. C., Neves, R. A. L., Meijer, H. A. J., and Peters, W.: Evaluation of a field-deployable NafionTM-based air-drying system for collecting whole air samples and its application to stable isotope measurements of CO_2 , *Atmos. Meas. Tech.*, 13, 4051–4064, <https://doi.org/10.5194/amt-13-4051-2020>, 2020.
- Perdue, N., Sharp, Z., Nelson, D., Wehr, R., and Dyroff, C.: A rapid high-precision analytical method for triple oxygen isotope analysis of CO_2 gas using tunable infrared laser direct absorption spectroscopy, *Rapid Commun. Mass Spectrom.*, 36, e9391, <https://doi.org/10.1002/rcm.9391>, 2022.
- Prokhorov, I., Kluge, T., and Janssen, C.: Laser absorption spectroscopy of rare and doubly substituted carbon dioxide isotopologues, *Anal. Chem.*, 91, 15491–15499, <https://doi.org/10.1021/acs.analchem.9b03316>, 2019.
- Saenger, C. P., Schauer, A. J., Heitmann, E. O., Huntington, K. W., and Steig, E. J.: How ^{17}O excess in clumped isotope reference-frame materials and ETH standards affects reconstructed temperature, *Chem. Geol.*, 563, 120059, <https://doi.org/10.1016/j.chemgeo.2021.120059>, 2021.
- Sakai, S., Matsuda, S., Hikida, T., Shimono, A., McManus, J. B., Zahniser, M., Nelson, D., Dettman, D. L., Yang, D., and Ohkouchi, N.: High-precision simultaneous $^{18}\text{O}/^{16}\text{O}$, $^{13}\text{C}/^{12}\text{C}$, and $^{17}\text{O}/^{16}\text{O}$ analyses for microgram quantities of CaCO_3 by tunable infrared laser absorption spectroscopy, *Anal. Chem.*, 89, 11846–11852, <https://doi.org/10.1021/acs.analchem.7b03582>, 2017.
- Steuer, P. M., Scheeren, H. A., Nelson, D. D., McManus, J. B., and Meijer, H. A. J.: Simultaneous measurement of $\delta^{13}\text{C}$, $\delta^{18}\text{O}$ and $\delta^{17}\text{O}$ of atmospheric CO_2 – performance assessment of a dual-laser absorption spectrometer, *Atmos. Meas. Tech.*, 14, 4279–4304, <https://doi.org/10.5194/amt-14-4279-2021>, 2021.
- Steuer, P. M., Scheeren, H. A., Koren, G., Adnew, G. A., Peters, W., and Meijer, H. A. J.: Interannual variations in the $\Delta(^{17}\text{O})$ signature of atmospheric CO_2 at two mid-latitude sites suggest a close link to stratosphere–troposphere exchange, *Atmos. Chem. Phys.*, 24, 11005–11027, <https://doi.org/10.5194/acp-24-11005-2024>, 2024.
- Stoltmann, T., Casado, M., Daëron, M., Landais, A., and Kassi, S.: Direct, precise measurements of isotopologue

- abundance ratios in CO_2 using molecular absorption spectroscopy: Application to $\Delta^{17}\text{O}$, *Anal. Chem.*, 89, 10129–10132, <https://doi.org/10.1021/acs.analchem.7b02853>, 2017.
- Thiemens, M. H., Jackson, T. L., and Brenninkmeijer, C. A. M.: Observation of a mass independent oxygen isotopic composition in terrestrial stratospheric CO_2 , the link to ozone chemistry, and the possible occurrence in the Martian atmosphere, *Geophys. Res. Lett.*, 22, 255–257, <https://doi.org/10.1029/94GL02996>, 1995.
- Thiemens, M. H., Chakraborty, S., and Jackson, T. L.: Decadal $\Delta^{17}\text{O}$ record of tropospheric CO_2 : Verification of a stratospheric component in the troposphere: 10 yr record of $\Delta^{17}\text{O}$ of tropospheric CO_2 , *J. Geophys. Res.-Atmos.*, 119, 6221–6229, <https://doi.org/10.1002/2013JD020317>, 2014.
- Tuzson, B., Mohn, J., Zeeman, M. J., Werner, R. A., Eugster, W., Zahniser, M. S., Nelson, D. D., McManus, J. B., and Emmenegger, L.: High precision and continuous field measurements of $\delta^{13}\text{C}$ and $\delta^{18}\text{O}$ in carbon dioxide with a cryogen-free QCLAS, *Appl. Phys. B*, 92, 451–458, <https://doi.org/10.1007/s00340-008-3085-4>, 2008.
- Wacker, U., Fiebig, J., and Schoene, B. R.: Clumped isotope analysis of carbonates: comparison of two different acid digestion techniques, *Rapid Commun. Mass Spectrom.*, 27, 1631–1642, <https://doi.org/10.1002/rcm.6609>, 2013.
- Wang, Z., Nelson, D. D., Dettman, D. L., McManus, J. B., Quade, J., Huntington, K. W., Schauer, A. J., and Sakai, S.: Rapid and precise analysis of carbon dioxide clumped isotopic composition by tunable infrared laser differential spectroscopy, *Anal. Chem.*, 92, 2034–2042, <https://doi.org/10.1021/acs.analchem.9b04466>, 2020.
- Wavelength Electronics: Application Note AN-LD18 Rev. A – Optimizing Laser Diode Control, <https://www.teamwavelength.com/download/applicationtechnotes/an-ld18.pdf> (last access: 2 December 2025), 2020.
- Wostbrock, J. A. G., Cano, E. J., and Sharp, Z. D.: An internally consistent triple oxygen isotope calibration of standards for silicates, carbonates and air relative to VSMOW2 and SLAP2, *Chem. Geol.*, 533, 119432, <https://doi.org/10.1016/j.chemgeo.2019.119432>, 2020.
- Yanay, N., Wang, Z., Dettman, D. L., Quade, J., Huntington, K. W., Schauer, A. J., Nelson, D. D., McManus, J. B., Thirumalai, K., Sakai, S., Rebaza Morillo, A., and Mallik, A.: Rapid and precise measurement of carbonate clumped isotopes using laser spectroscopy, *Sci. Adv.*, 8, eabq0611, <https://doi.org/10.1126/sciadv.abq0611>, 2022.
- Yanay, N., Quade, J., Wang, Z., Waseem, M. T., and Dettman, D. L.: Alteration of carbonate clumped isotope composition by burial heating in foreland sediments of the Himalaya, *Geochim. Cosmochim. Acta*, 394, 15–31, <https://doi.org/10.1016/j.gca.2025.02.023>, 2025.
- Young, E. D., Galy, A., and Nagahara, H.: Kinetic and equilibrium mass-dependent isotope fractionation laws in nature and their geochemical and cosmochemical significance, *Geochim. Cosmochim. Acta*, 66, 1095–1104, [https://doi.org/10.1016/s0016-7037\(01\)00832-8](https://doi.org/10.1016/s0016-7037(01)00832-8), 2002.
- Zhang, N., Prokhorov, I., Kueter, N., Li, G., Tuzson, B., Magyar, P. M., Ebert, V., Sivan, M., Nakagawa, M., Gilbert, A., Ueno, Y., Yoshida, N., Röckmann, T., Bernasconi, S. M., Emmenegger, L., and Mohn, J.: Rapid high-sensitivity analysis of methane clumped isotopes ($\Delta^{13}\text{CH}_3\text{D}$ and $\Delta^{12}\text{CH}_2\text{D}_2$) using mid-infrared laser spectroscopy, *Anal. Chem.*, 97, 1291–1299, <https://doi.org/10.1021/acs.analchem.4c05406>, 2025.