



Supplement of

Retrieval of aerosol properties from aerosol optical depth measurements with high temporal resolution and spectral range

Angelos Karanikolas et al.

Correspondence to: Angelos Karanikolas (angelos.karanikolas@pmodwrc.ch)

The copyright of individual parts of the supplement might differ from the article licence.

S1. GRASP-AOD from PFR data validation

Table S1: Statistics of the differences between GRASP-AOD from PFR data retrievals and AERONET inversions from almucantar scans for AOD at 500 nm > 0.1. The properties corresponding to fine mode correspond also to AOD_f>0.04 and AE>1, while the coarse mode properties, to AOD_c>0.04 and AE<1.5. We also include the AOD at 500 nm comparison between the PFR and AERONET inversions from almucantar scans.

Parameter	mean	median	St.dev.	P95th-P5th	R	median of the parameter - reference	Number of measurements
AOD 500 nm	-0.003	-0.003	0.009	0.027	0.99	0.154	1500
AOD _f 500 nm	-0.002	-0.002	0.013	0.040	0.98	0.131	1170
AOD _c 500 nm	-0.003	-0.003	0.007	0.022	0.99	0.114	356
C _{VT}	-0.008	-0.006	0.015	0.047	0.94	0.047	1500
C _{Vf}	-0.001	-0.002	0.007	0.022	0.79	0.021	1170
C _{Vc}	-0.022	-0.019	0.018	0.057	0.93	0.082	356
R _{eff}	-0.084	-0.004	0.225	0.722	0.91	0.306	1500
R _{Vf}	0.018	0.019	0.023	0.075	0.71	0.174	1170
R _{Vc}	-0.368	-0.304	0.337	1.109	0.10	1.750	356

Median uncertainties:

AERONET-SDA:

U-AOD_f=0.010

10 U-AOD_c=0.006

AERONET inversions from almucantar scans:

U-R_{Vf}=0.01 μm

U-R_{Vc}=0.096 μm

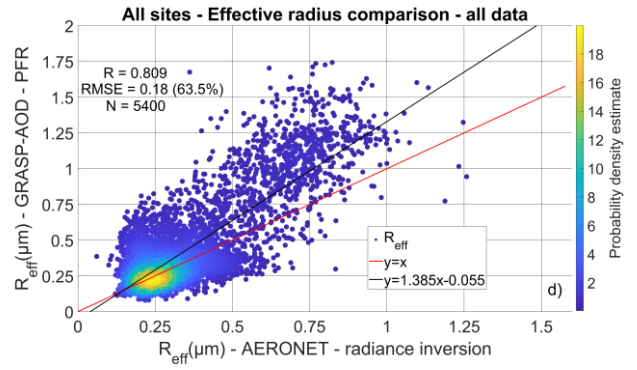
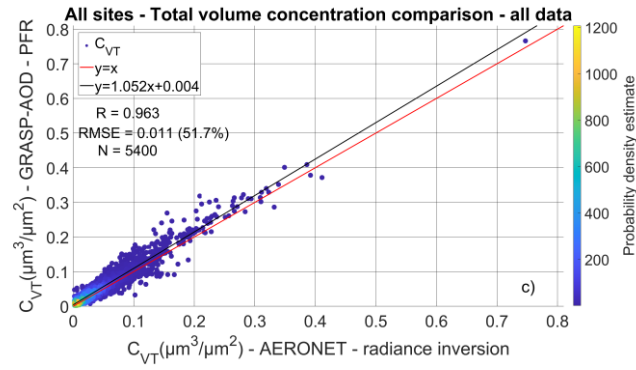
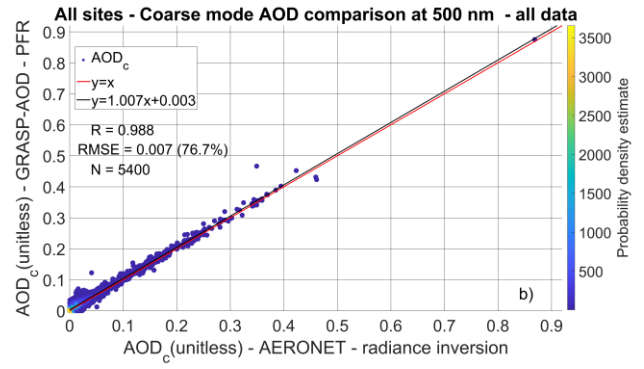
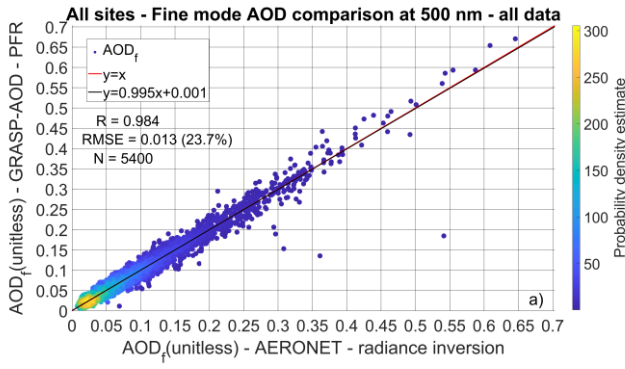


Figure S1: Scatter plot of AOD_f (a), AOD_c (b), C_{VT} (c) and R_{eff} (d) for the GRASP-AOD from PFR data and AERONET inversions from almucantar scans retrievals from all four locations without any selection criteria except $AOD_{440}>0.02$. The plots include the correlation factor (R), the root mean square error (RMSE) and the number of observations (N). The colour bar shows the density of the points. We also include the linear fit between the datasets and the $y=x$ line.

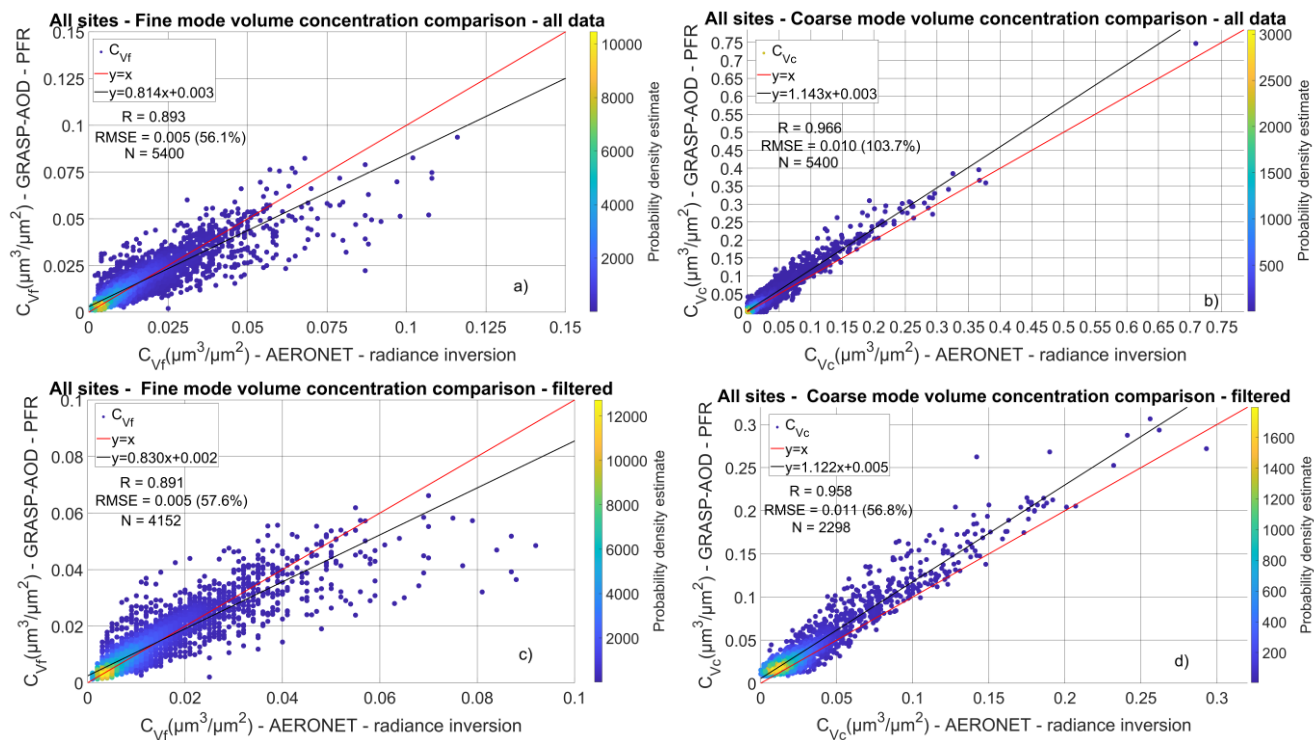


Figure S2: Scatter plot of C_{Vf} (a, c) and C_{Vc} (b, d) for the GRASP-AOD from PFR data and AERONET inversions from almucantar scans from all four locations. Panels a and b correspond to the entire datasets and panels c and d to the selected data.

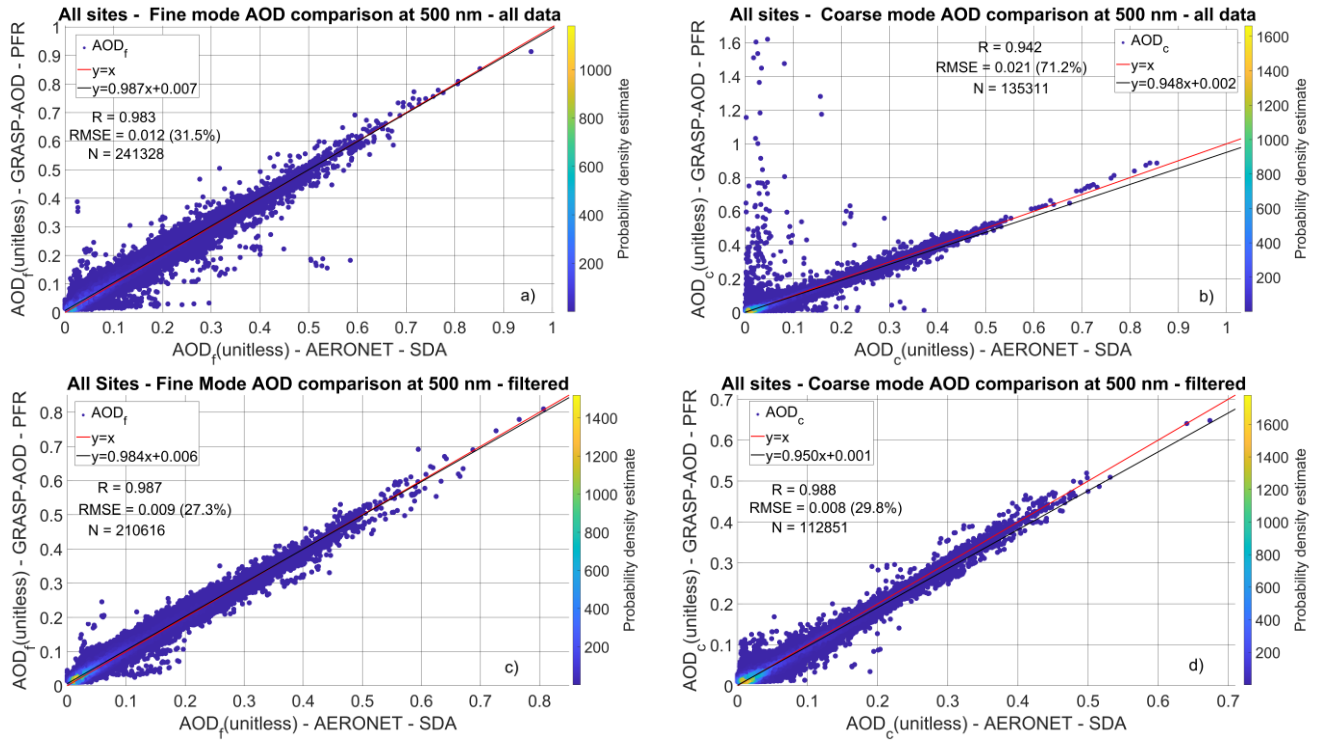


Figure S3: Scatter plot of AOD_f (a, c) and AOD_c (b, d) for the GRASP-AOD from PFR data and AERONET inversions from almucantar scans from all four locations. Panels a and b correspond to the entire datasets and panels c and d to the selected data.

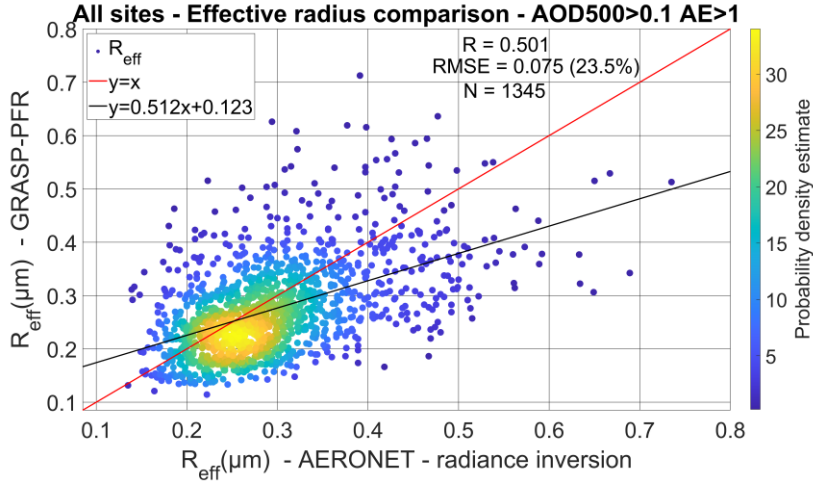


Figure S4: Scatter plot of R_{eff} for the GRASP-AOD from PFR data and AERONET inversions from almucantar scans for data corresponding to $AOD > 0.1$ at 500 nm and $AE > 1$.

S2. Data screening

AERONET inversions data screening:

We rejected all data corresponding to AOD, AOD_f and AOD_c differences at 500 nm between AERONET inversions from almucantar scans and retrievals by the AERONET direct sun output and spectral deconvolution algorithm according to the following empirically defined thresholds of keeping data:

- 1. Coincident AOD, AOD_f and AOD_c differences at 500 nm <0.03 (7.5 minutes seconds threshold).
- 2. Common daily AOD median differences <0.015 for AOD and <0.018 for AOD_f and AOD_c.
- 3. 80th-20th percentile of daily AOD, AOD_f and AOD_c difference <0.055.

Direct sun AOD data screening:

We rejected data corresponding to AOD differences (30 seconds threshold) between PFR and CIMEL direct sun output according to the following thresholds:

- 1. Coincident AOD differences <0.09 for 380 and 440 nm, <0.06 for 500 nm and <0.04 for 870 nm.
- 2. Common daily AOD median differences <0.05 for 380 and 440 nm, <0.014 for 500 nm and <0.009 for 870 nm.
- 3. 80th-20th percentile of daily AOD difference <0.09 for 380 and 440 nm, <0.03 for 500 nm and <0.02 for 870 nm.

S3. Refractive index climatologies

Table S2: Refractive index climatologies for all stations.

Month	RRI				IRI			
	440 nm	675 nm	870 nm	1020 nm	440 nm	675 nm	870 nm	1020 nm
Davos								
Annual for all months	1.378	1.441	1.465	1.4621	0.0073	0.0026	0.0021	0.0018
Hohenpeissenberg								
Annual for all months	1.469	1.459	1.453	1.448	0.0032	0.0035	0.0038	0.0039
Izana								
1	1.476	1.472	1.448	1.436	0.0023	0.0006	0.0009	0.0012
2	1.476	1.472	1.448	1.436	0.0023	0.0006	0.0009	0.0012
3	1.476	1.472	1.448	1.436	0.0023	0.0006	0.0009	0.0012
4	1.484	1.477	1.454	1.442	0.0024	0.0007	0.0012	0.0016
5	1.484	1.477	1.454	1.442	0.0024	0.0007	0.0012	0.0016
6	1.484	1.477	1.454	1.442	0.0024	0.0007	0.0012	0.0016
7	1.480	1.475	1.452	1.440	0.0023	0.0006	0.0010	0.0013
8	1.480	1.475	1.452	1.440	0.0023	0.0006	0.0010	0.0013

9	1.475	1.473	1.449	1.438	0.0023	0.0005	0.0008	0.0010
10	1.475	1.473	1.449	1.438	0.0023	0.0005	0.0008	0.0010
11	1.475	1.473	1.449	1.438	0.0023	0.0005	0.0008	0.0010
12	1.476	1.472	1.448	1.436	0.0023	0.0006	0.0009	0.0012
Lindenberg								
1	1.489	1.474	1.469	1.461	0.0070	0.0068	0.0083	0.0090
2	1.489	1.474	1.469	1.461	0.0070	0.0068	0.0083	0.0090
3	1.469	1.462	1.461	1.456	0.0072	0.0070	0.0081	0.0086
4	1.469	1.462	1.461	1.456	0.0072	0.0070	0.0081	0.0086
5	1.453	1.453	1.453	1.450	0.0061	0.0057	0.0066	0.0069
6	1.471	1.461	1.457	1.450	0.0050	0.0048	0.0057	0.0060
7	1.457	1.451	1.449	1.444	0.0054	0.0056	0.0067	0.0071
8	1.461	1.453	1.451	1.445	0.0055	0.0059	0.0069	0.0073
9	1.449	1.446	1.446	1.442	0.0057	0.0063	0.0073	0.0077
10	1.470	1.461	1.459	1.453	0.0051	0.0053	0.0059	0.0060
11	1.470	1.461	1.459	1.453	0.0051	0.0053	0.0059	0.0060
12	1.479	1.467	1.464	1.457	0.0061	0.0061	0.0071	0.0075

55

S4. Scenarios, weights and rating for GRASP self-consistency tests

The settings are selected depending on the performance of self-consistency tests, AOD and AE. The self-consistency tests are evaluated through case-by-case inspection and a rating system. We selected 10 scenarios for the parameters C_{Vf} , C_{Vc} , R_{Vf} and R_{Vc} corresponding to various usual and unusual or even extreme conditions (Table S3). We also assigned for each scenario a weight based on the frequency it appears on the AERONET data included in the GRASP-AOD from PFR data validation in the four common stations. For each scenario we calculate the AOD using the GRASP forward model and provide that AOD (Table S4) to the inversion mode of GRASP to retrieve back the aerosol size properties we selected. Then we calculate the difference of the aerosol size properties and AOD between the forward model and inversion to evaluate the self-consistency. The procedure is repeated for various initial guesses treating one parameter as variable every time. Each parameter includes a weight based on the performance in the PFR validation and an uncertainty based on either the GAW-PFR or AERONET uncertainty estimates (AOD) or the standard deviation of the differences between GRASP-AOD from PFR data and AERONET inversions from almucantar scans (Table S4). The weights of each scenario and parameter and the uncertainty estimates in combination with the differences between the forward model and inversion, provide a combined rating according to Eq. S1. The lower the rating, the more self-consistency the inversion showed. After a provisional selection of initial guesses, we repeated the self-consistency tests for all their combinations to evaluate the performance and find potentially unstable combinations. From the combinations that showed no unusually worse self-

consistency from the rest, we selected initial guesses based on the AOD and AE that they correspond according to the forward model (Table S8). The final selection is in the end of this section after Table S8.

Provisional selection of initial guesses:
 C_{Vf} and C_{Vc} : 0.001, 0.005, 0.006, 0.008, 0.009
 R_{Vf} : 0.1, 0.15, 0.225
 R_{Vc} : 1.75, 2.25

80 Table S3: Scenarios for forward model runs used for the self-consistency tests to retrieve aerosol properties from BTS spectroradiometer. Fixed parameters: $RRI=1.49$, $IRI=0.009$, $\sigma_{Vf}=0.4$ and $\sigma_{Vc}=0.7$.

Scenario number	Scenario name	C_{Vf} ($\mu m^3/\mu m^2$)	C_{Vc} ($\mu m^3/\mu m^2$)	R_{Vf} (μm)	R_{Vc} (μm)	AOD 500nm	Weight_scen
1	lrhc	0.1	0.12	0.4	4	0.722	0.01
2	srhc	0.1	0.12	0.1	1.5	0.626	0.01
3	lrlc	0.003	0.005	0.4	4	0.022	0.01
4	srhc	0.003	0.005	0.1	1.5	0.021	0.01
5	moder1	0.01	0.035	0.15	1.8	0.114	1
6	moder2	0.01	0.035	0.2	2.5	0.112	1
7	mrhc	0.1	0.12	0.15	2.5	0.398	0.02
8	mrhc	0.1	0.12	0.15	2.5	0.025	0.01
9	mrhflc	0.05	0.005	0.15	2.5	0.338	0.05
10	mrlfhc	0.003	0.07	0.15	2.5	0.085	0.15

Table S4: Weights and uncertainties (AOD parameters) or standard deviations of the differences in the PFR comparisons (aerosol size properties and residuals) for each parameter.

Parameter	Weight_par	σ_{par}
ΔC_{Vf}	0.85	0.006
ΔC_{Vc}	0.85	0.015
ΔR_{Vf}	0.6	0.038
ΔR_{Vc}	0.1	0.503
$\Delta \sigma_{Vf}$	0.01	0.168
$\Delta \sigma_{Vc}$	0.01	0.090
res. rel.	0.50	0.021
res. abs.	1	0.002
mean ΔAOD	0.75	0.010
median ΔAOD	1	0.010
ΔAOD st.dev.	0.75	0.010

Rating calculation:

$$85 \quad Rating = \sum_{scenn=1}^{10} (Weight_scenn \times \sum_{parn=1}^{11} (|100 \times \frac{Weight_{par} \Delta par}{\sigma_{par}}|)) \quad (S1)$$

Table S5: Initial guesses of C_{Vf} and C_{Vc} and the corresponding rating for each wavelength selection.

Initial guess	Rating		Initial guess	Rating	
C_{Vf}	16wl	7wl	C_{Vc}	16wl	7wl
0.001	16.9	1310.4	0.001	13.5	2759.5
0.003	33.8	2734.7	0.003	80.6	311.0
0.005	14.0	2803.9	0.005	12.1	273.1
0.006	82.8	2755.7	0.006	49.5	248.0
0.007	13.5	2759.5	0.007	95.2	266.3
0.008	12.5	2800.7	0.008	14.4	253.3
0.009	12.6	2852.0	0.009	12.4	263.2
0.01	13.3	2859.3	0.01	12.5	359.2
0.02	101.3	2877.2	0.03	25.2	354.9
0.03	137.4	2977.3	0.05	25.0	365.5
0.05	142.7	2860.2	0.09	13.4	393.0
0.09	218.0	2759.3	0.12	14.4	379.2

Table S6: Initial guesses of R_{Vf} and R_{Vc} and the corresponding rating for each wavelength selection.

Initial guess	Rating		Initial guess	Rating	
R_{Vf}	16wl	7wl	R_{Vc}	16wl	7wl
0.1	55.8	1476.6	1.75	3.5	308.6
0.125	14.6	3034.5	2	15.3	1549.4
0.15	12.5	2802.2	2.25	6.7	1680.3
0.175	106.7	2943.6	2.5	8.5	1759.2
0.2	130.3	3030.6	2.75	10.0	2688.2
0.225	25.6	2962.9	3	12.6	2734.2
0.25	2249.9	2948.8	3.25	57.4	2776.1
0.275	2338.7	2929.7	3.5	164.5	2812.9
0.3	4373.9	2915.8	3.75	353.4	2836.8
0.325	4486.1	2907.4	4	298.5	2865.9
0.35	4677.8	3273.2	-	-	-

0.375	4750.5	3115.5	-	-	-
-------	--------	--------	---	---	---

Table S7: Initial guesses of IRI and the corresponding rating for each wavelength selection.

Input inv.	Rating	
IRI	16wl	7wl
0.001	80.3	2871.4
0.002	28.3	2857.1
0.003	25.7	2842.5
0.006	19.7	2797.5
0.009	13.5	2759.5
0.012	79.1	2724.1
0.015	29.4	2692.1
0.02	130.8	2682.5
0.04	93.3	2797.4
0.06	149.4	2868.5

90 Table S8: AOD and AE for different SD parameters from GRASP forward model runs.

C_{vr}($\mu\text{m}^3/\mu\text{m}^2$)	C_{vc}($\mu\text{m}^3/\mu\text{m}^2$)	R_{vr}(μm)	R_{vc}(μm)	AOD at 500 nm	AE
0.001	0.001	0.15	2.25	0.008	1.606
0.001	0.001	0.1	1.75	0.006	1.583
0.001	0.001	0.225	3	0.009	1.233
0.001	0.005	0.15	2.25	0.012	0.844
0.005	0.001	0.15	2.25	0.034	1.987
0.005	0.005	0.15	2.25	0.039	1.606
0.006	0.006	0.15	2.25	0.046	1.606
0.008	0.008	0.15	2.25	0.062	1.606
0.009	0.009	0.15	2.25	0.069	1.606
0.009	0.009	0.1	1.75	0.051	1.583
0.009	0.009	0.225	3	0.081	1.233
0.001	0.009	0.15	2.25	0.016	0.559
0.009	0.001	0.15	2.25	0.061	2.044
0.009	0.006	0.15	2.25	0.066	1.742
0.006	0.009	0.15	2.25	0.049	1.441

Final selection of initial guesses for BTS retrievals:

$R_{Vc}=1.75 \mu\text{m}$ always

95 $\sigma_{Vf}=0.4 \mu\text{m}$ always

$\sigma_{Vc}=0.7 \mu\text{m}$ always

For $AE < 0.6$

$C_{Vf}=0.001 \mu\text{m}^3 / \mu\text{m}^2$

100 $C_{Vc}=0.009 \mu\text{m}^3 / \mu\text{m}^2$

$R_{Vf1}=0.15 \mu\text{m}$

$R_{Vf2}=0.225 \mu\text{m}$

For $AE > 1.9$

105 $C_{Vf}=0.009 \mu\text{m}^3 / \mu\text{m}^2$

$C_{Vc}=0.001 \mu\text{m}^3 / \mu\text{m}^2$

$R_{Vf1}=0.1 \mu\text{m}$

$R_{Vf2}=0.15 \mu\text{m}$

110 For $AE \geq 0.6$ and $AE < 1.3$ and $AOD < 0.05$ at 500 nm

$C_{Vf1}=0.005 \mu\text{m}^3 / \mu\text{m}^2$

$C_{Vc1}=0.005 \mu\text{m}^3 / \mu\text{m}^2$

$R_{Vf1}=0.15 \mu\text{m}$

$C_{Vf2}=0.006 \mu\text{m}^3 / \mu\text{m}^2$

115 $C_{Vc2}=0.006 \mu\text{m}^3 / \mu\text{m}^2$

$R_{Vf2}=0.225 \mu\text{m}$

For $AE \geq 1.3$ and $AE < 1.9$ and $AOD < 0.05$ at 500 nm

$C_{Vf}=0.005 \mu\text{m}^3 / \mu\text{m}^2$

120 $C_{Vc}=0.005 \mu\text{m}^3 / \mu\text{m}^2$

$R_{Vf1}=0.1 \mu\text{m}$

$R_{Vf2}=0.15 \mu\text{m}$

For $AE \geq 0.6$ and $AE < 1.3$ and $AOD \geq 0.05$ at 500 nm

125 $C_{Vf}=0.009 \mu\text{m}^3 / \mu\text{m}^2$

$C_{Vc}=0.009 \mu\text{m}^3 / \mu\text{m}^2$

$R_{Vf1}=0.15\text{ }\mu\text{m}$
 $R_{Vf2}=0.225\text{ }\mu\text{m}$

130 For $AE\geq 1.3$ and $AE<1.9$ and $AOD\geq 0.05$ at 500 nm

$C_{Vf}=0.009\text{ }\mu\text{m}^3/\text{ }\mu\text{m}^2$
 $C_{Ve}=0.009\text{ }\mu\text{m}^3/\text{ }\mu\text{m}^2$
 $R_{Vf1}=0.1\text{ }\mu\text{m}$
 $R_{Vf2}=0.15\text{ }\mu\text{m}$

135

S5. Wildfire episode

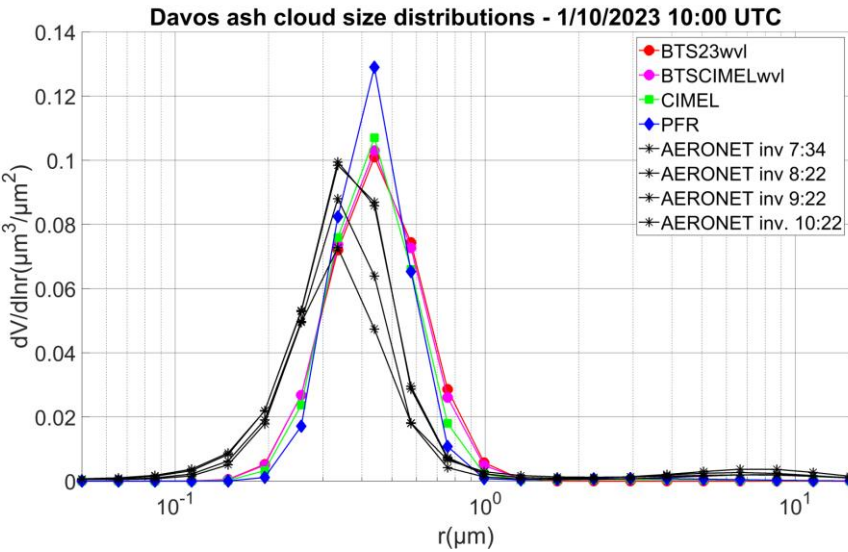


Figure S5: Size distributions from GRASP-AOD from PFR data, GRASP-AOD from BTS data and GRASP-AOD from CIMEL data (coloured lines) for a coincident measurement of AOD and the four closest AERONET size distributions (black lines).

140 Initial guesses and refractive index:

$C_{Vf}:0.007\text{ }\mu\text{m}^3/\text{ }\mu\text{m}^2$
 $C_{Ve}:0.001\text{ }\mu\text{m}^3/\text{ }\mu\text{m}^2$
 $R_{Vf}: 0.145\text{ }\mu\text{m}$
 $R_{Ve}: 3.154\text{ }\mu\text{m}$
 $\sigma_{Vf}:0.4\text{ }\mu\text{m}$
 $\sigma_{Ve}:0.7\text{ }\mu\text{m}$
 $RRI: 1.401$

145

IRI: 0.003

150 BTS AOD wavelengths:

304, 310, 320, 330, 340, 350, 370, 390, 410, 440, 480, 500, 540, 610, 675, 750, 777, 845, 880, 1020, 1240, 1550 and 1640 nm