Supplement Information

Physical and chemical characterisation of PM emissions from two ships operating in European Emission Control Areas

Moldanová, J., Fridell, E., Winnes, H., Holmin-Fridell, S., Boman, J., Jedynska, A., Tishkova, V., Demirdjian, B., Joulie, S., Bladt, H., Ivleva, N., P., Niessner, R.

Table S1. Properties of the investigated ships

Ship	Туре	Length [m]	Gross tonnage	Built year	Max/average speed [knots]
S1	Dry cargo	166	18 773	1987	14.9/13.0
S2	RoPax Ferry	240	46 353	2001	21.5/17.7

Table S2. Engine parameters for the campaign experiments. S1, S2: ships investigated; HFO1%, HFO0.5%: HFO used by the investigated engine with approximate fuel sulphur content, ME-full, ME-low: main engine with full and low engine-load conditions

Measurement/	S1_	S1_	S1_	S2_	S2_	S2_
Engine parameter	HFO1%	HFO1%	MGO	HFO1%	HFO0.5%	MGO_
	_ME-full	_ME-low	_AE	_ME-full	_ME-full	ME-full
Fuel consumption						
(kg/h)	760	257	83	648	635	619
Fuel consumption						
(g/kWh)	211.5	192.3	203.9	189.4	185.7	181.0
Power (kW)	3 592	1 336	405	3 420	3 420	3 420
Nominal engine speed (rpm)	750	750	1 000	510	510	510
Actual engine speed (rpm)	720	570	870	435	435	435
Gas flow in stack					16 200,	
$(nm^3/h)^*$	20 922	7 667	2415	16 283	14 600	16 800
Temperature in exhaust gas (°C)	292	290	302	360	360	360

^{*} Calculated from fuel consumption and fuel composition, normalised to 273.15 K

Table S3. Results of fuel (column 3-7) and lubricant (column 8,9) analyses. Lubricants in investigated main engines on S1 and S2 ships were analysed.

		S1_	S2_	S2_	S1_	S2_	S1_	S2_		Uncertainty		
		HFO1%	HFO1%	HFO0.5%	MGO	MGO	Lub	Lub				
	Unit	ME	_ME	_ME	_AE	_ME	_ME	_ME	HFO	MGO	Lub	
Density												
(15°C)	kg/m³	977.3	988.7	943.3	834.1	846.4	908.3	927	±1.5	±0.5	±1.5	
Water	% V/V	<0.10	0.14	<0.10	< 0.10	<0.10	0.3	0.11	-	-	-	
S	% m/m	0.91	0.96	0.58	0.03	0.1	0.53	0.92	±10%	±34%	±10%	
Ash	% m/m	0.02	0.02	0.01	< 0.01	< 0.01	2.7	2.7	±67%	-	±1.5%	
V	mg/kg	34	20	6	<1	<1	20	71	±58%	-	±41%	
Na	mg/kg	8	11	7	<1	<1	20	32	±41%	-	±25%	
Al	mg/kg	16	20	16	<1	<1	6	4	±34%	-	±34%	
Si	mg/kg	14	18	15	<1	<1	8	18	±33%	-	±33%	
Fe	mg/kg	16	9	7	<1	<1	10	25	±34%	-	±28%	
Ni	mg/kg	16	15	9	<1	<1	12	60	±54%	-	±41%	
Ca	mg/kg	5	8	4	<1	<1	8230	7670	±36%	-	±2.8%	
Mg	mg/kg	<1	1	<1	<1	<1	38	37	±>100%	-	±15%	
Pb	mg/kg	<1	<1	<1	<1	<1	<1	<1	-	-	-	
Zn	mg/kg	2	1	2	<1	<1	330	440	±44%	-	±8.6%	
Р	mg/kg	<1	<1	<1	<1	<1	279	266	-	-	±18%	
K	mg/kg	<1	1	<1	<1	<1	5	7	±>100%	-	±20%	
С	% m/m	87.51	87.93	87.13	86.02	86.29	-	-	±2.8%	±2.8%	-	
Н	% m/m	11.01	10.68	12.11	13.66	13.54	-	-	±6.9%	±6.3%	-	
N	% m/m	0.39	0.42	0.3	<0.10	< 0.10	-	-	±>100%	-	-	
0	% m/m	0.35	0.44	0.34	< 0.30	< 0.30	-	-	±>100%	-	-	
Net speci-												
fic heat	MJ/kg	41.09	40.86	41.67	42.92	42.75	-	-	±1.0%	±0.9%	-	

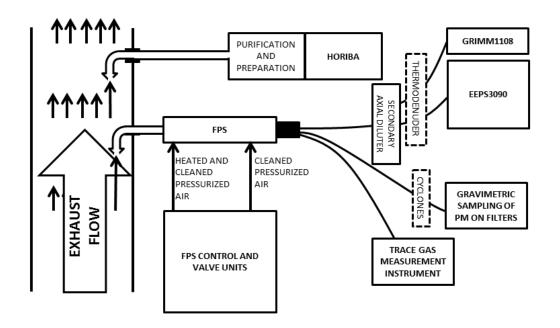


Figure S1. The measurement setup. Exhaust was sampled through an isokinetic probe to the Dekati Fine Particle Sampler (FPS control and valve unit) and led to the flow divider. From the flow divider one line was led through secondary dilution step (Dekati DAD-100) and optionally thermodenuder (Dekati ELA 423) to EEPS (Engine Exhaust Particle Sizer, Model 3090, TSI Inc.) and aerosol spectrometer (GRIMM 1.108). Second line was led optionally through $PM_{2.5}$ and PM_{10} cyclones followed by filter holders. The vacuum pumps behind the filter holders were connected to gas meters and rotameters for sample flow velocity and volume control. The third line was also led to trace gas measurement instrument for supervision of the dilution. Gas sampling was performed from a second probe in the exhaust channel.

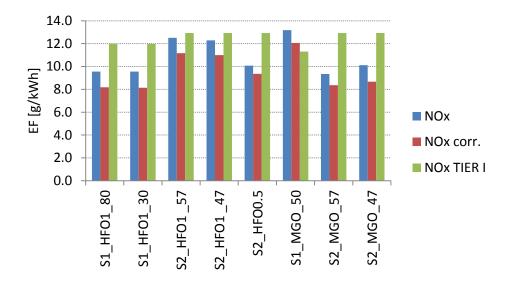
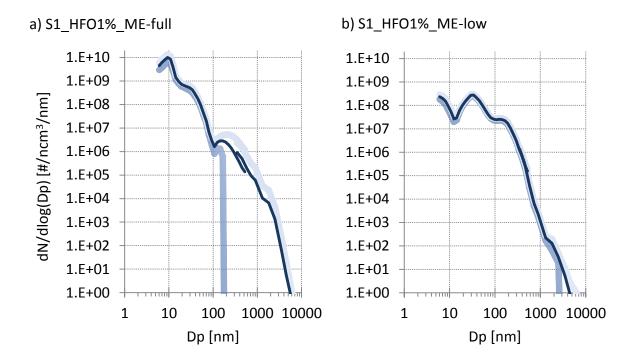


Figure S2. Emission factors for NO_X measured on investigated engines. NO_X corr. is $EF(NO_X)$ corrected for ambient conditions (humidity and temperature) as in ISO 8178-1 1996 clause 13.3, NO_X TIER I is the maximum allowed $EF(NO_X)$ for the engine calculated according to the TIER I NOx emission standard.



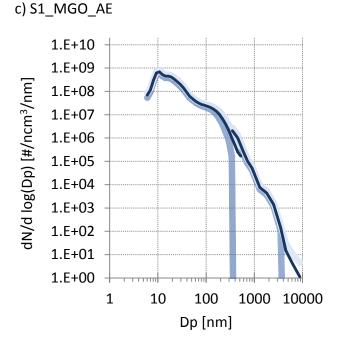


Figure S3 Particle number distributions for 3 different experiments on ship S1. The light-blue line shows 1 standard deviation interval around the mean. In size range 300-500 nm the double lines represent results from EEPS and GRIMM instruments, respectively.

Table S4. Emission factors in mg kg⁻¹ fuel for elements in PM analysed by EDXRF (S and Ca analysed also as SO₄²⁻ and Ca⁺ by IC) on filter samples. In the upper part are presented mean emission factors, in the middle part EF resulted from analyses performed in the 2 laboratories are shown. In the bottom part, mean relative uncertainties (Rel. uc. = mean uncertainty/mean concentration of a group of samples) for 4 groups of samples (S1 HFO, S1 MGO, S2 HFO, S2 MGO) are presented together with mean coefficient of variance (CV) of the investigated multiple samples (2 triplets sampled in HFO exhaust).

Sample	type			S	V	Ni	Fe	Cr	Mg	Al	Si	Co	K	Р	Zn	Ca
S1	HFO 1%	ME-full	PM1	88.5	21.0	13.6	5.5	0.29	2.1	2.3	2.3	<d.l.< td=""><td>0.31</td><td>1.8</td><td>1.1</td><td>7.6</td></d.l.<>	0.31	1.8	1.1	7.6
S1	HFO 1%	ME-full	PM10	34.8	20.3	13.6	5.8	0.40	5.4	3.1	2.1	<d.l.< td=""><td>0.05</td><td>1.0</td><td>1.1</td><td>8.3</td></d.l.<>	0.05	1.0	1.1	8.3
S1	HFO 1%	ME-full	TSP	102.0	19.8	16.1	5.0	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>3.6</td><td>15.7</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>3.6</td><td>15.7</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>3.6</td><td>15.7</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>3.6</td><td>15.7</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>3.6</td><td>15.7</td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td>3.6</td><td>15.7</td></d.l.<></td></d.l.<>	<d.l.< td=""><td>3.6</td><td>15.7</td></d.l.<>	3.6	15.7
S1	HFO 1%	ME-low	PM1	18.1	12.6	9.6	3.3	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>0.64</td><td>2.2</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>0.64</td><td>2.2</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>0.64</td><td>2.2</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>0.64</td><td>2.2</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>0.64</td><td>2.2</td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td>0.64</td><td>2.2</td></d.l.<></td></d.l.<>	<d.l.< td=""><td>0.64</td><td>2.2</td></d.l.<>	0.64	2.2
S1	HFO 1%	ME-low	PM10	18.0	7.4	5.6	1.7	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>2.0</td><td><d.l.< td=""><td>0.30</td><td>0.9</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>2.0</td><td><d.l.< td=""><td>0.30</td><td>0.9</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>2.0</td><td><d.l.< td=""><td>0.30</td><td>0.9</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td>2.0</td><td><d.l.< td=""><td>0.30</td><td>0.9</td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td>2.0</td><td><d.l.< td=""><td>0.30</td><td>0.9</td></d.l.<></td></d.l.<>	2.0	<d.l.< td=""><td>0.30</td><td>0.9</td></d.l.<>	0.30	0.9
S1	HFO 1%	ME-low	TSP	18.0	9.9	9.2	4.3	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>2.5</td><td><d.l.< td=""><td>7.6</td><td>2.4</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>2.5</td><td><d.l.< td=""><td>7.6</td><td>2.4</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>2.5</td><td><d.l.< td=""><td>7.6</td><td>2.4</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td>2.5</td><td><d.l.< td=""><td>7.6</td><td>2.4</td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td>2.5</td><td><d.l.< td=""><td>7.6</td><td>2.4</td></d.l.<></td></d.l.<>	2.5	<d.l.< td=""><td>7.6</td><td>2.4</td></d.l.<>	7.6	2.4
S2	HFO 1%	ME-full	PM2.5	36.3	8.9	7.9	1.3	0.08	<d.l.< td=""><td>0.11</td><td>0.97</td><td>0.44</td><td><d.l.< td=""><td><d.l.< td=""><td>0.35</td><td>2.3</td></d.l.<></td></d.l.<></td></d.l.<>	0.11	0.97	0.44	<d.l.< td=""><td><d.l.< td=""><td>0.35</td><td>2.3</td></d.l.<></td></d.l.<>	<d.l.< td=""><td>0.35</td><td>2.3</td></d.l.<>	0.35	2.3
S2	HFO 1%	ME-full	PM10	37.6	8.5	8.1	1.4	0.13	0.9	0.97	0.22	0.35	<d.l.< td=""><td><d.l.< td=""><td>0.24</td><td>2.1</td></d.l.<></td></d.l.<>	<d.l.< td=""><td>0.24</td><td>2.1</td></d.l.<>	0.24	2.1
S2	HFO 0.5%	ME-full	PM2.5	22.6	2.3	5.7	0.65	0.09	0.3	0.45	<d.l.< td=""><td>0.35</td><td><d.l.< td=""><td><d.l.< td=""><td>0.35</td><td>1.6</td></d.l.<></td></d.l.<></td></d.l.<>	0.35	<d.l.< td=""><td><d.l.< td=""><td>0.35</td><td>1.6</td></d.l.<></td></d.l.<>	<d.l.< td=""><td>0.35</td><td>1.6</td></d.l.<>	0.35	1.6
S2	HFO 0.5%	ME-full	PM10	28.5	2.5	6.3	0.91	<d.l.< td=""><td>1.0</td><td>0.97</td><td><d.l.< td=""><td>0.26</td><td><d.l.< td=""><td><d.l.< td=""><td>0.16</td><td>1.9</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	1.0	0.97	<d.l.< td=""><td>0.26</td><td><d.l.< td=""><td><d.l.< td=""><td>0.16</td><td>1.9</td></d.l.<></td></d.l.<></td></d.l.<>	0.26	<d.l.< td=""><td><d.l.< td=""><td>0.16</td><td>1.9</td></d.l.<></td></d.l.<>	<d.l.< td=""><td>0.16</td><td>1.9</td></d.l.<>	0.16	1.9
S2	MGO	ME-full	PM2.5	1.1	0.21	<d.l.< td=""><td>0.048</td><td>0.02</td><td><d.l.< td=""><td><d.l.< td=""><td>0.28</td><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.3</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	0.048	0.02	<d.l.< td=""><td><d.l.< td=""><td>0.28</td><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.3</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td>0.28</td><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.3</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	0.28	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.3</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.3</td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td>1.3</td></d.l.<></td></d.l.<>	<d.l.< td=""><td>1.3</td></d.l.<>	1.3
S2	MGO	ME-full	PM10	1.6	0.17	0.068	0.052	0.11	<d.l.< td=""><td><d.l.< td=""><td>0.14</td><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>0.24</td><td>1.3</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td>0.14</td><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>0.24</td><td>1.3</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	0.14	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>0.24</td><td>1.3</td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td>0.24</td><td>1.3</td></d.l.<></td></d.l.<>	<d.l.< td=""><td>0.24</td><td>1.3</td></d.l.<>	0.24	1.3
S1	MGO	AE	PM1	2.4	0.007	0.015	0.098	0.17	2.8	0.97	0.16	<d.l.< td=""><td><bl< td=""><td>0.047</td><td>1.2</td><td>7.8</td></bl<></td></d.l.<>	<bl< td=""><td>0.047</td><td>1.2</td><td>7.8</td></bl<>	0.047	1.2	7.8
S1	MGO	AE	PM10	2.6	0.007	0.015	0.098	0.17	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.4</td><td>9.5</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.4</td><td>9.5</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.4</td><td>9.5</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.4</td><td>9.5</td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td>1.4</td><td>9.5</td></d.l.<></td></d.l.<>	<d.l.< td=""><td>1.4</td><td>9.5</td></d.l.<>	1.4	9.5
S1	MGO	AE	TSP	2.7	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.7</td><td>11.2</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.7</td><td>11.2</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.7</td><td>11.2</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.7</td><td>11.2</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.7</td><td>11.2</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.7</td><td>11.2</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.7</td><td>11.2</td></d.l.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td>1.7</td><td>11.2</td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td>1.7</td><td>11.2</td></d.l.<></td></d.l.<>	<d.l.< td=""><td>1.7</td><td>11.2</td></d.l.<>	1.7	11.2
S1	HFO 1%	Lab1	PM2.5	66.9	18.0	13.8	5.3	<d.l.< td=""><td>-</td><td>-</td><td>-</td><td>0.6</td><td><d.l.< td=""><td>-</td><td>1.1</td><td>5.6</td></d.l.<></td></d.l.<>	-	-	-	0.6	<d.l.< td=""><td>-</td><td>1.1</td><td>5.6</td></d.l.<>	-	1.1	5.6
S1	HFO 1%	Lab 2	PM2.5	78.3	23.9	13.5	5.7	0.3	2.1	2.3	2.3	0.7	0.3	1.8	1.0	9.6
S1	HFO 1%	Lab 1	PM10	23.7	20.1	14.9	5.7	<d.l.< td=""><td>-</td><td>-</td><td>-</td><td>0.6</td><td><d.l.< td=""><td>-</td><td>1.3</td><td>7.2</td></d.l.<></td></d.l.<>	-	-	-	0.6	<d.l.< td=""><td>-</td><td>1.3</td><td>7.2</td></d.l.<>	-	1.3	7.2
S1	HFO 1%	Lab 2	PM10	45.8	20.6	12.3	5.9	0.4	5.4	3.1	2.1	0.6	0.1	1.0	0.8	9.4
S1	MGO	Lab 1	PM2.5	<d.l.< td=""><td><d.l.< td=""><td><d.l.< td=""><td><b.v.< td=""><td><d.l.< td=""><td>-</td><td>-</td><td>-</td><td><d.l.< td=""><td><d.l.< td=""><td>-</td><td>1.4</td><td>7.3</td></d.l.<></td></d.l.<></td></d.l.<></td></b.v.<></td></d.l.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><d.l.< td=""><td><b.v.< td=""><td><d.l.< td=""><td>-</td><td>-</td><td>-</td><td><d.l.< td=""><td><d.l.< td=""><td>-</td><td>1.4</td><td>7.3</td></d.l.<></td></d.l.<></td></d.l.<></td></b.v.<></td></d.l.<></td></d.l.<>	<d.l.< td=""><td><b.v.< td=""><td><d.l.< td=""><td>-</td><td>-</td><td>-</td><td><d.l.< td=""><td><d.l.< td=""><td>-</td><td>1.4</td><td>7.3</td></d.l.<></td></d.l.<></td></d.l.<></td></b.v.<></td></d.l.<>	<b.v.< td=""><td><d.l.< td=""><td>-</td><td>-</td><td>-</td><td><d.l.< td=""><td><d.l.< td=""><td>-</td><td>1.4</td><td>7.3</td></d.l.<></td></d.l.<></td></d.l.<></td></b.v.<>	<d.l.< td=""><td>-</td><td>-</td><td>-</td><td><d.l.< td=""><td><d.l.< td=""><td>-</td><td>1.4</td><td>7.3</td></d.l.<></td></d.l.<></td></d.l.<>	-	-	-	<d.l.< td=""><td><d.l.< td=""><td>-</td><td>1.4</td><td>7.3</td></d.l.<></td></d.l.<>	<d.l.< td=""><td>-</td><td>1.4</td><td>7.3</td></d.l.<>	-	1.4	7.3
S1	MGO	Lab 2	PM2.5	2.3	0.007	0.015	0.20	0.17	2.8	1.0	0.16	<b.v.< td=""><td><b.v.< td=""><td>0.047</td><td>0.9</td><td>8.4</td></b.v.<></td></b.v.<>	<b.v.< td=""><td>0.047</td><td>0.9</td><td>8.4</td></b.v.<>	0.047	0.9	8.4
S1	Rel. uc.	HFO 1%		3.6%	3.8%	3.7%	4.0%	42.9%	17.9%	9.9%	8.8%	11.1%	-	11.9%	14.1%	5.3%
S2	Rel. uc.	HFO 1%,	0.5%	3.6%	5.5%	4.1%	12.5%	>100%	45.7%	44.0%	25.6%	20.8%	-	-	37.6%	11.0%
S1	Rel. uc.	MGO		4.2%	-	-	20.5%	40.8%	13.0%	14.0%	52.0%	-	-	>100%	7.7%	4.5%
S2	Rel. uc.	MGO		5.0%	48.1%	87.1%	>100%	>100%	-	-	43.3%	-	-	-	41.5%	14.1%
S1, S2	Mean CV	HFO 1%		15.2%	12.2%	10.1%	14.9%	78.5%	47.1%	31.8%	19.0%	20.1%	141.4%	19.3%	31.4%	16.8%

Table S4. Sample Pearson correlation coefficients r for emission factors for elements measured by EDXRF on filter samples and for EF(PM mass) measured on the same samples. Three groups with high correlation are marked with different colours. Correlation is based on 15 samples, in the magenta group only 5-6 pairs had both masses above the detection limit.

	S	V	Ni	Fe	Cr	Mg	Al	Si	Co	Zn	Ca	PM
S	1	0.752	0.773	0.628	0.493	0.013	0.441	0.802	0.436	-0.056	0.331	0.683
V		1	0.947	0.958	0.784	0.587	0.804	0.947	0.703	0.470	0.500	0.899
Ni			1	0.908	0.617	0.393	0.697	0.882	0.558	0.449	0.397	0.925
Fe				1	0.863	0.662	0.905	0.961	0.449	0.490	0.537	0.876
Cr					1	0.902	0.986	0.804		0.604	0.747	0.696
Mg						1	0.847	0.500		0.755	0.834	0.442
Al							1	0.765	-0.843	0.674	0.773	0.703
Si								1		0.555	0.652	0.869
Co									1	0.863	0.500	0.473
Zn										1	0.946	0.383
Ca											1	0.301

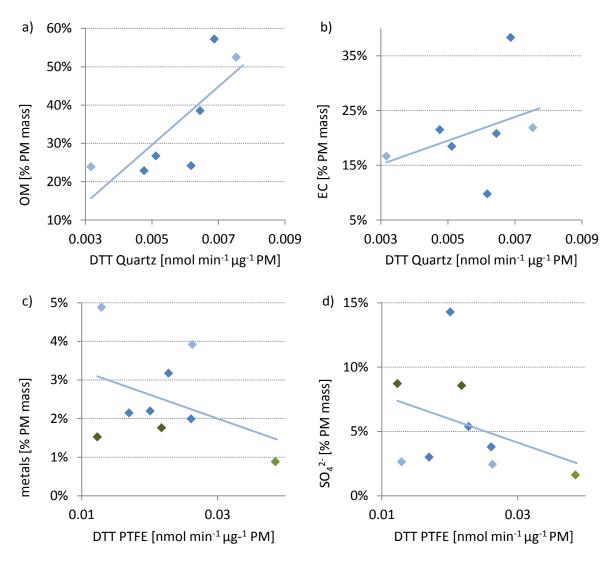



Figure S4. Relative contributions of PM compounds to PM mass (in wt%) plotted against oxidative potential measured on quartz (a, b) and PTFE (c, d) filter samples. a - OM, b - BC, c - metals analysed with EDXRF, d – sulphate calculated from S analysed by EDXRF. Color coding of points: dark blue – HFO fuel, S1, light blue – MGO fuel S1, dark green – HFO fuels S2, light green – MGO fuel S2.









Figure S5. Size distribution of primary soot-type particle and its lognormal fit (solid line) for a - S1_HFO1%_ME-full experiment (based on 502 images) and b - S1_MGO_AE experiment (based on 477 images)

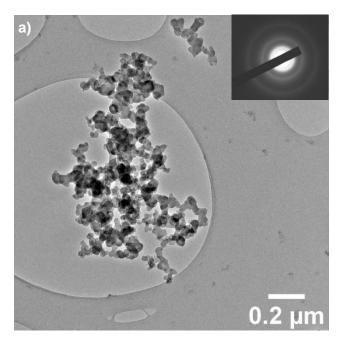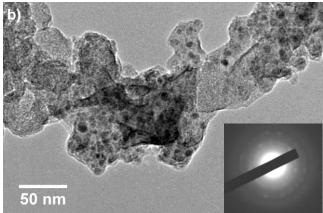

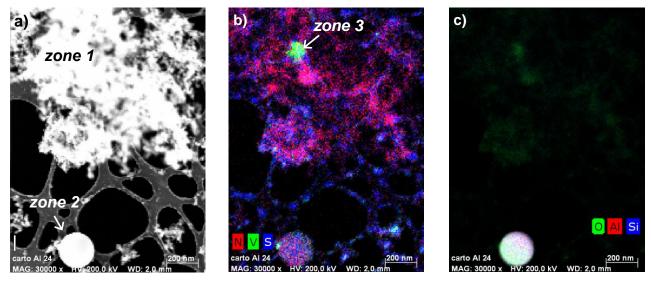

Figure~S6.~a-transmission~electron~microscopy~(TEM)~picture~of~a~small~soot-type~aggregate~and~its~corresponding~SAED~pattern,~b-zoom~on~soot-type~particles~with~dark~dots~and~its~associated~SAED~pattern



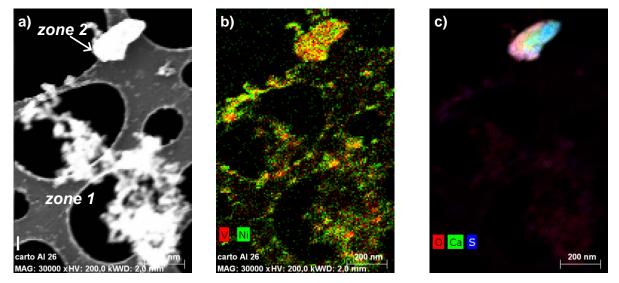


Figure S8. a – STEM image of a soot agglomerate (zone 1) and a char-mineral particle (zone 2) from the $S1_HFO1\%_ME$ -full experiment. Composition of the soot agglomerate: C 76.8 wt%, N 17.2 wt%, O 5.9 wt%, traces of V, Ca and S (about 0.1 wt% of each element). b, c – elemental composition map for V and Ni (b) and for O, Ca and S (c) of particles in a.

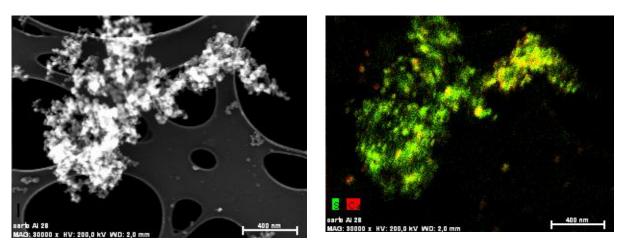


Figure S9. a-STEM image of a soot agglomerate collected in S1_MGO_AE experiment. b- elemental composition map for Ca, and S of the soot agglomerate in a.

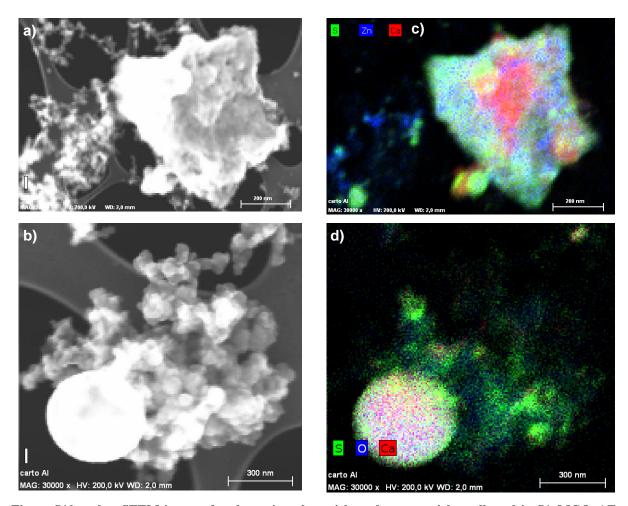


Figure S10. a, b – STEM image of a char-mineral particle and soot particles collected in S1_MGO_AE experiment. Composition of the char-mineral particle in a: C 66.5 wt%, O 24.8 wt%, Ca 7.8 wt%, S 0.7 wt%, P 0.2 wt%; Composition of the char-mineral particle in b: C 73.3wt%, O 24.3 wt%, Ca 2.1 wt%, S 0.3 wt%. c – elemental composition map for Ca, S and Zn of particles in a. d – elemental composition map for Ca, S and O of particles in b.

a) b)

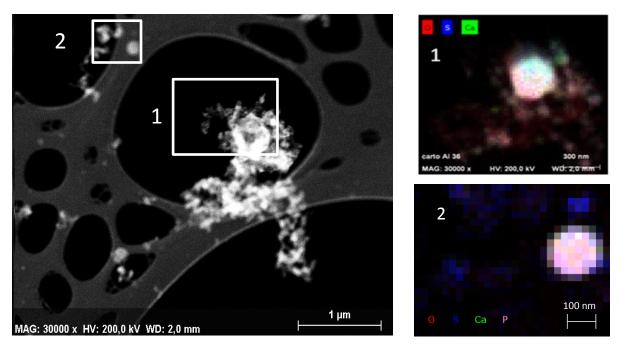


Figure S11. a - STEM image of soot agglomerates with a large (\sim 500 nm) char-mineral particle (zone 1) and smaller char-mineral particle (zone 2). Composition of char-mineral particle in zone 1: C 58.4 wt%, O 35.1 wt%, Ca 3.7 wt%, S 2.8 wt%; composition in zone 2: C 51.7 wt%, O 39.8 wt%, Ca 5.6 wt%, P 2.9 wt% and S 0.1 wt%. The small particles have traces of S only. b - elemental composition map corresponding to the zone 1 (O, S, Ca) and zone 2 (O, S, Ca, P) in a.

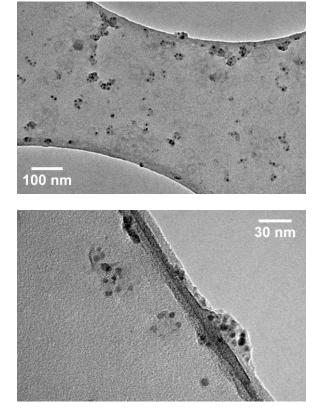


Figure S12. TEM image of organic particles.

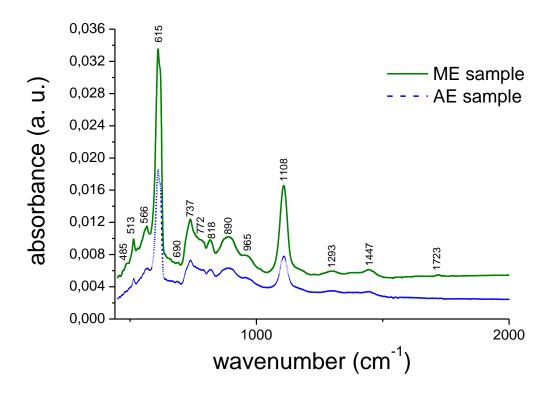


Figure S13. FTIR spectra of PM sampled in auxiliary engine (AE) and main engine (ME) exhaust. Peaks at 485 and 818 cm⁻¹ are linked to the presence of aromatic ring vibrations, medium peaks at 737, 772, 818, 890 cm⁻¹ to C-H out of plane vibrations in aromatics compounds (Socrates, 2004). A weak peak at 1723 cm⁻¹ is probably due to C=O in ketone, ester, anhydride or aldehyde (DEAN'S, 2004). Medium peaks at 513 and 965 cm⁻¹ are due to V-O vibration of the vanadium oxide V_2O_5 (Botto et al., 1997, Clauws et al., 1985), medium peak at 566 cm⁻¹ and its shoulder at 558 cm⁻¹ come from Fe-O vibration of the iron oxide Fe₃O₄ (Namduri et al., 2008). The very strong peak at 615 cm⁻¹, its shoulder at 620 cm⁻¹ and a weak peak at 690 cm⁻¹ come from the C-S stretching of sulphide compounds (DEAN'S, 2004). The very strong peak at 1108 cm⁻¹ indicates the symmetric stretch of SO₂ in sulfone, C=S vibrations of thiocarbonyl compounds or C-O-C asymmetric stretch (DEAN'S 2004; Socrates, 2004). A weak peak at 1293 cm⁻¹ are probably linked to C-N stretching in aromatic aryl-NH₂ compounds (DEAN'S, 2004). A weak peak at 1447 cm⁻¹ can correspond to C-N-H bending in amide compounds (DEAN'S, 2004) or ammonium ion NH₄⁺ (Maria et al., 2002).

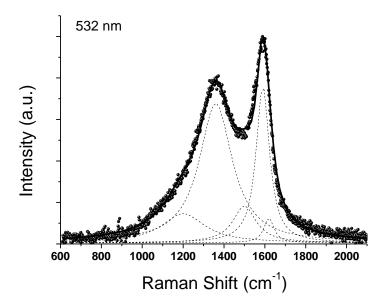


Figure S14. Raman spectra of the cumulative S1_MGO1%_ME sample. Five bands are identified (Sadezky et al., 2005): G, D_1 , D_2 , D_3 , and D_4 . The G band (1580 cm⁻¹) corresponds to the E_{2g} symmetry mode of the graphite lattice. The D_1 band (1350 cm⁻¹) originates from A_{1g} symmetry mode in disordered graphite; D2 band (1620 cm⁻¹) - from E_{2g} symmetry stretching mode of disordered graphite; D_3 band (1500 cm⁻¹) is related to amorphous carbon (a mixture of sp² and sp³); and D_4 band (1200 cm⁻¹) is assigned to A_{1g} symmetry mode of disordered graphite.