

Supplement of Atmos. Meas. Tech., 7, 2829–2838, 2014
<http://www.atmos-meas-tech.net/7/2829/2014/>
doi:10.5194/amt-7-2829-2014-supplement
© Author(s) 2014. CC Attribution 3.0 License.



Supplement of

The influence of temperature calibration on the OC–EC results from a dual-optics thermal carbon analyzer

J. Pavlovic et al.

Correspondence to: J. S. Kinsey (kinsey.john@epa.gov)

1 **Supplemental Information**

2 **The influence of temperature calibration on the OC-EC results from a Dual Optics Thermal Carbon**
3 **Analyzer**


4 **Jelica Pavlovic^a, John S. Kinsey^{b*}, and Michael D. Hays^b**

5 ^a Oak Ridge Institute for Science and Education, Oak Ridge, TN 37831, USA

6 ^b U.S. Environmental Protection Agency, Office of Research and Development, National Risk Management
7 Research Laboratory, Research Triangle Park, NC 27711, USA

8

9

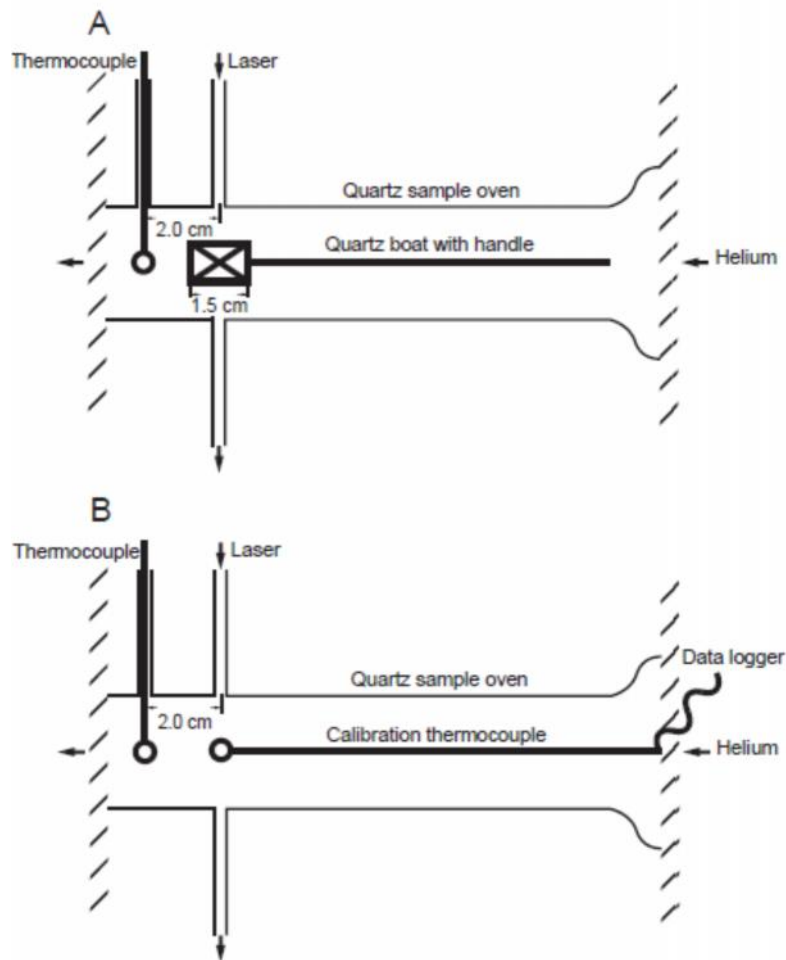

10

11 Figure S1. The sample analysis set (A) and calibration set (B) of the Sunset Laboratory Carbon Analyzer.
12 *Note the position of the oven temperature sensor relative to the filter sample.*