



Supplement of

High-resolution continuous-flow analysis setup for water isotopic measurement from ice cores using laser spectroscopy

B. D. Emanuelsson et al.

Correspondence to: B. D. Emanuelsson (daniel.emmanuelsson@vuw.ac.nz)

The copyright of individual parts of the supplement might differ from the CC-BY 3.0 licence.

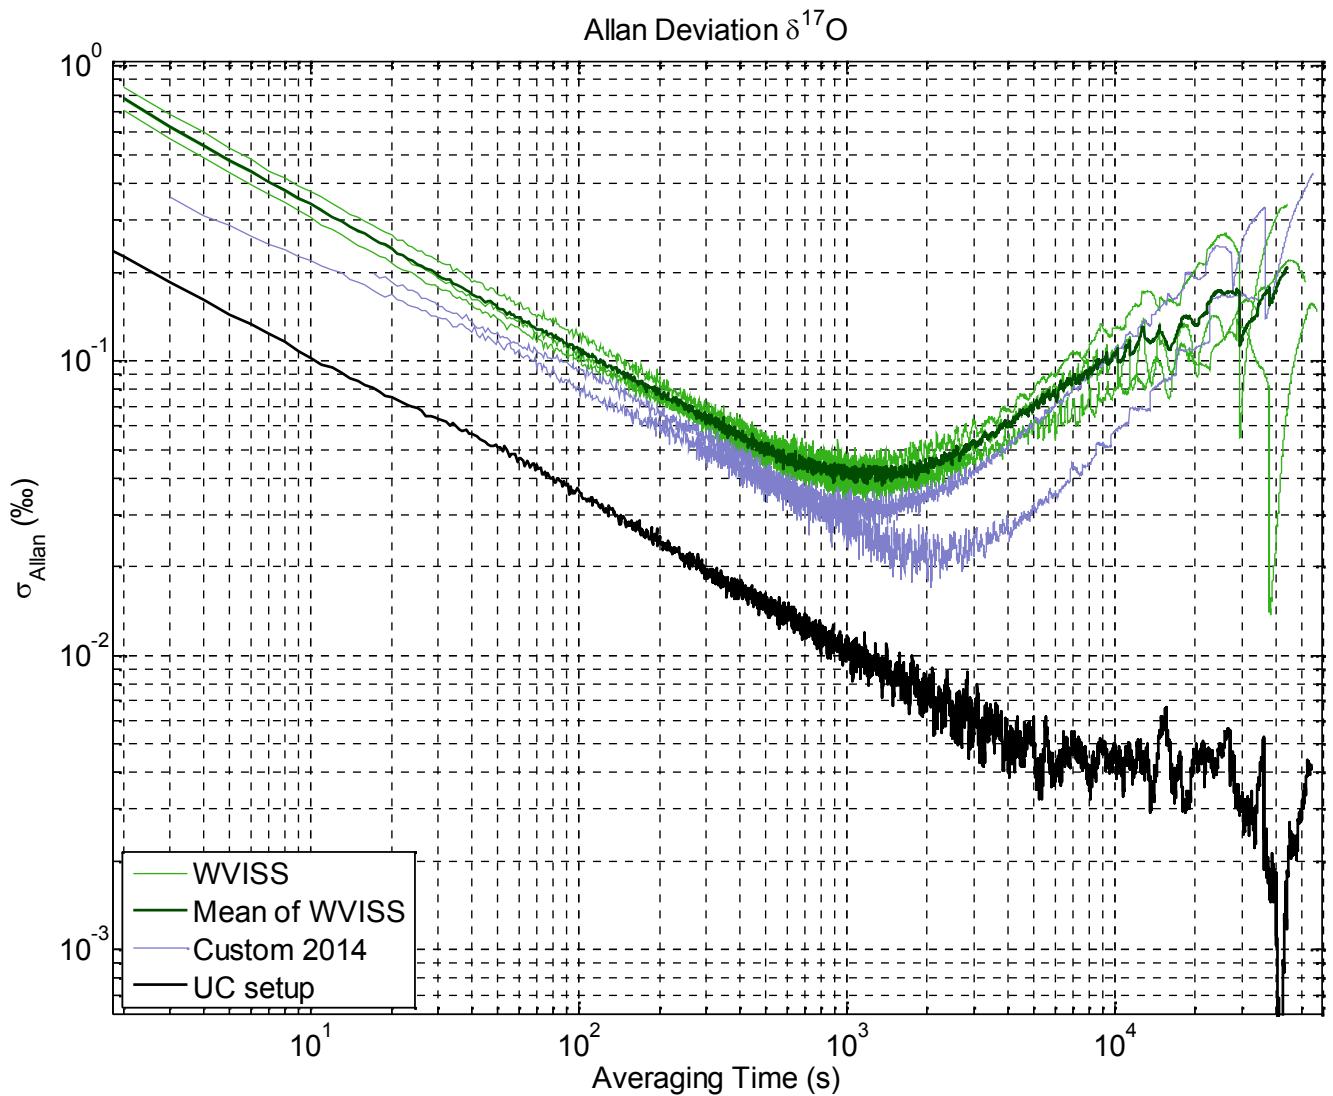


Figure S1. Allan deviation as a function of averaging time for ^{17}O for stability tests on the WVISS (green lines), the custom 2014 (blue lines) and from the UC setup (black line).

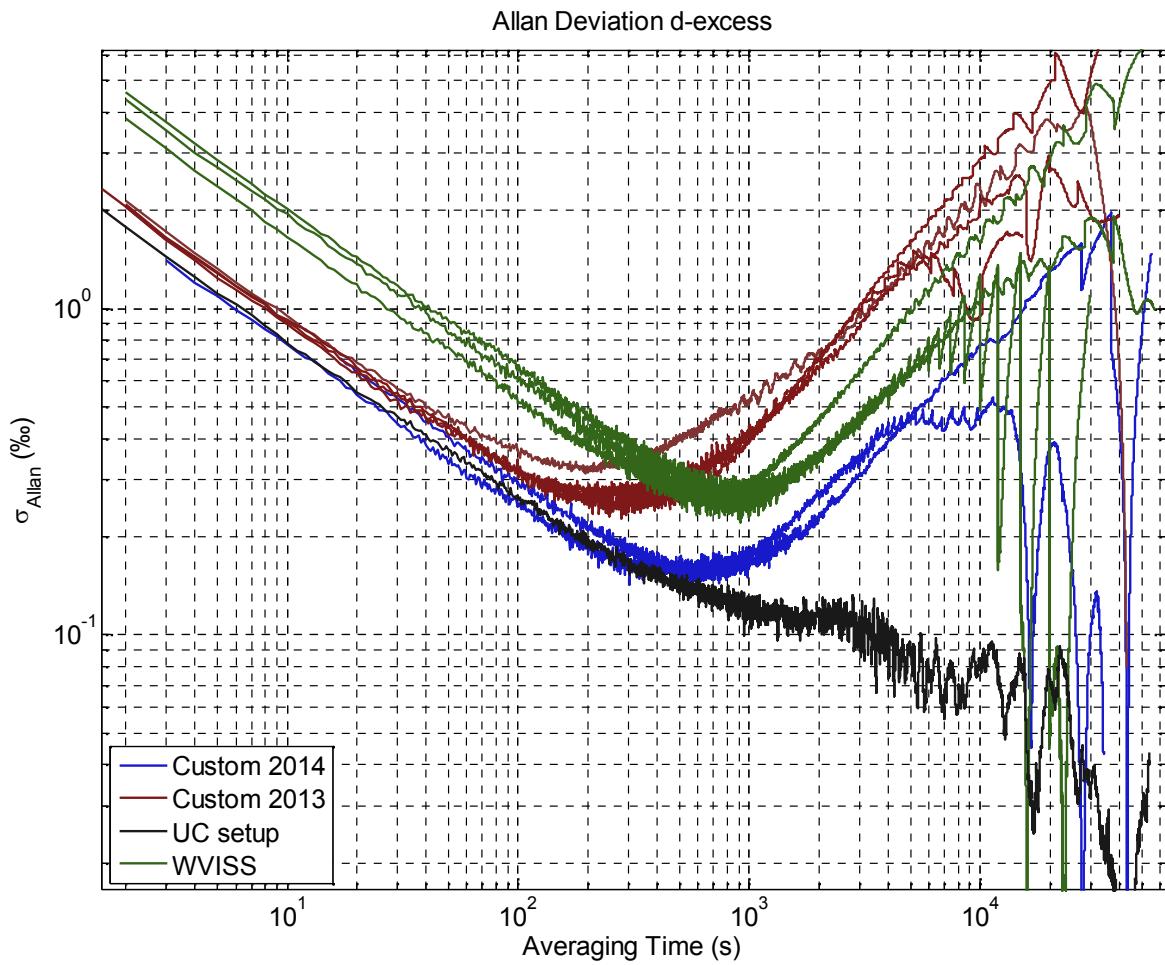


Figure S2. Allan deviation as a function of averaging time for d-excess for stability tests on the custom setups (2013 brown lines and 2014 blue lines), the WVISS (green lines), and from the UC setup (black line).