

Atmospheric Measurement Techniques Discussions is the access reviewed discussion forum of *Atmospheric Measurement Techniques*

Inter-comparison of NH₃ measurement techniques

K. von Bobruzski et al.

Field inter-comparison of eleven atmospheric ammonia measurement techniques

K. von Bobruzski^{1,2}, C. F. Braban¹, D. Famulari¹, S. K. Jones¹, T. Blackall³,
T. E. L. Smith³, M. Blom⁴, H. Coe⁵, M. Gallagher⁵, M. Ghalaieny⁵, M. R. McGillen⁵,
C. J. Percival⁵, J. D. Whitehead⁵, R. Ellis⁶, J. Murphy⁶, A. Mohacsi⁷,
H. Junninen⁹, A. Pogany⁸, S. Rantanen⁹, M. A. Sutton¹, and E. Nemitz¹

¹Centre for Ecology & Hydrology, Edinburgh, UK

²Leibniz-Institute for Agricultural Engineering, Potsdam, Germany

³Department of Geography, King's College London, London, UK

⁴Energy Research Foundation of the Netherlands, Petten, The Netherlands

⁵School of Earth, Atmospheric and Environmental Science, University of Manchester, Manchester, UK

⁶Department of Physics, University of Toronto, Toronto, Canada

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



⁷ Research Group on Laser Physics of the Hungarian Academy of Sciences,
Budapest, Hungary

⁸ Department of Optics and Quantum Electronics, University of Szeged, Szeged, Hungary

⁹ Department of Physics, University of Helsinki, Helsinki, Finland

Received: 2 July 2009 – Accepted: 19 July 2009 – Published: 4 August 2009

Correspondence to: E. Nemitz (en@ceh.ac.uk)

Published by Copernicus Publications on behalf of the European Geosciences Union.

AMTD

2, 1783–1835, 2009

Inter-comparison of NH₃ measurement techniques

K. von Bobruzski et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Abstract

Eleven instruments for the measurement of ambient concentrations of atmospheric ammonia gas (NH_3), based on eight different measurement methods were inter-compared above an intensively managed agricultural field in late summer 2008 in S. Scotland. To test the instruments over a wide range of concentrations, the field was fertilised with urea midway through the experiment, leading to an increase in the average concentration from 10 to 100 ppbv. The instruments deployed included three wet-chemistry systems, one with offline analysis (annular rotating batch denuder, RBD) and two with online-analysis (Annular Denuder sampling with online Analysis, AMANDA; AiRRmonia), two Quantum Cascade Laser Absorption Spectrometers (a large-cell dual system, DUAL-QCLAS, and a compact system, c-QCLAS), two photo-acoustic spectrometers (WaSul-Flux, Nitrolux-100), a Cavity Ring Down Spectrometer (CRDS), a Chemical Ionisation Mass Spectrometer (CIMS), an ion mobility spectrometer (IMS) and an Open-Path Fourier Transform Infra-Red (OP-FTIR) spectroscopy. Each instrument was compared with each other and with the average concentration of all instruments. An overall good agreement of hourly average concentrations between the instruments ($R^2 > 0.84$), was observed for NH_3 concentrations at the field of up to 120 ppbv with the slopes against the average ranging from 0.67 (DUAL-QCLAS) to 1.13 (AiRRmonia) with intercepts of -0.74 ppbv (RBD) to $+2.69$ ppbv (CIMS). More variability was found for performance for lower concentrations (< 10 ppbv). Here the overruling factors affecting measurement precision are (a) the inlet design, (b) the state of inlet filters (where applicable), and (c) the quality of gas-phase standards (where applicable). By reference to the fast (1 Hz) instruments deployed during the study, it was possible to characterize the response times of the slower instruments.

AMTD

2, 1783–1835, 2009

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



1 Introduction

Ammonia (NH_3) plays an important role in atmospheric chemistry. It represents the major alkaline gas and is therefore important for the neutralization of acidic gases and the formation of particulate matter (Duyzer et al., 1994; Asman et al., 1998). Deposition of atmospheric NH_3 to ecosystem can lead to effects such as eutrophication and acidification of soils, contributing to forest decline and a decrease in biological diversity (Fangmeier et al., 1994; Sutton et al., 1995; Ferm, 1998). As a consequence, many measurement methods for NH_3 have been developed. Ambient measurement of NH_3 concentrations is difficult due to several factors: ambient levels vary widely, from 5 pptv in remote regions (Janson et al., 2001; Sutton et al., 2001) to 500 ppbv near sources (Krupa, 2003). Ammonia occurs in gaseous, particulate and liquid phases which add further complexity to its measurement (Warneck, 1988), since the measurement technique should be specific to the gas-phase and not modify the gas-aerosol equilibrium which depends on environmental conditions (Mozurkewich, 1993). In addition, NH_3 is “sticky” and interacts with surfaces of materials, often leading to slow inlet response times (Yokelson et al., 2003). Finally, NH_3 is emitted by people, increasing the potential for sample contamination (Sutton et al., 2000b).

Currently, bulk denuder techniques are the most widely used method for sampling NH_3 and operate by stripping the gas phase NH_3 from the air stream (Ferm, 1979; Keuken et al., 1988). The main disadvantages of this manual sampling method are the low temporal-resolution, and when high-frequency measurements (e.g., hourly) are needed, the manpower required becomes considerable. Moreover, the manual handling, including sample preparation, wet-chemical analysis and sample storage, increase the chances of sample contamination. In the 1980s systems were developed, based on wet effluent diffusion denuder (WEDD) techniques, to collect stripping solution at regular intervals into test tubes (e.g., Keuken et al., 1988), this automated the process of sample preparation and extraction, while still retaining the need for manual off-line analysis. In a next step, in the 1990s these WEDDs and mist chambers were

AMTD

2, 1783–1835, 2009

Inter-comparison of NH_3 measurement techniques

K. von Bobruzski et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



coupled to NH_4^+ online analysers in the field (Simon et al., 1991; Simon and Dasgupta, 1993; Wyers et al., 1993; Blatter et al., 1994; Erisman et al., 2001).

In parallel, spectroscopic techniques for NH_3 were developed, such as the use of chemiluminescence NO_x monitors with NH_3 converters (e.g., Breitenbach and Shelef, 1973), Differential Optical Absorption Spectroscopy (DOAS; Gall et al., 1991), Tunable Diode Laser Absorption Spectroscopy (TDLAS; Grisar et al., 1987; Warland et al., 2001) and Fourier Transform Infra-Red spectroscopy (FTIR; Galle et al., 2000). While many of these techniques have been deployed successfully to measure concentrations and emissions downwind of strong sources, it has only been over the past 15 years that spectroscopic techniques have gradually become sufficiently sensitive and robust for field application at typical ambient concentrations (0.1 to 10 ppbv). Approaches more recently applied for ammonia measurements include photoacoustic spectroscopy (e.g. Harren et al., 2000; Pushkarsky et al., 2002), Chemical Ionization Mass Spectrometry (CIMS; e.g., Nowak et al., 2007; Norman et al., 2007), quantum cascade laser absorption spectrometers (QCLAS; e.g., McManus et al., 2002) and Ion Mobility Spectrometry (IMS; e.g., Myles et al., 2006).

Some experiments have been carried out to compare NH_3 measurement techniques. Wiebe et al. (1990) reported a test of four methods: FTIR, filter-pack, denuders (simple and annular) and a transition flow reactor. Williams et al. (1992) conducted an inter-comparison of five instruments: a photofragmentation/laser-induced fluorescence (PF/LIF) instrument, a molybdenum oxide annular denuder sampling/chemiluminescence detection (MOADS) system, a tungsten oxide denuder sampling/chemiluminescence detection (DARE) system, a method based on citric acid coated denuder sampling coupled with ion chromatographic analysis (CAD/IC), and a method using an oxalic acid coated filter pack sampling coupled with colorimetric analysis (FP/COL). For selection within the Netherlands National Air Quality Monitoring Network (NAQMN) six analysers were studied by Mennen et al. (1996): a wet-annular rotating denuder, a WO_3 -coated thermodenuder, a V_2O_5 -coated thermodenuder, a DOAS system, a photoacoustic monitor and a chemiluminescence NO_x monitor with

Inter-comparison of NH_3 measurement techniques

K. von Bobruzski et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

NH₃ converter. In addition, there were smaller inter-comparisons between two instruments: a field study on Tenerife by Milford et al. (2000) included an AMANDA instrument (see below) and a diffusion scrubber flow injection analyzer (DS-FIA). Fehsenfeld et al. (2002) reported a comparison of a CIMS with a citric acid denuder and a molybdenum oxide (MoO_x) converter. Nowak et al. (2006) compared two different CIMS instruments in the field: a NOAA chemical Science Division (NOAA-CSD) apparatus and the Georgia tech (GT) low pressure reactor.

The development of new continuous measurement approaches has motivated two major inter-comparison campaigns in recent years: a laboratory inter-comparison of gaseous NH₃ with seven instruments were performed by Schwab et al. (2007): a TD-LAS, a wet scrubbing long-path absorption spectrometer (LOPAP), a WEDD system, an IMS, a photo-acoustic absorption analyzer, and a modified chemiluminescence analyzer. The emphasis of this short inter-comparison was on the accuracy and time-response of these approaches under laboratory conditions while sampling from a common manifold. In addition, Norman et al. (2009) realised an inter-comparison of three instruments at a Swiss grassland site: a modified Proton Transfer reaction Mass Spectrometer (PTR-MS; Norman et al., 2007) and two wet chemistry techniques, based on a horizontal denuder technique (GRAEGOR; Thomas et al., 2009), and a diffusion membrane sampler (AiRRmonia; Erisman et al., 2001). Further, Whitehead et al. (2008) made measurements between a QCLAS, a TDLAS and an AMANDA instrument.

The work presented here included eight different atmospheric NH₃ measurement methods implemented in eleven different instruments, focussing on comparison of the techniques under typical field conditions. Ammonia was measured over intensively managed grassland in Scotland, between 20 August and 4 September 2008. The field was fertilised on 28 August 2008 to stimulate emission from the field and test the instrumentation over a wide concentration range, including regimes that are typical for moderately agricultural mixed land use and also near-sources. The aim was to assess instrument performance and characterise the instrument response times. In addition to the description of time series, we used regression analyses for concentrations over the

Inter-comparison of NH₃ measurement techniques

K. von Bobruzski et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

entire concentration range and, separately, below 10 ppbv to assess the performance at low concentrations in more detail. Three of the instruments were also used for micrometeorological flux measurements based either on the flux gradient technique (AMANDA, WaSul-Flux or eddy-covariance (DUAL-QCLAS), but these results will be presented elsewhere.

2 Methodology

2.1 Site description

The measurements were made at a micrometeorological field site in southern Scotland (55°52' N, 3°2' W, 190 m a.s.l.) on an intensively managed grassland area (Easter Bush), located about 1 km to the west of the Pentland Hills with peaks of up to 500 m (see Milford et al., 2001; Whitehead et al., 2008). The Easter Bush site is divided into two fields, each approximately 5 ha, more than 90% of which is covered by *Lolium perenne* (perennial ryegrass). The dividing line between the fields runs NW to SE, and in the following analysis the fields to the NE and SW of the measurement equipment are referred to as N field and S field, respectively. The Pentland Hills channel the wind so that on average 60% of the wind comes clearly from the S field and 19% clearly from the N field (Milford et al., 2001). Both fields receive the same management and have been used for cattle and sheep grazing in recent years. Easter Bush is an intensive flux monitoring site of the NitroEurope IP measurement programme (Sutton et al., 2007) and has hosted several studies on NH₃ flux measurements (Milford et al., 2001; Whitehead et al., 2008). The inter-comparison experiment took place from 20 August to 4 September 2008 with the instruments placed on the boundary between the two fields (Fig. 1). All instruments were deployed with an inlet height of 1.1 m above ground, with the exception of the DUAL-QCLAS (1.95 m), as this was also used for eddy-covariance flux measurements.

Inter-comparison of NH₃ measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Fertilisation took place on 28 August 2008 on both the N and S field, with 35 kg N ha^{-1} in the form of urea.

2.2 Environmental conditions during the field experiment

Figure 2 presents the time series of hourly data of precipitation, temperature and relative humidity. The wind direction and speed are represented by the direction and length of the arrows respectively. The mean wind speed was around 3 m s^{-1} . Several rain events occurred during the campaign with the maximum amount being 4.9 mm h^{-1} on 20 August 2008. There was no rain during the fertilisation on 28 August 2008 and therefore no NH_3 was washed into the ground immediately after fertilisation (see Sect. 3.1). The relative humidity never decreased below 58%. The mean temperature was 12.8°C . Overall August 2008 was wet in eastern Scotland, receiving about twice as much rainfall compared with the long-term average (mean since 1961; values for Leuchars; Eden, 2008). This high level of precipitation led to the formation of a “pond” near to the measurement site in the N field. Although the accumulating water was pumped away on several occasions, the associated rotting vegetation is likely to have created an additional and heterogeneous NH_3 source near the instruments, for NE wind directions. The few occurrences of this wind direction were therefore excluded from the regression analysis presented below.

Figure 2 also includes a time-series of NH_4^+ aerosol in $\text{PM}_{2.5}$ measured with a MARGA instrument, similar to GRAEGOR (Thomas et al., 2009), except that it deploys online cation analysis rather than FIA and a $\text{PM}_{2.5}$ inlet cyclone, at the Auchencorth EMEP site, 10 km south of Easter Bush. From previous simultaneous measurements, there is close ($\pm 20\%$) agreement between NH_4^+ concentrations at Auchencorth and Easter Bush. This time-series is included because it is possible that some of the NH_3 measurement techniques deployed here may show some cross-sensitivity to NH_4^+ aerosol. NH_4^+ concentrations were below $1 \mu\text{g m}^{-3}$ except for 30 and 31 August 2008.

Inter-comparison of NH_3 measurement techniques

K. von Bobruzski et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



2.3 Measurement techniques

The characteristics of the ammonia measurement systems deployed in the inter-comparison are summarised in Table 1, and can be described as followed:

2.3.1 Wet-chemistry analysers

- Two of three wet chemistry instruments deployed (RBD, AMANDA) are based on the denuder principle described by Ferm (1979), whereby gas phase NH_3 is stripped from the air stream through diffusion to the denuder glass walls, without collecting the NH_4^+ aerosol phase, since gas molecules diffuse quicker than particles to a moistened/acidified tube wall. In a third instrument (AiRRmonia), a diffusion membrane was used to strip the gas phase from the air stream. All three instruments were developed by the Energy Research Foundation of the Netherlands (ECN, Petten, NL). The instruments were housed in weather proof enclosures and placed at the measurement height, with inlets of <0.1 m length.

Annular Rotating Batch Denuder (RBD)

- In the RBD instrument (Keuken et al., 1988), air is pumped at 27 l min^{-1} through the annulus formed by two horizontal concentric rotating glass tubes (with a diameter of 45 mm), which is wetted with a thin layer of collecting liquid (specify the solution). Ammonia is absorbed into this thin layer of collection solution over a sampling time of 40 min within each hour, after which the sample (10 to 15 ml) is pumped off to an autosampler holding 20 ml test tubes. The collecting solution contains 2.0 g l^{-1} NaOH, 3.4 ml l^{-1} $>98\%$ formic acid and 0.5 mg l^{-1} thymol as biocide. All samples were analysed for NH_4^+ offline on an Ammonia Flow Injection Analyser (AMFIA, ECN, Petten, NL), based on analysis by selective ion membrane and conductivity measurement (Genfa and Dasgupta, 2000). For analysis, 0.5 M NaOH solution is added to the sample, resulting in the conversion of NH_4^+ to gas-phase $\text{NH}_{3(g)}$ in solution. As the solution then

Inter-comparison of NH_3 measurement techniques

K. von Bobrutzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



passes a semi-permeable Teflon membrane, $\text{NH}_{3(g)}$ permeates the membrane and is dissolved in a counter stream of deionised water. Then NH_3 is re-ionised to NH_4^+ and is detected by conductivity (Sutton et al., 2000a; Erisman et al., 2001; Milford et al., 2001). This technique is precise and reasonably specific, but it has been shown to be somewhat cross-sensitive to selected amines at high concentrations (Husted et al., 2000). In addition to NH_3 it is possible to use the RBD to capture other water soluble inorganic trace gases like HNO_3 , HCl , SO_2 and H_2O_2 (Keuken et al., 1988), which would need to be quantified by a different analytical technique such as anion chromatography.

AMANDA

The technique of Ammonia Measurement by ANnular Denuder sampling with online Analysis (AMANDA) was developed by Wyers et al. (1993). The system used here consists of three annular wet rotating denuder inlets, similar to that used in the RBD, located at different heights (0.39 m, 1.07 m, and 2.20 m). Unlike in the RBD, however, the stripping solution (0.5 g l^{-1} NaHSO_4 containing 0.2 ml l^{-1} 37% HCHO as a biocide) is continuously pumped from the denuders to a common detector block, where the three concentrations are analysed sequentially by the same selective ion membrane/conductivity technique as deployed in the AMFIA. In the denuders a constant liquid level is maintained by the use of an independent peristaltic pump, controlled by a conductivity measurement along the denuder. This particular instrument has been upgraded with a newer detection block, using two conductivity measurements. One conductivity cell monitors the initial conductivity of the deionised water, while a second conductivity cell monitors the NH_4^+ content after the membrane exchange. The difference in both readings of the conductivity cells is a measure for the original NH_3 content in the sampled air. This approach takes into account changes in the water quality during longer service intervals. The instrument reports one concentration gradient every 7.5 min, but the overall instrument response time is limited by the exchange of the stripping solution within the denuder (see Sect. 3.3 below).

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



The AiRRmonia is a further development of the AMANDA technique. As with the AMANDA, it was originally developed by ECN (Energy Research Centre of the Netherlands, Petten, NL), but has been further improved and commercialised (Mechatronics Instruments b.v., Hoorn, NL) to provide a sensitive, easy-to-use NH₃ monitor (Erisman et al., 2001). Unlike the RBD and AMANDA, the instrument uses a Teflon membrane to strip the NH₃ from the airflow into a deionised water flow. The detection system of NH₃ is similar to that of the AMANDA, also using the double conductivity measurement. Precision and stability of this instrument are further improved through the use of syringe pumps for reagents and solutions, which undergo less variation due to changes in pump tubing and temperature than the peristaltic pumps used in the AMANDA. The AiRRmonia inlet consists of stainless steel with a length of 5 cm and a diameter of 1/8".

2.3.2 Quantum cascade laser absorption spectroscopy (QCLAS)

QCLAS is an infrared absorption technique that makes use of the rich spectral absorption region in the mid-infrared, in which most species of interest in the atmosphere have resolvable absorption features. Both laser systems used here were produced by Aerodyne Research Inc. (Billerica, MA, USA), and operate with the light source of a thermoelectrically cooled pulsed Quantum Cascade (QC) laser (Alpes Lasers, Neuchatel, Switzerland). Their design was similar to the closed path configuration described by McManus et al. (2002). These lasers scan over a narrow range of wave numbers chosen to contain an absorption feature of the trace gas of interest, which for ammonia is at a wavelength of 10.3 μm. Both instruments use astigmatic Herriott multipass absorption cells, to increase the effective path length, while providing a fast spot measurement.

In the data acquisition protocol chosen for this study, the spectra were recorded and averaged over the data acquisition time of one second, with the resulting spectra fitted to known spectral line profiles from the HITRAN (High-resolution TRANsmission)

Inter-comparison of NH₃ measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



molecular spectroscopic database (Rothmann et al., 1998). In principle, this approach provides an absolute measurement.

DUAL-QCLAS

The DUAL-QCLAS uses two separate thermoelectrically cooled pulsed Quantum Cascade (QC) lasers for the potential measurement of two trace gases at different wave lengths. The two beams are brought together (with the pulses separated in time) and directed into either one of two astigmatic Herriott multipass absorption cells where they undergo 238 reflections, before leaving the cell and arriving at a cryogenically cooled HgCdTe infrared detector. The large (5 l) cell provides an effective path length of 210 m, while the small (0.3 l) cell provides a path length of 56 m. The large cell is used for higher precision measurement applications whilst the small cell (used here) provides the fast time response required for eddy covariance flux measurements. Data were recorded at a rate of 5 Hz to be averaged up later for the purpose of the concentration inter-comparison reported here. Background measurements were made typically every 15 min and background spectra were subtracted from the measurements prior to the wave fit. For this purpose, NH₃ free air was generated using a customized Pd/AL₂O₃ catalyst heated to 300°C. The inlet was a 2 m length of 1/4 inch (OD) PFA tube, which was co-located with an ultrasonic anemometer (model HS; Gill Instruments Ltd., Lymington, UK) for the purpose of flux measurements. A general calibration factor of 1.23 was applied to the DUAL-QCLAS data based on the field based calibration. For more information and studies of the DUAL-QCLAS see Whitehead et al. (2008).

Compact QCLAS (c-QCLAS)

The c-QCLAS uses a single QC laser and a single cell with a volume of 0.5 l and an effective path length of 76 m. Air was drawn into the optical cell through a short (<0.1 m) quartz inlet that was heated to 40°C and coated with a hydrophobic siloxyl coating. The inlet contains a critical orifice that drops the pressure in the optical cell

Inter-comparison of NH₃ measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



to approximately 45 Torr while keeping a constant flow rate of approximately 9 l min^{-1} . The inlet employed a virtual impactor to separate particles inertially, while allowing the gases with the majority ($\sim 90\%$) of the flow to enter the optical cell. The quartz inlet was connected to the optical cell via $\sim 3\text{ m } 3/8''$ PFA tubing. Background measurements were performed every 30 min by flushing the quartz inlet using dry nitrogen. Standard addition calibrations were performed every two hours with a permeation tube standard, added either into ambient air or dry nitrogen.

2.3.3 Photoacoustic spectroscopy

Two instruments measured NH_3 concentration using photoacoustic spectroscopy. A light source is tuned to an absorption feature of the target species and molecules are excited to a higher quantum state. Modulating the light source results in a periodic temperature change, giving rise to a periodic pressure change that is an acoustic signal if the modulation frequency is in the acoustic range. The intensity of the acoustic signal, which can be detected by a sensitive microphone, is proportional to the concentration of the light-absorbing species (Harren et al., 2000).

Diode laser based photoacoustic system (WaSul-Flux)

This new instrument combines near-infrared photoacoustic spectroscopy with pre-concentration sampling as described in more detail elsewhere (Pogány et al., 2008). The instrument is built into a $19'' 6\text{ U}$ temperature controlled instrument box and has an additional waterproof housing. The photoacoustic detection unit consists of a fibre-coupled DFB diode laser light source (FOL15DCWD-A82-19560-A from Furukawa Inc.) with $\sim 40\text{ mW}$ output light power at 1532 nm , and an acoustically optimized photoacoustic cell with an electret microphone (Knowles, EK 3029) for measuring the photoacoustic signal. Ammonia is concentrated from the sampled air by a tungsten (VI) oxide coated preconcentration unit. The instrument has three gas inlets and is therefore suitable for measuring NH_3 concentration at three different heights above the ground. The

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



sampling lines were 6 m long Teflon tubes with 8 mm inner diameter, heated to $\sim 50^{\circ}\text{C}$ by self-regulating heating tape and included filters which were replaced weekly. The pre-concentration time can be adjusted to match the air concentrations. Here the integration time was varied between 15 and 45 min according to the actual concentration.

- 5 Before fertilization all three inlets were placed at the same height and the reported data are the averages of the three measurements. After fertilization, the inlets were operated in gradient configuration and the reported data represent the measurement of the middle height.

Nitrolux-100

- 10 The Nitrolux-100 (Pranalytica Inc., Santa Monica, CA, USA) is an ambient NH_3 analyser that uses resonant photoacoustic spectroscopy and a line-tunable CO_2 laser to provide continuous or on-demand measurements (Pushkarsky et al., 2003). The excited NH_3 molecules undergo collisional deactivation, which converts the absorbed energy into periodic local heating at the modulation frequency of the laser. The resulting
- 15 acoustic waves are detected with minimal interferences by other compounds at typical concentrations in a non-polluted atmosphere (Cowen et al., 2004). The instrument was originally developed for clean room applications in the semiconductor industry, but has been more widely used for ambient measurements. It is operated with an inlet filter to remove dust and NH_4^+ , with a manufacturer recommended lifetime of three months,
- 20 while the instrument should be calibrated by the manufacturer every six months. The Nitrolux-100 was operated with a 4 m $\frac{1}{4}$ " OD Teflon inlet which was insulated and heated to $\sim 35^{\circ}\text{C}$. The inlet was sheltered by an inverted plastic funnel.

2.3.4 Cavity Ring Down Spectroscopy (CRDS)

- 25 Cavity Ring Down Spectroscopy (CRDS) is a direct absorption technique, which uses pulsed or continuous light sources and has a significant higher sensitivity than other conventional absorption spectroscopy (Berden et al., 2000). The EnviroSense 1000

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Analyzer (Picarro Inc., Sunnyvale, CA, USA) monitors NH_3 in air using this approach. CRDS uses a pair of mirrors facing each other. A brief pulse of laser light is injected into the cavity, and it passes back and forth between the mirrors, while a fraction leaks through the mirror. Ammonia absorbs some of the light and thus the amount of light in the cavity decreases faster-it makes fewer passes. A CRDS setup measures how long it takes for the light to drop to a certain percentage of its original amount, and this “ringdown time” is used to calculate the concentration of the absorbing substance in the gas mixture in the cavity. Like the Nitrolux-100, the Picarro CRDS uses an inlet filter and is calibrated by the manufacturer. The CRDS was operated with a 4 m $1/4''$ OD Teflon inlet which was insulated and warmed with heating tape ($\sim 35^\circ\text{C}$). Again, the inlet was sheltered by an inverted plastic funnel. For detailed information see Rella (2008).

2.3.5 Chemical Ionisation Mass Spectrometry (CIMS)

Chemical Ionisation Mass Spectrometry (CIMS) techniques use ion-molecule reactions to selectively ionize and detect trace species of interest in ambient air with high sensitivity and fast time response. The CIMS method uses a reagent ion to ionise a neutral species, and the product ion resulting from this process is identified and quantified by a quadrupole mass analyser. The distinction between chemical ionization mass spectrometry and other mass spectrometry techniques is the use of ion molecule reactions for the selective ionization of compounds of interest in the complicated matrix of ambient air. In the system deployed here, NH_3 was detected using $\text{H}^+(\text{C}_3\text{H}_6\text{O})_2$ as a reagent ion (Marcy et al., 2005; Nowak et al., 2007). The configuration of the CIMS deployed here is described elsewhere (Hagg and Szabo, 1986; Slusher et al., 2004; Crounse et al., 2006; Huey et al., 2006; Neuman et al., 2006; Nowak et al., 2007). The instrument sampled air through a 0.1 m long $3/8''$ OD PFA inlet, temperature controlled to $40 \pm 1^\circ\text{C}$. Inlet flow was 19.5 l min^{-1} , with 0.88 l min^{-1} being subsampled through a pinhole into the ionization region, where reaction of NH_3 with $\text{H}^+(\text{C}_3\text{H}_6\text{O})_2$ proceeds. The instrumental signal was calibrated every hour using a standard addition from a calibrated permeation tube oven.

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



2.3.6 Ion mobility spectrometer (IMS)

Ion mobility spectrometers separate chemical substances on the basis of velocity of gas-phase ions in an electrical field (Eiceman and Karpas, 1994). Ions are introduced into an electrical field and the time of flight is measured. The sample molecules are first ionized by β -radiation from a ^{63}Ni source. The formation of positive ions is dominated by the proton-transfer reaction (Sunner et al., 1988) from water clusters to substances that have proton affinity higher than water (697 kJ mol^{-1}). This includes ammonia (854 kJ mol^{-1}). The charged ions are pulsed through a shutter grid into the drift region, where they are separated by mobility and detected at the end of the drift tube by an electrometer. The instrument is not very specific and the NH_3 measurement can suffer from the cross sensitivity of other compounds of similar mobility if they also have a proton affinity greater than water, while the quantification can be compromised by competing ion reactions. More details on the IMS technique are given in Hill et al. (1990) and Bacon et al. (1998). In this field study the commercial ion mobility spectrometer RAID I was used (Bruker Daltonik GmbH, Bremen, Germany). Sampling gas flow was 0.4 l min^{-1} and the sampling line was 2 m non-heated Teflon tubing. Heating was not applied to avoid contamination from the evaporation of NH_4^+ aerosols, although the response time to the concentration peaks might be improved with a heated sampling line.

2.3.7 Open-path Fourier Transform Infra-Red (OP-FTIR) Spectroscopy

Fourier Transform Infra-Red (FTIR) spectroscopy can be used to identify and quantify substances by their molecular absorption of infra-red radiation at specific wavelengths. An open-path configuration permits the estimation of path-integrated average concentrations of a gas species of interest over path lengths of up to 1 km. OP-FTIR has been shown to be a useful tool for the measurement of NH_3 from agricultural sources (e.g., Griffith and Galle, 2000). In the present study, a MIDAC M4401 portable FTIR spectrometer with Stirling cooled MCT detector module was used in conjunction with

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



a 20'' infra-red (IR) source in a bi-static open-path configuration (path length of 102 to 105 m). Both the FTIR spectrometer and IR source were aligned at 1.3 to 1.4 m above ground. The spectrometer was operated at a resolution of 0.5 cm^{-1} and eight sample scans were co-added for each spectrum.

5 Measured spectra were analysed for NH_3 using the NH_3 infra-red absorption features at 968 cm^{-1} and 932 cm^{-1} (accounting for interference by H_2O and CO_2 absorption). Concentration retrievals were performed using the MALT software (Griffith, 1996). MALT iteratively computes synthetic spectra (convolved to the spectrometer line shape) from the HITRAN absorption line database (Rothman et al., 1998) until the
10 mean-squared difference between the synthetic and measured spectra is minimised. The resultant concentrations used for the best-fit synthetic spectrum yield the path-integrated NH_3 (as well as H_2O and CO_2) mixing ratios (in ppbv) for the measured open-path.

2.4 Calibration and treatment of aerosol components

15 The wet chemistry instruments were calibrated weekly with individual liquid standards and a common liquid standard was run on all analytical systems. The CIMS and c-QCLAS were calibrated regularly with their own gas-phase standards. As noted above, the Nitrolux-100 and CRDS were calibrated by manufacturers and operated within the specified calibration intervals. The WaSul-Flux and IMS were calibrated by the operating groups prior to the campaign by comparison against wet-chemistry reference
20 systems.

An inter-comparison calibration (standard addition to ambient air) from a common NH_3 gas cylinder took place during the campaign. The concentration range and number of step increases varied between instruments. A similar calibration scheme is described in Schwab et al. (2007). For each instrument a calibration bias from a NH_3 gas
25 cylinder and a corresponding measured NH_3 concentration (gas std. bias) was calculated (see Table 2). This gas-phase measurement was used only as a check for most

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



instruments, except for the DUAL-QCLAS, for which it provided the primary calibration, yielding a calibration factor of 1.23.

As outlined in the instrument descriptions above, the wet chemistry systems strip the gas phase from the sample stream, while the aerosol phase passes through the sampling system. The c-QCLAS uses a virtual impactor to prevent most of the particles from entering the detection cell. The Nitrolux-100, CRDS and WaSul-Flux employ filters to prevent aerosol components from contaminating the detection cell. This has the potential to lead to artifacts due to aerosol dynamics on the filter. Indeed, the Nitrolux-100 was initially operated with a used filter and reported elevated NH_3 concentration levels compared with the other instruments (the deviation correlating with temperature), suggesting that the NH_3 originated from NH_4NO_3 volatilisation from the filter. Following replacement of this filter, the measurements Nitrolux-100 measurements were found to agree with the other techniques. The early data were therefore excluded from the data analysis. It appears that, for ambient measurements, the filters provided by the manufacturer have a much shorter lifetime than stated by the manufacturer. The stated lifetime is possibly more appropriate for the clean room applications for which the instrument had originally been developed.

3 Results

3.1 Time series analysis

Figure 3b and c shows the time series of measured NH_3 during the inter-comparison period of all instruments, measured at different temporal resolutions (1 min to 1 h). Different vertical scales were used to present the time series before and after the fertilisation on 28 August 2008. The NH_3 traces from the instruments at their individual time resolution (Table 1) are presented in two groups for increased clarity, separating wet chemistry analysers (Fig. 3b) and spectroscopic techniques (Fig. 3c). In addition, the wind direction is indicated in Fig. 3a. Before the fertilisation, there were brief NH_3

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



peaks in the time series of the DUAL-QCLAS and CIMS of up to 18 ppbv. Except for these individual events, the NH_3 level measured by all instruments ranged up to 10 ppbv before the fertilisation event on 28 August 2008. After fertilisation, NH_3 concentrations increased up to 120 ppbv, with such high concentrations continuing until 29 August 2008 around 14:00. The early NH_3 peaks and some periods of disagreement coincided with periods when the wind came from the rotting vegetation source in the N field as indicated by the shaded areas in Fig. 3a–c.

Overall the absolute NH_3 concentrations of all instruments revealed the same features and agreed closely with each other. By contrast, the different time resolution of the instruments resulted in slightly different features of the temporal NH_3 structure. Of the wet chemistry instruments, the 1 min data of the AiRRmonia analyser shows additional NH_3 variations during the fertilisation peak (29 August 2008), which the AMANDA and RBD failed to capture because of their lower time resolution. Similar differences can be seen in the comparison of the spectrometric techniques.

3.2 Instruments inter-comparison

For the regression analysis data from each instrument was block-averaged to hourly values in order to match the time resolution of the slowest instrument (RBD). In addition, wind directions from the sectors 0° to 150° and 310° to 360° were excluded from the analysis, due to the heterogeneous source from the rotting vegetation in the N field. Figure 4a–j depicts NH_3 concentrations from each instrument compared with the NH_3 reference ($\text{NH}_{3\text{-ref}}$), together with the results of the linear regression analysis. The $\text{NH}_{3\text{-ref}}$ was computed as the average over all instruments that were operational at a given time, excluding the OP-FTIR, for which too few data points were available.

Overall a high correlation between all instruments is observed, with $R^2 > 0.84$. The DUAL-QCLAS, c-QCLAS, Nitrolux, CRDS and CIMS comparisons with $\text{NH}_{3\text{-ref}}$ have a slope < 1 (Fig. 4d, e, g, h, and i), with the DUAL-QCLAS and the CIMS lowest at 0.67 and 0.80. The RBD, AiRRmonia, WaSul-Flux and IMS comparisons with the $\text{NH}_{3\text{-ref}}$ have a slope > 1 , but have negative intercepts of -0.74 ppbv (RBD) to -0.32 ppbv

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



(IMS) (Fig. 4a, c, f, and j). The AMANDA instrument was closest to $\text{NH}_{3\text{-ref}}$, with a slope of 1 and an intercept of 0.20 ppbv (Fig. 4b). Relatively high intercepts were observed by the CIMS, CRDS and Nitrolux compared with the other instruments. It is thought that the CRDS and Nitrolux intercept might be due to a local contamination source which was either on the sampling post, sample tubing (both came from the same batch of tubing) or most likely the inlet filters. It should be noted that for the IMS, only data from before fertilisation and after the fertilisation plume had diminished could be used, because above about 30 ppbv the IMS becomes strongly non-linear due to the consumption of the parent ions and the formation of clusters, which shifts the mobility. The consequence was a reduced dataset, biased towards smaller concentrations.

Accurate measurement of NH_3 at background levels is more challenging. For this reason, the linear regression for periods when $\text{NH}_{3\text{-ref}} < 10$ ppbv was calculated separately (Table 2). The R^2 against $\text{NH}_{3\text{-ref}}$ varied from 0.52 (Nitrolux) to 0.90 (AiRRmonia). The slope of AMANDA and IMS against $\text{NH}_{3\text{-ref}}$ were > 1 and all others were < 1 , e.g. 0.42 (Nitrolux) to 0.95 (CIMS) with intercepts from -0.61 to 3.42 ppbv. The highest intercept values were measured for CIMS, CRDS and Nitrolux and again for the latter two inlet/filter contamination are thought to be the cause.

The bias (%) between two instruments is defined according to Eq. (1), where m is the slope of the regression analysis when forced through zero.

$$\text{bias} = (m - 1) * 100. \quad (1)$$

The biases reported in Table 2 represent the percentage difference of the full range NH_3 concentration (overall bias) and the bias derived from concentrations < 10 ppbv (10 ppbv bias). The overall bias for all instruments were reasonably small, ranging from -12.9% (CIMS) to 10.9% (AiRRmonia) except for the DUAL-QCLAS, whereas the 10 ppbv biases showed more variability. Also included in Table 2 is the bias of a reading based on a calibration through standard addition from an NH_3 calibration cylinder. It turned out not to be easy to provide a common, reliable and portable gas-phase calibration standard suitable for the large range of flow rates of the different

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



instruments. Because these are based on standard additions to ambient air, they only reflect the error on the response (slope) and do not include the intercept. Calibration results were more variable than the slopes derived from the regression analysis and should therefore be treated with caution.

5 For the wet-chemistry analysers a liquid intercalibration was performed using common 50, 100 and 500 ppbv aqueous standard on the three analytical systems and the outcome is again the regression with the measured percentage difference. For the three wet-chemistry instruments the used liquid standards showed excellent agreement concerning the liquid standard bias (Table 2).

10 The OP-FTIR was operated manually in the field and the dataset is much reduced compared with the other instruments (9h). Thus, it is not included in the hourly data analysis. Instead, Fig. 5 compares the OP-FTIR data at 2 min time resolution against the other fast response instruments (c-QCLAS, DUAL-QCLAS and CIMS).

15 The data of the OP-FTIR agreed best with the DUAL-QCLAS (Fig. 5) with a slope of 0.82 (Table 3), which was reading lower compared to the other instruments (Fig. 4d) with the c-QCLAS providing the best match with the reference here. Further, the regression analysis revealed for the FTIR a high intercept of >3.74 ppbv compared with all other instruments.

20 While for graphical representation the analysis of an individual instrument against a common $\text{NH}_{3\text{-ref}}$ provides a digestible overview over the results, the full information of the inter-comparison is only revealed through correlation between each of the eleven instruments with each other. Tables 4 and 5 show the results of the regression analysis of all hourly data, while Tables 6 and 7 show the results of the regression confined to data points where both instruments reported concentrations of less than 10 ppbv. Each of the four tables contains two separate diagonal parts with information. The results
25 provided are for the regression of the instrument on the vertical axis (row) against the instrument on the horizontal axis (column). For example, the regression analysis of the

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



RBD against the AMANDA for the entire data range is:

$$\text{RBD} = 0.86 * \text{AMANDA} + 1.41 \text{ ppb}, \quad R^2 = 0.93, \quad \text{bias} = -11.1\%$$

while the regression analysis of the AMANDA vs. RBD is not included. Although derived from the regression fit of $y=ax$, the bias does not always fully represent a clear picture of the combined effects of the average discrepancy between two instruments specify by slope and intercept. For example, due to a lack of data and high intercept values for some instruments, the datasets in these scatter plots showed a distributed appearance and the linear regression line was difficult to draw (Table 8). Thus all four parameters need to be considered when interpreting the performance of two instruments against each other.

For the overall data range the slopes of the AMANDA, AiRRmonia, c-QCLAS, WaSul-Flux, Nitrolux and CRDS varied by $\pm 20\%$ with each other (Table 4). For the data limited to <10 ppbv the slopes between RBD, AiRRmonia, WaSul-Flux and IMS were all within $\pm 20\%$ of unity (Table 6). High intercepts were found for correlations of CIMS, Nitrolux and CRDS with all other instruments (Bold numbers in Tables 4 and 6), with values from 1.60 to 6.14 ppbv for the full data range and from 1.21 to 3.92 ppbv for data <10 ppbv. For the full data range, R^2 values <0.90 were limited for inter-comparisons involving RBD, CIMS or IMS (Table 5). For <10 ppbv, an $R^2 > 0.80$ was achieved for any comparison between AMANDA, AiRRmonia and c-QCLAS (Table 7). The DUAL-QCLAS (Italic numbers in Tables 5 and 7) was biased towards lower values, compared with all other instruments.

Table 8 contains two separate diagonal parts with information and presents a visual support to the results from Tables 4 to 7. The results provided are for the regression of the instrument on the vertical axis (row) against the instrument on the horizontal axis (column) for the entire data range (white). The grey diagonal part shows the plots for NH_3 concentration <10 ppbv and it is to read from the instruments in the horizontal axis (row) against instruments in the vertical axis (column).

AMTD

2, 1783–1835, 2009

Inter-comparison of NH_3 measurement techniques

K. von Bobruzski et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



3.3 Characterisation of instrument time responses

For analysing the time response of the different instrument setups (including inlets) a short time-series of each instrument was compared against data of a well-performing fast-response instrument, for which the 1 min data from the c-QCLAS was chosen. A

5 running mean was calculated from the c-QCLAS data as:

$$c'(t) = f c(t) + (1 - f) c'(t - 1) \quad (2)$$

where $c'(t)$ is the smoothed concentration, $c(t)$ is the measured concentration and f is a smoothing factor defined below, which would be unity for an instrument that is equally as fast as the c-QCLAS. Equation (2) simulates the response of a concentration measurement which is subject to a memory effect, which may be either due to the turnover time in an air volume, liquid pool or due to adsorption/desorption in inlet lines. For each instrument f was determined by fitting the smoothed c-QCLAS time series to the data reported by the instrument. This approach is demonstrated in Fig. 6, where f is adjusted for the smoothed c-QCLAS time series to match the data from the AMANDA.

15 The e-folding time of the instrument was determined as $\tau_{1/e} = 1/f$ min, which is reported in Table 9 together with the 50 and 95% response times (τ_{50} , τ_{95}). The corresponding deviation is mentioned as well.

The AMANDA reports 7.5 min data, but it appeared to take 32.2 ± 3.7 min to completely settle. The replacement of the liquid pool in the denuder appears to limit this time response of the instrument. A similar observation was made for the RBD. The AiRRmonia seemed to have the less time delays in the system, because τ_{95} of 14.4 ± 4.0 min closely matched the internal measurement cycle of 10.0 min.

20 The IMS derived with $\tau_{95} = 34.9 \pm 6.4$ min the highest delay with reported data of 3 s, but the restricted amount of qualified this statement. The instruments CIMS and DUAL-QCLAS revealed time responses as the c-QCLAS and this approach is therefore not suitable to characterise them further. They are therefore not listed in Table 9.

Inter-comparison of NH₃ measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



4 Discussion

4.1 Overall measurement accuracy

The instruments tested in the present study revealed good correlation with $R^2 > 0.84$ for one hour averages compared with $\text{NH}_3\text{-ref}$. The CIMS, CRDS and Nitrolux revealed elevated intercepts compared with the other instruments pointing at a possible contamination of the inlet filters (CRDS and Nitrolux), inlets or both. The detected results during this campaign are in line with the studies listed below. Measurements of RBD, AMANDA, AiRRmonia, WaSul-Flux and c-QCLAS were within $\pm 25\%$ for concentrations of 10 to 120 ppbv.

It should be noted that, although an attempt was made to eliminate the effect of spatial heterogeneity, emissions from grazed and fertilised grassland are expected to show some variability. It was neither possible to link up all instrument to a common inlet (e.g. the wet chemistry instruments do not use an inlet tube), nor was this the purpose of the experiment, in which we wanted to test independent systems with the respective inlets as they would have been operated by the different groups in the field. There is some indication that at times, instruments that were located more closely to each other (e.g. WaSul-Flux/AMANDA/RBD/AiRRmonia and CIMS/DUAL-QCLAS/c-QCLAS/Nitrolux/CRDS) agreed more closely with each other, but this observation was not consistent.

Previous comparison campaigns have already illustrated the challenges involved in measuring ambient NH_3 concentrations accurately, especially at low concentrations. The results in the study of Wiebe et al. (1990) showed an agreement within $\pm 30\%$ for NH_3 concentration > 1.5 ppbv with time resolution of minimum four hours for the filter packs and the annular denuders. The five instruments compared by William et al. (1992) yielded an agreement of within a factor of two for NH_3 concentration > 0.5 ppbv. In detail the CAD/IC and PF/LIF revealed accorded within 15% for NH_3 concentration of 0.2 to 5.0 ppbv for a time resolution of 2 to 8 h. The framework of the NAQMN study by Mennen et al. (1996) determined a general applicability for all

Inter-comparison of NH_3 measurement techniques

K. von Bobruzski et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



requirements for air quality monitoring on one hour sampling. Further, the DOAS and the NO_x converter instruments reached $R^2 > 0.9$ compared with the wet-annular rotating denuder, but both were only useful during high NH_3 concentration near stacks or stables. In the study by Mennen et al. (1996), the photoacoustic monitor was eliminated due to high maintenance demands and because of leaving only 1% useful data. During the campaign of Milford et al. (2000) AMANDA and DS-FIA showed an overall difference of 35% for a sampling time of 30 min, but with substantial scatter. Fehsenfeld et al. (2002) reported for CIMS and MoO_x converter method $R^2 > 0.9$ compared with the citric acid denuder (sampling time minimum two hours). The average concentration difference compared with the denuder was 0.8 for the CIMS and 1.75 for the MoO_x converter method. Two CIMS instruments tested during the field study in Nowak et al. (2006) measured $R^2 = 0.71$ and concentration difference of 17% (time resolution one minute) with NH_3 concentrations from 0.4 to 0.13 ppbv. Milford et al. (2009) compared measurements with three AMANDA systems and a mini-WEDD system. The NH_3 measurements showed good agreement between the instruments (<20% difference) for some periods, but with poorer agreement on some individual days, due to variable performance of the automatic wet chemistry detection systems.

Of particular interest here are the results of the recent laboratory inter-comparison study of Schwab et al. (2007), because it followed a complementary approach (being laboratory based) while including some of the same instruments tested here. The seven instruments tested during the laboratory comparison agreed within 25% of the expected calibration value. The IMS and Nitrolux yielded biases of $\pm 25\%$ with slower time response than the TDLAS (similar to the QCLAS used here). Further, the wet chemical instruments LOPAP and WEDD worked well in the calibration tests in view of absolute accuracy of measured concentrations, but a disadvantage was the slower time response of the WEDD.

In the recent field intercomparison of Norman et al. (2009) the slopes of hourly uncorrected data of PTR-MS (an alternative CIMS technique using a different ionisation scheme), GRAEGOR (based on the same collection and analytical technique as the

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



AMANDA, but with lower flow rates) and AiRRmonia ranged between 0.78 to 0.97 for NH_3 concentrations from 2 to 25 ppbv. During atmospheric conditions favouring condensation in inlet lines, the PTR-MS underestimated NH_3 concentrations. The authors point out the need to put more emphasis on the inlet designs for future campaigns. Whitehead et al. (2008) reported that their concentration measurements from the QCLAS and the AMANDA instrument correlated well, with $R^2=0.84$. However, the QCLAS underestimated fluxes by 64% compared with the AMANDA instrument.

4.2 Instrument specific issues

While providing a good response to the concentrations, the Nitrolux and CRDS measurements in the present study were subject to a similar high intercept compared with the other instruments. There were two aspects common to these instruments: they shared the same sampling line, which may have been contaminated, but they also both use inlet filters, exchanged infrequently (up to 3 months, according to manufacturers), which may collect NH_4NO_3 which then could dissociate at low concentrations, providing a (temperature dependent) offset. This process clearly affected the Nitrolux data at the start of the experiment, taken with an old filter, which were discarded from the analysis. This inlet/filter issue may also have affected the regressions of these instruments, especially over the low concentration range, as the intercept may not be stable in time. Apart from this issue, both instruments are convenient to operate as they are both manufacturer calibrated with long service intervals.

The only other instrument using an inlet filter is the WaSul-Flux, which operates on a similar principle as the Nitrolux. However, its filter was changed weekly, minimising the effect of NH_4NO_3 volatilisation. An attempt was made to investigate the potential of NH_4NO_3 interference on those instruments that do not remove the aerosol phase. In the c-QCLAS inlet a virtual impactor removes the coarse aerosol fraction, while the CIMS preferentially extracts charged ions into the drift tube and thus favours gas molecules over the aerosol. No filters were used on the IMS and the DUAL-QCLAS, but the residence time in the analysis cell of the DUAL-QCLAS is of the order of 0.2 s and

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



laboratory tests have found NH_4NO_3 interference to be negligible. In the wet chemistry systems aerosols are thought to pass the inlet uncollected. Unfortunately, the regional NH_4^+ concentration was fairly constant during the campaign (Fig. 2), except for a period which coincided with the fertiliser emission peak of NH_3 , during which NH_4^+ still made a minor contribution to total NH_x . In particular, the effect of inlet heating (to 50°C) on NH_4NO_3 volatilisation in the WaSul-Flux inlet could not be investigated.

The WaSul-Flux performed well against the other instruments, but has a relatively slow time response (45 min) at the background concentrations. It can achieve a detection limit of 0.25 ppbv at 45 min time resolution (Table 1), which may still not be sufficient for all applications. Work is underway to improve the sensitivity.

By contrast, the IMS is highly sensitive, but less specific and affected by competing ion chemistries, which makes it applicable only to situations of low NH_3 and where no interfering compounds are to be expected. Its comparatively poor performance over the entire concentration range is misleading as concentrations >20 ppbv had to be removed due to saturation. It shows one of the best correlations with the average at the sub-10 ppbv comparison ($R^2=0.87$, Table 2).

Three instruments deployed here (DUAL-QCLAS, c-QCLAS and CIMS) have the potential to provide a fast NH_3 spot measurement, of particular interest for aircraft applications and eddy-covariance flux measurements. The QCLAS technique (like OP-FTIR) in principle provides an absolute measurement of the concentration. However, without calibration, the instruments turned out to significantly underestimate the concentration. The c-QCLAS was calibrated at regular intervals in the field with a permeation tube calibration source, while a regular zero calibration but a one-off span calibration were applied to the DUAL-QCLAS, with average span calibration factors in the region of 1.3 and 1.2, respectively. This difference in the calibration approach is likely to be responsible for the poorer performance of the DUAL-QCLAS during this campaign. In addition, the DUAL-QCLAS was set up for eddy-covariance flux measurements, with a relatively long inlet, which may have added further uncertainty. The DUAL-QCLAS sampled air through a 2 m length of $1/4$ inch PFA tubing. Due to the “sticky” nature of

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

NH₃, this can have an impact on NH₃ measurements (Shaw et al., 1998; Whitehead et al., 2008). This may therefore partly explain the under-estimate in the NH₃ concentration at the peak concentrations. Against this possible argument, it should be noted that the DUAL-QCLAS showed one of the highest R^2 values (0.98 for the full dataset), with a small intercept compared with other instruments (Fig. 4d and Table 6), indicating a significant but rather constant slope of ~ 1.2 . By contrast, the c-QCLAS was one the better performing instruments tested here.

The CIMS provides a fast, highly sensitive technique. Like the c-QCLAS it requires continuous gas-phase calibration in the field. This was the first field deployment of this particular instrument, which showed more scatter than most instruments. Although, it should be noted that it is uncertain how much of this scatter is natural variability and how much is represented by instrumental noise. In a recent deployment of this instrument (manuscript in preparation), which employed a similar inlet design and throughput, large variability in NH₃ signal was observed on a second by second basis, such variability was not present in the background and calibration cycles, indicating that the inlet is able to respond to rapid changes in [NH₃] associated with different plumes and is therefore capturing real rather than artifactual variability. It appears that, as with the c-QCLAS approach, stability in the instrument response coupled with the need for a reliable gas-phase calibration source is the limiting factor in improving performance. This is consistent with the observations of Nowak et al. (2006), who reported the need for very frequent calibrations for an airborne CIMS instrument, especially when targeting background concentrations.

The OP-FTIR instrument averages over a path-length of 100 m which possibly limits comparability with the other point measurement techniques. Furthermore, measurements were made over a more limited concentration range. Yet, the comparison with the other fast-response techniques is encouraging (Fig. 5). Like the c-QCLAS, the OP-FTIR should also provide an absolute measurement but reports some of the lowest concentrations. At very low concentrations, instrument noise may exceed the signal from NH₃, which may explain the high intercept (>3.74 ppbv) in comparison with other

Inter-comparison of NH₃ measurement techniques

K. von Bobruzki et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

detection methods. Interestingly, both QCLAS and OP-FTIR underestimate the concentration when used in absolute (uncalibrated) mode and both rely on the accuracy of the same absorption line information of the HITRAN database.

5 All three wet chemistry systems used here are based on flow injection analysis using a selective ion membrane, which is known to have some cross sensitivity for some amines (Husted et al., 2000). Although probably unimportant here, they may make a more significant contribution in other situations, e.g., of organic animal manure emissions. Using batch sampling and off-line analysis, the RBD is the most “manual” technique included here. It is surprising that the RBD performed better (compared with the average) at small concentrations than over the entire concentration range (Table 2).
10 This is possibly due to sample carry-over in situations of highly variable concentrations. AMANDA and AiRRmonia compared well with each other and, together with WaSul-Flux and IMS (and closely followed by c-QCLAS), achieved the best agreement with each other over the low concentration range. AMANDA and IMS read somewhat higher than the other instruments. The excellent agreement on the common liquid standard within $\pm 3\%$ (Table 2) indicates that the wet chemistry instruments are stable and easy to calibrate, as long as the collection efficiency can be assumed to be 100% and the flow rates are well established. The WaSul-Flux instrument was compared against an AMANDA in previous measurement campaigns (Pogány et al., 2009),
20 where a correlation coefficient of 0.98 was found between the photoacoustic signal and the concentration readings of AMANDA for concentrations 0 to 120 ppbv, which agrees with the correlation coefficients for $\text{NH}_{3\text{-ref}}$ in this campaign (0.98, Fig. 4f), and the correlation coefficients between WaSul-Flux and the wet-chemistry instruments (0.98 for AMANDA and Airrmonia and 0.95 for the RBD; Table 5).

25 4.3 Time responses

The additional capture of NH_3 variations of instruments with higher time resolution, shown in Sect. 3.1, is consistent with the observations of Norman et al. (2009). The calculated time response for the instruments in Sect. 3.3 showed higher values than

Inter-comparison of NH_3 measurement techniques

K. von Bobruzski et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



stated by the manufacturers (Table 1). This is particularly true for the AMANDA system for which the actual response time was estimated to be 37 min. A similar observation was made for the GRAEGOR analyser, based on the same horizontal annular denuder design, but using a lower liquid flow rate (Thomas et al., 2009). Faster response could be achieved by further minimising the liquid pool in the denuders. For AiRRmonia, the calculated time response of 14.4 ± 4.0 min time to obtain 95% of the signal is only slightly slower than the 10 min measurement cycle (Table 1). The same is true for CRDS and Nitrolux with 13.4 ± 5.0 min and 10.9 ± 2.5 min to obtain 95% of the signal, respectively, as compared with instrument recording every 6 s (Table 1). During the study of Schwab et al. (2007), a TDLAS reached a value near 35 ppbv within 6 min, whereas IMS and Nitrolux had the slowest time response of all the instruments investigated in their experiment. The same observations were made during this inter-comparison, where the IMS presented the slowest time response, probably due to the use of internal materials which are not optimised for NH_3 measurements.

5 Conclusions

This paper reports an inter-comparison of eleven instruments for measuring atmospheric NH_3 at ambient concentrations, representing the largest NH_3 inter-comparison under typical field conditions to date. The approaches deployed included automated wet chemistry techniques, optical, photo-acoustic and mass spectrometric techniques. There were differences in the concentrations reported, but overall the high correlation with $R^2 > 0.84$ compared with the average of all instruments used, is very encouraging. The correlation worsens if only concentrations < 10 ppbv are considered. Concentrations of RBD, AMANDA, AiRRmonia, WaSul-Flux and c-QCLAS agreed within $\pm 25\%$ for concentrations > 10 ppbv. Some reasons for variability were identified: inlet length greatly affects measurement precision and time-response. Where used, inlet filters need to be changed very frequently (e.g. daily to weekly), at much shorter intervals than stated by some manufacturers. Instruments based on chemical ionisation mass spectroscopy and quantum cascade laser absorption spectroscopy need to be cali-

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



brated continuously, and the provision of a reliable gas-phase calibration source in the field determines their measurement precision. Wet chemistry instruments show good long-term stability, are housed to operate with very short inlets and the liquid part of the system is easier to calibrate. They provide a reliable differentiation between gas-phase NH_3 and aerosol NH_4^+ , which could not be validated for the other instruments during this study. Not all instruments tested here are suitable for accurate measurements at concentrations <1 ppbv, while the application of ion mobility spectroscopy is limited to low concentrations (<20 ppbv) and conditions with no competing pollutants. Despite recent advances in technologies, the continuous measurement of ammonia remains a challenging and costly enterprise, in terms of capital investment or running costs or both.

Acknowledgements. The measurements were supported by the UK Natural Environment Research Council (NERC) through grant nos. NE/E018505/1 and NE/E018092/1, the UK Department for Environment, Food and Rural Affairs and its devolved administrations through the Acid Deposition Processes Project and through the European Commission Integrated Project NitroEurope. The corresponding author was recipient of exchange grant no. 2153 of the Nitrogen in Europe (NinE) project of the European Science Foundation. C. F. Braban gratefully acknowledges the loan of the CRDS and technical support from EnviroTechnology and Picarro. King's College London gratefully acknowledges the loan of equipment to carry out this research from the UK NERC Field Spectroscopy Facility.

References

- Asman, W. A. H., Sutton, M. A., and Schjorring, J. K.: Ammonia: emission, atmospheric transport and deposition, *New Phytol.*, 139, 27–48, 1998.
- Bacon, T., Webber, K., and Carpio, R. A.: Contamination monitoring for ammonia, amines, and acid gases utilizing ion mobility spectroscopy (IMS), in: *Metrology, Inspection and Process Control for Microlithography XII*, Proc. SPIE-Int. Soc. Opt. Eng., 3332, ISBN 0-8194-2777-2, 1998.
- Berden, G., Peeters, R., and Meijer, G.: Cavity ring-down spectroscopy: Experimental schemes and applications, *Int. Rev. Phys. Chem.*, 19, 565–607, 2000.
- Blatter, A., Neftel, A., Dasgupta, P. K., and Simon, P. K.: A combined wet effluent denuder and mist chamber system for deposition measurements of NH_3 , NH_4 , HNO_3^- and NO_3 , in:

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



- Physicochemical Behaviour of Atmospheric Pollutants, edited by: Angeletti, G. and Restelli, G., European Commission, Brussels, 767–772, 1994.
- Breitenbach, L. P. and Shelef, M.: Development of a method for the analysis of NO₂ and NH₃ by NO⁻ measuring instruments, J. Air Pollut. Control Assoc., 23, 128–131, 1973.
- 5 Cowen, K., Summer, A. L., Dindal, A., Riggs, K., Willenberg, Z., Hatfield, J., Pfeffer, R., and Scoggin, K.: Environmental Technology Verification Report. Pranalytica, Inc. Nitrolux 1000 Ambient NH₃ Analyser, ETV 2004.
- Crounse, J. D., McKinney, K. A., Kwan, A. J., and Wennberg, P. O.: Measurement of gas-phase hydroperoxides by chemical ionization mass spectrometry, Anal. Chem., 78, 6726–6732, 10 2006.
- Duyzer, J. H., Verhagen, H. L. M., Weststrate, J. H., Bosveld, F. C., and Vermetten, A. W. M.: The dry deposition of ammonia onto a Douglas fir forest in the Netherlands, Atmos. Environ., 29, 1241–1253, 1994.
- Eden, P.: Weather log August 2008, R. Met. S., Weather, 63, 10, doi:10.1002/wea.336, 2008.
- 15 Eiceman, G. A. and Karpas, Z.: Ion Mobility Spectrometry, CRC Press, Boca Raton, FL, 1994.
- Erismann, J. W., Otjes, R., Hensen, A., Jongejan, P., van den Bulk, P., Khlystov, A., Moels, H., and Slanina, S.: Instrument development and application in studies and monitoring of ambient NH₃, Atmos. Environ., 35, 1913–1922, 2001.
- Fangmeier, A., Hadwiger-Fangmeier, A., van der Eerden, L., and Jäger, H.-J.: Effects of atmospheric ammonia on vegetation – a review, Environ. Pollut., 86, 43–82, 1994.
- 20 Fehsenfeld, F. C., Huey, L. G., Leibrock, E., Dissly, R., Williams, E., Ryerson, T. B., Norton, R., Sueper, D. T., and Hartsell, B.: Results from an informal intercomparison of ammonia measurement techniques, J. Geophys. Res., 107(D24), 4812, doi:10.1029/2001JD001327, 2002.
- 25 Ferm, M.: Method for determination of atmospheric NH₃, Atmos. Environ., 13, 1385–1393, 1979.
- Ferm, M.: Atmospheric ammonia and ammonium transport in Europe and critical loads: a review, Nutr. Cycl. Agroecosys., 51, 5–17, 1998.
- Gall, R., Perner, D., and Ladstätter-Weissenmayer, A.: Simultaneous determination of NH₃, SO₂, NO and NO₂ by direct UV-absorption in ambient air, Fresen. J. Anal. Chem., 340, 646–649, 1991.
- 30 Galle, B., Bergquist, B., Ferm, M., Törnquist, K., Griffith, D. W. T., Jensen, N. O., and Hansen, F.: Measurement of ammonia emissions from spreading of manure using gradient FTIR

Inter-comparison of NH₃ measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



techniques, *Atmos. Environ.*, 34, 4907–4915, 2000.

Genfa, Z. and Dasgupta, P. K.: A Continuous Film-Recirculable Drop Gas-Liquid Equilibration Device. Measurement of Trace gaseous NH_3 , *Anal. Chem.*, 72, 3165–3170, 2000.

Grisar, R., Preier, H., Schmidtke, G., and Restelli, G.: Monitoring of gaseous pollutants by tunable diode lasers, *EC Air pollution Report 3*, CEC, Brussels, Belgium, 1987.

Griffith, D. W. T.: Synthetic calibration and quantitative analysis of gas phase infrared spectra, *Appl. Spectrosc.*, 50, 59–70, 1996.

Griffith, D. W. T. and Galle, B.: Flux measurements of NH_3 , N_2O and CO_2 using dual beam FTIR spectroscopy and the flux-gradient technique, *Atmos. Environ.*, 34, 1087–1098, 2000.

Hagg, C. and Szabo, I.: New Ion-Optical Devices Utilizing Oscillatory Electric-Fields. Stability of Ion Motion in a Two-Dimensional Octopole Field, *Int. J. Mass Spectrom.*, 73, 277–294, 1986.

Harren, F. J. M., Cotti, G., Oomens, J., and te Lintel Hekkert, S.: Photoacoustic Spectroscopy in Trace Gas Monitoring, *Encyclopedia of Analytical Chemistry*, edited by: Meyers, R.A., John Wiley & Sons Ltd, Chichester, 2203–2226, 2000.

Hill Jr., H. H., Slems, W. F., St. Louis, R. H., and McMinn, D. G.: Ion Mobility Spectrometry, *Anal. Chem.*, 62, 1201A–1209A, 1990.

Husted, S., Hebborn, C. A., Mattsson, M., and Schjoerring, J. K.: A critical experimental evaluation of methods for determination of NH_4^+ in plant tissue, xylem sap and apoplastic fluid, *Physiol. Plantarum*, 109, 167–179, 2000.

Janson, R., Rosman, K., Karlsson, A., and Hansson, H.-C.: Biogenic emissions and gaseous precursors to forest aerosols, *Tellus B*, 53, 423–440, 2001.

Lammel, G.: Determination of NH_3 and nitric acid using a diffusion denuder method, *Fresen. J. Anal. Chem.*, 340, 684–686, 1991.

Langford, A. O., Goldan, P. D., and Fehsenfeld, F. C.: A Molybdenum Oxide Annular Denuder System for Gas Phase Ambient NH_3 Measurements, *J. Atmos. Chem.*, 8, 359–376, 1989.

Keuken, M. P., Schoonebeek, C. A. M., van Wensveen-Louter, A., and Slanina, J.: Simultaneous sampling of NH_3 , HNO_3 , HCl , SO_2 and H_2O_2 in ambient air by wet annular denuder system, *Atmos. Environ.*, 22, 2541–2548, 1988.

Krupa, S. V.: Effects of atmospheric ammonia (NH_3) on terrestrial vegetation: a review, *Environ. Pollut.*, 124, 179–221, 2003.

Marcy, T. P., Gao, R. S., Northway, M. J., Popp, P. J., Stark, H., and Fahey, D. W.: Using chemical ionization mass spectrometry for detection of HNO_3 , HOI , and ClONO_2 in the atmosphere,

AMTD

2, 1783–1835, 2009

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



- Int. J. Mass Spectrom., 243, 63–70, 2005.
- McManus, J. B., Nelson, D. D., Shorter, J. H., Zahniser, M. S., Mueller, A., Bonetti, Y., Beck, M., Hofstetter, D., and Faist, J.: Quantum cascade lasers for open- and closed-path measurement of trace gases, in: Diode lasers and applications in atmospheric sensing, edited by: Fried, A., Proc. SPIE, 4817, 22–33, 2002.
- McManus, J. B.; Shorter, J. H.; Nelson, D. D., and Zahniser, M. S.: Compact Quantum Cascade Laser Instrument for Rapid, High Sensitivity Measurements of Trace Gases in Air, Sensors, 2007 IEEE, 1341–1344, 2007.
- Mennen, M. G., van Elzakker, B. G., van Putten, E. M., Uiterwijk, J. W., Regts, T. A., van Hellenmond, J., Wyer, G. P., Otjes, R. P., Verhage, A. J. L., Wouters, L. W., Heffels, C. J. G., Roemer, F. G., van den Beld, L., and Tetteroo, J. E. H.: Evaluation of automatic ammonia monitors for application in an air quality monitoring network, Atmos. Environ., 30, 3239–3256, 1996.
- Milford, C., Sutton, M. A., Allen, A. G., Karlsson, A., Davison, B. M., James, J. D., Rosman, K., Harrison, R. M., and Sape, J. N.: Marine and land-based influence on atmospheric ammonia and ammonium over Tenerife, Tellus B, 52, 273–289, 2000.
- Milford, C., Theobald, M. R., Nemitz, E., and Sutton, M.: Dynamics of NH_3 exchange in response to cutting and fertilising an intensively-managed grassland, Water Air Soil Poll., 1, 167–176, 2001.
- Milford, C., Theobald, M. R., Nemitz, E., Hargreaves, K. J., Horvath, L., Raso, J., Dämmgen, U., Neftel, A., Jones, S. K., Hensen, A., Loubet, B., Cellier, P., and Sutton, M. A.: Ammonia fluxes in relation to cutting and fertilization of an intensively managed grassland derived from an inter-comparison of gradient measurements, Biogeosciences, 6, 819–834, 2009, <http://www.biogeosciences.net/6/819/2009/>.
- Mozurkewich, M.: The Dissociation-Constant of Ammonium-Nitrate and Its Dependence on Temperature, Relative-Humidity and Particle-Size, Atmos. Environ., 27, 261–270, 1993.
- Myles, L., Meyers, T. P., and Robinson, L.: Atmospheric NH_3 measurement with an ion mobility spectrometer, Atmos. Environ., 40, 5745–5752, 2006.
- Neuman, J. A., Parrish, D. D., Trainer, M., Ryerson, T. B., Holloway, J. S., Nowak, J. B., Swanson, A., Flocke, F., Roberts, J. M., Brown, S. S., Stark, H., Sommariva, R., Stohl, A., Peltier, R., Weber, R., Wollny, A. G., Sueper, D. T., Hubler, G., and Fehsenfeld, F. C.: Reactive nitrogen transport and photochemistry in urban plumes over the North Atlantic Ocean, J. Geophys. Res., 111, D23S54, doi:10.1029/2005JD007010, 2006.

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



- Norman, M., Hansel, A., and Wisthaler, A.: O²⁺ as reagent ion in the PTR-MS instrument: detection of gas-phase ammonia, *Int. J. Mass Spectrom.*, 265, 382–287, 2007.
- Norman, M., Spirig, C., Wolff, V., Trebs, I., Flechard, C., Wisthaler, A., Schnitzhofer, R., Hansel, A., and Nefftel, A.: Intercomparison of ammonia measurement techniques at an intensively managed grassland site (Oensingen, Switzerland), *Atmos. Chem. Phys.*, 9, 2635–2645, 2009, <http://www.atmos-chem-phys.net/9/2635/2009/>.
- Nowak, J. B., Huey, L. G., Russell, A. G., Tian, D., Neuman, J. A., Orsini, D., Sjostedt, S. J., Sullivan, A. P., Tanner, D. J., Nenes, A., Edgerton, E., and Fehsenfeld, F. C.: Analysis of urban gas phase ammonia measurements from the 2002 Atlanta Aerosol Nucleation and Real-Time Characterization Experiment (ANARChE), *J. Geophys. Res.*, 111, D17308, doi:10.1029/2006JD007113, 2006.
- Nowak, J. B., Neumann, J. A., Kozai, K., Huey, L. G., Tanner, D. J., Holloway, J. S., Ryerson, T. B., Frost, G. J., McKeen, S. A., and Fehsenfeld, F. C.: A chemical ionization mass spectrometry technique for airborne measurements of NH₃, *J. Geophys. Res.*, 112, D10S02, doi:10.1029/2006JD007589, 2007.
- Pogány, A., Mohácsi, Á., Varga, A., Bozóki, Z., Galbács, Z., Horváth, L., and Szabó, G.: A compact NH₃ detector with sub-ppb accuracy using near-infrared photoacoustic spectroscopy and preconcentration sampling, *Environ. Sci. Technol.*, 43, 826–830, 2009.
- Pushkarsky, M. B., Webber, M. E., Baghdassarian, O., Narasimhan, L. R., and Patel, C. K. N.: Laserbased photoacoustic ammonia sensor for industrial applications, in special issue: Trends in Laser Sources, Spectroscopic Techniques and Their Applications to Trace Gas Detection, *Appl. Phys. B-Lasers O.*, 75(1–2), 391–396, 2002.
- Pushkarsky, M. B., Webber, M. E., and Patel, C. K. N.: Ultra-sensitive ambient ammonia detection using CO₂ laser-based photoacoustic spectroscopy, *Appl. Phys. B-Lasers O.*, 77, 381–385, 2003.
- Rella, C.: Picarro's NH₃ analyzer for Ambient Air Monitoring, 6. Nationales NH₃-Treffen. Hannover, Deutschland, 19/20 November 2008.
- Rothmann, L. S., Rinsland, C. P., Goldman, A., Massie, S. T., Edwards, D. P., Flaud, J. M., Perrin, A., Camy-Peyret, C., Danna, V., Mandin, J. Y., Schroeder, J., McCann, A., Gamache, R. R., Wattson, R. B., Yoshino, K., Chance, K. V., Jucks, K. W., Brown, L. R., Nemtchinov, V., and Varanasi, P.: The HITRAN molecular spectroscopic database and HAWKS (HITRAN atmospheric workstation), 1996 Edition, *J. Quant. Spectrosc. Ra.*, 60, 665–710, 1998.
- Schwab, J. J., Li, Y., Bae, M.-S., Demerjian, K. L., Hou, J., Zhou, X., Jensen, B., and Pryor,

Inter-comparison of NH₃ measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



- S. C.: A laboratory intercomparison of real-time gaseous ammonia measurement methods, *Environ. Sci. Technol.*, 41, 8412–8429, 2007.
- Shaw, W. J., Spicer, C. W., and Kenny, D. V.: Eddy correlation fluxes of trace gases using a tandem mass spectrometer, *Atmos. Environ.*, 32, 2887–2898, 1998.
- 5 Simon, P. K., Dasgupta, P. K., and Vecera, Z.: Wet effluent denuder coupled liquid/ion chromatography systems, *Anal. Chem.*, 63, 1237–1242, 1991.
- Simon, P. K. and Dasgupta, P. K.: Wet effluent denuder coupled liquid/ion chromatography systems: annular and parallel plate denuders, *Anal. Chem.*, 65, 1134–1139, 1993.
- Slusher, D. L., Pitteri, S. J., Haman, B. J., Tanner, D. J., and Huey, L. G.: A chemical ionization
 10 technique for measurement of pernitric acid in the upper troposphere and the polar boundary layer, *Geophys. Res. Lett.*, 28, 3875–3878, 2001.
- Sunner, J., Nicol, G., and Kebarle, P.: Factors Determining Relative Sensitivity of Analytes in Positive Mode Atmospheric-Pressure Ionization Mass-Spectrometry, *Anal. Chem.*, 60, 1300–1307, 1988.
- 15 Sutton, M., Fowler, D., Burkhardt, J. K., and Milford, C.: Vegetation atmosphere exchange of ammonia: canopy cycling and the impacts of elevated nitrogen inputs, *Water Air Soil Poll.*, 85, 2057–2063, 1995.
- Sutton, M. A., Nemitz, E., Milford, C., Fowler, D., Moreno, J., San Jose, R., Wyers, G. P., Otjes, R. P., Harrison, R., Husted, S., and Schjoerring, J. K.: Micrometeorological measurement of
 20 net NH_3 fluxes over oilseed rape during two vegetation periods, *Agr. Forest. Meteorol.*, 105, 351–369, 2000a.
- Sutton, M. A., Dragosits, U., Tang, Y. S., and Fowler, D.: Ammonia emissions from non agricultural sources in the UK, *Atmos. Environ.*, 34, 855–869, 2000b.
- Sutton, M. A., Tang, Y. S., Dragosits, U., Fournier, N., Dore, T., Smith, R. I., Weston, K. J., and
 25 Fowler, D.: A spatial analysis of atmospheric ammonia and ammonium in the UK, *TheScientificWorld*, 1(S2), 275–286, 2001.
- Sutton, M. A., Nemitz, E., Erisman, J. W., Beier, C., Butterbach Bahl, K., Cellier, W., de Vries, P., Cotrufo, F., Skiba, U., Di Marco, C., Jones, S., Laville, P., Soussana, J. F., Loubet, B., Twigg, M., Famulari, D., Whitehead, J., Gallagher, M. W., Neftel, A., Flechard, C. R., Herrmann, B., Calanca, P. L., Schjoerring, J. K., Daemmgen, U., Horvath, L., Tang, Y. S., Emmett,
 30 B. A., Tietema, A., Peñuelas, J., Kesik, M., Brueggemann, N., Pilegaard, K., Vesala, T., Campbell, C. L., Olesen, J. E., Dragosits, U., Theobald, M. R., Levy, P., Mobbs, D. C., Milne, R., Viovy, N., Vuichard N., Smith, J. U., Smith, P., Bergamaschi, P., Fowler, D., and Reis,

Inter-comparison of NH_3 measurement techniques

K. von Bobruzski et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



S.: Challenges in quantifying biosphere-atmosphere exchange of nitrogen species, *Environ. Pollut.*, 150, 125–139, 2007.

Thomas, R. M., Trebs, I., Otjes, R., Jongejan, P. A. C., ten Brink, H., Phillips, G., Kortner, M., Meixner, F. X., and Nemitz, E.: An automated analyzer to measure surface-atmosphere exchange fluxes of water soluble inorganic aerosol compounds and reactive trace gases, *Environ. Sci. Technol.*, 43(5), 1412–1418, 2009.

Tittel, F. K., Richter, D., and Fried, A.: Mid-infrared laser applications in spectroscopy, in: *Topics in Applied Physics*, vol. 89, edited by: Sorokina, I. T. and Vodopyanov, K. L., Springer-Verlag, 445–516, 2003.

10 Warland, J. S., Dias, G. M., and Thurtell, G. W.: A tunable diode laser system for ammonia flux measurement over multiple plots, *Environ. Pollut.*, 114, 215–221, 2001.

Warneck, P.: *Chemistry of the Natural Atmosphere*, Academic Press, New York, 1988.

Whitehead, J. D., Longley, I. D., and Gallagher, M. W.: Seasonal and diurnal variation in atmospheric NH_3 in an urban environment measured using a quantum cascade laser absorption spectrometer, *Water Air Soil Poll.*, 183, 317–329, 2007.

15 Whitehead, J. D., Twigg, M., Famulari, D., Nemitz, E., Sutton, M. A., Gallagher, M. W., and Fowler, D.: Evaluation of Laser Absorption Spectroscopic Techniques for Eddy Covariance Flux Measurements of NH_3 , *Environ. Sci. Technol.*, 42, 2041–2046, 2008.

20 Wiebe, H. A., Anlauf, K. G., Tuazon, E. C., Winer, A. M., Biermann, H. W., Appel, B. R., Solomon, P. A., Cass, G. R., Ellestad, T. G., Knapp, K. T., Peake, E., Spicer, C. W., and Lawson, P. A.: A comparison of measurements of atmospheric ammonia by filter packs, transition-flow reactors, simple and annular denuders and Fourier-Transform Infrared Spectroscopy, *Atmos. Environ. A-Gen.*, 1019–1028, 1990.

25 Williams, E. J., Sandholm, S. T., Bradshaw, J. D., Schendel, J. S., Langford, A. O., Quinn, P. K., LeBel, P. J., Vay, S. A., Roberts, p. D., Norton, R. B., Watkins, B. A., Buhr, M. P., Parrish, D. D., Calvert, J. G., and Fehsenfeld, F. C.: An intercomparison of five ammonia measurement techniques, *J. Geophys. Res.*, 97, 591–611, 1992.

Wyers, G. P., Otjes, R. P., and Slanina, J.: A continuous flow denuder for the measurement of ambient concentrations and surface fluxes of NH_3 , *Atmos. Environ.*, 27A, 2085–2090, 1993.

30 Yokelson, R. J., Christian, T. J., Bertschi, I. T., and Hao, W. M.: Evaluation of adsorption effects on measurements of ammonia, acetic acid and methanol, *J. Geophys. Res.*, 108, 46–49, 2003.

Inter-comparison of NH_3 measurement techniques

K. von Bobruzski et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Table 1. Summary of the characteristics of the instruments.

Instrument	Manufacturer	Air rate [l min ⁻¹]	Used timeresolution/ used time average [s]	Precision [ppbv]	Range [ppbv]
RBD	Energy Research Foundation of the Netherlands (ECN) (Keuken et al., 1988)	27	2400/3600	0.02	not specified
AMANDA	Energy Research Foundation of the Netherlands (ECN) (Wyers et al., 1993)	28	450/450	0.02	0.02–500
AiRRmonia	R&R Mechatronics	1	600/60	0.05	0.04–500
DUAL-QCLAS	Aerodyne Research, Inc. (ARI) (Whitehead et al., 2008)	15	0.2/60	0.018	not specified
c-QCLAS	Aerodyne Research, Inc. (ARI) (McManus et al., 2007)	8.9	1/60	0.05	not specified
WaSul-Flux	Hilase Ltd.	4	300–1800/ 300–1800	0.25	0.25–1 000 000
Nitrolux-100	Pranalytica Inc. (Cowen et al., 2004)	1.2–1.6	3/300	0.1	0.1–200
CRDS	Enviro Sense1000 Analyzer, Picarro (Berden et al., 2000)	1	3/300	0.07	0.07–25
CIMS	Georgia Institute of Technology CIMS team (Nowak et al., 2007)	19.5	1/60	0.94	not specified
IMS	Bruker Daltonik	0.4	4/60	not specified	Variable, dependent on other substances present
OP-FTIR	MIDAC Corp.	n/a	8/120	not specified	not specified

AMTD

2, 1783–1835, 2009

**Inter-comparison of
NH₃ measurement
techniques**

K. von Bobruzski et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Inter-comparison of NH₃ measurement techniques

K. von Bobruzki et al.

Table 2. Correlation of hourly NH₃ concentrations less than 10 ppbv ($z=1.1$ m) between each instrument and the NH_{3-ref}. Also shown are the bias for the entire data range and the data <10 ppbv, as well as the gas and liquid standard biases for all instruments.

Instrument	<10 ppbv regression				Overall bias [%]	Gas Std. bias [%]	Liquid Std. bias [%]
	Slope	Intercept [ppbv]	R^2	Bias [%]			
RBD	0.89	−0.33	0.85	−20.1	+5.65	+13.37	+2.62
AMANDA	1.02	−0.08	0.85	+0.62	−0.63	−24.71	+0.85
AiRRmonia	0.83	−0.02	0.90	−17.7	+10.9	−18.3	−2.96
CIMS	0.95	+1.93	0.65	+54.5	−12.9	−0.26	N/A
c-QCLAS	0.72	+0.71	0.81	−12.8	−4.02	−23.2	N/A
DUAL-QCLAS	0.86	−0.19	0.66	−20.6	−32.1	0*	N/A
WaSul-Flux	0.81	−0.15	0.85	−22.0	+1.27	−	N/A
Nitrolux	0.42	+3.42	0.52	+2.51	+1.69	−	N/A
CRDS	0.50	+3.14	0.56	+26.0	+5.10	−12.48	N/A
IMS	1.15	−0.61	0.87	−2.63	−2.90	−	N/A

* After calibration using this gas standard.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Inter-comparison of
NH₃ measurement
techniques

K. von Bobruzki et al.

Table 3. Summary of linear regression results of the OP-FTIR against c-QCLAS, DUAL-QCLAS and CIMS at 2 min time resolution from the data shown in Fig. 5.

	Slope	Intercept (ppbv)	R^2
c-QCLAS	0.54	4.39	0.97
DUAL-QCLAS	0.82	3.74	0.92
CIMS	0.43	5.37	0.63

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Table 4. Inter-comparison of linear correlations between each instrument of the full data range. Slopes are given in the bottom half and intercepts are indicated by the top (grey) of the matrix. Bold numbers indicate noticeable high intercepts.

		RBD	AMANDA	AiRRmonia	CIMS	c-QCLAS	DUAL-QCLAS	WaSul-Flux	Nitrolux	CRDS	IMS
		Intercept [ppbv]									
RBD	Slope	–	1.41	0.70	3.65	1.17	1.09	0.55	6.14	3.63	0.10
AMANDA		0.86	–	1.08	3.51	–0.62	0.34	–0.86	1.82	2.27	0.04
AiRRmonia		0.97	1.12	–	3.92	0.34	0.57	0.16	2.95	2.93	0.02
CIMS		0.74	0.76	0.65	–	–2.46	–0.38	–1.07	4.12	1.60	0.78
c-QCLAS		0.86	0.96	0.83	1.09	–	0.64	0.47	5.73	3.25	0.10
DUAL-QCLAS		0.54	0.69	0.59	0.64	0.65	–	–1.13	2.46	1.81	0.40
WaSul-Flux		0.90	1.02	0.90	1.06	1.00	1.55	–	3.09	3.02	0.19
Nitrolux		0.77	0.96	0.85	0.97	0.90	1.53	0.92	–	–0.03	–2.22
CRDS		0.81	0.93	0.83	1.09	1.04	1.60	0.92	1.00	–	–1.13
IMS		1.12	0.88	1.11	0.30	0.93	0.69	1.11	0.95	0.65	–

Inter-comparison of NH₃ measurement techniques

K. von Bobruzski et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Table 5. Inter-comparison of correlation coefficients and biases between each instrument of the full data range. Biases are given in the bottom half and correlation coefficients are indicated by the top (grey) of the matrix. Italic numbers indicate high biases of Dual-QCLAS.

	RBD	AMANDA	AiRRmonia	CIMS	c-QCLAS	DUAL-QCLAS	WaSul-Flux	Nitrolux	CRDS	IMS
	R^2									
RBD	–	0.93	0.93	0.82	0.87	0.95	0.95	0.84	0.86	0.80
AMANDA	–11.1	–	0.99	0.76	0.92	0.97	0.98	0.98	0.98	0.90
AiRRmonia	–1.77	9.41	–	0.74	0.91	0.98	0.98	0.96	0.97	0.82
CIMS	–18.8	–15.6	–26.8	–	0.89	0.94	0.79	0.75	0.71	0.58
c-QCLAS	–11.7	–5.91	–15.8	1.96	–	0.97	0.93	0.93	0.93	0.70
DUAL-QCLAS	–43.4	–29.8	–38.9	–37.7	–33.0	–	0.98	0.97	0.91	0.66
WaSul-Flux	–8.85	–0.3	–9.50	3.19	1.80	48.3	–	0.95	0.95	0.82
Nitrolux	–12.4	0.33	–9.83	8.00	2.62	65.0	–1.40	–	0.99	0.57
CRDS	–10.7	–0.2	–10.6	14.7	13.8	86.4	–0.12	0.37	–	0.20
IMS	14.3	–10.9	10.9	–60.8	–5.58	–19.9	15.2	–51.1	–60.5	–

Inter-comparison of NH₃ measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Table 6. Inter-comparison of linear correlations between each instrument of data less than 10 ppbv with. Slopes are given in the bottom half and intercepts are indicated by the top (grey) of the matrix. Bold numbers indicate noticeable high intercepts.

	RBD	AMANDA	AiRRmonia	CIMS	c-QCLAS	DUAL-QCLAS	WaSul-Flux	Nitrolux	CRDS	IMS
	Intercept [ppbv]									
RBD	–	0.37	0.48	3.08	1.22	0.48	0.27	3.92	3.82	0.02
AMANDA	1.15	–	0.20	2.94	1.02	0.34	–0.06	3.75	3.42	–0.09
AiRRmonia	0.85	0.73	–	2.64	0.84	0.05	0.01	3.26	3.58	–0.14
CIMS	0.71	0.68	0.89	–	–0.64	0.26	–0.81	2.5	1.21	–0.89
c-QCLAS	0.79	0.64	0.86	0.81	–	0.16	–0.68	3.47	3.45	–0.64
DUAL-QCLAS	0.86	0.70	1.03	0.35	0.78	–	0.09	3.90	3.91	0.30
WaSul-Flux	0.85	0.77	0.94	0.57	1.03	0.79	–	3.47	3.75	0.10
Nitrolux	0.40	0.40	0.51	0.52	0.53	0.43	0.52	–	–0.05	–2.22
CRDS	0.25	0.46	0.44	0.69	0.46	0.24	0.58	1.02	–	–1.13
IMS	1.14	0.93	1.17	0.68	1.15	0.75	1.13	0.95	0.65	–

Slope

Inter-comparison of NH₃ measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Table 7. Inter-comparison of correlation coefficients and biases between each instrument of data less than 10 ppbv. Biases are given in the bottom half and correlation coefficients are indicated by the top (grey) of the matrix. Italic numbers indicate high biases of Dual-QCLAS.

	RBD	AMANDA	AiRRmonia	CIMS	c-QCLAS	DUAL-QCLAS	WaSul-Flux	Nitrolux	CRDS	IMS
	R^2									
RBD	–	0.81	0.79	0.37	0.72	0.51	0.77	0.21	0.09	0.79
AMANDA	26.8	–	0.91	0.40	0.81	0.52	0.90	0.45	0.46	0.83
AiRRmonia	–0.46	–22.7	–	0.55	0.91	0.62	0.85	0.79	0.43	0.73
CIMS	105	66.7	91.6	–	0.43	0.20	0.54	0.44	0.55	0.40
c-QCLAS	12.6	–14.9	6.66	–31.6	–	0.63	0.82	0.33	0.27	0.66
DUAL-QCLAS	<i>10.5</i>	<i>–16.8</i>	<i>5.40</i>	<i>–58.5</i>	<i>–16.2</i>	–	0.62	0.06	0.11	0.46
WaSul-Flux	–6.87	–23.7	–5.45	–59.9	–12.3	–17.5	–	0.62	0.50	0.78
Nitrolux	101	12.3	16.6	–1.96	35.7	146	41.8	–	0.72	0.57
CRDS	107	32.8	46.0	–6.32	45.5	96.3	68.4	1.21	–	0.20
IMS	14.8	<i>–9.45</i>	<i>12.5</i>	<i>–50.7</i>	–2.33	–12.2	16.0	–51.1	–60.5	–

Inter-comparison of NH₃ measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close



























































































Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Table 8. Linear regression between each instrument of data for the entire data range (bottom left) and less than 10 ppbv (shaded top right).

	RBD	AMANDA	AiRRmonia	CIMS	c-QCLAS	DUAL-CLAS	WaSul-Flux	Nitrolux	CRDS	IMS
RBD	-									
AMANDA		-								
AiRRmonia			-							
CIMS				-						
c-QCLAS					-					
DUAL-CLAS						-				
WaSul-Flux							-			
Nitrolux								-		
CRDS									-	
IMS										-

Inter-comparison of NH₃ measurement techniques

K. von Bobruzki et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



**Inter-comparison of
NH₃ measurement
techniques**

K. von Bobruzki et al.

Table 9. Analysis of the response time of AMANDA, RBD, WaSul-Flux, AiRRmonia, Nitrolux CRDS and IMS in comparison to c-QCLAS with corresponding statistical parameters.

	$\tau_{1/e}$ (min)	τ_{50} (min)	τ_{95} (min)
AMANDA	10.7±1.3	7.4±0.9	32.2±3.7
RBD	28.7±4.2	19.9±2.9	85.9±12.5
WaSul-Flux	19.1±5.4	13.3±3.7	57.3±16.1
AiRRmonia	4.8±1.4	3.4±0.9	14.4±4.0
Nitrolux	3.6±0.8	2.5±0.6	10.9±2.5
CRDS	4.5±1.7	3.1±1.2	13.4±5.0
IMS	11.6±2.1	8.1±1.5	34.9±6.4

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Inter-comparison of NH_3 measurement techniques

K. von Bobritzki et al.



Fig. 1. Intensively managed grassland site (Easter Bush) with instruments, looking from the S field towards the N field.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Inter-comparison of NH₃ measurement techniques

K. von Bobruzki et al.

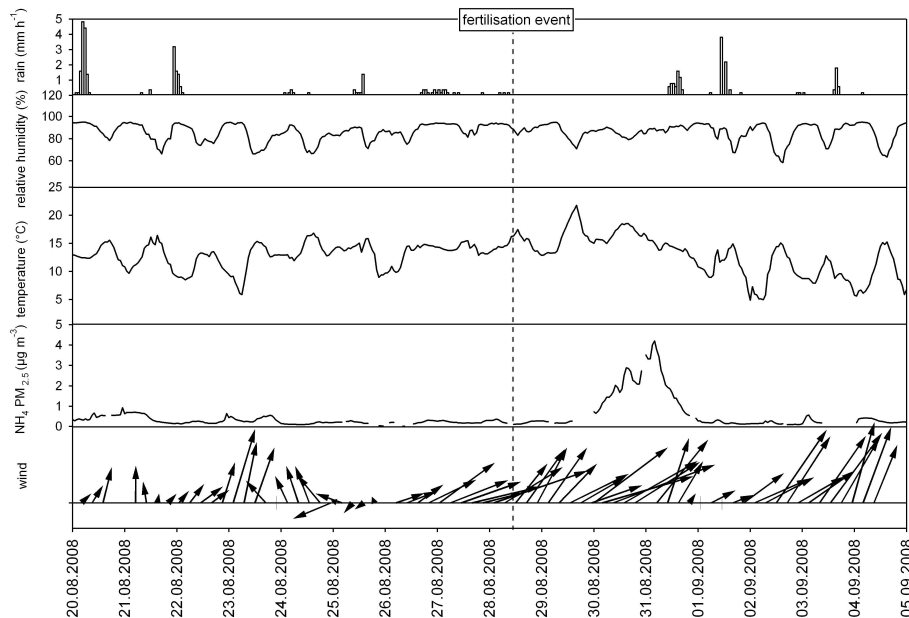


Fig. 2. Time series of hourly data from selected meteorological variables during the campaign. The aerosol NH₄⁺ concentration was measured using a MARGA monitor (see text) at the Auchencorth EMEP site, 10 km south of the Easter Bush field site.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Inter-comparison of NH₃ measurement techniques

K. von Bobruzki et al.

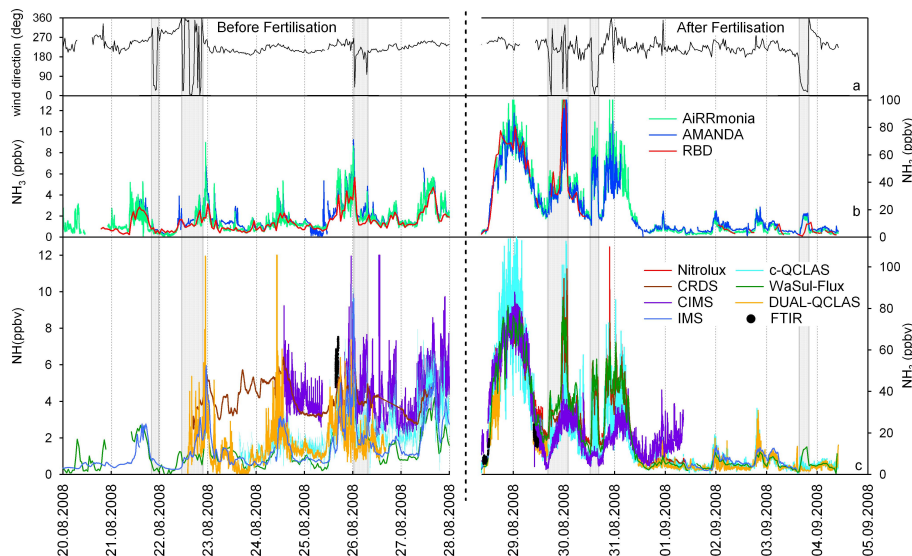


Fig. 3. Time series of NH₃ for all instruments ($z=1.1$ m): **(a)** occurring wind direction; **(b)** instrument time series: AiRRmonia (green), AMANDA (blue), RBD (red); **(c)** instrument time series: Nitrolux (red), CRDS (brown), CIMS (purple), IMS (blue), c-QCLAS (cyan), WaSul-Flux (green), DUAL-QCLAS (orange), OP-FTIR (black). Note the different scales used to show the data before and after fertilisation on 28 August 2008. The shaded areas indicate periods during which the wind came from the N field.

[Title Page](#)
[Abstract](#)
[Introduction](#)
[Conclusions](#)
[References](#)
[Tables](#)
[Figures](#)
[◀](#)
[▶](#)
[◀](#)
[▶](#)
[Back](#)
[Close](#)
[Full Screen / Esc](#)
[Printer-friendly Version](#)
[Interactive Discussion](#)


Inter-comparison of NH₃ measurement techniques

K. von Bobruzki et al.

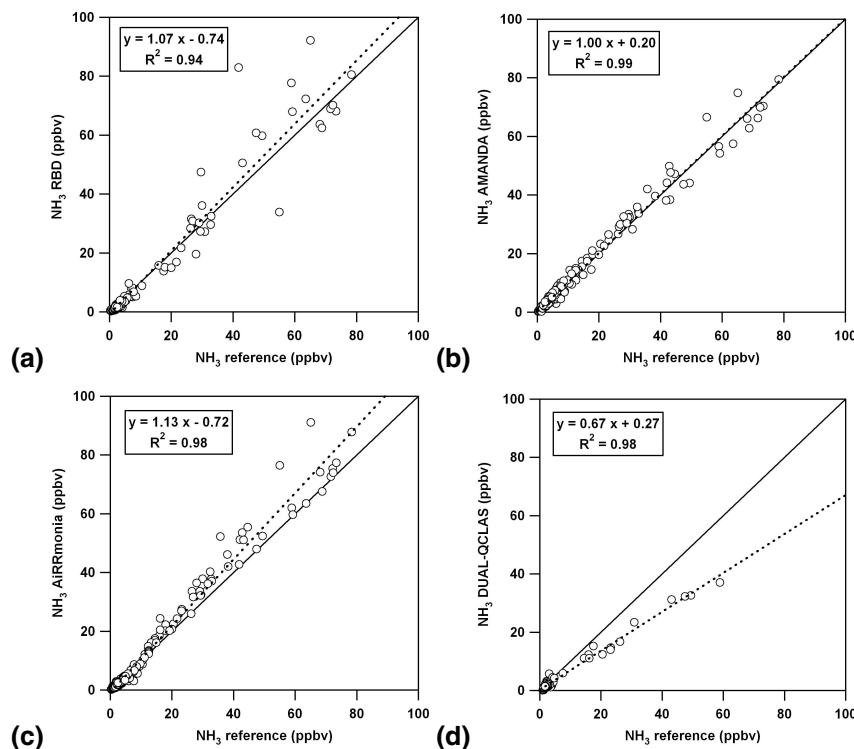


Fig. 4. Scatter plots showing correlation of hourly NH₃ concentrations (z=1.1 m) between all instruments and the NH_{3-ref} screened for wind direction (150–310°). The solid line gives the 1:1 line and the dashed line the result of the axis regression.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Inter-comparison of NH₃ measurement techniques

K. von Bobruzki et al.

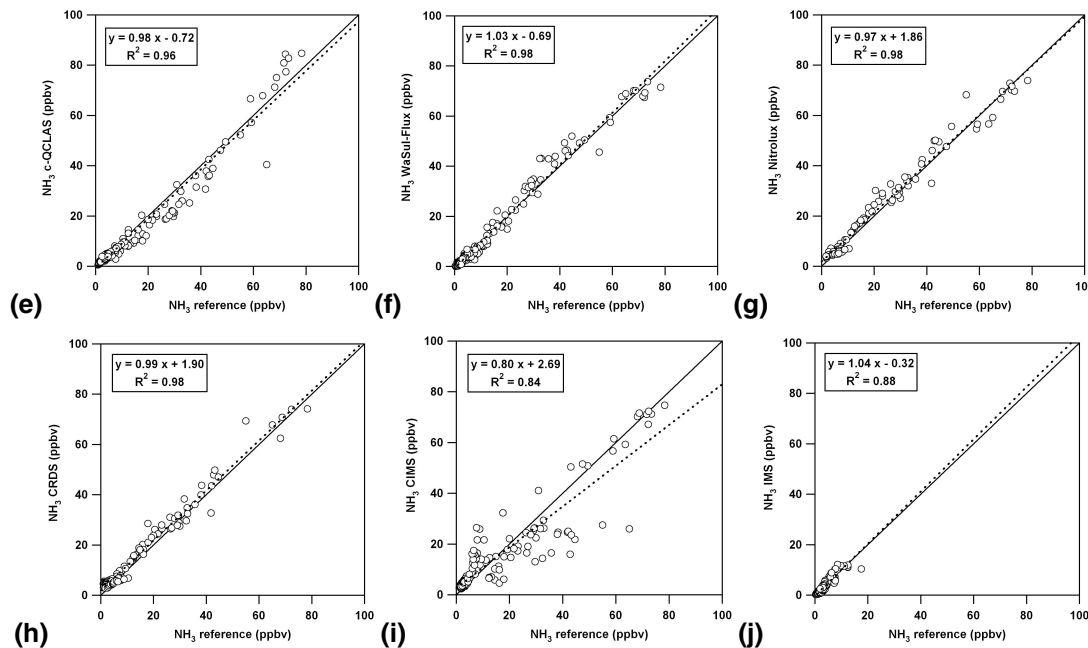


Fig. 4. Continued.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

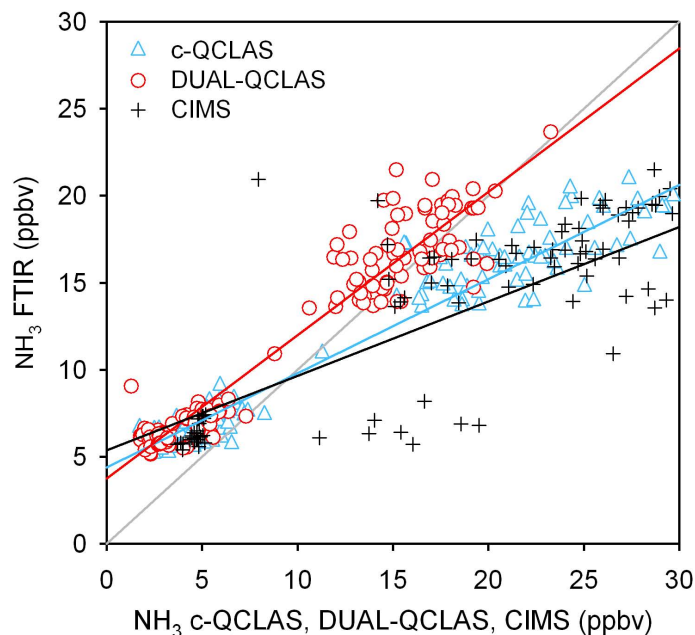


Fig. 5. Scatter plots of OP-FTIR against c-QCLAS, DUAL-QCLAS and CIMS at 2 min time resolution, including regression lines and the 1:1 line (grey).

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Inter-comparison of NH_3 measurement techniques

K. von Bobruzki et al.

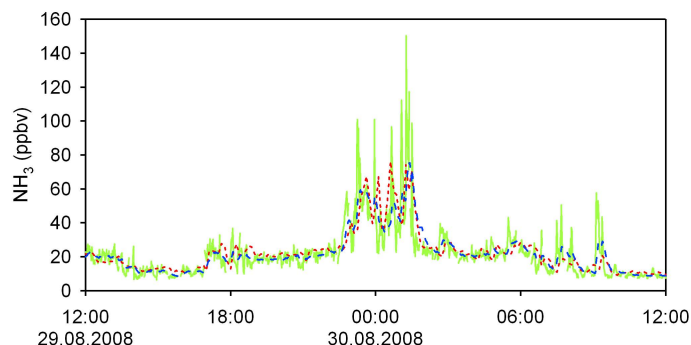


Fig. 6. Comparison of the time-series of the AMANDA (red/dotted) and the c-QCLAS (green) for a 24 h period from 29 to 30 August 2008. The c-QCLAS smoothed concentration $c'(t)$ (blue/dashed) was calculated with $f=0.08$, selected by eye as a fit to the AMANDA data.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)