

This discussion paper is/has been under review for the journal Atmospheric Measurement Techniques (AMT). Please refer to the corresponding final paper in AMT if available.

**Ground-based FTS
comparison and ACE
validation at Eureka
during IPY**

R. L. Batchelor et al.

Four Fourier transform spectrometers and the Arctic polar vortex: instrument intercomparison and ACE-FTS validation at Eureka during the IPY springs of 2007 and 2008

R. L. Batchelor¹, F. Kolonjari¹, R. Lindenmaier¹, R. L. Mittermeier², W. Daffer³, H. Fast², G. Manney^{3,4}, K. Strong¹, and K. A. Walker^{1,5}

¹Department of Physics, University of Toronto, Toronto, Ontario, Canada

²Environment Canada, Downsview, Ontario, Canada

³Jet Propulsion Laboratory, California Institute of Technology, Pasadena, California, USA

⁴New Mexico Institute of Mining and Technology, Socorro, New Mexico, USA

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

⁵ Department of Chemistry, University of Waterloo, Waterloo, Ontario, Canada

Received: 6 October 2009 – Accepted: 19 October 2009 – Published: 6 November 2009

Correspondence to: R. L. Batchelor (rbatchelor@atmosph.physics.utoronto.ca)

Published by Copernicus Publications on behalf of the European Geosciences Union.

AMTD

2, 2881–2917, 2009

**Ground-based FTS
comparison and ACE
validation at Eureka
during IPY**

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

Abstract

The Canadian Arctic Atmospheric Chemistry Experiment Validation Campaigns have been carried out at Eureka, Nunavut (80.05° N, 86.42° W) during the polar sunrise period since 2004. During the International Polar Year (IPY) springs of 2007 and 2008, three ground-based Fourier transform infrared (FTIR) spectrometers were operated simultaneously. This paper presents a comparison of trace gas measurements of stratospherically important species involved in ozone depletion, namely O₃, HCl, ClONO₂, HNO₃ and HF, recorded with these three spectrometers. Total column densities of the gases measured with the new Canadian Network for the Detection of Atmospheric Change (CANDAC) Bruker 125HR are shown to agree to within 3.5% with the existing Environment Canada Bomem DA8 measurements. After smoothing both of these sets of measurements to account for the lower spectral resolution of the University of Waterloo Portable Atmospheric Research Interferometric Spectrometer for the Infrared (PARIS-IR), the measurements were likewise shown to agree with PARIS-IR to within 7%. Concurrent measurements of these gases were also made with the satellite-based Atmospheric Chemistry Experiment Fourier Transform Spectrometer (ACE-FTS) during overpasses of Eureka during these time periods. While one of the mandates of the ACE satellite mission is to study ozone depletion in the polar spring, previous validation exercises have identified the highly variable polar vortex conditions of the spring period to be a challenge for validation efforts. In this work, comparisons between the CANDAC Bruker 125HR and ACE-FTS have been used to develop strict criteria that allow the ground- and satellite-based instruments to be confidently compared. When these criteria are taken into consideration, there is shown to be no significant bias between the ACE-FTS and ground-based FTIR spectrometer for any of these gases.

AMTD

2, 2881–2917, 2009

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

1 Introduction

Ground-based instruments that measure the chemical composition of the atmosphere, through techniques such as solar-absorption spectroscopy, provide a key data set for the validation of satellite remote-sensing instruments (e.g., Dils et al., 2006; Vigouroux et al., 2007; Kerzenmacher et al., 2008; Dupuy et al., 2009). Biases and differences that are observed between ground-based and satellite instruments are, however, difficult to quantify due to the range of viewing geometries, and differences between individual instruments that are considered in a particular comparison. Side-by-side instrument intercomparisons, for example, have shown that total column densities of key stratospheric trace gases measured by ground-based Fourier transform infrared (FTIR) spectrometers may exhibit differences of several percent, even during times of stable atmospheric conditions and when retrieval algorithms are made as consistent as possible (Goldman et al., 1999; Griffith et al., 2003; Meier et al., 2005; Wunch et al., 2007; Batchelor et al., 2009). Validation of the Atmospheric Chemistry Experiment – Fourier Transform Spectrometer (ACE-FTS) has likewise shown large differences between ground-based and satellite instruments, particularly during the highly-variable Arctic spring-time (e.g., Wolff et al., 2008; Mahieu et al., 2008). Comparisons made under these conditions thus require a comprehensive understanding of both the validating instrument and the viewing geometry with respect to polar vortex dynamics.

The Canadian Arctic ACE Validation Campaigns have been carried out during the polar sunrise period at the Polar Environment Atmospheric Research Laboratory (PEARL) at Eureka, Nunavut, Canada (80.05° N, 86.42° W) since 2004 (Kerzenmacher et al., 2005; Fu et al., 2008; Fraser et al., 2008). The 2007 and 2008 campaigns extended from mid-February until mid-April, and were additionally complemented by instrumentation installed at PEARL by the Canadian Network for the Detection of Atmospheric Change during 2006. One of these additions was a high-resolution Bruker 125HR Fourier transform spectrometer (Batchelor et al., 2009). This allowed simultaneous measurements of atmospheric composition to be made throughout the cam-

AMTD

2, 2881–2917, 2009

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

paigned by four Fourier transform spectrometers: three ground-based and one satellite-borne.

This paper provides an in-depth intercomparison between the three ground-based FTIR spectrometers co-located at PEARL during the International Polar Year Canadian Arctic ACE Validation Campaigns of 2007 and 2008, and validation of ACE-FTS data from the same period. Meteorological conditions were quite different between the two campaigns, with many measurements in 2007 being made inside the polar vortex where heterogeneous chemistry and ozone-depleting processes were occurring. A polar stratospheric warming prior to the start of the campaign in 2008, however, resulted in most of the measurements being made outside the vortex. As such, the two years provide a wide range of atmospheric conditions for the intercomparison. Key stratospheric trace-gas species O_3 , chlorine reservoirs HCl and ClONO₂, fluorine reservoir HF and nitrogen reservoir HNO₃ are investigated. Derived meteorological data along the instruments' line-of-sight are used to account for the changing conditions of the polar stratosphere, and a comprehensive set of measurement comparison criteria are identified for satellite validation near the polar vortex edge.

The paper is laid out as follows: Section 2 introduces the measurement site and the four FTIR spectrometers. Section 3 details the methodology used for the analyses, and is followed by the detailed intercomparison of the three ground-based instruments in Sect. 4. Section 5 then extends the ground-based intercomparison to include and validate measurements from the ACE-FTS using the Bruker 125HR Fourier transform spectrometer, before finishing with conclusions in Sect. 6.

2 Measurement site and instrumentation

The Polar Environment Atmospheric Research Laboratory, situated on Ellesmere Island, Nunavut, Canada (80.05° N, 86.42° W, 610 m a.s.l.) is a modern, high-Arctic atmospheric research laboratory run by the Canadian Network for the Detection of Atmospheric Change (CANDAC). Atmospheric measurements made at PEARL sample

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



the atmosphere from the ground to 100 km. The PEARL site is situated 15 km from the Environment Canada Eureka Weather Station, and over 400 km from the nearest permanent settlement. At only 1100 km from the North Pole, it is a clean-air site in an ideal location for studying polar processes involved in ozone depletion. In addition, PEARL is ideally situated for the validation of polar-orbiting satellites, which typically pass nearby several times a day.

The three ground-based FTIR spectrometers in operation at PEARL during the 2007 and 2008 validation campaigns were the Environment Canada ABB Bomem DA8 (henceforth the DA8) and the CANDAC Bruker IFS 125HR (henceforth the 125HR), which were both permanently housed in the PEARL FTS lab, and the campaign-only University of Waterloo Portable Atmospheric Research Interferometric Spectrometer for the Infrared (PARIS-IR). The three spectrometers were physically located within meters of each other, and shared a common solar beam from a custom-built solar tracker located on the roof of the laboratory. Approximately 1/3 of the beam was directed to the PARIS-IR, and the other 2/3 was alternately directed to the 125HR and the DA8. Details of each of the instruments are given below.

2.1 Environment Canada ABB Bomem DA8

The Environment Canada ABB Bomem DA8 FTIR spectrometer was installed at PEARL in 1993 and has provided atmospheric solar absorption spectra each spring over the past fifteen years (Donovan et al., 1997; Farahani et al., 2007; Paton-Walsh et al., 2008; Fu et al., 2008; Fast et al., 2009). The DA8 spectrometer is a vertically aligned Michelson interferometer equipped with two separate detectors: an InSb and a HgCdTe (commonly known as an MCT). Used with a KBr beamsplitter and a set of narrow band interference filters, the DA8 can record radiation over the spectral range from 700 cm^{-1} to 5000 cm^{-1} at a resolution of 0.004 cm^{-1} (where resolution is defined as $1/\text{maximum optical path difference (MOPD)}$ and $\text{MOPD}=250\text{ cm}$). Eight interference filters are used in sequence in order to optimize the signal-to-noise ratio (SNR). Measurements each consist of four co-added spectra, taking approximately twelve minutes,

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Fourier transformed with a Hamming apodization.

2.2 CANDAC Bruker IFS 125HR

The CANDAC Bruker IFS 125HR FTIR spectrometer is a high-resolution spectrometer that was installed at PEARL in August 2006 and operates throughout the sunlit parts of the year. It has been described in depth by Batchelor et al. (2009). Like the DA8, the 125HR measures on either an InSb or MCT detector with a KBr beamsplitter and uses a sequence of narrow band interference filters covering the 600–4300 cm^{-1} spectral range. Solar absorption measurements made during the IPY Arctic campaigns each consist of four co-added spectra recorded in both the forwards and backwards directions (taking approximately six minutes) at a resolution of 0.004 cm^{-1} (MOPD=250 cm). No apodization is applied to these measurements.

2.3 University of Waterloo PARIS-IR

The University of Waterloo Portable Atmospheric Research Interferometric Spectrometer for the Infrared is an ABB Bomem custom-built interferometer that is based on the design of the Fourier transform spectrometer onboard the Atmospheric Chemistry Experiment, and is built from its spare parts. A resolution of 0.02 cm^{-1} (MOPD= ± 25 cm, with resolution defined to be consistent with the ACE-FTS, i.e. 0.5/MOPD) is achieved using corner cube reflectors mounted on a pivoting arm to introduce an optical path difference, as detailed in Fu et al. (2008). Interferograms are recorded on a sandwich InSb/MCT detector with no filters, allowing the entire 750–4400 cm^{-1} spectral region to be measured simultaneously. Each IPY spring measurement consists of 20 co-added spectra, taking approximately six minutes, with no applied apodization.

2.4 ACE-FTS

In addition to the three ground-based instruments, the Atmospheric Chemistry Experiment (also known as SCISAT) also made measurements over Eureka during the cam-

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



paigns. ACE was launched in August 2003, and orbits the Earth in a 74° inclined circular orbit (Bernath et al., 2005). One of its primary aims is to observe the polar regions during active periods of ozone depletion chemistry, notably during the polar springtime. As such, it has multiple measurements over Eureka during this time period.

5 The primary instrument onboard ACE is a Fourier transform spectrometer which simultaneously measures vertical profiles of more than 30 different atmospheric species, as well as temperature and pressure, using the solar occultation method (Bernath et al., 2005). The spectral range of the ACE-FTS is comparable to that of the ground-based FTIR spectrometers, with a spectral resolution of 0.02 cm^{-1} , however, the satellite-
10 borne spectrometer has considerably more vertical resolution (typically 3–4 km) than any of the ground-based instruments (Boone et al., 2005).

3 Data analysis

3.1 Ground-based FTIR spectrometers

15 Total column densities of O_3 , HCl, ClONO_2 , HNO_3 and HF covering the region between the ground and 100 km have been determined from the recorded spectra of each of the ground-based spectrometers in a consistent manner. Atmospheric profiles were retrieved from the spectra using SFIT2 (Pougatchev et al., 1995), a profile retrieval algorithm based on the optimal estimation technique of Rodgers (1976, 2000) whereby a calculated spectrum is fitted to the measured one by adjustment of the atmospheric
20 profile. Total column densities were determined by integrating the retrieved trace gas and atmospheric density profiles throughout the column. The HITRAN 2004+updates line list was used with SFIT2 v3.92c for the 125HR and PARIS-IR retrievals and v3.91 for the DA8 (the differences between the two versions being insignificant for this work). The retrieval parameters used have been described in Batchelor et al. (2009). The only
25 difference from that work is that for PARIS-IR, retrievals have been performed on a 29-rather than the 38-layer grid used for the DA8 and 125HR, to allow for its lower spectral

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

**Ground-based FTS
comparison and ACE
validation at Eureka
during IPY**R. L. Batchelor et al.

5 resolution. This has been previously shown to result in differences in the retrieved column of less than 0.6% (Wunch et al., 2007), but helps to reduce unphysical oscillations in the retrieved profile. A priori volume mixing ratio (VMR) profiles and covariances, described in Sung et al. (2009), were consistent for all three instruments, while ad hoc
10 SNR ratios, which are used for determining the measurement covariance, were selected for each gas for each instrument using the trade-off curve method described in Batchelor et al. (2009) to customize for the noise level in the spectra of the individual instruments. A summary of the spectral microwindows that have been fitted for each of the retrievals is presented in Table 1. The degrees of freedom of signal (DOFS),
15 defined in this case as the trace of the averaging kernel, as well as an estimated error in the total column is also given. These have been calculated for each of the gases as described in Batchelor et al. (2009).

3.2 ACE-FTS

15 Trace gas volume mixing ratio and temperature/pressure profiles are retrieved from ACE-FTS spectra with a nonlinear least squares global fitting algorithm, as detailed in Boone et al. (2005). Profiles are retrieved from the cloud tops, or approximately 5 km in clear conditions, to approximately 100 km. ACE-FTS v2.2 measurements (including updates for O₃, N₂O₅ and HDO) have been extensively validated against other
20 satellites and ground-based instruments, and show typical relative differences of 1–8% for O₃ (Dupuy et al., 2009), 5–10% for HCl (Mahieu et al., 2008), 1–14% for ClONO₂ (Wolff et al., 2008), 5–10% for HF (Mahieu et al., 2008) and 2–28% for HNO₃ (Wolff et al., 2008) globally through the stratosphere. Satellite validation near the polar vortex edge is, however, a challenge (as shown, for example, in Wolff et al., 2008; Mahieu et al., 2008) and as such, the validation of ACE during the highly variable Arctic sunrise period requires special consideration. This is the primary goal of the Canadian
25 Arctic ACE Validation Campaigns. Previous comparisons between trace gas columns measured by the DA8, PARIS-IR and ACE-FTS from 2004–2006 have been presented in Fu et al. (2008) and Sung et al. (2009). As in previous validation activities, this work

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

uses ACE-FTS v2.2+O₃ updates.

3.3 Derived meteorological products

Solar absorption measurements sample the air mass between the sun and the instrument along the line-of-sight. During the spring period, the solar zenith angle is large, and as such, the air mass being sampled at a given altitude may be a considerable distance from the instrument itself. To account for this, especially when considering the polar vortex and changes in chemistry occurring around its edge, meteorological products are derived at locations along the line-of-sight using the GEOS Version 5.0.1 (GEOS-5) analyses (Reinecker et al., 2007). These products are Derived Meteorological Products (DMPs), and in this work, have been calculated for both the ground- and satellite-based measurements at series of altitudes in the stratosphere, namely at 14, 18, 20, 22, 24, 26, 30, 36 and 46 km, with ground-based line-of-sight calculations as described in Fu et al. (2008) and satellite-based calculations as described in Manney et al. (2007). The DMPs include temperature, pressure, winds, potential temperature and scaled potential vorticity. A full description of the data set used can be found in Manney et al. (2007). Scaled potential vorticity (sPV) from the DMPs has been used in this work to differentiate the extra- and inner-vortex air masses at each altitude. An sPV of $1.2 \times 10^{-4} \text{ s}^{-1}$ has been used as a proxy for the outer edge of the polar vortex, while an sPV of $1.6 \times 10^{-4} \text{ s}^{-1}$ has been used for the inner edge (e.g., Manney et al., 2008).

4 Ground-based spectrometer intercomparison

4.1 Methodology

The 2007 and 2008 campaigns were designed to provide the best instrument comparison conditions possible for the time of the year. As previously discussed, the three FTIR

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

spectrometers shared a solar tracker, with the lower-resolution PARIS-IR measuring simultaneously with the alternately measuring 125HR and DA8 high-resolution instruments. Measurements with the high-resolution instruments were made successively with matching filters, in order to reduce the time between compared measurements, while PARIS-IR measured the full spectral range simultaneously.

During the polar spring period, the sun is very low and the air mass that is being sampled can vary considerably through the course of the day. As such, individual pairs of measurements from the ground-based instruments have been compared with stringent requirements for spatial and temporal agreement. This was made possible because the three instruments shared a solar tracker, thus were looking through identical or nearly identical air masses, and the measurements were made to maximize the agreement between similar measurements. PARIS-IR measurements were made simultaneously with those of the other two instruments, thus individual PARIS-IR measurements were compared with the corresponding DA8 and 125HR measurements that were less than six minutes apart in starting time. This represents the time taken for one PARIS-IR measurement. DA8 and 125HR measurements were recorded alternately, due to their larger solar beam requirements, and as such the time between compared measurements was necessarily larger. A limitation of 15 min between start times, allowing for the twelve minute interferogram recording time of the DA8 plus a couple of minutes to physically switch the beam between instruments, has been used.

While the 125HR and DA8 have near-identical spectral resolutions, and thus also see the atmosphere in a very similar way, PARIS-IR has a significantly lower spectral resolution. This results in a retrieved atmospheric profile that is less vertically resolved and more strongly influenced by the a priori profile than that retrieved by the higher-resolution instruments. The effect of this reduced resolution has been investigated in this work. Comparisons were first made without accounting for the difference in resolution in the retrieved profile, and were then repeated using total columns for the high-resolution instruments that were smoothed using the PARIS-IR averaging kernel, as described in Rodgers and Connor (2003). To do this, each profile retrieved by

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

the higher-resolution instruments was interpolated to the PARIS-IR retrieval grid and smoothed using a representative PARIS-IR averaging kernel and a priori VMR profile, following Eq. (1) (reproduced from Rodgers and Connor, 2003, Eq. 4):

$$\mathbf{x}_s = \mathbf{x}_a + \mathbf{A}(\mathbf{x}_h - \mathbf{x}_a) \quad (1)$$

where \mathbf{x}_s is the smoothed profile, \mathbf{x}_a is the PARIS-IR a priori profile (which, in this case, was identical to that used by the other two instruments), \mathbf{A} is the PARIS-IR averaging kernel and \mathbf{x}_h is the high-resolution instrument's retrieved profile. Total columns were then determined from the smoothed profile, using air mass densities derived from the daily pressure and temperature profiles measured over Eureka (Batchelor et al., 2009).

4.2 Results and discussion

Total column measurements of O_3 , HCl, ClONO_2 , HNO_3 and HF, as retrieved without accounting for the smoothing in the lower-resolution PARIS-IR, are shown in Fig. 1 for the 2007 and 2008 campaigns. Note that the very weak ClONO_2 absorption features mean that retrievals are not reliable for PARIS-IR, and thus have not been included. Also shown in Fig. 1 is the scaled potential vorticity through the mid-stratosphere (at 18, 22 and 26 km), indicating the conditions of the measurements relative to the vortex edge. The very different dynamical conditions over Eureka during these two years are clear, with measurements in 2007 being made well inside the polar vortex from approximately days 67 to 83, and measurements during 2008 being made no further in than the edge of the vortex region throughout the campaign. Thus measurements made during 2007 are more likely to sample air that has been subject to ozone-depleting chemical processes than those made during 2008. Consistent between the two years, however, is the comparison between the three FTIR spectrometers. The DA8 and 125HR show excellent agreement, with the range of variation over each spring in all of the gases being well captured. The agreement with PARIS-IR is more variable. For O_3 and HCl, the comparison is excellent, while there is an obvious bias in the HNO_3 results. Through both years, PARIS-IR consistently under estimates the total column

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



of this gas, with the bias being greater when the HNO_3 column is large. In HF, there are high biases in the PARIS-IR data at the highest solar zenith angles, early in the campaigns, but these disappear by about day 75 when the sun is slightly higher in the sky.

5 From the properties of the HNO_3 bias, we suspected that the cause of the difference between the FTIR spectrometers was due to a higher contribution of the a priori to the lower-resolution instrument's retrievals. During this time of year, our climatological mean a priori column (derived from the SPARC 2000 climatology averaged over latitudes greater than 68° N during the sunlit parts of the year) is considerably lower than
10 the real HNO_3 columns, which have been building up throughout the polar night. If this was indeed the cause of the discrepancy, then smoothing the profiles retrieved with the higher-resolution instruments by the PARIS-IR averaging kernel and a priori profile should result in a better comparison. Figure 2 illustrates the smoothing process. In the top panel, the unsmoothed 125HR HNO_3 total columns for 2008 are shown with the corresponding PARIS-IR columns. The a priori column is also plotted, showing clearly that the a priori is much lower than the columns retrieved from the measurements. The slight variation in the a priori column from day to day reflects the changing atmospheric density profile. The middle panel shows the 125HR HNO_3 columns before (red) and after (cyan) they have been smoothed using Eq. (1). The smoothing effect inherent in
15 the lower-resolution PARIS-IR retrievals is clear – the smoothed 125HR measurements are typically much closer to the a priori than the unsmoothed ones. The new comparison between PARIS-IR and the 125HR (smoothed) is shown in the bottom panel, and the improvement in the comparison is significant. A correlation plot highlighting the improvement in the correlation between the HNO_3 columns after the smoothing is shown in Fig. 3.
20
25

It should be noted that under these conditions, we expect that the absolute values measured by the higher-resolution 125HR and DA8 instruments would be more representative of the true atmosphere than those measured by PARIS-IR, due to the lower information content in the PARIS-IR measurements. The smoothing effects of the in-

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

struments are, however, largely taken into consideration in the error budget, with higher quoted uncertainties for the PARIS-IR total columns (Table 1) reflecting the higher uncertainty relating to the greater smoothing in these measurements.

The smoothing process was applied to the retrieved 125HR and DA8 profiles in a similar manner for each of the other gases, and the revised time series (excluding ClONO₂) are shown in Fig. 4. A summary of the comparisons, including mean difference, standard deviation and correlation for both the smoothed and unsmoothed total column comparisons and incorporating both 2007 and 2008 data to cover a wide range of conditions, is shown in Table 2.

For the two gases for which the biggest biases were seen in Fig. 1, notably HNO₃ and HF, the agreement between the three spectrometers is substantially improved by accounting for the differences in resolution. The fact that the difference in O₃ columns increases with smoothing is unfortunate but real – there is much more sensitivity to the vertical distribution of the gas for the 125HR and DA8 than for PARIS-IR, as shown by the DOFS in Table 1. During this time of year, when the path of the sunlight through the atmosphere is very long, there may be considerable differences in the distribution of trace gases along the line-of-sight. Having more vertical information thus helps with the correct profile distribution of the gas, variations of which can have quite substantial effects on the column. As the information content in the O₃ measurements in particular is so high, it is thus not surprising to see a significant change to the 125HR/DA8 O₃ column after accounting for the vertical profile smoothing effect quantified by the PARIS-IR averaging kernel. Fortunately the difference in total columns between the instruments is still fairly small, and, as for all of the compared gases after smoothing, well within the error estimates of the individual measurements.

After accounting for the larger smoothing effect of the lower resolution PARIS-IR, the total column differences between the three spectrometers are less than 3.5% for the 125HR and DA8, and less than 6.5% for the comparisons between the 125HR or DA8 and the PARIS-IR. These differences are comparable in magnitude with other side-by-side instrument comparisons carried out at Eureka (Fu et al., 2008; Paton-Walsh et al.,

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

2009; Batchelor et al., 2009) and around the globe (Goldman et al., 1999; Meier et al. 2005; Griffiths et al., 2005; Wunch et al., 2007).

5 Ground- and satellite-based spectrometer intercomparison

5.1 Methodology

5 Having shown that measurements from the three ground-based spectrometers are comparable, validation of the satellite-based ACE-FTS has been carried out using just the 125HR. Following standard conventions, spectra were considered coincident if the 125HR and ACE-FTS measurements were recorded within 12 h and the distance between the ACE 30-km tangent point and PEARL was less than 1000 km.

10 Due to the difference in altitude sensitivity between the two instruments, partial, rather than total, column densities have been compared using ACE-FTS profiles smoothed to the resolution of the 125HR, as described by Eq. (1). As in previous validation activities, for this comparison, each ACE-FTS profile was interpolated to the 38-layer altitude grid used for the 125HR retrievals, and then smoothed with the 125HR
15 averaging kernel and a priori profile corresponding to the matching 125HR spectrum. In the tropospheric region where no ACE-FTS data were available, the profile values were filled with the corresponding 125HR's a priori profile for the calculation. Partial columns were then determined for each measurement pair for the altitude range for which ACE-FTS data existed for that measurement and where the sensitivity of the
20 125HR measurement, as determined from the sums of each row of the averaging kernel matrix, was at least 0.5 (Vigouroux et al., 2007; Wolff et al., 2008; Kerzenmacher et al., 2008).

Comparisons were made for O_3 , HCl, HF, HNO_3 , and $ClONO_2$, with the mean and standard deviation of the differences between each pair of ACE-FTS and 125HR partial
25 column values calculated. While the exact altitude range included in the partial column varied from pair to pair, these typically ranged from approximately 6–43 km (O_3), 8–

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

38 km (HCl), 15–26 km (ClONO₂), 8–29 km (HNO₃) and 10–43 km (HF). Attempts to quantify the causes of differences in the partial columns determined from each spectrometer were investigated using the DMPs described in Sect. 3, and were used to further enhance the coincidence criteria.

5.2 Results and discussion

Figure 5 shows the partial columns, the percentage differences between the ACE-FTS and 125HR measurements (using $(ACE-FTS - 125HR)/125HR$), the distance between the two measurements, and the sPV for each of the gases for 2007 (top) and 2008 (bottom), respectively. The sPV along the line-of-sight has been determined for both the ACE-FTS and the 125HR as described in Sect. 3. From the number density profiles of each gas, it was determined that peak values were typically at approximately 18 km, thus sPV values from that altitude were used as a proxy for the dynamical conditions being experienced for each measurement.

From the plot, we can see that while sometimes the partial columns measured by the two spectrometers are comparable, at other times there are considerable differences. Occasionally these differences can be explained by either the physical distance between the measurements or by the fact that one measurement is recorded inside the polar vortex while the other is recorded outside (for example the HCl measurements on day 64, 2007). At other times, however, this does not fully explain the differences (for example on day 70, 2007 for the HF measurements). The differences observed between the ACE-FTS and 125HR using these simple time and location criteria, i.e., 12 h and 1000 km (from 30-km tangent point to PEARL) are shown in Table 3.

From Table 3, some significant differences in the mean and especially in the standard deviation can be seen between the two years, with the more dynamically variable 2007 in most cases showing greater scatter in the differences (as seen by the standard deviation) than in the more dynamically quiet 2008. We believe this reflects the number of measurements that capture spectra measured in different locations relative to the location of the polar vortex. While the mean differences determined by this comparison are

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



comparable to those determined in previous ACE-FTS validation exercises, we took the investigation a step further to better single out measurement pairs that should be comparable due to well-matched atmospheric conditions, thus improving our confidence in the quality of the comparison.

5 Looking first at the distance-between-measurements criterion, we determined that the 1000-km criterion, as measured from the ACE 30-km tangent point to the station, was not a particularly accurate representation of the distance between the actual air masses being sampled. Based on the derived meteorological product determinations of the longitude and latitude along the lines-of-sight of the measurement, we found
10 that some measurements meeting the 1000-km criterion were actually sampling air masses that were more than 1000 km apart, while other measurements which sampled air masses that were closer than 1000 km together were being excluded. An example of this is shown in Fig. 6, which shows two sets of differences for the 2007 O₃ comparison. The distance between the ACE 30-km tangent point and PEARL is shown
15 in black and the distance between the 18-km altitudes along the lines-of-sights of both the ACE and 125HR measurements is shown in orange. In order to ensure that all measurements that were within 1000 km of each other throughout the partial column were included, our ACE-FTS measurement sample was expanded to include all measurements within 2000 km of PEARL (based on the 30-km tangent point altitude), in
20 order to subsequently filter them to 1000 km based on the distance between measurement points within the partial column. We also investigated the time criterion, but found little difference in the combinations that would be used for the comparison if the time criterion was set for 6, 12 or 18 h. This was a result of the limitation of sunlight for the ground-based instruments and the sunrise/sunset viewing geometry of the ACE-FTS.

25 To further refine the comparisons, for each pair, a plot of the sPV at each of the eight DMP altitudes along the line-of-sight for each instrument was constructed, with only those altitudes within the corresponding partial column altitude range being considered. Additional plots showing the temperature at each DMP location, the retrieved volume mixing ratio, and the distance between the measurement points were con-

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

structured. Examples of two of these plots, one showing a good match, and one showing a poor match, are shown in Figs. 7 and 8, respectively.

From these plots, we were able to determine whether the measurement conditions being sampled by the two instruments were similar throughout the height range of each comparison. The sPV and temperature profiles provided key information on the air mass with respect to the polar vortex and likely chemical processing conditions within, while the distance plot provided a measure of the physical separation of the sampled air masses. The retrieved VMR profiles provided additional information on where in the partial column the measurements were diverging. Note that the profiles shown for the ACE-FTS are the smoothed profiles, thus the smoothing effect of the 125HR has been taken into consideration. From the plots, it was clear that the sPV along the lines-of-sight was an important comparison criterion, as cases when both measurements were inside or both were outside, or even both measured through the vortex edge typically showed good agreement in the partial columns, while pairs for which the sPV was divergent typically had poorer agreement, as would be expected from the different air masses sampled. Temperature served as an additional important criterion, as within the polar vortex, chemical processing is highly dependent on temperature. As such, significant differences in temperature along the lines-of-sight for the two profiles, even when the sPV is similar, can indicate large differences in the sampled air masses.

Using the information gained by the plots, more rigorous coincidence criteria were developed to better identify comparable measurement pairs. While the temporal criterion of 12 h remained, the spatial coincidence criterion was tightened, requiring the distance between the measurement points at each of the DMP altitudes (rather than solely for the ACE 30-km tangent point to PEARL) to be within 1000 km. Differences in sPV between the two measurements at each altitude along the line-of-sight were restricted to less than $0.3 \times 10^{-4} \text{ s}^{-1}$, ensuring that the air masses relative to the polar vortex edge were similar for both measurements. Finally, the maximum temperature difference at each altitude point was set to 10 K.

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

**Ground-based FTS
comparison and ACE
validation at Eureka
during IPY**R. L. Batchelor et al.

The mean percentage differences between the pairs remaining after these new criteria were applied, as well as the standard deviations, are shown in Table 4. It can be seen that these stringent comparison requirements have significantly reduced the number of pairs contributing to the comparisons, particularly in 2007 when measurements made at Eureka were frequently near the edge of the polar vortex. However, both the mean differences and standard deviations between the two measurements have typically been reduced, and we are confident that these measurement pairs are highly comparable. Having applied the stringent criteria, the differences between the two instruments are in agreement with previous ground-based FTIR/ACE-FTS comparisons of these five gases (Dupuy et al., 2009; Mahieu et al., 2008; Wolff et al., 2008). No clear bias is seen from year-to-year, and, in all cases, the difference between the measurements is zero to within one standard deviation. As such, we can confidently say that the ACE-FTS shows excellent agreement with ground-based spectroscopic measurements made in the highly-variable spring-time northern polar stratosphere.

6 Conclusions

The 2007 and 2008 Canadian Arctic ACE Validation Campaigns at Eureka, Nunavut, have provided an excellent opportunity to compare measurements by four Fourier transform infrared spectrometers during the highly-variable Arctic polar sunrise period. Comparisons between the three ground-based FTIR spectrometers have shown small inter-instrumental differences well within the estimated uncertainties of the measurements and consistent with side-by-side intercomparisons conducted around the world. Total column trace gas measurements of O₃, HCl, ClONO₂, HF and HNO₃ made with the higher-resolution CANDAC Bruker 125HR were shown to compare with the comparable resolution Environment Canada ABB Bomem DA8 to within 3.5%. Measurements of O₃, HCl, HF and HNO₃ from both of these instruments were shown to agree to within 6.5% with the lower-resolution University of Waterloo PARIS-IR when the higher-resolution instruments' retrieved profiles were smoothed with the a priori profiles and

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

averaging kernels of PARIS-IR to account for the larger smoothing effect of that instrument. The importance of this smoothing was demonstrated, particularly for cases when the atmospheric total column is considerably different from the a priori value.

Validation of the ACE-FTS v2.2 (with O₃ updates) results from this time was also carried out with the 125HR. Strict coincidence criteria for use around the polar vortex were determined, utilizing DMP data along the lines-of-sight of both instruments. These criteria were: measurement times less than 12 h; distance between measurement points at multiple altitudes within the partial column less than 1000 km; differences in sPV between measurements at multiple altitudes within the partial column less than $0.3 \times 10^{-4} \text{ s}^{-1}$; and temperature differences at each altitude less than 10 K. After applying these criteria, the mean biases between the ACE-FTS and 125HR for 2007/2008 were 1.1/−1.5%, 4.9/−0.2%, −2.9/−15.3%, 1.1/−4.8% and 5.2/1.1% for O₃, HCl, ClONO₂, HNO₃, and HF, respectively, and within one standard deviation in all cases. Thus it can be concluded that satellite validation can be conducted with ground-based measurements made around the polar vortex edge, provided that comparison criteria are enhanced to account for vortex conditions along the line-of-sight, and that no significant bias can be identified in the ACE-FTS partial columns at this time of year.

Acknowledgements. This work would not have been possible without the support of the Canadian Space Agency (CSA), the Environment Canada (EC) Eureka Weather Station, and the Canadian Network for the Detection of Atmospheric Change (CANDAC). We particularly acknowledge the assistance of the CANDAC Operations Team, J. Drummond (Principal Investigator), P. Fogal (PEARL Facilities Manager), A. Harrett, A. Khmel, P. Loewen, O. Mikhailov and M. Okraszewski for their assistance in collecting the measurements and transporting us between the lab and the station, and the EC meteorological technicians for launching many radio- and ozone-sonde balloons for us. The Canadian Arctic ACE Validation Campaigns are supported by the CSA, EC, Natural Sciences and Engineering Research Council (NSERC) and the Northern Scientific Training Program. CANDAC and PEARL are funded by the Atlantic Innovation Fund/Nova Scotia Research Innovation Trust, Canadian Foundation for Climate and Atmospheric Sciences (CFCAS), Canadian Foundation for Innovation, CSA, EC, Government of Canada IPY funding, NSERC, Ontario Innovation Trust, Ontario Research Fund and the Po-

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



lar Continental Shelf Program. Work carried out at the Jet Propulsion Laboratory, California Institute of Technology was done under contract with the National Aeronautics and Space Administration. The Atmospheric Chemistry Experiment, also known as SCISAT, is a Canadian-led mission mainly supported by the CSA and NSERC.

5 References

Batchelor, R. L., Strong, K., Lindenmaier, R. L., Mittermeier, R., Fast, H., Drummond, J. R., and Fogal, P. F.: A new Bruker IFS 125HR FTIR spectrometer for the Polar Environment Atmospheric Research Laboratory at Eureka, Canada – measurements and comparison with the existing Bomem DA8 spectrometer, *J. Atmos. Ocean. Tech.*, 26, 1328–1340, doi:10.1175/2009JTECHA1215.1, 2009.

Bernath, P. F., McElroy, C. T., Abrams, M. C., Boone, C. D., Butler, M., Camy-Peyret, C., Carleer, M., Clerbaux, C., Coheur, P.-F., Colin, R., DeCola, P., DeMaziere, M., Drummond, J. R., Dufour, D., Evans, W. F. J., Fast, H., Fussen, D., Gilbert, K., Jennings, D. E., Llewellyn, E. J., Lowe, R. P., Mahieu, E., McConnell, J. C., McHugh, M., McLeod, S. D., Michaud, R., Midwinter, C., Nassar, R., Nichitiu, F., Nowlan, C., Rinsland, C. P., Rochon, Y. J., Rowlands, N., Semeniuk, K., Simon, P., Skelton, R., Sloan, J. J., Soucy, M.-A., Strong, K., Tremblay, P., Turnbull, D., Walker, K. A., Walkty, I., Wardle, D. A., Wehrle, V., Zander, R., and Zou, J.: Atmospheric Chemistry Experiment (ACE): mission overview, *Geophys. Res. Lett.*, 32, L15S01, doi:10.1029/2005GL022386, 2005.

Boone, C. D., Nassar, R., Walker, K. A., Rochon, Y., McLeod, S. D., Rinsland, C. P., and Bernath, P. F.: Retrievals for the Atmospheric Chemistry Experiment Fourier Transform Spectrometer, *Appl. Optics*, 44, 7218–7231, 2005.

Dils, B., De Mazière, M., Müller, J. F., Blumenstock, T., Buchwitz, M., de Beek, R., Demoulin, P., Duchatelet, P., Fast, H., Frankenberg, C., Gloudemans, A., Griffith, D., Jones, N., Kerzenmacher, T., Kramer, I., Mahieu, E., Mellqvist, J., Mittermeier, R. L., Notholt, J., Rinsland, C. P., Schrijver, H., Smale, D., Strandberg, A., Straume, A. G., Stremme, W., Strong, K., Sussmann, R., Taylor, J., van den Broek, M., Velazco, V., Wagner, T., Warneke, T., Wiacek, A., and Wood, S.: Comparisons between SCIAMACHY and ground-based FTIR data for total columns of CO, CH₄, CO₂ and N₂O, *Atmos. Chem. Phys.*, 6, 1953–1976, 2006, <http://www.atmos-chem-phys.net/6/1953/2006/>.

AMTD

2, 2881–2917, 2009

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

Donovan, D. P., Fast, H., Makino, Y., Bird, J. C., Carswell, A. I., Davies, J., Duck, T. J., Kaminski, J. W., McElroy, C. T., Mittermeier, R. L., Pal, S. R., Savastiouk, V., Velkov, D., and White-
way, J. A.: Ozone, column ClO, and PSC measurements made at the NDSC Eureka Ob-
servatory (80° N, 86° W) during the spring of 1997, *Geophys. Res. Lett.*, 24, 2709–2712,
1997.

Dupuy, E., Walker, K. A., Kar, J., Boone, C. D., McElroy, C. T., Bernath, P. F., Drummond, J. R.,
Skelton, R., McLeod, S. D., Hughes, R. C., Nowlan, C. R., Dufour, D. G., Zou, J., Nichitiu, F.,
Strong, K., Baron, P., Bevilacqua, R. M., Blumenstock, T., Bodeker, G. E., Borsdorff, T.,
Bourassa, A. E., Bovensmann, H., Boyd, I. S., Bracher, A., Brogniez, C., Burrows, J. P.,
Catoire, V., Ceccherini, S., Chabrillat, S., Christensen, T., Coffey, M. T., Cortesi, U., Davies, J.,
De Clercq, C., Degenstein, D. A., De Mazière, M., Demoulin, P., Dodion, J., Firanski, B., Fis-
cher, H., Forbes, G., Froidevaux, L., Fussen, D., Gerard, P., Godin-Beekmann, S., Goutail, F.,
Granville, J., Griffith, D., Haley, C. S., Hannigan, J. W., Höpfner, M., Jin, J. J., Jones, A.,
Jones, N. B., Jucks, K., Kagawa, A., Kasai, Y., Kerzenmacher, T. E., Kleinböhl, A., Kleko-
ciuk, A. R., Kramer, I., Küllmann, H., Kuttippurath, J., Kyrölä, E., Lambert, J.-C., Livesey, N. J.,
Llewellyn, E. J., Lloyd, N. D., Mahieu, E., Manney, G. L., Marshall, B. T., McConnell, J. C., Mc-
Cormick, M. P., McDermid, I. S., McHugh, M., McLinden, C. A., Mellqvist, J., Mizutani, K., Mu-
rayama, Y., Murtagh, D. P., Oelhaf, H., Parrish, A., Petelina, S. V., Piccolo, C., Pommereau, J.-
P., Randall, C. E., Robert, C., Roth, C., Schneider, M., Senten, C., Steck, T., Strandberg, A.,
Strawbridge, K. B., Sussmann, R., Swart, D. P. J., Tarasick, D. W., Taylor, J. R., Tétard, C.,
Thomason, L. W., Thompson, A. M., Tully, M. B., Urban, J., Vanhellemont, F., Vigouroux, C.,
von Clarmann, T., von der Gathen, P., von Savigny, C., Waters, J. W., Witte, J. C., Wolff, M.,
and Zawodny, J. M.: Validation of ozone measurements from the Atmospheric Chemistry
Experiment (ACE), *Atmos. Chem. Phys.*, 9, 287–343, 2009,

<http://www.atmos-chem-phys.net/9/287/2009/>.

Farahani, E. E., Fast, H., Mittermeier, R. L., Makino, Y., Strong, K., McLandress, C., Shep-
herd, T. G., Chipperfield, M. P., Hannigan, J. W., Coffey, M. T., Mikuteit, S., Hase, F., Blumen-
stock, T., and Raffalski, U.: Nitric acid measurements at Eureka obtained in winter 2001–
2002 using solar and lunar Fourier transform absorption spectroscopy: comparisons with
observations at Thule and Kiruna and with results from three-dimensional models, *J. Geo-
phys. Res.*, 112, D01305, doi:10.1029/2006JD00709605, 2007.

Fraser, A., Goutail, F., Strong, K., Bernath, P. F., Boone, C., Daffer, W. H., Drummond, J. R.,
Dufour, D. G., Kerzenmacher, T. E., Manney, G. L., McElroy, C. T., Midwinter, C., McLin-

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

den, C. A., Nichitiu, F., Nowlan, C. R., Walker, J., Walker, K. A., Wu, H., and Zou, J.: Inter-comparison of UV-visible measurements of ozone and NO₂ during the Canadian Arctic ACE validation campaigns: 2004–2006, *Atmos. Chem. Phys.*, 8, 1763–1788, 2008, <http://www.atmos-chem-phys.net/8/1763/2008/>.

5 Fast, H., Mittermeier, R. L., and Makino, Y.: A ten-year record of Arctic trace gas total column measurements at Eureka, from 1997 to 2006, using the Bomem DA8 Fourier transform spectrometer, in preparation, 2009.

Fu, D., Walker, K. A., Mittermeier, R. L., Strong, K., Sung, K., Fast, H., Bernath, P. F., Boone, C. D., Daffer, W. H., Fogal, P., Kolonjari, F., Loewen, P., Manney, G. L., and
10 Mikhailov, O.: Simultaneous atmospheric measurements using two Fourier transform infrared spectrometers at the Polar Environment Atmospheric Research Laboratory during spring 2006, and comparisons with the Atmospheric Chemistry Experiment-Fourier Transform Spectrometer, *Atmos. Chem. Phys. Discuss.*, 8, 5305–5358, 2008, <http://www.atmos-chem-phys-discuss.net/8/5305/2008/>.

15 Goldman, A., Paton-Walsh, C., Bell, W., Toon, G. C., Blavier, J.-F., Sen, B., Coffey, M. T., Hannigan, J. W., and Mankin, W. G.: Network for the detection of stratospheric change Fourier transform infrared intercomparison at Table Mountain facility, November 1996, *J. Geophys. Res.*, 104, 30481–30503, 1999.

Griffith, D. W. T., Jones, N. B., McNamara, B., Walsh, C. P., Bell, W., and Bernardo, C.: Inter-comparison of NDSC Ground-Based Solar FTIR Measurements of Atmospheric Gases at
20 Lauder, New Zealand, *J. Atmos. Ocean. Tech.*, 20, 1138–1153, 2003.

Kerzenmacher, T. E., Walker, K. A., Strong, K., Berman, R., Bernath, P. F., Boone, C. D., Drummond, J. R., Fast, H., Fraser, A., MacQuarrie, K., Midwinter, C., Sung, K., McElroy, C. T., Mittermeier, R. L., Walker, J., and Wu, H. J.: Measurements of O₃, NO₂ and temperature during the 2004 Canadian Arctic ACE Validation Campaign, *Geophys. Res. Lett.*, 32, L16S07, doi:10.1029/2005GL023032, 2005.

25 Kerzenmacher, T., Wolff, M. A., Strong, K., Dupuy, E., Walker, K. A., Amekudzi, L. K., Batchelor, R. L., Bernath, P. F., Berthet, G., Blumenstock, T., Boone, C. D., Bramstedt, K., Brogniez, C., Brohede, S., Burrows, J. P., Catoire, V., Dodion, J., Drummond, J. R., Dufour, D. G., Funke, B., Fussen, D., Goutail, F., Griffith, D. W. T., Haley, C. S., Hendrick, F., Höpfner, M., Huret, N., Jones, N., Kar, J., Kramer, I., Llewellyn, E. J., López-Puertas, M., Manney, G., McElroy, C. T., McLinden, C. A., Melo, S., Mikuteit, S., Murtagh, D., Nichitiu, F., Notholt, J.,
30 Nowlan, C., Piccolo, C., Pommereau, J.-P., Randall, C., Raspollini, P., Ridolfi, M., Richter, A.,

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

Schneider, M., Schrems, O., Silicani, M., Stiller, G. P., Taylor, J., Tétard, C., Toohey, M., Vanhellefont, F., Warneke, T., Zawodny, J. M., and Zou, J.: Validation of NO₂ and NO from the Atmospheric Chemistry Experiment (ACE), *Atmos. Chem. Phys.*, 8, 5801–5841, 2008, <http://www.atmos-chem-phys.net/8/5801/2008/>.

5 Mahieu, E., Duchatelet, P., Demoulin, P., Walker, K. A., Dupuy, E., Froidevaux, L., Randall, C., Catoire, V., Strong, K., Boone, C. D., Bernath, P. F., Blavier, J.-F., Blumenstock, T., Coffey, M., De Mazière, M., Griffith, D., Hannigan, J., Hase, F., Jones, N., Jucks, K. W., Kagawa, A., Kasai, Y., Mebarki, Y., Mikuteit, S., Nassar, R., Notholt, J., Rinsland, C. P., Robert, C., Schrems, O., Senten, C., Smale, D., Taylor, J., Tétard, C., Toon, G. C., Warneke, T.,
10 Wood, S. W., Zander, R., and Servais, C.: Validation of ACE-FTS v2.2 measurements of HCl, HF, CCl₃F and CCl₂F₂ using space-, balloon- and ground-based instrument observations, *Atmos. Chem. Phys.*, 8, 6199–6221, 2008, <http://www.atmos-chem-phys.net/8/6199/2008/>.

Manney, G. L., Daffer, W. H., Strawbridge, K. B., Walker, K. A., Boone, C. D., Bernath, P. F.,
15 Kerzenmacher, T., Schwartz, M. J., Strong, K., Sica, R. J., Krüger, K., Pumphrey, H. C., Lambert, A., Santee, M. L., Livesey, N. J., Remsberg, E. E., Mlynczak, M. G., and Russell III, J. R.: The high Arctic in extreme winters: vortex, temperature, and MLS and ACE-FTS trace gas evolution, *Atmos. Chem. Phys.*, 8, 505–522, 2008, <http://www.atmos-chem-phys.net/8/505/2008/>.

20 Manney, G. L., Daffer, W. H., Zawodny, J. M., Bernath, P. F., Hoppel, K. W., Walker, K. A., Knosp, B. W., Boone, C., Remsberg, E. E., Santee, M. L., Harvey, V. L., Pawson, S., Jackson, D. R., Deaver, L., McElroy, C. T., McLinden, C. A., Drummond, J. R., Pumphrey, H. C., Lambert, A., Schwartz, M. J., Froidevaux, L., McLeod, S., Takacs, L. L., Suarez, M. J., Trepte, C. R., Cuddy, D. C., Livesey, N. J., Harwood, R. S., and Waters, J. W.: Solar occultation satellite data and derived meteorological products: sampling issues and comparisons with Aura Microwave Limb Sounder, *J. Geophys. Res.*, 112, D24S50, doi:10.1029/2007JD008709, 2007.

Meier, A., Paton-Walsh, C., Bell, W., Blumenstock, T., Hase, F., Goldman, A., Steen, A., Kift, R., Woods, P., and Kondo, Y.: Evidence of reduced measurement uncertainties from an FTIR instrument intercomparison at Kiruna, Sweden, *J. Quant. Spectrosc. Ra.*, 96, 75–84, 2005.

30 Paton-Walsh, C., Mittermeier, R. L., Bell, W., Fast, H., Jones, N., and Meier, A.: An intercomparison of ground-based solar FTIR measurements of atmospheric gases at Eureka, Canada, *J. Atmos. Ocean. Tech.*, 25, 2028–2036, doi:10.1175/2008JTECHA1060.1, 2008.

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

**Ground-based FTS
comparison and ACE
validation at Eureka
during IPY**

R. L. Batchelor et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

- Pougatchev, N. S., Connor, B. J., and Rinsland, C. P.: Infrared measurements of the ozone vertical distribution above Kitt Peak, *J. Geophys. Res.*, 100(D8), 16689–16697, 1995.
- Rodgers, C. D.: Retrieval of atmospheric temperature and composition from remote measurements of thermal radiation, *Rev. Geophys. Space Ge.*, 14, 609–624, 1976.
- 5 Rodgers, C. D.: *Inverse Methods for Atmospheric Sounding: Theory and Practice*, World Scientific Publishing Co. Pte. Ltd, Singapore, 238 pp., 2000.
- Rodgers, C. D. and Connor, B. J.: Intercomparison of remote sounding instruments, *J. Geophys. Res.*, 108(D3), 4116, doi:10.1029/2002JD002299, 2003.
- Sung, K., Strong, K., Mittermeier, R. L., Walker, K. A., Fu, D., Kerzenmacher, T., Fast, H.,
10 Bernath, P. F., Boone, C. D., Daffer, W. H., Drummond, J. R., Kolonjari, F., Loewen, P., MacQuarrie, K., and Manney, G. L.: Ground-based column measurements at Eureka, Nunavut made with two FT-IR spectrometers in spring 2004 and 2005, and comparisons with the ACE-FTS, in preparation, 2009.
- Vigouroux, C., De Mazière, M., Errera, Q., Chabrilat, S., Mahieu, E., Duchatelet, P., Wood, S.,
15 Smale, D., Mikuteit, S., Blumenstock, T., Hase, F., and Jones, N.: Comparisons between ground-based FTIR and MIPAS N₂O and HNO₃ profiles before and after assimilation in BASCOE, *Atmos. Chem. Phys.*, 7, 377–396, 2007,
<http://www.atmos-chem-phys.net/7/377/2007/>.
- Wunch, D., Taylor, J. R., Fu, D., Bernath, P., Drummond, J. R., Midwinter, C., Strong, K., and
20 Walker, K. A.: Simultaneous ground-based observations of O₃, HCl, N₂O and CH₄ over Toronto, Canada by three Fourier transform spectrometers with different resolutions, *Atmos. Chem. Phys.*, 7, 1275–1292, 2007,
<http://www.atmos-chem-phys.net/7/1275/2007/>.
- Wolff, M. A., Kerzenmacher, T., Strong, K., Walker, K. A., Toohey, M., Dupuy, E., Bernath, P. F.,
25 Boone, C. D., Brohede, S., Catoire, V., von Clarmann, T., Coffey, M., Daffer, W. H., De Mazière, M., Duchatelet, P., Glatthor, N., Griffith, D. W. T., Hannigan, J., Hase, F., Höpfner, M., Huret, N., Jones, N., Jucks, K., Kagawa, A., Kasai, Y., Kramer, I., Küllmann, H., Kuttippurath, J., Mahieu, E., Manney, G., McElroy, C. T., McLinden, C., Mébarki, Y., Mikuteit, S., Murtagh, D., Piccolo, C., Raspollini, P., Ridolfi, M., Ruhnke, R., Santee, M., Senten, C.,
30 Smale, D., Tétard, C., Urban, J., and Wood, S.: Validation of HNO₃, ClONO₂, and N₂O₅ from the Atmospheric Chemistry Experiment Fourier Transform Spectrometer (ACE-FTS), *Atmos. Chem. Phys.*, 8, 3529–3562, 2008,
<http://www.atmos-chem-phys.net/8/3529/2008/>.

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Table 1. Summary of retrieval microwindows and interfering species, with estimated total uncertainty and DOFS. Multiple microwindows are fitted simultaneously where more than one region is specified. Interfering trace gas species are scale fitted, unless profile fitting is indicated by a (P). Total uncertainty has been calculated, with individual uncertainties resulting from measurement, smoothing and model parameter errors added in quadrature, as described in Batchelor et al., 2009. The DOFS are representative values for spectra recorded at the beginning of March, when solar zenith angles of are typically $>80^\circ$. Abbreviations used in the headers are 125=125HR and PIR=PARIS-IR.

Gas	Micro-window(s) (cm^{-1})	Interfering Species	Total Uncertainty			DOFS		
			(%)			125	DA8	PIR
			125	DA8	PIR	125	DA8	PIR
O ₃	1000.0– 1004.5	H ₂ O, CO ₂ , O ₃ 676, O ₃ 667, O ₃ 686, O ₃ 668, C ₂ H ₄	3.9	3.7	6.8	~7.5	~7.5	~4.5
HCl	2775.72– 2775.8 2821.4 – 2821.62 2925.75– 2926.05	O ₃ , CH ₄ , N ₂ O HDO, N ₂ O CH ₄ , NO ₂ , OCS, O ₃	3.4	3.1	11.8	~3	~3	~1
ClONO ₂	779.85– 780.45 782.55– 782.87 938.3– 939.3	O ₃ (P), CO ₂ (P), HNO ₃ O ₃ (P), CO ₂ (P), H ₂ O, HNO ₃ CO ₂ (P)	3.9	2.7	N/A	~1	~1	N/A
HNO ₃	867.5– 870.0	H ₂ O, OCS, NH ₃	8.1	10.1	10.3	~3.5	~3.5	~1
HF	4038.78– 4039.1	H ₂ O, CH ₄ , HDO	5.8	4.4	13.0	~2.5	~2.5	~1

[Title Page](#)
[Abstract](#)
[Introduction](#)
[Conclusions](#)
[References](#)
[Tables](#)
[Figures](#)
[◀](#)
[▶](#)
[◀](#)
[▶](#)
[Back](#)
[Close](#)
[Full Screen / Esc](#)
[Printer-friendly Version](#)
[Interactive Discussion](#)


Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Table 2. Comparisons between the three ground-based spectrometers, conducted using both unsmoothed, and smoothed 125HR and DA8 total columns from 2007 and 2008, as described in the text. Note that no smoothing is necessary for the 125HR-DA8 comparisons, as they have the same resolution. $\text{Difference} = (\text{inst 1} - \text{inst 2}) / 0.5(\text{inst 1} + \text{inst 2})$, and $\text{Mean} = \text{mean of these differences, calculated as a percentage}$. One standard deviation from the mean is also shown (Std Dev). The instrument names have been abbreviated: 125=125HR, and PIR=PARIS-IR. R^2 and Slope are derived from correlation plots, examples of which are shown in Fig. 3. n indicates the number of matched pairs included in the statistics.

Gas	Instrument	Unsmoothed				Smoothed				n
		Mean (%)	Std Dev (%)	R^2	Slope	Mean (%)	Std Dev (%)	R^2	Slope	
O ₃	125-PIR	1.15	3.75	0.98	1.18	6.46	3.76	0.98	1.12	266
	DA8-PIR	2.14	4.72	0.96	1.10	5.44	5.35	0.94	1.01	142
	125-DA8	1.50	2.16	0.99	0.95					92
HCl	125-PIR	-5.08	3.33	0.98	1.02	1.40	3.62	0.98	0.90	293
	DA8-PIR	-1.62	5.21	0.96	0.87	2.16	5.34	0.97	0.80	441
	125-DA8	3.50	4.74	0.97	0.83					174
ClONO ₂	125-DA8	-1.35	23.84	0.97	0.92					89
HNO ₃	125-PIR	15.08	7.27	0.89	0.55	5.86	5.01	0.91	0.76	232
	DA8-PIR	17.78	8.59	0.87	0.53	4.66	6.42	0.87	0.75	157
	125-DA8	2.52	4.14	0.97	0.88					102
HF	125-PIR	-4.48	7.96	0.93	0.93	-2.85	7.80	0.95	1.31	230
	DA8-PIR	-1.86	7.73	0.91	0.97	-1.34	8.48	0.89	1.09	285
	125-DA8	3.00	5.32	0.97	1.07					112

[Title Page](#)
[Abstract](#)
[Introduction](#)
[Conclusions](#)
[References](#)
[Tables](#)
[Figures](#)
[Back](#)
[Close](#)
[Full Screen / Esc](#)
[Printer-friendly Version](#)
[Interactive Discussion](#)

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Table 3. Mean percentage differences between ACE-FTS and 125HR partial columns (calculated as described in the text), one standard deviation from the mean (also as a percentage) and the number of pairs of measurements (n) used in these calculations, for both 2007 and 2008. Note that the partial column altitude ranges varied for each individual comparison, but were typically around 6–43 km (O_3), 8–38 km (HCl), 15–26 km (ClONO₂), 8–29 km (HNO₃) and 10–43 km (HF).

	2007			2008		
	Mean (%)	Standard deviation (%)	n	Mean (%)	Standard deviation (%)	n
O_3	−7.45	10.60	46	−4.26	6.30	60
HCl	0.28	9.76	56	−1.93	7.67	67
ClONO ₂	−4.94	15.98	44	−17.60	16.92	58
HNO ₃	−1.55	8.66	43	−4.90	7.85	56
HF	10.57	15.11	58	3.41	14.37	41

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

Table 4. As for Table 3, but for pairs remaining after applying rigorous co-location criteria.

	2007			2008		
	Mean (%)	Standard deviation (%)	<i>n</i>	Mean (%)	Standard deviation (%)	<i>n</i>
O ₃	1.11	6.57	10	−1.51	4.30	14
HCl	4.86	8.05	16	−0.23	5.38	23
ClONO ₂	−2.86	14.24	16	−15.33	22.62	37
HNO ₃	1.09	8.36	17	−4.77	6.97	32
HF	5.23	8.88	14	1.14	16.81	15

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

**Ground-based FTS
comparison and ACE
validation at Eureka
during IPY**

R. L. Batchelor et al.

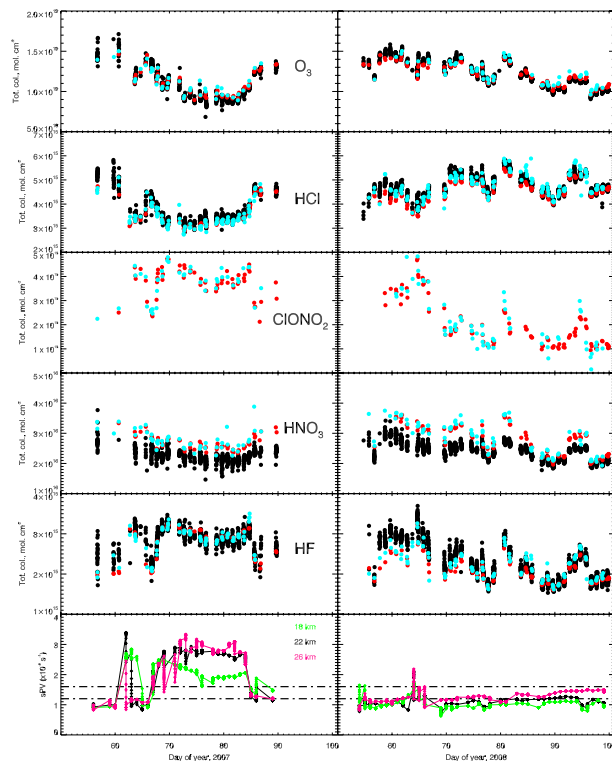


Fig. 1. Time series showing total column densities of (from top to bottom): O₃, HCl, ClONO₂, HNO₃ and HF for the 2007 (left panels) and 2008 (right panels) campaigns. 125HR measurements are shown in red, DA8 in cyan and PARIS-IR in black. The scaled potential vorticity (SPV) at 18, 22 and 26 km is shown in the bottom panel for each year, with approximate locations of the vortex inner and outer edges marked by the dot-dashed lines. Error bars are omitted for clarity. See Table 1 for total uncertainties.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

**Ground-based FTS
comparison and ACE
validation at Eureka
during IPY**

R. L. Batchelor et al.

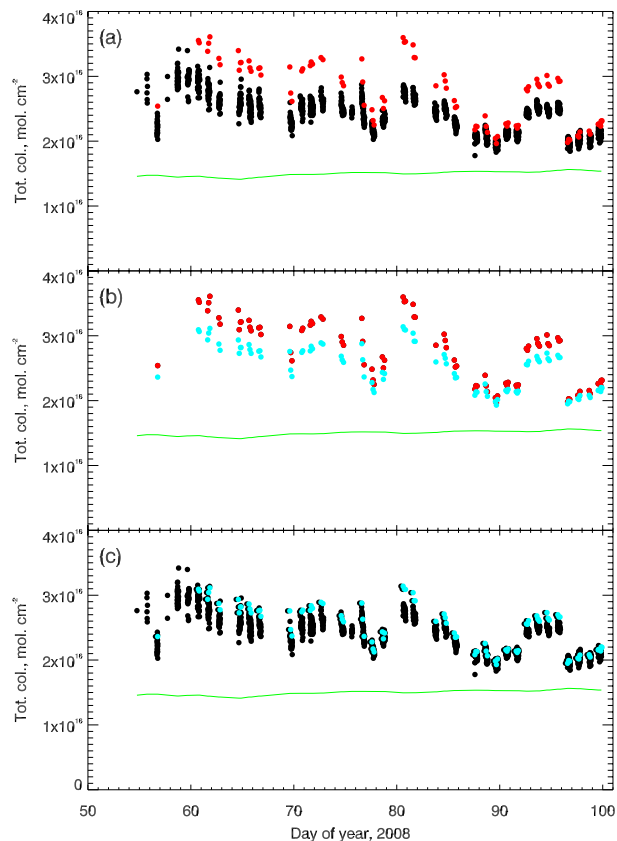


Fig. 2. Illustration of the smoothing process defined by Eq. (1). **(a)** shows the total HNO_3 column measured by the 125HR in red, and by PARIS-IR in black. The a priori column is shown by the green line. **(b)** shows the same 125HR measurements in red, and the resulting 125HR measurements after smoothing via Eq. (1) in cyan. **(c)** shows the new comparison between the smoothed 125HR (cyan) and PARIS-IR (black).

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

**Ground-based FTS
comparison and ACE
validation at Eureka
during IPY**

R. L. Batchelor et al.

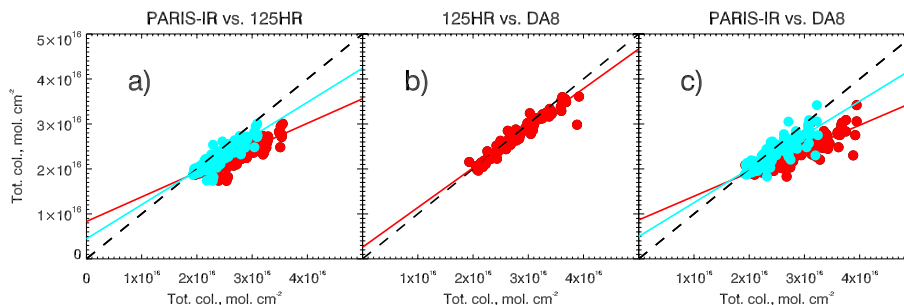


Fig. 3. Total column HNO₃ plots demonstrating the correlation between each combination of the three instruments, before (red) and after (cyan) smoothing of the high-resolution measurements by the PARIS-IR averaging kernel. The 1-to-1 line is shown in black. **(a)** PARIS-IR (*y*-axis) vs. 125HR (*x*-axis); **(b)** 125HR (*y*-axis) vs. DA8 (*x*-axis); **(c)** PARIS-IR (*y*-axis) vs. DA8 (*x*-axis). Note that no smoothing is necessary for the 125HR-DA8 comparison, as they are already at the same resolution. Slopes and correlation coefficients are given in Table 2.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

**Ground-based FTS
comparison and ACE
validation at Eureka
during IPY**

R. L. Batchelor et al.

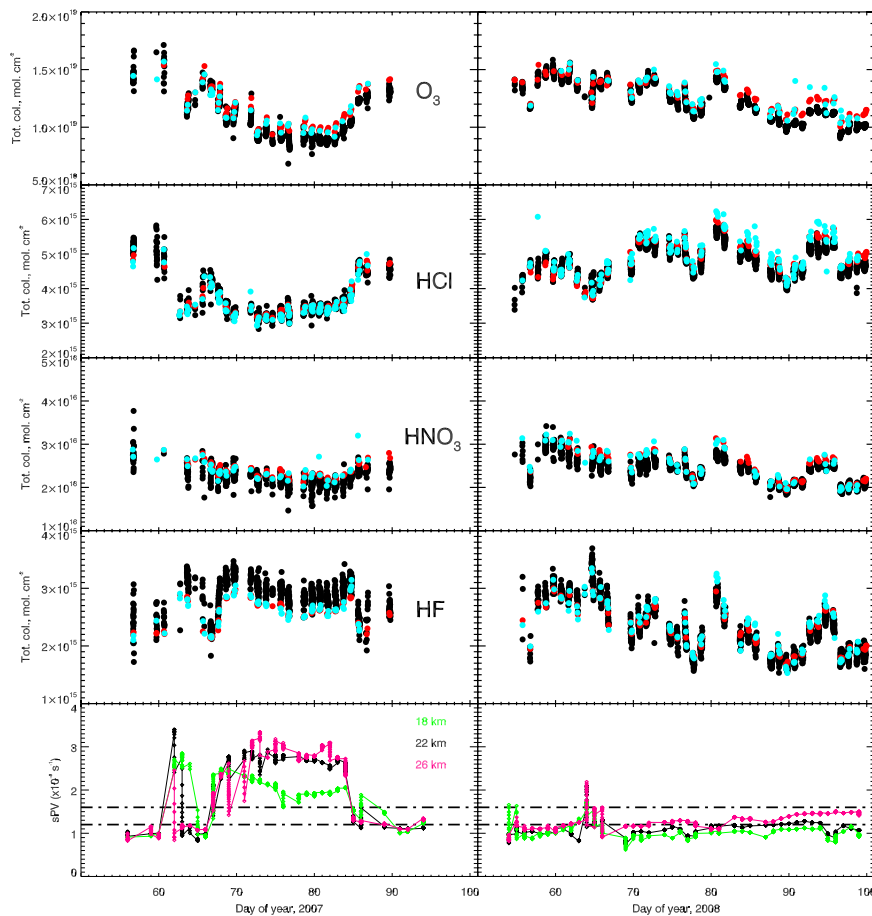


Fig. 4. Same as Fig. 1, with 125HR and DA8 smoothed to match the PARIS-IR resolution. Comparison statistics are given in Table 2.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

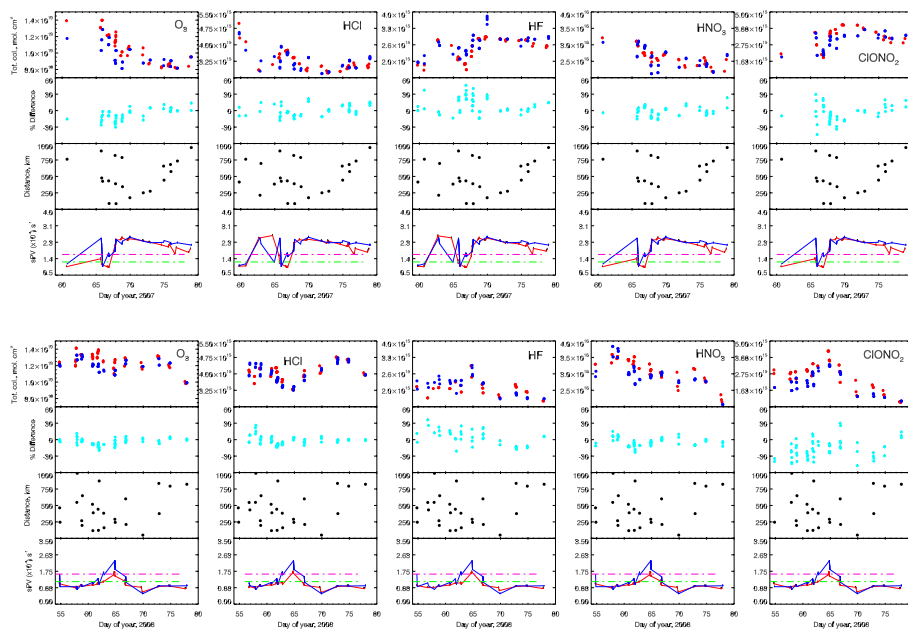


Fig. 5. Time series from 2007 (top plots) and 2008 (bottom plots) for (from left to right) O₃, HCl, HF, HNO₃ and ClONO₂. For each sub-plot, from top to bottom: Partial columns determined for ACE-FTS (blue) and 125HR (red); the percentage difference between the ACE-FTS and 125HR partial columns ($(ACE-FTS - 125HR)/125HR$); the distance between the two measurements as measured from the ACE 30-km tangent point to PEARL; and the sPV for both ACE-FTS (red) and 125HR (blue) at 18 km. The vortex edge region is marked by green dashed (outer) and magenta dashed (inner) lines.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

**Ground-based FTS
comparison and ACE
validation at Eureka
during IPY**

R. L. Batchelor et al.

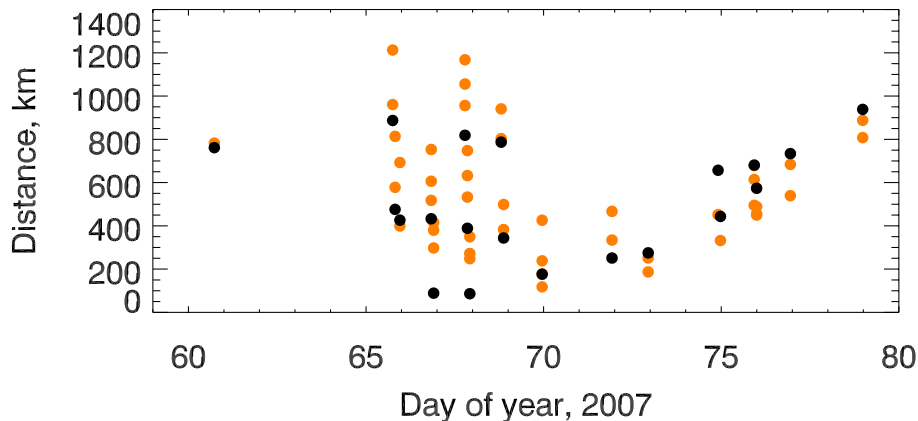


Fig. 6. Distance between comparable ACE-FTS and 125HR measurements, as measured from the ACE 30-km tangent point to PEARL (black) and from the measurement location at 18 km for both instruments (orange).

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

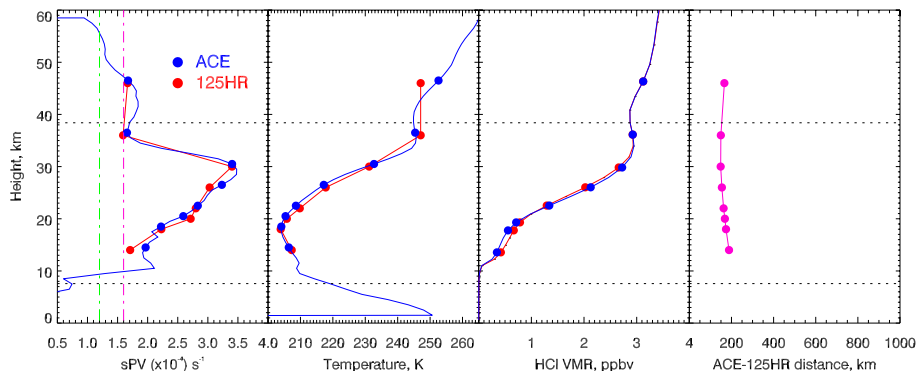


Fig. 7. Sample plots for determining the comparability of ACE-FTS and 125HR measurements. Plots show **(a)** the sPV (with inner and outer edge of the vortex marked with magenta and green dashed lines, respectively), **(b)** temperature, **(c)** HCl VMR profile (where the ACE-FTS profile has been smoothed to match the 125HR), and **(d)** distance between ACE-FTS and 125HR measurements, with data being determined from DMPs along the lines-of-sight of each instrument. Dotted lines indicate the altitude range for the partial column used in this comparison. ACE-FTS information is shown in blue, and 125HR is shown in red. This example shows a well-matched comparison between HCl measurements made on 13 March 2007. The difference in the 9.82–38.40 km partial columns is 1.4%.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

Ground-based FTS comparison and ACE validation at Eureka during IPY

R. L. Batchelor et al.

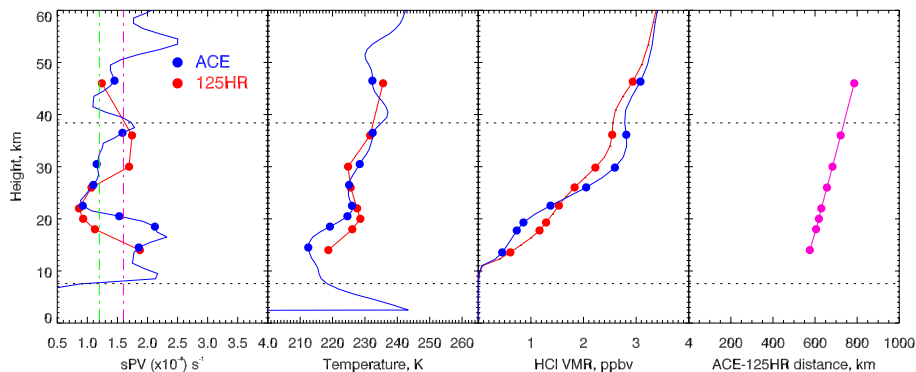


Fig. 8. As for Fig. 6, but demonstrating a less-well-matched comparison pair recorded on 6 March 2007. Note the differences in sPV at 30 and 18 km, with the two instruments each sampling a combination of air masses located inside and outside the polar vortex. The difference between the two measurements over the 11.02–38.40 km partial column is 10.0%.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion