

This discussion paper is/has been under review for the journal Atmospheric Measurement Techniques (AMT). Please refer to the corresponding final paper in AMT if available.

# Influence of the calibration on experimental UV index at a midlatitude site, Granada (Spain)

M. Antón<sup>1,2</sup>, J. E. Gil<sup>1,2</sup>, A. Cazorla<sup>1,2</sup>, J. M. Vilaplana<sup>3</sup>, F. J. Olmo<sup>1,2</sup>, and L. Alados-Arboledas<sup>1,2</sup>

<sup>1</sup>Centro Andaluz de Medioambiente (CEAMA), Universidad de Granada, Granada, Spain

<sup>2</sup>Departamento de Física Aplicada, Universidad de Granada, Granada, Spain

<sup>3</sup>Estación de Sondeos Atmosférico El Arenosillo, INTA, Huelva, Spain

Received: 28 July 2010 – Accepted: 12 August 2010 – Published: 10 December 2010

Correspondence to: M. Antón (mananton@unex.es)

Published by Copernicus Publications on behalf of the European Geosciences Union.

**AMTD**

3, 5645–5670, 2010

## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

## Abstract

The ultraviolet (UV) index is the variable most commonly used to inform the general public about the levels and potential harmful effects of UV radiation incident at Earth's surface. This variable is derived from the output signal of the UV radiometers applying conversion factors obtained by calibration methods. This paper focused on the influence of the use of two of these methods (called one-step and two-steps methods) on the resulting experimental UV Index (UVI) as measured by a YES UVB-1 radiometer located in a midlatitude station, Granada (Spain) for the period 2006–2009. In addition, it is also analyzed the difference with the UVI values obtained when the calibration factors provided by the manufacturer are used. For this goal, the detailed characterization of the UVB-1 radiometer obtained in the first Spanish calibration campaign of broadband UV radiometers at the “El Arenosillo” INTA station in 2007 is used. In addition, modeled UVI data derived from the LibRadtran/UVSPEC radiative transfer code are compared with the experimental values recorded at Granada for cloud-free conditions.

The absolute mean differences between the measured and modeled UVI data at Granada are around 5% using the one-step and two-steps calibration methods. This result indicates the excellent performance of these two techniques for obtaining UVI data from the UVB-1 radiometer. In contrast, the application of the calibration factor supplied by the manufacturer produces a high overestimation (~14%) of the UVI values. This fact generates unreliable alarming high UVI data in summer when the manufacturer's factor is used. Thus, days with an extreme erythemal risk (UVI higher than 10) increase up to 46% of all cases measured between May and September at Granada when the manufacturer's factor is applied. This percentage is reduced to a more reliable value of 3% when the conversion factors obtained with the two-steps calibration method are used. All these results report about the need of a sound calibration of the broadband UV instruments in order to obtain reliable measurements.

## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



## 1 Introduction

The well-known depletion of the stratospheric ozone layer in the past decades caused concern about increasing ultraviolet (UV) radiation at surface (United Nations Environment Programme, UNEP, 2006). This radiation is beneficial for several biological reactions in appropriate doses (e.g., Webb and Holick, 1988), but the overexposure can be very detrimental for humans, plants, animals and materials (Diffey, 1991, 2004).

The UV index (UVI) is a dimensionless magnitude commonly used to inform people about the UV radiation levels with the objective of recommending people to take precautionary measures against their harmful effects on human health (e.g., Vanicek et al., 2000). The erythema or sunburn of human skin is the adverse effect most usually associated with UV radiation overexposure, receiving a high attention in society. This effect is generally quantified by weighing the solar UV radiation (280–400 nm) with the erythema spectral response (McKinlay and Diffey, 1987), resulting in the so-called ultraviolet erythema radiation (UVER). UVI is defined as 40 times UVER (expressed in watts per square meter) according to the joint recommendation of the World Meteorological Organization (WMO), the World Health Organization (WHO), the United Nations Environmental Programme (UNEP), and the International Commission on Non-Ionizing Radiation Protection (ICNIRP) (WMO, 1998; WHO, 2002).

It is well documented that UVI at the Iberian Peninsula reaches very high values (e.g., Martínez-Lozano et al., 2002; Marín et al., 2005; Antón et al., 2009a) due to the high solar elevations that can be reached at these latitudes throughout the year. This fact together with the changes in the population's behavior associated with sun overexposure makes indispensable to obtain high-quality UVI measurements in this region in order to inform people and to reduce the risk of health damage. In this sense, according to the study by Lopez-Abente et al. (2002), during the period 1952–1996, the melanoma (the most dangerous type of skin cancer) annually increased about 8% in Spain.

### Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



The broadband UV radiometer is the instrument most widely used to measure UVER data due to their low cost and easy maintenance (WMO, 1996). Nevertheless, the relationship between the output signal (voltage) and the final product (UVER or UVI) given by these instruments is highly complex. Thus, these UV radiometers require an elaborate calibration procedure (Lantz et al., 1999; Leszczynski et al., 1998; Hülsen and Gröbner, 2007). In this sense, the intercomparison of broadband UV radiometers with respect to a reference spectroradiometer (traceable to international standards) is a practical way for improving the accuracy and comparability of the measurements performed by different instruments (Leszczynski et al., 1995; Bais et al., 2000; Gröbner et al., 2007; Vilaplana et al., 2009).

In this context, it is highly interesting to study different calibration methods for measuring daily UV index in order to improve the accuracy of these values. The WMO adopted two methodologies for the calibration of the broadband UV radiometers: one-step and two-steps methods (Bais et al., 1999). In the one-step method, the calibration factor is directly derived from the comparison between the raw signal of the broadband UV radiometer and the erythemally integrated irradiance measured by one reference spectroradiometer. The two-steps method involves two stages. Initially, the output signal of the broadband UV radiometer is compared with the effective irradiance from the reference spectroradiometer. Finally, these effective response units are converted to erythemal units.

In spite of its great interest, only a few studies jointly analyze both methods (e.g., Vilaplana et al., 2006). In this sense, our paper analyzes the application of the calibration factor provided by the manufacturer and the factors derived from the one-step and two-steps methods in order to obtain experimental daily UV index at Granada (Southeastern Spain). For this goal, these experimental UVI values are compared with respect to UVI data derived from a multilayer transfer model for cloud-free conditions. In addition, the evolution of the measured UVI data for all sky conditions is analyzed for the period of study which ranges four whole years (2006–2009).

The instrumentation and the data used in this paper are described in Sect. 2. Section 3 describes the calibration methods used in this work to obtain experimental UVI values. Section 4 presents and discusses the application of the different methods for obtaining UV Index and, finally, Sect. 5 summarizes the main conclusions.

## 2 Data

### 2.1 Ground-based measurements

The Atmospheric Physics Group (GFAT) of the University of Granada operates the radiometric station located on the rooftop of the Andalusian Center for Environmental Studies building (CEAMA, 37.17° N, 3.61° W, 680 m a.s.l.).

The broadband UV radiometer installed at this station is a model UVB-1 manufactured by Yankee Environment System (YES). This radiometer has a spectral range between 280 and 400 nm, and a spectral sensitivity very close to the standard erythral spectrum (McKinlay and Diffey, 1987). The output voltages are sampled every ten seconds and recorded as 1-min average on a Campbell CR10X data acquisition system. This UVB-1 instrument took part in the first Spanish calibration campaign of ultraviolet broad-band radiometers at the “El Arenosillo” INTA station in Huelva (Spain), from 20 August to 15 September 2007. This campaign included the spectral and angular characterization of the instruments, and the outdoor intercomparison with respect to a well-calibrated Brewer spectroradiometer (Vilaplana et al., 2009). The voltages provided by UVB-1 instrument are converted to UVER values applying the calibration factors provided by the manufacturer and the coefficients derived from two calibration methods using the data recorded in the El Arenosillo’s campaign 2007 as it is widely explained in the Sect. 2.3.

The cloud cover has been characterized in the oktas (i.e., eighths of sky). This variable is derived from the All-Sky Imager which was developed by the GFAT team. This instrument provides images of the whole sky dome in daytime, and it is used for

## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



## Influence of the calibration on experimental UV index

M. Antón et al.

[Title Page](#)

[Abstract](#)

[Introduction](#)

[Conclusions](#)

[References](#)

[Tables](#)

[Figures](#)

[⏪](#)

[⏩](#)

[◀](#)

[▶](#)

[Back](#)

[Close](#)

[Full Screen / Esc](#)

[Printer-friendly Version](#)

[Interactive Discussion](#)



research associated with radiative transfer in the atmosphere (Cazorla et al., 2008, 2009). This All-Sky Imager is a custom adaptation of a scientific CCD camera, and it basically consists of a digital color video camera mounted with a fish-eye lens (180° FOV) pointing to the zenith. In addition, the camera is protected against the environmental factors, and a solar-shadow system is used to avoid direct incidence of the Sun beam on the lens.

The aerosol information was retrieved from a CIMEL CE-318 sun-photometer which is the standard instrument used in the AERONET network (Holben et al., 1998). The direct sun measurements at 340, 380, 440, 500, 670, 870, and 1020 nm were used to retrieve the aerosol optical depth (AOD), and the Angstrom's coefficients following the methodology proposed by Alados-Arboledas et al. (2003a). Periodically Langley plots at high location in Sierra Nevada Range (2200 m a.s.l.) have been performed to determine the calibration constants for this sun-photometer (Alcántara-Ruiz, 2004).

## 2.2 UV index estimations

The estimated values of UV index were derived from the LibRadtran software package whose main tool is the UVSPEC model, developed by Mayer and Kylling (2005).

The UVSPEC code consists of a multiple scattering radiative transfer model which computes plane-parallel radiative transfer in the Earth's atmosphere under cloudless or cloudy conditions. The pSseudospherical DIScreeT Ordinate Radiative Transfer (SDIS-ORT) method numerically solves the radiative-transfer equation in a vertically non-homogeneous plane-parallel atmosphere, running in 16 stream mode.

We implemented the UVSPEC model for a standard midlatitude atmosphere under cloud-free conditions. Aerosols were assumed to be an urban type, and the impact of the aerosol loading in the boundary is expressed by means of the Angstrom's coefficients ( $\beta$  and  $\alpha$ ) retrieved by the Cimel sun-photometer (see Sect. 2.1). In addition, we set to constant values of 0.9 and 0.7 for the single scattering albedo and the asymmetry factor. These values are set based on averages of the Cimel sun-photometer measurements at 440 nm obtained during August 2003 at Granada (Lyamani et al., 2006). The

model uses the daily total ozone column (TOC) provided by the Ozone Monitoring Instrument (OMI) (Levelt et al., 2006). The OMI data used in this work were retrieved from the OMI-TOMS algorithm which is based on the long-standing NASA TOMS V8 retrieval algorithm (Bhartia and Wellemeyer, 2002). In general, there is an excellent agreement between the OMI-TOMS and ground-based measurements. The work by Antón et al. (2009b) reported that the OMI-TOMS data are on average a mere 2.0% lower than Brewer TOC measurements in five Spanish ground-based stations. Finally, the daily UV Index corresponding to local solar noon (minimum solar zenith angle, SZA) was estimated using all available information.

### 3 Calibration procedures

#### 3.1 Manufacturer

The calibration factors supplied by Yankee E. S. for the UVB-1 radiometer are a function of the SZA. Thus, it is possible to obtain a polynomial function by means of a linear regression analysis from the ten values of the calibration factors provided by the manufacturer for SZA between 22° and 65°. In this sense, we propose the following polynomial third-order dependence between CF values and the SZA:

$$CF(SZA) = 0.136 + 0.019 \times SZA - 4.9 \times 10^{-5} \times SZA^2 + 5.1 \times 10^{-7} \times SZA^3 \quad (1)$$

where CF is the calibration factor in  $Wm^{-2}/V$  and SZA is the solar zenith angle in degrees.

Figure 1 shows the dependence of the ten calibration factors (in black) provided by the manufacturer on the SZA values below 65°. The red line corresponds to the polynomial function given by the above expression. From this function, the sensor output in volts can be multiplied by CF in order to obtain the “manufacturer” UVER values. In this figure, the dashed line represents the fixed value of  $0.141 Wm^{-2}/V$  proposed by the manufacturer when the dependence on SZA is not utilized.

## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



It is worth noting that the calibration factors supplied by the manufacturer are the same for all instruments of the model YES UVB-1.

### 3.2 One-step method

To our knowledge, only two versions of the one-step method can be found in the literature. One of them is based on the ratio between broadband radiometer's measurements and integrated spectrophotometer's values (Leszczynski et al., 1998; Bais et al., 1999). The another one consists of a first-order linear dependence between the measurements given by the two instruments (Bodhaine et al., 1998; Grainger et al., 1993; Nunez et al., 1997). The work of Cancillo et al. (2005) compared the performance of these two procedures and proposed a second-order dependence in order to improve the calibration performance for high solar elevations.

Figure 2 (left) shows the ratio between the erythemally integrated irradiance given by the Brewer spectroradiometer and the UVB-1 radiometer output voltage as a function of the SZA during the Arenosillo's campaign 2007. The horizontal line represents the mean ratio ( $0.1275 \pm 0.0006 \text{ Wm}^{-2}/\text{V}$ ), which is taken by the ratio method as the calibration factor. For calculating this mean ratio, we have selected radiative and voltage values for SZA less than  $65^\circ$  and cloud-free conditions in order to minimize systematic errors attributed to deviations of the angular response of the UVB-1 radiometer.

The relationship between the Brewer erythemally integrated irradiance and the UVB-1 output voltage for SZA smaller than  $65^\circ$  is shown in the Fig. 2 (right) together with the regression line corresponding to the first-order model. The slope of this line ( $0.1260 \pm 0.0005 \text{ Wm}^{-2}/\text{V}$ ) is the calibration factor derived from the linear regression analysis.

The calibration factors calculated by this method are about 10% lower than the fixed value provided by the manufacturer. This result shows evidence that each instrument needs an individual calibration and that a unique general calibration factor should not be applied.

## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion





### 3.3 Two-steps method

This method requires the laboratory characterization of the spectral and angular responses of the broadband UV radiometers. The whole description of the two-steps method is beyond the scope of this paper, but it can be found in the works of Webb et al. (2006), Hülsen and Gröbner (2007) and Vilaplana et al. (2009). These reference works propose the following expression to convert the raw signal of broadband UV radiometer into erythemal units ( $\text{Wm}^{-2}$ ) is:

$$E_{\text{CIE}} = (U - U_{\text{offset}}) C f_n(\text{SZA}, \text{TOC}) \text{Coscor}(\text{SZA}) \quad (2)$$

where:

- $E_{\text{CIE}}$  is erythemal UV irradiance in  $\text{Wm}^{-2}$ .
- $U$  is the measured electrical signal by the broadband radiometer in  $V$ .
- $U_{\text{offset}}$  is the electrical offset for dark conditions in  $V$ .
- $C$  is the absolute calibration coefficient in  $\text{Wm}^{-2}/V$ .
- $f_n(\text{SZA}, \text{TOC})$  is the conversion function (unitless).
- $\text{Coscor}(\text{SZA})$  is the cosine correction function in dependence of the SZA (unitless).

Here, we present the results obtained for our YES UVB-1 radiometer from El Arenosillo campaign 2007. The absolute calibration coefficient is obtained as the averaged ratio between the output voltage of the UVB-1 radiometer and the effective UV irradiance calculated by the integration of the Brewer spectral irradiance weighted by the actual spectral response of the broadband radiometer which is characterized indoor, in the laboratory. Only values for SZA lower than  $65^\circ$  were considered for the

## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



calculation of this absolute calibration coefficient. The value obtained for our UVB-1 radiometer was  $0.1150 \pm 0.006 \text{ Wm}^{-2}/\text{V}$ .

The conversion function transforms the effective irradiance to erythemally weighted irradiance. Thus, this function informs about the deviation between the actual spectral response of the UVB-1 radiometer and the standard erythemal action spectrum. It can be expressed as a look up table derived from a radiative transfer model (Vilaplana et al., 2009). This table depends on the parameters with major spectral influence in the UV range: the solar zenith angle and the total ozone column. Figure 3 (left) shows the variation of the normalized conversion function with respect to SZA, for a constant TOC value of 300 DU. When SZA changes from  $0^\circ$  to  $80^\circ$ , the relative differences in the conversion function are less than 20%. In addition, Fig. 3 (right) shows the variation of the normalized conversion function with respect to TOC for a constant SZA value of  $40^\circ$ . The relative difference between the value of the conversion function for 200 DU and the value for 500 DU is around 14%.

Finally, the cosine correction function informs about the cosine error; the deviation that the broadband UV instrument experiences with respect to the ideal angular response. This function is also derived from indoor measurements in the laboratory. Figure 4 shows the variation of the cosine correction function of the UVB-1 radiometer with respect to the SZA. It is shown that the angular correction of this instrument is around 5% for SZA values smaller than  $20^\circ$ , and it is between 10% and 15% for SZA valued higher than  $50^\circ$ .

## 4 Experimental UV index

The daily UV index obtained applying the manufacturer coefficients and the one-step and two-steps calibration methods are compared. To analyze the differences between the experimental UVI obtained under different calibration methods, we use, as reference, the UVI derived from the LibRadtran/UVSPEC radiative transfer code (see Sect. 2.2). In general, the daily UVI estimations provided by models are calculated for

### Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



solar noon, thus in order to make a comparison with experimental UVI values, these have to be also obtained at solar noon. In addition, since cloud-free sky conditions are especially interesting cases for the comparison with radiative transfer model results, the relative differences between the different calibration methods were obtained for those particular conditions. The selection of the cloud-free conditions was performed by means of the All-Sky Imager (see Sect. 2.1). Thus, days with zero oktas at solar noon were classified as cloud-free cases. The percentage of days selected with this restrictive threshold at Granada for period 2006–2007 was 45%, which indicates the high number of cloud-free situations in South Spain.

In order to compare the UVSPEC estimations with experimental results, three linear regressions were performed between UVI estimations and the experimental values obtained applying the manufacture's factor and the two calibration procedures. The slopes and the statistical parameters obtained in the three regression analyses are shown in Table 1. Correlation between the measured and modeled UVI data sets are significantly high for the three datasets ( $R^2 \sim 0.98$ ), with a significantly small spread (RMSE  $\sim 8\%$ ). It can be seen that the slopes are very close to 1 for the experimental values derived from the one-step and two-steps methods. Table 1 presents also the MBE (mean bias error) and the MABE (mean absolute bias error) parameters obtained for the three data sets. These statistics are obtained by the following expressions:

$$\text{MBE} = 100 \times \frac{1}{N} \sum_{i=1}^N \frac{\text{UVI}_{\text{measured}} - \text{UVI}_{\text{modelled}}}{\text{UVI}_{\text{modelled}}} \quad (3)$$

$$\text{MABE} = 100 \times \frac{1}{N} \sum_{i=1}^N \frac{|\text{UVI}_{\text{measured}} - \text{UVI}_{\text{modelled}}|}{\text{UVI}_{\text{modelled}}} \quad (4)$$

The small positive value ( $\sim 1\%$ ) of the MBE for the one-step and two-steps methods indicates that the experimental UVI data obtained by these calibration techniques present a slight overestimation of the UVI estimations. In addition, the MABE parameters for

## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



these two calibration techniques present values around 5% which indicates a good agreement between measured and modeled UVI data at Granada. This result agrees with other inter-comparison works using the LibRadtran/UVSPEC code and experimental data (e.g., Mayer et al., 1997; Kylling et al., 1998; de Backer et al., 2001). The uncertainty of MBE and MABE parameters given by their standard error is always lower than 0.7%, indicating the high statistical significance of the reported values. The scatter plot presented in Fig. 5 (the solid line is the zero bias line, unit slope) confirms this high degree of proportionality. All these results show the excellent effectiveness of the two calibration methods applied to obtain UVI information from YES UVB-1 records.

On the other hand, Fig. 5 shows that the UVI data obtained applying the calibration factors provided by the manufacturer clearly overestimate the UVI derived from the UVSPEC model (the slope of the regression line is 0.85). This behavior is corroborated by the high positive value ( $\sim 14\%$ ) of the MBE parameter. Moreover, the MABE parameter presents a similar absolute value which reveals the presence of a notable bias with a small statistical spread. Figure 5 also shows that this bias is lower for small UVI values than for high UVI values. Thus, when the relative differences between measured and modeled UVI are plotted as function of SZA (not shown), it can be seen a clear dependence between these two variables. We obtain a MBE value of 9% for SZA greater than  $50^\circ$  (small UVI values), and a value of 16% for SZA smaller than  $30^\circ$  (high UVI values). All these results show the unreliability of the calibration factors provide by the manufacturer, revealing the great importance of the individual calibration of the broadband UV radiometers. Therefore, the general calibration factors supplied by the manufacturer should not be applied for broadband UV radiometers corresponding to the same model and manufacturer.

The relative differences between the experimental UVI values derived from the one-step and two steps calibration methods are small (lower than 4%) for the YES UVB-1 broadband radiometer installed at Granada. This result is related to the high solar elevations recorded at solar noon in South Spain (SZA lower than  $65^\circ$ ). Thus, it is expected that the differences between UVI values obtained by the one-step and two

## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



steps methods could increase for instruments located at higher latitudes. When all information is available, the use of the two-steps method is recommended by several organizations responsible for calibration protocols of broadband UV radiometers because of its higher accuracy (Bais et al., 1999; Webb et al., 2003).

Figure 6 shows the evolution of the daily UVI at Granada during four years (2006–2009) using the two-steps calibration method and the manufacturer’ calibration factors. These daily values have been obtained applying the standard definition proposed by the WHO (2002). According to this proposal, the daily UV Index corresponds to the daily maximum 30 min averaged UVER measured at the earth’s surface. It can be seen that the annual solar cycle (driven by astronomical factors) and the total ozone annual cycle explain the sinusoidal evolution of the UVI values. In addition, the figure shows significant day-to-day variability which is mainly associated with changes in the cloud cover (Alados-Arboledas et al., 2003b). These short-term UVI changes are also affected by the day-to-day fluctuations of the aerosol load (di Sarra et al., 2002) and the total ozone column (Antón et al., 2008).

Category labels associated with numerical interval of the UVI are a practice tool to inform people about the erythemal risk (sunburn of the human skin). In this sense, COST-713 Action “Long term changes and climatology of UV radiation over Europe” established a universal category with intervals ranging from low erythemal risk (0–3), moderate (4–6), high (7–9) and extreme (>10) (Vanicek et al., 2000). Days classified as cases with high and extreme erythemal risk correspond to 22.1% and 1.2% of all cases, respectively, when the two-steps method is applied to the calibration of the UVB-1 radiometer installed at Granada. This result agrees with Marín et al. (2005) who found high erythemal risk between 18% and 25% of all days at nine ground-based stations located in East Spain. These cases are mainly recorded between the late spring and the beginning of autumn (many cloud-free days). Thus, if the analysis is limited between May and September, then the 46.7% and 2.8% of all cases in these months correspond to high and extreme erythemal risk at Granada.

## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



The UVI values obtained applying the manufacturer's factors clearly overestimate the real UVI data at Granada (Fig. 6). Thus, using this calibration, days classified as extreme erythemal risk correspond to 46% of all cases measured between May and September. Therefore, the use of unsuitable calibration factors could generate alarming high UVI values. These results enhance the interest of an appropriate characterization of the broadband UV radiometer in order to report reliable UVI values.

## 5 Conclusions

Some important conclusions may be drawn from this work. First of all, this study has verified that although the manufacturer provides the same calibration factors for all YES UVB-1 radiometers, each instrument needs an individual characterization in order to obtain its real calibration factors. In this sense, the actual conversion factor corresponding to the UVB-1 instrument localized at Granada is around 10% smaller than the calibration factor supplied by the manufacturer. This result indicates that a unique general calibration factor should not be applied to the YES UVB-1 radiometers.

Two calibration techniques (one-step and two-steps) have been used in this work for determining the calibration factors of our broadband UV radiometer. From these conversion factors, the experimental daily UVI values at Granada have been reported for the period 2006–2009. The comparison between these experimental values and the estimations derived from a radiative transfer model confirm that the UVI values derived from the manufacturer's calibration is inadequate, generating alarming high UVI values in summer. In contrast, both one-step and two-steps methods provide reliable data with mean values of the relative differences between measured and modeled UVI data around 5%. Finally, although two-steps method is recommended by several organizations because of its higher accuracy, the simpler one-step method provide very similar experimental UVI data at Granada (relative differences lower than 4%) due to the high solar elevations reached in this location throughout the year.

All these results underline the importance of an accurate characterization of broadband UV radiometers in order to obtain highly reliable UV irradiance data.

*Acknowledgements.* Authors thank the organizers (El Arenosillo/INTA team and AIRE/UEX team) of the first Spanish inter-comparison campaign of broadband UV instruments at El Arenosillo station in 2007. Manuel Antón thanks Ministerio de Ciencia e Innovación and Fondo Social Europeo for the award of a postdoctoral grant (Juan de la Cierva). This work was partially supported by the Andalusian Regional Government through project P08-RNM-3568, the Spanish Ministry of Science and Technology through project CGL2007-66477-C02-01.

## References

- Alados-Arboledas, L., Lyamani, H., and Olmo, F. J.: Aerosol size properties at Armilla, Granada (Spain), *Q. J. Roy. Meteorol. Soc.*, 129, 1395–1413, 2003a.
- Alados-Arboledas, L., Alados, I., Foyo-Moreno, I., Olmo, F. J., and Alcántara, A.: The influence of clouds on surface UV erythemal irradiance, *Atmos. Res.*, 66, 273–290, 2003b.
- Alcántara-Ruiz, A., Olmo, F. J., and Alados-Arboledas, L.: Langley calibrations of sunphotometer at Sierra Nevada, Granada, Spain, *Optica pura y Aplicada*, 37, 3263–3269, 2004.
- Antón, M., Serrano, A., Cancillo, M. L., and García, J. A.: Total ozone and solar erythemal irradiance in southwestern Spain: Day-to-day variability and extreme episodes, *Geophys. Res. Lett.*, 35, L20804, doi:10.1029/2008GL035290, 2008.
- Antón, M., Serrano, A., Cancillo, M. L., and García, J. A.: Experimental and forecasted values of the UV index in South-Western Spain, *J. Geophys. Res.*, 114, D05211, doi:10.1029/2008JD011304, 2009a.
- Antón, M., López, M., Vilaplana, J. M., Kroon, M., McPeters, R., Bañón, M., and Serrano, A.: Validation of OMI-TOMS and OMI-DOAS total ozone column using five Brewer spectroradiometers at the Iberian Peninsula, *J. Geophys. Res.*, 114, D14307, doi:10.1029/2009JD012003, 2009b.
- Bais, A., Topaloglou, C., Kazadzis, S., Blumthaler, M., Schreder, J., Schmalwieser, A., Herniques, D., and Janouch, M.: Report of the LAP/COST/WMO intercomparison of erythemal radiometers, Technical Report TD 1051, WMO/GAW, 1999.

## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Bhartia, P. K. and Wellemeyer, C.: TOMS-V8 total O<sub>3</sub> algorithm, in: OMI Algorithm Theoretical Basis Document, vol. II, OMI Ozone Products, edited by: Bhartia, P. K., available at: [http://eosps0.gsfc.nasa.gov/eos\\_homepage/for\\_scientists/atbd/index.php](http://eosps0.gsfc.nasa.gov/eos_homepage/for_scientists/atbd/index.php), NASA Goddard Space Flight Cent., Greenbelt, Md., 15–31, 2002.

5 Bodhaine, B. A., Dutton, E. G., McKenzie, R. L., and Johnston, P. V.: Calibrating broad-band UV instruments: Ozone and solar zenith angle dependence, *J. Atmos. Ocean. Tech.*, 15, 916–926, 1998.

Cancillo, M. L., Serrano, A., Antón, M., García, J. A., Vilaplana, J. M., and de la Morena, B.: An improved outdoor calibration procedure for broadband ultraviolet radiometers, *Photoch. Photobio.*, 81, 860–865, 2005.

10 Cazorla, A., Olmo, F. J., and Alados-Arboledas, L.: Development of a sky imager for cloud cover assessment, *J. Opt. Soc. Am. A*, 25(1), 29–39, 2008.

Cazorla, A., Shields, J. E., Karr, M. E., Olmo, F. J., Burden, A., and Alados-Arboledas, L.: Technical Note: Determination of aerosol optical properties by a calibrated sky imager, *Atmos. Chem. Phys.*, 9, 6417–6427, doi:10.5194/acp-9-6417-2009, 2009.

15 de Backer, H., Koepke, P., Bais, A., de Cabo, X., Frei, T., Gillotay, D., Haite, C., Heikkilä, A., Kazantzidis, A., Koskela, T., Kyrö, E., Lapeta, B., Lorente, J., Masson, K., Mayer, B., Plets, H., Redondas, A., Renaud, A., Schauburger, G., Schmalwieser, A., Schwander, H., and Vanicek, K.: Comparison of measured and modelled uv indices for the assessment of health risks, *Meteorol. Appl.*, 8, 267–277, 2001.

di Sarra, A., Cacciani, M., Chamard, P., Cornwall, C., DeLuisi, J. J., Di Iorio, T., Disterhoft, P., Fiocco, G., Fua, D., and Monteleone, F.: Effects of desert dust and ozone on the ultraviolet irradiance at the Mediterranean island of Lampedusa during PAUR II, *J. Geophys. Res.*, 107(D18), 8135, doi:10.1029/2000JD000139, 2002.

25 Diffey, B.: Solar ultraviolet radiation effects on biological systems, *Phys. Med. Biol.*, 36, 299–328, 1991.

Diffey, B.: Climate change, ozone depletion and the impact on ultraviolet exposure of human skin, *Phys. Med. Biol.*, 49, R1–R11, 2004.

Grainger, R. G., Basher, R. E., and McKenzie, R. L.: UV-B Robertson-Berger meter characterization and field calibration. *Appl. Opt.*, 32, 343–349, 1993.

30 Gröbner, G., Hülsen, G., Vuilleumier, L., Blumthaler, M., Vilaplana, J. M., Walker, D., and Gil, J. E.: Report of the PMOD/WRC-COST Calibration and Intercomparison of Erythematol radiometers Davos, Switzerland, 28 July–23 August 2006,



## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

available at: [http://i115srv.vu-wien.ac.at/uv/COST726/COST726\\_Dateien/Results/PMOD\\_WRC\\_COST726\\_campaign\\_2006\\_R.pdf](http://i115srv.vu-wien.ac.at/uv/COST726/COST726_Dateien/Results/PMOD_WRC_COST726_campaign_2006_R.pdf), last access: 1 June, 2010.

Holben, B. N., Eck, T. F., Slutsker, I., Tanré, D., Buis, J. P., Setzer, A., Vermote, E., Reagan, J. A., Kaufman, Y. J., Nakajima, T., Lavenu, F., Jankowiak, I., and Smirnov, A.: AERONET – A federated instrument network and data archive for aerosol characterization, *Remote Sens. Environ.*, 66(1), 1–16, 1998.

Hülßen, G. and Gröbner, G.: Characterization and calibration of ultraviolet broadband radiometers measuring erythemally weighted irradiance, *Appl. Optics*, 46, 5877–5886, 2007.

Kylling, A., Bais, A. F., Blumthaler, M., Schreder, J., Zerefos, C. S., and Kosmidis, E.: Effect of aerosols on solar UV irradiances during the photochemical activity and solar ultraviolet radiation campaign, *J. Geophys. Res.*, 103, 26051–26060, 1998.

Lantz, K., Disterhoft, P., DeLuisi, J. J., Early, E., Thompson, A., Bigelow, D., and Slusser, J.: Methodology for deriving clear-sky erythemal calibration factors for UV broadband radiometers of the U.S. central UV calibration facility, *J. Atmos. Ocean. Tech.*, 16, 1736–1752, 1999.

Leszczynski, K., Jokela, K., Ylianttila, L., Visuri, R., and Blumthaler, M.: Report of the WMO/STUK Intercomparison of Erythemally-Weighted Solar UV Radiometers, Spring/Summer 1995, World Meteorological Organization (WMO), WMO/GAW Rep. 112, 1995.

Leszczynski, K., Jokela, K., Ylianttila, L., Visuri, R., and Blumthaler, M.: Erythemally weighted radiometers in solar UV monitoring: results from the WMO/STUK intercomparison, *Photoch. Photobio.*, 67(2), 212–221, 1998.

Levelt, P. F., Hilsenrath, E., Leppelmeier, G. W., Van den Oord, G. H. J., Bhartia, P. K., Tamminen, J., De Haan, J. F., and Veefkind, J. P.: The ozone monitoring instrument, *IEEE T. Geosci. Remote*, 44, 1093–1101, 2006.

López-Abente, G., Pollán, M., Aragonés, N., Pérez, B., Llácer, A., Pérez, J., Medrano, M. J., Boix, R., Diez, M., González, P., Navas, A., Almazán, J., Jiménez, M. T., and de Pedro, J.: Tendencias de la mortalidad en España, 1952–1996, Ed. Centro Nacional de Epidemiología, 2002, ISBN 84-688-0730-3, available at: <http://www2.uca.es/hospital/TM/portada.html>, last access: 1 June, 2010.

Lyamani, H., Olmo, F. J., Alcántara, A., and Alados-Arboledas, L.: Atmospheric aerosols during the 2003 heat wave in southeastern Spain II: Microphysical columnar properties and radiative forcing, *Atmos. Environ.*, 40, 6465–6476, 2006.

## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



- Marín, M. J., Sola, Y., Tena, F., Utrillas, M. P., Campmany, E., de Cabo, X., Lorente, J., and Martínez-Lozano, J. A.: The UV index on the Spanish Mediterranean Coast, *Photoch. Photobio.*, 81, 659–665, 2005.
- 5 Martínez-Lozano, J. A., Tena, F., and Marín, M. J.: UV index experimental values during the years 2000 and 2001 from the Spanish Broadband UVB radiometric network, *Photoch. Photobio.*, 76, 181–187, 2002.
- Mayer, B., Seckmeyer, G., and Kylling, A.: Systematic long-term comparison of spectral UV measurements and UVSPEC modelling results, *J. Geophys. Res.*, 102, 8755–8767, 1997.
- 10 Mayer, B. and Kylling, A.: Technical note: The libRadtran software package for radiative transfer calculations – description and examples of use, *Atmos. Chem. Phys.*, 5, 1855–1877, doi:10.5194/acp-5-1855-2005, 2005.
- McKinlay, A. F. and Diffey, B. L.: A reference spectrum for ultraviolet induced erythema in human skin, *CIE J.*, 6, 21–27, 1987.
- 15 Nunez, M., Michael, K., Turner, D., Wall, M., and Nilsson, C.: A satellite-based climatology of UV-B irradiance for antarctic coastal regions, *Int. J. Climatol.*, 17, 1029–1054, 1997.
- United Nations Environment Programme (UNEP): United Nations Environmental Programme: Environmental effects of ozone depletion and its interactions with climate change: 2006 assessment, Tech. Rep., UNEP, Nairobi, Kenya, 2006.
- 20 Vanicek, K., Frei, T., Lytinska, Z., and Schmalwieser, A.: UV-index for the Public, Report of the COST-713 Action, European Commission, Brussels, Belgium, 2000.
- Vilaplana, J. M., Cachorro, V. E., Sorribas, M., Luccini, E., de Frutos, A., Berjón, A., and de la Morena, B.: Modified calibration procedures for a Yankee Environmental System UVB-1 biometer based on spectral measurements with a Brewer spectrophotometer, *Photoch. Photobio.*, 82, 508–514, 2006.
- 25 Vilaplana, J. M., Serrano, A., Antón, M., Cancillo, M. L., Parias, M., Gröbner, J., Hulsen, G., Zablocky, G., Díaz, A., and de la Morena, B. A.: Report of the El Arenosillo/ INTA-COST calibration an intercomparison campaign of UVER broadband radiometers, “El Arenosillo”, available at: <http://www-med-fysik.vu-wien.ac.at/uv/COST726/COST726.Dateien/Results/Report.El.Arenosillo.pdf>, last access: 1 June 2010, August–September 2007, COST Office, ISBN 978-84-692-2640-7, Huelva, Spain, 64 pp., 2009.
- 30 Webb, A. and Holick, M.: The role of sunlight in the cutaneous production of vitamin D3, *Annu. Rev. Nutr.*, 8, 375–399, 1998.

## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Webb, A., Gardiner, B., Leszczynski, K., Mohnen, V., Johnston, P., Harrison, N., and Bigelow, D.: Quality assurance in monitoring solar ultraviolet radiation: The state of the art, Tech. Rep. 146, World Meteorological Organization, Geneva, Switzerland, 2003.

Webb, A., Gröbner, J., and Blumthaler, M.: A Practical Guide to Operating Broadband Instruments Measuring Erythemally Weighted Irradiance, Office for Official Publications of the European Communities, ISBN 92-898-0032-1, 21 pp., 2006.

World Health Organization (WHO): Protection against exposure to ultraviolet radiation, Tech. Rep. WHO/EHG #17, Geneva, Switzerland, 1995.

World Health Organization (WHO): Global solar UV index: A practical guide, WHO/SDE/OEH/02.2, WHO, Geneva, Switzerland, 2002.

World Meteorological Organization (WMO): WMO-UMAP workshop on broadband UV radiometers, Tech. Rep. 120, WMO/Global Atmosphere Watch, Geneva, Switzerland, 1996.

World Meteorological Organization (WMO): Report of the WMO-WHO meeting of experts on standardization of UV indices and their dissemination to the public, Les Diablerets, Switzerland, 21–24 July 1997, Tech. Rep. 127, WMO/Global Atmosphere Watch, Geneva, Switzerland, 1998.

## Influence of the calibration on experimental UV index

M. Antón et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion




**Table 1.** Parameters obtained in the correlation between measured and modeled UVI data. Experimental measurements are derived from manufacturer and one-step and two-steps methods, and modeled data are from LibRadtran/UVSPEC code. The parameters are as follows: the slope of the regression, the coefficients of correlation ( $R^2$ ), the root mean square errors (RMSE), the mean bias error (MBE), and the mean absolute bias error (MABE). The relative differences are calculated as measured minus modeled, divided by the modeled UVI data.

	Slope	$R^2$	RMSE (%)	MBE (%)	MABE (%)
Manufacturer	$0.85 \pm 0.01$	0.98	7.9	$+13.5 \pm 0.8$	$14.2 \pm 0.7$
One-step method	$0.99 \pm 0.01$	0.98	8.4	$+1.3 \pm 0.7$	$5.6 \pm 0.6$
Two-steps method	$0.99 \pm 0.01$	0.99	7.8	$+1.3 \pm 0.6$	$5.1 \pm 0.5$

**Influence of the calibration on experimental UV index**

M. Antón et al.

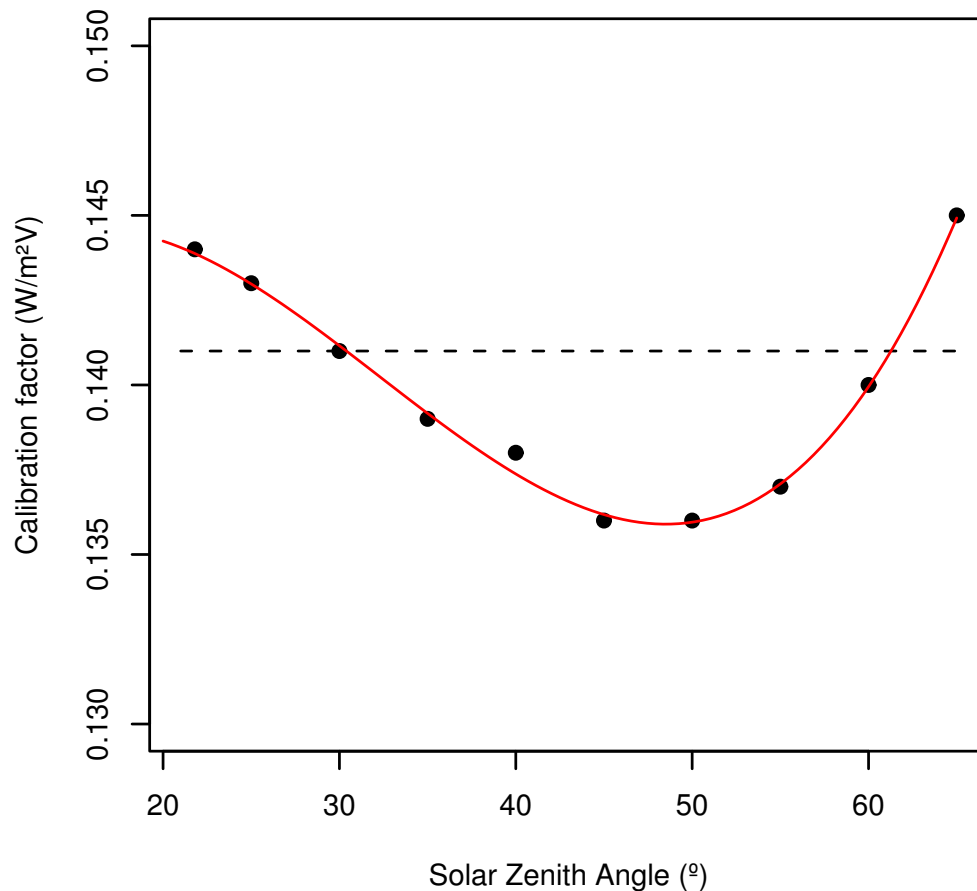


**Fig. 1.** Dependence of the calibration factors provided by the manufacturer (in black) on the solar zenith angles below  $65^\circ$ . The red line corresponds to the polynomial function given by the expression 1. The dashed line represents the fixed value of  $0.141 \text{ Wm}^{-2}/\text{V}$  proposed by the manufacturer when the dependence on solar zenith angle is not utilized.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

## Influence of the calibration on experimental UV index


M. Antón et al.

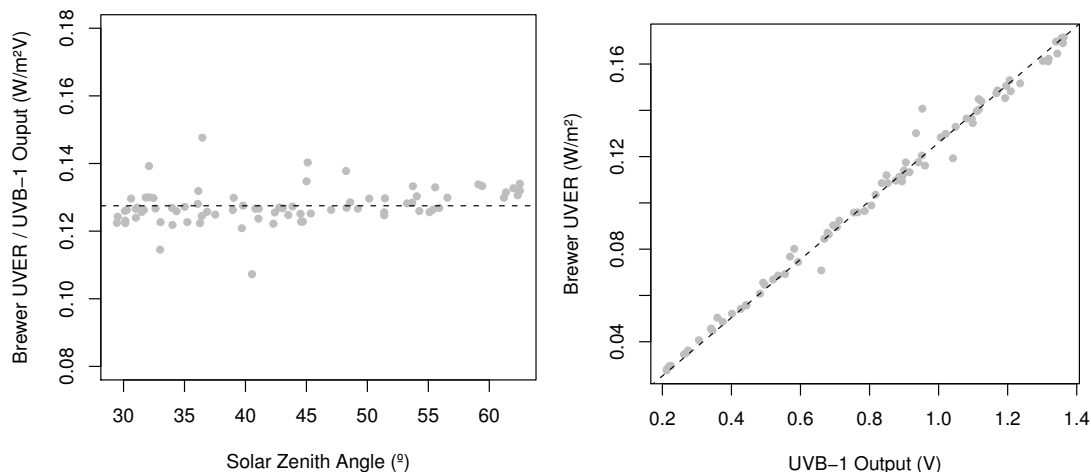

**Fig. 2.** Left: The ratio between the erythemally integrated irradiance given by the Brewer spectroradiometer and the YES UVB-1 radiometer output voltage as a function of the solar zenith angle during the Arenosillo's campaign 2007. The horizontal line represents the mean ratio ( $0.1275 \text{ Wm}^{-2}/\text{V}$ ). Right: Relationship between the Brewer erythemally integrated irradiance and the UVB-1 output voltage for SZA smaller than  $65^\circ$  together with the regression line corresponding to the first-order model.


**Influence of the calibration on experimental UV index**

M. Antón et al.

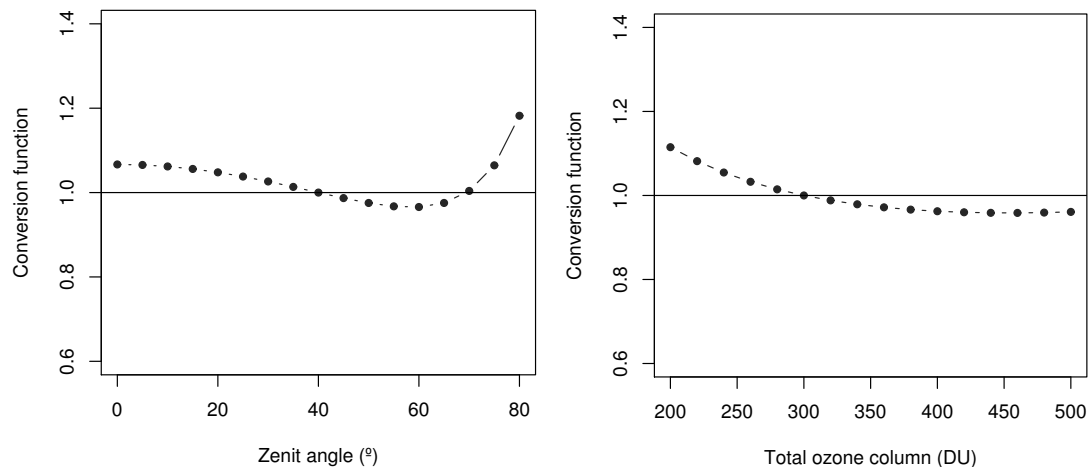

**Fig. 3.** Left: Variation of the normalized conversion function with respect to the solar zenith angle, for a constant total ozone column of 300 DU. Right: Variation of the normalized conversion function with respect to the total ozone column, for a constant solar zenith angle of  $40^\circ$ .

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

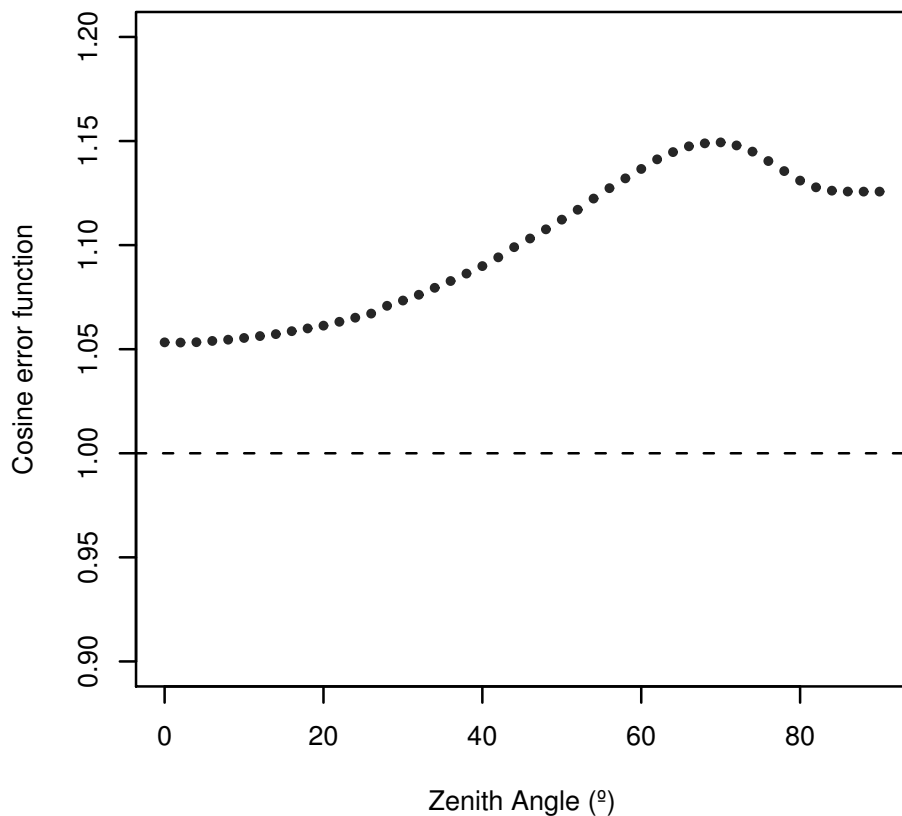

**Fig. 4.** Variation of the cosine correction function of the YES UVB-1 radiometer with respect to the solar zenith angle.

**Influence of the calibration on experimental UV index**

M. Antón et al.

Title Page

Abstract Introduction

Conclusions References

Tables Figures

◀ ▶

◀ ▶

Back Close


Full Screen / Esc

Printer-friendly Version

Interactive Discussion





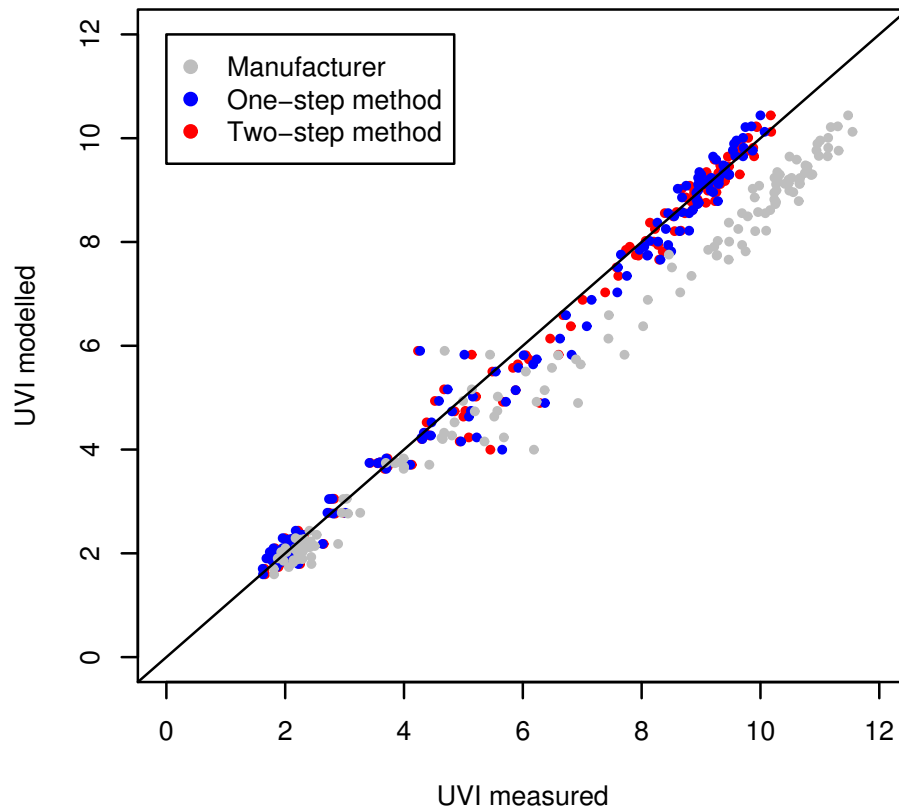

**Fig. 5.** Relationship between UVI estimations derived from LibRadtran/UVSPEC model and experimental UVI data obtained applying the manufacture’s factor and the two calibration procedures. The solid line is the zero bias line, unit slope.

**Influence of the calibration on experimental UV index**

M. Antón et al.

Title Page

Abstract Introduction

Conclusions References

Tables Figures

⏪ ⏩

◀ ▶


Back Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



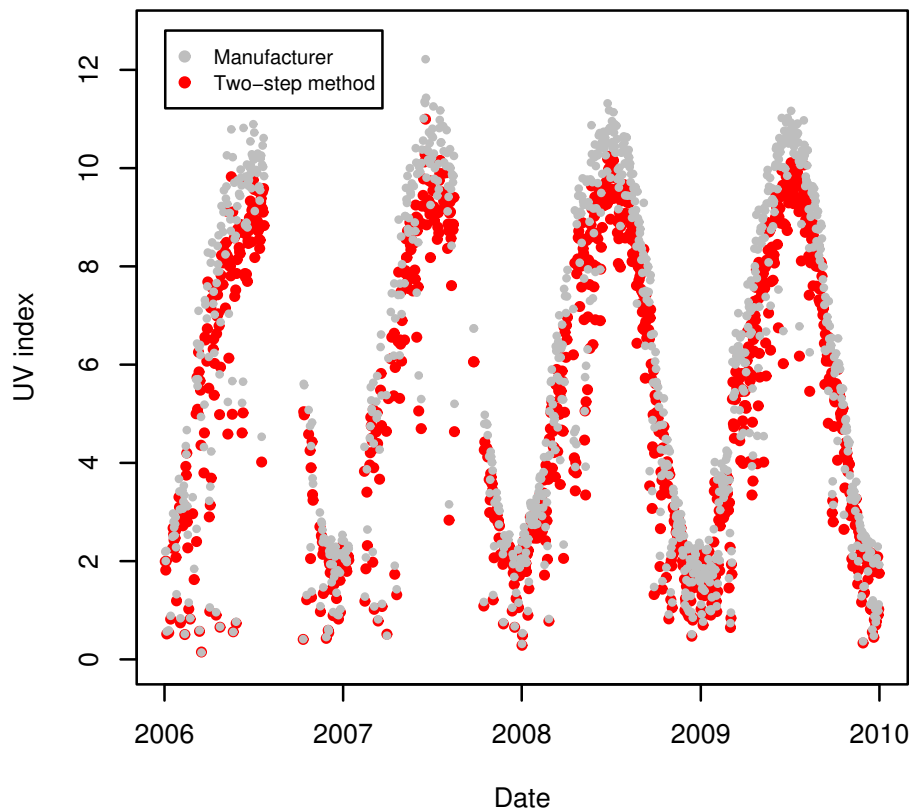

**Fig. 6.** Temporal evolution of the daily UVI at Granada during four years (2006–2009) using the two-steps calibration method and the manufacturer' calibration factors.

**Influence of the calibration on experimental UV index**

M. Antón et al.

Title Page

Abstract Introduction

Conclusions References

Tables Figures

⏪ ⏩

◀ ▶

Back Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

