

Interactive comment on “Performance of a corona ion source for measurement of sulfuric acid by chemical ionization mass spectrometry” by A. Kürten et al.

A. Kürten et al.

kuerten@iau.uni-frankfurt.de

Received and published: 11 February 2011

The comment was uploaded in the form of a supplement:
<http://www.atmos-meas-tech-discuss.net/3/C2691/2011/amtd-3-C2691-2011-supplement.pdf>

Interactive comment on Atmos. Meas. Tech. Discuss., 3, 5295, 2010.

C2691

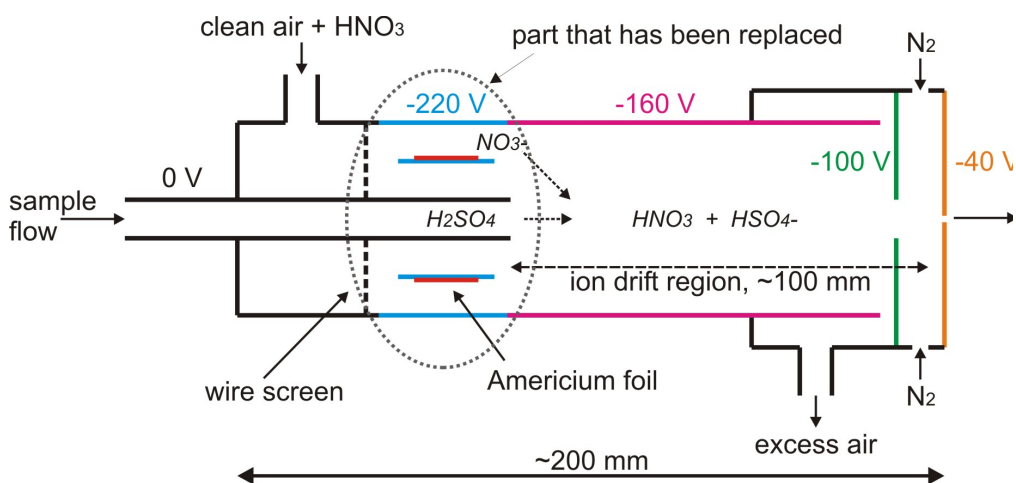


Fig. 1.

C2692

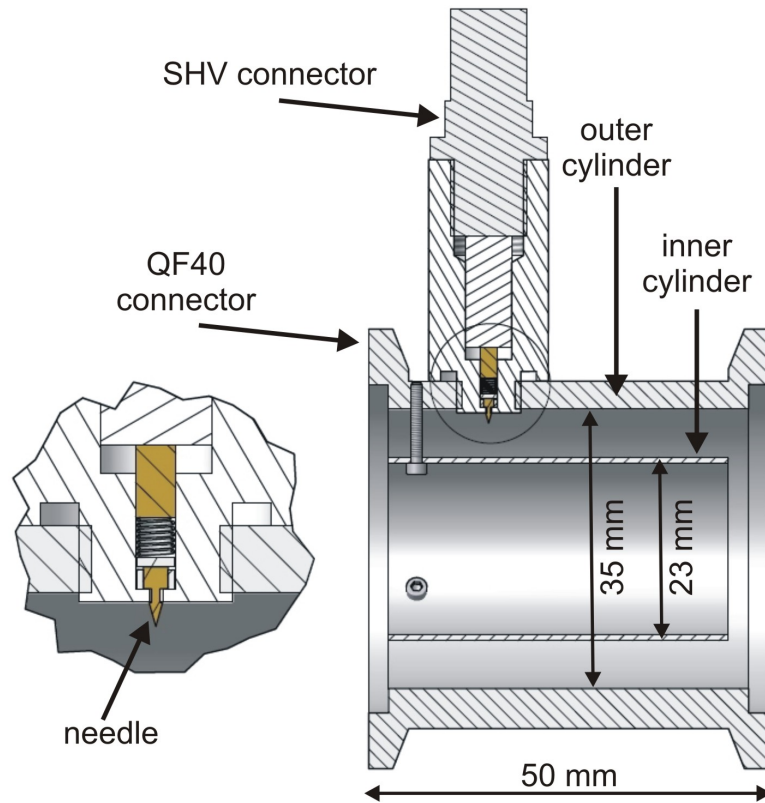


Fig. 2.

C2693

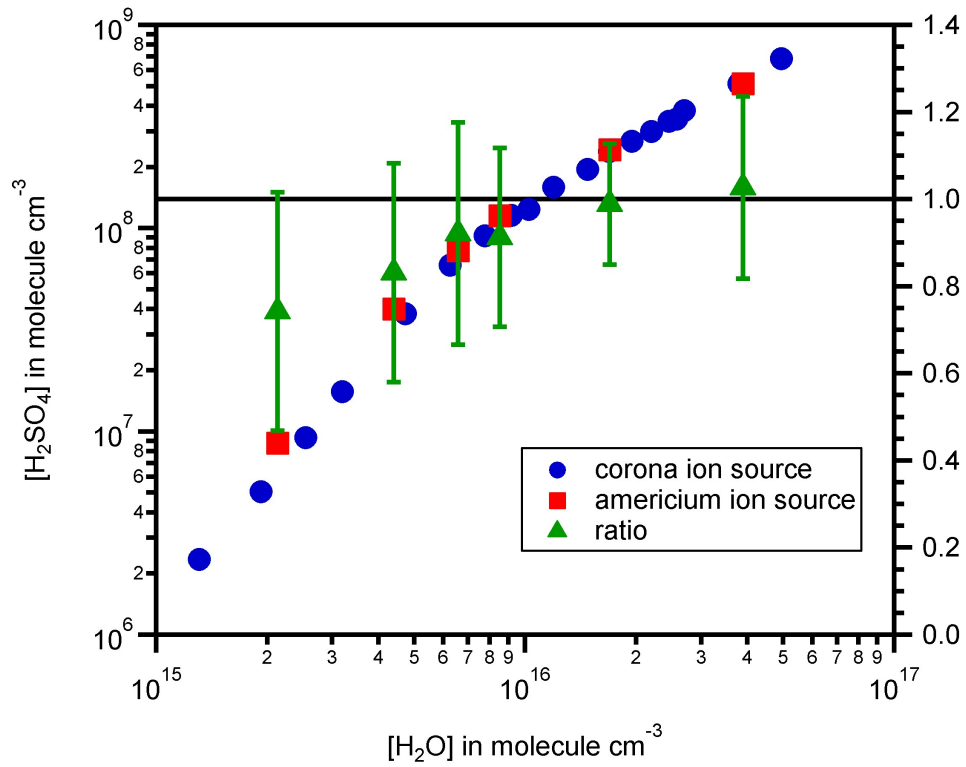


Fig. 3.

C2694