

This discussion paper is/has been under review for the journal Atmospheric Measurement Techniques (AMT). Please refer to the corresponding final paper in AMT if available.

Initial investigation of the wavelength dependence of optical properties measured with a new multi-pass aerosol extinction differential optical absorption spectrometer (AE-DOAS)

R. T. Chartier¹ and M. E. Greenslade^{1,*}

¹University of New Hampshire, Department of Chemistry, Durham, NH 03824, USA

*now at: RTI International, Research Triangle Park, NC, USA

Received: 28 August 2011 – Accepted: 19 September 2011 – Published: 12 October 2011

Correspondence to: M. E. Greenslade (margaret.e.greenslade@unh.edu)

Published by Copernicus Publications on behalf of the European Geosciences Union.

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

[Title Page](#)

[Abstract](#)

[Introduction](#)

[Conclusions](#)

[References](#)

[Tables](#)

[Figures](#)

[⏪](#)

[⏩](#)

[◀](#)

[▶](#)

[Back](#)

[Close](#)

[Full Screen / Esc](#)

[Printer-friendly Version](#)

[Interactive Discussion](#)

Abstract

Atmospheric aerosols directly affect climate by scattering and absorbing radiation. The magnitude of the impact is dependent upon the wavelength of light, but is often estimated near 550 nm. When light scattering and absorption by aerosols is approximated, the wavelength dependence of the refractive index for specific components is lost. As a result, climate models would have inherent uncertainties for aerosol contributions to radiative forcing when considering the entire solar spectrum. An aerosol extinction differential optical absorption spectrometer has been developed to directly measure aerosol extinction at mid-ultraviolet to near infrared wavelengths. The instrument consists of a spectrometer coupled to a closed White-type multi-pass gas cell with an adjustable path length of up to approximately 20 m. Laboratory measurements of various gases are compared with known absorption cross sections. Additionally, the extinction of monodisperse samples of polystyrene latex spheres are measured and compared to Mie theory generated with refractive index values from the literature to validate the new instrument. The polystyrene experiments also emphasize the ability of the new instrument to retrieve the wavelength dependent refractive index, especially in the ultraviolet wavelength regions where variability is expected. The spectrometer will be a significant advancement for determining wavelength dependent complex refractive indices in future laboratory studies as well as provide the ability to monitor ambient aerosol light extinction.

1 Introduction

The Earth's radiation balance is directly impacted by aerosols that can scatter and absorb radiation. Further, this balance is indirectly affected by aerosols as they can serve as cloud condensation nuclei (CCN), which can alter cloud properties and change how clouds interact with solar and terrestrial radiation. Characterizing the optical properties of aerosols in relationship to their direct effects on climate has been the focus of select

AMTD

4, 6315–6349, 2011

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



studies, while many focus on experimentally determining optical properties or modeling their climate effects (Bates et al., 2006; Ge et al., 2010; Kanakidou et al., 2005; Massoli et al., 2009; Moffet and Prather, 2009). Model simulations have led to the conclusion that the radiative forcing by anthropogenic aerosols is comparable in magnitude to that of some greenhouse gases (IPCC, 2007). Despite this recent progress, some large uncertainties still remain in the understanding of aerosol optical properties, classification and loading. Decreasing specific uncertainties, such as the wavelength dependence of scattering and absorption by aerosols, can lead to improved understanding of climate change.

The wavelength dependence of aerosol optical properties, specifically the aerosol optical depth (AOD), is typically approximated in current research by the Ångström exponent, introduced by Anders Ångström (Ångström, 1929, 1930). The equation describing the wavelength dependent optical depth of particulate matter is:

$$\tau_a = \beta \lambda^{-\alpha} \quad (1)$$

where τ_a is the aerosol optical depth in the atmosphere, β is the turbidity coefficient defined by Ångström at a wavelength of $1 \mu\text{m}$, λ is the wavelength (μm) where τ_a is observed, and α is the Ångström exponent, which is equivalent to the ratio of the natural log of Eq. (1) at two different wavelengths. However, based on the work of Mie, Ångström notes that this equation is only valid over a limited wavelength range (Ångström, 1929). In fact, Eck and co-workers showed that ambient measurements of biomass burning and urban/industrial aerosols was better fit with a second order polynomial function than the linear representation of Eq. (1) for the wavelength range from 340 to 1020 nm (Eck et al., 1999). This observed curvature is an indication that Eq. (1) cannot be used over this large wavelength range or the range of the solar spectrum. In contrast, observations of desert dust were consistently represented by Eq. (1). The authors attribute their mixed results to differences in the size distributions of aerosols, where the former is more likely to be accumulation mode while the later is centered in the coarse mode (Eck et al., 1999).

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

The Bergstrom et al. (2002) study of aerosols in the north Atlantic (TARFOX) investigated the wavelength dependence of the absorption of black carbon particles (Bergstrom et al., 2002). In their work, they investigated size effects as implicated by Eck as well as the wavelength dependence of the refractive index (RI). Bergstrom et al. (2002) also compiled data from previous studies and in comparison with their work, indicate that the complex refractive index (CRI), where the CRI (m) is given as $m = n + ki$ with n being the real part and k being the imaginary part, of soot ranges from (1.3 to 2.2) + (0.8 to 1.3) i between 300–3000 nm (Bergstrom et al., 2002). The authors indicate that the single scattering albedo (SSA – the ratio of scattering efficiency to total extinction efficiency) from aerosols of black carbon mixed with non-absorbing species decreases with increasing wavelength, which contrasts with results for mineral dust aerosol SSA that increases with increasing wavelength (Bergstrom et al., 2002). A single scenario does not account for these cases.

In addition to the above, the classifications of aerosols used to broadly define their optical properties and climate impact have recently been expanded from broader categories such as black carbon, organic carbon and inorganic species to include brown carbon (BrC) and yellow carbon (Andreae and Gelencser, 2006; Bond and Bergstrom, 2006; Kirchstetter et al., 2004; Moosmuller et al., 2011; Yang et al., 2009). The colored organic compounds which make up these new classifications have increases in absorption, sometimes significant, with decreasing wavelength, especially into the ultraviolet (UV) wavelength region (Andreae and Gelencser, 2006; Moosmuller et al., 2011). The wavelength dependent absorption of BrC leads to $\alpha_{\text{abs}} > 1$, but different methods of determination yield different results. For example, ground based optical filter methods result in α_{abs} from 1 to 3.5, but solution phase results from aerosol extracts are much higher, with values between 4.7 and 16 (Bond, 2001; Bones et al., 2010; Chen and Bond, 2010; Hecobian et al., 2010; Hoffer et al., 2006; Kirchstetter et al., 2004; Marley et al., 2009; Yang et al., 2009). This discrepancy in α_{abs} for aerosols and their extracts needs to be reconciled. Therefore, it is important to quantify the wavelength dependence of the aerosol optical properties, especially the CRI, as systematically as

possible, with preference for (in situ) techniques.

The optical properties of aerosols are impacted by the wavelength dependence of the CRIs of the chemical species from which they are composed. The wavelength dependence of the RI for some aerosol components is known. Techniques such as ellipsometry and vacuum ultraviolet reflectance spectroscopy can be used to obtain both the real and imaginary portion of the CRI (French et al., 2007). Once known, the values can be used in theoretical models, such as Mie calculations, to generate estimates for the aerosol optical properties. For example, the wavelength dependence of the CRI for polystyrene and polystyrene latex spheres (PSLs), where the later are often used as a calibration tool in aerosol research, has been studied. Recently, a number of reported RI values including some dating back to the 1950s for polystyrene were employed in a comprehensive paper (Miles et al., 2010a). The wavelength range for most of the values was longer than 400 nm, so we do not incorporate all of them in our work (Miles et al., 2010a). But we do consider that Miles et al. (2010a) mention the lower refractive indices reported by Ma et al. (2003) in comparison to other literature values and that the previous measurements were made with different forms of polystyrene, bulk or suspension (Ma et al., 2003; Miles et al., 2010a). We consider several values for the RI reported near 589 nm: French et al. (2007) report $1.591 + 0.047i$ for PS-677 at 590 nm, Ma et al. (2003) report 1.584 at 590 nm, Nikolov and Ivanov (2000) report 1.592 at 588 nm, while, the manufacturer, Thermo Scientific reports 1.59 at 589 nm (French et al., 2007; Ma et al., 2003; Nikolov and Ivanov, 2000). There is little variation in RI at this wavelength, leading to small differences in calculated optical properties, but the values diverge with decreasing wavelength. Approaching the UV ($\lambda < 400$ nm), there is significant variability in the CRI values that may result from differences in the manufacturing processes for the polystyrene samples or measurement uncertainty. There are many types of polystyrene that have different physical and chemical properties such as molecular weights, densities and polarities. The variation in the CRI is matched by fluctuations in the extinction results for aerosols composed of polystyrene especially since some of the CRI changes are abrupt and significant. To our knowledge, below

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



**Initial investigation of
an aerosol extinction
spectrometer**R. T. Chartier and
M. E. Greenslade

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

$\lambda = 370$ nm, the RI of polystyrene has only been studied by French et al. (2007). Their data show a large and dramatic increase in the imaginary portion of the CRI below 230 nm and from approximately 300–400 nm (French et al., 2007). Measurements at UV wavelengths are of particular importance when monitoring aerosol optical properties because this is a region of potentially dramatic change in optical properties for certain types of aerosols, especially those with some color like BrC (Andreae and Gelencser, 2006; Bond and Bergstrom, 2006; Kirchstetter et al., 2004; Moosmuller et al., 2011; Yang et al., 2009). Variable optical properties can be used for classification and may be significant at higher altitudes for climate predictions.

A variety of instruments measure aerosol optical properties, but this is often only at a single wavelength or a few select wavelengths. Some instruments have been designed to measure aerosol optical properties as a function of wavelength. For example, differential optical absorption spectroscopy (DOAS) or similar techniques have been used to directly measure aerosol extinction (the sum of scattering and absorption) (Honninger et al., 2004; Mogili et al., 2007; Schnaiter et al., 2003; Schnaiter et al., 2005; Si et al., 2009; Takashima et al., 2009; Virkkula et al., 2005). This technique uses a broadband light source to determine the differential spectra of a sample versus background. It is most commonly used to determine the concentration of trace gas species in the atmosphere, but it has also been used to measure aerosol extinction.

With long, open paths, these instruments can have low detection limits for aerosol extinction (Honninger et al., 2004; Si et al., 2010; Takashima et al., 2009). However, typical DOAS instruments with open paths can only be used to measure the optical properties of a bulk aerosol sample (Platt and Stutz, 2008) and therefore cannot be used to differentiate between aerosol type and the specific optical properties of the constituents of that aerosol sample. A limited number of laboratory instruments based on DOAS are capable of measuring aerosol extinction over the majority of the solar spectrum, some at atmospherically relevant particle concentrations. An optical extinction cell (OES) was developed to measure extinction at three wavelengths (467, 530, 660 nm), but the sample path length is 330.2 cm, which makes this instrument sensitive

**Initial investigation of
an aerosol extinction
spectrometer**R. T. Chartier and
M. E. Greenslade

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

5 enough to only measure very concentrated aerosol samples (Virkkula et al., 2005). An Ocean Optics UV/Vis spectrometer has been coupled to an environmental chamber to measure the extinction of mineral dust from 250–800 nm, but the sample path length of 66.5 ± 0.5 cm leads to a detection limit useful only for high particle concentrations (Mogili et al., 2007). A dual-beam long path extinction spectrometer (LOPES) has been used to measure aerosol extinction from 200–1100 nm with a 2.5 nm spectral resolution (Schnaiter et al., 2003, 2005). The 10 m LOPES instrument uses a corner cube design and is able to accurately measure extinction over the entire wavelength range with a lower detection limit of 20 Mm^{-1} , which is adequate for measuring extinction in polluted urban areas where total extinction can reach levels of upwards of 1000 Mm^{-1} (Andreae et al., 2008; Schnaiter et al., 2005). A commercial white light aerosol spectrometer (WELAS) available from PALAS GmbH (Germany) operates from 370–780 nm and has been employed by Flores et al. (2009) to determine aerosol extinction and retrieve refractive indices, however, these are reported as an average from 400–800 nm and are not wavelength resolved (Flores et al., 2009). A cavity attenuated phase shift (CAPS) spectroscopy instrument has been tested at 445 and 632 nm with an effective path length of 2 km and is reported to have a precision of $\sim 0.2 \text{ Mm}^{-1}$, but is limited to a single wavelength per experiment (Massoli et al., 2010). Cavity ring down (CRD) instruments have been built with several wavelength channels or small spectral ranges, including 1550, 1520, 1064, 683, 675, 620, 570–540, 532, 425–385, 390, 355 nm, with excellent precision (Baynard et al., 2007; Bulatov et al., 2002; Butler et al., 2009; Dinar et al., 2008; Mellon et al., 2011; Miles et al., 2010b; Moosmuller et al., 2005; Pettersson et al., 2004; Smith and Atkinson, 2001; Spindler et al., 2007; Strawa et al., 2003; Strawa et al., 2006).

25 Our aerosol extinction differential optical absorption spectrometer (AE-DOAS) is unique because it is a broadband instrument and continuously covers nearly the entire solar spectrum from 220 to 1050 nm with better than 0.5 nm resolution. In the following, we will show that the AE-DOAS has high sensitivity in repeat measurements. Further, its wavelength calibration was investigated and confirmed using gases which absorb

Initial investigation of an aerosol extinction spectrometerR. T. Chartier and
M. E. Greenslade

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

strongly in this range, specifically ozone and acetone. The results are compared with known absorption cross sections from the literature for wavelength agreement. The accuracy is investigated with aerosols, specifically PSLs, and a closure loop is generated with a Mie theory model. Our results are compared with previous studies of the wavelength dependence of the RI of polystyrene, though only one direct comparison with prior research is possible at UV wavelengths (French et al., 2007; Ma et al., 2003; Nikolov and Ivanov, 2000). We will show that the strong changes seen in the UV region for the imaginary portion of the CRI by French et al. (2007) were not observed in our particular polystyrene sample. By monitoring various sizes of PSLs, the closure loop provides a way to determine the wavelength dependent CRI for polystyrene (Abo Riziq et al., 2007; Lang-Yona et al., 2009; Miles et al., 2010a). Our results further emphasize the need to monitor the wavelength dependence of aerosol optical properties.

2 Experimental

A bench-top AE-DOAS was custom manufactured by Cerex Monitoring Solutions, LLC (CMS UV-5000) to monitor aerosol extinction, despite the use of absorption in the historical name. This system consists of a 1000 watt continuous duty xenon (Xe) lamp, fiber-optically coupled to a White-type multi-pass gas cell, and then to a single beam UV/Vis spectrometer as shown in Fig. 1. The White-type multiple reflection system is made using three separate concave mirrors, each having the same radius of curvature. The distance between the mirrors is twice the focal length in order to clearly reproduce the image of the light source on the mirrors (White, 1942). The Xe lamp and coated mirrors provide spectral coverage ranging from the mid-ultraviolet to near infrared (approximately 220–1050 nm) at a resolution of better than 0.5 nm. The lamp intensity is not smooth over the entire spectral range but rather contains a large broad peak spanning the UV and visible up to approximately 750 nm. At wavelengths between 780–880 nm, the lamp intensity is low, and after 900 nm there are sharp emission peaks from the Xe lamp. This is all corrected for by routinely taking background measurements, but sharp

features can be seen in some spectra and the instrumental detection limit at a specific wavelength is directly related to the lamp intensity at that wavelength.

The stainless steel multi-pass gas cell (left-half of Fig. 1) has outer dimensions of 73.0 cm × 19.2 cm × 7.5 cm and an internal volume of approximately 5.8 l. Spacers present in the bottom of the gas cell minimize the internal volume and reduce sample residence times. The path length can range from 2.44 to 19.51 m and is adjusted by counting the number of reflections on the primary mirror. Alignment of the incident beam within the multi-pass cell is achieved by slight movements of the mirrors in conjunction with monitoring the lamp spectrum shape and intensity. A fiber optic cable transfers the light back to the spectrometer. The spectrometer consists of a grating and a 3078 element linear diode array (LDA), which is standard for UV/Vis spectroscopy. In this work, a path length of 19.51 m was used for all experiments unless otherwise noted.

Instrumental detection limits are commonly defined as 3σ of the baseline noise of two consecutive measurements, and a typical example of the AE-DOAS wavelength dependent detection limit is shown in Fig. 2. The detection limit shown was calculated using two consecutive measurements of particle free nitrogen with a path length of 19.51 m and an integration time of 180 s. The increases in detection limit seen in Fig. 2 below 235 nm and above 700 nm are due to the decreased intensity of the lamp and variable mirror reflectivity. The average detection limit of the AE-DOAS from 235–700 nm is 32.5 Mm^{-1} . For comparison, the lower detection limit of the LOPES instrument is reported to be 20 Mm^{-1} ; however, a comparable average is not reported (Schnaiter et al., 2005). The lower detection limit of the AE-DOAS measurement shown in Fig. 2 is 12.6 Mm^{-1} at 366 nm and has been observed to be as low as 6.2 Mm^{-1} at approximately 350 nm during background sampling before subsequent experiments. The detection limit of the AE-DOAS is variable, but can be calculated for any experiment by finding 3σ of the baseline for the last two zero measurements before the sample is introduced. Based on the lamp spectrum and detection limit, we will primarily use the instrument in the 235–700 nm wavelength range.

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

**Initial investigation of
an aerosol extinction
spectrometer**R. T. Chartier and
M. E. Greenslade

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Experiments were conducted with gas phase species, specifically ozone and acetone samples, as a wavelength calibration to show that the detector was properly aligned. The gas of interest is directed through the gas cell by positioning a small pump (Hargraves mini diaphragm pump, H037A-11) operating at 3 l min^{-1} at the outlet.

5 The ozone was produced by a spark discharge ozone generator and was monitored with a path length of 9.75 m. For the acetone experiment, an open vessel containing liquid acetone was simply placed at the inlet to the gas cell and the vapor pressure entrained sufficient acetone into the sample flow to allow measurement.

The absorption of light by gas phase species can interfere with aerosol extinction measurements. Based on three year local maxima observed at a UNH operated field site (Thompson Farm) for 40 gas phase species and literature values for absorption cross sections, it was determined that the most significant interferences would occur in the UV and that the most important species to monitor are ozone, nitrogen dioxide, sulfur dioxide, and water (<http://airmap.unh.edu/>). As long as significant concentration changes of these gases are not encountered during the course of an ambient experiment, interferences can be accounted for by measuring filtered, aerosol free ambient air as a background. For the gas phase experiments presented here, laboratory air was used as a background and compared to laboratory air enhanced in the species of interest. In the laboratory aerosol experiments, nitrogen is used as a background and for aerosol generation to minimize gas phase interferences.

Polystyrene latex spheres have a small ($\leq 5\%$) coefficient of variation in diameter and are often used as a proxy for monodisperse spherical aerosols. PSLs interact with light as predicted by Mie theory, and therefore make a good calibration standard for aerosol measurement techniques (Baynard et al., 2007; Cai et al., 2006; Galli et al., 2001; Lang-Yona et al., 2010; Liu et al., 2010; Miles et al., 2010a). All PSL solutions in this work were made fresh and mixed in test tubes by diluting 15 drops of 10% w/w PSL solution (Duke Scientific Corporation, now part of Thermo Scientific) in 20 ml deionized water (J. T. Baker, HPLC Water). To measure a monodisperse PSL aerosol sample the setup in Fig. 3 was used. In detail, the aerosol sample was atomized then dried

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

to a relative humidity of $<3\%$ by flowing over molecular sieves housed in a diffusion dryer. The dried aerosol sample was size selected at the diameter of the PSLs by a differential mobility analyzer (DMA-TSI model 3080L). The monodisperse PSL sample then enters the AE-DOAS where continuous extinction measurements are made as the sample flows through the gas cell. Upon exiting the gas cell, the aerosol sample enters the condensation particle counter (CPC-TSI model 3775). The uncertainty of the counted particle concentrations is $\pm 10\%$. Particle concentration varies as a function of time during an experiment.

The highest AE-DOAS extinction signal for an experiment is assumed to correspond to the maximum aerosol concentration for the experimental trial. A time offset is defined as the difference between the start time of the AE-DOAS measurement with the highest extinction and the time the maximum concentration was measured by the CPC. For all PSL measurements discussed in this work the time offset from the AE-DOAS measurement to the aerosol concentration measurement was between 8.5–10.5 min.

Mie calculations using three different sets of refractive indices for polystyrene were performed using Fortran and MatLab programs (<http://www.hiwater.org/Mie/calcs.html>), based on that of Bohren and Huffman, (Bohren and Huffman, 1983; Mätzler, 2002). The first calculation is generated using the RI of PSLs given by the manufacturer, Duke Scientific Corporation now a division of Thermo Scientific, as 1.59 at 589 nm and using this value at all wavelengths (<http://www.thermoscientific.com/wps/portal/ts/products/detail?navigationId=L10397&categoryId=87439&productId=11962886>). This does not give an indication of the wavelength dependence for our experiments but rather is an approximation similar to assumptions made in some climate modeling studies. The manufacturer does discuss the wavelength dependence to the RI of the PSL in a technical document (http://www.thermo.fr/eThermo/CMA/PDFs/Various/File_3936.pdf), but references previously published data (Boundy and Boyer, 1952; Ma et al., 2003). The second set of RI data is wavelength dependent and was derived from experimental data fit to determine dispersion coefficients of Cauchy's equation (Ma et al., 2003; Nikolov and Ivanov, 2000). The results of Nikolov and Ivanov (2000) are similar to Ma

**Initial investigation of
an aerosol extinction
spectrometer**R. T. Chartier and
M. E. Greenslade

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

et al. (2003), but the former do not report index of refraction values below 436 nm; the Ma et al. (2003) data is reported for wavelengths greater than 370 nm, and we use their data to 370 nm and further extrapolate into the UV. The third set was determined experimentally and is reported from 207–1033 nm (French et al., 2007). The two sets of wavelength dependent RIs we use in our calculations differ somewhat in the real portion of the CRI (n), while only French et al. (2007) data includes a non-negligible imaginary portion of the CRI (k). The calculated Mie extinction values were then compared with the experimental results to complete a closure loop. Because of the capabilities of the AE-DOAS, closure studies can be completed at a particular PSL size and displayed as aerosol extinction cross section versus wavelength. Aerosol extinction cross section is analogous to the gas phase molecular absorption cross section and is calculated as the raw extinction value (cm^{-1}) divided by the particle number concentration (particles cm^{-3}) to yield units of $\text{cm}^2 \text{particle}^{-1}$. Alternatively, the value of Q_{ext} , which is the dimensionless efficiency of extinction calculated by dividing the extinction cross section by the geometric cross section of the aerosols, can be plotted versus size parameter (χ), which is defined as $\pi d/\lambda$, where the diameter (d) is varied. The later method is reported for a single λ but can be duplicated at many different wavelengths and has been used previously to validate CRD instruments (Baynard et al., 2007; Miles et al., 2010a). It can also be used to determine the CRI at each specific wavelength by fitting the data (Abo Riziq et al., 2007; Dinar et al., 2008; Erlick et al., 2011; Flores et al., 2009; Freedman et al., 2009; Kim et al., 2010; Lack et al., 2006; Lang-Yona et al., 2009; Mack et al., 2010; Miles et al., 2010a, b).

3 Results

Ozone has broad absorption bands throughout the UV/Vis spectrum and high concentrations can be readily observed by the AE-DOAS (Voigt et al., 2001). The absorption of ozone measured by the AE-DOAS is shown in Fig. 4. This is the Hartley band which spans from approximately 200–300 nm with an intense absorption peak centered at

255 nm. Figure 4 also compares our results with literature (Bogumil et al., 2003). It was necessary to adjust the AE-DOAS spectrum by adding 1 nm to the result to achieve excellent agreement with the literature spectrum. The literature absorption cross section was used to determine that approximately 650 ppbv of ozone was present during the measurements.

Initially, acetone was identified in laboratory air as a gas phase interference near $\lambda = 275$ nm due to changing signal in background measurements. Subsequent laboratory experiments described above yielded the spectrum in Fig. 5. By comparing with literature results for acetone absorption (Meyrahn et al., 1986), also seen in Fig. 5, the interfering species was confirmed. No adjustment was required for the wavelength in this case and the alignment of the spectrometer and the linear diode array is confirmed with the standard path length. The acetone concentration during the experiment shown in Fig. 5 was determined to be 190 ppmv. Acetone is commonly used in the building and its concentration will change so the background must be monitored during ambient experiments.

An experimentally obtained wavelength dependent spectrum of the extinction cross section for 300 nm diameter PSLs is shown in Fig. 6. On the wavelength axis, each open circle shown is the smoothed average across ten raw experimental data points. Intensity of the extinction cross section is displayed as an average of eleven spectral retrievals completed on three different days, where the error bars represent one standard deviation of the mean. Additional experiments were performed at various path lengths and yielded similar results, though these are not shown here. Each size of PSL has a unique aerosol extinction cross section spectrum as a function of wavelength due to size effects. We do not show those other spectrum here but instead focus on closure comparisons with Mie theory.

Mie calculations performed using a Cauchy representation of RI are shown in Fig. 6 as filled triangles (Ma et al., 2003), while calculations using the CRI retrieved from experiments are shown as filled squares (French et al., 2007). The Mie calculation using the constant RI reported by the manufacturer(<http://www.thermoscientific.com/wps/>

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

portal/ts/products/detail?navigationId=L10397&categoryId=87439&productId=11962886),
are displayed as filled diamonds in Fig. 6. There is clearly a difference between the two
wavelength dependent theoretical results, though the general shape of the spectra
agree with a few minor issues. The theoretical calculation using the constant manu-
5
factorer's RI has a spectral shape which does not match as well as the spectra from
the wavelength dependant RI. Specifically, the intensity is decreased in the UV for our
experimental spectrum, but there is a peak seen with the constant RI model. Also, with
the constant manufacturer's RI, there is a blue shift of each of the peaks in comparison
10
to the experimental AE-DOAS spectrum. For the other two theoretical results, it is clear
that the RI calculated from Cauchy coefficients from Ma et al. (2003) overestimates the
extinction cross sections from 220–400 nm. The intensity of the extinction cross sec-
tion model based on the French et al. (2007) complex RI most closely matches the
AE-DOAS spectrum.

Since the aerosol extinction cross section spectra are unique for each PSL size, we
15
present an alternative view of this data. A representation of the size dependent aerosol
extinction is reported in Fig. 7 as Q_{ext} versus size parameter at a wavelength of 248 nm.
It is especially important to investigation the UV region because few experimental or
theoretical results are available for these wavelengths. The experimental measure-
ments are depicted as open circles and the error bars are one standard deviation of
20
the mean for multiple measurements. The solid black line in Fig. 7 is the Mie theory
calculation using the French et al. (2007) CRI, $m = 1.826 + 0.059i$, reported at a wave-
length of 248 nm (French et al., 2007). The agreement is excellent as the experimental
data overlaps with the Mie theory model in all cases.

Good agreement between experiment and theory is obtained for 248 nm, however,
25
this agreement varies at other wavelengths. Aerosol Q_{ext} versus size parameter for a
wavelength of 335 nm is shown in Fig. 8, with open circles representing the experimen-
tal data. The solid black line in Fig. 8 is the same theoretical calculation as in Fig. 7, but
using the complex RI of $m = 1.686 + 0.197i$ reported at a wavelength of 335 nm (French
et al., 2007). A dotted light grey line is added to Fig. 8 and is a Mie theory calculation

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

using the real portion of the French et al. (2007) wavelength dependent CRI but with the imaginary portion of the CRI set to zero. This variation improves the agreement between theory and experiment.

In addition to comparing the experimental results with several Mie theory simulations, we have retrieved the CRI at the wavelengths studied in detail ($\lambda = 248$ and 335 nm) using methods previously described in the literature (Abo Riziq et al., 2007; Dinar et al., 2008; Erlick et al., 2011; Flores et al., 2009; Freedman et al., 2009; Kim et al., 2010; Lack et al., 2006; Lang-Yona et al., 2009; Mack et al., 2010; Miles et al., 2010a, b). For this work, we have used an interface from J. M. Flores to retrieve the CRI using the data in Figs. 7 and 8. At wavelengths of 248 nm and 335 nm, PSL are found to have a CRI of $m = 1.81(\pm 0.03) + 0.05(\pm 0.07)i$ and $1.72(\pm 0.02) + 0.005(\pm 0.03)i$, respectively. Mie theory curves from the retrieved RI are also shown on Figs. 7 and 8 as grey dot-dash lines. The curves are similar to those based on the French et al. (2007) data, though improvements in the fit are visible for the $\lambda = 335$ nm case.

4 Discussion

The AE-DOAS spectrum of ozone shown in Fig. 4 was taken at concentrations that are greater than most polluted conditions. This high concentration could have led to minor broadening and the need for the 1 nm wavelength offset. Alternatively, it is possible that the alignment to the spectrometer was imperfect during this sampling with a path length of 9.75 m, and this misalignment may have led to the observed small shift in wavelength. This problem will not contribute to issues in our aerosol measurements because they are completed with a longer path length and further the aerosol extinction is broad so small shifts in the wavelength calibration would not be significant. It should also be noted that this relatively short path length means that ambient measurements using longer path lengths may contain interferences from lower ozone concentrations. As pointed out previously, this can be overcome during measurements of ambient aerosol extinction by frequently monitoring the background gas intensity using

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

filtering at regular intervals. Alternatively, if the concentration is expected to change rapidly on the measurement time scale, then the ozone concentration could be monitored directly and the spectrum corrected using well know absorption coefficients for ozone. In order to better confirm the alignment of the system at the standard configuration with a path length of 19.51 m, acetone was monitored. The agreement between the literature and experimental spectra in Fig. 5 is excellent. There is no wavelength offset needed and none was used for the remainder of the experiments as the alignment was consistent.

In Fig. 6, it is clear that Mie theory generated by the Cauchy derived RI and the constant manufacturer's RI specified at 589 nm differs from the experimental spectrum of 300 nm PSL at wavelengths into the UV (Ma et al., 2003). The agreement between the spectrum of 300 nm PSL and the Mie theory calculations made using the French et al. (2007) wavelength dependent CRI provides the best agreement between our results and the three theoretical spectra (French et al., 2007). Using this model represented by filled squares that includes the imaginary part of the CRI, the agreement is especially improved at wavelengths less than 300 nm in the UV region of the spectrum. At wavelengths less than 370 nm, the Ma et al. (2003) data was not provide but rather has been extrapolated and this may have lead to the disagreement observed in Fig. 6. On the other hand, all of the theoretical 300 nm PSL extinction cross section spectra appear to be slightly enhanced over the experimentally determined values at wavelengths greater than 400 nm, suggesting that more light is reaching the AE-DOAS detector than is predicted by Mie theory. This over prediction is nearly resolved at wavelengths longer than 475 nm, where any remaining disagreement may result from enhanced forward scattering at longer wavelengths.

Closer examination of Fig. 6 reveals that even the good agreement achieved with the Mie theory calculations made using the French et al. (2007) wavelength dependent CRI has spectral regions with greater deviations. For example, the Mie theory calculations predicted higher extinction cross sections from 230–240 nm than were measured experimentally. Differences between the theory and measured extinction

cross section spectra in the wavelength range of approximately 300–370 nm can also be seen, though these are mostly within the error of the measurements. The agreement can be investigated in more detail by examining the value of Q_{ext} as a function of size parameter at specific wavelengths.

Figure 7 depicts the experimental and Mie theory calculated extinction efficiencies for various size PSLs at a wavelength of 248 nm. A wavelength of 248 nm was chosen for this calculation because Mie theory calculations appear to correlate well with the extinction measurements for 300 nm diameter PSL and for various other sizes. Further, the lamp is stable and the detection limit is low at a wavelength of 248 nm. This type of depiction of extinction efficiency displays broad maxima and minima called interference structure which is due to constructive and destructive interference, respectively, between rays of scattered light. In addition, there are often smaller sharp peaks which are referred to as ripple structure. The ripple structure is smoothed when broad size distributions are monitored, aerosols absorb light, or if there is dispersion in wavelength at the light source. For these reasons, minimal ripple structure is expected. The experimental results follow the interference structure calculated for Q_{ext} , specifically the theoretical trace is within the 1σ error bars at all measured sizes. The experimental results even follow the small amount ripple structure present in Fig. 7 as can be seen at the 220 nm diameter PSL (shown at a size parameter of nearly 3).

The extinction efficiency for various size PSLs at a wavelength of 335 nm is shown in Fig. 8. Experimental measurements at this wavelength deviate from theory in Fig. 6 and for other sizes studied; as such, the experimental and theoretical extinction efficiencies at $\lambda = 335$ nm were not expected to coincide. The disagreement is clear in Fig. 8, with strongest variability at size parameters greater than 2.5. Careful comparison of the m values used for both extinction efficiency cases, highlight that the imaginary portion of the CRI is nearly four times greater at 335 nm ($k = 0.197$) than 248 nm ($k = 0.059$) (French et al., 2007). The increase in the imaginary portion of the CRI leads to a smoothing of the interference structure indicative of an absorbing species. We would have expected the CRI to increase with decreasing wavelength, but French

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

UV wavelength regions. Valid CRI representations are available in other wavelength regions.

Several research groups are currently using the CRI as a floating parameter and fitting Mie theory calculations to experimental results (Abo Riziq et al., 2007; Dinar et al., 2008; Erlick et al., 2011; Flores et al., 2009; Freedman et al., 2009; Kim et al., 2010; Lack et al., 2006; Lang-Yona et al., 2009; Mack et al., 2010; Miles et al., 2010a, b; Spindler et al., 2007). This is shown to be successful even when the absorption parameter is not reported in conjunction with the extinction (or scattering) parameter (Lack et al., 2006; Mack et al., 2010). Our retrieved CRI are similar to those derived from the literature. At a wavelength of 248 nm, the retrieved CRI including its error is equivalent to the French et al. (2007) data and little difference is observed in the Mie theory results in Fig. 7. For $\lambda = 335$ nm, the retrieved CRI captures the interference and ripple features of the spectrum by improving agreement near a size parameter of 5.5, while not significantly decreasing agreement at other size parameters as seen in Fig. 8. Overall the retrieved CRI results are similar to those from the literature (French et al., 2007; Ma et al., 2003).

In conclusion, we have displayed the capabilities of a new instrument for monitoring aerosol extinction. The AE-DOAS is shown to be accurate and sensitive through experiments of gas phase species and polystyrene latex spheres. Further, this work clearly displays the importance of having correct CRI values at all wavelengths. Figure 6 demonstrates the variability between our results and the three different literature motivated models. Here, the three similar models emphasize that small changes in the overall value of the CRI can lead to changes in shape and intensity in the extinction cross section spectrum as a function of wavelength. Further, the effect of modest changes in the imaginary portion of the CRI at UV wavelengths as modeled in Fig. 8 can have a significant impact on the representation of extinction efficiency. The CRI of aerosol components is used as an input for climate models and it is important to consider the wavelength dependence of the values used. The importance of the UV wavelengths is due to rapid intensity changes in solar irradiance and new classification

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



of aerosols such as BrC and yellow carbon that have changing CRI in this wavelength region. As a result, any uncertainties in the wavelength dependent CRI may be magnified in climate models.

In future work, we will perform a detailed analysis of our data for PSL through a minimization routine to determine the complex RI from extinction efficiency representations at additional wavelengths, especially in the UV range where little data currently exists. We will also be studying a variety of samples in the laboratory and preparing the AE-DOAS for ambient measurements.

Acknowledgements. We gratefully acknowledge the contribution of J. Michael Flores to this work as he supplied the user friendly interface for retrieving refractive indices. We wish to thank Roger H. French for providing us with the numerical values used to generate the figures in his 2007 paper. This work was funded by the University of New Hampshire, College of Engineering and Physical Sciences. RTC acknowledges funding from the UNH Chemistry Department and Graduate School. MEG completed much of the writing of this manuscript during the 2010 GAIN writing retreat funded by ADVANCE Grant, NSF-0620101 and ADVANCE Grant, NSF-0620087.

References

- Abo Riziq, A., Erlick, C., Dinar, E., and Rudich, Y.: Optical properties of absorbing and non-absorbing aerosols retrieved by cavity ring down (CRD) spectroscopy, *Atmos. Chem. Phys.*, 7, 1523–1536, doi:10.5194/acp-7-1523-2007, 2007.
- AIRMAP: <http://airmap.unh.edu/>, last access: 29 September 2011.
- Andreae, M. O. and Gelencsér, A.: Black carbon or brown carbon? The nature of light-absorbing carbonaceous aerosols, *Atmos. Chem. Phys.*, 6, 3131–3148, doi:10.5194/acp-6-3131-2006, 2006.
- Andreae, M. O., Schmid, O., Yang, H., Chand, D., Yu, J. Z., Zeng, L. M., and Zhang, Y. H.: Optical properties and chemical composition of the atmospheric aerosol in urban Guangzhou, China, *Atmos. Environ.*, 42, 6335–6350, 2008.
- Ångström, A.: On the atmospheric transmission of sun radiation and on dust in the air, *Geografiska Ann. A.*, 11, 156–166, 1929.

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



- Ångström, A.: On the atmospheric transmission of sun radiaton. II., *Geografiska Ann. A.*, 12, 130–159, 1930.
- Bates, T. S., Anderson, T. L., Baynard, T., Bond, T., Boucher, O., Carmichael, G., Clarke, A., Erlick, C., Guo, H., Horowitz, L., Howell, S., Kulkarni, S., Maring, H., McComiskey, A., Middlebrook, A., Noone, K., O'Dowd, C. D., Ogren, J., Penner, J., Quinn, P. K., Ravishankara, A. R., Savoie, D. L., Schwartz, S. E., Shinozuka, Y., Tang, Y., Weber, R. J., and Wu, Y.: Aerosol direct radiative effects over the northwest Atlantic, northwest Pacific, and North Indian Oceans: estimates based on in-situ chemical and optical measurements and chemical transport modeling, *Atmos. Chem. Phys.*, 6, 1657–1732, doi:10.5194/acp-6-1657-2006, 2006.
- Baynard, T., Lovejoy, E. R., Pettersson, A., Brown, S. S., Lack, D., Osthoff, H., Massoli, P., Ciciora, S., Dube, W. P., and Ravishankara, A. R.: Design and application of a pulsed cavity ring-down aerosol extinction spectrometer for field measurements, *Aerosol Sci. Technol.*, 41, 447–462, 2007.
- Bergstrom, R. W., Russell, P. B., and Hignett, P.: Wavelength dependence of the absorption of black carbon particles: Predictions and results from the TARFOX experiment and implications for the aerosol single scattering albedo, *J. Atmos. Sci.*, 59, 567–577, 2002.
- Bogumil, K., Orphal, J., Homann, T., Voigt, S., Spietz, P., Fleischmann, O. C., Vogel, A., Hartmann, M., Kromminga, H., Bovensmann, H., Frerick, J., and Burrows, J. P.: Measurements of molecular absorption spectra with the SCIAMACHY pre-flight model: instrument characterization and reference data for atmospheric remote-sensing in the 230–2380 nm region, *J. Photoch. Photobio. A.*, 157, 167–184, 2003.
- Bohren, C. F. and Huffman, D. K.: *Absorption and Scattering of Light by Small Particles*, Wiley, New York, 1983.
- Bond Research Group: Aerosol characterization: Mie calculation: http://www.hiwater.org/Mie_calcs.html, last access: 29 September 2011.
- Bond, T. C.: Spectral dependence of visible light absorption by carbonaceous particles emitted from coal combustion, *Geophys. Res. Lett.*, 28, 4075–4078, 2001.
- Bond, T. C. and Bergstrom, R. W.: Light absorption by carbonaceous particles: An investigative review, *Aerosol Sci. Technol.*, 40, 27–67, 2006.
- Bones, D. L., Henricksen, D. K., Mang, S. A., Gonsior, M., Bateman, A. P., Nguyen, T. B., Cooper, W. J., and Nizkorodov, S. A.: Appearance of strong absorbers and fluorophores in limonene-O₃ secondary organic aerosol due to NH₄⁺-mediated chemical aging over long time scales, *J. Geophys. Res.-Atmos.*, 115, D05203, doi:10.1029/2009JD012864, 2010.

**Initial investigation of
an aerosol extinction
spectrometer**R. T. Chartier and
M. E. Greenslade

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

properties retrieval and radiative forcing over northwestern China during the 2008 China-US joint field experiment, *J. Geophys. Res.-Atmos.*, 115, D00K12, doi:10.1029/2009JD013263, 2010.

5 Hecobian, A., Zhang, X., Zheng, M., Frank, N., Edgerton, E. S., and Weber, R. J.: Water-Soluble Organic Aerosol material and the light-absorption characteristics of aqueous extracts measured over the Southeastern United States, *Atmos. Chem. Phys.*, 10, 5965–5977, doi:10.5194/acp-10-5965-2010, 2010.

Hoffer, A., Gelencsér, A., Guyon, P., Kiss, G., Schmid, O., Frank, G. P., Artaxo, P., and Andreae, M. O.: Optical properties of humic-like substances (HULIS) in biomass-burning aerosols, *Atmos. Chem. Phys.*, 6, 3563–3570, doi:10.5194/acp-6-3563-2006, 2006.

10 Hönninger, G., von Friedeburg, C., and Platt, U.: Multi axis differential optical absorption spectroscopy (MAX-DOAS), *Atmos. Chem. Phys.*, 4, 231–254, doi:10.5194/acp-4-231-2004, 2004.

IPCC: Climate Change 2007: The Physical Science Basis. Contribution of Working Group I to the Fourth Assessment Report of the Intergovernmental Panel on Climate Change, edited by: Solomon, S., D. Qin, M. Manning, Z. Chen, M. Marquis, K.B. Averyt, M. Tignor and H.L. Miller, Cambridge University Press, Cambridge, UK and New York, US, 996, 2007.

15 Kanakidou, M., Seinfeld, J. H., Pandis, S. N., Barnes, I., Dentener, F. J., Facchini, M. C., Van Dingenen, R., Ervens, B., Nenes, A., Nielsen, C. J., Swietlicki, E., Putaud, J. P., Balkanski, Y., Fuzzi, S., Horth, J., Moortgat, G. K., Winterhalter, R., Myhre, C. E. L., Tsigaridis, K., Vignati, E., Stephanou, E. G., and Wilson, J.: Organic aerosol and global climate modelling: a review, *Atmos. Chem. Phys.*, 5, 1053–1123, doi:10.5194/acp-5-1053-2005, 2005.

20 Kim, H., Barkey, B., and Paulson, S. E.: Real refractive indices of alpha- and beta-pinene and toluene secondary organic aerosols generated from ozonolysis and photo-oxidation, *J. Geophys. Res.-Atmos.*, 115, D24212, doi:10.1029/2010JD014549, 2010.

25 Kirchstetter, T. W., Novakov, T., and Hobbs, P. V.: Evidence that the spectral dependence of light absorption by aerosols is affected by organic carbon, *J. Geophys. Res.-Atmos.*, 109, D21208, doi:10.1029/2004JD004999, 2004.

Lack, D. A., Lovejoy, E. R., Baynard, T., Pettersson, A., and Ravishankara, A. R.: Aerosol absorption measurement using photoacoustic spectroscopy: Sensitivity, calibration, and uncertainty developments, *Aerosol Sci. Technol.*, 40, 697–708, 2006.

30 Lang-Yona, M., Rudich, Y., Segre, E., Dinar, E., and Abo-Riziq, A.: Complex Refractive Indices of Aerosols Retrieved by Continuous Wave-Cavity Ring Down Aerosol Spectrometer, *Anal.*

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Chem., 81, 1762–1769, 2009.

Lang-Yona, N., Abo-Riziq, A., Erlick, C., Segre, E., Trainic, M., and Rudich, Y.: Interaction of internally mixed aerosols with light, *Phys. Chem. Chem. Phys.*, 12, 21–31, 2010.

Liu, B. Y. H., Romay, F. J., Dick, W. D., Woo, K. S., and Chiruta, M.: A Wide-Range Particle Spectrometer for Aerosol Measurement from 0.010 μm to 10 μm , *Aerosol Air Qual. Res.*, 10, 125–139, 2010.

Ma, X. Y., Lu, J. Q., Brock, R. S., Jacobs, K. M., Yang, P., and Hu, X. H.: Determination of complex refractive index of polystyrene microspheres from 370 to 1610 nm, *Phys. Med. Biol.*, 48, 4165–4172, 2003.

Mack, L. A., Levin, E. J. T., Kreidenweis, S. M., Obrist, D., Moosmüller, H., Lewis, K. A., Arnott, W. P., McMeeking, G. R., Sullivan, A. P., Wold, C. E., Hao, W.-M., Collett Jr., J. L., and Malm, W. C.: Optical closure experiments for biomass smoke aerosols, *Atmos. Chem. Phys.*, 10, 9017–9026, doi:10.5194/acp-10-9017-2010, 2010.

Marley, N. A., Gaffney, J. S., Tackett, M., Sturchio, N. C., Heraty, L., Martinez, N., Hardy, K. D., Marchany-Rivera, A., Guilderson, T., MacMillan, A., and Steelman, K.: The impact of biogenic carbon sources on aerosol absorption in Mexico City, *Atmos. Chem. Phys.*, 9, 1537–1549, doi:10.5194/acp-9-1537-2009, 2009.

Massoli, P., Kebejian, P. L., Onasch, T. B., Hills, F. B., and Freedman, A.: Aerosol Light Extinction Measurements by Cavity Attenuated Phase Shift (CAPS) Spectroscopy: Laboratory Validation and Field Deployment of a Compact Aerosol Particle Extinction Monitor, *Aerosol Sci. Technol.*, 44, 428–435, 2010.

Massoli, P., Bates, T. S., Quinn, P. K., Lack, D. A., Baynard, T., Lerner, B. M., Tucker, S. C., Brioude, J., Stohl, A., and Williams, E. J.: Aerosol optical and hygroscopic properties during TexAQS-GoMACCS 2006 and their impact on aerosol direct radiative forcing, *J. Geophys. Res.-Atmos.*, 114, D00F07, doi:10.1029/2008JD011604, 2009.

Mätzler, C.: MATLAB Functions for Mie Scattering and Absorption – Version 2. Research Report (No. 2002-11), Institut für Angewandte Physik, 2002.

Mellon, D., King, S. J., Kim, J., Reid, J. P., and Orr-Ewing, A. J.: Measurements of Extinction by Aerosol Particles in the Near-Infrared Using Continuous Wave Cavity Ring-Down Spectroscopy, *J. Phys. Chem. A*, 115, 774–783, 2011.

Meyrahn, H., Pauly, J., Schneider, W., and Warneck, P.: Quantum Yields for the Photodissociation of Acetone in Air and an Estimate for the Life Time of Acetone in the Lower Troposphere, *J. Atmos. Chem.*, 4, 277–291, 1986.

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



- Miles, R. E. H., Rudic, S., Orr-Ewing, A. J., and Reid, J. P.: Influence of Uncertainties in the Diameter and Refractive Index of Calibration Polystyrene Beads on the Retrieval of Aerosol Optical Properties Using Cavity Ring Down Spectroscopy, *J. Phys. Chem. A*, 114, 7077–7084, 2010a.
- 5 Miles, R. E. H., Rudic, S., Orr-Ewing, A. J., and Reid, J. P.: Measurements of the wavelength dependent extinction of aerosols by cavity ring down spectroscopy, *Phys. Chem. Chem. Phys.*, 12, 3914–3920, 2010b.
- Moffet, R. C. and Prather, K. A.: In-situ measurements of the mixing state and optical properties of soot with implications for radiative forcing estimates, *P. Natl. Acad. Sci. USA*, 106, 11872–11877, 2009.
- 10 Mogili, P. K., Yang, K. H., Young, M. A., Kleiber, P. D., and Grassian, V. H.: Environmental aerosol chamber studies of extinction spectra of mineral dust aerosol components: Broadband IR-UV extinction spectra, *J. Geophys. Res.-Atmos.*, 112, D21204, doi:10.1029/2007JD008890, 2007.
- 15 Moosmuller, H., Varma, R., and Arnott, W. P.: Cavity ring-down and cavity-enhanced detection techniques for the measurement of aerosol extinction, *Aerosol Sci. Technol.*, 39, 30–39, 2005.
- Moosmüller, H., Chakrabarty, R. K., Ehlers, K. M., and Arnott, W. P.: Absorption Ångström coefficient, brown carbon, and aerosols: basic concepts, bulk matter, and spherical particles, *Atmos. Chem. Phys.*, 11, 1217–1225, doi:10.5194/acp-11-1217-2011, 2011.
- 20 Nikolov, I. D. and Ivanov, C. D.: Optical plastic refractive measurements in the visible and the near-infrared regions, *Appl. Optics*, 39, 2067–2070, 2000.
- Pettersson, A., Lovejoy, E. R., Brock, C. A., Brown, S. S., and Ravishankara, A. R.: Measurement of aerosol optical extinction at 532 nm with pulsed cavity ring down spectroscopy, *J. Aerosol Sci.*, 35, 995–1011, 2004.
- 25 Platt, U. and Stutz, J.: *Differential Optical Absorption Spectroscopy: Principles and Applications*, Springer, New York, 2008.
- Schnaiter, M., Horvath, H., Mohler, O., Naumann, K. H., Saathoff, H., and Schock, O. W.: UV-VIS-NIR spectral optical properties of soot and soot-containing aerosols, *J. Aerosol Sci.*, 34, 1421–1444, 2003.
- 30 Schnaiter, M., Schmid, O., Petzold, A., Fritzsche, L., Klein, K. F., Andreae, M. O., Helas, G., Thielmann, A., Gimmler, M., Mohler, O., Linke, C., and Schurath, U.: Measurement of wavelength-resolved light absorption by aerosols utilizing a UV-VIS extinction cell, *Aerosol*

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

Sci. Technol., 39, 249–260, 2005.

Si, F. Q., Xie, P. H., Dou, K., Zhan, K., Liu, Y., Xu, J., and Liu, W. Q.: Determination of the atmospheric aerosol optical density by multi axis differential optical absorption spectroscopy, *Acta Phys. Sin.-Ch Ed.*, 59, 2867–2872, 2010.

5 Smith, J. D. and Atkinson, D. B.: A portable pulsed cavity ring-down transmissometer for measurement of the optical extinction of the atmospheric aerosol, *Analyst*, 126, 1216–1220, 2001.

Spindler, C., Riziq, A. A., and Rudich, Y.: Retrieval of aerosol complex refractive index by combining cavity ring down aerosol spectrometer measurements with full size distribution information, *Aerosol Sci. Technol.*, 41, 1011–1017, 2007.

10 Strawa, A. W., Castaneda, R., Owano, T., Baer, D. S., and Paldus, B. A.: The measurement of aerosol optical properties using continuous wave cavity ring-down techniques, *J. Atmos. Ocean. Tech.*, 20, 454–465, 2003.

15 Strawa, A. W., Elleman, R., Hallar, A. G., Covert, D., Ricci, K., Provencal, R., Owano, T. W., Jonsson, H. H., Schmid, B., Luu, A. P., Bokarius, K., and Andrews, E.: Comparison of in situ aerosol extinction and scattering coefficient measurements made during the Aerosol Intensive Operating Period, *J. Geophys. Res.*, 111, D05S03, doi:10.1029/2005JD006056, 2006.

20 Takashima, H., Irie, H., Kanaya, Y., Shimizu, A., Aoki, K., and Akimoto, H.: Atmospheric aerosol variations at Okinawa Island in Japan observed by MAX-DOAS using a new cloud-screening method, *J. Geophys. Res.-Atmos.*, 114, D18213, doi:10.1029/2009JD011939, 2009.

Thermo Fisher Scientific: http://www.thermo.fr/eThermo/CMA/PDFs/Various/File_3936.pdf, last access: 29 September 2011.

25 Thermo Fisher Scientific: <http://www.thermoscientific.com/wps/portal/ts/products/detail?navigationId=L10397\&categoryId=87439\&productId=11962886>, last access: 29 September 2011.

Virkkula, A., Ahlquist, N. C., Covert, D. S., Sheridan, P. J., Arnott, W. P., and Ogren, J. A.: A three-wavelength optical extinction cell for measuring aerosol light extinction and its application to determining light absorption coefficient, *Aerosol Sci. Technol.*, 39, 52–67, 2005.

30 Voigt, S., Orphal, J., Bogumil, K., and Burrows, J. P.: The temperature dependence (203–293 K) of the absorption cross sections of O₃ in the 230–850 nm region measured by Fourier-transform spectroscopy, *J. Photoch. Photobio. A*, 143, 1–9, 2001.

White, J. U.: Long optical paths of large aperture, *J. Opt. Soc. Am.*, 32, 285–288, 1942.

Yang, M., Howell, S. G., Zhuang, J., and Huebert, B. J.: Attribution of aerosol light absorption to black carbon, brown carbon, and dust in China – interpretations of atmospheric measurements during EAST-AIRE, *Atmos. Chem. Phys.*, 9, 2035–2050, doi:10.5194/acp-9-2035-2009, 2009.

**Initial investigation of
an aerosol extinction
spectrometer**

R. T. Chartier and
M. E. Greenslade

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

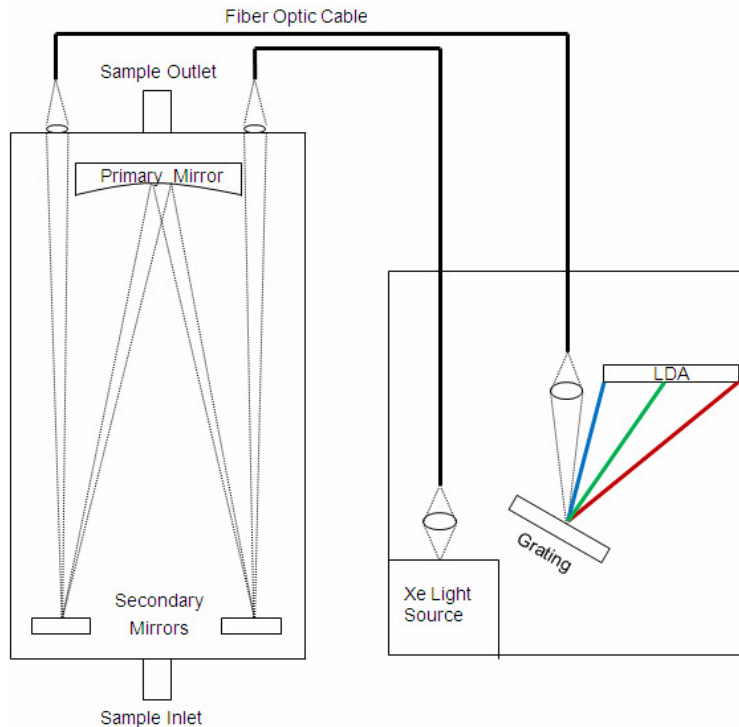


Fig. 1. A schematic of the benchtop AE-DOAS system. Light from the xenon lamp in the rack mountable spectrometer (shown on the right) is focused onto a fiber optic cable for transfer into the multi-pass gas cell (shown on the left). After a number of passes in the gas cell, the reflected light is focused onto a second fiber optic cable and detected by the spectrometer. The spectrometer consists of a grating and a 3078 element linear diode array. The typical gas cell path length is 19.51 m, unless otherwise noted.

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and M. E. Greenslade

Title Page

Abstract Introduction

Conclusions References

Tables Figures

⏪ ⏩


⏴ ⏵

Back Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



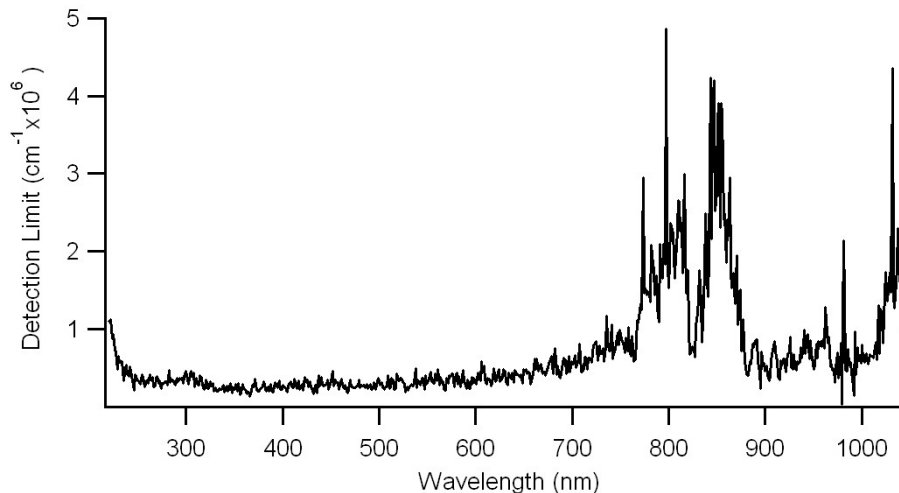
**Initial investigation of
an aerosol extinction
spectrometer**R. T. Chartier and
M. E. Greenslade

Fig. 2. The AE-DOAS detection limit is shown as a function of wavelength. This data is smoothed by averaging over five recorded wavelength values. It is clear that the detection limit is steady over the center of the solar spectrum from 235–700 nm. At wavelengths outside this range, the detection limit increases due to low lamp intensity.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

**Initial investigation of
an aerosol extinction
spectrometer**R. T. Chartier and
M. E. Greenslade

Fig. 3. A flow diagram of experimental setup used to measure the optical properties of a monodisperse PSL sample with the AE-DOAS. A = atomizer, DD = diffusion dryer, DMA = differential mobility analyzer, AE-DOAS = aerosol extinction differential optical absorption spectrometer, which is shown in detail in Fig. 1, and CPC = condensation particle counter. Additional instrument details are given in the experimental section.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

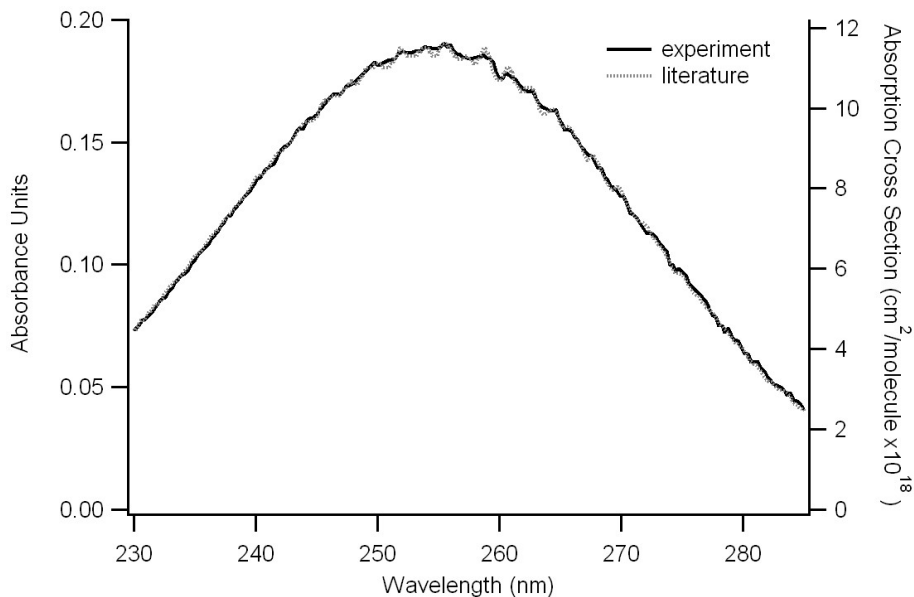


Fig. 4. The UV absorption spectrum of the Hartley band of ozone measured with an AE-DOAS path length of 9.75 m is shown as a solid black line. This is compared to the dotted grey line showing the absorption cross section spectrum of ozone (shown on the right y-axis) (Bogumil et al., 2003). A wavelength adjustment equivalent to adding one nanometer to the experimental spectrum is required to match the fine spectral structure seen in the literature spectrum.

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

Title Page

Abstract Introduction

Conclusions References

Tables Figures

⏪ ⏩

◀ ▶

Back Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

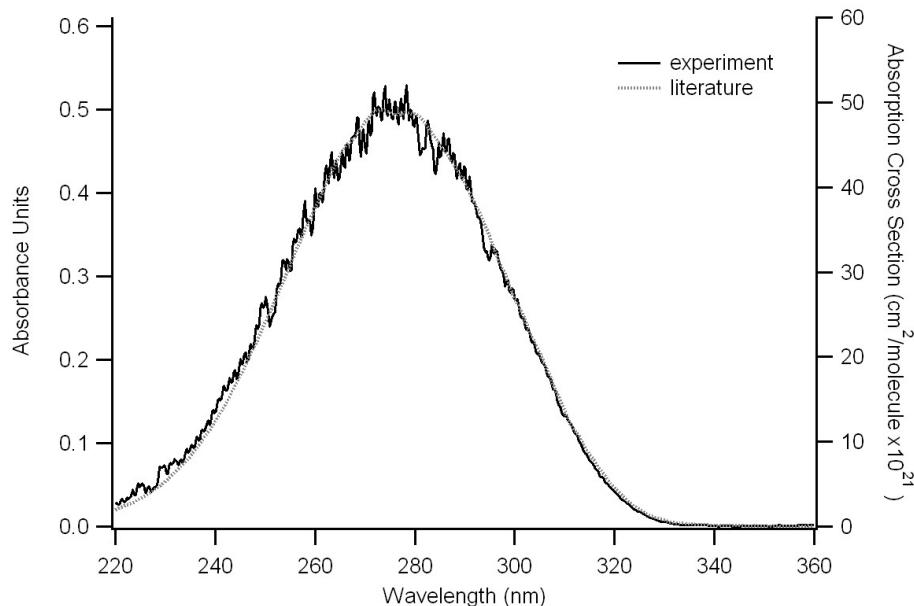


Fig. 5. The UV absorption spectrum obtained with the AE-DOAS of acetone with a 5-point boxcar average is shown as a solid black line. This is compared with the dotted grey line showing the absorption cross section spectrum of gas phase acetone (shown on the right y-axis) (Meyrahn et al., 1986).

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

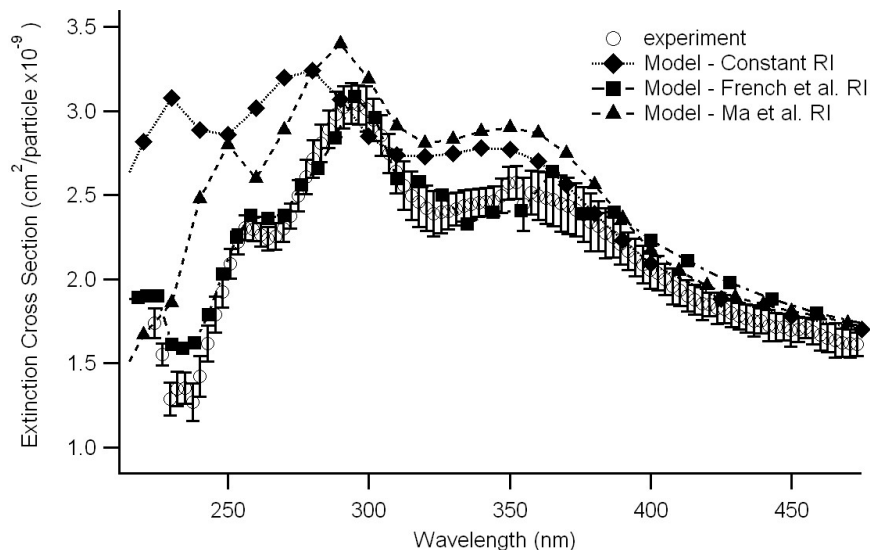


Fig. 6. The extinction cross section spectrum measured by the AE-DOAS for 300 nm PSL is shown as open circles. The experimental error bars represent 1σ of the mean. Mie theory calculations are performed with various values for the RI. The result based on the constant manufacturer's reported RI is shown as solid diamonds, the RI derived from Ma et al. (2003) based on the Cauchy coefficients is shown as solid diamonds and French et al.'s (2007) experimentally determined CRI is solid squares. The calculations show improved convergence at wavelengths greater than 475 nm and are therefore not shown.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

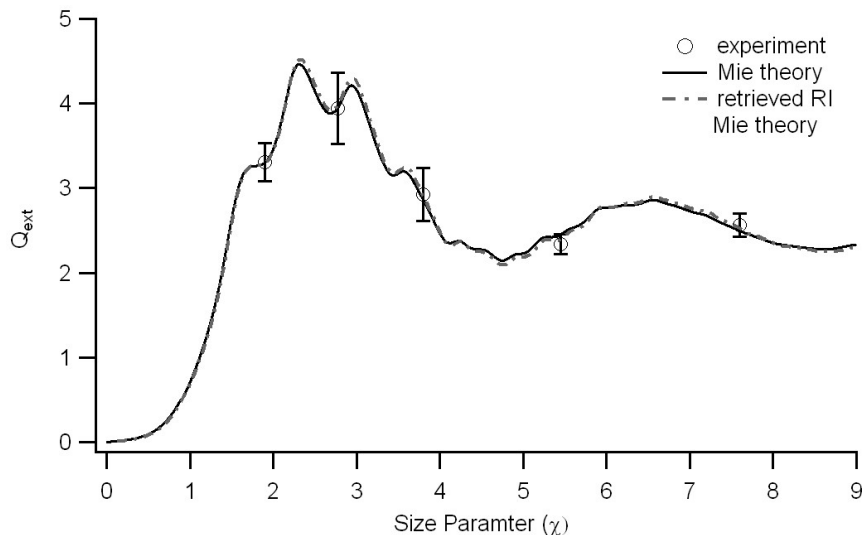


Fig. 7. The experimentally measured Q_{ext} versus size parameter for PSL at a wavelength of 248 nm are shown as open circles. The black line is the Mie theory calculation performed with a CRI from French et al. (2007) ($m = 1.826 + 0.059i$ at $\lambda = 248$ nm). The grey dot-dash line is the Mie theory calculation for the CRI retrieved from the experimental data ($m = 1.82 + 0.05i$). The experimental extinction efficiency is reported for PSL diameters of 150 nm, 220 nm, 300 nm, 430 nm, and 600 nm (from left to right) and the reported error bars are 1σ for repeat measurements.

[Title Page](#)
[Abstract](#)
[Introduction](#)
[Conclusions](#)
[References](#)
[Tables](#)
[Figures](#)
[⏪](#)
[⏩](#)
[◀](#)
[▶](#)
[Back](#)
[Close](#)
[Full Screen / Esc](#)
[Printer-friendly Version](#)
[Interactive Discussion](#)

Initial investigation of an aerosol extinction spectrometer

R. T. Chartier and
M. E. Greenslade

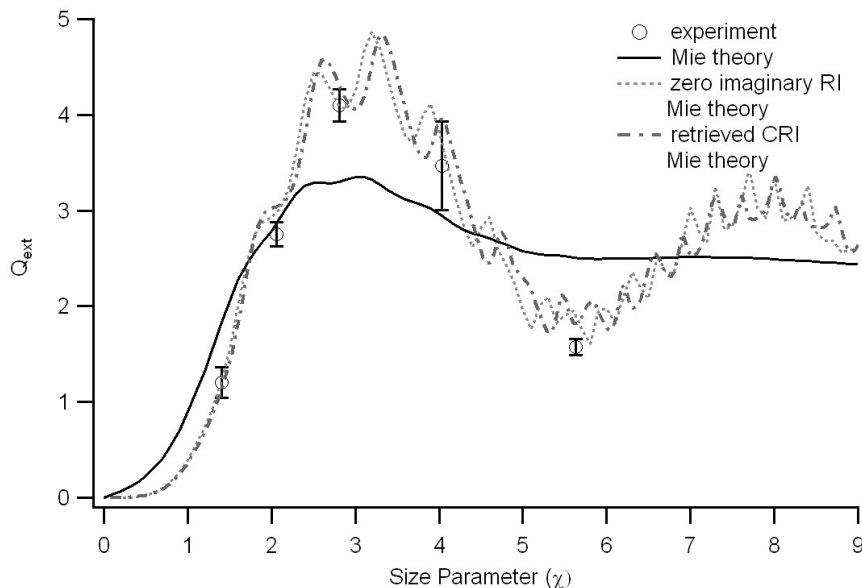


Fig. 8. At a wavelength of 335 nm, the Q_{ext} measured by the AE-DOAS (open circles) does not match the Q_{ext} predicted by Mie theory generated with the French et al. (2007) CRI ($m = 1.686 + 0.197i$) shown as the black line. The Mie theory generated when the imaginary portion of this CRI is reduced to zero is shown in the light gray dotted line. The grey dot-dash line is the Mie theory calculation for the CRI retrieved from the experimental data ($m = 1.72 + 0.005i$). Errors bars are 1σ on repeat experimental measurements.

[Title Page](#)
[Abstract](#)
[Introduction](#)
[Conclusions](#)
[References](#)
[Tables](#)
[Figures](#)
[◀](#)
[▶](#)
[◀](#)
[▶](#)
[Back](#)
[Close](#)
[Full Screen / Esc](#)
[Printer-friendly Version](#)
[Interactive Discussion](#)