

Received: 3 October 2011 – Accepted: 18 October 2011 – Published: 24 October 2011

Correspondence to: Z. Mariani (zmariani@atmosph.physics.utoronto.ca)

Published by Copernicus Publications on behalf of the European Geosciences Union.

AMTD

4, 6411–6448, 2011

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Abstract

The Extended-range Atmospheric Emitted Radiance Interferometer (E-AERI) is a moderate resolution (1 cm^{-1}) Fourier transform infrared spectrometer for measuring the absolute downwelling infrared spectral radiance from the atmosphere between 400 and 3000 cm^{-1} . The extended spectral range of the instrument permits monitoring of the 400–550 cm^{-1} (20–25 μm) region, where most of the infrared surface cooling currently occurs in the dry air of the Arctic. Spectra from the E-AERI have the potential to provide information about radiative balance, trace gases, and cloud properties in the Canadian high Arctic. Calibration, performance evaluation, and certification of the E-AERI were performed at the University of Wisconsin Space Science and Engineering Centre from September to October 2008. The instrument was then installed at the Polar Environment Atmospheric Research Laboratory (PEARL) Ridge Lab at Eureka, Nunavut, in October 2008, where it acquired one year of data. Measurements are taken every seven minutes year-round, including polar night when the solar-viewing spectrometers at PEARL are not operated. A similar instrument, the University of Idaho's Polar AERI (P-AERI), was installed at the Zero-altitude PEARL Auxiliary Laboratory (OPAL) from March 2006 to June 2009. During the period of overlap, these two instruments provided calibrated radiance measurements from two altitudes. A fast line-by-line radiative transfer model is used to simulate the downwelling radiance at both altitudes; the largest differences (simulation-measurement) occur in spectral regions strongly influenced by atmospheric temperature and/or water vapour. The presence of two AERI instruments at close proximity but two different altitudes allowed for an investigation of the surface radiative forcing by a thin, low ice cloud; the ice cloud resulted in a 6% increase in irradiance. The presence of clouds creates a large surface radiative forcing in the Arctic, particularly in the $750\text{--}1200\text{ cm}^{-1}$ region where the downwelling radiance is several times greater than clear-sky radiances, which is significantly larger than in other more humid regions.

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



1 Introduction

The Canadian Network for the Detection of Atmospheric Change (CANDAC) has equipped the Polar Atmospheric Environment Research Laboratory (PEARL) at Eureka, Nunavut (80° N, 86° W) for measurements during International Polar Year (IPY, project 196) and beyond. One of the instruments at PEARL is the Extended-range Atmospheric Emitted Radiance Interferometer (the E-AERI). This instrument measures the absolute downwelling infrared radiation spectrum for studies of the Arctic radiation budget and atmospheric composition. The E-AERI was installed in October 2008 and acquired one full year of measurements at the PEARL Ridge Lab.

AERI instruments were developed at the University of Wisconsin Space Science and Engineering Centre (UW-SSEC) from 1989 to 1998 using an MR100 spectroradiometer developed from an MB-120 interferometer designed for industrial applications by ABB Bomem Inc. of Quebec, Canada (Collard et al., 1995). A suite of AERI instruments was then developed for the Atmospheric Radiation Measurement (ARM) (DOE, 1990) Climate Research Facility sites in the Southern Great Plains (Oklahoma), the North Slope of Alaska, and the Tropical Western Pacific (Stokes and Schwartz, 1994; Knuteson et al., 2004a). In addition to the downwelling radiance measurements, measurements of the atmospheric state (e.g. radiosonde profiles) are made at these sites allowing for radiance simulations (Ellingson and Wiscombe, 1996). These AERI systems have collected over a decade of data at the ARM sites and have been used to generate climatologies in downwelling infrared radiance (Turner and Gero, 2011) and to investigate long-term trends (Gero and Turner, 2011). In addition to the ARM AERIs, other AERI instruments include the Marine AERI (M-AERI) (Minnett, 2001), the University of Denver's high-resolution AERI-X deployed at the PEARL Ridge Lab from 1994–2002 (Olson et al., 1996), and the University of Idaho's Polar AERI (P-AERI) (Walden et al., 2005; Rowe et al., 2008).

The newest generation AERI (e.g. the E-AERI installed at PEARL) was developed by ABB under commercial license from UW-SSEC. These AERIs incorporate the newest

AMTD

4, 6411–6448, 2011

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

Infrared emission measurements in the Arctic using a new extended-range AERIZ. Mariani et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

generation of ABB Bomem's Fourier Transform Infrared (FTIR) spectroradiometer, a UW blackbody cavity, the latest signal conditioning units, and a new detector/Stirling cooler with an extended lifetime. The new AERI configuration allows in-field replacement of the Stirling cooler and metrology laser. The software has been updated with a combination of ABB software for data acquisition and the instrument communication/control interface and UW software for post-processing and atmospheric science functions to ease future evolution of hardware and science functions by each party. The new AERIs also include front-end and back-end enclosures that protect against atmospheric precipitation and temperature variation, respectively. In addition to these modifications, the E-AERI extends the spectral coverage range of a standard AERI (550–3000 cm⁻¹) to 400–3000 cm⁻¹.

The thermal emitted radiance measured by the E-AERI is primarily dependent on the water vapour content and temperature of the atmosphere in cloud-free scenes. Therefore, temperature and humidity profiles of the planetary boundary layer can be retrieved from AERI and E-AERI spectra, as demonstrated in Feltz et al. (1998), Smith et al. (1999), and Turner et al. (2000). This allows for high-temporal-resolution records and analyses of temperature and water vapour changes due to mesoscale meteorological features. The sampling interval of approximately seven minutes allows the study of short-term meteorological phenomena in the lower atmosphere, e.g. inversion developments, cloud effects, and front passages.

The spectral range of the E-AERI covers the so-called “dirty window” (around 400 cm⁻¹, or 20 μm), where most of the infrared cooling currently occurs in the dry air of the Arctic. The importance of the far infra-red (IR) for mid-to-upper tropospheric cooling has been well demonstrated in Clough et al. (1992). Due to climate change, the water vapour content of the Arctic atmosphere is expected to increase, with a corresponding change in downwelling radiance. Such a regime shift should be visible in the E-AERI data record. In addition, the far IR is important for cloud thermodynamic phase determination, as demonstrated by Rathke et al. (2002). A previous extended-range version of the AERI system was deployed at the Surface Heat Budget of the Arctic

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Ocean Ice Station in 1997; this AERI was used to investigate the far infrared H₂O continuum (Tobin, 1999) and to characterize the phase and microphysical properties of mixed phase Arctic boundary layer clouds (Turner, 2005).

Retrievals of total columns of various trace gases (e.g. CH₄, CO, CO₂, O₃, N₂O) using a prototype version of the retrieval algorithm SFIT2 (Pougatchev et al., 1995; Rinsland et al., 1998) modified to analyze emission features are currently being evaluated. Recently, retrievals of CO with high sensitivity to the lower troposphere have been demonstrated for the AERI systems (Yurganov et al., 2010). In contrast to solar absorption measurements of atmospheric trace gases, which depend on sunlit clear-sky conditions, the use of emission spectra allows measurements year-round (except during precipitation events or when clouds are present). This capability allows the E-AERI to provide temporal coverage throughout the four months of polar night, when the PEARL Bruker 125HR solar absorption FTIR spectrometer is not operated (Batchelor et al., 2009).

The installation of the E-AERI at PEARL was preceded by the P-AERI, which was deployed at the Zero-altitude PEARL Auxiliary Laboratory (OPAL) from March 2006 to June 2009. The two instruments are similar, but the P-AERI does not provide spectral coverage below 550 cm⁻¹. In addition, the E-AERI was housed in the PEARL Ridge lab at an altitude of 610 m, while the P-AERI was operated 15 km away at an altitude of 10 m. Having two AERI instruments close in proximity at these altitudes presents an opportunity for investigation of the lowest 600 m of atmosphere, potentially including differences in trace gases, aerosols, and low-level liquid and ice clouds. Other instrumentation at OPAL that provides information for cloud studies includes the Millimeter Wave Cloud Radar (MMCR), which measures equivalent radar reflectivity, Doppler velocity, spectral width, and Doppler spectra over 2-s intervals, and UW's Arctic High Spectral Resolution Lidar (AHSRL), which measures aerosol backscatter cross section and particulate circular depolarization ratio (Eloranta, 2005). These can be used to determine cloud heights, thicknesses, composition, internal structure and vertical motions with high vertical and temporal resolution.

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



HB, AB, and then Sky View (SV) in the following order: HB AB SV SV SV SV SV SV SV SV SV AB HB. This is useful for quick measurements of the sky to detect changes in frontal passages. The E-AERI is usually operated in slow sampling mode, following the pattern: HB AB SV AB HB. This method sandwiches each SV measurement between blackbody measurements, improving the calibration of the spectra. The instrument performs two Michelson mirror sweeps (forward and backward) for each spectrum. Co-adding spectra for the blackbodies takes about two minutes, and for the sky view it takes about three minutes, such that 127 co-adds are performed for each blackbody measurement and 248 co-adds are performed for each SV measurement.

2.3 Instrument enclosure

A temperature control unit maintains of the back-end enclosure at a constant temperature, this contains all electronics and the FTS, and can operate between -30°C and $+40^{\circ}\text{C}$. The front-end enclosure protects against precipitation (both rain and snow) but is not stabilized in temperature; it is free running near the ambient temperature. It is detachable to enable it to be sealed to the external side of a wall, as is done at PEARL. A hatch, actuated by precipitation sensors or directly by the user or instrument commanding script, can be closed to protect the optical head, or opened to look at the atmosphere. Two Vaisala DRD11A precipitation sensors (one elevated and one flush with the enclosure) detect any precipitation occurring. In the presence of precipitation, the system will automatically close the hatch and turn itself off in a self-protection mode that does not allow sky measurement. After the precipitation ends, the system returns to normal acquisition mode. Rearranging the placement of the sensors may be required since they failed to detect falling snow several times during the first year of measurements. Temperature, pressure, relative humidity, and sun sensors are also monitored in the enclosure to obtain knowledge of the measurement conditions.

2.4 Blackbodies

The two calibration blackbodies are of identical construction, each consisting of a thermally isolated cavity which is painted with a high-emissivity diffuse black paint. Each cavity contains a heater, a feedback thermistor and three thermistor sensors. In principle, each blackbody's temperature can be set using the instrument's software. For operation at PEARL, the HB is set at 310 K and the AB operates at the outside temperature.

The E-AERI calibration methodology uses a pair of HB/AB views bracketing the SV measurement. The blackbody temperatures are fit to a linear function of time to account for changes in the instrument temperature during a calibration sequence. Similarly, a linear interpolation to the SV time is performed for each HB and AB measurement. The approach used for radiometric calibration of the E-AERI system is based on that of Revercomb et al. (1988).

2.5 Data products

The standard E-AERI data product consists of calibrated downwelling radiance spectra from the two detectors: 400–1800 and 1800–3000 cm^{-1} . Combined, these form a continuous spectrum from 400–3000 cm^{-1} . Two data description files and one summary file contain measurement time, instrument parameter metrics, mean radiance, imaginary radiance, corrective offset, responsivity, brightness temperature (sometimes referred to as radiance temperature), blackbody temperature drift, and scene Noise Equivalent Spectral Radiance (NESR) from each detector for each seven-minute sampling interval. The radiance data are automatically processed using instrument-related corrections such as those described in Sect. 2.4 as well as in Knuteson et al. (2004b), resulting in calibrated radiances with a standardized spectral scale in real time.

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

2.6 System software architecture

The E-AERI software system performs all necessary data calibration in real-time. The software also performs a series of quality control checks in real-time and allows unattended operation of the system. The data is accessible via a digital network with an on-board storage capacity of several days. The monitoring Graphical User Interface (GUI) supports interactive use of the instrument and monitors the state of the instrument. Calibrated spectra and some auxiliary parameters are displayed at the end of each scan. Within each window of the monitoring GUI, the radiance, air temperature, Stirling cooler current, and instrument temperature are displayed. Thirty crucial instrument parameters are also monitored using the GUI. Table 2 lists the variables that are used as real-time quality metrics for the E-AERI. If one of these parameters falls outside of a tolerable range, the operators are alerted.

3 Instrument performance

3.1 Performance evaluations

Measurements of the NESR were performed in Quebec City (before shipping to Eureka) and again at Eureka. The root-mean-square of the variation in the calibrated radiances from 284 spectra of the HB determines the NESR. NESR measurements taken at Eureka are shown in Fig. 2. The observed increase in noise at 667 cm^{-1} and from $2300\text{--}2400\text{ cm}^{-1}$ is due to CO_2 absorption inside the instrument, which reduces responsivity. For both the long wavelength (LW; MCT) and short wavelength (SW; InSb) bands, the NESR is well below the specified requirement; about one-half and one-third of the specification for the LW and SW, respectively. One exception is in the region around 400 cm^{-1} ; due to the higher NESR at this edge of the LW band, a new detector will be installed in fall 2011.

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Title Page	
Abstract	Introduction
Conclusions	References
Tables	Figures
⏪	⏩
◀	▶
Back	Close
Full Screen / Esc	
Printer-friendly Version	
Interactive Discussion	

The E-AERI was sent to UW-SSEC for calibration and performance evaluation in September 2008. A four-body test was performed using the AB, HB (set to 330 K for these tests), an intermediate blackbody (temperature between AB and HB, around 318 K), and an Ice-Blackbody (IB) at 273 K. The intermediate body and IB are used as external reference sources to verify blackbody temperature knowledge. These external reference sources are calibrated using the same National Institute of Standards and Technology traceable approach as used for the other blackbodies. During the test period, the scene mirror views each blackbody to measure the blackbody temperatures over several hours to ensure stability and reduce the noise level.

Calibration verification test results are shown in Fig. 3 for the intermediate body and IB. Water vapour has strong absorption between 1450 and 1800 cm^{-1} and CO_2 has strong absorption around 667 and 2380 cm^{-1} , resulting in the observed discrepancies in these regions. The IB measurement has an offset of 0.2 K; this is comparable to the error of ± 0.2 K for other AERI systems (Knuteson et al., 2004a). This error can be due to incorrect placement of the ice-body (too far away or not exactly centred).

A side-by-side comparison with two UW AERI systems, the AERI-07 (with an extended-range detector) and the AERI-Bago (AERI-03), was performed. These instruments have been employed in numerous measurement campaigns and are considered reliable benchmarks for measurement inter-comparison purposes (Knuteson et al., 2004a). Results from these comparisons indicate that agreement between the E-AERI and the other two instruments is comparable to the agreement between the AERI-07 and AERI-Bago, as shown in Fig. 4, verifying the accuracy of the E-AERI radiances (UW-SSEC, 2008).

Three field-of-view tests were performed on the zenith-sky, HB, and AB views and confirmed proper optical alignment of the source and reference blackbody cavities. Wavenumber calibration was performed by finding an effective laser wavenumber value for the HeNe laser that provides the best spectral match for regions of regular spectral lines. The wavenumber knowledge was found to be 0.0018 cm^{-1} , which is better than the 0.01 cm^{-1} requirement. A spectral line stability test was performed by tracking any



movement in the 1918 cm^{-1} water line during the ambient blackbody measurements for twenty hours. The wavenumber stability also meets the requirement of $<10\text{ ppm}$.

3.2 Side-by-side comparisons with the P-AERI at sea-level

Prior to its installation at the PEARL Ridge Lab, the E-AERI was operated side-by-side with the P-AERI at OPAL for several days. The P-AERI has been extensively characterized (Walden et al., 2005; Rowe et al., 2008) and the data at Eureka have been quality controlled (Rowe et al., 2011a,b). With exception of the E-AERI's extended range ($400\text{--}550\text{ cm}^{-1}$), the P-AERI has similar specifications to the E-AERI and a measurement period that overlaps the E-AERI's, providing an opportunity for comparing the two instruments and evaluating the E-AERI spectra. Coincident E-AERI and P-AERI radiances recorded on 20 October 2008 are shown in Fig. 5 for the P-AERI spectral range of 500 to 3000 cm^{-1} . The radiances agree within $\pm 1\text{ mW}/(\text{m}^2\text{ sr cm}^{-1})$ for the MCT detector and $\pm 0.2\text{ mW}/(\text{m}^2\text{ sr cm}^{-1})$ for the InSb detector with the exception of the spectral regions: $1450\text{--}1800\text{ cm}^{-1}$ and $2300\text{--}2400\text{ cm}^{-1}$. Discrepancies between 1450 and 1800 cm^{-1} are due to humidity inside the E-AERI. After ten days in the dry Arctic air, the water vapour inside the E-AERI evaporated and such discrepancies ceased to exist. Discrepancies between 2300 and 2400 cm^{-1} are due to CO_2 absorption in the instrument, which reduces responsivity. These results are comparable to the AERI-07 and AERI-03 comparisons.

4 A first look at PEARL E-AERI spectra

4.1 Impact of clouds on the radiation budget

The ability of AERI systems to detect the presence of clouds and provide information about cloud properties has been well demonstrated (e.g. Collard et al., 1995; DeSlover et al., 1999; Shaw et al., 2005; Turner, 2005,). Figure 6a shows E-AERI measurements

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

made on 16 April 2009 at 00:08 UTC (Universal Time Coordinated) and 17:57 UTC. The MMCR indicates that on 16 April, early-morning clear skies were followed by a thick cloud layer above Eureka for the remainder of the afternoon and evening (Fig. 7). The top panel of Fig. 7 shows the measured equivalent radar reflectivity (dBZ), the middle panel shows the measured Doppler velocity (m s^{-1}), and the bottom panel shows the measured spectral width (m s^{-1}). This figure shows slowly descending cirrus clouds. The cloud is mostly ice until around 09:00 UTC; then the spectral width increases (as indicated by the appearance of green shading), which may be due to the presence of liquid water. The E-AERI radiance increases after 04:00 UTC in the $400\text{--}600\text{ cm}^{-1}$ and $750\text{--}1400\text{ cm}^{-1}$ regions due to emission by cloud particles, correlating with the MMCR's detection of a low-altitude, relatively thick ($\sim 2\text{ km}$) cirrus cloud that first appeared above Eureka at 04:00 UTC. Figure 6b displays the brightness temperature measured by the E-AERI throughout the day. Periods of increased brightness temperature correlate with increased cloud cover above Eureka. The averaged radiance over $750\text{--}1200\text{ cm}^{-1}$ increases from 4.4 to $21.6\text{ mW}/(\text{m}^2\text{ sr cm}^{-1})$ and the brightness temperature increases 44 %.

Measurements made by an AERI instrument at the Southern Great Plains Cloud and Radiation Testbed show considerably smaller increases (typically an increase from ~ 10 to $\sim 30\text{ mW}/(\text{m}^2\text{ sr cm}^{-1})$ averaged over $750\text{--}1200\text{ cm}^{-1}$) in the presence of similarly thick clouds (Turner et al., 2000), while previous measurements in the high Arctic taken at the Surface Heat Budget of the Arctic Ocean (SHEBA) show increases similar or larger to those made by the E-AERI in Eureka (typically $>40\%$ increase in brightness temperature averaged over $750\text{--}1200\text{ cm}^{-1}$) (Turner, 2005). Thus the impact of clouds on the radiation budget is greater in the Arctic than in other more humid regions due to the extremely cold and dry Arctic air and hence to the main atmospheric window being more transparent. This coincides with model results suggesting that the impact of clouds on the radiative budget is most pronounced for the Arctic (Vavrus, 2004). Such large increases in radiance and brightness temperatures in these spectral regions provide a proxy for cloud detection and enable analysis of cloud optical depth, phase,

and particle size (Turner, 2005). Cloud detection is crucial in the post-processing of E-AERI data since temperature and trace gas retrievals using SFIT2 are significantly more difficult in cloudy scenes.

4.2 Investigation of the lower 610 m using the P-AERI

E-AERI measurements were recorded at the PEARL Ridge Lab from October 2008 to September 2009. Comparisons between coincident E-AERI (at 610 m) and P-AERI (at 10 m) measurements of radiance from October 2008–April 2009 are shown in Fig. 8. Radiances were averaged on an hourly basis and used to calculate radiance differences. Each column of Fig. 8 corresponds to a single coincident hourly-averaged P-AERI–E-AERI spectrum. Typical temperature profiles for the high Arctic frequently exhibit temperature inversions (due to the extremely cold surface) for the first two kilometers above the surface; thus temperatures at the Ridge Lab are typically ~ 20 K warmer than at OPAL depending on the time of year. This is reflected in the $600\text{--}800\text{ cm}^{-1}$ CO_2 band (which is where the largest differences in Fig. 8 occur), corresponding to warmer temperatures at the Ridge Lab and a smaller CO_2 column (due to the 600 m elevation difference) resulting in greater E-AERI radiances. Other periods with large differences between the instruments correspond to the occurrence of ice crystals, high aerosol concentrations, fog or low cloud cover. For instance, the large radiance differences (red bands) in February occur on days for which low-level clouds were present above Eureka. For the low-level clouds that exist below 610 m, only the P-AERI can measure the increased emission from the cloud particles; hence the radiance difference increases for such days.

4.3 Comparisons with simulated radiances

Clear-sky comparisons between the E-AERI and P-AERI measurements at 00:08 UTC on 4 April 2009, are shown in Fig. 9a, with the residuals (P-AERI–E-AERI) in Fig. 9d. Large negative residuals in the $600\text{--}800\text{ cm}^{-1}$ and $2200\text{--}2400\text{ cm}^{-1}$ spectral regions

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



correspond to differences $>14\%$ and $>50\%$, respectively. Such differences are expected due to the large temperature difference at the two sites and the absorption by CO_2 , emphasizing the dependence of the radiative budget on the atmospheric temperature profile. Positive residuals typically occur in more transparent spectral regions where CO_2 absorption does not exist; they are positive due to the additional 600 m of atmospheric emission measured by the P-AERI. The measured radiance differences provide insight into the spectral regions that experience increasing or decreasing downwelling radiance at different altitudes.

The 4 April 2009 radiances were simulated using a Fast Line-By-Line Radiative Transfer Model (FLBLRTM) for an altitude of 10 m (P-AERI) and 610 m (E-AERI). The FLBLRTM is a faster version of a standard Line-By-Line Radiative Transfer Model (LBLRTM), as developed in Clough et al. (2005). This is achieved by replacing the computationally expensive section of the LBLRTM code that calculates absorption coefficients directly from a spectral database with absorption coefficient lookup tables set on a wavenumber, pressure, and temperature grid. Although the absorption coefficient has an absorber amount dependency, it is generally insignificant for atmospheric cases (Turner, 1995). Water vapour is an exception and is treated differently in that two tables are required to represent it instead of one as with other absorbers. In addition to speeding up the calculation, the use of tables also reduces the amount of code and hence enables the code to be relatively easy to tailor to a specific problem.

For this work, absorption coefficient tables for H_2O , CO_2 , O_3 , N_2O , CO , CH_4 , O_2 and N_2 were created for the spectral region from 400 to 3000 cm^{-1} on a grid interval of 0.005 cm^{-1} . The spectral line data are taken from HITRAN 2008 (Rothman et al., 2009). The H_2O continuum is accounted for by CKD2.4 continuum model (Clough et al., 1989) and in all cases the Voigt line shape is assumed.

The radiances are computed for clear skies with no aerosols. Temperature, pressure, and relative humidity data from Vaisala radiosondes launched near OPAL were interpolated to 00:08 UTC on 4 April and included in the simulation. Results from the model simulations are shown in Fig. 9b and agree with E- and P-AERI radiances within

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

AHSRL, which was deployed at Eureka in August 2005 and was operated throughout the period of interest. The circular particulate depolarization ratio was $>20\%$ below ~ 700 m (indicating ice crystals), and the backscatter cross-section above the ice crystal layer was $<10^{-6} \text{ m}^{-1} \text{ sr}^{-1}$ (indicating that liquid water clouds or precipitation were not associated with the ice crystal event). Both of these conditions pass the criteria used to screen for ice crystals in Lesins et al. (2009).

Ice crystal radiances were compared to clear-sky radiances measured the day before at 00:08–00:18 UTC on 4 April 2009, as shown in Fig. 11. The temperature difference between the PEARL Ridgley Lab and OPAL during the time of measurement was 2 K, accounting for small differences in the $600\text{--}800 \text{ cm}^{-1}$ CO_2 band (radiation emitted by ice crystals on 5 April also contribute to differences in this region, but to a lesser degree). Radiance measurements made during these two time intervals were averaged, and both instruments' differences (ice–clear) are shown. The P-AERI measured the largest increases in radiance since it was located below the ice crystal cloud and received emission from the ice particles. For instance, the largest ice–clear sky difference increase was 104% for the P-AERI and only 6% for the E-AERI averaged over $750\text{--}1000 \text{ cm}^{-1}$, indicating the large difference in downwelling radiance at these two altitudes.

Longwave downwelling radiances were converted to longwave downwelling all-sky irradiance using the method of Cox et al. (2011). The longwave downwelling thermal emission from the cloud was obtained by differencing the cloudy-sky and clear-sky irradiances; the clear-sky irradiance was obtained from an LBLRTM calculation using vertical profiles that were interpolated between the two radiosondes that bracket the time of the P-AERI measurement. This is important to avoid inclusion of irradiance contributions in spectral regions associated with the temperature structure and not the cloud since the irradiance calculation integrates over the whole spectrum. A $6\% \pm 1\%$ increase in downward irradiance from the ice cloud was measured by the P-AERI. The E-AERI measured a negligible increase, consistent with its location near the top of the ice cloud. A 6% irradiance increase for this thin cloud (<600 m thick) is in

agreement with the measured surface forcing of up to 36 % of the downward irradiance from thicker ice clouds (>2 km) found in Lesins et al. (2009). Given the frequency of ice crystal events at Eureka, this can have important consequences for the surface energy balance in the Arctic region.

5 Conclusions

A new extended-range AERI has been installed in the Canadian high Arctic. The E-AERI was calibrated and passed certification testing at the UW-SSEC in September 2008. Clear-sky inter-comparison tests between the E-AERI and UW's AERI-07 and AERI-Bago indicate comparable agreement between all three instruments. The performance of the E-AERI instrument meets or exceeds all initial design specifications for 1.0 cm^{-1} resolution infrared spectral observations with high absolute accuracy, with the exception of higher NESR values around 400 cm^{-1} . The E-AERI was installed at PEARL in October 2008. Side-by-side comparisons with the P-AERI in cloud-free conditions indicate agreement that is comparable to results from the UW-SSEC tests over most of the E-AERI's spectral range. Infrared radiance spectra of the sky and two calibrated blackbodies have been collected continuously approximately every seven minutes year-round, including both clear-sky and cloudy conditions.

A FLBLRTM was used to simulate clear-sky radiances at two altitudes and agrees with E- and P-AERI radiances for the majority of the spectrum. The largest differences between measured and simulated radiances occur in spectral regions that are strongly influenced by atmospheric temperature and/or water vapour, illustrating the model's dependence on accurate meteorological data from radiosondes. The difference between the downwelling radiance at two altitudes is shown to be highly variable during the measurement overlap period for different spectral regions due to meteorological changes, such as cloud cover and temperature.

The E-AERI's measured radiance has been shown to increase by over 400 % in the $750\text{--}1200 \text{ cm}^{-1}$ region in the presence of clouds, correlating with the MMCR and

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



AHSRL's detection of clouds above Eureka. This increase is larger for the Arctic than in other more humid regions, indicating that cloud cover plays a crucial role in the Arctic's radiative budget. A 6% increase in irradiance from a thin (<600 m thick) ice cloud for the P-AERI (below the cloud) and a negligible increase for the E-AERI (above the cloud) were found. Future detailed investigation of periods of large differences in the P-AERI–E-AERI radiances is planned to further investigate the impact of different meteorological events on the radiative budget in the high Arctic.

The implementation of a new emission version of the SFIT2 retrieval code is currently underway so that measurements of trace gases above Eureka can be performed using E-AERI spectra. Obtaining total columns of various trace gases (e.g. O₃, CO, CH₄, N₂O) using SFIT2 will provide insight into the atmospheric composition above Eureka throughout polar night. The E-AERI observations will provide a climatology of the infrared radiation budget and total columns of trace gases. For a comprehensive investigation of the radiative exchange in the Arctic, the E-AERI is supported by the AHSRL and MMCR, as well as an aerosol photometer suite and Baseline Surface Radiation Network (BSRN) instrumentation, all located at PEARL.

Acknowledgements. The Polar Environment Atmospheric Research Laboratory (PEARL) is operated by the Canadian Network for the Detection of Atmospheric Change (CANDAC). CANDAC/PEARL funding partners are: the Arctic Research Infrastructure Fund, Atlantic Innovation Fund/Nova Scotia Research Innovation Trust, Canadian Foundation for Climate and Atmospheric Science, Canadian Foundation for Innovation, Canadian Space Agency (CSA), Environment Canada (EC), Government of Canada International Polar Year, Natural Sciences and Engineering Research Council (NSERC), Ontario Innovation Trust, Ontario Research Fund, Indian and Northern Affairs Canada, and the Polar Continental Shelf Program. Spring visits to PEARL were made as part of the Canadian Arctic ACE Validation Campaigns, led by Kaley A. Walker and supported by CSA, EC, NSERC and the Northern Student Training Program. Thanks to CANDAC operators Ashley Harrett, Alexei Khmel, Paul Loewen, Oleg Mikhailov, Keith MacQuarrie and Matt Okraszewski who have helped with the P-AERI and E-AERI measurements at PEARL. Thanks to Stephane Lantagne from ABB Bomem for his work installing the E-AERI at PEARL. Thanks also to the staff at the Eureka Weather station for their support and hospitality.

References

- Batchelor, R., Strong, K., Lindenmaier, R., Mittermeier, R., Fast, H., Drummond, J. R., and Fogal, P.: A New Bruker IFS 125HR FTIR Spectrometer for the Polar Environment Atmospheric Research Laboratory at Eureka, Nunavut, Canada: Measurements and Comparison with the Existing Bomem DA8 Spectrometer, *J. Atmos. Ocean. Tech.*, 26, 1328–1340, 2009.
- Clough, S. A., Kneizys, F. X., and Davies, R. W.: Line shape and the water vapor continuum, *Atmos. Res.*, 23, 229–241, 1989.
- Clough, S. A., Iacono, M., and Moncet, J.-L.: Line-by-line calculations of atmospheric fluxes and cooling rates: Application to water vapour, *J. Geophys. Res.*, 97, 15761–15785, 1992.
- Clough, S. A., Shephard, M., Mlawer, E., Delamere, J., Iacono, M., Cady-Pereira, K., Boukabara, S., and Brown, P.: Atmospheric radiative transfer modeling: a summary of the AER codes, *J. Quant. Spectrosc. Ra.*, 91, 233–244, 2005.
- Collard, A. D., Ackerman, S. A., Smith, W. L., Ma, H. E., Revercomb, H. E., Knuteson, R. O., and Lee, S. C.: Cirrus cloud properties derived from high spectral resolution infrared spectrometry during FIRE II, Part III: Ground-based HIS results *J. Atmos. Sci.*, 52, 4264–4275, 1995.
- Cox, C., Walden, V., and Rowe, P.: A comparison of the atmospheric conditions at Barrow, Alaska and Eureka, Canada (2006–2008), in preparation for *J. Geophys. Res.*, 2011.
- DeSlover, D. H., Smith, W. L., Piironen, P. K., and Eloranta, E. W.: A methodology for measuring cirrus cloud visible-to-infrared spectral optical depth ratios, *J. Atmos. Ocean. Tech.*, 16, 251–262, 1999.
- DOE: Atmospheric Radiation Measurement Program plan, U.S. Department of Energy, Washington, DC, DOE/ER-0442 and DOE/ER-0441, 135 pp., 1990.
- Ellingson, R. and Wiscombe, W.: The Spectral Radiance Experiment (SPECTRE): Project description and sample results, *B. Am. Meteorol. Soc.*, 77, 1967–1985, 1996.
- Eloranta, E. W.: High spectral resolution lidar, Lidar: Range-Resolved Optical Remote Sensing of the Atmosphere, in: Springer Series in Optical Sciences, edited by: Weitkamp, K., Springer-Verlag, 143–163, 2005.
- Feltz, W., Smith, W., Knuteson, R., Revercomb, H., Woolf, H., and Howell, H.: Meteorological applications of temperature and water vapor retrievals from the ground-based Atmospheric Emitted Radiance Interferometer (AERI), *J. Appl. Meteorol.*, 37, 857–875, 1998.

AMTD

4, 6411–6448, 2011

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Rothman, L., Gordon, I., Barbe, A., Chris Benner, D., Bernath, P., Birk, M., Boudon, V., Brown, L., Campargue, C., Champion, J., Chance, K., Coudert, L., Dana, V., Devi, V., S. Fally, Flaud, J.-M., Gamache, R. R., Goldman, A., Jacquemart, D., Kleiner, I., Lacome, N., Lafferty, W. J., Mandin, J.-Y., Massie, S. T., Mikhailenko, S. N., Miller, C. E., Moazzen-Ahmadi, N., Naumenko, O. V., Nikitin, A. V., Orphal, J., Perevalov, V. I., Perrin, A., Predoi-Cross, A., Rinsland, C. P., Rotger, M., Simeckova, M., Smith, M. A. H., Sung, K., Tashkun, S. A., Tennyson, J., Toth, R. A., Vandaele, A. C., and Vander Auwera, J.: The HITRAN 2008 molecular spectroscopic database, *J. Quant. Spectrosc. Ra.*, 110, 533–572, 2009.

Rowe, P., Miloshevich, L., Turner, D., and Walden, V.: Quantification of a dry bias in radiosonde humidity profiles over Antarctica, *J. Atmos. Ocean. Tech.*, 25, 1529–1541, 2008.

Rowe, P., Neshyba, S., and Walden, V.: Responsivity-based criterion for accurate calibration of FTIR emission spectra: theoretical development and bandwidth estimation, *Opt. Express*, 19, 5451–5463, 2011a.

Rowe, P., Neshyba, S., Cox, C., and Walden, V.: A responsivity-based criterion for accurate calibration of FTIR emission spectra: identification of in-band low-responsivity wavenumbers, *Opt. Express*, 19, 5930–5941, 2011b.

Schneider, M., Romero, P. M., Hase, F., Blumenstock, T., Cuevas, E., and Ramos, R.: Continuous quality assessment of atmospheric water vapour measurement techniques: FTIR, Cimel, MFRSR, GPS, and Vaisala RS92, *Atmos. Meas. Tech.*, 3, 323–338, doi:10.5194/amt-3-323-2010, 2010.

Shaw, J., Nugent, P., Pust, N., Thurairajah, B., and Mizutani, K.: Radiometric cloud imaging with an uncooled microbolometer thermal infrared camera, *Opt. Express*, 13, 5807–5817, 2005.

Smith, W. L., Feltz, W. F., Knuteson, R. O., Revercomb, H. B., Howell, H. B., and Woolf, H. M.: The retrieval of planetary boundary layer structure using ground-based infrared spectral radiance measurements, *J. Atmos. Ocean. Tech.*, 16, 323–333, 1999.

Stokes, G. M. and Schwartz, S. E.: The Atmospheric Radiation Measurement (ARM) Program: Programmatic background and design of the Cloud and Radiation Testbed, *B. Am. Meteorol. Soc.*, 75, 1201–1221, 1994.

Tobin, D., Best, F., Brown, P., Clough, S., Dedecker, R., Ellingson, R., Garcia, R., Howell, H., Knuteson, R., Mlawer, E., Revercomb, H., Short, J., van Delst, P., and Walden, V.: Downwelling spectral radiance observations at the SHEBA ice station: Water vapor continuum measurements from 17 to 26 μm , *J. Geophys. Res.*, 104, 2081–2092, 1999.

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

- Turner, D. D.: Arctic mixed-phase cloud properties from AERI-lidar observations: Algorithm and results from SHEBA, *J. Appl. Meteorol.*, 44, 427–444, 2005.
- Turner, D. D. and Gero, P. J.: Downwelling 10 μm radiance temperature climatology for the Atmospheric Radiation Measurement Southern Great Plains site, *J. Geophys. Res.*, 116, D08212, doi:10.1029/2010JD015135, 2011.
- Turner, D. D., Feltz, W. F., and Ferrare, R. A.: Continuous water vapor profiles from operational ground-based active and passive remote sensors, *B. Am. Meteorol. Soc.*, 81, 1301–1317, 2000.
- Turner, D. S.: Absorption Coefficient Estimation Using A Two Dimensional Interpolation Procedure, *J. Quant. Spectrosc. Ra.*, 53, 633–637, 1995.
- UW-SSEC: UW Final Report on ABB-Bomem E-AERI-001, Certification Testing, University of Wisconsin, 9 December 2008, 1–12 pp., 2008.
- Vavrus, S.: The Impact of Cloud Feedbacks on Arctic Climate under Greenhouse Forcing, *J. Climate*, 17, 603–615, 2004.
- Walden, V. P., Town, M., Halter, B., and Storey, J.: First measurements of the infrared sky brightness at Dome C, Antarctica, *Publ. Astron. Soc. Pac.*, 117, 300–308, 2005.
- Yurganov, L., McMillan, W., Wilson, C., Fischer, M., Biraud, S., and Sweeney, C.: Carbon monoxide mixing ratios over Oklahoma between 2002 and 2009 retrieved from Atmospheric Emitted Radiance Interferometer spectra, *Atmos. Meas. Tech.*, 3, 1319–1331, doi:10.5194/amt-3-1319-2010, 2010.

Table 1. E-AERI instrument performance.

Item	Performance
General System Elements	<ul style="list-style-type: none"> – ABB Bomem MR-300 Michelson interferometer with PC computer interface – Full-aperture temperature-controlled calibration reference sources – Automated system for providing sequential views of the sky (zenith) and two blackbodies (one at ambient temperature, one at 37°C) for radiometric calibration – Environmental Monitoring System, for blackbody temperature data – Computer and Data Handling System, for sequencing all E-AERI operations and data handling, including acquisition, processing, display, and networking
* Spectral range	400–3000 cm ⁻¹ (3.3–25 μm)
* Spectral resolution	1.0 cm ⁻¹ , unapodized maximum optical path difference [OPD] of 1 cm
* Spatial and angular FOV	46 ± 1 mrad full angle
* Radiometric calibration absolute accuracy	<1 % of ambient blackbody radiance
* Reproducibility	<0.2% of ambient blackbody radiance
* Blackbody cavity characterization	<ul style="list-style-type: none"> – Temperature Knowledge: ±0.1 °C of absolute temperature – Emissivity knowledge: better than ±0.1 % – Temperature stability: better than 0.05 °C over viewing period (> 120 s)
* Nonlinearity knowledge	Better than 0.1 %
* Polarization	<0.1 %
* Wavelength calibration	Channel wavenumber knowledge: better than 0.01 cm ⁻¹
* Noise (RMS for 2-min blackbody view)	<p><0.4 mW (m² sr cm⁻¹)⁻¹ for 420–1400 cm⁻¹ (except 667 cm⁻¹, where CO₂ in the instrument reduces responsivity)</p> <p><0.015 mW (m² sr cm⁻¹)⁻¹ for 2000–2600 cm⁻¹ (except 2300–2400 cm⁻¹, where CO₂ in the instrument reduces responsivity)</p>
Temporal sampling	<p>Repeat cycle: ≈7 min</p> <p>Interferometer scan period: <2 s</p>
Detectors	<p>Two detectors are mounted in sandwich configuration covering two spectral regions:</p> <p>Channel one (400–1800 cm⁻¹): extended-range photoconductive mercury cadmium telluride (MCT)</p> <p>Channel two (1800–3000 cm⁻¹): photovoltaic indium antimonide (InSb)</p>
Beamsplitter	Potassium bromide (KBr)
Operational requirement	<p>Automatic control system hardware contains these features:</p> <ul style="list-style-type: none"> – Scheduled sequencing of the following operations: <ul style="list-style-type: none"> Scene switching between sky and blackbody views Interferometer and housekeeping data acquisition and transfer – Capability of remotely changing the operation listed above – 24-h continuous operations with data output at 7-min intervals – Linear stirling-cycle cryo-cooler keeps detectors cooled down below 70 K – Real-time display with flags for out-of-limit conditions

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

[Title Page](#)
[Abstract](#)
[Introduction](#)
[Conclusions](#)
[References](#)
[Tables](#)
[Figures](#)
[Back](#)
[Close](#)
[Full Screen / Esc](#)
[Printer-friendly Version](#)
[Interactive Discussion](#)


Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

[Title Page](#)

[Abstract](#) [Introduction](#)

[Conclusions](#) [References](#)

[Tables](#) [Figures](#)

[◀](#) [▶](#)

[◀](#) [▶](#)

[Back](#) [Close](#)

[Full Screen / Esc](#)

[Printer-friendly Version](#)

[Interactive Discussion](#)

Table 1. Continued.

Item	Performance
Operating environment	Operating temperature: – Spectroradiometer (back-end) enclosure: -30° to $+40^{\circ}\text{C}$ – Input and calibration (front-end) enclosure: -70° to $+40^{\circ}\text{C}$
Data products	Primary (required for scientific use): – Calibrated spectra – Standard deviation for blackbody and sky views – Calibration coefficient and blackbody temperature Secondary (auxiliary information for real-time monitoring and quality control): – Ambient air temperature – Ambient pressure – Ambient humidity – Instrument housekeeping data

Items with a * indicate performance metrics verified during calibration at UW-SSEC.



Table 2. Parameter metrics used when monitoring the status of the E-AERI. The normal operating range customized for operation at Eureka lies between the limits shown.

Parameter	Normal Operating Limits
AB Temperature	243.15, 313.15 K
HB Temperature	263.15, 353.15 K
Outside Temperature	233.15, 323.15 K
Rack Ambient Temperature	277.15, 319.15 K
Rain Intensity	2.5, 3.2 V
AB Maximum Temperature Difference	0.1 K
HB Maximum Temperature Difference	0.7 K
B Support Structure Temperature	233.15, 323.15 K
Air Temperature near Blackbodies	233.15, 343.15 K
SCE Temperature	273.15, 333.15 K
Air Humidity	1, 99 %
HB Stability	-0.5, 0.5 K
Mirror Motor Temperature	233.15, 363.15 K
Atmospheric Pressure	750.0, 1040.0 Pa
336 Kelvin (Reference)	2426.96, 2433.04 Ω
293 Kelvin (Reference)	10 480.04, 10 493.96 Ω
249 Kelvin (Reference)	97 232, 98 272 Ω
Motor Driver Temperature	273.15, 323.15 K
Interferometer Window Temperature	293.596, 324.924 K
Encoder Scene Confirm	-5, 5 0.01°
LW HB NEN	0, 1 mW/(m ² sr cm ⁻¹)
SW HB NEN	0, 0.1 mW/(m ² sr cm ⁻¹)
Air Temperature near Interferometer	293.87, 322.09 K
LW Responsivity	0.0104, 5 Counts/mW/(m ² sr cm ⁻¹)
SW Responsivity	0.0112, 20 Counts/mW/(m ² sr cm ⁻¹)
Cooler Compressor Temperature	290.398, 350.202 K
Cooler Current	0.03, 0.086 Amp
Cooler Expander Temperature	285.0, 368.4 K
Detector Temperature	61.3, 70.4 K

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Discussion Paper | Discussion Paper | Discussion Paper | Discussion Paper | Discussion Paper

Title Page

Abstract Introduction

Conclusions References

Tables Figures

⏪ ⏩

◀ ▶

Back Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

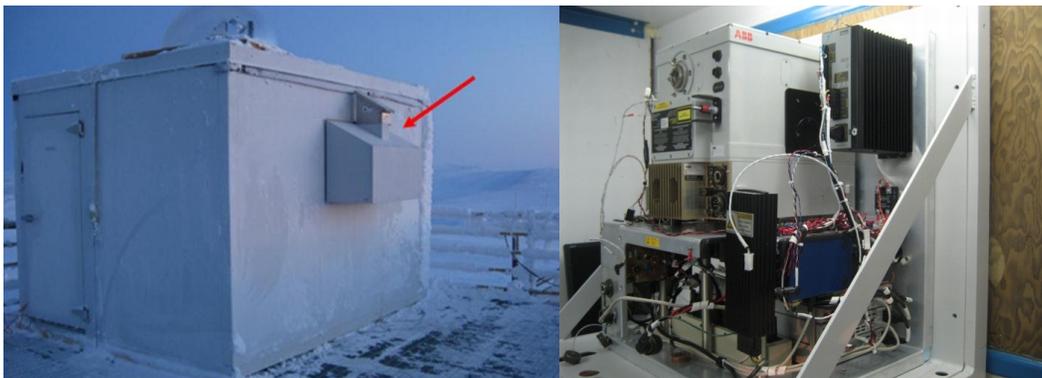


Fig. 1. Exterior (left panel, red arrow) and interior (right panel) views of the E-AERI installed on the roof of the PEARL Ridge Lab using the thru-wall configuration. Left panel: the hatch is closed during precipitation events (Photo: Stephane Lantagne). Right panel: the back-end of the E-AERI instrument with its internal protective enclosure removed, showing the MR-300 series interferometer housing and electronics (Photo: Zen Mariani).

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

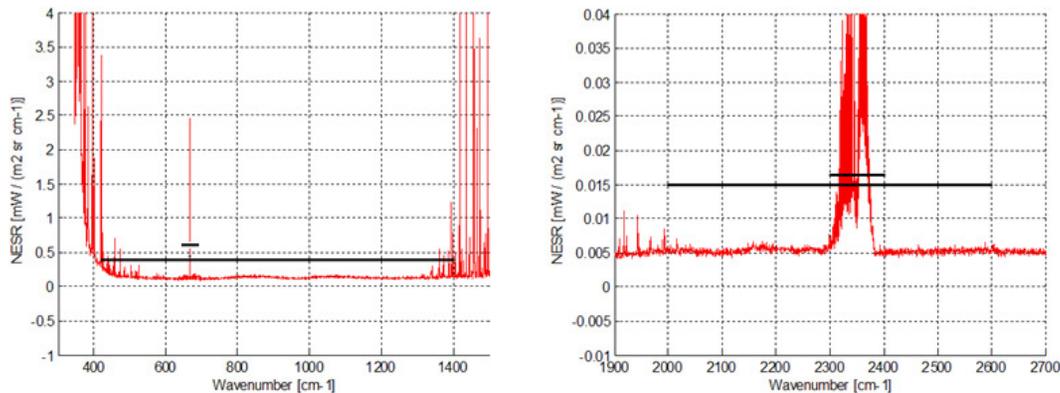


Fig. 2. NESR test for the MCT (Left panel) and InSb (right panel) detectors performed in Eureka. The solid black line indicates the specified requirement for the NESR test. The elevated black line indicates the spectral region where the NESR is expected to increase due to CO₂ in the instrument.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

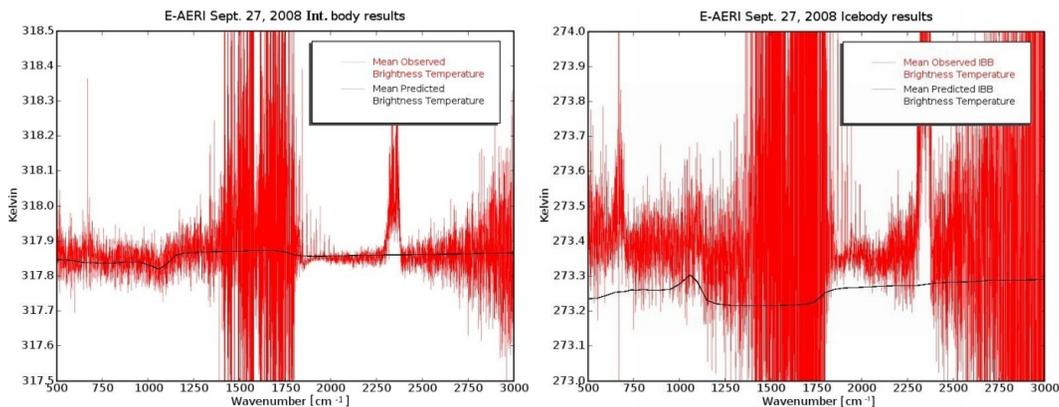


Fig. 3. Laboratory radiometric calibration verification “four-body” test results conducted at UW-SSEC on 27 September 2008 before deployment to Eureka. Left panel: intermediate blackbody brightness temperature spectrum. Right panel: IB brightness temperature spectrum. The measured spectrum (red) is the temporal-averaged calibrated radiance converted to equivalent blackbody brightness temperature. Note the y-axis range in both panels is 1 K. The black line indicates the predicted blackbody temperature.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

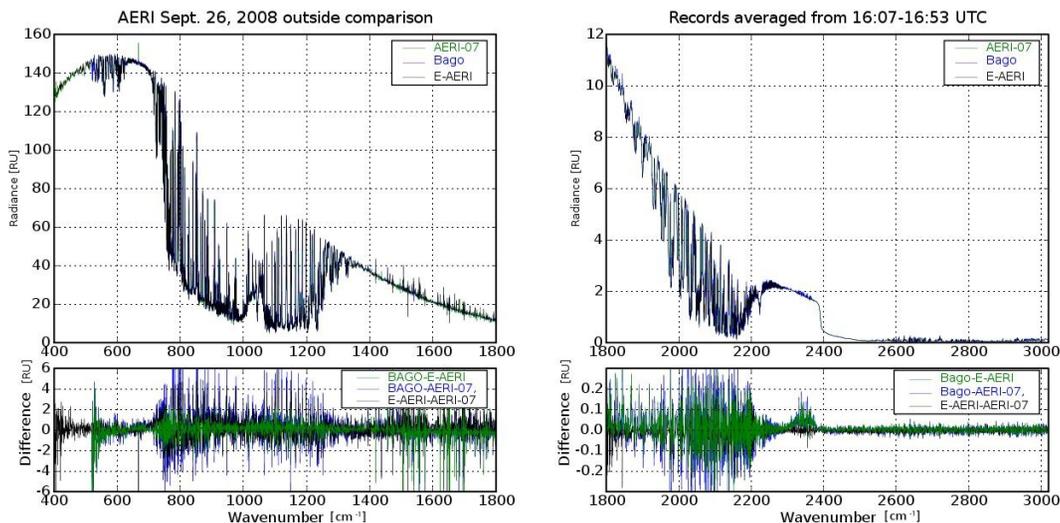


Fig. 4. Radiance measurements during two outside side-by-side tests performed at UW. Top panels display measured radiance ($\text{RU} = \text{mW}/(\text{m}^2 \text{sr cm}^{-1})$) with residuals in the bottom panels.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

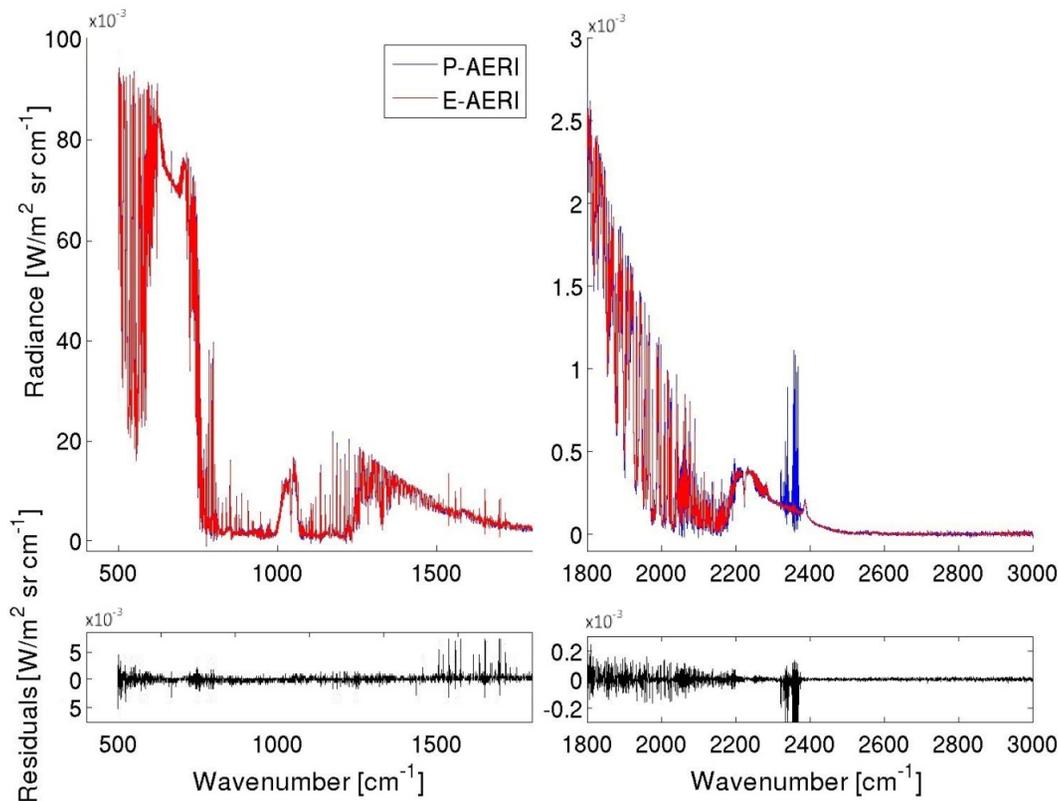


Fig. 5. Side-by-side comparisons between the E- and P-AERI instruments within the P-AERI spectral range on 20 October 2008. Top panels display measured radiance with residuals in the bottom panels.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

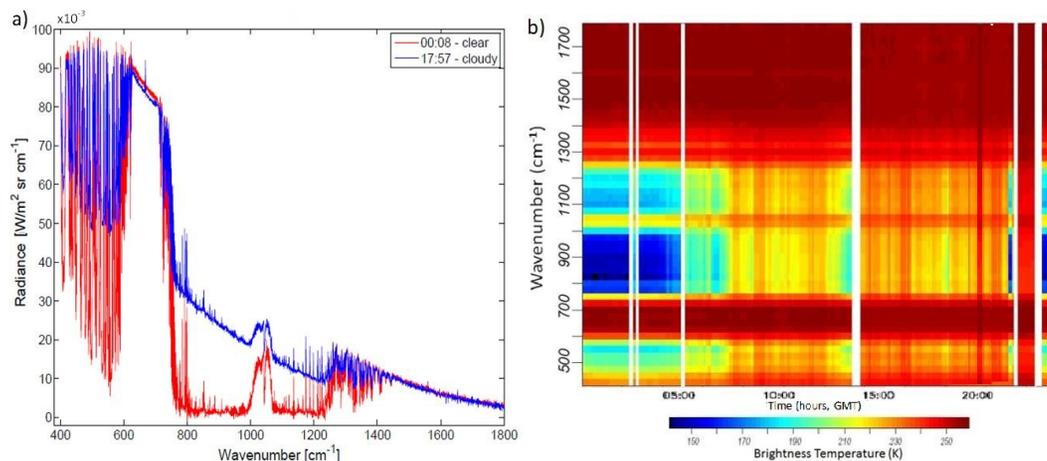


Fig. 6. (a) E-AERI measurements of radiance on 16 April 2009 at 00:08 UTC (red) and 17:57 UTC (blue). (b) Brightness temperatures measured throughout 16 April 2009. White spaces correspond to periods of no measurement (instrument reboot, precipitation). Only the longwave spectral region (up to 1800 cm^{-1}) is shown for clarity.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[⏴](#)[⏵](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

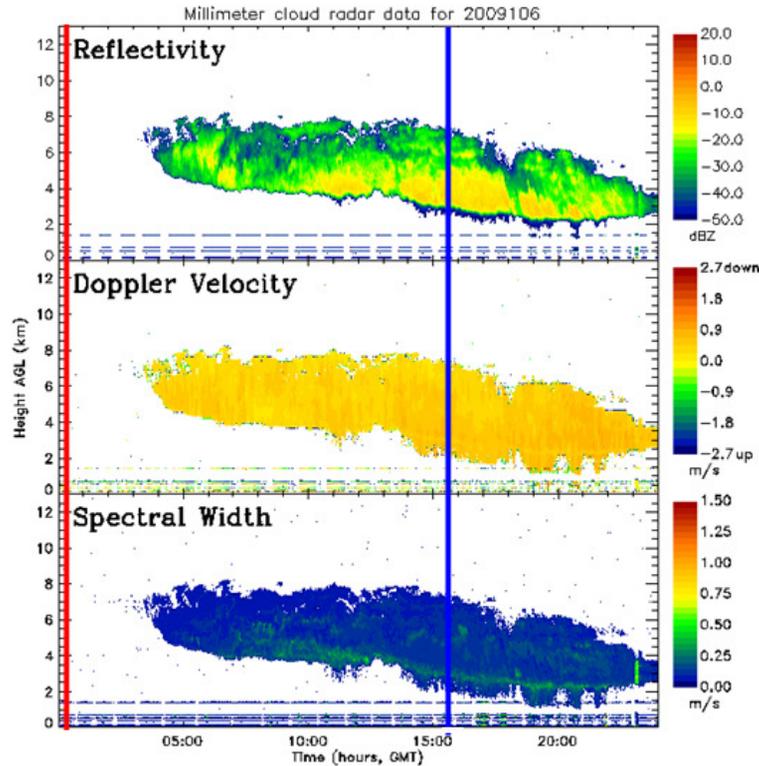


Fig. 7. MMCR reflectivity, Doppler velocity, and spectral width plots for 16 April 2009. Red and blue vertical bars correspond to the time of E-AERI measurements, at 00:08 UTC and 17:57 UTC, respectively, shown in Fig. 6a.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

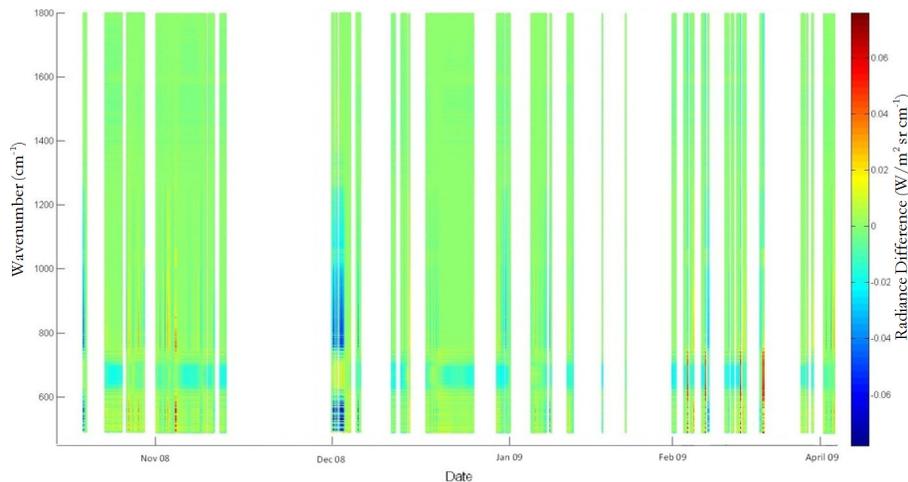


Fig. 8. Hourly-averaged coincident radiance difference measurements (P-AERI–E-AERI) from 22 October 2008–5 April 2009. Only the longwave radiances are shown for clarity. White spaces correspond to periods with no measurement overlap due to precipitation or instrument maintenance.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

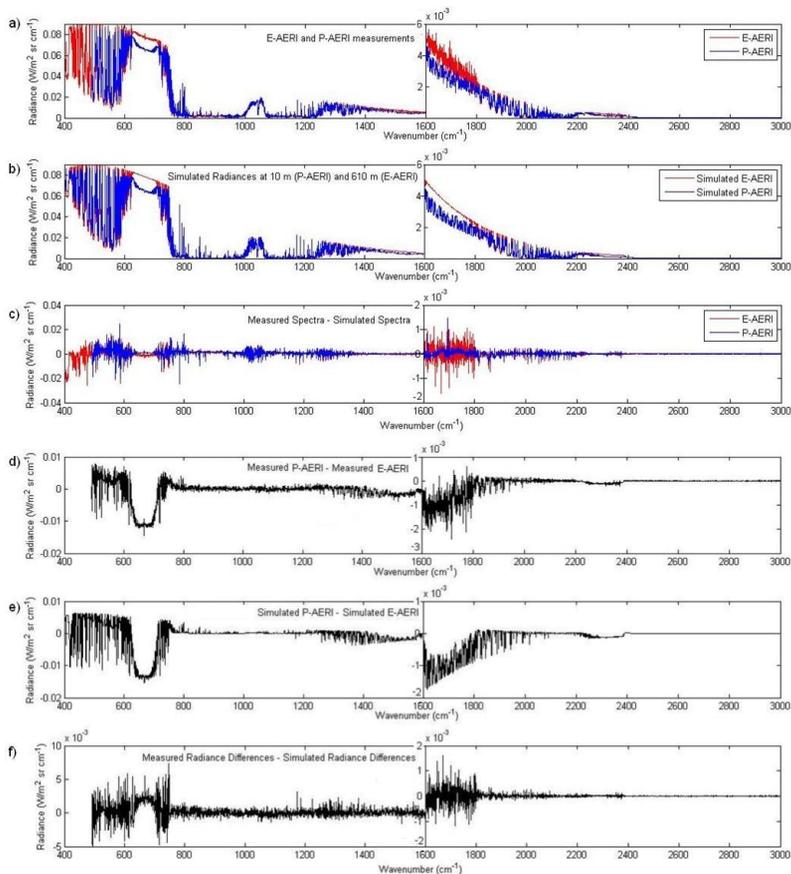


Fig. 9. (a) E-AERI (red) and P-AERI (blue) measured radiances at 00:08 UTC on 4 April 2009 with (b) simulated spectra shown below. (c) Differences between the measured and simulated spectra (a–b). (d) Measured residuals (P-AERI–E-AERI) with (e) simulated residuals shown below. (f) Differences between the measured and simulated radiance differences (d–e).

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

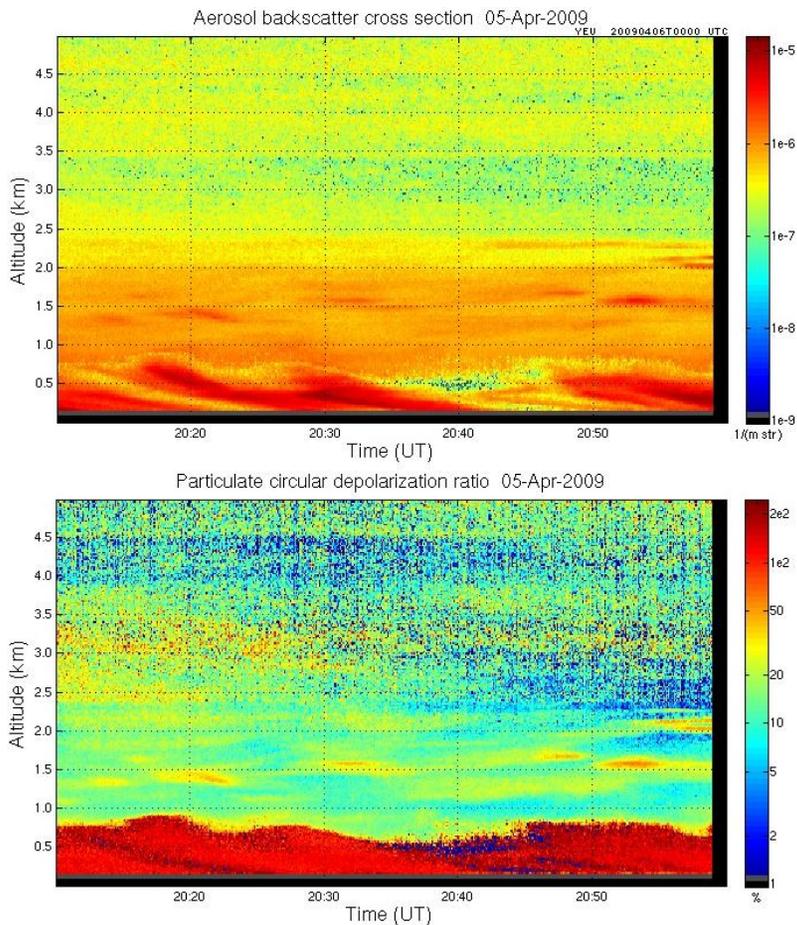


Fig. 10. AHSRL measurements of backscatter cross section (top panel) and particulate circular depolarization ratio (bottom panel) between 20:10 and 21:00 UTC on 5 April 2009. From 20:30–20:40 UTC, the top of the ice crystal layer was below 610 m, where the E-AERI is located.

Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

Title Page

Abstract Introduction

Conclusions References

Tables Figures

◀ ▶

◀ ▶

Back Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Infrared emission measurements in the Arctic using a new extended-range AERI

Z. Mariani et al.

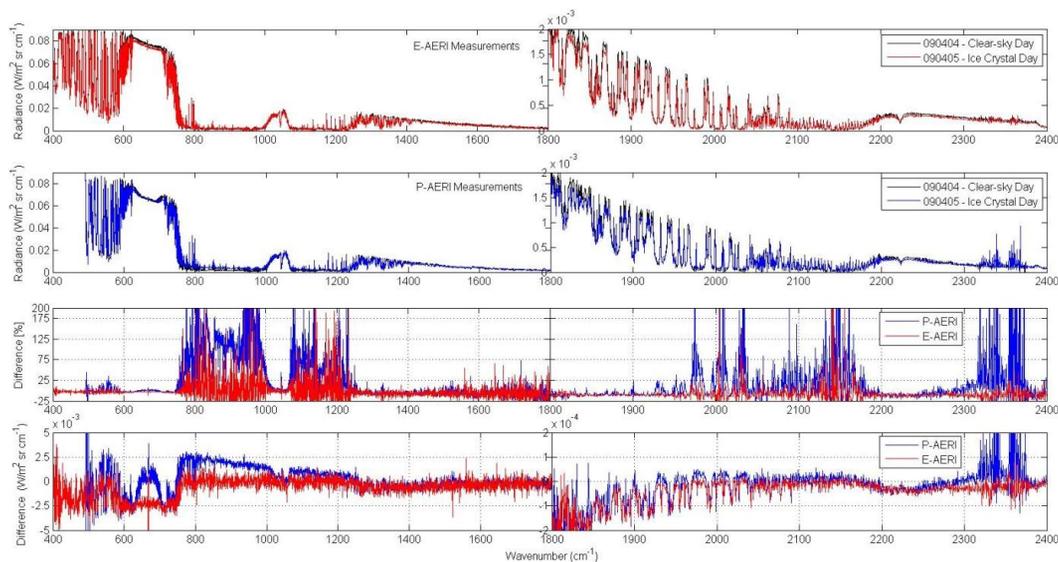


Fig. 11. Radiance measurements for 4 April 2009 (00:08–00:18 UTC) and 5 April 2009 (20:30–20:40 UTC) for the E-AERI (top panel) and P-AERI (second panel). Bottom panels are differences between the ice crystal and clear-sky radiances, given as a percentage (ice crystal–clear sky/clear sky) and in radiance for both instruments.