

Sensitivity of Laser
Induced
Fluorescence
instruments

L. K. Whalley et al.

This discussion paper is/has been under review for the journal Atmospheric Measurement Techniques (AMT). Please refer to the corresponding final paper in AMT if available.

Reporting the sensitivity of Laser Induced Fluorescence instruments used for HO₂ detection to an interference from RO₂ radicals and introducing a novel approach that enables HO₂ and certain RO₂ types to be selectively measured

L. K. Whalley^{1,2}, M. A. Blitz^{1,2}, M. Desservettaz¹, P. W. Seakins^{1,2}, and D. E. Heard^{1,2}

¹School of Chemistry, University of Leeds, Leeds, LS2 9JT, UK

²National Centre for Atmospheric Science, University of Leeds, Leeds, LS2 9JT, UK

Received: 11 June 2013 – Accepted: 29 June 2013 – Published: 9 July 2013

Correspondence to: L. K. Whalley (lisakw@chem.leeds.ac.uk)

Published by Copernicus Publications on behalf of the European Geosciences Union.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

Abstract

Laboratory studies have revealed that alkene-derived RO_2 and longer-chain alkane-derived RO_2 ($> \text{C}_3$) radicals rapidly convert to HO_2 and then to OH in the presence of NO in a Fluorescence Assay by Gas Expansion (FAGE) detection cell (Fuchs et al., 2011). Three different FAGE cells that have been used to make ambient measurements of OH and HO_2 in the University of Leeds ground-based instrument have been assessed to determine the sensitivity of each cell, when operating in HO_2 detection mode, to RO_2 radicals. The sensitivity to this interference was found to be highly dependent on cell design and operating parameters. Under the operating conditions employed during fieldwork undertaken in the Borneo rainforest in 2008, an OH yield of 17 % was experimentally determined for both ethene- and isoprene-derived RO_2 radicals. The high pumping capacity of this system, resulting in a short residence time, coupled with poor mixing of NO into the ambient air-stream for the titration of HO_2 to OH effectively minimised this potential interference. An OH yield of 46 % was observed for ethene-derived RO_2 radicals when a smaller detection cell was used, in which the mixing of NO into the ambient air was improved and the cell residence times were longer. For a newly developed RO_x LIF cell, used for detection of HO_2 and RO_2 radicals, when running in HO_x mode an OH yield of 95 % was observed for ethene-derived RO_2 radicals.

In experiments in which conditions ensured the conversion of RO_2 to OH was complete, the yields of OH from a range of different RO_2 species agreed well with model predictions based on the Master Chemical Mechanism version 3.2. For ethene and isoprene derived RO_2 species, the relative sensitivity of FAGE was found to be close to that for HO_2 with an OH yield of 100 % and 92 % respectively. For the longer-chain alkane-derived RO_2 radicals, model predicted OH yields were highly dependent upon temperature. A model predicted OH yield of 74 % at 298 K and 36 % at 255 K were calculated for cyclohexane derived RO_2 radicals and an experimental yield of 38 % was

AMTD

6, 6249–6292, 2013

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

observed indicating that the temperature within the cell was below ambient owing to the supersonic expansion of the airstream in the low pressure cell.

These findings suggest that observations of HO₂ by some LIF instruments world-wide may be higher than the true value if the instruments were sensitive to these RO₂ species. If this is the case, it becomes necessary to compare atmospheric chemistry model simulations to HO₂* observations, where HO₂* = [HO₂] + α [RO₂] and α is the mean fractional contribution of the RO₂ species that interfere (RO₂i). This methodology, however, relies on model simulations of speciated RO₂ radicals, as instrumentation to make speciated RO₂ measurements does not currently exist. Here we present an approach that enables the concentration of HO₂ and RO₂i to be selectively determined by varying the concentration of NO injected into a FAGE cell. Measurements of [HO₂] and [RO₂i] taken in London are presented.

1 Introduction

OH and HO₂ radicals, collectively termed HO_x, together with RO₂ radicals, control the oxidative chemistry in the atmosphere, being responsible for the transformation of primary emissions into secondary pollutants such as NO₂, O₃ and particulates. OH radicals control the lifetime of some greenhouse gases (e.g. CH₄), the production of acidic species (e.g. H₂SO₄) and aerosol precursors such as oxygenated volatile organic compounds. Understanding the behaviour of free-radicals in the atmosphere is of paramount importance in understanding the lifetimes of pollutants and hence the spatial scales of their transport. Predictive models for future air quality and climate change contain complex chemical schemes, and comparison with measurements of free-radicals (the concentrations of which are controlled only by local chemistry and not by transport) in the present atmosphere constitutes one of the best validations of these schemes (Heard and Pilling, 2003). OH and HO₂ radicals in the troposphere have been measured since the early 1990s using laser induced fluorescence (LIF) spectroscopy at low pressure (Fluorescence Assay by Gas Expansion, or the FAGE technique) orig-

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



inally developed by Hard et al. (1979, 1984). The technique employs 308 nm radiation, produced using a variety of laser technologies, to excite OH radicals, which fluoresce; this emission (also at 308 nm) is detected and used to quantify OH. It is also possible to simultaneously detect HO₂ in a second fluorescence cell, by chemical conversion to OH through reaction with NO and subsequent detection by LIF. The technique has been employed by several groups worldwide for the detection of OH and HO₂ (Hofzumahaus et al., 1996; Mather et al., 1997; Kanaya et al., 1999; Creasey et al., 2001; Faloona et al., 2001; Hanisco et al., 2002; Holland et al., 2003; Heard and Pilling, 2003; Stone et al., 2012). Specific to this work, the Leeds ground-based FAGE instrument has been operational since 1996 and has detected OH and HO₂ under a variety of conditions ranging from urban (Heard et al., 2004) to clean marine (Whalley et al., 2010). Although the FAGE technique represents an extremely sensitive (typical OH detection limits are in the low to mid 10⁵ molecule cm⁻³) (Heard and Pilling, 2003) and selective method for OH and HO₂ detection, ambient HO_x concentrations are themselves extremely low (OH concentrations are typically a few 10⁶ molecule cm⁻³) (Stone et al., 2012), thus, care needs to be taken to ensure that any measurement is not biased by any chemical or spectral interference.

A well-documented example of an OH interference comes from the earliest tropospheric LIF instruments (Davis et al., 1981; Ortgies et al., 1980; Shirinzadeh et al., 1987), which used off-resonant pulsed laser excitation of the OH radical at 282 nm, via the $A^2\Sigma^+(v' = 1) \leftarrow X^2\Pi_i(v'' = 0)$ transition. These instruments were found to suffer from a considerable interference from laser-generated OH formed by the laser photolysis of ambient ozone and subsequent reaction of O(¹D) with ambient water vapour:



The use of OH detection at lower pressure (reducing [H₂O] and hence the rate of R2), lower laser energy per pulse (the OH artefact signal depends on the square of the laser energy) and switching to excitation at 308 nm (the H₂O/O₃ interference is

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



30 times lower than at 282 nm) almost completely overcame this problem. Holland et al. (2003), however, observed an interference in the presence of ozone and water vapour that appeared to be a dark reaction on the walls of their detection cell which produced a source of HO₂ radicals; the authors report a signal equivalent to 5.4 × 10⁷ molecule cm⁻³ of HO₂ in the presence of 50 ppbv O₃ and at a relative humidity of 60 %. This interference has been characterised in detail and is subtracted from their ambient HO₂ measurements.

In the presence of the added NO used to convert HO₂ to OH inside the fluorescence cell, and hence enable HO₂ to be measured, organic peroxy radicals (RO₂) also have the potential to be chemically converted to OH via:



Due to the low pressure employed in FAGE detection, however, R4 is slow (~ 12 s⁻¹ for CH₃O at 1 Torr) and, given the very short residence time in FAGE between NO injection and the detection region of typically just a few milliseconds (Creasey et al., 1997b), it was assumed, until recently, that RO₂ radicals were not converted to OH to any large extent. In support of this, Ren et al. (2004) reported no interference upon introduction of C₁–C₄ alkane derived RO₂ radicals in the Penn. State FAGE system, and concluded that there was no evidence of any significant interferences for OH or HO₂ measurements in the atmosphere, including in highly polluted urban environments. Only recently has an interference from alkene and aromatic derived RO₂ species been reported (Fuchs et al., 2011). Unlike alkane-derived RO₂ species which are formed via H-atom abstraction from the parent alkane and subsequent addition of O₂ (Reaction R6), the major pathway to alkene-derived RO₂ formation is via OH addition across

the double bond followed by O₂ addition (Reaction R7):



The β -hydroxyalkylperoxy radical formed reacts with NO to form a β -hydroxyalkoxy radical (Reaction R8) which can either react with O₂ (Reaction R9) or decompose to a hydroxyalkyl radical (Reaction R10) which then reacts rapidly with O₂ to form a carbonyl and HO₂ (Reaction R11). Compared to the slow RO + O₂ reaction ($k = 1.65 \times 10^{-15} \text{ cm}^3 \text{ molecule}^{-1} \text{ s}^{-1}$, for $R = \text{CH}_3$, (Reaction R9), Orlando et al., 2003), decomposition and subsequent reaction of the hydroxyalkyl radical (CH₂OH) with O₂ is fast ($k = 9.6 \times 10^{-12} \text{ cm}^3 \text{ molecule}^{-1} \text{ s}^{-1}$, Atkinson et al., 1997). Fuchs et al. (2011) found, due to this rapid decomposition pathway, that RO₂ species formed from alkene and aromatic precursors were detected as OH with relative sensitivities greater than 80% with respect to that for detection of HO₂ in their FAGE system. The level of the interference was found to be highly dependent upon the NO concentration injected and reaction time between injection and OH detection, which was varied by Fuchs et al. (2011) suggesting that other FAGE instruments with different cell designs and operational parameters may display different sensitivities towards this interference. FAGE cells used for airborne HO₂ measurements tend to have longer inlets to extend through the fuselage of the aircraft and, hence, sampled air tends to have longer residence times in these cell types compared to cells used solely for ground measurements. Very recently, Mao et al. (2012) reported an average RO₂ sensitivity of ~ 60% with respect to that for HO₂ for a selection of alkene-derived RO₂ species in the Penn.

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

State FAGE instrument, whilst Vaughan et al. (2012) reported a sensitivity to ethene-derived RO_2 radicals of 40 % with respect to that for HO_2 for the University of Leeds aircraft FAGE instrument (Commane et al., 2010). Ultimately the measurement bias on the HO_2 concentrations reported from past field studies will depend upon the individual FAGE instruments utilised (because of variations in key operating parameters such as residence time) and the concentration and speciation of RO_2 present. Many FAGE groups now report HO_2^* for comparison with atmospheric chemistry box models (Lu et al., 2012) where $\text{HO}_2^* = [\text{HO}_2] + \alpha [\text{RO}_2]$, and α is the mean fractional contribution of the RO_2 species that interfere (RO_{2i}) in a particular instrument which has been determined experimentally.

Together with an HO_2 interference, FAGE measurements of OH are reported to have an interference for one instrument type in forested environments (Mao et al., 2012). The authors postulate that OH may be generated in their FAGE cell in the presence of ozone and alkenes with laser-generated OH within the cell being ruled out. Similar to the HO_2 interference reported here, this OH interference may be dependent upon the particular design of this FAGE cell, for example the residence time between sampling and detection and, as such, the extent that other OH measurements suffer from this interference is unknown, meaning that it is critical that a set of standardised experiments are performed on different FAGE cell types used for ambient detection of OH to assess the extent of any interference. Good agreement between two independent OH measurements made using Differential Optical Absorption Spectroscopy (DOAS) and LIF was observed during a series of experiments performed in the SAPHIR atmospheric simulation chamber under a range of atmospheric conditions (Fuchs et al., 2012) suggesting that the Julich FAGE system, at least, does not suffer an interference when detecting OH under the conditions studied.

In this paper we report results from interference studies performed using the University of Leeds ground-based FAGE instrument (Creasey et al., 1997a) measuring in HO_2 mode (NO added to the detection cell) and discuss the likely impact of the RO_2 interference on previous field studies. We also compare absolute yields of OH from

alkene-derived and higher alkane-derived RO₂ species in the presence of NO where conditions allowed reactions to proceed to completion and compare with MCMv3.2 recommendations.

2 Experimental

5 HO₂ and RO₂ radicals were generated prior to FAGE detection by two different methods: a steady-state turbulent flow tube reactor calibrated for absolute radical concentrations and a time-resolved laser flash photolysis system. Each method will be described in turn.

2.1 Steady state experiments

10 The FAGE calibration system (described in detail by Commane et al., 2010) acts as a turbulent flow reactor and generates known and equal quantities of OH and HO₂ radicals by the 184.9 nm photolysis of H₂O vapour by a Hg penray lamp in a humidified air stream (Reactions R12 and R13):



With knowledge of the product of the lamp flux and irradiation exposure time past the lamp (determined by N₂O actinometry, Commane et al., 2010) the concentration of OH and HO₂ may be determined; typical radical concentrations generated by this method range from < 10⁷–10⁹ molecule cm⁻³. RO₂ radicals (in the presence of HO₂ from R13) were generated by introducing the parent hydrocarbon into the FAGE calibration system approximately 2.5 cm after the penray lamp. The OH generated in the calibration photolysis region reacted rapidly with the hydrocarbon introduced, Reaction (R6), generating RO₂ radicals. To assess the magnitude of any HO₂ interference suffered during previous ambient field measurements, a number of individual peroxy

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

radical species were generated and introduced into three different fluorescence cells (Fig. 1) which have been used during field deployments by the Leeds group (further details on the fieldwork FAGE detection cells tested are given below). The peroxy radicals tested were derived from methane, propane, ethene, isoprene, toluene, cyclohexane and methanol. A small flow (~ 10 – 150 Standard Cubic Centimetre per Minute, SCCM) of a dilute (0.1–5 %) hydrocarbon mix in N_2 (ethene, isoprene, toluene, cyclohexane or methanol) or a 100 % hydrocarbon flow of propane (10 SCCM) or methane (500 SCCM) was introduced into a 20–40 Standard Litre per Minute (SLM) humidified air-stream approximately 5 cm before the exit of the calibration tube. The residence time within the calibration flow tube (~ 10 ms at 40 SLM) was sufficient to ensure complete conversion of OH to RO_2 before being sampled in the fluorescence cells. In the case of ethene, at an initial concentration of 3.1×10^{14} molecule cm^{-3} , it takes ~ 1 ms for complete conversion of OH to RO_2 , using a rate coefficient, $k_{C_2H_4+OH}$, equal to 2.86×10^{-11} molecule $^{-1}$ cm^3 s^{-1} (Cleary et al., 2006). This could be experimentally verified by observing the complete loss of the OH signal upon addition of the hydrocarbons when no NO was added to the FAGE expansion cells; this complete loss of OH signal was observed even for the slowest reacting hydrocarbon species (e.g. methane).

FAGE detection cells

The University of Leeds ground-based FAGE instrument described in detail elsewhere (Whalley et al., 2010) was assessed to determine the magnitude of the HO_2 interference from selected RO_2 species under configurations employed in two recent field studies. The first, the Oxidants and Particle Photochemical Processes (OP3) (Hewitt et al., 2010) which took place in the Borneo rainforest (Whalley et al., 2011) and the second, the Hill Cap Cloud Thuringer – 2010 (HCCT-2010) (Whalley et al., 2013) which aimed to quantify the loss of radicals to cloud droplets.

The operational parameters of the different FAGE fluorescence cells considered are quite different and are summarised in Table 1. During OP3, one 22 cm internal diame-

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

ter cylindrical, stainless steel fluorescence cell was used to make sequential measurements of OH and HO₂ (Fig. 1a). Air was drawn into the cell via a 5 cm tall, 2.54 cm diameter turret through a 1 mm diameter pinhole nozzle in a flat plate (0.1 mm thickness). The cell was maintained at approximately 0.9 Torr using a Roots blower backed by a rotary pump (Leybold)). The cell was connected to the pump system via a 10 cm ID, 5 m length stainless steel flexible hose. NO was injected into the cell 7.5 cm below the nozzle via a custom-built injection ring containing four injection points, spaced 4 cm apart, and made from 1.6 mm (ID) tubing in a square arrangement located around the air stream. 50 SCCM NO was injected into the cell via a computer-controlled solenoid valve (Metron Semiconductors) and calibrated mass flow controller (MKS 1179A, range 0–50 SCCM) during the second half of the collection period when the laser was tuned to the OH transition. As only one cell was used for sequential detection of OH and HO₂, the conditions were optimised to maximise the sensitivity towards OH. Under these conditions the conversion of HO₂ to OH was only ~ 10 %, most likely due to poor mixing of the NO into the ambient air flow caused by the particular flow characteristics created by the combination of the 1 mm diameter pinhole nozzle and the pressure and pumping speeds employed. The 10 % conversion of HO₂ to OH determined assumes that there is no preferential loss of either radical in the calibration system, i.e. that the concentration of OH and HO₂ are equal as they enter the FAGE detection cell. This assumption has previously been verified by addition of sufficient CO to the calibration system so as to rapidly convert all the OH to HO₂ (Reaction R14) and the HO₂ signal was observed to double in the presence of CO. The radicals sampled, or converted from HO₂, were electronically excited at 308 nm, approximately 13 cm below the sampling nozzle using a tuneable, 5 KHz pulse repetition frequency laser (Nd: YAG pumped Ti: Sapphire, Photonics Industries) with the fluorescence at the same wavelength detected perpendicular to the laser axis by a filtered (Barr Associates filter, transmission > 50 % at 308 nm) channel photo-multiplier, CPM, (Perkin Elmer) and gated-photon counting.

During the HCCT-2010 campaign one FAGE fluorescence cell was also used to measure both radical species. The cell was operated from the top of a 22 m high tower to

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

co-locate with hill-cap cloud measurements and ensure that the radical measurements were performed in full cloud. As a result of these requirements a smaller cell, based on the University of Leeds aircraft FAGE fluorescence cell (Commane et al., 2010), was used to make sequential measurements of OH and HO₂ (Fig. 1b); operational details are provided in Table 1. NO (10 SCCM) was injected into this cell via 3.2 mm ID stainless tubing inserted into the centre of the ambient air stream. This configuration resulted in a high conversion of HO₂ to OH (~ 90%). Ambient air was drawn into the cell through a 1 mm diameter pinhole nozzle into a 4.5 cm (ID) stainless steel cylinder. The cell was held at 1 Torr and was connected to the roots-rotary pump system described above via 30 m of flexible hosing (5 cm ID). Laser light was delivered from the Nd : YAG pumped Ti : Sapphire laser system to the cell via a 30 m fibre optic. The distance between sampling nozzle and detection was 18 cm with the NO injected ~ 8 cm below the nozzle.

The third FAGE cell tested for an RO₂ interference was a recently developed fluorescence cell designed for the detection of RO₂ radicals, alongside OH and HO₂, using the “RO_xLIF” methodology outlined by Fuchs et al. (2008). The RO₂ cell is operated in two modes, providing a measurement of the sum of OH + HO₂ in HO_x mode and the sum of OH + HO₂ + RO₂ in RO_x mode. Experiments were run on this third FAGE cell to determine the magnitude of the HO₂ interference suffered from a variety of RO₂ species in the HO_x mode.

A similar FAGE fluorescence cell as the one described above (Fig. 1a) was modified by coupling it to a differentially pumped reaction tube (held at approximately 30 Torr) to allow for conversion of RO₂ radicals to OH (Fig. 1c). The reaction tube is an 83 cm high, 6.4 cm diameter aluminium tube which has been coated with halocarbon wax to minimise radical wall losses. Ambient air (7.5 SLM) is drawn into the reaction tube through a 1 mm diameter pinhole drilled into a thin (1 mm thickness), flat plate aluminium inlet nozzle. In HO_x mode, 250 SCCM of CO (5% in N₂, BOC) is flowed into the centre of the reaction tube just beneath the inlet (~ 2 cm below) via a 6.4 mm (ID) stainless steel tube. Hydroxyl radicals are converted to HO₂ by reaction with CO (Reaction R14) as

Sensitivity of Laser Induced Fluorescence Instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

they pass through the reaction tube. Air (~ 5 SLM) from the reaction tube is sampled by the FAGE detection cell (held at approximately 1.5 Torr) via a 4 mm diameter pinhole nozzle sat on a 5 cm tall turret. Ambient HO_2 (and ambient OH which was converted to HO_2 in the reaction tube) is titrated to OH by NO injected into the cell 7.5 cm below the nozzle and detected by LIF; 100 SCCM of NO was injected into this fluorescence cell to maximise the conversion of HO_2 to OH. In RO_x mode, 25 SCCM of a 500 ppmv NO standard in N_2 (BOC) was added to the CO flow to promote conversion of RO_2 to OH (Reactions R3–R5); the excess CO present rapidly converts OH to HO_2 (Reaction R14) and helps to minimise the overall loss of the radicals to the walls of the reaction tube. Ambient RO_2 , HO_2 and OH radicals (converted to HO_2 in the reaction tube) enter the FAGE detection cell, are reconverted to OH by NO and detected as described above.



2.2 Time-resolved experiments using laser flash photolysis


The time-resolved setup was based on a laser-induced pump and probe OH reactivity technique developed by Sadanaga et al. (2004) which uses pulsed 266 nm light to photolyse ozone in a flow tube to generate $\text{O}(^1\text{D})$ and, by the subsequent reaction of $\text{O}(^1\text{D})$ with H_2O vapour, OH radicals (Reaction R1–2). The flow tube used here was 173 cm in length with an internal diameter of 5 cm; a schematic of the experimental set-up is shown in Fig. 2. The total flow was typically 10 SLM and the pressure in the flow tube was 300 Torr, which was controlled by a valve throttling a rotary pump (Leybold). A FAGE cell was located approximately halfway along the flow tube, held perpendicular to the flow tube, and sampled the gas flow through a 1 mm diameter pinhole nozzle that was located within 1 cm of the central axis of the flow tube. A YAG laser (Spectron SL803) was used to generate $\sim 10 \text{ mJ pulse}^{-1}$ of 266 nm photolysis radiation with a 10 ns pulse width; the beam profile was shaped using a Galilean telescope to produce a collimated beam with a diameter of ~ 2 cm and directed along the flow tube

Pyrex 5 L bulbs. Pressure gauges (MKS) were used to determine the bulb concentrations and the pressure in the flow tube and FAGE cell.

The OH generated (approximately 10^{10} molecule cm^{-3}) via the photolysis of ozone in the presence of H_2O vapour (Reactions R1–2) reacted rapidly with the added reagents in the presence of O_2 forming peroxy radicals (Reaction R6) or in the case of methanol, HO_2 formed via the following reactions:



or



OH reacts with methanol, predominantly forming CH_2OH (reported yields of 0.75–0.85, Atkinson et al., 2004) (Reaction R15) which then rapidly reacts with O_2 (9.6×10^{-12} cm^3 molecule $^{-1}$ s $^{-1}$) (Atkinson et al., 2004) to form HO_2 (Reaction R16). The other, minor, abstraction channel produces CH_3O , which reacts slower with O_2 (1.92×10^{-15} cm^3 molecule $^{-1}$ s $^{-1}$) (Atkinson et al., 2004) to produce HO_2 (Reaction R17, 18). HO_2 generated in the system was detected by adding nitric oxide (NO – 99.95 %, BOC) to the FAGE expansion cell (Fig. 2) to titrate to OH for subsequent detection (Reaction R5). The NO flow, controlled by a mass flow controller (Brookes) (0–50 SCCM), was injected into the centre of the FAGE cell, via 3.2 mm stainless steel tubing, approximately 13.75 cm below the pinhole. The fluorescence signal observed when NO is added to the expansion cell derives from OH and converted HO_2 ($\text{OH} + \alpha\text{HO}_2$), where α is equal to the titration efficiency of Reaction (R5), which is a function of the amount of NO added and the contact time in the expansion cell. For complete conversion of HO_2 to OH in the detection cell α will equal 1. If this is the case, in the presence and absence of methanol there should be no overall change in the initial fluorescence signal when NO was added as the OH lost in Reaction (R15) is rapidly converted to HO_2

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



interference) using Eq. (1):

$$\text{Relative OH yield} = \frac{\text{HO}_x \text{ signal}_{(\text{reagent})} - \text{HO}_2 \text{ signal}}{\text{HO}_2 \text{ signal}} \quad (1)$$

The flows of hydrocarbons were adjusted so that equivalent OH reactivities ($k_{\text{HC}+\text{OH}}[\text{HC}]$) for each of the hydrocarbons tested were used to ensure that any other loss of OH in the turbulent flow reactor (e.g. loss to walls) did not bias the relative yields determined.

In a number of experiments the NO concentration added to detection cell A was varied and the ratio of the OH signal observed for propane-derived RO₂ radicals relative to ethene-derived RO₂ radicals were compared and are shown in Table 1 and Fig. 6. As the NO concentration was reduced the interference from alkene-derived RO₂ radicals decreased. By varying [NO], it becomes possible to discriminate ambient RO₂ radicals from ambient HO₂ radicals and this is discussed further in Sect. 4.2.

3.2 Time-resolved experiments

To determine the absolute yield of OH from different RO₂ radicals in the presence of NO, a range of RO₂ radicals (or HO₂ in the case of methanol) were generated by the addition of different parent hydrocarbons to the flow tube described in Sect. 2.2 coupled to a FAGE cell in which there was sufficient time for complete conversion of RO₂ to OH. The time-resolved OH signals observed for a selection of RO₂ species tested are shown in Fig. 3, and Table 2 summarises the OH yields for all RO₂ investigated.

As the initial OH concentration generated and subsequent HO₂ or RO₂ concentration generated within the flow tube were uncalibrated, the absolute OH yields within the FAGE expansion cell from the different RO₂ species were determined by comparing with the OH signal observed from HO₂ generated in the methanol experiments which has a 100% yield. An exponential function of the form: $y = y_0 + A \times \exp(-B \times x)$ was fitted to each OH temporal profile associated with the different RO₂ species investigated. To

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



determine the relative yields of OH, the ratio of the *A* factor for each fit relative to the *A* factor determined for the methanol fit was calculated using Eq. (2):

$$\text{Relative OH yield} = A \text{ factor}_{(\text{reagent})} : A \text{ factor}_{(\text{methanol})} \quad (2)$$

In agreement with Fuchs et al. (2011), a large OH yield from alkene-derived RO₂ radicals was observed (see Table 2) when NO was present in the FAGE cell. Smaller, but still significant, OH yields were also observed for RO₂ radicals derived from cyclohexane, *n*-butane and *n*-pentane (Table 2); the OH signal observed for propane-derived RO₂ radicals was negligible (upper limit of 4 %).

In several experiments, it was found that ethene and propene-derived RO₂ radicals when compared to HO₂ from methanol had OH yields greater than one. The formation of β hydroxy peroxy radicals is fast in the flow tube, and, if complete RO₂ titration to HO₂ and ultimately to OH is occurring in the FAGE cell then the ratio of the OH signals observed in the presence of ethene, propene and methanol is expected to equal one. A value greater than one suggests incomplete conversion of methanol to HO₂ in the flow tube. It was observed in experiments where the Pyrex bulb containing methanol was left for a full day before use to allow for mixing (such an experiment is displayed in Fig. 3) rather than just a couple of hours, that yields close to one were obtained indicating that in several of the experiments there may have been insufficient methanol reaching the flow tube owing to extremely slow mixing of the gas bulb. To ensure that the results are not biased by a possible problem with methanol, the third column in Table 2 shows the OH yields referenced with respect to ethene (calculated using Eq. 3):

$$\text{Relative OH yield} = A \text{ factor}_{(\text{reagent})} : A \text{ factor}_{(\text{ethene})} \quad (3)$$

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion


4 Discussion

4.1 Time-resolved model-measurement comparison

Under conditions optimised for complete conversion of RO₂ radicals to OH in a FAGE cell with added NO, i.e. very long reaction times, the yield of HO₂ from a number of alkene-derived RO₂ species compares favourably to the MCMv3.2 predictions of the OH yield determined using Eq. (4) after a reaction time of 9.8 ms as shown in Fig. 4 and Table 2, suggesting that the yield of HO₂ from other RO₂ species not measured here can be derived with some confidence from MCM predictions.

$$\text{MCM OH yield} = \frac{\text{modelled [OH] generated}}{\text{model initialised [RO}_2\text{]}} \quad (4)$$

For > C₃ alkane-derived RO₂ species, the MCM also predicts a non-zero HO₂ yield. For these species, reaction with NO produces an alkoxy radical which can react with O₂ or isomerise forming a β-hydroxyalkylperoxy radical in the presence of O₂, which for the case of *n*-butane derived peroxy radical is:



The alkoxy radical, C₄H₉O, may also react with NO under FAGE conditions:



As shown in Reactions (R8)–(R11) the β-hydroxyalkylperoxy radical can react further with NO and decompose rapidly in the presence of O₂ to form HO₂. However, as seen in Fig. 4, the MCM over-predicts the yield of HO₂ at 298 K from *n*-pentane and cyclohexane derived peroxy radicals, and under-predicts the OH yield from *n*-butane-derived

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

alkanes. The modelled to measured agreement for *n*-pentane and cyclohexane derived RO₂ radicals can be improved if the rate coefficient for isomerisation (Reaction R21) is reduced by assuming a lower temperature; it was found by varying the temperature in the model that 255 K provided the best agreement for all RO₂ species considered (Fig. 4). In the case of cyclohexane, the rate coefficient for isomerisation (taken from the MCMv3.2) decreases from $6.3 \times 10^4 \text{ s}^{-1}$ to $2.1 \times 10^3 \text{ s}^{-1}$ as the temperature was reduced from 298 K to 255 K. Stevens et al. (1994) report a temperature of 245 K within the Penn. State FAGE instrument as an airstream enters the detection cell and accelerates to velocities of $> 300 \text{ ms}^{-1}$; at the laser detection axis the velocity is reduced to $\sim 50 \text{ ms}^{-1}$ and the air temperature increases to ambient levels once more. Similarly, measurements of rotational temperatures and computational fluid dynamic (CFD) calculations performed to determine the temperature and density profiles of an airstream within the Leeds FAGE detection cells (Fig. 1a) suggest that air temperatures drop as low as 25 K in the first 2 cm in the detection cell beneath the pinhole as the airstream expands supersonically and reaches velocities of 750 ms^{-1} before slowing and increasing back to ambient temperatures at the detection axis (Creasey et al., 1997b). Taking these temperature profiles into account, it is expected that the mean temperature experienced between pinhole and the detection axis will be below ambient and if this is the case the rate coefficient for isomerisation will slow considerably (Orlando et al., 2003). At lower temperatures the reaction between an alkoxy radical and NO (Reaction R19) can begin to compete with the isomerisation (Reaction R21) and can, as a result, lower the overall OH yield observed from these RO₂ radicals. This effect reduces the agreement between the experimental and modelled OH yield from *n*-butane-derived RO₂ further suggesting that the rate coefficient for isomerisation of the C₄H₉O alkoxy radical may actually be faster than assumed in the model. There is very little information on the temperature dependence associated with the rate of β hydroxyalkoxy decomposition in the literature. A theoretical temperature dependence for the rate of decomposition of

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



extent of the interference suffered is directly proportional to residence time within the jet and inversely proportional to the mean temperature experienced by the jet (Eq. 6). The level of interference suffered with respect to [NO] is complex. Increasing the concentration will increase the rates of Reactions (R3) and (R5) but also increases the rate of Reaction (R19). For alkoxy radicals which display a strong temperature dependence with respect to isomerisation, as is the case for the alkoxy radical derived from cyclohexane (CHEXO), increasing NO concentrations beyond a certain concentration may actually lead to a reduction in the level of interference observed as R19 begins to competes effectively with R21. Model simulations looking at the yield of OH from cyclohexane-derived RO₂ radicals predict that at a residence time of 9.8 ms (time over which time-resolved experiments were run) the yield of OH will increase with increasing [NO] until a NO concentration of 1.2×10^{14} molecule cm⁻³ is reached and then the yield will begin to decrease as [NO] increases further. Note, if the residence time is increased, less NO is required to achieve the maximum yield and vice versa. Under the experimental conditions discussed in this paper (i.e. [NO] $\leq 1 \times 10^{14}$ molecule cm⁻³), the OH yield should have been directly proportional to [NO]:

$$\text{Interference} \propto \frac{\text{Residence time} \cdot [\text{NO}]}{\text{Temperature}} \quad (6)$$

Fuchs et al. (2011) observed a large under-prediction of the OH yield from cyclohexane-derived RO₂ radicals in the presence of NO and suggested that the model under-prediction for the yield of OH from this species may reflect a missing ring opening mechanism in the MCM which could promote further HO₂ formation. Fuchs et al. (2011) used MCMv3.1 which did not contain a ring opening mechanism to estimate the expected level of interference in the Julich FAGE system. An additional degradation pathway for CHEXO which includes a ring opening route, is included in MCMv3.2 leading to the yield of HO₂ (and ultimately OH, following further reaction) from cyclohexane-derived RO₂ radicals approximately doubling when switching from MCMv3.1 to MCMv3.2 chemistry.

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

A lower effective yield of OH from cyclohexane derived RO₂ radicals (relative to ethene derived RO₂ radicals) was observed in the time-resolved experiments (Table 2) compared to experiments on cell C (Table 1). The model is able to reproduce the relative yields observed in both experiments if the concentration of NO that mixes into the jet expansion in cell C is lower (by a factor of 10) than the [NO] that was actually injected; the required reduction in modelled NO for cell C was consistent for all RO₂ species studied. Under this scenario, the competition of R19 with R21 is reduced leading to an increased yield of OH in cell C experiments.

4.2 Minimising the RO₂ interference further

As highlighted in Table 1, a decrease in the amount of NO injected into the cell reduces the OH yield from ethene-derived RO₂ radicals. Reducing the sensitivity of the instrument to the interference, however, leads to a concomitant reduction in HO₂ sensitivity. As only one NO molecule is required to titrate one HO₂ radical to OH, whilst two or more are required for RO₂ to OH titration, it is possible to begin to discriminate between HO₂ and RO₂ by reducing the amount of NO mixed into the jet as shown in Fig. 6. At an NO concentration of 1×10^{13} molecule cm⁻³, approximately twenty HO₂ radicals titrate to OH for one RO₂ radical conversion to OH; determined from the ratio: relative OH yield (propane): relative OH yield (ethene) with “relative OH yield” calculated using Eq. (1). At this NO concentration the 5 min limit of detection of the instrument for HO₂ will be $\sim 4 \times 10^6$ molecule cm⁻³ and, although higher than detection limits from earlier campaigns (e.g. the HO₂ LOD during the SOAPEX campaign which took place in Cape Grim in Australia was 5.4×10^5 molecule cm⁻³ for 2.5 min integration time) (Creasey et al., 2003), the instrument remains sufficiently sensitive for ambient HO₂ detection with minimal RO₂ interference ($\sim 5\%$). It should be noted that good agreement between the MCMv3.2 model and observations can only be achieved if it is assumed that 5.5 times less NO is mixed fully into the air sample within the FAGE cell than is actually injected.

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



As demonstrated by Fig. 6, by varying the amount of NO injected it is possible to switch from conditions where certain RO₂ types are efficiently converted to OH (NO > 5 × 10¹³ molecule cm⁻³) to conditions where the conversion is poor (NO < 1 × 10¹³ molecule cm⁻³). With knowledge of the conversion efficiency of RO₂ and HO₂ at different NO concentrations, changing the NO flow during ambient measurements can selectively provide a measurement of the concentration of RO_{2i} and HO₂ by solving simultaneous Eqs. (7 and 8):

$$\text{HO}_x \text{ signal}_{\text{low} [\text{NO}]} = C_{\text{HO}_2, \text{low} [\text{NO}]} \cdot ([\text{HO}_2] + \alpha_{\text{low} [\text{NO}]}[\text{RO}_{2i}]) \quad (7)$$

$$\text{HO}_x \text{ signal}_{\text{high} [\text{NO}]} = C_{\text{HO}_2, \text{high} [\text{NO}]} \cdot ([\text{HO}_2] + \alpha_{\text{high} [\text{NO}]}[\text{RO}_{2i}]) \quad (8)$$

Where HO_x signal is the fluorescence signal observed in cts s⁻¹ mW⁻¹, C_{HO₂} is the sensitivity of the instrument to HO₂ (determined by calibration) at a particular NO flow in units of cm³ molecule⁻¹ cts⁻¹ mW⁻¹ and α is the mean fractional contribution of RO_{2i} at a selected [NO].

During a recent field project, the Clean air for London campaign (ClearLo), this approach was adopted during ambient measurements. The NO concentration injected into a FAGE cell (cell type A) used during the campaign for sequential measurements of OH and HO₂ was varied between ~ 1 and 9 × 10¹³ molecule cm⁻³; a measurement of the total [RO₂] was determined simultaneously using the RO_xLIF cell C operating in RO_x mode. The campaign average diurnal profile of HO₂, alkene/aromatic or long-chain alkane-derived RO₂ and short-chain alkane-derived RO₂ radicals selectively measured is provided in Fig. 7. An alternative approach to partial speciation of RO₂ radical classes would be to use two FAGE cells in which the RO₂ interference is minimised in the first (e.g. cell A, run at a low [NO]) and maximised in the second (e.g. cell C, HO_x mode, run at a high [NO]).

4.3 Impact on previous field studies

The University of Leeds ground-based FAGE instrument has been operational since 1996 and has taken part in 17 campaigns. In some of the earlier campaigns good conversion of HO₂ to OH was achieved as two independent cells were used (Creasey et al., 2002; Creasey et al., 2003; Smith et al., 2006), with the conditions of one cell optimised for HO₂ detection, and so a significant portion of interfering RO₂i, if present, may also have been titrated to OH, constituting an interference. Many of the previous campaigns took place under relatively clean, unpolluted conditions, for example EASE-96 (Carslaw et al., 1999a), EASE-97 (Creasey et al., 2002), SOAPEX (Creasey et al., 2003), NAMBLEX (Smith et al., 2006), CHABLIS (Bloss et al., 2010), RHAMBLE (Whalley et al., 2010) where the concentrations of RO₂i are likely low and methyl peroxy radicals, which do not give an interference (Ren et al., 2004), were expected to be the dominant RO₂ species; e.g. during EASE-96 the model predicted that 92 % of peroxy radicals present were either HO₂ (53 %) or CH₃O₂ (39 %) during unpolluted conditions (Carslaw et al., 1999a). Similarly, for the SOS project (Vaughan et al., 2012), which took place in Cape Verde, models predicted that ~ 90 % of peroxy radicals were either HO₂ or CH₃O₂. In general, models run for these campaigns tended to over-predict HO₂ despite additional HO₂ loss mechanisms such as reaction with halogen oxides and/or heterogeneous loss to aerosol surfaces in the model description. In contrast, under polluted, urban conditions (e.g. PUMA, Heard et al., 2004, TORCH-1, Emmerson et al., 2007) models either significantly under-predicted HO₂ observations (PUMA) (Emmerson et al., 2005) or were in relatively good agreement (TORCH-1) (Emmerson et al., 2007). If elevated concentrations of alkene-derived, aromatic-derived and higher-alkane derived RO₂ species were present, the true ambient HO₂ concentrations, as opposed to HO₂^{*}, were likely lower than reported. It is possible, although difficult to verify without observations of speciated RO₂ that the conclusions drawn from these observations, for example, that additional HO₂ sources in models are required to replicate observations, may be in error.

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Under the operating conditions employed during the OP3 campaign, the instrument was relatively insensitive to detection of RO₂ species. The experiments presented here reveal a 17 % yield of OH due to the decomposition of ethene-derived RO₂ in the presence of NO in the FAGE detection cell under OP3 conditions. This provides an upper limit to the HO₂ yield from RO₂ species during OP3 as, under conditions in which the interference signal was maximised (Sect. 3.2), ethene-derived RO₂ species provided the largest HO₂ yield compared with other RO₂ species. Model simulations (Whalley et al., 2011) suggested that up to 2.1×10^8 molecule cm⁻³ of potentially interfering RO₂ species were present at solar noon during OP3 (with isoprene derived peroxy radicals contributing ~ 60 % to this total), and thus up to 3.5×10^7 molecule cm⁻³ of the HO₂ concentration may be attributed to these species (~ 10 % of the total HO₂ signal observed (Whalley et al., 2011)). Model comparisons with the radical measurements made during the campaign demonstrated a large missing OH source and over-predicted the HO₂ observations. The small positive bias on the HO₂ observations, owing to the small yield of HO₂ from RO₂ species, only serves to reduce the modelled to measured agreement further. For the HCCT-2010 campaign, the potential impact of the interfering RO₂ species is greater (Table 1, Fig. 5) owing to the smaller cell (with a longer inlet) and longer residence time employed. The campaign took place in a pine forest, close to the summit of Mount Schmücke in the Thüringer Wald mountain range in East Germany, during September and October 2010. VOC measurements were made downwind of the measurement site. Only low concentrations of isoprene (50 pptv) were detected, however, suggesting that the concentration of RO_{2i} were also low.

5 Conclusions and further work

Recent studies conducted on a number of different fluorescence cells used in the FAGE instrument at Leeds have demonstrated that alkene- and aromatic-derived RO₂ species can yield appreciable quantities of OH upon addition of NO in FAGE detection cells and, therefore, positively bias HO₂ observations if left uncorrected. Many FAGE groups

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



now report HO_2^* for comparison with atmospheric chemistry box models to include any interference from RO_2 . As demonstrated in this study, the magnitude of this interference is critically dependent on the cell design, quantity of NO used in the titration, the residence time and mean temperature of the air stream within the FAGE cell. The interference may be minimised by reducing NO concentrations and/or residence time, and although such a reduction will also reduce the sensitivity of the instrument to HO_2 (albeit to a lesser extent than the reduction in the sensitivity to RO_2 radicals) it will still be possible to detect ambient levels HO_2 using FAGE.

In laboratory, laser-flash photolysis experiments, under conditions optimised for complete conversion of RO_2 radicals to OH in a FAGE cell, the yield of HO_2 from a number of alkene-derived RO_2 species could be measured, and compared favourably with MCMv3.2 predictions. This suggests that the yield of HO_2 from other alkene-derived or aromatic-derived RO_2 species not tested here, but which are expected to exhibit high yields, could be determined from MCM predictions. The ability to discriminate between HO_2 and RO_2 radicals, as illustrated for the ClearLo project, is not only of great value for field measurements (and subsequent model comparisons), but such instrumentation may be used to selectively determine the yield of HO_2 in laboratory experiments under conditions where RO_2 radicals may also be present. Important applications, for example, would be the experimental verification of a significant prompt HO_2 yield from OH initialised isoprene oxidation, as proposed by Peeters et al. (2009) or prompt HO_2 yields from OH initialised oxidation of aromatics (Nehr et al., 2012).

This study demonstrates that some of the previous HO_2 measurements that depend upon chemical titration to OH by NO may suffer an interference due to partial detection of RO_2 radicals. Under conditions where there are significant alkene, aromatic or long-chain alkanes present, the HO_2^* concentration which was measured will have been higher than the HO_2 concentration that was actually present. Models have over-estimated HO_2 concentrations under such conditions, and this over-estimation would only increase if the observations of HO_2 were corrected for the interference suggesting there is a major gap in our understanding of the chemistry controlling these radicals.

Supplementary material related to this article is available online at:
[http://www.atmos-meas-tech-discuss.net/6/6249/2013/
amtd-6-6249-2013-supplement.pdf](http://www.atmos-meas-tech-discuss.net/6/6249/2013/amtd-6-6249-2013-supplement.pdf).

Acknowledgements. We would like to thank the National Centre for Atmospheric Science (NCAS) for financial support and EUROCHAMP is acknowledged for PWS.

References

- Atkinson, R., Baulch, D. L., Cox, R. A., Hampson, R. F., Kerr, J. A., Rossi, M. J., and Troe, J.: Evaluated kinetic, photochemical and heterogeneous data for atmospheric chemistry, 5. IUPAC subcommittee on gas kinetic data evaluation for atmospheric chemistry, *J. Phys. Chem. Ref. Data*, 26, 521–1011, 1997.
- Atkinson, R., Baulch, D. L., Cox, R. A., Crowley, J. N., Hampson, R. F., Hynes, R. G., Jenkin, M. E., Rossi, M. J., and Troe, J.: Evaluated kinetic and photochemical data for atmospheric chemistry: Volume I – gas phase reactions of O_x, HO_x, NO_x and SO_x species, *Atmos. Chem. Phys.*, 4, 1461–1738, doi:10.5194/acp-4-1461-2004, 2004.
- Bloss, C., Wagner, V., Jenkin, M. E., Volkamer, R., Bloss, W. J., Lee, J. D., Heard, D. E., Wirtz, K., Martin-Reviejo, M., Rea, G., Wenger, J. C., and Pilling, M. J.: Development of a detailed chemical mechanism (MCMv3.1) for the atmospheric oxidation of aromatic hydrocarbons, *Atmos. Chem. Phys.*, 5, 641–664, doi:10.5194/acp-5-641-2005, 2005.
- Bloss, W. J., Camredon, M., Lee, J. D., Heard, D. E., Plane, J. M. C., Saiz-Lopez, A., Bauguitte, S. J.-B., Salmon, R. A., and Jones, A. E.: Coupling of HO_x, NO_x and halogen chemistry in the antarctic boundary layer, *Atmos. Chem. Phys.*, 10, 10187–10209, doi:10.5194/acp-10-10187-2010, 2010.
- Carlsaw, N., Creasey, D. J., Heard, D. E., Lewis, A. C., McQuaid, J. B., Pilling, M. J., Monks, P. S., Bandy, B. J., and Penkett, S. A.: Modeling OH, HO₂, and RO₂ radicals in the marine boundary layer – 1. Model construction and comparison with field measurements, *J. Geophys. Res.-Atmos.*, 104, 30241–30255, doi:10.1029/1999jd900783, 1999a.

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Carlsaw, N., Jacobs, P. J., and Pilling, M. J.: Modeling OH, HO₂, and RO₂ radicals in the marine boundary layer 2. Mechanism reduction and uncertainty analysis, *J. Geophys. Res.-Atmos.*, 104, 30257–30273, doi:10.1029/1999jd900782, 1999b.

5 Cleary, P. A., Romero, M. T. B., Blitz, M. A., Heard, D. E., Pilling, M. J., Seakins, P. W., and Wang, L.: Determination of the temperature and pressure dependence of the reaction OH + C₂H₄ from 200–400 K using experimental and master equation analyses, *Phys. Chem. Chem. Phys.*, 8, 5633–5642, doi:10.1039/B612127f, 2006.

10 Commane, R., Floquet, C. F. A., Ingham, T., Stone, D., Evans, M. J., and Heard, D. E.: Observations of OH and HO₂ radicals over West Africa, *Atmos. Chem. Phys.*, 10, 8783–8801, doi:10.5194/acp-10-8783-2010, 2010.

Creasey, D. J., HalfordMaw, P. A., Heard, D. E., Pilling, M. J., and Whitaker, B. J.: Implementation and initial deployment of a field instrument for measurement of OH and HO₂ in the troposphere by laser-induced fluorescence, *J. Chem. Soc. Faraday T.*, 93, 2907–2913, doi:10.1039/A701469d, 1997a.

15 Creasey, D. J., Heard, D. E., Pilling, M. J., Whitaker, B. J., Berzins, M., and Fairlie, R.: Visualisation of a supersonic free-jet expansion using laser-induced fluorescence spectroscopy: Application to the measurement of rate constants at ultralow temperatures, *Appl. Phys. B-Lasers O.*, 65, 375–391, doi:10.1007/s003400050285, 1997b.

20 Creasey, D. J., Heard, D. E., and Lee, J. D.: OH and HO₂ measurements in a forested region of north-western Greece, *Atmos. Environ.*, 35, 4713–4724, doi:10.1016/S1352-2310(01)00090-5, 2001.

Creasey, D. J., Heard, D. E., and Lee, J. D.: Eastern Atlantic Spring Experiment 1997 (EASE97) 1. Measurements of OH and HO₂ concentrations at Mace Head, Ireland, *J. Geophys. Res.-Atmos.*, 107, 4091, doi:10.1029/2001jd000892, 2002.

25 Creasey, D. J., Evans, G. E., Heard, D. E., and Lee, J. D.: Measurements of OH and HO₂ concentrations in the Southern Ocean marine boundary layer, *J. Geophys. Res.-Atmos.*, 108, 4475, doi:10.1029/2002jd003206, 2003.

Davis, D. D., Rodgers, M. O., Fischer, S. D., and Asai, K.: An experimental assessment of the O₃/H₂O interference problem in the detection of natural levels of OH via laser induced fluorescence, *Geophys. Res. Lett.*, 8, 69–72, 1981.

30 Emmerson, K. M., Carlsaw, N., Carpenter, L. J., E., H. D., Lee, J. D., and Pilling, M. J.: Urban atmospheric chemistry during the PUMA Campaign 1: Comparison of modelled OH and HO₂ concentrations with measurements, *J. Atmos. Chem.*, 52, 143–164, 2005.

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

- Emmerson, K. M., Carslaw, N., Carslaw, D. C., Lee, J. D., McFiggans, G., Bloss, W. J., Gravestock, T., Heard, D. E., Hopkins, J., Ingham, T., Pilling, M. J., Smith, S. C., Jacob, M., and Monks, P. S.: Free radical modelling studies during the UK TORCH Campaign in Summer 2003, *Atmos. Chem. Phys.*, 7, 167–181, doi:10.5194/acp-7-167-2007, 2007.
- 5 Faloon, I., Tan, D., Brune, W., Hurst, J., Barket, D., Couch, T. L., Shepson, P., Apel, E., Riemer, D., Thornberry, T., Carroll, M. A., Sillman, S., Keeler, G. J., Sagady, J., Hooper, D., and Paterson, K.: Nighttime observations of anomalously high levels of hydroxyl radicals above a deciduous forest canopy, *J. Geophys. Res.-Atmos.*, 106, 24315–24333, doi:10.1029/2000jd900691, 2001.
- 10 Fuchs, H., Holland, F., and Hofzumahaus, A.: Measurement of tropospheric RO₂ and HO₂ radicals by a laser-induced fluorescence instrument, *Rev. Sci. Instrum.*, 79, 084104, doi:10.1063/1.29687121, 2008.
- Fuchs, H., Bohn, B., Hofzumahaus, A., Holland, F., Lu, K. D., Nehr, S., Rohrer, F., and Wahner, A.: Detection of HO₂ by laser-induced fluorescence: calibration and interferences from RO₂ radicals, *Atmos. Meas. Tech.*, 4, 1209–1225, doi:10.5194/amt-4-1209-2011, 2011.
- 15 Fuchs, H., Dorn, H.-P., Bachner, M., Bohn, B., Brauers, T., Gomm, S., Hofzumahaus, A., Holland, F., Nehr, S., Rohrer, F., Tillmann, R., and Wahner, A.: Comparison of OH concentration measurements by DOAS and LIF during SAPHIR chamber experiments at high OH reactivity and low NO concentration, *Atmos. Meas. Tech.*, 5, 1611–1626, doi:10.5194/amt-5-1611-2012, 2012.
- 20 Hanisco, T. F., Smith, J. B., Stimpfle, R. M., Wilmouth, D. M., Anderson, J. G., Richard, E. C., and Bui, T. P.: In situ observations of HO₂ and OH obtained on the NASA ER-2 in the high-CIO conditions of the 1999/2000 Arctic polar vortex, *J. Geophys. Res.-Atmos.*, 107, 8283, doi:10.1029/2001jd001024, 2002.
- 25 Hard, T. M., O'Brien, R. J., Cook, T. B., and Tsongas, G. A.: Interference Suppression in OH Fluorescence Detection, *Appl. Optics*, 18, 3216–3217, doi:10.1364/Ao.18.003216, 1979.
- Hard, T. M., O'Brien, R. J., Chan, C. Y., and Mehrabzadeh, A. A.: Tropospheric Free-Radical Determination by Fage, *Environ. Sci. Technol.*, 18, 768–777, doi:10.1021/Es00128a009, 1984.
- Heard, D. E. and Pilling, M. J.: Measurement of OH and HO₂ in the troposphere, *Chem. Rev.*, 30, 5163–5198, doi:10.1021/Cr020522s, 2003.
- Heard, D. E., Carpenter, L. J., Creasey, D. J., Hopkins, J. R., Lee, J. D., Lewis, A. C., Pilling, M. J., Seakins, P. W., Carslaw, N., and Emmerson, K. M.: High levels of the

**Sensitivity of Laser
Induced
Fluorescence
instruments**

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

hydroxyl radical in the winter urban troposphere, *Geophys. Res. Lett.*, **31**, L18112, doi:10.1029/2004gl020544, 2004.

Heicklen, J.: The Decomposition of Alkyl Nitrites and the Reactions of Alkoxy Radicals, in: *Advances in Photochemistry*, edited by: Volman, D. H., Hammond, G. S., and Gollnick, K., Vol. 14, John Wiley & Sons, Inc., Hoboken, NJ, USA, doi:10.1002/9780470133446.ch4, 2007.

Hewitt, C. N., Lee, J. D., MacKenzie, A. R., Barkley, M. P., Carslaw, N., Carver, G. D., Chappell, N. A., Coe, H., Collier, C., Commane, R., Davies, F., Davison, B., DiCarlo, P., Di Marco, C. F., Dorsey, J. R., Edwards, P. M., Evans, M. J., Fowler, D., Furneaux, K. L., Gallagher, M., Guenther, A., Heard, D. E., Helfter, C., Hopkins, J., Ingham, T., Irwin, M., Jones, C., Karunaharan, A., Langford, B., Lewis, A. C., Lim, S. F., MacDonald, S. M., Mahajan, A. S., Malpass, S., McFiggans, G., Mills, G., Misztal, P., Moller, S., Monks, P. S., Nemitz, E., Nicolas-Perea, V., Oetjen, H., Oram, D. E., Palmer, P. I., Phillips, G. J., Pike, R., Plane, J. M. C., Pugh, T., Pyle, J. A., Reeves, C. E., Robinson, N. H., Stewart, D., Stone, D., Whalley, L. K., and Yin, X.: Overview: oxidant and particle photochemical processes above a south-east Asian tropical rainforest (the OP3 project): introduction, rationale, location characteristics and tools, *Atmos. Chem. Phys.*, **10**, 169–199, doi:10.5194/acp-10-169-2010, 2010.

Hofzumahaus, A., Aschmutat, U., Hessling, M., Holland, F., and Ehhalt, D. H.: The measurement of tropospheric OH radicals by laser-induced fluorescence spectroscopy during the POPCORN field campaign, *Geophys. Res. Lett.*, **23**, 2541–2544, doi:10.1029/96gl02205, 1996.

Holland, F., Hofzumahaus, A., Schafer, R., Kraus, A., and Patz, H. W.: Measurements of OH and HO₂ radical concentrations and photolysis frequencies during BERLIOZ, *J. Geophys. Res.-Atmos.*, **108**, 8246, doi:10.1029/2001jd001393, 2003.

Ianni, J. C.: available at: www.kintecus.com (last access: 10 June 2013), in Windows version 2.80 ed., 2002.

Jenkin, M. E., Saunders, S. M., and Pilling, M. J.: The tropospheric degradation of volatile organic compounds: a protocol for mechanism development, *Atmos. Environ.*, **31**, 81–104, doi:10.1016/S1352-2310(96)00105-7, 1997.

Jenkin, M. E., Saunders, S. M., Wagner, V., and Pilling, M. J.: Protocol for the development of the Master Chemical Mechanism, MCM v3 (Part B): tropospheric degradation of aromatic volatile organic compounds, *Atmos. Chem. Phys.*, **3**, 181–193, doi:10.5194/acp-3-181-2003, 2003.

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

- Kanaya, Y., Sadanaga, Y., Matsumoto, J., Sharma, U. K., Hirokawa, J., Kajii, Y., and Akimoto, H.: Nighttime observation of the HO₂ radical by an LIF instrument at Oki island, Japan, and its possible origins, *Geophys. Res. Lett.*, 26, 2179–2182, doi:10.1029/1999gl900475, 1999.
- Kukui, A. and Le Bras, G.: Theoretical study of the thermal decomposition of several beta-chloroalkoxy radicals, *Phys. Chem. Chem. Phys.*, 3, 175–178, doi:10.1039/B007644i, 2001.
- Lu, K. D., Rohrer, F., Holland, F., Fuchs, H., Bohn, B., Brauers, T., Chang, C. C., Häseler, R., Hu, M., Kita, K., Kondo, Y., Li, X., Lou, S. R., Nehr, S., Shao, M., Zeng, L. M., Wahner, A., Zhang, Y. H., and Hofzumahaus, A.: Observation and modelling of OH and HO₂ concentrations in the Pearl River Delta 2006: a missing OH source in a VOC rich atmosphere, *Atmos. Chem. Phys.*, 12, 1541–1569, doi:10.5194/acp-12-1541-2012, 2012.
- Mao, J., Ren, X., Zhang, L., Van Duin, D. M., Cohen, R. C., Park, J.-H., Goldstein, A. H., Paulot, F., Beaver, M. R., Crounse, J. D., Wennberg, P. O., DiGangi, J. P., Henry, S. B., Keutsch, F. N., Park, C., Schade, G. W., Wolfe, G. M., Thornton, J. A., and Brune, W. H.: Insights into hydroxyl measurements and atmospheric oxidation in a California forest, *Atmos. Chem. Phys.*, 12, 8009–8020, doi:10.5194/acp-12-8009-2012, 2012.
- Mather, J. H., Stevens, P. S., and Brune, W. H.: OH and HO₂ measurements using laser-induced fluorescence, *J. Geophys. Res.-Atmos.*, 102, 6427–6436, doi:10.1029/96jd01702, 1997.
- Nehr, S., Bohn, B., and Wahner, A.: Prompt HO₂ formation following the reaction of OH with aromatic compounds under atmospheric conditions, *J. Phys. Chem. A*, 116, 6015–6026, doi:10.1021/Jp210946y, 2012.
- Orlando, J. J., Tyndall, G. S., and Wallington, T. J.: The atmospheric chemistry of alkoxy radicals, *Chem. Rev.*, 103, 4657–4689, doi:10.1021/Cr020527p, 2003.
- Ortgies, G., Gericke, K. H., and Comes, F. J.: Is UV laser-induced fluorescence a method to monitor tropospheric OH?, *Geophys. Res. Lett.*, 7, 905–908, doi:10.1029/Gl007i011p00905, 1980.
- Peeters, J., Nguyen, T. L., and Vereecken, L.: HO_x radical regeneration in the oxidation of isoprene, *Phys. Chem. Chem. Phys.*, 11, 5935–5939, 2009.
- Ren, X. R., Harder, H., Martinez, M., Faloon, I. C., Tan, D., Leshner, R. L., Di Carlo, P., Simpas, J. B., and Brune, W. H.: Interference testing for atmospheric HO_x measurements by laser-induced fluorescence, *J. Atmos. Chem.*, 47, 169–190, doi:10.1023/B:Joch.0000021037.46866.81, 2004.

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

Sadanaga, Y., Yoshino, A., Watanabe, K., Yoshioka, A., Wakazono, Y., Kanaya, Y., and Kajii, Y.: Development of a measurement system of OH reactivity in the atmosphere using a laser-induced pump and probe technique, *Rev. Sci. Instr.*, 75, 2648–2655, 2004.

Saunders, S. M., Jenkin, M. E., Derwent, R. G., and Pilling, M. J.: Protocol for the development of the Master Chemical Mechanism, MCM v3 (Part A): tropospheric degradation of non-aromatic volatile organic compounds, *Atmos. Chem. Phys.*, 3, 161–180, doi:10.5194/acp-3-161-2003, 2003.

Shirinzadeh, B., Wang, C. C., and Deng, D. Q.: Pressure-Dependence of Ozone Interference in the Laser Fluorescence Measurements of OH in the Atmosphere, *Appl. Optics*, 26, 2102–2105, 1987.

Smith, S. C., Lee, J. D., Bloss, W. J., Johnson, G. P., Ingham, T., and Heard, D. E.: Concentrations of OH and HO₂ radicals during NAMBLEX: measurements and steady state analysis, *Atmos. Chem. Phys.*, 6, 1435–1453, doi:10.5194/acp-6-1435-2006, 2006.

Stevens, P. S., Mather, J. H., and Brune, W. H.: Measurement of tropospheric OH and HO₂ by laser-induced fluorescence at low-pressure, *J. Geophys. Res.-Atmos.*, 99, 3543–3557, doi:10.1029/93jd03342, 1994.

Stone, D., Whalley, L. K., and Heard, D. E.: Tropospheric OH and HO₂ radicals: field measurements and model comparisons, *Chem. Soc. Rev.*, 41, 6348–6404, doi:10.1039/C2cs35140d, 2012.

Vaughan, S., Ingham, T., Whalley, L. K., Stone, D., Evans, M. J., Read, K. A., Lee, J. D., Moller, S. J., Carpenter, L. J., Lewis, A. C., Fleming, Z. L., and Heard, D. E.: Seasonal observations of OH and HO₂ in the remote tropical marine boundary layer, *Atmos. Chem. Phys.*, 12, 2149–2172, doi:10.5194/acp-12-2149-2012, 2012.

Whalley, L. K., Furneaux, K. L., Goddard, A., Lee, J. D., Mahajan, A., Oetjen, H., Read, K. A., Kaaden, N., Carpenter, L. J., Lewis, A. C., Plane, J. M. C., Saltzman, E. S., Wiedensohler, A., and Heard, D. E.: The chemistry of OH and HO₂ radicals in the boundary layer over the tropical Atlantic Ocean, *Atmos. Chem. Phys.*, 10, 1555–1576, doi:10.5194/acp-10-1555-2010, 2010.

Whalley, L. K., Edwards, P. M., Furneaux, K. L., Goddard, A., Ingham, T., Evans, M. J., Stone, D., Hopkins, J. R., Jones, C. E., Karunaharan, A., Lee, J. D., Lewis, A. C., Monks, P. S., Moller, S. J., and Heard, D. E.: Quantifying the magnitude of a missing hydroxyl radical source in a tropical rainforest, *Atmos. Chem. Phys.*, 11, 7223–7233, doi:10.5194/acp-11-7223-2011, 2011.

Whalley, L. K., Stone, D., George, I., Mertes, S., Van Pinxteren, D., Fomba, K. W., Herrmann, H., and Heard, D. E.: The influence of clouds on radical concentrations: observations of OH and HO₂ during the Hill Cap Cloud Thuringer (HCCT) campaign in 2010, to be submitted, 2013.

AMTD

6, 6249–6292, 2013

**Sensitivity of Laser
Induced
Fluorescence
instruments**

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Table 1. Experimentally determined OH yields (derived using Eq. 1) from peroxy radicals ($\text{RO}_2 \rightarrow \text{HO}_2 \rightarrow \text{OH}$) in continuous flow experiments for FAGE cells operated under fieldwork conditions.

Source of peroxy radicals	Flow of NO (SCCM)	Cell A, OH yield Residence time: ~ 0.9 ms ¹ Typical NO flow used during fieldwork: 50 SCCM ² Flow rate through pinhole: 4.8 SLM Cell Pressure: 0.9 Torr	Cell B, OH yield Residence time: ~ 1.9 ms ³ Typical NO flow used during fieldwork: 10 SCCM Flow rate through pinhole: 3 SLM Cell Pressure: 1 Torr	Cell C, OH yield Residence time: ~ 60 ms ³ Typical NO flow used during fieldwork: 100 SCCM Flow rate through pinhole: 3.5 SLM Cell Pressure: 1.5 Torr
Ethene	10	0.057 ± 0.033	0.463 ± 0.030	–
	20	0.073 ± 0.029	–	–
	30	0.098 ± 0.025	–	–
	40	0.157 ± 0.047	–	–
	50	0.172 ± 0.057	–	–
Methanol	100	–	–	0.947 ± 0.073
	50	0.756 ± 0.273	–	–
Isoprene	50	0.178 ± 0.075	–	0.849 ± 0.057
Propane	50	0.00 ± 0.053	0.00 ± 0.102	–
Methane	100	–	–	0.00 ± 0.091
Cyclohexane	100	–	–	0.606 ± 0.051
Toluene	100	–	–	0.874 ± 0.072

¹ Determined by computational fluid dynamics, for further details refer to Creasey et al. (1997b).

² Experiments during which the NO concentration was varied from 10–50 SCCM and compared to modelled OH yields (see Fig. 6) suggest that NO that mixes into the air flow is actually 5.5 times less than the NO that is injected.

³ Estimated from comparison of experimentally determined OH yield from ethane-derived RO_2 radicals and MCM-predicted yields (see Fig. 5).

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Table 2. OH yields in time-resolved experiments from peroxy radicals determined using Eqs. (2) and (3); the MCMv3.2 OH yield is provided in the final columns for comparison. The modelled OH yield was determined using Eq. (4) calculated after 9.8 ms integration time. The model was constrained with a $[\text{NO}] = 1 \times 10^{14}$ molecule cm^{-3} and a temperature = 298 K (fourth column) or $[\text{NO}] = 1 \times 10^{14}$ molecule cm^{-3} and a temperature = 255 K (final column).

Source of peroxy radicals	OH yield (referenced to methanol)	OH Yield (referenced to ethene)	MCM OH yield (referenced to initial $[\text{RO}_2]$) at 298 K	MCM OH yield (referenced to initial $[\text{RO}_2]$) at 255 K
Methanol	1.00 ± 0.08	0.85 ± 0.09	1.00	–
Isoprene	1.03 ± 0.11	0.92 ± 0.04	0.90	–
Ethene	1.17 ± 0.09	1.00 ± 0.08	0.99	0.90
Cyclohexane	0.45 ± 0.09	0.38 ± 0.08	0.74	0.36
Propane	0.042 ± 0.008	0.034 ± 0.008	0.01	–
Propene	1.17 ± 0.13	–	–	–
<i>n</i> -butane	0.35 ± 0.04	0.18 ± 0.01	0.13 (0.12)	0.12
<i>n</i> -pentane	–	0.48 ± 0.01	0.62 (0.49)	0.49

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

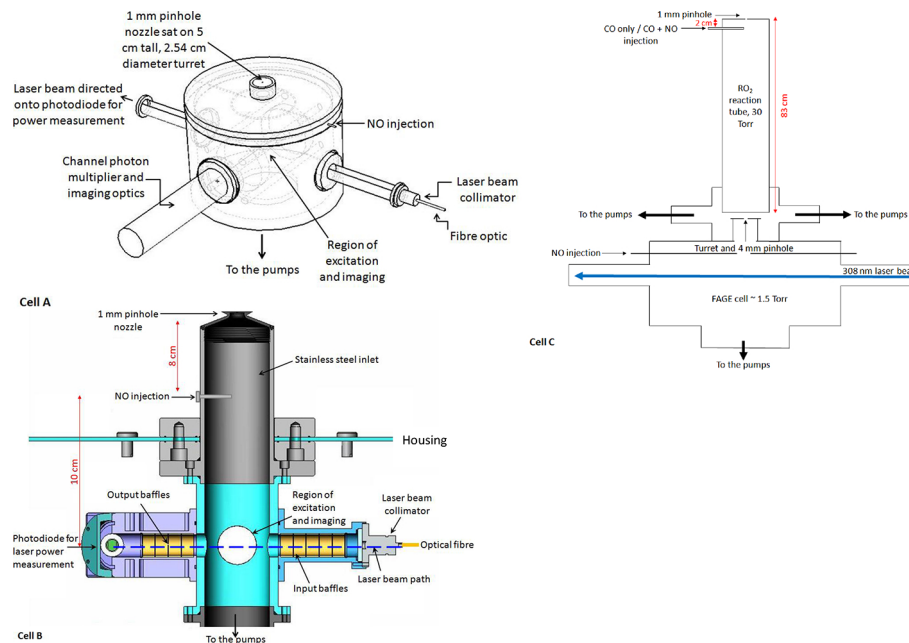


Fig. 1. Schematics highlighting the key features of the three FAGE cells tested. Cell A was used for sequential OH and HO₂ detection during the OP3 project; dotted line highlights internal cell components. Cell B was used to make sequential tower-based measurements of OH and HO₂ during the HCCT campaign. Cell C represents the coupling of a reaction tube to a FAGE cell (cell A design) for detection of RO₂ radicals by LIF, see text for further details.

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

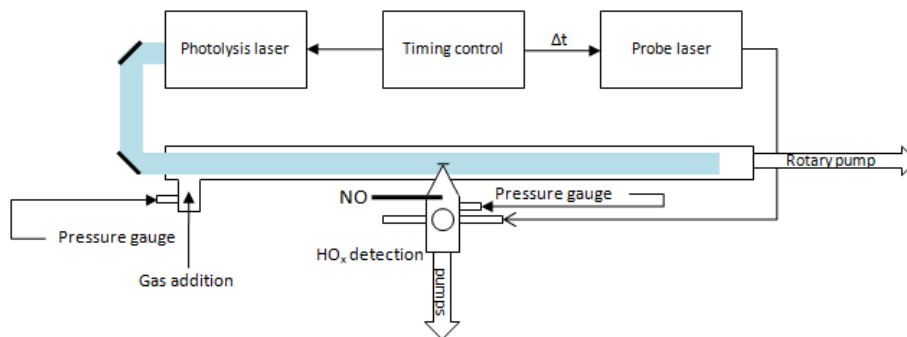


Fig. 2. Schematic highlighting the key features of the laser flash-photolysis time-resolved experimental set-up.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

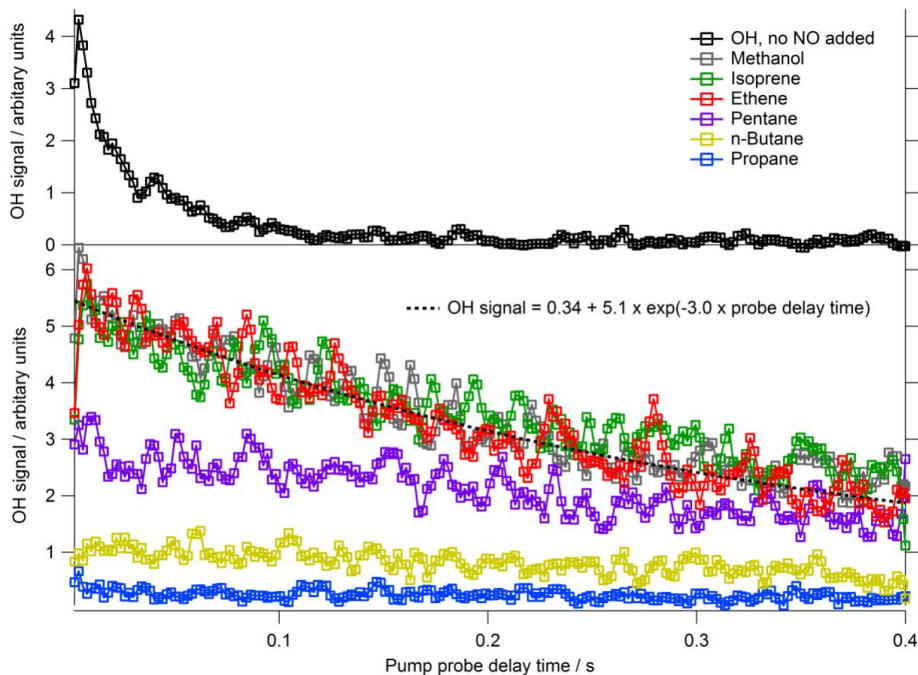


Fig. 3. upper panel: Time evolution of OH formed in the flow tube by laser-photolysis of O_3 in humidified air in the presence of isoprene with no NO added to the FAGE cell. Lower panel: Typical time-resolved experiments showing the OH signal from isoprene (green), ethene (red), methanol (grey), *n*-pentane (purple), *n*-butane (mustard) and propane (blue) derived peroxy radicals that was observed when 6 SCCM NO was added to the FAGE cell. The dashed line shows the fit to the OH signal from ethene-derived RO_2 radicals of the function: $y = y_0 + A \times \exp(-B \times x)$. The relative yields were determined from the ratio of the A factors. See Table 2 for the yields determined.

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page	
Abstract	Introduction
Conclusions	References
Tables	Figures
◀	▶
◀	▶
Back	Close
Full Screen / Esc	
Printer-friendly Version	
Interactive Discussion	



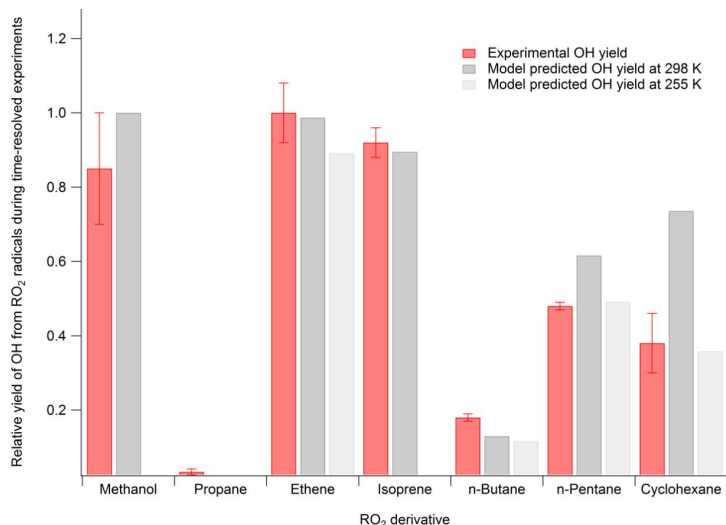


Fig. 4. Time-resolved OH yields (using apparatus outlined in Fig. 2) from different peroxy radicals (RO₂ → HO₂ → OH) under low-pressure FAGE conditions in the presence of NO (red bars); the errors represent the 1σ variability of the determined experimental yield. The Kintecus model predicted OH yields, assuming a reaction time of 9.8 ms and an initial NO concentration of 1 × 10¹⁴ molecule cm⁻³, based on MCMv3.2 chemistry (model schemes provided in SI), assuming a temperature of 298 K (dark grey bars) are also shown for comparison. The model predicted OH yield at 255 K for ethene, *n*-butane, *n*-pentane and cyclohexane are represented by the light grey bars. The strong temperature dependence for the rate of isomerisation/decomposition of the alkoxy radicals reduces the model predicted OH yield as reaction between alkoxy radicals + NO Reaction (R19) begins to compete; there is currently no information on the temperature dependence of isoprene-derived alkoxy radical decomposition in the literature.

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Title Page

Abstract Introduction

Conclusions References

Tables Figures

⏪ ⏩

⏴ ⏵

Back Close

Full Screen / Esc




Printer-friendly Version

Interactive Discussion



Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

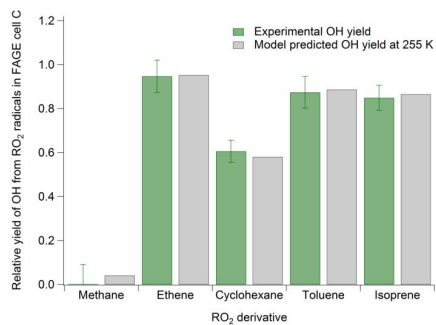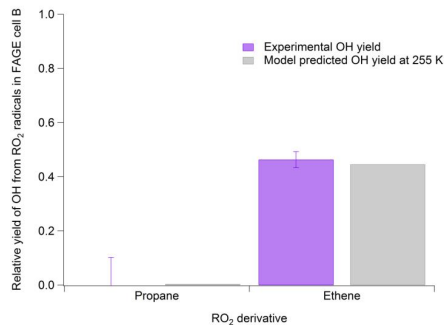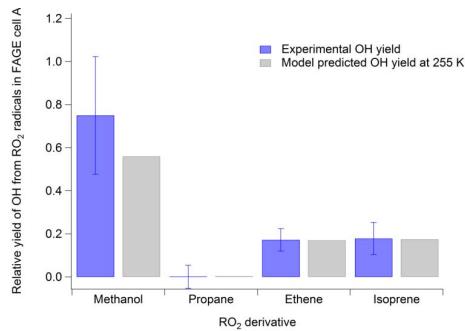[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

Fig. 5. Upper panel: The OH yields from different peroxy radicals ($\text{RO}_2 \rightarrow \text{HO}_2 \rightarrow \text{OH}$) in cell A in the presence of NO (blue bars); the errors represent the 1σ variability of the determined experimental yield. The model predicted OH yields (grey bars) assuming a reaction time of 0.9 ms, temperature of 255 K and an initial NO concentration of 1×10^{14} molecule cm^{-3} , based on MCMv3.2 chemistry are also shown for comparison. Middle panel: The OH yields from different peroxy radicals ($\text{RO}_2 \rightarrow \text{HO}_2 \rightarrow \text{OH}$) in cell B in the presence of NO (purple bars); the errors represent the 1σ variability of the determined experimental yield. The model predicted OH yields (grey bars) assuming a reaction time of 1.9 ms, temperature of 255 K and an initial NO concentration of 1×10^{14} molecule cm^{-3} , based on MCMv3.2 chemistry are also shown for comparison. Lower panel: The OH yields from different peroxy radicals ($\text{RO}_2 \rightarrow \text{HO}_2 \rightarrow \text{OH}$) in cell C in the presence of NO (green bars); the errors represent the 1σ variability of the determined experimental yield. The model predicted OH yields (grey bars) assuming a reaction time of 60 ms, an initial NO concentration of 1×10^{13} molecule cm^{-3} and a temperature of 255 K based on MCMv3.2 chemistry are also shown for comparison; there is currently no information on the temperature dependence of isoprene- or toluene-derived alkoxy radical decomposition in the literature so the rate coefficient at 298 K is assumed.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

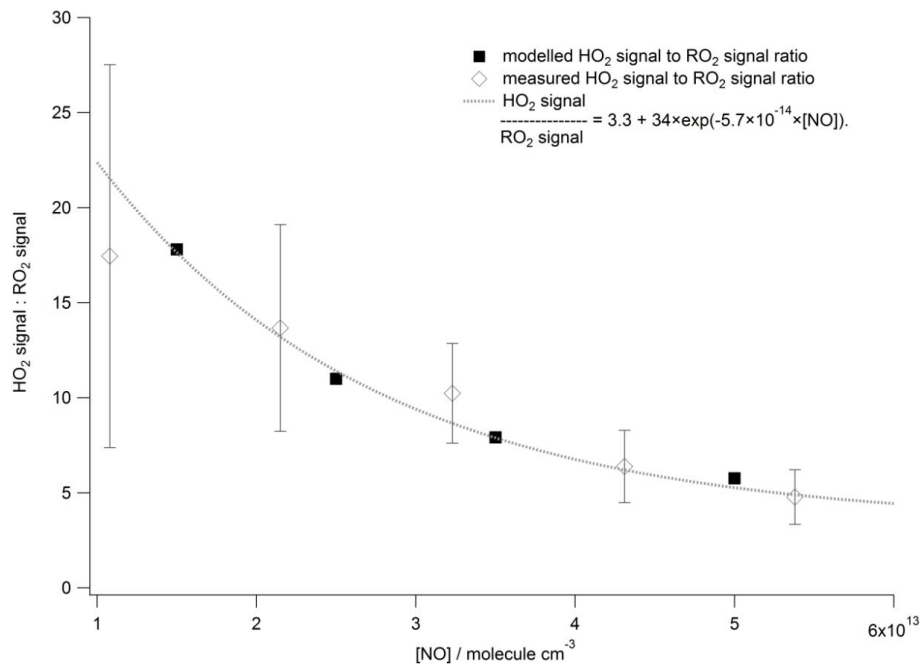


Fig. 6. Modelled (filled squares) and measured (open diamonds) ratio of the OH yield from $\text{HO}_2 \text{ signal} : \text{RO}_2 \text{ signal}$ as a function of NO concentration. For best agreement with model predictions, it has to be assumed that the NO concentration that mixes into the ambient air stream is 5.5 times lower than the amount actually injected. The dashed line represents the line of best fit for the modelled HO₂ signal to RO₂ signal ratio as a function of NO. The error bars represent the fractional error associated with each measured ratio determined from the 1σ standard deviation of the experiments conducted.

Sensitivity of Laser Induced Fluorescence instruments

L. K. Whalley et al.

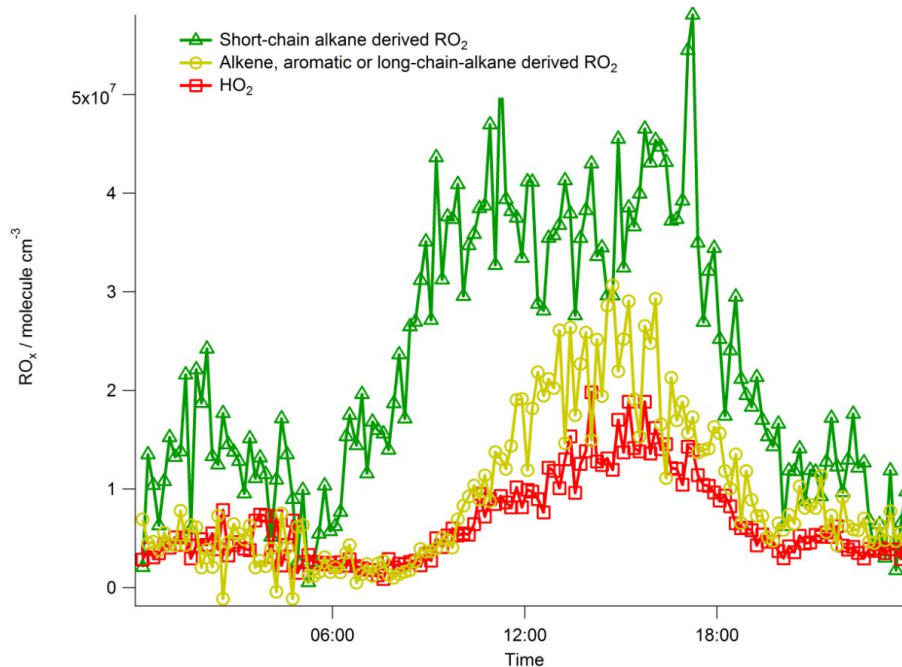


Fig. 7. Campaign average diurnals of short-chain alkane RO₂ radicals (green), HO₂ (red) and alkene or aromatic or long-chain-alkane derived RO₂ radicals (mustard) from the ClearLo project which took place in London (North Kensington) from the 21 July to 18 August 2012.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)