



Interactive  
Comment

## ***Interactive comment on “Investigation of ground-based microwave radiometer calibration techniques at 530 hPa” by G. Maschwitz et al.***

**G. Maschwitz et al.**

gmasch@meteo.uni-koeln.de

Received and published: 15 June 2013

The comment was uploaded in the form of a supplement:  
<http://www.atmos-meas-tech-discuss.net/6/C1319/2013/amtd-6-C1319-2013-supplement.pdf>

Interactive comment on Atmos. Meas. Tech. Discuss., 6, 989, 2013.

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

Discussion Paper



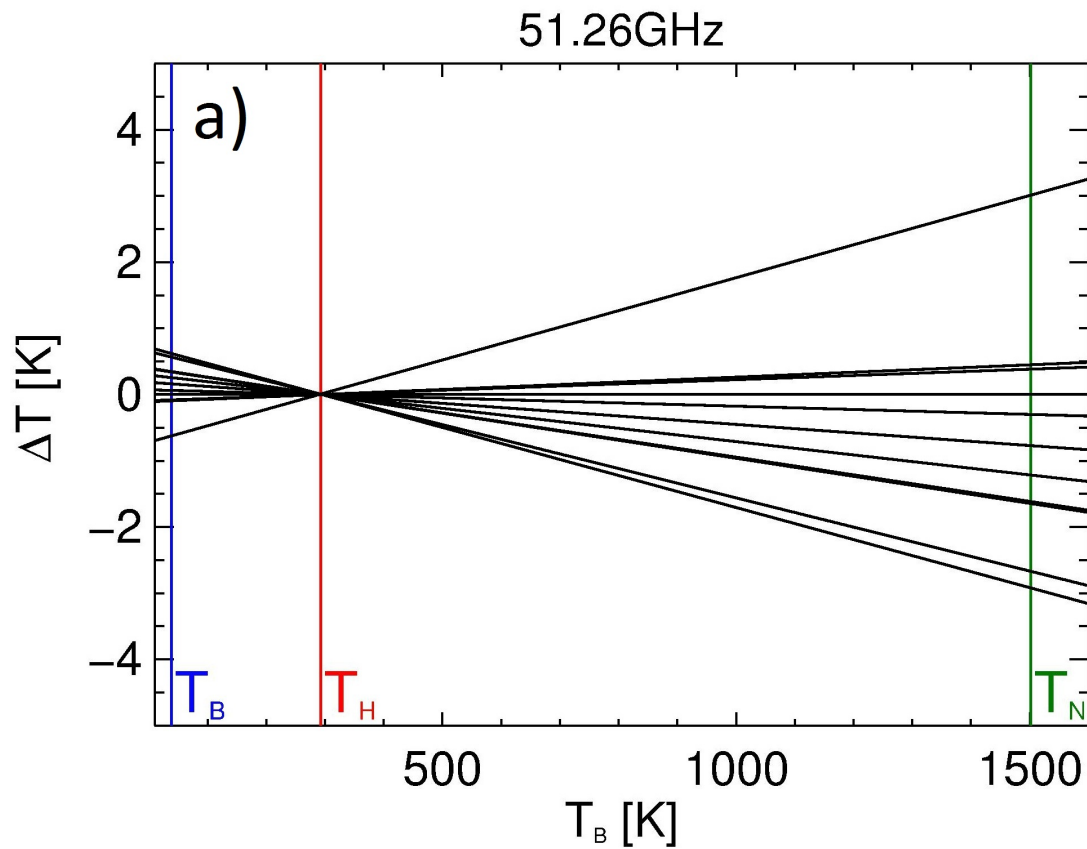


Fig. 1.

[Interactive  
Comment](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)[Discussion Paper](#)

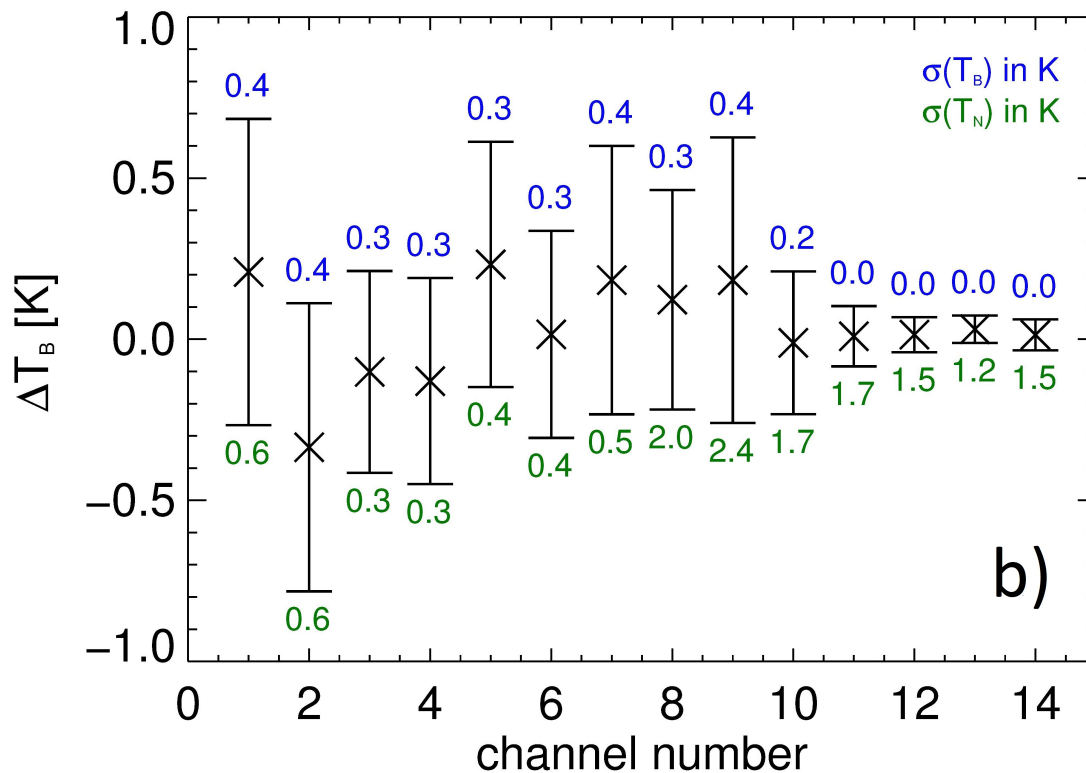
[Interactive  
Comment](#)

Fig. 2.

[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)[Discussion Paper](#)

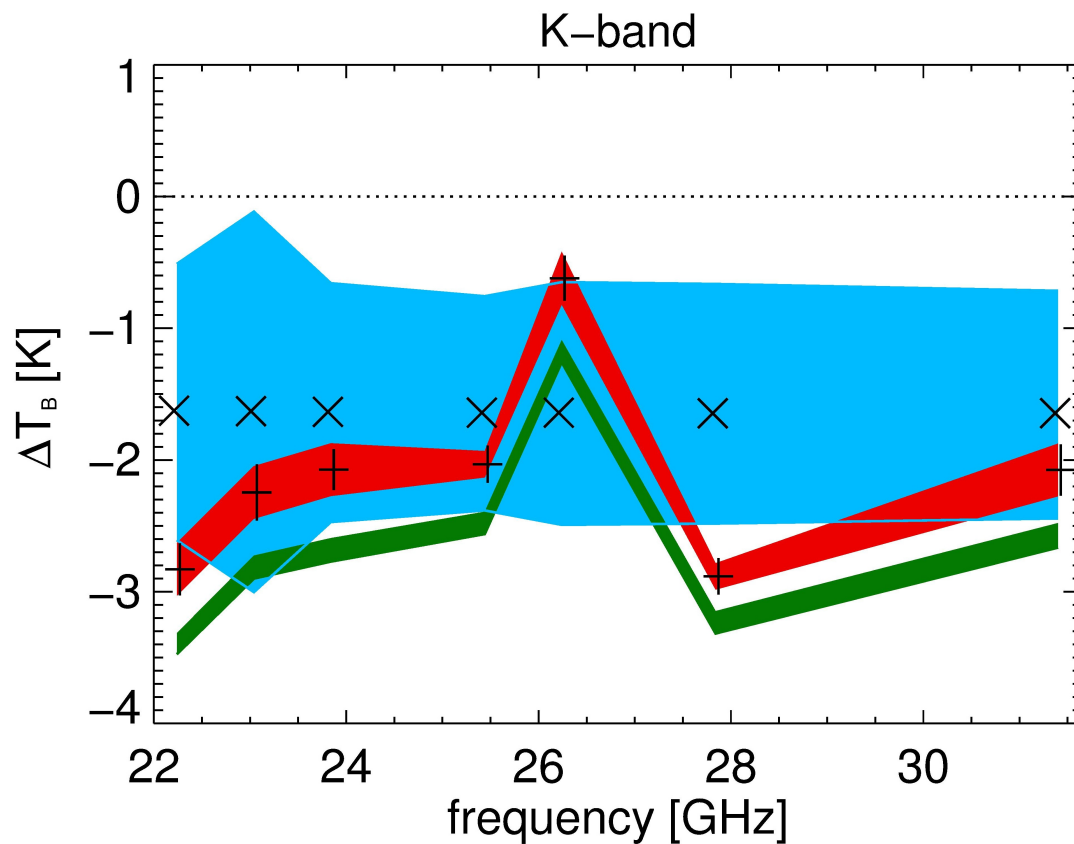
[Interactive  
Comment](#)

Fig. 3.

[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)[Discussion Paper](#)

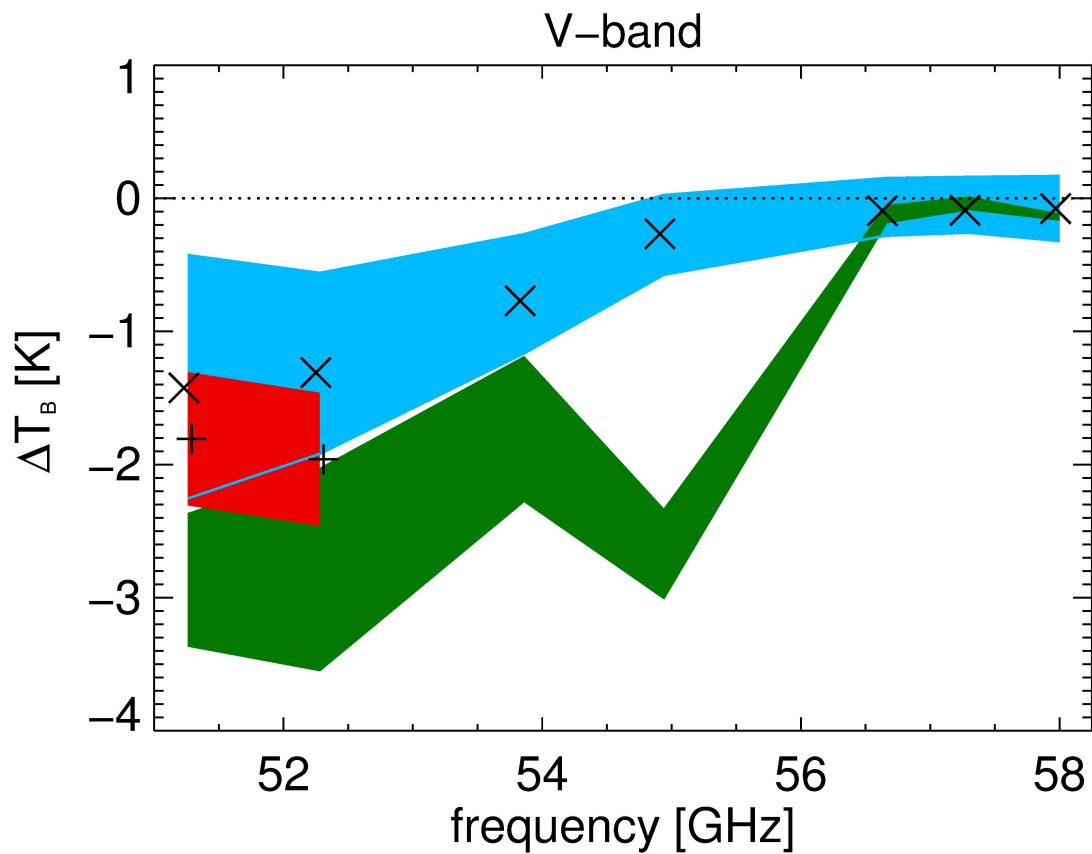
[Interactive  
Comment](#)

Fig. 4.

[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)[Discussion Paper](#)