

This discussion paper is/has been under review for the journal Atmospheric Measurement Techniques (AMT). Please refer to the corresponding final paper in AMT if available.

# Determination of alkyl amines in atmospheric aerosol particles: a comparison of gas chromatography-mass spectrometry and ion chromatography approaches

R.-J. Huang<sup>1,3,4</sup>, W.-B. Li<sup>2</sup>, Y.-R. Wang<sup>2</sup>, Q. Y. Wang<sup>5</sup>, K.-F. Ho<sup>5,6</sup>, J. J. Cao<sup>5</sup>, G. H. Wang<sup>5</sup>, X. Chen<sup>2</sup>, I. El Haddad<sup>1</sup>, Z. X. Zhuang<sup>2,7</sup>, X. R. Wang<sup>2,7</sup>, A. S. H. Prévôt<sup>1</sup>, C. D. O'Dowd<sup>3</sup>, and T. Hoffmann<sup>4</sup>

<sup>1</sup>Laboratory of Atmospheric Chemistry, Paul Scherrer Institute (PSI), 5232 Villigen, Switzerland

<sup>2</sup>Department of Chemistry and The MOE Key Laboratory of Spectrochemical Analysis & Instrumentation, College of Chemistry and Chemical Engineering, Xiamen University, Xiamen 361005, China

<sup>3</sup>Centre for Climate and Air Pollution Studies, Ryan Institute, National University of Ireland Galway, University Road, Galway, Ireland

AMTD  
7, 2127–2152, 2014

Determination of alkyl amines in atmospheric aerosol particles

R.-J. Huang et al.

<a href="#">Title Page</a>	
<a href="#">Abstract</a>	<a href="#">Introduction</a>
<a href="#">Conclusions</a>	<a href="#">References</a>
<a href="#">Tables</a>	<a href="#">Figures</a>
<a href="#">◀</a>	<a href="#">▶</a>
<a href="#">◀</a>	<a href="#">▶</a>
<a href="#">Back</a>	<a href="#">Close</a>
<a href="#">Full Screen / Esc</a>	
<a href="#">Printer-friendly Version</a>	
<a href="#">Interactive Discussion</a>	

<sup>4</sup>Institute of Inorganic and Analytical Chemistry, Johannes Gutenberg-University of Mainz, Duesbergweg 10–14, 55128 Mainz, Germany

<sup>5</sup>Key Laboratory of Aerosol Science and Technology, SKLLQG, Institute of Earth Environment, Chinese Academy of Sciences, Xi'an 710075, China

<sup>6</sup>School of Public Health and Primary Care, The Chinese University of Hong Kong, Hong Kong, China

<sup>7</sup>Center for Environmental Science and Technology, Xiamen Huaxia Vocational College, Xiamen 361024, China

Received: 29 January 2014 – Accepted: 26 February 2014 – Published: 5 March 2014

Correspondence to: R.-J. Huang (rujin.huang@psi.ch)

Published by Copernicus Publications on behalf of the European Geosciences Union.

AMTD

7, 2127–2152, 2014

**Determination of alkyl amines in atmospheric aerosol particles**

R.-J. Huang et al.

[Title Page](#)

[Abstract](#)

[Introduction](#)

[Conclusions](#)

[References](#)

[Tables](#)

[Figures](#)

◀

▶

◀

▶

[Back](#)

[Close](#)

[Full Screen / Esc](#)

[Printer-friendly Version](#)

[Interactive Discussion](#)



## Abstract

In recent years low molecular weight alkyl amines have been recognized to play an important role in particle formation and growth in the lower atmosphere. However, major uncertainties are associated with their atmospheric processes, sources and sinks, 5 mostly due to the lack of ambient measurements and the difficulties in accurate quantification of alkyl amines at trace level. In this study, we present the evaluation and optimization of two analytical approaches, i.e., gas chromatography-mass spectrometry (GC-MS) and ion chromatography (IC), for the determination of alkyl amines in aerosol particles. Alkyl amines were converted to carbamates through derivatization 10 with isobutyl chloroformate for GC-MS determination. A set of parameters affecting the analytical performances of the GC-MS approach, including reagent amount, reaction time and pH value, was evaluated and optimized. The accuracy is 84.3–99.1 %, and the limits of detection obtained are 1.8–3.9 pg. For the IC approach, a solid phase extraction (SPE) column was used to separate alkyl amines from interfering cations before IC 15 analysis. 1–2 % (v/v) of acetone (or 2–4 % (v/v) of acetonitrile) was added to the eluent to improve the separation of alkyl amines on the IC column. The limits of detection obtained are 2.1–15.9 ng and the accuracy is 55.1–103.4 %. The lower accuracy can be attributed to evaporation losses of amines during the sample concentration procedure. Measurements of ambient aerosol particle samples collected in Hong Kong show that 20 the GC-MS approach is superior to the IC approach for the quantification of primary and secondary alkyl amines due to its lower detection limits and higher accuracy.

## 1 Introduction

Organic nitrogen (ON) is ubiquitous in the atmosphere, and yet a poorly characterized component of atmospheric aerosols. Compared to oxygenated organics which have 25 been extensively studied in the past decade (Hallquist et al., 2009; Hoffmann et al., 2011), much less attention has been devoted to ON in atmospheric aerosols and, thus

<a href="#">Title Page</a>	
<a href="#">Abstract</a>	<a href="#">Introduction</a>
<a href="#">Conclusions</a>	<a href="#">References</a>
<a href="#">Tables</a>	<a href="#">Figures</a>
<a href="#">◀</a>	<a href="#">▶</a>
<a href="#">◀</a>	<a href="#">▶</a>
<a href="#">Back</a>	<a href="#">Close</a>
<a href="#">Full Screen / Esc</a>	
<a href="#">Printer-friendly Version</a>	
<a href="#">Interactive Discussion</a>	

the sources, composition and atmospheric processes of ON are poorly constrained. Addition of nitrogen to an organic structure can increase the potential carcinogenic and mutagenic effects (Kameda, 2011) as well as the extinction coefficient of a compound (Nguyen et al., 2012). It can also increase the hygroscopicity of aerosols and thereby the ability to act as cloud condensation nucleus because several organic nitrogen groups (e.g., amines and nitrates) have high water solubility. Therefore, it is crucial to understand the ON composition in order to get better knowledge of aerosol effects on health, air quality and climate.

Among a wide variety of ON, amines are unique in their base-stabilization capacity.

Especially, low molecular weight aliphatic amines such as dimethylamine and ethylamine can substantially enhance the ternary nucleation of sulphuric acid particles by a stepwise accretion of the basic molecules and concomitant addition of acid molecules in the critical clusters (Kirkby et al., 2011). The formation of aminium salts from heterogeneous reactions of amines with organic and inorganic acids can further contribute to post-nucleation growth of nanoparticles, which increases the particle number concentration by preventing coagulation from pre-existing particles (Wang et al., 2010; Smith et al., 2010). The reactive uptake of amines and subsequent displacement of ammonium on the particles provide additional pathway for gas-to-particle conversion of amines (Qiu et al., 2011; Chan and Chan, 2012). The mechanisms discussed above support the observations of ambient particle-phase amines in various domains such as in boreal forests (Mäkelä et al., 2001; Smith et al., 2010), in urban and rural areas (Pratt et al., 2009; Smith et al., 2010; Vandenboer et al., 2011; Huang et al., 2012), and in the remote marine boundary layer (Facchini et al., 2008).

Amines have been measured so far in atmospheric ultrafine and fine particles by a number of online mass spectrometric techniques including compact time-of-flight aerosol mass spectrometry (C-TOF-AMS) (Sorooshian et al., 2008), aerosol time-of-flight mass spectrometry (ATOFMS) (Huang et al., 2012), atmospheric pressure interface time-of-flight mass spectrometry (APi-TOF-MS) (Junninen et al., 2010), and thermal desorption chemical ionization mass spectrometry (TDCIMS) (Smith et al., 2010).

## Determination of alkyl amines in atmospheric aerosol particles

R.-J. Huang et al.

[Title Page](#)

[Abstract](#)

[Introduction](#)

[Conclusions](#)

[References](#)

[Tables](#)

[Figures](#)

◀

▶

[Back](#)

[Close](#)

[Full Screen / Esc](#)

[Printer-friendly Version](#)

[Interactive Discussion](#)

However, these mass spectrometric observations cannot provide quantitative determination of specific amines. For example, AMS response factors for various aminium salts have been reported to vary as much as 10 times that of ammonium nitrate depending on the composition of the salt, which limit the method to amine identification only (Silva et al., 2008). The TDCIMS analysis reported the levels of amines as the molar ratio of average ion abundance for each aminium compound to the total average ion abundance observed, rather than as the absolute concentrations (Smith et al., 2010).

Quantitative determination of amines in ambient aerosol particles is mainly based on chromatographic techniques such as ion chromatography (IC) (Henning et al., 2003; Facchini et al., 2008; Erupe et al., 2010; Vandenboer et al., 2011; Praplan et al., 2012), gas chromatography (GC) (Akyüz, 2008) and high performance liquid chromatography (HPLC) (Yang et al., 2005; Müller et al., 2009; Ruiz-Jimenez et al., 2012). IC allows the determination of low molecular weight alkyl amines including tertiary amines without derivatization. However, certain amines are often co-eluted as a single peak (e.g., diethylamine and trimethylamine) or interfered by other abundant cations present in aerosol particles (e.g.,  $\text{NH}_4^+$  and  $\text{K}^+$ ) (Vandenboer et al., 2011) due to the low separation efficiency and resolution of IC. For determination with GC and HPLC, the derivatization of amines is generally mandatory to improve the separation efficiency and the detection limits. The typical derivatization reagents for amines include o-phthaldialdehyde, dansyl chloride, isobutyl chloroformate, and 4-nitrophenyl trifluoroacetate (Pan et al., 1997; Akyüz, 2008; Huang et al., 2009; Ruiz-Jiménez et al., 2012). Nevertheless, the derivatization reagents are suitable only for primary and secondary amines, but not for tertiary amines due to the absence of a replaceable hydrogen atom.

In this paper, we present two analytical approaches (i.e., gas chromatography-mass spectrometry (GC-MS) and IC) for the determination of alkyl amines in aerosol particles. We focused on  $\text{C}_1\text{--C}_6$  alkyl amines because these low molecular weight alkyl amines are thought to release to the atmosphere in the largest quantity. The

## Determination of alkyl amines in atmospheric aerosol particles

R.-J. Huang et al.

[Title Page](#)

[Abstract](#)

[Introduction](#)

[Conclusions](#)

[References](#)

[Tables](#)

[Figures](#)

◀

▶

[Back](#)

[Close](#)

[Full Screen / Esc](#)

[Printer-friendly Version](#)

[Interactive Discussion](#)

parameters affecting the analytical performances of both methods are extensively evaluated and optimized.

## 2 Experimental

### 2.1 Standards and PM<sub>2.5</sub> samples

5 2.0 mg mL<sup>-1</sup> stock standard solution was prepared in 0.1 M HCl aqueous solution, which contains a mixture of the hydrochloride salts of methylamine (MA, 99 %, J&K Scientific), dimethylamine (DMA, > 99 %, Aladdin Chemical), trimethylamine (TMA, > 98 %, Sigma Aldrich), ethylamine (EA, > 98 %, Tokyo Chemical Industry), diethylamine (DEA, > 98.5 %, Tokyo Chemical Industry), triethylamine (TEA, > 98.5 %, Tokyo 10 Chemical Industry), *n*-propylamine (PA, > 99 %, Acros) and *n*-butylamine (BA, > 98 %, Tokyo Chemical Industry). A series of working standard solutions was prepared by sequential dilution of the stock standard solution. The alkaline methanol solution was prepared by dissolving KOH in methanol until saturation, followed by filtration through a 0.45 µm filter. All other chemicals used were of analytical reagent grade. Deionized 15 water (18 MΩ cm) was used for preparation of all aqueous solutions.

The 24 h integrated PM<sub>2.5</sub> (particulate matter with an aerodynamic diameter < 2.5 µm) samples were collected on pre-fired (500 °C, 3 h) quartz filters (8" × 10") in August and November 2011 and February and May 2012 (24 samples and 4 field blanks) in Tung Chung, Hong Kong (22°17'20" N, 113°56'37" E) by using high-volume air samplers. A portion was taken from each filter and placed into a 15 mL screw capped brown 20 vial to which 5 mL 0.1 M HCl was added. The samples were extracted in an ultrasonic bath at room temperature for 15 min. This extraction procedure was repeated 3 times. Finally, the extracts were combined for each filter and filtered with 0.2 µm syringe filter (PTFE membrane).

<a href="#">Title Page</a>	
<a href="#">Abstract</a>	<a href="#">Introduction</a>
<a href="#">Conclusions</a>	<a href="#">References</a>
<a href="#">Tables</a>	<a href="#">Figures</a>
<a href="#">◀</a>	<a href="#">▶</a>
<a href="#">◀</a>	<a href="#">▶</a>
<a href="#">Back</a>	<a href="#">Close</a>
<a href="#">Full Screen / Esc</a>	
<a href="#">Printer-friendly Version</a>	
<a href="#">Interactive Discussion</a>	

## 2.2 GC-MS analysis

The sample extracts and standard solution were subjected to derivatization before the GC-MS analysis. To 15 mL of filtered extracts (or standard solution), 5 mL of phosphate buffer (pH 12), 5 mL of toluene and 200  $\mu$ L of isobutyl chloroformate (IBCF) were added.

5 The solution was shaken in a mechanical shaker at room temperature for 15 min. The toluene extracts containing the target analytes were then transferred to another vial and concentrated to 1 mL under a gentle  $N_2$  stream at room temperature. 500  $\mu$ L of alkaline methanol was added to the concentrated extracts, and the mixture was shaken for 5 min for removal of the excess of IBCF. 1.5 mL of 1 M NaOH was subsequently added, 10 and the mixture was shaken for another 5 min.

The mixture was centrifuged and 1.0  $\mu$ L of the toluene extracts was injected into a GC-MS system (Shimadzu QP 2010 Plus, Shimadzu, Japan). A fused-silica capillary column (30 m  $\times$  0.25 mm i.d.,  $d_f$ : 0.25  $\mu$ m, Rxi-5MS, Shimadzu, Japan) was used for chromatographic separation. High-purity helium (99.999 %) was used as a carrier gas 15 at a constant flow of 1.0  $\text{mL min}^{-1}$ . The temperature of the injector was set to 280  $^{\circ}\text{C}$  and the transfer line was 280  $^{\circ}\text{C}$ . The temperature of the GC oven was programmed as follows: initial temperature 80  $^{\circ}\text{C}$  (hold 3 min), 5  $^{\circ}\text{C min}^{-1}$  to 140  $^{\circ}\text{C}$  (hold 3 min), and then 30  $^{\circ}\text{C min}^{-1}$  to 200  $^{\circ}\text{C}$  (hold 3 min). The MS was operated in the electron impact (EI) ionization mode with an acceleration energy of 70 eV. A solvent delay of 4.0 min 20 preceded the MS spectra acquisition in the full-scan mode (in the range  $m/z$  30–450) or in the selected ion monitoring (SIM) mode in the following sequence: 4.00–6.15 min,  $m/z$ : 57, 58, 116; 6.15–6.50 min,  $m/z$ : 72, 130, 145; 6.50–7.86 min,  $m/z$ : 57, 72, 130; 7.86–9.25 min,  $m/z$ : 57, 158, 173; 9.25–10.69 min,  $m/z$ : 57, 86, 144; 10.69–12.56 min, 25  $m/z$ : 57, 100, 173. The use of SIM mode is an advantage for eliminating potential interference from sample matrix (or from the sample pretreatment steps) because it greatly enhances the selectivity (by monitoring characteristic  $m/z$  fragments) and sensitivity of the method.

## Determination of alkyl amines in atmospheric aerosol particles

R.-J. Huang et al.

[Title Page](#)

[Abstract](#)

[Introduction](#)

[Conclusions](#)

[References](#)

[Tables](#)

[Figures](#)

◀

▶

◀

▶

[Back](#)

[Close](#)

[Full Screen / Esc](#)

[Printer-friendly Version](#)

[Interactive Discussion](#)

## 2.3 IC analysis

15 mL aliquots of filtered extracts were passed through a cleaned and conditioned cation-exchange solid phase extraction column (SPE, Oasis MCX, Waters). The analytes were eluted using 3 mL of NH<sub>3</sub>/methanol (5 : 95, v/v) solutions. The resulting eluate was adjusted to pH 8.8 and then concentrated to 1 mL under a gentle N<sub>2</sub> stream at room temperature. A 25 µL aliquot of the concentrated eluate (or standard solution) was injected into a Metrohm 861 IC analytical system with non-suppressed detection (Metrohm, 861 Advanced Compact IC). The IC was equipped with a dual-piston pump, a degas assembly and digital conductivity detection. Analysis was accomplished with a Metrosep C4 (150 mm × 4 mm i.d.) with Metrosep C4 guard column, which was chosen due to its advantage in the analysis of amines and common inorganic cations with non-suppressed conductivity detection. The optimized eluent solution contained 6 mM HNO<sub>3</sub>/1.0 % (v/v) acetone solution at a flow rate of 0.4 mL min<sup>-1</sup>. Separation was carried out under isocratic conditions and at a room temperature of approximately 20 °C. Data processing was performed with IC Net 2.3 software.

## 2.4 Quality assurance

For every 10 samples, a procedural blank and a spiked sample, namely, real samples spiked with known amounts of amine standards, were measured to check for interference and cross-contamination. External standard method was used for quantitative determination of the analytes. Because carbamates are not commercially available, the calibration curves were made by derivatizing the standard solutions of amines following the same procedures used for real samples. The limits of detection are defined as the minimum detectable peaks of individual species with a signal-to-noise (S/N) ratio of 3 : 1. The recoveries were determined by the analysis of the spiked samples. The reproducibility (relative standard deviation, RSD) was determined by measuring five identical samples that were subjected to the same pretreatment procedure. Four field blank samples were collected and measured, giving the average field blank values as

## Determination of alkyl amines in atmospheric aerosol particles

R.-J. Huang et al.

[Title Page](#)

[Abstract](#)

[Introduction](#)

[Conclusions](#)

[References](#)

[Tables](#)

[Figures](#)

◀

▶

◀

▶

[Back](#)

[Close](#)

[Full Screen / Esc](#)

[Printer-friendly Version](#)

[Interactive Discussion](#)

follows:  $0.04 \text{ ng m}^{-3}$  of MA,  $1.10 \text{ ng m}^{-3}$  of DMA,  $< 0.03 \text{ ng m}^{-3}$  of EA,  $1.22 \text{ ng m}^{-3}$  of DEA,  $0.29 \text{ ng m}^{-3}$  of PA, and  $0.28 \text{ ng m}^{-3}$  of BA. All data reported here were corrected for the field blanks.

### 3 Results and discussion

#### 5 3.1 Determination of amines with GC-MS

##### 3.1.1 Effect of pH on the derivatization

The low molecular weight alkyl amines are not detectable without derivatization when injected into a nonpolar GC column (5 % diphenyl 95 % dimethylpolysiloxane) (see Fig. 1a), due to their high volatilities and high polarities as reflected in their boiling points and oil–water partition coefficients  $\log P_{\text{o/w}}$  (see Table 1). The formation of carbamate derivatives via reactions with isobutyl chloroformate (IBCF) (Akyüz, 2008) can significantly improve the chromatographic properties of primary and secondary amines, leading to well resolved peaks on the GC chromatogram (Fig. 1b), because the carbamates have lower volatilities and polarities as well as higher thermal stabilities compared to the amines. The derivatization proceeds rapidly in aqueous alkaline media since it promotes the deprotonation of aminium (R1). The latter are the most likely form of amines in ambient aerosol particles. High pH-values also shift the derivatization reaction to the product side through neutralization of the  $\text{H}^+$  formed in this reaction (R2).




Figure 2 shows the effect of pH values on the derivatization efficiencies of MA, DMA, EA, DEA, PA and BA. When the pH value is below 7, most amines remain in the

AMTD

7, 2127–2152, 2014

## Determination of alkyl amines in atmospheric aerosol particles

R.-J. Huang et al.

[Title Page](#)

[Abstract](#)

[Introduction](#)

[Conclusions](#)

[References](#)

[Tables](#)

[Figures](#)

◀

▶

◀

▶

[Back](#)

[Close](#)

[Full Screen / Esc](#)

[Printer-friendly Version](#)

[Interactive Discussion](#)



## Determination of alkyl amines in atmospheric aerosol particles

R.-J. Huang et al.

protonated form that cannot react with IBCF to form the carbamate derivatives. The derivatization proceeds progressively with the increase of the pH value and reaches the maximum efficiencies for all investigated alkyl amine when the pH values are higher than 9. This pH threshold is somewhat lower than the theoretical values ( $pK_a + 1$ , i.e.,

5 11.58–12.09), where the amines are mostly present in the neutralized form that can react with IBCF. This phenomenon can be explained by the removal of derivatives from the aqueous solution by toluene which, together with the neutralization of the  $\text{H}^+$  formed, accelerates the shifting of Reactions (R1) and (R2) to the right. Therefore, pH 10 was selected as the optimized value in this study.

### 3.1.2 Effect of reagent amount and reaction time on the derivatization efficiency

Figure 3 shows that, compared to the theoretical molar ratio of 1:1 for the derivatization of amines with IBCF, a much higher IBCF/amine ratio is needed to ensure a sufficient efficiency. Interestingly, the derivatization efficiency for DMA, DEA, PA and BA is much higher than for MA and EA at a low IBCF/amine ratio. For example, at the IBCF/amine molar ratio of 5–10, the efficiency is around 80 % for DMA, DEA, PA and BA, but only about 20 % for MA and EA. This can be attributed to the increased number and/or chain length of the alkyl group(s) in DMA, DEA, PA and BA, which enhances the electron density at the nitrogen atoms of these amines and thereby their nucleophilic reactivity towards the derivatization agent IBCF. The DMA, DEA, PA and BA approach their maximum derivatization efficiencies at the IBCF/amine molar ratios > 100, while the molar ratios are > 250 in the case of MA and EA. Given that IBCF can also react with certain amino acids (Sobolevsky et al., 2004), an equivalent molar ratio of IBCF/amine of 500 was selected for the analysis of real samples.

With the optimized pH value and IBCF/amine molar ratio the derivatization of amines with IBCF is very efficient. The temporal behavior of the derivatization efficiency is shown in Fig. 4. Quantitative determinations were achieved for DMA, DEA, PA and BA after about 5 min and for MA and EA after 10 min, respectively. Again, the faster

Title Page	
Abstract	Introduction
Conclusions	References
Tables	Figures
◀	▶
◀	▶
Back	Close
Full Screen / Esc	

Printer-friendly Version

## Interactive Discussion



### 3.2.2 Influence of interfering cations

A common issue associated with IC analysis of alkyl amines is the interference from in-organic cations such as  $\text{Na}^+$ ,  $\text{K}^+$ ,  $\text{Mg}^{2+}$ ,  $\text{Ca}^{2+}$  and  $\text{NH}_4^+$ , which are typically 1–3 orders of magnitude more concentrated than alkyl amines (Müller et al., 2009; Vandenboer et al., 2011). Co-elution of these interfering cations with the analytes may be problematic for the quantification of alkyamines. As shown in Fig. 6a, MA and  $\text{K}^+$ , DMA and  $\text{Mg}^{2+}$ , and BA and  $\text{Ca}^{2+}$  co-elute on the Metrosep C4 column. To minimize such interference the solid phase extraction (SPE) cartridges were used before IC analysis. It was found that the Oasis MCX cation-exchange cartridges can efficiently remove most of the interfering cations. However, it was also observed that some alkyl amines were lost by evaporation during the concentration step after SPE treatment. The evaporation loss is particularly significant for MA (~ 40 %), DMA (~ 35 %) and TMA (~ 85 %), most probably because they are much more volatile than other alkyl amines. Interestingly, the loss for MA and DMA is smaller than that for TMA although the former two species have higher vapour pressure compared to TMA. One explanation for this observation is the potential interaction of MA (DMA) with solvent molecules by hydrogen bonding, which compensates for their high volatility. The evaporation loss can be reduced by decreasing the pH value of the solution due to the transformation of alkyl amines to their protonated salts which significantly decreases the volatility. The optimized pH value is 8.8, where the interference from  $\text{NH}_3$  ( $\text{pK}_a$  9.25) and losses of alkyl amines are minimized.

### 3.3 Comparison of the methods

Table 2 shows the reproducibility, recovery and limit of detection (LOD) of the IC and GC-MS methods. The precision of the IC (2.4–15.7 % RSD) and GC-MS (1.7–6.2 % RSD) methods can be considered to be very satisfactory in view of multiple sources of error that contributed to total RSD values (e.g., error from sample pretreatment and error of the IC and GC-MS detection). The recoveries range from 84.3 % to 99.1 % for

[Title Page](#)

[Abstract](#)

[Introduction](#)

[Conclusions](#)

[References](#)

[Tables](#)

[Figures](#)

◀

▶

◀

▶

[Back](#)

[Close](#)

[Full Screen / Esc](#)

[Printer-friendly Version](#)

[Interactive Discussion](#)

**Determination of alkyl amines in atmospheric aerosol particles**

R.-J. Huang et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

revealed slightly higher amine concentrations compared to the IC method. In general, the GC-MS method is superior to the IC method, considering its higher accuracy and lower detection limits which are crucial for the quantification of alkyl amines that are often present at trace levels (from subng m<sup>-3</sup> to some hundred ngm<sup>-3</sup>) in ambient aerosol particles (Ge et al., 2011, and references therein).

**Acknowledgements.** The research leading to these results has received funding from the European Community's Seventh Framework Programme (FP7/2007-2013) under grant agreement no. 290605 and the National Nature Scientific Foundation of China (21105084).

## References

10 Akyüz, M.: Simultaneous determination of aliphatic and aromatic amines in ambient air and airborne particulate matters by gas chromatography-mass spectrometry, *Atmos. Environ.*, 42, 3809–3819, 2008.

15 Chan, L. P. and Chan, C. K.: Displacement of ammonium from aerosol particles by uptake of triethylamine, *Aerosol Sci. Tech.*, 46, 236–247, 2012.

20 Erupe, M. E., Liberman-Martin, A., Silva, P. J., Malloy, Q. G. J., Yonis, N., Cocker III, D. R. C., and Purvis-Roberts, K. L.: Determination of methylamines and trimethylamine-N-oxide in particulate matter by non-suppressed ion chromatography, *J. Chromatogr. A*, 1217, 2070–2073, 2010.

25 Facchini, M. C., Decesari, S., Rinaldi, M., Carbone, C., Finessi, E., Mircea, M., Fuzzi, S., Moretti, F., Tagliavini, E., Ceburnis, D., and O'Dowd, C. D.: Important source of marine secondary organic aerosol from biogenic amines, *Environ. Sci. Technol.*, 42, 9116–9121, 2008.

Ge, X. L., Wexler, A. S., and Clegg, S. L.: Atmospheric amines – Part I. A review, *Atmos. Environ.*, 45, 524–546, 2011.

30 Hallquist, M., Wenger, J. C., Baltensperger, U., Rudich, Y., Simpson, D., Claeys, M., Dommen, J., Donahue, N. M., George, C., Goldstein, A. H., Hamilton, J. F., Herrmann, H., Hoffmann, T., Iinuma, Y., Jang, M., Jenkin, M. E., Jimenez, J. L., Kiendler-Scharr, A., Maenhaut, W., McFiggans, G., Mentel, Th. F., Monod, A., Prévôt, A. S. H., Seinfeld, J. H., Suratt, J. D., Szmigielski, R., and Wildt, J.: The formation, properties and impact of sec-

[Title Page](#)

[Abstract](#)

[Introduction](#)

[Conclusions](#)

[References](#)

[Tables](#)

[Figures](#)

◀

▶

[Back](#)

[Close](#)

[Full Screen / Esc](#)

[Printer-friendly Version](#)

[Interactive Discussion](#)

ondary organic aerosol: current and emerging issues, *Atmos. Chem. Phys.*, 9, 5155–5236, doi:10.5194/acp-9-5155-2009, 2009.

Henning, S., Weingartner, E., Schwikowski, M., Gäggeler, H. W., Gehrig, R., Hinz, K.-P., Trimborn, A., Spengler, B., and Baltensperger, U.: Seasonal variation of water-soluble ions of the aerosol at the high-alpine site Jungfraujoch (3580 m a.s.l.), *J. Geophys. Res.*, 108, D14030, doi:10.1029/2002JD002439, 2003.

Hoffmann, T., Huang, R.-J., and Kalberer, M.: Atmospheric analytical chemistry, *Anal. Chem.*, 83, 4649–4664, 2011.

Huang, G., Hou, J., and Zhou, X. L.: A measurement method for atmospheric ammonia and primary amines based on aqueous sampling, OPA derivatization and HPLC analysis, *Environ. Sci. Technol.*, 43, 5851–5856, 2009.

Huang, Y. L., Chen, H., Wang, L., Yang, X., and Chen, J. M.: Single particle analysis of amines in ambient aerosol in Shanghai, *Environ. Chem.*, 9, 202–210, 2012.

Junninen, H., Ehn, M., Petäjä, T., Luosujärvi, L., Kotiaho, T., Kostiainen, R., Rohner, U., Gonin, M., Fuhrer, K., Kulmala, M., and Worsnop, D. R.: A high-resolution mass spectrometer to measure atmospheric ion composition, *Atmos. Meas. Tech.*, 3, 1039–1053, doi:10.5194/amt-3-1039-2010, 2010.

Kameda, T.: Atmospheric chemistry of polycyclic aromatic hydrocarbons and related compounds, *J. Health Sci.*, 57, 504–511, 2011.

Kirkby, J., Curtius, J., Almeida, J., Dunne, E., Duplissy, J., Ehrhart, S., Franchin, A., Gagne, S., Ickes, L., Kuerten, A., Kupc, A., Metzger, A., Riccobono, F., Rondo, L., Schobesberger, S., Tsagkogeorgas, G., Wimmer, D., Amorim, A., Bianchi, F., Breitenlechner, M., David, A., Dommen, J., Downard, A., Ehn, M., Flagan, R. C., Haider, S., Hansel, A., Hauser, D., Jud, W., Junninen, H., Kreissl, F., Kvashin, A., Laaksonen, A., Lehtipalo, K., Lima, J., Lovejoy, E. R., Makhmutov, V., Mathot, S., Mikkila, J., Minginette, P., Mogo, S., Nieminen, T., Onnela, A., Pereira, P., Petaja, T., Schnitzhofer, R., Seinfeld, J. H., Sipila, M., Stozhkov, Y., Stratmann, F., Tome, A., Vanhanen, J., Viisanen, Y., Vrtala, A., Wagner, P. E., Walther, H., Weingartner, E., Wex, H., Winkler, P. M., Carslaw, K. S., Worsnop, D. R., Baltensperger, U., and Kulmala, M.: Role of sulphuric acid, ammonia and galactic cosmic rays in atmospheric aerosol nucleation, *Nature*, 476, 429–433, 2011.

Mäkelä, J. M., Yli-Koivisto, S., Hiltunen, V., Seidl, W., Swietlicki, E., Teinilä, K., Sillanpää, M., Koponen, I. K., Paatero, J., Rosman, K., and Hämeri, K.: Chemical composition of aerosol during particle formation events in boreal forest, *Tellus B*, 53, 380–393, 2001.

**Determination of alkyl amines in atmospheric aerosol particles**

R.-J. Huang et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Müller, C., Iinuma, Y., Karstensen, J., van Pinxteren, D., Lehmann, S., Gnauk, T., and Herrmann, H.: Seasonal variation of aliphatic amines in marine sub-micrometer particles at the Cape Verde islands, *Atmos. Chem. Phys.*, 9, 9587–9597, doi:10.5194/acp-9-9587-2009, 2009.

5 Nguyen, T. B., Lee, P. B., Updyke, K. M., Bones, D. L., Laskin, J., Laskin, A., and Nizkorodov, S. A.: Formation of nitrogen- and sulfur-containing light-absorbing compounds accelerated by evaporation of water from secondary organic aerosols, *J. Geophys. Res.*, 117, D01207, doi:10.1029/2011JD016944, 2012.

10 Pan, L., Chong, J. M., and Pawliszyn, J.: Determination of amines in air and water using derivatization combined with solid-phase microextraction, *J. Chromatogr. A*, 773, 249–260, 1997.

Praplan, A. P., Bianchi, F., Dommen, J., and Baltensperger, U.: Dimethylamine and ammonia measurements with ion chromatography during the CLOUD4 campaign, *Atmos. Meas. Tech.*, 5, 2161–2167, doi:10.5194/amt-5-2161-2012, 2012.

15 Pratt, K. A., Hatch, L. E., Prather, K. A. Seasonal volatility dependence of ambient particle phase amines, *Environ. Sci. Technol.*, 43, 5276–5281, 2009.

Qiu, C. and Zhang, R. Y.: Multiphase chemistry of atmospheric amines, *Phys. Chem. Chem. Phys.*, 15, 5738–5752, 2013.

20 Ruiz-Jiménez, J.; Hautala, S., Parshintsev, J., Laitinen, T., Hartonen, K., Petäjä, T., Kulmala, M., and Riekkola, M.-L.: Aliphatic and aromatic amines in atmospheric aerosol particles: comparison of three ionization techniques in liquid chromatography-mass spectrometry and method development, *Talanta*, 97, 55–62, 2012.

Silva, P. J., Erupe, M. E., Price, D., Elias, J., Malloy, Q. G., Li, Q., Warren, B., Cocker III, D. R.: Trimethylamine as precursor to secondary organic aerosol formation via nitrate radical reaction in the atmosphere, *Environ. Sci. Technol.*, 42, 4689–4696, 2008.

25 Smith, J. N., Barsanti, K. C., Friedli, H. R., Ehn, M., Kulmala, M., Collins, D. R., Scheckman, J. H., Williams, B. J., and McMurry, P. H.: Observations of aminium salts in atmospheric nanoparticles and possible climatic implications, *P. Natl. Acad. Sci. USA*, 107, 6634–6639, 2010.

30 Sobolevsky, T. G., Revelsky, A. I., Revelsky, N. I. A., Miller, B., and Oriedo, V.: Simultaneous determination of fatty, dicarboxylic and amino acids based on derivatization with isobutyl chloroformate followed gas chromatography-positive ion chemical ionization mass spectrometry, *J. Chromatogr. B*, 800, 101–107, 2004.

**Determination of alkyl amines in atmospheric aerosol particles**

R.-J. Huang et al.

[Title Page](#)

[Abstract](#)

[Introduction](#)

[Conclusions](#)

[References](#)

[Tables](#)

[Figures](#)

◀

▶

◀

▶

[Back](#)

[Close](#)

[Full Screen / Esc](#)

[Printer-friendly Version](#)

[Interactive Discussion](#)

**Determination of alkyl amines in atmospheric aerosol particles**

R.-J. Huang et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[|◀](#)[▶|](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

## Determination of alkyl amines in atmospheric aerosol particles

R.-J. Huang et al.

**Table 1.** The physicochemical parameters of alkyl amines.

Alkyl amine	Boiling point, °C	Vapor pressure, kPa at 20 °C	pK <sub>a</sub> , 25 °C	Oil water distribution coefficient, log $P_{o/w}$
MA	-7	186.1	10.66	-0.173
DMA	7	170.3	10.73	-0.38
TMA	3.5	91.7	9.8	-0.152
EA	17	116.5	10.8	-0.177
DEA	56	26.0	11.09	-0.109
TEA	90	6.9	10.24	1.45
PA	49	33.0	10.58	-0.184
BA	77.8	9.1	10.62	3.56

[Title Page](#)

[Abstract](#)

[Introduction](#)

[Conclusions](#)

[References](#)

[Tables](#)

[Figures](#)

◀

▶

◀

▶

[Back](#)

[Close](#)

[Full Screen / Esc](#)

[Printer-friendly Version](#)

[Interactive Discussion](#)

## Determination of alkyl amines in atmospheric aerosol particles

R.-J. Huang et al.

**Table 2.** The analytical performance of GC-MS and IC method.

Alkyl amine	GC-MS			IC		
	Reproducibility % (n = 5)	Recovery % (n = 3)	LOD (pg), injection volume 1 $\mu$ L (n=6)	Reproducibility % (n = 5)	Recovery % (n = 3)	LOD (ng), injection volume 25 $\mu$ L (n = 6)
MA	2.6	86.4 $\pm$ 2.8	3.8	12.2	55.1 $\pm$ 8.6	2.1
DMA	3.6	99.1 $\pm$ 4.1	1.8	15.7	60.2 $\pm$ 9.7	3.8
EA	2.1	96.0 $\pm$ 1.8	2.5	4.3	88.5 $\pm$ 1.9	2.2
DEA	1.7	98.6 $\pm$ 2.1	3.7	4.6	95.9 $\pm$ 1.5	4.1
TEA	–	–	–	5.1	101.3 $\pm$ 1.6	15.9
PA	2.0	84.3 $\pm$ 1.7	3.7	–	–	–
BA	6.2	93.0 $\pm$ 4.9	3.9	2.4	103.4 $\pm$ 2.3	3.8

<a href="#">Title Page</a>	<a href="#">Abstract</a>	<a href="#">Introduction</a>
<a href="#">Conclusions</a>	<a href="#">References</a>	
<a href="#">Tables</a>	<a href="#">Figures</a>	
<a href="#">◀</a>	<a href="#">▶</a>	
<a href="#">◀</a>	<a href="#">▶</a>	
<a href="#">Back</a>	<a href="#">Close</a>	
<a href="#">Full Screen / Esc</a>		

[Printer-friendly Version](#)

[Interactive Discussion](#)

## Determination of alkyl amines in atmospheric aerosol particles


R.-J. Huang et al.

**Table 3.** Determination of alkyl amines in PM<sub>2.5</sub> collected on 14 May 2012, in Tung Chung, Hong Kong.

Alkyl amine	Concentration (ng m <sup>-3</sup> ), n = 3		Ratio GC-MS/IC
	GC-MS	IC	
MA	6.62 ± 0.35	4.34 ± 0.43	1.5
DMA	24.32 ± 0.95	13.95 ± 0.70	1.7
EA	5.37 ± 0.17	3.82 ± 0.12	1.4
DEA	112.40 ± 3.42	111.86 ± 2.35	1.0
TEA	–	< 6.38	–
PA	0.41 ± 0.01	–	–
BA	1.74 ± 0.09	1.45 ± 0.06	1.2

**Determination of alkyl amines in atmospheric aerosol particles**

R.-J. Huang et al.

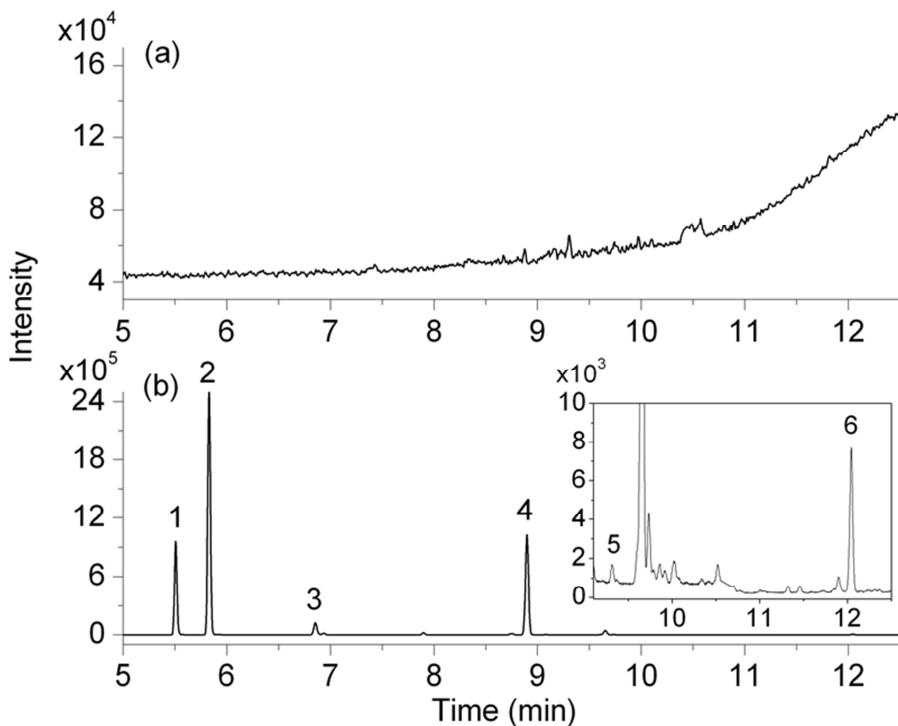


**Fig. 1.** Typical GC-MS chromatograms for the analysis of alkyl amines in ambient aerosol sample before (a) and after (b) derivatization with the derivatizing agent IBCF. Peak assignments: (1) MA, (2) DMA, (3) EA, (4) DEA, (5) PA and (6) BA.

- [Title Page](#)
- [Abstract](#) [Introduction](#)
- [Conclusions](#) [References](#)
- [Tables](#) [Figures](#)
- [◀](#) [▶](#)
- [◀](#) [▶](#)
- [Back](#) [Close](#)
- [Full Screen / Esc](#)

[Printer-friendly Version](#)[Interactive Discussion](#)

**Determination of alkyl amines in atmospheric aerosol particles**

R.-J. Huang et al.

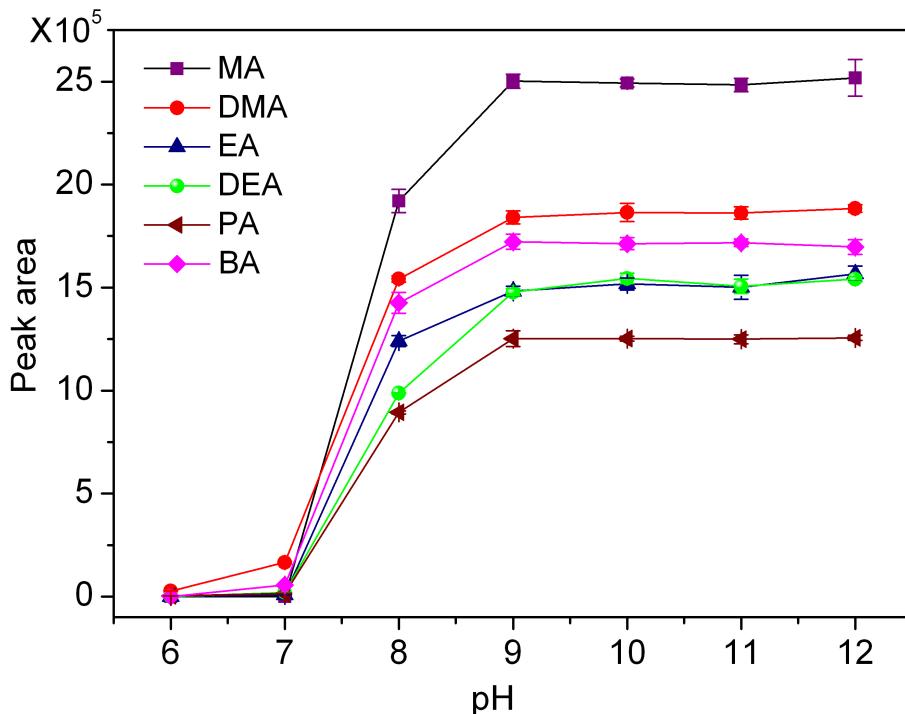
**Fig. 2.** Effect of pH on the derivatization efficiency of different alkyl amines.

[Title Page](#) [Abstract](#) [Introduction](#)  
[Conclusions](#) [References](#)  
[Tables](#) [Figures](#)  
[◀](#) [▶](#)  
[◀](#) [▶](#)  
[Back](#) [Close](#)  
[Full Screen / Esc](#)

[Printer-friendly Version](#)  
[Interactive Discussion](#)


**Determination of alkyl amines in atmospheric aerosol particles**

R.-J. Huang et al.

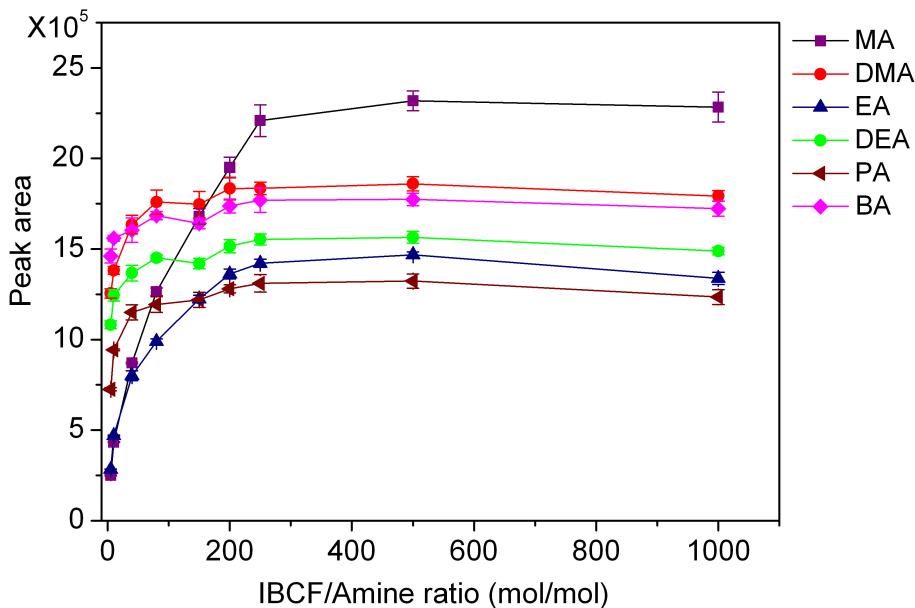**Fig. 3.** Effect of the IBCF amount on the derivatization efficiency of different alkyl amines.

**Determination of alkyl amines in atmospheric aerosol particles**

R.-J. Huang et al.

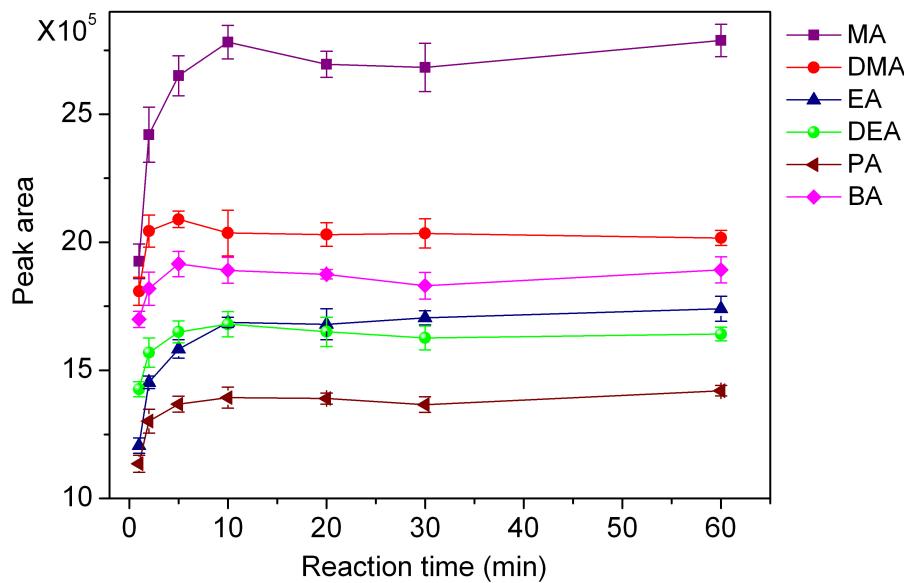
**Fig. 4.** Time-dependent derivatization of different alkyl amines.

- [Title Page](#)
- [Abstract](#) [Introduction](#)
- [Conclusions](#) [References](#)
- [Tables](#) [Figures](#)
- [◀](#) [▶](#)
- [◀](#) [▶](#)
- [Back](#) [Close](#)
- [Full Screen / Esc](#)

[Printer-friendly Version](#)[Interactive Discussion](#)

**Determination of alkyl amines in atmospheric aerosol particles**


R.-J. Huang et al.

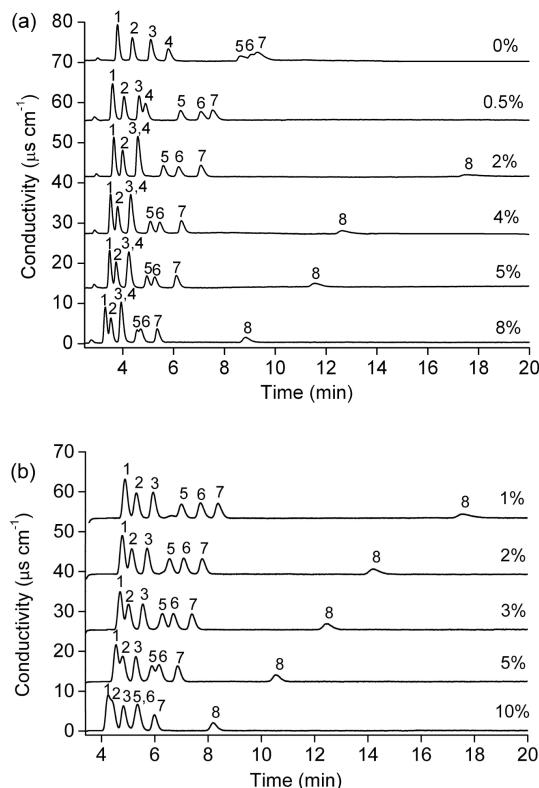

**Fig. 5.** Effect of the addition of acetonitrile **(a)** and acetone **(b)** in eluent solution (6 mM HNO<sub>3</sub>) on the IC separation of alkyl amines. Peak assignments: (1) MA, (2) EA, (3) DMA, (4) PA, (5) BA, (6) DEA, (7) TMA and (8) TEA. Note that PA was not studied in **(b)** because its concentration is very low in the ambient samples, as shown in Table 3.

**Determination of alkyl amines in atmospheric aerosol particles**

R.-J. Huang et al.

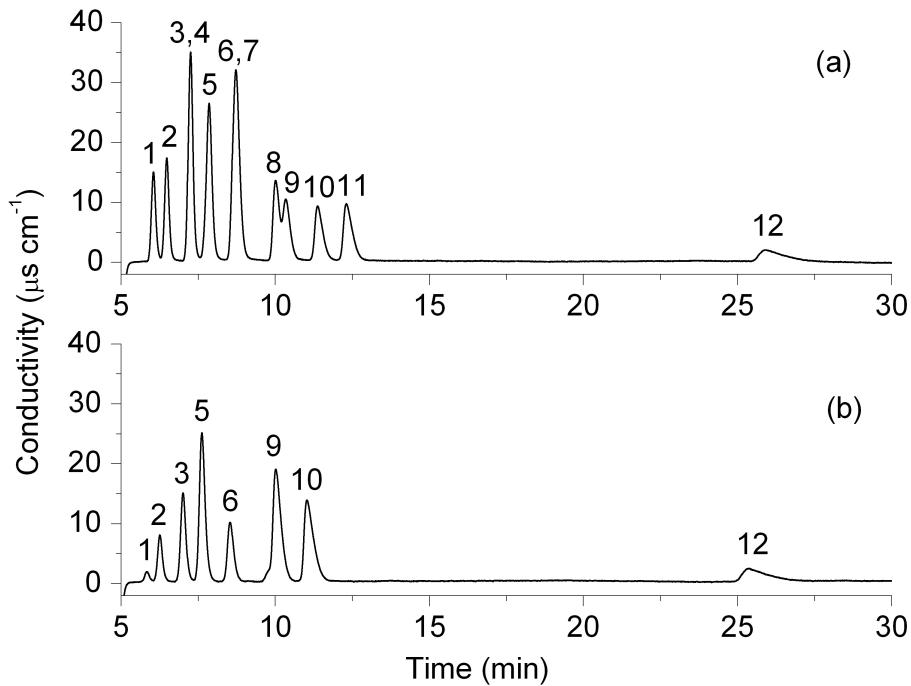

**Fig. 6.** IC chromatograms of alkyl amines before (a) and after (b) SPE pre-separation to minimize the interfering ions. Peak assignments: (1)  $\text{Na}^+$ , (2)  $\text{NH}_4^+$ , (3) MA, (4)  $\text{K}^+$ , (5) EA, (6) DMA, (7)  $\text{Mg}^{2+}$ , (8)  $\text{Ca}^{2+}$ , (9) BA, (10) DEA, (11) TMA and (12) TEA. Note that ~85 % of TMA was lost by evaporation during the concentration step after SPE, reflected in the absence of TMA peak in (b).