

Supplement of Atmos. Meas. Tech. Discuss., 7, 5223–5249, 2014
<http://www.atmos-meas-tech-discuss.net/amtd-7-5223-2014/>
doi:10.5194/amtd-7-5223-2014-supplement
© Author(s) 2014. CC Attribution 3.0 License.



Supplement of

Collection efficiency of the Soot-Particle Aerosol Mass Spectrometer (SP-AMS) for internally mixed particulate black carbon

M. D. Willis et al.

Correspondence to: M. D. Willis (megan.willis@mail.utoronto.ca) and T. B. Onasch (onasch@aerodyne.com)

Collection Efficiency of the Soot-Particle Aerosol Mass Spectrometer (SP-AMS) for Internally Mixed Particulate Black Carbon

Supplementary Information

M.D. Willis, A.K.Y. Lee, T.B. Onasch, E.C. Fortner, L.R. Williams,
A.T.Lambe, D.R. Worsnop, and J.P.D. Abbatt

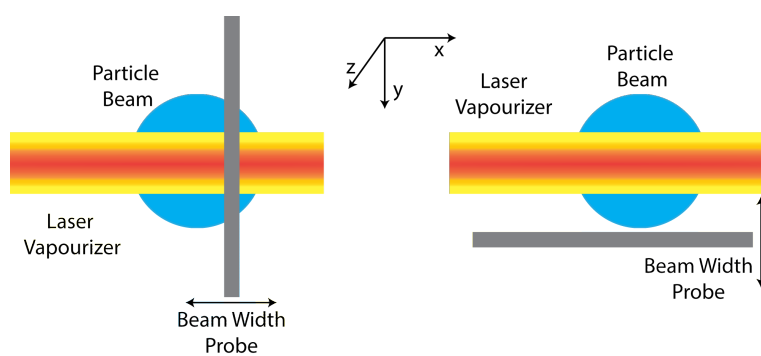


Figure S1: Schematic of beam width probe orientation. Left: BWP orientation for particle beam width measurements, the BWP is situated perpendicular to the laser beam and is moved horizontally. Right: BWP orientation for effective laser beam width estimation, the BWP is moved vertically.

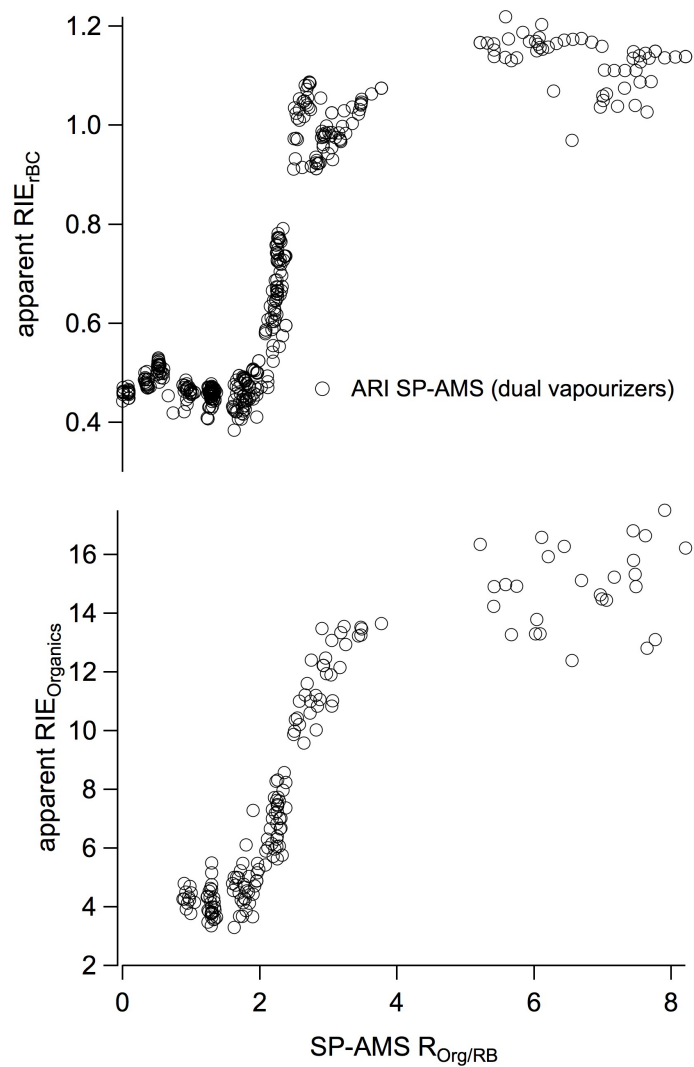


Figure S2: $RIE_{rBC,app}$ (top) and $RIE_{Org,app}$ (bottom) measured as a function of BES coating thickness, demonstrating an increase in sensitivity that reaches saturation at $R_{Org/RB} \sim 3$. Data are plotted against SP-AMS derived $R_{Org/RB}$ because particle mass analyzer measurements were not available during this experiment. $RIE_{Org,app}$ values were obtained from SP-AMS data using measured d_{va} values and assuming that coated particles have a core-shell structure. Data from ARI SP-AMS (SN 215-039).

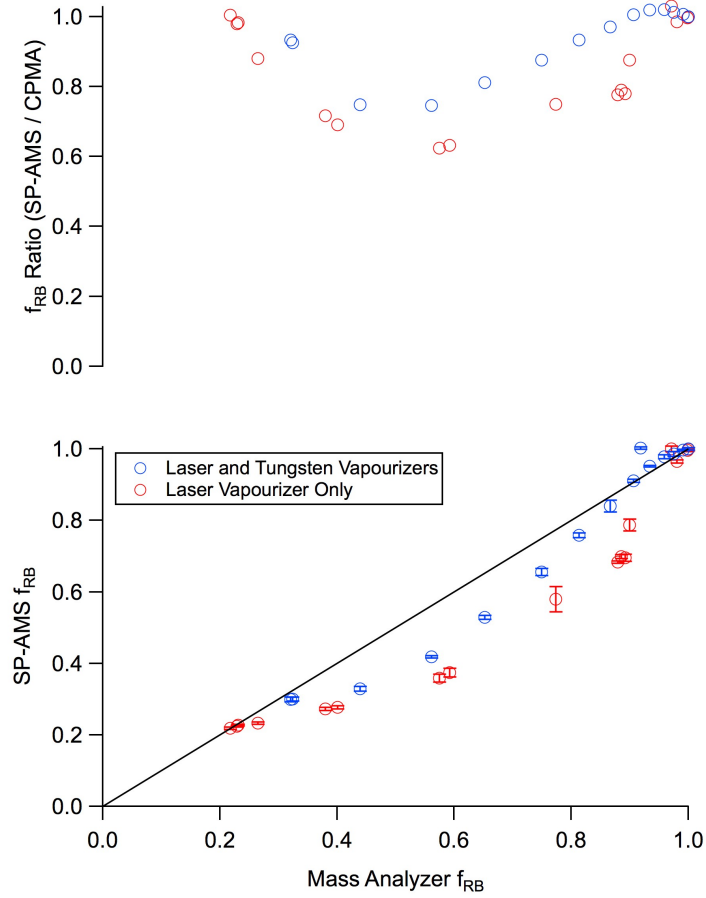


Figure S3: Top: The ratio of SP-AMS fraction of Regal Black (f_{RB}) to the particle mass analyzer f_{RB} as a function of $R_{Org/RB}$. Data from ARI SP-AMS (SN 215-039 (blue) and 215-130 (red)) showing an approximately 40% underestimate in f_{RB} when CE effects are not accounted for. Bottom: The fraction of Regal Black in BES coated particles (f_{RB}), obtained from particle mass measurements, plotted against the fraction of Regal Black obtained from SP-AMS mass loadings using uncorrected RIE_{TBC} (0.2) and RIE_{Org} (1.4).