

MAX-DOAS measurements of HONO slant column densities during the MAD-CAT Campaign: inter-comparison, sensitivity studies on spectral analysis settings, and error budget

5 Yang Wang^{1,2}, Steffen Beirle¹, Francois Hendrick³, Andreas Hilboll^{4,5}, Junli Jin^{6,7}, Aleksandra A. Kyuberis⁸, Johannes Lampel^{9,1}, Ang Li², Yuhua Luo², Lorenzo Lodi¹⁰, Jianzhong Ma⁶, Monica Navarro¹¹, Ivan Ortega¹², Enno Peters⁴, Oleg L. Polyansky^{10,8}, Julia Remmers¹, Andreas Richter⁴, O. Puentedura¹¹, Michel Van Roozendael³, André Seyler⁴, Jonathan Tennyson¹⁰, Rainer Volkamer¹², Pinhua Xie^{2,13}, Nikolai F. Zobov⁸ and Thomas Wagner¹

10 ¹ Max Planck Institute for Chemistry, Mainz, Germany

² Anhui Institute of Optics and Fine Mechanics, Key laboratory of Environmental Optics and Technology, Chinese Academy of Sciences, Hefei, 230031, China

³ Belgian Institute for Space Aeronomy – BIRA-IASB, Brussels, Belgium

⁴ Institute of Environmental Physics, University of Bremen, Bremen, Germany

15 ⁵ Center for Marine Environmental Sciences (MARUM), University of Bremen, Bremen, Germany

⁶ Chinese Academy of Meteorological Sciences, Beijing, China

⁷ CMA Meteorological Observation Centre, Beijing, China

⁸ Institute of Applied Physics, Russian Academy of Sciences, Nizhny Novgorod, Russia

⁹ Institute of Environmental Physics, University of Heidelberg, Heidelberg, Germany

20 ¹⁰ Department of Physics and Astronomy, University College London, Gower St, London WC1E 6BT, UK

¹¹ Área de Investigación Instrumentación Atmosférica, INTA, Torrejón de Ardoz, Spain

¹² Department of Chemistry and Biochemistry, University of Colorado, Boulder, CO, USA

25 ¹³ CAS Center for Excellence in Urban Atmospheric Environment, Institute of Urban Environment, Chinese Academy of Sciences, Xiamen, 361021, China

Correspondence to: Yang Wang (y.wang@mpic.de); Ang Li (angli@aiofm.ac.cn)

Abstract.

In order to promote the development of the passive DOAS technique the Multi Axis DOAS – Comparison campaign for Aerosols and Trace gases (MAD-CAT) was held at the Max Planck Institute for Chemistry in Mainz, Germany from June to 30 October 2013. Here, we systematically compare the differential slant column densities (dSCDs) of nitrous acid (HONO) derived from measurements of seven different instruments. We also compare the tropospheric difference of SCDs (delta SCD) of HONO, namely the difference of the SCDs for the non-zenith observations and the zenith observation of the same elevation sequence. Different research groups analysed the spectra from their own instruments using their individual fit software. All the fit errors of HONO dSCDs from the instruments with cooled large-size detectors are mostly in the range of 35 0.1 to 0.3×10^{15} molecules cm^{-2} for an integration time of 1 min. The fit error for the mini MAX-DOAS is around 0.7×10^{15} molecules cm^{-2} . Although the HONO delta SCDs are normally smaller than 6×10^{15} molecules cm^{-2} , consistent time series of HONO delta SCDs are retrieved from the measurements of different instruments. Both fits with a sequential Fraunhofer reference spectrum (FRS) and a daily noon FRS lead to similar consistency. Apart from the mini-MAX-DOAS, the

systematic absolute differences of HONO delta SCDs between the instruments are smaller than 0.63×10^{15} molecules cm^{-2} . The correlation coefficients are higher than 0.7 and the slopes of linear regressions deviate from unity by less than 16% for the elevation angle of 1° . The correlations decrease with an increase of elevation angle. All the participants also analysed synthetic spectra using the same baseline DOAS settings to evaluate the systematic errors of HONO results from their 5 respective fit programs. In general the errors are smaller than 0.3×10^{15} molecules cm^{-2} , which is about half of the systematic difference between the real measurements.

The differences of HONO delta SCDs retrieved in the selected three spectral ranges 335-361nm, 335-373nm and 335-390nm are considerable (up to 0.57×10^{15} molecules cm^{-2}) for both real measurements and synthetic spectra. We performed 10 sensitivity studies to quantify the dominant systematic error sources and to find a recommended DOAS setting in the three spectral ranges. The results show that water vapour absorption, temperature and wavelength dependence of O_4 absorption, temperature dependence of Ring spectrum, and polynomial and intensity offset correction all together dominate the systematic errors. We recommend a fit range of 335-373nm for HONO retrievals. In such fit range the overall systematic 15 uncertainty is about 0.87×10^{15} molecules cm^{-2} , much smaller than those in the other two ranges. The typical random uncertainty is estimated to be about 0.16×10^{15} molecules cm^{-2} , which is only 25% of the total systematic uncertainty for most 20 of the instruments in the MAD-CAT campaign. In summary for most of the MAX-DOAS instruments for elevation angle below 5° , half daytime measurements (usually in the morning) of HONO delta SCD can be over the detection limit of 0.2×10^{15} molecules cm^{-2} with an uncertainty of $\sim 0.9 \times 10^{15}$ molecules cm^{-2} .

1 Introduction

Nitrous acid (HONO) is an important precursor of the OH radical, which prominently controls the self-cleaning capacity of 20 the troposphere (Alicke et al., 2003; Kleffmann et al., 2005; Acker et al., 2006; Monks et al., 2009; Elshorbagy et al., 2010). The gas-phase reaction of NO with the OH radical (Stuhl and Niki, 1972 and Pagsberg et al., 1997) mostly determines the daytime HONO concentration. However, recent field measurements (Neftel et al., 1996; Kleffmann et al., 2005; Sörgel et al., 2011; Li et al., 2012 and 2014 and Wong et al., 2012) and laboratory studies (Akimoto et al., 1987; Rohrer et al., 2005) 25 reported much larger HONO concentrations than predicted by the gas-phase reactions. These findings imply some missing daytime sources of HONO. Laboratory and field studies suggest that the missing daytime sources consist of heterogeneous reactions on various surfaces such as the ground, forests, buildings, and aerosols (Su et al., 2008 and 2011; Li et al., 2014; and references therein), emissions from soil (Su et al., 2011 and references therein), and a potential gas-phase reaction between HO_x and NO_x (Li et al., 2014).

The overall effect of the proposed missing HONO sources in the troposphere remains widely unknown because of the lack of 30 measurements of HONO and its relevant precursor species at higher altitudes above the ground (Li et al., 2014). The surface HONO concentrations can be well quantified by ground-based in-situ instruments, like the LOPAP (long path absorption photometer) technique (Heland et al., 2001; Kleffmann et al., 2006 and Li et al., 2012) and long-path DOAS (Trick, 2004

and references therein). Besides these techniques, four other optical absorption techniques have been used for the detection of HONO, i.e., cavity ring down spectroscopy (Wang and Zhang, 2000), FTIR spectroscopy (Hanst et al., 1982), tunable diode laser spectroscopy (Schiller et al., 2001) and CE-DOAS (Hoch et al., 2014). To quantify the distribution of HONO in elevated layers of the troposphere, the in-situ LOPAP technique has been mounted aboard on an airship Zeppelin platform 5 (Li et al., 2014). However, because of the large cost of operating such a flight platform, the corresponding data sets are limited in time and space.

Since about 15 years ago, the Multi Axis - Differential Optical Absorption Spectroscopy (MAX-DOAS) technique, which is based on the DOAS spectral analysis technique (Platt and Stutz, 2008, and references therein), has been widely used owing to its potential to retrieve the vertical distribution of trace gases and aerosols in the lower part of the troposphere from 10 scattered sunlight spectra recorded at multiple elevation angles using relatively simple and low-cost ground-based instrumentation (Hönniger and Platt, 2002; Bobrowski et al., 2003; Van Roozendael et al., 2003; Hönniger et al., 2004; Wagner et al., 2004 and Wittrock et al., 2004). Hendrick et al. (2014) reported the first MAX-DOAS measurements of vertical column densities (VCDs) and near-surface volume mixing ratios (VMRs) of HONO in the Beijing area, China. Because of its simple and automatic operation at the ground, MAX-DOAS is well suited to continuously acquire HONO 15 vertical distributions over longer time periods. However, due to the typically low HONO VMRs in the troposphere (between about 50 ppt to 2000 ppt near the surface in urban areas (Li et al., 2012)) and the moderate cross section with the maximum of about $5 \times 10^{-19} \text{ cm}^2 \text{ molecules}^{-1}$ in the UV range, the atmospheric HONO absorption is rather weak, and it can also be systematically interfered by strong absorptions of other trace gases (e.g. O₃ and NO₂) and instrument-related spectral structures. So far few efforts have been devoted to study these error sources in HONO DOAS fits of MAX-DOAS spectra. 20 Furthermore, many research groups have developed their own MAX-DOAS instruments equipped with various types of spectrometers, detectors, and entrance optics. Thus the inter-comparison of HONO measurements and retrieval results from different MAX-DOAS instruments is essential to evaluate MAX-DOAS HONO results and associated uncertainties.

The Multi Axis DOAS – Comparison campaign for Aerosols and Trace gases (MAD-CAT) held at the Max Planck Institute for Chemistry in Mainz, Germany in June and July 2013 (http://joseba.mpch-mainz.mpg.de/mad_cat.htm). During MAD- 25 CAT campaign, eleven MAX-DOAS instruments from different groups (listed in the website of <http://joseba.mpch-mainz.mpg.de/equipment.htm>) were operated in parallel, providing an opportunity to assess the consistency of different HONO measuring MAX-DOAS systems for the first time. In this study, only the direct output values, namely the slant column density (SCD) of HONO in the troposphere, derived from the spectral analysis (DOAS fit) of the acquired MAX-DOAS spectra are compared between the instruments and discussed with respect to their systematic error sources based on 30 sensitivity tests. The inter-comparison activities in this study follow similar work done for NO₂ and HCHO during the Cabauw Intercomparison campaign of Nitrogen Dioxide measuring Instruments (CINDI) (Piters et al., 2012) in The Netherlands in June–July 2009 (Roscoe et al., 2010 and Pinardi et al., 2013).

In addition to the measured spectra, a set of synthetic spectra generated by the SCIATRAN radiative transfer model (RTM) (Rozanov et al., 2014) was analysed for the first time. These spectra are simulated based on various atmospheric scenarios

including not only HONO, but also other relevant trace gases and aerosols. Because the HONO SCDs of the synthetic spectra are known, the bias of the retrieved SCDs from the true values can be easily quantified.

This paper is structured as follows. Section 2 gives an overview of the MAD-CAT campaign and participating instruments. Section 3 presents inter-comparison results of the HONO SCD derived from real measurements and synthetic spectra 5 between the participants. In Section 4 we focus on sensitivity tests to assess possible interferences in the HONO SCD retrievals. Recommended analysis settings are given together with an error budget in Section 5. The conclusions are presented in Section 6.

2 Field experiment

2.1 The MAD-CAT inter-comparison campaign

10 The Multi Axis DOAS – Comparison campaign for Aerosols and Trace gases (MAD-CAT) was held at the Max Planck Institute for Chemistry (MPIC) in Mainz, Germany. The measurement site is located in the outskirts of the city of Mainz, close to agricultural fields in the west. The large city of Frankfurt am Main with about 0.7 million inhabitants is about 30 km away from the measurement site in the northeast. All the MAX-DOAS instruments from eleven participating groups were operated on the roof of MPIC during the intensive measurement phase from 7 June until 6 July, 2013. Only the 15 measurements in the period from 12 June to 5 July are included in the HONO inter-comparison activity due to the time coverage of the participating instruments. Although many of the instruments are designed to measure in various azimuth angles, in this study only the measurements in the main azimuth direction of 51 °northeast are included. The same elevation angle sequence of 1 °, 2 °, 3 °, 4 °, 5 °, 6 °, 8 °, 10 °, 15 °, 30 ° and 90 ° was applied by all instruments. A description of the MAD-CAT measurement campaign can be found at http://joseba.mpch-mainz.mpg.de/mad_cat.htm. Data from this campaign has 20 been so far used e.g. in Ortega et al. (2015), Lampel et al. (2015 and 2016b) and Peters et al. (2016).

2.2 Instruments

25 Seven of the eleven groups participated in the HONO inter-comparison activity. The primary information on the instruments is listed in Tab. 1. The instruments use different types of detectors, spectrometers and optical systems. Except the instrument of CMA, which is a “mini-MAX-DOAS” from Hoffmann Messtechnik GmbH in Germany, all other instruments are self-built. Only the mini-MAX-DOAS instrument integrates the entrance optics and fibre coupled spectrograph in a hermetically sealed metal box positioned outdoors. The other six instruments have two separate parts: one is indoors with a fibre coupled spectrograph located in a temperature stabilised box; the other is outdoors with the entrance optics and pointing telescope. The Heidelberg and CMA instruments used small-size compact spectrographs. The other instruments were equipped with large size spectrometers with thermoelectrically cooled imaging CCD array detectors. The 30 data availability from the different instruments is shown in Supplementary Fig. S1. Because the different instruments applied

different integration times (see Tab. 1) and scanning speeds, and also partly performed measurements in other directions, different numbers of elevation sequences per hour are acquired (see Fig. S1 in the Supplement). Typical numbers of elevation sequences per hour range from 2.8 (BIRA) to 9.4 (MPIC).

3. Results and inter-comparison

5 HONO presents prominent absorption structures in the spectral range from 335 to 390 nm. The DOAS technique (Platt and Stutz, 2008, and references therein) can be applied to spectra of scattered sunlight to retrieve SCDs of HONO. In this section we present the inter-comparison of HONO SCD results derived from real measurements and synthetic spectra between the participants. For the analyses of both sets of spectra, recommended baseline settings for the DOAS spectral analysis are provided. These baseline setting are derived from the sensitivity studies outlined in section 4 and also based on the
10 experiences in Hendrick et al. (2014). The details of the baseline setting are given in Table 2 and described in section 3.1.

3.1 Baseline HONO analysis settings

The sensitivity studies in section 4 indicate that the wavelength range of 335 to 373 nm is the optimal choice for the baseline DOAS settings because of the low systematic error in that wavelength range. A similar wavelength range of 337 to 375 nm was also used in Hendrick et al. (2014). The slightly different wavelength range compared to Hendrick et al. (2014) is due to
15 the limitation of the upper edge of the wavelength range of the Bremen instrument. Absorption cross sections of HONO, NO₂, O₃, BrO, O₄, and HCHO were convolved to the spectral resolution of the individual instruments and included in the fit. The solar I₀ correction was applied to the O₃ and NO₂ cross sections (Aliwell et al., 2002). To correct the wavelength dependence of the NO₂ AMF (see Section 4.5), the Taylor series terms of $\lambda\sigma_{NO_2}$ and $\sigma_{NO_2}^2$ (with λ the wavelength, and σ_{NO_2} the NO₂ cross section) (Pukite et al., 2010) (the details are given in section 4.5) were included in the fit. The effect of
20 rotational Raman scattering was considered by including a Ring spectrum (Shefov 1959; Grainger and Ring, 1962; Chance and Spurr, 1997; Solomon et al., 1987; Wagner et al., 2009). The Ring spectrum was calculated according to Chance and Spurr (1997) based on the high resolution solar atlas of Kunucz et al. (1984) for a temperature of 250 K and convoluted to the respective instrumental resolution. To account for different wavelength dependencies of the filling-in in clear and cloudy skies, an additional Ring spectrum as described in Wagner et al. (2009) was included.

25 To correct for the strong Fraunhofer lines, a Fraunhofer reference spectrum (FRS) I_{FRS} was included in the DOAS fit of a measured spectrum I_m as indicated in Eq. (1):

$$I_m = I_{FRS} \times e^{-\sigma \times (SCD_m - SCD_{FRS}) + P} = I_{FRS} \times e^{-\sigma \times dSCD + P} \quad (1)$$

Where σ is HONO cross section; SCD_m and SCD_{FRS} are the SCD of HONO of the measured spectra and the FRS, respectively; P represents absorptions of other trace gases and scatterings. Therefore the difference of SCD_m and SCD_{FRS} is
30 retrieved from the DOAS fits and usually referred to as differential SCD (dSCD).

Thus the SCDs from the DOAS fits actually represent the difference between the SCD of the measured spectra and the FRS. This difference is usually referred to as differential SCD (dSCD).

Equation 1 can be further written as Eq.2,

$$I_m = I_{FRS} \times e^{-\sigma \times (SCD_m^{Trop} + SCD_m^{Strat} - SCD_{FRS}^{Trop} - SCD_{FRS}^{Strat}) + P} \quad (2)$$

5 Where SCD_m and SCD_{FRS} are separated as tropospheric (SCD_m^{Trop} and SCD_{FRS}^{Trop}) and stratospheric (SCD_m^{Strat} and SCD_{FRS}^{Strat}) SCDs. If the zenith measurement in the same elevation sequence as the off-axis spectra is used as I_{FRS} such a FRS is referred to as “sequential FRS” in this study, Because the stratospheric light path only substantially depends on the SZA but not the elevation angle (Clément et al., 2010; Peters et al., 2012; Hendrick, 2014), it follows:,

$$SCD_m^{Strat} \approx SCD_{FRS}^{Strat} \quad (3)$$

10 Therefore Eq. 2 can be written as Eq. 4,

$$I_m \approx I_{FRS} \times e^{-\sigma \times (SCD_m^{Trop} - SCD_{FRS}^{Trop}) + P} \quad (4)$$

It indicates the difference of the tropospheric SCDs and is extracted from the DOAS fit with a sequential Fraunhofer reference and is usually referred to as delta SCDs (Hönniger et al. 2004).

15 The delta SCDs can be also extracted by another approach. First retrieving the dSCDs for all the elevation angles (including zenith view) using a single zenith spectrum (typically around noon) on one day. This FRS is referred to as “daily noon FRS” in this study. The dSCDs for off-zenith ($dSCD_m$) and zenith views ($dSCD_{zenith}$) in the same elevation sequence are indicated as Eq. 5 and 6, respectively,

$$dSCD_m = SCD_m^{Trop} + SCD_m^{Strat} - SCD_{FRS}^{Trop} - SCD_{FRS}^{Strat} \quad (5)$$

$$dSCD_{zenith} = SCD_{zenith}^{Trop} + SCD_{zenith}^{Strat} - SCD_{FRS}^{Trop} - SCD_{FRS}^{Strat} \quad (6)$$

20 Subtracting $dSCD_{zenith}$ from the respective $dSCD_m$ in the corresponding elevation sequence (Hönniger et al. 2004; Pinardi et al., 2013 and Ma et al., 2013) is represented as Eq. 7

$$dSCD_m - dSCD_{zenith} = SCD_m^{Trop} + SCD_m^{Strat} - SCD_{zenith}^{Trop} - SCD_{zenith}^{Strat} \quad (7)$$

Same with Eq. 3, $SCD_m^{Strat} \approx SCD_{zenith}^{Strat}$ because of the similar light path in the stratosphere for the off-zenith and zenith view in the same elevation sequence.

25 Therefore the delta SCDs is derived as shown in Eq. 8.

$$\text{delta SCD} = dSCD_m - dSCD_{zenith} \approx SCD_m^{Trop} - SCD_{zenith}^{Trop} \quad (8)$$

In principle the delta SCDs from the two schemes should be the same, but the fits using a daily noon FRS are usually more strongly affected by changes of instrumental properties and interferences of stratospheric absorptions (e.g. O_3) than those using a sequential FRS. To quantify the effect of the different types of FRS, we compare the HONO delta SCDs from both 30 methods.

3.2 Results of HONO delta SCDs and dSCDs, and fit errors

Figure 1 presents examples of DOAS fits of one spectrum measured by the AIOFM instrument using the baseline setting with either the sequential FRS (left) or daily noon FRS (right), respectively. The fits were performed using the WINDOAS software (Fayt and van Roozendael, 2009). The HONO absorption structures are well retrieved using both types of FRS. The difference of the retrieved HONO dSCDs between the two fits is mainly due to the different HONO absorption in the two FRS. The same reason also leads to the differences of the retrieved dSCDs of the other trace gases. The difference is substantially larger for the trace gases with considerable stratospheric contributions, e.g. O₃ and BrO, because the stratospheric light paths around noon for the daily noon FRS are much shorter than those during sunset or sunrise. Also the root mean square (RMS) of the fit residual of 4.5×10^{-4} (corresponding to a HONO dSCD error of 2.6×10^{14} molecules cm⁻²) using a sequential FRS is slightly smaller than the RMS of 5.7×10^{-4} (corresponding to HONO dSCD error of 3.1×10^{14} molecules cm⁻²) using a daily noon FRS.

Figure 2a shows the hourly averaged HONO delta SCDs at 1° elevation angle derived from the measurements of the AIOFM instrument during the whole comparison period; Figure 2b shows the corresponding averaged diurnal variation. A large variability of the HONO delta SCDs is found between -1×10^{15} molecules cm⁻² (negative value probably due to the effect of water vapour absorption, see Section 4.1) and 5×10^{15} molecules cm⁻². In general, the highest values are found in the morning. In addition to the HONO delta SCDs, delta SCDs of oxygen dimer (O₄) are also shown in Fig. 2. Since the atmospheric O₄ mixing ratio is rather constant and well known, variations of the O₄ delta SCDs can be used as an indicator for variations of the atmospheric absorption path length (e.g. Erle et al., 1995; Hönniger et al., 2004; Sinreich et al., 2013; Wang et al., 2014; and references therein). As can be seen in Fig. 2b, the delta SCDs of HONO and O₄ show systematically different diurnal variations indicating that the observed variation of the HONO delta SCDs is not an artefact caused by the variation of the light path length but mainly reflects the variation of the atmospheric HONO concentration.

HONO dSCDs are retrieved by each group using the same baseline analysis settings as shown in Tab. 2. For the inter-comparison of the different data sets, we first averaged the HONO dSCDs for individual elevation angles of each instrument during periods of one hour, in which all the instruments have more than two measurement sequences (see Fig. S1 in the Supplement).

Figure 3 shows an example of the time series of the hourly averaged HONO delta SCDs for individual elevation angles derived from each instrument using the fits with a sequential or a daily noon FRS as well as the HONO dSCDs using a daily noon FRS on 3 July 2013. The results for the five selected elevation angles are shown in Fig. 3. Similar results are also found for the other elevation angles, see Supplementary Fig. S2. On this day all the instruments provide credible data, and also rather large HONO dSCDs and delta SCDs are observed in the morning, in particular at lower elevation angles. The large HONO values in the morning could be due to a high NO₂ concentration (NO₂ dSCD of up to 1×10^{17} molecules cm⁻²) and a fast photolysis of HONO (e.g. Hendrick et al., 2014). Note, however, that because of unknown instrumental problems, CMA and Boulder didn't participate in the comparisons of the delta SCDs for a sequential FRS and dSCDs for a daily noon FRS,

respectively, but other instruments are not affected. As can be seen in Fig. 3, much better agreements between the instruments are obtained for the delta SCDs than for the dSCDs; From all instruments a similar diurnal evolution and elevation angle dependence of the HONO delta SCDs is retrieved. A detailed quantitative analysis of the deviations of the HONO results between the instruments is provided in the statistical analysis in section 3.3

5 Figure 4a presents the hourly averaged fit errors of the HONO dSCDs using a daily noon FRS plotted against the solar zenith angle (SZA) for the whole comparison period. The fit errors depend on the random and systematic structures of the spectral residual. Systematic structures are mainly caused by instrumental shortcomings, possible non-considered atmospheric absorption structures, as well as imperfect corrections of rotational Raman scattering, temperature dependences of atmospheric absorptions, and wavelength dependences of absorption light paths (namely air mass factor (AMF)). Increasing

10 fit errors with increasing SZA are found for all the instruments due to the reduction of the solar radiance and the increase of stratospheric absorptions (e.g. ozone). In addition fit errors of HONO dSCD under cloudy and clear days are quite similar due to the fact that the MAX-DOAS instruments automatically change the exposure time of spectrometer based on the brightness of the sky. Therefore the similar exposure saturation level is reached during clear and cloudy days. The largest fit

15 error is found for the CMA instrument due to the relatively low signal to noise ratio of the detector. The second largest fit error is found for the MPIC instrument due to the very short integration time (Fig. 4b). The fit errors of other instruments are similar and in the range 0.15×10^{15} molecules cm^{-2} to 0.5×10^{15} molecules cm^{-2} for $\text{SZA} < 60^\circ$. Because the random noise of an instrument depends on integration time, which is different for different instruments (see Fig. 4b), the fit errors are scaled to a typical integration time of 1 minute in order to make the results directly comparable (see Fig. 4c). Note that we applied a linear scaling, which is not strictly correct since the photon noise shows a square-root dependency of the number of observed

20 photons. However, since the MAX-DOAS instruments are not radiometrically calibrated, we applied a linear scaling to achieve a first order normalisation for the effect of the integration time. Similar normalized fit errors are found for the instruments using cooled large-size detectors (BIRA, Bremen, AIOFM, Boulder and MPIC). Although both the Heidelberg and CMA instruments use compact spectrometers, Fig. 4c demonstrates that the Avantes spectrometer (<http://www.avantes.com>) in the Heidelberg instrument has a much lower noise level than the ocean optics USB 2000

25 (<http://oceanoptics.com/>) in the CMA instrument. Figure 4d also indicates that the fit errors with daily noon FRS are generally higher than those with sequential FRS for all instruments. The difference is especially large for the Bremen instrument, probably due to a known temperature stability problem of the spectrometer during the MADCAT campaign.

Because of the instrumental straylight, possible imperfect correction of the dark current and electronic offset signal in the measured spectra, and vibrational Raman scattering (Lampel et al., 2015), usually an intensity offset correction is included

30 in the DOAS fit procedure (e.g. Noxon, 1975; Fayt and van Roozendael, 2009). However, the effect of spectral straylight and its correction by the intensity offset fit could interfere with retrievals of the species with low optical depths (Coburn, 2011). It is known that spectral straylight typically depends on the sky colour. Thus the strength of the corresponding spectral interferences also depends on the actual sky condition during the measurement. The fitted intensity offsets for most of the instruments are lower than 1% of the mean intensity in the fit window for analyses with both types of FRS (details can

be found in the Supplementary Figs. S3a and b). Much larger offsets are found only for the CMA instrument, especially in the morning and afternoon.

The shift of the wavelength calibration of the measured spectra with respect to the FRS is mathematically determined and corrected in the DOAS fit procedure. The wavelength shift can be caused by the tilt effect (typically <2pm) (Lampel et al., 5 2017) and dominated by the mechanical deformation of a spectrometer, which is usually sensitive to variations of the ambient temperature. The averaged diurnal variations of the shifts derived from the fits with a daily noon FRS and a sequential FRS are smaller than 0.015nm and 0.05nm, respectively (the detailed results can be found in the Supplementary Fig. S3c and d, respectively). As expected, the shifts for the sequential FRS are much smaller than those for the daily noon FRS.

10 **3.3 Statistical inter-comparisons**

In this Section, we apply the statistical analysis method introduced in Roscoe et al. (2010) and Pinardi et al. (2013) to the inter-comparison of HONO results (delta SCDs and dSCDs) from the individual instruments. The results from the Heidelberg, BIRA, Bremen, and AIOFM instruments are averaged as reference values because of their almost full time coverage, low fitting errors, and good agreement. In addition the selection is also because the Boulder and CMA instruments 15 are affected by some unknown instrumental problems. In the following discussions, we assume the reference values as the truth, but this is not necessarily the case. We implement two methods for the comparisons:

- 1) To derive an overview of the general agreement between the retrieval results by different instruments for the whole measurement period, mean absolute differences and standard deviations of HONO results from the reference values are summarized for individual elevation angles. Meanwhile a set of histograms of the absolute differences is prepared.
- 20 2) To investigate how well the different instruments capture the diurnal variation of the HONO dSCDs, for eight selected days with pronounced diurnal variations of the HONO dSCDs and delta SCDs (12, 15, 17, 18 and 30 June as well as 1, 2 and 3 July 2013), a set of scatter plots with linear regressions of the results from the different instruments against the reference values is prepared.

We performed the two comparisons for the two HONO delta SCDs from the fits with a sequential FRS or a daily noon FRS 25 as well as for the HONO dSCDs with a daily noon FRS. Note that in the figures below, only the results for the elevation angles 1°, 3°, 5°, 8°, 15° (also 90° only for dSCDs with a daily noon FRS) are shown, but similar conclusions can be drawn for the other elevation angles. The mean absolute differences and standard deviations as well as the correlation coefficients, slopes and intercepts of the linear regressions derived from comparisons of HONO dSCDs (noon FRS) and delta SCDs of different instruments with respect to the reference values are presented in Fig. 5. In general linear correlations of the three 30 HONO results decrease with an increase of elevation angle for all the instruments, probably due to the low values and small value ranges. However, there are no dependences of the absolute differences and standard deviations on the elevation angles for most of the instruments, except the CMA instrument. The comparison results of HONO delta SCDs derived the fits with either a sequential FRS or a daily noon FRS are quite similar with each other, however mostly different from those of HONO

dSCDs with a daily noon FRS, for individual instruments. In the following we separately discuss the comparisons of three HONO results.

For the HONO delta SCDs with a sequential FRS, figure 5 indicates that larger standard deviations are found for MPIC ($\sim 0.6 \times 10^{15}$ molecules cm^{-2}), Boulder ($\sim 0.3 \times 10^{15}$ molecules cm^{-2}), and Bremen ($\sim 0.3 \times 10^{15}$ molecules cm^{-2}) compared to the other instruments (~ 0.16 to $\sim 0.28 \times 10^{15}$ molecules cm^{-2}), consistent with the fit errors shown in Fig. 4. Also different absolute differences are found for the different instruments: MPIC ($\sim -0.53 \times 10^{15}$ molecules cm^{-2}), BIRA ($\sim 0.34 \times 10^{15}$ molecules cm^{-2}), and Bremen ($\sim -0.23 \times 10^{15}$ molecules cm^{-2}) display larger differences than the other instruments (~ -0.1 to $\sim 0.04 \times 10^{15}$ molecules cm^{-2}). The different absolute differences might be related to possible errors of the elevation angles, interferences of systematic instrumental structures in the fits (e.g., nonlinearity of the detector response and stray light) and differences in the implementations of DOAS fits. The histograms of the absolute differences from the reference values for each instrument are shown in Supplementary Fig. S4. A symmetric and quasi-Gaussian shape of the histograms is found for all the instruments. From the histograms the same standard deviation and the mean absolute differences between the instruments as in Fig. 5 are derived. In addition for the eight selected days with pronounced diurnal variations of the HONO values, linear regressions are performed and slopes and correlation coefficients are derived from the scatter plots of the HONO delta SCDs with a sequential FRS for each instrument against the reference values. The results of the linear regressions and the linear correlation coefficients are displayed in Fig. 5 (the corresponding scatter plots are provided in the supplementary Fig. S5). As can be seen for 1° elevation angle, all instruments agree well: the scatter plots show compact correlations with correlation coefficients mostly larger than 0.95 (a lower value of 0.86 is only found for the MPIC instrument); the slopes are close to unity with deviations smaller than 16% and intercepts smaller than 0.5×10^{15} molecules cm^{-2} . Smaller correlation coefficients and larger deviations of the slopes and intercepts are found for large elevation angles due to the rather low values and the small range of HONO delta SCDs.

For the HONO delta SCDs derived from fits with a daily noon FRS, we follow the same comparison procedures as for the HONO delta SCDs from fits with a sequential FRS. All five parameters shown in Fig. 5 are quite similar to the results for the sequential FRS for all the instruments. Only the slopes for 15° elevation angle are different, but this phenomenon is due to the low HONO delta SCDs and small value ranges. To directly show the agreement of the HONO delta SCDs from the fits with the two types of FRS, the mean biases and standard deviations as well as the correlation coefficients, slopes and intercepts of linear regressions derived from the comparisons of two HONO delta SCDs are presented in Fig. 6 (the corresponding histograms of absolute differences between them and their scatter plots are presented in Supplementary Figs. S6 and S7, respectively). Figure 6 indicates that for each instrument and each elevation angle there are no significant mean differences ($< \pm 0.04 \times 10^{15}$ molecules cm^{-2}) and standard deviations ($< 0.23 \times 10^{15}$ molecules cm^{-2}). The correlation coefficients (> 0.92) and slopes (deviations $< 13\%$) are quite close to unity for all the instruments. Only moderate deterioration of correlation coefficients and slopes for the 15° elevation angle are found for some of the instruments.

For the HONO dSCDs derived from fits with a daily noon FRS shown in Fig. 5, the standard deviations are slightly larger than those for the comparisons of the two HONO delta SCDs. This could be caused by the different HONO absorptions in

the daily noon FRS of the different instruments and interferences by the stratospheric species, e.g. ozone. The correlation coefficients are mostly slightly better than for HONO delta SCDs (except for the BIRA instrument) probably due to the slightly larger values of the HONO dSCDs especially for high elevation angles. For the off-zenith observations, Bremen, AIOFM and MPIC have similar mean differences and intercepts for the HONO dSCDs as those for the HONO delta SCDs, 5 while Heidelberg and BIRA show larger and smaller values. This finding is probably caused by differences of the HONO dSCDs for zenith view between the different instruments. For the CMA instrument, its agreement with the other instruments is better for the HONO dSCDs than for the HONO delta SCDs. The reason could be an unknown instrumental problem of the zenith observations of the CMA instrument.

In general a consistent temporal variation and elevation angle dependence of the HONO delta SCDs and dSCDs has been 10 retrieved from the different instruments. The discrepancy of HONO dSCDs from the fits with a daily noon FRS between the instruments is systematically larger than those of the HONO delta SCDs, which can be consistently retrieved from the fits with a daily noon or a sequential FRS.

3.4 Synthetic spectra and inter-comparisons

In general it is difficult to quantify the biases of the retrieved HONO dSCDs with respect to the true atmospheric state for 15 real MAX-DOAS measurements as the true HONO column is not known. Thus, to assess these biases in more detail, we generated a set of synthetic spectra using the RTM SCIA TRAN, version 3.6.0 (03 Dec 2015), in a pseudo-spherical atmosphere (Rozanov et al., 2014) for the same measurement geometries (elevation angles and azimuth angle) and similar sun geometries (16 combinations of SZA and solar azimuth angle (SAA)) as the real measurements. Detailed information on the RTM simulations is given in Section 1 of the supplement. The simulated delta SCDs at 355nm corresponding to the 20 synthetic spectra are in the range 0.4 to 6×10^{15} molecules cm⁻² (see Supplementary Fig. S8b), covering the range of values of the real measurements (see Fig. 2a). Note that there is no random noise added into the synthetic spectra since the main objective of this study is to quantify the systematic difference of the retrieved values from the truth. Also it was found that noise has a negligible effect on the systematic differences, see Section 4.9.

Two versions of synthetic spectra were generated with different input of water vapour cross sections. The H₂O cross section 25 from the HITRAN 2012 (Rothman et al., 2013) database and from the newly published POKAZATEL line lists (Polyansky et al., 2016) are used by the RTM to generate version (V) 1 and 2 of the synthetic spectra, respectively. Note that absorption structures below 388 nm exist in the POKAZATEL H₂O cross section, but not in HITRAN. Thus actually there is no H₂O absorption included in the UV range (used in this study) of V1 synthetic spectra. The POKAZATEL H₂O absorption around 363 nm was recently identified in MAX-DOAS and Long-path (LP)-DOAS measurements and could impact the HONO 30 retrieval (Lampel et al., 2016). And they also found that the POKAZATEL line lists underestimate the real H₂O cross section by a factor of about 2.6. Thus the POKAZATEL H₂O cross section multiplied by 2.6 is used in the RTM. Both the V1 and V2 synthetic spectra are used in the sensitivity studies presented in Section 4, while only the V1 data set is used for the inter-comparison activities.

Six institutes analysed the V1 synthetic spectra using their respective fit software (see Tab. 1). The DOAS settings are almost the same as those for the inter-comparison of the real measurements presented in Tab. 2. The only difference is that the retrievals are implemented with and without including an intensity offset in the fits. Analyses are performed using a noon (for SAA of 166°) and a sequential FRS. The four settings of the DOAS fits are listed in Tab. 3. Note that only a constant 5 term is used for the setting of including intensity offset correction in the fit, because of the negligible impact on the analyses when including a linear term. Figure 7 shows an example of DOAS fit of the V1 synthetic spectrum for a SAA of 166° and EA of 1° using the setting #4 in Tab. 3. The retrieved optical depths of the relevant species are comparable to those for the real measurement shown in Fig. 2a. And the residual structure is smaller than half of that for the real measurement due to the absence of random noise in the synthetic spectrum. We did the comparisons between the results from the different institutes 10 for the HONO delta SCDs (all the four fit settings) and for the HONO dSCDs (only setting #1 and #2 (noon FRS)). The mean biases and standard deviations as well as the correlation coefficients, slopes and intercepts of the linear regressions derived from the comparisons of HONO dSCDs (noon FRS) and delta SCDs of different groups with respect to the simulated real values as are presented in Fig. 8. The comparison results are plotted against labels of the different DOAS 15 settings in Tab. 3 (the corresponding histograms of the absolute differences and scatter plots are also provided in Supplementary Figs. S9 and S10, respectively). In general, Fig. 8 indicates that much larger mean absolute differences for the dSCDs than for the delta SCDs are found, meanwhile much lower correlations are found for the HONO dSCDs than for the delta SCDs, mainly due to the interference of stratospheric species, e.g. ozone. Correlation coefficients (> 0.91) for the HONO delta SCDs are close to unity for all the groups. The similar mean absolute differences and slopes of HONO delta SCDs between setting #1 and #4 as well as between setting #2 and #3 indicate that the effect of using different FRS on the 20 HONO delta SCDs is negligible for all the groups. However, the effect of intensity offset correction (comparisons between setting #1 and #2 as well as between setting #3 and #4) on the HONO delta SCDs is found to be considerable (about 0.3 to 0.7×10^{15} molecules cm^{-2}) for all the groups. The smallest mean absolute differences of the HONO delta SCDs with respect to the real values are smaller than 0.23×10^{15} molecules cm^{-2} , which are found for setting #1 and #4 (without intensity offset correction) for BIRA, Bremen, AIOFM, MPIC and CMA, and for setting #2 and #3 (with intensity offset correction) for 25 Heidelberg and INTA. The different phenomenon of the intensity offset effect on HONO delta SCD between the two groups of institutes might be caused by differences in the implementation of intensity offset correction in the DOAS fit software codes. Peters et al. (2016) already demonstrated that different linear fit approach of the intensity offset correction implemented in the DOAS fit can considerably impact the retrieved dSCDs. However nonlinear fits used in QDOAS, WINDOAS, and MDOAS were not included in their study. The difference of the nonlinear and linear fit of the intensity 30 offset correction could also be considerable. However, apart from the effect of intensity offset correction by excluding Heidelberg and INTA, the systematic difference of HONO delta SCDs between the groups with the same DOAS setting is smaller than 0.3×10^{15} molecules cm^{-2} .

4 Sensitivity studies

In this Section we perform sensitivity studies to assess the systematic effect of the absorptions of H_2O , O_4 and NO_2 , the Ring spectrum, polynomial, intensity offset and shift corrections on the HONO delta SCD retrievals. We also evaluate the effect of variations of the instrument properties including the wavelength calibration, the instrumental resolution and random noise.

5 The studies are implemented on both the V1 and V2 synthetic spectra. In addition measurements of the AIOFM instrument on two days of 16 and 18 June, 2013 are analysed, which were selected because of the low and high HONO delta SCDs observed on the two days, respectively. The WINDOAS software is used to implement DOAS fits in the study. And a sequential FRS is used in the DOAS fits.

4.1 Residual around 363 nm and the effect of the H_2O absorption in the UV spectral range

10 In the baseline fit of HONO, a systematic large residual structure around 363nm was found as shown in Fig. 9. If the fit spectral range extends to 390 nm, the residual structure becomes more prominent. Lampel et al. (2016a) demonstrated that a considerable H_2O absorption can be found in MAX-DOAS observations around 363nm. They also showed that the POKAZATEL H_2O cross section (Polyansky et al., 2016) can well represent this absorption structure. In Fig. 10a for a measured spectrum by the AIOFM instrument, the residual structures from the fits with and without the POKAZATEL H_2O
15 cross section are compared. Especially for the large fit range the residual structures around 363 nm can be minimised by including the POKAZATEL H_2O cross section. The corresponding fit results of the H_2O absorptions are also shown in Fig. 10a. In Fig. 10b the corresponding results for the fits of the V2 synthetic spectra are shown. Compared to the results of the measured spectra, the residuals do not contain noise, and the improvement of the residual for the fits by including the H_2O cross section becomes even more obvious. The fit results of the V1 synthetic spectra, in which no H_2O absorption below
20 388nm is included, are also shown in Fig. 10c for the comparison with those of the V2 synthetic spectra in Fig. 10b. The effect of including H_2O cross section on the fit residual and the artificially fitted H_2O absorption are quite low. In addition we compared HONO delta SCDs from fits with and without the H_2O cross section for the selected AIOFM measurements on
25 16 and 18 June, 2013, and for the V2 and V1 synthetic spectra (for details see Supplementary Fig. S11). The difference is up to 1.5×10^{15} molecules cm^{-2} and is and linearly correlated with the retrieved H_2O delta SCDs with a correlation coefficient of one. These findings demonstrate that the H_2O absorption could mainly contribute to the residual structure around 363nm if the H_2O cross section is not included in the DOAS fit, and can considerably interfere with the HONO absorption. And the interference is stronger for larger H_2O absorptions. Thus we conclude that the POKAZATEL H_2O cross section should be included in the DOAS fits. However it also needs to be noted that the effect of including H_2O cross section on the HONO
30 delta SCDs is found not only for the V2 synthetic spectra (with UV H_2O absorption), but also for the V1 synthetic spectra(without UV H_2O absorption). It indicates a possible spectral interference of the POKAZATEL H_2O cross section with the structures of other absorptions, e.g. O_4 (also reported in Lampel et al., 2016a). Figure 9 indicates that the absorption peak of H_2O around 363nm overlaps with the O_4 structures. Further investigations, improved O_4 cross sections and H_2O

cross sections for UV wavelengths are needed to clarify this hypothesis. In addition it is important to note that the POKAZATEL H₂O cross section scaled by 2.6 is used in the fits for the real measurements and synthetic spectra because of the known underestimation (Lampel et al., 2016a).

4.2 Candidate fit spectral ranges and interference species

5 There are four prominent absorption bands of HONO in the spectral range of 335 nm to 390 nm (see Fig. 11a). Thus fits of HONO absorptions could be implemented in different spectral ranges covering e.g. two, three or four HONO absorption bands. Note that it is unreasonable to extend to the wavelength range below 335 nm as strong ozone absorptions and low signal to noise ratios can significantly deteriorate the retrievals and the magnitude of the differential absorption cross-section of HONO decreases here significantly. We compared the HONO delta SCDs between retrieved in the three spectral ranges
10 of 335-361 nm, 335-373 nm and 335-390 nm for the V1 synthetic spectra and the selected AIOFM measurements (see Supplementary Fig. S12). The difference is about 0.6×10^{15} molecules cm⁻² on average and can not be explained by the wavelength dependence of AMF, since this effect can only cause differences of the HONO SCDs of up to 0.03×10^{15} molecules cm⁻² on average (for details see Supplementary Fig. S13). Therefore the dependence of the retrieved HONO delta SCDs on the fit ranges can be mainly attributed to spectral interferences of the HONO absorption with other absorption
15 structures or instrumental issues. Typical optical depths of the species (based on the measurements during the whole campaign) included in the HONO retrievals are shown in Fig. 11a. In order to assess the possibility of spectral interferences with HONO, we calculated the correlation coefficients of the cross sections of different species with HONO. The determined correlation coefficients are then scaled with typical atmospheric optical depths of the respective species to roughly estimate their potential for spectral interferences with the HONO absorption. The results shown in Fig. 11b indicate that the strongest
20 interferences are expected from NO₂, O₄ and the Ring effect. Their individual effects on the HONO retrieval are discussed in the following Sections 4.3 to 4.5.

4.3 Influence of the O₄ absorption on the HONO analysis

Lampel et al., 2016a reported considerable differences between the three currently available literature O₄ cross sections (Greenblatt et al., 1990, Hermans et al., 1999, and Thalman and Volkamer, 2013). For a typical O₄ dSCD of 2×10^{43} molecules² cm⁻⁵, the optical depths of the differences amount to up to 1×10^{-3} , which is comparable with typical HONO optical depths of up to 3×10^{-3} . Considering the known wavelength calibration problem of the Greenblatt O₄ cross section (Piters et al., 2012), the other two cross sections are probably the best candidates for DOAS fits. We investigate the effects of changing the O₄ cross sections, in the fits on the HONO delta SCDs for the synthetic spectra and the selected AIOFM measurements on 16 June. Similar diurnal variation of the differences of the HONO delta SCDs between the analyses with the Thalman and the Hermans O₄ cross section are found for both the synthetic spectra and the measured spectra (see Fig. S14a in the supplement). Since the synthetic spectra are simulated using the Thalman et al. O₄ cross section, this finding
25
30

indicates that the atmospheric O₄ absorption is best described by the Thalman et al. O₄ cross section. In addition we found that the differences of the HONO delta SCDs are well linearly correlated with the differences of the O₄ delta SCDs with a correlation coefficient of about 0.96 (the scatter plots are provided in the Supplementary Fig. S14b). This finding indicates a spectral interference between (errors of the) O₄ absorption and the retrieved HONO delta SCDs.

5 The temperature dependence of the O₄ cross section is reported in Thalman and Volkamer (2013). The difference of the O₄ cross sections between at 203 K and at 293 K is about 20% around 360nm. The Thalman O₄ cross section at 203k is orthogonalised to that at 293k based on Gram-Schmitt's algorithm using a polynomial of second degree. The orthogonalised O₄ cross section is normalized by an arbitrary factor to be shown in a comparable scale with the other cross sections in Fig.9. The prominent structure at 203 K indicates that the temperature dependence of O₄ cross section probably interferes with the 10 HONO absorption. Moreover, the overlap of the structures of the temperature dependence of O₄ cross section with the H₂O absorption band around 363 nm indicates the potential interplay of the O₄ temperature dependence, the H₂O absorption, and the HONO absorption.

In the DOAS fit it is assumed that the AMF (or atmospheric light path) in a spectral range of the fit is constant. However, it is well known that the light path actually depends on the wavelength (Richter, 1997; Marquard et al., 2000; Puķīte et al., 15 2010; and references therein). This problem could also play a role for the fit of the O₄ absorption in the HONO retrievals. The so-called Taylor series approach (TSA) developed by Puķīte et al. (2010) could approximately solve this problem by including a linear term ($\lambda\sigma_{O_4}$) and a square term ($\sigma_{O_4}^2$) of the O₄ cross section in the fit (λ and σ_{O_4} are the wavelength and absorption cross section of O₄, respectively). The two TSA terms of O₄ orthogonalised to the O₄ cross section are shown in Fig. 9. The interplay of Taylor terms of the O₄, the structure of the O₄ temperature dependence, and the H₂O absorption 20 could impact the retrieved HONO delta SCDs. To test these interference effects in more detail, we compare the HONO delta SCDs from the fits with six different settings for the O₄ absorptions (listed in Tab. 4) for the V1 / V2 synthetic spectra and for the selected AIOFM spectra. In these sensitivity studies all other fit settings are kept unchanged (baseline DOAS settings, but without an intensity offset included for the synthetic spectra). For the synthetic spectra, we calculate the differences of the retrieved HONO delta SCDs using the six O₄ settings and three spectral ranges with respect to the real HONO delta 25 SCDs (as used in the calculation of the synthetic spectra). We also calculated similar differences, but with respect to the results of the baseline retrieval (O₄ setting #1 in 335-373 nm, see Tab. 4) for the synthetic spectra and the measured spectra. In general the smallest differences of fitted HONO delta SCDs from the real values are found for the wavelength range 335-373 nm. For this wavelength range, also the variation of the fitted HONO delta SCDs by changing the O₄ setting is smallest. Similar differences are found with respect to the real HONO delta SCDs of the synthetic spectra and the retrieved HONO 30 delta SCDs using the baseline settings (the detailed results are provided in the supplementary figures S15a,b). Therefore we conclude that the wavelength range 335-373 nm is the best suited spectral range to minimise the O₄-related interference effects on the HONO retrievals. Another important finding is that for the wavelength ranges 335 – 373 nm and 335 – 390 nm the results for the real measurements and the synthetic spectra are similar. Thus we recommend using one Thalman O₄ cross

section at 293K in the fits. The variation of the HONO delta SCDs by changing the O₄ setting indicates the remaining systematic uncertainty related to the O₄ effects.

4.4 Influence of the Ring spectrum

The temperature dependence of the Ring spectrum can contribute to a difference of optical depth of about 5×10^{-5} K⁻¹ around

5 355nm (with respect to a typical Ring optical depth shown in Fig. 11a) based on the study of Lampel el al., 2016a. For the analysis of absorbers with small optical depths, Lampel el al., 2016a recommends including two Ring spectra representing two different temperatures in the fits. To test the effect of the temperature dependence of the Ring effect on the HONO retrievals, we compare the HONO delta SCDs derived using three different Ring settings (see Tab. 4), which are either a Ring spectrum for 250 K, for 273 K or both of them (one is orthogonalised to the other).

10 The Ring effect on the retrieved HONO delta SCDs is quite different between for the measured and synthetic spectra in the three spectral ranges, especially for Ring setting #3 (the detailed results are provided in the supplementary Fig. S16). Based on the obtained results we recommend using a Ring spectrum at one temperature in HONO retrievals. Furthermore due to the small difference of HONO delta SCDs between Ring Setting #1 and #2, it is reasonable to arbitrarily select 250 K for the generation of Ring spectrum. The variations of the HONO delta SCDs for different Ring settings (about 0.35, 0.2, and 0.12

15 $\times 10^{15}$ molecules cm⁻² in the spectral ranges of 335-361, 335-373, and 335-390 nm, respectively on average) indicate the remaining systematic uncertainty related to the Ring effect.

4.5 AMF wavelength dependence caused by the NO₂ absorption

The optical depth of the NO₂ absorption can be large, up to about 0.15, which is much larger than the typical optical depth of HONO (up to 0.003). Similar to O₄, wavelength dependence of absorption caused by NO₂ is also expected. The TSA method

20 (Pukite et al., 2010) could also be applied for NO₂. We compare the HONO delta SCDs from the three fits with different NO₂ settings listed in Tab. 4, which are a) the original NO₂ cross section, b) including also the linear Taylor term and c) including also the linear and square Taylor terms, for both the synthetic and measured spectra. The results indicate that the NO₂ effect on HONO delta SCDs is negligible in the wavelength range 335-373 nm, but considerable in the other two ranges. Also very consistent results for the synthetic spectra and measured spectra are found. Reduction of residual spectral structures related to the NO₂ absorption by a use of the TSA method in DOAS fits can be found in the three wavelength ranges. Thus to minimise the NO₂ effects, we recommend including the two additional Taylor terms of NO₂ in the HONO fit. The detailed results are provided in the supplementary Fig. S17.

4.6 Influence of the degree of the polynomial

To account for the broad spectral structures, e.g., related to atmospheric scattering processes, polynomial fits are included in

30 DOAS retrievals. The polynomial degree is usually chosen depending on the spectral range and spectral characteristics of the

target species. To quantify the uncertainty of the retrieved HONO delta SCDs related to the choice of the degree of the polynomial in the three spectral ranges, we compare the HONO delta SCDs retrieved by the three fits with different degree of the polynomial (see Tab. 4), including degree 3, 4 and 5, for both the synthetic and measured spectra (). The variation of the HONO delta SCDs for different polynomial degrees is smaller in the wavelength range 335-373 nm than in the other two spectral ranges. Also the deviation of the retrieved HONO delta SCDs from the real delta SCDs is generally smallest in the wavelength range 335-373nm (the detailed results are provided in the supplementary Fig. S18). Based on the obtained results the wavelength range 335-373nm is the best suited spectral range to minimise the polynomial-related uncertainty of HONO retrievals. The effect of the degree of the polynomial on the HONO results in the wavelength range 335-373 nm is small. However because in some cases short time variations of the sky conditions might happen in real measurements, we recommend to select a higher polynomial degree, which can better account for such changes. A fifth degree polynomial is used for HONO retrievals in this study.

4.7 Effect of the intensity offset

To compensate for additional artificial intensity signals like instrumental stray light or insufficient corrections of the dark current or electric offset, an intensity offset correction is normally included in the DOAS fits. The intensity offset correction is implemented by a non-linear fit in the WINDOAS software (Fayt and van Roozendael, 2009) in this study. Considerable interferences of the intensity offset with the retrievals of trace gases, especially with small optical depths, were reported e.g. by Coburn et al. (2011). To test the effect of the intensity offset on the HONO analysis in the three spectral ranges, we compare the HONO delta SCDs for different degrees of polynomial for the intensity offset correction (see Tab. 4), including fits without an offset correction and with polynomials of degree 0, 1 and 2 for the offset correction, for both the synthetic and measured spectra. Significant changes of the HONO delta SCDs by including an intensity offset compared to a fit without an intensity offset are found for both synthetic and measured spectra (for details see the supplementary Fig. S19). Because the intensity offset is expected to be zero for the synthetic spectra, the retrieved non-zero intensity offsets and their influence on the HONO delta SCDs imply a significant interference with HONO retrievals. In spite of these possible interferences, taking into account typical instrumental problems (like spectrograph straylight), the consideration of an intensity offset correction in the fit is still recommended for the HONO retrieval. The effect of spectrograph straylight can not be quantified here because it needs a sophisticated Lab measurement, which was not available during the campaign. In addition it should be noted that the interference between the fitted intensity offset and the retrieved HONO delta SCDs as found for the synthetic spectra constitutes a relevant systematic uncertainty of the HONO retrieval, which causes deviations of 0.55, 0.35, and 0.25×10^{15} molecules cm^{-2} in the spectral ranges of 335-361, 335-373, and 335-390 nm, respectively on average.

4.8 Effect of the wavelength calibration and instrumental slit function

In this Section the effect of changes of wavelength calibration on the HONO delta SCDs is tested. The tests are done for either excluding or including a wavelength shift in the fit. In a particular test, we manually shifted the synthetic spectra by

0.025 nm because changes of the wavelength calibration of the MAX-DOAS instruments are smaller than 0.015 nm during one day in the campaign (see Supplementary Fig. S3c). The HONO delta SCDs derived from the shifted spectra are compared to those derived from the original spectra. The differences are only considerable for the fits not including the wavelength shift correction in the fit (leading to differences of 0.2 to 0.4×10^{15} molecules cm^{-2} , in the three spectral ranges).

5 The differences are negligible once the shift correction is accounted for in the fit.

In addition changes of the instrumental slit function could occur. We test the effect of changes of the slit function on the HONO retrieval using the synthetic spectra. The cross sections were convoluted with a wrong Gaussian slit function with a FWHM of 0.525 nm (instead of 0.50 nm). Then we analysed the synthetic spectra with the new convoluted cross sections. The HONO delta SCDs derived from the new fits are compared with those using the correct slit function. The systematic 10 differences are only around -0.02 to -0.13×10^{15} molecules cm^{-2} . Here it should be noted that actual changes of the slit function are usually smaller than assumed in this test. For example, a change of only 0.004 nm is found for the AIOFM instrument during the whole comparison period. Thus we conclude that the changes of the slit function are usually not important for the HONO analysis. But it needs to be noted that asymmetric changes and wavelength dependence changes of the slit function are not considered in the test study.

15 **4.9 Effect of random noise**

The measured spectra are subject to several sources of random noise (i.e., photon noise or electronic noise). To quantify the effect of noise on the HONO analysis, Gaussian random noise with a signal to noise ratio (SNR) of 3000 is added into the V1 synthetic spectra. We compare the HONO delta SCDs and the fit errors of the synthetic spectra with noise and without noise. The comparison results are shown in Fig. 12. The results indicate that the fit errors increase from around 0.1×10^{15} 20 molecules cm^{-2} for spectra without noise to $\sim 0.24 \times 10^{15}$ molecules cm^{-2} for the noisy spectra. The largest increase of the fit error is found for the wavelength range 335–361 nm. However, it should be noted that in the spectral range of 335–373 nm the fit error for the synthetic spectra with noise is rather low (about 0.15×10^{15} molecules cm^{-2}), which is similar to that of the real measurements of the best instruments as shown in Fig. 4. We find no considerable systematic effect of noise on the HONO delta SCDs. However, the standard deviations of the HONO delta SCDs for the spectra either including or excluding 25 noise are considerable and in the range of 0.12×10^{15} molecules cm^{-2} to 0.22×10^{15} molecules cm^{-2} . The largest standard deviation is found in the wavelength range 335–361 nm.

5. Recommended analysis settings and error budget

Systematic uncertainties of the HONO retrieval related to the different error sources in the three spectral ranges are summarized in Fig. 13a based on the sensitivity studies presented in Section 4. In addition to these errors, the error of the 30 HONO cross section is estimated as 5% (Stutz et al., 2000). Fig. 13a indicates that the uncertainties related to the intensity

offset fit, the O₄ and H₂O absorptions, and the Ring effect are usually the prominent errors sources. Another important finding is that the spectral range of 335-373 nm has the lowest systematic uncertainty. Systematic biases of the retrieved HONO delta SCDs for the synthetic spectra compared to the real values and random uncertainties (corresponding to the noise of SNR of 3000) are shown in Fig. 13b for the three spectral ranges. Smallest systematic and random uncertainties are 5 again found for the spectral range of 335-373 nm with a random uncertainty typically smaller than 25% of the systematic uncertainty. Therefore we recommend to retrieve HONO in the spectral range of 335-373nm. In addition, as discussed in Section 4.1, the POKAZATEL H₂O cross section is suggested to be included in HONO retrievals in 335-373nm. The other fit settings should be kept as they are in the baseline DOAS setting (see Tab. 2).

6 Conclusions

10 HONO dSCDs and delta SCDs derived from the seven MAX-DOAS instruments during the MAD-CAT campaign held in Mainz were systematically compared. The fit errors of the HONO dSCDs derived from the instruments with cooled large-size detectors were found to be in the range of about 0.1 to 0.3×10^{15} molecules cm⁻² for an integration time of one minute, while the fit error for the mini MAX-DOAS instrument is around 0.7×10^{15} molecules cm⁻². Although the HONO delta SCDs (the difference of the HONO SCDs for the non-zenith observations and the zenith observation of the same elevation 15 sequence) are usually smaller than 6×10^{15} molecules cm⁻², time series of the HONO delta SCDs retrieved from different instruments are well consistent. Similar consistent results between the instruments are found for the fits with a sequential FRS and a daily noon FRS. Except for the mini-MAX-DOAS instrument, the systematic absolute differences of the HONO delta SCDs between the instruments are smaller than 0.63×10^{15} molecules cm⁻², while the standard deviations are smaller 20 than 0.68×10^{15} molecules cm⁻². The correlation coefficients of the HONO delta SCDs from the different instruments with respect to the reference values are higher than 0.7 and the slopes of linear regressions deviate from unity by less than 16% for the elevation angle of 1°, but the correlations decrease with increasing elevation angles. All instruments can well observe the temporal variation of the HONO delta SCDs for low elevation angles. The maximum value of the HONO delta SCDs of about 6×10^{15} molecules cm⁻² is usually found in the morning. The HONO delta SCD rapidly decrease after sunrise due to 25 the photolysis of HONO. They are typically below the detection limit of 0.2×10^{15} molecules cm⁻² in the afternoon. In addition the deviations of the HONO dSCDs derived from the fits with daily noon FRS between the instruments are generally larger than those of the HONO delta SCDs mainly due to the different HONO absorptions in the noon FRS and the interferences by the stratospheric species, e.g. ozone. Furthermore, there are no considerable systematic differences of the HONO delta SCDs from the fits with the sequential FRS and the daily noon FRS for all the instruments except the mini MAX-DOAS instrument. The standard deviations are lower than 0.23×10^{15} molecules cm⁻².

30 We evaluated the consistency of the DOAS fits by the different groups by using synthetic spectra, for which the real HONO dSCD and delta SCDs are known. The differences of the HONO dSCDs from the real values are much larger than those of

the HONO delta SCDs for all groups mainly due to the interferences by the stratospheric species. The smallest differences ($<0.23 \times 10^{15}$ molecules cm^{-2}) of the HONO delta SCDs from the real values are found for the DOAS settings without the intensity offset correction for most groups, but for two groups the smallest differences are found if the intensity offset correction was included. The different effect of the intensity offset correction might be due to the different implementation 5 of intensity offset correction in the software codes of DOAS fits. Apart from the effect of intensity offset correction, the systematic differences of HONO delta SCDs for the synthetic spectra between the groups (caused by implementation of DOAS fits in the software packages) are smaller than 0.3×10^{15} molecules cm^{-2} , about half of the systematic differences of the real measurements between the different instruments. However the exact reason in the codes of software, which cause the difference, is unknown here. We can only generally attribute the differences of HONO results to the differences of the codes 10 of DOAS software.

We compared the HONO delta SCDs obtained from fits with a sequential FRS in three spectral ranges (335-361 nm, 335-373 nm and 335-390 nm) and found significant differences. The HONO delta SCDs in the wavelength ranges 335-361 nm and 335-390 nm are systematically different from those in the wavelength range 335-373 nm by -0.08×10^{15} molecules cm^{-2} and $+0.57 \times 10^{15}$ molecules cm^{-2} , respectively. To characterize the dominant systematic error sources and to find the best 15 suited DOAS settings for the HONO analysis, we performed various sensitivity studies based on the synthetic spectra and selected measurements from the AIOFM instrument. The main findings are listed below:

- 1) Systematic residual structures are found around 363 nm, which are most probably caused by the H_2O absorption around this wavelength. Meanwhile if the POKAZATEL H_2O cross section is included in the spectral analysis, a systematic increase of the HONO delta SCDs of up to 1.5×10^{15} molecules cm^{-2} is found. Because of the two phenomenon, we 20 recommend including the POKAZATEL H_2O cross section in the fits. The uncertainty caused by the potential interference of the absorption of H_2O and other species (in particular O_4) with the HONO absorption is found to be about 0.13×10^{15} molecules cm^{-2} in the wavelength range 335-373 nm and 0.5×10^{15} molecules cm^{-2} in the wavelength range 335-390 nm.
- 2) We investigated further potential interferences with all spectral structures included in the HONO analysis and found that 25 the strong effects also from interferences of NO_2 , O_4 , and the Ring spectrum.
- 3) Analysis results using different O_4 cross sections indicated that the O_4 Thalman cross section describes the real atmospheric O_4 absorptions best and should be used in the HONO analysis. Systematic uncertainties related to the wavelength dependence of the AMF caused by the O_4 absorptions and its temperature dependence are about 0.5×10^{15} molecules cm^{-2} in the wavelength range 335-361 nm, 0.1×10^{15} molecules cm^{-2} in the wavelength range 335-373 nm and 30 0.2×10^{15} molecules cm^{-2} in the wavelength range 335-390 nm.
- 4) The uncertainties related to the temperature dependence of Ring effect are about 0.35×10^{15} molecules cm^{-2} in the wavelength range 335-361 nm, 0.2×10^{15} molecules cm^{-2} in the wavelength range 335-373 nm and 0.12×10^{15} molecules cm^{-2} in the wavelength range 335-390 nm. However, the results of the sensitivity tests are not completely conclusive, thus we still recommend to simply using a Ring spectrum only for one temperature in the HONO analysis.

5) We also investigated the wavelength dependence of the AMF caused by the NO₂ absorption. We found that the effect on the HONO retrievals can be well compensated by the Taylor series approach from Puķīte et al. (2010). Thus we suggest including the linear and square Taylor terms in the HONO analysis.

6) The systematic uncertainties related to the choice of the polynomial are about 0.2×10^{15} molecules cm⁻² in the wavelength range 335-361 nm, 0.04×10^{15} molecules cm⁻² in the wavelength range 335-373 nm and 0.25×10^{15} molecules cm⁻² in the wavelength range 335-390 nm. Thus we conclude that the spectral range 335-373 nm, is the best choice to minimize the influence of the choice of the polynomial on the HONO results.

5

7) The systematic uncertainties related to the intensity offset are about 0.55×10^{15} molecules cm⁻² in the wavelength range 335-361 nm, 0.35×10^{15} molecules cm⁻² in the wavelength range 335-373 nm, and 0.25×10^{15} molecules cm⁻² in the wavelength range 335-390 nm. Although the results from the synthetic spectra (which are not subject to any artificial offsets) indicate a systematic interference between the fitted intensity offset and the retrieved HONO delta SCDs, we still recommend including the intensity offset in the fit, because for real measurements it can correct instrumental shortcomings like spectrograph straylight.

10

8) Variations of the instrumental wavelength calibration, the instrument slit function, and random noise have only little contribution to the systematic uncertainties of the HONO retrievals.

15

In summary we find that the total systematic uncertainty from the different error sources is much smaller in the spectral range 335-373 nm (0.87×10^{15} molecules cm⁻²) compared to that in the other two investigated spectral ranges. Moreover, the systematic bias of the measured HONO delta SCDs from the simulated real values in the synthetic spectra are also smallest in the wavelength range 335-373 nm (about 0.02×10^{15} molecules cm⁻²). Thus 335-373 nm is the recommended fit range for HONO retrievals.

20

In this spectral range, the typical random uncertainty is about 0.16×10^{15} molecules cm⁻², which is only 25% of the total systematic uncertainty. These results are obtained for an assumed SNR of 3000, which is close to what the best instruments considered achieved in this study. As a final result we conclude that most of the MAX-DOAS instruments can well observe atmospheric HONO absorptions in situations with HONO delta SCDs higher than 0.2×10^{15} molecules cm⁻². Further work should aim to better quantify the spectral interferences between the absorptions of HONO and other absorbers in the selected spectral range. Also further studies on the interference between the HONO absorption and the intensity offset correction are recommended.

25

Acknowledgements: This work was supported by Max Planck Society-Chinese Academy of Sciences Joint Doctoral Promotion Programme and National Natural Science Foundation of China (Grant No.: 41275038 and 41530644).

30

References

Acker, K., Möller, D., Wiegrecht, W., Meixner, F.X., Bohn, B., Gilge, S., Plass - Dülmer, C. and Berresheim, H.: Strong daytime production of OH from HNO₂ at a rural mountain site, *Geophysical Research Letters*, 33(2), doi: 10.1029/2005GL024643, 2006.

5 Akimoto, H., Takagi, H., and Sakamaki, F.: Photoenhancement of the nitrous acid formation in the surface reaction of nitrogen dioxide and water vapor: Extra radical source in smog chamber experiments, *Int. J. Chem. Kinet.*, 19, 539-551, doi:10.1002/kin.550190606, 1987.

Alicke, B., Geyer, A., Hofzumahaus, A., Holland, F., Konrad, S., Pätz, H.W., Schäfer, J., Stutz, J., Volz - Thomas, A. and Platt, U.: OH formation by HONO photolysis during the BERLIOZ experiment, *Journal of Geophysical Research: Atmospheres*, 108(D4), doi:10.1029/2001JD000579, 2003.

10 Aliwell, S. R., Van Roozendael, M., Johnston, P. V., Richter, A., Wagner, T., Arlander, D. W., Burrows, J. P., Fish, D. J., Jones, R. L., Tørnkvist, K. K., Lambert, J.-C., Pfeilsticker, K., and Pundt, I.: Analysis for BrO in zenith-sky spectra: An intercomparison exercise for analysis improvement, *J. Geophys. Res.*, 107, D140, doi:10.1029/2001JD000329, 2002.

Bobrowski, N., Hönniger, G., Galle, B. and Platt, U.: Detection of bromine monoxide in a volcanic plume, *Nature*, 423, 15 273-276, 2003.

Bogumil, K., Orphal, J., Homann, T., Voigt, S., Spietz, P., Fleischmann, O. C., Vogel, A., Haitmann, M., Kromminga, H., Bovensmann, H., Frerick, J., and Burrows, J. P.: Measurements of molecular absorption spectra with the SCIAMACHY pre-flight model: instrument characterization and reference data for atmospheric remote-sensing in the 230–2380 nm region, *J. Photoch. Photobio. A*, 157, 167-184, 2003.

20 Bussemer, M.: Der Ring-Effekt: Ursachen und Einfluß auf die spektroskopische Messung stratosphärischer Spurenstoffe, Diploma thesis, Heidelberg University, Heidelberg, Germany, 1993.

Chance, K. V. and Spurr, R. J. D.: Ring effect studies: Rayleigh scattering, including molecular parameters for rotational Raman scattering, and the Fraunhofer spectrum, *Appl. Optics*, 36, 5224-5230, 1997.

Cléner, K., Van Roozendael, M., Fayt, C., Hendrick, F., Hermans, C., Pinardi, G., Sperr, R., Wang, P., and De Maziere, M.: 25 Multiple wavelength retrieval of tropospheric aerosol optical properties from MAXDOAS measurements in Beijing, *Atmos. Meas. Tech.*, 3, 863–878, 2010.

Coburn, S., Dix, B., Sinreich, R., and Volkamer, R.: The CU ground MAX-DOAS instrument: characterization of RMS noise limitations and first measurements near Pensacola, FL of BrO, IO, and CHOCHO, *Atmos. Meas. Tech.*, 4, 2421-2439, doi:10.5194/amt-4-2421-2011, 2011.

30 Danckaert, T., Fayt, C., Van Roozendael, M., De Smedt, I., Letocart, V., Merlaud, A., and Pinardi, G.: QDOAS Software User Manual, Belgian Institute for Space Aeronomy (BIRA -IASB), 2012.

Elshorbany, Y.F., Kleffmann, J., Kurtenbach, R., Lissi, E., Rubio, M., Villena, G., Gramsch, E., Rickard, A.R., Pilling, M.J. and Wiesen, P.: Seasonal dependence of the oxidation capacity of the city of Santiago de Chile, *Atmospheric Environment*, 44(40), 5383-5394, 2010.

Erle, F., Pfeilsticker, K., and Platt, U.: On the influence of tropospheric clouds on zenith-scattered light measurements of stratospheric species, *Geophys. Res. Lett.*, 22, 2725-2728, 1995.

5 Fayt, C. and van Roozendael, M.: WinDOAS 2.1 Software User Manual, IASB/BIRA (<http://www.oma.be/GOME/GOMEBrO/WinDOAS-SUM-210b.pdf>), 2009.

Fleischmann, O. C., Hartmann, M., Burrows J. P., and Orphal, J.: New ultraviolet absorption cross-sections of BrO at atmospheric temperatures measured by time-windowing Fourier transform spectroscopy, *J. Photochem. Photobiol. A*, 10 168, 117-132, 2004.

Gil, M., Yela, M., Gunn, L. N., Richter, A., Alonso, I., Chipperfield, M. P., Cuevas, E., Iglesias, J., Navarro, M., Puentedura, O., and Rodríguez, S.: NO₂ climatology in the northern subtropical region: diurnal, seasonal and interannual variability, *Atmos. Chem. Phys.*, 8, 1635-1648, doi:10.5194/acp-8-1635-2008, 2008.

Grainger, J. F. and Ring, J.: Anomalous Fraunhofer line profiles, *Nature*, 193, 762, 1962.

15 Greenblatt, G. D., Orlando, J. J., Burkholder, J. B., and Ravishankara, A. R.: Absorption Measurements of Oxygen between 330 and 1140 nm, *J. Geophys. Res.*, 95, 18 577-18 582, 1990.

Hanst, P.L., Wong, N.W., Bragin, J.: A long path infra-red study of Los Angeles smog, *Atmospheric Environment* 5, 969-981, doi:10.1016/0004-6981(82)90183-4, 1982.

Heland, J., Kleffmann, J., Kutenbach, R., and Wiesen, P.: A new instrument to measure gaseous nitrous acid (HONO) in the atmosphere, *Environ. Sci. Technol.*, 35, 3207-3212, doi: 10.1021/es000303t, 2001.

20 Hendrick, F., Müller, J.-F., Clémér, K., Wang, P., De Mazière, M., Fayt, C., Gielen, C., Hermans, C., Ma, J. Z., Pinardi, G., Stavrakou, T., Vlemmix, T., and Van Roozendael, M.: Four years of ground-based MAX-DOAS observations of HONO and NO₂ in the Beijing area, *Atmos. Chem. Phys.*, 14, 765-781, doi:10.5194/acp-14-765-2014, 2014.

Hermans, C., Vandaele, A. C., Carleer, M., Fally, S., Colin, R., Jenouvrier, A., Coquart, B., and Mérianne, M.-F.: 25 Absorption Cross-Sections of Atmospheric Constituents: NO₂, O₂, and H₂O, *Environ. Sci. & Pollut. Res.*, 6, 151-158, doi:10.1007/BF02987620, <http://dx.doi.org/10.1007/BF02987620>, 1999.

Hönninger, G. and Platt, U.: Observations of BrO and its vertical distribution during surface ozone depletion at Alert, *Atmos. Environ.*, 36, 2481-2489, 2002.

Hönninger, G., Friedeburg, C. von and Platt, U., Multi axis differential optical absorption spectroscopy (MAX-DOAS), 30 *Atmos. Chem. Phys.*, 4, 231-254, 2004.

Hoch, D. J., Buxmann, J., Sihler, H., Pöhler, D., Zetzsch, C., and Platt, U.: An instrument for measurements of BrO with LED-based Cavity-Enhanced Differential Optical Absorption Spectroscopy, *Atmos. Meas. Tech.*, 7, 199-214, doi:10.5194/amt-7-199-2014, 2014.

Jin, J., Ma, J., Lin, W., Zhao, H., Shaiganfar, R., Beirle, S. and Wagner, T.: MAX-DOAS measurements and satellite validation of tropospheric NO₂ and SO₂ vertical column densities at a rural site of North China, *Atmospheric Environment*, 133, 12-25, 2016a.

Jin J., Ma, J., Lin, W., Zhao, H.: Characteristics of NO₂ Tropospheric column density over a rural area in the North China Plain (in Chinese), *J. Appl. Meteo. Sci.*, 27(3), 303-311, doi:10.11898/1001-7313.20160305, 2016b.

Kleffmann, J., Gavriloaiei, T., Hofzumahaus, A., Holland, F., Koppmann, R., Rupp, L., Schlosser, E., Siese, M. and Wahner, A.: Daytime formation of nitrous acid: A major source of OH radicals in a forest, *Geophysical Research Letters*, 32(5), doi: 10.1029/2005GL022524, 2005.

Kleffmann, J., Lörzer, J. C., Wiesen, P., Kem, C., Trick, S., Volkamer, R., Rodenas, M., and Wirtz, K.: Intercomparison of the DOAS and LOPAP techniques for the detection of nitrous acid (HONO), *Atmos. Environ.*, 40, 3640–3652, doi:10.1016/j.atmosenv.2006.03.027, 2006.

Kraus, S.: DOASIS, A Framework Design for DOAS, PhD-thesis, University of Mannheim, http://hci.iwr.uni-heidelberg.de/publications/dip/2006/Kraus_PhD2006.pdf, 2006.

Krautwurst, S.: Charakterisierung eines neu aufgebauten MAX-DOAS-Systems und Interpretation von ersten Messergebnissen zu dem Spurenstoff NO₂, Diplomarbeit, Fachhochschule Coburg, Coburg, Germany, 2010.

Kurucz, R.L., Furenlid, I., Brault, J. and Testerman, L.: Solar Flux Atlas from 296 to 1300 nm, in *National Solar Observatory Atlas*, Harvard Univ., Cambridge, Mass, 1984.

Lampel, J., Frieß, U., and Platt, U.: The impact of vibrational Raman scattering of air on DOAS measurements of atmospheric trace gases, *Atmos. Meas. Tech.*, 8, 3767-3787, doi:10.5194/amt-8-3767-2015, 2015.

Lampel, J., Pöhler, D., Polyansky, O. L., Kyuberis, A. A., Zobov, N. F., Tennyson, J., Lodi, L., Frieß, U., Wang, Y., Beirle, S., Platt, U., and Wagner, T.: Detection of water vapour absorption around 363 nm in measured atmospheric absorption spectra and its effect on DOAS evaluations, *Atmos. Chem. Phys. Discuss.*, doi:10.5194/acp-2016-388, in review, 2016a.

Lampel, J., Wang, Y., Hilboll, A., Beirle, S., Sihler, H., Pukite, J., Platt, U., and Wagner, T.: The tilt-effect in DOAS observations, *Atmos. Meas. Tech. Discuss.*, <https://doi.org/10.5194/amt-2017-168>, in review, 2017.

Li, X., Brauers, T., Häseler, R., Bohn, B., Fuchs, H., Hofzumahaus, A., Holland, F., Lou, S., Lu, K.D., Rohrer, F. and Hu, M.: Exploring the atmospheric chemistry of nitrous acid (HONO) at a rural site in Southern China, *Atmospheric Chemistry and Physics*, 12(3), 1497-1513, doi:10.5194/acp-12-1497-2012, 2012.

Li, X., Rohrer, F., Hofzumahaus, A., Brauers, T., Häseler, R., Bohn, B., Broch, S., Fuchs, H., Gomm, S., Holland, F. and Jäger, J., Missing gas-phase source of HONO inferred from Zeppelin measurements in the troposphere, *Science*, 344(6181), 292-296, doi: 10.1126/science.1248999, 2014.

Ma, J. Z., Beirle, S., Jin, J. L., Shaiganfar, R., Yan, P., and Wagner, T.: Tropospheric NO₂ vertical column densities over Beijing: results of the first three years of ground-based MAX-DOAS measurements (2008–2011) and satellite validation, *Atmos. Chem. Phys.*, 13, 1547-1567, doi:10.5194/acp-13-1547-2013, 2013.

Marquard, L. C., Wagner, T., and Platt, U.: Improved Air Mass Factor Concepts for Scattered Radiation Differential Optical Absorption Spectroscopy of Atmospheric Species, *J. Geophys. Res.*, 105, 1315–1327, 2000.

Meller, R. and Moortgat, G. K.: Temperature dependence of the absorption cross sections of formaldehyde between 223 and 323 K in the wavelength range 225–375 nm, *J. Geophys. Res.*, 105, 7089–7101, 2000

5 Monks, P.S., Granier, C., Fuzzi, S., Stohl, A., Williams, M.L., Akimoto, H., Amann, M., Baklanov, A., Baltensperger, U., Bey, I. and Blake, N.: Atmospheric composition change—global and regional air quality, *Atmospheric environment*, 43(33), 5268-5350, 2009.

Neftel, A., Blatter, A., Hesterberg, R. and Staffelbach, T.: Measurements of concentration gradients of HNO_2 and HNO_3 over a semi-natural ecosystem. *Atmospheric Environment*, 30(17), 3017-3025, doi: 10.1016/1352-2310(96)00011-8, 1996.

10 Noxon, J. F. Nitrogen-Dioxide in Stratosphere and Troposphere Measured by Ground-Based Absorption Spectroscopy. *Science*, 189(4202):547-549, 1975.

Ortega, I., Koenig, T., Sinreich, R., Thomson, D., and Volkamer, R.: The CU 2-D-MAX-DOAS instrument – Part 1: Retrieval of 3-D distributions of NO_2 and azimuth-dependent OVOC ratios, *Atmos. Meas. Tech.*, 8, 2371-2395, doi:10.5194/amt-8-2371-2015, 2015.

15 Ortega, I., Coburn, S., Berg, L. K., Lantz, K., Michalsky, J., Ferrare, R. A., Hair, J. W., Hostetler, C. A., and Volkamer, R.: The CU 2-D-MAX-DOAS instrument – Part 2: Raman scattering probability measurements and retrieval of aerosol optical properties, *Atmos. Meas. Tech.*, 9, 3893-3910, doi:10.5194/amt-9-3893-2016, 2016.

Pagsberg, P., E. Bjergbakke, E. Ratajczak, and Sillesen A.: Kinetics of the gas phase reaction $\text{OH} + \text{NO} (+\text{M}) \rightarrow \text{O} (+\text{M})$ and the determination of the UV absorption cross sections of HONO , *Chem. Phys. Lett.*, 272, 383-390, doi:10.1016/S0009-2614(97)00576-9, 1997.

20 Peters, E., Wittrock, F., Großmann, K., Frieß, U., Richter, A., and Burrows, J. P.: Formaldehyde and nitrogen dioxide over the remote western Pacific Ocean: SCIAMACHY and GOME-2 validation using ship-based MAX-DOAS observations, *Atmos. Chem. Phys.*, 12, 11179-11197, doi:10.5194/acp-12-11179-2012, 2012.

Peters, E., Pinardi, G., Seyler, A., Richter, A., Wittrock, F., Bösch, T., Burrows, J. P., Van Roozendael, M., Hendrick, F., Drosoglou, T., Bais, A. F., Kanaya, Y., Zhao, X., Strong, K., Lampel, J., Volkamer, R., Koenig, T., Ortega, I., Piters, A., Puentedura, O., Navarro, M., Gómez, L., Yela González, M., Remmers, J., Wang, Y., Wagner, T., Wang, S., Saiz-Lopez, A., García-Nieto, D., Cuevas, C. A., Benavent, N., Querel, R., Johnston, P., Postylyakov, O., Borovski, A., Elokhov, A., Bruchkouski, I., Liu, C., Hong, Q., Liu, H., Rivera, C., Grutter, M., Stremme, W., Khokhar, M. F., and Khayyam, J.: Investigating differences in DOAS retrieval codes using MAD-CAT campaign data, *Atmos. Meas. Tech. Discuss.*, doi:10.5194/amt-2016-358, in review, 2016.

25 Pinardi, G., Van Roozendael, M., Abuhassan, N., Adams, C., Cede, A., Clémer, K., Fayt, C., Frieß, U., Gil, M., Herman, J., Hermans, C., Hendrick, F., Irie, H., Merlaud, A., Navarro Comas, M., Peters, E., Piters, A. J. M., Puentedura, O., Richter, A., Schönhardt, A., Shaiganfar, R., Spinei, E., Strong, K., Takashima, H., Vrekoussis, M., Wagner, T.,

Wittrock, F., and Yilmaz, S.: MAX-DOAS formaldehyde slant column measurements during CINDI: intercomparison and analysis improvement, *Atmos. Meas. Tech.*, 6, 167-185, doi:10.5194/amt-6-167-2013, 2013.

Piters, A. J. M., Boersma, K. F., Kroon, M., Hains, J. C., Van Roozendael, M., Wittrock, F., Abuhassan, N., Adams, C., Akrami, M., Allaart, M. A. F., Apituley, A., Beirle, S., Bergwerff, J. B., Berkhou, A. J. C., Brunner, D., Cede, A., Chong, J., Clémer, K., Fayt, C., Fries, U., Gast, L. F. L., Gil-Ojeda, M., Goutail, F., Graves, R., Griesfeller, A., Grossmann, K., Hemerijckx, G., Hendrick, F., Henzing, B., Herman, J., Hermans, C., Hoexum, M., van der Hoff, G. R., Irie, H., Johnston, P. V., Kanaya, Y., Kim, Y. J., Klein Baltink, H., Kreher, K., de Leeuw, G., Leigh, R., Merlaud, A., Moerman, M. M., Monks, P. S., Mount, G. H., Navarro-Comas, M., Oetjen, H., Pazmino, A., Perez-Camacho, M., Peters, E., du Piesanie, A., Pinardi, G., Puentedura, O., Richter, A., Roscoe, H. K., Schönhardt, A., Schwarzenbach, B., Shaiganfar, R., Sluis, W., Spinei, E., Stolk, A. P., Strong, K., Swart, D. P. J., Takashima, H., Vlemmix, T., Vrekoussis, M., Wagner, T., Whyte, C., Wilson, K. M., Yela, M., Yilmaz, S., Zieger, P., and Zhou, Y.: The Cabauw Intercomparison campaign for Nitrogen Dioxide measuring Instruments (CINDI): design, execution, and early results, *Atmos. Meas. Tech.*, 5, 457-485, doi:10.5194/amt-5-457-2012, 2012.

Platt, U. and Stutz, J.: *Differential Optical Absorption Spectroscopy*. Springer-Verlag Heidelberg, Berlin, 229-375, 2008.

Polyansky, O. L., Kyuberis, A. A., Lodi, L., Tennyson, J., Ovsyannikov, R. I., and Zobov, N.: ExoMol molecular line lists XX: high accuracy computed line list for hot $H_2^{16}O$, *Mon. Not. R. Astron. Soc.*, 2016.

Pukite, J., Kühl, S., Deutschmann, T., Platt, U. and Wagner, T.: Extending differential optical absorption spectroscopy for limb measurements in the UV, *Atmospheric Measurement Techniques*, 3(3), 631-653, doi:10.5194/amt-3-631-2010, 2010.

Richter, A.: *Absorptionsspektroskopische Messungen stratosphärischer Spurengase über Bremen*, 53N, Ph.D. thesis, University of Bremen, Bremen, Germany, 1997.

Rohrer, F., Bohn, B., Brauers, T., Brüning, D., Johnen, F.-J., Wahner, A., and Kleffmann, J.: Characterisation of the photolytic HONO-source in the atmosphere simulation chamber SAPHIR, *Atmos. Chem. Phys.*, 5, 2189-2201, doi:10.5194/acp-5-2189-2005, 2005.

Roscoe, H. K., Van Roozendael, M., Fayt, C., du Piesanie, A., Abuhassan, N., Adams, C., Akrami, M., Cede, A., Chong, J., Clémer, K., Friess, U., Gil Ojeda, M., Goutail, F., Graves, R., Griesfeller, A., Grossmann, K., Hemerijckx, G., Hendrick, F., Herman, J., Hermans, C., Irie, H., Johnston, P. V., Kanaya, Y., Kreher, K., Leigh, R., Merlaud, A., Mount, G. H., Navarro, M., Oetjen, H., Pazmino, A., Perez-Camacho, M., Peters, E., Pinardi, G., Puentedura, O., Richter, A., Schönhardt, A., Shaiganfar, R., Spinei, E., Strong, K., Takashima, H., Vlemmix, T., Vrekoussis, M., Wagner, T., Wittrock, F., Yela, M., Yilmaz, S., Boersma, F., Hains, J., Kroon, M., Piters, A., and Kim, Y. J.: Intercomparison of slant column measurements of NO_2 and O_4 by MAX-DOAS and zenith-sky UV and visible spectrometers, *Atmos. Meas. Tech.*, 3, 1629-1646, doi:10.5194/amt-3-1629-2010, 2010.

Rothman, L., Gordon, I., Babikov, Y., Barbe, A., Benner, D. C., Bernath, P., Birk, M., Bizzocchi, L., Boudon, V., Brown, L., Campargue, A., Chance, K., Cohen, E., Coudert, L., Devi, V., Drouin, B., Fayt, A., Flaud, J.-M., Gamache, R., Harrison,

J., Hartmann, J.-M., Hill, C., Hodges, J., Jacquemart, D., Jolly, A., Lamouroux, J., Roy, R. L., Li, G., Long, D., Lyulin, O., Mackie, C., Massie, S., Mikhailenko, S., Müller, H., Naumenko, O., Nikitin, A., Orphal, J., Perevalov, V., Perrin, A., Polovtseva, E., Richard, C., Smith, M., Starikova, E., Sung, K., Tashkun, S., Tennyson, J., Toon, G., Tyuterev, V., and Wagner, G.: The HITRAN 2012 molecular spectroscopic database, *Journal of Quantitative Spectroscopy and Radiative Transfer*, 130, 4-50, doi:<http://dx.doi.org/10.1016/j.jqsrt.2013.07.002>, hITRAN2012 special issue, 2013.

5 Rozanov, V.V., Rozanov, A.V., Kokhanovsky, A.A. and Burrows, J.P. : Radiative transfer through terrestrial atmosphere and ocean: software package SCIA TRAN. *Journal of Quantitative Spectroscopy and Radiative Transfer*, 133, 13-71, 2014.

10 Schiller, C. L., Locquiao, S., Johnson, T. J., Harris, G. W.: Atmospheric measurements of HONO by tunable diode laser absorption spectroscopy, *Journal of Atmospheric Chemistry* 40, 275–293, doi: 10.1023/A:1012264601306, 2001.

15 Shefov, N. N.: Spectroscopic, photoelectric, and radar investigations of the aurora and the nightglow, Izd. Akad. Nauk., 1, 25-28, 1959.

Sinreich, R., Merten, A., Molina, L., and Volkamer, R.: Parameterizing radiative transfer to convert MAX-DOAS dSCDs into near-surface boxaveraged mixing ratios and vertical profiles, *Atmos. Meas. Tech.*, 6, 1521-1532, 2013.

20 Solomon, S., Schmeltekopf, A. L., and Sanders, R. W.: On the interpretation of zenith sky absorption measurements, *J. Geophys. Res.*, 92, 8311–8319, 1987.

25 Sörgel, M., Regelin, E., Bozem, H., Diesch, J.-M., Drewnick, F., Fischer, H., Harder, H., Held, A., Hosaynali-Beygi, Z., Martinez, M., and Zetzsch, C.: Quantification of the unknown HONO daytime source and its relation to NO₂, *Atmos. Chem. Phys.*, 11, 10433-10447, doi:[10.5194/acp-11-10433-2011](https://doi.org/10.5194/acp-11-10433-2011), 2011.

30 Stuhl, F. and Niki H.: Flash photochemical study of the reaction OH + NO + M using resonance fluorescent detection of OH, *J. Chem. Phys.*, 57, 3677-3679, doi:[10.1063/1.1678826](https://doi.org/10.1063/1.1678826), 1972.

35 Stutz, J., Kim, E. S., Platt, U., Bruno, P., Perrino, C., and Febo, A.: UV-vis Absorption Cross-Section of Nitrous Acid, *J. Geophys. Res.*, 105, 14585–14592, 2000.

40 Su, H., Cheng, Y.F., Shao, M., Gao, D.F., Yu, Z.Y., Zeng, L.M., Slanina, J., Zhang, Y.H. and Wiedensohler, A.: Nitrous acid (HONO) and its daytime sources at a rural site during the 2004 PRIDE - PRD experiment in China. *Journal of Geophysical Research: Atmospheres*, 113(D14), doi: [10.1029/2007JD009060](https://doi.org/10.1029/2007JD009060), 2008.

45 Su, H., Cheng, Y., Oswald, R., Behrendt, T., Trebs, I., Meixner, F.X., Andreae, M.O., Cheng, P., Zhang, Y. and Pöschl, U.: Soil nitrite as a source of atmospheric HONO and OH radicals, *Science*, 333(6049), 1616-1618, doi: [10.1126/science.1207687](https://doi.org/10.1126/science.1207687), 2011.

50 Thalman, R. M. and Volkamer, R.: Temperature Dependent Absorption Cross-Sections of O₂-O₂ collision pairs between 340 and 630 nm and at atmospherically relevant pressure, *Phys. Chem. Chem. Phys.*, 15, 15371-15381, doi:[10.1039/c3cp50968k](https://doi.org/10.1039/c3cp50968k), 2013.

55 Trick, S.: Formation of nitrous acid on urban surfaces, Ph.D. thesis, Universitat Heidelberg, Heidelberg, Germany, 2004.

Van Roozendael, M., Fayt, C., Post, P., Hermans, C., Lambert, J.-C.: Retrieval of BrO and NO₂ from UV-Visible Observations, in: Sounding the troposphere from space: a new Era for Atmospheric Chemistry. The TROPOSAT Final Report. Peter Borrell, Patricia M. Borrell, John P. Burrows and Ulrich Platt (editors), Springer Verlag, 155-166, 2003

Vandaele, A. C., Hermans, C., Simon, P. C., Carleer, M., Colin, R., Fally, S., M éienne, M.-F., Jenouvrier, A., and Coquart, 5 B.: Measurements of the NO₂ absorption cross section from 42000 cm⁻¹ to 10000 cm⁻¹ (238-1000 nm) at 220 K and 294 K, J. Quant. Spectrosc. Ra., 59, 171-184, 1998.

Wagner, T., B. Dix, C. von Friedeburg, Frie ß, U., Sanghavi, S., Sinreich, R. and Platt, U.: MAX-DOAS O₄ measurements: A new technique to derive information on atmospheric aerosols—Principles and information content, J. Geophys. Res., 109, D22205, 2004.

10 Wagner, T., Beirle, S., and Deutschmann, T.: Three-dimensional simulation of the Ring effect in observations of scattered sun light using Monte Carlo radiative transfer models, Atmos. Meas. Tech., 2, 113-124, 2009.

Wang, L. and Zhang, J.: Detection of nitrous acid by cavity ring-down spectroscopy, Environmental science & technology, 34(19), 4221-4227, doi: 10.1021/es0011055, 2000

15 Wang, Y., Li, A., Xie, P. H., Wagner, T., Chen, H., Liu, W. Q., and Liu, J. G.: A rapid method to derive horizontal distributions of trace gases and aerosols near the surface using multi-axis differential optical absorption spectroscopy, Atmos. Meas. Tech., 7, 1663-1680, doi:10.5194/amt-7-1663-2014, 2014.

Wittrock, F., Oetjen, H., Richter, A., Fietkau, S., Medeke, T., Rozanov, A., and Burrows, J. P.: MAX-DOAS measurements of atmospheric trace gases in Ny-Alesund – Radiative transfer studies and their application, Atmos. Chem. Phys., 4, 955–966, 2004.

20 Wong, K. W., Tsai, C., Lefer, B., Haman, C., Grossberg, N., Brune, W. H., Ren, X., Luke, W., and Stutz, J.: Daytime HONO Vertical gradients during SHARP 2009 in Houston, TX, Atmos. Chem. Phys., 12, 635–652, doi:10.5194/acp-12-635-2012, 2012.

Figures

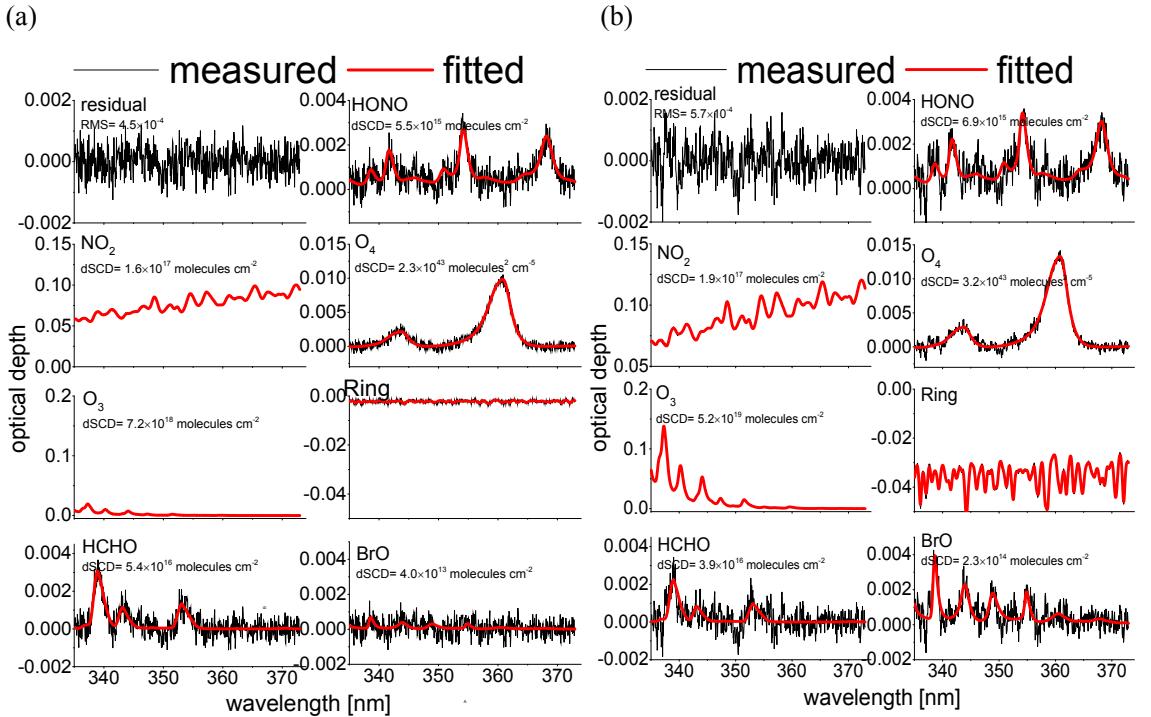


Figure 1: Examples of HONO fits of a spectrum acquired by the AIOFM instrument at around 04:00 UTC on 18 June 2013 for 1° elevation angle and 50° azimuth angle. A sequential FRS around 03:58 UTC (a) or a noon FRS around 11:30 UTC (b) are respectively used.

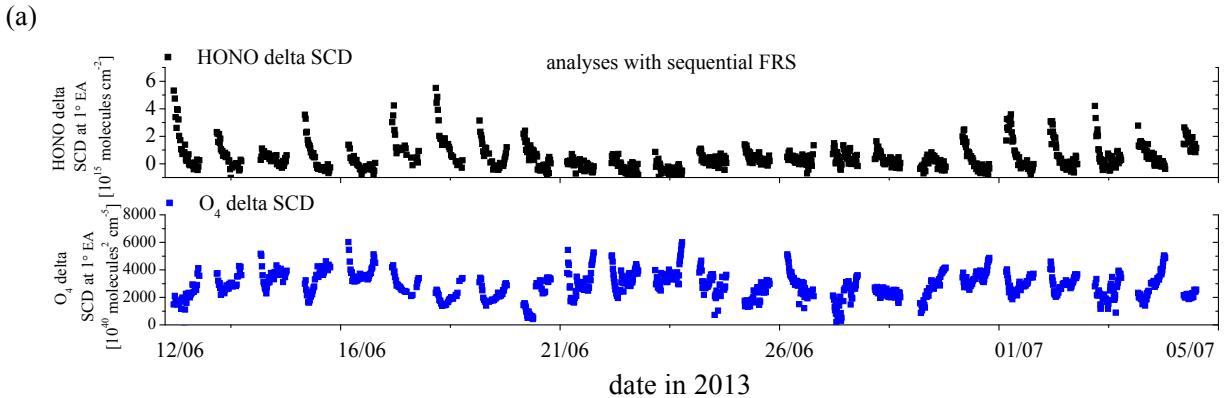


Figure 2: (a) The hourly averaged HONO and O₄ delta SCDs for 1° elevation angle (using a sequential FRS) derived from the measurements of the AIOFM instrument during the whole comparison period. (b) For the same data, the averaged diurnal variations and the respective standard deviations (error bars) in each hour are given.

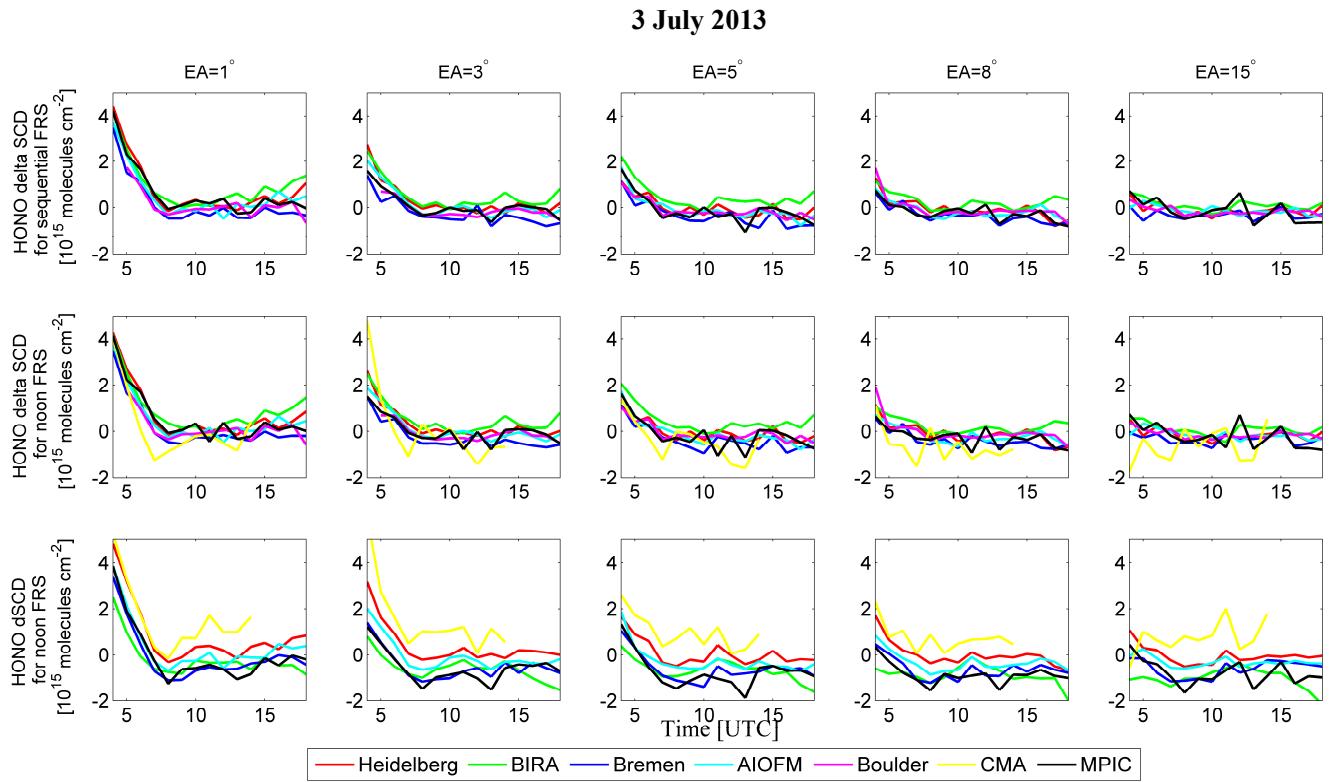


Figure 3: Time series of the hourly averaged values of HONO delta SCDs using a sequential FRS and a daily noon FRS as well as the HONO dSCDs with a daily noon FRS for different elevation angles and participating instruments on 3 July 2013.

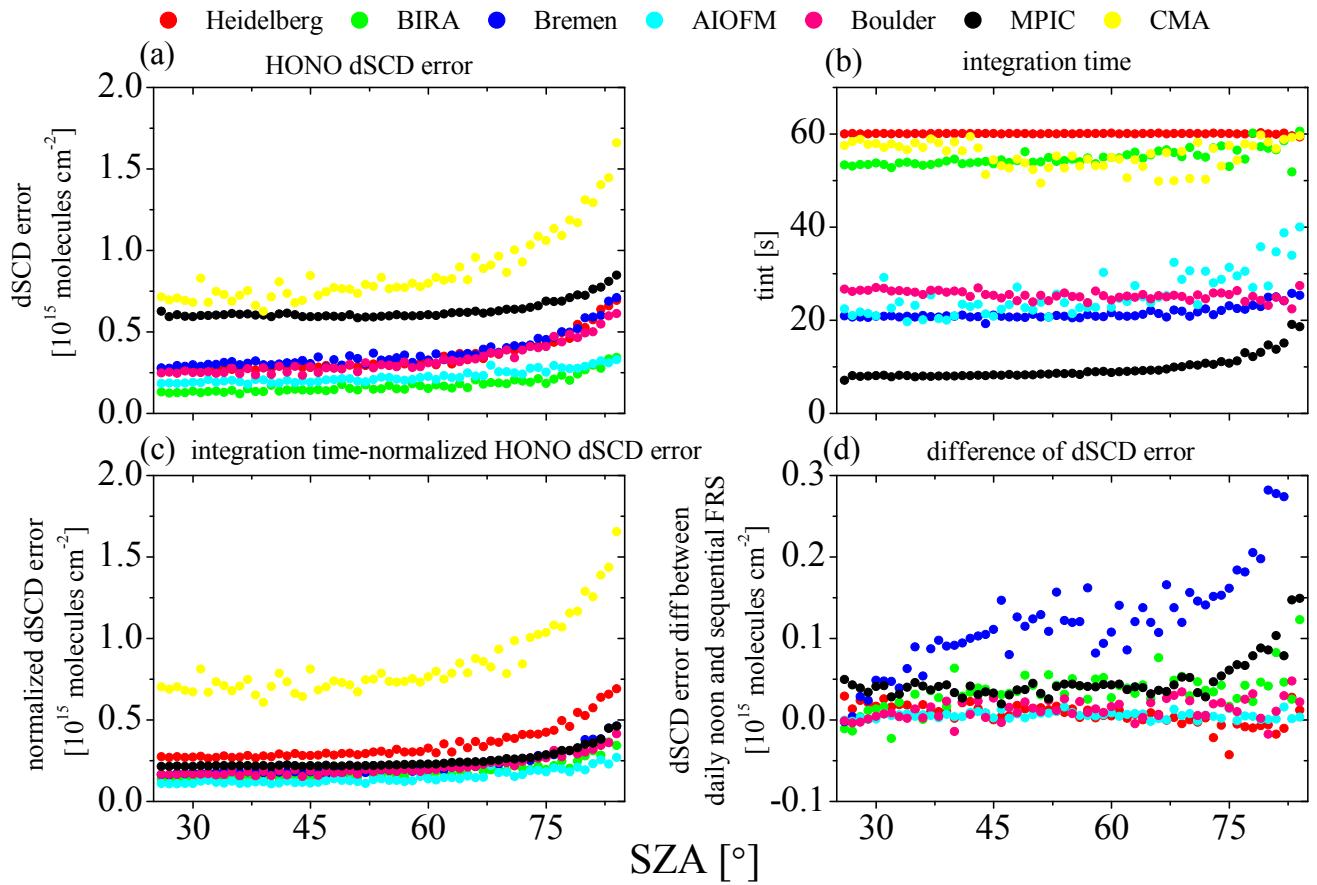


Figure 4: Comparison of different fit errors as a function of the SZA between participating instruments: a) Averaged HONO dSCD fit errors for spectra at 1 ° elevation angle using a daily noon FRS, b) integration time c) normalized HONO dSCD fit errors according to an integration time of one minute, d) differences of the HONO dSCD fit errors with either a daily noon FRS or a sequential FRS.

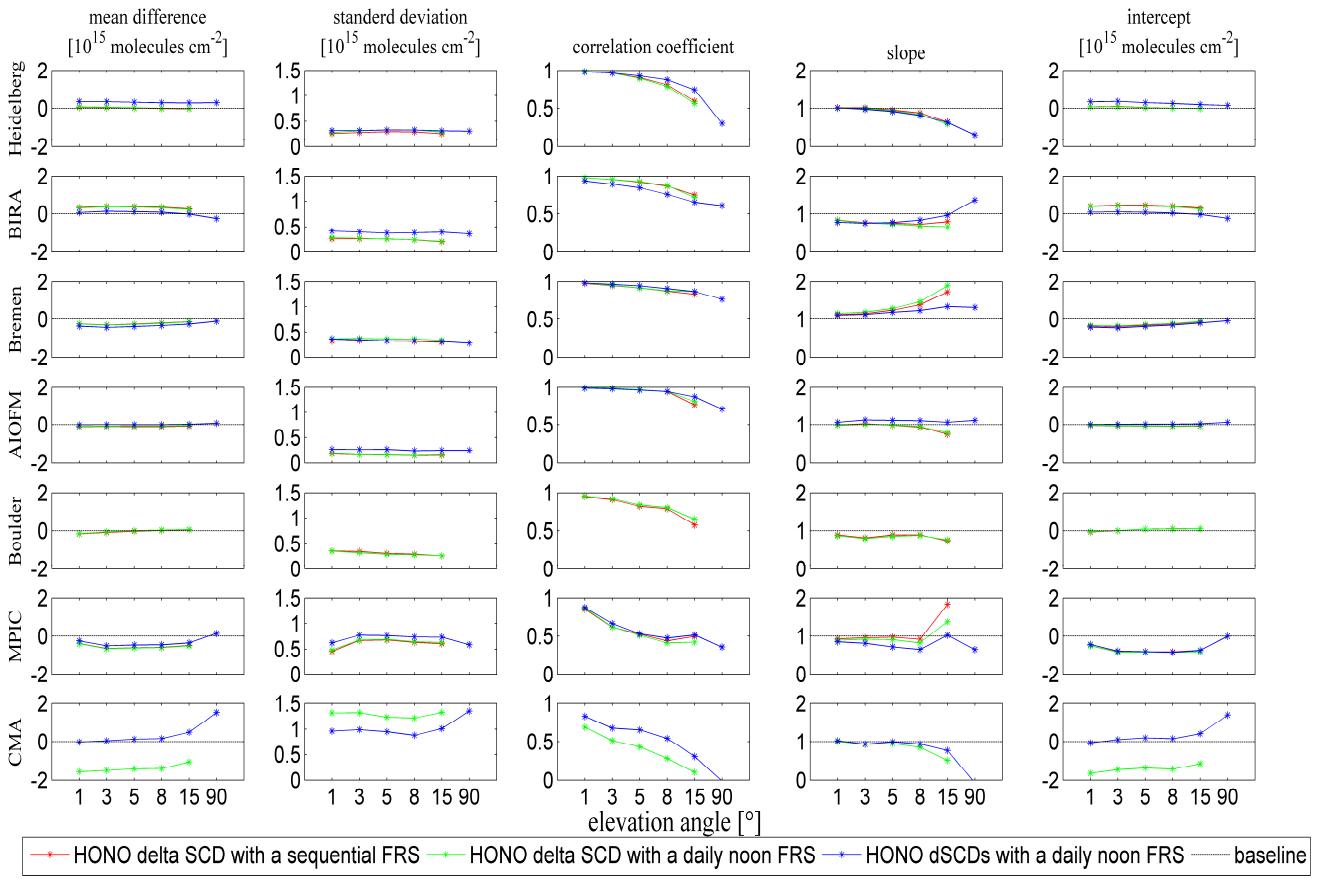


Figure 5: Mean differences and standard deviations as well as correlation coefficients, slopes and intercepts of linear regressions derived from comparisons of the HONO delta SCDs and dSCDs retrieved from different instruments with reference values as function of the elevation angle. The HONO delta SCDs are derived from fits with a sequential FRS (red curves) and a daily noon FRS (green curves). The HONO dSCDs are derived from fits with a daily noon FRS (blue curves).

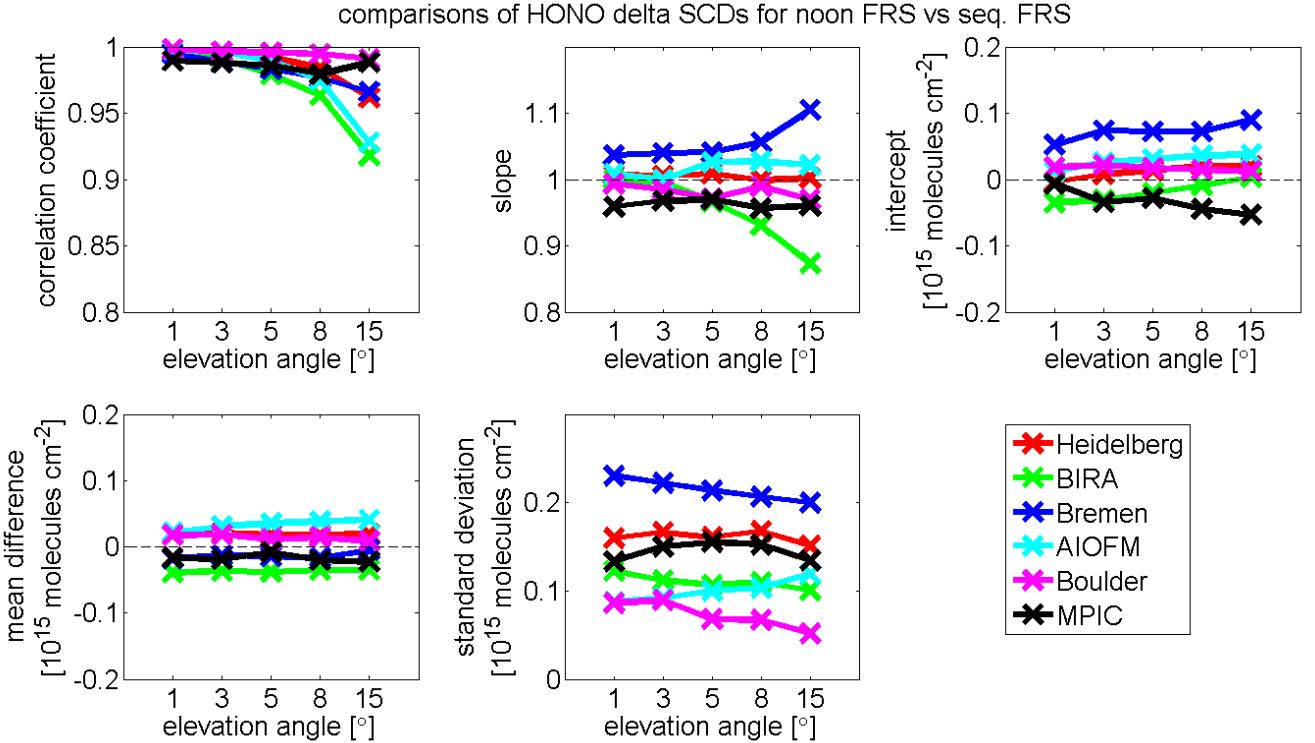


Figure 6: correlation coefficients, slopes and intercepts of linear regressions as well as mean differences and standard deviations derived from the comparisons of the HONO delta SCDs retrieved by fits between with a daily noon FRS and a sequential FRS as function of the elevation angle for individual instruments. The color curves indicate different instruments.

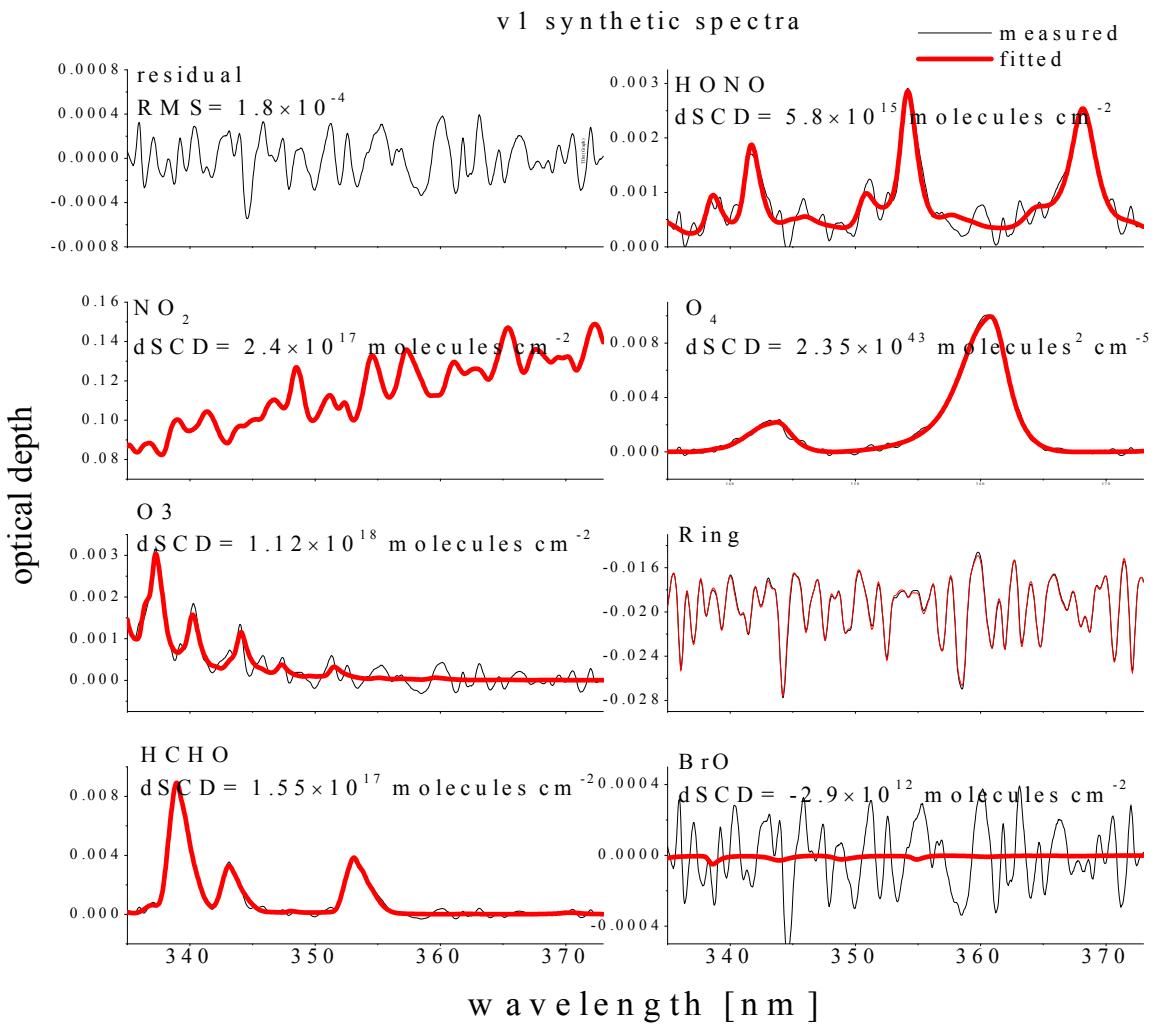


Figure 7: Example of a HONO fit of a V1 synthetic spectrum for a SAA of 166° and EA of 1° using the DOAS setting with a sequential FRS without the intensity offset correction (setting #4 in Table 4).

comparisons of HONO delta SCDs
and dSCDs for synthetic spectra

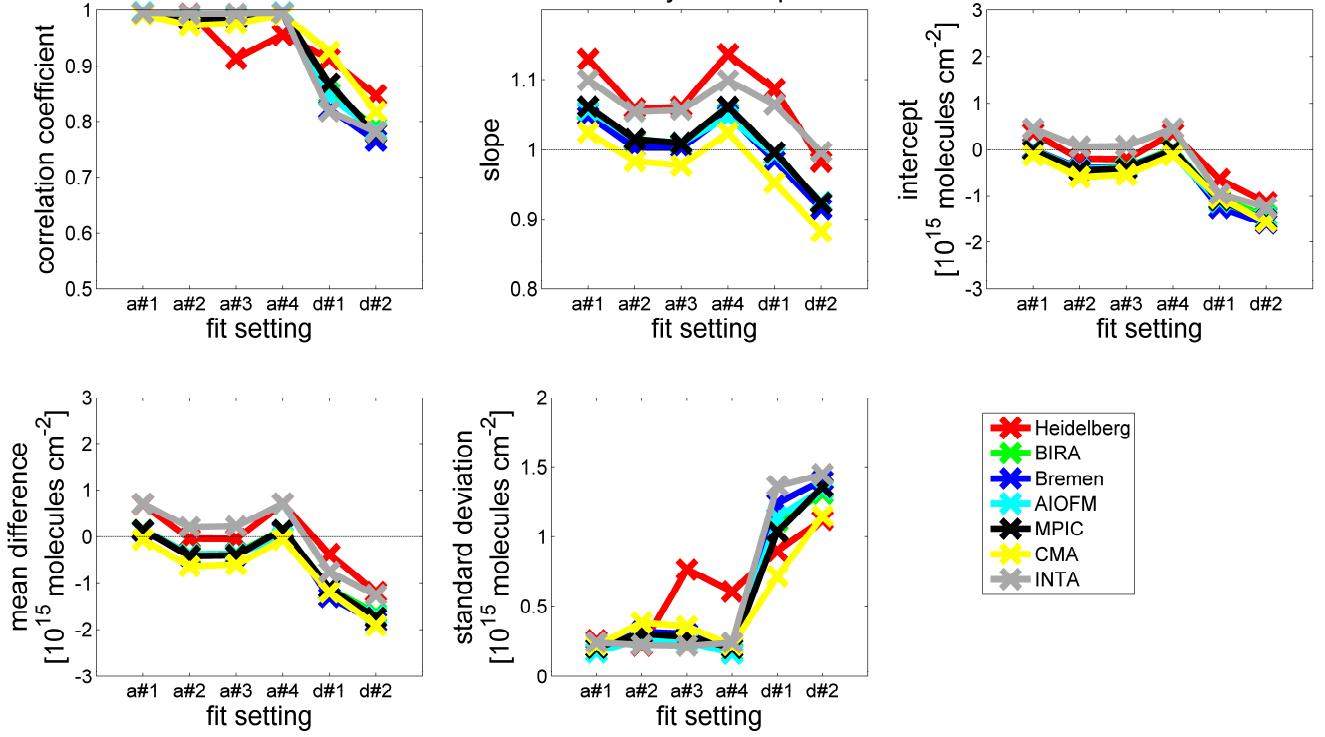


Figure 8: correlation coefficients, slopes and intercepts of linear regressions as well as mean differences and standard deviations derived from the comparisons of the HONO delta SCDs and dSCDs between retrieved from the V1 synthetic spectra and the simulated real values as function of the DOAS fit setting number for individual institutes. The color curves indicate different institutes. “a#1”, “a#2”, “a#3”, and “a#4” in the labels of x-axis indicate the HONO delta SCD retrieved by fits with DOAS setting #1, #2, #3 and #4 (see Table 4), respectively. And “d#1” and “d#2” indicate the HONO dSCDs retrieved by fits with DOAS setting #1 and #2, respectively.


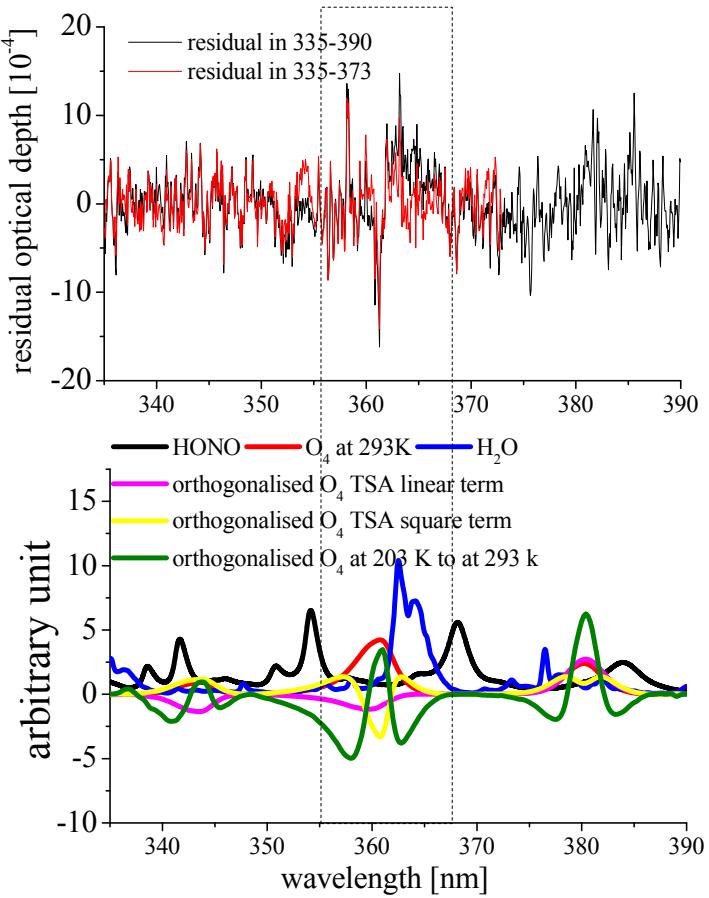


Figure 9: Top: Residual structure from baseline fits with a sequential FRS of the measured spectrum at 1° elevation angle around noon on 16 June, 2013 in the spectral range of 335-390 nm (black) and 335-373 nm (red). Bottom: normalised absorption cross sections used in the HONO baseline fit.

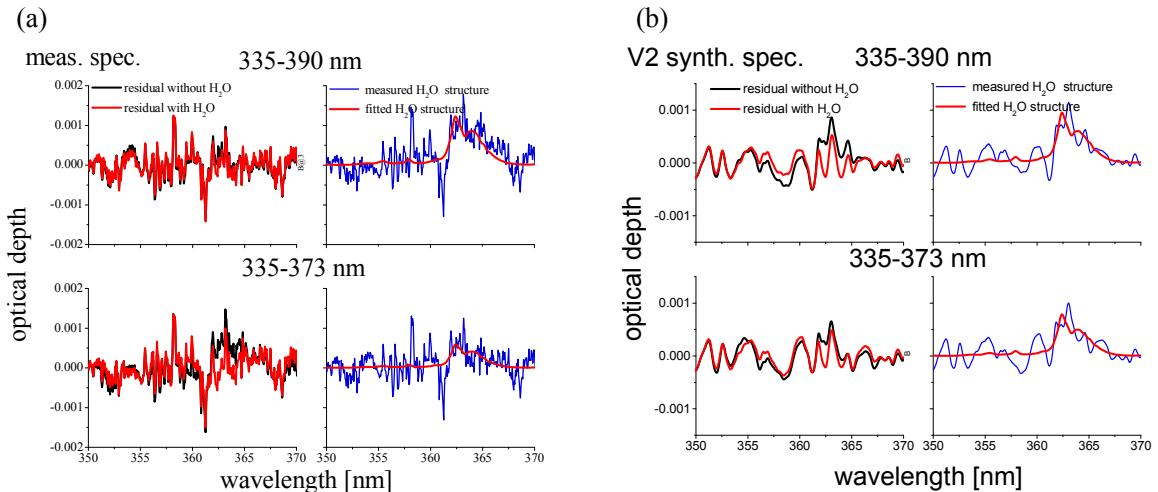

(c)


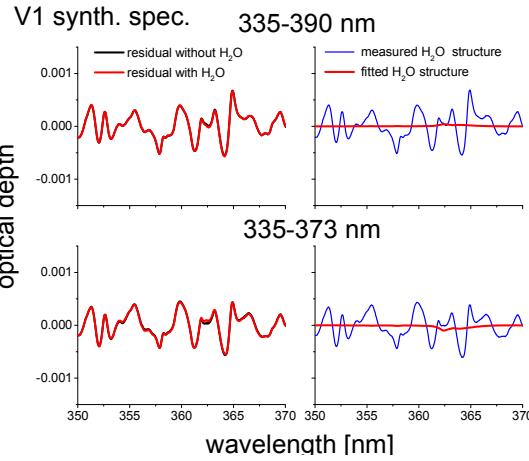


Figure 10: (a) Residual structures (left) and H_2O fit results (right) for the same measured spectrum as in Fig. 9 for the fits either with (red) or without (black) the POKAZATEL H_2O cross section. The upper and lower two subfigures represent fits in the spectral range of 335–390 nm and 335–373 nm, respectively. (b) and (c) are same as (a), but for the V2 and V1 synthetic spectra for a SAA of 166° and EA of 1° , respectively.

(a)

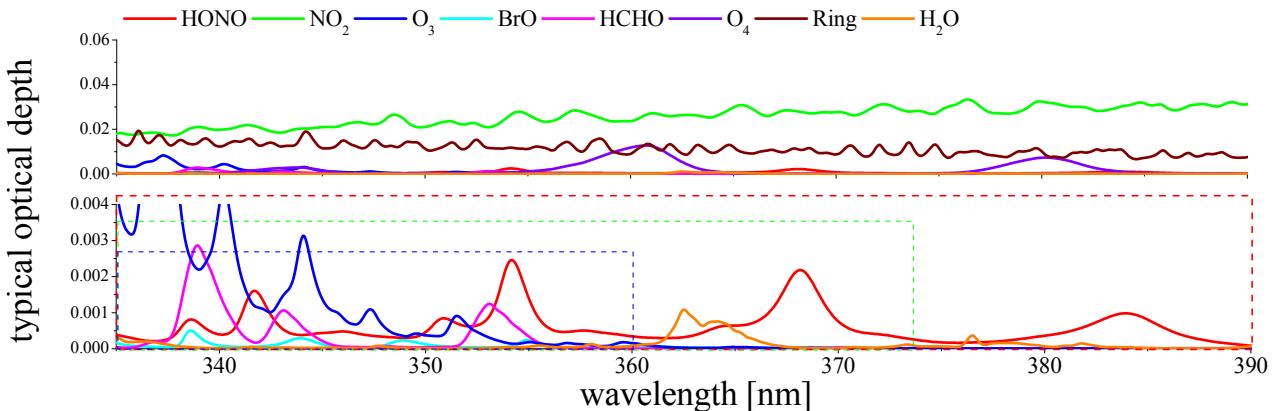

(b)

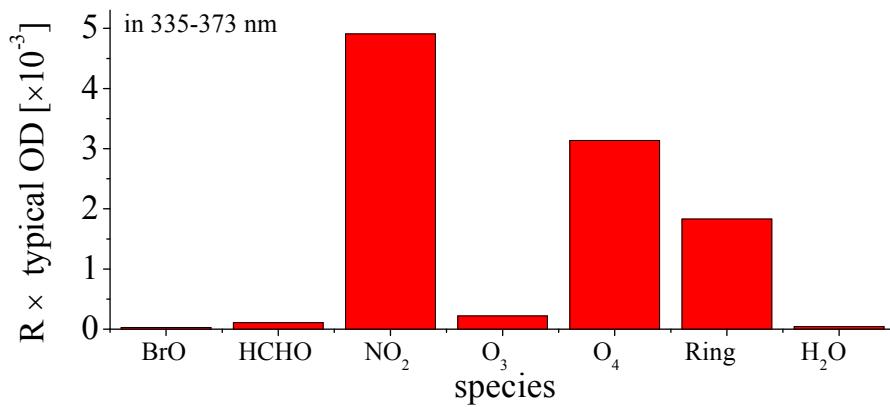


Figure 11: (a) Typical optical depths of the absorption species as the function of wavelength in the wavelength range for HONO retrieval; the dashed colored squares in the lower subplot indicate the wavelength ranges 335 nm up to 360 nm, 373 nm and 390 nm, respectively; (b) Correlation coefficients of the different cross sections multiplied with typical optical depths of respective species (based on the measurements during the whole campaign) with the HONO cross sections in the spectral range 335–373 nm.

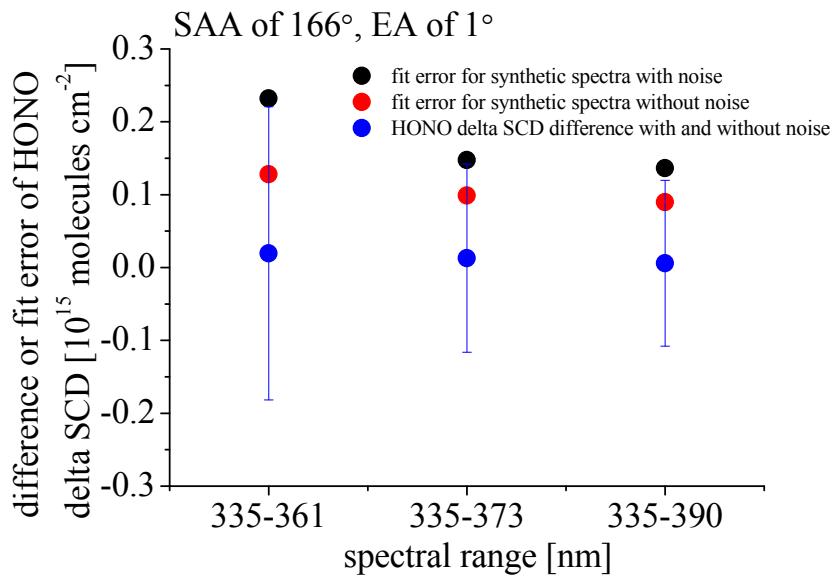


Figure 12: Comparison of the averaged fit errors of the HONO delta SCDs between for synthetic spectra with and without noise (black and red dots), and the averaged differences of the HONO delta SCDs between derived from the two synthetic spectra (blue dots). The error bars indicate the corresponding standard deviations of the differences.

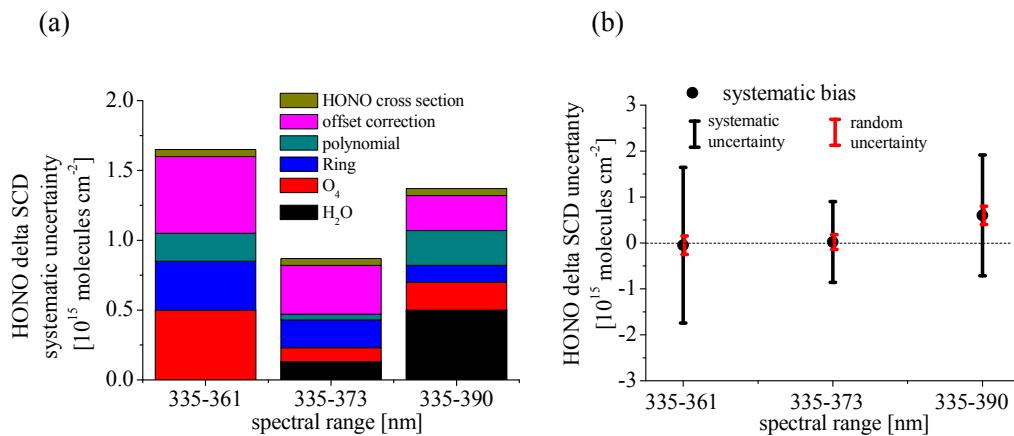


Figure 13: (a) Systematic uncertainties of the HONO delta SCDs with respect to different error sources for the three spectral ranges. (b) Systematic biases from the real values, of the retrieved HONO delta SCDs (black dots) derived from the synthetic spectra in the three spectral ranges; black and red bars indicate typical total systematic and random uncertainties (for a SNR of 3000) of the retrieved HONO delta SCDs.

Tables

Table 1 Overview on instrumental properties and analysis software used by the different institutes participating in the HONO comparison activity

Institute	Detector Characteristics	Observed wavelengths (nm)	FWHM (nm)	Pixel Sampling (nm)	Integration time per spectrum (s)	Field of view (° FWHM)	Manufacturer	Instrument Reference	Fit software	Inter-comparison activity ^e	
										Real Meas.	Synth.
Heidelberg	AvaSpec-ULS 2048 pixels back-thinned Hamamatsu S11071-1106 CCD	294-459	0.59 at 334 nm	~0.09	~60	0.2	Envimes	Lampel et al. (2015)	DOASIS ¹	×	×
BIRA	2D Back-illuminated CCD, 2048×512 pixels (-40°C)	300-386	0.49	~0.04	~55	0.5	self-built	Clémer et al., (2010)	QDOAS ²	×	×
Bremen	2D Back-illuminated CCD, 1340×400 pixels (-35°C)	308-376	0.43	~0.05	~20	0.8	self-built	Peters et al. (2012)	NLIN ³	×	×
AIOFM ^a	2D Back-illuminated CCD, 2048×512 pixels (-40°C)	288-410	0.35	~0.06	~25	0.4	self-built	Wang et al. (2014)		×	×
Boulder	2D Back-illuminated CCD, 1340x400 pixels (-30°C)	329-472	0.78	~0.07	~25	0.95	self-built	Ortega et al. (2015, 2016)	WINDO AS ⁴	×	
MPIC ^b	DV420A-BU, Andor 2D back-illuminated CCD, 1024x255 pixels (-30°)	319-457	0.6-0.8	~0.14	~10	0.6	self-built	Krautwurst, 2010	WINDO AS ⁴ / MDOAS ⁵	× (WINDO AS ⁴)	(MDO AS ⁵)
CMA ^c	2048 pixel, Sony ILX511 CCD	292-447	0.6-0.8		<=60	0.8	Hoffmann Messtechnik GmbH	Jin et al. (2016a and b)	WINDO AS ⁴	×	×
INTA ^d	-	-	-	-	-	-	-	-	LANA ⁶		×

a. Anhui Institute of Optics and Fine Mechanics, Chinese Academy of Sciences

b. Max Planck Institute for Chemistry

c. China Meteorological Administration

d. Área de Investigación e Instrumentación Atmosférica, Madrid, Spain.

e. The flag indicates whether the group participates in the inter-comparison activity of the real measurements and the synthetic spectra or not.

1. Reference: Kraus, 2006.
2. Reference: Danckaert et al., 2012.
- 3: Reference: Richter, 1997.
4. Reference: Fayt and van Roozendael, 2009.
5. Reference: J. Remmers, DOAS fits implemented by MATLAB, personal communication, 2013.
6. Reference: Gil et al., 2008.

Table 2 Baseline DOAS analysis settings of HONO delta SCDs and dSCDs for the comparison activity and recommended settings. ✓ indicates the item for recommended setting is same as that for baseline setting.

Parameter	Baseline setting	Recommended setting
Fitting spectral range	335-373 nm	✓
Wavelength calibration	Calibration based on Fraunhofer lines of Kurucz solar spectrum (Kurucz et al., 1984)	✓
Cross sections		
HONO	Stutz et al. (2000), 296 K	✓
	Vandaele et al. (1998), 220 K and 298 K, I_0 -corrected* (10^{17} molecules cm^{-2})	✓
NO ₂	Taylor terms (see Pukīte et al. 2010) with respect to σ_{NO_2} at 298 K : $\lambda\sigma_{NO_2}$, $\sigma_{NO_2}^2$	
O ₃	Bogumil et al., (2003), 223 K and 243 K, I_0 -corrected* (10^{20} molecules cm^{-2})	✓
BrO	Fleischmann et al. (2004), 223 K	✓
O ₄	Thalman and Volkamer (2013), 293 K	✓
HCHO	Meller and Moortgat (2000), 297 K	✓
H ₂ O (vapor)	Not included	Polyansky et al. (2016) scaled by 2.6 (Lampel et al., 2016a)
Ring effect	Ring spectrum calculated based on Kurucz solar atlas and Ring scaled with $(\lambda/354 \text{ nm})^4$ (Wagner et al., 2009)	✓
Intensity offset	Polynomial of order 1 (corresponding to 2 coefficients)	✓
Polynomial term	Polynomial of order 5 (corresponding to 6 coefficients)	✓
Wavelength adjustment	All spectra are shifted and stretched against FRS	✓
Fraunhofer Reference	1. daily noon FRS (at 11:30)	✓
Spectrum (FRS)	2. sequential FRS	

* solar I_0 correction, Aliwell et al., 2002

Table 3 Four DOAS fit settings:

Setting	Intensity offset fit (constant)	Noon FRS	Sequential FRS
#1	No	Yes	No
#2	Yes	Yes	No
#3	Yes	No	Yes
#4	No	No	Yes

Table 4 DOAS fit settings for the sensitivity studies with respect to O₄, Ring, NO₂, polynomial and intensity offset correction in Section 4.

item	type	fit setting
O ₄	#1	O ₄ at 293 K
	#2	O ₄ at 293 K + Taylor linear term of O ₄
	#3	O ₄ at 293 K + Taylor linear term of O ₄ + Taylor square term of O ₄
	#4	O ₄ at 293 K and 203 K
	#5	O ₄ at 293 K and 203 K + Taylor linear term of O ₄ at 293 K
	#6	O ₄ at 293 K and 203 K + Taylor linear term of O ₄ at 293 K + Taylor square term of O ₄ at 293 K
Ring	#1	Ring at 250 K
	#2	Ring at 273 K
	#3	Ring at 250 K and 273 K
NO ₂	#1	NO ₂
	#2	NO ₂ + Taylor linear term of NO ₂
	#3	NO ₂ + Taylor linear term of NO ₂ + Taylor square term of NO ₂
Polynomial	#1	Polynomial of degree 5
	#2	Polynomial of degree 4
	#3	Polynomial of degree 3
offset	#1	No offset correction
	#2	Polynomial of degree 0
	#3	Polynomial of degree 1
	#4	Polynomial of degree 2