

INITIAL REVISION

RESPONSE TO REVIEWER #1

We appreciate the comments and the revision carried out by Reviewer #1 and we understand his/her concerns. We would like to kindly ask him/her to review our paper again, after incorporating his/her suggestions. Thank you very much.

General comments.

The manuscript by Romero-Trigueros et al. address an important issue regarding air quality monitoring of benzene by transportable GC-PID. The tests are reported clearly and the implications discussed appropriately. However, my main concerns about the manuscript are:

- 10 **1) Focusing on benzene: It would be more relevant to have investigated all the species analysed by this specific GC-PID, often referred to as "BTEX analyser" (for benzene, toluene, ethylbenzene, and xylenes).**

Focusing on benzene is supported by the fact that this is the only VOC in the European Union with limit values and a standardized method for measuring its concentration in air. It is true that adding toluene, ethylbenzene and xylenes to our work would have improved the paper but these species were out of our goal.

- 15 Measuring toluene, ethylbenzene and xylenes would have meant either repeating the tests for these species – increasing the project cost (more reference gases for each of them) and time; or having worked with a reference gas mixture with all these components, which would have increased the uncertainty of the mixture composition and its stability.

For all of this and, mainly, because benzene was our target VOC, we only carried out the tests with benzene.

- 20 Nevertheless, in the future, the rest of compounds could be further investigated.

- 25 **2) Previously reported influence of pressure: A previous publication from the same authors in a different journal reported that data from this type of GC-PID might be affected by pressure difference. These issues hint at a disputable publication strategy spreading results of the characterization of this monitor in several manuscripts, increasing the publication count of the authors, but diluting the relevant information for the users of this type of monitors. Therefore, I would recommend to reject this manuscript.**

It is true that we have published another paper related to the influence of pressure on GC-PID benzene measurements. These two papers, together with many more tests that have not been published, are the results of a PhD thesis. We believe that those tests with interesting results should be published independently in order to be treated deeper. If all the tests were to be included and discussed in a single publication, its length would have been too long.

- 30 A paper similar to ours, dealing with water vapour interference in H₂S monitors, was recently published in AMT journal and it was considered to be sufficiently comprehensive for this. This paper can be read here:

<https://www.atmos-meas-tech.net/9/2669/2016/amt-9-2669-2016.html>

- 35 For all of this, we would like to kindly ask Reviewer #1 to review the corrected manuscript again and consider it for publication. We really appreciate it.

Specific comments.

5 - **The content of the manuscript is well reflected in the abstract but it has been omitted that temperature influence has also been tested. Even though the result is that the temperature has no influence, it might be worth to emphasize this result in the abstract (or even in the title of the manuscript).**

The reviewer is right and temperature influence should be mentioned in the abstract and be also mentioned in the title of the manuscript. These have been done. Please refer to the new title and abstract.

- **page 3, line 25-26: Tests with temperature should have their dedicated experimental section and the results should be reported only in section 3.2.**

10 Temperature tests are now treated as a main goal of the manuscript together with humidity (accordingly to previous comment) and, therefore, the manuscript has changed accordingly. Sections 2.2.2 and 3.1 are now devoted to the influence of sample temperature.

15 - **page 4, line 7: It should be clarified (possibly in the introduction) that the EN Standard the authors are referring to citation "EU, 2008".**

20 "EU, 2008" refers to Directive 2008/50/EC. "EN, 2015" refers to EN Standard 14662-3:2015 and this has been stated clearer in the introduction (line 27 in page 1 and line 5 in page 2, respectively). However, the preliminary test in section 3.2 was carried out according to EN Standard 14662-3:2005, which is the previous version of the standard. This is because these tests were carried out before the release of the new version. This is all explained in the new section 2.2.3.1. The water interference test of the new version is also explained in this section (line 7 in page 5).

25 Luckily enough, from the further tests that we performed in section 2.2.3.2 we were able to calculate the new parameter b_{th} , and these results have been included in section 3.2 (line 14, page 6).

- **page 5, line 7: The sentence starting with "This influence has a negative sign,..." should be revised as the wording seems odd.**

The wording has been changed to "This is a negative influence, that is, ..." (line 10, page 6)

30 - **page 6, line 4-5: Statistics have been used but are poorly described in this one sentence. What is the value for $p=0.05$ and 14 degrees of freedom and what are n_1 and n_2 ? This should be improved and clarified for readers that are not familiar with such statistic tools.**

35 The information missing has been added (t-value for $p=0.05$ and 14 degrees of freedom is 2.145 and n_1 and n_2 are the number of data in the least-square regressions of Figure 2 (for nominal benzene concentrations of 5 and 40 $\mu\text{g}/\text{m}^3$, respectively). Also, a mistake was detected. Our calculated t-value is higher than the tabulated one, which means that we reject the null hypothesis, that is, there are significant differences in the two slopes not attributed to random errors. (Line 2, page 7).

- page 6, line 20-24: It could be discussed in a bit more detailed how the results reported in the literature might have suffered from the presented influence of RH, given the reported environmental conditions of the measurements.

5 A thorough revision of literature has been carried out in order to find works where benzene was measured with a similar instrument to that used in this work. Many works use active or passive sampling followed by *ex situ* thermal desorption and GC-PID or GC-FID (e.g. Marc et al., 2016; Fracasso et al. (2010); Allou et al. 2008; Tran et al., 2000). There are a few of them that use *in situ* GC-FID (e.g. Zhang et al. 2017; Durana et al. 2006) and *in situ* GC-PID (e.g. Bruno et al., 2001; Kelessis et al., 2006; Villanueva et al., 2012). Bruno et al. (2001) and Villanueva et al. (2012) use gas chromatographs from Syntech Spectras so a study of the influence of humidity in their
10 measurements could be done as long as calibration details and relative humidity data are provided.

Bruno et al. (2001) mainly focused on source apportionment and they do not provide information related to ambient humidity. The average concentration of benzene during the sampling period was $4 \pm 1.6 \mu\text{g}/\text{m}^3$ so measurements were close to the annual limit value but, mainly, below it, so around 2% bias is expected at 20 °C and 50% relative humidity if calibration was carried out with dry gases.

15 Villanueva et al. (2012) intercompared tropospheric ozone, benzene and toluene by a commercial DOAS and conventional monitoring techniques. The instrument used to measure benzene and toluene was the same as the one used in our work. They mention the use of certified gas mixtures to calibrate their instruments. There is no mention to water vapour in the mixtures so it is assumed that they are dry gases. Their results show that average levels for ozone, benzene and toluene obtained with DOAS were higher than those obtained with UV photometry for ozone
20 and GC-PID for the aromatics. The largest differences found are for benzene. Although the water interference found in our work is compatible with the results obtained in Villanueva et al. (2012), we would need to know the pair of values temperature and relative humidity to assess the extend of the water vapour interference.

These discussions have been added in the corrected manuscript (from line 13 on in page 8).

25 - from page 6, line 25: This whole paragraph is a bit strange to me. It is not clear if the discussion is related to findings (or speculation?) of the authors or from the literature (in which case, references would be missing). The paragraph starts with "have been proved", but then rest reads like possible explanation for the observed influence of humidity on the results. Moreover, if the effect of water on preconcentration and chromatographic separation is not discussed (e.g. baseline, peak shapes, etc.) because is thought not to be relevant, this should be briefly motivated. Do authors expect the water concentration at the detector when
30 benzene elutes to be the same as the ambient water concentration during sampling?

There was a missing reference that has been added (MSA, 2005) in line 28, page 7. The technical document can be found in

<http://media.msanet.com/NA/USA/PermanentInstruments/GasSensorsTransmitters/SaveToxSafeVOC/07-2092WhitePaperPID.pdf>

35 The baseline did not change when zero gas with different amount fractions of water vapour was measured. The peak shapes did not change either when measuring a constant amount fraction of benzene with different amount fractions of humidity. This is why we think that water vapour does not interfere in the preconcentration and separation steps. This has been included in the final manuscript (line 24, page 7)

Although the amount fraction of water vapour was not measured at the outlet of the instrument, it is assumed to be the same as the inlet, because this instrument does not have any dryer or scrubber.

- 5 - **page 7, line 25: If "presumably" TEX are also affected, authors should at least mention briefly why they did not include them in their present work and if they are planning to do it in the near future. If they do have results for these compounds, they should not be withdrawn and included in the present manuscript.**

As mentioned previously, these species were out of the scope of this work. We only studied benzene as it is the only VOC with limit values in air quality in the European Union. This has been stated clearer in the manuscript (line 24, page 2).

10 **Technical corrections**

- **page 1, line 25: typo "h0ematologic"**

Thanks. This has been changed in the corrected manuscript (line 1, page 2).

- **page 2, line 28: Trigueros et al., 2016 is missing in the bibliography**

15 It appears now as Romero-Trigueros et al. and, therefore, it has been changed accordingly in the text (line 22, page 2 and line 5 page 3).

- **page 3, line 12-13: use either commas or long dash (–) to separate "the ratio of the actual mass of water vapour present in the sample to the mass of the dry air"**

20 The comma has been removed (line 18, page 3).

- **page 4, line 5: replace "pressure" with "humidity"**

Thanks. This has been changed in section 2.2.2.

- 25 - **page 4, line 20: I suggest to use "with different absolute humidity (AH) values"**

The word "values" has been added to the sentence. Thank you. (line 19, page 5).

- **page 5, line 20: Word order: "the initial temperature of the sample being irrelevant in the whole process"**

Thank you for the suggestion. (line 5, page 6)

30

- **page 9, line 24: This is not a DOI, this is an URL.**

Thanks for this. (line 12, page 11)

- **page 9, line 32: Remove "http://dx.doi.org/".**

35 Thanks. (line 20, page 11)

RESPONSE TO REVIEWER #2

General Comments

The manuscript provides the influence of ambient humidity on benzene measurements carried out with an automated in situ GC-PID that is the instrument usually used in air quality monitoring networks. I consider that is an interesting study and therefore, I recommend the manuscript for publication in Atmospheric Measurement Techniques. Some specific comments are given below to be clarified by authors before publication.

Thank you for this and your valuable suggestions.

Specific Comments

10 **Pag. 2 27. What is the brand, model of the dynamic dilution system? Please include in the text.**

Our dynamic dilution system was built in-house. This has been clarified in the text (line 4, page 3). All the description in the text regarding the humidifier, the flow rate and temperature control refers to this in-house built system. Some of its parts (such as the humidifier) were designed by the authors and some of them were bought (such as the mass flow controllers).

15 **Pag. 3, line 18. Is the mixture benzene in nitrogen a SRM, if so please indicate it. Who is the supplier of the gas cylinder? Which is the purity? Please, indicate it in the text.**

The mixture of benzene in nitrogen was provided by Abelló Linde. Its concentration was certified by Linde according to the Standard ISO 6141:2007. The expanded uncertainty of the amount fraction of benzene in the mixture was 5%. This information has been added to the manuscript (line 24 on in page 3).

20 **Are the flow meters calibrated periodically? How?**

The mass flow controllers are at least annually calibrated against a Gilian Gilibrator (a NIOSH primary standard air flow calibrator) available in our lab. If the deviation of the MFC measurements is higher than 1% then the measurements are corrected with a calibration line. If lower, this bias is accepted and accounted for in the uncertainty assessment of the concentration of the gas mixtures.

25 **Pag. 4, line 10. Authors refer to Standard EN 14662-3:2005 in order to calculate the coefficient brh to see the influence of relative humidity but this standard is already cancelled and the equation 2 does not appear in the EN 14662-3:2015. Why do authors think that this equation has been removed from the updated Standard?**

30 We think that tests were likely changed because of the non-conformities of analysers with the Standard criterion for the span concentration. It is true that the span concentration ($40 \mu\text{g}/\text{m}^3$) is quite high and such high levels are not usually found in the ambient air if measured away from the emission sources. However, from our point of view, it is interesting to test other concentrations apart from the limit value. From our perspective, testing this influence

with a value in between the annual limit and the span (around $20 \mu\text{g}/\text{m}^3$) would be interesting to detect important biases at high benzene amount fractions, which can be present, for instance, in industrial areas. These has been stated in lines 17 on in page 6.

5 **If the relative humidity is so important at high concentration of benzene as demonstrated in the manuscript, why it has been deleted?**

I am afraid we cannot answer this question. We guess that manufacturers may have been having issues with passing this test and, arguing that ambient concentrations of benzene are not usually as high as $40 \mu\text{g}/\text{m}^3$, they may have put pressure on normalizers to soften the performance criterion.

Table 1. if (0.01) is the standard deviation, please indicate it in the table.

10 It is the standard deviation. This information has been added in Tables 1 and 2.

Table 3 . A “(“should be before $\mu\text{g}/\text{m}^3$) in Cmeas. What is qt? in the text are defined qz and qH2O but not qt.

q_t is the total flow rate, that is, the sum of q_z , $q_{\text{H}_2\text{O}}$ and the flow rate from the reference gas mixture. This has been specified in the caption of Table 3.

15 **On the other hand, have the authors checked the memory effect when using high concentration of benzene (40 $\mu\text{g}/\text{m}^3$)?**

Indeed, we did. We followed standard EN 14662-3:2005 for this test (standard EN 14662-3:2016 does not substantially change this test). We measured a nominal concentration of benzene in air of $45 \mu\text{g}/\text{m}^3$ and then we switched to zero air. We carried out this test for Analyser I and II. For Analyser I we obtained the following 3 sequential measurement results: $46.59 \mu\text{g}/\text{m}^3$, $-0.01 \mu\text{g}/\text{m}^3$ and $-0.01 \mu\text{g}/\text{m}^3$. For Analyser II we obtained: $45.05 \mu\text{g}/\text{m}^3$, $0.32 \mu\text{g}/\text{m}^3$ and $0.31 \mu\text{g}/\text{m}^3$. Both analysers met the performance criteria of the Standard for this test (a measurement $< 20\%$ of the annual limit value for analysis n.2 (the one right after changing the concentration to zero) and $< 10\%$ of the annual limit value for analysis n.3). Analyser II measured $0.05 \mu\text{g}/\text{m}^3$ in a fourth analysis and $0.01 \mu\text{g}/\text{m}^3$ in a fifth one, so we can conclude that this effect is not significant in this type of instruments. In any case, every time we changed the concentration of benzene we excluded the first measurement from the data analysis.

Technical comments

Pag. 1, line 25: revise “h0ematologic”

Thanks for spotting this. (line 1, page 2)

30 **Pag. 1 , line 29. Reference properly the Standard EN in reference section. The standard number is missing.**

We have added the whole number of the standard in the text (line 5, page 2).

Pag. 4. , line 7 and pag. 5, line 4. I think that authors should change “2005” by “2015”.

We have explained that the tests were carried out according to Standard EN 14662-3:2005 as these were carried out before the publication of the new standard. We have also described the differences between the two standards regarding the humidity influence. (line 22 in page 4, and lines 7 on in page 5).

5 **Pag. 4, line 18. Section 2.2.2.1 should be 2.2.2.2**

Thanks for spotting this.

Pag. 5, line 6. Revise the sentence: Moreover, coefficient. . . In air.

10 This sentence has been reworded to “Moreover, calculated coefficients b_{th} for both analysers turned out to be higher than 4% (the maximum variation allowed in the Standard EN 14662-3:2005) when the tests were carried out with 40 $\mu\text{g}/\text{m}^3$ of benzene in air”. This has been accordingly changed in the manuscript (line 11, page 6).

15

20

Influence of ~~environmental~~ sample temperature and environmental humidity on measurements of benzene in ambient air by transportable GC-PID

Cristina Romero-Trigueros¹, Marta Doval Miñarro², [Esther González Duperón¹](#), Enrique González Ferradás¹

¹Chemical Engineering Department, School of Chemistry, University of Murcia, 30071, Murcia, Spain

²Chemical and Environmental Engineering Department, Technical University of Cartagena, Paseo Alfonso XIII, 52, 30203 Cartagena, Murcia, Spain

Correspondence to: Marta Doval Miñarro (marta.doval@upct.es)

10 **Abstract.** Calibration of *in situ* analysers of air pollutants is usually done with dry standards. In this paper, the influence of sample temperature and environmental humidity on benzene measurements by gas chromatography coupled with a photo ionisation detector (GC-PID) ~~is~~ are studied. Two reference gas mixtures (40 µg/m³ and 5 µg/m³ nominal concentration benzene in air) were subjected to two temperature cycles (20 °C / 5 °C / 20 °C and 20 °C / 35 °C / 20 °C) and measured with two identical GC-PIDs. The change in sample temperature did not produce any significant change in readings. Regarding ambient humidity,

15 ~~Two identical~~ the chromatographs were calibrated for benzene with dry gases and subjected to measure reference standards with humidity (20% and 80% at 20 °C). When measuring a concentration of 0.5 µg/m³ benzene in air, the levels of humidity tested did not produce any significant interference in measurements taken with any of the analysers. However, when measuring a concentration of 40 µg/m³, biases in measurements of 18% and 21% for each analyser, respectively, were obtained when the relative humidity of the sample was 80% at 20 °C. Further tests were carried out to study the nature of this interference. Results

20 show that humidity interference depends on both the amount fractions of water vapour and benzene. If benzene concentrations in an area are close to its annual limit value (5 µg/m³), biases of 2.2% can be expected when the absolute humidity is 8.6 g/cm³ –corresponding to a relative humidity of 50% at 20 °C-. This can be accounted for in the uncertainty budget of measurements with no need for corrections. If benzene concentrations are above the annual limit value, biases become higher. Thus, in these cases, actions should be taken to reduce the humidity interference, as an underestimation of benzene concentrations may cause

25 a mismanagement of air quality in these situations.

1 Introduction

Benzene is one of the species regulated in the European Union (EU) in air quality by Directive 2008/50/EC (EU, 2008). Its harmful health effects have been studied during the last five decades (Bahadar et al., 2014; Gist and Burg, 1997; Haley, 1977; Smith, 2010). Evidence for an association with childhood leukaemia (D'Andrea and Reddy, 2016a) and alterations in

hematologic and liver profiles in adults (D'Andrea and Reddy, 2016b) is lately growing. The major source of benzene in cities is gasoline, as it is one of its components as well as a product of its combustion (von Schneidmesser et al., 2010).

Continuous measurements of benzene concentrations in air monitoring stations are carried out using automated pumped sampling with in situ gas chromatography. This analytical method must comply with the requirements of Standard EN 14662-3:2015 (EN, 2015). After separation of the organic components, they are usually quantified by a flame ionisation detector (FID) – not specific for BTEX (benzene, toluene, ethylbenzene and xylenes) - or by a photo ionisation detector (PID) – a more specific one for aromatics -. Liaud et al. (Liaud et al., 2014) recently compared the performance of a transportable gas chromatograph coupled with a photo ionisation detector (GC-PID) to a thermo-desorption device coupled to GC-FID. This study revealed that the transportable GC-PID was the most sensitive technique allowing an efficient separation and quantification of the six BTEX compounds in 12 minutes.

PIDs consist of an ultraviolet lamp which produces high energy photons that collide with the molecules of the target gas and ionise them, as long as their ionisation potentials are below the energy of the photons (Peng et al., 2010). PIDs are compact yet they exhibit high performance, featuring excellent response characteristics and detection sensitivity on a ppb scale (Peng et al., 2010). As main drawbacks, they have been reported high power consumption and susceptibility to humidity (Barksy et al., 1985; Peng et al., 2010).

There are several works in the literature that assess the performance of the PID to measure volatile organic compounds (Adamia et al., 1991; Barksy et al., 1985; Coy et al., 2000; LeBouf et al., 2013; Mouradian and Flannery, 1994). However, most of them are related to measurement of species in work places. Occupational concentrations of pollutants are usually at mg/m³ levels whereas regulated concentrations of ambient air pollutants are, in most cases, at µg/m³ levels. Particularly, the European annual limit value for benzene is 5 µg/m³ (EU, 2008). These low concentrations require a specific assessment of the influence of the environmental conditions on measurements of benzene in air. In a recent paper by the authors, the influence of pressure on benzene measurements by GC-PID was studied (Romero-Trigueros et al., 2016). In this work, we focus on the influence of sample temperature and humidity on ambient measurements of benzene obtained with a commercial transportable GC-PID. Although the instrument that we test also measures toluene, ethylbenzene and xylenes, in this work, we only focus on benzene as it is currently the only VOC with limit values in air quality.

2 Materials and methods

2.1 Experimental set-up

The influence of sample temperature and humidity was studied with two identical type-approved on-site BTEX Syntech Spectras GC955 chromatographs, named analysers I and II, equipped with photo ionisation detectors. The air sample is forced through a built-in preconcentration system. Hydrocarbons are preconcentrated on Tenax GR, thermally desorbed and

Código de campo cambiado

Con formato: Inglés (Reino Unido)

Con formato: Inglés (Reino Unido)

separated on an AT-5 capillary column (15 m length x 0.32 mm i.d. x 1 µm HELIFLEX coating). The two analysers are preconfigured to identify as benzene the signals detected by the PID in the windows 176–212 s and 148–182 s, respectively. Each measurement cycle lasts for 15 min.

An in-house designed dynamic dilution system devoted to test analyser performance was used for the generation of known concentrations of benzene in zero air at controlled conditions. This chamber has been described elsewhere (Romero-Trigueros et al., 2016) and only a brief description is given here.

Purified compressed ambient air was used as zero gas. Humidity was added to a portion of the zero air by means of an in-house designed humidifier (Figure 1a). The humidifier consists of a glass sphere with two lateral inlets (1 and 2) for the zero air to enter and exit the humidifier, respectively. Water is pumped through a glass tube (3) inserted in a third inlet located at the bottom of the sphere (4). The water impacts the top of the sphere and falls down creating a wet film on the walls which favours the mass transfer. The water is collected at the bottom of the sphere (5) and taken to a container provided with thermal insulation where it is stored. When the system is working, the water from the container is pumped to the humidifier through a thermostatic bath where its temperature is readjusted. The whole system is leak-tested and relative humidities up to 99% are attainable depending on the temperatures of the zero air and the humidifying water, and the ratio of zero air flowrate through the humidifier to the flowrate of dry zero air. In Figure 1b a schematic of the humidifying system integrated in one of the lines of dry zero air is shown.

Sample relative humidity and temperature were measured with a Testo 645 thermo hygrometer (precision ± 1%). From these values, the humidity mixing ratio, W ; -the ratio of the actual mass of water vapour present in the sample to the mass of the dry air- was derived. The water vapour flow rate, q_{H_2O} (l/min), added to the flow of zero air, q_z (l/min), was calculated using Eq. (1). It is important to know this flow so that the final concentration of benzene in the reference mixture is calculated accounting for it. Thus, any decrease in benzene measurements when measuring wet samples cannot be attributed to the dilution effect of water vapour.

$$q_{H_2O} = W \cdot q_z \cdot \frac{28.8}{18} \quad (1)$$

A high concentration mixture of benzene in nitrogen (1000 µg/m³ nominal concentration, 5% expanded uncertainty) from a gas cylinder (Abelló Linde, Spain) was mixed with the humidified zero air to attain the experimental concentrations required.

The gas mixture was certified by Abelló Linde according to Standard ISO 6141:2007. The flow of gas in each branch, Figure 1b, was controlled and measured with Bronkhorst mass flow controllers (0–0.4 l/min range for the benzene in nitrogen mixture, and 0–12 l/min for the zero air). The mass flow controllers are at least annually calibrated against a Gilian Gilibrator (a NIOSH primary standard air flow calibrator) available in our lab.

Sample temperature was changed and controlled by flowing the sample through an in-house made thermostatic bath. The whole piping system right after the thermostatic bath –which included the MFCs, the humidifier, the mixing area and the sampling manifold– was set up inside a thermally controlled chamber to maintain the sample temperature, and sample inlet pressure was set up to be equal to normal atmospheric one (101.3 ± 0.2 kPa). Control of ambient conditions is pivotal to ensure

that changes on measurements are due to the effect of the environmental parameter under test humidity and not to other environmental conditions. ~~Nevertheless, in order to achieve higher absolute humidities the sample temperature was increased in some of the tests to 35 °C. Therefore, influence of sample temperature was firstly evaluated and results showed that this variable had no influence on measurements.~~

5 2.2 Experimental methods

2.2.1 Calibration

The analysers used in this work have three different calibration options, namely, a linear calibration using a least squares regression; a calibration line forced through the origin; and finally, a non-linear regression. All three calibration options were tested with eight different mixtures of benzene in air with concentrations ranging from 0.0 to 47.2 µg/m³ (0.0, 0.65, 2.60, 5.20, 10.4, 15.6, 26.3, 36.7 and 47.2 µg/m³). Thus, three calibration curves were obtained and the squared sum of residuals of the concentration tested was obtained for each calibration. The lowest sum of squares (1.16) was obtained with the non-linear (quadratic) calibration, followed by the least squares regression (1.66) and the linear regression forced through the origin (1.78). Therefore, the quadratic option was chosen every time the analysers were calibrated. Calibration was performed at 20 °C and using dry gases.

15 2.2.2 Design of experiments to study the influence of pressure sample temperature on the analyser readings

~~In order to study the influence of sample temperature on the analysers, Two temperature cycles were performed, two reference gas mixtures (40 µg/m³ and 5 µg/m³ nominal concentration) were measured with analysers I and II at different temperatures. Two temperature cycles were performed, First cycle was performed at 20 °C, then changed to 5 °C and back to 20 °C (temperature control precision ±2 °C). The second one was performed at 20 °C, then changed to 35 °C and back to 20 °C again.~~

20 ~~Once the sample temperature was stabilised 4 measurements were taken at each concentration level.~~

2.2.3. Design of experiments to study the influence of humidity on the analyser readings

2.2.3.1 First set of experiments

As a first approach to the subject, the tests described in Standard EN 14662-3:2005 were carried out after calibrating the analysers according to Section 2.2.1. ~~These tests were carried out before the release of the 2015 version of the Standard and this is why they were performed according to the previous version.~~ These tests consist of measuring a reference mixture of 0.5 µg/m³ nominal concentration benzene in air with a relative humidity of 20% and 80% at 20 °C and comparing the results.

Standard EN 14662-3:2005 defines the influence of the relative humidity by means of coefficient b_{rh} , calculated as:

$$b_{rh} = \frac{|\bar{c}_{rh,max} - \bar{c}_{rh,min}|}{|\bar{c}_{rh,max} + \bar{c}_{rh,min}|/2} \cdot 100 \quad (2)$$

Where $\bar{c}_{rh,max}$ and $\bar{c}_{rh,min}$ are the average of 6 consecutive readings when measuring the reference gas mixture (0.5 $\mu\text{g}/\text{m}^3$ nominal concentration benzene in air) with an 80% and 20% relative humidity, respectively, at 20 °C. Standard EN 14662-3:2005 establishes that b_{rh} has to be lower than 4%.

The tests were repeated with a reference mixture of 40 $\mu\text{g}/\text{m}^3$ nominal concentration benzene in air with the same relative humidities and temperature. A significant difference in readings was noticed when working with the high concentration reference mixture with both analysers. Further tests with analyser I were then performed to study in depth this phenomenon.

It is worth noting that the test for evaluating the influence of ambient humidity in the new version of the Standard EN 14662, from 2015, has substantially changed. The current version requires testing benzene at the annual limit value with relative humidity of 80% at 20 °C and comparing the measurements with those obtained with the same benzene amount fraction with no humidity. Parameter b_{rh} is now calculated as:

$$b_{rh} = \frac{x_{+w} - x_{-w}}{c_w}$$

where x_{+w} is the average of the measurements at concentration of the annual limit value in the presence of water vapour, in $\mu\text{g}/\text{m}^3$; x_{-w} is the average of the measurements at concentration of the annual limit value in the absence of water vapour, in $\mu\text{g}/\text{m}^3$ and c_w is the water vapour concentration of the test (19 mmol/mol). Calculated parameter b_{rh} has to be $\leq 0.015 \mu\text{g}/\text{m}^3/(\text{mmol}/\text{mol})$.

2.2.23.12 Second set of experiments

An in-depth study of the influence of humidity on measurements was carried out by measuring several reference mixtures of benzene in air (5 $\mu\text{g}/\text{m}^3$ nominal concentration) with different absolute humidity (AH) values ranging from 0 and 32 g/m^3 . These tests were repeated with a reference mixture of 40 $\mu\text{g}/\text{m}^3$ nominal concentration of benzene in air.

~~Humidities~~Humidity in the range 0-17 g/m^3 were/was obtained at 20 °C and relative humidities/humidity ranging from 0 to 99%. Higher absolute humidities/humidity were/was attained increasing the working temperature to 35 °C. ~~Given that the temperature of the test was not constant, a preliminary evaluation of the influence of sample temperature on measurements was performed. For this, two reference gas mixtures (40 $\mu\text{g}/\text{m}^3$ and 5 $\mu\text{g}/\text{m}^3$ nominal concentration) were measured with analyser I at different temperatures. Two temperature cycles were performed. First cycle was performed at 20 °C, then changed to 5 °C and back to 20 °C (temperature control precision ± 2 °C). The second one was performed at 20 °C, then changed to 35 °C and back to 20 °C again. Once the sample temperature was stabilised 4 measurements were taken at each concentration level.~~Results/Results in section 3.1 showed that sample temperature inside the tested range did not influence benzene measurements. Thus, this parameter can be changed in order to achieve a high absolute humidity in the samples.

3 Results and discussion

3.2.1 Influence of sample temperature on benzene measurements

As mentioned in Section 2.2.2.2, a preliminary test to evaluate the influence of sample temperature was carried out. The rationale for this was to know if this parameter affects the readings. If it is not the case, temperature can be changed during the tests and, therefore, the maximum absolute humidity tested is not limited by the saturation humidity of the sample at 20 °C. Table 2.1 shows the results of the tests when analyser I measured two reference gas mixtures (40 µg/m³ and 5 µg/m³ nominal concentration benzene in air) subjected to two temperature cycles (20 °C / 5 °C / 20 °C and 20 °C / 35 °C / 20 °C). Similar results were obtained for analyser II. As it can be seen, the change in sample temperature did not produce any significant change in readings and, thus, temperature was increased to 35 °C in some of the tests in order to work with a higher absolute humidity in our reference gas mixtures. The non-dependence of measurements on sample temperature can be explained by the fact that the sample is heated initially in the oven to 50 °C up to 70 °C, being the initial temperature of the sample being irrelevant in the whole process.

3.1.2 Compliance with the requirements of EN 14662-3:2005

Table 4.2 summarises the results obtained when carrying out the tests described in section 2.2.3.1. Whereas humidity does not have a significant influence on readings at 0.5 µg/m³ level, it does at 40 µg/m³ (calculated b_{rh} coefficients of 18% and 21% for analyser I and II, respectively). This is a negative influence, has a negative sign, that is, readings are lower than expected when the relative humidity increases for a constant temperature. Moreover, calculated coefficient b_{rh} for both analysers is turned out to be higher than 4% (the maximum variation allowed in the Standard EN 14662-3:2005) when the tests were carried out with 40 µg/m³ of benzene in air allows when working with the highest amount fraction of benzene in air. In order to study deeper this phenomenon, the tests described in section 2.2.2 were carried out and the results are shown in section 3.3. Compliance of analyser I with the requirements of the new Standard were calculated from a set of results in Table 3 (T= 20 °C, relative humidity= 81%, $C_{ref}= C_w= 5.31 \mu\text{g}/\text{m}^3$, $C_{meas}=C_w=4.99$, $C_w= 18.3 \text{ mmol}/\text{mol}$) A value of b_{rh} equal to 0.0175 µg/m³/(mmol/mol) was obtained, which is higher than the new performance criterion (0.015 µg/m³/(mmol/mol)) - From our perspective, testing this influence with a value in between the annual limit and the span (e.g. 20 µg/m³) would be interesting to detect important biases at high benzene amount fractions which can be present, for instance, in industrial areas or close to petrol stations.

3.2 Influence of sample temperature on benzene measurements

As mentioned in Section 2.2.2.2, a preliminary test to evaluate the influence of sample temperature was carried out. The rationale for this was to know if this parameter affects the readings. If it is not the case, temperature can be changed during the tests and, therefore, the maximum absolute humidity tested is not limited by the saturation humidity of the sample at 20 °C. Table 2 shows the results of the tests when analyser I measured two reference gas mixtures (40 µg/m³ and 5 µg/m³ nominal

concentration benzene in air) subjected to two temperature cycles (20 °C / 5 °C / 20 °C and 20 °C / 35 °C / 20 °C). As it can be seen, the change in sample temperature did not produce any significant change in readings and, thus, temperature was increased to 35 °C in some of the tests in order to work with a higher absolute humidity in our reference gas mixtures. The non-dependence of measurements on sample temperature can be explained by the fact that the sample is heated in the oven up to 70 °C, being the initial temperature of the sample irrelevant in the whole process.

3.3 Influence of humidity on benzene measurements

Table 3 summarises the humidity conditions, the reference concentration of benzene generated (after considering the dilution effect of water vapour), the average reading of analyser I and the calculated relative difference from the reference concentration of each test. These differences were plotted against the absolute humidity of the test, Figure 2.

There is a clear linear relationship between analyser readings and absolute humidity. For a given benzene amount fraction, the higher the absolute humidity in the sample the lower the chromatograph readings. This result was previously obtained by Barksy et al. (Barksy et al., 1985) but using concentrations of volatile organic compounds at ppm levels.

The data in Figure 2 were fitted by linear least-squares regression, which gave the following equations: $E = -1.066 \cdot AH + 4.783$ ($r^2 = 0.91$) and $E = -1.557 \cdot AH - 3.341$ ($r^2 = 0.94$) for nominal reference benzene concentrations of $5 \mu\text{g}/\text{m}^3$ and $40 \mu\text{g}/\text{m}^3$,

respectively. E is the relative difference between the reference concentration generated in the test chamber and the analyser reading. Differences between the slopes were studied to find out whether they were significantly different; for this, we used a t-value calculated from $t = (m_1 - m_2) / \text{SE}(m_1 - m_2)$, where m_1 and m_2 are the slopes of the two straight lines compared and $\text{SE}(m_1 - m_2)$ is the standard error of the difference, calculated as the square root of the quadratic sum of the standard error of each slope. A t-value of 2.272 was obtained. This value was ~~lower~~ higher than the critical one (2.145) for $p = 0.05$ and 14 degrees of freedom ($df = (n_1 - 2) + (n_2 - 2)$, where n_1 and n_2 are the number of data in the least-square regressions of Figure 2), which meant that the difference in the slopes was significant and could not be attributed to random measurement error. This is interesting as it shows that the variation of readings by effect of ambient humidity is more pronounced at higher ambient ratios of benzene. Moreover, higher concentrations of benzene are more affected by ambient water vapour as for the same absolute humidity, relative differences are higher in the tests at $40 \mu\text{g}/\text{m}^3$ than at $5 \mu\text{g}/\text{m}^3$.

For 35 °C and 80% relative humidity ($31 \text{g}/\text{m}^3$ absolute humidity approx.) the bias in readings was 33% and 47% for a reference concentration of benzene in air of $5 \mu\text{g}/\text{m}^3$ and $40 \mu\text{g}/\text{m}^3$, respectively. These conditions, although a bit extreme, can easily occur in many locations (e.g. Mediterranean areas in summer). Less extreme conditions can also have an important bias in readings (for instance, at 20 °C and 50% relative humidity there is a 2.2% bias in the concentration readings at $5 \mu\text{g}/\text{m}^3$ level and 13% at $40 \mu\text{g}/\text{m}^3$). Considering a location where mean annual benzene concentrations are close to the annual limit value ($5 \mu\text{g}/\text{m}^3$), a bias in measurements of approximately 2% can be easily expected due to a water vapour mixing ratio close to $8.6 \text{g}/\text{cm}^3$. This bias can be acceptable, taking into consideration that benzene data quality objective in current legislation for fixed measurements is 25%. Thus, it should be incorporated to the uncertainty budget of the measurements with no need for further corrections. Moreover, if ambient concentrations are below the annual limit value, the interference of environmental humidity

although not negligible will not change the air quality situation of that area. However, if benzene ambient ratios are above, measurements will be systematically underestimated by effect of ambient humidity, precisely in those areas where a stricter control of concentrations is required. It could be the case of a location that apparently meets the air quality limits because concentrations are underestimated but, in reality, its environmental situation is not acceptable. Thus, it is in these cases where humidity interference on measurements should be addressed. Areas with concentrations of benzene above the annual limit value are widely reported in the literature (Anttila et al., 2016; Bruinen De Bruin et al., 2008; Licen et al., 2016; Al Madhoun et al., 2011).

In our tests, the baseline did not change when zero gas with different amount fractions of water vapour was measured. The peak shapes and the elution times did not change either when measuring a constant amount fraction of benzene with different amount fractions of humidity. This led us to think that water vapour does not interfere in the preconcentration and separation steps and it is the PID the part of the instrument most affected by the humidity.

The effect of humidity on PID performance has been proved to be double (MSA, 2005). Despite the ionising potential of water vapour being higher than the energy of the PID, it can produce a small background signal at high non-condensing relative humidity, overestimating VOC concentrations. The second effect is the quenching of part of the UV light. When the analysers have been calibrated with dry gases and they measure a sample with humidity, the water vapour molecules in the sample absorb part of the UV radiation emitted. For a given concentration of benzene, the higher the absolute humidity in the sample the higher the absorption of UV radiation and the less energy available to ionise the molecules of benzene. This bias depends not only on the water vapour concentration but also on the benzene one, as we have checked in our tests. For a given concentration of humidity, if the concentration of benzene is very low (e.g. $0.5 \mu\text{g}/\text{m}^3$) the residual UV radiation, that is, the radiation not absorbed by the water vapour, is enough to ionise and, therefore, quantify all the molecules of benzene in the sample. This seems to be the case of the tests conducted in section 3.1 at $0.5 \mu\text{g}/\text{m}^3$, as no effect was observed when changing the amount fraction of water vapour in the reference mixture. However, as the amount fraction of benzene increases, the residual UV radiation may not be able to ionise all the molecules of benzene, as it is apparently happening with the samples with $5 \mu\text{g}/\text{m}^3$ and $40 \mu\text{g}/\text{m}^3$ benzene in air. From these two effects –background signal and radiation quenching–, the latter seems to be the most influencing as there is a decrease in readings with humidity and not an increase as it would be expected from a background signal effect.

A third phenomenon may be occurring as well. The benzene radical cation formed after ionisation of benzene can react with water to give hydroxycyclohexadienyl radical, which in turn can dissociate to benzene and OH radicals (Eberhardt, 1981). This effect is in line with the quenching effect of water vapour as both of them reduce the amount of ionised benzene reaching the electrodes.

There are a few works in the literature that use *in situ* GC-PID to measure benzene in air (Bruno et al., 2001; Kelessis et al., 2006; Villanueva et al., 2012). Bruno et al. (2001) and Villanueva et al. (2012) use gas chromatographs from Syntech Spectras

Código de campo cambiado

Con formato: Español (España)

Con formato: Español (España)

so a study of the influence of humidity in their measurements could be done as long as calibration details and relative humidity data are provided.

Bruno et al. (2001) mainly focused on source apportionment and they do not provide information related to ambient humidity. The average concentration of benzene during the sampling period was $4 \pm 1.6 \mu\text{g}/\text{m}^3$ so measurements were close to the annual limit value but, mainly, below it, so around 2% bias is expected at 20 °C and 50% relative humidity if calibration was carried out with dry gases. Villanueva et al. (2012) intercompared tropospheric ozone, benzene and toluene by a commercial DOAS and conventional monitoring techniques. The instrument used to measure benzene and toluene was the same as the one used in our work. They mention the use of certified gas mixtures to calibrate their instruments. There is no mention to water vapour in the mixtures so it is assumed that they are dry gases. Their results show that average levels for ozone, benzene and toluene obtained with DOAS were higher than those obtained with UV photometry for ozone and GC-PID for the aromatics. The largest differences found are for benzene. Although the water interference found in our work is compatible with the results obtained in Villanueva et al. (2012), it may not explain the whole difference between the analytical techniques used, which is up to 50% in some cases. A quantification in this paper of the bias in their measurements by GC-PID due to water vapour is not possible due to lack of temperature and relative humidity data.

- 15 The influence of humidity on many air quality monitoring techniques has always been a major problem. PID detectors are not the only ones affected. FID were proved to be affected as well (LeBouf et al., 2013); however, these tests were performed at ppm levels. Among the reference measurement techniques to measure air pollutants, chemiluminescence with ozone to measure NO and NO₂ is also humidity-dependent (Gerboles et al., 2003; Hayden, 2003; Miñarro and Ferradás, 2012; Steinbacher et al., 2007); and also UV photometry to measure ozone (Wilson and Birks, 2006). Recently, Bluhme et al.
- 20 (Bluhme et al., 2016) have shown that measurements of SH₂ by UV fluorescence are also affected. The interference mechanism is different in each technique but the result is always an underestimation of measurements. Some manufacturers have opted for adding filters or driers to their equipment in order to keep humidity in the sample to a minimum. These implementations have been proved to reduce biases in some cases (Bluhme et al., 2016; Steinbacher et al., 2007; Wilson and Birks, 2006). An alternative to scrubbers, which have the drawback of potentially adsorbing the target molecule, is calibration with wet gases.
- 25 Ideally, calibration procedures should be done at the same ambient conditions as sampling. Calibration with wet gases may reduce measurement uncertainty due to environmental humidity in many cases. However, a thorough work regarding short and long-term stability of wet calibration gases in gas cylinders should be first tackled by metrology institutes. Using wet calibration gases obtained by dynamic dilution could bridge the gap and help reduce the uncertainty of benzene measurements and other pollutants in ambient air.
- 30 The behaviour observed in this work is likely to be shown by GC-PID instruments by other manufacturers, although to a different extent, which means that benzene concentrations –and, presumably, given the nature of the interference, ethylbenzene, toluene and xylenes concentrations as well- may be systematically underestimated. In areas where ambient concentrations of benzene are usually above the annual limit value, the humidity interference on measurements should be urgently addressed. A joint effort from manufacturers, metrology institutes and users is advisable to reduce the bias due to

ambient humidity on BTEX measurements obtained by GC-PID –but also on measurements of other atmospheric pollutants-, as reliable data is the starting point for a correct environmental management.

Conclusions

In this work, the influence of sample temperature and ambient humidity on benzene measurements obtained with an automated *in situ* GC-PID is studied.

Sample temperature turned out not to influence measurements between 5 and 35 °C. Regarding humidity, the chromatograph was calibrated with dry gases, which is nowadays a current practice, and, subsequently, different amount fractions of humidity were added to the reference mixture. The absolute humidity tested ranged from 0 to 31 g/cm³. The dilution effect of adding water vapour was taken into account in the reference concentration calculation.

When measuring 5 µg/m³ of benzene in air, biases in readings ranged from 1 to 32% depending on the absolute humidity in the gas mixture. For an absolute humidity close to 8.6 g/cm³ –corresponding to a relative humidity of 50% at 20 °C- the bias in measurements is about 2.2%. Tests were repeated with a 40 µg/m³ benzene in air mixture. In this case, biases of up to 47% were obtained when the absolute humidity in the sample was 30 g/cm³. A less extreme absolute humidity in the sample (8 g/cm³) produced a bias of approximately 13%. Results show that water vapour interference depends on both the water and benzene amount fractions in the sample.

If the concentrations of benzene in a certain location are far below the annual limit value (5 µg/m³), the bias due to water interference can be acceptable, taking into consideration that benzene data quality objective in current legislation for fixed measurements is 25%. Thus, it should be incorporated to the uncertainty budget of the measurements with no need for further corrections. Moreover, if ambient concentrations are below the annual limit value, the interference of environmental humidity although not negligible will not change the air quality situation of that area. However, if benzene ambient ratios are above, measurements will be systematically underestimated by effect of ambient humidity, precisely in those areas where a stricter control of concentrations is required. Thus, it is in these cases where humidity interference on measurements should be addressed. Using appropriate scrubbers or wet calibration gases could help reduce measurement uncertainty of benzene and many other air pollutants monitored with analytical techniques also affected by water vapour.

Acknowledgements

We would like to acknowledge the Consejería de Agua, Agricultura y Medio Ambiente of the Comunidad Autónoma de la Región de Murcia for its financial support and for the facilities to carry out this work.

References

- Adamia, T., Budovich, V., Nevjagskaya, I., Shlyakhov, A. and Jakovlev, S.: Effect of temperature on the sensitivity of the photoionization detector, *J. Chromatogr. A*, 540, 441–448, doi:10.1016/S0021-9673(01)88836-1, 1991.
- Anttila, P., Stefanovska, A., Nestorovska-Krsteska, A., Grozdanovski, L., Atanasov, I., Golubov, N., Ristevski, P., Toceva, M., Lappi, S. and Walden, J.: Characterisation of extreme air pollution episodes in an urban valley in the Balkan Peninsula, *Air Qual. Atmos. Heal.*, 9(2), 129–141, doi:10.1007/s11869-015-0326-7, 2016.
- 5 Bahadar, H., Mostafalou, S. and Abdollahi, M.: Current understandings and perspectives on non-cancer health effects of benzene: A global concern, *Toxicol. Appl. Pharmacol.*, 276(2), 83–94, doi:10.1016/j.taap.2014.02.012, 2014.
- Barksy, J. B., Hee, S. S. Q. and Clark, C. S.: An Evaluation of the Response of Some Portable, Direct-Reading 10.2 eV and 11.8 eV Photoionization Detectors, and a Flame Ionization Gas Chromatograph for Organic Vapors in High Humidity Atmospheres, *AIHA J.*, 46(1), 9–14, doi:10.1080/15298668591394293, 1985.
- 10 Bluhme, A. B., Ingemar, J. L., Meusinger, C. and Johnson, M. S.: Water vapor inhibits hydrogen sulfide detection in pulsed fluorescence sulfur monitors, *Atmos. Meas. Tech.*, 9(6), 2669–2673, doi:10.5194/amt-9-2669-2016, 2016.
- Bruinen De Bruin, Y., Koistinen, K., Kephelopoulos, S., Geiss, O., Tirendi, S. and Kotzias, D.: Characterisation of urban inhalation exposures to benzene, formaldehyde and acetaldehyde in the European Union: Comparison of measured and modelled exposure data, *Environ. Sci. Pollut. Res.*, 15(5), 417–430, doi:10.1007/s11356-008-0013-4, 2008.
- 15 Bruno, P., Caselli, M., De Gennaro, G. and Traini, A.: Source apportionment of gaseous atmospheric pollutants by means of an absolute principal component scores (APCS) receptor model, *Anal. Bioanal. Chem.*, 371(8), 1119–1123, doi:10.1007/s002160101084, 2001.
- 20 Coy, J. D., Bigelow, P. L., Buchan, R. M., Tessari, J. D. and Parnell, J. O.: Field Evaluation of a Portable Photoionization Detector for Assessing Exposure to Solvent Mixtures, *AIHAJ - Am. Ind. Hyg. Assoc.*, 61(2), 268–274, doi:10.1080/15298660008984536, 2000.
- D’Andrea, M. A. and Reddy, G. K.: Adverse Health Effects of Benzene Exposure Among Children Following a Flaring Incident at the British Petroleum Refinery in Texas City, *Clin. Pediatr. (Phila.)*, 55(3), 219–227, doi:10.1177/0009922815594358, 2016a.
- 25 D’Andrea, M. A. and Reddy, G. K.: Detrimental Health Effects of Benzene Exposure in Adults After a Flaring Disaster at the BP Refinery Plant in Texas City, *Disaster Med. Public Health Prep.*, 10(2), 233–239, doi:10.1017/dmp.2015.160, 2016b.
- Eberhardt, M. K.: Reaction of benzene radical cation with water. Evidence for the reversibility of hydroxyl radical addition to benzene, *J. Am. Chem. Soc.*, 103(13), 3876–3878, doi:10.1021/ja00403a042, 1981.
- 30 EN: Ambient air. Standard method for the measurement of benzene concentrations. Automated pumped sampling with in situ gas chromatography, 2015.
- EU: Directive 2008/50/EC of the European Parliament and of the Council of 21 May 2008 on ambient air quality and cleaner air for Europe, *Off. J. Eur. Communities*, 152, 1–43, doi:http://eur-

- lex.europa.eu/LexUriServ/LexUriServ.do?uri=OJ:L:2008:152:0001:0044:EN:PDF, 2008.
- Gerboles, M., Lagler, F., Rembges, D. and Brun, C.: Assessment of uncertainty of NO₂ measurements by the chemiluminescence method and discussion of the quality objective of the NO₂ European Directive, *J. Environ. Monit.*, 5(4), 529, doi:10.1039/b302358c, 2003.
- 5 Gist, G. L. and Burg, J. R.: Benzene—a Review of the Literature from a Health Effects Perspective, *Toxicol. Ind. Health*, 13(6), 661–714, doi:10.1177/074823379701300601, 1997.
- Haley, T. J.: Evaluation of the health effects of benzene inhalation, *Clin. Toxicol.*, 11(5), 531, doi:<http://dx.doi.org/10.3109/15563657708988218>, 1977.
- Hayden, K. L.: Partitioning of reactive atmospheric nitrogen oxides at an elevated site in southern Quebec, Canada, *J. Geophys. Res.*, 108(D19), 4603, doi:10.1029/2002JD003188, 2003.
- 10 Kelessis, A. G., Petrakakis, M. J. and Zoumakis, N. M.: Determination of benzene, toluene, ethylbenzene, and xylenes in urban air of Thessaloniki, Greece, *Environ. Toxicol.*, 21(4), 440–443, doi:10.1002/tox.20197, 2006.
- LeBouf, R. F., Slaven, J. E. and Coffey, C. C.: Effect of calibration environment on the performance of direct-reading organic vapor monitors, *J. Air Waste Manage. Assoc.*, 63(5), 528–533, doi:10.1080/10962247.2013.772926, 2013.
- 15 Liaud, C., Nguyen, N. T., Nasreddine, R. and Le Calvé, S.: Experimental performances study of a transportable GC-PID and two thermo-desorption based methods coupled to FID and MS detection to assess BTEX exposure at sub-ppb level in air, *Talanta*, 127, 33–42, doi:10.1016/j.talanta.2014.04.001, 2014.
- Licen, S., Tolloi, A., Briguglio, S., Piazzalunga, A., Adami, G. and Barbieri, P.: Small scale spatial gradients of outdoor and indoor benzene in proximity of an integrated steel plant, *Sci. Total Environ.*, 553, 524–531, doi:10.1016/j.scitotenv.2016.02.071, 2016.
- 20 Al Madhoun, W. A., Ramli, N. A., Yahaya, A. S., Yusuf, N. F. F. M., Ghazali, N. A. and Sansuddin, N.: Levels of benzene concentrations emitted from motor vehicles in various sites in Nibong Tebal, Malaysia, *Air Qual. Atmos. Heal.*, 4(2), 103–109, doi:10.1007/s11869-010-0083-6, 2011.
- [MSA. Photoionization detectors. Technology for detection of Volatile Organic Compounds, 2005.](http://media.msanet.com/NA/USA/PermanentInstruments/GasSensorsTransmitters/SaveToxSafeVOC/07-2092WhitePaperPID.pdf)
25 <http://media.msanet.com/NA/USA/PermanentInstruments/GasSensorsTransmitters/SaveToxSafeVOC/07-2092WhitePaperPID.pdf> (last accessed: 24 June 2017)
- Miñarro, M. D. and Ferradás, E. G.: Performance evaluation of two commercial chemiluminescence NO_x analysers according to European Standard EN 14211., *J. Environ. Monit.*, 14(2), 383–90, doi:10.1039/c1em10601e, 2012.
- Mouradian, R. F. and Flannery, J. P.: Effect of Oxygen Content on Calibration of Portable VOC Instruments, *Am. Ind. Hyg. Assoc. J.*, 55(11), 1084–1086, doi:10.1080/15428119491018385, 1994.
- 30 Peng, F., Luo, T., Yuan, Y. and Qiu, L.: Performance of optimized TVOCs sensor, *Procedia Eng.*, 7, 392–398, doi:10.1016/j.proeng.2010.11.064, 2010.
- von Schneidmesser, E., Monks, P. S. and Plass-Duelmer, C.: Global comparison of VOC and CO observations in urban areas, *Atmos. Environ.*, 44(39), 5053–5064, doi:10.1016/j.atmosenv.2010.09.010, 2010.

Smith, M. T.: Advances in Understanding Benzene Health Effects and Susceptibility, *Annu. Rev. Public Health*, 31(1), 133–148, doi:10.1146/annurev.publhealth.012809.103646, 2010.

Steinbacher, M., Zellweger, C., Schwarzenbach, B., Bugmann, S., Buchmann, B., Ordóñez, C., Prevot, A. S. H. and Hueglin, C.: Nitrogen oxide measurements at rural sites in Switzerland: Bias of conventional measurement techniques, *J. Geophys. Res.*

5 *Atmos.*, 112(11), 1–13, doi:10.1029/2006JD007971, 2007.

[Romero-Trigueros](#), C. R., Miñarro, M. D., Duperón, E. G., Marzal, F. J. and Ferradás, E. G.: Study of the effect of sample pressure on in situ BTEX chromatographs, *Environ. Monit. Assess.*, doi:10.1007/s10661-016-5674-8, 2016.

Villanueva, F., Notario, A., Mabilia, R., Albaladejo, J., Cabanas, B. and Martínez, E.: Intercomparison of tropospheric O₃, benzene and toluene measured by a commercial doas system and conventional monitoring techniques, *Fresenius Environ.*

10 *Bull.*, 21(12 B), 4040–4050, 2012.


Wilson, K. L. and Birks, J. W.: Mechanism and elimination of a water vapor interference in the measurement of ozone by UV absorbance, *Environ. Sci. Technol.*, 40(20), 6361–6367, doi:10.1021/es052590c, 2006.

15


20

25

30

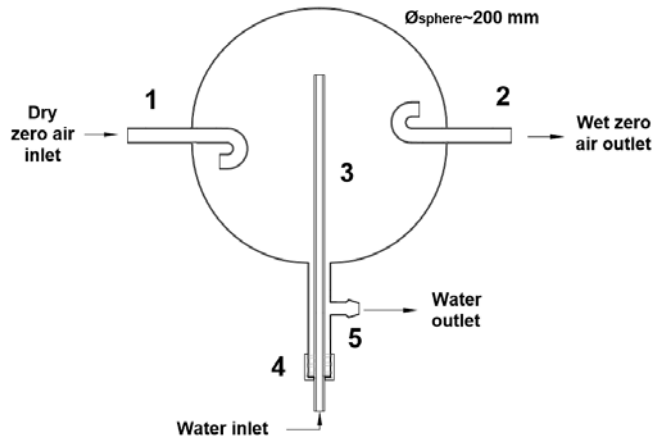

a)

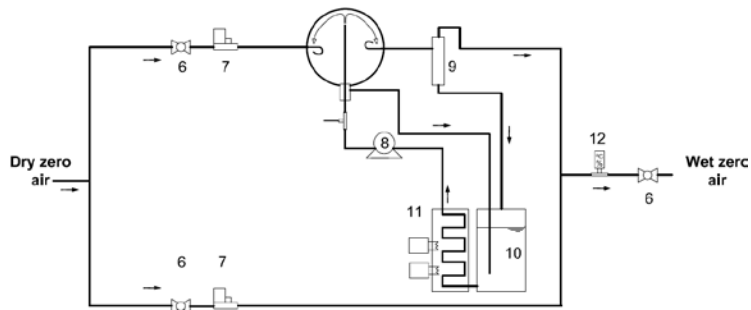

5

b)

Figure 1: Schematic of the (a) humidifier and (b) the elements that comprise the humidifying system used in this work. 1: dry zero air inlet, 2: wet zero air outlet, 3 and 4: water inlet, 5: water outlet, 6: shut-off valves, 7: mass flow controllers, 8: water pump, 9: cyclone, 10: water container, 11: thermostatic bath, 12: thermo-hygrometer.

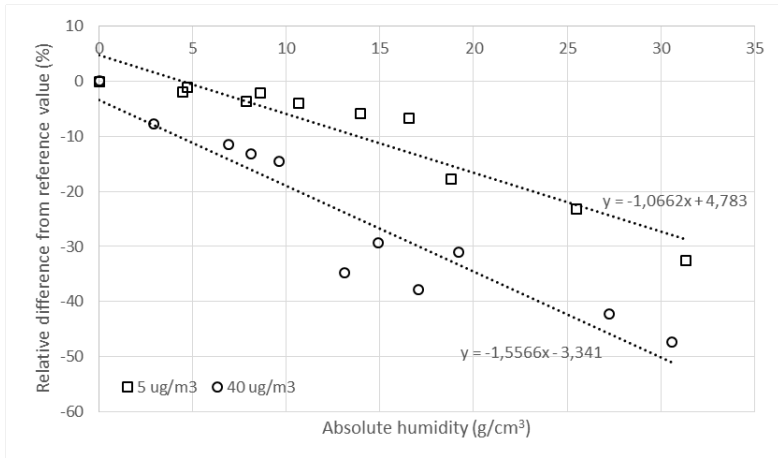


Figure 2: Relative differences in readings from the reference value of concentration as a function of the absolute humidity of the sample.

5

10

15

20

Table 1: Analyser readings when subjected to changes in ambient humidity for a constant reference concentration and sensitivity coefficient to humidity (b_{RH}). Test temperature: $20 \pm 2^\circ\text{C}$

5

Temperature cycle	20 °C	5 °C	20 °C
Average reading of concentration ($\mu\text{g}/\text{m}^3$) when measuring a benzene concentration of $39.96 \mu\text{g}/\text{m}^3$	$39.96 \pm(0.45)$	$39.69 \pm(0.26)$	$39.82 \pm(0.29)$
Average reading of concentration ($\mu\text{g}/\text{m}^3$) when measuring a benzene concentration of $4.77 \mu\text{g}/\text{m}^3$	$4.77 \pm(0.08)$	$4.76 \pm(0.06)$	$4.78 \pm(0.06)$
Temperature cycle	20 °C	35 °C	20 °C
Average reading of concentration ($\mu\text{g}/\text{m}^3$) when measuring a benzene concentration of $39.96 \mu\text{g}/\text{m}^3$	$39.82 \pm(0.29)$	$39.78 \pm(0.50)$	$39.87 \pm(0.25)$
Average reading of concentration ($\mu\text{g}/\text{m}^3$) when measuring a benzene concentration of $4.77 \mu\text{g}/\text{m}^3$	$4.78 \pm(0.06)$	$4.77 \pm(0.10)$	$4.78 \pm(0.11)$

Table 2: Analyser I readings when subjected to changes in sample temperature. In brackets, the standard deviation of the measurements.

10

<u>Test nominal concentration: 0.5 µg/m³</u>	<u>Average value</u>	<u>Average value</u>
	<u>Analyser I (µg/m³)</u>	<u>Analyser II (µg/m³)</u>
<u>20% relative humidity</u>	<u>0.53 (0.01)</u>	<u>0.55 (0.01)</u>
<u>80% relative humidity</u>	<u>0.51 (0.01)</u>	<u>0.53 (0.01)</u>
<u><i>b_{rh}</i> (%)</u>	<u>3.1</u>	<u>3.9</u>
<u>Test nominal concentration: 40 µg/m³</u>		
<u>20% relative humidity</u>	<u>44.3 (0.17)</u>	<u>46.7 (0.47)</u>
<u>80% relative humidity</u>	<u>36.9 (0.23)</u>	<u>37.9 (0.18)</u>
<u><i>b_{rh}</i> (%)</u>	<u>18.2</u>	<u>20.8</u>

Table 24: Analyser readings when subjected to changes in ambient humidity for a constant reference concentration and sensitivity coefficient to humidity (*b_{rh}*). Test temperature: 20 ± 2 °C. In brackets, the standard deviation of the measurements.

T= 20 ± 2 °C; Cstd= 1053.5 ± 26.3 µg/m³; q_z= 11.636 ± 0.002 l/min

RH (%)	AH (g/cm ³)	W (g H ₂ O/g dry air)	q _{H2O} (l/min)	q _t (l/min)	C _{ref} (µg/m ³)	C _{meas} (µg/m ³)	Diff (%)
0.4	0.0689	5.74·10 ⁻⁵	1.069·10 ⁻³	11.697	5.40	5.40	0.00
26	4.480	0.00373	0.0695	11.765	5.37	5.27	-1.95
50	8.616	0.00718	0.134	11.830	5.34	5.23	-2.20
62	10.68	0.00890	0.166	11.862	5.33	5.12	-3.95
81	13.96	0.0116	0.217	11.913	5.31	4.99	-5.94
96	16.54	0.0138	0.257	11.953	5.29	4.93	-6.70

T= 35 ± 2 °C; Cstd= 1053.5 ± 26.3 µg/m³; q_z= 11.637 ± 0.002 l/min

RH (%)	AH (g/cm ³)	W (g H ₂ O/g dry air)	q _{H2O} (l/min)	q _t (l/min)	C _{ref} (µg/m ³)	C _{meas} (µg/m ³)	Diff (%)
0.2	0.0345	2.871·10 ⁻⁵	5.347·10 ⁻⁴	11.697	5.40	5.40	0.00
12	4.70	0.00392	0.0730	11.769	5.37	5.31	-1.12
20	7.84	0.00653	0.122	11.818	5.35	5.15	-3.75
48	18.82	0.0157	0.292	11.988	5.27	4.34	-17.8
65	25.48	0.0212	0.395	12.091	5.23	4.01	-23.3
80	31.36	0.0261	0.487	12.183	5.19	3.50	-32.6

T= 25 ± 2 °C; Cstd= 1053.5 ± 26.3 µg/m³; q_z= 9.099 ± 0.002 l/min

RH (%)	AH (g/cm ³)	W (g H ₂ O/g dry air)	q _{H2O} (l/min)	q _t (l/min)	C _{ref} (µg/m ³)	C _{meas} (µg/m ³)	Diff (%)
1.1	0.190	1.579·10 ⁻⁴	2.299·10 ⁻³	9.461	40.07	40.08	0.02
17	2.929	0.00244	0.0355	9.494	39.93	36.85	-7.72
40	6.893	0.00574	0.0836	9.543	39.73	35.18	-11.46
47	8.099	0.00675	0.0983	9.557	39.67	34.43	-13.21
76	13.10	0.0109	0.1589	9.618	39.42	25.70	-34.80
99	17.06	0.0142	0.207	9.666	39.23	24.37	-37.87

T= 35 ± 2 °C; Cstd= 1053.5 ± 26.3 µg/m³; q_z= 9.098 ± 0.002 l/min

RH (%)	AH (g/cm ³)	W (g H ₂ O/g dry air)	q _{H2O} (l/min)	q _t (l/min)	C _{ref} (µg/m ³)	C _{meas} (µg/m ³)	Diff (%)
--------	-------------------------	----------------------------------	--------------------------	------------------------	---------------------------------------	----------------------------------------	----------

1.8	0.706	$5.88 \cdot 10^{-3}$	$8.56 \cdot 10^{-3}$	9.466	40.05	40.09	0.10
25	9.604	0.0080	0.117	9.574	39.60	33.83	-14.56
38	14.90	0.0125	0.182	9.640	39.33	27.82	-29.28
49	19.21	0.0161	0.235	9.693	39.12	26.95	-31.10
70	27.24	0.0229	0.333	9.791	38.72	22.38	-42.20
78	30.57	0.0257	0.374	9.832	38.56	20.28	-47.41

Table 3: Relative and absolute humidity, reference concentration of benzene, average reading of analyser I and relative difference between measurements and reference values. q_t is the total flow rate, calculated as the sum of q_{bz} , q_{H_2O} and the flow rate from the benzene reference gas mixture.

MINOR REVISION

Response to Reviewer#1

First of all, we would like to thank reviewer#1 for taking the time to review our paper again and for his/her valuable suggestions, which have definitively improved our paper.

Review of the manuscript entitled "Influence of sample temperature and environmental humidity on measurements of benzene in ambient air by transportable GC-PID", by Romero-Trigueros et al.

General comments.

The manuscript by Romero-Trigueros et al. address an important issue regarding air quality monitoring of benzene by transportable GC-PID. The tests are reported clearly and the implications discussed appropriately. My main concerns have been addressed in an appropriate way. I recommend the manuscript in its present form for publication in AMT, even if I spotted a few instances where the manuscript could still be improved slightly. See my comments below.

Specific comments.

- page 2, lines 6-7: I suggest to use "selective" rather than "specific".

This change has been addressed.

- page 3, line 23 (equation (1)): What are the numbers 28.8 and 18 and what are their units?

These are the molar masses of dry air and water in g/mol, respectively. This explanation has been added to the text. When changing units from mol to litre (for instance, by multiplying and dividing by 22.4 litres in normal conditions, the units of both sides of the equation agree).

- page 6, section 3.2: Because b_{rh} is defined twice, I suggest for clarity to rename the latter one b_{rh}(new) or at least differentiate it in some way (also the units are different).

Thanks for this suggestion, which has been implemented.

- page 6, lines 17-19: Is there any reason why the suggested test has not been performed?

This sentence refers to the new version of Standard EN 14662. In the old version two different concentrations were tested (0.5 and 40 µg/m³) but in the new one, tests are performed only at 5 µg/m³. As it is discussed later in the paper, the higher the benzene concentration the higher the interference for a given water vapour amount fraction. That is why we suggest performing these tests at higher benzene amount fraction. One can argue that 40 µg/m³ is too high and that is why we suggest an intermediate concentration around 20 µg/m³. In order to clarify this discussion in the paper, we have added a sentence in page 5 line 16 to catch the attention of the reader in the fact that the higher concentration of benzene has been removed from the tests. Later, in page 6 we have reworded the sentence starting in line 17 to make our point clearer.

- page 15, Table 1: The given benzene concentrations in the first column are calculated from the standard concentration and dilution (nominal). What is the uncertainty on these values?

The expanded uncertainties of the reference values have been added to Table 1.

- page 16, Table 2: The authors could consider introducing the newer b_{rh} values as well.

The value of the coefficient according to EN 14662 has been added in Table 2.

Technical corrections

- page 2, lines 6-7: Fix the use of hyphens/dashes.
- page 2, line 7: Fix the reference ("Liaud et al. (2014) recently...").
- page 5, line 5: No comma after "(AH)" and replace "from 0 and 32" by "from 0 to 32".
- page 6, line 16: Missing full stop after first parenthesis.
- page 9, line 15, Fix the use of hyphens/dashes.
- page 9, lines 18-19: Avoid paragraphs with only one sentence.

Thanks for spotting all these typos.

- page 10, lines 20/30: Use a consistent abbreviation for "AIHAJ" (page 12, lines 7-8).
In order to be consistent also with the rest of the references, we have opted for *Am. Ind. Hyg. Assoc. J.*

- page 11, line 11: Is there also a link available? (state the date of last access).
EN Standards are not public, they have to be bought. In our case, our institution has access to read them online but this is not possible for everybody. For this reason, we think it is better not to include a link.

- page 11, line 13: State the date of last access.
This date has been included.

- page 12, line 20: Fix the name "Mar??nez".
This has been fixed and changed to Martínez.

- page 14, Figure 2: I suggest to use E and AH for the equations, as in the main text, and to use the same amount of significant digits.
The x- and y-axis titles have been changed to AH and E as suggested.

- page 18, Table 3: Include the name of the variables in the table caption.
The name of the variables not stated in the original caption have been included as well.

Influence of sample temperature and environmental humidity on measurements of benzene in ambient air by transportable GC-PID

Cristina Romero-Trigueros¹, Marta Doval Miñarro², Esther González Duperón¹, Enrique González Ferradás¹

¹Chemical Engineering Department, School of Chemistry, University of Murcia, 30071, Murcia, Spain

²Chemical and Environmental Engineering Department, Technical University of Cartagena, Paseo Alfonso XIII, 52, 30203 Cartagena, Murcia, Spain

Correspondence to: Marta Doval Miñarro (marta.doval@upct.es)

10 **Abstract.** Calibration of *in situ* analysers of air pollutants is usually done with dry standards. In this paper, the influence of
sample temperature and environmental humidity on benzene measurements by gas chromatography coupled with a photo
ionisation detector (GC-PID) are studied. Two reference gas mixtures (40 µg/m³ and 5 µg/m³ nominal concentration benzene
in air) were subjected to two temperature cycles (20 °C / 5 °C / 20 °C and 20 °C / 35 °C / 20 °C) and measured with two
identical GC-PIDs. The change in sample temperature did not produce any significant change in readings. Regarding
15 ambient humidity, the chromatographs were calibrated for benzene with dry gases and subjected to measure reference
standards with humidity (20% and 80% at 20 °C). When measuring a concentration of 0.5 µg/m³ benzene in air, the levels of
humidity tested did not produce any significant interference in measurements taken with any of the analysers. However,
when measuring a concentration of 40 µg/m³, biases in measurements of 18% and 21% for each analyser, respectively, were
obtained when the relative humidity of the sample was 80% at 20 °C. Further tests were carried out to study the nature of this
20 interference. Results show that humidity interference depends on both the amount fractions of water vapour and benzene. If
benzene concentrations in an area are close to its annual limit value (5 µg/m³), biases of 2.2% can be expected when the
absolute humidity is 8.6 g/cm³ –corresponding to a relative humidity of 50% at 20 °C-. This can be accounted for in the
uncertainty budget of measurements with no need for corrections. If benzene concentrations are above the annual limit value,
biases become higher. Thus, in these cases, actions should be taken to reduce the humidity interference, as an
25 underestimation of benzene concentrations may cause a mismanagement of air quality in these situations.

1 Introduction

30 Benzene is one of the species regulated in the European Union (EU) in air quality by Directive 2008/50/EC (EU, 2008). Its
harmful health effects have been studied during the last five decades (Bahadar et al., 2014; Gist and Burg, 1997; Haley,
1977; Smith, 2010). Evidence for an association with childhood leukaemia (D'Andrea and Reddy, 2016a) and alterations in

hematologic and liver profiles in adults (D'Andrea and Reddy, 2016b) is lately growing. The major source of benzene in cities is gasoline, as it is one of its components as well as a product of its combustion (von Schneidmesser et al., 2010).

Continuous measurements of benzene concentrations in air monitoring stations are carried out using automated pumped sampling with in situ gas chromatography. This analytical method must comply with the requirements of Standard EN 14662-3:2015 (EN, 2015). After separation of the organic components, they are usually quantified by a flame ionisation detector (FID) – not ~~specific-selective~~ for BTEX (benzene, toluene, ethylbenzene and xylenes) - or by a photo ionisation detector (PID) – a more ~~specific-selective~~ one for aromatics–. Liaud et al. (Liaud et al., 2014) recently compared the performance of a transportable gas chromatograph coupled with a photo ionisation detector (GC-PID) to a thermo-desorption device coupled to GC-FID. This study revealed that the transportable GC-PID was the most sensitive technique allowing an efficient separation and quantification of the six BTEX compounds in 12 minutes.

PIDs consist of an ultraviolet lamp which produces high energy photons that collide with the molecules of the target gas and ionise them, as long as their ionisation potentials are below the energy of the photons (Peng et al., 2010). PIDs are compact yet they exhibit high performance, featuring excellent response characteristics and detection sensitivity on a ppb scale (Peng et al., 2010). As main drawbacks, they have been reported high power consumption and susceptibility to humidity (Barksy et al., 1985; Peng et al., 2010).

There are several works in the literature that assess the performance of the PID to measure volatile organic compounds (Adamia et al., 1991; Barksy et al., 1985; Coy et al., 2000; LeBouf et al., 2013; Mouradian and Flannery, 1994). However, most of them are related to measurement of species in work places. Occupational concentrations of pollutants are usually at mg/m³ levels whereas regulated concentrations of ambient air pollutants are, in most cases, at µg/m³ levels. Particularly, the European annual limit value for benzene is 5 µg/m³ (EU, 2008). These low concentrations require a specific assessment of the influence of the environmental conditions on measurements of benzene in air. In a recent paper by the authors, the influence of pressure on benzene measurements by GC-PID was studied (Romero-Trigueros et al., 2016). In this work, we focus on the influence of sample temperature and humidity on ambient measurements of benzene obtained with a commercial transportable GC-PID. Although the instrument that we test also measures toluene, ethylbenzene and xylenes, in this work, we only focus on benzene as it is currently the only VOC with limit values in air quality.

2 Materials and methods

2.1 Experimental set-up

The influence of sample temperature and humidity was studied with two identical type-approved on-site BTEX Syntech Spectras GC955 chromatographs, named analysers I and II, equipped with photo ionisation detectors. The air sample is forced through a built-in preconcentration system. Hydrocarbons are preconcentrated on Tenax GR, thermically desorbed

Con formato: Inglés (Reino Unido)

Código de campo cambiado

and separated on an AT-5 capillary column (15 m length x 0.32 mm i.d. x 1 μ m HELIFLEX coating). The two analysers are preconfigured to identify as benzene the signals detected by the PID in the windows 176–212 s and 148–182 s, respectively. Each measurement cycle lasts for 15 min.

An in-house designed dynamic dilution system devoted to test analyser performance was used for the generation of known concentrations of benzene in zero air at controlled conditions. This chamber has been described elsewhere (Romero-Trigueros et al., 2016) and only a brief description is given here.

Purified compressed ambient air was used as zero gas. Humidity was added to a portion of the zero air by means of an in-house designed humidifier (Figure 1a). The humidifier consists of a glass sphere with two lateral inlets (1 and 2) for the zero air to enter and exit the humidifier, respectively. Water is pumped through a glass tube (3) inserted in a third inlet located at the bottom of the sphere (4). The water impacts the top of the sphere and falls down creating a wet film on the walls which favours the mass transfer. The water is collected at the bottom of the sphere (5) and taken to a container provided with thermal insulation where it is stored. When the system is working, the water from the container is pumped to the humidifier through a thermostatic bath where its temperature is readjusted. The whole system is leak-tested and relative humidities up to 99% are attainable depending on the temperatures of the zero air and the humidifying water, and the ratio of zero air flowrate through the humidifier to the flowrate of dry zero air. In Figure 1b a schematic of the humidifying system integrated in one of the lines of dry zero air is shown.

Sample relative humidity and temperature were measured with a Testo 645 thermo hygrometer (precision \pm 1%). From these values, the humidity mixing ratio, W -the ratio of the actual mass of water vapour present in the sample to the mass of the dry air- was derived. The water vapour flow rate, q_{H_2O} (l/min), added to the flow of zero air, q_z (l/min), was calculated using Eq. (1), where 28.8 and 18 are the molar masses of dry air and water, respectively, in g/mol. It is important to know this flow so that the final concentration of benzene in the reference mixture is calculated accounting for it. Thus, any decrease in benzene measurements when measuring wet samples cannot be attributed to the dilution effect of water vapour.

$$q_{H_2O} = W \cdot q_z \cdot \frac{28.8}{18} \quad (1)$$

A high concentration mixture of benzene in nitrogen (1000 μ g/m³ nominal concentration, 5% expanded uncertainty) from a gas cylinder (Abelló Linde, Spain) was mixed with the humidified zero air to attain the experimental concentrations required. The gas mixture was certified by Abelló Linde according to Standard ISO 6141:2007. The flow of gas in each branch, Figure 1b, was controlled and measured with Bronkhorst mass flow controllers (0–0.4 l/min range for the benzene in nitrogen mixture, and 0–12 l/min for the zero air). The mass flow controllers are at least annually calibrated against a Gilian Gilibrator (a NIOSH primary standard air flow calibrator) available in our lab.

Sample temperature was changed and controlled by flowing the sample through an in-house made thermostatic bath. The whole piping system right after the thermostatic bath –which included the MFCs, the humidifier, the mixing area and the sampling manifold- was set up inside a thermally controlled chamber to maintain the sample temperature. Sample inlet pressure was set up to be equal to normal atmospheric one (101.3 \pm 0.2 kPa). Control of ambient conditions is pivotal to

ensure that changes on measurements are due to the effect of the environmental parameter under test and not to other environmental conditions.

2.2 Experimental methods

2.2.1 Calibration

5 The analysers used in this work have three different calibration options, namely, a linear calibration using a least squares regression; a calibration line forced through the origin; and finally, a non-linear regression. All three calibration options were tested with eight different mixtures of benzene in air with concentrations ranging from 0.0 to 47.2 $\mu\text{g}/\text{m}^3$ (0.0, 0.65, 2.60, 5.20, 10.4, 15.6, 26.3, 36.7 and 47.2 $\mu\text{g}/\text{m}^3$). Thus, three calibration curves were obtained and the squared sum of residuals of the concentration tested was obtained for each calibration. The lowest sum of squares (1.16) was obtained with the non-
10 linear (quadratic) calibration, followed by the least squares regression (1.66) and the linear regression forced through the origin (1.78). Therefore, the quadratic option was chosen every time the analysers were calibrated. Calibration was performed at 20 °C and using dry gases.

2.2.2 Design of experiments to study the influence of sample temperature on the analyser readings

In order to study the influence of sample temperature on the analysers, two reference gas mixtures (40 $\mu\text{g}/\text{m}^3$ and 5 $\mu\text{g}/\text{m}^3$
15 nominal concentration) were measured with analysers I and II at different temperatures. Two temperature cycles were performed. First cycle was performed at 20 °C, then changed to 5 °C and back to 20 °C (temperature control precision ± 2 °C). The second one was performed at 20 °C, then changed to 35 °C and back to 20 °C again. Once the sample temperature was stabilised 4 measurements were taken at each concentration level.

2.2.3. Design of experiments to study the influence of humidity on the analyser readings

20 2.2.3.1 First set of experiments

As a first approach to the subject, the tests described in Standard EN 14662-3:2005 were carried out after calibrating the analysers according to Section 2.2.1. These tests were carried out before the release of the 2015 version of the Standard and this is why they were performed according to the previous version. These tests consist of measuring a reference mixture of 0.5 $\mu\text{g}/\text{m}^3$ nominal concentration benzene in air with a relative humidity of 20% and 80% at 20 °C and comparing the results.

25 Standard EN 14662-3:2005 defines the influence of the relative humidity by means of coefficient b_{rh} , calculated as:

$$b_{rh} = \frac{|\bar{c}_{rh,max} - \bar{c}_{rh,min}|}{|\bar{c}_{rh,max} + \bar{c}_{rh,min}|/2} \cdot 100 \quad (2)$$

Where $\bar{C}_{rh,max}$ and $\bar{C}_{rh,min}$ are the average of 6 consecutive readings when measuring the reference gas mixture (0.5 $\mu\text{g}/\text{m}^3$ nominal concentration benzene in air) with an 80% and 20% relative humidity, respectively, at 20 °C. Standard EN 14662-3:2005 establishes that b_{rh} has to be lower than 4%.

The tests were repeated with a reference mixture of 40 $\mu\text{g}/\text{m}^3$ nominal concentration benzene in air with the same relative humidities and temperature. A significant difference in readings was noticed when working with the high concentration reference mixture with both analysers. Further tests with analyser I were then performed to study in depth this phenomenon.

It is worth noting that the test for evaluating the influence of ambient humidity in the new version of the Standard EN 14662, from 2015, has substantially changed. The current version requires testing benzene at the annual limit value with relative humidity of 80% at 20 °C and comparing the measurements with those obtained with the same benzene amount fraction with no humidity. Parameter b_{rh} is now calculated as:

$$b_{rh,new} = \frac{x_{+w} - x_{-w}}{c_w}$$

where x_{+w} is the average of the measurements at concentration of the annual limit value in the presence of water vapour, in $\mu\text{g}/\text{m}^3$; x_{-w} is the average of the measurements at concentration of the annual limit value in the absence of water vapour, in $\mu\text{g}/\text{m}^3$; and c_w is the water vapour concentration of the test (19 mmol/mol). Calculated parameter $b_{rh,new}$ has to be $\leq 0.015 \mu\text{g}/\text{m}^3/(\text{mmol}/\text{mol})$. It is interesting to note that this test is not carried out anymore at 40 $\mu\text{g}/\text{m}^3$.

2.2.3.2 Second set of experiments

An in-depth study of the influence of humidity on measurements was carried out by measuring several reference mixtures of benzene in air (5 $\mu\text{g}/\text{m}^3$ nominal concentration) with different absolute humidity (AH), values ranging from 0 ~~and to~~ 32 g/m^3 .

These tests were repeated with a reference mixture of 40 $\mu\text{g}/\text{m}^3$ nominal concentration of benzene in air.

Humidity in the range 0-17 g/m^3 was obtained at 20 °C and relative humidity ranging from 0 to 99%. Higher absolute humidity was attained increasing the working temperature to 35 °C. Results in section 3.1 showed that sample temperature inside the tested range did not influence benzene measurements. Thus, this parameter can be changed in order to achieve a high absolute humidity in the samples.

3 Results and discussion

3.1 Influence of sample temperature on benzene measurements

As mentioned in Section 2.2.2, a test to evaluate the influence of sample temperature was carried out. The rationale for this was to know if this parameter affects the readings. If it is not the case, temperature can be changed during the tests and, therefore, the maximum absolute humidity tested is not limited by the saturation humidity of the sample at 20 °C. Table 1 shows the results of the tests when analyser I measured two reference gas mixtures (40 $\mu\text{g}/\text{m}^3$ and 5 $\mu\text{g}/\text{m}^3$ nominal

concentration benzene in air) subjected to two temperature cycles (20 °C / 5 °C / 20 °C and 20 °C / 35 °C / 20 °C). Similar results were obtained for analyser II. As it can be seen, the change in sample temperature did not produce any significant change in readings and, thus, temperature was increased to 35 °C in some of the tests in order to work with a higher absolute humidity in our reference gas mixtures. The non-dependence of measurements on sample temperature can be explained by the fact that the sample is heated initially in the oven to 50 °C, the initial temperature of the sample being irrelevant in the whole process.

3.2 Compliance with the requirements of EN 14662-3:2005

Table 2 summarises the results obtained when carrying out the tests described in section 2.2.3.1. Whereas humidity does not have a significant influence on readings at 0.5 µg/m³ level, it does at 40 µg/m³ (calculated b_{rh} coefficients of 18% and 21% for analyser I and II, respectively). This is a negative influence, that is, readings are lower than expected when the relative humidity increases for a constant temperature. Moreover, calculated coefficient b_{rh} for both analysers turned out to be higher than 4% (the maximum variation allowed in the Standard EN 14662-3:2005) when the tests were carried out with 40 µg/m³ of benzene in air. In order to study deeper this phenomenon, the tests described in section 2.2.2.2 were carried out and the results are shown in section 3.3. Compliance of analyser I with the requirements of the new Standard ~~were was~~ calculated from a set of results in Table 3 (T= 20 °C, relative humidity= 81%, $C_{ref}= C_w= 5.31 \mu\text{g}/\text{m}^3$, $C_{meas}=C_w=4.99$, $C_w= 18.3 \text{ mmol}/\text{mol}$). A value of b_{hr_new} equal to 0.0175 µg/m³/(mmol/mol) was obtained, which is higher than the new performance criterion (0.015 µg/m³/(mmol/mol)). ~~This interference would be even larger if the tests were conducted at 40 µg/m³ (see Section 3.3).~~ From our perspective, ~~when type-approving GC-PID analysers, testing the humidity interference with testing this influence with~~ a value in between the annual limit and the span (e.g. 20 µg/m³) would be interesting to detect important biases at high benzene amount fractions, which can be present, for instance, in industrial areas or close to petrol stations.

Con formato: Fuente: Cursiva

Con formato: Fuente: Cursiva

3.3 Influence of humidity on benzene measurements

Table 3 summarises the humidity conditions, the reference concentration of benzene generated (after considering the dilution effect of water vapour), the average reading of analyser I and the calculated relative difference from the reference concentration of each test. These differences were plotted against the absolute humidity of the test, Figure 2.

There is a clear linear relationship between analyser readings and absolute humidity. For a given benzene amount fraction, the higher the absolute humidity in the sample the lower the chromatograph readings. This result was previously obtained by Barksy et al. (Barksy et al., 1985) but using concentrations of volatile organic compounds at ppm levels.

The data in Figure 2 were fitted by linear least-squares regression, which gave the following equations: $E= -1.066 \cdot AH + 4.783$ ($r^2=0.91$) and $E= -1.557 \cdot AH - 3.341$ ($r^2=0.94$) for nominal reference benzene concentrations of 5 µg/m³ and 40 µg/m³, respectively. E is the relative difference between the reference concentration generated in the test chamber and the analyser reading. Differences between the slopes were studied to find out whether they were significantly different; for this, we used a

t-value calculated from $t = (m_1 - m_2) / SE(m_1 - m_2)$, where m_1 and m_2 are the slopes of the two straight lines compared and $SE(m_1 - m_2)$ is the standard error of the difference, calculated as the square root of the quadratic sum of the standard error of each slope. A t-value of 2.272 was obtained. This value was higher than the critical one (2.145) for $p=0.05$ and 14 degrees of freedom ($df=(n_1-2)+(n_2-2)$), where n_1 and n_2 are the number of data in the least-square regressions of Figure 2), which meant
5 that the difference in the slopes was significant and could not be attributed to random measurement error. This is interesting as it shows that the variation of readings by effect of ambient humidity is more pronounced at higher ambient ratios of benzene. Moreover, higher concentrations of benzene are more affected by ambient water vapour as for the same absolute humidity, relative differences are higher in the tests at $40 \mu\text{g}/\text{m}^3$ than at $5 \mu\text{g}/\text{m}^3$.

For $35 \text{ }^\circ\text{C}$ and 80% relative humidity ($31 \text{ g}/\text{m}^3$ absolute humidity approx.) the bias in readings was 33% and 47% for a
10 reference concentration of benzene in air of $5 \mu\text{g}/\text{m}^3$ and $40 \mu\text{g}/\text{m}^3$, respectively. These conditions, although a bit extreme, can easily occur in many locations (e.g. Mediterranean areas in summer). Less extreme conditions can also have an important bias in readings (for instance, at $20 \text{ }^\circ\text{C}$ and 50% relative humidity there is a 2.2% bias in the concentration readings at $5 \mu\text{g}/\text{m}^3$ level and 13% at $40 \mu\text{g}/\text{m}^3$). Considering a location where mean annual benzene concentrations are close to the annual limit value ($5 \mu\text{g}/\text{m}^3$), a bias in measurements of approximately 2% can be easily expected due to a water
15 vapour mixing ratio close to $8.6 \text{ g}/\text{cm}^3$. This bias can be acceptable, taking into consideration that benzene data quality objective in current legislation for fixed measurements is 25%. Thus, it should be incorporated to the uncertainty budget of the measurements with no need for further corrections. Moreover, if ambient concentrations are below the annual limit value, the interference of environmental humidity although not negligible will not change the air quality situation of that area. However, if benzene ambient ratios are above, measurements will be systematically underestimated by effect of ambient
20 humidity, precisely in those areas where a stricter control of concentrations is required. It could be the case of a location that apparently meets the air quality limits because concentrations are underestimated but, in reality, its environmental situation is not acceptable. Thus, it is in these cases where humidity interference on measurements should be addressed. Areas with concentrations of benzene above the annual limit value are widely reported in the literature (Anttila et al., 2016; Bruinen De Bruin et al., 2008; Licen et al., 2016; Al Madhoun et al., 2011).

25 In our tests, the baseline did not change when zero gas with different amount fractions of water vapour was measured. The peak shapes and the elution times did not change either when measuring a constant amount fraction of benzene with different amount fractions of humidity. This led us to think that water vapour does not interfere in the preconcentration and separation steps and it is the PID the part of the instrument most affected by the humidity.

The effect of humidity on PID performance has been proved to be double (MSA, 2005). Despite the ionising potential of
30 water vapour being higher than the energy of the PID, it can produce a small background signal at high non-condensing relative humidity, overestimating VOC concentrations. The second effect is the quenching of part of the UV light. When the analysers have been calibrated with dry gases and they measure a sample with humidity, the water vapour molecules in the sample absorb part of the UV radiation emitted. For a given concentration of benzene, the higher the absolute humidity in the sample the higher the absorption of UV radiation and the less energy available to ionise the molecules of benzene. This bias

depends not only on the water vapour concentration but also on the benzene one, as we have checked in our tests. For a given concentration of humidity, if the concentration of benzene is very low (e.g. $0.5 \mu\text{g}/\text{m}^3$) the residual UV radiation, that is, the radiation not absorbed by the water vapour, is enough to ionise and, therefore, quantify all the molecules of benzene in the sample. This seems to be the case of the tests conducted in section 3.1 at $0.5 \mu\text{g}/\text{m}^3$, as no effect was observed when

5 changing the amount fraction of water vapour in the reference mixture. However, as the amount fraction of benzene increases, the residual UV radiation may not be able to ionise all the molecules of benzene, as it is apparently happening with the samples with $5 \mu\text{g}/\text{m}^3$ and $40 \mu\text{g}/\text{m}^3$ benzene in air. From these two effects –background signal and radiation quenching–, the latter seems to be the most influencing as there is a decrease in readings with humidity and not an increase as it would be expected from a background signal effect.

10 A third phenomenon may be occurring as well. The benzene radical cation formed after ionisation of benzene can react with water to give hydroxycyclohexadienyl radical, which in turn can dissociate to benzene and OH radicals (Eberhardt, 1981). This effect is in line with the quenching effect of water vapour as both of them reduce the amount of ionised benzene reaching the electrodes.

There are a few works in the literature that use *in situ* GC-PID to measure benzene in air (Bruno et al., 2001; Kelessis et al.,

15 2006; Villanueva et al., 2012). Bruno et al. (2001) and Villanueva et al. (2012) use gas chromatographs from Syntech Spectras so a study of the influence of humidity in their measurements could be done as long as calibration details and relative humidity data are provided.

Bruno et al. (2001) mainly focused on source apportionment and they do not provide information related to ambient humidity. The average concentration of benzene during the sampling period was $4 \pm 1.6 \mu\text{g}/\text{m}^3$ so measurements were close

20 to the annual limit value but, mainly, below it, so around 2% bias is expected at $20 \text{ }^\circ\text{C}$ and 50% relative humidity if calibration was carried out with dry gases. Villanueva et al. (2012) intercompared tropospheric ozone, benzene and toluene by a commercial DOAS and conventional monitoring techniques. The instrument used to measure benzene and toluene was the same as the one used in our work. They mention the use of certified gas mixtures to calibrate their instruments. There is no mention to water vapour in the mixtures so it is assumed that they are dry gases. Their results show that average levels for

25 ozone, benzene and toluene obtained with DOAS were higher than those obtained with UV photometry for ozone and GC-PID for the aromatics. The largest differences found are for benzene. Although the water interference found in our work is compatible with the results obtained in Villanueva et al. (2012), it may not explain the whole difference between the analytical techniques used, which is up to 50% in some cases. A quantification in this paper of the bias in their measurements by GC-PID due to water vapour is not possible due to lack of temperature and relative humidity data.

30 The influence of humidity on many air quality monitoring techniques has always been a major problem. PID detectors are not the only ones affected. FID were proved to be affected as well (LeBouf et al., 2013); however, these tests were performed at ppm levels. Among the reference measurement techniques to measure air pollutants, chemiluminescence with ozone to measure NO and NO₂ is also humidity-dependent (Gerboles et al., 2003; Hayden, 2003; Miñarro and Ferradás, 2012; Steinbacher et al., 2007); and also UV photometry to measure ozone (Wilson and Birks, 2006). Recently, Bluhme et

al. (Bluhme et al., 2016) have shown that measurements of SH_2 by UV fluorescence are also affected. The interference mechanism is different in each technique but the result is always an underestimation of measurements. Some manufacturers have opted for adding filters or driers to their equipment in order to keep humidity in the sample to a minimum. These implementations have been proved to reduce biases in some cases (Bluhme et al., 2016; Steinbacher et al., 2007; Wilson and Birks, 2006). An alternative to scrubbers, which have the drawback of potentially adsorbing the target molecule, is calibration with wet gases. Ideally, calibration procedures should be done at the same ambient conditions as sampling. Calibration with wet gases may reduce measurement uncertainty due to environmental humidity in many cases. However, a thorough work regarding short and long-term stability of wet calibration gases in gas cylinders should be first tackled by metrology institutes. Using wet calibration gases obtained by dynamic dilution could bridge the gap and help reduce the uncertainty of benzene measurements and other pollutants in ambient air.

The behaviour observed in this work is likely to be shown by GC-PID instruments by other manufacturers, although to a different extent, which means that benzene concentrations –and, presumably, given the nature of the interference, ethylbenzene, toluene and xylenes concentrations as well- may be systematically underestimated. In areas where ambient concentrations of benzene are usually above the annual limit value, the humidity interference on measurements should be urgently addressed. A joint effort from manufacturers, metrology institutes and users is advisable to reduce the bias due to ambient humidity on BTEX measurements obtained by GC-PID –but also on measurements of other atmospheric pollutants-, as reliable data is the starting point for a correct environmental management.

Conclusions

In this work, the influence of sample temperature and ambient humidity on benzene measurements obtained with an automated *in situ* GC-PID is studied.

Sample temperature turned out not to influence measurements between 5 and 35 °C. Regarding humidity, the chromatograph was calibrated with dry gases, which is nowadays a current practice, and, subsequently, different amount fractions of humidity were added to the reference mixture. The absolute humidity tested ranged from 0 to 31 g/cm³. The dilution effect of adding water vapour was taken into account in the reference concentration calculation.

When measuring 5 µg/m³ of benzene in air, biases in readings ranged from 1 to 32% depending on the absolute humidity in the gas mixture. For an absolute humidity close to 8.6 g/cm³ –corresponding to a relative humidity of 50% at 20 °C- the bias in measurements is about 2.2%. Tests were repeated with a 40 µg/m³ benzene in air mixture. In this case, biases of up to 47% were obtained when the absolute humidity in the sample was 30 g/cm³. A less extreme absolute humidity in the sample (8 g/cm³) produced a bias of approximately 13%. Results show that water vapour interference depends on both the water and benzene amount fractions in the sample.

If the concentrations of benzene in a certain location are far below the annual limit value (5 µg/m³), the bias due to water interference can be acceptable, taking into consideration that benzene data quality objective in current legislation for fixed

measurements is 25%. Thus, it should be incorporated to the uncertainty budget of the measurements with no need for further corrections. Moreover, if ambient concentrations are below the annual limit value, the interference of environmental humidity although not negligible will not change the air quality situation of that area. However, if benzene ambient ratios are above, measurements will be systematically underestimated by effect of ambient humidity, precisely in those areas where a stricter control of concentrations is required. Thus, it is in these cases where humidity interference on measurements should be addressed. Using appropriate scrubbers or wet calibration gases could help reduce measurement uncertainty of benzene and many other air pollutants monitored with analytical techniques also affected by water vapour.

Acknowledgements


We would like to acknowledge the Consejería de Agua, Agricultura y Medio Ambiente of the Comunidad Autónoma de la Región de Murcia for its financial support and for the facilities to carry out this work.

References

- Adamia, T., Budovich, V., Nevjagskaya, I., Shlyakhov, A. and Jakovlev, S.: Effect of temperature on the sensitivity of the photoionization detector, *J. Chromatogr. A*, 540, 441–448, doi:10.1016/S0021-9673(01)88836-1, 1991.
- Anttila, P., Stefanovska, A., Nestorovska-Krsteska, A., Grozdanovski, L., Atanasov, I., Golubov, N., Risteovski, P., Toceva, M., Lappi, S. and Walden, J.: Characterisation of extreme air pollution episodes in an urban valley in the Balkan Peninsula, *Air Qual. Atmos. Heal.*, 9(2), 129–141, doi:10.1007/s11869-015-0326-7, 2016.
- Bahadar, H., Mostafalou, S. and Abdollahi, M.: Current understandings and perspectives on non-cancer health effects of benzene: A global concern, *Toxicol. Appl. Pharmacol.*, 276(2), 83–94, doi:10.1016/j.taap.2014.02.012, 2014.
- Barksy, J. B., Hee, S. S. Q. and Clark, C. S.: An Evaluation of the Response of Some Portable, Direct-Reading 10.2 eV and 11.8 eV Photoionization Detectors, and a Flame Ionization Gas Chromatograph for Organic Vapors in High Humidity Atmospheres, *A m. Ind. Hyg. Assoc. J.*, 46(1), 9–14, doi:10.1080/15298668591394293, 1985.
- Bluhme, A. B., Ingemar, J. L., Meusinger, C. and Johnson, M. S.: Water vapor inhibits hydrogen sulfide detection in pulsed fluorescence sulfur monitors, *Atmos. Meas. Tech.*, 9(6), 2669–2673, doi:10.5194/amt-9-2669-2016, 2016.
- Bruinen De Bruin, Y., Koistinen, K., Kephelopoulos, S., Geiss, O., Tirendi, S. and Kotzias, D.: Characterisation of urban inhalation exposures to benzene, formaldehyde and acetaldehyde in the European Union: Comparison of measured and modelled exposure data, *Environ. Sci. Pollut. Res.*, 15(5), 417–430, doi:10.1007/s11356-008-0013-4, 2008.
- Bruno, P., Caselli, M., De Gennaro, G. and Traini, A.: Source apportionment of gaseous atmospheric pollutants by means of an absolute principal component scores (APCS) receptor model, *Anal. Bioanal. Chem.*, 371(8), 1119–1123, doi:10.1007/s002160101084, 2001.
- Coy, J. D., Bigelow, P. L., Buchan, R. M., Tessari, J. D. and Parnell, J. O.: Field Evaluation of a Portable Photoionization


- Detector for Assessing Exposure to Solvent Mixtures, *AHHAJ—Am. Ind. Hyg. Assoc. J.*, 61(2), 268–274, doi:10.1080/15298660008984536, 2000.
- D’Andrea, M. A. and Reddy, G. K.: Adverse Health Effects of Benzene Exposure Among Children Following a Flaring Incident at the British Petroleum Refinery in Texas City, *Clin. Pediatr. (Phila.)*, 55(3), 219–227, doi:10.1177/0009922815594358, 2016a.
- D’Andrea, M. A. and Reddy, G. K.: Detrimental Health Effects of Benzene Exposure in Adults After a Flaring Disaster at the BP Refinery Plant in Texas City, *Disaster Med. Public Health Prep.*, 10(2), 233–239, doi:10.1017/dmp.2015.160, 2016b.
- Eberhardt, M. K.: Reaction of benzene radical cation with water. Evidence for the reversibility of hydroxyl radical addition to benzene, *J. Am. Chem. Soc.*, 103(13), 3876–3878, doi:10.1021/ja00403a042, 1981.
- 10 EN: [14662](#) Ambient air. Standard method for the measurement of benzene concentrations. Automated pumped sampling with in situ gas chromatography, 2015.
- EU: Directive 2008/50/EC of the European Parliament and of the Council of 21 May 2008 on ambient air quality and cleaner air for Europe, *Off. J. Eur. Communities*, 52, 1–43, <http://eur-lex.europa.eu/LexUriServ/LexUriServ.do?uri=OJ:L:2008:152:0001:0044:EN:PDF>, 2008. ~~(Last accessed: 12 september~~
- 15 ~~09/2017)~~
- Gerboles, M., Lagler, F., Rembges, D. and Brun, C.: Assessment of uncertainty of NO₂ measurements by the chemiluminescence method and discussion of the quality objective of the NO₂ European Directive, *J. Environ. Monit.*, 5(4), 529, doi:10.1039/b302358c, 2003.
- Gist, G. L. and Burg, J. R.: Benzene—a Review of the Literature from a Health Effects Perspective, *Toxicol. Ind. Health*, 20 13(6), 661–714, doi:10.1177/074823379701300601, 1997.
- Haley, T. J.: Evaluation of the health effects of benzene inhalation, *Clin. Toxicol.*, 11(5), 531, doi:10.3109/15563657708988218, 1977.
- Hayden, K. L.: Partitioning of reactive atmospheric nitrogen oxides at an elevated site in southern Quebec, Canada, *J. Geophys. Res.*, 108(D19), 4603, doi:10.1029/2002JD003188, 2003.
- 25 Kelessis, A. G., Petrakakis, M. J. and Zoumakis, N. M.: Determination of benzene, toluene, ethylbenzene, and xylenes in urban air of Thessaloniki, Greece, *Environ. Toxicol.*, 21(4), 440–443, doi:10.1002/tox.20197, 2006.
- LeBouf, R. F., Slaven, J. E. and Coffey, C. C.: Effect of calibration environment on the performance of direct-reading organic vapor monitors, *J. Air Waste Manage. Assoc.*, 63(5), 528–533, doi:10.1080/10962247.2013.772926, 2013.
- Liaud, C., Nguyen, N. T., Nasreddine, R. and Le Calvé, S.: Experimental performances study of a transportable GC-PID and two thermo-desorption based methods coupled to FID and MS detection to assess BTEX exposure at sub-ppb level in air, 30 *Talanta*, 127, 33–42, doi:10.1016/j.talanta.2014.04.001, 2014.
- Licen, S., Tolloi, A., Briguglio, S., Piazzalunga, A., Adami, G. and Barbieri, P.: Small scale spatial gradients of outdoor and indoor benzene in proximity of an integrated steel plant, *Sci. Total Environ.*, 553, 524–531, doi:10.1016/j.scitotenv.2016.02.071, 2016.

- Al Madhoun, W. A., Ramli, N. A., Yahaya, A. S., Yusuf, N. F. F. M., Ghazali, N. A. and Sansuddin, N.: Levels of benzene concentrations emitted from motor vehicles in various sites in Nibong Tebal, Malaysia, *Air Qual. Atmos. Heal.*, 4(2), 103–109, doi:10.1007/s11869-010-0083-6, 2011.
- MSA. Photoionization detectors. Technology for detection of Volatile Organic Compounds, 2005.
- 5 <http://media.msanet.com/NA/USA/PermanentInstruments/GasSensorsTransmitters/SaveToxSafeVOC/07-2092WhitePaperPID.pdf> (last accessed: 24 June 2017)
- Miñarro, M. D. and Ferradás, E. G.: Performance evaluation of two commercial chemiluminescence NO_x analysers according to European Standard EN 14211., *J. Environ. Monit.*, 14(2), 383–90, doi:10.1039/c1em10601e, 2012.
- Mouradian, R. F. and Flannery, J. P.: Effect of Oxygen Content on Calibration of Portable VOC Instruments, *Am. Ind. Hyg. Assoc. J.*, 55(11), 1084–1086, doi:10.1080/15428119491018385, 1994.
- 10 Peng, F., Luoa, T., Yuan, Y. and Qiu, L.: Performance of optimized TVOCs sensor, *Procedia Eng.*, 7, 392–398, doi:10.1016/j.proeng.2010.11.064, 2010.
- von Schneidemesser, E., Monks, P. S. and Plass-Duelmer, C.: Global comparison of VOC and CO observations in urban areas, *Atmos. Environ.*, 44(39), 5053–5064, doi:10.1016/j.atmosenv.2010.09.010, 2010.
- 15 Smith, M. T.: Advances in Understanding Benzene Health Effects and Susceptibility, *Annu. Rev. Public Health*, 31(1), 133–148, doi:10.1146/annurev.publhealth.012809.103646, 2010.
- Steinbacher, M., Zellweger, C., Schwarzenbach, B., Bugmann, S., Buchmann, B., Ordóñez, C., Prevot, A. S. H. and Hueglin, C.: Nitrogen oxide measurements at rural sites in Switzerland: Bias of conventional measurement techniques, *J. Geophys. Res. Atmos.*, 112(11), 1–13, doi:10.1029/2006JD007971, 2007.
- 20 Romero-Trigueros, C. R., Miñarro, M. D., Duperón, E. G., Marzal, F. J. and Ferradás, E. G.: Study of the effect of sample pressure on in situ BTEX chromatographs, *Environ. Monit. Assess.*, doi:10.1007/s10661-016-5674-8, 2016.
- Villanueva, F., Notario, A., Mabilia, R., Albaladejo, J., Cabanas, B. and Martínez, E.: Intercomparison of tropospheric O₃, benzene and toluene measured by a commercial doas system and conventional monitoring techniques, *Fresenius Environ. Bull.*, 21(12 B), 4040–4050, 2012.
- 25 Wilson, K. L. and Birks, J. W.: Mechanism and elimination of a water vapor interference in the measurement of ozone by UV absorbance, *Environ. Sci. Technol.*, 40(20), 6361–6367, doi:10.1021/es052590c, 2006.

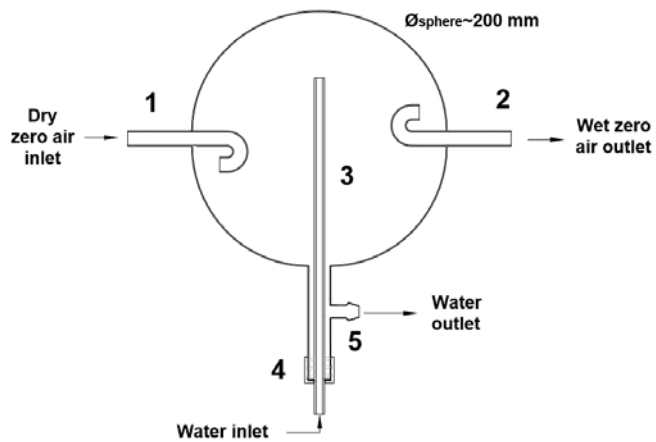

a)

5

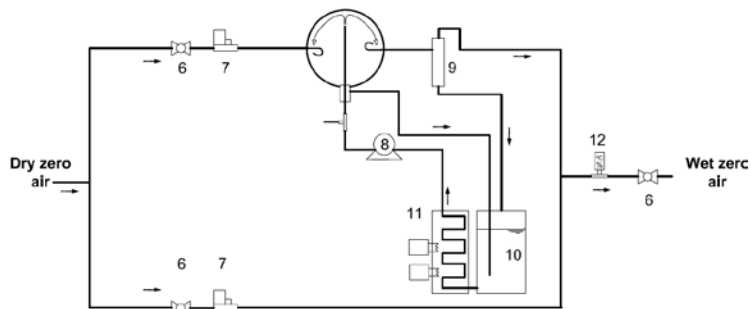

b)

10 Figure 1: Schematic of the (a) humidifier and (b) the elements that comprise the humidifying system used in this work. 1: dry zero air inlet, 2: wet zero air outlet, 3 and 4: water inlet, 5: water outlet, 6: shut-off valves, 7: mass flow controllers, 8: water pump, 9: cyclone, 10: water container, 11: thermostatic bath, 12: thermo-hygrometer.

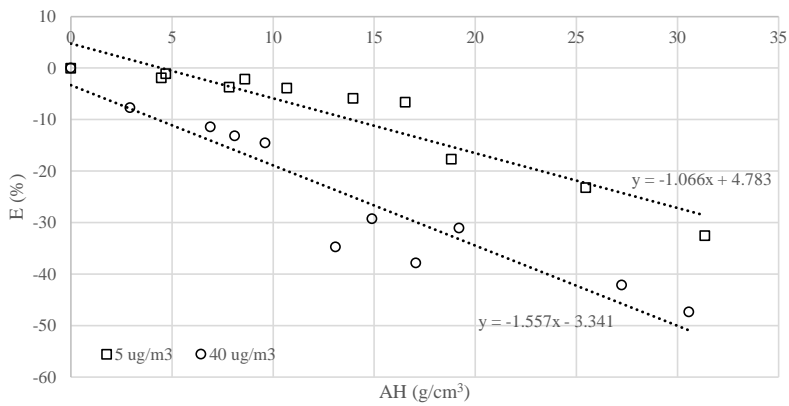
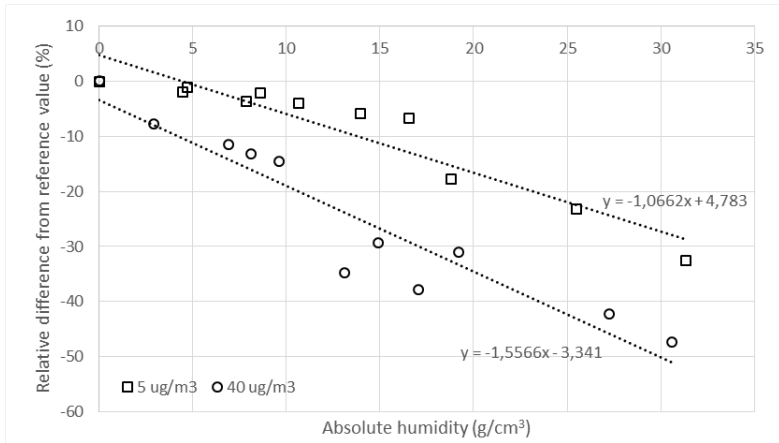


Figure 2: Relative differences in readings from the reference value of concentration as a function of the absolute humidity of the sample.

Temperature cycle	20 °C	5 °C	20 °C
Average reading of concentration ($\mu\text{g}/\text{m}^3$) when measuring a benzene concentration of $39.96 \pm 0.30 \mu\text{g}/\text{m}^3$	39.96 (0.45)	39.69 (0.26)	39.82 (0.29)
Average reading of concentration ($\mu\text{g}/\text{m}^3$) when measuring a benzene concentration of $4.77 \pm 0.08 \mu\text{g}/\text{m}^3$	4.77 (0.08)	4.76 (0.06)	4.78 (0.06)
Temperature cycle	20 °C	35 °C	20 °C
Average reading of concentration ($\mu\text{g}/\text{m}^3$) when measuring a benzene concentration of $39.96 \pm 0.30 \mu\text{g}/\text{m}^3$	39.82 (0.29)	39.78 (0.50)	39.87 (0.25)
Average reading of concentration ($\mu\text{g}/\text{m}^3$) when measuring a benzene concentration of $4.77 \pm 0.08 \mu\text{g}/\text{m}^3$	4.78 (0.06)	4.77 (0.10)	4.78 (0.11)

5 Table 1: Analyser I readings when subjected to changes in sample temperature. In brackets, the standard deviation of the measurements.

Test nominal concentration: 0.5 µg/m ³	Average value	
	Analyser I (µg/m ³)	Analyser II (µg/m ³)
20% relative humidity	0.53 (0.01)	0.55 (0.01)
80% relative humidity	0.51 (0.01)	0.53 (0.01)
<i>b_{rh}</i> (%)	3.1	3.9

Test nominal concentration: 40 µg/m ³		
20% relative humidity	44.3 (0.17)	46.7 (0.47)
80% relative humidity	36.9 (0.23)	37.9 (0.18)
<i>b_{rh}</i> (%)	18.2	20.8

Test nominal concentration: 5 µg/m ³		
<u>0% relative humidity</u>	<u>5.31 (0.06)</u>	
<u>80% relative humidity</u>	<u>4.99 (0.07)</u>	
<u><i>b_{rh, new}</i> (µg/m³/(mmol/mol))</u>	<u>0.0175</u>	

Con formato: Sin Superíndice / Subíndice

Con formato: Sin Superíndice / Subíndice

Tabla con formato

Con formato: Fuente: Negrita, Sin Cursiva

Con formato: Fuente: Negrita, Sin Cursiva

Con formato: Fuente: Sin Negrita

Con formato: Fuente: Sin Negrita

Con formato: Fuente: Sin Negrita

5 Table 2: Analyser readings when subjected to changes in ambient humidity for a constant reference concentration and sensitivity coefficients to humidity (*b_{rh}*) and *b_{rh, new}*. Test temperature: 20 ± 2 °C. In brackets, the standard deviation of the measurements.

Con formato: Fuente: Cursiva

10

15

$T = 20 \pm 2 \text{ }^\circ\text{C}$; $C_{std} = 1053.5 \pm 26.3 \text{ } \mu\text{g}/\text{m}^3$; $q_z = 11.636 \pm 0.002 \text{ l}/\text{min}$; $q_{std} = 0.05999 \pm 6.265 \cdot 10^{-5} \text{ l}/\text{min}$

RH (%)	AH (g/cm ³)	W (g H ₂ O/g dry air)	q _{H2O} (l/min)	q _t (l/min)	C _{ref} (μg/m ³)	C _{meas} (μg/m ³)	EDiff (%)
0.4	0.0689	5.74·10 ⁻⁵	1.069·10 ⁻³	11.697	5.40	5.40	0.00
26	4.480	0.00373	0.0695	11.765	5.37	5.27	-1.95
50	8.616	0.00718	0.134	11.830	5.34	5.23	-2.20
62	10.68	0.00890	0.166	11.862	5.33	5.12	-3.95
81	13.96	0.0116	0.217	11.913	5.31	4.99	-5.94
96	16.54	0.0138	0.257	11.953	5.29	4.93	-6.70

Con formato: Subíndice

$T = 35 \pm 2 \text{ }^\circ\text{C}$; $C_{std} = 1053.5 \pm 26.3 \text{ } \mu\text{g}/\text{m}^3$; $q_z = 11.637 \pm 0.002 \text{ l}/\text{min}$; $q_{std} = 0.05999 \pm 6.265 \cdot 10^{-5} \text{ l}/\text{min}$

RH (%)	AH (g/cm ³)	W (g H ₂ O/g dry air)	q _{H2O} (l/min)	q _t (l/min)	C _{ref} (μg/m ³)	C _{meas} (μg/m ³)	EDiff (%)
0.2	0.0345	2.871·10 ⁻⁵	5.347·10 ⁻⁴	11.697	5.40	5.40	0.00
12	4.70	0.00392	0.0730	11.769	5.37	5.31	-1.12
20	7.84	0.00653	0.122	11.818	5.35	5.15	-3.75
48	18.82	0.0157	0.292	11.988	5.27	4.34	-17.8
65	25.48	0.0212	0.395	12.091	5.23	4.01	-23.3
80	31.36	0.0261	0.487	12.183	5.19	3.50	-32.6

Con formato: Subíndice

$T = 25 \pm 2 \text{ }^\circ\text{C}$; $C_{std} = 1053.5 \pm 26.3 \text{ } \mu\text{g}/\text{m}^3$; $q_z = 9.099 \pm 0.002 \text{ l}/\text{min}$; $q_{std} = 0.3599 \pm 4.125 \cdot 10^{-4} \text{ l}/\text{min}$

RH (%)	AH (g/cm ³)	W (g H ₂ O/g dry air)	q _{H2O} (l/min)	q _t (l/min)	C _{ref} (μg/m ³)	C _{meas} (μg/m ³)	EDiff (%)
1.1	0.190	1.579·10 ⁻⁴	2.299·10 ⁻³	9.461	40.07	40.08	0.02
17	2.929	0.00244	0.0355	9.494	39.93	36.85	-7.72
40	6.893	0.00574	0.0836	9.543	39.73	35.18	-11.46
47	8.099	0.00675	0.0983	9.557	39.67	34.43	-13.21
76	13.10	0.0109	0.1589	9.618	39.42	25.70	-34.80
99	17.06	0.0142	0.207	9.666	39.23	24.37	-37.87

Con formato: Subíndice

$T = 35 \pm 2 \text{ }^\circ\text{C}$; $C_{std} = 1053.5 \pm 26.3 \text{ } \mu\text{g}/\text{m}^3$; $q_z = 9.098 \pm 0.002 \text{ l}/\text{min}$; $q_{std} = 0.3599 \pm 4.125 \cdot 10^{-4} \text{ l}/\text{min}$

RH (%)	AH (g/cm ³)	W (g H ₂ O/g dry air)	q _{H2O} (l/min)	q _t (l/min)	C _{ref} (μg/m ³)	C _{meas} (μg/m ³)	EDiff (%)
--------	-------------------------	----------------------------------	--------------------------	------------------------	---------------------------------------	----------------------------------------	-----------

Con formato: Subíndice

1.8	0.706	$5.88 \cdot 10^{-3}$	$8.56 \cdot 10^{-3}$	9.466	40.05	40.09	0.10
25	9.604	0.0080	0.117	9.574	39.60	33.83	-14.56
38	14.90	0.0125	0.182	9.640	39.33	27.82	-29.28
49	19.21	0.0161	0.235	9.693	39.12	26.95	-31.10
70	27.24	0.0229	0.333	9.791	38.72	22.38	-42.20
78	30.57	0.0257	0.374	9.832	38.56	20.28	-47.41

5 Table 3: Relative (RH) and absolute (AH) humidity, mass fraction of water vapour in the dry air (W), reference concentration of benzene (C_{ref}), average reading of analyser I (C_{meas}) and relative difference between measurements and reference values (E). q_t is the total flow rate, calculated as the sum of the flowrate of zero air (q_z), water vapour (q_{H2O}) and the flow rate from the benzene reference gas mixture (q_{std}). C_{std} is the amount fraction of benzene in the gas cylinder.