



A sampler for atmospheric volatile organic compounds by copter unmanned aerial vehicles

Karena A. McKinney^{1,2*}, Daniel Wang², Jianhuai Ye², Jean-Baptiste de Fouchier², Patricia C. Guimarães^{3,4}, Carla E. Batista^{3,4}, Rodrigo A. F. Souza^{3,4}, Eliane G. Alves^{3,5}, Dasa Gu⁶, Alex B. Guenther⁶, Scot T. Martin^{2,7*}

¹Department of Chemistry, Colby College, Waterville, Maine, 04901, USA

²School of Engineering and Applied Sciences, Harvard University, Cambridge, Massachusetts, 02138, USA

³Post-graduate Program in Climate and Environment, National Institute of Amazonia Research and Amazonas State University, Manaus, Amazonas, 69060-001, Brazil

⁴School of Technology, Amazonas State University, 69065-020, Manaus, Amazonas, Brazil

⁵Department of Biogeochemical Processes, Max Planck Institute for Biogeochemistry, Jena, Germany

⁶Department of Earth System Science, University of California, Irvine, California, 92697, USA

⁷Department of Earth and Planetary Sciences, Harvard University, Cambridge, Massachusetts, 02138, USA

Correspondence to: Karena A. McKinney (kamckinn@colby.edu) and Scot T. Martin (scot_martin@harvard.edu)

Submitted to *Atmospheric Measurement Techniques*



1 **Abstract.** A sampler for volatile organic compounds (VOCs) was developed for deployment on
2 a copter-technology unmanned aerial vehicle (UAV). The sampler was designed to collect VOCs
3 on up to five commercially available VOC-adsorbent cartridges for subsequent offline analysis
4 by thermal-desorption gas chromatography. The sampler had a mass of 0.90 kg and dimensions
5 of 19 cm × 20 cm × 5 cm. Power consumption was <3 Wh in a typical 30 min flight,
6 representing <3% of the total UAV battery capacity. Autonomous sampler operation and data
7 collection in flight were accomplished with a microcontroller. Sampling flows of 100 to 400
8 sccm were possible, and a typical flow of 150 sccm was used to balance VOC capture efficiency
9 with sample volume. The overall minimum detection limit for the sampling volumes and the
10 analytical method was close to 2 ppt for isoprene and monoterpenes. The sampler was mounted
11 to a commercially available UAV and flown in August 2017 over tropical forest in central
12 Amazonia. Samples were collected sequentially for 10 min each at several different altitude-
13 latitude-longitude collection points. The species identified, their concentrations, and their
14 uncertainties are presented and discussed in the context of the sampler design and capabilities.
15 Finally, design challenges and possibilities for next-generation samplers are addressed.



16 **1. Introduction**

17 Biogenic volatile organic compound (VOC) emissions from forests vary widely across
18 plant species, ecosystem type, season, time of day, and environmental conditions at many scales,
19 including from 10's to 100's of m (Gu et al., 2017;Fuentes et al., 2000;Goldstein and Galbally,
20 2007;Alves et al., 2018;Greenberg et al., 2004;Guenther et al., 2006;Klinger et al., 1998;Kuhn et
21 al., 2004;Pugh et al., 2011;Wang et al., 2011). These variations can have significant effects on
22 and be affected by atmospheric chemistry, air quality, and climate (Chameides et al.,
23 1988;Fuentes et al., 2000;Laothawornkitkul et al., 2009;Goldstein et al., 2009;Kesselmeier et al.,
24 2013;Peñuelas and Staudt, 2010). They may also be indicators of ecosystem change, plant health,
25 and stress (Karl et al., 2008;Kravitz et al., 2016;Niinemets, 2010;Peñuelas and Llusia, 2003).
26 Most field observations of biogenic VOC emissions are made from fixed-location towers and
27 tethered balloons or from aircraft flying at high velocities well above the forest canopy (see
28 Table 1 of Alves et al., (2016) for a summary of studies in the Amazon). As such, detailed
29 information on the spatial distribution of emissions at 10's to 100's of meters has been difficult
30 to obtain. Thus, this scale is not represented in current VOC data sets, yet it reflects the primary
31 scale for VOC emission and uptake and is precisely the missing link in advancing our present-
32 day understanding of VOCs in atmospheric chemistry. This information is even more scarce in
33 remote areas, such as the Amazon rainforest, that are very important sources of VOCs to the
34 global atmosphere. In addition, knowledge of VOC concentrations as a function of height
35 throughout the boundary layer is needed to better constrain emissions, chemical reactions, and
36 atmospheric mixing of these compounds. New approaches that are suited to spatially resolved
37 sampling at these intermediate scales is therefore needed by the atmospheric chemistry
38 community.



39 Small, commercially available unmanned aerial vehicles (UAVs, commonly called
40 drones) have the potential to fill this gap in knowledge due to their extreme maneuverability
41 (Villa et al., 2016). UAVs are available as either fixed wing aircraft, helicopters, or multicopters.
42 Multicopters (most often quad- or hexacopters) offer the advantages of being highly
43 maneuverable and easy to fly, as well as offering straightforward accessory mounting options.
44 Flight durations of up to 45 min and payload capacities of 6 kg are attainable with mid-priced,
45 commercially available copter-type UAVs. Development or adaptation of air sensors for UAV
46 platforms is, however, still in the early stages. To date, several researchers have utilized UAVs to
47 carry sensors to measure atmospheric trace gases *in situ* (Villa et al., (2016) and references
48 therein.) Commercially available sensors for some trace gases (e.g., CO₂, CO, and NO_x) are
49 sufficiently compact to be carried by a UAV, but these are often limited by insufficient
50 sensitivity or difficult calibration (Cross et al., 2017). *In situ* techniques for quantifying VOCs at
51 the required sensitivity (< 10 ppt) are, however, large and complex instruments that exceed the
52 payload capacity of mid-range UAVs available to most researchers (Lindinger et al., 1998; Millet
53 et al., 2005; Blake et al., 2009; Kim et al., 2013).

54 As an alternative, the UAV platform offers the possibility to collect air samples for later
55 laboratory analysis. Black et al. (2018) used a commercial quadcopter to collect samples of
56 airborne mercury by drawing air through gold-coated quartz cartridges for later analysis by cold
57 vapor atomic fluorescence spectroscopy. The results showed the ability to resolve vertical
58 concentration profiles above a source and to differentiate between urban and rural mercury
59 concentrations. Although remote control of the sampler was not implemented, the authors
60 suggested this as a possible future improvement. Chang et al. (2016) demonstrated the use of a
61 whole air sampling apparatus mounted on a multicopter UAV platform to collect air samples for



62 off-line analysis. The sampler consisted of a single evacuated 2-L canister with a remote-
63 controlled valve actuated by a separate remote control unit independent of the UAV controller.
64 The flow rate and total sample volume was not monitored during flight. The authors successfully
65 detected VOCs, CO, CO₂, and CH₄ in the collected air samples and were able to distinguish
66 between samples collected upwind and downwind of an exhaust shaft. Both studies cite
67 maneuverability in three dimensions, spatial resolution, and the ability to evaluate emissions
68 from otherwise inaccessible locations as key advantages of UAV-based atmospheric sampling.
69 They also point out flight stability, an easily accessed and symmetrically positioned mounting
70 location, low cost, and lack of engine exhaust as features of battery-powered multicopters that
71 make them particularly well suited for environmental applications. While the ability to detect
72 atmospheric trace species and to map spatial gradients depends strongly upon the target species,
73 including its atmospheric variability and the detection threshold of the analytical method, these
74 several studies suggest that UAV-based sample collection is a viable approach that promises to
75 greatly expand access to previously inaccessible locations and to provide a means to map spatial
76 patterns in atmospheric trace species concentrations.

77 The use of VOC-adsorbent cartridges to capture VOCs from air with subsequent analysis
78 by thermal-desorption gas-chromatography mass spectrometry (TD-GC-MS) is well established
79 (Woolfenden, 2010a; Pankow et al., 2012). The adsorbent cartridges are small glass or metal
80 tubes, typically 9 cm in length and 0.64 cm in diameter. The cartridges are filled with a sorbent
81 material with a high affinity for VOCs. The cartridges provide a lightweight (10 g), simple,
82 sensitive, and quantitative approach for determining a wide range of VOCs at ambient
83 atmospheric levels. The challenge is to design and construct an automated sample collection
84 system for cartridges suited to deployment on a multicopter UAV.



85 The primary scientific requirement of the sampler is that the total mass of analyte
86 collected be greater than the detection limit of the analytical system for that compound. In the
87 case of a volatile organic compounds detected by GC-MS, the detection limit has typically been
88 ca. 10 pg. For a sample volume of a few liters of air, which can be collected in 5 to 15 min by
89 typical flow rates through adsorbent cartridges, this corresponds to a VOC detection limit of less
90 than 10 pptv (Pankow et al., 2012). Commercial detectors are now available with detection limits
91 of < 1 pg, including the GC-ToF-MS used for this study (Hoker et al., 2015), implying an order
92 of magnitude lower detectable VOC mixing ratios. This suggests that detection of VOCs in
93 cartridge samples collected within current multicopter flight durations is feasible. Automated
94 operation of the sampler, controlled either algorithmically based on elapsed time or position, or
95 remotely by sending commands to the sampler during flight, is desirable. Furthermore, the mass
96 and dimensions of the sampler must fit within the payload capacity of available UAV platforms.
97 Herein, the design, operation, and field validation of a VOC sampler using adsorption/thermal
98 desorption cartridges on a mid-size copter-technology UAV that meets these requirements is
99 described, and an example data set collected in central Amazonia including a discussion of
100 uncertainties is presented.

101 **2. Experimental**

102 **2.1. Flight platform**

103 The UAV platform was a DJI Matrice 600 Professional Grade (Figure 1), which is a
104 hexacopter design with onboard stabilization. With propeller arms extended, the UAV measured
105 1.668 m across by 0.759 m high. Without the sampler attached, it weighed 9.6 kg with its six
106 batteries installed (model TB48S; 130 Wh, 18 V). The maximum ascent rate was 5 m s⁻¹, and the
107 maximum horizontal speed was 18 m s⁻¹. It had GPS positioning and maintained two-way



108 communication with DJI programs developed for iPad and Android tablet systems. The
109 positioning accuracy was ± 0.5 m in the vertical and ± 1.5 m in the horizontal. The maximum
110 flight time specified by the manufacturer was 40 min without a payload and 18 min for the
111 maximum payload mass of 5.5 kg at sea level. The VOC sampler was mounted to a mounting
112 frame underneath the UAV platform (DJI Matrice 600 Series Z15 Gimbal Mounting Connector
113 kit). Testing for the sampler load of this study indicated 25 min of flight time with a margin of
114 security of an additional 5 min. Actual battery use in each flight depended on the flight plan and
115 strength of local winds during the flight. The UAV was tested to a horizontal flight distance of
116 1000 m and a height of 150 m. A ceiling of 500 m above local ground level is hard-wired into
117 the device by the manufacturer.

118 **2.2. Sampler description**

119 Figure 2 shows the full system schematic, including the pump system flow paths and the
120 major power and signal connections within the sampler casing. The sampler requires a pump to
121 draw air flow through the sorbent cartridge, flow and pressure sensors, a flow regulation valve,
122 and a cartridge selection manifold to allow for multiple samples, as well as electronics to provide
123 power, issue commands, and collect data from the sensors during flight. The overall system
124 layout of the sampler is designed to fit a standalone, modular form factor in order to simplify
125 installation and troubleshooting as well as to maximize electromechanical compatibility with
126 multiple UAV platforms in the field. A table with a complete list of the sampler components is
127 provided in the Supplement.

128 *Casing.* The sampling system resides in a rectangular acrylic casing that can be opened
129 for easy access for repairs and software updates to the onboard microcontroller. The completed
130 sampler measures 19 cm \times 20 cm \times 5 cm. The casing remains closed and attached to the chassis



131 of the UAV platform for exchanging sorbent cartridges between flights. The sampler casing is
132 directly integrated to the underside of the UAV chassis and does not interfere with standard
133 flight operations, including the functionality of the Matrice 600's automatically retracting
134 landing legs. The total sampler mass is 0.90 kg. The flight time decreases approximately linearly
135 with increasing payload mass below 5 kg. Based on the relationship between payload mass and
136 flight time provided by the UAV manufacturer, the decrease in flight time for a 1-kg payload is
137 estimated as 3.4 min (DJI.com).

138 *Flow system.* The cartridge sampling requires a sample stream at a calibrated flow rate in
139 order to determine the volume captured over the sampling period. The sample flow is drawn
140 through the system by a Parker CTS Micro Diaphragm pump, which can pull between 100 and
141 600 sccm of flow in a compact form factor. The volumetric flow of the pump is a function of the
142 pressure drop across the inlet and outlet, and is controlled via an adjustable pinch valve (Model
143 44560; US Plastic Corp.) at the output of the flow system. The pump is driven by a 5.0 VDC
144 brush-sleeve bearing motor. A mass flow sensor (Model D6F-P; Omron) was installed upstream
145 of the pump to provide a continuous analog output signal corresponding to the mass flow at
146 standard temperature and pressure. The flow sensor supports a flow range of 0 to 1000 sccm and
147 includes a built-in cyclone dust segregation system, which diverts particulates from the sensor
148 element. The mass flow sensor was calibrated periodically against a reference standard in the lab.
149 The mass flow rate is converted into a volumetric flow rate using the measured pressure at the
150 flow sensor and atmospheric temperature. The sample volume is obtained by integrating the
151 volumetric flow rate over time. The flow sensor also serves as an indicator of sampler
152 malfunction due to factors such as valve failure or obstruction of the flow by debris during flight.



153 *Pressure system.* An absolute pressure transducer (MX4100AP; NXP) is positioned
154 adjacent to the flow sensor in order to measure the pressure in the flow path. The measured
155 pressure is also used with atmospheric temperature to convert mass flow rate to volumetric flow
156 rate as UAV altitude changes. The device operates across a pressure range of 20 to 10^5 kPa. It
157 outputs an analog voltage signal recorded by the microcontroller that can be converted to a
158 pressure value.

159 *Manifold.* Activation of each sample cartridge is achieved with a solenoid valve manifold
160 (Model 161T102; NResearch Inc.) consisting of five independently actuated two-way, normally-
161 closed solenoid valves. All five valves have a nominal orifice of 1.0 mm and share a common
162 output port. The manifold is controlled by a valve driver board (CoolDrive Model 161D5X24;
163 NResearch Inc.). Valve actuation requires 200 mA at 24 V. The board uses a holding voltage that
164 is one third of the actuation voltage and is automatically achieved within 100 ms of activating the
165 solenoid. The five solenoid valves are independently controlled using 5 V logic level signals.

166 *Control system.* Autonomous sampler operation and data collection in flight is accomplished
167 with an Arduino Uno microcontroller. The microcontroller coordinates the activation and
168 operation of the pump and valves using a pre-programmed algorithm based on elapsed flight
169 time and collects data from the sensors.

170 *Electrical system.* The sampling system is powered by the 18 VDC output provided by
171 the UAV batteries via the power distribution board onboard the Matrice 600. Voltage regulators
172 provide 5 VDC output for the pump, sensors, and Arduino Uno driver boards, as well as 24 VDC
173 output for the valve manifold. The system consumes 2.5 Wh of electricity during a 30-min flight
174 (25 min of sample time), which is less than 2% of the total UAV battery capacity. The remaining
175 98% of battery capacity is available for UAV flight operations. The use of a separate onboard



176 battery to power the sampler was considered; however, the extra power capacity was more than
177 offset by the effect of the weight of an additional battery on total available flight time.

178 **2.3. Sampling methods**

179 Air samples are collected using cartridge tubes packed with Tenax TA and Carbograph 5TD
180 (Markes International, Inc. C2 -AXXX-5149). Tenax TA is a relatively weak sorbent that
181 collects components with volatility less than benzene (e.g., monoterpenes and sesquiterpenes),
182 whereas Carbograph 5TD shows strong sorbate affinity and captures low-molecular-weight
183 VOCs with carbon number of C₃ to C₈ (Woolfenden, 2010a). The combination of these sorbent
184 materials enables sampling of VOCs with carbon number from C₃ to C₃₀. Both of the sorbent
185 materials are hydrophobic and suitable for air sampling at high RH conditions. Prior to sampling,
186 tubes are preconditioned at 320 °C for 2 h, then at 4 h at 330 °C for 4 h, and are then capped
187 using 0.25-inch (6.35-mm) Swagelok fittings with PTFE ferrules and kept sealed until they are
188 installed on the sampler just prior to flight.

189 The sorbent cartridges are mounted at the sampler inlet to ensure that the sample gas that
190 passes through the cartridges has not contacted other surfaces in the flow system, thus preventing
191 potential analyte losses or contamination from the flow system tubing. The cartridges are
192 oriented in a vertical position for sampling since horizontal installation can cause “channeling”
193 to occur as a result of sorbent falling away from the walls of the cartridge (ASTM International,
194 2015). No particle or ozone filter was used upstream of the cartridges to prevent loss of analytes
195 on the filter surfaces.

196 A constant low volumetric flow rate is required to allow for optimal sorbent-sorbate
197 interaction and uptake onto the sorbent matrix. A target flow rate of 150 sccm was defined to
198 maximize both VOC capture efficiency and sample volume (Woolfenden, 2010b;Markes



199 International Ltd., 2014). Based on the relationship between sample volume and minimum
200 detection limit reported by past studies (Pankow et al., 2012), a minimum sampling volume of
201 1.5 L per adsorbent cartridge collected is targeted. This results in 10 min of sampling time per
202 cartridge. Two to three cartridge samples of this volume can be collected in a single flight while
203 also carrying out take-off/landing and transits between sampling locations. The Arduino Uno
204 microcontroller provides the operational flexibility to obtain smaller or larger sample volumes by
205 utilizing either more tubes and shorter collection times or fewer tubes and longer collection
206 times, respectively, during a single flight.

207 Alongside the sampling, blanks are collected to examine sampling artifacts such as
208 passive diffusion of VOCs into the tube. For the blanks, a sorption cartridge is installed on the
209 UAV and uncapped, but the sampling valve is not opened during flight. After sample collection,
210 the sample tubes and blanks are capped using the Swagelok fittings with PTFE ferrules, and
211 stored at room temperature. The collected tubes are transported from Brazil to USA for
212 chromatographic analysis. Tubes were analyzed within 1 week after collection. Under proper
213 transport and storage, sample artifacts were minimal and did not influence the results (Pollmann
214 et al., 2005).

215 **2.4. Analysis by thermal desorption gas chromatography mass spectrometry (TD-GC-MS)**

216 The cartridge tubes are mounted into a thermally desorbing autosampler (TD-100,
217 Markes International, Inc). The VOCs are pre-concentrated at 10 °C followed by injection into a
218 gas chromatograph (GC, model 7890B, Agilent Technologies, Inc) equipped with time-of-flight
219 mass spectrometer (Markes BenchTOF-SeV) and flame ionization detector (TD-GC-
220 FID/TOFMS) (Woolfenden and McClenny, 1999; ASTM International, 2015). Internal standards
221 tetramethylethylene and decahydronaphtalene are injected into each sample prior to analysis. The



222 system is calibrated daily with a commercial standard from Apel-Riemer Environmental Inc. (c.f.
223 Supplement). The external gas standard is prepared using a dynamic dilution system and the
224 effluent is added to sorbent cartridges under conditions similar to those used for sampling. The
225 calibration cartridges are then analyzed using the same thermal desorption GC analysis method.
226 Response factors for additional VOCs are determined using liquid standards injected on the
227 cartridges or using FID signals by effective carbon number (Faiola et al., 2012).
228 The mixing ratio X_{VOC} of VOCs is calculated from the measured mass of each compound in the
229 sample and the volumetric flow rate according to the following governing equation:

$$230 \quad X_{\text{VOC}} = \text{moles VOC} / \text{moles air} = (m_{\text{VOC}} R T) / (M_{\text{VOC}} P Q \tau) \quad (\text{Eq. 1})$$

231 where m_{VOC} is the mass of the VOC measured in the sample, M_{VOC} is the molar mass, R is the
232 gas constant, T is the temperature, P is the pressure, Q is the volumetric flow rate, and τ is the
233 sampling time.

234 The detection limit of the GC-TOFMS analysis for isoprene is 1 pg, which is 0.25 ppt for
235 a 1.5-L sample. The detection limit of the measurement is, however, limited by the uncertainty in
236 the background (blank), which is typically ca. 10 pg, equivalent to 2.5 ppt or 5%, whichever is
237 greater, for a 1.5-L sample, and by the uncertainty in the in-flight flow rate measurement, which
238 is 15%. Combining these factors, the overall uncertainty in the measured mixing ratio is then the
239 greater of 3 ppt or 20%.

240 **2.5. Computational fluid dynamics (CFD) simulation**

241 CFD simulations are carried out using SOLIDWORKS Flow Simulation (Ver. 2017
242 SP3.0) (Waltham, USA). Dimensions and an input geometric model of the UAV are obtained
243 from the DJI company (DJI Downloads). A box with the dimensions and location of the sampler
244 is added to the geometry file. The propellers are simulated by discs of the same diameter, and to



245 simulate a hovering UAV a downward velocity of 11 m s^{-1} is imposed through each disc so that
246 the lift produced by the motors balanced the system weight. Boundary conditions include
247 atmospheric pressure far from the UAV. The pressure is used for a basis of simulation and
248 comparison, and it may not represent the actual value during the sampling. The results are
249 optimized by performing iterations until the pressure difference between the last two iterations
250 was within 2 Pa.

251 **3. Results and discussion**

252 Samples were collected on August 2, 2017 of the dry season in central Amazonia at the
253 Manaus Botanical Gardens (“MUSA”) of the Adolfo Ducke Forest Reserve. It is a $10 \text{ km} \times 10$
254 km area set aside since 1963 to the north of Manaus, Amazonas, Brazil, and it has served as a
255 study site for several thousand publications. Three major terra firme forest classifications
256 describe the forest, including valley, slope, and plateau forests (Ribeiro et al., 1994;Oliveira et
257 al., 2008). The tree canopy height is typically in the range of 25 to 30 m. The UAV equipped
258 with the sample collector was launched and recovered from a platform of $3.5 \text{ m} \times 3.5 \text{ m}$ atop a
259 42-m tower (3.0032° S , 59.9397° W , 120 m above sea level). Samples were collected on the
260 UAV at point A (3.0030° S , 59.9333° W , 122 m above sea level; Figure S1). The collection
261 point was 711 m from the launch point. The UAV successfully flew to the sample location
262 repeatedly based on pre-programmed GPS coordinates. Three samples were collected in separate
263 flights at heights of 60 m, 75 m, and 100 m relative to the ground level at the tower location. A
264 sample flow rate of 150 sccm and duration of 10 min duration were used to collect a total sample
265 volume of 1.5 L. For comparison, VOC collections were performed concurrently atop the MUSA
266 Tower with a hand-held motorized pump (Model 210-1002, SKC). These samples were collected
267 using a flow rate of 200 sccm and sampling time of 20 min for a total sample volume of 2.0 L.



268 Data from the sampler showing flow and pressure for the three in-flight samples are
269 shown in Figure 3. To conserve battery power, the pump is turned off between samples and no
270 data are recorded. The results show that each valve successfully activated. After the initial start
271 up, a uniform flow rate of 150 sccm and a pressure of 1 atm is maintained during each sampling
272 period. The measured flow rate is used to calculate the volume of each sample to account for
273 small variations in flow.

274 VOC mixing ratios determined from the samples collected by the UAV sampler and from
275 atop the tower are presented in Table 1. VOC concentrations depend on many conditions,
276 including season, time of day, temperature, light levels (i.e., cloudiness), height above the
277 canopy, and canopy composition, which can vary on spatial scales of 10's of meters.
278 Nevertheless, the results demonstrate reasonable consistency between samples collected by the
279 UAV and on the tower, separated by 711 m. They also suggest that vertical concentration
280 gradients can be assessed using this method. Further analysis and scientific interpretation of
281 these results and a larger data set are the subject of a separate publication (Batista et al., 2018).

282 The possible effects of air circulation created by the UAV multicopter rotors on the
283 sampling was considered. The flow field is also a factor in determining the sampler placement.
284 As there are no published computational fluid dynamics (CFD) studies specifically of the DJI
285 Matrice 600, CFD simulations of the UAV were performed. As shown in Fig. 4a, the pressure
286 difference between the area underneath the sampling box and the area under the propellers was
287 calculated as <100 Pa, indicating that the effect of the UAV on the pressure in the sampling
288 region is minimal. This suggests that any possible effects of UAV pressure fields on any pressure
289 sensitive sensor mounted in this area would be small.



290 Figure 4b shows the calculated air velocity distribution around the UAV. The simulation
291 suggests that air enters the sampling region from above the propellers, undergoes turbulent
292 recirculation to the UAV sampling region, and then is ejected below the UAV. This is consistent
293 with the CFD study by Ventura Diaz and Yoon (2018), which suggested the sample represented
294 an air parcel extending approximately 1 m above the UAV. In addition, the simulation shows
295 that the air flushing time in the sample region is fast (i.e., several seconds) compared to the
296 timescale of VOC sampling (i.e., 5-10 min). The simulations thus indicate that the sampler
297 performs representative real-time sampling of ambient VOC concentrations averaged across
298 several meters around the UAV.

299 Several other studies investigated the effects of a multicopter on air sampling and reached
300 similar conclusions. Roldan et al. (2015) simulated flow around a quadcopter and validated the
301 simulations with air velocity measurements. The results showed that air speeds were greatest
302 near the propellers and smallest near the center of the UAV. The optimal location for air sensors
303 was at the center of the vehicle. Further testing involved measurements of CO₂ concentrations
304 with an onboard sensor near a CO₂ source, with and without the propellers rotating. There were
305 small differences (<5%) in the measured CO₂ concentrations, supporting the conclusions of the
306 simulations. Similarly, Black et al. (2018) demonstrated that no difference was observed in the
307 measured atmospheric mercury concentrations using a copter-based sampler when the UAV was
308 powered as compared to when it was unpowered. Together with the results of the current
309 simulations, these studies suggest that valid measurements of many atmospheric gas
310 concentrations can be obtained from multicopter platforms.

311 One of the key constraints on VOC sample collection by UAVs is the flight duration.
312 Although the manufacturer specifies a maximum flight time of 40 min, when carrying the



313 sampler under tested flight conditions and factoring in a margin of safety, the maximum flight
314 duration is limited to 25 min. Because the volumetric flow rate is also constrained to <200 sccm
315 for the manufacturer-recommended operation of the cartridges to avoid breakthrough, the
316 maximum air volume that can be collected during a flight is 5.0 L. Equation 1 in conjunction
317 with the method detection limit of 10 pg suggests a minimum detectable atmospheric mixing
318 ratio of 1 ppt for this sample volume at standard temperature and pressure. This sensitivity is
319 sufficient for abundant primary emissions such as isoprene and monoterpenes, which can have
320 mixing ratios of 10^2 to 10^4 ppt in tropical forests (Yáñez-Serrano et al., 2018). It may not,
321 however, be sufficient for quantifying primary compounds in other ecosystems with low-
322 emitting flora species, such as forests at higher latitudes or other ecosystem types such as
323 grasslands. It may also not allow for the detection of species of lower concentrations such as
324 sesquiterpenes. Characterization of these compounds is needed to fully understand the reactive
325 chemistry and aerosol formation potential of VOCs in forest environments. Additional strategies
326 to be explored for these compounds include more-rapid flow through the cartridge for low-
327 volatility compounds for which breakthrough is less of a concern or parallel sampling with
328 several cartridges simultaneously followed by common desorption at the TD-GC/MS.

329 There is a trade-off between the number of samples collected per flight and the individual
330 sample volume. Collecting multiple samples in one flight necessitates smaller volumes for each
331 sample and thus higher detection limits. Subject to the overall flight time limitation, the design of
332 the sampler allows flexibility in the sample count and duration to best achieve the experimental
333 objectives. For each individual flight, scientific choices can be made whether to collect a single,
334 large volume sample to target less-abundant species or multiple smaller samples for surveying
335 the major VOC components.



336 A number of strategies can ameliorate these limitations. To facilitate the continuous
337 operation of the UAV, multiple sets of batteries can be used. One set is charged while another set
338 is in use. After each flight, the depleted batteries can be replaced with the spare fully charged set
339 and the UAV launched immediately instead of waiting for the batteries to charge. This allows the
340 number of samples collected to be maximized. Extension of the sample time can also be
341 achieved by initiating a sample on one flight, pausing while the UAV returns for battery
342 replacement, then returning to the same location and resuming collection with the same
343 cartridge. A modification on this approach would be to use a single cartridge to collect air at the
344 same location and time of day over multiple days, resulting in an average for that time period.

345 A major goal of ongoing development of the sampler is to enable operation either
346 remotely through tablet-based software or with a pre-programmed GPS-based flight trajectory.
347 Both of these operational modes require real-time communication among the sampler, the UAV
348 on-board computer, and the user control interface on the tablet. The Arduino Uno
349 microcontroller is unable to communicate with the UAV on-board computer. To address this
350 issue, an ongoing step in the development is the replacement the Arduino Uno microcontroller
351 with a Raspberry Pi miniature computer. Communication between the sampler and user interface
352 also can enable development of custom software as a diagnostic tool that enables monitoring the
353 status of the valves and pump during the flight. This capability can be important to alert the user
354 to problems during flight, such as the failure of valves or the pump to be activated, as has
355 occurred occasionally on windy days due to strong vibration.

356 Together with the flight capabilities offered by modern day UAV platforms, this sampler
357 opens the door to studying VOC emission and uptake at previously inaccessible scales. In the



358 long term, data from this project will shed light on atmospheric chemistry, biodiversity, and
359 ecosystem stress within the context of global climate change.

Acknowledgments. Support from the Harvard Climate Change Solutions Fund is gratefully acknowledged. The Museu de Amazonia of the Manaus Botanical Gardens kindly provided access and logistical support. A Senior Visitor Research Grant of the Amazonas State Research Foundation (FAPEAM) is acknowledged.

References.

- Alves, E. G., Jardine, K., Tota, J., Jardine, A., Yáñez-Serrano, A. M., Karl, T., Tavares, J., Nelson, B., Gu, D., Stavrou, T., Martin, S., Artaxo, P., Manzi, A., and Guenther, A.: Seasonality of isoprenoid emissions from a primary rainforest in central Amazonia, *Atmos. Chem. Phys.*, 16, 3903-3925, 10.5194/acp-16-3903-2016, 2016.
- Alves, E. G., Tóta, J., Turnipseed, A., Guenther, A. B., Vega Bustillos, J. O. W., Santana, R. A., Cirino, G. G., Tavares, J. V., Lopes, A. P., Nelson, B. W., de Souza, R. A., Gu, D., Stavrou, T., Adams, D. K., Wu, J., Saleska, S., and Manzi, A. O.: Leaf phenology as one important driver of seasonal changes in isoprene emissions in central Amazonia, *Biogeosciences*, 15, 4019-4032, 10.5194/bg-15-4019-2018, 2018.
- Batista, C. E., Guimarães, P. C., Ribeiro, I. O., Medeiros, A. S. S., Ye, J., Barbosa, R. G., Oliveira, R. L., Duvoisin Jr., S., Gu, D., Guenther, A. B., McKinney, K. A., Martins, L. D., Martin, S. T., and Souza, R. A. F.: Atmospheric organic molecules variable at the intermediate scale of forest sub-type studied by a copter unmanned aerial vehicle over the Amazon forest, *Environmental Science Letters*, in preparation, 2018.
- Black, O., Chen, J., Scircle, A., Zhou, Y., and Cizdziel, J. V.: Adaption and use of a quadcopter for targeted sampling of gaseous mercury in the atmosphere, *Environmental Science and Pollution Research*, 25, 13195-13202, 10.1007/s11356-018-1775-y, 2018.
- Blake, R. S., Monks, P. S., and Ellis, A. M.: Proton-Transfer Reaction Mass Spectrometry, *Chemical Reviews*, 109, 861-896, 10.1021/cr800364q, 2009.
- Chameides, W., Lindsay, R., Richardson, J., and Kiang, C.: The role of biogenic hydrocarbons in urban photochemical smog: Atlanta as a case study, *Science*, 241, 1473-1475, 10.1126/science.3420404, 1988.
- Chang, C. C., Wang, J. L., Chang, C. Y., Liang, M. C., and Lin, M. R.: Development of a multicopter-carried whole air sampling apparatus and its applications in environmental studies, *Chemosphere*, 144, 484-492, 2016.
- Cross, E. S., Williams, L. R., Lewis, D. K., Magoon, G. R., Onasch, T. B., Kaminsky, M. L., Worsnop, D. R., and Jayne, J. T.: Use of electrochemical sensors for measurement of air



pollution: correcting interference response and validating measurements, *Atmos. Meas. Tech.*, 10, 3575-3588, [10.5194/amt-10-3575-2017](https://doi.org/10.5194/amt-10-3575-2017), 2017.

DJI Downloads: <https://www.dji.com/matrice600/info#downloads>.

DJI.com: <https://www.dji.com/matrice600-pro>.

Faiola, C. L., Erickson, M. H., Fricaud, V. L., Jobson, B. T., and VanReken, T. M.: Quantification of biogenic volatile organic compounds with a flame ionization detector using the effective carbon number concept, *Atmos. Meas. Tech.*, 5, 1911-1923, [10.5194/amt-5-1911-2012](https://doi.org/10.5194/amt-5-1911-2012), 2012.

Fuentes, J. D., Gu, L., Lerdau, M., Atkinson, R., Baldocchi, D., Bottenheim, J. W., Ciccioli, P., Lamb, B., Geron, C., Guenther, A., Sharkey, T. D., and Stockwell, W.: Biogenic hydrocarbons in the atmospheric boundary layer: a review, *Bulletin of the American Meteorological Society*, 81, 1537-1575, [10.1175/1520-0477\(2000\)081<1537:bhitab>2.3.co;2](https://doi.org/10.1175/1520-0477(2000)081<1537:bhitab>2.3.co;2), 2000.

Goldstein, A. H., and Galbally, I. E.: Known and unexplored organic constituents in the earth's atmosphere, *Environmental Science & Technology*, 41, 1514-1521, [10.1021/es072476p](https://doi.org/10.1021/es072476p), 2007.

Goldstein, A. H., Koven, C. D., Heald, C. L., and Fung, I. Y.: Biogenic carbon and anthropogenic pollutants combine to form a cooling haze over the southeastern United States, *Proceedings of the National Academy of Sciences*, 106, 8835-8840, [10.1073/pnas.0904128106](https://doi.org/10.1073/pnas.0904128106), 2009.

Greenberg, J. P., Guenther, A. B., Ptron, G., Wiedinmyer, C., Vega, O., Gatti, L. V., Tota, J., and Fisch, G.: Biogenic VOC emissions from forested Amazonian landscapes, *Global Change Biology*, 10, 651--662, [10.1111/j.1365-2486.2004.00758.x](https://doi.org/10.1111/j.1365-2486.2004.00758.x), 2004.

Gu, D., Guenther, A. B., Shilling, J. E., Yu, H., Huang, M., Zhao, C., Yang, Q., Martin, S. T., Artaxo, P., Kim, S., Seco, R., Stavrou, T., Longo, K. M., Tóta, J., de Souza, R. A. F., Vega, O., Liu, Y., Shrivastava, M., Alves, E. G., Santos, F. C., Leng, G., and Hu, Z.: Airborne observations reveal elevational gradient in tropical forest isoprene emissions, *Nature Communications*, 8, 15541, [10.1038/ncomms15541](https://doi.org/10.1038/ncomms15541), 2017.

Guenther, A., Karl, T., Harley, P., Wiedinmyer, C., Palmer, P. I., and C., G.: Estimates of global terrestrial isoprene emissions using MEGAN (Model of Emissions of Gases and Aerosols from Nature), *Atmospheric Chemistry and Physics*, 6, 3181--3210, [10.5194/acp-6-3181-2006](https://doi.org/10.5194/acp-6-3181-2006), 2006.

Hoker, J., Obersteiner, F., Bönisch, H., and Engel, A.: Comparison of GC/time-of-flight MS with GC/quadrupole MS for halocarbon trace gas analysis, *Atmos. Meas. Tech.*, 8, 2195-2206, [10.5194/amt-8-2195-2015](https://doi.org/10.5194/amt-8-2195-2015), 2015.

Karl, T., Guenther, A., Turnipseed, A., Patton, E. G., and Jardine, K.: Chemical sensing of plant stress at the ecosystem scale, *Biogeosciences*, 5, 1287-1294, [10.5194/bg-5-1287-2008](https://doi.org/10.5194/bg-5-1287-2008), 2008.

Kesselmeier, J., Guenther, A., Hoffmann, T., Piedade, M. T., and Warnke, J.: Natural volatile organic compound emissions from plants and their roles in oxidant balance and particle formation, in: *Amazonia and Global Change*, American Geophysical Union, 183-206, 2013.

Kim, S., Guenther, A., and Apel, E.: Quantitative and qualitative sensing techniques for biogenic volatile organic compounds and their oxidation products, *Environmental Science: Processes & Impacts*, 15, 1301, [10.1039/c3em00040k](https://doi.org/10.1039/c3em00040k), 2013.



- Klinger, L. F., Greenburg, J., Guenther, A., Tyndall, G., Zimmerman, P., M'Bangui, M., Moutsamboté, J. M., and Kenfack, D.: Patterns in volatile organic compound emissions along a savanna-rainforest gradient in central Africa, *Journal of Geophysical Research: Atmospheres*, 103, 1443-1454, [10.1029/97jd02928](https://doi.org/10.1029/97jd02928), 1998.
- Kravitz, B., Guenther, A. B., Gu, L., Karl, T., Kaser, L., Pallardy, S. G., Peñuelas, J., Potosnak, M. J., and Seco, R.: A new paradigm of quantifying ecosystem stress through chemical signatures, *Ecosphere*, 7, e01559, [10.1002/ecs2.1559](https://doi.org/10.1002/ecs2.1559), 2016.
- Kuhn, U., Rottenberger, S., Biesenthal, T., Wolf, A., Schebeske, G., Ciccioli, P., Brancaleoni, E., Frattoni, M., Tavares, T. M., and Kesselmeier, J.: Seasonal differences in isoprene and light-dependent monoterpene emission by Amazonian tree species, *Global Change Biology*, 10, 663-682, [10.1111/j.1529-8817.2003.00771.x](https://doi.org/10.1111/j.1529-8817.2003.00771.x), 2004.
- Laothawornkitkul, J., Taylor, J. E., Paul, N. D., and Hewitt, C. N.: Biogenic volatile organic compounds in the Earth system, *New Phytologist*, 183, 27-51, [doi:10.1111/j.1469-8137.2009.02859.x](https://doi.org/10.1111/j.1469-8137.2009.02859.x), 2009.
- Lindinger, W., Hansel, A., and Jordan, A.: On-line monitoring of volatile organic compounds at pptv levels by means of proton-transfer-reaction mass spectrometry (PTR-MS) medical applications, food control and environmental research, *International Journal of Mass Spectrometry and Ion Processes*, 173, 191-241, [https://doi.org/10.1016/S0168-1176\(97\)00281-4](https://doi.org/10.1016/S0168-1176(97)00281-4), 1998.
- Markes International Ltd.: Thermal desorption technical support - Application Note 5: Advice on sorbent selection, tube conditioning, tube storage and air sampling., Markes International Ltd., 2014.
- Millet, D. B., Donahue, N. M., Pandis, S. N., Polidori, A., Stanier, C. O., Turpin, B. J., and Goldstein, A. H.: Atmospheric volatile organic compound measurements during the Pittsburgh Air Quality Study: Results, interpretation, and quantification of primary and secondary contributions, *Journal of Geophysical Research: Atmospheres*, 110, [doi:10.1029/2004JD004601](https://doi.org/10.1029/2004JD004601), 2005.
- Niinemets, Ü.: Mild versus severe stress and BVOCs: thresholds, priming and consequences, *Trends in Plant Science*, 15, 145-153, [10.1016/j.tplants.2009.11.008](https://doi.org/10.1016/j.tplants.2009.11.008), 2010.
- Oliveira, A. N. d., Amaral, I. L. d., Ramos, M. B. P., Nobre, A. D., Couto, L. B., and Sahdo, R. M.: Composição e diversidade florístico-estrutural de um hectare de floresta densa de terra firme na Amazônia Central, Amazonas, Brasil (Translation: Composition and floristic-structural diversity of one hectare of dense terra firme forest in Central Amazonia, Amazonas, Brazil), *Acta Amazonica*, 38, 627-641, 2008.
- Pankow, J. F., Luo, W., Melnychenko, A. N., Barsanti, K. C., Isabelle, L. M., Chen, C., Guenther, A. B., and Rosenstiel, T. N.: Volatilizable Biogenic Organic Compounds (VBOCs) with two dimensional Gas Chromatography-Time of Flight Mass Spectrometry (GC × GC-TOFMS): sampling methods, VBOC complexity, and chromatographic retention data, *Atmos. Meas. Tech.*, 5, 345-361, [10.5194/amt-5-345-2012](https://doi.org/10.5194/amt-5-345-2012), 2012.
- Peñuelas, J., and Llusà, J.: BVOCs: plant defense against climate warming?, *Trends in Plant Science*, 8, 105-109, [10.1016/S1360-1385\(03\)00008-6](https://doi.org/10.1016/S1360-1385(03)00008-6), 2003.



Peñuelas, J., and Staudt, M.: BVOCs and global change, *Trends in Plant Science*, 15, 133-144, <https://doi.org/10.1016/j.tplants.2009.12.005>, 2010.

Pollmann, J., Ortega, J., and Helmig, D.: Analysis of atmospheric sesquiterpenes: Sampling losses and mitigation of ozone interferences, *Environmental Science & Technology*, 39, 9620--9629, 10.1021/es050440w, 2005.

Pugh, T. A. M., MacKenzie, A. R., Langford, B., Nemitz, E., Misztal, P. K., and Hewitt, C. N.: The influence of small-scale variations in isoprene concentrations on atmospheric chemistry over a tropical rainforest, *Atmos. Chem. Phys.*, 11, 4121-4134, 10.5194/acp-11-4121-2011, 2011.

Ribeiro, J. E. L. S., Nelson, B. W., Silva, M. F. d., Martins, L. S. S., and Hopkins, M.: Reserva Florestal Ducke: Diversidade E ComposiÇÃo Da Flora Vascular, *Acta Amazonica*, 24, 19-30, 10.1590/1809-43921994242030, 1994.

Roldán, J., Joossen, G., Sanz, D., del Cerro, J., and Barrientos, A.: Mini-UAV Based Sensory System for Measuring Environmental Variables in Greenhouses, *Sensors*, 15, 3334, 2015.

Ventura Diaz, P., and Yoon, S.: High-Fidelity Computational Aerodynamics of Multi-Rotor Unmanned Aerial Vehicles, in: 2018 AIAA Aerospace Sciences Meeting, AIAA SciTech Forum, American Institute of Aeronautics and Astronautics, 2018.

Villa, T., Gonzalez, F., Miljevic, B., Ristovski, Z., and Morawska, L.: An Overview of Small Unmanned Aerial Vehicles for Air Quality Measurements: Present Applications and Future Perspectives, *Sensors*, 16, 1072, 10.3390/s16071072, 2016.

Wang, X., Situ, S., Guenther, A., Chen, F. E. I., Wu, Z., Xia, B., and Wang, T.: Spatiotemporal variability of biogenic terpenoid emissions in Pearl River Delta, China, with high-resolution land-cover and meteorological data, *Tellus B*, 63, 241-254, 10.1111/j.1600-0889.2010.00523.x, 2011.

Woolfenden, E.: Sorbent-based sampling methods for volatile and semi-volatile organic compounds in air: Part 1: Sorbent-based air monitoring options, *Journal of Chromatography A*, 1217, 2674--2684, 10.1016/j.chroma.2009.12.042, 2010a.

Woolfenden, E.: Sorbent-based sampling methods for volatile and semi-volatile organic compounds in air. Part 2. Sorbent selection and other aspects of optimizing air monitoring methods, *Journal of Chromatography A*, 1217, 2685--2694, 10.1016/j.chroma.2010.01.015, 2010b.

Woolfenden, E. A., and McClenny, W. A.: Compendium Method TO-17: Determination of Volatile Organic Compounds in Ambient Air Using Active Sampling Onto Sorbent Tubes, US EPA, Cincinnati, OH, 1999.

Yáñez-Serrano, A. M., C., N. A., E., B., Gomes Alves, E., Ganzeveld, L., Bonn, B., Wolff, S., Sa, M., Yamasoe, M., Williams, J., Andreae, M. O., and Kesselmeier, J.: Monoterpene chemical speciation in the Amazon tropical rainforest: variation with season, height, and time of day at the Amazon Tall Tower Observatory (ATTO), *Atmos. Chem. Phys.*, 18, 3403 - 3418, 10.5194/acp-18-3403-2018, 2018.



Table 1. Summary of biogenic VOC types and concentrations collected on 2 August 2017. Results are shown for sample collection by the UAV-based sampler at 711 m from the tower launch location as well as by use of a hand-held pump at the top of the tower. Local time is -4 h to UTC. ^aSampling height as relative to ground level at the MUSA tower. ^bOnly major monoterpenes are listed here. In addition to isoprene and monoterpenes, four sesquiterpenes including β -caryophyllene were detected. “n.d.” denotes that the VOC concentration was below the detection limit of the instrument.

Sample	Local time	Location (Distance to Tower, m)	Sampling height ^a (m)	Isoprene (ppt)	α -Pinene (ppt)	β -Pinene (ppt)	d-Limonene (ppt)	α -thujene (ppt)	Tricyclene (ppt)	Camphene (ppt)	Total Monoterpenes ^b (ppt)
1	11:15										
	-										
2	11:35	711 m	75	429.3 \pm 68.7	33.7 \pm 5.4	7.0 \pm 1.1	n.d. ^c	1.4 \pm 0.2	0.7 \pm 0.1	0.5 \pm 0.1	43.6 \pm 7.0
	11:15										
3	11:35	Tower top	42	622.0 \pm 99.5	65.7 \pm 10.5	12.7 \pm 2.0	n.d.	1.6 \pm 0.3	1.1 \pm 0.2	n.d.	82.0 \pm 13.1
	13:15										
4	13:35	711 m	100	912.7 \pm 146.0	41.6 \pm 6.7	9.2 \pm 1.5	3.2 \pm 0.5	0.5 \pm 0.1	0.5 \pm 0.1	0.4 \pm 0.1	56.2 \pm 9.0
	15:15										
5	15:35	711 m	60	579.7 \pm 92.8	37.0 \pm 5.9	8.6 \pm 1.4	n.d.	2.2 \pm 0.4	1.4 \pm 0.2	1.8 \pm 0.3	51.1 \pm 8.2
	15:15										
5	15:35	Tower top	42	784.3 \pm 125.5	39.8 \pm 6.4	7.5 \pm 1.2	0.5 \pm 0.1	2.5 \pm 0.4	0.2 \pm 0.1	0.4 \pm 0.1	51.3 \pm 8.2

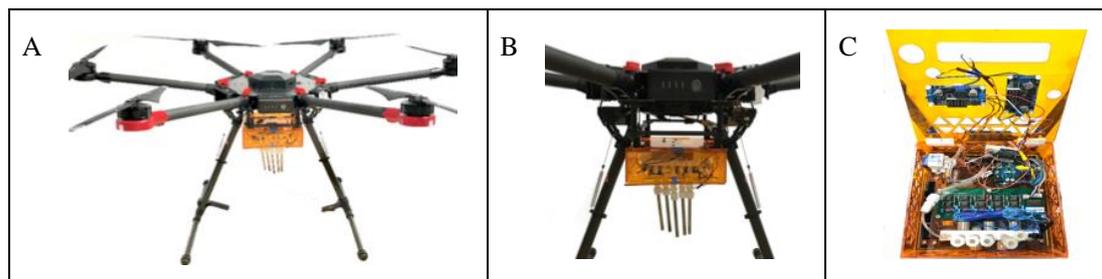


Figure 1. UAV equipped with VOC sampler: (A) DJI Matrice 600 hexacopter UAV. (B) Custom-built sampler visible in orange mounted to UAV. Five VOC sorbent cartridges (Markes International, Inc) are seen on the undercarriage. (C) Sampler with lid open to show pump and electronics package seen in panel B for differentially actuating sample flow through the sorbent cartridges.

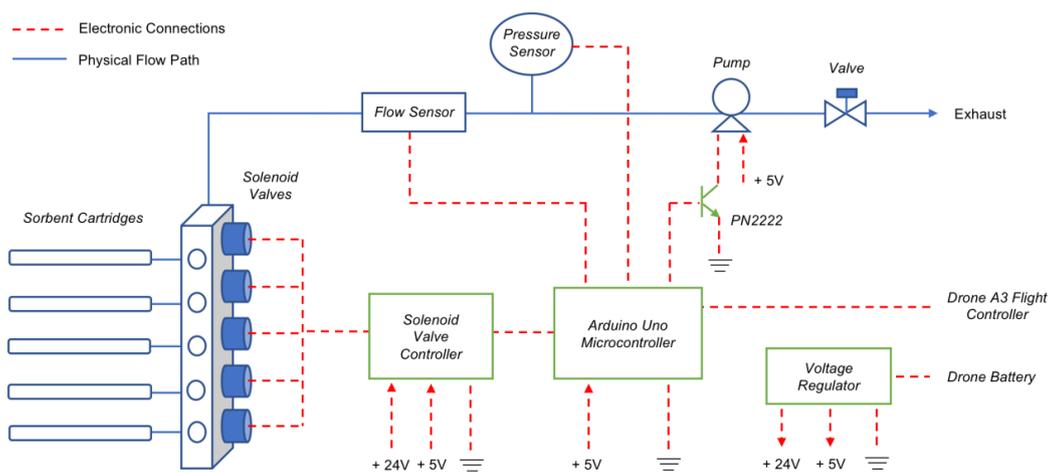


Figure 2. Schematic diagram of sampling device. All components are powered by onboard batteries on the UAV and are controlled by an Arduino Uno microcontroller. Gas flows from the ambient atmosphere through the sorbent cartridges and out to the pump and exhaust.

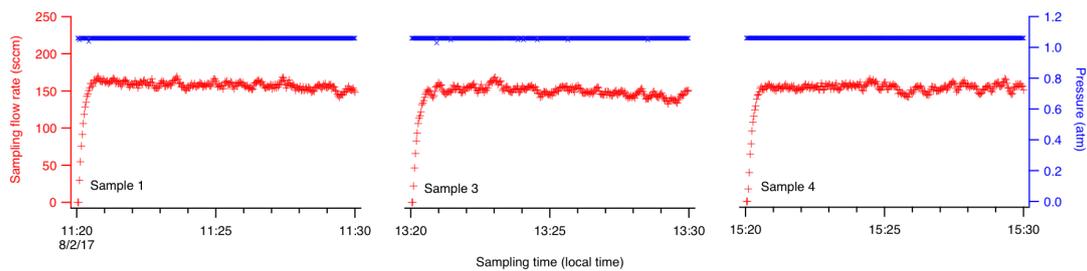


Figure 3. Time series of diagnostic data collected during the VOC-sampling UAV flights.

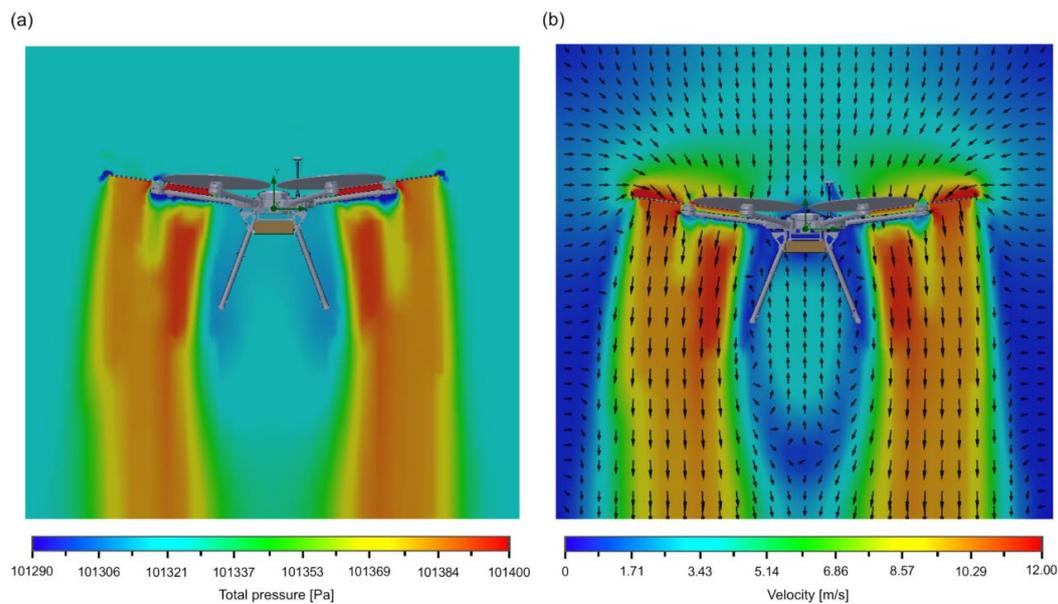


Figure 4.