

Dear reviewers,

We like to thank you for your helpful comments on our paper titled “Upgrade and automation of the JPL Table Mountain Facility tropospheric ozone lidar (TMTOL) for near-ground ozone profiling and satellite validation”.

The original comments are in bold, followed by our replies. An additional file, highlighting the changes introduced in the manuscript, is also included.

Reviewer #1

General comments:

1) clarify the 5% accuracy in the abstract to avoid confusion

Based on your comments, some modifications were introduced in the abstract (see first specific comment).

2) suggest adding description of the auto alignment feature.

Based on your suggestion, the following explanation was included as part of the system automation description:

The alignment module was implemented to control the alignment of the beams in order to optimize the data quality of the acquisition. For the alignment of each transmitted beam, a step-stare scanning is conducted along two perpendicular axes. After finishing the scanning along the first axis, the centroid of the acquired data as function of the mirror position is calculated at a given alignment altitude and the mirror readjusted to the calculated position. This procedure is then repeated for the second axis. Due to the narrower FOV of the high altitude receiver compared to the other two receiver sets, transmitted beams are aligned using the signals from the high altitude channels at about 5000 m AGL. The alignment of the other two receivers is manually checked about two times a year, although no large readjustments are typically required.

Specific comments:

P1, L8-9, “An agreement of 5 % or better with the ozonesonde down to an altitude range of 100-m above ground was demonstrated.” It looks very ambitious to conclude the accuracy “5%” just based on one intercomparison experiment between the lidar and tethered ozonesonde (Figure 8). There are two coincident ozonesonde profiles in the May 25 case study (page 14-18 and Figure 11). The discrepancies between the sondes and lidar are not quantified well in the context although the explanations about these discrepancies are provided. But it can be seen that these discrepancies have exceeded 5% at many altitudes even excluding the STE layers in Figure 11 by a visual check. So, it looks like the authors made favorable conclusions by using selective results. Please clarify.

Comparing a lidar retrieval with a free-flying ozonesonde is always complex, as the measured volume might be quite different. This is especially true in cases like the ones shown as part of the 24-h run, when wind speeds were between 15 and 20 m/s. Additionally, the long-term comparison shown in Fig. 13 indicate an agreement better than 10%, even considering the 100 m difference between the ozone photometer.

Having said this, we included some rewording in the abstract to take in account the fact that only one lidar - tethered balloon comparison is shown:

“An agreement of 5 % or better with the ozonesonde down to an altitude range of 100-m above ground was demonstrated.” was changed to *“An agreement of about 5 % with the ozonesonde down to an altitude range of 100-m above ground was observed.”*

Additionally, results corresponding to the long-term comparison conducted between the surface ozone meter and the first valid retrieved bin are now included:

“Comparisons between the lowest point retrieved by the lidar and a co-located surface ozone photometer showed no sign of drift over a two-month test period and an agreement better than 10 %.”

P1, L 13-14, “These comparisons revealed localized differences between sonde and lidar, possibly owing to the differing vertical resolutions (about 52m for lidar and at least 120m for sonde).” What is the corresponding altitude range for the 52-m resolution for the lidar retrievals? 52m is probably the highest resolution of the lidar while ozonesonde has a constant resolution about 100m from surface to ~35km.

The 52-m resolution corresponds to the lowest part of the retrieval (analog signal from the new very-near-range receiver). In order to clarify the statement, the following change was made:

“These comparisons revealed localized differences between sonde and lidar, possibly owing to the differing vertical resolutions (between 52 m and 380 m for lidar and about 100m for the sonde).”

Further details of the lidar resolution scheme used for the lidar/sonde comparison can be found in P15, L6-9.

P2, L9, have you given what TEMPO stands for somewhere?

An explanation of the TEMPO (Tropospheric Emissions: Monitoring Pollution) acronym is now included in the text.

P3, L16-17, pure H₂ or D₂ without buffer gas? Can you give the conversion efficiencies (or the UV pulse energy sent into the sky) for both wavelengths?

No buffer gas is used in the Raman cells. Unfortunately no accurate conversion efficiencies can be provided at this point. Reference test conducted on this topic at TMF can be found in Haner et al., 90, nevertheless the cell length is now different (4 m vs 2 m in the cited paper).

P3, L26, what are the sizes of the receivers for the low altitude channel?

The diameter of the low altitude receivers (50 mm) is now included as part of the description.

P4, L2, what does APC stand for? There are a lot of acronyms in this paper. They are well known in some particular fields (e.g., computer science, satellite), but probably not so for everyone and need to spell out at the 1st time in use.

Based on the reviewer recommendations, explanations for the following acronyms were included: TROPOspheric Monitoring Instrument (TROPOMI), Tropospheric Emissions: Monitoring

Pollution (TEMPO), differential absorption lidar (DIAL), Hierarchical Data Format version 5 (HDF5), electrochemical concentration cell (ECC).

P5, L13, “the alignment module was. . . the acquisition.” Alignment of laser beam with receiver is critical for correct lidar retrievals. Since autonomous alignment is an important feature of the whole autonomous system, can you provide additional description about how your auto alignment works?

Additional description of the alignment procedure is now included (answered in the general comments section).

P6, L1, Table 1 showing detailed numbers of lidar profiles in each month is not closely related to this paper.

Table 1 is included to provide an insight of the datasets already available for TROPOMI validation.

P7, L10-13, 1) the location of the citation is not appropriate. Suggest to put (Kovalev and Bristow, 1996) and Wang et al., 1997) after “dual DIAL measurements”. 2) The statement is a little confusing, or incomplete. Reduction of aerosol interference will naturally reduce the uncertainty in DIAL retrieval. But you say reduction of aerosol interference will increase the ozone retrieval uncertainty potentially by inducing other larger errors. The readers will wonder what are the uncertainty sources with larger errors. Please clarify.

The trade-off between aerosol error correction and random error increase is explained in Wang et al. 97.:

“Therefore, although the three-wavelength dual DIAL appears to have a somewhat larger statistical error, it can be used to reduce substantially the systematic error of the stratospheric ozone measurements in the presence of volcanic aerosols. The system error is also almost unaffected by aerosol loading spatial inhomogeneity and aerosol optical properties.”

The sentence was modified in order to better reflect this compromise:

“Additionally, it has to be mentioned that although dual DIAL measurements help to reduce the systematic error caused by the aerosol influence on the retrieval, it is at the expense of increasing the overall statistical uncertainty on the ozone retrieval (Wang et al., 97).”

P7-8, the authors try to justify the ozone DIAL retrieval with a wavelength pair of 266- 289nm without an aerosol correction with two pages of words. This might be ok by considering that the focus of this paper is the description of the autonomous features of lidar system and this particular lidar is located at a high-elevation site where the sky is relatively clean. But I have following comments: 1) the ozone DIAL can’t measure accurately in the presence of fire smoke where the aerosol gradients could be even larger than the assumed profile in Figure 4. Especially forest fire occurs frequently in CA recently. 2) The aerosol layer is assumed at a low altitude, 500m AGL, in Figure 4. The percentage uncertainty due to aerosol interference could be much larger at a higher altitude because of ozone number density typically decreases with altitude in troposphere. In addition, the 266-nm laser is not able to cover the altitude higher than 3000m AGL as you mentioned in the paper. 3) There exist some aerosol correction methods for two-wavelength ozone DIALs such as Alvarez II et al. 2011 (cited earlier for another purpose); Immmler 2003, Kuang et al., 2011, Sullivan et al., 2014. I believe you still need to mention them although you don’t apply aerosol correction because of some reasons.

We agree with the comments made by the reviewer regarding the limited range of the selected wavelength pair and the need of aerosol correction methods in order to mitigate the effects of strong aerosol plumes in the retrieval accuracy. Nevertheless, and as the reviewer also points out, the main purpose of the wavelength selection discussion is to justify the election of the wavelength DIAL pair for the new very-near-range receiver considering that only a range of about 1000 m is required, that the aerosol load at TMF is typically small, and that there are only a few possible combinations based on the current TMTOL setup. The wavelength selection discussion doesn't intend to provide a general answer to the DIAL wavelength selection problem, but a solution for a specific problem under specific conditions.

Since ozone studies in the presence of different types of aerosols might be part of the applications of the new very-near-range receiver, the following sentence was added:

In case of stronger aerosol loads, the aerosol influence might be further reduced by applying an aerosol correction algorithm (Alvarez et al., 2011; Immler, 2003; Kuang et al., 2011; Sullivan et al., 2014).

P10, in terms of the error induced by the timing offset between the two wavelengths, similar issue has been investigated in previous literature (e.g., Figure 4 in Kuang et al., 2013). How does your result compare to previous ones?

Results are similar after considering the difference in the DIAL wavelengths used in both cases. A citation for the mentioned article was included.

P12, L24, “there is a very good agreement (less than 5% difference). . .”. This statement is not accurate since you mention one sentence later “some deviations between 70 m AGL and 100 AGL” are “less than 10%”. Maybe should change to say “mostly less than 5%” or constrain the altitudes above 100m.

The suggested addition (“*mostly less than 5%*”) was included.

P12, L29, “a 17-sample Savitsky-Golay derivative filter was used”. Why is the filtering window length different with “9 samples for the analog detection mode and 31 samples for the photon-counting mode” which was mentioned earlier?

The difference in the window length is related to the purpose of the analysis. In the case of Figure 7, the analysis focuses on the systematic errors introduced by the differential efficiency component and its relation with the minimum achievable range. A short window allows to get a better spatial resolution on the near end of the retrieval at the price of increasing the random uncertainty. In the case of comparisons with radiosondes, the window length is increased in order to reduce the random uncertainty. As a consequence, biased points at the lower end of the retrieval are now included in the first bins of the retrieval and the minimum (unbiased) achievable range increases from about 70 m to about 100 m.

P18, L21, “a good correlation between these two quantities is observed”, what is the correlation coefficient between the Lidar and i49? Is 10% (a mean value) an exact value or an approximation? Looks like Fig. 12 has sufficient samples so that an exact value of the mean difference can be statistically meaningful.

Mean difference and number of points is now included as part of Fig. 13 (previously Fig. 12). The text was modified to reflect the accurate number (7.2% instead of 10%).

P18, L25, “The result of this comparison show a very similar difference of about 5- 10% between ozone sonde measurements at 100m AGL and surface ozone measurements.” If “the result” is an unpublished result and is not given in the paper either, I suggest adding “not shown” to avoid confusion.

“Not shown” was included at the end of the sentence to avoid confusion.

P18, L 31, “As a result, the system is now capable of performing measurements autonomously from about 70m AGL up to about 15km.” Also P19, L9, “. . .the lowermost 70m AGL. . .”. There are large discrepancies between the lidar and tethered sonde below 100 m (Figure 8), which actually has not been explained very in the context. Moreover, the first lidar altitude grid is also 100m for the intercomparison with the surface observations (Figure 12). These facts clearly suggest the lidar retrievals below 100m are relatively unreliable. I suggest changing “70m” to “100m” to avoid confusion.

Minimum altitude was changed to 100 m following the observations of the reviewer.

Reviewer #2

General comments:

- In section 2 “Instrument description”, the reader would benefit from a diagram of the transmitter and receiver layout of the lidar to better follow the instrument description.

Following the reviewer suggestion, a diagram of the TMTOL was included (Fig. 1).

- Through the manuscript, some acronyms are frequently used but not explained e.g. TROPOMI or TEMPO whereas other acronyms which are used only once are explained e.g. SRS.

A general revision of the acronym use was conducted.

- The authors use AGL and ASL in their altitude nomenclature. This might be confusing to the reader especially if the figure shows the ASL altitude, but the text is describing it in AGL altitude. The figures would need both labels and more consistency would improve the manuscript’ Ideally, only one of the two is used.

We partially agree with the observations of the reviewer with regard to the use AGL and ASL. Nevertheless, since Table Mountain Facility (TMF) is located at a relatively high altitude (2285 m ASL) and part of this work focuses in very-near range measurements (between 100 m and 1000 m AGL), we also consider that some aspects of the work are better explained using AGL altitude while others can be better analyzed using ASL altitude. For example, in the case of the very-near-range receiver technical discussion, differential efficiency and the effects of acquisition delay between both channels of the DIAL system are only relative to the lidar position (very similar to AGL altitude) and independent of its ASL altitude. In the second part of the discussion, when the system performance is compared to tethered-balloon measurements and the stratospheric intrusion event is analyzed, the use of ASL altitude emphasizes the fact that TMF is at a relatively high altitude.

Based on this considerations, some changes were made in the use of ASL and AGL to improve the manuscript consistency.

- Even though “satellite validation” is stated in the title, an example of at least one simultaneous measurement of the lidar and satellite is missing.

Unfortunately the TROPOMI ozone profile data product is still under development and no data is yet available for publication. The following sentence was added to clarify this:

“Unfortunately the TROPOMI ozone profile data product is still under development. For this reason, no comparisons are included in this work.”

Specific comments:

P3L15: SRS is only used once, no need to add the acronym.

This is addressed in a previous answer to reviewer #1.

P3L24-25: FOV is only used once, no need to add the acronym. It is not clear how two fibers in the focal point of the telescope can have two FOVs and separate the atmospheric volume. Also, what are the size of the FOVs.

The acronym is now used also as part of the auto-alignment description. Regarding the wavelength separation, the paper mentioned that both fibers are in the same focal plane, not the same focal point. By keeping fibers in the same focal plane and slightly displacing them from the focal point, two FOVs can be achieved. Further information regarding this setup (i.e. FOVs) can be found in McDermid et al., 2002.

Table 1: Clarify if the observations were simultaneously and in the same volume with TROPOMI. If so, it would be very interesting to see at least one of the measurements.

Experiments conducted for TROPOMI validation consist in 1-hour measurement periods centered around the predicted daily overpass time. This is now clarified as part of Table 1 discussion:

Together with the regular 2-hour experiments typically conducted at TMF as part of NDACC activities, regular 1-hour daytime measurements were carried out during forecasted overpasses in support of the validation of the TROPospheric Monitoring Instrument (TROPOMI) onboard the Sentinel-5 Precursor satellite.

The lack of a comparison with TROPOMI ozone profiles is explained in a previous answer.

P6L5: ABL is only used once, no need to add the acronym.

The acronym was removed.

P7L16-19: This is a very long sentence and could be separated.

Sentence was reformulated.

Because the daytime operation is important for the validation satellite-borne ozone instruments and considering the low intensity of the Raman scattering (about two orders of magnitude lower than Rayleigh scattering) the use of wavelengths in the blind region of the solar spectrum is preferred.

P7L22-23: Consider removing the indent and combine the two paragraphs since the second paragraph refers to the first one and gives another argument why this technique can't be used.

Following the reviewer suggestions, the paragraphs were merged.

P8L14-16: It is not clear why a pellicle beamsplitter is preferred since the other detector can be adjusted to have no differences in the overlap function. Clarify "overlap function" because the same term is used in P10L12.

Although the detector position might be adjusted to compensate the optical path difference introduced by a thick beamsplitter, this would add additional complexity to the setup and an additional degree of freedom at the time of aligning the system. Additionally, a pellicle beamsplitter eliminates ghosts, which also can affect the behavior of the system in the near range regime.

P10L29-31: With the information of the typical concentration Figure 6 becomes meaningful. Consider adding it to the figure description or change the label to Error percentage.

Typical concentration was included as part of the figure description.

P11L8-9: When conducting this test, I wonder how the different wavelengths dependence of the PMT from 288.9nm to 260nm influence the result.

Since the PMT efficiency is not range dependent, no contribution to the differential efficiency is expected.

P12L17: Clarify if the measurements are co-located / same volume measurements.

Co-located was added to clarify the type of comparison described in the section.

"...a set of measurements by a co-located ozonesonde tethered system..."

Figure 7: The Error becomes only meaningful if related to a value / expressed in percentage.

Typical concentration was included as part of the figure description.

Figure 8. Indicate that the ASL altitude is used.

Figures 8, 10 and 12 were modified to indicate that ASL altitude is used.

P14L7-8: In this sentence, the ASL and AGL altitude is used. A consistent use of one or the other would help the reader.

Since for some aspects of the discussion (i.e. comparison with previous discussion about differential efficiency). In order to clarify the discussion, ASL altitude is reported together with the AGL altitude.

P15L4 and Figure 10: Please clarify what surface ozone measurements unit is used.

In all cases, surface ozone measurements were conducted by a co-located Thermo Scientific Model 49i unit. This is now clarified in the Figure 10 description as well as in the corresponding discussion:

“...surface ozone measurements carried out by the co-located Thermo Scientific Model 49i.”

P16L1-2: Adding a subtraction plot would clearly show the good agreement.

A subtraction plot was added to the figure.

P18L1-2: Figure 10 is in ASL altitude, but the text uses AGL altitude.

As in the previous case, ASL altitude is included in the discussion to simplify the reading.

P18L3: Please clarify the sentence “As can be seen in Fig. 11b”.

Further description of the well-mixed layer is now included as part of the figure description.

As can be seen in Fig. 12b, this low ozone layer sits on top of a well-mixed layer (no vertical gradient in the potential temperature) that extends up to 120 m AGL (2405 m ASL) and is trapped between two inversions.

P18L17: The time frame of the “Long-term stability” test is very short. Typically, with the change of the yearly seasons (e.g. temperature, humidity) the stability of an optical system might change. I would consider this test as a preliminary “Long-term stability” test.

We agree with the observations of the reviewer. Preliminary was added to the comparison description to emphasize this.

“...a preliminary long-term comparison between the...”

P19L5: It is referred to other TMF lidars, what are they.

The other TMF lidars are a stratospheric ozone lidar and a water vapor Raman lidar. The following clarification was included:

...(a stratospheric ozone lidar and a water vapor Raman lidar)...

Technical comments:

Please check through the manuscript if “collocated” or “co-located” is the right term.

Corrected.

P5L22: replace “S5P” with “ESA Sentinel-5 Precursor”

This is replaced in the new manuscript version.

P7L5: add . . .“of” the Raman cells. . .

Corrected.

P7L17: add . . .“of” satellite-borne. . .

Corrected.

P10L7: “the the” should read “that the”

Corrected.

P10L8: remove . . .“on” the receiver

Corrected.

P10L19: “user” should read “used”

Corrected.

Upgrade and automation of the JPL Table Mountain Facility tropospheric ozone lidar (TMTOL) for near-ground ozone profiling and satellite validation

Fernando Chouza¹, Thierry Leblanc¹, Mark Brewer¹, and Patrick Wang¹

¹Jet Propulsion Laboratory, California Institute of Technology, Wrightwood, CA, USA

Correspondence: Fernando Chouza (keil@jpl.nasa.gov)

Abstract. As part of the international efforts to monitor air quality, several satellite missions ~~were deployed (e.g. TROPOMI)~~ such as the TROPOspheric Monitoring Instrument (TROPOMI) were deployed and others, like ~~TEMPO~~ Tropospheric Emissions: Monitoring Pollution (TEMPO), are planned for the near future. In support of the validation of these missions, major upgrades to the tropospheric ozone lidar located at the Jet Propulsion Laboratory Table Mountain Facility (TMF) were recently performed. These modifications include the full automation of the system, which now allows unattended measurements during frequent satellite overpasses, and a new receiver that extends the measurement capabilities of the system down to 100 m above surface.

The automation led to the systematic operation of the lidar during daily TROPOMI overpasses, providing more than 139 reference profiles since January 2018. Ozone profiles retrieved using the new lidar receiver were compared to ozonesonde profiles obtained from a ~~co-located~~ co-located tethered balloon. An agreement of about 5 % ~~or better~~ with the ozonesonde down to an altitude range of 100-m above ground was ~~demonstrated~~ observed. Furthermore, the stability of the receiver configuration was investigated. Comparisons between the lowest point retrieved by the lidar and a co-located surface ozone photometer showed no sign of drift over a two-month test period and an agreement better than 10 %. Finally, measurements from a 24-hour intensive measurement period during a stratospheric intrusion event showed good agreement with two free flying ozonesondes. These comparisons revealed localized differences between sonde and lidar, possibly owing to the differing vertical resolutions (~~about 52 m between 52 m and 380 m~~ for lidar and ~~at least 120 m for about 100 m for the~~ sonde).

Copyright statement. Copyright 2018 California Institute of Technology. U.S. Government sponsorship acknowledged.

1 Introduction

Ozone plays different roles in the troposphere depending on its location. At ground level, a high ozone concentration affects the air quality, posing a hazard for human health (WHO, 2003), animals and vegetation (Mauzerall and Wang, 2001), while in the upper troposphere, ozone acts as an effective greenhouse gas (Stocker, 2014). Tropospheric ozone has two major sources, namely stratospheric ozone downward mixing (Leblanc et al., 2011; Langford et al., 2018) and photochemical processes

involving carbon monoxide and volatile organic compounds in the presence of nitrogen oxides (Su et al., 2017). Although both these processes occur naturally, the increasing anthropogenic emission of ozone precursors as a result of the expanding industrial activity led to an increase in the tropospheric background ozone concentrations with respect to pre-industrial levels (Horowitz, 2006; Young et al., 2013). The concentration of tropospheric ozone can fluctuate over relative small temporal and spatial scales as the result of different factors, including the emission rate of precursors, solar radiation intensity and advection processes (Hu et al., 2012). Although significant progress has been made during the last decades in the understanding and modeling of these processes and their relative impact, there are still major gaps in our knowledge. Additionally, and as a result of the stricter emissions control policies and air quality regulations, there is an increasing need of high temporal and spatial resolution ozone concentration measurements for air quality analysis and forecasting (Moltchanov et al., 2015).

Over the past decade, several missions focused on the investigation and monitoring of atmospheric pollutants based on solar-synchronous satellites instruments (Veefkind et al., 2012; Levelt et al., 2018) and others, like the geosynchronous satellite [TEMPOmission Tropospheric Emissions: Monitoring Pollution \(TEMPO\)](#), are expected to be launched soon (Zoogman et al., 2017). While this kind of missions provide large spatial coverage and important information about long-range transport processes, their coarse vertical resolution and daytime-only temporal coverage remain a limiting factor for addressing some key aspects of the pollutant life-cycle in the boundary layer and episodic events.

Due to its relative high temporal and vertical resolution, the lidar technique is able to provide measurements to close the gap between localized high temporal resolution measurements typically provided by in-situ instruments and the coarse resolution measurements provided by satellites. This allows not only to study boundary layer processes, but also provides valuable information for satellite validation purposes (Newchurch et al., 2016). While this make lidars a very useful tool for atmospheric and validation studies, their high complexity typically requires the presence of a trained operator, posing a limitation to operation schedules and time-coverage. In addition the lidar technique inherently cannot provide reliable measurements at very near-range (i.e., typically below a few hundred of meters).

Hence, over the past few years, several efforts were conducted to increase the reliability of lidars, to automate their operation, and to extend downward their measurement range. As a result, several instruments capable of long-term unattended operation were developed (e.g. Engelmann et al., 2016; Strawbridge et al., 2018), and different approaches for low range measurements were proposed, including airborne measurements (Langford et al., 2011; Aggarwal et al., 2018), scanning lidars (Machol et al., 2009), and multi-receiver systems (Kuang et al., 2013; Farris et al., 2018).

The present work describes a series of upgrades to the JPL Table Mountain Facility tropospheric ozone lidar (TMTOL) hardware and software that allow the system to better reach the needs of current and future air quality and satellite validation studies. The upgrades include the possibility of conducting unattended measurements based on a given schedule and the extension of the measurement range down to 100 m above ground level (AGL).

The paper is organized as follows. Section 2 provides a brief description of the system previous to the modifications presented in this paper. Section 3 describes the hardware and software modifications introduced as part of the system automation. Section 4 provides a description of the new receiver for very-near-range measurements. Section 5 presents the validation of the new receiver by means of a comparison with an ozone sensor deployed on a tethered balloon as well as a case study that shows the

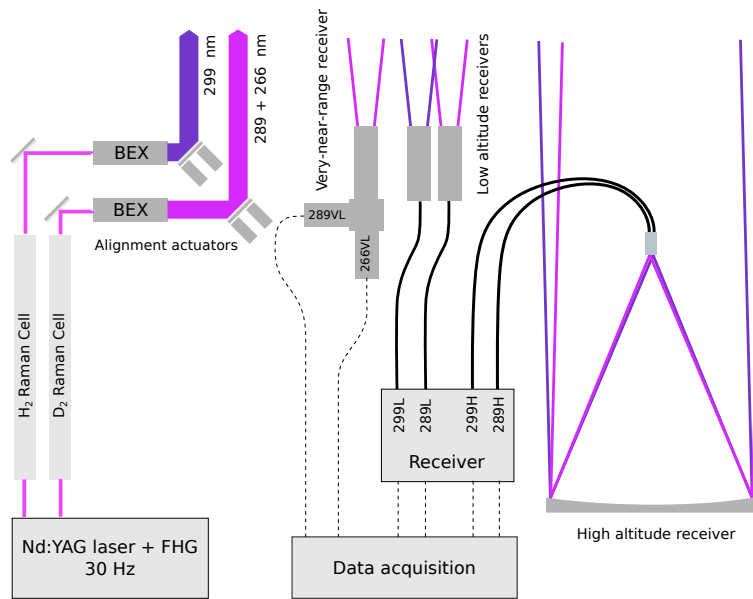


Figure 1. Current transmitter and receiver layout of TMTOL. BEX stands for beam expander. The new very near-range receiver is also shown.

potential of unattended operations enabled by the system automation. A summary of the key achievements presented on this paper and an outlook of future developments are presented in section 6.

2 Instrument description

The TMTOL operations (34.3820° N; 117.6818° W, 2285 m above sea level (ASL)) originally started in 1991 with the alternate measurement of aerosols and ozone (McDermid et al., 1991). The system was redesigned in 1999 to provide routine measurements of tropospheric ozone in the middle and upper troposphere for the Network for the Detection of Atmospheric Composition Change (NDACC) (McDermid et al., 2002). As part of the re-design, the aerosol measurement capability was removed and a new receiver, based on a larger Newtonian telescope (0.91 m diameter) and interference filters, replaced the spectrometer-based previous configuration.

Since the last description of the instrument presented in McDermid et al. (2002), a few modifications were introduced (Figure 1). The old Nd:YAG laser, which operated at a repetition rate of 10 Hz and a 266 nm pulse power of about 50 mJ, was replaced by a Spectra Physics PIV-400, which contains two independent Nd:YAG lasers operating at a repetition rate of 30 Hz. Each side of the laser is followed by second- and fourth-harmonic generators, giving place to two independent 266 nm beams with a pulse power of about 65 mJ each. The fundamental and second-harmonic wavelengths are separated from the 266 nm beams by dichroic beamsplitters and redirected to beam dumps. Each of these two 266 nm beams is then focused into 3.6 m long cells (original cells were only 2 m long) made of 19-mm-outer-diameter stainless steel tubes ended by sapphire windows and filled

with high pressure gas for stimulated Raman shifting (~~SRS~~) to longer wavelengths (Haner and McDermid, 1990). One of these Raman cells is filled with D₂ at 4000 kPa, which shifts the 266 nm pump beam to 288.9 nm (first Stokes). The other cell is filled with H₂ at the same pressure, which shifts the pump beam to 299.1 nm (first Stokes). After passing through the Raman cells, both beams are re-collimated, expanded five times and sent into the atmosphere. The last turning mirrors are mounted on
5 motor-controlled mirror holders, which allow the independent pointing of the beams for alignment purposes.

The lidar receiver remained almost unchanged with respect to the last system update. Up to now, the system operated with two receiver units to accommodate the dynamic range of the upper and lower troposphere atmospheric backscatter. The high altitude receiver, covering approximately the range between 6000 m and 17000 m ASL, consists of a 0.91-m-diameter parabolic mirror with a focal length of 2.54 m. On its focal plane, an arrangement of two optic fibers collects the backscattered
10 light and directs it to a filter and detector arrangement. This dual fiber arrangement allows the receiver to have two separate fields of view (FOVs), and thus, by pointing each transmitted beam to a separate atmospheric volume, separate the two ~~DIAL~~
differential absorption lidar (DIAL) wavelengths. The low altitude receiver, covering a range between 3200 m and 6000 m ASL, consists of two independent 50-mm-diameter refractive telescope arrangements fiber-coupled to the corresponding filters and detectors. The original setup included a chopper wheel which was removed due to thermal issues. Tests performed after
15 this change showed no impact in the retrieved ozone profiles.

3 Automation

As mentioned before, one of the main objectives of the system upgrade was to add autonomous measurement capability, which would allow to perform scheduled measurements, as required for satellite missions validation, without adding workload on the lidar operators. Furthermore, the automation of this lidar will serve as a test bench for the future development of a fully
20 autonomous mobile lidar system.

Figure ~~1~~2 presents a block diagram of the new automated system. The power distribution on the system is based on a 3 kV A APC UPS followed by an APC Ethernet controlled switched rack power distribution unit. This setup provides uninterrupted power and allows the remote power control and restart of all lidar subsystems, excluding the laser and the chiller unit.

The system control, data acquisition and storage is based on a standard desktop PC, which connects with the rest of the
25 devices with an Ethernet interface. For the case of existing subsystems that only support an RS232 interface (laser, alignment motor controller and the laser trigger generator), a Moxa NPort 5610-8-DT Ethernet-RS232 converter was included. The control and status acquisition of the dome and telescope hatch is implemented with a Moxa ioLogik E1214 remote Ethernet I/O device. Additional system monitoring is available through two Amcrest 2K webcams with Ethernet interface. These two cameras allow the operator to have a full view of the system, including the dome hatch and the laser. A meteorological station, a
30 Vaisala DRD11A rain sensor and an all-sky camera are connected to the control computer in order to provide real time weather information to the lidar control software. Since the system dome hatch does not have any protective window, an additional direct connection between the rain sensor and the dome hatch control was added in order to ensure that, even in the case of a crash in the control software or computer, the system cover will be closed in case of precipitation events.

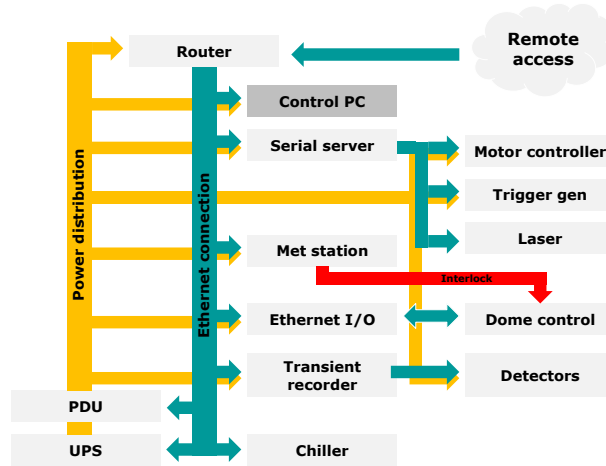


Figure 2. Block diagram describing the the power distribution (orange) and data transfer (green) between different subsystems of the lidar. Hatch hardware interlock based on rain sensing is shown in red.

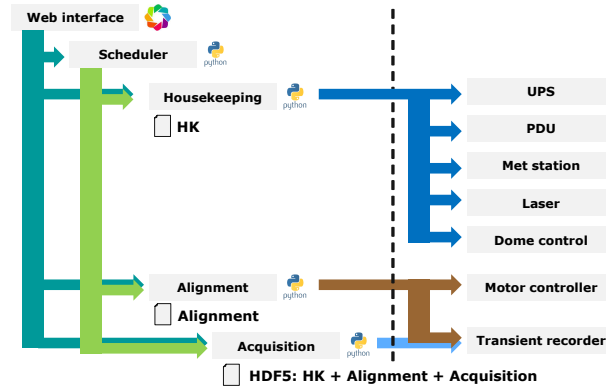


Figure 3. Block diagram of the new acquisition and lidar control software.

The data acquisition system is based on Licel transient recorders. On its original configuration, four TR20-12 modules were used to acquire the signals corresponding to the low and high range receivers. For the new near-range receiver (Sec. 4), a second rack with two TR20-16 (photon-counting and 16-bit analog detection) was added. Additionally, in order to simplify the automation process, the original Licel transient recorder rack interface (DIO-32HS) was replaced with an Ethernet card interface.

Laser and data acquisition timing are generated by a Stanford Research DG535 followed by a Quantum Composer Model 9520.

The new lidar control and data acquisition software were designed in a modular approach to ease the debugging process and reduce the complexity of porting the software to other lidar systems existing at TMF. Since the system is now designed to

operate in autonomous mode, the possibility of analyzing the system status from a remote place is a very important feature. For this purpose, a web interface was developed. In this way, any device with a web browser connected to the TMF network can be used to check the system status. The software described in this section was implemented in Python (www.python.org). The Python library Bokeh (<http://bokeh.pydata.org>) was used for the implementation of the system web interface and data acquisition visualization.

The general structure of the software is presented in Fig. 23. The interaction with the lidar hardware is implemented in the housekeeping, alignment and acquisition modules. The housekeeping module is in charge of performing most of the tasks that were previously conducted by the lidar operator. This includes the monitoring of the power quality, turning on and off each lidar subsystem and analyzing if the meteorological conditions reported by the meteorological station are adequate for the lidar operation. The alignment module was implemented to control the alignment of the beams in order to optimize the data quality of the acquisition. For the alignment of each transmitted beam, a step-stare scanning is conducted along two perpendicular axes. After finishing the scanning along the first axis, the centroid of the acquired data as function of the mirror position is calculated at a given alignment altitude and the mirror readjusted to the calculated position. This procedure is then repeated for the second axis. Due to the narrower FOV of the high altitude receiver compared to the other two receiver sets, transmitted beams are aligned using the signals from the high altitude channels at about 5000 m AGL. The alignment of the other two receivers is manually checked about two times a year, although no large readjustments are typically required. Finally, the acquisition module is in charge of retrieving the data from the Licel transient recorders and storing the data.

For the data storage, the Hierarchical Data Format version 5 (HDF5 format) was chosen. The acquisition software is currently setup to store one file every minute. This includes the average of the acquired lidar profiles, as well as different environmental variables like the site meteorological conditions, last system alignment profiles and trigger timing information. In this way, a complete track of the system status is stored together with the actual lidar data. This information would help keep track of the system health and track down the cause of any issue found during the data analysis process.

The software and hardware automation described in this section has been operational since beginning of 2018. Together with the regular 2-hour experiments typically conducted at TMF as part of NDACC activities, regular 1-hour daytime measurements were carried out during forecasted overpasses in support of the validation of the ~~TROPOMI instrument onboard the S5P satellite.~~ TROPospheric Monitoring Instrument (TROPOMI) onboard the Sentinel-5 Precursor satellite. Unfortunately the TROPOMI ozone profile data product is still under development. For this reason, no comparisons are included in this work. In both cases, experiments were conducted in autonomous mode, independently if an operator was on-site or not. Table 1 provides an overview of the number of experiments conducted after TMTOL automation upgrade.

4 Near-range receivers

As part of the lidar upgrade, a new receiver for the retrieval of ozone profiles between 100 m and 1000 m AGL was built. Since this altitude range typically overlaps with the atmospheric boundary layer (~~ABL~~) and given that the typically high aerosol

Table 1. Number of experiments conducted during 2018 as part of the TROPOMI validation and NDACC activities. Measurements reported for September are only up to September 13.

Month	TROPOMI	NDACC
January	16	9
February	13	10
March	9	12
April	17	16
May	26	20
June	17	12
July	12	13
August	20	16
September	9	5

concentration found in this layer can affect the accuracy of the DIAL technique, a quantification of this effect and an evaluation of alternative solutions to mitigate it were conducted.

Equation 1 presents the different factors to be considered during the ozone retrieval process (Leblanc et al., 2016b)

$$N_{O_3}(z) = \frac{1}{\Delta\sigma_{O_3}} \left[\frac{\partial}{\partial z} \left(\ln \frac{P_{OFF}(z)}{P_{ON}(z)} \right) - \Delta\sigma_M N_a(z) - \left(\sum_{ig} \Delta\sigma_{ig}(z) N_{ig}(z) \right) - \Delta\alpha_p(z) + \Lambda\beta(z) + \Lambda\eta(z) + \Lambda Z(z) \right] \quad (1)$$

- 5 where N_{O_3} is the retrieved ozone number concentration, $\Delta\sigma_{O_3}$ is the differential absorption cross-section, P_{OFF} and P_{ON} are the number of photons collected by each detector after pile-up correction and background subtraction, $\Delta\sigma_M$ is the differential Rayleigh cross-section along the beam path up to altitude z and back, N_a is the air number density, $\Delta\sigma_{ig}$ is the differential cross-section along the beam path up to altitude z and back for the atmospheric constituent ig , N_{ig} is the number concentration of the constituent ig , $\Delta\alpha_p$ is the extinction differential due to particles and computed along the beam path up to altitude z and back, $\Lambda\beta$ is the effect of the difference in the atmospheric backscatter coefficient between both DIAL wavelengths, $\Lambda\eta$ represents the effect of the difference in efficiency of both receivers and ΛZ represents the effect of timing differences between both DIAL channels.

- Proposed solutions for the correction of the aerosol effects include the dual DIAL (Kovalev and Bristow, 1996) (Kovalev and Bristow, 1996) and the Raman DIAL (McGee et al., 1993) techniques, as well as aerosol corrections based on the assumption of aerosol properties (e.g. Eisele and Trickl, 2005). In the first case, three different wavelengths to create two DIAL pairs are needed. This could be achieved by using remaining pump, first and second Stokes wavelengths coming out from one of the two Raman cells. Although this might be an attractive idea, this would require a reoptimization of the Raman cells to increase the amount of pump power converted to second Stokes. This reoptimization would require lowering the cell pressure (Haner and McDer-

mid, 1990) and will have as secondary effect the reduction on the first Stokes conversion efficiency. This will, in turn, reduce the accuracy of the mid and long range channels. As an alternative, the two DIAL wavelengths and the remaining pump of one of the cells could be used. In this case, since two different beams would have to be received, the overlap function of the channels would vary independently after system alignment, making difficult to achieve unbiased measurements at very short ranges. Additionally, it has to be mentioned that although dual DIAL measurements help to reduce the systematic error caused by the aerosol influence on the retrieval, it is at the expense of increasing the overall statistical uncertainty on the ozone retrieval (Kovalev and Bristow, 1996; Wang et al., 1997; Alvarez et al., 2011) (Wang et al., 1997).

On the other hand, the Raman DIAL technique, as in the case of dedicated aerosol Raman lidars, make use of the atmospheric Raman scattering by nitrogen or oxygen to retrieve aerosol extinction profiles. Based on this, a correction for the extinction and backscatter differential between DIAL wavelengths can be calculated. Because the daytime operation is important for the validation satellite-borne ozone instruments and ~~given that the Raman scattering from atmospheric oxygen and nitrogen is more than considering the low intensity of the Raman scattering (about two orders of magnitude smaller than the Rayleigh scattering, lower than Rayleigh scattering)~~ the use of wavelengths in the blind region of the solar spectrum is preferred. This discards the possibility of using Raman scattering stimulated by the standard DIAL wavelengths used by TMTOL (288.9 nm and 299.1 nm), and limits the application of the Raman DIAL technique to the vibrational Raman scattering of nitrogen (283.6 nm) and oxygen (277.5 nm) induced by the non-converted 266 nm energy leaving the Raman cells.

The measurements performed at the output of both Raman cells showed a remaining 266 nm pulse power of about 2 mJ on each side. Considering that the system reported by Lazzarotto et al. (2001) used a 266 nm laser with a pulse power of 120 mJ, a repetition rate of 10 Hz and a 20-cm-diameter telescope to provide 5 percent accuracy ozone profiles up to 700 m, a quick estimation indicates that the available 266 nm power would not meet the range requirements previously mentioned while keeping a reasonable size receiver and similar accuracy and averaging time as the previously mentioned study. Although using the already existing 0.91-m-diameter telescope receiver would have increased by a factor of 20 the received power, achieving full overlap at altitudes as low as 100 m would have required major modifications on the system.

As an alternative to the previously mentioned approaches, a standard DIAL receiver based on the 266/288.9 nm wavelength pair and a small 50-mm-diameter refractive telescope was implemented. Although the use of the 266 nm laser wavelength is typically discourage for ozone DIALs due to the very high ozone absorption at this wavelength, this doesn't pose a limitation in this case, where only a short range is covered. Among available wavelength pairs (Fig. 34), the 266/288.9 nm pair is the one that maximizes the $\Delta\sigma_{O_3}/\Delta\lambda$ ratio. The high absorption represents an advantage as it improves the accuracy of the DIAL retrieval for a given signal-to-noise ratio (SNR), reduces the impact of aerosols on the retrieval and the use of the output corresponding to only one Raman cell makes the alignment process easier as it helps to reduce the overlap difference between the two channels. Furthermore, this wavelength pair minimizes the cross-sensitivity with SO_2 compared with the other available pairs, and has a smaller cross-sensitivity with NO_2 than the 288.9/299.1 nm pair.

Figure 4-5 presents a comparison of the error introduced in the ozone retrieval as a function of the selected wavelength pair and aerosol Ångström exponent for a given aerosol distribution. The aerosol distribution corresponds to an optical depth (OD) of 0.1 assuming a lidar ratio of 70 sr. Given that the total-column OD rarely goes above 0.1 at TMF (based on AERONET

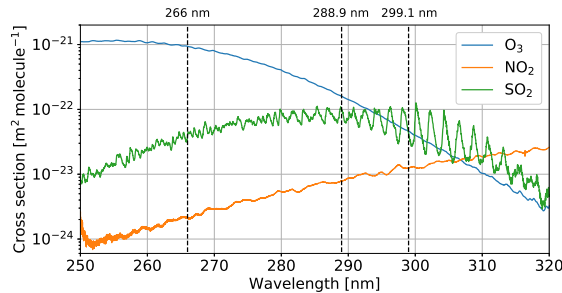


Figure 4. Absorption cross section for ozone (blue), nitrogen dioxide (green) and sulfur dioxide (orange) in the UV region of the spectrum (300 K; 775 hPa). Wavelengths transmitted by TMTOL are also shown (back, dashed)

[Aerosol Robotic Network](#) data) and considering that the proposed aerosol distribution contains a strong gradient between 400 m and 500 m, the results obtained from this estimations can be considered a worst case scenario for typical operation conditions. The results are compatible with the analysis based on the $\Delta\sigma_{O_3}/\Delta\lambda$ ratio. The largest rejection to aerosol influence is obtained by the 266/288.9 nm wavelength pair, with a maximum deviation of less than 20 percent for an Ångström exponent equal to 0 and a typical ozone concentration of $1 \times 10^{18} \text{ m}^{-3}$. In the case of a more typical Ångström exponent of 1, the deviation is reduced to 10 percent, assuming the same ozone concentration. [Furthermore, under the presence of atypically high aerosol loads \(e.g. wildfire smoke\), the aerosol influence in the retrieval might be further reduced by applying an aerosol correction algorithm \(Immler, 2003; Alvarez et al., 2011; Kuang et al., 2011; Sullivan et al., 2014\).](#)

Since only short ranges are covered by this receiver (Fig. 56), a 45:55 pellicle beamsplitter (Thorlabs BP145B5) is used to divide the received power and send it to each of the receivers. Although this means losing half the received power, the use of a pellicle beamsplitter reduces the difference in the optical path of each receiver compared to a traditional thick beamsplitter, and thus, minimizes the difference in the overlap function between receivers. The 288.9 nm receiver arm uses a 2-inch 288.9 nm band-pass filter (1 nm full width at half maximum (FWHM)) to block solar light and the 266 nm DIAL wavelength. The 266 nm receiver uses a stack of two off-the-shelf 1-inch band-pass filters, a 10 nm FWHM filter that blocks most of the incoming solar radiation followed by a 1 nm FWHM that increases the rejection of the solar background and the 288.9 nm wavelength. After filtering, the beams are focused over the surface of H11901P-113 Hamamatsu photomultiplier tubes (PMTs), giving place to an image of about 2 mm diameter for far-field radiation. Because both cells output non-converted 266 nm laser radiation, the laser and acquisition triggering was modified to interleave the pulses of each of the DIAL wavelength pairs. This eliminates possible cross-talk between DIAL receivers.

The signals generated by the PMTs are fed into two Licel TR20-16 transient recorders modules (photon-counting and 16-bit analog detection). Because measurements between 100 m and 1000 m AGL require a receiver with a dynamic range of about 30 dB, the combination of analog and photon counting detection allows to obtain a good compromise between accuracy and averaging time. First tests conducted with the receiver setup previously described showed strong oscillations in the first bins of the analog detection channels that compromised their use. In order to investigate the causes for this issue, artificial

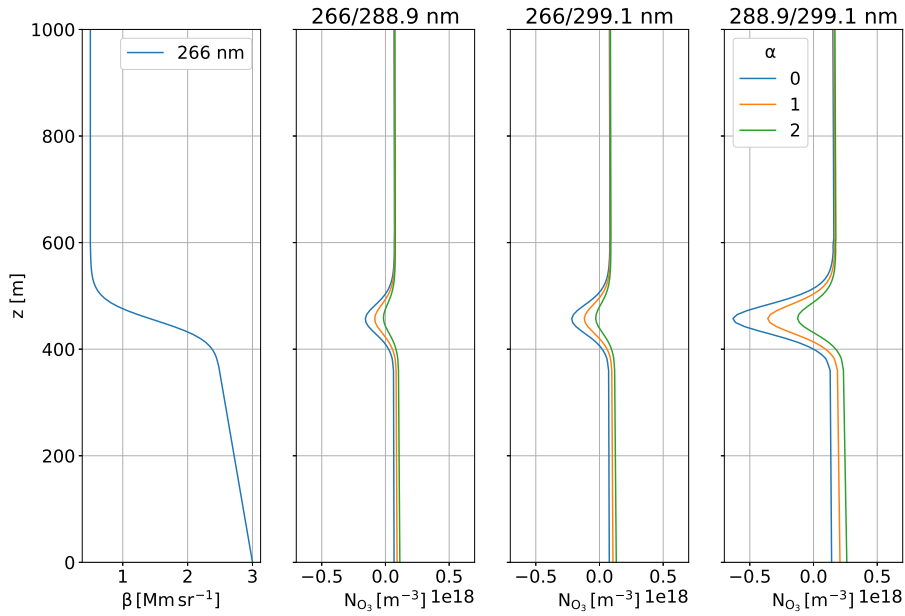


Figure 5. Aerosol error contribution (differential backscatter and extinction contributions) based for the different available DIAL wavelength pairs and three different Ångström exponents (α).

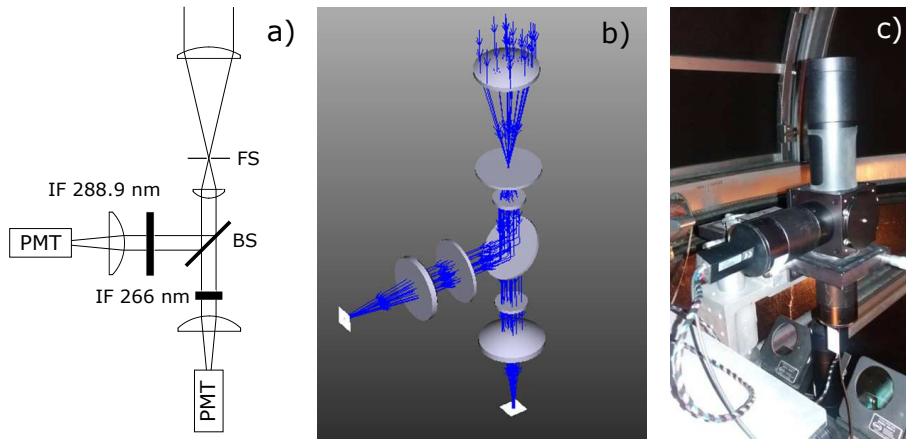


Figure 6. a) Scheme of the new very-near-range receivers. BS is a pellicle beam splitter, IF are interference filters and PMT are photomultipliers. b) Photo of the actual setup. Motor-controlled mirrors corresponding to the main wavelength pair of the system (288.9/299.1 nm) are shown on the bottom.

signals with similar slew-rate (750 kV s^{-1}) to the ones generated by the receiver were fed to the Licel transient recorders. The results showed the same oscillations, indicating ~~the-the~~ that the problem is most likely associated with the anti-aliasing filter in conjunction with the high slew-rate signals generated by the laser pulses entering ~~on~~ the receiver field of view at very low altitudes. Based on these tests, the receiver alignment was modified to reduce the received signal slew-rate and thus, minimize the impact of this issue.

Along with the dynamic range consideration mentioned before, the retrieval of very-near-range measurements typically involve a careful optical design in order to achieve full overlap at low altitudes while minimizing the system field of view and associated solar background. Since any range dependent difference between the efficiency of each of both receiver arms will be directly translated into a source of error during the retrieval process, special care has to be taken with regard to differences in the optical paths, inhomogenities on the PMTs surface sensitivities, timing and linearity of the transient recorders.

As part of the tests conducted on the Licel transient recorders, a sine wave generated by a signal generator was fed into both transient recorders via a T and a set of matched length cables. Signals triggering the signal generator and each of the receivers were generated by a Quantum Composer 9250 pulse generator. The results show a relative trigger delay of 23 ns between the transient recorders ~~user-used~~ for this very-near-range receiver. In order to discard differences in the signals used to trigger each transient recorder, the common trigger input available in rack was used to trigger both transient recorders from the same trigger source. The results were consistent with the ones observed when triggering both transient recorders independently. Tests conducted along several days showed no change in the relative delay. Although this delay represents only about half sampling bin, the DIAL technique is very sensitive to relative delays between on and off sides, especially at very short ranges (Kuang et al., 2013). It can be shown that the effect of a delay between the trigger of both DIAL channels ΔZ can be written

$$\Delta Z(z) = 2 \frac{\partial}{\partial z} \left[\ln \left(1 + \frac{\Delta R}{z} \right) \right] \quad (2)$$

where ΔR is the shift in meters of the on channel with respect to the off channel.

Figure 6-7 shows the error generated as a function of the range for a set of delays between the on and the off channels of the 266/288.9 nm wavelength pair.

As can be seen, for the delay observed between the two transient recorders (23 ns or 3.45 m), an overestimation of about $0.5 \times 10^{18} \text{ m}^{-3}$ is introduced. For a typical concentration of $1 \times 10^{18} \text{ m}^{-3}$, this represents an overestimation in the ozone concentration of about 50 percent at 100 m. By introducing a relative delay between the trigger signals of both transient recorders, this error source was eliminated.

After correcting the effects of the relative trigger delay, and in order to further investigate the systematic error sources of the receiver, an estimation of the differential efficiency was performed. The differential efficiency condenses a set of different error

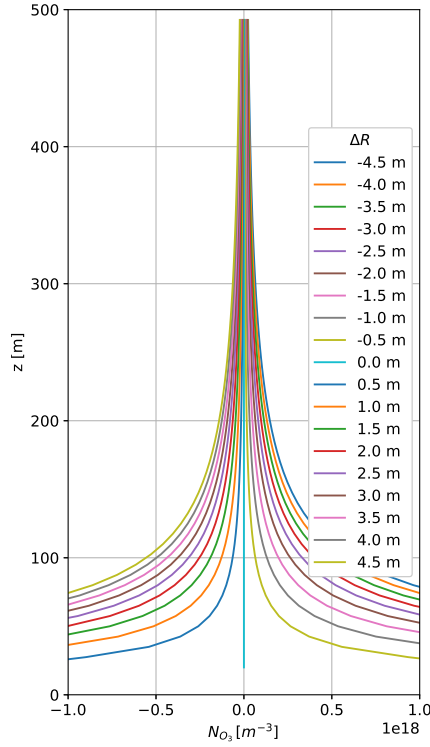


Figure 7. Error generated as a function of the delay ΔR between the 266 nm and the 288.9 nm channels. Positive delays correspond to the 266 nm channel being triggered after the 288.9 nm channel. A typical ozone concentration is about $1 \times 10^{18} \text{ m}^{-3}$.

sources, including differences in the receiver arm overlap functions, PMT surface sensitivities, PMT and transient recorder linearity, among others. The differential efficiency contribution to the ozone retrieval can be written as

$$\Lambda\eta(z) = \frac{\partial}{\partial z} \left(\ln \frac{\eta_{OFF}(z)}{\eta_{ON}(z)} \right) \quad (3)$$

where η is the efficiency of each receiver arm.

- 5 In order to evaluate the actual contribution of differential efficiency ($\Lambda\eta$) to the retrieval accuracy, a set of tests replacing the 266 nm interference filter by a second 1-inch 288.9 nm interference filter was conducted. Because the power of the transmitted 288.9 nm beam is about 10 times larger than the one of the 266 nm beam, an OD1 filter was added on the 266 nm arm in order

to achieve a signal with a similar intensity. Since the wavelength received by each receiver arm is the same in this configuration, it can be shown that

$$k_{inst} \frac{\eta_{OFF}(z)}{\eta_{ON}(z)} = \frac{P_{OFF}(z)}{P_{ON-288.9}(z)} \quad (4)$$

where k_{inst} is a constant that condenses all range-independent instrumental parameters (i.e. transmitted power, optical efficiency), $P_{ON-288.9}$ is the power received on the 266 nm detector when the 266 nm IF filter is replaced by a 288.9 nm filter. Replacing Eq. 4 in Eq. 3

$$\Lambda\eta(z) = \frac{\partial}{\partial z} \left(\ln \frac{P_{OFF}(z)}{P_{ON-288.9}(z)} \right) \quad (5)$$

The result of the test conducted with this configuration is presented in Fig. 78. The profiles were retrieved based on a 20 minutes measurement during daytime. The derivative of the logarithm is calculated with a fourth-order Savitsky-Golay derivative filter and a window length of 9 samples for the analog detection mode and 31 samples for the photon-counting mode.

As can be seen, the differential efficiency contribution of the analog pair is very close to zero for altitudes above 50 m AGL, while for the case of photon-counting channels, no differential efficiency effects are observed above 200 m AGL. The difference observed between analog and photon-counting channels can be attributed to the non linearity of the photon-counting channels at high count-rates due to pile-up effect.

5 System validation

5.1 Validation with tethered-balloon

As part of the validation efforts of the new very-near-range channels, a set of measurements by an ozonesonde tethered system were carried out. This experiment was intended to provide a link between surface ozone measurements available at TMF (Thermo Scientific Model 49i) and the first valid data-points of the new receiver (about 100 m AGL). In this way, the minimum achievable range and accuracy of the new setup can be determined. The ozone measurement system consists of an iMet-1 radiosonde and an EN-SCI ~~ECC~~ Electrochemical concentration cell (ECC) ozonesonde tied to a balloon and driven by a winder/unwinder system built by ~~NOAA~~ the National Oceanic and Atmospheric Administration (Schnell et al., 2016). This setup provides vertical profiles of pressure, temperature, humidity, GPS position and ozone concentration up to altitudes of about 200 m AGL (2485 m ASL). The profiles corresponding to one of the tests carried out as part of the validation process on June 7 are shown in Fig. 89. As can be seen, there is a very good agreement (mostly less than 5 % difference) between the sonde and the lidar as well as between the sonde and the surface ozone measurements. Lidar retrievals look unbiased down to about 70 m AGL (2355 m ASL), with some deviations (less than 10 %) between 70 m AGL and 100 m AGL (2355 m ASL and 2385 m ASL). These deviations might have different causes, like aerosol contamination or electronic noise.

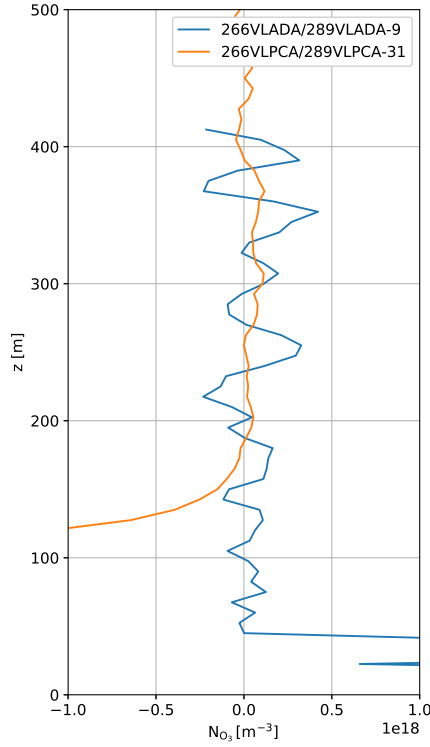


Figure 8. Error of the new very-near-range receiver as a result of the differential efficiency $\Delta\eta(z)$ using photon-counting (solid, orange) and analog detection mode (solid, blue). A typical ozone concentration is about $1 \times 10^{18} \text{ m}^{-3}$.

The lidar measurements correspond to 1 hour average (19:58-20:58 UT), while the sonde measurements were conducted for about 30 minutes (19:45-20:15 UT). For the lidar retrieval between ground and 2600 m AGLASL, a 17-sample Savitsky-Golay derivative filter was used, giving place to a 52 m vertical resolution following the definitions presented in Leblanc et al. (2016a). Above 2600 m ASL, the vertical resolution decreases to 200 m. Uncertainties are provided according to the definitions presented in Leblanc et al. (2016b).

In the first 15 m AGL (2300 m ASL), the sonde measurements indicate an increasing ozone concentration with respect to the measurements conducted at surface level. This variation in the ozone concentration was observed repeatedly during the tethered-balloon validation process, suggesting that a comparison between the first valid lidar point and surface measurements might not always be a good validation approach. This result is compatible with previous studies conducted in forested areas

(Gerosa et al., 2017; Makar et al., 2017).

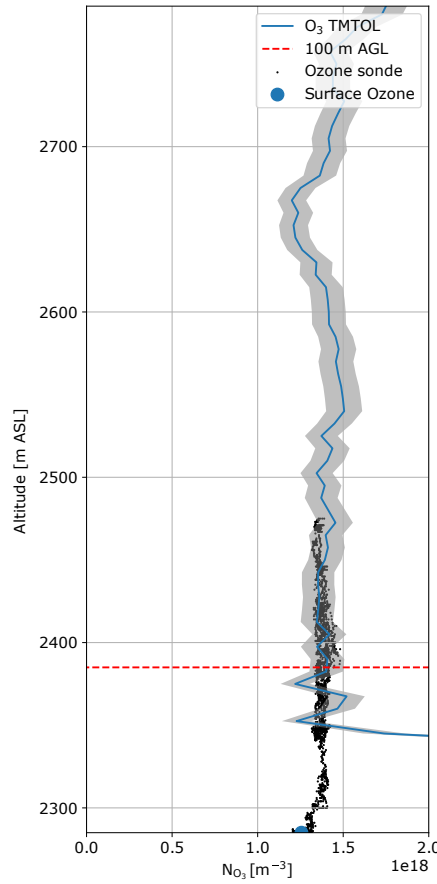


Figure 9. Comparison between the TMTOL very-near-range receiver retrieval (solid, blue), an ozonesonde tethered system (dots, black) and a surface ozone monitor (dot, blue). Lidar retrieval $1 - \sigma$ uncertainty is shown (gray, shaded).

While regular tethered balloon experiments would have provided further confidence on the receiver accuracy and minimum achievable range, tethered balloon operations demonstrated to be difficult at TMF due to relative scarce low-wind conditions and the high amount of trees surrounding the site.

5.2 May 25th: 24h case-study

- 5 In the frame of the system upgrade validation, a 24-hour run (25-05-2018 1:00 UT to 26-05-2018 1:00 UT) was conducted during a forecasted stratospheric intrusion. During the experiment, two sets of ozone EN-SCI ECC ozonesonde, i-Met 1 and Vaisala RS-41 radiosondes were launched to validate the retrievals of the very-near-range channels.

In order to provide a general overview of the synoptic meteorological situation during the stratospheric intrusion event analyzed in this section, MERRA-2 reanalysis ozone concentration, humidity and winds are shown in Fig 9-10 for two different

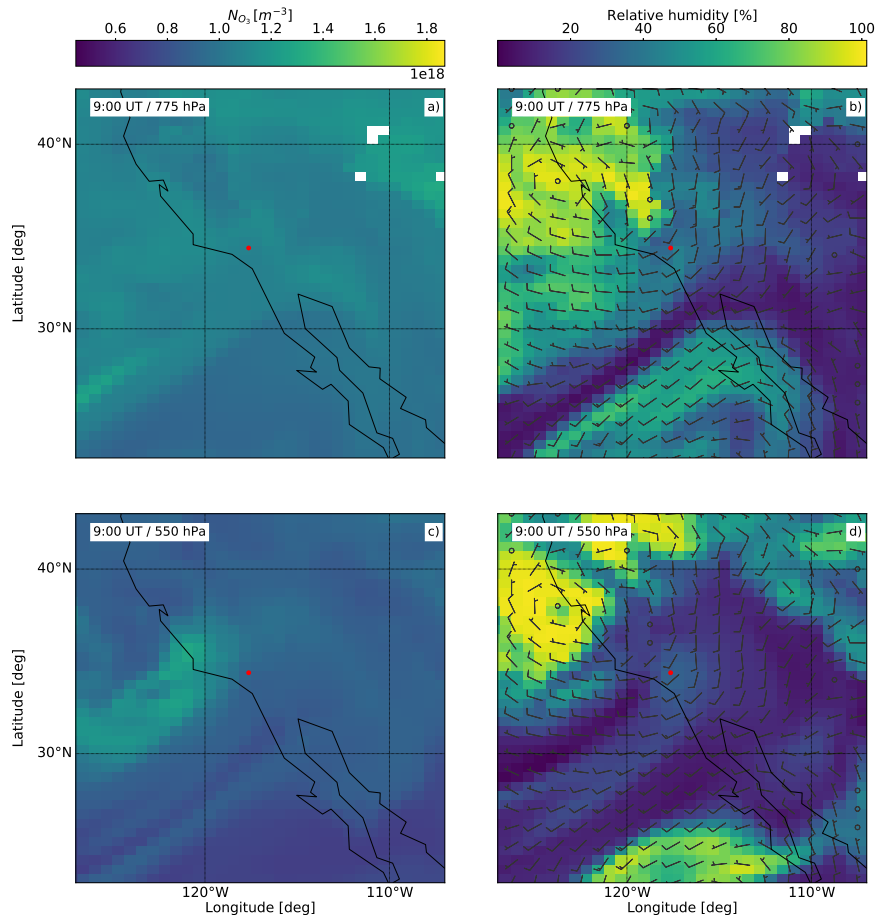


Figure 10. MERRA-2 reanalysis at 9:00 UT on 25 May 2018 for two different pressure levels (775 hPa and 550 hPa). a,c) Ozone number concentration. b,d) Relative humidity and wind speed/direction. TMF site location is indicated with a red dot.

model levels (775 hPa and 550 hPa) at 9:00 UT. The 775 hPa model level corresponds approximately to the TMF site surface, while the 550 hPa level corresponds approximately to an altitude of 5 km ASL. The general synoptic situation was dominated by a cyclonic system in the north and an anti-cyclone in the south. Ozone concentration at 775 hPa shows only slight spatial variations around TMF, while at 550 hPa, an ozone-rich dry plume associated with the stratospheric intrusion can be seen approaching TMF from the west.

Retrieved ozone concentration profiles in the lower troposphere for this intensive measurement period are shown in Fig. 4011a, together with a detailed view of the first 500 m AGL (Fig. 4011b) and a comparison with a collocated-co-located surface ozone measurement unit (Fig. 4011c). These retrievals correspond to the merging of the new very-near-range channels and the preexisting mid-range channels. Between 2355 m and 2600 m ASL, retrievals are based on the analog channels of the very-near-range receiver (52 m vertical resolution), while between 2550 m and 3185 m ASL are based on the photon-counting channels (200 m vertical resolution). Finally, above 3085 m and up to 6000 m ASL, the retrieval corresponds to the mid-range

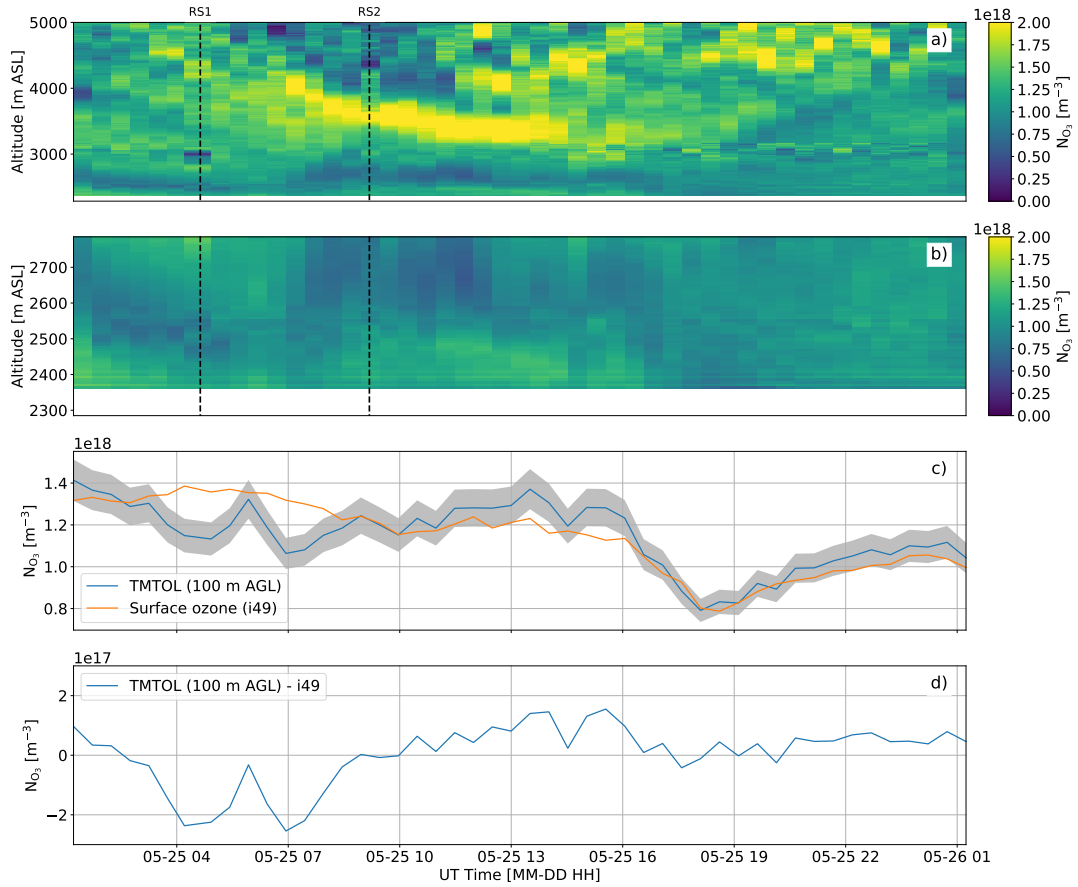


Figure 11. Experiment result overview. a) Ozone number concentration between ground level and 5000 m. b) Detail of the first 500 m AGL ([2785 m ASL](#)) acquired with the new very-near-range receiver. c) comparison between the [co-located Thermo Scientific Model 49i](#) surface ozone measurements and the lidar retrieval at 100 m AGL ([2385 m ASL](#)), together with $1 - \sigma$ uncertainty. d) [difference between the lidar retrieval at 100 m AGL \(2385 m ASL\) and the surface ozone meter \(i49\)](#).

receivers (380 m vertical resolution). In the overlap region between the very-near-range and the mid-range receiver, the mean is presented. The temporal resolution is 30 minutes.

A first qualitative comparison indicate a good agreement between the top of the very-near-channel and the bottom of the mid-range channels as well as between the 100 m AGL ([2385 m ASL](#)) lidar retrieval and the surface ozone measurements

[carried out by the co-located Thermo Scientific Model 49i](#). Although this doesn't provide a full validation of the new channel, it provides further confidence to the tests performed with the tethered balloon system and presented in the previous subsection.

The high ozone concentration visible in Fig. [4-11a](#) above 3000 m [ASL](#) is in qualitative agreement with a stratospheric intrusion event and with the forecast/reanalysis provided by the models. Below the intrusion, a thin layer of about 200 m depth characterized by a relatively low ozone concentration can also be recognized. Since this kind of fine structures are typically not reproduced by operational models and since they provide valuable information to evaluate the performance of the receiver, a comparison between the lidar retrieval and the two ozonesondes launched during the experiment is presented in Fig. [4-12](#). This will allow to determine whether or not this corresponds to a real feature and what is the expected accuracy of the new receiver.

Figure [4-12](#) presents the intercomparison between the two ozone sondes and the lidar-retrieved ozone profiles. Potential temperature, humidity and wind profiles retrieved by the radiosonde are also shown. During the launch of this first sonde (4:40 UT), no strong signature of the atmospheric intrusion was visible neither in the lidar nor in the ozone sonde. A general good agreement between the lidar- and the sonde-retrieved ozone profile is visible in Fig. [4-12a](#). In the very-near range, the thin layer of low ozone concentration visible in Fig. [4-11](#) can be found between 100 m and 200 m AGL ([2385 m and 2485 m ASL](#)), while in the case of the sonde, a thicker and less pronounced layer of low ozone concentration was observed between 200 m and 700 m AGL ([2485 m and 2985 m ASL](#)). As can be seen in Fig. [4-12b](#), this [low ozone](#) layer sits on top of a well mixed layer ([no vertical gradient in the potential temperature](#)) that extends up to 120 m AGL ([2405 m ASL](#)) and is trapped between two inversions. The relative high humidity of this layer, of up to about 40%, suggests that it might be a stable marine air layer advected from the ocean over TMF.

In contrast to the previous case, the retrievals corresponding to the second launch (9:11 UT) show a strong signature of the stratospheric intrusion on both, the lidar and the sonde retrievals. While the lidar shows the intrusion maximum ozone concentration at 3.8 km ASL, the sonde shows it at about 4.2 km ASL. The magnitude of the ozone concentration is also different, with the sonde showing a peak value of about $1.8 \times 10^{18} \text{ m}^{-3}$ and the lidar $2.3 \times 10^{18} \text{ m}^{-3}$. This difference can be attributed to different causes, including ozone spatiotemporal variability combined with the sonde drift and differences between the vertical resolution of the sonde and the lidar. Compared to the previous case, the lidar shows a better agreement with the surface ozone measurement and the sonde in the first hundreds of meters. The thin low ozone concentration layer observed by the lidar and the first launched sonde was also observed during the second launch. Nevertheless, in this case, the agreement between the lidar and the sonde is much better regarding both, its vertical extension and ozone concentration. As in the previous case, this thin layer is trapped between two inversions and has a high relative humidity. HYSPLIT backward trajectories calculated for this layer (not shown) confirmed the marine origin of this layer.

5.3 Long-term stability

Since optical stability is a key factor in order to obtain reliable unbiased measurements in the very-near range, a [preliminary](#) long-term comparison between the first valid lidar data point (100 m AGL) and the [co-located](#) surface ozone meter deployed at TMF was conducted. The results, corresponding to a period of 2 months between 13 July and 12 September 2018,

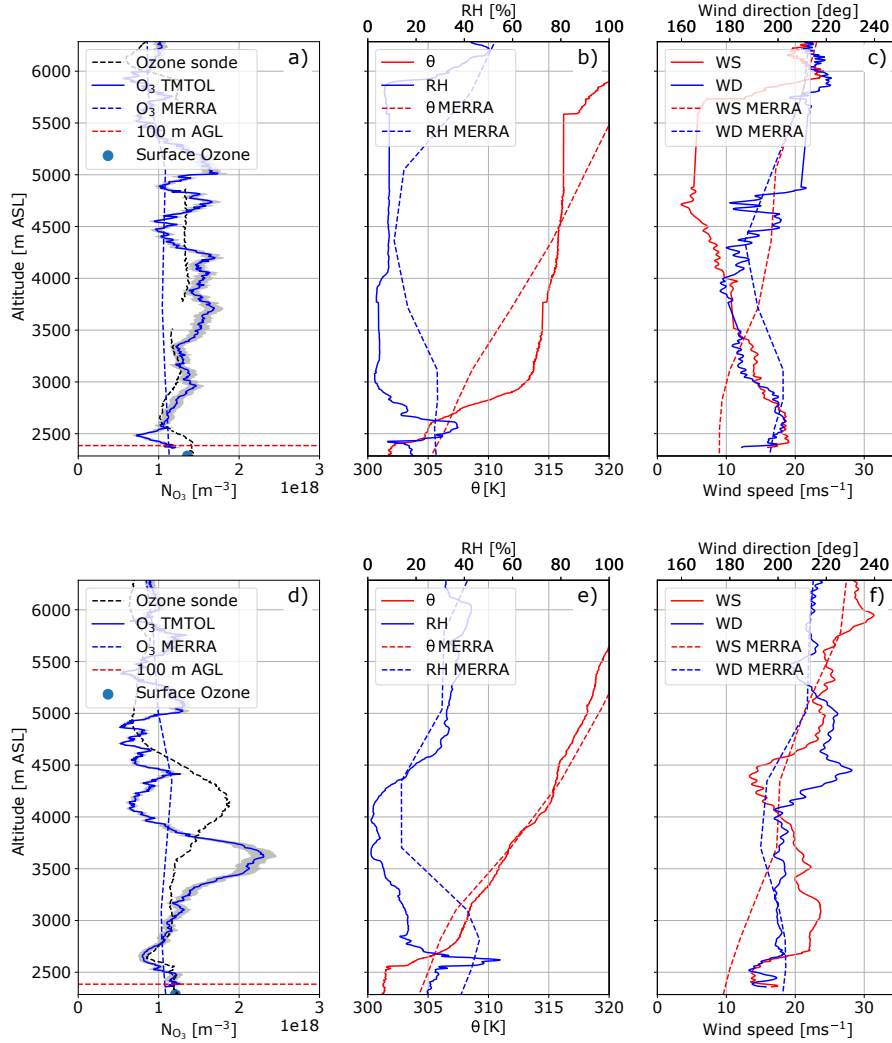


Figure 12. Comparison between the retrieved lidar ozone profile (together with $1 - \sigma$ uncertainty), ~~collocated~~co-located radiosondes, surface ozone meter and MERRA-2 reanalysis at the time of the first (upper row, 4:40 UT) and second launch (lower row, 9:10 UT). a,d) Lidar ozone profile (solid, blue), ozone sonde profile (dashed, black), MERRA-2 ozone concentration and surface ozone measurements (light blue). b,e) Radiosonde potential temperature (solid, red), MERRA-2 potential temperature (dashed, red), radiosonde relative humidity (solid, blue) and MERRA-2 relative humidity (dashed, blue). c,f) Radiosonde wind speed (solid, red), MERRA-2 wind speed (dashed, red), radiosonde wind direction (solid, blue) and MERRA-2 wind direction (dashed, blue).

are presented in Fig. ~~12~~13. A good correlation between these two quantities is observed, with consistent ~~10~~7.2% lower values recorded by the surface ozone meter compared to the lidar. A similar difference was observed during the tethered balloon validation experiments (Fig. ~~89~~9) and is mentioned in different works conducted on very-near ground zone vertical profiles as being related to ozone depletion in the first few meters above ground (Fontan et al., 1992). As additional validation, a similar

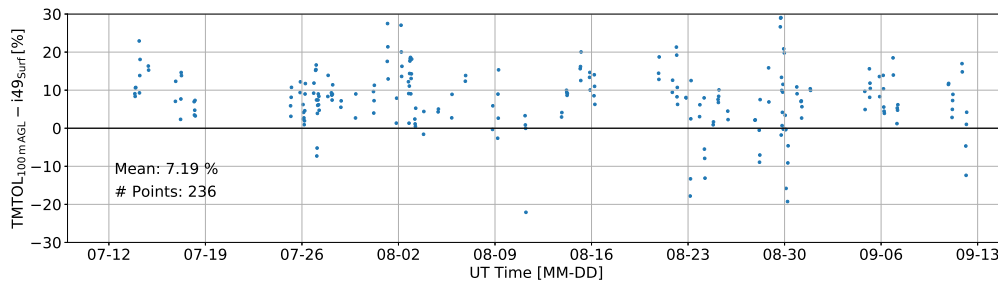


Figure 13. Relative difference between the first valid lidar data point (100 m AGL) and the ~~co-located~~ co-located i49 surface ozone meter for the period comprehended between 13 July and 12 September 2018. Each point corresponds to a 30 minute average.

comparison was conducted between the historical ozone sonde profile record from TMF and available ~~co-located~~ co-located surface ozone measurements. The result of this comparison show a very similar difference of about 5-10% between ozone sonde measurements at 100 m AGL and surface ozone measurements (not shown).

6 Conclusions

- 5 As part of the efforts conducted at TMF to provide accurate and regular measurements for satellite validation and process analysis purposes, a set of modifications were introduced in the TMTOL system. As a result, the system is now capable of performing measurements autonomously from about ~~70 m~~ 100 m AGL up to about 15 km.

Since the start of the autonomous operations to September 12th 2018, 139 1-hour measurement periods during TROPOMI overpasses were acquired. This extensive dataset not only provides valuable information for the analysis and evaluation of
 10 TROPOMI retrievals, but also demonstrates the potential of autonomous operations for the validation of the upcoming TEMPO mission. Additionally, based on this experience, lidar hardware and automation algorithms developed as part of TMTOL automation upgrade are expected to be implemented on the other TMF lidars (a stratospheric ozone lidar and a water vapor Raman lidar), allowing schedule-based autonomous operations for all three TMF lidars.

In order to overcome the issues associated with the tethered balloon operations at TMF, there are plans underway to deploy
 15 an ozone monitor on an unmanned aerial vehicle to provide further validation data for the very-near-range receiver as well as to investigate the lowermost ~~70 m~~ 100 m AGL, not covered by the new receiver.

Finally, another upgrade to include aerosol measurement capability is currently being developed. Such upgrade would allow to better characterize the distribution and properties of the aerosols typically found over TMF and thus, better determine to which extent this might affect the ozone retrievals.

- 20 *Data availability.* Part of the lidar data used for this study is publicly available at TOLNet (<https://www-air.larc.nasa.gov/missions/TOLNet/>) and NDACC (<http://www.ndacc.org/>) websites. For additional data or information please contact the authors.

Competing interests. The authors declare that they have no conflict of interest.

Acknowledgements. The work described here was carried out at the Jet Propulsion Laboratory, California Institute of Technology, under agreements with the National Aeronautics and Space Administration. The authors acknowledge funding from the Tropospheric Chemistry
5 Program of the NASA Earth Science and Division. The authors would like to thank Andy Langford for the fruitful discussion on the stratospheric intrusion event presented in this work. The authors further thank the MERRA-2 team for providing the data used in this study.

References

- Aggarwal, M., Whiteway, J., Seabrook, J., Gray, L., Strawbridge, K., Liu, P., O'Brien, J., Li, S.-M., and McLaren, R.: Airborne lidar measurements of aerosol and ozone above the Canadian oil sands region, *Atmospheric Measurement Techniques*, 11, 3829–3849, <https://doi.org/10.5194/amt-11-3829-2018>, <https://www.atmos-meas-tech.net/11/3829/2018/>, 2018.
- Alvarez, R., Senff, C., Langford, A., Weickmann, A., Law, D., Machol, J., Merritt, D., Marchbanks, R., Sandberg, S., Brewer, W., et al.: Development and application of a compact, tunable, solid-state airborne ozone lidar system for boundary layer profiling, *Journal of Atmospheric and Oceanic Technology*, 28, 1258–1272, 2011.
- Eisele, H. and Trickl, T.: Improvements of the aerosol algorithm in ozone lidar data processing by use of evolutionary strategies, *Applied optics*, 44, 2638–2651, 2005.
- Engelmann, R., Kanitz, T., Baars, H., Heese, B., Althausen, D., Skupin, A., Wandinger, U., Komppula, M., Stachlewska, I. S., Amiridis, V., et al.: The automated multiwavelength Raman polarization and water-vapor lidar Polly XT: the neXT generation, *Atmospheric Measurement Techniques*, 9, 1767–1784, 2016.
- Farris, B. M., Gronoff, G. P., Carrion, W., Knepp, T., Pippin, M., and Berkoff, T. A.: Demonstration of an off-axis parabolic receiver for near-range retrieval of lidar ozone profiles, *Atmospheric Measurement Techniques Discussions*, 2018, 1–11, <https://doi.org/10.5194/amt-2018-178>, <https://www.atmos-meas-tech-discuss.net/amt-2018-178/>, 2018.
- Fontan, J., Minga, A., Lopez, A., and Druilhet, A.: Vertical ozone profiles in a pine forest, *Atmospheric Environment. Part A. General Topics*, 26, 863–869, 1992.
- Gerosa, G., Marzuoli, R., Monteleone, B., Chiesa, M., and Finco, A.: Vertical ozone gradients above forests. Comparison of different calculation options with direct ozone measurements above a mature forest and consequences for ozone risk assessment, *Forests*, 8, 337, 2017.
- Haner, D. A. and McDermid, I. S.: Stimulated Raman shifting of the Nd:YAG fourth harmonic (266 nm) in H₂, HD, and D₂, *IEEE Journal of Quantum Electronics*, 26, 1292–1298, <https://doi.org/10.1109/3.59670>, 1990.
- Horowitz, L. W.: Past, present, and future concentrations of tropospheric ozone and aerosols: Methodology, ozone evaluation, and sensitivity to aerosol wet removal, *Journal of Geophysical Research: Atmospheres*, 111, 2006.
- Hu, X.-M., Doughty, D. C., Sanchez, K. J., Joseph, E., and Fuentes, J. D.: Ozone variability in the atmospheric boundary layer in Maryland and its implications for vertical transport model, *Atmospheric Environment*, 46, 354–364, 2012.
- Immler, F.: A new algorithm for simultaneous ozone and aerosol retrieval from tropospheric DIAL measurements, *Applied Physics B*, 76, 593–596, 2003.
- Kovalev, V. A. and Bristow, M. P.: Compensational three-wavelength differential-absorption lidar technique for reducing the influence of differential scattering on ozone-concentration measurements, *Applied optics*, 35, 4790–4797, 1996.
- Kuang, S., Newchurch, M., Burris, J., Wang, L., Buckley, P. I., Johnson, S., Knupp, K., Huang, G., Phillips, D., and Cantrell, W.: Nocturnal ozone enhancement in the lower troposphere observed by lidar, *Atmospheric environment*, 45, 6078–6084, 2011.
- Kuang, S., Newchurch, M. J., Burris, J., and Liu, X.: Ground-based lidar for atmospheric boundary layer ozone measurements, *Applied optics*, 52, 3557–3566, 2013.
- Langford, A., Senff, C., Alvarez, R., Banta, R., Hardesty, R., Parrish, D., and Ryerson, T.: Comparison between the TOPAZ airborne ozone lidar and in situ measurements during TexAQS 2006, *Journal of Atmospheric and Oceanic Technology*, 28, 1243–1257, 2011.

- Langford, A., Alvarez, R., Brioude, J., Evan, S., Iraci, L., Kirgis, G., Kuang, S., Leblanc, T., Newchurch, M., Pierce, R., Senff, C., and Yates, E.: Coordinated profiling of stratospheric intrusions and transported pollution by the Tropospheric Ozone Lidar Network (TOL-Net) and NASA Alpha Jet experiment (AJAX): Observations and comparison to HYSPLIT, RAQMS, and FLEXPART, *Atmospheric Environment*, 174, 1 – 14, <https://doi.org/https://doi.org/10.1016/j.atmosenv.2017.11.031>, <http://www.sciencedirect.com/science/article/pii/S1352231017307768>, 2018.
- Lazzarotto, B., Frioud, M., Larchevêque, G., Mitev, V., Quaglia, P., Simeonov, V., Thompson, A., van den Bergh, H., and Calpini, B.: Ozone and water-vapor measurements by Raman lidar in the planetary boundary layer: error sources and field measurements, *Appl. Opt.*, 40, 2985–2997, <https://doi.org/10.1364/AO.40.002985>, <http://ao.osa.org/abstract.cfm?URI=ao-40-18-2985>, 2001.
- 10 Leblanc, T., Walsh, T. D., McDermid, I. S., Toon, G. C., Blavier, J.-F., Haines, B., Read, W. G., Herman, B., Fetzer, E., Sander, S., Pongetti, T., Whiteman, D. N., McGee, T. G., Twigg, L., Sumnicht, G., Venable, D., Calhoun, M., Dirisu, A., Hurst, D., Jordan, A., Hall, E., Miloshevich, L., Vömel, H., Straub, C., Kampfer, N., Nedoluha, G. E., Gomez, R. M., Holub, K., Gutman, S., Braun, J., Vanhove, T., Stiller, G., and Hauchecorne, A.: Measurements of Humidity in the Atmosphere and Validation Experiments (MOHAVE)-2009: overview of campaign operations and results, *Atmospheric Measurement Techniques*, 4, 2579–2605, <https://doi.org/10.5194/amt-4-2579-2011>,
15 <https://www.atmos-meas-tech.net/4/2579/2011/>, 2011.
- Leblanc, T., Sica, R. J., Van Gijssel, J. A., Godin-Beekmann, S., Haeferle, A., Trickl, T., Payen, G., and Gabarrot, F.: Proposed standardized definitions for vertical resolution and uncertainty in the NDACC lidar ozone and temperature algorithms–Part 1: Vertical resolution, *Atmospheric Measurement Techniques*, 9, 4029–4049, 2016a.
- Leblanc, T., Sica, R. J., van Gijssel, J. A. E., Godin-Beekmann, S., Haeferle, A., Trickl, T., Payen, G., and Liberti, G.: Proposed standardized
20 definitions for vertical resolution and uncertainty in the NDACC lidar ozone and temperature algorithms – Part 2: Ozone DIAL uncertainty budget, *Atmospheric Measurement Techniques*, 9, 4051–4078, <https://doi.org/10.5194/amt-9-4051-2016>, <https://www.atmos-meas-tech.net/9/4051/2016/>, 2016b.
- Levelt, P. F., Joiner, J., Tamminen, J., Veefkind, J. P., Bhartia, P. K., Stein Zweers, D. C., Duncan, B. N., Streets, D. G., Eskes, H., McLinden, C., et al.: The Ozone Monitoring Instrument: overview of 14 years in space, *Atmospheric Chemistry and Physics*, 18, 5699–5745, 2018.
- 25 Machol, J. L., Marchbanks, R. D., Senff, C. J., McCarty, B. J., Eberhard, W. L., Brewer, W. A., Richter, R. A., Alvarez, R. J., Law, D. C., Weickmann, A. M., et al.: Scanning tropospheric ozone and aerosol lidar with double-gated photomultipliers, *Applied optics*, 48, 512–524, 2009.
- Makar, P., Staebler, R., Akingunola, A., Zhang, J., McLinden, C., Kharol, S., Pabla, B., Cheung, P., and Zheng, Q.: The effects of forest canopy shading and turbulence on boundary layer ozone, *Nature communications*, 8, 15 243, 2017.
- 30 Mauzerall, D. L. and Wang, X.: Protecting agricultural crops from the effects of tropospheric ozone exposure: reconciling science and standard setting in the United States, Europe, and Asia, *Annual Review of Energy and the Environment*, 26, 237–268, 2001.
- McDermid, I. S., Haner, D. A., Kleiman, M. M., Walsh, T. D., and White, M. L.: Differential absorption lidar systems for tropospheric and stratospheric ozone measurements, *Optical Engineering*, 30, 30 – 30 – 9, <https://doi.org/10.1117/12.55768>, <https://doi.org/10.1117/12.55768>, 1991.
- 35 McDermid, I. S., Beyerle, G., Haner, D. A., and Leblanc, T.: Redesign and improved performance of the tropospheric ozone lidar at the Jet Propulsion Laboratory Table Mountain Facility, *Appl. Opt.*, 41, 7550–7555, <https://doi.org/10.1364/AO.41.007550>, <http://ao.osa.org/abstract.cfm?URI=ao-41-36-7550>, 2002.
- McGee, T. J., Gross, M., Ferrare, R., Heaps, W., and Singh, U.: Raman dial measurements of stratospheric ozone in the presence of volcanic aerosols, *Geophysical Research Letters*, 20, 955–958, <https://doi.org/10.1029/93GL00751>, <http://dx.doi.org/10.1029/93GL00751>, 1993.

- Moltchanov, S., Levy, I., Etzion, Y., Lerner, U., Broday, D. M., and Fishbain, B.: On the feasibility of measuring urban air pollution by wireless distributed sensor networks, *Science of The Total Environment*, 502, 537–547, 2015.
- Newchurch, M. J., Kuang, S., Leblanc, T., Alvarez, R. J., Langford, A. O., Senff, C. J., Burris, J. F., McGee, T. J., Sullivan, J. T., DeYoung, R. J., et al.: TOLNET—A Tropospheric Ozone Lidar Profiling Network for Satellite Continuity and Process Studies, in: *EPJ Web of Conferences*, vol. 119, p. 20001, EDP Sciences, 2016.
- Schnell, R. C., Johnson, B. J., Oltmans, S. J., Cullis, P., Sterling, C., Hall, E., Jordan, A., Helmig, D., Petron, G., Ahmadov, R., Wendell, J., Albee, R., Boylan, P., Thompson, C. R., Evans, J., Hueber, J., Curtis, A. J., and Park, J.: Quantifying wintertime boundary layer ozone production from frequent profile measurements in the Uinta Basin, UT, oil and gas region, *Journal of Geophysical Research: Atmospheres*, 121, 11,038–11,054, <https://doi.org/10.1002/2016JD025130>, <https://agupubs.onlinelibrary.wiley.com/doi/abs/10.1002/2016JD025130>, 2016.
- 10 Stocker, T.: *Climate change 2013: the physical science basis: Working Group I contribution to the Fifth assessment report of the Intergovernmental Panel on Climate Change*, Cambridge University Press, 2014.
- Strawbridge, K. B., Travis, M. S., Firanski, B. J., Brook, J. R., Staebler, R., and Leblanc, T.: A fully autonomous ozone, aerosol and night time water vapor LIDAR: a synergistic approach to profiling the atmosphere in the Canadian oil sands region, *Atmospheric Measurement Techniques Discussions*, 2018, 1–56, <https://doi.org/10.5194/amt-2018-108>, <https://www.atmos-meas-tech-discuss.net/amt-2018-108/>, 2018.
- 15 Su, W., Liu, C., Hu, Q., Fan, G., Xie, Z., Huang, X., Zhang, T., Chen, Z., Dong, Y., Ji, X., et al.: Characterization of ozone in the lower troposphere during the 2016 G20 conference in Hangzhou, *Scientific reports*, 7, 17 368, 2017.
- Sullivan, J., McGee, T., Sumnicht, G., Twigg, L., and Hoff, R.: A mobile differential absorption lidar to measure sub-hourly fluctuation of tropospheric ozone profiles in the Baltimore–Washington, DC region, *Atmospheric Measurement Techniques*, 7, 3529–3548, 2014.
- 20 Veefkind, J., Aben, I., McMullan, K., Förster, H., De Vries, J., Otter, G., Claas, J., Eskes, H., De Haan, J., Kleipool, Q., et al.: TROPOMI on the ESA Sentinel-5 Precursor: A GMES mission for global observations of the atmospheric composition for climate, air quality and ozone layer applications, *Remote Sensing of Environment*, 120, 70–83, 2012.
- Wang, Z., Nakane, H., Hu, H., and Zhou, J.: Three-wavelength dual differential absorption lidar method for stratospheric ozone measurements in the presence of volcanic aerosols, *Applied optics*, 36, 1245–1252, 1997.
- 25 WHO: *Health aspects of air pollution with particulate matter, ozone and nitrogen dioxide: report on a WHO working group*, Bonn, Germany 13-15 January 2003, 2003.
- Young, P., Archibald, A., Bowman, K., Lamarque, J.-F., Naik, V., Stevenson, D., Tilmes, S., Voulgarakis, A., Wild, O., Bergmann, D., et al.: Pre-industrial to end 21st century projections of tropospheric ozone from the Atmospheric Chemistry and Climate Model Intercomparison Project (ACCMIP), *Atmospheric Chemistry and Physics*, 13, 2063–2090, 2013.
- 30 Zoogman, P., Liu, X., Suleiman, R., Pennington, W., Flittner, D., Al-Saadi, J., Hilton, B., Nicks, D., Newchurch, M., Carr, J., et al.: Tropospheric emissions: Monitoring of pollution (TEMPO), *Journal of Quantitative Spectroscopy and Radiative Transfer*, 186, 17–39, 2017.