

## Referees' Comments to the Authors

### Reviewer 1

We thank Reviewer 1 for his/her constructive comments

Our responses and changes are given below in red; changes to the text are shown in bold

5

#### 1 Specific Comments

Abstract: the abstract is clearly summarizing the paper. However, I think than one important aspect of the paper is missing. This paper showed that the Lidar signal is affected when the external windows transmission is dropping below 90


10 **Line 20 changed from lidar pulse energy is low to lidar pulse energy falls below 90%**

Introduction: I 62-67. This paragraph is farfetched. A ceilometer is measuring attenuated backscatter that is not proportional to Ice Water Content. If there is a link between these quantities, please add an equation and the references to support your conclusion. If not, I would suggest I would suggest dropping this 10% requirement in the introduction and the section 5.2.

15 **New text (line 64) with references added for clarification: for example, Illingworth et al, (2019) show that a calibration accuracy of 10% is needed when deriving 'O-B' statistics obtained by comparing the observed ceilometer backscatter ('O') from Saharan dust with the forward modelled backscatter ('B') from the ECMWF CAMS model.**

20 **(line 69) In most models the ice particle density is usually assumed to be inversely proportional to particles size (e.g. Brown and Francis, 1995) so IWC is proportional to particle and for a given lidar ratio and small amounts of attenuation, the requirement is for a ceilometer calibration accurate to be 10%.**

25 The attached figure from Illingworth et al (2019) shows the O-B statistics for the ceilometer backscatter observed during a Saharan dust outbreak, and the forward modelled backscatter from the ECMWF CAMS model. The lower right hand panel shows that they agree to within 10% - this conclusion would not have been possible if the ceilometer were not calibrated to within 10%.

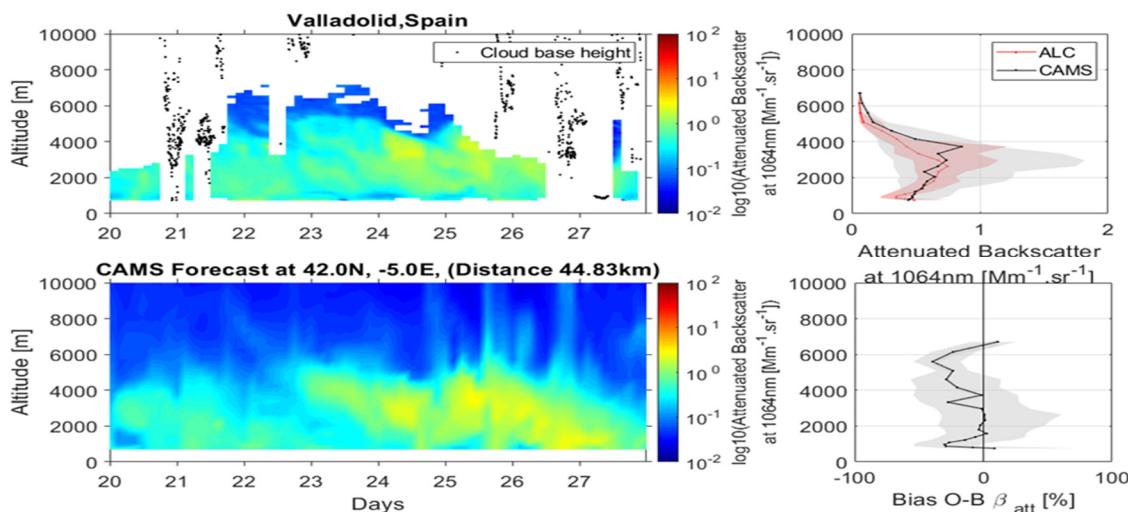

Section 3 line 204. This is a crucial part of your algorithm. To my understanding, it means that the calibration is valid only when the windows transmission and the energy are higher than 90%. Many instruments will be excluded by this criterion. Please perform a short sensitivity study on this criterion. Please also mention that your calibration is valid only in these conditions and that the authors recommend using the instruments only in this case.

We have made some further investigations and find that when the window transmission falls then the backscatter trace becomes very noisy. We believe this is because any dust layer on the window is inhomogeneous and whereas the whole window is used for monitoring the window transmission, the actual backscatter signal is only affected by the dust on the central spot of the window that is illuminated by the laser. Accordingly the problem is more serious than implied by the reviewer. When the window is dusty not only is the calibration unreliable but so is the backscatter signal.

We have made the following changes:

- 40 1. An extra phrase in the abstract after line 33 stating: **In all cases, if quantitative and reliable backscatter observations are to be obtained it is essential to keep the window clean. This may be a challenge in dusty locations.**
2. Extra sentence after line 209 at the end of the paragraph c:

**For quantitative calibrations and observations of backscatter it is essential that the window be kept clean. It may be possible to correct the observed backscatter for low pulse energy, but seems most unlikely that corrections can be made for the low window transmission because any dust or dirt covering on the window is probably not homogenous. It may be difficult to keep the window clean in locations where dust is common.**

- 50 3. In the conclusions we have added after line 503:  
**Instrument malfunction can be identified by sudden changes in calibration. If either the window transmission or the pulse energy falls below 90% of normal values, then clearly the instrument sensitivity and the calibration will be different. When the window transmission falls below 90% the backscatter becomes noisy, probably due to the inhomogeneous nature of the layer of dust or dirt on the window, consequently it is essential that the window is kept clean if reliable data are to be obtained. If the pulse energy falls below 90% then it should be possible to correct the backscatter signal but the precise accuracy of this technique remains to be determined.**

Section 4.1 Wiegner et al (2019) suggested that “error sources beyond the water vapor absorption might be dominant” for CL31. What will be the impact if you drop the water vapor correction? Would you have a better agreement with the Lufft CHM15k?

60 65 Without the water vapour correction, there is an annual cycle of change in calibration of about 12 %. (see Section 4.1, third paragraph: **for a water vapour path of 2 cm, a typical summer value in the UK, the change in water vapour transmission varies from about 0.77 to 0.75 (about 3%) as the peak laser emissivity increases from 900 to 916 nm. The typical water vapour path in winter is 1cm leading to a transmission of about 0.85, so if no water vapour correction was made, one would expect an apparent annual cycle of the calibration coefficient of about 12%.** ) To highlight this

annual cycle which would be introduced to the calibration if the water vapour absorption was not corrected for, we have also added this point to the caption of figure 7.

Section 4.3. line 322. Could you give more details on these outliers? These outliers could be used to identify instrument malfunctions.

70 New text added line 339: **The 2% of outliers all have high lidar ratios; they are probably from occasional profiles that do not completely attenuate the lidar signal.**

Section 4.4. could you comment on the high calibration coefficient for Benson and Exeter?

New text added, line 352: **The anomalously high calibration coefficients for Benson and Exeter are probably due to some unknown instrument malfunction as the window transmission and transmit power are recorded as normal. The large value of the calibration coefficient is correcting for this effect, but also flags that there is a malfunction in the instrument.**

Section 4.4 l355. Again, a quick sensitivity study might be useful to filter precisely the C2 outliers. Is your calibration still valid when the windows transmission is below 90%? Do you recommend not to use the data when the transmission is low has it affect the signal by 50%. This could be one major conclusion of the paper as it would affect the operational maintenance of ceilometer networks.

80 See response above for comment on Section 3 line 204

Section 5.1: Please add references to the saturation for photon-counting detectors. This is not a new challenge.

85 We have looked for an appropriate reference but apart from our personal communication, we cannot find one. Do you have a recommended reference we could use?

Line 381-382: There is a contradiction between this sentence and line 390. Either the negative backscatter can be used to remove the saturated profile, either not. Please replace the sentence “. . .to remove these profiles” by “. . .to remove most of these profiles”.

90 Contradiction removed and reworded for clarification (line 409): **To increase confidence that only saturated profiles are used, a cloud height threshold was also imposed, as demonstrated in Figure 11; this shows a histogram of the uncalibrated integrated attenuated backscatter for profiles in liquid water cloud at Aberporth.**

Section 5.2 line 416: Do you filter the data at 1km, 2.2km (line 401) or at an height that is instrument specific (line 405)

95 This has been clarified by the addition of the sentence (line 437) **The lower height limit is often higher than 1 km, however, due to the instrument-specific region of saturation.**

(Clouds lower than 1km should not be used for the calibration of the Met Office Lufft CHM15k due to overlap but these profiles would all be filtered out anyway due to removing profiles that cause saturation).

100 Section 5.2: l426. Keep the 10% only if the demonstration in the introduction is more robust.

See response to above

Section 6 line 436. Is the wavelength the only problem? What about the laser power and the instrument sensitivity?

Additional text added (line 455): **different power, and different detector sensitivities**

105 Line 444: Please add a clear reference to support that drizzle scattering is almost wavelength independent

Two references added (line 465) : **Drizzle drops are large compared to the wavelength of the lidar and hence the scattering is almost wavelength-independent for 1064 and 910nm lidars (since we are close to the geometric optics regime), as shown by Westbrook et al. (2010b).**

110 **The code of Hogan (2006) confirms that for drizzle, multiple scattering is negligible.**

Conclusion: I recommend to add that the calibration is valid only when the windows transmission and the energy pulse are above 90% and that a maintenance should be performed if it is not the case.

Added (see comment above)

115 2 Technical corrections

Introduction: I48. Please mention some operational weather models you are referring to.

Some examples added: **Operational weather forecasting models such as those operated by the ECMWF and MeteoFrance**

120 Section 2.2 I110 and table 1: please check the maximum range for Vaisala CL31. According to the manual, the typical message contains 770 gates with a 10 meter resolution. Therefore the maximal range is 7.7km.

Corrected to 7.7 km

Section 4. I235. Please mention the Lufft CHM8k that is measuring at 905nm and specify that it the CHM15k that is measuring at 1064nm (I238)

125 **Changed to specify that the Lufft CHM15k operate at 1064 nm so do not need correcting for water vapour absorption but that the Lufft CHM8k operate at 905 nm and so do require a correction.**

Section 4.2 I279. Could you change the sentence “that confuse the non-expert” by that might confuse the non-expert”. One could argue that the cosmetic feature is the confusing process.

Changed as recommended to **that might confuse**.

130 L300: please check the reference formatting.

Corrected

Section 5 line 364: Please mentioned CHM15k. This section is not valid for CHM8k measuring a 905nm.

Added CHM15k

135 Section 5.1 | 370 Please mention that the receiver type also has an influence on the saturation ( photon-counting )

Type of receiver added in

**Reviewer 2**

We thank Reviewer 2 for his/her constructive comments

140 Our responses and changes are given below in red; changes to the text are shown in bold

Specific Comments

Abstract, lines 16-19: Vaisala ceilometers in operational use are often set so that not all signal above 2.4 km has been range-corrected; should you add here a maximum cloud altitude of 2.4 km?

145 We have added '**care must be taken to only use profiles where the range correction is implemented**'.

Abstract, line 28: It's not clear which instrument you are referring to, and whether you mean a minimum threshold altitude of 2 km.

150 We have rewritten this section so that it reads '**The more sensitive ceilometer model operating at 1064 nm is unaffected by water vapour attenuation but is more prone to saturation in liquid clouds; such profiles can be recognised and rejected and, despite the more restricted sample of cloud profiles, a robust calibration is readily achieved. In the UK, the running mean 90-day calibration coefficients varied by about 4% over a period of one year.**'

Page 2, line 46: It is possible to operate these instruments with 5 m resolution.

155 This has been changed to **5 m** resolution

160 Page 3, lines 105-107. This statement is not quite true. It is often preferable to operate at as high a pulse repetition rate as possible in order to increase sensitivity; the limitation is also determined by expected sensitivity in terms of avoiding 'second-trip' echoes. For low-powered ceilometer systems, you may not expect to obtain any signals above 15 km even after averaging, hence a high repetition rate of 10 kHz is suitable, whereas high-powered lidar systems are capable of detecting polar stratospheric clouds at 15-25 km, or designed for observing other atmospheric parameters in the stratosphere-mesosphere, and require a lower repetition rate. It may also depend on the detector.

165 We have removed the line '**Due to the low power of ceilometers, they have a much higher pulse repetition rate compared to high-power lidars, to compensate for this lower power and to increase the signal to noise ratio.**' And replaced it with the line '**Ceilometers generally operate at low power, so, to increase signal-to-noise ratio, they tend to have higher pulse repetition rate compared to high-power lidars; the returns from distant signals are generally very low so 'second trip' echoes are not usually a problem.**'

170 Page 3, line 111, and Table 1: Maximum range of CL31 in standard mode is 7.7 km (770 gates with 10 m vertical resolution, 385 gates with 20 m vertical resolution). If operated at 5 m vertical resolution then maximum range is 7.5 km (1500 gates).

The table has been corrected to read **7.7 km**. We have also clarified in the legend that The Met Office CL31 ceilometers have a vertical resolution of 20 m, apart from at Exeter CL31 where the vertical resolution is 10 m.

175 Page 4, line 116: Not airline pilots, but aviation forecasters and air traffic control!

**Airline pilots corrected to aviation forecasters and air traffic control**

Page 4, lines 136-137: The O'Connor et al. (2004) paper shows that S is constant for droplet size distributions with median volume diameters in the range of 10 to 50  $\mu\text{m}$  and states that it starts to fall for distributions with median volume diameters above 50  $\mu\text{m}$ .

180 **Corrected from 100  $\mu\text{m}$  to 50  $\mu\text{m}$**

Page 8, lines 260-261: Do you mean ' at a wavelength of about 910 nm '?

**Deleted 'between' from sentence**

Page 8, line 270 & 273: Suggest that you include NWP or operational forecast, i.e. 'a convection-permitting variable resolution regional NWP model' and 'ECMWF operational forecast model'.

185 **Changed to 'a convection-permitting variable resolution regional NWP model' and 'ECMWF operational forecast model'.**

Page 8, lines 276-279: I suggest you expand this to explain that some signals above 2.4 km may not have been range-corrected, which is why they are not suitable.

190 Sentence expanded to read 'This is done to avoid the background noise signal leading to apparent clouds at high altitudes that confuse the non-expert, so for the calibration procedure, profiles above 2.4 km are not suitable as the return signal may not have been range corrected'

Page 9, lines 292-302: This feature could be due to the range-dependent multiple scattering factor not being calculated correctly at close ranges (the telescope alignment not being perfect for example).

195 Inserted 'We suspect that this is a result of the instrument detector saturating or range dependent multiple scattering not being calculated at close ranges because of imperfect telescope alignment.'

Page 10, line 340: Could add here that the method works for both coastal locations and inland.

**Added in 'from both coast and inland sites' at end of paragraph.**

Page 12, line 410: Unlike the Vaisala ceilometers operated in 'standard mode'. The instrument settings can be altered so that this change in processing at 2.4 km is not switched on.

200 Reference to Vaisala ceilometers removed from this line to avoid confusion. Line change to **The Lufft ceilometers have a range correction applied to the full attenuated backscatter profile, therefore they are not restricted by a change in processing at 2.4 km**

Page 13, line 444: As you state later in the next sentence and the next paragraph, drizzle and ice scattering aren't wavelength-independent, so I suggest revising this sentence.

205 **Reworded to remove contradiction and two references added: Drizzle drops are large compared to the wavelength of the lidar and hence the scattering is almost wavelength-independent for 1064**

and 910nm lidars (since we are close to the geometric optics regime), as shown by Westbrook et al. (2010b).

The code of Hogan (2006) confirms that for drizzle, multiple scattering is negligible.

210 Page 13, lines 455-457: Have you checked the impact of multiple scattering for drizzle in your comparison of the two instruments? This may explain why the best fit does not lie on the 1-to-1 line; more multiple scattering would be expected for the Vaisala instrument.

Impact of multiple scattering in drizzle referenced

215

220

225

# A robust automated technique for operational calibration of ceilometers using the integrated backscatter from totally attenuating liquid clouds

Emma Hopkin<sup>1</sup>, Anthony J. Illingworth<sup>1</sup>, Cristina Charlton-Perez<sup>2</sup>, Chris D. Westbrook<sup>1</sup>, Sue  
230 Ballard<sup>2,3</sup>

<sup>1</sup>Department of Meteorology, University of Reading, Reading, UK

<sup>2</sup>Met Office, MetOffice@Reading, Reading, UK

<sup>3</sup>Deceased, 12<sup>th</sup> July 2018

235 *Correspondence to:* Emma Hopkin (EH@westgate.slough.sch.uk); Dr. C. Charlton-Perez (c.charlton-perez@metoffice.gov.uk)

**Abstract.** A simple and robust method for calibrating ceilometers has been tested in an operational environment demonstrating that the calibrations are stable to better than  $\pm 5\%$  over a period of a year. The method relies on using the integrated backscatter (B) from liquid clouds that totally extinguish the ceilometer signal; B is inversely proportional to the lidar ratio (S) of the backscatter to the extinction for cloud droplets. The calibration technique involves scaling the observed backscatter so that B matches the predicted value for S of  $18.8 \pm 0.8$  sr for cloud droplets, at ceilometer wavelengths. For accurate calibration, care must be taken to only use profiles where the range correction is implemented and to exclude any profiles having targets with different values of S, such as drizzle drops and aerosol particles, profiles that do not totally extinguish the ceilometer signal, profiles with low cloud bases that saturate the receiver, and any profiles where the window transmission or the lidar pulse energy is low, falls below 90%. A range dependent multiple scattering correction that depends on the ceilometer optics should also be applied to the profile. A simple correction for water vapour attenuation for ceilometers operating at around 910 nm wavelength a simple correction for water vapour attenuation is applied to the signal using the vapour profiles from a forecast analysis. For a generic ceilometer in the UK the 90-day running mean of the calibration coefficient over a period of 20 months is constant to within 3% with no detectable annual cycle, thus confirming the validity of the humidity and multiple scattering correction. For Gibraltar, where cloud cover is less prevalent than in the UK, the 90-day running mean calibration coefficient was constant to within 4%. The more sensitive ceilometer model operating at 1064 nm is unaffected by water vapour attenuation but is more prone to saturation in liquid clouds. We show that reliable calibration is still possible, provided the clouds used are above a certain altitude. The threshold is instrument dependent but is typically around 2 km. We also identify a characteristic signature of saturation, and remove any such profiles with this signature. Despite can be recognised and rejected and, despite the more restricted sample of cloud profiles, a robust calibration is readily achieved, and, in. In the UK, the running mean 90-day calibration coefficients varied by about 4% over a period of one year. The consistency of profiles observed by nine pairs of co-located ceilometers in the UK Met Office network operating at around 910 nm and 1064 nm provided independent validation of the calibration technique. In all cases, if quantitative and reliable backscatter observations are to be obtained it is essential to keep the window clean. This may be a challenge in dusty locations. EUMETNET is currently networking 700 European ceilometers so they can provide ceilometer

profiles in near real time to European weather forecast centres and has adopted the cloud calibration technique described in this paper for ceilometers with a wavelength of around 910 nm. (439 words)

265

## 1 Introduction

Ceilometers are simple, relatively inexpensive vertically pointing lidars that typically operate at wavelengths of 905-910 nm or 1064 nm. They can be left unattended for long periods and, as the name suggests, have mainly 270 been used for detecting cloud base height at airports where they are valuable for air safety issues. Recent studies have shown that, in addition to detecting the large backscattered return signal from cloud base, they can also provide vertical profiles of backscatter from both clouds and aerosols every 5-30 seconds with a range resolution as low as 105 m. Ceilometer profiles have been used in many research contexts; some examples are 275 for the Cloudnet scheme for validation of the representation of clouds in operational numerical weather prediction (NWP) forecast models (Illingworth et al., 2015), for aerosol profiling (Markowicz et al., 2008; Madonna et al., 2015), fog observations (Dupont et al., 2012) and the retrieval of mixing height levels (Münkel et al., 2007).

Many operational weather forecasting models such as those operated by the ECMWF and MeteoFrance now represent both clouds and aerosols by prognostic variables. Remote sensing observations are 280 needed to show that these models are providing unbiased estimates of aerosol and cloud properties, and ultimately for data assimilation into such models to improve forecasts of hazardous weather such as pollution episodes and severe convective storms producing flash floods. The European Ground-Based Observations of Essential Variables for Climate and Operational Meteorology (EG-CLIMET), which was a recent Cooperation in Science and Technology (COST) action financed by the European Union, noted that there are hundreds of 285 ceilometers deployed over Europe, which are currently under-exploited. EG-CLIMET recommended that the ceilometers be networked to provide users easy access to calibrated backscatter data (Illingworth et al., 2015). At the time of writing, profiles from 200 ceilometers from 17 countries are being distributed in near real time by the E-Profile programme of European Meteorological Services Network (EUMETNET, 2018) with the number expected to rise to about 700. The data formats, calibration techniques and retrieval algorithms are being 290 developed by COST action 1303: Towards operational ground based profiling with ceilometers, Doppler lidars and microwave radiometers for improving weather forecasts (<http://www.toprof.ima.cnr.it>).

If ceilometer data are to be used in an operational context, and potentially for data assimilation, accurate calibration is essential when verifying model performance by forward modelling the attenuated backscatter; for example, Illingworth et al. (2019) show that a calibration accuracy of 10% is needed when deriving O-B 295 statistics obtained by comparing the observed ceilometer backscatter ('O') from Saharan dust with the forward modelled backscatter ('B') from the ECMWF CAMS model. The World Meteorological Organisation requirements (OSCAR, 2018) suggest the goal for ice water content (IWC) observations is to have an accuracy of 10% and for aerosol optical extinction to have an absolute accuracy of  $0.01 \text{ km}^{-1}$ , but no fractional accuracy is quoted. Ice In most models the ice particle density is usually assumed to be inversely proportional to 300 particle size, (e.g. Brown and Francis, 1995) so IWC is proportional to extinction and, for a given lidar

ratio [and small amounts of attenuation](#), the requirement is for a ceilometer calibration [accuracy](#) to be [accurate to 10%](#).

The use of theoretical calibrations for lidars and radars based on an accurate budget of the losses and gains in the transmission and reception optics and in the electronics together with atmospheric attenuation can cause 305 large errors (Protat et al., 2011). Accordingly, it is preferable to find some natural target that has a known backscatter value. There are two such candidates for ceilometers: firstly, the backscatter from the molecules in the atmosphere and, secondly, the integrated backscatter profile from water clouds that totally extinguish the lidar beam. In this paper, we will focus on the second method. This method, using the attenuated backscatter signal from liquid water clouds, relies on the fact that the backscatter to extinction ratio (S) is a known value of 310 18.8 sr for wavelengths of relevance to ceilometers (O'Connor et al., 2004). The advantage of this method is that the backscatter values from liquid water clouds are very high (typically peaking at  $0.3 \text{ km}^{-1} \text{ sr}^{-1}$ ) so the signal to noise ratio of water cloud returns is very large. By contrast, the molecular signal close to the ground is over one hundred times lower than the cloud returns and of the order  $10^{-3} \text{ km}^{-1} \text{ sr}^{-1}$ , falling off exponentially with height. For an accurate estimate of the molecular return it is necessary to [average](#) the ceilometer profiles over 315 several hours on selected cloudless nights when there is negligible backscatter from thin cirrus clouds or aerosols (e.g. Tsaknakis et al., 2011; Wiegner et al., 2014).

In this paper, we present a development of the calibration technique using liquid clouds that can be implemented operationally and which avoids the aforementioned potential problems. We report on the values of the calibration for the Met Office network of ceilometers and show the calibration stability in time. In section 2, we 320 review the specifications and performance of the two ceilometer models in widespread use in Europe. The calibration algorithm is described in section 3 and the instrument model dependent corrections and calibration results are addressed in sections 4 and 5. Finally, in section 6, we report on collocated ceilometer comparisons and statistics of the stability and accuracy of the calibration.

## 2 Instrumentation

### 325 2.1 The Met Office Ceilometer Network

Figure 1 shows the locations of the 40 ceilometers in the UK that are presently reporting the full vertical profiles of the attenuated atmospheric backscatter, and are referred to in this paper as the ‘Met Office ceilometer network.’ The purple crosses show the location of the 29 Vaisala CL31 ceilometers and the red circles show the 330 11 Jenoptik CHM15k Nimbus ceilometers that have been used to test the ceilometer calibration technique. Nine sites have collocated Vaisala and Jenoptik ceilometers. Other Met Office ceilometers, many of which are the Vaisala CT25K model, report only cloud base height and are not discussed here, although the calibration technique can be applied to both the CT25K and the newer CL51 models. Note that Jenoptik no longer produce ceilometers; the manufacturing of them has been taken over by Lufft. From here on, we refer to these ceilometers as Lufft ceilometers, including those manufactured before production passed from Jenoptik to Lufft.

### 335 2.2 Vaisala CL31 ceilometers

The key technical properties of the ceilometers used by the Met Office are summarised in Table 1. In brief, the Vaisala CL31 ceilometers use an InGaAs diode laser which emits pulses with an energy of  $1.2 \mu\text{J}$  at a pulse repetition frequency (prf) of  $10 \text{ kHz}$  with a central wavelength of  $910 \pm 10\text{nm}$ , though the typical spectral width is more often  $4 \text{ nm}$  (Kotthaus et al. 2016, Markowicz et al. 2007). At these wavelengths, attenuation by water

340 vapour is significant, a fact overlooked by O'Connor et al. (2004). Due to the Ceilometers generally operate at low power of ceilometers, so, to increase the signal-to-noise ratio, they tend to have a much higher pulse repetition rates compared to high-power lidars, to compensate for this lower power and to increase the signal to noise ratio; the returns from distant signals are generally very low so 'second trip' echoes are not usually a problem. The CL31s have a single lens design, with the centre of the lens collimating the laser beam and the

345 outer part of the lens used for focussing the backscattered light onto the receiver, which uses an avalanche photo diode (APD) detector to process the signal (Münkel et al., 2007). Complete overlap of the transmitted beam at the receiver sample is achieved at a height of approximately  $70 \text{ m}$  (Martuccci et al., 2010) and the maximum range is 7.67 km.

Specification	Vaisala CL31	Lufft CHM15k
<b>Laser</b>	InGaAs Diode	Nd:YAG
<b>Centre Wavelength</b>	910 nm	1064 nm
<b>Wavelength Variability</b>	$\pm 10 \text{ nm}$	insignificant
<b>Optical Design</b>	Coaxial	biaxial
<b>Pulse Energy</b>	$1.2 \mu\text{J}$	$8 \mu\text{J}$
<b>Pulse Repetition Rate (PRF)</b>	$10 \text{ kHz}$	$5-7 \text{ kHz}$
<b>Temporal Resolution</b>	30 s	30 s
<b>Vertical Resolution</b>	<u>10/20 m *</u>	15 m
<b>Complete Overlap</b>	70 m	1000 m
<b>Maximum Detection Range</b>	<u>7.67 km</u>	15 km

350 Table 1: Summary of some technical characteristics and parameters of the Vaisala CL31 and Lufft CHM15k, as operated in the Met Office network. \*Exeter The Met Office CL31 has ceilometers have a vertical resolution of 20 m, apart from at Exeter CL31 where the vertical resolution is 10 m.

355 There are currently several different versions of the firmware in use by the Met Office ceilometer network. The various versions process the signal in different ways, applying “cosmetic” shifts to the data to avoid unphysical negative backscatter values. The original users for ceilometer data were airline pilots aviation forecasters and air traffic control and these cosmetic shifts were applied so that it was easier for non-experts to interpret the displays. Full details of the shifts and methods for correcting can be found in Kotthaus et al. (2016). These effects should certainly be corrected for in the study of smaller particles such as aerosols and ash; however, for the stronger signal from cloud particles the effect of these shifts on the calibration method shown here is negligible.

### 360 2.3 Lufft CHM15k Nimbus ceilometers

The Lufft ceilometers use a Nd:YAG laser and operate at a slightly longer wavelength of  $1064 \text{ nm}$  where the attenuation by water vapour is negligible. The APD detector employs a photon counting method. Due to the biaxial design of the Lufft ceilometers, full overlap is not reached until  $1 \text{ km}$  rather than  $70 \text{ m}$  for the CL31.

365 The pulse repetition frequency is in the range  $5-7 \text{ kHz}$  and the pulse energy is  $8 \mu\text{J}$ , which is six times higher than the Vaisala CL31 ceilometers. This higher pulse energy, combined with the different overlap

configuration, results in a much higher sensitivity of the CHM15k ceilometer, for detection of elevated aerosols such as volcanic ash plumes.

### 3 The calibration algorithm

Autocalibration of ceilometers using liquid water cloud was proposed by O'Connor et al. (2004) as a simple  
370 method that requires no additional instruments to compute a calibration coefficient. The technique relies on the use of the lidar ratio (ratio of extinction to backscatter, denoted  $S$ ) that is a constant for the droplets in liquid water cloud. Several studies have derived  $S$  from Mie theory: Pinnick et al. (1983) found that, for a wavelength of 1064 nm,  $S = 18.2$  sr; Wu et al. (2011) calculated an  $S$  of  $18.5 \pm 0.47$  sr for a wavelength of 1064 nm.

O'Connor et al. (2004) calculated an  $S$  of  $18.8 \pm 0.8$  sr for a wavelength of 905 nm and showed that this was  
375 essentially constant for the observed cloud droplet size distribution for a mean droplet size ranging from 10 to ~~10050~~  $\mu\text{m}$ , but  $S$  values were lower for drizzle having larger droplets. Since  $S$  is very similar at 905 nm and 1064 nm, we follow O'Connor et al. and use  $S = 18.8$  sr for both wavelengths.

The method compares this theoretical  $S$  to a calculated ‘apparent  $S$ ’. When the ceilometer signal is completely  
380 extinguished by the cloud, the total path integrated attenuated backscatter  $B$  is equal to the reciprocal of twice the lidar ratio:

$$B = \int_0^{\infty} \beta_{\text{observed}} dz = \int \beta_{\text{True}}(z) \exp[-2\tau(z)] dz \\ = \frac{1}{\eta S} \int \exp(-2\tau) d\tau = \frac{1}{2\eta S} \quad (1)$$

where  $B$  is the total integrated attenuated backscatter,  $\tau$  is the optical thickness,  $S$  is the theoretical lidar ratio, and  $\eta$  is a multiple scattering correction which is dependent on laser wavelength, beam divergence, telescope  
385 field of view, and altitude ( $z$ ). The multiple scattering corrections are height dependent and calculated for each gate using the fast method and code described by Hogan (2006; code available to download at <http://www.met.reading.ac.uk/clouds/multiscatter/>).  $\eta$  is usually between 0.7 and 0.85 for wavelengths between 905-1064 nm in liquid water clouds. The calibration technique involves multiplying the observed backscatter signal  $\beta_{\text{observed}}$  by a calibration coefficient,  $C$ , until  $B\eta = 0.0266 \text{ m}^{-1}$ , the value for water drops when  $S = 18.8$  sr.  
390 Note that  $C$  is a scaling factor, and is the reciprocal of the widely used ‘Calibration Constant’  $C_L$  that is often used for photon counting receivers, and is the factor by which the count should be divided to obtain a calibrated value (e.g. Wiegner et al., 2014).

The calibration technique will fail if there are targets contributing to  $B$  that have an  $S$  that is not equal to 18.8 sr. At ceilometer wavelengths, aerosols generally have  $S$  values above those for cloud droplets; marine aerosols  
395 have an  $S$  close to 20 sr, but most aerosols have values that are much higher and in the range 40 to 100 sr for dust, smoke and ash (e.g. Omar et al., 2009). If aerosols with  $S$  higher than 18.8 sr are included in profiles leading to total attenuation of the signal, then the value of  $B$  will be less than for cloud alone, and the apparent value of the calibration coefficient,  $C$ , will be too high. Conversely, drizzle has  $S$  values below those for cloud droplets, so if drizzle is included in the profile, the value of  $B$  will be higher than for cloud alone, and the value  
400 of  $C$  would be too low. The magnitude of the error due to aerosol depends on its optical depth beneath the cloud layer; therefore, we can circumvent this uncertainty by not selecting profiles which have large backscatter from

aerosol. The inclusion of profiles that are not totally extinguishing the ceilometer return will also lead to values of C that are too high, as will occasions when the window transmission is reduced or the pulse energy falls.

Figure 2a shows an example of an uncalibrated attenuating backscatter profile typical of those from stratocumulus clouds that is ideal for use in the liquid cloud calibration algorithm. Cloud is observed as the sharp peak in attenuated backscatter just above cloud base rising to a maximum value of  $0.28 \text{ km}^{-1} \text{ sr}^{-1}$  within a few range gates and clearly dominates the observed ceilometer return. The shaded area indicates the area of integration used in computing the total attenuated backscatter of the profile. The profile in Fig. 2b is for a stratocumulus cloud that completely attenuates the ceilometer return. However, in this case, it is unsuitable for calibration because there is a significant return from aerosol in the lowest 200 m of the profile, and a more gradual increase in attenuated backscatter below the peak at cloud base indicating the presence of drizzle below the cloud.

A new algorithm has been designed to automatically sift through all profiles of attenuated backscatter, selecting only those suitable for the cloud calibration according to a strict set of criteria. The method is fairly simple ensuring that it can be applied operationally with minimal impact on processing time. No absolute values of  $\beta_{att}$  are required by the algorithm to evaluate the criteria below, so the instrument can be completely uncalibrated, or the calibration currently applied can have a large error. The algorithm only requires a minimum of 10 suitable profiles in a day for a calibration coefficient to be calculated. This means the calibration algorithm is suitable for ceilometers at sites where liquid water cloud can be sparse and infrequent. There are two main sets of criteria that must be met by the profile of attenuated backscatter for it to be used to calculate a calibration coefficient:

1. Unsuitable individual profiles:

- a. Aerosol filter. In any single profile, if the aerosol under the cloud contributes more than 5% to the total integrated backscatter (as shown in Fig. 2b), then this profile is removed from the calibration. The transmission through the aerosol below the cloud attenuates the ceilometer beam and this attenuation increases with greater concentrations of aerosol. If the aerosol has a lidar ratio value twice the value assumed for cloud droplets, then this filter should limit the calibration error to a maximum of 5%.
- b. Peak sharpness filter. The peak backscatter magnitude must be a factor of 20 greater than the value 300 m above and below that peak. A liquid water cloud suitable for calibration must fully attenuate the ceilometer beam; therefore, the backscatter values should decrease rapidly in the gates immediately above the peak value. Additionally, drizzle or rain below the cloud may give a large backscatter signal and, like the aerosol, will distort the apparent lidar ratio. Hogan et al. (2003) report that individual liquid-water layers do not tend to occupy more than 300 m of the ceilometer profile, due to their strong attenuation. Our own observations of the data lead to the same conclusion. This filter should therefore remove profiles that do not fully attenuate the beam and those that contain drizzle or rain.
- c. Window transmission and pulse energy check. A check is made on the recorded instrument transmission (given as a percentage of how much of the instrument window is clear) and on the reported pulse energy (given as a percentage of a nominal amount). Both of these conditions can affect the true value of attenuated backscatter. For considering instrument and

445

calibration stability, periods affected by reduced window transmission and/or reduced pulse energy are filtered out at a threshold of 90% or less. For quantitative calibrations and observations of backscatter it is essential that the window be kept clean. It may be possible to correct the observed backscatter for low pulse energy, but seems most unlikely that corrections can be made for the low window transmission because any dust or dirt covering on the window is probably not homogenous. It may be difficult to keep the window clean in locations where dust is common.

450

## 2. Consistency of neighbouring profiles

455

- a. Lidar ratio stability – This filter traps errors due to patchy cloud cover or drizzle that may not have been identified by the first filter by checking that the apparent lidar ratio is the same as its nearest neighbours. The recommendation is to compare to 3 profiles either side; however, if the ceilometer is at a site where liquid water cloud is infrequent, this could be reduced to 1 or 2 profiles either side, with consequent degradation of the accuracy of the calibration coefficient. There must be at least 10 acceptable profiles for a calibration coefficient to be recorded for that day.

465

The operation of these filtering procedures in removing unsuitable profiles is illustrated in Fig. 3a, where a stratocumulus cloud layer located at about 1 km for the whole day is ideal for calibration. The liquid cloud backscatter signal, which has values greater than  $10^{-0.5} \text{ km}^{-1} \text{ sr}^{-1}$  (in the red region of the colour scale), appears as a thin layer above which there is only noise. Within the noise, the diurnal cycle of the skylight is visible. The noise in the data is visible as speckling, and is of the magnitude of less than  $10^{-3} \text{ km}^{-1} \text{ sr}^{-1}$ . There are also limited periods of broken, patchy cloud, which are identifiable by breaks in the layer of high backscatter, and limited periods of drizzle which are identifiable by the fall streaks (cyan colours of the order  $10^{-2.5} \text{ km}^{-1} \text{ sr}^{-1}$ ) below the cloud.

470

Figure 3b illustrates the two main filtering steps of the new calibration algorithm. The thick, light grey line shows the apparent S values for each individual profile that is acceptable and has removed those profiles between from 3.30 – 4.30 hours where there is drizzle and aerosol below the cloud base, but this still leaves some large apparent S values from 12.00 -15.00 hours that are due to broken cloud that does not totally extinguish the ceilometer return. The second filter checks for consistency between neighbouring profiles and successfully identifies and removes these spurious profiles where there is broken cloud.

475

The remaining profiles (i.e. those in black in Fig. 3b) give the values of apparent S which would be used to calculate C using Eq (1). It is evident that these values remain very constant over the course of the day, implying that the calibration of the instrument is very stable on this time scale. This is important, since our method can only be applied during cloudy conditions, which may be separated by intervals of several days. The stability of C implies we can interpolate between calibration events.

## 4 Calibration of 910 nm ceilometers

### 4.1 Water vapour attenuation

To complete the calibration of the Vaisala CL31 ceilometers (and others of similar wavelength – e.g. Vaisala CL51, CT25k, CT75k, Campbell Scientific CS135), the effect of atmospheric water vapour below the cloud on the laser signal must be considered. This is because the wavelength of these ceilometers (910 nm) is in a weak water vapour absorption band. Note that because the Lufft [CHM15k](#) ceilometers operate at 1064 nm, where there is a water vapour absorption window, those ceilometers do not require a correction; [however, the Lufft CHM8k operate at 905 nm and so would require a water vapour absorption correction.](#)

485 A recent paper by Wiegner and Gasteiger (2015) describes a method of correcting for water vapour attenuation for ceilometers at wavelengths around 910 nm by performing detailed line by line radiation transfer calculations and investigating the impact of the instrument emission spectrum (e.g. Vaisala states that for a CL31 the wavelength is  $910 \pm 10$  nm at  $25^{\circ}\text{C}$  and with a drift of  $0.3 \text{ nm K}^{-1}$ ). As the housing of the ceilometer lasers and detectors are temperature-controlled environments, the effect of laser wavelength drift due to temperature can be 490 considered insignificant. However, even if the potential for drift is ignored, Wiegner and Gasteiger's method still requires the use of a radiative transfer model or access to their "WAPL" database of absorption coefficients. Because the liquid cloud calibration method presented in this paper is intended for operational, real-time use, a simple, robust and computationally cheap method was required.

495 A simplified technique for correcting for the two-way water vapour attenuation has therefore been devised based on Markowicz et al. (2008) who show that the normalised spectrum of laser emission is wide enough to smooth out the individual water absorption lines so that for a water vapour path of 2 cm, a typical summer value in the UK, the change in water vapour transmission varies from about 0.77 to 0.75 (about 3%) as the peak laser emissivity increases from 900 to 916 nm. The typical water vapour path in winter is 1cm leading to a transmission of about 0.85, so if no water vapour correction was made, one would expect an apparent annual 500 cycle of the calibration coefficient of about 12%. The water vapour could be estimated using a microwave radiometer. Alternatively, it can be obtained from a numerical weather prediction (NWP) model. In this paper we take the latter approach. Cossu et al. (2015) have compared NWP output with the water vapour path derived from microwave radiometers and find that the mean bias of the NWP water vapour path is only 0.7mm.

505 A simple monotonic function has been fitted to data from Markowicz et al. (2008) in order to parameterise the two way attenuation by water vapour as a function of integrated water vapour (IWV) up to 2cm at wavelengths [between](#) of ~910 nm depicted in Fig. 4:

$$T_{wv} = 1 - 0.17IWV(z)^{0.52} \quad (3)$$

510 where  $T_{wv}$  is the two way transmission as a percentage of the transmission without water vapour attenuation and  $IWV(z)$  is the atmospheric water vapour content from the surface to height  $z$  in  $\text{g cm}^{-2}$ . The attenuated backscatter is then corrected using:

$$B = \int \beta_{att} \times C_{wv} dr, \text{ where } C_{wv} = \frac{1}{T_{wv}}. \quad (4)$$

The transmission calculation for each range gate requires the water vapour content obtained by integrating the water vapour density from the ground to each specific range gate, resulting in a transmission profile. For the automatic operational calibration of the Met Office ceilometers, water vapour density would be calculated from

515 the Met Office UKV model, a convection-permitting variable resolution regional [NWP](#) model run operationally over the UK (Tang et al., 2012), using pressure, temperature and specific humidity. A comparison of the detailed line-by-line Wiegner and Gasteiger method with the simpler approach using the water vapour density profiles obtained from the ECMWF [operational forecast](#) model provided by Maxime Hervo (Meteoswiss, Personal Communication, 2016) is shown in Fig. 5. The WAPL method is depicted in blue and the new, simple  
520 method is in red. The transmissivity profiles differ by a maximum of 2% for a total transmissivity of 0.85.

#### 4.2 Region of integration

For the Vaisala ceilometers in the Met Office network, a cosmetic feature in the firmware suppresses the range  
525 correction to the received power for heights above 2.4 km, except when there are clouds present. This is done to avoid the background noise signal leading to apparent clouds at high altitudes that [might](#) confuse the non-expert, [so for the calibration procedure, profiles above 2.4 km are not suitable as the return signal may not have been range corrected](#). In addition, Kotthaus et al. (2016) found that the attenuated backscatter in the lowest 200 m  
530 may be subject to artefacts so, in this calibration study of the Met Office's Vaisala ceilometers the cloud returns above 2.4 km and below 200 m are not used.

Figure 6 shows a histogram of the integrated attenuated backscatter, B, from liquid cloud as a function of the height of the maximum attenuated backscatter (used as an indicator of the height of the cloud), for profiles from an uncalibrated Met Office Vaisala CL31 situated at Middle Wallop (51.15° N, 1.57° W). Multiple scattering and water vapour attenuation below the cloud have been accounted for. Over 100,000 profiles were used, from  
535 the period September 2014 to December 2015. The numbers superimposed on the right side of the plot show the mean and standard deviation at 100m intervals of the range. For 16 of the 21 heights shown, the mean value is 0.021 sr<sup>-1</sup>. The other 5 gates differ by a maximum of only 0.002 sr<sup>-1</sup>. This provides confirmation both of the validity of the range dependent multiple scattering correction and the assumption of constant S for different water clouds.

540 Below 500 m there is, however, a slight change. The distribution of the integrated attenuated backscatter is still concentrated in a similar region as at other heights, but it also has a slight tail to the left. For profiles in this tail region below 500 m, the attenuated backscatter is smaller, which will result in a larger apparent lidar ratio. The mean value of the integrated attenuated backscatter at heights below 500 m decreases by 9.5% with the standard deviation increasing by 17%. We suspect that this is a result of the instrument detector saturating [or maybe range dependent multiple scattering not being calculated correctly at close ranges because of imperfect telescope alignment](#). When the cloud is very low, the cloud signal may be so strong at its peak that the true magnitude of the backscattered signal is not fully detected and, therefore, the integrated attenuated backscatter appears smaller when compared to other heights. It is also possible that this may, occasionally, be due to microphysical  
545 processes within the cloud. Nicholls (1984; [Pawlowska et al., 2000](#)) showed that there is a reduction in droplet number concentration below 450-500 m. [\(Pawlowska et al., 2000\)](#). This may, in some cases, be significant  
550

enough to affect the backscatter at this height. Therefore, we also reject profiles where the cloud is between 200 – 500 m.

### 4.3 Calibration results for Middle Wallop

Figure 7 shows a time series of the calibration results for the CL31 at Middle Wallop in Southern England over a period of 20 months. The top panel shows the mode of the calibration coefficient C, for each day with sufficient (minimum 10) attenuated backscatter profiles deemed suitable by the calibration algorithm. For example, the black cross on 25 October 2014 is the mode of the calibration coefficients calculated from the filtered S values (per profile) shown (in black) in Fig. 3b.

The results are for almost two years of data and establish that the calibration remains stable over time. The number of profiles used for the calculation of the daily value is different depending on the occurrence of cloud on each day. As the calibration algorithm requires only a minimum of 10 profiles to be included in the daily value of the mode, even a short period of cloud will be included for calibration purposes. This ensures that the technique can be applied to ceilometers in locations with climates that have relatively little cloud occurrence. For this site, the algorithm found a minimum of 8 days every month with profiles suitable for calibration, with slightly more suitable days during autumn and winter. The water vapour correction profiles are calculated from the Met Office UKV model at the grid point over the Chilbolton Observatory, which is approximately 15 km from Middle Wallop. The variables needed to calculate the transmission profiles were available every hour, and have been interpolated to the observational time.

The middle panel of Fig. 7 shows the daily mean and standard deviation for the same station and data. For the 20-month (574 days of data available) period, a calibration was possible on 320 days, or 56% of the days, and the average number of profiles per day was 292. There were just 7 days out of the 320 when the calibration coefficient, C, was approaching 2.0 rather than the median value of 1.4, so a 90-day running mean was calculated and is displayed in the lower panel of Fig. 7. This running mean had a value of C of 1.40 with a standard deviation of 0.021; this is less than 2% of the mean. The 2% of outliers all have high lidar ratios; they are probably from occasional profiles that do not completely attenuate the lidar signal. As both the mean height of the cloud base (and therefore the amount of multiple scattering) and the water vapour attenuation have a pronounced annual cycle, this low value of standard deviation is evidence of the appropriateness of the algorithms that correct for these two effects. Accordingly, it is recommended that for automatic, operational use for a ceilometer, without window transmission or pulse energy issues, a 3-month running average of the calibration coefficient be used.

### 4.4 Calibration results for the Met Office network

The calibration of all the Vaisala CL31 ceilometers in the Met Office network has been collated and is summarised in Fig. 8, where box and whisker plots are shown of the calibration coefficient for each of the CL31s, calculated from data for the period January – March 2015. All instruments have a calibration coefficient larger than 1.0, with the majority of the instruments having a coefficient of around 1.5. The range of coefficients for each station is small, with 50% of the data (contained within the box) being within 10% of the mean value. The anomalously high calibration coefficients for Benson and Exeter are probably due to some unknown

instrument malfunction as the window transmission and transmit power are recorded as normal. The large value of the calibration coefficient is correcting for this effect, but also flags that there is a malfunction in the

590 instrument. The colour code in Fig. 8 indicates the different firmware versions installed on the instruments within the Met Office ceilometer network. Stations using the 202 firmware, which are shaded pink (for example, Aberporth, Coningsby, Middle Wallop), tend to have an even smaller range of C values, with 50% of the data being within 8% or less of the mean. The network includes stations from Lerwick (60.16°N, 1.15°W) down to Gibraltar (36.14°N, 5.35°W), demonstrating that the calibration method has been successfully applied to a range 595 of different climates, from the North Sea down to the Mediterranean Sea. and from both coast and inland sites.

The water vapour correction of the data has been applied for the calibrations depicted in Fig. 8, as described in section 4.2. Ideally, the water vapour profiles for each specific site should be used to calculate the transmission correction. Due to data availability, only the model data for Chilbolton was available at this time. As the 600 calibration specifically requires a cloud base below 2.4 km and the air is generally well-mixed below cloud base, the water vapour path mixing is generally fairly constant and depends on the temperature and height of the cloud base. Therefore, it is assumed that the season is more important than the location and so the same water vapour profiles are used for all the ceilometers. In future, operational implementation, the site-specific vapour profile 605 would be used.

Figure 9 shows the calibration of the Gibraltar CL31 ceilometer in more detail and has the same format as Fig. 605 7, for 12 months at Gibraltar rather than the 20 months at Middle Wallop. As the UKV does not cover Gibraltar, the water vapour correction was calculated using data from the Met Office Global Unified Model. Due to the 610 climate, the number of occasions when there are suitable clouds for calibration is reduced at the Gibraltar site. In one year there were 51 days of suitable clouds, with each day having on average 128 profiles. However, from mid-May to mid-Sept. there were only two days where calibration was possible and in December there were 615 none. While this is in part due to a lower amount of stratocumulus compared to the UK, it was also caused by the window transmission. The Gibraltar ceilometer requires regular cleaning as the dust tends to build up on the window, reducing the transmission. Therefore, several days where the window transmission dropped below 90 % have been filtered out by the algorithm. The 4 crosses in Fig. 9a and 9b which show a calibration coefficient closer to 2.0 correspond to days where the profiles only just pass the 90 % window transmission check. 620 Nevertheless, Fig. 9c confirms that the 90-day running mean calibration coefficient over the twelve month period was 1.5 with a standard deviation of 0.05, or about 3%, and, as with the data in Fig. 7, there is no sign of an annual cycle in the calibration coefficient.

## 5 Calibration of 1064 nm ceilometers

We now address the issue of cloud calibration for the Lufft CHM15k ceilometers, which operate at a 620 wavelength of 1064 nm. It should be noted that many high power lidars have a channel at 1064 nm and can also be calibrated with the liquid cloud method. However, as they do not have the same firmware and hardware issues as ceilometers, high power lidars are not directly discussed here.

### 5.1 Saturation issue

Before the cloud calibration can be applied to the Lufft ceilometers, the issue of saturation must be addressed.

625 Due to the greater pulse energy (compared to Vaisala ceilometers) and the receiver type (photon-counting), the Lufft ~~ceilometer receiver~~ceilometers are much more prone to saturation. When saturation occurs, the backscatter reported for this profile is false – it is too low. Hence, these profiles that saturate need to be avoided. The exact magnitude of power at which the Lufft power saturates is unknown. However, it is possible to detect the majority of saturated profiles, because the saturation of the receiver usually causes the output to overshoot to 630 an unphysical negative value just above the cloud echo (Personal Communication, H. Wille, Lufft, 2017).

The first panel of Fig. 10 demonstrates the impact of saturation and the subsequent negative overshoot: the blue profile, from the lower cloud base where saturation has occurred, has a smaller magnitude than the red profile of the higher cloud that has not saturated. If a saturated profile were to be used for calibration, then the total attenuated backscatter recorded by the ceilometer would appear lower than a non-saturated profile and would, 635 therefore, systematically skew the calibration coefficient to be larger than it should be.

Because the profiles that saturate have this apparent layer of negative attenuated backscatter, this can be used as a check in the calibration algorithm to remove these profiles. There is a correlation between the negative backscatter and the magnitude of saturation: the larger the negative backscatter value, the greater the magnitude of saturation, but this relationship is not linear and so the saturation cannot be easily corrected (Personal

640 Communication, H. Wille, Lufft, 2017). Hence, in what follows, we simply filter out such profiles completely. To ensure it is the negative attenuated backscatter of a saturated profile that is detected and not just the random noise in the profile above the cloud (which appears as small positive and negative values varying randomly from gate to gate~~to~~) any profiles which have a layer of negative backscatter greater than 100 m are removed from the calibration.

645 ~~This method removes the majority of saturated profiles; however, those profiles which only just saturate the instrument receiver may not always result in a region of negative attenuated backscatter.~~ To increase confidence that ~~all saturated~~only unsaturated profiles are ~~being removed~~used, a cloud height threshold ~~can be~~was also imposed~~–, as demonstrated in~~ Figure 11; ~~this~~ shows a histogram of the uncalibrated integrated attenuated backscatter for profiles in liquid water cloud at Aberporth. The multiple scattering correction has been applied, 650 but profiles where the instrument saturates have not been filtered out. Therefore, one can see clearly the impact of saturation.

As shown for the Vaisala ceilometer calibration (Fig. 4), the integrated attenuated backscatter should be a constant, independent of the height. This is not the case for the Lufft ceilometer. This is because when the instrument saturates, the received power becomes limited to some (unknown) maximum power. Backscatter is 655 proportional to received power  $\times$  range<sup>2</sup> that means the integrated backscatter measured will appear to be a function of range. This is in contrast to the Vaisala ceilometer in Fig. 6 where saturation is not occurring. Therefore, Fig. 11 shows that saturation is occurring below a height of 2.2 km because of the systematic change in backscatter with range. Above 2.2 km, the integrated backscatter does not change systematically with height, showing that these higher-level clouds are not saturating the ceilometer receiver – since they are further away, 660 the received power is weaker and below the level where saturation occurs. The exact height where the integrated attenuated backscatter becomes constant will be instrument-specific as it will be dependent on instrument power

and on the individual receiver. However, with this simple test, the height threshold required can be easily found, thus allowing for the saturated profiles to be removed and calibration to be correctly calculated.

## 5.2 Calibrated results ~~for~~ of the Lufft instruments CHM15k ceilometers

665 The calibration algorithm can now be applied to the Lufft ceilometers in a way similar to the calibration of the Vaisala ceilometers. A couple of changes are included. ~~Unlike the Vaisala ceilometers, the~~ The Lufft ceilometers ~~have a range correction applied to the full attenuated backscatter profile, therefore they~~ are not restricted by a change in processing at 2.4 km, ~~so~~ the upper range limit of integration to compute B is increased to 4 km, which incorporates the vast majority of liquid clouds in the UK. Additionally, the higher cloud range 670 means the ceilometer beam must travel through a larger portion of the atmosphere, so the ratio filter (~~error criterion~~ 1a) is increased from 5% to 10%. Note that this may lead to a slightly larger uncertainty in C, but ~~this is done to decrease the amount of data that would otherwise be filtered out, we choose to make this compromise in order to obtain a reasonable number of calibration estimates per month.~~ The lower height limit is also changed, so that clouds below 1 km are not used. This is to avoid using profiles in the region where an 675 overlap correction is applied as there is a potential temperature dependency in the overlap function that has not been accounted for (Hervo et al., 2016). ~~The lower height limit is often higher than 1 km, however, due to the instrument-specific region of saturation.~~

At the 1064 nm wavelength there is no absorption by the water vapour molecules; ~~so~~ no water vapour correction is required. Figure 12 shows an example of the cloud calibration applied to a Lufft CHM15k 680 ceilometer situated at Aberporth, West Wales, for the twelve months of 2015. Because of the requirement to remove the ~~low~~ level clouds that resulted in saturation, calibration was only possible on 70 days or about 20% of the days. Each day had an average of 58 profiles; nevertheless, the 90-day running mean calibration coefficient over the year was 0.48 with a standard deviation of 0.02 or 4%, with no sign of any annual cycle. This standard deviation of 4% over the year is slightly higher than for the Vaisala ceilometers, probably because 685 of the relaxation of the threshold for aerosol to be considered negligible, but is well within the specified requirement of 10%.

The calibration has been applied to the rest of the Lufft ceilometers in the Met Office ceilometer network, as 690 shown in Fig. 13. Most of the sites have a relative calibration of less than 1.0; however, Coningsby has a particularly large calibration coefficient. This highlights the importance and need for a calibration of each instrument. For each site, the relative standard deviation is small.

## 6 Collocated comparisons

The majority (9 out of 11) of the Lufft ceilometers are collocated with a Vaisala ceilometer, allowing 695 comparisons between the two types. Figure 14 compares the observations of attenuated backscatter from the two ceilometers at Aberporth, which have both been calibrated using the cloud method. To make a fair comparison between the two instruments, it is necessary to choose the meteorological situation carefully. Aerosols are problematic, because the ceilometers operate at different ~~power, different detector sensitivities, and different~~ wavelengths, and the backscatter from aerosols is wavelength-dependent in a way that we do not know a-priori. We could analyse profiles in liquid clouds; however, we have already used these for calibration (so it would not

be a truly independent test). In addition, the backscatter profile in liquid clouds contains very large gradients  
700 which make any comparison extremely sensitive to small offsets in range and/or differences in range-gating  
between the two instruments. Rain profiles could potentially be used for the comparison: however, rain which  
reaches the ground may wet the telescope optics and affect the data.

Better targets for such comparisons are drizzle drops and ice particles. [These particles](#)[Drizzle drops](#) are large  
compared to the wavelength of the lidar, and hence the scattering is almost wavelength-independent [for 1064](#)  
705 [and 910nm lidars](#) (since we are close to the geometric optics regime), [as shown by Westbrook et al. \(2010b\)](#). At  
the same time, the extinction of the lidar beam is much more gradual than in liquid cloud, providing smoothly  
varying backscatter profiles, which can be interpolated onto a common grid with little error. If we use an ice  
case, we would need to account for the influence of specular reflections from oriented ice crystals (e.g.  
Westbrook et al 2010a). Therefore, in this example, a drizzle scene has been chosen. [The code of Hogan \(2006\)](#)  
710 [confirms that for drizzle, multiple scattering is negligible.](#)

To establish quantitatively whether the backscatter for drizzle drops at 1064 and 910nm are actually equal, Mie  
calculations were performed, assuming Gamma drop size distributions (Westbrook et al., 2010b). The results  
show that the backscatter at 1064nm is very similar to that at 910nm, but systematically smaller. The differences  
are very modest: between 5 and 8% for median drop diameter in the range 0.1-0.6mm, with most of the  
715 calculated values in this range close to 7%. Meanwhile the extinction is essentially identical for both  
wavelengths. Thus, if the calibration has been successful it would be expected that the backscatter profiles in  
drizzle would match very closely. However, the Lufft is systematically 7% smaller than the Vaisala, if no  
adjustment to account for the different wavelengths is made. Therefore, for this comparison, the Vaisala  
attenuated backscatter data have been reduced by 7%.

720 It is also necessary to consider the various technical issues already discussed earlier in the article when selecting  
profiles, in particular the need for the drizzle to be high enough to be in the fully overlapped region for the Lufft  
instrument, and below the 2.4km height above which the Vaisala ceilometer data range correction is variable.  
Therefore, the data used covers the period 00.00 to 15.00 GMT on 22<sup>nd</sup> April 2016, during which time there is  
725 drizzling cloud. The data are 10-minute averages of attenuated backscatter between 1.0 and 2.4 km and the  
Vaisala data has been regridded from 20 m resolution to 15 m resolution using linear interpolation. The  
quicklooks of the attenuated backscatter for the Vaisala and Lufft ceilometers are shown in Fig. 14a and Fig.  
14b, respectively.

730 [Figure 14c shows that there is a strong correlation close to the 1:1 line between the two ceilometers, as the](#)  
[intercept is close to zero and the slopes differ by less than 10%. Figure 14c shows a joint histogram of the](#)  
[attenuated backscatter measured by the two instruments. If the calibration of both instruments has been](#)  
[successful, we expect the data to lie around the 1:1 line \(red dashed line\), and indeed our data do lie close to this](#)  
[line. Performing a linear regression of the backscatter values from the two instruments, we find an intercept very](#)  
[close to zero, a slope of 0.91, and a high correlation coefficient of 0.95. This indicates that our calibration](#)  
[process has been successful, and that the combined errors in the calibrations from both instruments together are](#)  
735 [less than 10%.](#) The spread of the individual data points is rather larger than 10% and can be accounted for by the  
different resolutions and interpolation errors. This comparison of the two different types of ceilometers confirms

the reliability of this calibration method – the two independently calibrated ceilometers, each with their own challenges (e.g. water vapour, saturation), are consistent with each other. This result is important for an operational network such as the Met Office ceilometer network because it helps maintain a reliable, comparable  
740 stream of calibrated data, with water vapour and saturation successfully accounted for, from each instrument at each site.

## 7 Conclusion

In this paper, we have presented a robust algorithm to calibrate ceilometers based on the cloud calibration technique that relies on the fact that the lidar ratio of liquid water clouds is a known constant. This new method  
745 can be run operationally, removing unsuitable profiles where the cloud does not fully attenuate the ceilometer beam or where there is significant backscatter from aerosols. By excluding profiles when the low cloud leads to instrument saturation (particularly in the Lufft instruments) or when the window transmission is low, and by accounting for the attenuation of the ceilometer beam by water vapour (in the Vaisala instruments), we show that ceilometers from different manufacturers can be successfully calibrated using this method. -Instrument malfunction can be identified by sudden changes in calibration. If either the window transmission or the pulse energy falls below 90% of normal values, then clearly the instrument sensitivity and the calibration will be different. When the window transmission falls below 90% the backscatter becomes noisy, probably due to the inhomogeneous nature of the layer of dust or dirt on the window, consequently it is essential that the window is kept clean if reliable data are to be obtained. If the pulse energy falls below 90% then it should be possible to correct the backscatter signal but the precise accuracy of this technique remains to be determined.  
750  
755

It has been demonstrated that the running 90-day mean calibration coefficient for each instrument over a year is constant to better than 5% with no detectable annual cycle. At the time of writing, profiles from 200 ceilometers from 17 countries are being distributed in near real time by the E-Profile programme of European  
760 Meteorological Services Network (EUMETNET) with the number expected to rise to about 700. E-Profile has decided to calibrate the Vaisala ceilometers using the cloud calibration technique described in this paper.

*Author contributions:* EH wrote the paper. All authors contributed to the scientific ideas in the paper EH and CCP wrote the code to perform the calibration. CCP and SB provided EH with access to observational data. All authors discussed the results and edited the manuscript.

765 *Acknowledgements:* This study was jointly funded by a Natural Environment Research Council (NERC) PhD Studentship and the Met Office Industrial CASE Partnership. The authors would like to acknowledge the contribution of the COST Action ES1303 (TOPROF) and in particular Ewan O'Connor and Maxime Hervo for many helpful discussions. We would also like to thank Mariana Adam, Joelle Buxmann and Jacqueline Sugier (Met Office) for their help and support during this PhD project.

770 **8 References**

Brown, P.R. and Francis, P.N.: Improved measurements of the ice water content in cirrus using a total-water probe. *J. Atmos. Oceanic Technol.*, 12(2), pp.410-414, 1995

Cossu, F., Hocke, K., Martynov, A., Martius, O., and Mätzler, C.: Atmospheric water parameters measured by a ground-based microwave radiometer and compared with the WRF model, *Atmospheric Science Letters*, *Atmos. Sci. Lett.*, 16, 4, 465-472, 2015.

Dupont, J. C., Haeffelin, M., Protat, A., Bouniol, D., Boyouk, N., and Morille, Y.: Stratus–Fog Formation and Dissipation: A 6-Day Case Study, *Boundary-Layer Meteorology*, 143(1), 207-225, 2012.

Hervo, M., Poltera, Y., and Haefele, A.: An empirical method to correct for temperature-dependent variations in the overlap function of CHM15k ceilometers, *Atmos. Meas. Tech.*, 9, 2947-2959, <https://doi.org/10.5194/amt-9-2947-2016>, 2016.

Hogan, R. J., Illingworth, A. J., O'Connor, E. J., and Baptista, J. P. V. P.: Characteristics of mixed-phase clouds. II: A climatology from ground-based lidar, *Quarterly Journal of the Royal Meteorological Society Quart. J. Roy. Meteor. Soc.*, 129(592): 2117-2134, 2003.

Hogan, R. J.: Fast, approximate calculation of multiply scattered lidar returns, *Applied Optics*, 45, 5984-5992, 2006.

Illingworth, A.J., Cimini, D., Haefele, A., Haeffelin, M., Hervo, M., Kotthaus, S., Löhnert, U., Martinet, P., Mattis, I., O'Connor, E.J. and Pothast, R., 2018. How can Existing Ground-Based Profiling Instruments Improve European Weather Forecasts? In Press, *Bull. Amer. Meteor. Soc.*, 2019

Illingworth, A. J., Cimini, D., Gaffard, C., Haeffelin, M., Lehmann, V., Löhnert, U., O'Connor E. J., and Ruffieux, D.: Exploiting Existing Ground-Based Remote Sensing Networks to Improve High-Resolution Weather Forecasts, *Bulletin of the American Meteorological Society Bull. Amer. Meteor. Soc.*, 96, 12, 2107-2125, 2015.

Kotthaus, S., O'Connor, E. J., Münkel, C., Charlton-Perez, C., Haeffelin, M., Gabey, A. M., and Grimmond, C. S. B.: Recommendations for processing atmospheric attenuated backscatter profiles from Vaisala CL31 ceilometers, *Atmos. Meas. Tech.*, 9, 3769-3791, <https://doi.org/10.5194/amt-9-3769-2016>, 2016.

Madonna, F., Amato, F., Vande Hey, J., and Pappalardo, G.: Ceilometer aerosol profiling versus Raman lidar in the frame of the INTERACT campaign of ACTRIS, *Atmos. Meas. Tech.*, 8, 2207-2223, <https://doi.org/10.5194/amt-8-2207-2015>, 2015.

Markowicz, K. M., Flatau, P. J., Kardas, A. E., Remiszewska, J., Stelmaszczyk, K., and Woeste, L.: Ceilometer Retrieval of the Boundary Layer Vertical Aerosol Extinction Structure, *Journal of Atmospheric and J. Atmos. Oceanic TechnologyTechnol.*, 25, 6, 928-944, 2008.

Markowicz, K. M., Zielinski, T., Pietruczuk, A., Posyniak, M., Zawadzka, O., Makuch, P., Stachlewska, I. S., Jagodnicka, A. K., Petelski, T., Kumala, W., Sobolewski, P., and Stacewicz, T.: Remote sensing measurements of the volcanic ash plume over Poland in April 2010, *Atmospheric Environment*, 48, 66-75, 2012.

Münkel, C., Eresmaa, N., Räsänen, J., and Karppinen, A.: Retrieval of mixing height and dust concentration with lidar ceilometer, *Boundary-Layer Meteorol.*, 124, 117, <https://doi.org/10.1007/s10546-006-9103-3>, 2007.

Nicholls, S.: The dynamics of stratocumulus: Aircraft observations and comparisons with a mixed layer model, *Quarterly Journal of the Royal Meteorological Society Quart. J. Roy. Meteor. Soc.*, 110, 466, 783-820, 1984.

O'Connor, E. J., Illingworth, A. J., and Hogan, R. J.: A Technique for Autocalibration of Cloud Lidar, *Journal of Atmospheric and J. Atmos. Oceanic TechnologyTechnol.*, 21, 5, 777-786, 2004.

Omar, A.H., Winker, D. M., Vaughan, M. A., Hu, Y., Trepte, C. R., Ferrare, R. A., Lee, K., Hostetler, C. A., Kittaka, C., Rogers, R. R., Kuehn, R. E., and Liu Z.: The CALIPSO Automated Aerosol Classification and Lidar Ratio Selection Algorithm, *J. Atmos. Oceanic Technol.*, 26, 1994-2014, <https://doi.org/10.1175/2009JTECHA1231.1>, 2009.

815 OSCAR (Observing Systems Capability Analysis and Review Tool): <https://www.wmo-sat.info/oscar>, last access: 27 June 2018.

Pinnick, R. G., Jennings, S. J., Chýlek, P., Ham, C., and Grandy, W. T.: Backscatter and extinction in water clouds, *Journal of Geophysical Research J. Geophys. Res.*: Oceans, 88, C11, 6787-6796, 1983.

820 Pawlowska, H., Brenguier, J. L., and Burnet, F.: Microphysical properties of stratocumulus clouds. *Atmos. Res.*, 55, 15–33, 2000.

Protat, A., Bouniol, D., O'Connor, E. J., Klein Baltink, H., Verlinde, J., and Widener, K.: CloudSat as a Global Radar Calibrator, *J. Atmos. Oceanic Technol.*, 28, 445–452, <https://doi.org/10.1175/2010JTECHA1443.1>, 2011.

Tang, Y., Lean, H. W., and Bornemann, J.: The benefits of the Met Office variable resolution NWP model for forecasting convection. *Met. Apps.*, 20: 417-426. doi:10.1002/met.1300, 2013.

825 Tsaknakis, G., Papayannis, A., Kokkalis, P., Amiridis, V., Kambezidis, H. D., Mamouri, R. E., Georgouassis, G., and Avdikos, G.: Inter-comparison of lidar and ceilometer retrievals for aerosol and Planetary Boundary Layer profiling over Athens, Greece, *Atmos. Meas. Tech.*, 4, 1261-1273, <https://doi.org/10.5194/amt-4-1261-2011>, 2011.

830 Westbrook, C. D., Illingworth, A. J., O'Connor, E. J., Hogan, R. J.: Doppler lidar measurements of oriented planar ice crystals falling from supercooled and glaciated layer clouds, *Q. J. R. Meteorol. Soc.*, 136, 260–276, DOI:10.1002/qj.528, 2010a.

Westbrook, C. D., Hogan, R. J., O'Connor, E. J., and Illingworth, A. J.: Estimating drizzle drop size and precipitation rate using two-colour lidar measurements, *Atmos. Meas. Tech.*, 3, 671-681, <https://doi.org/10.5194/amt-3-671-2010>, 2010b.

835 Wiegner, M., Madonna, F., Binietoglou, I., Forkel, R., Gasteiger, J., Geiß, A., Pappalardo, G., Schäfer, K., and Thomas, W.: What is the benefit of ceilometers for aerosol remote sensing? An answer from EARLINET, *Atmos. Meas. Tech.*, 7, 1979-1997, <https://doi.org/10.5194/amt-7-1979-2014>, 2014.

Wiegner, M. and Gasteiger, J.: Correction of water vapor absorption for aerosol remote sensing with ceilometers, *Atmos. Meas. Tech.*, 8, 3971-3984, <https://doi.org/10.5194/amt-8-3971-2015>, 2015.

840 Wu, Y., Gan, C. M., Cordero, L., Gross, B., Moshary, F., and Ahmed, S.: Calibration of the 1064nm lidar channel using water phase and cirrus clouds, *Applied Optics*, 50, 21, 3987-3999, 2011.

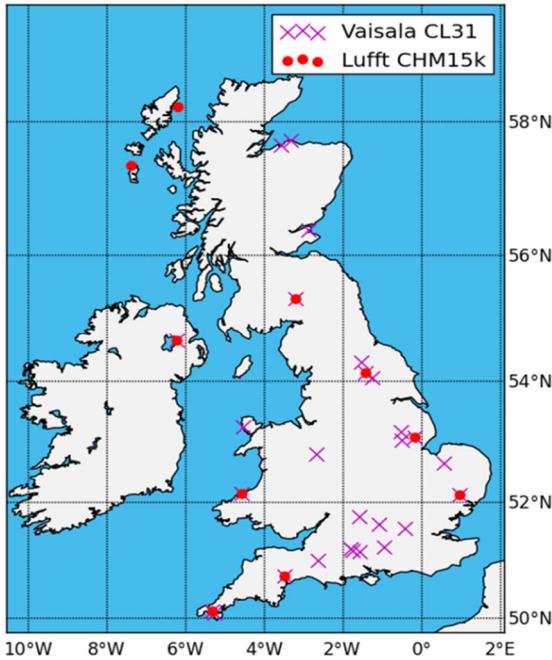


Figure 1: Location of Met Office ceilometers which record the full profile of attenuated backscatter. The Vaisala CL31s are indicated by a purple cross and the Lufft CHM15k by red dots.


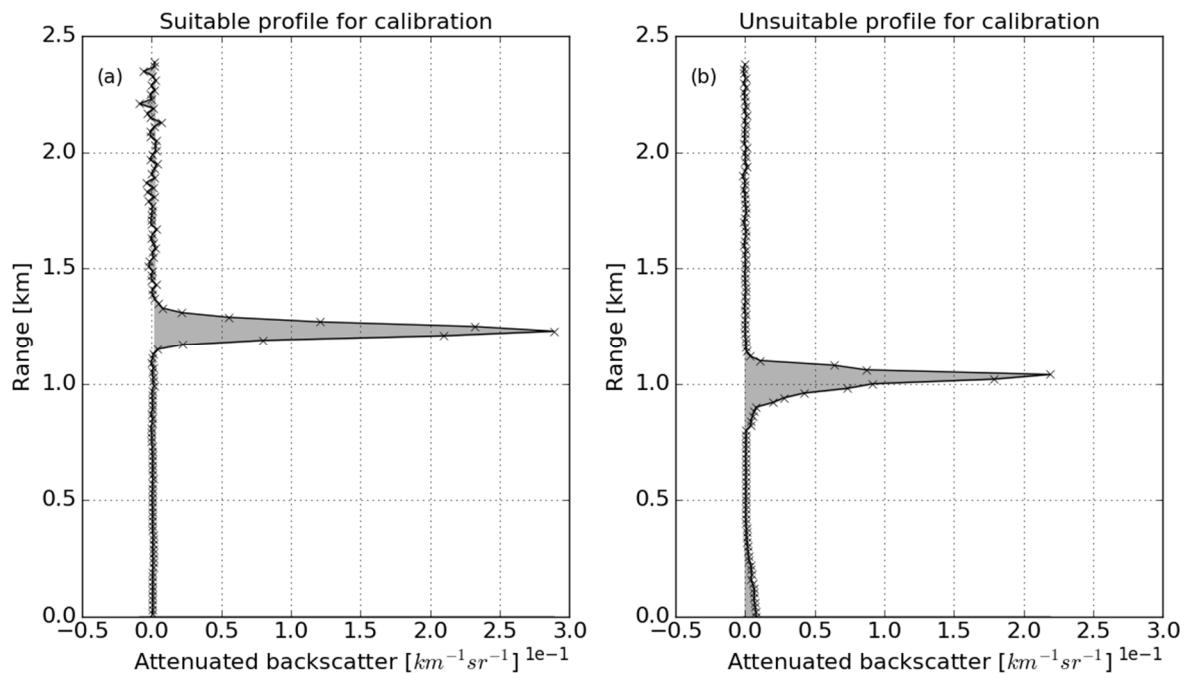


Figure 2: Profiles of attenuated backscatter through stratocumulus cloud. Panel (a) shows an example of a suitable profile for calibration. The integral of the profile (grey shaded area) is equal to  $\frac{1}{2\eta S}$  and, when calibrated, should give an S of  $18.8 \pm 0.8$  sr. Panel (b) shows an example of a profile unsuitable for calibration due to the high levels of aerosol in the first 200 m, indicated by the grey shading up to 200 m, and due to the

drizzle below the stratocumulus cloud, indicated by the slight increase in attenuated backscatter underneath the peak.

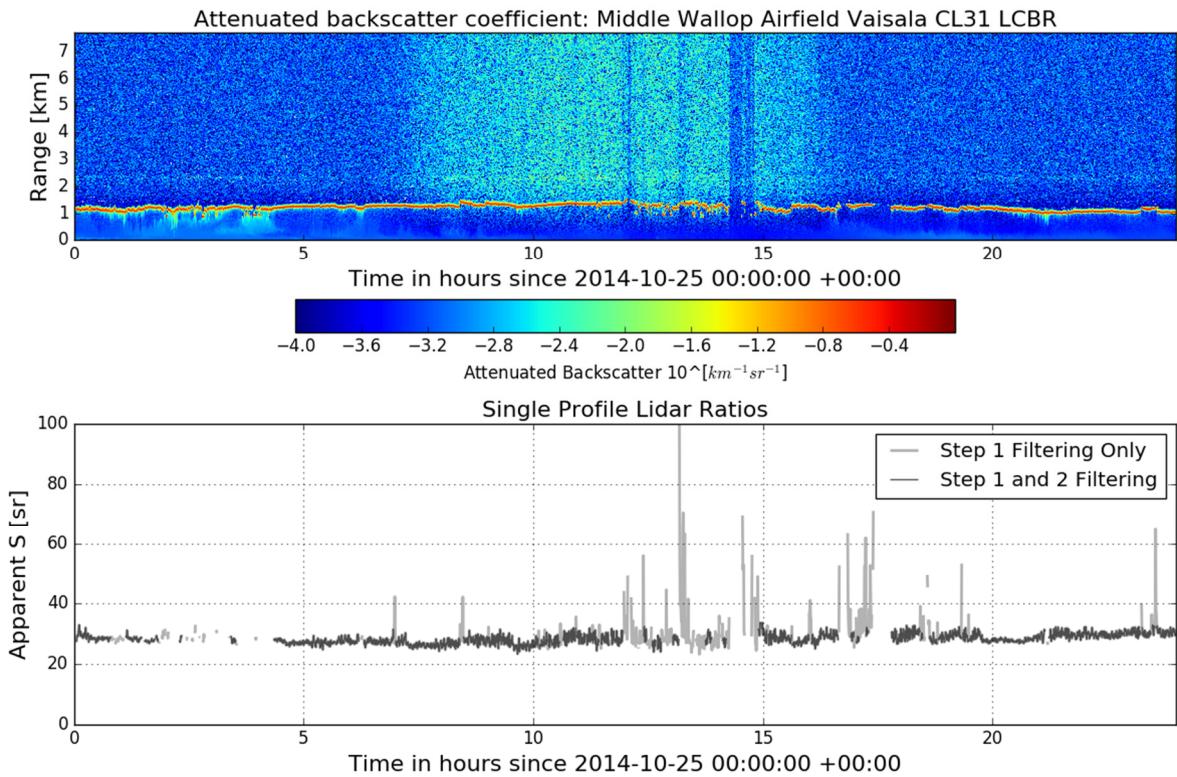

850 [Figure 3: \(a\) Uncalibrated attenuated backscatter vertical profiles \(colours shown on a log scale\) for 25th October 2014 from a CL31 ceilometer at Middle Wallop airfield \(51.1489 N, 1.5700 W\) and \(b\) the apparent lidar ratio for the same day. In panel \(b\), the grey line shows the apparent S for profiles that pass the step 1 filtering of the calibration algorithm and the black line shows the profiles that pass the step 2 filtering and are used to calculate the calibration coefficient.](#)

855

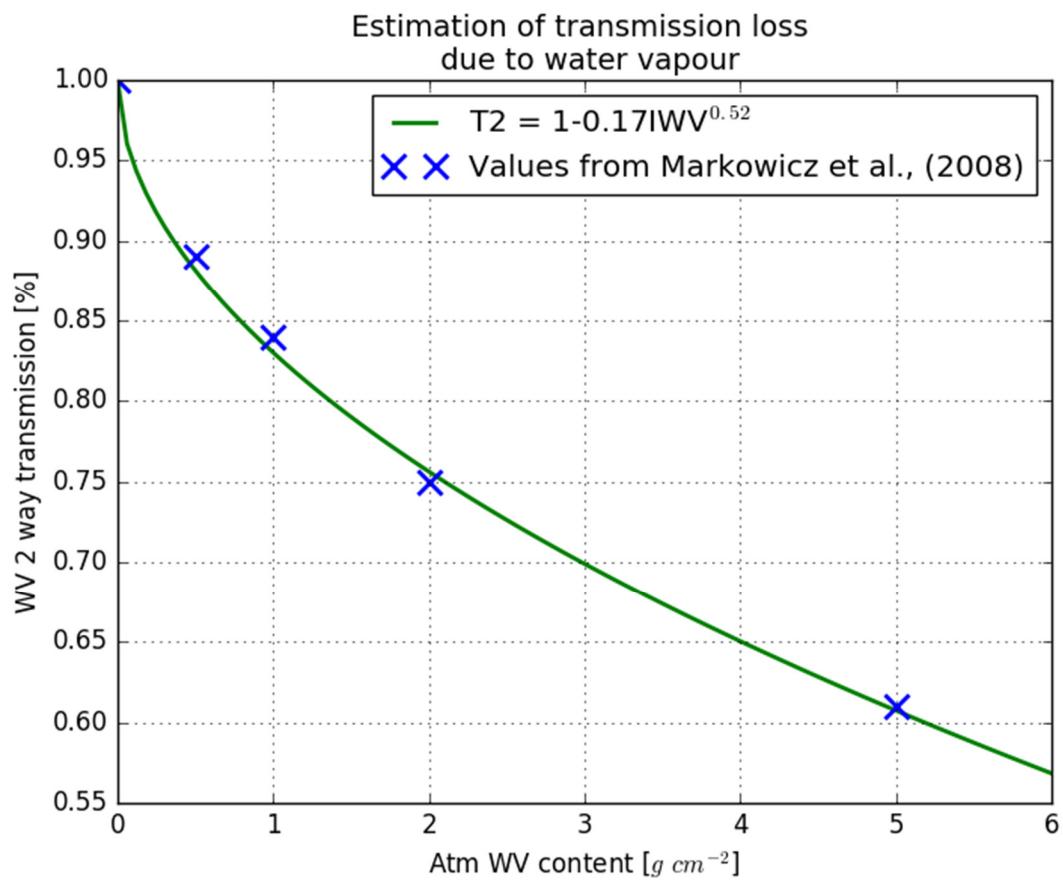


Figure 4: Estimated transmission loss due to the atmospheric water vapour content. The blue crosses are the values calculated by Markowicz et al. (2008) for a ceilometer with a wavelength of 910nm.

### Middle Wallop, 25-10-2014

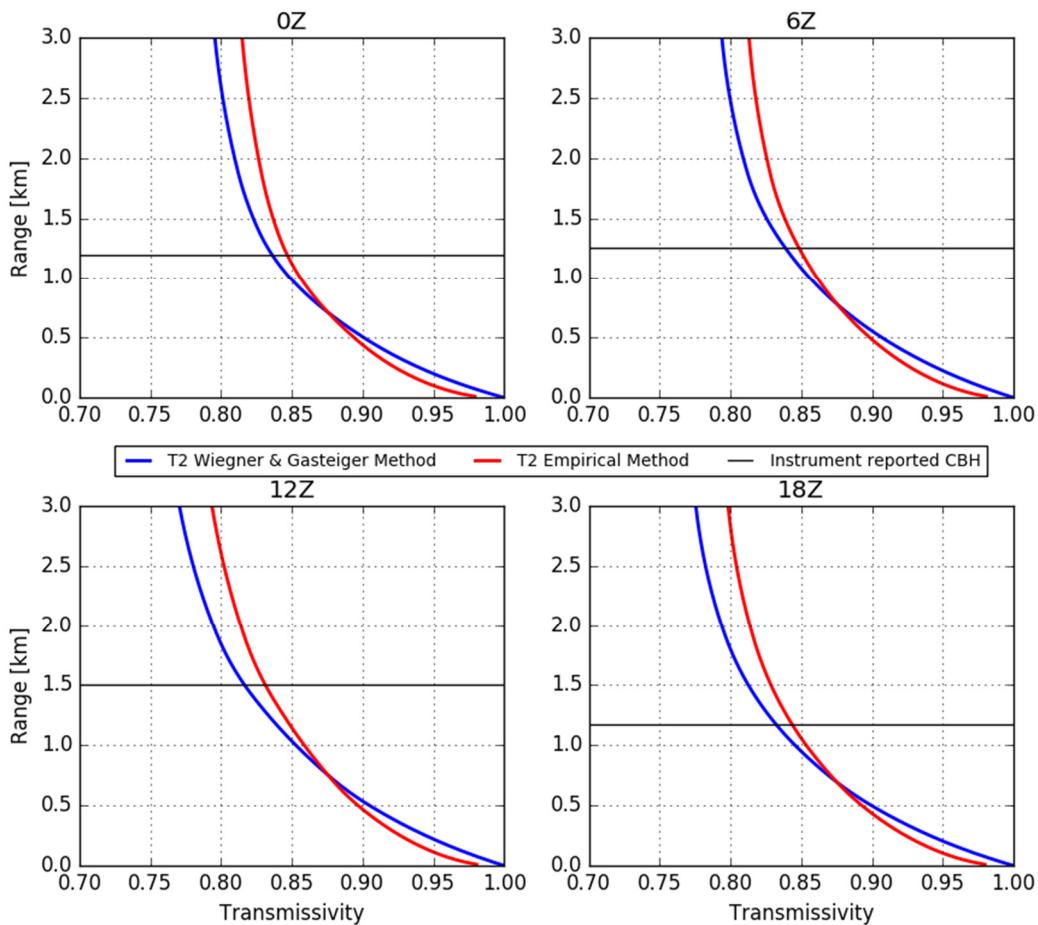


Figure 5: Comparison of water vapour transmission correction methods using ECMWF water vapour density profiles for 25th October 2014 at Middle Wallop, England. In blue, the transmissivity is calculated using WAPL (Wiegner and Gasteiger, 2015) and in red the transmissivity has been calculated using the empirical function shown in Fig. 4. The black lines show the instrument reported cloud base height at that time.

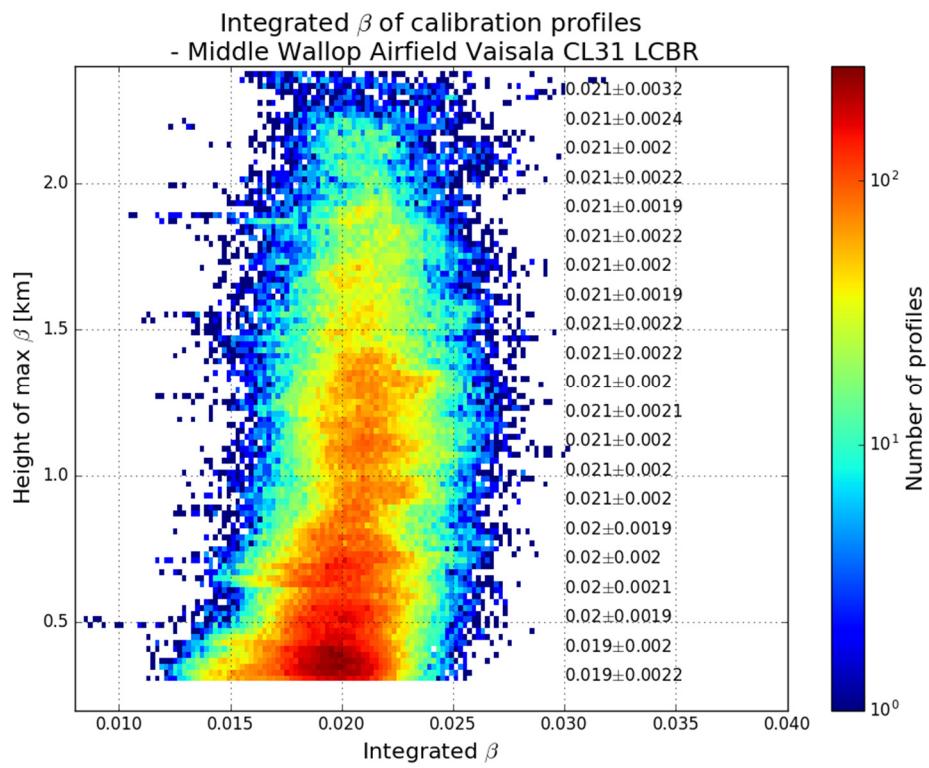
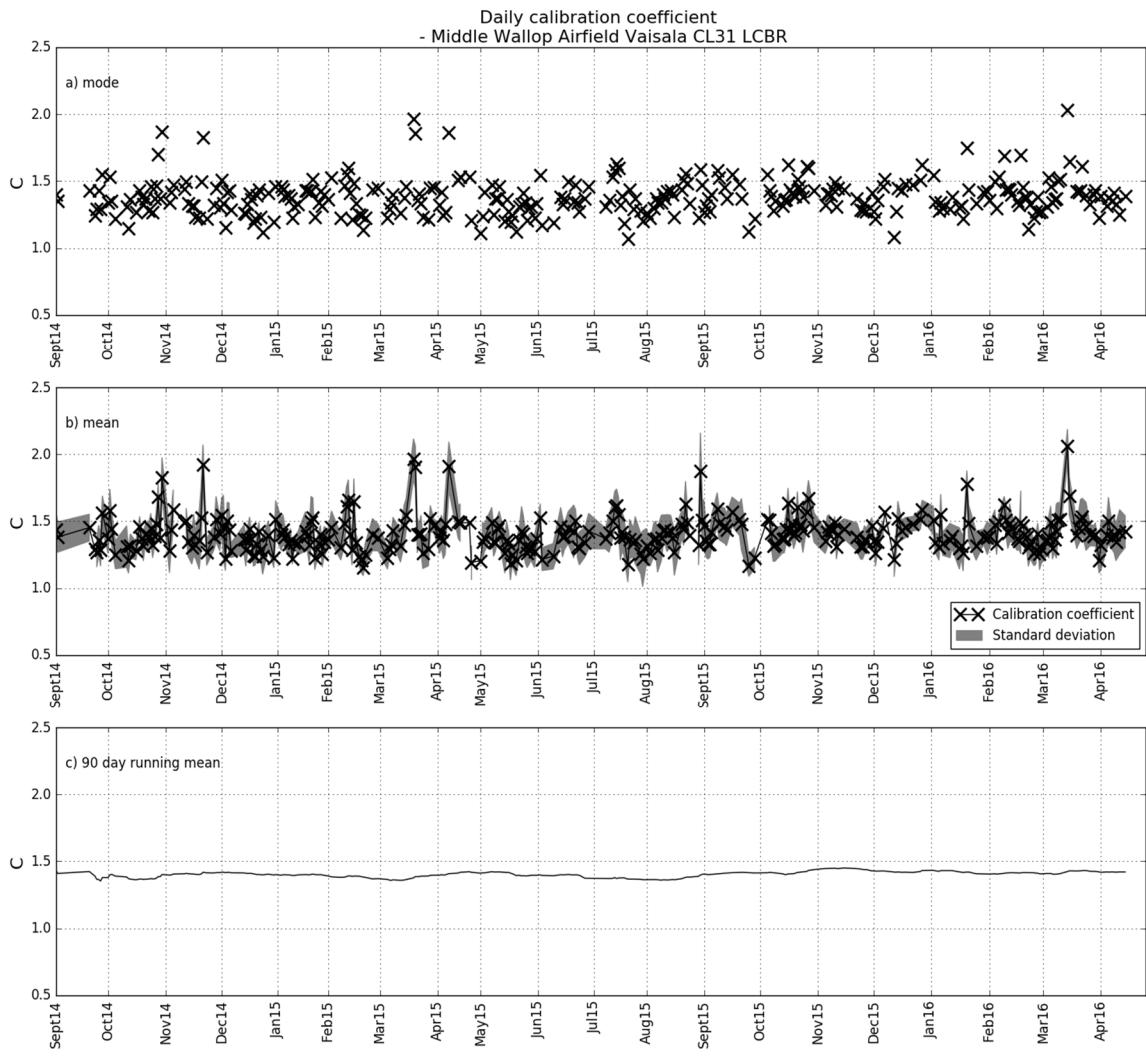


Figure 6: 2D histogram of integrated attenuated backscatter with range, with height dependent multiple scattering correction applied. Darker colours (towards red) indicate a higher density of profiles. The values shown along the right-hand side give the mean +/- the standard deviation of the integrated attenuated backscatter (units  $\text{sr}^{-1}$ ) at 100m intervals.

865



**Figure 7: Calibration Coefficient (C) for Middle Wallop CL31 from September 2014-April 2016. Each black cross represents a single day, calculated from profiles deemed suitable by the calibration algorithm. Panel a) shows the mode of C for each individual day, b) shows the mean of C for each day, with the standard deviation shaded in grey and c) shows a 90-day running mean for the 20-month period. The average of the daily modes is  $1.38 \pm 0.14$ , the average of the daily means is  $1.41 \pm 0.13$  and the average of the 90-day running means is  $1.40 \pm 0.021$ . The water vapour absorption correction has been applied, without which there would be an annual cycle in the calibration of about 12%.**

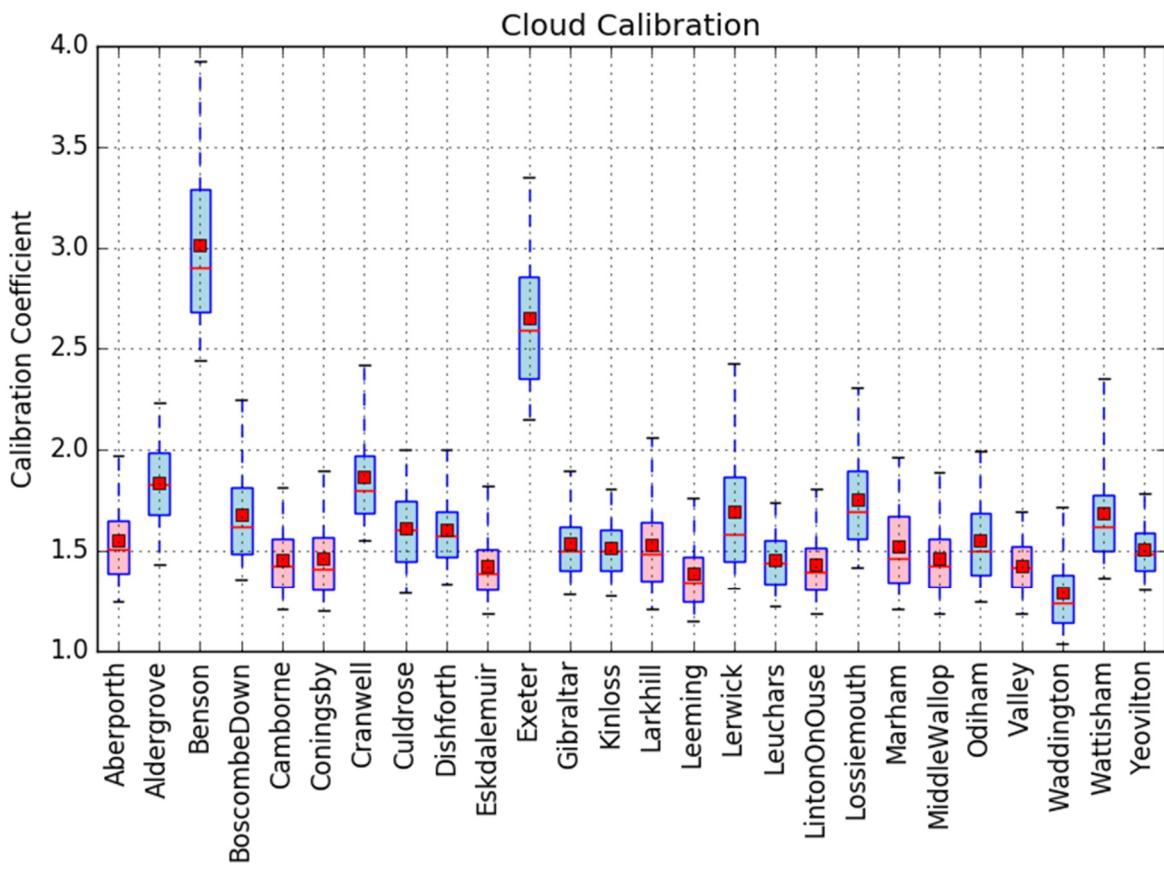


Figure 8: Calibration coefficient for each of the CL31 ceilometers in the UK Met Office network. 3 months of data (January-March 2015) have been used for each instrument. The number of suitable calibration profiles will be dependent on occurrences of cloud and, therefore, will vary for each instrument. The box outline represents 50 % of the calibration profiles and the whiskers extend to include 95% of the profiles (outliers have been excluded from plot). The horizontal red line in the box shows the median calibration coefficient and the smaller, filled box shows the mean. The boxplot is shaded by firmware version as given by the ceilometer files on 1st January 2015: pink for version 202 and blue for versions 170 and 172.

875

880

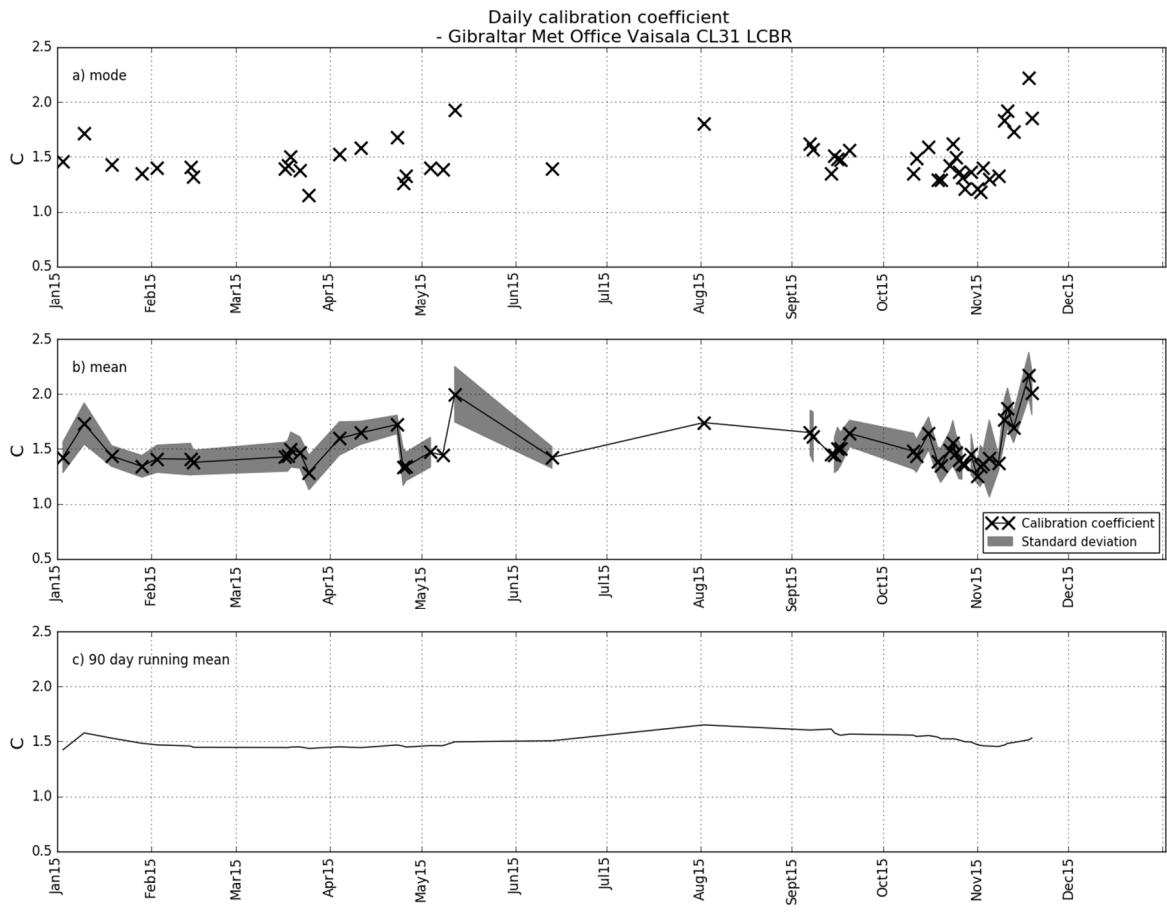


Figure 9: Calibration Coefficient (C) for Gibraltar CL31 from January-December 2015. Each black cross represents a single day, calculated from profiles deemed suitable by the calibration algorithm. Panel a) shows the mode of C for each individual day, b) shows the mean of C for each day, with the standard deviation shaded in grey and c) shows a 90-day running mean for the 12-month period. The average of the daily modes is  $1.48 \pm 0.21$ , the average of the daily means is  $1.51 \pm 0.19$  and the average of the 90-day running means is  $1.50 \pm 0.053$ .

885

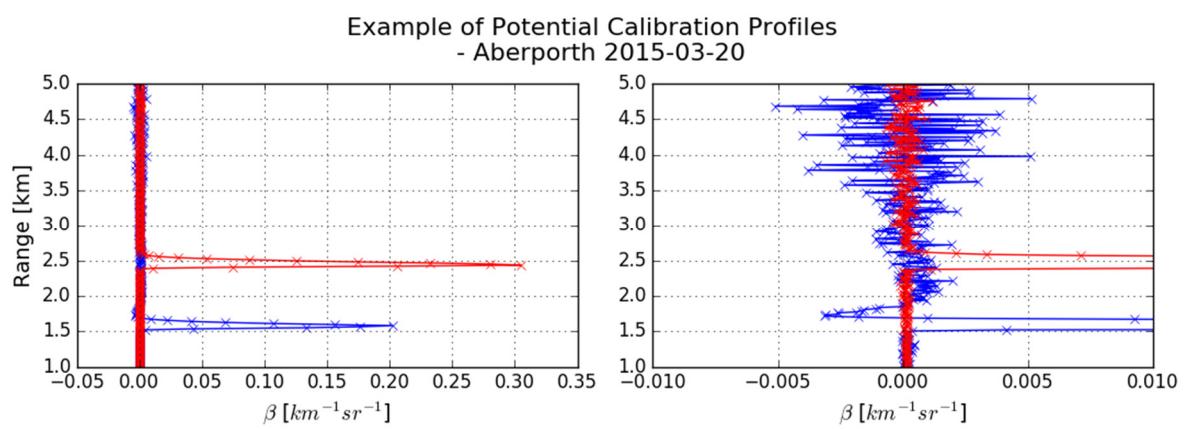
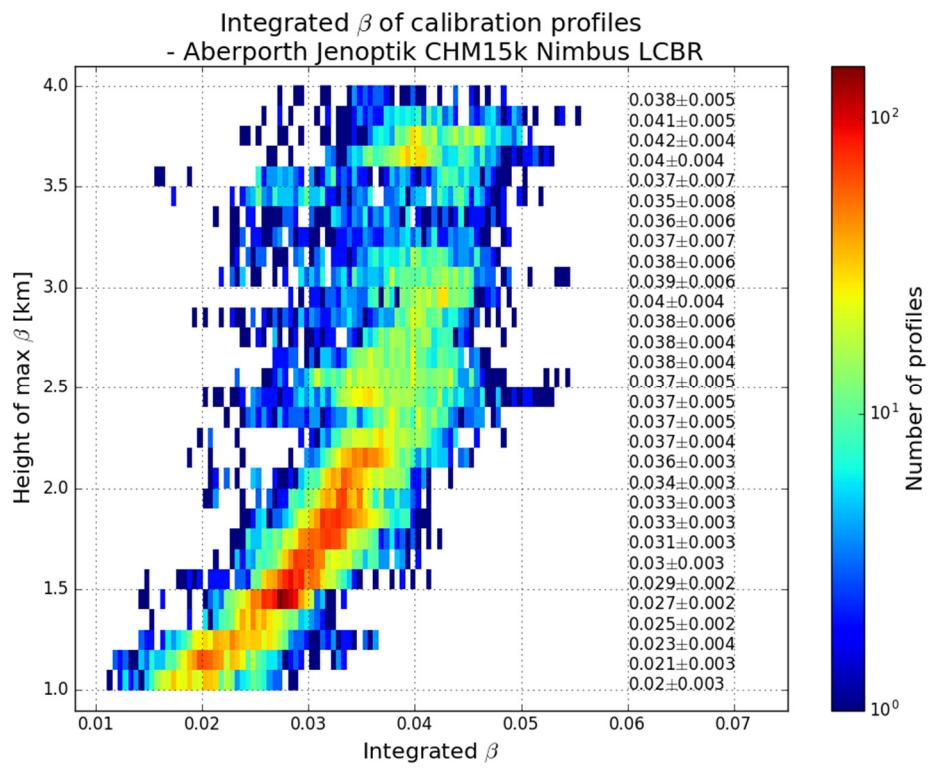
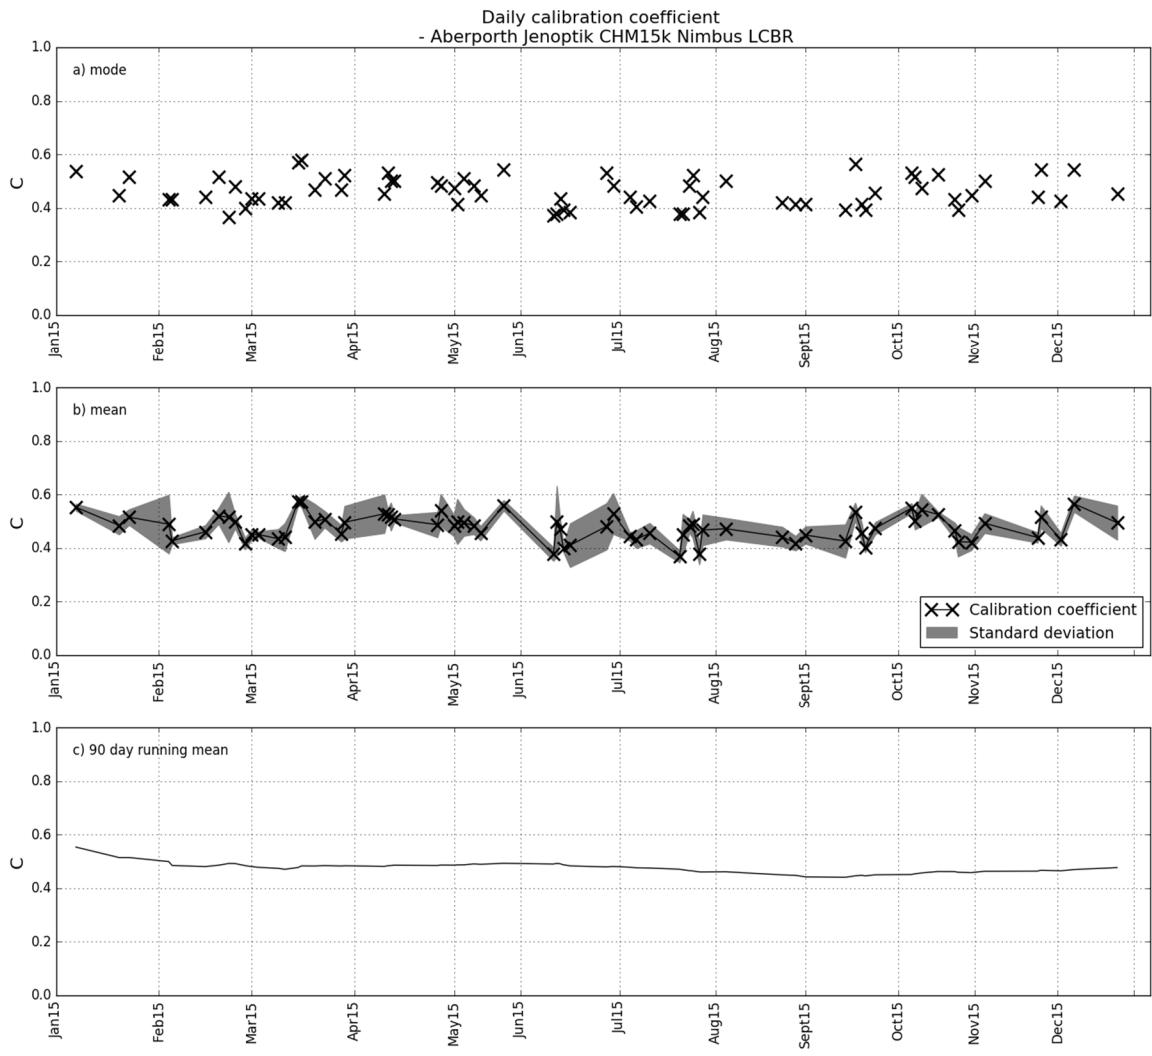


Figure 10: Two profiles of attenuated backscatter that detect liquid cloud from the Lufft CHM15k ceilometer at Aberporth on 20th March 2015 (second panel shows same plot on different scale). The profile in blue has a negative overshoot above the cloud, whereas the red profile does not.

890



**Figure 11:** As for Figure 6, but illustrating the saturation of the CHM15k ceilometer for most clouds with bases below 2km. 2D histogram of the value of the integrated attenuated backscatter in profiles used for calibration with range. A height dependent multiple scattering correction has been applied. Darker colours (towards red) indicate a higher density of profiles. The values shown along the right-hand side give the mean +/- the standard deviation of the integrated attenuated backscatter (units  $\text{sr}^{-1}$ ) at 100m intervals.



**Figure 12: Calibration coefficients for the Lufft CHM15k nimbus ceilometer at Aberporth ( $52.06^\circ$  N,  $4.33^\circ$  W).** Each black cross represents a single day, calculated from profiles deemed suitable by the calibration algorithm. Panel a) shows the mode of  $C$  for each individual day, b) shows the mean of  $C$  for each day, with the standard deviation shaded in grey and c) shows a 90-day running mean for the 12-month period. The average of the daily modes is  $0.46 \pm 0.05$ , the average of the daily means is  $0.48 \pm 0.05$  and the average of the 90-day running means is  $0.48 \pm 0.02$ .

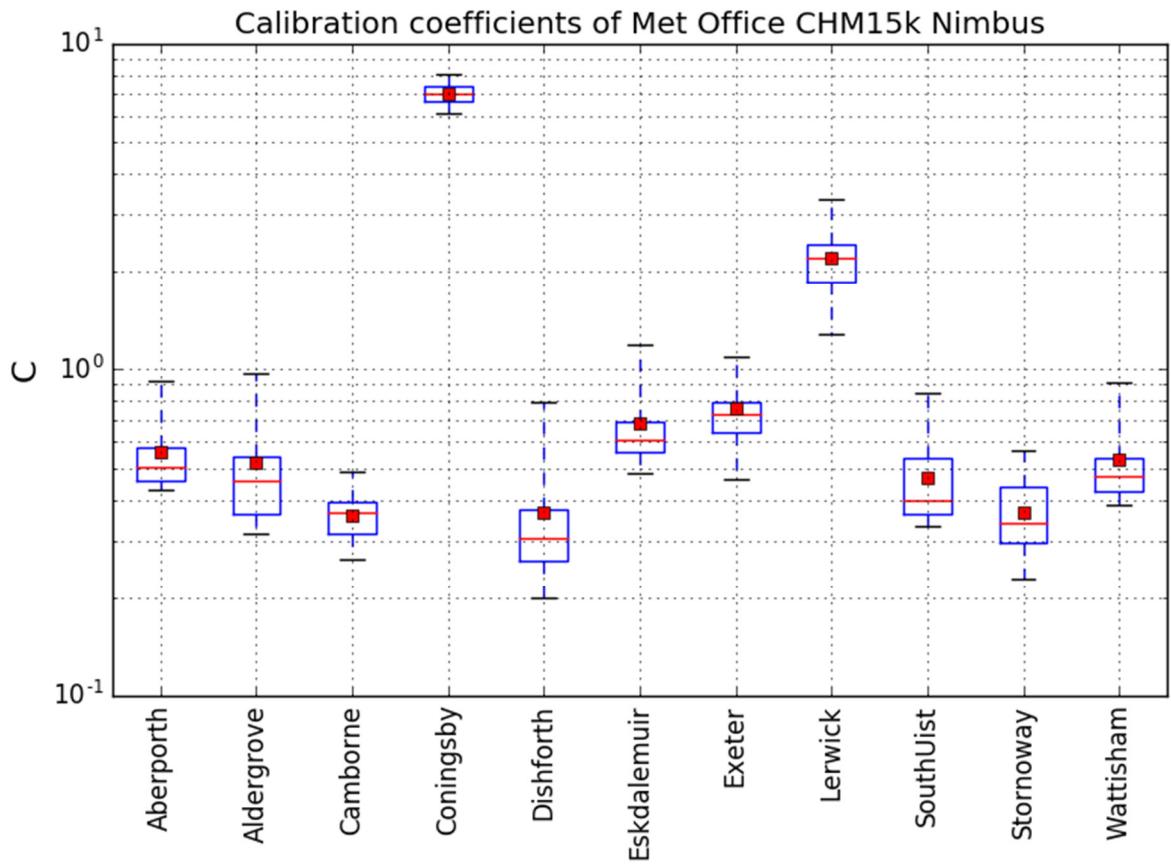


Figure 13: Calibration coefficient for each of the CHM15k Nimbus ceilometers in the UK Met Office network. 3 months of data (January–March 2016) have been used for each instrument. The number of suitable calibration profiles will be dependent on occurrences of cloud and therefore will vary for each instrument. The box outline represents 50 % of the calibration profiles and the whiskers extend to include 95% of the profiles (outliers have been excluded from plot). The horizontal red line in the box shows the median calibration coefficient and the smaller, filled box shows the mean.

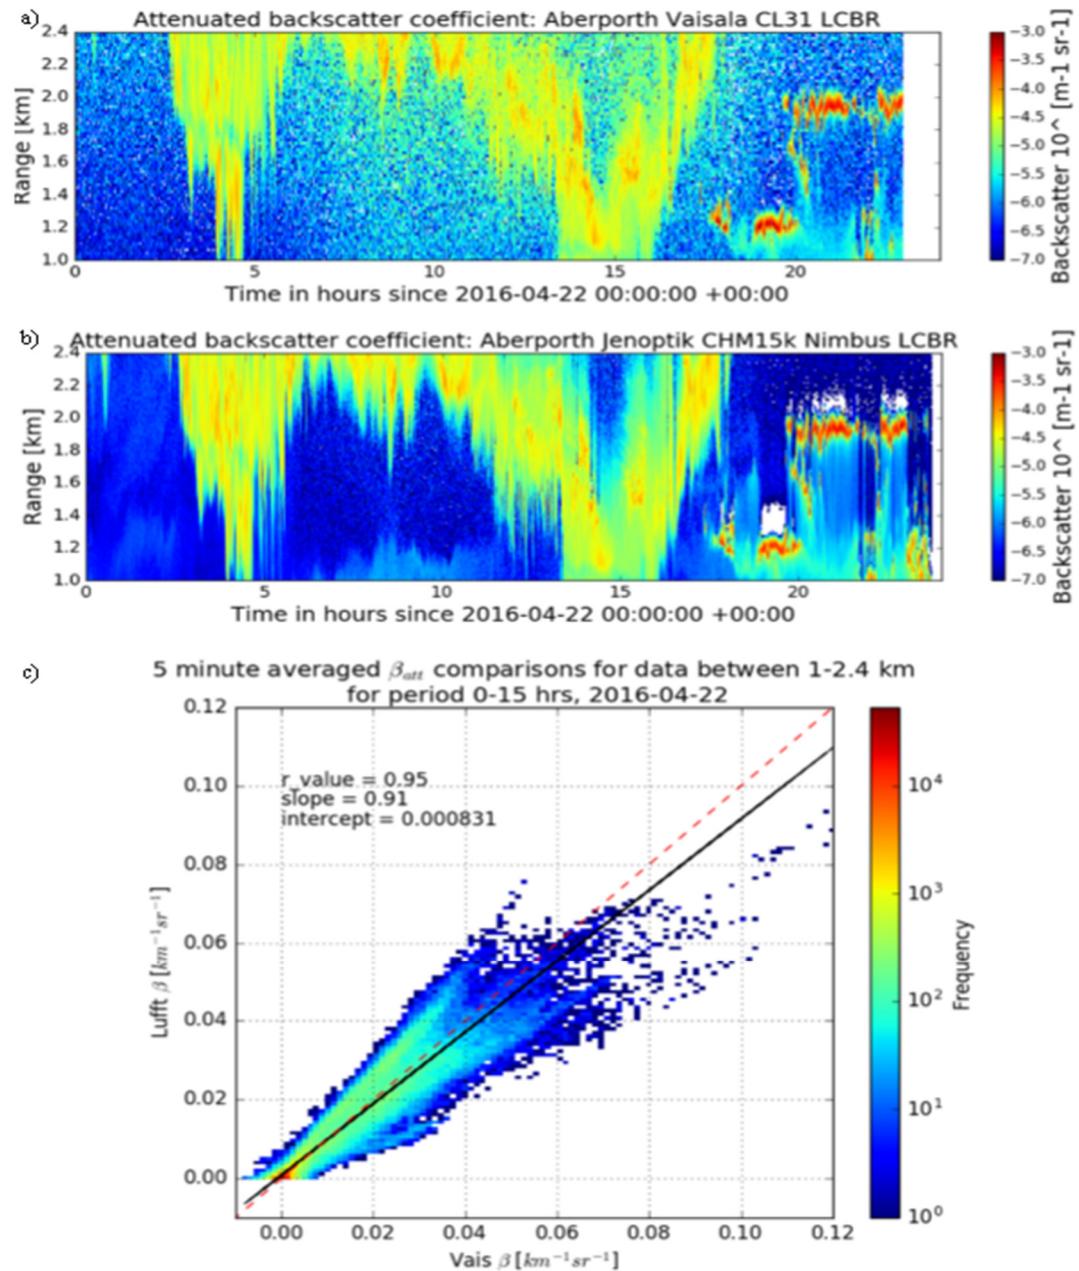


Figure 14: Quicklooks for the observed attenuated backscatter between 1 and 2 km are shown for the (a) Vaisala ceilometer and the (b) Lufft ceilometer. Panel (c) shows 5-minute averaged attenuated backscatter comparison for the Lufft and Vaisala ceilometers situated at Aberporth for 22/04/2016 between 0-15 GMT. Colour scale indicates the number of data points. Vaisala data has been corrected for water vapour attenuation and difference in wavelength, and has been interpolated to match the resolution of the Lufft ceilometer. The black line shows the linear fit of the data and the dashed red line is the 1:1 line.

910

915