

Response to Interactive Comment RC2 by Anonymous Referee #1 on Manuscript # amt-2019-11:

We would like to thank Reviewer #1 for their time and effort to provide detailed comments that have greatly improved the clarity of this work. We have responded to each comment below with the reviewer's comments shown in bold font and our responses immediately following them in plain font.

This is a clearly written manuscript that documents the performance of a closed-path absorption spectrometer for the measurement of NH₃ aboard an aircraft, with a particular emphasis on the utility of an active passivation technique.

The manuscript is appropriate for AMT, and should be published after addressing the following issues:

General comments: In several places (e.g. P2, L29; P3, L32; P4, L27; P4, L33), the manuscript uses the term 'detector' to refer to the instrument itself, whereas in other places, including in Figure 1, 'detector' is used to refer to the MCT detector that collects the transmitted radiation, but is not in contact with the gas flow of the system. I found the more general use of the term somewhat distracting/confusing and would suggest using either 'QC-TILDAS', 'spectrometer', or 'instrument' in whichever case is appropriate.

We have changed this term throughout the manuscript according to the reviewer's suggestions.

In the section discussing the vibrational and structural issues, the authors mention (P5, L35) 'reinforcing' the 'strain relief'. It was not clear to me if this involved providing more slack in the sampling lines, or making them more rigid. A little more information would be helpful.

We have amended the last sentence of Sect. 2.2.4 to read as: "However, this motion sensitivity could be minimized by keeping tubing lengths to a minimum and reinforcing the strain relief of the sample tubing connected to the QC-TILDAS enclosure inlet and outlet ports (e.g., rigidly securing all flexible tubing to the frame of equipment rack with cable ties) prior to installation on the aircraft."

In Section 4.1, the authors describe a zero overflow experiment. Does the (> 500 sccm) refer to the difference between the flow of zero air being delivered and the flow pulled by the instrument? Clarification would be useful.

Yes, we mean the 500 sccm flow to be the difference between the flow of zero air being supplied to the inlet and the flow pulled by the instrument. We have added the following sentence to clarify: "An overflow > 500 sccm (e.g., the difference between the flow of zero air being supplied to the inlet and the instrument's sample flow) was maintained to ensure that the sample stream was truly NH₃-free during this test.

In Section 5.1, the authors explore the impact of inlet aging and the use of the passivant on the time response of the system. While the proportion of the time response governed by the slow, "adsorptive", term was typically quite low ($D < 10\%$), the magnitude of the step change in concentration was rather large (50 ppb), so caution should be taken in extrapolating that result to ambient observations.

We have added the following caveat to Sect. 5.1: "While the proportion of the time response governed by the slow, "adsorptive", term was typically quite low ($D < 10\%$), the magnitude of the step change concentration utilized here is large (e.g., 50 ppb), so caution should be taken when extrapolating these results to ambient observations away from concentrated source regions."

Section 5.2.1 presents an interesting case study in which two intercepts of an intense NH₃ plume led to much different sampling efficiencies depending on whether or not the passivant was being added to the inlet, as the result of a recent pre-flight contamination. I found this section a bit confusing because the time period between 13:20 and 13:23, when

both the QC-TILDAS and the PTR-TOF-MS measured enhanced (and consistent) NH₃ is not described. One infers that the passivant was being used at the time, however it's not clear.

We have added the following clarification to this section in the paragraph where the PTR-NH₃ measurements are described:

5 “Passivant was not added to the PTR-ToF-MS; active continuous passivation was only applied the QC-TILDAS-based instrument during the selected times described above. It is clear by visual comparison to the PTR-ToF-MS that the non-passivated, “contaminated” QC-TILDAS instrument did not capture all of the expected ambient NH₃. This is evident from the differences in measured NH₃ mixing ratios reported in Fig. 8 during the time period between 13:20 and 13:23 when the QC-TILDAS was operated without passivant. During this time period the PTR-ToF-MS consistently measured more NH₃ than the QC-TILDAS, with the enhancement measured by the PTR during the plume intersect at 13:30 MDT showing an expected mixing ratio of ~45 ppbv. According to PTR-NH₃, the integrated NH₃ signal during the plume intersect at 13:30 MDT was only 14% less than the integrated NH₃ signal measured during the plume intersect at 14:00 MDT, and thus a significant enhancement in NH₃ should have been observed by the QC-TILDAS-based instrument. However, the non-passivated, “contaminated” QC-TILDAS-based instrument measured only a fraction of the NH₃ expected during the plume transect at 13:30 MDT, with the only attributable difference being NH₃ molecules adsorbing to the sampling surfaces.”

Specific comments:

P2, L11 – NH₃ is regulated under the Gothenburg protocol in some parts of the world.

20 We have added the following to the introduction: “While NH₃ is regulated under the Gothenburg protocol in some parts of the world (e.g., <http://www.unece.org/environmental-policy/conventions/air/guidance-documents-and-other-methodological-materials/gothenburg-protocol.html>), it remains an unregulated pollutant in the U.S. (Gilliland et al., 2008).”

P3, L33 – The ‘D’ in QC-TILDAS has traditionally stood for ‘differential’, not ‘direct’

25 We thank the reviewer for pointing out that prior usages of the acronym QC-TILDAS have referred to the ‘D’ as ‘differential’. Aerodyne Research Inc., the manufacturer of the mini-TILDAS NH₃ monitor used in these experiments, has recently changed the ‘D’ to stand for ‘direct’ since they feel it better reflects the measurement method. While there are prior publications that use ‘differential’, newer papers and manufacturer’s spec/product sheets (e.g.,

30 <http://www.aerodyne.com/sites/default/files/Product%20sheet%20NH3.pdf>) are now using the word ‘direct’.

P7, L41 (and subsequently) ‘Hydroscopic’ should be ‘hygroscopic’

We have made this correction.

Figure 8 caption – ‘colorded’ should be ‘colored’

We have made this correction.

Response to the interactive short comment on manuscript # amt-2019-11:

The manuscript assesses the performance of a closed-path, airborne-based ammonia instrument (Aerodyne Res. Inc.) by demonstrating the performance of active passivation under flight conditions. Ammonia is incredibly challenging to measure anywhere (with any technique) due to the significant adsorption/desorption effects on instrument/inlet surfaces, particularly on an airborne-based platform where temperatures, humidities, and ambient ammonia concentrations can vary dramatically. The authors show greatly improved performance when using the passivated versus unpassivated flows for sampling large NH_3 concentrations (10s-100s ppbv NH_3) from farms and biomass burning plume. The documentation of the instrument performance versus flight maneuvers was particularly valuable. This manuscript represents a large advance in airborne-based ammonia measurements, and the authors' experiences on using passivant additions in addition to /in lieu of frequent cleaning are important for future implementation of closed-path ammonia instruments in specific but also ammonia sampling more generally (laboratory experiments, calibrations, etc.). However, there remain some areas that require greater clarification to put the research in the proper context.

1. The response times, and applicability, to smaller NH_3 variations should be discussed (and backgrounds relevant to very low free tropospheric values, <ppbv). The detection limit needs better justification.

Thank you for these comments. See our responses below each specific comment/suggestion related to these topics.

In this study, the step change of NH_3 was created by turning off the calibration gas. The change is around 85 – 115 ppbv. This variation is uncommon for sites away from source regions. At high NH_3 concentrations and large variations, NH_3 observations may be less impacted by surface interaction because a “clean” sampling line only has a finite number of adsorption sites which could be quickly fill up under this condition. This effect has been reported by Ellis et al.(2010), and it may explain why passivation did not help to increase the response time of the instrument. At low NH_3 concentrations, a greater fraction of NH_3 molecules may interact with the inner surface.

We agree that a limitation of these experiments is a lack of tests with lower mixing ratios of NH_3 , which could affect the applicability of these results to some specific applications, namely the remote free troposphere. As the commenters point out, the effect of decreasing instrument response time with increasing step change concentration has already been extensively characterized by Ellis et al. Therefore, the main goal of this paper is to further the works of Ellis et al. (2010) and Roscioli et al. (2016) by characterizing the effects of passivant addition on instrument time response in flight. For this discussion we also note that the results of Ellis et al. were reproducible in our own experiments when time profiles were generated with various levels of step change concentrations. One of which included a step change from ambient levels of NH_3 (e.g., between 5 and 12 ppbv) to zero, which was generated by switching on the overflow injection of NH_3 -free air at the inlet tip after a period of sampling near homogeneous levels of ambient NH_3 for several minutes. All the same, we agree with the commenters that the text should be amended to clarify that these results may be most applicable to near source sampling because the instrument utilized for these experiments was optimized for sampling large and rapid gradients of NH_3 in smoke.

In response to this and the next comment, we have added the following text to Section 4.4:

“All the same, further measurements are recommended for assessing sampling biases that could arise during field measurements of low mixing ratios of NH_3 in clean environments following long periods of exposure to near source level concentrations. The potential for an adsorption-related “memory effect” of NH_3 (e.g., Williams et al., 1992) on the sampling surfaces following long-term exposure to high concentrations of NH_3 is discussed in following sections.”

And we added this text to Section 5.1.1: “In this study, the instrument response is rigorously tested with a single step change of NH_3 created by turning off a 50 ppbv calibration gas mixture. We note that such large variations in NH_3 mixing ratio may


not been full applicable to field measurements in unpolluted regions away from concentrated sources of NH_3 . As described by Ellis et al. (2010), large gradients in NH_3 may be less impacted by surface interactions because “clean” sampling surfaces only have a finite number of adsorption sites that could be quickly filled under high NH_3 conditions. At lower NH_3 concentrations, a greater fraction of NH_3 molecules may interact with the inner surfaces. This could explain why passivation did not help to increase the response time of the instrument.”

Roscioli et al. showed that t_{90} of a similar instrument was 12 sec for a step change of 3 ppbv (from 0 to 3 ppbv) without passivation (2). When 4 ppmv passivant was applied, t_{90} decreased to 2 sec for the same step change. The instrument can be considered clean since it was flushed with NH_3 -free and low NH_3 gases. Therefore, even a “clean” closed-path instrument may not be capable for high-frequency (>1 Hz) field application with small NH_3 variations without passivation, and passivant additions may still not work for fast operation (> 1 Hz) under clean conditions. The authors should discuss in more details about the applicability and effectiveness of passivation to field applications with relatively low NH_3 concentrations (e.g. flux measurements in rural area and airborne observations away from sources).

We greatly appreciate your comments with respect to the comparison of time responses that we collected with those reported by Roscioli et al. (2016). While we frame the results of the time response tests so that they can be directly compared to the works of Ellis et al. (2010) and Roscioli et al. (2016), we believe that it is difficult to compare the level of cleanliness of two different instrument systems. In this particular case, it may not be fair to say that our “clean” (aka. pristine, out-of-the-box, never-used-in-the-field) instrument is the same level of cleanliness as the copiously flushed, yet previously deployed instrument used by Roscioli et al. We are fortunate to know the history of both instruments, and surmise that the QC-TILDAS utilized by Roscioli et al. (2016) more closely resembles an instrument with a mid-level of cleanliness (similar to what we define as a “typical” operating condition) rather than the pristine, out-of-the-box condition that we referred to as “clean” in this work. This is because the instrument utilized by Roscioli et al. was a dual channel QC-TILDAS optimized to measure NH_3 as well as HNO_3 (aka. two well-known sticky molecules). Prior to lab tests, the instrument was deployed aboard the NSF/NCAR C-130 research aircraft in the 2014 FRAPPE field campaign where it had been exposed to near source levels of NH_3 and urban emissions in the Colorado Front Range. Further, during the lab tests, the dual channel instrument was used to test several strong bases as passivant agents for NH_3 and several strong acids as passivant agents for HNO_3 . In our experience with contamination and cleaning of sampling surfaces, we found that the instrument flow path could only be truly cleaned by replacing tubing and inlet components where possible and by performing several cycles of ethanol/water rinse followed by week-long periods of flushing the sample flow path with NH_3 -free air. The dual channel instrument was solely flushed with NH_3 -free air prior to lab experiments, but sampling surfaces were not systematically cleaned and replaced. For these reasons, we categorize the instrument used by Roscioli et al. as an instrument operating under a middle level of cleanliness, like our “typical” operating condition. We also point out that Roscioli et al. (2016) found that the NH_3 time response of the instrument continually improved with increasing passivation concentration, presumably with an eventual lower limit somewhere at or above the volumetric flush time. Therefore, the degree to which one wants to achieve >1 Hz sensitivity can be determined by the amount of passivant added to the sampling system. In the case of the flights discussed here, we made a compromise between passivant use and time response in order to achieve a reasonable temporal response while not using an excessive amount of passivant. All the same, we agree with the commenters that further discussion is warranted about the applicability and effectiveness of active continuous passivation to field applications with relatively low NH_3 concentrations, such as flux measurements in rural areas and measurements away from sources. We now include this statement in Sect. 4 and reiterate this point in Sect. 5. See the text pasted in response to comment above.

Fig. 10: Because of the nature of the very large concentrations measured, it is hard to discern just how well the instrument/technique can observe cleaner, free tropospheric ammonia levels after seeing large plumes. For example, while the correlation is impressive in Fig. 10 and shows the value of this overall approach, with a several second response time for NH_3 , the “peaks” and “valleys” may still be attenuated to some extent. It would be helpful to show a plot against a true 1 Hz tracer correlation instead of two instruments with 2-3 second response times.


We agree with the commenters suggestion of trying to compare with a true 1 Hz tracer. We have identified acetonitrile, measured with the PTR-ToF-MS, as a better 1-Hz tracer that is well correlated with NH_3 in smoke. Unfortunately, we do not have measurements from the PTR-ToF-MS during RF15 when the aircraft performed transects of the S. Sugarloaf fire and the NH_3 instrument was systematically operated with and without passivant in flight through smoke. Instead, we use measurements of acetonitrile from the Bear Trap Fire (RF09) conducted on 09 August 2018 to perform a similar linear regression comparison of fine structure features as that described earlier in Sect. 5.2.2. Briefly, we conducted linear regression analysis of scatter plots of NH_3 versus CH_3CN incrementally averaged from 1 to 5 seconds until linear regression resulted in a maximum R^2 value. We found the best fits resulted from regressions of measured NH_3 with the 1-Hz reported and 2-second averaged CH_3CN ($R^2 > 0.97$ and within 0.001 of each other). A timeseries of NH_3 and CH_3CN from an example plume transect of the Bear Trap Fire in RF09 is included here for discussion with the commenters and mentioned briefly in the text, but since we cannot produce the same figure for RF15 when the NH_3 instrument was systematically tested with and without passivant, we feel that adding this as a figure to the paper does not add much to the discussion. We also note that there is little hysteresis in the recovery of background ratios of NH_3 to CH_3CN following the plume transect in RF09.

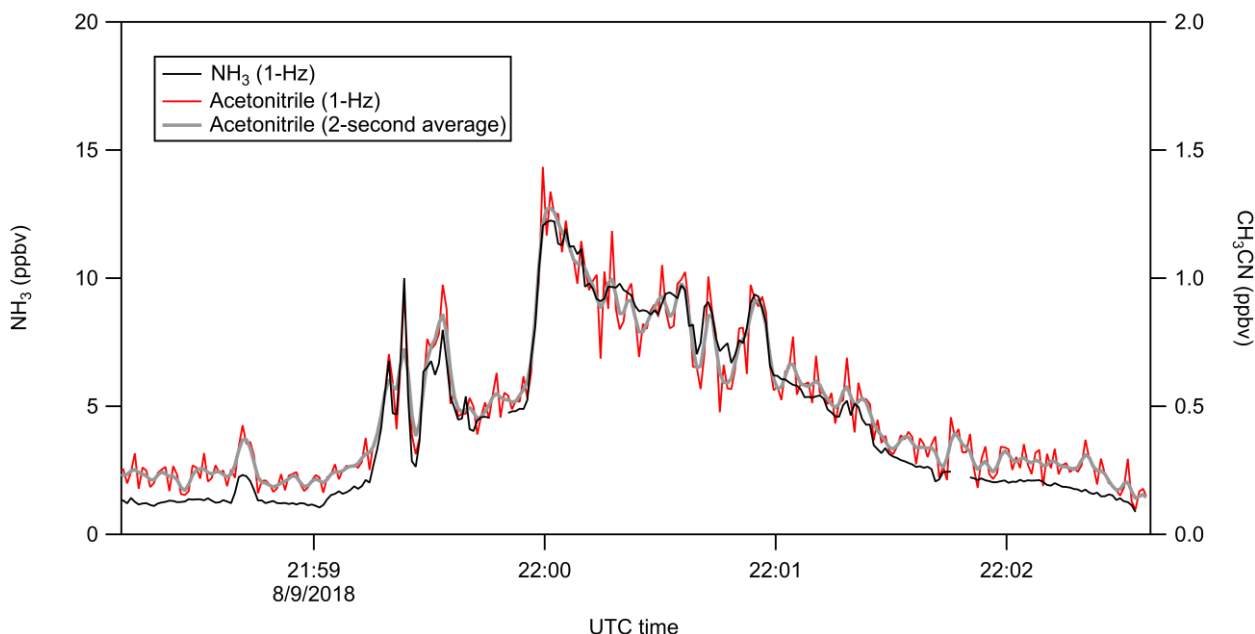

We assert that the NH_3 observations are well correlated with the 1-Hz reported CH_3CN data as well as the 2-second average of CH_3CN in the discussion by adding the following text to the end of Sect. 5.2.2: “Since the time response of the CO measurement was limited by its sample flow rate and inlet configuration, we also compare NH_3 to acetonitrile (CH_3CN) measured by the PTR-ToF-MS. CH_3CN is well correlated with NH_3 in smoke, and may be more representative of a true 1-Hz tracer owing to operation of the instrument inlet at a flow rate of ~ 15 SLPM. However, there are no measurements from the PTR-ToF-MS during RF15, the research flight during which the NH_3 instrument was systematically tested with and without passivant. Instead, we use measurements of CH_3CN from the Bear Trap Fire (RF09) conducted on 09 August 2018 to perform a similar linear regression analysis of fine structure features of measured NH_3 versus CH_3CN , with CH_3CN incrementally averaged up to 5 seconds. We find the best fits result from linear regressions of measured NH_3 with the 1-Hz reported and 2-second averaged CH_3CN ($R^2 > 0.97$ and within 0.001 of each other).“

There are also some differences between the start and end of the plumes in Fig. 10 in terms of the NH_3/CO ratio. As one progresses in the plume, the NH_3/CO ratio seems to get higher, which would be consistent if the background is growing. Differences in plume chemistry across the transect may be a reason for this, too. However, outside the plume (start/end of timeseries), the NH_3/CO level isn’t the same, either.

We recognize that there could be differences in the NH_3/CO ratio between the start and end of the plumes in Fig. 10. Indeed, differences in background mixing ratios of NH_3 compared to CO before and after the first transect of the S. Sugarloaf fire are apparent when the NH_3 and CO signals in Fig. 10 are magnified by a factor of 50 and 10, respectively. To highlight this difference, we have amended the time series in Fig. 10 as follows:

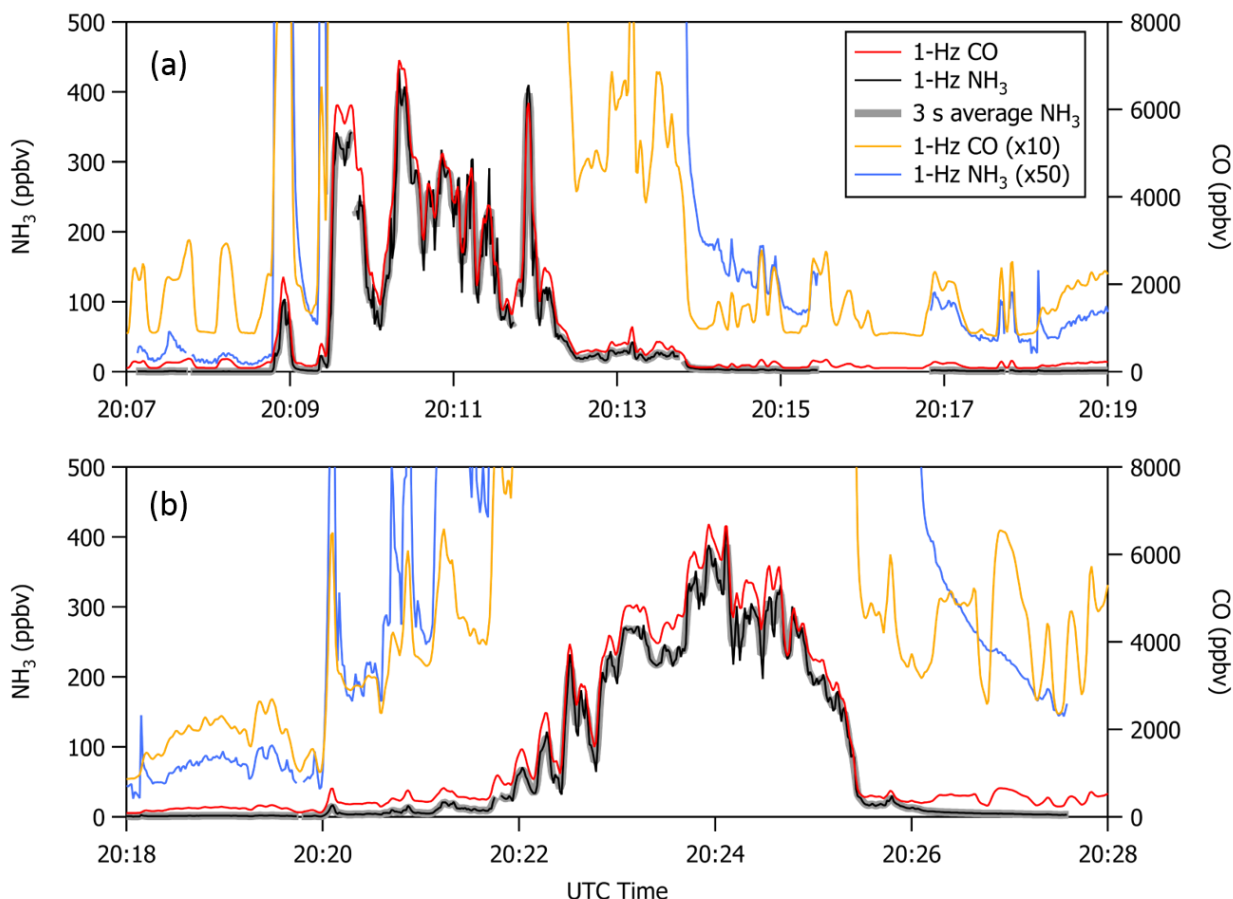

5

Updated caption for Fig. 10:

Time series of 1-Hz NH_3 (black lines) and CO (red lines) measured during a crosswind transect of the smoke plume from the South Sugarloaf Fire (RF15) on 26 August 2018. The transects represent nearly identical passes through the smoke plume with the only perturbation of the NH_3 instrument being operated (a) with passivant and (b) without passivant. Changes in fine structure features of NH_3 have the strongest R^2 correlation with CO when the NH_3 measurements are averaged to 3 s. A x50 magnified view of 1-Hz NH_3 (blue lines) and x10 magnified view of CO (orange lines) shows differences in background levels of NH_3 compared to CO before and after each plume transect.

10

[As context for this discussion, we note that the instrument inlet was overblown with NH_3 -free air for the duration of a 2-hour pre-flight exercise prior to take off. Following take-off, the instrument sampled a maximum of 5 ppbv NH_3 during ascent out of Boise and was then exposed to < 1 ppbv NH_3 for 1-hour during transit to the S. Sugarloaf fire.]


15

As the commenters suggest, there could be several causes for the differences in NH_3/CO ratio observed before and after the plume transect in Fig. 10. One reason could be physical differences in plume chemistry, mixing, or background composition. Another could be “memory effects” in the sample plumbing due to retention of NH_3 adsorbed to sampling surfaces following exposure to NH_3 mixing ratios in excess of 400 ppbv (Williams, et al., 1992). The observation could also reflect some combination of both. While distinct differences in background are apparent in Fig. 10, we note that differences in

20

background before and after the plume were not always observed during WE-CAN research flights (e.g., RF07 conducted on 06 August 2018 described in the next section of this response). Since the root of the differences are not immediately obvious and because differences seem to vary among the WE-CAN research flights, we now also include a response time for the signal recovery shown in Fig. 10 assuming the worst-case scenario that the differences in background are solely attributed to memory effects on the sampling surfaces. In this worst case, the time for the NH_3 measurement following the plume transect to recover to near background mixing ratio levels observed prior to the plume transect (e.g., 1 ppbv) is roughly 250 s. This time frame most closely resembles $t_{99,obs}$ for the “typical” operating condition when operated with or without passivant. To highlight the commenter’s points, we have amended Sect. 5.2.2 with the following text: “Differences in background mixing ratios of NH_3 and CO measured before and after the first transect of the smoke plume from the S. Sugarloaf fire are apparent in the magnified timeseries for each in Fig. 10. The differences in NH_3/CO ratio observed at 20:14 UTC and 20:25 UTC following in-smoke measurements of NH_3 that exceeded 400 ppbv could have resulted from physical differences in plume chemistry, mixing or background composition on either side of the plume, adsorption-related memory effects in the sample plumbing due to retention of NH_3 molecules adsorbed to the sampling surfaces (Williams et al., 1992), or a combination of both. Since the root of the differences are difficult to distinguish and may vary among the WE-CAN research flights, we utilized these differences to characterize the instrument time response given the worst-case scenario that the differences in background observed in Fig. 10 are solely attributed to memory effects on the sampling surfaces. In this worst case, the response time for the NH_3 measurement following the plume transect to recover to near background mixing ratio levels observed prior to the plume transect (e.g., 1 ppbv) is roughly 250 s. The time frame most closely resembles $t_{99,obs}$ for the “typical” condition when the instrument is operated with or without passivant. This recovery time and “typical” cleanliness condition are within our expectations for the instrument during this research flight (RF15) since the instrument had routinely been used to sample near source concentrations of NH_3 in smoke during several prior consecutive research flights without refreshing the sampling surfaces between flights.”

Related to this overall point, on the large y-scale axis (500 ppbv NH_3) in Fig. 10, while the concentration looks to be “close” to zero, in reality on this scale it could be numerous ppbv NH_3 . Even if the instrument response time is nominally on the order of a few seconds, going from 400 ppbv NH_3 to sub ppbv NH_3 could take a long time and may result in biases in clean conditions in the free troposphere. It may be helpful to show a vertical profile of NH_3 in the ascent out of Greeley (where high agricultural emission concentrations exist) and compare it to another, short-lived boundary layer tracer that would be highly enhanced in the boundary layer vs. the free troposphere. On the left below, I show a vertical profile of NH_3 from the NASA DISCOVER-AQ California in the San Joaquin Valley (taken from Sun et al., 2015), where the importance of the authors’ large improvement is clearly validated (needed), but where concerns of going very high NH_3 to nominally sub-ppbv NH_3 at high altitude could still be an issue even with this approach. Also attached on the right is a profile of NO_2 , ethane, and CN in the Greeley area from DISCOVER-AQ Colorado. I’m not sure if these are necessarily the best tracers per se from a quick look, but one can see very sharp gradients at the top of the boundary layer, and it would be illustrative to see how the shape of the NH_3 profile compares to other ~ short-lived tracers when ascending/descending across the mixed layer height. WE-CAN should have plenty of such measurements on the C-130 to compare.

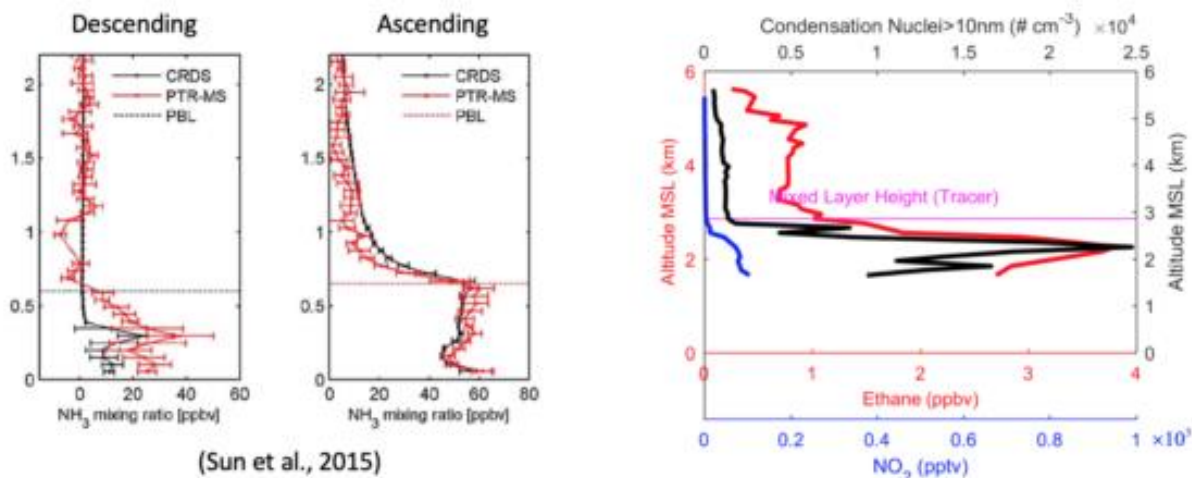

(Sun et al., 2015)

We agree that comparing vertical profiles from an ascent and descent is a great suggestion. While we do not have extensive enough vertical information from the test flights near Greeley, we do have a spiral over the California Central Valley about 60 miles southeast of Sacramento during WE-CAN research flight RF07 conducted on 06 Aug 2018. The spiral aimed to sample aged smoke in the Central Valley, and thus consisted of a descent followed by a spiraling ascent spanning between 4.5 km and 1.2 km AGL. As such, the observations (shown below) likely reflect a combination of aged smoke and agricultural emissions. Changes in NH_3 are consistent with changes observed for other tracers. While it may appear that there is some hysteresis in NH_3 compared to CO and CH_4 around 1.5 km as the aircraft ascends through the mixed layer, a closer look (e.g., NH_3 magnified $\times 10$ in the figure below) shows that NH_3 mixing ratios immediately drop to ≤ 200 pptv. To put these observations into context of the "memory effect" discussion above, it should be noted that the maximum NH_3 mixing ratio prior to ascent during the spiral in RF07 was < 15 ppbv compared to the background measured in RF15 following a smoke plume transect where NH_3 was > 400 ppbv. A systematic analysis of the WE-CAN research flights for physical differences in plume chemistry, mixing, background composition, and hysteresis with plume concentration are beyond the scope of this work, but several of these topics are forthcoming in WE-CAN publications. Therefore, we include the discussion of a worst-case scenario of hysteresis in the manuscript, and only provide the following plots of vertical profiles for discussion with the commenters.


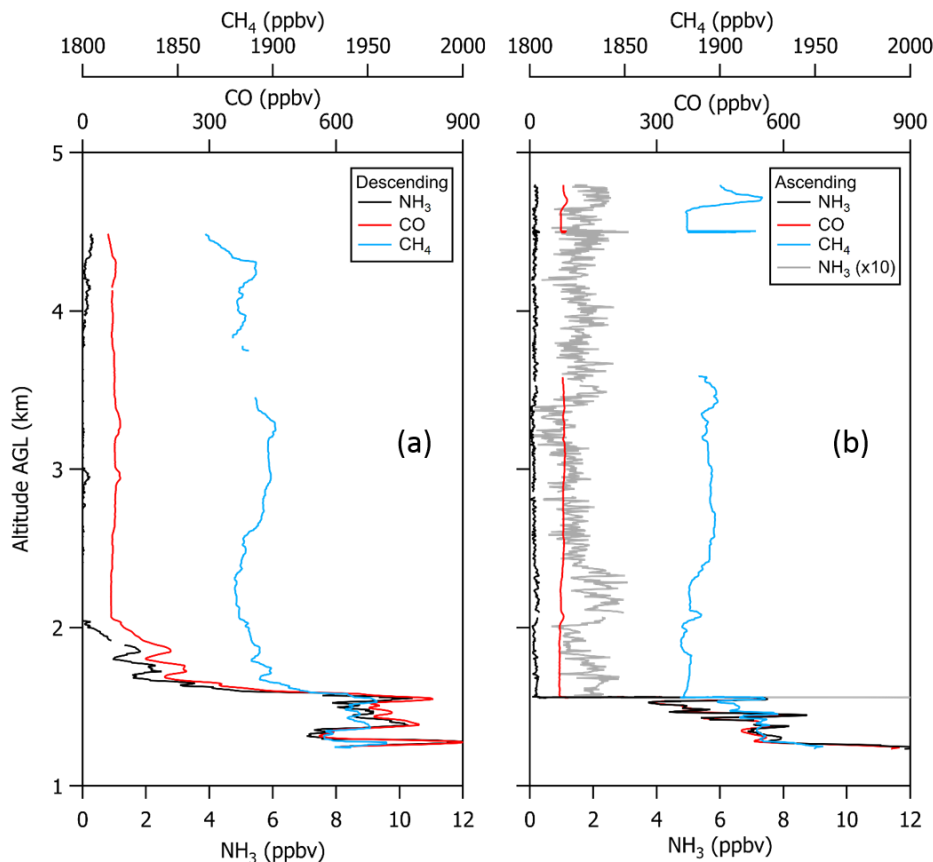


Figure 3: It is hard to see on Fig. 3a, but the constant altitude segments seem to show quite a bit of variability in the background, say, from -0.2 to +0.2 ppbv NH_3 within an altitude level for a given 1 Hz measurement. This calls to question as well the accuracy of anything < 0.5 ppbv, given that the background is changing by 0.4 ppbv. What were the ascent rates/g's after each constant altitude leg? The 50 pptv NH_3 sensitivity to typical flight maneuvers mentioned in the text doesn't seem consistent with Fig. 3a. If most of the variability is due to the ascent portions (g-forces), then perhaps a 1 Hz timeseries of the constant leg would be helpful. Also, how "polluted" was NH_3 prior to overfilling the inlet for a zero for these flights upon takeoff in Broomfield? How often was it zeroed vs. sampling? 10% duty cycle? Entire flight? 50%? The wording wasn't clear in the text for this portion of the flight.

The symbols and error bars in Fig. 3 represent the mean and 3s standard deviation of the mean measured zero level during constant altitude legs. Here, we purposefully depict the 3s standard deviation to illustrate the range of variability with respect to 3 times the Allan deviation, which we defined as the instrument's limit of detection. However, it is true that the zero signal level in Fig. 3 spans ± 200 pptv around zero, or 400 pptv total. While we continue to report 3 times the precision as determined from the Allan variance since this is how the detection limit for similar instruments is reported in the literature, we have added the following to Sect. 4.1: "We note that the true detection limit of the instrument in flight may be better represented by the full range of variability about the mean zero signal level from the observations in Fig. 3 (e.g., an instrument detection limit of 400 pptv)." We have also added this information to the abstract.

Ascent profiles were typically performed at ~1000 ft/min. The 50 pptv sensitivity reported in Fig 4 and Sect. 4.2 is specific to turbulence and turns. To further clarify the variations in NH_3 zero signal level with altitude in Fig. 3, accelerations at the onset of an ascent at 1000 ft/min were measured to be 0.4 g for the up-down motion, 0.1 g for the side-side motion, and 0.07 g in the fore-aft motion. Given the accelerations during ascent and the slopes of the measured motion sensitivities (in units of ppbv/g) determined from Fig. 4., it is reasonable to expect as much as 400 ppt of variability from motion sensitivity. Sect. 4.1 and 4.2 have been updated with the following text to clarify the observations during ascent between constant altitude legs in Fig. 3: “It should also be noted that large accelerations in the up-down and fore-aft dimensions are also significant at the onset of vertical ascent. Accelerations measured in the up-down and fore-aft motions at the onset of a 1000 ft/min vertical ascent were measured to be 0.4 g and 0.08 g, respectively. Given the slopes above, these accelerations correspond to a maximum change in NH_3 zero signal level of 400 pptv during ascent, which is consistent with the variability in zero signal level observed in Fig. 3 when ascending between constant altitude legs.”

We have also added a time series of the vertical ascent profile while overblowing the inlet tip with NH_3 -free air to the bottom of Fig. 3, as shown here.

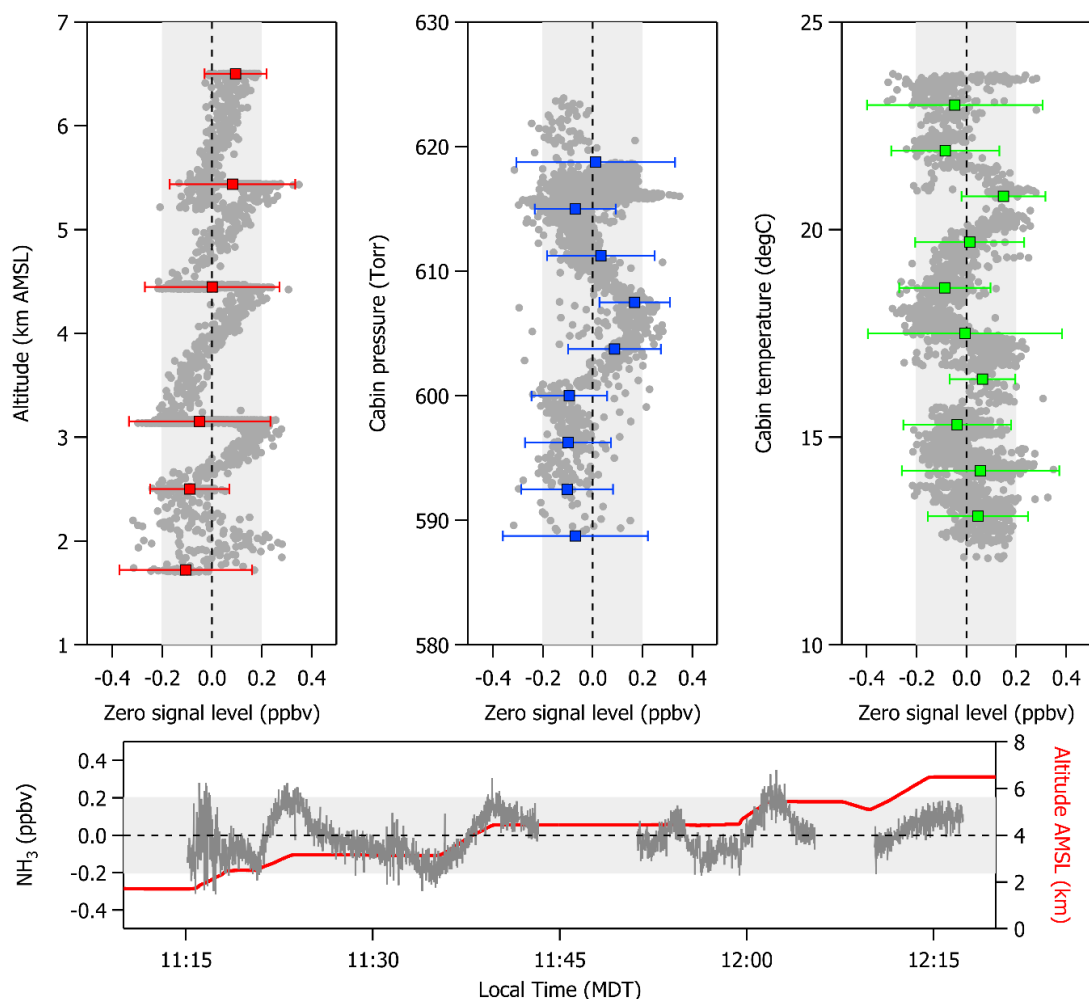

Updated caption for Fig. 3:

In-flight variations in zero signal level (in units of ppbv of NH_3) with respect to changes in (a) altitude, (b) cabin pressure, and (c) cabin temperature. A time series (d) illustrates the effects of motion sensitivity on the zero signal level as the aircraft

initiates an ascent and then levels off at a constant altitude. Gray symbols and lines represent the 1 s average of all of the 10-Hz data points collected in flight while overblowing the inlet tip with NH₃-free air; the red line in the time series is altitude AMSL. Colored symbols and error bars in the vertical profiles represent the average NH₃ zero signal and 3s standard deviation for each constant altitude level, 5 Torr increments in cabin pressure, and 2°C increments in cabin temperature.

5 Variations are largely within ± 200 pptv (denoted by the light gray shaded areas).

For further context, we have also added the following detail to Sect. 4.2: “For these experiments, the instrument inlet was continuously overflowed with NH₃-free air for the duration of a 3-hour pre-flight exercise prior to take off. Overflowing the inlet was purposefully done to keep the instrument system free of contaminants (e.g., exhaust from other aircraft and ground-based support equipment) prior to sampling in flight.”

We added similar info to Sect. 5.2.2: “During WE-CAN, the NH₃ instrument was typically zeroed between crosswind transects of a wildfire smoke plume when in background air and either just prior to or during turns. The instrument was zeroed every 10-20 mins during transits from Boise to the wildfires sampled with the frequency of zeros depending on the transit time. Zeros measured during WE-CAN research flights were typically collected for a period of 1 to 2 minutes, a duration much greater than the instrument response time, to ensure that zeros were measured well within 90% of the final zero signal level. Prior to each research flight, the NH₃ instrument was overflowed with NH₃-free air for the duration of a 2-hour pre-flight exercise.”

20 **Table 2: I really appreciated the mass balance in Table 2/discussion (neat experiment!), though even here differences of ~ 10% of counting molecules still could mean significant backgrounds still exist relative to very clean conditions (though I recognize this mass balance counting is within the instrument uncertainty).**

25 **In summary of all of the above, taking 3 times the 1 Hz precision doesn’t seem justified for the detection limit, nor an assessment of instrument accuracy at low concentrations. It seems the instrument is well designed for fires/agriculture but future work is still needed for clean conditions after such large plumes (or more justification in the manuscript). This is particularly true when going from dirty to clean conditions, given the many sampling biases that still may exist for ammonia.**

30 We have updated the discussion about detection limit given the 400 pptv variability in Fig. 3. We have also added notes about sampling biases in accord with the responses above.

2. Validity of using bi-exponential decay model and meaning of the parameters should be addressed:

35 **The bi-exponential decay model is essential to the discussion about instrument response time. The authors used the bi-exponential decay model to determine the response times of the instrument to associate gas exchange and the interaction of NH₃ molecules with sampling surfaces. The fit results were also used to extrapolate the 90% and 99% signal recovery times (t_{90} and t_{99}). Therefore, it is necessary to address the validity of the bi-exponential decay model.**

40 **The bi-exponential decay model was first introduced to characterize response time of QC-TILDAS to NH₃ changes by Ellis et al.(1). However, the validity of the model was not discussed in the original work. Here, we propose to use the following a simplified surface-air exchange model to derive the biexponential decay model and discuss its validity.**

45 **After a step change, changes of the mixing ratio of NH₃ inside the instrument χ is caused by 1) the difference of NH₃ mixing ratio between the gas currently inside the chamber and the newly introduced gas (χ_0); 2) adsorption or desorption to the inner surface of the instrument. These processes can be expressed as**

$$\frac{d\chi}{dt} = \frac{Q}{V}(\chi_0 - \chi) + \kappa(\chi_s(t) - \chi)$$

where Q is the flow rate and V is the inner volume of the instrument; κ is the conductance of NH_3 between surface and air interface; χ_s is the compensation point of the inner surface (adsorption occurs when $\chi > \chi_s$, desorption occurs when $\chi < \chi_s$). The compensation point is a function of time and its variation depends on historical changes of NH_3 concentration inside the instrument. When there are no phase changes and chemical reactions, and the surface is not saturated by NH_3 or exhausted of NH_3 during the process, χ_s could be simplified as

$$\frac{d\chi_s}{dt} = \kappa(\chi - \chi_s).$$

When the surface is clean such that $\chi_s \ll \chi$, χ_s equation can be approximated as

$$\frac{d\chi_s}{dt} = \kappa\chi.$$

For the step change described in this study, $\chi_0=0$. Combine all the equations, we have

$$\frac{d^2\chi}{dt^2} + \left(\frac{Q}{V} + \kappa\right) \frac{d\chi}{dt} = \kappa^2\chi.$$

The general solution to the differential equation is

$$\begin{aligned} \chi &= A_1 \exp \left[-\frac{1}{2} \left(\sqrt{\left(\frac{Q}{V}\right)^2 + 2\left(\frac{Q}{V}\right)\kappa + 5\kappa^2} + \left(\frac{Q}{V}\right) + \kappa \right) t \right] \\ &\quad + A_2 \exp \left[\frac{1}{2} \left(\sqrt{\left(\frac{Q}{V}\right)^2 + 2\left(\frac{Q}{V}\right)\kappa + 5\kappa^2} - \left(\frac{Q}{V}\right) - \kappa \right) t \right] \\ &= A_1 \exp \left(-\frac{t}{\tau_1} \right) + A_2 \exp \left(-\frac{t}{\tau_2} \right) \end{aligned}$$

It can be seen from above derivation that the bi-exponential decay model approximates the universal solution of the differential equations, but it only works under certain conditions - the most important one is the relative cleanliness of the surface. After certain time, χ will approach χ_s and the solution to the differential equations becomes significantly more complicated and is unlikely to follow biexponential decay model. The authors should clarify the applicability of the bi-exponential decay model.

Given the validity of the bi-exponential decay model, it may be more reliable to derive t_{90} and t_{99} using observed time series directly if the measurements are not noisy.

τ_1 and τ_2 represents the combined effects of both gas exchange and air-surface exchange instead of representing the effects separately. Therefore, the statements about τ_1 and τ_2 from line 22 to line 24 on page 10 should be removed.

We greatly appreciate the time and effort by the commenters to provide us with a detailed surface-air exchange model for the bi-exponential decay. We would be happy to include your model in this paper or future papers if a peer-reviewed reference can be provided. However without that, we feel that derivations of this model are beyond the scope of this paper, and it seems more appropriate for the commenters to develop this model as the originators of these concepts. All the same, we agree that the bi-exponential fits do not always provide a perfect representation of the observations, which could indicate

instances where the model fails to adequately describe the physical system. As suggested by the commenters, we now also include values for t_{90} and t_{99} in Table 1 that are directly determined from the observations in Fig. 5. The new parameters are denoted as $t_{90,obs}$ and $t_{99,obs}$. However, we also continue to frame the results using the existing bi-exponential decay model in the literature for the following reasons: 1) as a way to provide context for fitting the time response profiles, 2) for consistency with the approach utilized in the peer-reviewed literature for similar instruments (Zahniser et al., 1995; Ellis et al., 2010; Roscioli et al., 2016), and 3) for ease of comparison to prior assessments with similar instrumentation by Ellis et al. (2010) and Roscioli et al. (2016).

3. Uncertainty of response time may not be representative:

The uncertainty of the response time is currently estimated using error propagation of the fitted results. However, given the exponential nature of the issue, parameters like t_{90} and t_{99} may have a skewed distribution (i.e. log-normal distribution) with a long tail. This behavior may not be correctly captured by error propagation method. If fitted results are used, Monte Carlo method should be used. If the real time series is used, t_{90} could be estimated as the standard deviation of time stamps of observations with NH₃ between the $90 - \sigma_{obs}$ percentile and the $90 + \sigma_{obs}$ percentile.


For comparison to the uncertainties derived from error propagation of the bi-exponential fit coefficients, we now also include an observation-based determination of the uncertainties for $t_{90,obs}$ and $t_{99,obs}$ in Sect. 4.3. These uncertainties reflect the Δt spread in times associated with the $90 \pm 1\%$ and $99 \pm 1\%$ signal recovery levels, where $\pm 1\%$ on the signal recovery level corresponds to ± 0.5 ppbv for a 50 ppbv step change, which is within the instrument's limit of detection.

Summary: The authors have shown a marked improvement in the use of airborne-based ammonia measurements. In fact, these measurements are the most impressive and reliable to date in the literature and have set a new standard for all future campaigns (airborne and ground-based). The technique has applicability to Picarro and other closed-path sensors, as well as calibration methods for open-path sensors (which, indeed, have to be “closed” typically for calibration). However, there are still many gremlins for airborne ammonia, particularly with its enormous dynamic range in concentration and adsorption issues, which get magnified for sub-ppbv NH₃ levels that are expected in the free (or at least upper) troposphere (Asian UT monsoon levels excepted, possibly). I hope the points above allow for some clarifications that strengthen the manuscript.

****others****

Page 11, line 4-10: The manuscript never mentions how the boundary layer height was determined. Was it known accurately in each case or simply assumed to be <1 km?

A well-mixed layer below roughly 1 km was initially assumed. There could be differences in the structure of the boundary layer for the different test flights, which could be due to the colder/wetter ambient conditions during the test flights in September 2017 compared to the warmer/drier conditions during test flights in July 2018. Unfortunately, we have very few parameters to compare from the test flights as the instrument payload was minimal in 2017 and not all instruments were fully operational/optimized at the time of the WE-CAN test flights in 2018. On the other hand, we reliably have potential temperature, which was collected during each flight as part of the aircraft's standard suite of measurements. Vertical profiles of potential temperature do indicate a planetary boundary layer height was primarily between 1 and 1.5 km for both the 2017 and 2018 test flights. Although, there could have been more than one mixed layer during the 2018 test flights. We have added the following text to Sect. 4.4: “All the same, further measurements are recommended for assessing sampling biases that could arise during field measurements of low mixing ratios of NH₃ in clean environments following long periods of exposure to near source level concentrations. The potential for a “memory effect” of NH₃ on the sampling surfaces following long-term exposure to high concentrations of NH₃ is discussed in following sections.” We have also modified Fig. 6 to include potential temperature and a rough guideline for the boundary layer height.

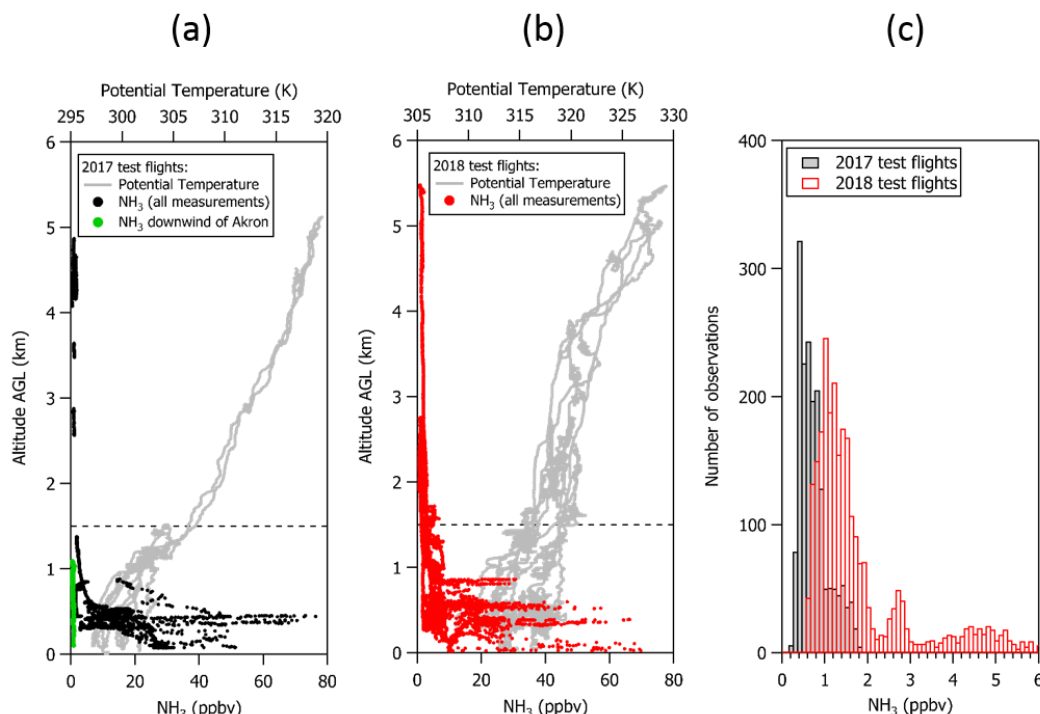

Updated caption for Fig. 6:

Vertical profiles of NH_3 (in ppbv) and potential temperature (in K) from (a) the first and third test flight in 2017 and (b) the test flights in 2018 when the instrument was operated without passivant. NH_3 mixing ratios as high as 80 ppbv were observed in the mixed boundary layer during missed approaches at Greeley-Weld County Airport and over northeastern Colorado compared to average mixing ratios of ~ 0.8 ppbv near Akron, Colorado following several days of rain. (c) Histograms of the corresponding NH_3 measurements collected above 1.5 km AGL (dashed line) show that measurements were frequently larger than 200 ppt, especially measurements that were collected in the free troposphere.

- 5
- 10 **Page 12, line 40-45: The authors should be aware that the relationship between water content and NH_3 adsorption is not necessarily linear. The interaction mechanism varies significantly depending on the amount of water present. A previous study by Vaithinen et al., 2018, has demonstrated this. Therefore, the two scenarios (dry vs 80% humidified) tested here may not be representative enough to tell the whole story.**
- 15 We appreciate the commenter's points. The Vaithinen et al. (2018) and Pogany et al. (2016) references have been added to Sect. 5.1.3 and we have amended the section with the following text: "We only measured two extreme relative humidity conditions for these tests, even though the relationship of surface interactions may be non-linear and vary greatly depending on the fraction of water vapor added as suggested by Pogany et al. (2016) and Vaithinen et al. (2018)."
- 20 And, "...a caveat of these tests is that the humidity levels tested here may not provide enough information to fully characterize the effects of passivant addition over the full range of dry to humid sampling conditions. Further characterization of the humidity dependence with and without passivant addition is recommended prior to future deployments of this instrument system (or similar QC-TILDAS instruments) in humid field environments."
- 25 **Page 13, line 40-43: It is not clear what criteria the authors used to determine that the NH_3 transmission shows little difference between the non-passivant and with-passivant transects. (By the response time/maximum reading/amount of the NH_3 measured?)**

The comparison is based on the amount of NH_3 measured by the detector. We have amended the text on Pg. 13 to clarify.

Figure 6a: It would be helpful to show the exact boundary layer height for this profile for better clarity.

We have amended Fig. 6 to include vertical profiles of potential temperature, which was measured as part of the aircraft's standard suite of parameters during the test flights. We agree that this is a helpful addition because of the subtle differences in mixed layers between the 2017 and 2018 test flight cases described above.

Figure 8 (upper): I am confused by the brown circles/dots labeled as beef and dairy. Do the small dots indicate smaller facilities as compared to the large circles? The two circles on the upper and lower right presumably refer to dairy but there is a dot in the center of each circle. Does this mean the facilities have both dairy and beef?

We greatly appreciate the commenters finding these typos. The smaller dots are meant to indicate smaller facilities in terms of head of cattle, and some of the beef and dairy animal operations are collocated. All the same, the original plot did have some defects in symbol outlines and layering that complicated its appearance. The plot, legend, and caption have been updated to clarify these differences.

The total power output of the system should be described, since power seemed to be an issue even on an aircraft.

We have added a Sect. 2.4 to describe the power, weight and space utilized by the instrument. The following text has been added in this new section. "The instrument system described above in the configuration that it was utilized aboard the C-130 aircraft requires the space of an entire NSF/NCAR G-V aircraft equipment rack (approximate dimensions 21.5" W x 28" D x 50" H). The equipment without the rack weighed approximately 150 kg and included a 30 kg uninterruptable power supply (UPS) and a 10 kg display laptop. The total power used by the instrument system was 1600 watts, with roughly one third of this total (600 watts) being dedicated to the main pumping system (Agilent, model Triscroll 600, 100 lbs installed). It is possible that the power, weight and space required for this instrument system can be reduced for future deployments by eliminating the UPS and display laptop. It may also be possible to reduce the size of the pump if different field applications allow for a lower sample flow rate to be used."

Abstract: "Flight-ready" in the abstract seems redundant for the topic; also "custom" is mentioned three times in the first sentence.

Agreed. We have implemented these changes.

For the Allan plot, what offset was applied and how much? As written, it is confusing.

We agree that the application of the offset is misleading as currently written. Owing to the vibration applied to the laser objective, the noise guidelines were offset by -150 ppt to align with the observations. The observations were not adjusted. We have updated Sect. 4.1 and the figure caption to clarify.

SilcoNert 2000 has been shown to work very well for ammonia and water vapor adsorption – can the authors – Pogány et al., Meas. Sci. Tech., <https://iopscience.iop.org/article/10.1088/0957-0233/27/11/115012/meta>.

We have added (Pogány et al., 2016) and (Vaitinen et al., 2018) to Sect. 5.1.3 to aid in discussion of the limitations of the humidity tests performed with and without passivant addition in this work. We have also added mention of other materials used in the past as potential passivant coatings to Sect. 2.2.5 via addition of the (Pogány et al., 2016) and (Yokelson et al., 2003) references. This reads: "Prior studies have shown inlet coatings such as a halocarbon wax (Yokelson et al., 2003) and SilcoNert 2000 (Pogány et al., 2016) can prevent the adsorption of NH_3 and water vapor on instrument sampling surfaces. While current coating technology can provide relatively non-sticky surfaces, we note that in field environments, these

surface treatments can quickly become overcoated with dust, salt, and other condensables, that ultimately compromise their non-stick properties. Continual re-application of a non-stick coating via the active continuous passivation method described here mitigates this issue.”

List of all relevant changes made in the manuscript:

1. Updates to the wording in the abstract accord to the commenter's and review's suggestions. Specifically, with respect to "Flight-ready" and "custom" being used several times in the text.
2. Addition of the following text to the Sect. 1: While NH_3 is regulated under the Gothenburg protocol in some parts of the world (e.g., <http://www.unece.org/environmental-policy/conventions/air/guidance-documents-and-other-methodological-materials/gothenburg-protocol.html>), it remains an unregulated pollutant in the U.S. (Gilliland et al., 2008)."
3. Clarification has been regarding the strain relief in Sect. 2.2.4.
4. 'Hydroscopic' was replaced with 'hygroscopic' throughout.
5. The word 'detector' was replaced with QC-TILDAS, instrument, or spectrometer throughout the manuscript according to the reviewer's suggestion.
6. Added a new Sect. 2.4 to include power, weight, and space occupied by the instrument aboard the C-130 as configured for these experiments.
7. Clarification about the overflow of NH_3 -free air at the inlet was added to Sect. 4.1 by adding the following sentence to the first paragraph: "An overflow > 500 sccm (e.g., the difference between the flow of zero air being supplied to the inlet and the instrument's sample flow) was maintained to ensure that the sample stream was truly NH_3 -free during this test."
8. We added clarification in Sect. 4.1 about how the measurements were collected for Fig. 3 by adding: "For these experiments, the instrument inlet was continuously overflowed with NH_3 -free air for the duration of a 3-hour pre-flight exercise prior to take off. Overflowing the inlet was purposefully done to keep the instrument system free of contaminants (e.g., exhaust from other aircraft and ground-based support equipment) prior to sampling in flight."
9. We updated the discussion of the detection limit according to the commenter's suggestions by adding: "We note that the true detection limit of the instrument in flight may be better represented by the full range of variability about the mean zero signal level from the observations in Fig. 3 (e.g., an instrument detection limit of 400 pptv)." to Sect. 4.1.
10. We updated the discussion in Sect. 4.2 about motion sensitivity according to the commenter's suggestions by adding: "It should also be noted that large accelerations in the up-down and fore-aft dimensions are also significant at the onset of vertical ascent. Accelerations measured in the up-down and fore-aft motions at the onset of a 1000 ft/min vertical ascent were measured to be 0.4 g and 0.08 g, respectively. Given the slopes above, these accelerations correspond to a maximum change in NH_3 zero signal level of 400 pptv during ascent, which is consistent with the variability in zero signal level observed in Fig. 3 when ascending between constant altitude legs."
11. Significant updates were made to all of Sect. 4.3 according to the commenter's suggestions. Specifically, we added: "For consistency with the approaches used in the peer-reviewed literature for characterizing the time response of a QC-TILDAS instrument and for ease of comparison to the values reported by Ellis et al. (2010) and Roscioli et al. (2016), we show the results of the bi-exponential fits in Table 1. However, the possibility remains that the time profiles collected here are not perfectly represented by the bi-exponential air-surface exchange model described by Eq. 1. Therefore, we also utilize the observations in Fig. 5 to directly derive the 90% and 99% signal recovery times (denoted as $t_{90, \text{obs}}$ and $t_{99, \text{obs}}$). In this case, uncertainties reflect the Δt spread in the observations associated with the $90 \pm 1\%$ and $99 \pm 1\%$ signal recovery levels, where $\pm 1\%$ on the signal recovery level corresponds to ± 0.5 ppbv for a 50 ppbv step change, which is well within the limit of detection. As indicated in Fig. 5 and Table 1, the instrument time response has a clear dependence with the cleanliness of the instrument sampling surfaces. Specifically, an instrument with "clean" sampling surfaces has a much faster time response ($t_{90, \text{obs}} < 1$ s) compared to an instrument with "dirty, or "contaminated", sampling surfaces ($t_{90, \text{obs}} = 143$ s). This effect is apparent regardless of how the t_{90} is determined."
12. The following was added to the end of Sect. 4.4 to address the concerns of the reviewer and the commenters: "All the same, further measurements are recommended for assessing sampling biases that could arise during field measurements of low mixing ratios of NH_3 in clean environments following long periods of exposure to near source level concentrations. The potential for an adsorption-related "memory effect" of NH_3 (e.g., Williams et al., 1992) on

the sampling surfaces following long-term exposure to high concentrations of NH₃ is discussed in following sections.”

13. The following was added to Sect. 5.1.1 according to suggestions by the reviewer and the commenters: “In this study, the instrument response is rigorously tested with a single step change of NH₃ created by turning off a 50 ppbv calibration gas mixture. We note that such large variations in NH₃ mixing ratio may not been full applicable to field measurements in unpolluted regions away from concentrated sources of NH₃. As described by Ellis et al. (2010), large gradients in NH₃ may be less impacted by surface interactions because “clean” sampling surfaces only have a finite number of adsorption sites that could be quickly filled under high NH₃ conditions. At lower NH₃ concentrations, a greater fraction of NH₃ molecules may interact with the inner surfaces. This could explain why passivation did not help to increase the response time of the instrument.”.
14. According to the reviewer’s suggestions, we also added, “While the proportion of the time response governed by the slow, “adsorptive”, term was typically quite low ($D < 10\%$), the magnitude of the step change concentration utilized here is large (e.g., 50 ppb), so caution should be taken when extrapolating these results to ambient observations away from concentrated source regions.”
15. We added the following to the first paragraph of Sect. 5.1.3: “We only measured two extreme relative humidity conditions for these tests, even though the relationship of surface interactions may be non-linear and vary greatly depending on the fraction of water vapor added as suggested by Pogány et al. (2016) and Vaitinen et al. (2018).”
16. We added the following to the end of Sect. 5.1.3: “All the same, we reiterate that a caveat of these tests is that the humidity levels tested here may not provide enough information to fully characterize the effects of passivant addition over the full range of dry to humid sampling conditions. Further characterization of the humidity dependence with and without passivant addition is recommended prior to future deployments of this instrument system (or similar QC-TILDAS instruments) in humid field environments.
17. We added the following to the end of Sect. 5.1.4: “Prior studies have shown inlet coatings such as a halocarbon wax (Yokelson et al., 2003) and SilcoNert 2000 (Pogány et al., 2016) can prevent the adsorption on NH₃ and water vapor on instrument sampling surfaces. While current coating technology can provide relatively non-sticky surfaces, we note that in field environments, these surface treatments can quickly become overcoated with dust, salt, and other condensables, that ultimately compromise their non-stick properties. Continual re-application of a non-stick coating via the active continuous passivation method described here mitigates this issue. “
18. We updated the language in Sect. 5.2.1 to clarify the observations in Fig. 8. It now read as: “Passivant was not added to the PTR-ToF-MS; active continuous passivation was only applied the QC-TILDAS-based instrument during the selected times described above. It is clear by visual comparison to the PTR-ToF-MS that the non-passivated, “contaminated” QC-TILDAS instrument did not capture all of the expected ambient NH₃. This is evident from the differences in measured NH₃ mixing ratios reported in Fig. 8 during the time period between 13:20 and 13:23 when the QC-TILDAS was operated without passivant. During this time period the PTR-ToF-MS consistently measured more NH₃ than the QC-TILDAS, with the enhancement measured by the PTR during the plume intersect at 13:30 MDT showing an expected mixing ratio of ~45 ppbv. According to PTR-NH₃, the integrated NH₃ signal during the plume intersect at 13:30 MDT was only 14% less than the integrated NH₃ signal measured during the plume intersect at 14:00 MDT, and thus a significant enhancement in NH₃ should have been observed by the QC-TILDAS-based instrument. However, the non-passivated, “contaminated” QC-TILDAS-based instrument measured only a fraction of the NH₃ expected during the plume transect at 13:30 MDT, with the only attributable difference being NH₃ molecules adsorbing to the sampling surfaces.”
19. The following was added to Sect. 5.2.2 according to the commenter’s suggestions: “During WE-CAN, the NH₃ instrument was typically zeroed between crosswind transects of a wildfire smoke plume when in background air and either just prior to or during turns. The instrument was zeroed every 10-20 mins during transits from Boise to the wildfires sampled with the frequency of zeros depending on the transit time. Zeros measured during WE-CAN research flights were typically collected for a period of 1 to 2 minutes, a duration much greater than the instrument response time, to ensure that zeros were measured well within 90% of the final zero signal level. Prior to each research flight, the NH₃ instrument was overflowed with NH₃-free air for the duration of a 2-hour pre-flight exercise. Differences in background mixing ratios of NH₃ and CO measured before and after the first transect of the smoke plume from the S. Sugarloaf fire are apparent in the magnified timeseries for each in Fig. 10. The differences

in NH_3/CO ratio observed at 20:14 UTC and 20:25 UTC following in-smoke measurements of NH_3 that exceeded 400 ppbv could have resulted from physical differences in plume chemistry, mixing or background composition on either side of the plume, an adsorption-related memory effect in the sample plumbing due to retention of NH_3 molecules adsorbed to the sampling surfaces (Williams et al., 1992), or a combination of both. Since the root of the differences are difficult to distinguish and may vary among the WE-CAN research flights, we utilized these differences to characterize the instrument time response given the worst-case scenario that the differences in background observed in Fig. 10 are solely attributed to memory effects on the sampling surfaces. In this worst case, the response time for the NH_3 measurement following the plume transect to recover to near background mixing ratio levels observed prior to the plume transect (e.g., 1 ppbv) is roughly 250 s. The time frame most closely resembles $t_{99,obs}$ for the “typical” condition when the instrument is operated with or without passivant. This recovery time and “typical” cleanliness condition are within our expectations for the instrument during this research flight (RF15) since the instrument had routinely been used to sample near source concentrations of NH_3 in smoke during several prior consecutive research flights without refreshing the sampling surfaces between flights. “

20. We also amended the text in Sect. 5.2.2 according to the above changes: “A similar time resolution observed for the passivated and non-passivated NH_3 measurements is consistent with the sampling surfaces being relatively “clean” or having a “typical” level of cleanliness during this research flight. We also note that only a small fraction of NH_3 (<1%) is ejected from the sampling surfaces when passivant was re-added to the NH_3 instrument at 20:29 UTC following the second transect, thereby further indicating that only a small amount of NH_3 molecules were adsorbed to the instrument sampling surfaces during this flight.
21. We also added the following to the end of Sect. 5.2.2 according to the commenters suggestions: “Since the time response of the CO measurement was limited by its sample flow rate and inlet configuration, we also compare NH_3 to acetonitrile (CH_3CN) measured by the PTR-ToF-MS. CH_3CN is well correlated with NH_3 in smoke, and may be more representative of a true 1-Hz tracer owing to operation of the instrument inlet at a flow rate of ~15 SLPM. However, there are no measurements from the PTR-ToF-MS during RF15, the research flight during which the NH_3 instrument was systematically tested with and without passivant. Instead, we use measurements of CH_3CN from the Bear Trap Fire (RF09) conducted on 09 August 2018 to perform a similar linear regression analysis of fine structure features of measured NH_3 versus CH_3CN , with CH_3CN incrementally averaged up to 5 seconds. We find the best fits result from linear regressions of measured NH_3 with the 1-Hz reported and 2-second averaged CH_3CN (R^2 is > 0.97 and within 0.001 of each other).”
22. The conclusions were updated accordingly.
23. DOI’s for the data sets were updated with permanent DOI data links.
24. We added the following acknowledgment: “We thank the two anonymous reviewers as well as Da Pan, Xuehui Guo, and Mark Zondlo for helpful comments and suggestions that have greatly improved this manuscript.”
25. (Pogany et al., 2016), (Vaattinen et al., 2018), Williams et al., 1992) and (Yokelson et al., 2003) were added to the references.
26. Table 1 was updated to include $t_{90,obs}$ and $t_{99,obs}$
27. The caption for Fig. 2 was updated to clarify that the offset was applied to the guidelines in the Allan Variance plots not the data.
28. Fig. 3 was updated to include a time series (Panel d) to illustrate the effects of motion sensitivity on the zero signal level as the aircraft initiates ascent and then levels off at a constant altitude.
29. Fig. 6 was updated to include vertical profiles of potential temperature as an indicator of the boundary layer height.
30. The brown symbols in Fig. 8 were updated to clarify that they are sized by number of head of cattle.
31. Fig. 10 was updated with magnified views of the NH_3 and CO measurements to highlight differences in background measured before and after transect of a concentrated smoke plume.
32. All figure captions were updated according to the modifications listed above.

Evaluation of ambient ammonia measurements from a research aircraft using a closed-path QC-TILDAS spectrometer operated with active continuous passivation

Ilana B. Pollack¹, Jakob Lindaas¹, J. Robert Roscioli², Michael Agnese², Wade Permar³, Lu Hu³, and
5 Emily V. Fischer¹

¹Department of Atmospheric Science, Colorado State University, Fort Collins, Colorado, 80523, USA

²Aerodyne Research Inc., Billerica, Massachusetts, 01821, USA

³Department of Chemistry and Biochemistry, University of Montana, Missoula, Montana 59812, USA

Correspondence to: Ilana B. Pollack (ipollack@rams.colostate.edu) or Emily V. Fischer (evf@rams.colostate.edu)

10 **Abstract.** A closed-path quantum cascade tunable infrared laser direct absorption spectrometer (QC-TILDAS) was outfitted
with an inertial inlet for filter-less separation of particles ~~and several custom-designed components including, a custom-~~
~~designed an~~ aircraft inlet, a ~~custom-built~~ vibration isolation mounting plate, and a ~~custom-built~~ system for optionally adding
active continuous passivation for gas-phase measurements of ammonia (NH₃) from a research aircraft. The ~~flight-ready~~
15 instrument was then deployed on the NSF/NCAR C-130 aircraft during research flights and test flights associated with the
Western wildfire Experiment for Cloud chemistry, Aerosol absorption and Nitrogen (WE-CAN) field campaign. The ~~flight-~~
~~ready~~ instrument was configured to measure large, rapid gradients in gas-phase NH₃, over a range of altitudes, in smoke
(e.g., ash and particles), in the boundary layer (e.g., during turbulence and turns), in clouds, and in a hot aircraft cabin (e.g.,
average aircraft cabin temperatures expected to exceed 30 °C during summer deployments). Important design goals were to
20 minimize motion sensitivity, maintain a reasonable detection limit, and minimize NH₃ “stickiness” on sampling surfaces to
maintain fast time response in flight. The observations indicate that addition of a high frequency vibration to the laser
objective in the QC-TILDAS and mounting the QC-TILDAS on a custom-designed vibration isolation plate were successful
in minimizing motion sensitivity of the instrument during flight. Allan variance analyses indicate that the in-flight precision
of ~~the flight-ready instrument~~ the instrument is 60 ppt at 1 Hz corresponding to a 3 σ detection limit of 180 ppt. Zero signals
span ± 200 pptv, or 400 pptv total, with cabin pressure and temperature and altitude in flight. The option for active
25 continuous passivation of the sample flow path with 1H,1H-perfluorooctylamine, a strong perfluorinated base, prevented
adsorption of both water and basic species to instrument sampling surfaces. Characterization of the time response in flight
and on the ground showed that adding passivant to a “clean” instrument system had little impact on the time response. In
contrast, passivant addition greatly improved the time response when sampling surfaces became contaminated prior to a test
flight. The observations further show that passivant addition can be a useful tool for used to maintaining a rapid response for
30 in-situ NH₃ measurements over the duration of an airborne field campaign (e.g., ~2 months ~~for WE-CAN test and research~~
~~flights~~) since passivant addition also helps to prevent future build-up of water and basic species on instrument sampling
surfaces. Therefore, we recommend the use of active continuous passivation with closed-path NH₃ instruments when rapid
(> 1 Hz) collection of NH₃ is important for the scientific objective of a field campaign (e.g., ~~measuring fluxes~~, sampling
from aircraft or another mobile research platform). Passivant addition can be useful for maintaining optimum operation and
35 data collection in NH₃-rich/humid environments or when contamination of sampling surfaces is likely, yet frequent cleaning
is not possible. Passivant addition may not be necessary for fast operation, even in polluted environments, if sampling
surfaces can be cleaned when the time response has degraded.

1 Introduction

Ammonia (NH₃) is the dominant alkaline gas in the atmosphere and plays an important role in many atmospheric processes.
40 Major sources of atmospheric NH₃ include agricultural activities (e.g., application of fertilizer and volatilization from animal
wastes) (e.g., (Galloway et al., 2003; Pinder et al., 2007; Reis et al., 2009; Erisman et al., 2008; Balasubramanian et al.,

2015; Leen et al., 2013), light duty gasoline vehicles equipped with three-way catalytic converters (e.g., (Kean et al., 2009; Burgard et al., 2006), biomass burning (e.g., (Hegg et al., 1988; Bray et al., 2018), water and sewage treatment plants, and some industrial production activities (e.g., chemical production plants (Zhu et al., 2015)). Atmospheric reactions of NH_3 with acids formed from the oxidation of sulfur dioxide (SO_2) and nitrogen oxides ($\text{NO}_x = \text{NO} + \text{NO}_2$) can lead to formation of fine particulate matter (Behera and Sharma, 2010; Fenn et al., 2003), which has strong implications for human health, regional air quality, atmospheric visibility, radiative forcing, and nitrogen deposition in sensitive ecosystems (Pope, 2002; Zhu et al., 2015; Erisman et al., 2008; Asman et al., 1998; Krupa, 2003; IPCC, 2007).

Anthropogenic NH_3 emissions are becoming increasingly important to study due to intensification of agricultural activities and animal husbandry (e.g., concentrated animal feeding operations) (Galloway et al., 2008). ~~yet NH_3 remains an unregulated pollutant (Gilliland et al., 2008).~~ While NH_3 is regulated under the Gothenburg protocol in some parts of the world (e.g., <http://www.unece.org/environmental-policy/conventions/air/guidance-documents-and-other-methodological-materials/gothenburg-protocol.html>), it remains an unregulated pollutant in the U.S. (Gilliland et al., 2008). Having instruments that can collect high-sensitivity, fast-response *in-situ* measurements of NH_3 are essential for directly measuring NH_3 emissions fluxes (e.g., from animal husbandry, agricultural fertilization) and eddy covariance fluxes (e.g., associated with deposition/evaporation processes), characterizing concentrations and emissions rates in plumes (e.g., from urban areas with emissions dominated by traffic, concentrated animal feeding operations, and wildfires), and sampling from mobile platforms (e.g., instrumented aircraft and ground-based vehicles). There are several techniques and types of instruments that can be used for rapid measurements of atmospheric NH_3 , including mass spectrometric methods (e.g., (Nowak et al., 2007)) and optical methods based upon open path absorption (e.g., (Miller et al., 2014; Ni et al., 2015)), closed path absorption (e.g., (Griffith and Galle, 2000; Ellis et al., 2010; Leen et al., 2013; Martin et al., 2016; Leifer et al., 2017)), and photoacoustic spectroscopy (e.g., (Schmohl et al., 2002; Pushkarsky, et al., 2002; Pogány et al., 2009)). The mass spectrometric method has been effectively leveraged aboard research aircraft (Nowak et al., 2007; Nowak et al., 2010), and the compact footprint associated with the photoacoustic approaches are useful for many applications. Open and closed path direct absorption approaches are highly applicable to the NH_3 concentration ranges expected during ambient monitoring. Open-path instruments typically have lower power consumption, higher data collection rates, and no time delays or sampling surface interactions due to inlet tubing (e.g. (Miller et al., 2014)). Closed-path systems afford the advantage of minimal data loss when sampling in potentially high particle/aerosol conditions such as in dust, smoke, precipitation/icing, and salt deposition events (e.g., (Sun et al., 2015; Leen et al., 2013)), and allow for more control over environmental influences (e.g., temperature, pressure, and water vapor). They are also able to be directly zeroed and calibrated during operation. However, closed path systems typically rely on inlet tubing to supply ambient air to the ~~detector/instrument~~, and thus the effects of inlet tubing length (and inlet complexity, especially when deployed aboard airborne research platforms) on the instrument time response can be significant. To add to these existing challenges, NH_3 is notorious for being a “sticky” molecule. Its ability to readily adsorb and/or desorb from sampling surfaces makes it a difficult gas-phase species for which to measure large, rapid changes and it is a particularly difficult measurement for which to determine accurate *in-situ* background, or zero, levels. Recent laboratory studies showed dramatic improvements in NH_3 transmission through a commercially-available, closed-path spectrometer, and thus dramatic improvements in measurement time response, when the instrument’s sampling surfaces were actively and continuously passivated with a strong perfluorinated base (e.g., 1H,1H-perfluorooctylamine) (Roscioli et al., 2016). The passivant coating works by extending a nonpolar chemical group into the sample flow path that prevents the adsorption of both water and basic species to the sampling surfaces, yet the passivant chemical does not interfere with NH_3 detection due to the highly-specific nature of detection.

Here we describe the first opportunities to evaluate and carefully characterize the effects of adding passivant to an optical absorption based, closed-path gas-phase NH_3 monitoring system aboard a research aircraft. We note that although this is not the first aircraft deployment of an optical-based NH_3 monitor (Leen et al, 2013; Hacker et al., 2016; Schiferl et al, 2016; Miller et al., 2015; Leifer et al., 2017), this is the first opportunity to evaluate the effects and the value of adding a passivant to the sample stream of an optical-based instrument for airborne measurement applications. We start by characterizing the performance of the non-passivated instrument aboard a research aircraft in flight (e.g., precision, detection limit, motion sensitivity, and stability over time) with respect to fluctuations in cabin pressure, cabin temperature, and changes in altitude. We then evaluate the instrument time response with and without active continuous passivation under a variety of operating

conditions. We report several different methods for zeroing the instrument, and offer recommendations for each method based on the sampling environment. Lastly, we provide recommendations for using active passivation for atmospheric measurements of NH_3 with optical-based, closed-path instrumentation in a variety of field measurement scenarios and environmental conditions.

5 2 Methods

2.1 Airborne sampling

Airborne measurements were collected aboard the NSF/NCAR C-130 research aircraft during the Western wildfire Experiment for Cloud chemistry, Aerosol absorption and Nitrogen (WE-CAN) field campaign in summer 2018 and during 16 test-flight hours prior to the WE-CAN deployment. The aircraft conducted seventeen research flights of roughly 6-8 hour
10 duration between 20 July and 31 August in 2018, three test flights of 2-3 hour duration between 21 September and 29 September in 2017, and two test flights on 13 July and 17 July in 2018. Research flights were conducted in the northwestern U.S. with aircraft operations based out of Boise, Idaho; test flights were conducted in the northeastern Colorado Front Range based out of the National Center for Atmospheric Research (NCAR) Research Aviation Facility in Broomfield, Colorado. The 2018 test and research flights were conducted under average ambient temperature and humidity conditions expected for
15 summer in Idaho and Colorado; 2017 test flights were performed under lower than average ambient temperature (e.g., average ambient temperature was 12 °C) and higher than average relative humidity (e.g., the average relative humidity was >70%) conditions for Colorado. WE-CAN research flights provided a number of opportunities to evaluate multiple aspects of the NH_3 instrument in flight and within concentrated smoke plumes. Several missed approaches performed at Greeley-Weld County Airport during the test flight period provided several opportunities to characterize the instrument's time
20 response with and without passivant under a variety of instrument operating conditions. Aircraft maneuvers were performed during several of the test flights and are used here to assess instrument precision, detection limit, and motion sensitivity in flight. Changes in instrument zero signal level with cabin pressure, cabin temperature and changes in altitude were extensively tested during the test flights by overflowing the inlet tip with NH_3 -free air for large periods of the flight. The aircraft also often sampled ambient air in the free troposphere during the test flights and when in transit to wildfires during
25 the 2018 deployment; these measurements are used for evaluating different methods for zeroing the instrument, ambient NH_3 levels in the free troposphere, and the instrument detection limit.

2.2 Instrumentation

The flight-ready, closed-path, optical-based NH_3 monitoring system described here consists of a combination of commercially-available and custom-built components including: 1) a commercially-available infrared absorption
30 spectrometer that serves as the heart of the NH_3 monitor, 2) a commercially-available inertial inlet that acts as a filter-less separator of particles from the sample stream, 3) a custom-built aircraft inlet, 4) a custom-designed vibration isolation mounting system for the spectrometer, and 5) a custom-built optional system for adding passivant to the sample stream.

2.2.1 NH_3 detection

~~The NH_3 detector used for these experiments~~ utilized is a compact, single-channel, closed-path, quantum-cascade tunable infrared laser direct absorption spectrometer (QC-TILDAS), model TILDAS-CS, for measuring NH_3 . The QC-TILDAS that
35 is commercially available from Aerodyne Research Inc., and ~~The QC TILDAS has been~~ described in detail in the literature (McManus et al., 1995; McManus et al., 2007; McManus et al., 2010; Zahniser et al., 1995). Briefly, a high sample flow rate (e.g., >10 standard liters per minute, SLPM, with standard conditions defined as 760 Torr and 0°C) is drawn
40 through a 76-m multipass absorption cell into which the output of a single-mode quantum cascade laser is coupled. The optical output of the laser is swept across an NH_3 absorption feature located at 967.34634 cm^{-1} . This strong rotational-vibrational (ro-vibrational) absorption feature is within the Q-branch of the ν_2 band of NH_3 . The instrumental linewidth is

typically 0.012 cm^{-1} (360 MHz) FWHM, and is largely defined by the operating pressure of the absorption cell, which was held constant at 40 Torr for these experiments. The laser is scanned across 0.315 cm^{-1} , and the resulting absorption features are detected on fast mercury cadmium telluride (MCT) detector (Vigo System). The pressure- and doppler-broadened spectral peaks are fit using a Voigt lineshape model. The QC-TILDAS ~~detector~~ is capable of up to 10 Hz collection of absolute NH_3 concentrations. NH_3 mixing ratios were typically collected at 10 Hz, and subsequently averaged to 1-Hz for WE-CAN research flights and for selected analyses described below.

Figure 1a is a schematic of the NH_3 monitoring system as it was configured for use on the NSF/NCAR C-130 aircraft. With WE-CAN objectives in mind, the instrument was configured to measure NH_3 over a range of altitudes, in smoke (e.g., large and rapid gradients in NH_3 and in ash and particle-rich air), while systematically following a smoke plume in the mixed boundary layer (e.g., in turbulence with frequent turns), and during summer near Boise, ID (e.g., large, rapid gradients in cabin temperature and average temperatures often exceeding $30\text{ }^\circ\text{C}$). In ground-based field studies and laboratory experiments, the optical bench of the QC-TILDAS is ideally operated between 20 and $25\text{ }^\circ\text{C}$ for maximum stability of the laser power, optical alignment, and spectroscopic absorption signal. In anticipation of cabin temperatures exceeding $30\text{ }^\circ\text{C}$, the set point for the QC-TILDAS optical bench temperature was intentionally set to the upper end of this range at $25\text{ }^\circ\text{C}$.

Further, the instrument flow path was purged with ultrahigh purity (UHP) N_2 overnight and when there was no power or access to the aircraft in order to keep the sampling surfaces as clean as possible. Previous experiments (Nowak et al., 2007) found that the rise/decay characteristics of NH_3 instruments operated during aircraft missions (e.g., running for several hours, sitting idle overnight, and running again the next day) were only reproducible when a flow of clean, dry N_2 was used to purge the inlet during periods of instrument inactivity. Therefore, anytime the instrument is powered off, a purge flow of 40 standard centimetres per minute (sccm) of UHP N_2 is introduced just upstream of the pressure control valve to flush the instrument in the reverse direction of the sample flow path, as indicated in Fig. 1a. We found that the instrument could reach a stable zero signal level more quickly when it had been purged overnight compared to times when the instrument sat idle without purge flow. The instrument response time could also be maintained for a longer operational time period (e.g. weeks to months) between cleanings when the instrument flow path was purged between uses.

2.2.2 Inertial Inlet

The NH₃ QC-TILDAS ~~detector~~ is typically operated with a heated inertial inlet positioned upstream of the spectrometer to provide filter-less separation of particles >300 nm from the sample stream, as shown in Fig. 1a. Coupling an inertial inlet with a QC-TILDAS has been well established following several laboratory and ground-based field experiments (Ellis et al., 2010; Ferrara et al., 2012; Tevlin et al., 2017; von Bobrutzki et al., 2010; Zöll et al., 2016). The inertial inlet is described in detail by Ellis et al. (2010) and Roscioli et al. (2016). Briefly, the inertial inlet used in these experiments consists of a quartz tube (12.7 mm o.d., 10.4 mm i.d.) with an integral, conical-shaped critical orifice roughly 1 mm in diameter positioned at about half the length of the tube, as shown in Fig. 1a. After passing through the orifice, gas (and particulates) are accelerated to a higher speed at a lower pressure (between 40 and 100 Torr) through the latter half of the 12.7 mm quartz tube, and then pass into a second quartz tube (25.2 mm o.d., 22.2 mm i.d.) that is sleeved around the 12.7 mm tube. The sample flow is split into two branches with approximately 90% of the total flow through the critical orifice (denoted by the blue arrow in Fig. 1a) being forced to make an 180° turn around the edge of the 12.7 mm tubing to continue to the spectrometer, and the other 10% (denoted by the orange arrow in Fig. 1a) being dumped via the straight section of 25.2 mm tube into the main pumping system. The inertia of particles with aerodynamic diameters greater than ~300 nm is too large to follow the gas stream around the 180° turn, thereby forcing the particles into the 10% of the flow stream that is directed to the pumping system. Ellis et al. (2010) reported that the inertial inlet, which acts like a form of virtual impactor, removes more than 50% of particles larger than 300 nm. A tee positioned immediately upstream of the critical orifice allows for pressure measurements using a baraton transducer (range 0-1000 Torr), which is used in determining the sample flow rate, and an auxiliary draw that allows the dead volume around the base of the conical-shaped critical orifice to be actively flushed. The flow rate of the auxiliary draw ranges from 160 to 500 sccm with changes in ambient pressure at the inlet tip. The inertial inlet is housed in a fiberglass enclosure, with the inside of the enclosure maintained at 40°C.”

2.2.3 Aircraft Inlet

A heated aircraft inlet constructed of perfluoroalkoxy fluoropolymer (PFA) allows for maximum transmission of NH₃ from the inlet tip to the ~~detector~~ ~~spectrometer~~, as shown in Fig. 1a. Inlet components are housed inside a 36 cm long stainless steel strut that extends beyond the boundary layer of the aircraft, and consists of: 1) an inlet tip made of 6 cm long 3/8” o.d., 1/4” i.d. PFA tubing, 2) a machined PFA block serving as an injection manifold for calibration and passivation gases, and 3) a 24 cm length of 3/8” o.d., 1/4” i.d. PFA tubing leading down the length of the strut. Another 71 cm length of 3/8” o.d., 1/4” i.d. PFA tubing directs the sample flow from the base of the inlet strut to the enclosure containing the inertial inlet, which is mounted to an equipment rack inside the aircraft cabin. The inlet tip is designed to be mounted with a standard stainless steel, bored-through compression fittings from the inside of the strut to minimize protrusions from the inlet end cap and to maintain the inlet tip at 35°C in flight to prevent it from freezing. The tip of the PFA inlet tubing was cut with a slight rear-facing bias from the direction of flight and extended only ~6 mm from the face of the inlet end cap to minimize particle ingestion and disruption of the boundary layer near the inlet tip. The PFA injection block located just inside the inlet strut end cap has outer dimensions of 8.3 cm long x 3.6 cm wide x 1.5 cm thick and a 6-cm long 1/4” i.d. inner sample channel to match the i.d. of the tubing used for the inlet tip and sample line. Aircraft inlets of similar design and construction were used during the 2014 Front Range Air Pollution Experiment (FRAPPE) aboard the C-130 aircraft and during the 2017 Utah Winter Fine Particulate Study aboard the NOAA Twin Otter. Another 36 cm long segment of 3/8” o.d., 1/4” i.d. PFA tubing then brings sample flow from the inertial inlet box to the QC-TILDAS, which is co-located in the same equipment rack inside the aircraft cabin. As shown in previous studies, PFA tubing and fittings are used wherever possible along the sample pathway, and tubing lengths are kept to a minimum and heated wherever possible (Neuman et al, 1999; Schmohl et al., 2001; Mukhtar et al., 2003; Leifer et al., 2017). Components housed within the aircraft inlet strut are heated to 40°C. The tubing between the inlet strut and the inertial inlet and between the inertial inlet and the QC-TILDAS are not actively heated; however, they are wrapped in flame-resistant polymer felt (DuPont Nomex) for thermal isolation. Although several reports specifically highlight the benefits of heated inlet components for measurements of NH₃ (Ellis et al., 2010; Nowak et al., 2007; Tevlin et al., 2017), these sections of tubing were left unheated in order to reduce the instrument’s power load on the aircraft and because the residence time in these segments of tubing is short (e.g., <0.15 s due to the high sample flow rate and low pressure) and aircraft cabin temperatures were anticipated to exceed 30°C in flight.

2.2.4 Vibration isolation system

To reduce motion sensitivity in-flight, the QC-TILDAS ~~detector~~ was mounted on a custom-designed, vibrationally-isolated plate (e.g., Fig. 1b) before being mounted in the aircraft equipment rack as shown in Fig. 1c. The mounting plate consisted of eight total vertically mounted wire rope vibration isolators (Enidine) that allow the spectrometer enclosure (containing the optical cell, laser, MCT detector, and optical bench) to float in all three dimensions and remain isolated from direct contact with the aircraft equipment rack. Two isolators (Enidine, WR3 series) were mounted along the inner face of each of the fore-aft facing legs of the mounting plate frame and spaced 13 cm apart; two additional isolators (Enidine, WR4 series) were positioned on top of the outboard and inboard legs of the mounting plate frame base and spaced 22.5 cm apart. The QC-TILDAS is then affixed to the mounting frame via the isolators as indicated in Fig. 1b and 1c. The advantage of this “springed” mounting plate is that it mitigates the effects of high frequency vibrations endemic to the aircraft, which can result in acoustic noise in the instrument, uncontrolled vibration of the optical bench, and general misalignment of the optics. In addition, it relieves strain on the instrument chassis when the frame of the aircraft equipment rack flexes during aircraft maneuvers. Hard stops were added to the mounting plate frame to satisfy aircraft crash loads in the forward and aft directions. Hardware was selected based on structural analysis calculations including finite element analysis given the vibrations and the loads expected aboard the NSF/NCAR C-130 aircraft. The mounting plate is similar in design to previous vibration isolation apparatuses used on research aircraft with Quantum Cascade Laser Systems (QCLS) (B. Daube, Personal Communication, 2017); although, this specific mounting system was unique to the NH₃ instrument deployed during the 2017 and 2018 WE-CAN flights. Additionally, the laser objective, an optic that guides the laser beam into the optical cavity, is vibrated at a high-frequency (~200 Hz) to wash out etalon fringe motion induced by aircraft accelerations. The frequency and amplitude of the vibrations applied to the laser objective can be adjusted to accommodate a variety of moving platforms. Several months prior to installation on the C-130 aircraft, a cabled tilting system (located at Aerodyne in Billerica, MA) was used to simulate the effects of in-flight forces on the QC-TILDAS ~~detector~~ as it was mounted to the vibration isolation plate within the aircraft equipment rack. Additional tests were performed on the hangar floor in Broomfield, CO immediately before installation of the instrument aboard the aircraft by manually tipping and shaking the equipment rack. The “tilt and shake” tests performed in both locations were conducted with the instrument powered on and operating under “zero” measure conditions by overblowing the sample inlet port with NH₃-free air. The center frequency and frequency sweep of the piezoelectric stack mounted on the laser collection objective as well as the general optical alignment within the enclosure were optimized during these tests. From these tests, we additionally learned that external forces acting on the inlet and outlet tubing associated with the sample stream were putting strain on the optical bench and resulting in notable deviations from zero in the NH₃ absorption signal. Therefore, however, this motion sensitivity could be minimized by keeping tubing lengths to a minimum and reinforcing the strain relief of the sample tubing connected to the QC-TILDAS enclosure stream inlet and outlet ports to the QC-TILDAS enclosure (e.g., rigidly securing all flexible tubing to the frame of equipment rack with cable ties) was reinforced prior to installation on the aircraft.

2.2.5 Passivant addition system

Owing to the “stickiness” of NH₃, the QC-TILDAS and inlet sampling surfaces can be compromised when they are coated with as little as a single monolayer of adsorptive matter; the build-up can cause the instrument’s time response to gradually become slower (Roscioli et al., 2016). Although sampling surfaces can be periodically refreshed by cleaning them with solvents, frequent cleaning may not always be possible or practical during field intensives. One solution, recommended by Roscioli et al. (2016), is to actively and continuously passivate the instrument sampling surfaces with a chemical coating that prevents adsorption of water and basic species. Therefore, we designed and deployed a non-commercial system that allowed for the option of passivant addition to the sample stream to this NH₃ instrument system. This work reports the first-time application of adding passivant to a closed-path, optical-based NH₃ instrument aboard a research aircraft, and serves as an evaluation of the flight-ready instrument’s time response on the ground and in-flight under a variety of conditions and with and without passivant.

For these tests, the flight instrument is outfitted with an option for adding 1H,1H-perfluorooctylamine (C₈H₄F₁₅N, CAS Number: 307-29-9) vapor to the sample stream using a similar apparatus as that used in laboratory experiments by Roscioli

et al. (2016). 1H,1H-perfluorooctylamine (purchased from Synquest Laboratories and used without further purification) is a liquid at room temperature and pressure (e.g., 20°C and 760 Torr). Vapors of the passivant are entrained in a 200 sccm flow of UHP N₂ regulated with a mass flow controller (Alicat) and introduced to the sample flow path as close to the inlet tip as possible. Given the configuration for WE-CAN, this means that the C8 passivant is injected roughly 10 cm downstream of the aircraft inlet tip via the middle port of the PFA injection block as shown in Fig. 1a. The liquid passivant is contained in a PFA impinger (Saville), and a pair of stainless steel quick connects (Swagelok) are used to connect the impinger inline between the mass flow controller and the injection port (e.g., Fig 1d). N₂ carrier gas was intentionally not bubbled through the liquid to avoid splattering the liquid onto the impinger walls and/or lodging droplets of passivant in the delivery tubing. When disconnected, the quick connects isolate the supply of passivant from the flow path allowing it to be safely removed from the aircraft overnight and for refilling. Tests without passivation could also be easily performed simply by disconnecting the quick-connects from the impinger and re-connecting them to each other without the impinger in line. Bypassing the impinger in this manner allows for constant dilution of the sample stream by a known amount of N₂ carrier gas flow regardless of whether the passivant chemical is being added. For future applications, a set of solenoid valves can be added to the impinger system for automated computer control of passivant addition or passivant bypass. For the laboratory experiments and WE-CAN flights described here and with the passivant liquid held near room temperature (e.g., 25°C), the typically usage rate of the C8 compound was ~5 grams in 20 hours.

A C7 version of the passivant chemical, 1H,1H-perfluoroheptylamine (C₇H₄F₁₃N, CAS Number: 423-49-4), was used in a separate set of tests performed in the laboratory between the 2017 and 2018 flight period, and is discussed further in Sect. 4.3. Disadvantages of adding passivant to the sample stream for NH₃ measurements include the use of hazardous materials and the cost of consumable chemicals. Both the C8 compound (1H,1H-perfluorooctylamine) and the C7 version (1H,1H-perfluoroheptylamine) are strong corrosives, contain an amine group, and are highly fluorinated. While these chemicals pose no immediate danger when properly handled, the long term exposure effects are unknown. In addition, these compounds have been identified as potentially potent, long-lived greenhouse gases (Hong et al., 2013); although, we anticipate the environmental impacts to be minor given the small quantities and low addition rates used for this application.

2.3 Calibration

The PFA injection block is configured such that calibration and passivation gases can be introduced to the sample flow path within 6-12 cm of the inlet tip (e.g., Fig. 1a). The QC-TILDAS is calibrated via standard addition to the sample stream with a known concentration of NH₃ generated from a temperature-regulated (40 ± 0.1°C) permeation device filled with anhydrous NH₃ (Kin-Tek), and zeroed by overflowing the inlet tip with a source of NH₃-free air. As described in detail in Ellis et al. (2010), three-way switching solenoid valves and a vacuum manifold are used to actively flush zero and calibration gases from the injection tubing when measuring ambient air. A continuous flow of UHP N₂ at 40 sccm was sufficient to transport all of the NH₃ vapor emitted from the permeation device to the inlet tip. The stability of the permeation device was maintained overnight when there was no power and access aboard the aircraft by removing it to a laboratory where it could be kept heated and under a constant (40 sccm) flow of UHP N₂. The emission rate of the permeation device was calibrated before and after the test flight period using the NOAA ultraviolet (UV) optical absorption system (Neuman et al., 2003). The average emission rate measured with the NOAA system before and after the WE-CAN deployment period was 407 ± 10 ng min⁻¹. The NOAA calibration has a reported uncertainty of ±10%, which is mainly due to the uncertainty in the 185 nm absorption cross section for NH₃ used for interpreting results from the optical absorption system (Neuman et al., 2003). In this work, we refine the uncertainty of the NOAA calibration of the emission rate of the permeation device used in these experiments by utilizing more recent assessments of the NH₃ absorption cross section reported in the literature. Here, we use a weighted average of the NH₃ absorption cross sections reported by Froyd and Lovejoy (2012) (4.67 ± 0.08 × 10⁻¹⁸ cm²), Chen et al. (1998) (4.7 ± 0.5 × 10⁻¹⁸ cm²) and Cheng et al. (2006) (4.7 ± 0.5 × 10⁻¹⁸ cm²). The weighted mean utilized here (4.7 ± 0.1 × 10⁻¹⁸ cm²) is in agreement within the uncertainties with the value reported by Neuman et al. (2003) (e.g., 4.4 ± 0.3 × 10⁻¹⁸ cm²). Combining in quadrature the ±2% uncertainty associated with the weighted mean of the absorption cross section, the ±2.5% uncertainty in the stability of the permeation device between pre- and post-project calibrations with the NOAA UV optical absorption system, and a conservative estimate of ±6% for other sources of uncertainty associated with the NOAA calibration system, we determine a total estimated uncertainty of ±7% for the emission rate of the permeation

device used in these experiments. The permeation rate of the NH₃ permeation device was specifically selected for NH₃ concentrations expected while sampling concentrated plumes of wildfire smoke during WE-CAN (e.g., mixing ratios \geq 50 ppbv). During flight, the instrument sample flow rate varies with altitude due to changes in ambient pressure upstream of the critical orifice inside the quartz inertial inlet. As a result, calibration concentrations range from 50 ppbv at 620 Torr (e.g., on the ground in Broomfield, CO at 1.729 m AMSL (above mean seal level)) to 100 ppbv at 310 Torr (e.g., near 7.4 km AMSL). Since the orifice inside the inertial inlet is truly critical, the in-flight sample flow rate can be calculated as $F_{alt} = F_{grd} \cdot (P_{alt}/P_{grd})$ from a pre-flight measurement of pressure and sample flow on the ground using a primary flow calibration unit (DryCal Definer 220) and the pressure measured in flight just upstream of the critical orifice inside the inertial inlet using a 0-1000 Torr Baratron pressure transducer (MKS Instruments, model 722B), as shown in Fig. 1a.

2.4 Power, weight and space

The instrument system described above in the configuration that it was utilized aboard the C-130 aircraft requires the space of an entire NSF/NCAR G-V aircraft equipment rack (approximate dimensions 21.5" W x 28" D x 50" H). The equipment without the rack weighed approximately 150 kg and included a 30 kg uninterruptable power supply (UPS) and a 10 kg display laptop. The total power used by the instrument system was 1600 watts, with roughly one third of this total (600 watts) being dedicated to the main pumping system (Agilent, model Triscroll 600, 100 lbs installed). It is possible that the power, weight and space required for this instrument system can be reduced for future deployments by eliminating the UPS and display laptop. It may also be possible to reduce the size of the pump if different field applications allow for a lower sample flow rate to be used.

3 Methods for measuring instrument zero

Ellis et al. (2010) recommended that background checks of the NH₃ instrument would optimally be performed by removing NH₃ from ambient air while keeping the humidity level constant. Historically, ambient NH₃ monitors have been zeroed in several ways, including overblowing the inlet tip with dry synthetic air or UHP N₂ from a cylinder (Nowak et al., 2010; von Bobruzki et al., 2010), overblowing the inlet tip with chemically scrubbed ambient air sources (Nowak et al., 2007; Nowak et al., 2006; Fehsenfeld et al., 2002), sampling through oxalic acid coated filters (Norman et al., 2009), or passing ambient air through heated metal catalysts (Norman et al., 2007; Tevlin et al., 2017). However, significant effort and cost can be required to routinely generate a large enough supply of NH₃-free air to overblow the inlet of the NH₃ instrument described here (e.g., >10 SLPM), and at low enough zero levels to be considered truly NH₃-free by instruments with low detection limits of a few hundred pptv or less. Our evaluation and recommendations reported below take these factors into consideration.

In the months leading up to the 2017 test flights, we tested five different sources of NH₃-free air in the laboratory. First, we used dry, ultrapure synthetic "zero" air (UZA) from a compressed gas cylinder (AIRGAS). We assert that this bottled source of UZA provides a measure of the "true" instrument zero to which we then compared all other tested sources. Second, we tested the output of a commercial zero air generator (ZAG) (Teledyne, model 701H). Third, we tested a chemical NH₃ scrubbing system that included a compressor pump (KNF Neuberger) for pushing ambient air through a single all-metal trap filled with an NH₃ scrubbing reagent (Permapure). Fourth, we tested 4 Å molecular sieve (Delta Absorbents). And, fifth, we combined the chemical scrubber in tandem with the 4 Å molecular sieve. Scrubber materials were contained individually in separate traps constructed from KF-40 stainless steel tubing and vacuum fittings (LDS Vacuum). The endcaps were outfitted with stainless steel mesh screens to prevent solid scrubber materials from migrating towards the instrument inlet and ~~detector~~the spectrometer. Traps were warmed from the outside using heating tape (Omega Engineering) for selected experiments. Traps were cleaned prior to being filled with scrubbing media by rinsing the surfaces with water and then ethanol before baking the empty housings and fittings overnight at 250 °C.

We found UZA cylinders to provide the lowest and most reliable zero measure. The ZAG was also able to achieve a zero signal level consistent with that measured from a UZA cylinder. Although not ideal for use in flight owing to its weight,

space and power needs, the ZAG is a plentiful and cost-effective source of NH_3 -free air for laboratory and ground-based field experiments. We also found the ZAG useful for pre-flight operations exceeding 3 hours and for ground-based maintenance days aboard the aircraft, so that consumable cylinders could be conserved. For the chemical scrubber, we elected to use a hygroscopic phosphoric acid scrubbing reagent (Permapure) that does an acid-base neutralization reaction to remove gas-phase NH_3 from an ambient air sample, as this product had been found to be successful for generating a source of NH_3 -free air in previous airborne field campaigns (Nowak et al., 2007). However, we found that this particular chemical scrubbing reagent could not achieve a true zero on its own. The lowest possible zero level achieved with a fresh trap of the chemical scrubber was 200 pptv above true, which is larger than the on-ground detection limit (100 pptv, see Sect. 3.1) and on par with the in-flight detection limit (200 pptv). The NH_3 signal from the chemical scrubber increased with usage and was closer to 1 ppbv after several days. Cleaning the trap and refreshing the scrubbing media reagent did not result in any improvement. It is possible that the volume of the chemical scrubber trap was not large enough to scrub all of the NH_3 from the supply of ambient air required to overflow the instrument. However, similar offsets above true zero were observed in a separate experiment where the chemical scrubber was supplied with UZA from a cylinder instead of ambient air via the compressor, suggesting that the scrubbing reagent actually outgassed small amounts of NH_3 . An independently purchased supply of this chemical scrubbing media produced similar results confirming that the original reagent material had not been compromised prior to these tests. In a fourth test, we used 4 Å molecular sieve to remove NH_3 from an ambient air sample. While this was able to achieve a true zero, the volume of material that could be used and the flow rate required to overflow the instrument inlet limited the lifetime of the trap. The lifetime of this trap could be extended by increasing surface area contact time with the absorbing material, which could be achieved by increasing the length of the trap or by linking multiple traps in series. A disadvantage of 4 Å molecular sieve is that it also absorbs water. This means that the operational lifetime of the molecular sieve is greatly limited in humid environments, and since the molecular sieve dries the NH_3 -free air source the output is no different than that of a bottled source of UZA or the ZAG. In a fifth experiment, the chemical scrubber was used to remove the bulk of NH_3 from ambient air and followed in series by a trap filled with 4 Å molecular sieve to remove any remaining NH_3 . The combined trap was successful in achieving a true zero, and the lifetime of the trap was noticeably longer (2-4 hours) than that of molecular sieve alone (1-2 hours).

Although the chemical scrubber (operated with or without the molecular sieve) may be the closest option to a source of NH_3 -free ambient air, the NH_3 scrubbing reagent is hygroscopic and needs to be carefully monitored for condensate accumulation even when heated. Heavy contamination of the instrument sampling surfaces is possible from species outgassing from the chemical scrubbing reagent, especially if the chemical reagent becomes moisture saturated. Contamination of the instrument from the scrubber system is hard to predict and time consuming to remedy once it happens. While the molecular sieve effectively absorbs residual NH_3 in the combined trap, it does not prevent contamination from compounds larger than 4 Å that could result from the moisture-saturated chemical reagent. A contamination of this type was observed during the 2017 test flight period and is described in Sect. 5. Further, while the cost of molecular sieve is negligible and the material can easily be regenerated, the non-regenerative chemical reagent can significantly accumulate in expense over time depending on usage rate. In our tests, the chemical scrubbing reagent lasted a few weeks before being compromised. However, the actual lifetime depends on how NH_3 -rich and humid the operational environment is and how consistently the trap is heated.

Following this assessment, we elected to only evaluate and compare the UZA cylinder and the combined chemical scrubber/molecular sieve during the 2017 test flights. Even though cylinders are rapidly consumed at the high sample flow rate and thus were replaced prior to each of our flights, we ultimately found this source to be the most convenient and cost-effective method for zeroing the NH_3 instrument system during WE-CAN test and research flights. As might be expected, cylinders of dry UHP N_2 produced the same zero signal level as a bottled source of UZA, and thus can be utilized as an alternative (and sometimes less costly) NH_3 -free source for zeroing the instrument. It should also be noted that the calibration signal from standard addition of NH_3 on top of a zero background signal generated with UHP N_2 can be different by as much as 10% from a calibration signal measured on top of a background produced with UZA owing to differences in pressure (or collisional) broadening of the NH_3 spectral lines in the ν_2 absorption band with different carrier gases (Pearman and Garratt, 1975; Owen et al., 2013).

4 Evaluation of the non-passivated instrument on the ground and in flight

4.1 Precision, detection limit, and stability

Continuously overflowing the inlet tip with NH_3 -free air (~~>500 sccm~~) during one of the test flights allowed for characterization of any flight-induced artifacts in the detected absorption signal above a constant, low-level background. An overflow > 500 sccm (e.g., the difference between the flow of zero air being supplied to the inlet and the instrument's sample flow) was maintained to ensure that the sample stream was truly NH_3 -free during this test. The measured zero signal level on the ground and in flight was the same when tested with a UZA cylinder, a UHP N_2 cylinder, or the combined chemical reagent/molecular sieve scrubber. Ambient signal levels were checked periodically for a few minutes at a time throughout the flight to confirm that measured ambient levels were greater than or equal to the measured zero signal level. Measured zero signal levels were consistently within a factor of three of the in-flight instrument precision with changes in altitude up to the 5 km AGL (or ~6 km AMSL, which was the upper range of the C-130 with the WE-CAN payload). Ambient measurements were consistently greater than zero and frequently above the 200 pptv detection limit, even in the free troposphere.

Figure 2 depicts two time segments of data collected at 10 Hz while measuring NH_3 -free air. One is a 10-minute segment collected in flight in the boundary layer near 1.4 km AGL (e.g., Fig. 2a); the other is a 2-hour segment collected in the laboratory (e.g., Fig. 2b). The instrument was operated without passivant in both cases. Instrument precision, calculated as the Allan deviation or the square root of the Allan variance (Werle et al., 1993), is 430 pptv at 10 Hz and 60 pptv at 1 Hz in flight and 130 pptv at 10 Hz and 40 pptv at 1 Hz on the ground. An offset was applied to the The Allan variance from the 10-Hz data collected in flight, ~~and~~ reflects the effects of a frequency-swept vibration applied to the laser objective to reduce motion sensitivity due to optical feedback from the objective. The frequency and amplitude of the vibration were specifically tuned to minimize motion sensitivity at 1 Hz for this flight application. If we define the detection limit as three times the instrument precision, then the estimated 1-Hz detection limits are 180 pptv in flight and 120 pptv on the ground. Therefore, vibrations associated with the C-130 in flight lead to larger detection limit by a factor of 1.5. Since the instrument was not operated without the vibration isolation mounting plate or high frequency vibration of the laser objective during the test flight period, we have no direct comparison for how these added features impacted the measurements. The same precision and detection limit are determined from an Allan variance analysis of NH_3 data at a constant mixing ratio of 50 ppbv, collected when calibration gas was added to the sample stream. With averaging, the Allan variance plots suggest that the in-flight detection limit can be reduced to 75 pptv over and averaging period of 5 seconds and 60 pptv over 10 seconds.

Figure 3 shows that zero and calibration signal levels were largely insensitive to in-flight fluctuations in cabin pressure and temperature and changes in altitude within the ± 200 pptv detection limit, as shown in Fig. 3. For these experiments, the instrument inlet was continuously overflowed with NH_3 -free air for the duration of a 3-hour pre-flight exercise prior to take off. Overflowing the inlet was purposefully done to keep the instrument system free of contaminants (e.g., exhaust from other aircraft and ground-based support equipment) prior to sampling in flight. A slight positive trend was observed in the zero signal level with increasing altitude during an ascent profile between the ground in Broomfield, Colorado and 6.5 km AMSL; however, there is little variability in the average-mean zero signal measured during constant altitude legs and the 3σ standard deviation of each average-mean is within the ± 200 pptv detection limit of zero. Constant altitude legs were performed roughly every 1 km for a period of 5-10 minutes during the ascent profile. The more apparent increasing trend between NH_3 zero signal level and increasing altitude between these straight and level flight legs likely reflects a change in the measured zero signal level due to motion sensitivity of the instrument during ~~vertical~~ accelerations associated with the aircraft's ascent, as described in detail in the next section. Overall, changes in the zero signal level with altitude are largely within the ± 200 pptv detection limit over the entire altitude range tested. We note that the true detection limit of the instrument in flight may be better represented by the full range of variability about the mean zero signal level from the observations in Fig. 3 (e.g., an instrument detection limit of 400 pptv).

Instrument stability was evaluated over the 2-month duration of the WE-CAN intensive and test flight period. Zero signal levels drifted <10% from average, and calibration signal levels drifted <2% from average over the entire period. Variability

in the calibration correction factor applied to the measured data to generate final NH₃ mixing ratios is <1%. We estimate that the total uncertainty associated with the reported 1-Hz measurement is ±12% of the measured NH₃ mixing ratio plus the 200 pptv detection limit, where the uncertainty of the measured NH₃ mixing ratio is calculated by quadrature addition of the associated individual uncertainties. The individual uncertainties include: the permeation rate of the calibration source as measured by the NOAA UV calibration system (±7%), the stability of calibration (±2%) and zero (±10%) measurements over the deployment period, changes in NH₃ mixing ratio with changes in flow rates (e.g., ±1% each for dilution of calibration gas into the sample flow, calibration gas addition to the sample flow, and passivant addition to the sample flow as measured with the DryCal flow calibrator), and changes in NH₃ calibration signal with changes up to 10 Torr in QC-TILDAS optical cell pressure (±1%). Changes in measured NH₃ signal with deliberate changes in optical cell temperature over a 5°C range were <0.1%, and thus are considered negligible in the uncertainty calculations.

4.2 Motion sensitivity

Figure 4 shows the sensitivity of the QC-TILDAS to in-flight accelerations measured during the test flight period. Maneuvers performed at 2.6 km AGL while measuring NH₃-free air at 10-Hz show excursions in the NH₃ signal with respect to acceleration (denoted here as ΔNH₃/g). The ΔNH₃/g observed for each direction of motion is determined from the slope of a scatter plot of NH₃ (in ppb) versus acceleration (in g). Slopes are 3 ppb/g, 1 ppb/g and 5 ppb/g for the side-side, up-down, and fore-aft motions, respectively. These excursions are not due to real changes in NH₃ mixing ratios in the ambient air sample; instead they reflect an artifact in the measured zero signal associated with physical movement of the absorption cell optics with accelerations in the side-side, up-down, and fore-aft motions of the aircraft during flight. In particular, excursions in the absorption measurements are likely affected by micro displacements in the distance between the laser and laser objective. Owing to the orientation of the laser objective with respect to the direction of flight in the spectrometer box, micro displacements in the fore-aft direction are expected to have the largest effect. For atmospheric research objectives, accelerations during ascent/descent, turbulence and turns are of particular importance since most flight plans require sampling in the mixed boundary layer, transecting emissions plumes, and performing spirals and/or sawtooth-shaped vertical profiles. Figure 4 shows that the largest accelerations of aircraft motion, specifically during turbulence and turns, are experienced in the vertical plane. Scaling accelerations observed during turbulence in the mixed boundary layer at 0.3 km AGL and turns performed near 2.6 km AGL to the ΔNH₃/g observed in all three dimensions during maneuvers indicates that changes in NH₃ signal during turbulence and turns are < 50 pptv, a factor of four less than the detection limit. It should also be noted that large accelerations in the up-down and fore-aft dimensions are also significant at the onset of vertical ascent. Accelerations measured in the up-down and fore-aft motions at the onset of a 1000 ft/min vertical ascent were measured to be 0.4 g and 0.08 g, respectively. Given the slopes above, these accelerations correspond to a maximum change in NH₃ zero signal level of 400 pptv during ascent, which is consistent with the variability in zero signal level observed in Fig. 3 when ascending between constant altitude legs.

4.3 Time response of the non-passivated instrument

The time response of the NH₃ instrument can be determined from a step change response in NH₃ concentration, as described in detail by Zahniser et al. (1995), Ellis et al. (2010) and Roscioli et al. (2016). Briefly, for these experiments, a step change in NH₃ concentration is generated by switching off calibration gas while overblowing NH₃-free air at the inlet tip. Ellis et al. (2010) and Roscioli et al. (2016) As shown in Fig-5, showed that the decrease in NH₃ mixing ratio is-was well represented by a bi-exponential decay of the functional form as shown in Eq. (1):

$$y = y_0 + A_1 \exp\left(\frac{-(t-t_0)}{\tau_1}\right) + A_2 \exp\left(\frac{-(t-t_0)}{\tau_2}\right) \quad (1)$$

where y_0 represents the mixing ratio reached at the end of the decay, A_1 and A_2 are constants that sum to the stable mixing ratio of NH₃ prior to the calibration being switched off, and τ_1 and τ_2 are the decay time constants. τ_1 is typically fast and has been referred to in the literature to correspond largely to the gas exchange time of the flow path and optical cell (~ 0.4 s); τ_2 can be significantly slower and is commonly associated in the literature with the interaction of NH₃ molecules with sampling

surfaces (Zahniser et al., 1995; Ellis et al., 2010; Miller et al., 2014; Roscioli et al., 2015). The instrument time response can then be quantified as the time (t) that it takes for the NH_3 calibration signal to return to some percent of the final zero signal level after the calibration gas was switched off (t_0). Given the double exponential nature of the decay, the ratio of A_2 to ($A_1 + A_2$), defined as parameter D and reported as percent in previous works (Ellis et al., 2010), can also be a useful tool for describing the fraction of NH_3 slowed in reaching the ~~detector-QC-TILDAS~~ due to interactions with the sampling surfaces.

Instrument time response is commonly reported as the $1/e$, 75%, and 90% signal recovery times (with the latter denoted here as t_{90}). With an overall instrument uncertainty of $\pm 12\%$, this instrument's time response is adequately characterized using t_{90} . Further, owing to this particular instrument's low detection limit and robust stability over time, we also report for reference t_{99} , the response time associated with a 99% signal recovery.

All step change profiles were measured with the instrument configured for use aboard the aircraft, as shown in Fig. 1, and were collected during pre-flight operations on the ground prior to the test flights or in the laboratory between test flight periods. Table 1 summarizes the coefficients and corresponding 1σ standard deviations from a ~~fit of each bi-exponential fit of each time profile decay~~ shown in Fig. 5. ~~Reduced chi-square values from fits of the bi-exponential decay profiles shown in Fig. 5 and Table 1 ranged from 0.4 to 1.3.~~ Also included in Table 1 are the resultant values for $\%D$, t_{90} and t_{99} extrapolated from the fit coefficients, with uncertainties for these values reflecting propagation of the 1σ standard deviations of the fit coefficients and an uncertainty of ± 0.1 s for t_0 . ~~From Fig. 5, it appears that a bi-exponential fit does not always do a good job of approximating the observations. Indeed, reduced chi-square values from bi-exponential fit of the decay profiles ranged from 0.4 to 1.3.~~ ~~All step change profiles were measured with the instrument configured for use aboard the aircraft, as shown in Fig. 1, and were collected during pre-flight operations on the ground prior to the test flights or in the laboratory between test flight periods. As indicated in Fig. 5 and Table 1, the instrument time response has a clear dependence with the cleanliness of the instrument sampling surfaces. Specifically, an instrument with "clean" sampling surfaces has a much faster time response ($t_{90} < 1$ s) compared to an instrument with "dirty, or "contaminated", sampling surfaces ($t_{90} = 180$ s).~~

~~Indeed, a~~ triple exponential decay with the functional form shown in Eq. (2):

$$y = y_0 + A_1 \exp\left(\frac{-(t-t_0)}{\tau_1}\right) + A_2 \exp\left(\frac{-(t-t_0)}{\tau_2}\right) + A_3 \exp\left(\frac{-(t-t_0)}{\tau_3}\right) \quad (2)$$

produces better fits to the time profiles shown in Fig. 5. ~~Albeit, the coefficient associated with the third time constant (A_3) is small (e.g., A_3 is $< 5\%$ on average of the sum of the coefficients (e.g., $[A_3/(A_1 + A_2 + A_3)]$) and $< 23\%$ on average of the sum of the coefficients associated with the latter two time constants (e.g., $[A_3/(A_2 + A_3)]$). While the physical basis for using a triple exponential fit is not forthright, it is possible might have physical meaning in terms of the instrument time response if that there is more than one time constant associated with the gas exchange rate through the sample flow pathway, or if there is more than one time constant associated with the interaction of NH_3 molecules with the sampling surfaces, or a combination of these effects.~~ In the case of multiple time constants associated with the gas exchange rate, it is possible that different residence times could arise from the different pressure regimes of the sample flow pathway (e.g., the portion of the sample flow path at ambient pressure upstream of the critical orifice in the inertial inlet versus the portion of the sample flow path downstream of the critical orifice at pressures between 40 and 100 Torr). In the case of NH_3 molecules interacting with the sampling surfaces, additional time constants could be related to ~~differing variability in the~~ levels of cleanliness along the sample flow path. For example, inlet tubing and components were cleaned/replaced following contamination, but the optical cell in the QC-TILDAS was not; thus, more than one time constant might be most plausible, especially for the "typical" and "contaminated" time profiles that were collected following contamination. ~~the coefficient associated with the third time constant (A_3) is small (e.g., A_3 is $< 5\%$ on average of the sum of the coefficients (e.g., $[A_3/(A_1 + A_2 + A_3)]$) and $< 23\%$ on average of the sum of the coefficients associated with the latter two time constants (e.g., $[A_3/(A_2 + A_3)]$). For consistency with the approaches used in the peer-reviewed literature for characterizing the time response of a QC-TILDAS instrument and for ease of comparison to the values reported by Ellis et al. (2010) and Roscioli et al. (2016), we show the results of the bi-exponential fits in Table 1. However, the possibility remains that the time profiles collected here are not perfectly represented by the bi-exponential air-surface exchange model described by Eq. 1. Therefore, we also utilize the observations in Fig. 5 to directly derive the 90% and 99% signal recovery times (denoted as $t_{90, \text{obs}}$ and $t_{99, \text{obs}}$). In this case, uncertainties~~

reflect the Δt spread in the observations associated with the $90\pm 1\%$ and $99\pm 1\%$ signal recovery levels, where $\pm 1\%$ on the signal recovery level corresponds to ± 0.5 ppbv for a 50 ppbv step change, which is well within the limit of detection. All the same, we elect to report the results of the bi-exponential fits in this work for the following reasons: 1) there is more physical basis for relating a bi-exponential fit to the passivation experiments conducted in this work, 2) the results can be directly compared to the results of bi-exponential fits for similar instrumentation reported by Ellis et al. (2010) and Roseoli et al. (2016), and 3) the coefficient associated with the third time constant (A_3) is small (e.g., A_3 is $< 5\%$ on average of the sum of the coefficients (e.g., $[A_3/(A_1 + A_2 + A_3)]$) and $< 23\%$ on average of the sum of the coefficients associated with the latter two time constants (e.g., $[A_3/(A_2 + A_3)]$).

As indicated in Fig. 5 and Table 1, the instrument time response has a clear dependence with the cleanliness of the instrument sampling surfaces. Specifically, an instrument with “clean” sampling surfaces has a much faster time response ($t_{90, obs} < 1$ s) compared to an instrument with “dirty, or “contaminated”, sampling surfaces ($t_{90, obs} = 180$ – 143 s). This effect is apparent regardless of how the t_{90} is determined.

4.4 In-flight measurements with the non-passivated instrument

NH₃ was measured over a range of altitudes, including several kilometers in the free troposphere (e.g., Fig. 6a). Measured NH₃ mixing ratios were as much as 80 ppbv during missed approaches at Greeley-Weld County Airport and in the boundary layer (< 1.5 km AGL) over animal husbandry and agricultural operations in northeastern Colorado during the test flights. In contrast, NH₃ mixing ratios in the boundary layer near Akron, Colorado were around 1 ppbv following a few days of rain during the 2017 test flights. We were also fortunate to have the opportunity to sample clear air in the free troposphere for a 10–20 minute period during each of the 2017 and 2018 test flights. A histogram of the NH₃ measured in the free troposphere over the northeastern Colorado Front Range during the test flights (e.g., Fig. 6b) indicates that free tropospheric NH₃ mixing ratios were frequently greater than 0.4 ppbv during the September 2017 test flight period, a factor roughly two times greater than the detection limit, and frequently greater than 1 ppbv in July 2018 following a period of higher ambient temperatures and less rain. It should be noted that calibrations at very low NH₃ mixing ratios (e.g., sub 1 ppbv to 10 ppbv) were not performed during the test flights because the in-flight calibration source was optimized for the NH₃ mixing ratios expected in concentrated wildfire smoke during WE-CAN research flights (e.g., > 50 ppbv). However, calibrations of the QC-TILDAS detector performed by the manufacturer and during separate experiments in the laboratory prior to installation on the aircraft show linearity within the instrument uncertainty for NH₃ calibration mixing ratios ranging from a few ppbv to hundreds of ppbv. All the same, further measurements are recommended for assessing sampling biases that could arise during field measurements of low mixing ratios of NH₃ in clean environments following long periods of exposure to near source level concentrations. The potential for an adsorption-related “memory effect” of NH₃ (e.g., Williams et al., 1992) on the sampling surfaces following long-term exposure to high concentrations of NH₃ is discussed in following sections.

5 The effects of adding passivant

5.1 Passivated instrument time response on the ground

5.1.1 “Clean” vs. “dirty” instrument conditions

As indicated in Fig. 5 and Table 1, the improvement in instrument time response when passivant is added has a clear dependence with how “clean” or “dirty” the instrument system is. More specifically, there is no difference in time response for the “clean” instrument when operated with and without the C8 passivant, yet the time response increasingly improves with passivant addition to an instrument with increasingly compromised sampling surfaces (e.g., Fig. 5a compared to Fig. 5c). In these tests, the “clean” case refers to a new instrument that had only been operated for a few months after being built and always under relatively pristine conditions (e.g., operated in a laboratory with dry NH₃-free air). In this “clean” case, the instrument can recover from a 50 ppbv step change in NH₃ in $t_{90} < 1$ s regardless of whether passivant is applied. The step change profiles collected under “typical” and very dirty, or “contaminated”, operating conditions demonstrate that adding

passivant can greatly improve the overall instrument time response and that the effect of adding passivant can be increasingly beneficial as sampling surfaces are further exposed to “dirty” sampling conditions. In this study, the instrument response is rigorously tested with a single step change of NH₃ created by turning off a 50 ppbv calibration gas mixture. We note that such large variations in NH₃ mixing ratio may not been full applicable to field measurements in unpolluted regions away from concentrated sources of NH₃. As described by Ellis et al. (2010), large gradients in NH₃ may be less impacted by surface interactions because “clean” sampling surfaces only have a finite number of adsorption sites that could be quickly filled under high NH₃ conditions. At lower NH₃ concentrations, a greater fraction of NH₃ molecules may interact with the inner surfaces. This could explain why passivation did not help to increase the response time of the instrument.

Before the instrument response could be characterized in flight with passivant under typical ambient operating conditions during the 2017 test flight period, the instrument sampling surfaces experienced a case of extreme contamination. The contamination was likely caused by the chemical scrubbing reagent, which had been used in several prior experiments to evaluate a scrubbed source of NH₃-free air, that was compromised by exposure to excessive moisture (e.g., the 2017 test flight period was particularly cold and rainy). Fortuitously, this “contaminated” case, albeit an atypical and non-optimal operating condition, presented a unique opportunity to test the power of passivation for improving, or in this case recovering, instrument time response. Under “contaminated” conditions, accumulation of NH₃ on the sampling surfaces was so severe that NH₃ was more prone to sticking on the contaminated inlet surfaces rather than being transmitted to the ~~detectors~~spectrometer. The time response of the contaminated system was so long (e.g., hours) that it could not be accurately measured (e.g., the instrument would need to run for several hours to achieve 99% signal recovery, which was not possible to accomplish in the time frame of the aircraft operations). Thus, Fig. 5c shows the time response of the “contaminated” instrument after one cleaning, where a 99% signal recovery could be observed within a few hours. The “contaminated” surfaces degraded the instrument time response from $t_{90} < 1$ s to 180 s and $t_{99} = 37$ s to 1200 s. As shown in Fig. 5c, adding a continuous flow of the C8 passivant to the contaminated system brought t_{90} back to 7 s and t_{99} to 180 s. Table 1 also shows a similar value of %D in the passivated case compared to a factor of 4 difference in %D for the non-passivated case when comparing the “contaminated” versus “clean” systems indicating that the time response of the contaminated system is dominated by interaction of NH₃ with the instrument sampling surfaces (τ_2). While the proportion of the time response governed by the slow, “adsorptive”, term was typically quite low ($D < 10\%$), the magnitude of the step change concentration utilized here is large (e.g., 50 ppb), so caution should be taken when extrapolating these results to ambient observations away from concentrated source regions.

Even though adding passivant to an already “contaminated” instrument cannot instantaneously reset the sampling surfaces to near pristine “clean” condition, the results in Table 1 show that passivant addition has a greater factor of improvement for increasingly “dirty” instruments (e.g., a factor of 2 improvement for “typical” conditions, and a factor of 25 improvement for “contaminated” conditions). Although NH₃ accumulation should be avoidable during normal operation even in polluted environments with frequent checks of the step-change time response and cleanings, we conclude that the option of adding passivant can be a useful tool for recovering instrument time response when fast measurements are required and routine maintenance/cleaning is not possible (e.g., when contamination occurs before or during a research flight or at a remote field site).

It should also be noted that the instrument’s time response following the contamination event could only be fully recovered by replacing contaminated tubing and performing multiple cleanings of any non-replaceable components between the inlet tip and the QC-TILDAS optical cell. Cleaning consisted of vigorously rinsing components with deionized water several times, followed by a few rinses with 200-proof ethanol, and finally blowing out each component for several minutes with compressed UZA or UHP N₂ until all traces of solvent were gone.

5.1.2 The effects of increasing passivant concentration

Previous experiments performed in the laboratory showed improvements in instrument time response with increasing addition of C8 passivant (Roscioli et al., 2016). In these experiments, Roscioli et al. (2016) observed nearly a factor of 6 improvement in t_{90} when passivant addition was increased from 1 ppm to 40 ppm. Our tests, reported in Fig. 7 with the

instrument operated under near “typical” conditions, confirm that the instrument time response can be increasingly improved by increasing the amount of passivant added at the inlet. While the improvement increases with increasing addition of passivant chemical, the improvements observed for this particular instrument system appear to be exponential with limited improvement when passivant concentrations exceed 60 ppmv.

5 5.1.3 The effects of humid vs. dry sampling conditions

In all cases presented in Table 1, except for the “contaminated” case, D is $< 10\%$ indicating that the time response of the instrument as configured for these experiments is not overly dominated by surface interactions, even when operated under typical in-field ambient measurement operating conditions and without passivant. This is likely because the instrument sampling surfaces are heated to prevent adsorption of water and basic species, as described in Ellis et al. (2010). All the same, it should be noted that the time response tests reported here were performed on top of a sample stream of NH_3 -free air supplied from a synthetic, dry bottled source or generated using a hygroscopic scrubbing media. Sample humidity is alleged to increase the relative importance of NH_3 surface interactions (Ellis et al., 2010), and thus differences in the instrument time response determined in a laboratory using dry air compared with that determined from data collected in a moist field environment could be significant (Nowak et al., 2007). However, previous observations with respect to sample humidity are inconsistent (Pogány et al., 2016). One study showed that humidity addition increased surface interactions (e.g., more NH_3 adsorption on sampling surfaces, (Ellis et al., 2010)), while another study showed NH_3 adsorption on sampling surfaces to decrease with increasing water content (Vaaitinen et al., 2014). Although the differences may be attributed to whether the sampling surfaces were sufficiently heated to prevent water adsorption on the sampling surfaces, we were compelled to further perform a few basic tests of the effects of humidity on this instrument’s time response with and without passivant addition. We only measured two extreme relative humidity conditions for these tests, even though the relationship of surface interactions may be non-linear and vary greatly depending on the fraction of water vapor added as suggested by Pogány et al. (2016) and Vaaitinen et al. (2018). This was done by overflowing a sample of dry versus 80% humidified air at the inlet tip. Dry air was sourced directly from a UZA cylinder; humidified air was generated by passing 9.2 slpm of UZA through a bubbler filled with dionized water and allowing it to re-mix with 2.2 slpm of dry UZA before overflowing the humidified air mixture at the inlet tip. Humidifying the sample stream to 80% instead of 100% was intentional to avoid condensation of saturated water vapor onto the sampling surfaces while still providing a rigorous test of the instrument time response in a humid environment (e.g., the average annual relative humidity in morning in the continental U.S. is $\sim 80\%$).

Figure 7 shows a slight difference in instrument time response between the humidified versus the dry air sample when the instrument is operated with heated inlet surfaces and without passivant, although the difference is close to being within one standard deviation of the measurement uncertainties. The observations in Fig. 7 are consistent with that observed by Ellis et al. (2010), which were performed using similar instrumentation and similar magnitude step changes in NH_3 mixing ratios. The time responses for both the dry and humidified air samples are increasingly improved when an increasing amount of the C8 passivant is added to the sample stream. This trend is similar to that observed by Roscioli et al. (2016) in dry air samples with the exception of a plateau in the time response improvements at high concentrations of passivant addition. Improvements in time response with passivant addition for the humidified air sample seem to be limited to the same ~ 60 ppmv threshold as the dry air sample. Overall, the differences in time response between the humidified and dry air samples appear to be small when using a heated inlet system regardless of whether passivant has been added. All the same, we reiterate that a caveat of these tests is that the humidity levels tested here may not provide enough information to fully characterize the effects of passivant addition over the full range of dry to humid sampling conditions. Further characterization of the humidity dependence with and without passivant addition is recommended prior to future deployments of this instrument system (or similar QC-TILDAS instruments) in humid field environments.

5.1.4 Other possible passivant chemicals

Table 1 demonstrates a similar improvement in instrument time response when a C7 passivant, 1H,1H-perfluorheptylamine, is implemented instead of the C8 passivant. Of significant difference is the usage rate of the C7 passivant, which is ~ 2 hours per gram compared to ~ 4 hours per gram for the C8 compound at a typical passivant addition flow rate of 200 sccm and

room temperature (~22°C). Longer carbon chain versions of the passivant chemical are expected to produce similar improvements in time response; however, longer chain species are likely to be more difficult to introduce into the sample stream due to reduced volatility.

- 5 Prior studies have shown inlet coatings such as a halocarbon wax (Yokelson et al., 2003) and SilcoNert 2000 (Pogány et al., 2016) can prevent the adsorption on NH₃ and water vapor on instrument sampling surfaces. While current coating technology can provide relatively non-sticky surfaces, we note that in field environments, these surface treatments can quickly become overcoated with dust, salt, and other condensables, that ultimately compromise their non-stick properties. Continual re-application of a non-stick coating via the active continuous passivation method described here mitigates this
10 issue.

5.2 The effects of adding passivant in flight

5.2.1 Test flights in the Colorado Front Range

Missed approaches at the Greeley-Weld County Airport in Colorado (40.4375° N, 104.633056° W, and 1,432 m AMSL) were performed on multiple occasions during 2017 and 2018 and provided opportunities to sample large, rapid gradients in
15 gas-phase NH₃ while operating the instrument with and without passivant addition. The aircraft often sampled emissions from nearby concentrated animal operations located south and east of the Greeley-Weld County Airport during the 29 September 2017 (e.g., flight tracks in Fig. 8) and 13 July 2018 flights. The aircraft reached a minimum altitude of 50 m AGL during the missed approaches; the maximum NH₃ mixing ratios were intercepted between 300 and 400 m AGL, and wind speeds were consistently between 4 and 5 m s⁻¹.

20 NH₃ enhancements observed near 13:30 Mountain Daylight Time (MDT) and 14:00 MDT during the 29 Sept 2017 flight represent intersects of the same NH₃ plume, yet differ by whether the “contaminated” instrument was operated without (e.g., cyan shaded areas near 13:30 MDT in Fig. 8) or with (e.g., orange shaded areas near 14:00 MDT in Fig. 8) the C8 passivant. Passivant addition is turned off by bypassing the impinger using the quick-connect fittings as described in Sect. 2. The large
25 drop in NH₃ signal at 13:23 MDT when the passivant impinger is bypassed indicates that the passivant coating is quickly stripped from the sampling surfaces (in about ~60 s) when the coating is not actively and continuously applied. As depicted in the cyan shaded area of the time series in Fig. 8, NH₃ mixing ratios measured by the non-passivated, “contaminated” instrument are significantly reduced. Only 5 ppbv was observed out of the ~45 ppbv of NH₃ expected during this plume transect suggesting that only ~10% of ambient gas-phase NH₃ molecules were actually transmitted to the QC-TILDAS
30 ~~detector~~ while ~90% were ~~absorbed-adsorbed~~ to the “contaminated” sampling surfaces. In contrast, a time series of NH₃ enhancements sampled during plume transects collected with a “clean” instrument system during the flight on 13 July 2018 (e.g., Fig. 9) shows little difference in the amount of NH₃ measured by transmission to the detector-spectrometer when the instrument is operated with passivant (e.g., orange shaded area at 13:46 MDT in Fig. 9) and without passivant (e.g., cyan shaded area at 13:55 MDT in Fig. 9). Therefore, we attribute the reduced transmission of NH₃ to the ~~detector-QC-TILDAS~~ in
35 the non-passivated and “contaminated” instrument system to increased retention of NH₃ due to ~~absorption-adsorption~~ on the walls of the “contaminated” sampling surfaces.

To further test this hypothesis, we quantify the relative amount of NH₃ ejected from the sampling surfaces when passivant is re-introduced to the sample stream (e.g., the red shaded areas in Fig. 8) following a non-passivated plume intersect (e.g., the
40 cyan shaded area in Fig. 8 that represents a period of sampling large NH₃ mixing ratios without passivant). Ejection occurs when passivant is re-added to the system and any NH₃ molecules that have adhered to the sampling surfaces during the non-passivated sampling period are released from the surfaces and replaced with the passivant coating. The ejection signal is a measure of the NH₃ molecules that are kicked off of the sampling surfaces and transmitted to the QC-TILDAS ~~detector~~, and manifests in the time series as an intense increase followed by a slightly less intense decrease in measured NH₃ mixing ratio
45 and an exponential decay (as depicted in Fig. 8). By adding up the amount of NH₃ ejected from the sampling surfaces with the amount of NH₃ measured by the non-passivated instrument, we can quantify the total amount of NH₃ that should have been transmitted to the ~~detector-spectrometer~~ for a specific sampling event (aka. NH₃ expected) compared to NH₃ actually

detected (NH_3 measured) to quantify how much NH_3 was absorbed to the sampling surfaces when the instrument was operated without passivant. To do this, we integrate the highlighted segments of Fig. 8, which represent plume transects sampled with and without passivant and ejection; results are reported in Table 2. From these results, we can make the following conclusions. First, the NH_3 ejected from the sampling surfaces when passivant is re-added accounts for nearly all of the missing NH_3 detected by the QC-TILDAS when the instrument system is operated without passivant. Second, passivant addition is capable of recovering a near-optimal instrument sampling capability even when the instrument is operated under non-optimal cleanliness conditions. These results are evident from the small percent difference between expected versus measured NH_3 during the feedlot plume intersects. Third, the likelihood of NH_3 adsorption to sampling surfaces increases with increasing build-up of water and basic species on the sampling surfaces, thereby decreasing the amount of NH_3 transmitted to the ~~detector~~ QC-TILDAS when the instrument is operated without passivant. This is demonstrated by a factor of six greater fraction of NH_3 ejected from the sampling surfaces during the 2017 “contaminated” case compared to the 2018 “clean” case. In general for both cases, the small percent difference in measured and expected NH_3 additionally demonstrates that the NH_3 plumes used for each case analysis likely originated from the same feedlot source and was intersected by the aircraft under similar meteorological (e.g., wind) conditions.

Additional qualitative information was unintentionally gained from a Proton Transfer Reaction Time of Flight Mass Spectrometer (PTR-ToF-MS) that was simultaneously deployed aboard the C-130 aircraft. The PTR-ToF-MS was operated with H_3O^+ reagent ion and positioned just aft of the QC-TILDAS-based instrument in the aircraft cabin. While previous studies have shown a PTR-ToF-MS to be successful in quantifying *in-situ* NH_3 mixing ratios from airborne measurement platforms (Müller et al., 2014; Norman et al., 2007), the PTR-ToF-MS deployed during WE-CAN was not optimized for measuring NH_3 and seemed to suffer from a previously-identified issue (e.g., high background signal correlated with the instrument’s ion source (Müller et al., 2016)). Since the primary objective of the PTR-ToF-MS during WE-CAN was to measure non-methane volatile organic compounds in smoke, the PTR-ToF-MS instrument inlet is non-specific and not calibrated for NH_3 . However, we were able to kinetically calculate an NH_3 mixing ratio from the raw PTR-ToF-MS instrument signal collected during the flight on 29 Sept 2017, and thus the PTR- NH_3 measurement (e.g., blue line in Fig. 8) can be used to qualitatively confirm the QC-TILDAS-based instrument observations in this study. Passivant was not added to the PTR-ToF-MS; active continuous passivation was only applied the QC-TILDAS-based instrument during the selected times described above. It is clear by visual comparison to the PTR-ToF-MS that the non-passivated, “contaminated” QC-TILDAS instrument did not capture all of the expected ambient NH_3 . This is evident from the differences in measured NH_3 mixing ratios reported in Fig. 8 during the time period between 13:20 and 13:23 when the QC-TILDAS was operated without passivant. During this time period the PTR-ToF-MS consistently measured more NH_3 than the QC-TILDAS, with the enhancement measured from by the PTR during the plume intersect at 13:30 MDT showing an expected mixing ratio of ~45 ppbv. According to PTR- NH_3 , the integrated NH_3 signal during the plume intersect at 13:30 MDT was only 14% less than the integrated NH_3 signal measured during the plume intersect at 14:00 MDT, and thus a significant enhancement in NH_3 should have been observed by the QC-TILDAS-based instrument. However, the non-passivated, “contaminated” QC-TILDAS-based instrument measured only a fraction of the NH_3 expected during the plume transect at 13:30 MDT, with the only attributable difference being NH_3 molecules adsorbing to the sampling surfaces even though the integrated NH_3 signal from the plume intersect at 13:30 MDT was 14% less than the integrated NH_3 signal measured during the plume intersect at 14:00 MDT. It should be noted that a large and variable background, which appeared to be inversely correlated with the H_3O^+ ion signal, prevented PTR- NH_3 from being determined for any of the 2018 WE-CAN test and research flights. NH_3 mixing ratios for the test flight on 29 Sept 2017 could only be calculated from the PTR-ToF-MS raw instrument signal because the H_3O^+ ion signal was ~10% lower in magnitude and significantly more stable than ion signal during the 2018 flights.

For further perspective, we would like to highlight that NH_3 measurements could only be collected with the “contaminated” instrument during the test flight on 29 September 2017 because of the option to add passivant to the sample stream. The contamination occurred only hours before take-off leaving too little time to disassemble and clean the instrument sampling surfaces prior to flight. In this case and without the option for passivant addition, the alternatives would have been to either cancel the flight and potentially miss an ideal sampling opportunity for addressing the project’s scientific goals or conduct

the research flight without NH₃ measurements. The latter would have been a significant loss if the NH₃ measurements were central to answering the project's scientific questions, as was the case for the 2018 WE-CAN field campaign.

5.2.2 Research flights in concentrated wildfire smoke during WE-CAN

Concentrated wildfire smoke plumes from the South Sugarloaf Fire in Nevada (41.812° N, 116.324° W) were sampled during a WE-CAN research flight on 26 August 2018 (RF15). The fire originated on 17 August 2018 and was caused by lightning. Winds were 12 to 16 m s⁻¹ and consistently blowing from the southwest to the northeast. Figure 10 shows NH₃ and carbon monoxide (CO) measurements from RF15 that were collected during two crosswind intercepts of the South Sugarloaf Fire smoke plume. Intercepts of the smoke plume were performed at 4400 m AMSL at roughly 75 and 200 km downwind of the South Sugarloaf Fire, and correspond to roughly 1 to 4 hours of aging since emission. The first smoke plume intercept at 20:08 UTC was conducted with passivant addition to the NH₃ instrument; the second pass at 20:21 UTC was non-passivated. Linear regression analysis confirms that NH₃ and CO measurements are strongly correlated ($R^2 > 0.9$) during both plume intersects. CO measurements were simultaneously collected aboard the C-130 during WE-CAN using a similar compact model, QC-TILDAS ~~detector-instrument~~ (Aerodyne). In contrast to the NH₃ instrument, the CO ~~detector-QC-TILDAS~~ was operated at an absorption wavelength of 2200 cm⁻¹, did not require a heated inertial inlet, was operated with a much lower sample flow rate (0.5 SLPM), and was recorded on a 1-Hz timescale. Additionally, ambient air was introduced to the CO instrument via a pressure-controlled, pumped bypass inlet system maintained at 1 SLPM and 265 Torr and constructed of 15 feet of 1/4" o.d. stainless steel tubing. We expect a slightly longer residence time (e.g., 1-2 s) for CO compared to NH₃ given the significantly lower sample flow rates and longer segments of tubing used with the CO instrument. During WE-CAN, the NH₃ instrument was typically zeroed between crosswind transects of a wildfire smoke plume when in background air and either just prior to or during turns. The instrument was zeroed every 10-20 mins during transits from Boise to the wildfires sampled with the frequency of zeros depending on the transit time. Zeros measured during WE-CAN research flights were typically collected for a period of 1 to 2 minutes, a duration much greater than the instrument response time, to ensure that zeros were measured well within 90% of the final zero signal level. Prior to each research flight, the NH₃ instrument was overflowed with NH₃-free air for the duration of a 2-hour pre-flight exercise.

Differences in background mixing ratios of NH₃ and CO measured before and after the first transect of the smoke plume from the S. Sugarloaf fire are apparent in the magnified timeseries for each in Fig. 10. The differences in NH₃/CO ratio observed at 20:14 UTC and 20:25 UTC following in-smoke measurements of NH₃ that exceeded 400 ppbv could have resulted from physical differences in plume chemistry, mixing or background composition on either side of the plume, an adsorption-related memory effect in the sample plumbing due to retention of NH₃ molecules adsorbed to the sampling surfaces (Williams et al., 1992), or a combination of both. Since the root of the differences are difficult to distinguish and may vary among the WE-CAN research flights, we utilized these differences to characterize the instrument time response given the worst-case scenario that the differences in background observed in Fig. 10 are solely attributed to memory effects on the sampling surfaces. In this worst case, the response time for the NH₃ measurement following the plume transect to recover to near background mixing ratio levels observed prior to the plume transect (e.g., 1 ppbv) is roughly 250 s. The time frame most closely resembles $t_{99,obs}$ for the "typical" condition when the instrument is operated with or without passivant. This recovery time and "typical" cleanliness condition are within our expectations for the instrument during this research flight (RF15) since the instrument had routinely been used to sample near source concentrations of NH₃ in smoke during several prior consecutive research flights without refreshing the sampling surfaces between flights.

Fine structure features in the time series (e.g., Fig. 10a and b) highlights ~~the-a~~ slightly faster time resolution ~~of-for~~ NH₃ compared to CO for the instruments as configured here. To quantify differences in the time resolution of the fine structure features observed, NH₃ measurements were incrementally averaged from 1 to 5 seconds until linear regression analysis of scatter plots of CO versus the averaged NH₃ data points resulted in a maximum R^2 value. Averaging NH₃ to 3 seconds resulted in the best fit (e.g., highest R^2 value) for both the passivated and non-passivated cases, indicating that NH₃ measurements acquired during WE-CAN were equally faster than the CO measurements regardless of whether passivant was added. A Ssimilar time resolution ~~observed~~ for the passivated and non-passivated NH₃ measurements ~~is consistent with~~ ~~indicates that~~ the sampling surfaces ~~being were~~ relatively "clean" ~~or having a "typical" level of cleanliness~~ during this

research flight. We also note that only a small fraction of NH_3 (<1%) is ejected from the sampling surfaces when passivant was re-added to the NH_3 instrument at 20:29 UTC following the second transect, thereby further indicating that only a small amount of NH_3 molecules were ~~not adsorbed~~ to the “clean” instrument sampling surfaces during this flight. No degradation in time resolution for the non-passivated NH_3 instrument during RF15, which was the second-to-last research flight of a 6-week field campaign where intense smoke plumes with NH_3 mixing ratios ranging from 50 to 400 ppbv were routinely sampled for 4-6 hours every 1 to 3 days, further demonstrates that routine passivant addition throughout the field deployment was instrumental in preventing sampling surfaces from getting “dirty”. Cleanings were only performed twice throughout the 6-week field campaign (roughly once every two weeks) when a gray-ish “smoky” residue could be visually observed on the inner sleeve of the glass inertial inlet; cleanings followed the procedure described in Sect. 4.

Since the time response of the CO measurement was limited by its sample flow rate and inlet configuration, we also compare NH_3 to acetonitrile (CH_3CN) measured by the PTR-ToF-MS. CH_3CN is well correlated with NH_3 in smoke, and may be more representative of a true 1-Hz tracer owing to operation of the instrument inlet at a flow rate of ~15 SLPM. However, there are no measurements from the PTR-ToF-MS during RF15, the research flight during which the NH_3 instrument was systematically tested with and without passivant. Instead, we use measurements of CH_3CN from the Bear Trap Fire (RF09) conducted on 09 August 2018 to perform a similar linear regression analysis of fine structure features of measured NH_3 versus CH_3CN , with CH_3CN incrementally averaged up to 5 seconds. We find the best fits result from linear regressions of measured NH_3 with the 1-Hz reported and 2-second averaged CH_3CN (R^2 is > 0.97 and within 0.001 of each other).

6 Conclusions

A closed-path QC-TILDAS instrument for measuring NH_3 ~~detector~~ was outfitted with an inertial inlet for filter-less separation of particles, a custom-designed aircraft inlet, a custom-built vibration isolation mounting plate, and the option for actively and continuously adding passivant to the sample stream. This flight-ready NH_3 instrument system was then deployed on the NSF/NCAR C-130 aircraft during test and research flights associated with the WE-CAN field campaign. The instrument was configured to measure large, rapid gradients in gas-phase NH_3 , over a range of altitudes, in smoke (e.g., ash and particles), in the boundary layer (e.g., during turbulence and turns), in clouds, and in a hot aircraft cabin. Important design goals were to minimize motion sensitivity, maintain a reasonable detection limit, and minimize NH_3 “stickiness” on sampling surfaces to maintain fast time response in flight. The addition of a high frequency vibration to the laser objective in the QC-TILDAS and mounting the QC-TILDAS on a custom-designed vibration isolation plate were successful for reducing motion sensitivity. Allan variance analyses of 10-Hz data collected near 1.4 km AGL indicate that the in-flight instrument precision for this system as configured for the C-130 aircraft is 60 ppt at 1 Hz, with a corresponding 3σ detection limit of 180 ppt. Owing to variations observed in flight with respect to changes in cabin pressure and temperature and changes in altitude, the full range of the instrument’s detection limit is likely closer to 400 pptv. The detection limit allowed measurement over a range of altitudes, and NH_3 mixing ratios in the free troposphere were frequently < 1 ppbv. Variations in NH_3 associated with turbulence and turns were also within the instrument’s limit of detection.

Characterization of the instrument’s time response in flight and on the ground with and without adding passivant showed that adding passivant to a “clean” or “typical” instrument system had little impact on the instrument’s time response. This observation is consistent with previous studies using non-passivated instruments (Ellis et al., 2010; von Bobruzki et al., 2010; Zöll et al., 2016; Whitehead et al., 2008) that clearly state the importance and necessity of careful instrument handling and rigorous experimental procedures for collecting high-quality, rapid-response measurements of NH_3 . In contrast, and as highlighted in this work, passivant addition can greatly improve the time response of an instrument with “contaminated” sampling surfaces, thereby ensuring that high-quality, rapid-response NH_3 measurements can continue to be collected during field intensives where instrument components can be difficult to regularly access and keep clean (e.g., during research flights associated with an airborne field campaign). A comparison of passivated and non-passivated NH_3 measurements from a flight conducted near the end of the WE-CAN field campaign further indicates the utility of passivant addition for preventing build-up of water and basic species on instrument sampling surfaces over long periods of time, thereby helping to keep the instrument relatively clean throughout a several-week long field intensive.

NH₃ accumulation on sampling surfaces should be avoidable during normal operation of the instrument, even in NH₃-rich and humid environments, with frequent checks of the step-change response and routine cleanings whenever a temporal profile from a step change indicates that the instrument response time has degraded. This may be especially true when sampling on the ground since a substantial volume of the sampling surfaces associated with the aircraft inlet can be eliminated. However, in the case where cleaning is not possible (e.g., when contamination occurs in flight or just prior, or when ground-based instrumentation cannot be easily accessed), adding passivant can be a useful tool for recovering time response and acts as an insurance policy for being able to continuously collect high-quality, fast-response measurements from mission critical instruments. The option for passivant addition proved to be especially advantageous during the WE-CAN test flight period since it allowed for continuous collection of high-quality, fast-response NH₃ measurements even when the instrument was compromised by a known contamination. Continuous addition of passivant during WE-CAN research flights had the added advantage of maintaining an optimum level of instrument cleanliness even when used to sample concentrated wildfire smoke plumes from 15+ research flights over the 6-week duration of the WE-CAN field intensive.

The observations presented here indicate that the active continuous passivation technique combined with a closed-path, optical-based NH₃ instrument can have utility when rapid (≥ 1 Hz or greater) collection of NH₃ is critical to the project's scientific objectives (e.g., measuring fluxes, sampling from aircraft or another mobile research platform). Passivant addition can help maintain an optimum level of operation and data collection in NH₃-rich/humid environments and/or when contamination of sampling surfaces is likely, yet frequent cleaning is not possible. Passivant addition may not be necessary for fast operation, even in polluted environments, if sampling surfaces can be cleaned whenever a step-change response to NH₃ shows time response has degraded.

Data availability. NH₃ measurements from the WE-CAN field campaign utilized in this work can be found at <https://doi.org/10.26023/2WAS-8Z23-QD0Z><https://data.eol.ucar.edu/dataset/548.022>. CO data from WE-CAN can be accessed at <https://doi.org/10.26023/Q888-WZRD-B70F><https://data.eol.ucar.edu/dataset/548.016>. CH₃CN data from WE-CAN can be access at <https://doi.org/10.26023/K9F4-2CNH-EQ0W>. Navigation, state parameters, and microphysics flight-level data provided by the UCAR/NCAR Earth Observing Laboratory are available from <https://doi.org/10.26023/G766-BS71-9V03><https://data.eol.ucar.edu/dataset/548.008>. Additionally, readers may contact the corresponding authors for data access.

Author contributions. IP prepared the manuscript with contributions from all co-authors. IP and JL designed and performed the laboratory and ground-based experiments and operated the NH₃ flight instrument during 2018 WE-CAN flights. All authors participated in instrument preparation and installation aboard the aircraft and in-flight data collection during the 2017 test flights.

Competing interests. The authors declare that they have no conflict of interest.

Acknowledgments. Funding for this work was provided by the National Science Foundation through grant number AGS-1650786. The authors wish to acknowledge Dr. Teresa Campos (NCAR) for providing CO measurements during WE-CAN; the scientists, engineers, and crew members of the WE-CAN Project Team that made these test and research flights possible; and the WE-CAN Data Archive Center at NCAR's Earth Observing Laboratory. We thank the two anonymous reviewers as well as Da Pan, Xuehui Guo, and Mark Zondlo for helpful comments and suggestions that have greatly improved this manuscript.

References

Asman, W. A. H., Sutton, M. A., and SchjØrring, J. K.: Ammonia: emission, atmospheric transport and deposition, New Phytol., 139, 27-48, <https://doi.org/10.1046/j.1469-8137.1998.00180.x>, 1998.

- Balasubramanian, S., Koloutsou-Vakakis, S., McFarland, D. M., and Rood, M. J.: Reconsidering emissions of ammonia from chemical fertilizer usage in Midwest USA, *J. Geophys. Res. Atmos.*, 120, 6232-6246, <https://doi.org/10.1002/2015JD023219>, 2015.
- 5 Behera, S. N., and Sharma, M.: Investigating the potential role of ammonia in ion chemistry of fine particulate matter formation for an urban environment, *Sci. Total Environ.*, 408, 3569-3575, <https://doi.org/10.1016/j.scitotenv.2010.04.017>, 2010.
- Bray, C. D., Battye, W., Aneja, V. P., Tong, D. Q., Lee, P., and Tang, Y.: Ammonia emissions from biomass burning in the continental United States, *Atmos. Environ.*, 187, 50-61, <https://doi.org/10.1016/j.atmosenv.2018.05.052>, 2018.
- 10 Burgard, D. A., Bishop, G. A., and Stedman, D. H.: Remote Sensing of Ammonia and Sulfur Dioxide from On-Road Light Duty Vehicles, *Environ Sci Technol*, 40, 7018-7022, <https://doi.org/10.1021/es061161r>, 2006.
- Chen, F. Z., Judge, D. L., Wu, C. Y. R., and Caldwell, J.: Low and room temperature photoabsorption cross sections of NH₃ in the UV region, *Planet. Space Sci.*, 47, 261-266, [https://doi.org/10.1016/S0032-0633\(98\)00074-9](https://doi.org/10.1016/S0032-0633(98)00074-9), 1998.
- 15 Cheng, B. M., Lu, H. C., Chen, H K., Bahou, M., Lee, Y. P., Mebel, A. M., Lee, L. C., Liang, M. C., Yung, Y. L. : Absorption Cross Sections of NH₃, NH₂D, NHD₂, and ND₃ in the Spectral Range 140-220 nm and Implications for Planetary Isotopic Fractionation, *Astrophys. J.*, 647, 1535, 2006.
- Ellis, R. A., Murphy, J. G., Pattey, E., van Haarlem, R., O'Brien, J. M., and Herndon, S. C.: Characterizing a Quantum Cascade Tunable Infrared Laser Differential Absorption Spectrometer (QC-TILDAS) for measurements of atmospheric ammonia, *Atmos. Meas. Tech.*, 3, 397-406, <https://doi.org/10.5194/amt-3-397-2010>, 2010.
- 20 Erisman, J. W., Sutton, M. A., Galloway, J., Klimont, Z., and Winiwarter, W.: How a century of ammonia synthesis changed the world, *Nat. Geosci.*, 1, 636, <https://doi.org/10.1038/ngeo325>, 2008.
- Fehsenfeld, F. C., Huey, L. G., Leibrock, E., Dissly, R., Williams, E., Ryerson, T. B., Norton, R., Sueper, D. T., and Hartsell, B.: Results from an informal intercomparison of ammonia measurement techniques, *J. Geophys. Res. Atmos.*, 107, ACH 28-21-ACH 28-14, <https://doi.org/10.1029/2001JD001327>, 2002.
- 25 Fenn, M. E., Baron, J. S., Allen, E. B., Rueth, H. M., Nydick, K. R., Geiser, L., Bowman, W. D., Sickman, J. O., Meixner, T., Johnson, D. W., and Neitlich, P.: Ecological Effects of Nitrogen Deposition in the Western United States, *BioScience*, 53, 404-420, [https://doi.org/10.1641/0006-3568\(2003\)053\[0404:EEONDI\]2.0.CO;2](https://doi.org/10.1641/0006-3568(2003)053[0404:EEONDI]2.0.CO;2), 2003.
- Ferrara, R. M., Loubet, B., Di Tommasi, P., Bertolini, T., Magliulo, V., Cellier, P., Eugster, W., and Rana, G.: Eddy covariance measurement of ammonia fluxes: Comparison of high frequency correction methodologies, *Agric. For. Meteorol.*, 158-159, 30-42, <https://doi.org/10.1016/j.agrformet.2012.02.001>, 2012.
- 30 Froyd, K. D., and Lovejoy, E. R.: Bond Energies and Structures of Ammonia–Sulfuric Acid Positive Cluster Ions, *J. Phys. Chem. A*, 116, 5886-5899, <https://doi.org/10.1021/jp209908f>, 2012.
- Galloway, J. N., Aber, J. D., Erisman, J. W., Seitzinger, S. P., Howarth, R. W., Cowling, E. B., and Cosby, B. J.: The Nitrogen Cascade, *BioScience*, 53, 341-356, [https://doi.org/10.1641/0006-3568\(2003\)053\[0341:TNC\]2.0.CO;2](https://doi.org/10.1641/0006-3568(2003)053[0341:TNC]2.0.CO;2), 2003.
- 35 Galloway, J. N., Townsend, A. R., Erisman, J. W., Bekunda, M., Cai, Z., Freney, J. R., Martinelli, L. A., Seitzinger, S. P., and Sutton, M. A.: Transformation of the Nitrogen Cycle: Recent Trends, Questions, and Potential Solutions, *Science*, 320, 889, <https://doi.org/10.1126/science.1136674>, 2008.

- Gilliland, A. B., Hogrefe, C., Pinder, R. W., Godowitch, J. M., Foley, K. L., and Rao, S. T.: Dynamic evaluation of regional air quality models: Assessing changes in O₃ stemming from changes in emissions and meteorology, *Atmos. Environ.*, 42, 5110-5123, <https://doi.org/10.1016/j.atmosenv.2008.02.018>, 2008.
- Griffith, D. W. T., and Galle, B.: Flux measurements of NH₃, N₂O and CO₂ using dual beam FTIR spectroscopy and the flux-gradient technique, *Atmos. Environ.*, 34, 1087-1098, [https://doi.org/10.1016/S1352-2310\(99\)00368-4](https://doi.org/10.1016/S1352-2310(99)00368-4), 2000.
- Hacker, J., Chen, D., Bai, M., Ewenz, C., Junkermann, W., Lieff, W., McManus, B., Neininger, B., Sun, J., Coates, T., Denmead, O., Flesch, T., McGinn, s., and Hill, J.: Using airborne technology to quantify and apportion emissions of CH₄ and NH₃ from feedlots, *Anim. Prod. Sci.*, 56, 190-203, <https://doi.org/10.1071/AN15513>, 2016.
- Hegg, D. A., Radke, L. F., Hobbs, P. V., and Riggan, P. J.: Ammonia emissions from biomass burning, *Geophys. Res. Lett.*, 15, 335-337, <https://doi.org/10.1029/GL015i004p00335>, 1988.
- Hong, A. C., Young, C. J., Hurley, M. D., Wallington, T. J., and Mabury, S. A.: Perfluorotributylamine: A novel long-lived greenhouse gas, *Geophys. Res. Lett.*, 40, 6010-6015, <https://doi.org/10.1002/2013GL058010>, 2013.
- IPCC: Climate Change 2007 - The Physical Science Basis: Working Group I Contribution to the Fourth Assessment Report of the IPCC, edited by: Solomon, S., Qin, D., Manning, M., Chen, Z., Marquis, M., Averyt, K. B., Tignor, M., and Miller, H. L., Cambridge University Press, 2007.
- Kean, A. J., Littlejohn, D., Ban-Weiss, G. A., Harley, R. A., Kirchstetter, T. W., and Lunden, M. M.: Trends in on-road vehicle emissions of ammonia, *Atmos. Environ.*, 43, 1565-1570, <https://doi.org/10.1016/j.atmosenv.2008.09.085>, 2009.
- Krupa, S. V.: Effects of atmospheric ammonia (NH₃) on terrestrial vegetation: a review, *Environ. Pollut.*, 124, 179-221, [https://doi.org/10.1016/S0269-7491\(02\)00434-7](https://doi.org/10.1016/S0269-7491(02)00434-7), 2003.
- Leen, J. B., Yu, X.-Y., Gupta, M., Baer, D. S., Hubbe, J. M., Kluzek, C. D., Tomlinson, J. M., and Hubbell, M. R.: Fast In Situ Airborne Measurement of Ammonia Using a Mid-Infrared Off-Axis ICOS Spectrometer, *Environ. Sci. Technol.*, 47, 10446-10453, <https://doi.org/10.1021/es401134u>, 2013.
- Leifer, I., Melton, C., Tratt, D. M., Buckland, K. N., Clarisse, L., Coheur, P., Frash, J., Gupta, M., Johnson, P. D., Leen, J. B., Van Damme, M., Whitburn, S., and Yurganov, L.: Remote sensing and in situ measurements of methane and ammonia emissions from a megacity dairy complex: Chino, CA, *Environ. Pollut.*, 221, 37-51, <https://doi.org/10.1016/j.envpol.2016.09.083>, 2017.
- Martin, N. A., Ferracci, V., Cassidy, N., and Hoffnagle, J. A.: The application of a cavity ring-down spectrometer to measurements of ambient ammonia using traceable primary standard gas mixtures, *Appl. Phys. B*, 122, 219, <https://doi.org/10.1007/s00340-016-6486-9>, 2016.
- McManus, J. B., Keabian, P. L., and Zahniser, M. S.: Astigmatic mirror multipass absorption cells for long-path-length spectroscopy, *Appl. Opt.*, 34, 3336-3348, <https://doi.org/10.1364/AO.34.003336>, 1995.
- McManus, J. B., Shorter, J. H., Nelson, D. D., and Zahniser, M. S.: Compact Quantum Cascade Laser Instrument for Rapid, High Sensitivity Measurements of Trace Gases in Air, *SENSORS*, 2007 IEEE, 1341-1344, <https://doi.org/10.1109/ICSENS.2007.4388659>, 2007.
- McManus, J. B., Zahniser, M. S., Nelson, D. D., Shorter, J. H., Herndon, S. C., Wood, E. C., and Wehr, R.: Application of quantum cascade lasers to high-precision atmospheric trace gas measurements, *Opt. Eng.*, 49, 111124, <https://doi.org/10.1117/1.3498782>, 2010.

- Miller, D. J., Sun, K., Tao, L., Khan, M. A., and Zondlo, M. A.: Open-path, quantum cascade-laser-based sensor for high-resolution atmospheric ammonia measurements, *Atmos. Meas. Tech.*, 7, 81-93, <https://doi.org/10.5194/amt-7-81-2014>, 2014.
- 5 Miller, D. J., Sun, K., Tao, L., Pan, D., Zondlo, M. A., Nowak, J. B., Liu, Z., Diskin, G., Sachse, G., Beyersdorf, A., Ferrare, R., and Scarino, A. J.: Ammonia and methane dairy emission plumes in the San Joaquin Valley of California from individual feedlot to regional scales, *J. Geophys. Res. Atmos.*, 120, 9718-9738, <https://doi.org/10.1002/2015JD023241>, 2015.
- 10 Mukhtar, S., Rose, A., Capareda, S., Boriack, C., Lacey, R., Shaw, B., and Parnell, C.: Assessment of ammonia adsorption onto Teflon and LDPE tubing used in pollutant stream conveyance, *Agricultural Engineering International: The CIGR Journal of Scientific Research and Development*, BC03012, 2003.
- Müller, M., Mikoviny, T., Feil, S., Haidacher, S., Hanel, G., Hartungen, E., Jordan, A., Märk, L., Mutschlechner, P., Schottkowsky, R., Sulzer, P., Crawford, J. H., and Wisthaler, A.: A compact PTR-ToF-MS instrument for airborne measurements of volatile organic compounds at high spatiotemporal resolution, *Atmos. Meas. Tech.*, 7, 3763-3772, <https://doi.org/10.5194/amt-7-3763-2014>, 2014.
- 15 Müller, M., Anderson, B. E., Beyersdorf, A. J., Crawford, J. H., Diskin, G. S., Eichler, P., Fried, A., Keutsch, F. N., Mikoviny, T., Thornhill, K. L., Walega, J. G., Weinheimer, A. J., Yang, M., Yokelson, R. J., and Wisthaler, A.: In situ measurements and modeling of reactive trace gases in a small biomass burning plume, *Atmos. Chem. Phys.*, 16, 3813-3824, <https://doi.org/10.5194/acp-16-3813-2016>, 2016.
- 20 Neuman, J. A., Huey, L. G., Ryerson, T. B., and Fahey, D. W.: Study of Inlet Materials for Sampling Atmospheric Nitric Acid, *Environ. Sci. Technol.*, 33, 1133-1136, <https://doi.org/10.1021/es980767f>, 1999.
- Neuman, J. A., Ryerson, T. B., Huey, L. G., Jakoubek, R., Nowak, J. B., Simons, C., and Fehsenfeld, F. C.: Calibration and Evaluation of Nitric Acid and Ammonia Permeation Tubes by UV Optical Absorption, *Environ. Sci. Technol.*, 37, 2975-2981, <https://doi.org/10.1021/es026422l>, 2003.
- 25 Ni, K., Köster, J. R., Seidel, A., and Pacholski, A.: Field measurement of ammonia emissions after nitrogen fertilization—A comparison between micrometeorological and chamber methods, *European Journal of Agronomy*, 71, 115-122, <https://doi.org/10.1016/j.eja.2015.09.004>, 2015.
- 30 Norman, M., Hansel, A., and Wisthaler, A.: O₂⁺ as reagent ion in the PTR-MS instrument: Detection of gas-phase ammonia, *Int. J. Mass Spectrom.*, 265, 382-387, <https://doi.org/10.1016/j.ijms.2007.06.010>, 2007.
- Norman, M., Spirig, C., Wolff, V., Trebs, I., Flechard, C., Wisthaler, A., Schnitzhofer, R., Hansel, A., and Neftel, A.: Intercomparison of ammonia measurement techniques at an intensively managed grassland site (Oensingen, Switzerland), *Atmos. Chem. Phys.*, 9, 2635-2645, <https://doi.org/10.5194/acp-9-2635-2009>, 2009.
- 35 Nowak, J. B., Huey, L. G., Russell, A. G., Tian, D., Neuman, J. A., Orsini, D., Sjostedt, S. J., Sullivan, A. P., Tanner, D. J., Weber, R. J., Nenes, A., Edgerton, E., and Fehsenfeld, F. C.: Analysis of urban gas phase ammonia measurements from the 2002 Atlanta Aerosol Nucleation and Real-Time Characterization Experiment (ANARChE), *J. Geophys. Res. Atmos.*, 111, n/a-n/a, <https://doi.org/10.1029/2006JD007113>, 2006.
- 40 Nowak, J. B., Neuman, J. A., Kozai, K., Huey, L. G., Tanner, D. J., Holloway, J. S., Ryerson, T. B., Frost, G. J., McKeen, S. A., and Fehsenfeld, F. C.: A chemical ionization mass spectrometry technique for airborne measurements of ammonia, *J. Geophys. Res.*, 112, <https://doi.org/10.1029/2006JD007589>, 2007.

- Nowak, J. B., Neuman, J. A., Bahreini, R., Brock, C. A., Middlebrook, A. M., Wollny, A. G., Holloway, J. S., Peischl, J., Ryerson, T. B., and Fehsenfeld, F. C.: Airborne observations of ammonia and ammonium nitrate formation over Houston, Texas, *J. Geophys. Res.*, 115, <https://doi.org/10.1029/2010JD014195>, 2010.
- Owen, K., Es-sebbar, E.-t., and Farooq, A.: Measurements of NH_3 linewidths and collisional broadening coefficients in N_2 , O_2 , CO_2 , and H_2O near 1103.46cm^{-1} , *J. Quant. Spectrosc. Radiat. Transfer*, 121, 56-68, <https://doi.org/10.1016/j.jqsrt.2013.02.001>, 2013.
- Pearman, G. I., and Garratt, J. R.: Errors in atmospheric CO_2 concentration measurements arising from the use of reference gas mixtures different in composition to the sample air, *Tellus*, 27, 62-66, <https://doi.org/10.3402/tellusa.v27i1.9885>, 1975.
- Pinder, R. W., Adams, P. J., and Pandis, S. N.: Ammonia Emission Controls as a Cost-Effective Strategy for Reducing Atmospheric Particulate Matter in the Eastern United States, *Environ. Sci. Technol.*, 41, 380-386, <https://doi.org/10.1021/es060379a>, 2007.
- Pogány, A., Mohácsi, Á., Varga, A., Bozóki, Z., Galbács, Z., Horváth, L., and Szabó, G.: A Compact Ammonia Detector with Sub-ppb Accuracy Using Near-Infrared Photoacoustic Spectroscopy and Preconcentration Sampling, *Environ. Sci. Technol.*, 43, 826-830, <https://doi.org/10.1021/es802638z>, 2009.
- Pogány, A., Balslev-Harder, D., Braban, C. F., Cassidy, N., Ebert, V., Ferracci, V., Hieta, T., Leuenberger, D., Martin, N. A., Pascale, C., Peltola, J., Persijn, S., Tiebe, C., Twigg, M. M., Vaitinen, O., van Wijk, J., Wirtz, K., and Niederhauser, B.: A metrological approach to improve accuracy and reliability of ammonia measurements in ambient air, *Meas. Sci. Technol.*, 27, 115012-115026, <https://doi.org/10.1088/0957-0233/27/11/115012>, 2016.
- Pope Iii, C. A.: Lung Cancer, Cardiopulmonary Mortality, and Long-term Exposure to Fine Particulate Air Pollution, *JAMA*, 287, 1132, <https://doi.org/10.1001/jama.287.9.1132>, 2002.
- Pushkarsky, M. B., Webber, M. E., Baghdassarian, O., Narasimhan, L. R., and Patel, C. K. N.: Laser-based photoacoustic ammonia sensors for industrial applications, *Appl. Phys. B*, 75, 391-396, <https://doi.org/10.1007/s00340-002-0967-8>, 2002.
- Reis, S., Pinder, R. W., Zhang, M., Lijie, G., and Sutton, M. A.: Reactive nitrogen in atmospheric emission inventories, *Atmos. Chem. Phys.*, 9, 7657-7677, <https://doi.org/10.5194/acp-9-7657-2009>, 2009.
- Roscioli, J. R., Zahniser, M. S., Nelson, D. D., Herndon, S. C., and Kolb, C. E.: New Approaches to Measuring Sticky Molecules: Improvement of Instrumental Response Times Using Active Passivation, *J. Phys. Chem. A*, 120, 1347-1357, <https://doi.org/10.1021/acs.jpca.5b04395>, 2016.
- Schiferl, L. D., Heald, C. L., Van Damme, M., Clarisse, L., Clerbaux, C., Coheur, P.-F., Nowak, J. B., Neuman, J. A., Herndon, S. C., Roscioli, J. R., and Eilerman, S. J.: Interannual Variability of Ammonia Concentrations over the United States: Sources and Implications, *Atmos. Chem. Phys. Discuss*, 1-42, <https://doi.org/10.5194/acp-2016-285>, 2016.
- Schmohl, A., Miklos, A., and Hess, P.: Effects of adsorption-desorption processes on the response time and accuracy of photoacoustic detection of ammonia, *Appl. Opt.*, 40, 2571-2578, <https://doi.org/10.1364/AO.40.002571>, 2001.
- Schmohl, A., Miklós, A., and Hess, P.: Detection of ammonia by photoacoustic spectroscopy with semiconductor lasers, *Appl. Opt.*, 41, 1815-1823, <https://doi.org/10.1364/AO.41.001815>, 2002.

- Sun, K., Tao, L., Miller, D. J., Zondlo, M. A., Shonkwiler, K. B., Nash, C., and Ham, J. M.: Open-path eddy covariance measurements of ammonia fluxes from a beef cattle feedlot, *Agric. For. Meteorol.*, 213, 193-202, <https://doi.org/10.1016/j.agrformet.2015.06.007>, 2015.
- 5 Tevlin, A. G., Li, Y., Collett, J. L., McDuffie, E. E., Fischer, E. V., and Murphy, J. G.: Tall Tower Vertical Profiles and Diurnal Trends of Ammonia in the Colorado Front Range, *J. Geophys. Res. Atmos.*, 122, 412,468-412,487, <https://doi.org/10.1002/2017JD026534>, 2017.
- Vaaitinen, O., Metsälä, M., Persijn, S., Vainio, M., and Halonen, L.: Adsorption of ammonia on treated stainless steel and polymer surfaces, *Appl. Phys. B*, 115, 185-196, <https://doi.org/10.1007/s00340-013-5590-3>, 2014.
- 10 [Vaaitinen, O., Metsälä, M., Halonen, L., Persijn, S., Leuenberger, D., Niederhauser, B. Effect of moisture on the adsorption of ammonia, *Appl. Phys. B*, 124, 189-197, <https://doi.org/10.1007/s00340-018-7054-2>, 2018.](#)
- 15 von Bobrutski, K., Braban, C. F., Famulari, D., Jones, S. K., Blackall, T., Smith, T. E. L., Blom, M., Coe, H., Gallagher, M., Ghalaieny, M., McGillen, M. R., Percival, C. J., Whitehead, J. D., Ellis, R., Murphy, J., Mohacsi, A., ~~Pogány~~Pogany, A., Junninen, H., Rantanen, S., Sutton, M. A., and Nemitz, E.: Field inter-comparison of eleven atmospheric ammonia measurement techniques, *Atmos. Meas. Tech.*, 3, 91-112, <https://doi.org/10.5194/amt-3-91-2010>, 2010.
- Werle, P., Mücke, R., and Slemr, F.: The limits of signal averaging in atmospheric trace-gas monitoring by tunable diode-laser absorption spectroscopy (TDLAS), *Appl. Phys. B*, 57, 131-139, <https://doi.org/10.1007/bf00425997>, 1993.
- Whitehead, J. D., Twigg, M., Famulari, D., Nemitz, E., Sutton, M. A., Gallagher, M. W., and Fowler, D.: Evaluation of Laser Absorption Spectroscopic Techniques for Eddy Covariance Flux Measurements of Ammonia, *Environ. Sci. Technol.*, 42, 2041-2046, <https://doi.org/10.1021/es071596u>, 2008.
- 20 [Williams, E. J., Sandholm, S. T., Bradshaw, J. D., Schendel, J. S., Langford, A. O., Quinn, P. K., LeBel, P. J., Vay, S. A., Roberts, P. D., Norton, R. B., Watkins, B. A., Buhr, M. P., Parrish, D. D., Calvert, J. G., Fehsenfeld, F. C., An intercomparison of five ammonia measurement techniques, *J. Geophys. Res.*, 97\(D11\), 11591– 11611, <https://doi.org/10.1029/92JD00721>, 1992.](#)
- 25 [Yokelson, R. J., T. J. Christian, I. T. Bertschi, and W. M. Hao, Evaluation of adsorption effects on measurements of ammonia, acetic acid, and methanol, *J. Geophys. Res.*, 108\(D20\), 4649, <https://doi.org/10.1029/2003JD003549>, 2003.](#)
- Zahniser, M. S., Nelson, D. D., McManus, J. B., Keabian, P. L., and Lloyd, D.: Measurement of Trace Gas Fluxes Using Tunable Diode Laser Spectroscopy [and Discussion], *Philos. Trans. R. Soc. A*, 351, 371-382, 1995.
- 30 Zhu, L., Henze, D. K., Bash, J. O., Cady-Pereira, K. E., Shephard, M. W., Luo, M., and Capps, S. L.: Sources and Impacts of Atmospheric NH₃: Current Understanding and Frontiers for Modeling, Measurements, and Remote Sensing in North America, *Current Pollution Reports*, 1, 95-116, <https://doi.org/10.1007/s40726-015-0010-4>, 2015.
- 35 Zöll, U., Brümmer, C., Schrader, F., Ammann, C., Ibrom, A., Flechard, C. R., Nelson, D. D., Zahniser, M., and Kutsch, W. L.: Surface-atmosphere exchange of ammonia over peatland using QCL-based eddy-covariance measurements and inferential modeling, *Atmos. Chem. Phys.*, 16, 11283-11299, <https://doi.org/10.5194/acp-16-11283-2016>, 2016.

Table 1. Summary of coefficients from fit to a bi-exponential decay and the resultant values for %D, t_{90} and t_{99} for time profiles generated from a step change in NH₃ mixing ratio under different levels of instrument “cleanliness”.

Level of instrument “cleanliness”	y_0	A_1	τ_1	A_2	τ_2	χ^2	%D	t_{90} (s)	t_{99} (s)
<i>Not passivated</i>									
Clean	0.27±0.01	95.3±0.6	0.200±0.002	5.1±0.1	18.9±0.5	0.40	5.1±0.1	0.6±0.1	37±4
Typical ^a	0.41±0.01	85.6±0.7	0.441±0.006	7.8±0.1	85±1	0.83	8.4±0.1	1.6±0.2	220±23
Contaminated	0.62±0.02	68.3±0.5	8.2±0.1	17.2±0.1	306±3	0.65	20.1±0.2	180±19	1200±127
<i>Passivated with C8 compound</i>									
Clean	0.32±0.01	90.8±0.6	0.225±0.003	7.9±0.1	18.5±0.4	0.52	8.0±0.1	0.8±0.1	45±5
Typical ^a	0.35±0.01	97.3±0.9	0.304±0.005	5.4±0.1	63±2	1.04	5.3±0.1	0.9±0.1	130±14
Contaminated	0.46±0.09	95.1±1.1	1.73±0.04	9.1±0.4	63±4	1.28	8.8±0.4	7±2	180±41
<i>Passivated with C7 compound^b</i>									
Typical ^a	0.86±0.01	109.0±0.5	0.390±0.003	5.3±0.1	36.7±0.7	0.40	4.7±0.1	1.3±0.1	135±14

^aRepresentative of the typical operating conditions of the instrument in an ambient field environment.

^bFor experiments performed in the lab after the contamination event and with the C7 compound, the aircraft inlet and inertial inlet were rinsed with solvents and dried with UZA and the sample tubing between the inertial inlet and QC TILDAS was replaced. Several components along the sample pathway were intentionally cleaned but not replaced with pristine surfaces so that a mid level of cleanliness could be assess and the benefits of adding C7 versus C8 passivant could be clearly observed. All sampling surfaces up to the optical cell in the QC TILDAS were thoroughly cleaned following these tests and prior to the 2018 WE CAN deployment.

Table 1. Summary of coefficients from fit to a bi-exponential decay and the resultant values for %D, t_{90} and t_{99} and the time responses derived directly from the observations ($t_{90,obs}$ and $t_{99,obs}$) for time profiles generated from a step change in NH_3 mixing ratio under different levels of instrument “cleanliness”.

<u>Level of instrument “cleanliness”</u>	<u>y_0</u>	<u>A_1</u>	<u>τ_1</u>	<u>A_2</u>	<u>τ_2</u>	<u>χ^2</u>	<u>%D</u>	<u>t_{90} (s)</u>	<u>t_{99} (s)</u>	<u>$t_{90,obs}$ (s)</u>	<u>$t_{99,obs}$ (s)</u>
<i>Not passivated</i>											
Clean	0.27±0.01	95.3±0.6	0.200±0.002	5.1±0.1	18.9±0.5	0.40	5.1±0.1	0.6±0.1	37±4	0.9±0.2	60±30
Typical ^a	0.41±0.01	85.6±0.7	0.441±0.006	7.8±0.1	85±1	0.83	8.4±0.1	1.6±0.2	220±23	5.6±1.1	335±40
Contaminated	0.62±0.02	68.3±0.5	8.2±0.1	17.2±0.1	306±3	0.65	20.1±0.2	180±19	1200±127	143±2	1700±100
<i>Passivated with C8 compound</i>											
Clean	0.32±0.01	90.8±0.6	0.225±0.003	7.9±0.1	18.5±0.4	0.52	8.0±0.1	0.8±0.1	45±5	1.7±0.2	90±55
Typical ^a	0.35±0.01	97.3±0.9	0.304±0.005	5.4±0.1	63±2	1.04	5.3±0.1	0.9±0.1	130±14	2.0±0.4	198±26
Contaminated	0.46±0.09	95.1±1.1	1.73±0.04	9.1±0.4	63±4	1.28	8.8±0.4	7±2	180±41	11±2	215±26
<i>Passivated with C7 compound^b</i>											
Typical ^a	0.86±0.01	109.0±0.5	0.390±0.003	5.3±0.1	36.7±0.7	0.40	4.7±0.1	1.3±0.1	135±14	1.8±0.2	185±28

^aRepresentative of the typical operating conditions of the instrument in an ambient field environment.

^bFor experiments performed in the lab after the contamination event and with the C7 compound, the aircraft inlet and inertial inlet were rinsed with solvents and dried with UZA and the sample tubing between the inertial inlet and QC-TILDAS was replaced. Several components along the sample pathway were intentionally cleaned but not replaced with pristine surfaces so that a mid-level of cleanliness could be assess and the benefits of adding C7 versus C8 passivant could be clearly observed. All sampling surfaces up to the optical cell in the QC-TILDAS were thoroughly cleaned following these tests and prior to the 2018 WE-CAN deployment.

5 **Table 2. The integrated sum of NH₃ detected (in units of ppbv) during intersect of a feedlot plume when the instrument was operated with passivant (orange shaded area in Fig. 8), without passivant (cyan shaded area), and during passivant ejection (red shaded area). Also reported for comparison is the total expected NH₃ signal from the non-passivated instrument plus ejection, the percent difference in the expected NH₃ signal from that measured with the passivated instrument, and the fraction of NH₃ ejected out of the total expected NH₃ signal.**

Test Case (Date)	NH ₃ measured without passivant	NH ₃ ejected	NH ₃ expected (=NH ₃ without passivant + NH ₃ ejected)	NH ₃ measured with passivant	Percent Difference [100*(meas-exp) / meas]	Fraction of NH ₃ ejected out of NH ₃ expected
“Clean” conditions (13 July 2018)	26,747.6	4,503.8	31,251.4	33,176.1	5.8	0.14
“Contaminated” conditions (29 Sept 2017)	2,564.0	14,159.5	16,723.5	24,353.4	31.3	0.85

Figure Captions

Figure 1: (a) Schematic of the instrument as configured for flight on the NSF/NCAR C-130 aircraft. The sample flow path (blue arrows) starts at the inlet tip, which is a short piece of 3/8" o.d., 1/4" i.d. PFA tubing that protrudes slightly from the face of the aircraft inlet strut. A PFA injection block (1/4" i.d.) housed inside the aircraft inlet strut allows calibration gases and passivant to be added to the sample stream within a few centimetres of the inlet tip. A 71-cm length of 3/8" o.d., 1/4" i.d. PFA tubing then directs ambient air into a quartz inertial inlet where particles >300 nm are separated from the sample stream, and a 36-cm length of 3/8" o.d., 1/4" i.d. PFA tubing directs the sample flow from the inertial inlet to the QC-TILDAS detector. The particle-rich stream is pumped away (orange arrows). The sample flow path is heated to 40 °C where possible to minimize interactions of NH₃ with sampling surfaces. The sample flow path is purged overnight in the reverse flow direction with 40 sccm of N₂ injected near the pressure control valve. A 0-1000 Torr range baratron (denoted as *P*) measures pressure just upstream of the critical orifice in the inertial inlet for active continuous determination of the sample flow rate. An auxiliary draw acts to flush the dead volume formed near the base of the conical-shaped critical orifice in the inertial inlet. (b) Solid model of the QC-TILDAS vibration isolation mounting plate. (c) Photograph of the QC-TILDAS mounted to the vibration isolation plate while installed aboard the C-130 aircraft. (d) Photograph of the impinger used for active continuous passivant addition.

Figure 2: 10-Hz measurements collected while overblowing NH₃-free air at the inlet tip (a) in flight in the boundary layer near 1.4 km AGL and (b) on the ground in the laboratory. Upper traces represent the raw 10-Hz data collected; lower traces depict the Allan variance of the corresponding data set. An offset of -150 pptv was applied to the noise guidelines (gray and dashed lines) in panel (a) to account for differences induced by reflect the vibration applied to the laser objective to reduce motion sensitivity in flight; the vibration was not applied during laboratory tests depicted in panel (b).

Figure 3: In-flight variations in zero signal level (in units of ppbv of NH₃) with respect to changes in (a) altitude, (b) cabin pressure, and (c) cabin temperature. Gray symbols represent the 1 s average of all of the 10-Hz data points collected in flight while overblowing the inlet tip with NH₃-free air. Colored symbols and error bars represent the average NH₃-zero signal and 3σ standard deviation for each altitude step of an ascent profile, 5 Torr increments in cabin pressure, and 2 °C increments in cabin temperature. Variations are largely within the 200 pptv detection limit (denoted by the light gray shaded areas).

Figure 3: In-flight variations in zero signal level (in units of ppbv of NH₃) with respect to changes in (a) altitude, (b) cabin pressure, and (c) cabin temperature. A time series (d) illustrates the effects of motion sensitivity on the zero signal level as the aircraft initiates ascent and then levels off at a constant altitude. Gray symbols and lines represent the 1 s average of all of the 10-Hz data points collected in flight while overblowing the inlet tip with NH₃-free air. Colored symbols and error bars represent the average NH₃-zero signal and 3σ standard deviation for each altitude step of an ascent profile, 5 Torr increments in cabin pressure, and 2 °C increments in cabin temperature. Variations are largely within ±200 pptv (denoted by the light gray shaded areas). Gaps in the time series represent times when the instrument was performing a calibration or measuring ambient air.

Figure 4: Maneuvers performed at 2.6 km AGL in flight while overblowing the inlet tip with NH₃-free air show changes in NH₃ zero signal (in units of ppbv) with respect to aircraft accelerations (in units of g) in the (a) side-side, (b) up-down, and (c) fore-aft motions. Changes in NH₃ zero signal associated with (d) turbulence in the mixed boundary layer at 0.3 km AGL and (e) during turns at 2.6 km AGL are < 50 ppt when scaled by the ΔNH₃/g observed in each individual dimension during maneuvers. Side-side and fore-aft accelerations are offset by +0.5 g for display purposes in plots (d) and (e).

Figure 5: Normalized NH₃ signal (in %) versus elapsed time (in seconds) following a step change in NH₃ mixing ratio generated by switching off calibration gas at *t*=0 s. Temporal profiles and associated bi-exponential fits are shown for the non-passivated and passivated instrument operated under (a) "clean", (b) "typical", and (c) "contaminated" sampling surface conditions. Fits ranged from *t*₀ to 400, 1000, and 3000 s for the "clean", "typical", and "contaminated" cases, respectively, in accord with the elapsed time collected for each time profile.

Figure 6: (a) Vertical profile of NH_3 from the first and third test flight in 2017 and the second test flight in 2018 when the instrument was operated without passivant show concentrations as high as 80 ppbv in the mixed boundary layer during missed approaches at Greeley-Weld County Airport and over northeastern Colorado compared to average mixing ratios of ~0.8 ppbv near Akron, CO following several days of rain. (b) Histograms of the corresponding NH_3 measurements collected in the free troposphere above 1.5 km AGL; ambient NH_3 measurements in the free troposphere were frequently greater than the 200 pptv detection limit.

Figure 6: Vertical profiles of NH_3 (in ppbv) and potential temperature (in K) from (a) the first and third test flight in 2017 and (b) the test flights in 2018 when the instrument was operated without passivant. NH_3 mixing ratios as high as 80 ppbv were observed in the mixed boundary layer during missed approaches at Greeley-Weld County Airport and over northeastern Colorado compared to average mixing ratios of ~0.8 ppbv near Akron, Colorado following several days of rain. (c) Histograms of the corresponding NH_3 measurements collected above 1.5 km AGL (dashed line) show that measurements were frequently larger than 200 ppt, especially measurements that were collected in the free troposphere.

Figure 7: Response times (t_{90} and t_{99}) and %D associated with increasing C8 passivant addition for a step change in NH_3 mixing ratio generated on top of a dry versus humidified background.

Figure 8: (upper) C-130 flight tracks and measured winds during the 29 Sept 2017 test flight. Colored segments of the flight tracks highlight enhancements in NH_3 measured downwind of concentrated animal operations (brown symbols sized by head of cattle) located southeast of Greeley-Weld County Airport. (lower) Time series of 1-Hz NH_3 mixing ratios measured using the “contaminated” QC-TILDAS instrument and kinetically calculated from a raw instrument signal obtained simultaneously aboard the C-130 aircraft by a Proton Transfer Reaction Time of Flight Mass Spectrometer (PTR-ToF-MS). Portions of the flight when the “contaminated” QC-TILDAS was non-passivated (at 13:30 MDT) and passivated (at 14:00 MDT) are highlighted by colored shaded areas in the time series. Passivant was disconnected from the QC-TILDAS instrument system between 13:23 and 13:34 MDT (as indicated by the gray shaded area); NH_3 ejection is observed when passivant is re-added to the system (red shaded area).

Figure 8: (upper) C-130 flight tracks and measured winds during the 29 Sept 2017 test flight. Colored segments of the flight tracks highlight enhancements in NH_3 measured downwind of concentrated animal operations located southeast of Greeley-Weld County Airport. (lower) Time series of 1 Hz NH_3 mixing ratios measured using the “contaminated” QC-TILDAS instrument and kinetically calculated from a raw instrument signal obtained simultaneously aboard the C-130 aircraft by a Proton Transfer Reaction Time of Flight Mass Spectrometer (PTR-ToF-MS). Portions of the flight when the QC-TILDAS was non-passivated (at 13:30 MDT) and passivated (at 14:00 MDT) are highlighted by colored shaded areas in the time series. Passivant was disconnected from the instrument system between 13:23 and 13:34 MDT (as indicated by the gray shaded area); NH_3 ejection is observed when passivant is re-added to the system (red shaded area).

Figure 9: Time series of 1-Hz NH_3 mixing ratios measured with a “clean” QC-TILDAS during the test flight on 13 July 2018. Portions of the flight when the QC-TILDAS was passivated (at 13:46 MDT) and non-passivated (at 13:58 MDT) are highlighted by colored shaded areas in the time series. Passivant was disconnected from the instrument system between 13:47 and 13:58 MDT (as indicated by the gray shaded area); NH_3 ejection is observed when passivant is re-added to the system (red shaded area).

Figure 10: Time series of 1-Hz NH_3 (black lines) and CO (red lines) measured during a crosswind transect of the smoke plume from the South Sugarloaf Fire (RF15) on 26 August 2018. The transects represent nearly identical passes through the smoke plume with the only perturbation of the NH_3 instrument being operated (a) with passivant and (b) without passivant. Changes in fine structure features of NH_3 have the strongest R^2 correlation with CO when the NH_3 measurements are averaged to 3 s. A x50 magnified view of 1-Hz NH_3 (blue lines) and a x10 magnified view of CO (orange lines) shows differences in background levels of NH_3 compared to CO before and after each plume transect.

Figure 10: Time series of 1 Hz NH_3 and CO measured during a crosswind transect of the smoke plume from the South Sugarloaf Fire (RF15) on 26 August 2018. Fine structure in NH_3 measurements, displayed as a 1 s average and a 3 s average,

correlate well with CO measurements. Similar time resolution for the passivated (a) and non-passivated (b) NH_3 measurements indicates that the sampling surfaces were “clean” during this research flight.

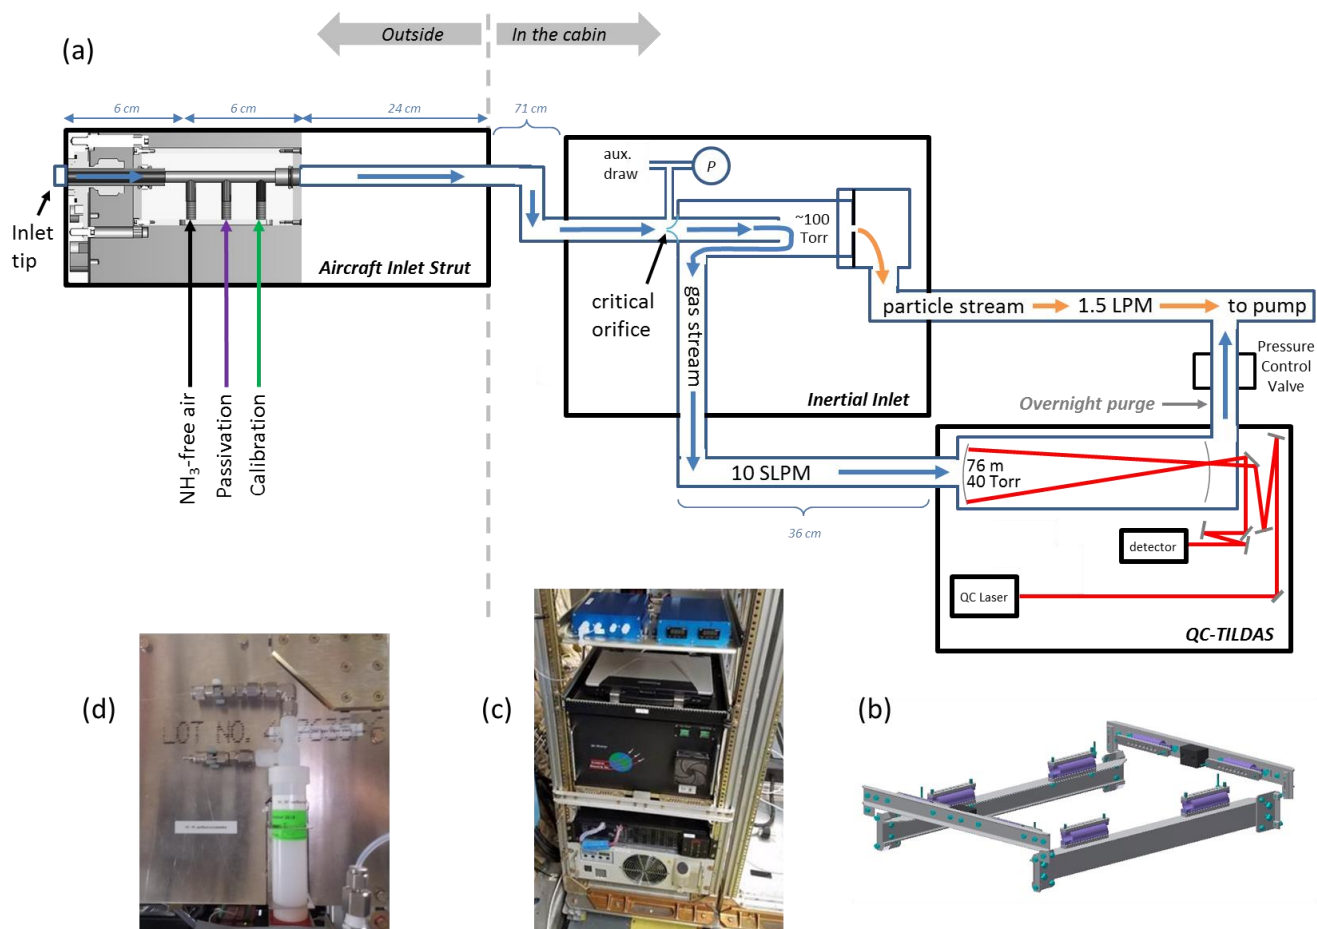


Figure 1: (a) Schematic of the instrument as configured for flight on the NSF/NCAR C-130 aircraft. The sample flow path (blue arrows) starts at the inlet tip, which is a short piece of 3/8" o.d., 1/4" i.d. PFA tubing that protrudes slightly from the face of the aircraft inlet strut. A PFA injection block (1/4" i.d.) housed inside the aircraft inlet strut allows calibration gases and passivant to be added to the sample stream within a few centimetres of the inlet tip. A 71-cm length of 3/8" o.d., 1/4" i.d. PFA tubing then directs ambient air into a quartz inertial inlet where particles >300 nm are separated from the sample stream, and a 36-cm length of 3/8" o.d., 1/4" i.d. PFA tubing directs the sample flow from the inertial inlet to the QC-TILDAS detector. The particle-rich stream is pumped away (orange arrows). The sample flow path is heated to 40 °C where possible to minimize interactions of NH₃ with sampling surfaces. The sample flow path is purged overnight in the reverse flow direction with 40 sccm of N₂ injected near the pressure control valve. A 0-1000 Torr range baratron (denoted as *P*) measures pressure just upstream of the critical orifice in the inertial inlet for active continuous determination of the sample flow rate. An auxiliary draw acts to flush the dead volume formed near the base of the conical-shaped critical orifice in the inertial inlet. (b) Solid model of the QC-TILDAS vibration isolation mounting plate. (c) Photograph of the QC-TILDAS mounted to the vibration isolation plate while installed aboard the C-130 aircraft. (d) Photograph of the impinger used for active continuous passivant addition.

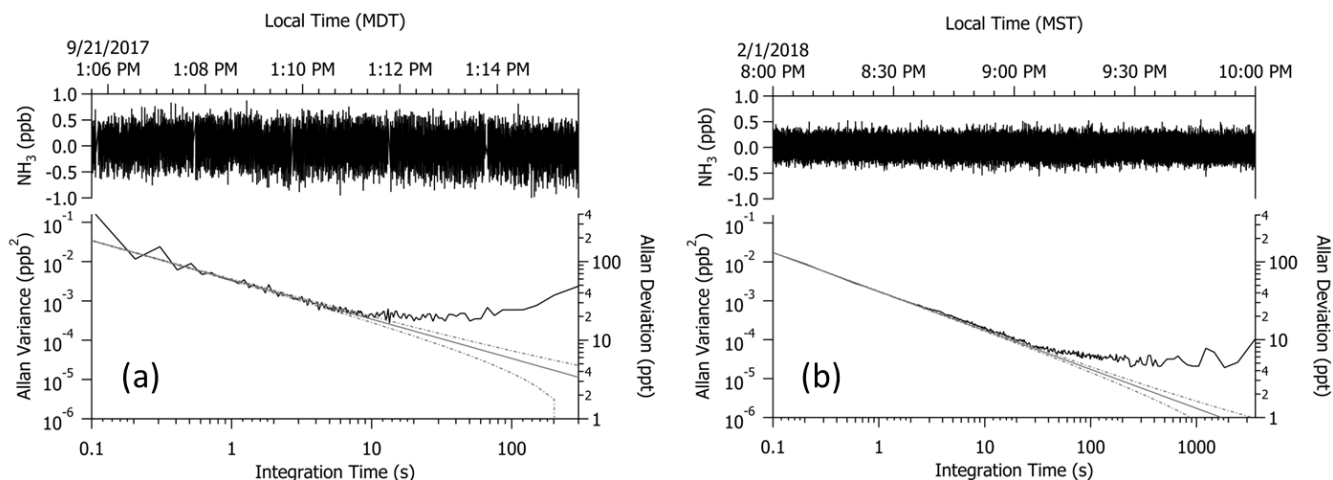
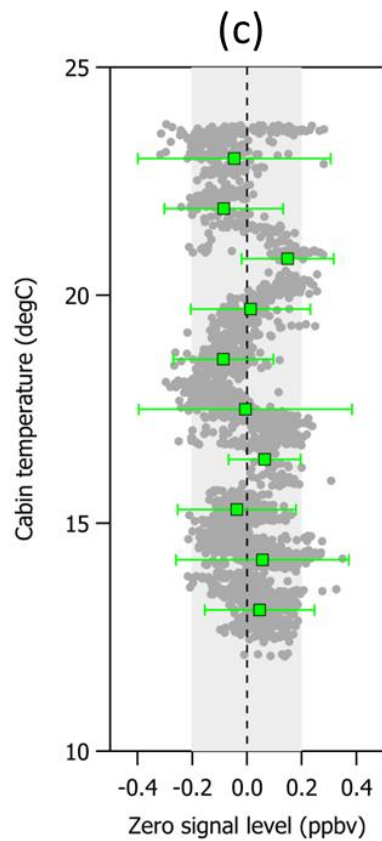
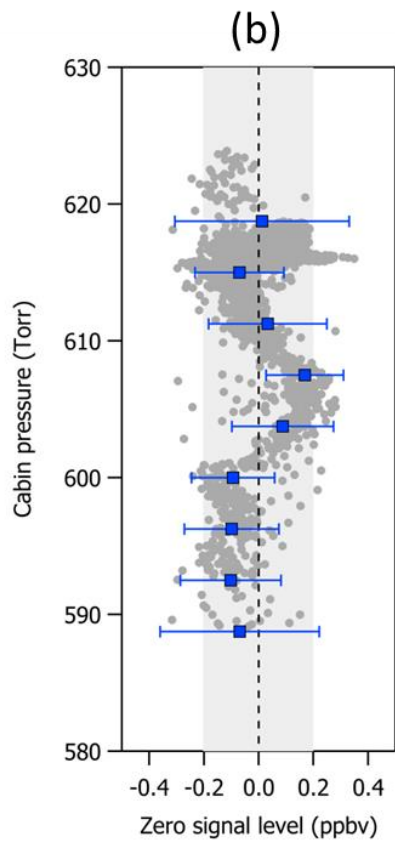
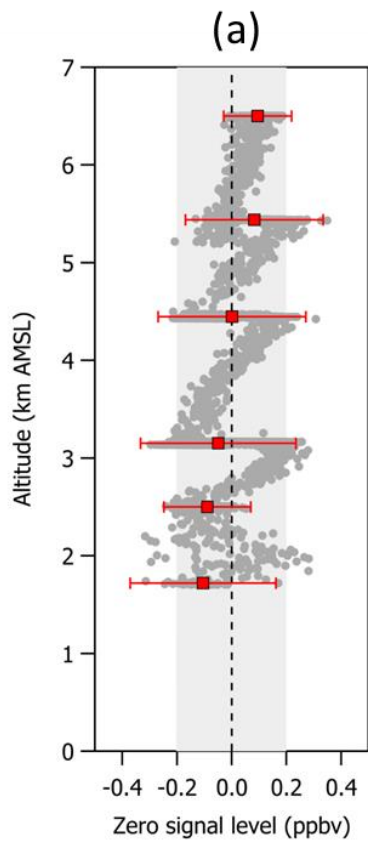


Figure 2: 10-Hz measurements collected while overblowing NH_3 -free air at the inlet tip (a) in flight in the boundary layer near 1.4 km AGL and (b) on the ground in the laboratory. Upper traces represent the raw 10-Hz data collected; lower traces depict the Allan variance in ppb^2 (left axis) and Allan deviation in ppt (right axis) of the corresponding data set. An offset of -150 pptv was applied to the ~~Allan noise guidelines (gray and dashed lines)~~ variance in panel (a) to ~~reflect account for differences induced by the~~ vibration applied to the laser objective to reduce motion sensitivity in flight; the vibration was not applied during laboratory tests depicted in panel (b).



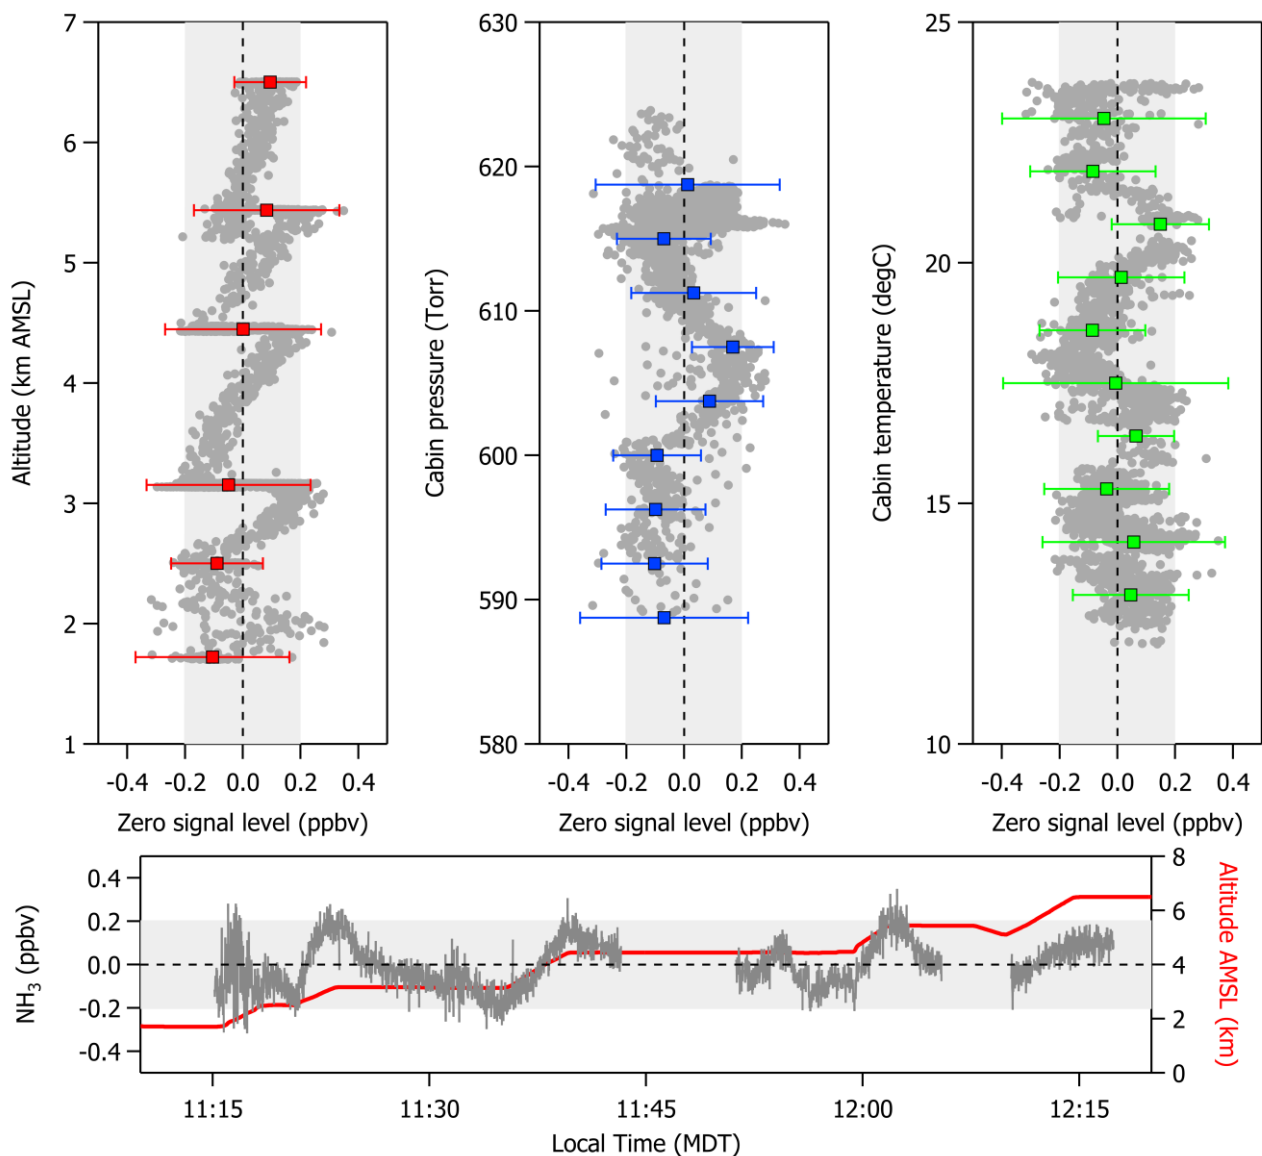


Figure 3: In-flight variations in zero signal level (in units of ppbv of NH_3) with respect to changes in (a) altitude, (b) cabin pressure, and (c) cabin temperature. Gray symbols represent the 1 s average of all of the 10-Hz data points collected in flight while overblowing the inlet tip with NH_3 -free air. Colored symbols and error bars represent the average NH_3 zero signal and 3σ standard deviation for each altitude step of an ascent profile, 5 Torr increments in cabin pressure, and 2°C increments in cabin temperature. Variations are largely within ± 200 ppbv detection limit (denoted by the light gray shaded areas). Gaps in the time series represent times when the instrument was performing a calibration or measuring ambient air.

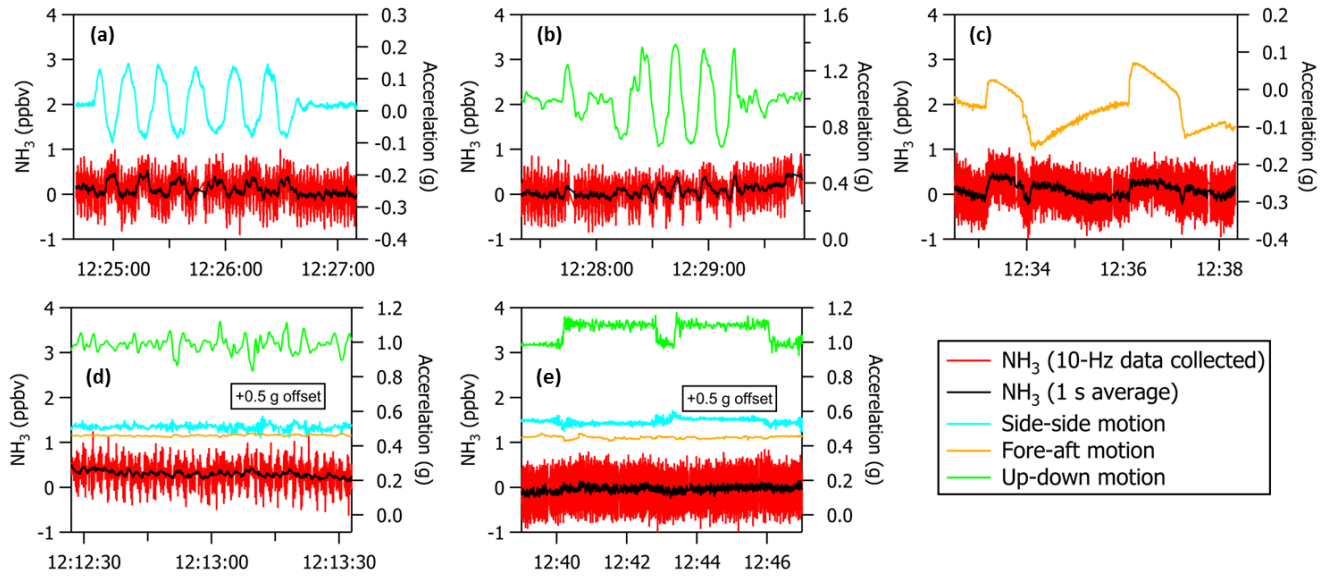


Figure 4: Maneuvers performed at 2.6 km AGL in flight while overblowing the inlet tip with NH₃-free air show changes in NH₃ zero signal (in units of ppbv) with respect to aircraft accelerations (in units of g) in the (a) side-side, (b) up-down, and (c) fore-aft motions. Changes in NH₃ zero signal associated with (d) turbulence in the mixed boundary layer at 0.3 km AGL and (e) during turns at 2.6 km AGL are < 50 ppt when scaled by the $\Delta\text{NH}_3/\text{g}$ observed in each individual dimension during maneuvers. Side-side and fore-aft accelerations are offset by +0.5 g for display purposes in plots (d) and (e).

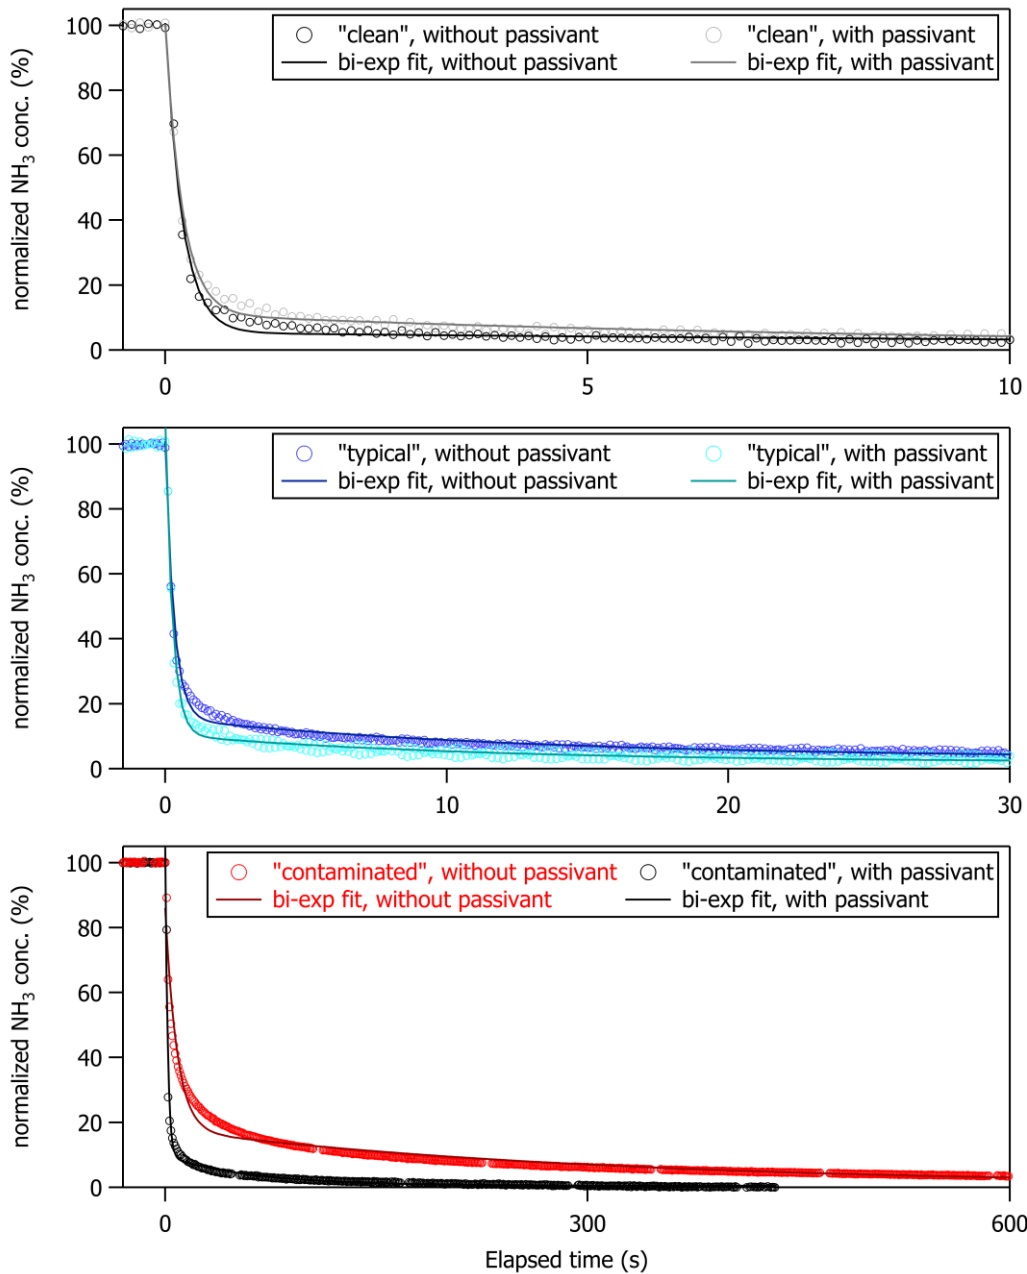


Figure 5: Normalized NH_3 signal (in %) versus elapsed time (in seconds) following a step change in NH_3 mixing ratio generated by switching off calibration gas at $t=0$ s. Temporal profiles and associated bi-exponential fits are shown for the non-passivated and passivated instrument operated under (a) "clean", (b) "typical", and (c) "contaminated" sampling surface conditions. Fits ranged from t_0 to 400, 1000, and 3000 s for the "clean", "typical", and "contaminated" cases, respectively, in accord with the elapsed time collected for each time profile.

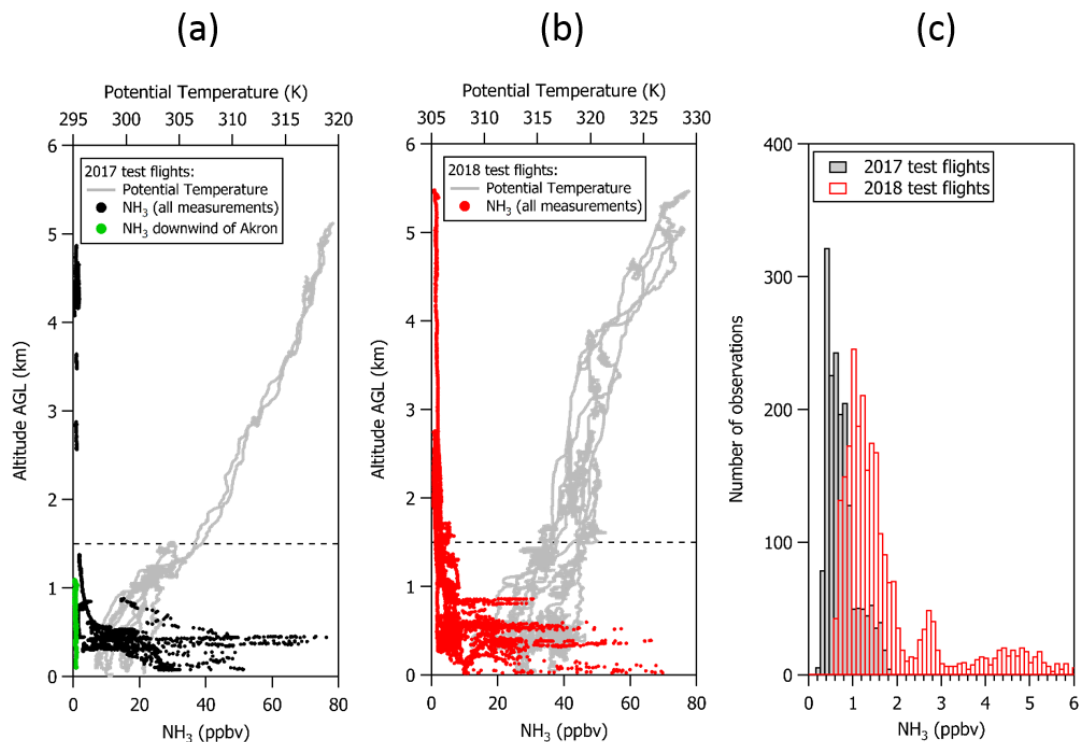


Figure 6: Vertical profiles of NH_3 (in ppbv) and potential temperature (in K) from (a) the first and third test flight in 2017 and (b) the test flights in 2018 when the instrument was operated without passivant. NH_3 mixing ratios as high as 80 ppbv were observed in the mixed boundary layer during missed approaches at Greeley-Weld County Airport and over northeastern Colorado compared to average mixing ratios of ~ 0.8 ppbv near Akron, Colorado following several days of rain. (c) Histograms of the corresponding NH_3 measurements collected above 1.5 km AGL (dashed line) show that measurements were frequently larger than 200 ppt, especially measurements that were collected in the free troposphere.

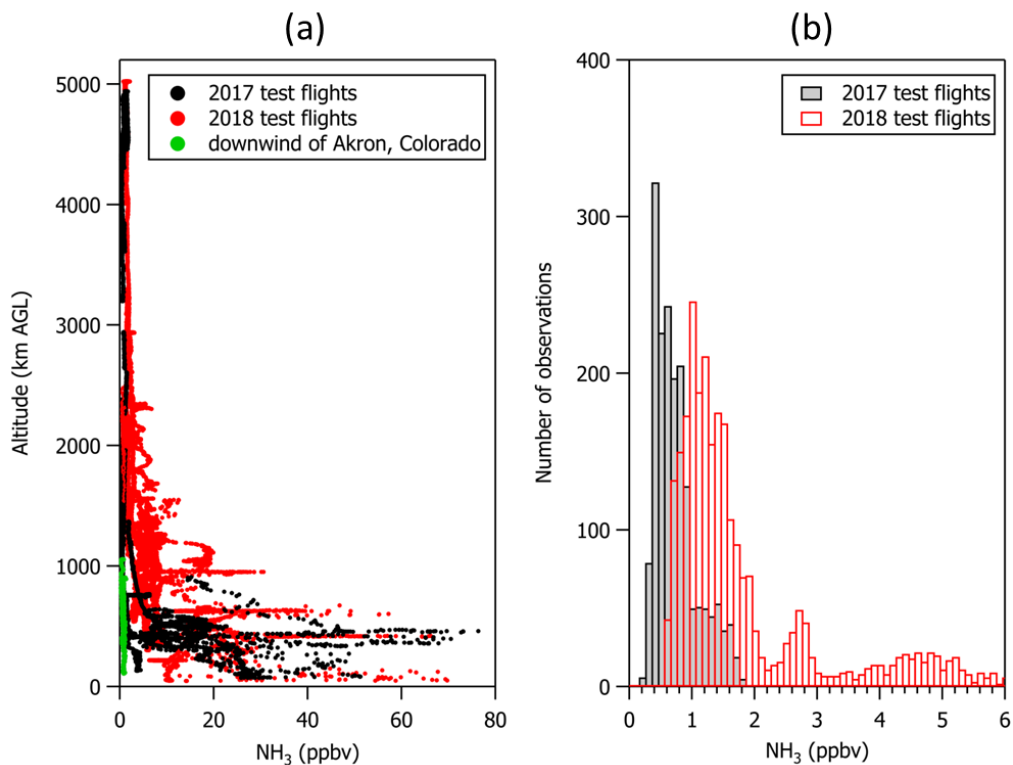


Figure 6: (a) Vertical profile of NH_3 from the first and third test flight in 2017 and the second test flight in 2018 when the instrument was operated without passivant show concentrations as high as 80 ppbv in the mixed boundary layer during missed approaches at Greeley Weld County Airport and over northeastern Colorado compared to average mixing ratios of ~0.8 ppbv near Akron, CO following several days of rain. (b) Histograms of the corresponding NH_3 measurements collected in the free troposphere above 1.5 km AGL; ambient NH_3 measurements in the free troposphere were frequently greater than the 200 pptv detection limit.

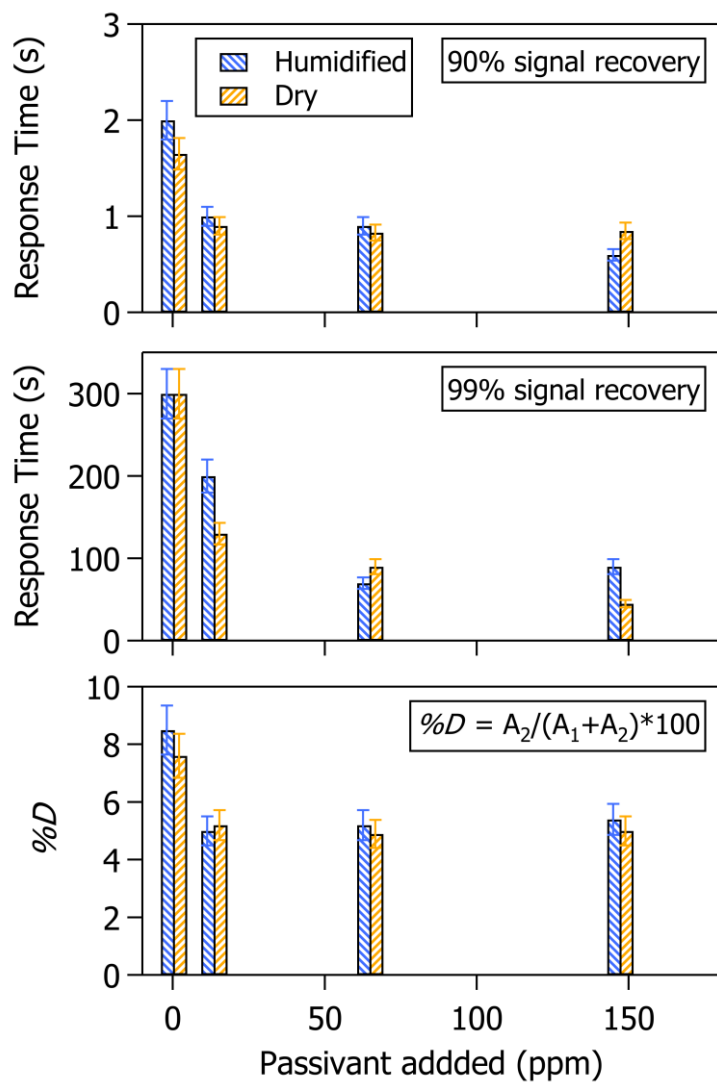
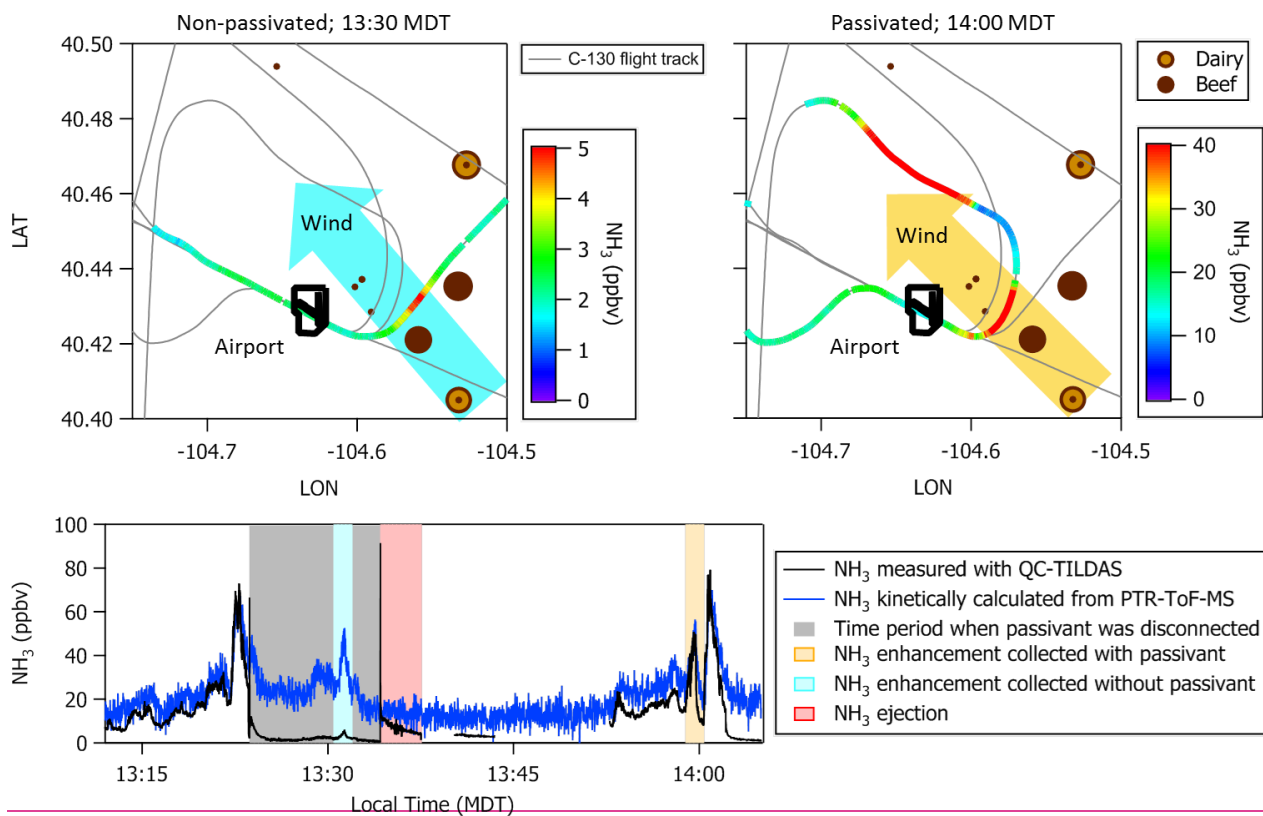


Figure 7: Response times (t_{90} and t_{99}) and %D associated with increasing C8 passivant addition for a step change in NH_3 mixing ratio generated on top of a dry versus humidified background.



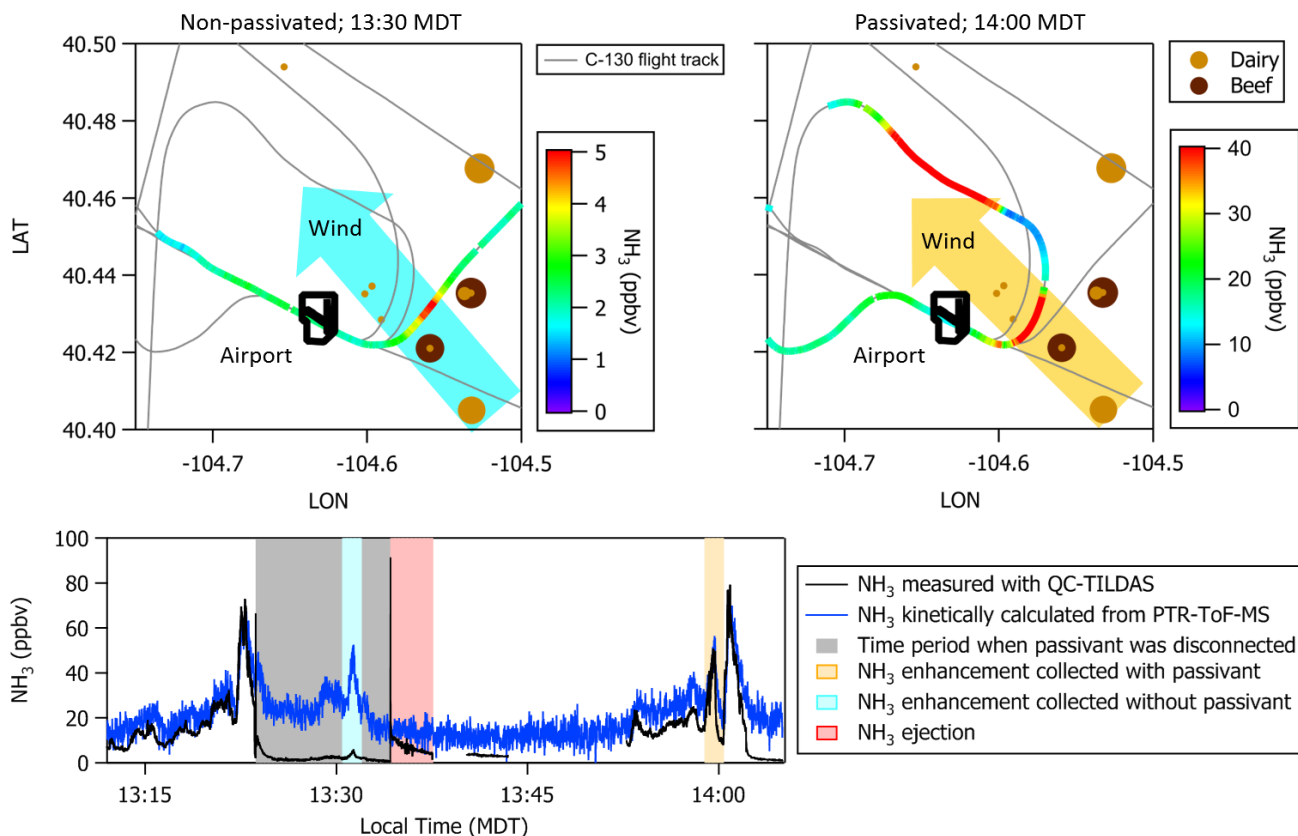


Figure 8: (upper) C-130 flight tracks and measured winds during the 29 Sept 2017 test flight. Colored segments of the flight tracks highlight enhancements in NH_3 measured downwind of concentrated animal operations (brown symbols sized by head of cattle) located southeast of Greeley-Weld County Airport. (lower) Time series of 1-Hz NH_3 mixing ratios measured using the “contaminated” QC-TILDAS instrument and kinetically calculated from a raw instrument signal obtained simultaneously aboard the C-130 aircraft by a Proton Transfer Reaction Time of Flight Mass Spectrometer (PTR-ToF-MS). Portions of the flight when the “contaminated” QC-TILDAS was non-passivated (at 13:30 MDT) and passivated (at 14:00 MDT) are highlighted by colored shaded areas in the time series. Passivant was disconnected from the QC-TILDAS instrument system between 13:23 and 13:34 MDT (as indicated by the gray shaded area); NH_3 ejection is observed when passivant is re-added to the system (red shaded area).

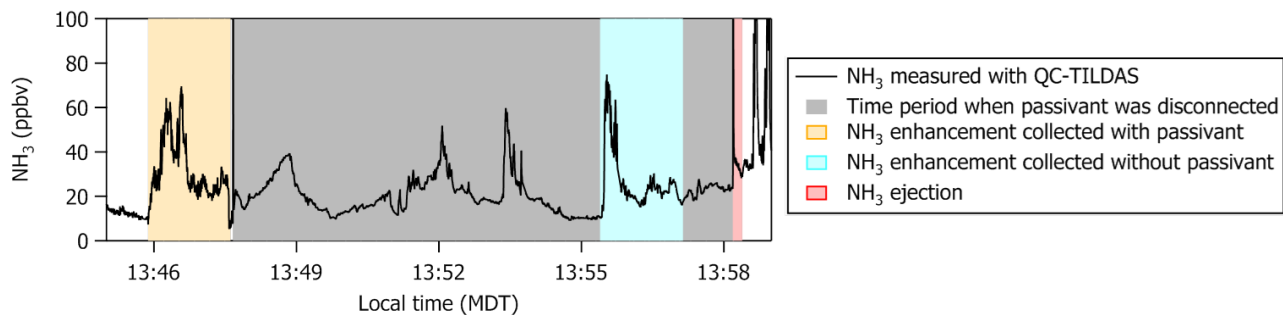
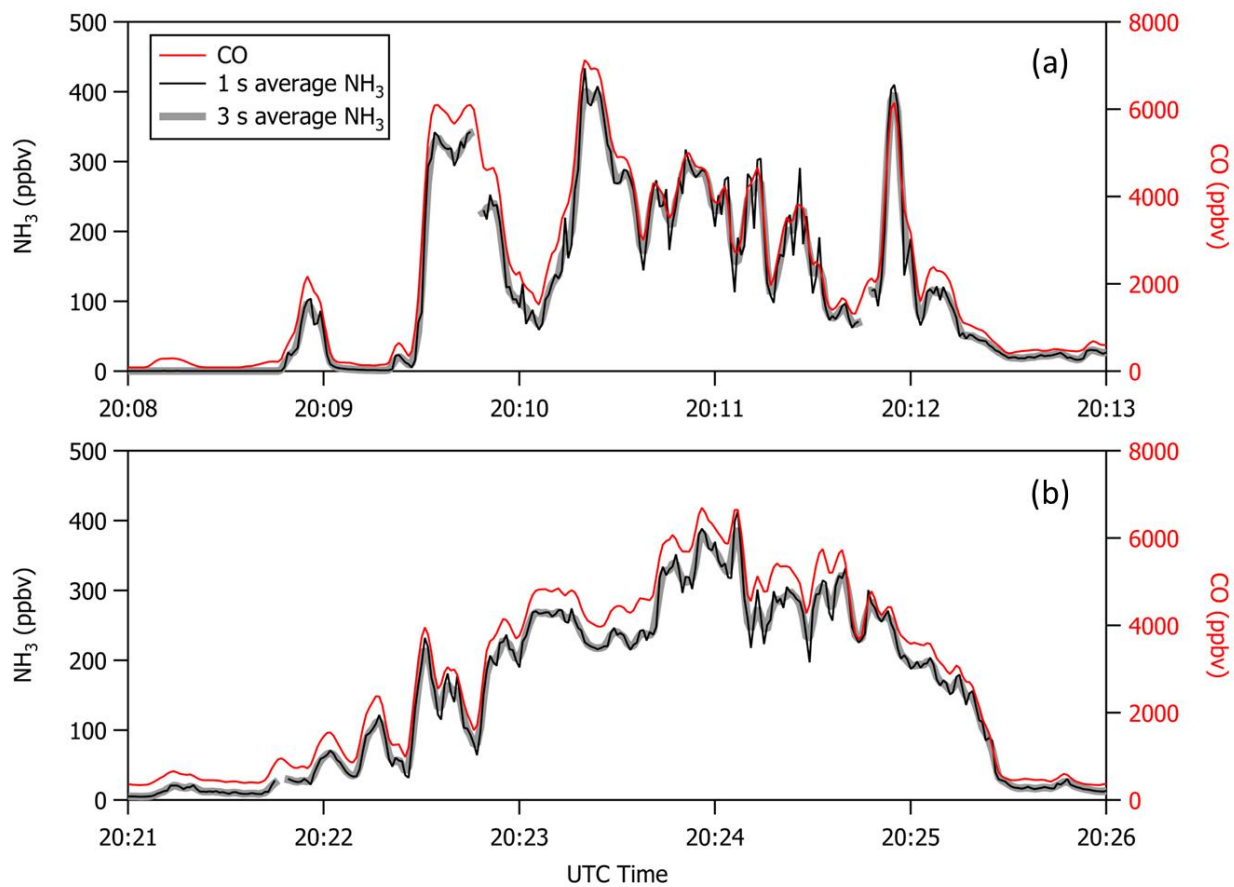


Figure 9: Time series of 1-Hz NH_3 mixing ratios measured with a “clean” QC-TILDAS during the test flight on 13 July 2018. Portions of the flight when the QC-TILDAS was passivated (at 13:46 MDT) and non-passivated (at 13:58 MDT) are highlighted by colored shaded areas in the time series. Passivant was disconnected from the instrument system between 13:47 and 13:58 MDT (as indicated by the gray shaded area); NH_3 ejection is observed when passivant is re-added to the system (red shaded area).



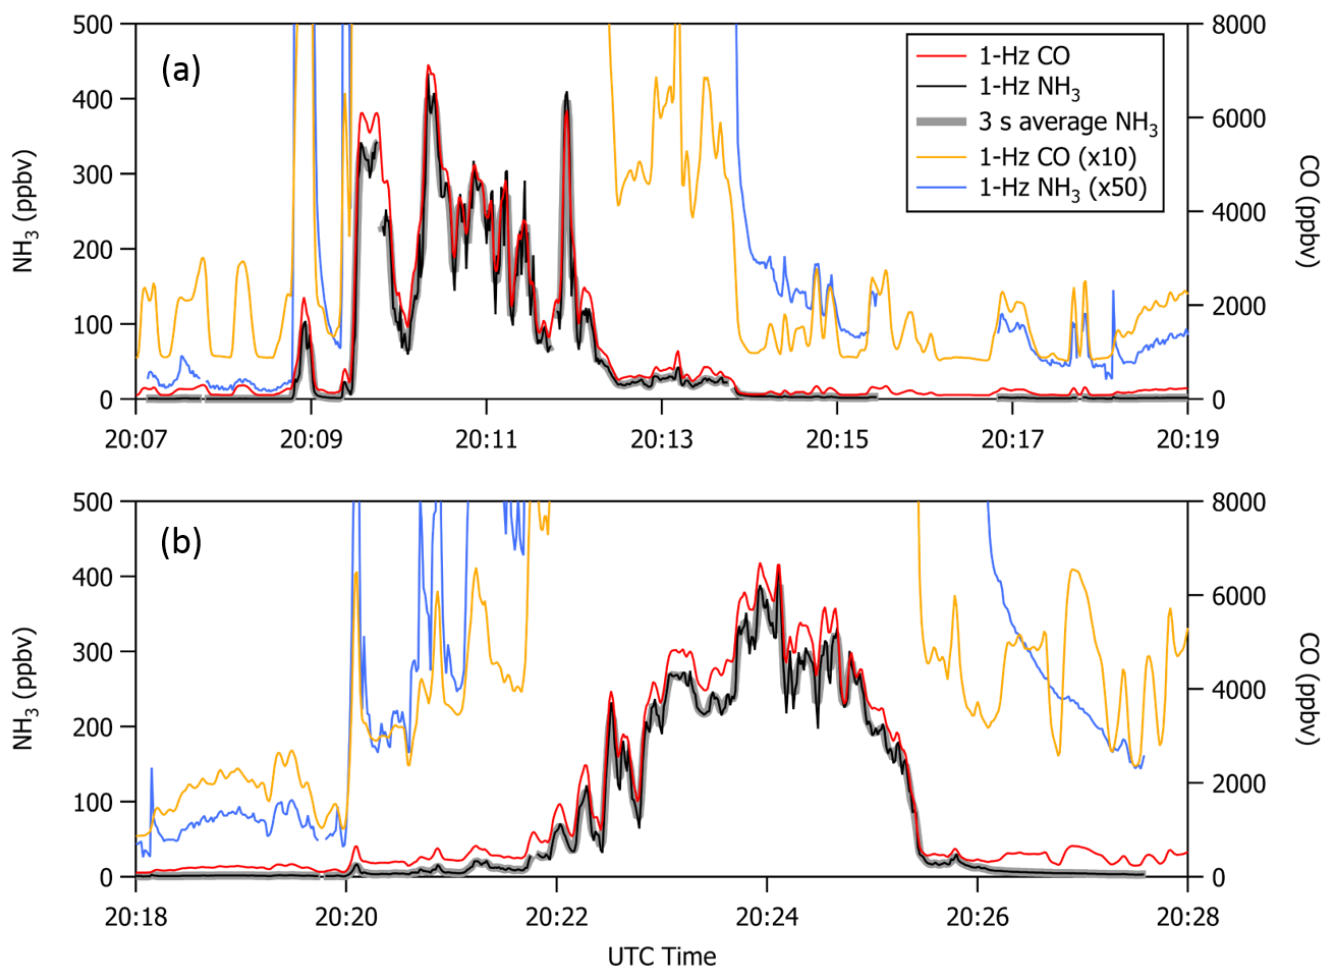


Figure 10: Time series of 1-Hz NH_3 (black lines) and CO (red lines) measured during a crosswind transect of the smoke plume from the South Sugarloaf Fire (RF15) on 26 August 2018. The transects represent nearly identical passes through the smoke plume with the only perturbation of the NH_3 instrument being operated (a) with passivant and (b) without passivant. Changes in fine structure features in NH_3 measurements, displayed as a 1 s average and a 3 s average, have the strongest R^2 correlation with CO measurements when the NH_3 measurements are averaged to 3 s. Similar time resolution for the passivated (a) and non-passivated (b) NH_3 measurements indicates that the sampling surfaces were “clean” during this research flight. A x50 magnified view of 1-Hz NH_3 (blue lines) and x10 magnified view of CO (orange lines) shows differences in background levels of NH_3 compared to CO before and after each plume transect.