

Intercomparison of nitrous acid (HONO) measurement techniques in a megacity (Beijing)

Leigh R. Crilley¹, Louisa J. Kramer¹, Bin Ouyang², Jun Duan³, Wenqian Zhang⁴, Shengrui Tong⁴, Maofa Ge⁴, Ke Tang³, Min Qin³, Pinghua Xie³, Marvin D. Shaw^{5,6}, Alastair C. Lewis^{5,6}, Archit Mehra⁷, Thomas J. Bannan⁷, Stephen D. Worrall⁷▲, Michael Priestley⁷^, Asan Bacak⁷, Hugh Coe⁷, James Allan^{7,6}, Carl J. Percival⁷!, Olalekan A. M. Popoola⁸, Roderic L. Jones⁸ and William J. Bloss¹.

¹School of Geography, Earth and Environmental Science, University of Birmingham, Edgbaston, Birmingham, B15 2TT, UK

²Lancaster Environment Centre, Lancaster University, LA1 4YQ, UK

10 ³Key Laboratory of Environment Optics and Technology, Anhui Institute of Optics and Fine Mechanics, Chinese Academy of Sciences, Hefei, 230031, China

⁴Beijing National Laboratory for Molecular Sciences (BNLMS), State Key Laboratory for Structural Chemistry of Unstable and Stable Species, CAS Research/Education Center for Excellence in Molecular Sciences, Institute of Chemistry, Chinese Academy of Sciences, Beijing 100190, China

15 ⁵Wolfson Atmospheric Chemistry Laboratories, University of York, Heslington, York, YO10 5DD, UK

⁶National Centre for Atmospheric Science, UK

⁷Centre for Atmospheric Science, School of Earth and Environmental Sciences, University of Manchester, Manchester, M13 9PL, UK

⁹Department of Chemistry, University of Cambridge, CB2 1EW, UK

20 ▲ Now at Chemical Engineering and Applied Chemistry, School of Engineering and Applied Sciences, Aston University, Birmingham, B4 7ET, UK

^ Now at: Atmospheric Science, Department of Chemistry and Molecular Biology, University of Gothenburg, Gothenburg, Sweden

! Now at Jet Propulsion Laboratory, 4800 Oak Grove Drive, Pasadena, CA 91109, USA

25

Correspondence to: William J. Bloss (w.j.bloss@bham.ac.uk)

Abstract. Nitrous acid (HONO) is a key determinant of the daytime radical budget in the daytime boundary layer, with quantitative measurement required to understand OH radical abundance. Accurate and precise measurements of HONO are therefore needed; however HONO is a challenging compound to measure in the field, in particular in a chemically complex and highly polluted environment. Here we report an inter-comparison exercise between HONO measurements performed by two wet chemical techniques (the commercially available LOPAP and a custom-built instrument) and two Broadband Cavity Enhanced Absorption Spectrophotometer (BBCEAS) instruments at an urban location in Beijing. In addition, we report a comparison of HONO measurements performed by Time of Flight Chemical Ionization Mass Spectrometer (ToF-CIMS) and Selected Ion FlowTube Mass Spectrometer (SIFT-MS) to the more established techniques (wet chemical and BBCEAS). The key finding from the current work was that all instruments agree on the temporal trends / variability in HONO ($r^2 > 0.97$), yet displayed some divergence in absolute concentrations, with the wet chemical methods consistently higher overall than the BBCEAS systems by between 12 and 39%. We found no evidence for any systematic bias in any of the instruments, with the exception of measurements near instrument detection limits. The causes of the divergence in absolute HONO concentrations

30
35

were unclear, and may in part have been due to spatial variability, i.e. differences in instrument location / inlet position but this observation may have been more associative than casual.

1 Introduction

5 Nitrous acid (HONO) is one of the key daytime sources of radicals in the boundary layer, as it readily undergoes photolysis to form the OH radical, the contribution of HONO photolysis to the OH budget can be significant in megacities, up to 33% in Beijing (Yang et al., 2014) and 40% in London (Lee et al., 2016) as well as forest (33%, Kleffmann et al. 2005) and rural areas (42%, Acker et al. 2006). The OH radical is the primary oxidant in the troposphere that drives chemical processing, principally the oxidation of volatile organic compounds (VOC) that lead to the formation of ozone and secondary organic
10 aerosols. There are a number of known sources of HONO including direct emissions, heterogeneous reactions, homogenous gas-phase reactions, biological processes and surface photolysis (see reviews by (Lammel and Cape 1996;Kleffmann, 2007;Spataro and Ianniello, 2014) and recently abiotic and biotic processes on soils and biocrusts (Weber et al., 2015;Kim and Or 2019). Across urban areas, high spatial heterogeneity in HONO concentration can be observed depending on the proximity to direct emission sources of HONO (Crilley et al., 2016;Lee et al., 2013). Despite, the importance of HONO to the overall
15 radical budget, the contributions of these different sources, particularly in the urban environment, are poorly understood (See e.g. (Lee et al., 2016;Michoud et al., 2014)).

As a result of the significance of HONO to tropospheric photochemistry, accurate and precise concentration measurements are required, but are challenging due to a number of known potential artefacts in the available approaches: Positive artefacts can
20 occur in inlet lines, as HONO is easily formed through heterogeneous reactions on wet surfaces (Zhou et al., 2003). Furthermore, the highly reactive nature of HONO means that within inlet lines wall interactions could also lead to a negative artefact, unless inert materials are employed (Pinto et al., 2014). Other challenges include interferences from species such as NO₂. There are a number of approaches to measure HONO that can be classed as either wet chemical, spectroscopic techniques or off-line methods (Spataro and Ianniello, 2014). Some of the main instrumentation used recently to measure ambient HONO
25 in the literature include differential optical absorption spectroscopy (DOAS, e.g. (Perner and Platt, 1979)), wet chemical techniques (e.g. Long Path Absorption Photometer (LOPAP), (Heland et al., 2001)), broadband cavity enhanced absorption spectroscopy (e.g. (Duan et al., 2018)), soft chemical ionization mass spectrometry (CIMS, e.g. (Veres et al., 2015)), on-line ion chromatography (e.g. (Stutz et al., 2010;Cheng et al., 2013)) and wet denuder (e.g. (Acker et al., 2004)). In order to compare reported measurements across studies, it is necessary to understand how the different approaches/techniques compare relative
30 to each other, under actual ambient (field) conditions.

There have been a number of studies reporting inter-comparisons between HONO instrumentation (e.g. (Stutz et al., 2010;Ródenas et al., 2013;Pinto et al., 2014;Kleffmann et al., 2006)). Generally, HONO measurements by DOAS systems are used as a reference during inter-comparison studies, as optical methods are artefact free with respect to sampling method, though impurities in the HONO and NO₂ reference spectra can affect retrievals (Stutz et al., 2010;Kleffmann et al., 2006). A
5 further complication with using DOAS systems as a reference is that the spatial averaging inherent in the system means that comparison with point measurements may be subject to bias due to spatial heterogeneities in HONO concentrations. Typically, most in-situ instruments report higher concentrations during the day compared to simultaneous measurements by a DOAS system, thought to be due to the positive interferences in the in-situ techniques (see e.g. (Febo et al., 1996;Appel et al., 1990;Stutz et al., 2010;Spindler et al., 2003)). An exception is the work by Kleffmann et al. (2006), who reported excellent
10 agreement between a LOPAP and DOAS system in both chamber based and field measurements of HONO under both day and night conditions. The reason for the better performance of the LOPAP is the two channel stripping coil employed in the LOPAP successfully corrects for positive artefacts and chemical interferences during measurement, as demonstrated by Kleffmann and Weisen (2008).

15 Recently, there have been multi-instrumental inter-comparison studies performed in ambient air and in simulation chambers. These include the Formal Intercomparison of Observations of Nitrous Acid (FIONA) project, which involved 18 instruments measuring within the European Photoreactor (EUPHORE) chamber over a wide range of HONO concentrations (Ródenas et al., 2013). While in general, good agreement was observed during the different experiments of FIONA, at high concentrations (>15 ppb) divergence was observed between some instruments possibly due to some instruments experiencing saturation
20 (Ródenas et al., 2013). These high HONO concentrations however are not typical even in highly polluted locations like Beijing (Tong et al. 2016; Wang et al. 2017). Pinto et al. (2014) described an inter-comparison of field measurements performed in Houston using a number of instruments for measuring HONO. The instruments tested included a long-path DOAS, a number of wet chemical (including a LOPAP), on-line ion-chromatography and a Time of Flight Chemical Ionisation Mass Spectrometer (ToF-CIMS) using iodide as a reagent ion CIMS. Overall, while good agreement between all the instruments
25 was observed in terms of the temporal trends, the absolute concentrations varied. Pinto and co-workers were unable to pinpoint the cause of the disagreement in absolute concentrations but speculated it might have been due to chemical interference in the in-situ techniques, and the effect of heterogeneous surface reactions due to the distance between some inlets.

Here, we report an inter-comparison exercise of co-located wet chemical and broadband cavity enhanced absorption
30 spectrophotometer (BBCEAS) instruments for measuring HONO in an urban location within Beijing. Ambient concentrations of HONO can vary by several orders of magnitude in Beijing, up to 9 ppb during haze events with a typical concentration of 1.44 ± 1.33 ppb (Wang et al., 2017), making it a challenging location for field measurements. In addition, we report a comparison of HONO retrievals by a ToF-CIMS and Selected Ion FlowTube Mass Spectrometer (SIFT-MS) to the more

established techniques (wet chemical and BBCEAS) for measuring HONO. Based on the inter-comparison findings, the factors that may have influenced the measured concentrations are investigated.

2 Method

2.1 Site description

5 Measurements were performed as part of the Air Pollution and Human Health in a Chinese megacity (APHH-Beijing, www.aphh.org.uk) program and of the ‘An integrated study of air pollution processes in Beijing’ (AIRPRO) project, which aimed to understand atmospheric processes affecting air pollution in Beijing. An overview of the APHH-Beijing project is provided in Shi et al. (2018). Measurements were performed at the Chinese Academy of Sciences’ Institute of Atmospheric Physics (IAP) tower campus, an urban site located near the 4th ring road in the northern suburbs of Beijing. There were two
10 field campaigns, the first took place during Nov-Dec 2016 (referred to as winter) and second during May-June 2017 (referred to as summer).

2.2 Instrument descriptions

An overview of all the instruments that measured ground-level HONO at IAP is provided in Table 1. As instruments of the same type were used in this study, throughout this paper the instruments will be referred to by their institution name, as per
15 Table 1. A brief description of each instrument follows.

2.2.1 University of Birmingham LOPAP

The University of Birmingham operated a LOPAP(QUMA Elektronik & Analytik GmbH) at IAP.. The LOPAP is a wet chemical technique and has been described in detail in Heland et al. (2001) and Kleffmann et al. (2002). Briefly, a stripping coil is used to sample gas-phase HONO into an acidic solution where it is derivatized into an azo dye. The light absorption of
20 the azo dye, principally at 550 nm (though higher wavelengths can also be used), is then measured with a spectrometer using an optical path length of 2.4 m. The LOPAP was operated and calibrated according to the standard procedures described in Kleffmann and Wiesen (2008). The time resolution of the LOPAP was 5 minutes and baseline measurements were taken at frequent intervals (8hrs). The operationally defined detection limit (2σ) of the LOPAP was calculated to be 35 and 5 ppt for winter and summer, respectively and varied due to changes in purity of reagents and zero air used. The LOPAP was housed
25 within a temperature controlled shipping container and sampled at a height of 3m above ground level.

2.2.2 Institute of Chemistry, Chinese Academy of Sciences wet chemical HONO analyser

ICCAS applied a custom-built instrument, described in detail elsewhere (Hou et al., 2016). It is a wet chemical technique similar in principle to the LOPAP. Gas-phase HONO is almost completely absorbed by an absorption solution into a two-

channel stripping coil, where it forms an azo dye, detected by absorption spectroscopy at a wavelength of 550 nm with an optical path length of 0.5 m. The instrument has a detection limit (2σ) of 134 ppt for a response time of 5 min. The ICCAS and BHAM instruments both used a similar outdoor sampling unit that employed a short quartz inlet (<2.5cm). While the BHAM and ICCAS instruments operated according to the same principles, there were two main differences. The first was the method for determining the baseline, the BHAM instrument used an overflow of N_2 while the ICCAS instrument replaced the reagents with water. The second was the optical path length, which was 2.0 and 0.5 m for the BHAM and ICCAS instruments, respectively.

2.2.3 University of Cambridge BBCEAS

The University of Cambridge ran a three-channel BBCEAS instrument during the campaign, with one channel measuring NO_2 and HONO simultaneously in the UV (362-374 nm) wavelength region. Reference absorption cross-sections of HONO (Stutz et al., 2000) and NO_2 (Voigt et al., 2002), were fitted to the absorption coefficient to retrieve HONO and NO_2 concentrations. Details of the instrument can be found in Kennedy et al. (2011). Two mirrors (Layertec 109053) with peak reflectivity of ~99.95% at 365 nm were used to form the cavity. Given an inter-mirror distance of 92 cm, the effective absorption pathlength in the case of an empty cavity was around 1.8 km. Both instrument inlet and the optical cavity were made of perfluoroalkoxy alkane (PFA) which is well known for its chemical inertness. The inlet line was ¼' outer diameter PFA tubing and was approximately 3m long. During the winter phase of the campaign, instrument inlet was placed at the top of the container and was about 3 m from ground. During the summer phase however, the instrument was moved to an adjacent container, also housing the other BBCEAS instrument, and the height of instrument inlet was changed accordingly from ~3 to ~2 m.

To allow a more stable cavity throughput (i.e. to minimise flow turbulence effect on the optical signal), the sampling flow was set to 2 LPM for the HONO/ NO_2 measurement channel. This was close to the very low end of the operational range of the flow controller (0-50 LPM), leading to the actual flow rate potentially differing from that set. Post-campaign analysis identified that this affected both the dilution factor (dilution of the sample flow by the two mirror purge lines) and the length the sample gas occupied in the cavity. A post-campaign calibration was therefore performed by injecting a known amount of NO_2 into the cavity under otherwise identical operating conditions, and a scaling factor of ~1.27 was found to be necessary to account for these two factors, and was then applied to the measured NO_2 and HONO concentrations.

2.2.4 Anhui Institute of Optics and Fine Mechanics BBCEAS

The custom-built BBCEAS instrument from the Anhui Institute of Optics and Fine Mechanics (AIOFM), Chinese Academy of Sciences has been described in detail in Duan et al. (2018); therefore only a brief description is given here. Light is emitted by a single light emitting diode with peak wavelength of 365 nm, FWHM of 13 nm and is introduced into the resonant cavity, consisting of a pair of high reflective (HR) mirrors with reflectivity of about 0.99985 at 368 nm, separated by 55.0 cm. The

emergent light intensity passing through the cavity exit mirror is received by an Ocean Optics QE65000 spectrometer through an optical fibre with 600 μm diameter, and a 0.22 numerical aperture.

In order to avoid the drift of the center wavelength of the LED, the temperature of the LED was controlled to be approximately 20 ± 0.05 °C by using a TEC unit. In order to prevent particulate matter from entering the cavity and reducing the effect of particulate matter on the effective absorption path, a 1 μm PTFE filter membrane (Tisch Scientific) was used in the front end of the sampling port. The time resolution of the IBBCEAS instrument was 1 min, and the 2σ detection limit of HONO was about 120 pptv. The fitting wavelength range was selected as 359–387 nm, with the same reference cross-sections used in the retrieval of NO_2 and HONO as for the University of Cambridge instrument. Sample loss and secondary formation of HONO were both considered in this instrument and the measurement error of HONO was estimated to be approximately 9%. The inlet line was $\frac{1}{4}$ ' outer diameter PFA tubing and was approximately 4m long.

2.2.5 University of Manchester ToF-CIMS

A time of flight chemical ionisation mass spectrometer (ToF-CIMS) (Lee et al. 2014), using an iodide ionisation system was coupled with a filter inlet for gases and aerosols (FIGAERO) originally developed by Lopez-Hilfiker et al. (2014) and recently described and characterised by Bannan et al. (2019). The detailed setup during this campaign can be found in Zhou et al. (2018). The FIGAERO enabled near simultaneous, real-time measurements of both the gas and particle phase composition. Only gas phase data is presented here, so of every 75 minutes of continuous data 35 minutes (particle phase mode) are omitted. The gas phase inlet consisted of 5 m $\frac{1}{4}$ " I.D. PFA tubing connected to a fast inlet pump with a total flow rate of 13 standard litres per minute (slm) from which the ToF-CIMS sub-sampled 2 slm.

Methyl iodide gas mixtures (CH_3I) in N_2 were made up in the field using a custom-made manifold (Bannan et al. 2014). 20 standard cubic centimetres per minute (sccm) of the CH_3I mixture was diluted in 4 slm N_2 and ionised by flowing through a Tofwerk X-ray ionisation source. This flow enters an ion molecule region (IMR) which was maintained at a pressure of 400 mbar using an SSH-112 pump fitted with an Aerodyne pressure control box to account for changes in ambient pressure. The IMR pressure is significantly higher than is usual for this CIMS instrument when using PO-210, but is necessary given the change in ionisation source in this study. Operation is comparable to the Breton et al., (2018) study who also used the same Tofwerk X-ray ionisation source. A short segmented quadrupole (SSQ) was positioned behind the IMR and was held at a pressure of 2 mbar using a Tri scroll 600 pump.

The CIMS instrument zero was determined by flowing dry nitrogen into the IMR periodically, and the backgrounds were applied consecutively. As shown in Figure S1 (Supporting Information), there was very little variability of this background during the measurement period. Though the overflowing of dry N_2 will have an effect on the sensitivity of the instrument to those compounds whose detection is water dependent, due to the low instrument backgrounds, the absolute error remains small

and we deem this an acceptable limitation in order to measure a vast suite of different compounds for which no best practice backgrounding method has been established. We therefore calculated the absolute error of 33 ppt as 3 sigma deviations of the background signal.

Field calibrations were regularly carried out using known concentration formic acid gas mixtures made in the manifold. The instrument was calibrated for a range of other species after the campaign, and relative calibration factors were derived using the measured formic acid sensitivity as has been performed previously (Le Breton et al., 2014; Le Breton et al., 2017; Bannan et al., 2014; Bannan et al., 2015). HONO was measured at m/z 174 as $I\cdot HNO_2^-$ during the period of 27th May – 17th June 2017. A stable and pure gas phase source of HONO was generated for calibrations using the method described by Ren et al. (2010) and Febo et al. (1995) and a sensitivity of 0.28 cps/ppt was applied to the data with a LOD of 33 ppt. Data analysis is performed using the “Tofware” package (version 2.5.11) running in the Igor Pro (WaveMetrics, OR, USA) environment. The mass axis was calibrated using I_1 , I_2^- and I_3^- . Extracted high resolution time series were then normalised to the iodide reagent ion trace. A limitation of the CIMS calibration approach for HONO is that it was not established as a function of humidity. This was not deemed necessary because there was an average variation of only 2% in the $I^-:H_2O^-$ ratio throughout the day.

2.2.6 University of York SIFT-MS

The data presented in this paper has been measured using a Voice200 Selected ion flow tube mass spectrometer (SIFT-MS, Syft Technologies, Christchurch, New Zealand). This instrument consists of a switchable reagent ion source capable of rapidly switching between multiple reagent ions. The ion source region where the reagent ions are generated in a microwave discharge, acts on an air/water mix at a pressure of approximately 440mTorr to generate the three reagent ions H_3O^+ , NO^+ , and O_2^+ . These ions are extracted into the upstream quadrupole chamber maintained at a pressure of approximately 5×10^{-4} torr, using a 70 L/s turbo-molecular pump. The reagent ions pass through an array of electrostatic lenses and the upstream quadrupole mass filter, and those not rejected by the mass filter are passed into the flow tube where they are carried along in a stream of nitrogen and selectively ionise target analytes. Gas phase data presented herein was determined using the H_3O^+ reagent ion only. Sampling was carried out at a height of ~3m using a gas phase inlet consisting of 3.5m ¼” I.D. PFA tubing connected to a diaphragm inlet pump (KNF) at a total flowrate of 5 standard litres per minute (slpm), from which the SIFT-MS sampled approximately 2 slpm through an in house built pressure controlled inlet maintaining a consistent absolute inlet pressure of 0.5 bar. The flow tube is pumped by a 35 m³/h scroll-type dry pump (Edwards) resulting in a mass flow controlled gas flow of 25 sccm for the nitrogen carrier gas (research grade, BOC) and a sample flow of 100sccm from the pressure controlled inlet system. These flows result in a continuous total flow tube pressure of 460 mTorr and a reaction time of approximately 8ms (Hera et al. 2018). During the campaign, gas phase backgrounds were established through regularly overflowing the sample inlet with dry nitrogen for 5 continuous minutes every hour. The determined HONO gas phase backgrounds in nitrogen were 110 ± 40 pptv during the measurement period presented and as such are unlikely to have a significant contribution on the ambient mixing ratio.

The bimolecular reaction of H_3O^+ and nitrous acid produces the products ions H_2NO_2 (m/z 48, 67%) and NO^+ (m/z 30, 33%). The rate constant (k) of this exothermic proton transfer reaction is calculated to be $2.7 \times 10^{-9} \text{ cm}^3\text{s}^{-1}$ with respect to hydronium (H_3O^+) and $2.2 \times 10^{-9} \text{ cm}^3\text{s}^{-1}$ with respect to hydronium mono-hydrate ($\text{H}_3\text{O}\cdot\text{H}_2\text{O}$)⁺ (Spangel and Smith, 2000). Nitrous acid does not undergo proton transfer with hydronium di-hydrate ($\text{H}_3\text{O}\cdot\text{H}_2\text{O}^2$)⁺ and tri-hydrate ($\text{H}_3\text{O}\cdot\text{H}_2\text{O}^3$)⁺ in SIFT-MS. Nitrous acid mixing ratios herein were determined using the branching ratio corrected protonated product ion m/z 48 intensity normalized to both H_3O^+ and $\text{H}_3\text{O}\cdot\text{H}_2\text{O}$ with their respective k values (Taipale et al, 2008). As such, calculated HONO mixing ratios using SIFT-MS should be independent of the humidity of the gas sample.

2.3 Formal inter-comparison

The formal inter-comparison of the four established techniques for measuring HONO (2 wet chemical and 2 BBCEAS) took place during the 9th-14th November 2016. All instruments had a sampling height of 3m during the inter-comparison, and inlets were located as close as possible to each other (Figure S2, Supporting Information). The BHAM and ICCAS instrument were housed within the same shipping container, with their respective inlet heads located beside each other on the roof. The CAM and AIOFM BBCEAS instruments were housed in separate containers, with inlets located approximately 5 and 10 m, respectively, from the two wet chemical inlet heads. At the completion of the formal winter intercomparison, the inlet locations changed for some of the instruments.

There was no formal inter-comparison between all four instruments in the summer campaign. The BHAM, CAM and ICCAS inlets were located in the same position as per the winter intercomparison at the start (22nd May - 30th June 2017). Therefore, further analysis was performed between these three instruments for this period to examine for any changes in their relationships compared to the winter measurements. The AIOFM instrument was housed within the same container as per the winter however, the inlet was located approximately 3 m further away from other instruments in the summer. On the 30th May, the CAM instrument was moved to the same container as the AIOFM, with the inlets located approx. 3 m from each other. The ToF-CIMS and SIFT-MS were not initially set up to measure HONO at IAP but were able to provide some useful data during the summer measurements and are therefore compared to the more established techniques. A schematic of inlet locations during the summer campaign is provided in Fig S3 (Supporting Information).

2.4 Data Analysis

The BHAM and ICCAS instruments were operated with a time response of 5 min, and as this was the longest (Table 1), 5 min averages were used for all instruments in the inter-comparison analyses. For each instrument, their normal quality control procedures were applied and only data that passed the quality control was used for subsequent analysis. Data analysis was performed in R (v 3.5.1) using the openair package (Carslaw and Ropkins, 2012) and the lmodel2 package for Reduced Major Axis (RMA) regression analysis.

3 Results

3.1 Winter formal intercomparison

3.1.1 Time series

The time series (Figure 1) demonstrates that while all instruments captured the same temporal trends, the absolute concentrations differed. The correlation coefficients from regression analyses show that there is little scatter between measurements from the different instruments with r values being consistently between 0.96 and 0.98 (Table 2 and Figure S4, Supporting Information). Overall, the BHAM LOPAP measurements were consistently the highest, followed by ICCAS, AIOFM and CAM. The slopes from the RMA analysis demonstrated that none of the instruments were in agreement (Table 2) within their stated error (Table 1) during the formal inter-comparison exercise. Therefore, in the following sections we investigate possible reasons to account for the lack of agreement between instruments.

3.1.2 Analysis of Co-efficient of Variance

We calculated the co-efficient of variance (CV) as a measure of the precision between the four instruments as per Eqn 1:

$$CV = \frac{\sigma}{\mu} \quad (1)$$

where μ is the mean and σ the standard deviation for the measurements by all four instruments at a given 5 min interval. The CV was used to compare the relative degree of variation between datasets and as a guide a CV of 0.1 is considered as acceptable by the US EPA for PM instruments. (Sousan et al., 2016). From Fig 2, the CV was fairly consistent throughout the winter inter-comparison, at an average of 0.28 ± 0.07 . The CV was however observed to increase at the end of the inter-comparison, coinciding with period of the lowest mean HONO concentration (< 1 ppb, Fig 2). An increase in the CV indicates worsening agreement between instruments, possibly due to the concentrations approaching the detection limit (DL) of some instruments (Table 1). NO_2 is a potential interferent for the measurement of HONO for both wet chemical and BBCEAS instruments (Heland et al., 2001). Both BBCEAS instruments use the Voigt et al. (2002) NO_2 cross-section, which has previously been shown to have negligible HONO absorption structures (Veitel, 2002, Kleffmann et al. 2006). We also note that HONO reference spectrum should contain little structure from NO_2 . Overall, Fig 2 demonstrates no apparent relationship between the CV and NO_2 . This likely reflects the efforts taken during processing and measurement to reduce the influence of interference from NO_2 in all instrument types.

3.1.3 Normalised difference analysis

Firstly, the systematic error for each instrument can be calculated by normalised sequential difference (NSD) according to Eqn 2 (Arnold et al., 2007):

$$NSD = \frac{(Conc_t - Conc_{t+1})}{(Conc_t \times Conc_{t+1})^{0.5}} \quad (2)$$

NSD is a method of calculating the variation between consecutive measurements for an individual instrument, where $Conc_t$ is the concentration measured at time t and $Conc_{t+1}$ the following measurement. The results are shown in Fig S5 (Supporting Information), and as each instrument showed a symmetrical and Gaussian distribution it suggests there was no internal systematic bias for any given instrument.

5

Secondly, we then examined the normalized difference (ND) between pairs of instruments to explore inter-instrument variability, calculated according to Eqn 3 (Pinto et al., 2014):

$$ND_{ij} = \frac{(C_i - C_j)}{(C_i + C_j)} \quad (3)$$

where C_i and C_j denote HONO levels measured by any pair of instruments (BHAM, ICCAS, AIOFM or CAM) calculated for each measurement period. For example, the ND for the BHAM and CAM instruments ($ND_{\text{BHAM-CAM}}$) would be calculated by $([\text{HONO}]_{\text{BHAM}} - [\text{HONO}]_{\text{CAM}}) / ([\text{HONO}]_{\text{BHAM}} + [\text{HONO}]_{\text{CAM}})$. We also calculated the co-efficient of divergence (CD), which is a normalized measure of the similarity between two measurement time series, derived via Eqn 4 (See Pinto et al. (2014) and references therein):

$$CD_{ij} = \sqrt{\left(\frac{1}{p}\right) \times \sum (ND_{ij})^2} \quad (4)$$

15 Where p is the number of observations and ND_{ij} is defined in Eqn 3. A CD of one means the time series are completely different, while of CD of zero indicates that they are identical. The calculated CD for each instrument pair is shown in Table 3 and demonstrate that each of the two overall approaches - wet chemical (BHAM and ICCAS) and BBCEAS (AIOFM and CAM) - agreed well internally. The ICCAS and AIOFM also agreed well, but CAM and BHAM had a higher CD with AIOFM and ICCAS (Table 3).

20

If there is no difference between a pair of instruments, then the calculated ND should be scattered around zero, and from Fig 3 this was not observed for any instrument pair, pointing to differences between instruments. The ND was evaluated as function of wind direction and measured HONO concentration (Fig 3), to explore if ambient concentration or spatial heterogeneity could explain the disagreements. From Figure 3, for all instrument pairs the highest ND, and therefore largest relative difference between instruments was at low HONO mixing ratios (ca. <1 ppb) and was also associated with a westerly direction. At high wind speeds, the ND was also high between all instrument pairs (Fig S6, Supporting Information). As we observed high ND at relatively high wind speeds, it would suggest that spatial variability in ambient HONO concentrations did not affect the intercomparison as high wind speeds typically homogenise ambient concentrations from point and local sources. Overall from Figs 3 and S5, the periods of low HONO concentration, high wind speeds and westerly winds all coincided during the formal winter intercomparison making it difficult to disentangle the influence of these factors on the observed ND.

30

3.1.4 Instrument agreement at low concentrations

There was evidence from the CV (Fig 2) and ND (Fig 3) analyses that the level of agreement between instruments decreased at low HONO mixing ratios. Therefore, we applied RMA correlation analysis for periods when the HONO level was below 2 ppb (as measured by CAM), and the results are shown in Table 4. From Table 4, the observed slopes between the BHAM-
5 ICCAS-AIOFM at low concentrations (<2 ppb) were similar to those for the whole winter inter-comparison dataset (Table 2) unlike when compared to the CAM instrument. This suggests that the difference in measured concentrations between these instruments (BHAM-CAM-AIOFM, as indicated by the slope) was not related to concentration. The decrease in the slope for the low concentrations between CAM and the other three instruments compared to whole inter-comparison (Tables 2 and 4, respectively), potentially pointing to changes in the CAM readings at lower concentrations. This change may be related to
10 differences in instrument sensitivity (Table 1).

3.2 Summer Measurements

While there was no formal intercomparison during the summer measurements, at the start of the summer measurements the BHAM, ICCAS and CAM instrument inlets were co-located as per the winter formal intercomparison (Figure S2). The relationship between instruments for this period is shown in Table 5. The agreement (gradient) between BHAM and ICCAS
15 improved in the summer to 0.91 compared to winter (0.77) but with slight changes in intercept (Tables 2 and 5). A change was also observed between CAM and ICCAS with a lower slope observed for the start of summer (Table 5) compared to winter intercomparison period (Table 2).

The AIOFM instrument started measuring halfway through the summer campaign, and while the instrument was housed in the
20 same container the inlet location was a few meters further from the other three instruments than in the winter inter-comparison (Figure S3). As a result, we compared the instrument readings for one week after the AIOFM instrument started measuring (7th-14th June 2017), with the results shown in Table 6. Note during this period the CAM instrument had moved to sample from the same container as AIOFM (Figure S3). From Table 6, the agreement between instruments of the same type were within their stated uncertainties for the summer. However, when comparing the between the two different instrument types (wet
25 chemical and BBCEAS, e.g. AIOFM-BHAM, etc), the agreement was notably worse compared to the winter (Tables 2 and 6). The exception was that the agreement between the BHAM and CAM, which was similar in the winter and summer (Tables 2 and 5), despite the CAM inlet being further away from BHAM inlet (Table 6).

Generally, the level of agreement between instruments varied between the summer and winter and this may reflect spatial
30 variability in HONO concentrations as some of the instrument inlet locations varied from summer to winter. In the summer, the CAM inlet moved closer to the AIOFM inlet and the agreement between the two BBCEAS improved to be within uncertainty (Table 6). However, we also note that the BHAM and ICCAS inlets were in the same location winter and summer

and yet the agreement between instruments changed considerably between the two measurement periods. We re-calculated the ND for two inter-comparison periods analysed in the summer (Tables 4 and 5) and found no relationship between the ND and wind direction (Figures S7 and S8, Supporting Information). This suggests that during the summer measurements the wind direction may have exerted less influence on the spatial variability of the HONO levels or that observed relationship between wind direction and ND in winter was associative not causal.

3.2.1 Performance of MANC ToF-CIMS

Measurements from the Manchester ToF-CIMS are compared to the BHAM and CAM instruments for the summer campaign as these instruments had the best data coverage for periods when the MANC instrument was measuring, as well as representing the typical upper and lower measurements (Fig S9, Supporting Information). In general the MANC instrument captured the temporal trends ($r > 0.84$) but recorded higher HONO concentrations than the other instruments (Table 7). Similar distributions were observed between the BHAM and MANC datasets, with the exception of a number of outliers for MANC (Figure 4). We note that MANC was not co-located with either BHAM or CAM instrument and while this will likely have affected the inter-comparison, the results do point to the MANC instrument capturing the temporal trends but at a higher concentration than the other instruments (157-239%, Table 7).

3.2.2 Performance of the YORK SIFT-MS

The York SIFT-MS was primarily used for measuring VOC fluxes and so did not typically measure at ground level. To enable an inter-comparison with the other techniques, the YORK instrument measured at ground level, from 1800 30/05/2017 until 0900 31/05/2017. The results are shown in Fig 5 and while the short time period and spatial distance between inlets (approx. 50m) limits the conclusions that can be drawn, it is clear that the YORK instrument captured the temporal trends (r of 0.9-0.96 compared to other techniques) and gave comparable concentrations to the BHAM instrument (slope of 0.78). Furthermore, we note that a co-located PTR-MS (PTR-TOR 1000, Ionicon) was unable to see a HONO signal despite both instruments using H_3O^+ to detect HONO.

4 Discussion

From the literature, the recent inter-comparison of ambient field measurements of HONO concentrations described by Pinto et al. (2014) is the most relevant to the current work. Overall, in their study Pinto and co-workers found that in general the level of disagreement between instruments was greater than the stated uncertainties for each instrument. While there was some evidence for a chemical interference (but Pinto and co-workers could not identify the compounds responsible definitively), there were additional factors that also appeared to affect the inter-comparison. The best agreement in Pinto et al. (2014) was found for instruments with co-located inlets compared to instruments with inlets several meters apart and so points to spatial heterogeneity in HONO concentrations (possibly due a source on the roof surface) affecting the inter-comparison. Overall, the

results from the current work are similar to that observed previously (Pinto et al. 2014), as there was a separation of up to 13 meters between some instrument inlets and this may have affected the results for the inter-comparison in the current work. With respect to photolysis, the lifetime of HONO at midday ranged from 17-300 and 9-33 min for winter and summer, respectively (depending upon weather / cloud cover / aerosol loading) and may have contributed to spatial heterogeneity in HONO concentrations. However, in the current work the results do not conclusively point to spatial heterogeneity in HONO concentrations affecting the results. As both the current work and Pinto et al. (2014) found some evidence for spatial heterogeneity in HONO concentrations affecting the intercomparison, this would suggest that to avoid this issue future studies should use a common inlet for all instruments in the field.

Duan et al. (2018) presented results of an inter-comparison at a rural site in China between a BBCEAS and a LOPAP, with good agreement observed (slope of 0.94 and r^2 0.89). The slope appeared to deviate from linearity above approximately 2 ppb suggesting that at higher concentrations the relationship was changing, as observed here between CAM and wet chemical techniques (BHAM and ICCAS) (Tables 2 and 4). A divergence in the measured concentrations at high concentrations was also observed for all instruments as part of the FIONA inter-comparison (Ródenas et al., 2013), but at much higher concentrations (>15 ppb) than most of those encountered here. However, we did not observe such a change in relationship at high and low concentrations between the AIOFM-BHAM/ICCAS, suggesting that this result was not related to instrument type. Furthermore, as the measurements from Duan et al. (2018) were performed in a rural site, conditions may also be more homogenous mix compared to an urban location and this may explain why there was better agreement between the LOPAP and BBCEAS in their study compared to the current work.

20

Throughout this work, the wet chemical techniques generally measured higher concentrations than the spectroscopic techniques, in agreement with previous studies (e.g. Stutz et al., 2010; Pinto et al., 2014). Pinto et al. (2014) suggested the possible cause may be a positive chemical interference in the wet chemical instruments. The observed dependence of the normalized difference between each instrument pair on wind direction may reflect changes in composition affecting the instrument readings. We note that the two-channel stripping coil used in the sampling inlet for both the BHAM and ICCAS instruments should account for any chemical interferences, particularly in the gas-phase (Kleffmann et al., 2002). The aerosol in Beijing is typically acidic (Song et al. 2018) and based on the effective Henry's law constant for HONO we would expect there to be little particle-phase nitrite (Kleffmann et al. 2006). This combined with the expected low uptake of particles by the LOPAP sampling inlet (in order of 1% for particles with a diameter between 50-800 nm, Broske et al. 2003) suggests that there would be limited chemical interference from particle-phase species. We also note that particle-phase chemical interference would likely be corrected for by the two-channel system.

In the current work, differences were observed between measurements from instruments of the same type (BBCEAS and wet chemical). The cause of this disagreement was difficult to pinpoint but may reflect differences in calibration and corrections applied by each group. In particular the BHAM and ICCAS instruments inlets were next to each other during the inter-

comparison (<0.5m), and thus the differences likely reflect more differences in the operating conditions of the BHAM and ICCAS instruments. Both instruments used the same nitrite standard for calibration. Notably, there is a significant difference in DL between the instruments (Table 1) likely due to the different methodologies for determining baseline correction. For example, the BHAM instrument used zero air sampled at the inlet to determine the baseline, whereas ICCAS used water introduced into the wet chemical side of the instrument. Tests have shown that water results in a lower baseline measurement for the LOPAP (approx. 80-100 ppt). We note that the ambient HONO was typically within the ppb range during the inter-comparison (Fig 1) and the effect of this baseline difference would be negligible at these levels. But at lower concentrations (low ppt), it would proportionally have a greater influence on the reported HONO levels by the BHAM and ICCAS instruments. High ND was observed at low concentration (<1ppb, Fig 3) and the difference in absolute baseline correction may explain this.

The scaling factor to correct for the discrepancy in flow rate applied to the CAM instrument after the campaigns is unlikely to be the cause of the disagreement between the two BBCEAS. The two BBCEAS systems agree to within $\pm 10\%$ for NO_2 measurements, and the larger disagreement for HONO (13%, Table 2) likely reflects higher spatial variability of ambient HONO compared to NO_2 , as the CAM and AIOFM inlets were the furthest apart during the formal winter inter-comparison. The agreement between the two BBCEAS decreased at lower concentrations and this may reflect differences in DL (Table 1). The two BBCEAS instruments were found to be in better agreement in the summer compared to the winter. This may reflect the inlets being closer in summer compared to the winter, however there was still a distance of 3m between inlets. We do not know the reasons why the agreement between the AIOFM and CAM instruments changed in the summer compared to winter. Whilst there were some variability in path length and purge flows between the two BBCEAS systems, these are not thought to account for the discrepancy as they did not vary winter to summer. Furthermore, another factor may be losses/production of HONO and NO_2 on the inlet filter and/or tubing losses/production that may also influence the intercomparison results as these were naturally different across systems due to different residence times (~ 3 s and ~ 0.5 s for the CAM and AIOFM BBCEAS, respectively). Laboratory tests using the same tubing material (Teflon) have however shown that neither the production nor the loss of HONO were significant in the CAM instrument (to less than a few percent) even at considerably longer inlet and cavity residence times, suggesting this was insignificant.

Generally, the agreement between instrument pairs varied from winter to summer, with the exception of CAM and BHAM instruments. As all instruments were operated and calibrated according to the same procedures in winter and summer, there were no changes in instrument operation that can explain these changes and as such, the cause is unclear. The concentrations observed during summer (mean of 1.2 ± 0.9 ppb (1σ)) were typically lower compared to the winter (mean of 2.35 ± 1.9 ppb (1σ)), and this may have affected the results.

5 Conclusions

Overall, from the winter inter-comparison all instruments were found to agree on the temporal trends and variability in HONO ($r > 0.97$) yet displayed some divergence in absolute concentrations (slopes of 0.61-0.88), with the wet chemical methods consistently somewhat higher than the BBCEAS systems. We found no evidence for any systematic bias in any of the instruments, with the exception of measurements near instrument detection limits. There was evidence that the relationship between some instruments varied for the different measurement periods (e.g. winter/summer) however the reason for this change was unclear. When considering the mass spectrometric methods (MANC ToF-CIMS and YORK SIFT-MS), these captured the temporal trends in HONO concentrations but were found to differ in absolute concentration relative to the other instrumentation.

10

There was no evidence for a definitive cause of systematic bias between the four instruments during the formal HONO inter-comparison, which might justify scaling or excluding results from one or more instruments. As a result, we could not say with confidence, which instrument (if any) provided the ‘correct’ measurement of HONO concentration. Therefore, to meet the needs of the wider APHH-Beijing program for a single ground level HONO measurement, a merged HONO dataset was produced using the mean and range concentration of the four instruments that participated in the formal winter inter-comparison (two wet chemical and two BBCEAS). This merged dataset will be used for future ground level analyses (e.g. model evaluation) across the APHH-Beijing program.

15

Authors contributions

Study conceived by BO and LC. Measurements were performed by LC, LK, BO, JD, WZ, MS, AM, TB, SW, JA and AB. Formal analysis performed by LC, LK and BO. All co-authors contributed to data curation. LC prepared the manuscript with contributions from all co-authors.

20

Competing Interests

The authors declare that they have no conflict of interest.

25 Acknowledgements

This work was funded by the UK Natural Environment Research Council (NERC), Medical Research Council and Natural Science Foundation of China under the framework of Newton Innovation Fund (NE/N007190/1 and NE/N007077/1). WJB, LJK and LRC acknowledge additional support by the UK NERC through the project Sources of Nitrous Acid in the Atmospheric Boundary Layer (SNAABL, NE/M013405/1). We acknowledge the support from Pingqing Fu, Zifa Wang, Jie Li and Yele Sun from IAP for hosting the APHH-Beijing campaign at IAP. We thank Zongbo Shi, Di Liu, Roy Harrison and

30

Tuan Vu from the University of Birmingham, Siyao Yue, Liangfang Wei, Hong Ren, Qiaorong Xie, Wanyu Zhao, Linjie Li, Ping Li, Shengjie Hou, Qingqing Wang from IAP, Rachel Dunmore, Ally Lewis and James Lee from the University of York, Kebin He and Xiaoting Cheng from Tsinghua University, and James Allan and Hugh Coe from the University of Manchester for providing logistic and scientific support for the field campaigns.

5

Data Availability

Original data are available on request from the authors and have been deposited in the (open access) CEDA repository, available for public download following the project embargo period.

References

- 10 Acker, K., Spindler, G., and Brüggemann, E.: Nitrous and nitric acid measurements during the INTERCOMP2000 campaign in Melpitz, *Atmospheric Environment*, 38, 6497-6505, <https://doi.org/10.1016/j.atmosenv.2004.08.030>, 2004.
- Acker K, Möller D, Wieprecht W, Meixner FX, Bohn B, Gilge S, Plass-Dülmer C, Berresheim H. Strong daytime production of OH from HNO₂ at a rural mountain site. *Geophysical Research Letters*. 33, L02809, doi:[10.1029/2005GL024643](https://doi.org/10.1029/2005GL024643), 2006.
- Appel, B., Winer, A., Tokiwa, Y., and Biermann, H. J. A. E. P. A. G. T.: Comparison of atmospheric nitrous acid measurements by annular denuder and differential optical absorption systems, 24, 611-616, 1990.
- 15 Arnold, J. R., Hartsell, B. E., Luke, W. T., Rahmat Ullah, S. M., Dasgupta, P. K., Greg Huey, L., and Tate, P.: Field test of four methods for gas-phase ambient nitric acid, *Atmospheric Environment*, 41, 4210-4226, <https://doi.org/10.1016/j.atmosenv.2006.07.058>, 2007.
- Bannan, T. J., Bacak, A., Muller, J. B. A., Booth, A. M., Jones, B., Le Breton, M., Leather, K. E., Ghalaieny, M., Xiao, P., Shallcross, D. E., and Percival, C. J.: Importance of direct anthropogenic emissions of formic acid measured by a chemical ionisation mass spectrometer (CIMS) during the Winter ClearfLo Campaign in London, January 2012, *Atmospheric Environment*, 83, 301-310, <https://doi.org/10.1016/j.atmosenv.2013.10.029>, 2014.
- 20 Bannan, T. J., Booth, A. M., Bacak, A., Muller, J. B. A., Leather, K. E., Le Breton, M., Jones, B., Young, D., Coe, H., Allan, J., Visser, S., Slowik, J. G., Furger, M., Prévôt, A. S. H., Lee, J., Dunmore, R. E., Hopkins, J. R., Hamilton, J. F., Lewis, A. C., Whalley, L. K., Sharp, T., Stone, D., Heard, D. E., Fleming, Z. L., Leigh, R., Shallcross, D. E., and Percival, C. J.: The first UK measurements of nitryl chloride using a chemical ionization mass spectrometer in central London in the summer of 2012, and an investigation of the role of Cl atom oxidation, 120, 5638-5657, doi:[10.1002/2014JD022629](https://doi.org/10.1002/2014JD022629), 2015.
- Bannan, T. J., Le Breton, M., Priestley, M., Worrall, S. D., Bacak, A., Marsden, N. A., Mehra, A., Hammes, J., Hallquist, M., Alfarra, M. R., Krieger, U. K., Reid, J. P., Jayne, J., Robinson, W., McFiggans, G., Coe, H., Percival, C. J., and Topping, D.: A method for extracting calibrated volatility information from the FIGAERO-HR-ToF-CIMS and its experimental application, *Atmos. Meas. Tech.*, 12, 1429-1439, [10.5194/amt-12-1429-2019](https://doi.org/10.5194/amt-12-1429-2019), 2019.
- 30

- Breton ML, Wang Y, Hallquist ÅM, Pathak RK, Zheng J, Yang Y, Shang D, Glasius M, Bannan TJ, Liu Q, Chan CK. Online gas-and particle-phase measurements of organosulfates, organosulfonates and nitrooxy organosulfates in Beijing utilizing a FIGAERO ToF-CIMS. *Atmospheric Chemistry and Physics*. 18, 10355-71, 2018.
- Bröske R, Kleffmann J, Wiesen P. Heterogeneous conversion of NO₂ on secondary organic aerosol surfaces: A possible source of nitrous acid (HONO) in the atmosphere? *Atmos. Chem. and Phys.* 3, 469-74, 2003.
- 5 Carslaw, D. C., and Ropkins, K.: openair — An R package for air quality data analysis, *Environmental Modelling & Software*, 27–28, 52-61, <http://dx.doi.org/10.1016/j.envsoft.2011.09.008>, 2012.
- Cheng, P., Cheng, Y., Lu, K., Su, H., Yang, Q., Zou, Y., Zhao, Y., Dong, H., Zeng, L., and Zhang, Y.: An online monitoring system for atmospheric nitrous acid (HONO) based on stripping coil and ion chromatography, *Journal of Environmental*
10 *Sciences*, 25, 895-907, [https://doi.org/10.1016/S1001-0742\(12\)60251-4](https://doi.org/10.1016/S1001-0742(12)60251-4), 2013.
- Crilley, L. R., Kramer, L., Pope, F. D., Whalley, L. K., Cryer, D. R., Heard, D. E., Lee, J. D., Reed, C., and Bloss, W. J.: On the interpretation of in situ HONO observations via photochemical steady state, *Faraday Discussions*, 189, 191-212, 10.1039/C5FD00224A, 2016.
- Duan, J., Qin, M., Ouyang, B., Fang, W., Li, X., Lu, K., Tang, K., Liang, S., Meng, F., Hu, Z., Xie, P., Liu, W., and Häsler,
15 R.: Development of an incoherent broadband cavity-enhanced absorption spectrometer for in situ measurements of HONO and NO₂, *Atmos. Meas. Tech.*, 11, 4531-4543, 10.5194/amt-11-4531-2018, 2018.
- Febo, A., Perrino, C., Gherardi, M., Sparapani, R. J. E. s., and technology: Evaluation of a high-purity and high-stability continuous generation system for nitrous acid, 29, 2390-2395, 1995.
- Febo, A., Perrino, C., and Allegrini, I. J. A. E.: Measurement of nitrous acid in Milan, Italy, by DOAS and diffusion denuders,
20 30, 3599-3609, 1996.
- Heland, J., Kleffmann, J., Kurtenbach, R., and Wiesen, P.: A New Instrument To Measure Gaseous Nitrous Acid (HONO) in the Atmosphere, *Environmental Science & Technology*, 35, 3207-3212, 10.1021/es000303t, 2001.
- Hera, D., Langford, V. S., McEwan, M. J., McKellar, T. I., and Milligan, D. B.: Negative Reagent Ions for Real Time Detection Using SIFT-MS, *Environments*, 4, 16, 2018.
- 25 Hou, S. Q., Tong, S. R., Ge, M. F., and An, J. L.: Comparison of atmospheric nitrous acid during severe haze and clean periods in Beijing, China, *Atmos Environ*, 124, 199-206, 10.1016/j.atmosenv.2015.06.023, 2016.
- Kennedy, O. J., Ouyang, B., Langridge, J. M., Daniels, M. J. S., Bauguitte, S., Freshwater, R., McLeod, M. W., Ironmonger, C., Sendall, J., Norris, O., Nightingale, R., Ball, S. M., and Jones, R. L.: An aircraft based three channel broadband cavity enhanced absorption spectrometer for simultaneous measurements of NO₃, N₂O₅ and
30 NO₂, *Atmos. Meas. Tech.*, 4, 1759-1776, 10.5194/amt-4-1759-2011, 2011.
- Kim M, Or D. Microscale pH variations during drying of soils and desert biocrusts affect HONO and NH₃ emissions. *Nature communications*. 10, 1-2, 2019.
- Kleffmann, J., Heland, J., Kurtenbach, R., Lorzer, J., and Wiesen, P.: A new instrument (LOPAP) for the detection of nitrous acid (HONO), *Environ Sci Pollut Res*, 48-54, 2002.

- Kleffmann J, Gavriloaiei T, Hofzumahaus A, Holland F, Koppmann R, Rupp L, Schlosser E, Siese M, Wahner A. Daytime formation of nitrous acid: A major source of OH radicals in a forest. *Geophysical Research Letters*. 32, L05818, doi:[10.1029/2005GL022524](https://doi.org/10.1029/2005GL022524), 2005.
- 5 Kleffmann, J., Lörzer, J., Wiesen, P., Kern, C., Trick, S., Volkamer, R., Rodenas, M., and Wirtz, K. J. A. E.: Intercomparison of the DOAS and LOPAP techniques for the detection of nitrous acid (HONO), 40, 3640-3652, 2006.
- Kleffmann, J.: Daytime Sources of Nitrous Acid (HONO) in the Atmospheric Boundary Layer, *ChemPhysChem*, 8, 1137-1144, [10.1002/cphc.200700016](https://doi.org/10.1002/cphc.200700016), 2007.
- Kleffmann, J., Wiesen, P. J. A. C., and Physics: Quantification of interferences of wet chemical HONO LOPAP measurements under simulated polar conditions, 8, 6813-6822, 2008.
- 10 Lammel G, Cape J. Nitrous acid and nitrite in the atmosphere. *Chemical Society Reviews*. 25, 361-9, 1996.
- Le Breton, M., Bacak, A., Muller, J. B., Bannan, T. J., Kennedy, O., Ouyang, B., Xiao, P., Bauguitte, S. J.-B., Shallcross, D. E., and Jones, R. L. J. A. M.: The first airborne comparison of N₂O₅ measurements over the UK using a CIMS and BBCEAS during the RONOCO campaign, 6, 9731-9743, 2014.
- Le Breton, M., Bannan, T. J., Shallcross, D. E., Khan, M. A., Evans, M. J., Lee, J., Lidster, R., Andrews, S., Carpenter, L. J., Schmidt, J., Jacob, D., Harris, N. R. P., Bauguitte, S., Gallagher, M., Bacak, A., Leather, K. E., and Percival, C. J.: Enhanced ozone loss by active inorganic bromine chemistry in the tropical troposphere, *Atmospheric Environment*, 155, 21-28, <https://doi.org/10.1016/j.atmosenv.2017.02.003>, 2017.
- 15 Lee, B. H., Wood, E. C., Herndon, S. C., Lefer, B. L., Luke, W. T., Brune, W. H., Nelson, D. D., Zahniser, M. S., and Munger, J. W.: Urban measurements of atmospheric nitrous acid: A caveat on the interpretation of the HONO photostationary state, 20 *Journal of Geophysical Research: Atmospheres*, 118, 2013JD020341, [10.1002/2013jd020341](https://doi.org/10.1002/2013jd020341), 2013.
- Lee, J., Whalley, L., Heard, D., Stone, D., Dunmore, R., Hamilton, J., Young, D., Allan, J., Laufs, S., Kleffmann, J. J. A. C., and Physics: Detailed budget analysis of HONO in central London reveals a missing daytime source, 16, 2747-2764, 2016.
- Lopez-Hilfiker, F. D., Mohr, C., Ehn, M., Rubach, F., Kleist, E., Wildt, J., Mentel, T. F., Lutz, A., Hallquist, M., Worsnop, D., and Thornton, J. A.: A novel method for online analysis of gas and particle composition: description and evaluation of a 25 *Filter Inlet for Gases and AEROsols (FIGAERO)*, *Atmos. Meas. Tech.*, 7, 983-1001, [10.5194/amt-7-983-2014](https://doi.org/10.5194/amt-7-983-2014), 2014.
- Michoud, V., Colomb, A., Borbon, A., Miet, K., Beekmann, M., Camredon, M., Aumont, B., Perrier, S., Zapf, P., Siour, G., Ait-Helal, W., Afif, C., Kukui, A., Furger, M., Dupont, J. C., Haefelin, M., and Doussin, J. F.: Study of the unknown HONO daytime source at a European suburban site during the MEGAPOLI summer and winter field campaigns, *Atmos. Chem. Phys.*, 14, 2805-2822, [10.5194/acp-14-2805-2014](https://doi.org/10.5194/acp-14-2805-2014), 2014.
- 30 Perner, D., and Platt, U.: Detection of nitrous acid in the atmosphere by differential optical absorption, 6, 917-920, doi:[10.1029/GL006i012p00917](https://doi.org/10.1029/GL006i012p00917), 1979.
- Pinto, J. P., Dibb, J., Lee, B. H., Rappenglück, B., Wood, E. C., Levy, M., Zhang, R.-Y., Lefer, B., Ren, X.-R., Stutz, J., Tsai, C., Ackermann, L., Golovko, J., Herndon, S. C., Oakes, M., Meng, Q.-Y., Munger, J. W., Zahniser, M., and Zheng, J.: Intercomparison of field measurements of nitrous acid (HONO) during the SHARP campaign, 119, 5583-5601, 35 doi:[10.1002/2013JD020287](https://doi.org/10.1002/2013JD020287), 2014.

- Ren, X., Gao, H., Zhou, X., Crouse, J., Wennberg, P., Browne, E., LaFranchi, B., Cohen, R., McKay, M., Goldstein, A. J. A. C., and Physics: Measurement of atmospheric nitrous acid at Bodgett Forest during BEARPEX2007, 10, 6283-6294, 2010.
- Ródenas, M., Muñoz, A., Alacreu, F., Brauers, T., Dorn, H.-P., Kleffmann, J., and Bloss, W.: Assessment of HONO measurements: The FIONA campaign at EUPHORE, in: Disposal of Dangerous Chemicals in Urban Areas and Mega Cities, 5 Springer, 45-58, 2013.
- Spanel, P. Smith, D. An investigation of the reaction of H_3O^+ and O_2^+ with NO , NO_2 , N_2O and HNO_2 in support of selected ion flow tube mass spectrometry. *Rapid Comms in Mass Spectrometry*, 14, 8, 2000
- Shi, Z., Vu, T., Kotthaus, S., Grimmond, S., Harrison, R. M., Yue, S., Zhu, T., Lee, J., Han, Y., Demuzere, M., Dunmore, R. E., Ren, L., Liu, D., Wang, Y., Wild, O., Allan, J., Barlow, J., Beddows, D., Bloss, W. J., Carruthers, D., Carslaw, D. C., 10 Chatzidiakou, L., Crilley, L., Coe, H., Dai, T., Doherty, R., Duan, F., Fu, P., Ge, B., Ge, M., Guan, D., Hamilton, J. F., He, K., Heal, M., Heard, D., Hewitt, C. N., Hu, M., Ji, D., Jiang, X., Jones, R., Kalberer, M., Kelly, F. J., Kramer, L., Langford, B., Lin, C., Lewis, A. C., Li, J., Li, W., Liu, H., Loh, M., Lu, K., Mann, G., McFiggans, G., Miller, M., Mills, G., Monk, P., Nemitz, E., O'Connor, F., Ouyang, B., Palmer, P. I., Percival, C., Popoola, O., Reeves, C., Rickard, A. R., Shao, L., Shi, G., Spracklen, D., Stevenson, D., Sun, Y., Sun, Z., Tao, S., Tong, S., Wang, Q., Wang, W., Wang, X., Wang, Z., Whalley, L., Wu, 15 X., Wu, Z., Xie, P., Yang, F., Zhang, Q., Zhang, Y., Zhang, Y., and Zheng, M.: Introduction to Special Issue – In-depth study of air pollution sources and processes within Beijing and its surrounding region (APHH-Beijing), *Atmos. Chem. Phys. Discuss.*, 2018, 1-62, 10.5194/acp-2018-922, 2018.
- Sousan, S., Koehler, K., Thomas, G., Park, J. H., Hillman, M., Halterman, A., and Peters, T. M.: Inter-comparison of low-cost sensors for measuring the mass concentration of occupational aerosols, *Aerosol Science and Technology*, 50, 462-473, 20 10.1080/02786826.2016.1162901, 2016.
- Spataro, F., and Ianniello, A.: Sources of atmospheric nitrous acid: State of the science, current research needs, and future prospects, *Journal of the Air & Waste Management Association*, 64, 1232-1250, 10.1080/10962247.2014.952846, 2014.
- Spindler, G., Hesper, J., Brüggemann, E., Dubois, R., Müller, T., and Herrmann, H. J. A. E.: Wet annular denuder measurements of nitrous acid: laboratory study of the artefact reaction of NO_2 with $\text{S}(\text{IV})$ in aqueous solution and comparison 25 with field measurements, 37, 2643-2662, 2003.
- Stutz, J., Kim, E. S., Platt, U., Bruno, P., Perrino, C., and Febo, A.: UV-visible absorption cross sections of nitrous acid, 105, 14585-14592, 10.1029/2000jd900003, 2000.
- Stutz, J., Oh, H.-J., Whitlow, S. I., Anderson, C., Dibb, J. E., Flynn, J. H., Rappenglück, B., and Lefer, B.: Simultaneous DOAS and mist-chamber IC measurements of HONO in Houston, TX, *Atmospheric Environment*, 44, 4090-4098, 30 <https://doi.org/10.1016/j.atmosenv.2009.02.003>, 2010.
- Song S, Gao M, Xu W, Shao J, Shi G, Wang S, Wang Y, Sun Y, McElroy MB. Fine-particle pH for Beijing winter haze as inferred from different thermodynamic equilibrium models. *Atmospheric Chemistry and Physics*. 10:7423-38, 2018.

- Taipale, R., Ruuskanen, T. M., Rinne, J., Kajos, M. K., Hakola, H., Pohja, T., and Kulmala, M.: Technical Note: Quantitative long-term measurements of VOC concentrations by PTR-MS; measurement, calibration, and volume mixing ratio calculation methods, *Atmos. Chem. Phys.*, 8, 6681-6698, 10.5194/acp-8-6681-2008, 2008.
- Tong, S., Hou, S., Zhang, Y., Chu, B., Liu, Y., He, H., ... & Ge, M. Exploring the nitrous acid (HONO) formation mechanism in winter Beijing: direct emissions and heterogeneous production in urban and suburban areas. *Faraday discussions*, 189, 213-230, 2016.
- Yang Q, Su H, Li X, Cheng Y, Lu K, Cheng P, Gu J, Guo S, Hu M, Zeng L, Zhu T. Daytime HONO formation in the suburban area of the megacity Beijing, China. *Science China Chemistry*. 57(7):1032-42. 2014.
- Veitel, H.: Vertical profiles of NO₂ and HONO in the planetary boundary layer, 2002.
- 10 Veres, P. R., Roberts, J. M., Wild, R. J., Edwards, P. M., Brown, S. S., Bates, T. S., Quinn, P. K., Johnson, J. E., Zamora, R. J., and de Gouw, J.: Peroxynitric acid (HO₂NO₂) measurements during the UBWOS 2013 and 2014 studies using iodide ion chemical ionization mass spectrometry, *Atmos. Chem. Phys.*, 15, 8101-8114, 10.5194/acp-15-8101-2015, 2015.
- Voigt, S., Orphal, J., and Burrows, J. P.: The temperature and pressure dependence of the absorption cross-sections of NO₂ in the 250–800 nm region measured by Fourier-transform spectroscopy, *Journal of Photochemistry and Photobiology A: Chemistry*, 149, 1-7, [https://doi.org/10.1016/S1010-6030\(01\)00650-5](https://doi.org/10.1016/S1010-6030(01)00650-5), 2002.
- Wang, J., Zhang, X., Guo, J., Wang, Z., and Zhang, M.: Observation of nitrous acid (HONO) in Beijing, China: Seasonal variation, nocturnal formation and daytime budget, *Science of The Total Environment*, 587-588, 350-359, <https://doi.org/10.1016/j.scitotenv.2017.02.159>, 2017.
- 20 Weber B, Wu D, Tamm A, Ruckteschler N, Rodriguez-Caballero E, Steinkamp J, Meusel H, Elbert W, Behrendt T, Soergel M, Cheng Y. Biological soil crusts accelerate the nitrogen cycle through large NO and HONO emissions in drylands. *Proceedings of the National Academy of Sciences*. 112, 15384-9, 2015.
- Zhou, W., Zhao, J., Ouyang, B., Mehra, A., Xu, W., Wang, Y., Bannan, T. J., Worrall, S. D., Priestley, M., Bacak, A. J. A. C., and Physics: Production of N₂O₅ and ClNO₂ in summer in urban Beijing, China, 18, 11581-11597, 2018.
- 25 Zhou X, He Y, Huang G, Thornberry TD, Carroll MA, Bertman SB. Photochemical production of nitrous acid on glass sample manifold surface. *Geophysical Research Letters*. 29, 26-1, 2002.

Table 1: Instrumentation measuring HONO at IAP.

Institution	Instrument	Manufacturer	DL (ppt)	Error	Time resolution	Reference
Birmingham (BHAM)	Wet Chemical (LOPAP.03)	QUMA	Winter: 35 Summer: 5 (2 σ , 30s)	10%	5 min	(Heland et al., 2001)
ICCAS	Wet Chemical	Custom built	134 (2 σ , 30s)	10%	5 min	(Hou et al. 2016)
Cambridge (CAM)	BBCEAS	Custom built	25 (1 σ , 60s)	9%	5 s	(Kennedy et al., 2011)
AIOFM	BBCEAS	Custom built	120 (2 σ , 60s)	9%	1 min	(Duan et al. 2018)
Manchester (MANC)	ToF-CIMS	Aerodyne Research Inc / Tofwerk.	33 (2 σ , 60s)	19 %	1 Hz	(Priestley et al., 2018)
York	SIFT-MS Voice ultra 200	Syft Technologies	130 (2 σ , 60s)	22%	19 secs (1min averaged)	(Hera et al., 2018)

Table 2: Results of the reduced major axis regression analysis with 95% confidence intervals during the formal winter inter-comparison. Variability shown is the 95% confidence interval of the slope and intercepts.

INSTRUMENTS	INTERCEPT	SLOPE	R	N
BHAM-ICCAS	0.09±0.04	0.77±0.01	0.97	865
BHAM-AIOFM	-0.18±0.03	0.71±0.01	0.98	1070
BHAM-CAM	-0.23±0.03	0.61±0.01	0.98	1125
ICCAS-AIOFM	-0.20±0.03	0.88±0.01	0.98	954
ICCAS-CAM	-0.38±0.04	0.82±0.01	0.97	991
AIOFM-CAM	-0.09±0.03	0.87±0.01	0.96	1206

Table 3: Calculated CD values for each instrument pair during the winter inter-comparison.

	ICCAS	AIOFM	CAM
BHAM	0.11	0.22	0.32
ICCAS	-	0.12	0.21
AIOFM	-	-	0.11

Table 4: RMA regression analysis (with 95% confidence intervals) for times when the abundance of HONO was less than 2 ppb as measured by CAM during the formal winter intercomparison period. Variability shown is the 95% confidence interval of the slope and intercepts.

INSTRUMENTS	INTERCEPT	SLOPE	R	N
BHAM-ICCAS	-0.01±0.06	0.82±0.02	0.96	437
BHAM-AIOFM	-0.25±0.03	0.76±0.01	0.98	529
BHAM-CAM	-0.06±0.03	0.53±0.01	0.95	613
ICCAS-AIOFM	-0.23±0.05	0.91±0.03	0.95	478
ICCAS-CAM	-0.12±0.05	0.68±0.02	0.91	556
AIOFM-CAM	0.07±0.03	0.72±0.02	0.92	655

Table 5: RMA regression relationships of HONO measured by BHAM-ICCAS-CAM during the co-located measurements at the start of the summer campaign (22nd May-30th May 2017). All three inlet locations were the same as the formal winter intercomparison. Variability shown is the 95% confidence interval of the slope and intercepts.

INSTRUMENTS	INTERCEPT	SLOPE	R	N
BHAM-ICCAS	-0.24±0.02	0.91±0.01	0.97	2061
BHAM-CAM	-0.34±0.02	0.61±0.01	0.90	1233
ICCAS-CAM	0.21±0.02	0.69±0.01	0.85	1346

5

Table 6: RMA regression relationships (with 95% confidence intervals) of HONO measured by all instruments in the middle of the summer campaign (7th-14th June 2017). Note that BHAM and ICCAS inlets were in same location for this period. The CAM instrument had moved to the same container as AIOFM, whose inlets were 3 meters apart. Variability shown is the 95% confidence interval of the slope and intercepts.

INSTRUMENTS	INTERCEPT	SLOPE	R	N
BHAM-ICCAS	0.17±0.04	0.93±0.03	0.90	900
BHAM-AIOFM	-0.18±0.03	0.61±0.02	0.81	1377
BHAM-CAM	0.02±0.03	0.65±0.02	0.86	1395
ICCAS-AIOFM	-0.08±0.02	0.43±0.01	0.81	1153
ICCAS-CAM	0.07±0.03	0.53±0.02	0.82	1167
AIOFM-CAM	0.20±0.01	1.07±0.02	0.92	1982

5

Table 7: RMA regression relationships of HONO measured by BHAM-CAMB-MANC for the whole summer period. Variability shown is the 95% confidence interval of the slope and intercepts.

INSTRUMENTS	INTERCEPT	SLOPE	R	N
BHAM-MANC	-0.35±0.06	1.57±0.04	0.84	1896
BHAM-CAM	0.00±0.02	0.63±0.01	0.84	4106
CAM-MANC	-0.30±0.05	2.39±0.05	0.88	2372

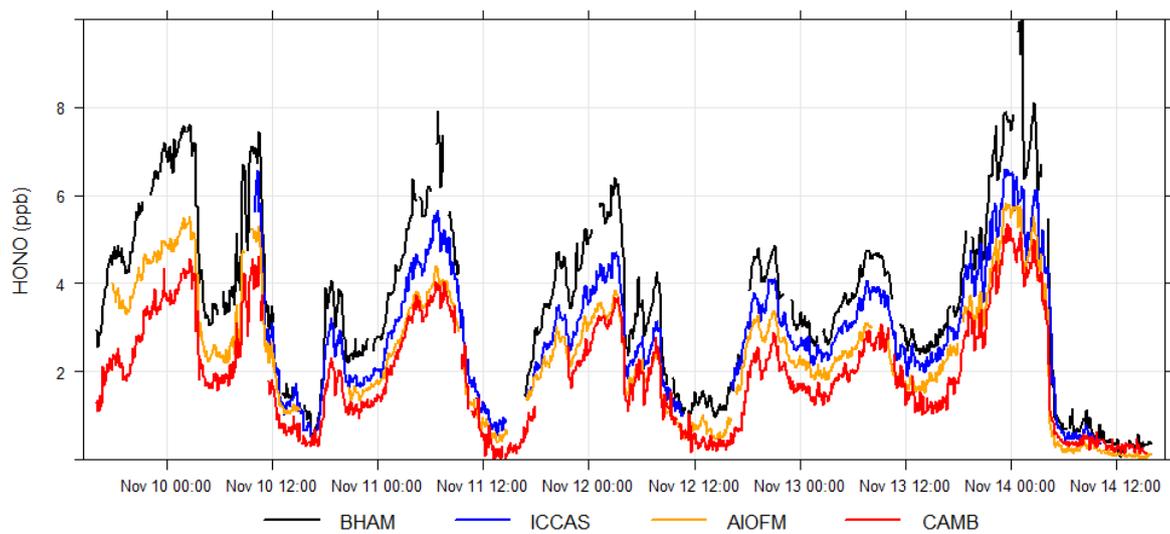


Figure 1: Time series of the measured mixing ratios during the formal winter inter-comparison for each instrument


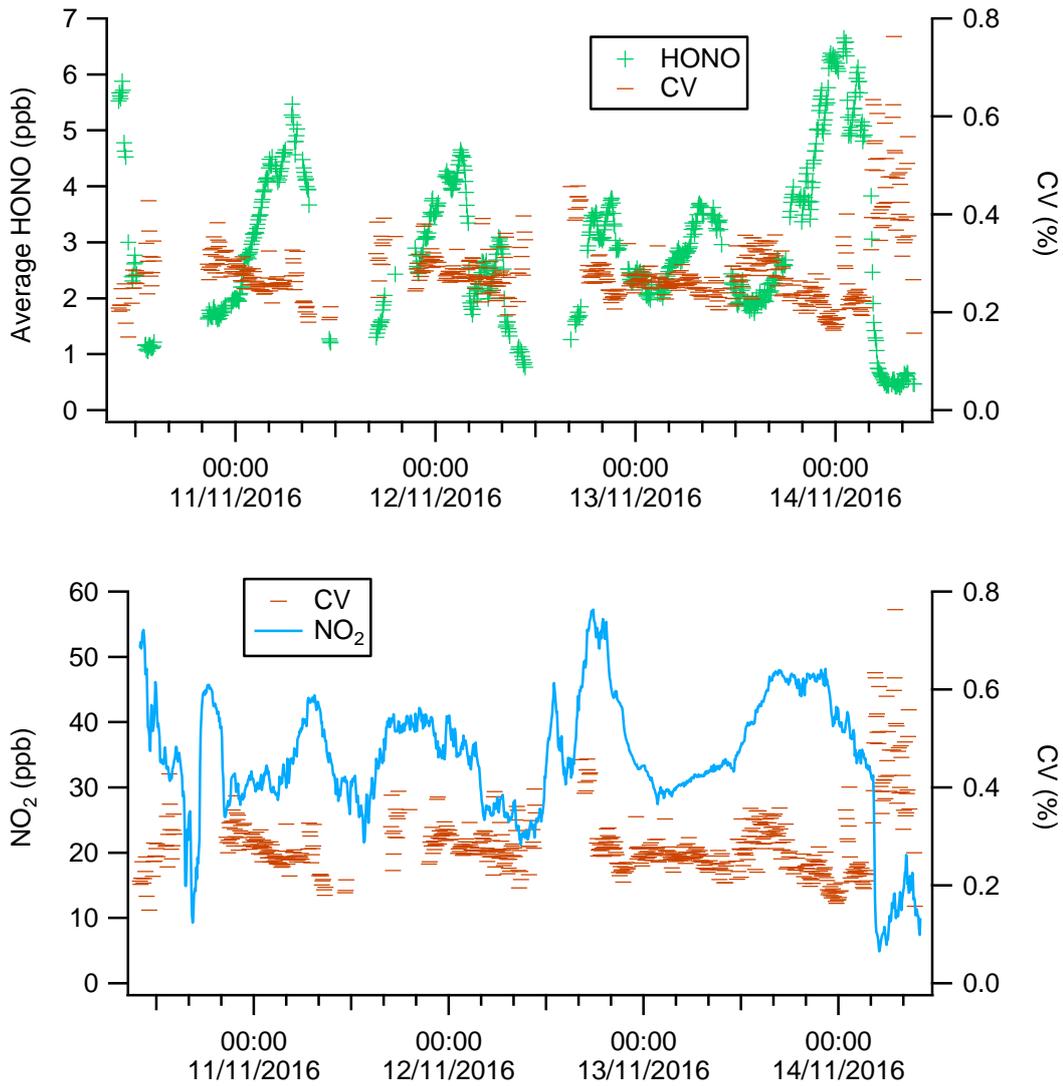


Figure 2: Time series of the co-efficient of variance (CV), mean mixing ratio of HONO (top) and NO₂ (bottom) during the winter inter-comparison. Note only when all four instruments were measuring were the mean HONO and CV calculated.

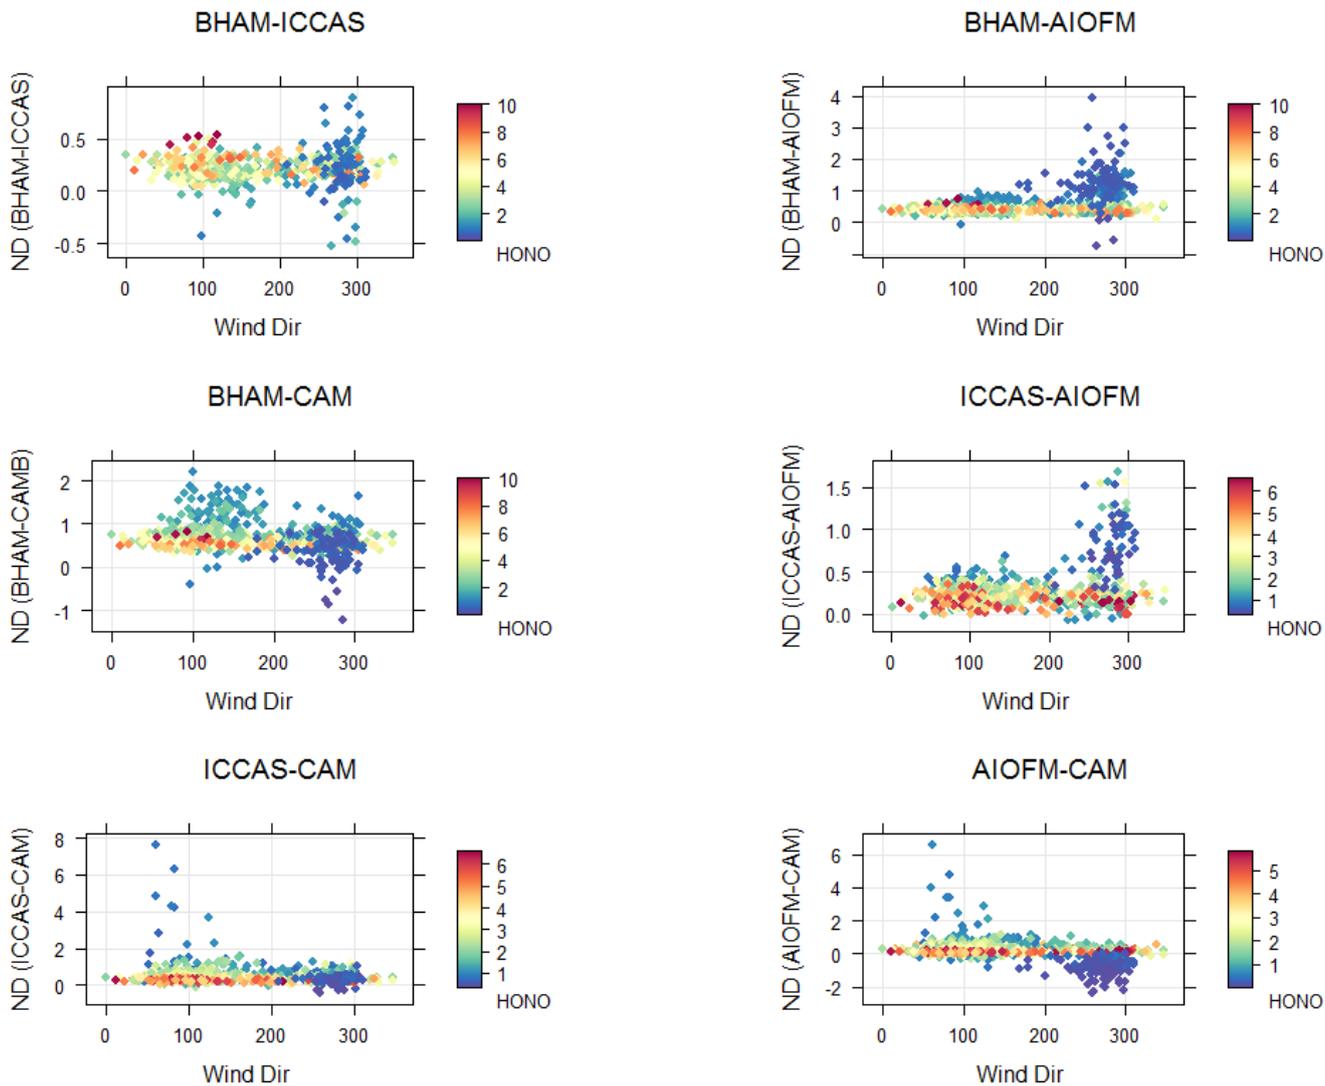

5 **Figure 3: Normalised Differences (ND) for each instrument pair as a function of wind direction coloured by measured HONO concentration for the winter intercomparison. Note the different scales for the y-axes and HONO abundance colour key.**

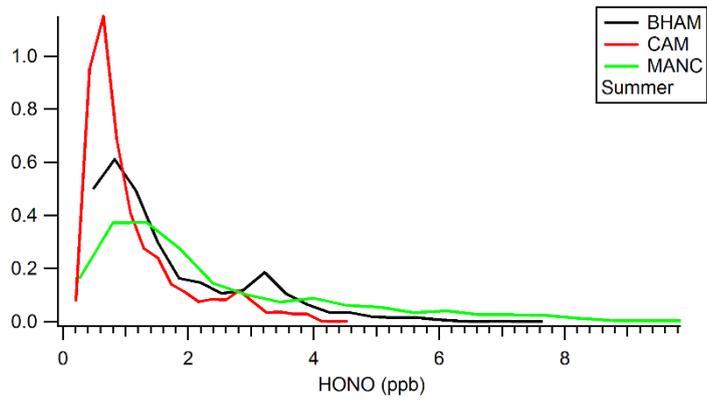


Figure 4: Histogram of measured summer concentrations (only for periods when all three instruments were measuring).

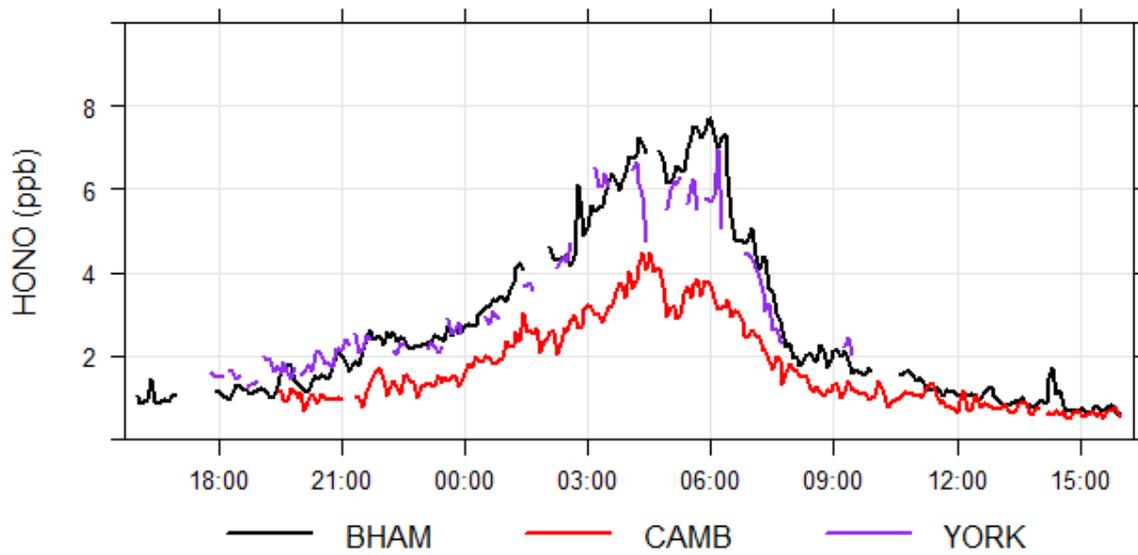


Figure 5: Time series for the period when the YORK instrument measured at ground level during the summer campaign.