

N₂O isotopocule measurements using laser spectroscopy: analyzer characterization and intercomparison

Stephen J. Harris^{1,2,*}, Jesper Liisberg^{3,*}, Longlong Xia⁴, Jing Wei⁵, Kerstin Zeyer⁵, Longfei Yu⁵, Matti Barthel⁶, Benjamin Wolf⁴, Bryce F.J. Kelly¹, Dioni I. Cendón², Thomas Blunier³, Johan Six⁶, Joachim Mohn⁵

¹School of Biological, Earth and Environmental Sciences, UNSW Sydney, NSW, Australia

²Australian Nuclear Science and Technology Organisation, Lucas Heights, NSW, Australia

10 ³University of Copenhagen, Niels Bohr Institute, Copenhagen, Denmark

⁴Karlsruhe Institute of Technology, IMK-IFU, Garmisch-Partenkirchen, Germany

⁵Empa, Laboratory for Air Pollution/Environmental Technology, Dübendorf, Switzerland

⁶ETH Zürich, Department of Environmental Systems Science, Zürich, Switzerland

Correspondence to: Joachim Mohn (email: joachim.mohn@empa.ch)

15 * These authors contributed equally to this work

Abstract. For the past two decades, the measurement of N₂O isotopocules – isotopically substituted molecules ¹⁴N¹⁵N¹⁶O, ¹⁵N¹⁴N¹⁶O and ¹⁴N¹⁴N¹⁸O of the main isotopic species ¹⁴N¹⁴N¹⁶O – has been a promising technique for understanding N₂O production and consumption pathways. The coupling of non-cryogenic and tuneable light sources with different detection schemes, such as direct absorption quantum cascade laser absorption spectroscopy (QCLAS), cavity ring-down spectroscopy (CRDS) and off-axis integrated cavity output spectroscopy (OA-ICOS), has enabled the production of commercially-available and field-deployable N₂O isotopic analyzers. In contrast to traditional isotope-ratio mass-spectrometry (IRMS), these instruments are inherently selective for position-specific ¹⁵N substitution and provide real-time data, with minimal or no sample pretreatment, which is highly attractive for process studies.

25

Here, we compared the performance of N₂O isotope laser spectrometers with the three most common detection schemes: OA-ICOS (N₂OIA-30e-EP, ABB-Los Gatos Research Inc.), CRDS (G5131-i, Picarro Inc.) and QCLAS (dual QCLAS and preconcentration (TREX)–mini QCLAS, Aerodyne Research Inc.). For each instrument, the precision, drift and repeatability of N₂O mole fraction [N₂O] and isotope data were tested. The analyzers were then characterized for their dependence on [N₂O], gas matrix composition (O₂, Ar) and spectral interferences caused by H₂O, CO₂, CH₄ and CO to develop analyzer-specific correction functions. Subsequently, a simulated two end-member mixing experiment was used to compare the accuracy and repeatability of corrected and calibrated isotope measurements that could be acquired using the different laser spectrometers.

35

Our results show that N₂O isotope laser spectrometer performance is governed by an interplay between instrumental precision, drift, matrix effects and spectral interferences. To retrieve compatible and accurate results, it is necessary to include appropriate reference materials following the identical treatment (IT)

principle during every measurement. Remaining differences between sample and reference gas compositions have to be corrected by applying analyzer-specific correction algorithms. These matrix and trace gas correction equations vary considerably according to N₂O mole fraction, complicating the procedure further. Thus, researchers should strive to minimize differences in composition between sample and reference gases. In closing, we provide a calibration workflow to guide researchers in the operation of N₂O isotope laser spectrometers in order to acquire accurate N₂O isotope analyses. We anticipate that this workflow will assist in applications where matrix and trace gas compositions vary considerably (e.g. laboratory incubations, N₂O liberated from wastewater or groundwater), as well as extending to future analyzer models and instruments focusing on isotopic species of other molecules.

10 1 Introduction

Nitrous oxide (N₂O) is a long-lived greenhouse gas with a 100-year global warming potential nearly 300 times that of carbon dioxide (CO₂; Forster et al., 2007), and is the largest emission source of ozone-depleting nitrogen oxides in the stratosphere (Ravishankara et al., 2009). In 2019, the globally averaged [N₂O] reached approximately 332 ppb compared to the pre-industrial level of 270 ppb (NOAA/ESRL, 2019). While this increase is known to be linked primarily to increased fertilizer use in agriculture (Bouwman et al., 2002; Mosier et al., 1998; Tian et al., 2015), understanding the underlying microbial processes producing and consuming N₂O has proved more challenging, and individual source contributions from sectors such as agricultural soils, wastewater management and biomass burning to global bottom-up estimates of N₂O emissions have large uncertainties (Denman et al., 2007). Stable isotopes are an effective tool for distinguishing N₂O sources and determining production pathways, which is critical for developing appropriate mitigation strategies (Baggs, 2008; Ostrom and Ostrom, 2011; Toyoda et al., 2017).

The N₂O molecule has an asymmetric linear structure (NNO), with the following most abundant isotopocules: ¹⁴N¹⁵N¹⁶O (¹⁵N^α-N₂O); ¹⁵N¹⁴N¹⁶O (¹⁵N^β-N₂O); ¹⁴N¹⁴N¹⁸O (¹⁸O-N₂O); and ¹⁴N¹⁴N¹⁶O (Yoshida and Toyoda, 2000). The terms ¹⁵N^α and ¹⁵N^β refer to the respective central and terminal positions of nitrogen (N) atoms in the NNO molecule (Toyoda and Yoshida, 1999). Isotopic abundances are reported in δ-notation, where $\delta^{15}\text{N} = R(^{15}\text{N}/^{14}\text{N})_{\text{sample}} / R(^{15}\text{N}/^{14}\text{N})_{\text{reference}} - 1$ denotes the relative difference in per mil (‰) of the sample versus atmospheric N₂ (AIR-N₂). The isotope ratio $R(^{15}\text{N}/^{14}\text{N})$ equals $x(^{15}\text{N})/x(^{14}\text{N})$, with x being the absolute abundance of ¹⁴N and ¹⁵N, respectively. Similarly, Vienna Standard Mean Ocean Water (VSMOW) is the international isotope ratio scale for δ¹⁸O. In practice, the isotope δ value is calculated from measurement of isotopocule ratios of sample and reference gases, with the latter being defined on the AIR-N₂ and VSMOW scales. By extension, δ¹⁵N^α denotes the corresponding relative difference of isotope ratios for ¹⁴N¹⁵N¹⁶O/¹⁴N¹⁴N¹⁶O, and δ¹⁵N^β for

$^{15}\text{N}^{14}\text{N}^{16}\text{O}/^{14}\text{N}^{14}\text{N}^{16}\text{O}$. The site-specific intramolecular distribution of ^{15}N within the N_2O molecule is termed ^{15}N -site preference (SP), and is defined as: $\text{SP} = \delta^{15}\text{N}^\alpha - \delta^{15}\text{N}^\beta$ (Yoshida and Toyoda, 2000). The term $\delta^{15}\text{N}^{\text{bulk}}$ is used to express the average $\delta^{15}\text{N}$ value, and is equivalent to $\delta^{15}\text{N}^{\text{bulk}} = (\delta^{15}\text{N}^\alpha + \delta^{15}\text{N}^\beta)/2$.

5 Extensive evidence has shown that SP, $\delta^{15}\text{N}^{\text{bulk}}$ and $\delta^{18}\text{O}$ can be used to differentiate N_2O source processes and biogeochemical cycling (Decock and Six, 2013; Denk et al., 2017; Heil et al., 2014; Lewicka-Szczebak et al., 2014, 2015; Ostrom et al., 2007; Sutka et al., 2003, 2006; Toyoda et al., 2005, 2017; Wei et al., 2017). Isotopocule abundances have been measured in a wide range of environments, including the troposphere (Harris et al., 2014a; Röckmann and Levin, 2005; Toyoda et al., 2013), agricultural soils
10 (Buchen et al., 2018; Ibraim et al., 2019; Köster et al., 2011; Mohn et al., 2012; Ostrom et al., 2007; Park et al., 2011; Pérez et al., 2001, 2006; Toyoda et al., 2011; Verhoeven et al., 2018, 2019; Well et al., 2008, 2009; Wolf et al., 2015), mixed urban-agricultural environments (Harris et al., 2017), coal and waste combustion (Harris et al., 2014b; Ogawa and Yoshida, 2005), fossil fuel combustion (Toyoda et al., 2008), wastewater treatment (Harris et al., 2015a, b; Wunderlin et al., 2012, 2013), groundwater (Koba et al.,
15 2009; Minamikawa et al., 2011; Nikolenko et al., 2019; Well et al., 2005, 2012), estuaries (Erler et al., 2015), mangrove forests (Murray et al., 2018), stratified water impoundments (Yue et al., 2018), and firn air and ice cores (Bernard et al., 2006; Ishijima et al., 2007; Prokopiou et al., 2017). While some applications like laboratory incubation experiments allow for analysis of the isotopic signature of the pure source, most studies require analysis of the source diluted in ambient air. This specifically applies to
20 terrestrial ecosystem research, since N_2O emitted from soils is immediately mixed with background atmospheric N_2O . To understand the importance of soil emissions for the global N_2O budget, two end-member mixing models commonly interpreted using Keeling or Miller-Tans plots are frequently used to back-calculate the isotopic composition of N_2O emitted from soils (Keeling, 1958; Miller and Tans, 2003).

25

N_2O isotopocules can be analyzed by isotope-ratio mass spectrometry (IRMS) and laser spectroscopic techniques, with currently available commercial spectrometers operating in the mid-infrared (MIR) region to achieve highest sensitivities. IRMS analysis of the N_2O intramolecular ^{15}N distribution is based on quantification of the fragmented (NO^+ , m/z 30 and 31) and molecular (N_2O^+ , m/z 44, 45 and 46) ions to
30 calculate isotope ratios for the entire molecule ($^{15}\text{N}/^{14}\text{N}$ and $^{18}\text{O}/^{16}\text{O}$) and the central (N^α) and terminal (N^β) N atom (Toyoda and Yoshida, 1999). The analysis of N_2O SP by IRMS is complicated by the rearrangement of N^α and N^β in the ion source, while analysis of $\delta^{15}\text{N}^{\text{bulk}}$ (45/44) involves correction for NN^{17}O (mass 45). IRMS can achieve repeatability as good as 0.1 ‰ for $\delta^{15}\text{N}$, $\delta^{18}\text{O}$, $\delta^{15}\text{N}^\alpha$ and $\delta^{15}\text{N}^\beta$ (Potter et al., 2013; Röckmann and Levin, 2005), but an inter-laboratory comparison study showed
35 substantial deviations in measurements of N_2O isotopic composition, in particular for SP (up to 10 ‰) (Mohn et al., 2014).

The advancement of mid-infrared laser spectroscopic techniques was enabled by the invention and availability of non-cryogenic light sources which have been coupled with different detection schemes, such as direct absorption quantum cascade laser absorption spectroscopy (QCLAS; Aerodyne Research Inc. [ARI]; Wächter et al., 2008), cavity ring-down spectroscopy (CRDS; Picarro Inc.; Berden et al., 2000) and off-axis integrated-cavity-output spectroscopy (OA-ICOS; ABB Los Gatos Research Inc.; Baer et al., 2002) to realize compact field-deployable analyzers. In short, the emission wavelength of a laser light source is rapidly and repetitively scanned through a spectral region containing the spectral lines of the target N₂O isotopocules. The laser light is coupled into a multi-path cell filled with the sample gas, and the mixing ratios of individual isotopic species are determined from the detected absorption using Beer's Law. The wavelengths of spectral lines of N₂O isotopocules with distinct ¹⁷O, ¹⁸O or position-specific ¹⁵N substitution are unique due to the existence of characteristic rotational-vibrational spectra (Rothman et al., 2005). Thus, unlike IRMS, laser spectroscopy does not require mass-overlap correction. However, the spectral lines may have varying degrees of overlap with those of other gaseous species, which, if unaccounted for, may produce erroneous apparent absorption intensities. One advantage of laser spectroscopy is that instruments can analyze the N₂O isotopic composition in gaseous mixtures (e.g. ambient air) in a flow-through mode, providing real-time data with minimal or no sample pretreatment, which is highly attractive to better resolve the temporal complexity of N₂O production and consumption processes (Decock and Six, 2013; Heil et al., 2014; Köster et al., 2013; Winther et al., 2018).

20

Despite the described inherent benefits of laser spectroscopy for N₂O isotope analysis, applications remain challenging and are still scarce for four main reasons:

- (1) two pure N₂O isotopocule reference materials (USGS51, USGS52) have only recently been made available through the United States Geological Survey (USGS) with provisional values assigned by Tokyo Institute of Technology (Ostrom et al., 2018). The lack of N₂O isotopocule reference materials was identified as a major reason limiting inter-laboratory compatibility (Mohn et al., 2014);
- (2) laser spectrometers are subject to drift effects (e.g. due to moving interference fringes), particularly under fluctuating laboratory temperatures, which limits their performance (Werle et al., 1993);
- (3) if apparent delta values retrieved from a spectrometer are calculated from raw uncalibrated isotopocule mole fractions, referred to here as a δ -calibration approach, an inverse concentration dependence may be introduced. This can arise if the analyzer measurements of isotopocule mole fractions are linear, yet the relationship between measured and true mole fractions have a non-zero intercept (e.g. Griffith et al., 2012; Griffith, 2018), such as due to baseline structures (e.g. interfering fringes; Tuzson et al. 2008); and
- (4) laser spectroscopic results are affected by mole fraction changes of atmospheric background gases (N₂, O₂, and Ar), herein called gas matrix effects, due to the difference of pressure-broadening coefficients (Nara et al., 2012), and potentially by spectral interferences from other atmospheric constituents (H₂O,

35

CO₂, CH₄, CO, etc.), herein called trace gas effects, depending on the selected wavelength region. The latter is particularly pronounced for N₂O due to its low atmospheric abundance in comparison to other trace gases.

5 Several studies have described some of the above effects for CO₂ (Bowling et al., 2003, 2005; Griffis et al., 2004; Griffith et al., 2012; Friedrichs et al., 2010; Malowany et al., 2015; Pataki et al., 2006; Pang et al., 2016; Rella et al., 2013; Vogel et al., 2013; Wen et al. 2013), CH₄ (Eyer et al., 2016; Griffith et al., 2012; Rella et al., 2013), and recently N₂O isotope laser spectrometers (Erler et al., 2015; Harris et al., 2014; Ibraim et al., 2018; Wächter et al., 2008). However, a comprehensive and comparative
10 characterization of the above effects for commercially-available N₂O isotope analyzers is lacking.

Here, we present an intercomparison study of commercially-available N₂O isotope laser spectrometers with the three most common detection schemes: (1) OA-ICOS (N₂OIA-30e-EP, ABB-Los Gatos Research Inc.); (2) CRDS (G5131-i, Picarro Inc.); (3) QCLAS (dual QCLAS and TREX–mini QCLAS,
15 ARI). Performance characteristics including precision, repeatability, drift and dependence of isotope measurements on [N₂O] were determined. Instruments were tested for gas matrix effects (O₂, Ar) and spectral interferences from enhanced trace gas mole fractions (CO₂, CH₄, CO, H₂O) at various [N₂O] to develop analyzer-specific correction functions. The accuracy of different spectrometer designs was then assessed during a laboratory-controlled mixing experiment designed to simulate two end-member mixing,
20 in which results were compared to calculated expected values, as well as to those acquired using IRMS (δ values) and gas chromatography (GC, N₂O concentration). In closing, we provide a calibration workflow that will assist researchers in the operation of N₂O and other trace gas isotope laser spectrometers in order to acquire accurate isotope analyses.

2 Materials and Methods

25 2.1 Analytical techniques

Operational details of the laser spectrometers tested in this study, including wavenumber regions, line positions and line strengths of N₂O, are provided in Table 1. In Fig. 1, selected N₂O rotational lines are shown in combination with the absorption lines of the atmospheric most abundant IR-active trace gases (H₂O, CO₂, CH₄, CO and O₃) within the different wavenumber regions used by the analyzers. Fig. 1 can
30 be used to rationalize possible spectral interferences within different wavenumber regions.

Table 1. Overview on the wavelength regions, line positions and line strengths of N₂O isotopocules, and key operating parameters for each laser spectrometer tested in this study.

Detection scheme (model; manufacturer)	N ₂ O range [ppb]	Wavenumber region (cm ⁻¹)	Isotopocules	Line positions (cm ⁻¹) / Line strength [cm ⁻¹ / (molecule cm ⁻²)]	Flow rate (cm ³ min ⁻¹)	Cell temperature (°C)	Cell pressure (hPa)	Internal plumbing volume (cm ³)	Effective volume at NTP (cm ³)	Measurement frequency (seconds)	References
OA-ICOS I (N ₂ OIA-30e-EP; ABB Los Gatos Research Inc.)	300 – 100000	2192.1 – 2192.5	¹⁴ N ¹⁴ N ¹⁶ O ¹⁴ N ¹⁵ N ¹⁶ O ¹⁵ N ¹⁴ N ¹⁶ O ¹⁴ N ¹⁴ N ¹⁸ O	2192.40 / 4.919·10 ⁻²⁰ 2192.44 / 4.919·10 ⁻²⁰ 2192.48 / 3.375·10 ⁻¹⁹ 2192.31 / 3.31·10 ⁻²¹ 2192.33 / 2.968·10 ⁻²¹ 2192.13 / 1.113·10 ⁻²¹	60	43.6	61	930	60.50	1.00	Baer et al. (2002) ABB-Los Gatos Research Inc. (2019)
CRDS I & II (G5131-i; Picarro Inc.)	300 – 1500	2195.7 – 2196.3	¹⁴ N ¹⁴ N ¹⁶ O ¹⁴ N ¹⁵ N ¹⁶ O ¹⁵ N ¹⁴ N ¹⁶ O ¹⁴ N ¹⁴ N ¹⁸ O	2196.21 / 5.161·10 ⁻²⁰ 2196.24 / 5.161·10 ⁻²⁰ 2195.76 / 2.734·10 ⁻²¹ 2195.80 / 2.197·10 ⁻²¹ 2195.95 / 1.431·10 ⁻²¹	25.2 (CRDS I) 12.5 (CRDS II)	40.2	100	40	4.22	3.41 (CRDS I) 2.54 (CRDS II)	Picarro Inc. (2019)
QCLAS I, II & III (CW-QC-TILDAS-SC-D; Aerodyne Research Inc.)	300 – 90000	2187.7 – 2188.15 and 2203.1 – 2203.4	¹⁴ N ¹⁴ N ¹⁶ O ¹⁴ N ¹⁵ N ¹⁶ O ¹⁵ N ¹⁴ N ¹⁶ O ¹⁴ N ¹⁴ N ¹⁸ O	2188.04 / 2.601·10 ⁻²¹ 2187.94 / 3.294·10 ⁻²¹ 2187.85 / 3.274·10 ⁻²¹ 2203.28 / 1.794·10 ⁻²¹	130 ^a	20 ^a	53.3 ^a	2100	104 ^a	1.00 ^a	Nelson (2008) Wächter et al. (2008)
TREX-QCLAS I (Modified CW-QC-TILDAS-76-CS; Aerodyne Research Inc.)	300 – 1500 ^{a,b}	2203.1 – 2203.4 ^a	¹⁴ N ¹⁴ N ¹⁶ O ¹⁴ N ¹⁵ N ¹⁶ O ¹⁵ N ¹⁴ N ¹⁶ O ¹⁴ N ¹⁴ N ¹⁸ O	2203.10 / 2.710·10 ⁻²¹ 2203.11 / 1.435·10 ⁻²¹ 2203.36 / 9.798·10 ⁻²² 2203.20 / 7.016·10 ⁻²² 2203.28 / 1.794·10 ⁻²¹	^c	20 ^a	35.6 ^a	620	20 ^a	1.00 ^a	Ibraim et al. (2018)

a) Dual QC-TILDAS and mini QC-TILDAS are flexible spectrometer platforms, which can be used with different parameter settings. The indicated numbers were chosen for the described experiments.

5 b) The mini QC-TILDAS spectrometer is used in combination with a preconcentration device (Ibraim et al., 2018), the indicated N₂O concentration range is prior to preconcentration.

c) The preconcentration – mini QC-TILDAS system is used in a repetitive batch cycle without a continuous sample gas flow (Ibraim et al., 2018, 2019).

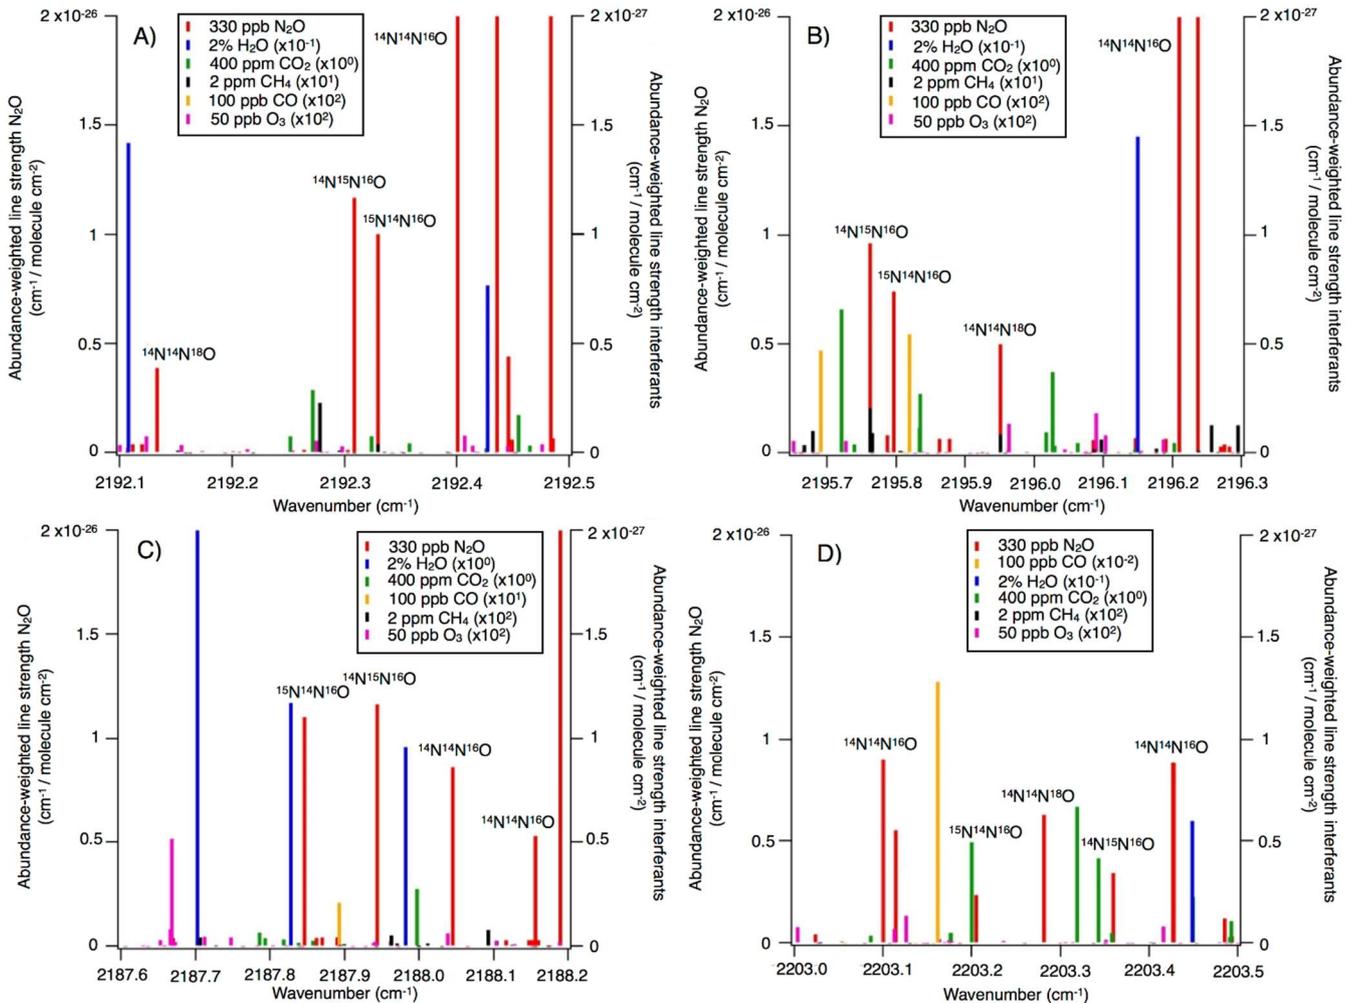


Fig. 1. N₂O isotopocule absorption line positions in the wavenumber regions selected for A) OA-ICOS; B) CRDS; and C & D) QCLAS techniques. Regions of possible spectral overlap from interfering trace gases such as H₂O, CO₂, CH₄ and CO are shown. The abundance-scaled line strengths of trace gases have been scaled with 10⁻¹ to 10² (as indicated) because they are mostly weaker than those of the N₂O isotopocules.

2.1.1 OA-ICOS (ABB-Los Gatos Research Inc.)

The N₂OIA-30e-EP (model 914-0027, serial number 15-830, ABB-Los Gatos Research Inc., USA) tested in this study was provided by the University of New South Wales (UNSW Sydney, Australia), and is herein referred to as OA-ICOS I (Table 1). The instrument employs the OA-ICOS technique integrated with a QCL (Baer et al., 2002). In short, the QCL beam is directed off axis into the cavity cell with highly-reflective mirrors, providing an optical path of several kilometers. For further details on the OA-ICOS technique, the reader is referred to the webpage of ABB-Los Gatos Research Inc. (ABB-Los Gatos Research Inc., 2019) and Baer et al. (2002).

The specific analyzer tested here was manufactured in June 2014, and has had no hardware modifications since then. It is also important to note that a more recent N₂OIA-30e-EP model (model 914-0060) is available, that in addition quantifies δ¹⁷O. We are unaware of any study measuring N₂O isotopocules at natural abundance and ambient mole fractions with the N₂OIA-30e-EP. The only studies published so far reporting N₂O isotope data apply the N₂OIA-30e-EP either at elevated [N₂O] in a standardized gas matrix or using ¹⁵N labelling, including Soto et al. (2015), Li et al. (2016), Kong et al. (2017), Brase et al. (2017), Wassenaar et al. (2018) and Nikolenko et al. (2019).

2.1.2 CRDS (Picarro Inc.)

Two G5131-i analyzers (Picarro Inc., USA) were used in this study: a 2015 model (referred to as CRDS I, serial number 5001-PVU-JDD-S5001, delivered September 2015) provided by the Niels Bohr Institute, University of Copenhagen, Denmark; and a 2018 model (referred to as CRDS II, serial number 5070-DAS-JDD-S5079, delivered June 2018) provided by Karlsruhe Institute of Technology, Germany (Table 1). In CRDS, the beam of a single-frequency continuous wave (cw) laser diode enters a three-mirror cavity with an effective pathlength of several km to support a continuous traveling light wave. A photodetector measures the decay of light in the cavity after the cw laser diode is shut off to retrieve the mole fraction of N₂O isotopocules. For more details we refer the reader to the webpage of Picarro Inc. (Picarro Inc., 2019) and Berden et al. (2000).

Importantly, the manufacturer-installed flow-restrictors were replaced in both analyzer models, as we noted reduced flow rates due to clogging during initial reconnaissance testing. In CRDS I, a capillary (inner diameter (ID): 150 μm, length: 81 mm, flow: 25.2 cm³ min⁻¹) was installed, while CRDS II was

equipped with a critical orifice (ID: 75 μm , flow: 12.5 $\text{cm}^3 \text{min}^{-1}$). Both restrictors were tested and confirmed leak-proof. Both analyzers had manufacturer-installed permeation driers located prior to the inlet of the cavity, which were not altered for this study. In December 2017, CRDS I received a software and hardware update as per the manufacturer's recommendations. The CRDS II did not receive any software or hardware upgrades as it was acquired immediately prior to testing.

To the best of our knowledge, the work presented in Lee et al. (2017) and Ji and Grundle (2019) are the only published uses of G5131-i models. A prior model (the G5101-i), which employs a different spectral region and does not offer the capability for $\delta^{18}\text{O}$ was used by Peng et al. (2014), Erler et al. (2015), Li et al. (2015), Lebegue et al. (2016) and Winther et al. (2018).

2.1.3 QCLAS (Aerodyne Research Inc.)

Three QCLAS instruments (ARI, USA; CW-QC-TILDAS-SC-D) were used in this study. One instrument (QCLAS I, serial number 046), purchased in 2013, was provided by Karlsruhe Institute of Technology, Germany and two instruments, purchased in 2014 (QCLAS II, serial number 065) and 2016 (QCLAS III, serial number 077), were supplied by ETH Zürich, Switzerland (Table 1). QCLAS I was used in all experiments presented in this study, while QCLAS II and III were only used to assess the reproducibility of drift reported in Sect. 3.1.

All instruments were dual cw QCL spectrometers, equipped with mirror optics guiding the two laser beams through an optical anchor point to assure precise coincidence of the beams at the detector. On the way to the detector, the laser beams are coupled into an astigmatic multipass cell with a volume of approx. 2100 cm^3 in which the beams interact with the sample air. The multiple passes through the absorption cell result in an absorption path length of approx. 204 m. The cell pressure can be selected by the user and was set to 53.3 mbar as a trade-off between line separation and sensitivity. This set point is automatically maintained by the TDLWintel software (Version 1.14.89 ARI, MA, USA), which compensates for variations in vacuum pump speed by closing or opening a throttle valve at the outlet of the absorption cell.

QCLAS instruments offer great liberty to the user as the system can also be operated with different parameter settings, such as the selection of spectral lines for quantification, wavenumber calibration, sample flow rate and pressure. Thereby different applications can be realized, from high flow eddy covariance studies or high mole fraction process studies to high-precision measurements coupled to a customized inlet system. In addition, spectral interferences and gas matrix effects can be taken into consideration by multi-line analysis, inclusion of the respective spectroscopic parameters in the spectral evaluation or adjustment of the pressure broadening coefficients. The spectrometers used in this study

(QCLAS I – III) were tested under standard settings but were not optimized for the respective experiments. QCLAS I was operated as a single laser instrument using laser one, to optimize spectral resolution of the frequency sweeps. It is important to note the mixing ratios returned by the instrument are solely based on fundamental spectroscopic constants (Rothman et al., 2005), so that corrections such as the dependence of isotope ratios on $[N_2O]$ have to be implemented by the user in the post processing.

To our knowledge, QCLAS instruments have so far predominately been used for determination of N_2O isotopic composition in combination with preconcentration (see below) or at enhanced mole fractions (Harris et al., 2015; Heil et al. 2014; Köster et al., 2013), except for Yamamoto et al. (2014) who had used a QCLAS (CW-QC-TILDAS-SC-S-N2OISO; ARI, USA) with one laser (2189 cm^{-1}) in combination with a closed chamber system. To achieve the precision and accuracy levels reported in their study, Yamamoto et al. (2014) corrected their measurements for mixing ratio dependence and minimized instrumental drift by measuring N_2 gas every 1hr for background-correction. These authors also showed that careful temperature control of their instrument in an air-conditioned cabinet was necessary for achieving optimal results.

2.1.4 TREX-QCLAS

A compact mini QCLAS device (CW-QC-TILDAS-76-CS, serial number 074, ARI, USA) coupled with a preconcentration system, called trace gas extractor (TREX) was provided by Empa, Switzerland. The spectrometer comprises a continuous-wave mid-infrared quantum cascade laser source emitting at 2203 cm^{-1} and an astigmatic multipass absorption cell with a path length of 76 m and a volume of approximately 620 cm^3 (Ibrahim et al., 2018) (Table 1). The TREX unit was designed and manufactured at Empa and is used to separate the N_2O from the sample gas prior to QCLAS analysis. Thereby, the initial $[N_2O]$ is increased by a factor of 200 – 300, other trace gases are removed and the gas matrix is set to standardized conditions. Before entering the TREX device, CO is oxidized to CO_2 using a metal catalyst (Sofnocat 423, Molecular Products Limited, GB). Water and CO_2 in sample gases were removed by a permeation dryer (PermaPure Inc., USA) in combination with a sodium hydroxide (NaOH) / magnesium perchlorate ($Mg(ClO_4)_2$) trap (Ascarite: 6 g, 10–35 mesh, Sigma Aldrich, Switzerland, bracketed by $Mg(ClO_4)_2$, $2 \times 1.5\text{ g}$, Alfa Aesar, Germany). Thereafter, N_2O is adsorbed on a HayeSepD (Sigma Aldrich, Switzerland) filled trap, cooled down to $125.1 \pm 0.1\text{ K}$ by attaching it to a copper baseplate mounted on a high-power Stirling cryo-cooler (CryoTel GT, Sunpower Inc., USA). N_2O adsorption requires $5.080 \pm 0.011\text{ L}$ of gas to have passed through the adsorption trap. For N_2O desorption, the trap is decoupled from the copper baseplate, while slowly heating it to 275 K with a heat foil (diameter 62.2 mm, 100 W, HK5549, Minco Products Inc., USA). Desorbed N_2O is purged with $1\text{--}5\text{ cm}^3\text{ min}^{-1}$ of synthetic air into the QCLAS cell for analysis. By controlling the flow rate and trapping time, the $[N_2O]$ in the QCLAS cell can be adjusted to 60–80 ppm at a cell pressure of $35.6 \pm 0.04\text{ mbar}$. A custom-written

LabVIEW program (Version 18.0.1, National Instruments Corp., USA) allows remote control and automatic operation of the TREX. So far, the TREX-QLCAS system has been successfully applied to determine N₂O emission, as well as N₂O isotopic signatures from various ecosystems (e.g. Mohn et al., 2012; Harris et al., 2014; Wolf et al., 2015; Ibraim et al., 2019).

5 2.1.5 GC-IRMS

IRMS analyses were conducted at ETH Zürich using a gas preparation unit (Trace Gas, Elementar, Manchester, UK) coupled to an IsoPrime100 IRMS (Elementar, Manchester, UK). [N₂O] analysis using gas chromatography was also performed at ETH Zürich (456-GC, Scion Instruments, Livingston, UK). GC-IRMS analyses were conducted as part of experiments described further in Section 2.4.8. Further
10 analytical details are provided in Supplementary Material 1.

2.2 Sample and reference gases

2.2.1 Matrix and interference test gases

Table 2 provides O₂, Ar and trace gas mole fractions of matrix gases and interference test gases used during testing. The four matrix gases comprised: synthetic air (matrix a, Messer Schweiz AG, Switzerland); synthetic air with Ar (matrix b, Carbagas AG, Switzerland); synthetic air with Ar, CO₂, CH₄ and CO at near-ambient mole fractions (matrix c, Carbagas AG, Switzerland); and high purity nitrogen gas (N₂, Messer Schweiz AG, Switzerland). Matrix gases were analyzed in the WMO GAW World Calibration Center at Empa (WCC Empa) for CO₂, CH₄, H₂O (G1301, Picarro Inc., USA), and N₂O and CO (CW-QC-TILDAS-76-CS; ARI, USA) against standards of the National Oceanic and
20 Atmospheric Administration/Earth System Research Laboratory/Global Monitoring Division (NOAA/ESRL/GMD). The [N₂O] in all matrix gases and N₂ were below 0.3 ppb. The three gas mixtures used for testing of spectral interferences contained higher mole fractions of either CO₂, CH₄ or CO in matrix gas b (Carbagas AG, Switzerland), which prevented spectroscopic analysis of other trace substances.

25

30

35

Table 2. O₂, Ar content and trace gas concentrations for matrix and interference test gases. Trace gas concentrations of matrix gases were analyzed by WMO GAW WCC Empa against standards of the NOAA/ESRL/GMD. For trace gas concentrations of interference test gases manufacturer specifications are given. Reported O₂ and Ar contents are according to manufacturer specifications. The given uncertainty is the uncertainty stated by the manufacturer or the standard deviation for analysis of n cylinders of the same specification.

Gas	Abbreviation	O ₂ ^{a)} [%]	Ar ^{a)} [%]	CO ₂ ^{b)} [ppm]	CH ₄ ^{b)} [ppb]	CO ^{b)} [ppb]	N ₂ O ^{b)} [ppb]	n
Matrix gases								
Synthetic air	matrix a	20.5±0.5	-	< 1	< 25	< 200	< 0.25	4
Synthetic air + Ar	matrix b	20.95±0.2	0.95±0.01	< 0.5	< 15	< 150	< 0.15	3
Synthetic air + Ar +CO ₂ + CH ₄ + CO	matrix c	20.95±0.4	0.95±0.02	397±3	2004±20	195±3	< 0.15	9
Nitrogen (6.0)	N ₂	< 0.00003	< 0.0001	< 0.2	< 1	< 1	< 0.05	2
		O ₂ ^{a)} [%]	Ar ^{a)} [%]	CO ₂ ^{a)} [%]	CH ₄ ^{a)} [ppm]	CO ^{a)} [ppm]	N ₂ O ^{a)} [ppb]	n
Interference test gases								
CO ₂ in synthetic air + Ar	CO ₂ in matrix b	21.06±0.2	0.94±0.01	4.02±0.04	n.a.	n.a.	n.a.	-
CH ₄ in synthetic air + Ar	CH ₄ in matrix b	20.79±0.4	0.96±0.02	n.a.	199±4	n.a.	n.a.	-
CO in synthetic air + Ar	CO in matrix b	20.95±0.4	0.95±0.02	n.a.	n.a.	20.6±0.4	n.a.	-

^{a)} manufacturer specifications

^{b)} analyzed at WMO GAW WCC Empa

10 n.a. not analyzed due to very high concentration of one trace substance, which affects spectroscopic analysis of other species

2.2.2 Reference gases (S1, S2) and pressurized air (PA1, PA2)

Preparation of pure and diluted reference gases

Two reference gases (S1, S2) with different N₂O isotopic composition were used in this study. Pure N₂O reference gases were produced from high purity N₂O (Linde, Germany) decanted into evacuated Luxfer aluminum cylinders (S1: P3333N, S2: P3338N) with ROTAREX valves (Matar, Italy) to a final pressure of maximum 45 bar to avoid condensation. Reference gas 1 (S1) was high purity N₂O only. For reference gas 2 (S2), high purity N₂O was supplemented with defined amounts of isotopically pure (>98%) ¹⁴N¹⁵NO (NLM-1045-PK), ¹⁵N¹⁴NO (NLM-1044-PK) (Cambridge Isotope Laboratories, USA) and NN¹⁸O using a ten-port two-position valve (EH2C10WEPH with 20 mL sample loop, Valco Instruments Inc., Switzerland). Since NN¹⁸O was not commercially available, it was synthesized using the following procedure: (1) ¹⁸O exchange of HNO₃ (1.8 mL, Sigma Aldrich) with 97% H₂¹⁸O (5 mL, Medical Isotopes Inc.) under reflux for 24 hours; (2) condensation of NH₃ and reaction controlled by LN₂; and (3) thermal decomposition of NH₄NO₃ in batches of 1 g in 150 mL glass bulbs with breakseal (Glasbläserei Möller AG, Switzerland) to produce NN¹⁸O. The isotopic enrichment was analyzed after dilution in N₂ (99.9999 %, Messer Schweiz AG) with a Vision 1000C quadrupole mass spectrometer (QMS) equipped with a customized ambient pressure inlet (MKS Instruments, UK). Triplicate analysis provided the following composition: 36.25 ± 0.10 % of NN¹⁶O and 63.75 ± 0.76 % of NN¹⁸O.

High [N₂O] reference gases (S1-a_{90ppm}, S1-b_{90ppm}, S1-c_{90ppm}, S2-a_{90ppm}) with a target mole fraction of 90 ppm were prepared in different matrix gases (a, b, c) using a two-step procedure. First, defined volumes of S1 and S2 were dosed into Luxfer aluminum cylinders (ROTAREX valve, Matar, Italy) filled with matrix gas (a, b and c) to ambient pressure using N₂O calibrated MFCs (Vögtlin Instruments GmbH, Switzerland). Second, the N₂O was gravimetrically diluted (ICS429, Mettler Toledo GmbH, Switzerland) with matrix gas to the target mole fraction. Ambient [N₂O] reference gases (S1-c_{330ppb}, S2-c_{330ppb}) with a target mole fraction of 330 ppb were prepared by dosing S1-c_{90ppm} or S2-c_{90ppm} into evacuated cylinders with a calibrated MFC, followed by gravimetric dilution with matrix c.

10 Analysis of reference gases and pressurized air

Table 3 details the trace gas mole fractions and N₂O isotopic composition of high and ambient [N₂O] reference gases, as well as commercial pressurized air (PA1 and PA2) used during testing. Trace gas mole fractions of high [N₂O] reference gases were acquired from the trace gas levels in the respective matrix gases (Table 2), while ambient [N₂O] reference gases and target as well as background gases were analyzed by WCC Empa. The isotopic composition of high [N₂O] isotope reference gases in synthetic air (S1-a_{90ppm}, S2-a_{90ppm}) was analyzed in relation to N₂O isotope standards (Cal1 – Cal3) in an identical matrix gas (matrix a) using laser spectroscopy (CW-QC-TILDAS-200; ARI, Billerica, USA). The composition of Cal1 – Cal3 are outlined in Supplementary Material 2.

20

25

30

35

Table 3. Trace gas concentrations and N₂O isotopic composition of high and ambient N₂O concentration reference gases, and pressurized air. Trace gas concentrations of high concentration reference gases were retrieved from the composition of matrix gases used for their production (see Table 2), trace gas concentrations in ambient concentration reference gases and pressurized air were analyzed by WMO GAW WCC Empa against standards of the NOAA/ESRL/GMD. The N₂O isotopic composition was quantified by laser spectroscopy (QCLAS) and preconcentration - laser spectroscopy (TREX-QCLAS) against reference gases previously analyzed by Tokyo Institute of Technology.

Gas	CO ₂ [ppm]	CH ₄ [ppb]	CO [ppb]	N ₂ O [ppb]	δ ¹⁵ N ^α vs AIR-N ₂ [‰]	δ ¹⁵ N ^β vs AIR-N ₂ [‰]	δ ¹⁸ O vs VSMOW [‰]
High N₂O concentration reference gases							
S1-a _{90ppm}	< 1	< 25	< 200	~90000	0.54±0.17	1.15±0.06	39.46±0.01
S1-b _{90ppm}	< 0.5	< 15	< 150	~90000	0.54±0.17	1.15±0.06	39.46±0.01
S1-c _{90ppm}	397±3	2004±20	195±3	~90000	0.54±0.17	1.15±0.06	39.46±0.01
S2-a _{90ppm}	< 1	< 25	< 200	~90000	51.43±0.06	55.14±0.09	100.09±0.03
S2-c _{90ppm}	397±3	2004±20	195±3	~90000	51.43±0.06	55.14±0.09	100.09±0.03
Ambient N₂O concentration reference gases							
S1-c _{330ppb}	399.78±0.04	2022±0.2	195±0.3	327.45±0.06	0.92±0.39	1.44±0.25	39.12±0.18
S2-c _{330ppb}	398.62±0.04	2020±0.2	193±0.3	323.97±0.06	52.38±0.10	55.61±0.12	99.59±0.03
High N₂O concentration source gas (SG) for two-end member mixing experiments (Sect. 2.4.8)							
SG1-a _{90ppm}	< 1	< 25	< 200	~90000	-	-	31.79±0.12
					24.35±0.32	22.94±0.33	
SG2-a _{90ppm}	< 1	< 25	< 200	~90000	51.43±0.06	55.14±0.09	100.09±0.03
Pressurized air							
Pressurized air (PA1)	200.55±0.07	2582±0.2	187±0.2	326.51±0.06	15.83±0.03	-3.39±0.14	44.66±0.02
Pressurized air (PA2)	437.99±0.36	2957±0.3	275±0.4	333.50±0.09	15.81±0.07	-	44.72±0.04
						3.31±0.004	

For high mole fraction reference gases in matrix b and c (S1-b_{90ppm}, S1-c_{90ppm}, S2-c_{90ppm}), the δ values acquired for S1-a_{90ppm} and S2-a_{90ppm} were assigned, since all S1 and S2 reference gases (irrespective of gas matrix) were generated from the same source of pure N₂O gas. Direct analysis of S1-b_{90ppm}, S1-c_{90ppm} and S2-c_{90ppm} by QCLAS was not feasible as no N₂O isotope standards in matrix b and c were available. The absence of significant difference (< 1 ‰) in N₂O isotopic composition between S1-b_{90ppm} and S1-c_{90ppm} in relation to S1-a_{90ppm} (and S2-c_{90ppm} to S2-a_{90ppm}) was assured by first statically diluting S1-b_{90ppm}, S1-c_{90ppm} and S2-c_{90ppm} to ambient N₂O mole fractions with synthetic air. This was followed by analysis using TREX-QCLAS (as described in Sect. 2.1.4) against the same standards used for S1-a_{90ppm}, S2-a_{90ppm} isotope analysis.

Ambient mole fraction N₂O isotope reference gases (S1-c_{330ppb}, S2-c_{330ppb}) and PA1 and PA2 were analyzed by TREX-QCLAS (Sect. 2.1.4) using N₂O isotope standards (Cal1 – Cal5) as outlined in Supplementary Material 2.

2.3 Laboratory setup, measurement procedures and data processing

2.3.1 Laboratory setup

All experiments were performed at the Laboratory for Air Pollution / Environmental Technology, Empa, Switzerland during June 2018 and February 2019. The laboratory was air conditioned to 295 K (± 1 K), with ± 0.5 K diel variations (Saveris 2, Testo AG, Switzerland), with the exception of a short period (7th to 8th July 2018), where the air conditioning was deactivated to test the temperature dependence of analyzers. Experiments were performed simultaneously for all analyzers, with the exception of the TREX-QCLAS, which requires an extensive measurement protocol and additional time to trap and measure N₂O (Ibraim et al., 2018) and thus could not be integrated concurrently with the other analyzers.

10

Fig. 2 shows a generalized experimental setup used for all experiments. Additional information for specific experiments is given in Section 2.4, and individual experimental setups are depicted in Supplementary Material 3. Gas flows were controlled using a set of mass flow controllers (MFC, model high-performance, Vögtlin Instruments GmbH, Switzerland) integrated into a MFC control unit (Contrec AG, Switzerland). All MFCs were calibrated by the manufacturer for whole air, which according to Vögtlin Instruments is valid for pure N₂ and pure O₂ as well. Operational ranges of applied MFCs ranged from 0–25 cm³ min⁻¹ to 0–5000 cm³ min⁻¹, and had reported uncertainties of 0.3 % of their maximum flow and 0.5 % of actual flow. To reduce the uncertainty of the flow regulation, the MFC with the smallest maximum flow range available was selected. The sum of dosed gas flows was always higher than the sum of gas consumption by analyzers, with the overflow exhausted to room air. Gas lines between gas cylinders and MFCs, as well as between MFCs and analyzers, were 1/8" stainless steel tubing (type 304, Supelco, Sigma-Aldrich Chemie GmbH, Switzerland). Manual two-way (SS-1RS4 or SS-6H-MM, Swagelok, Switzerland) or three-way valves (SS-42GXS6MM, Swagelok, Switzerland) were used to separate or combine gas flows.

20

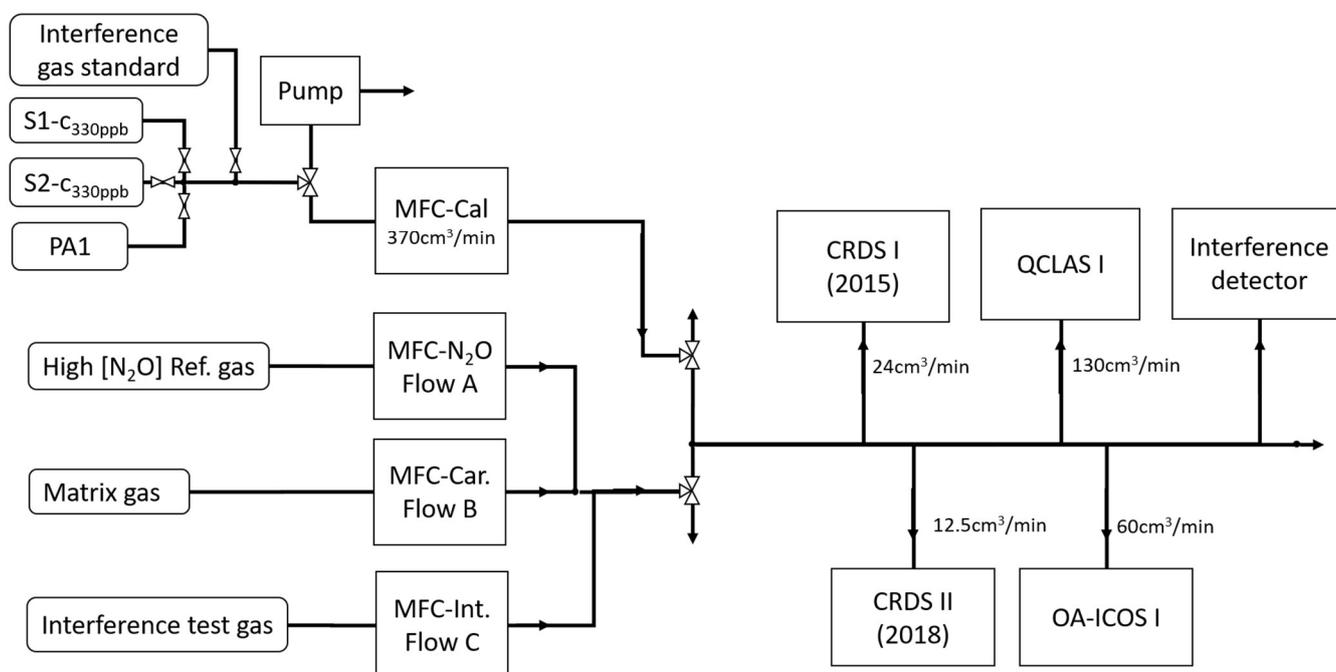


Fig. 2. The generalized experimental setup used for all experiments conducted in this study. The gases introduced via MFC flows A, B and C were changed according to the experiments outlined in Sect. 2.4. Table 2 and Table 3 provide the composition of the *matrix gases* (MFC B), *interference test gases* (MFC C) and *high [N₂O] concentration reference gases* (MFC A). Laboratory setups for each individual experiment are provided in Supplementary Material 3.

2.3.2 Measurement procedures, data processing and calibration

With the exception of Allan variance experiments performed in Sect. 2.4.1, all gas mixtures analyzed during this study were measured by the laser spectrometers for a period of 15 minutes, with the last 5 minutes used for data processing. Customized R-scripts (R Core Team, 2017) were used to extract the 5 min averaged data for each analyzer. Whilst the OA-ICOS and QCLAS instruments provide individual $^{14}\text{N}^{14}\text{N}^{16}\text{O}$, $^{14}\text{N}^{15}\text{N}^{16}\text{O}$, $^{15}\text{N}^{14}\text{N}^{16}\text{O}$ and $^{14}\text{N}^{14}\text{N}^{18}\text{O}$ mole fractions, the default data output generated by the CRDS analyzers are δ values, with underlying calculation schemes inaccessible to the user. Therefore, to remain consistent across analyzers, uncalibrated δ values were calculated for OA-ICOS and QCLAS instruments first, using literature values for the $^{15}\text{N}/^{14}\text{N}$ (0.0036782) and $^{18}\text{O}/^{16}\text{O}$ (0.0020052) isotope ratios of AIR-N₂ and VSMOW (Werner and Brand, 2001).

Each experiment was performed over the course of one day, and consisted of three phases: (1) an initial calibration phase; (2) an experimental phase; and (3) a final calibration phase. During phases (1) and (3), reference gases S1-C_{330ppb} and S2-C_{330ppb} were analyzed. On each occasion (i.e. twice a day), this was followed by the analysis of PA1, which was used to determine the long-term (day-to-day) repeatability of the analyzers. Phase (2) experiments are outlined in Sect. 2.4. Throughout all three phases, all measurements were systematically alternated with an Anchor gas measurement, the purpose of which was twofold: (1) to enable drift correction; and (2) as a means of quantifying deviations of the measured [N₂O] and δ values caused by increasing [N₂O] (Sect. 2.4.4), the removal of matrix gases (O₂ and Ar in Sect.

2.4.5) or addition of trace gases (CO₂, CH₄ and CO in Sect 2.4.6). Accordingly, the composition of the Anchor gas varied across experiments (see Sect. 2.4), but remained consistent throughout each experiment. A drift correction was applied to the data if a linear or non-linear model fitted to the Anchor gas measurement over the course of an experiment was statistically significant at $p < 0.05$. Otherwise, no drift correction was applied.

In Sects. 2.4.3 (repeatability experiments) and 2.4.8 (two end-member mixing experiments), trace gas effects were corrected according to Eqs. (1), (2) and (3) using derived analyzer-specific correction functions because the CO₂, CH₄ and CO composition of PA1 in Sect. 2.4.3 and the gas mixtures in Sect. 2.4.8 varied from those of the calibration gases S1-c_{330ppb} (S1) and S2-c_{330ppb} (S2):

$$[N_2O]_{tc,G} = [N_2O]_{meas,G} - \sum_x \left(\Delta[N_2O](\Delta[x]_G, [N_2O]_{meas,G}) \right) \quad (1)$$

$$\delta_{tc,G} = \delta_{meas,G} - \sum_x \left(\Delta\delta(\Delta[x]_G, \delta_{meas,G}) \right) \quad (2)$$

and,

$$\Delta[x]_G = [x]_G - \frac{[x]_{S1} + [x]_{S2}}{2} \quad (3)$$

where $[N_2O]_{tc,G}$ and $\delta_{tc,G}$ refer to the trace gas-corrected $[N_2O]$ and δ values ($\delta^{15}N^a$, $\delta^{15}N^b$ or $\delta^{18}O$) of sample gas G, respectively; $[N_2O]_{meas,G}$ and $\delta_{meas,G}$ are the raw uncorrected $[N_2O]$ and δ values measured by the analyzer for sample gas G, respectively; $\Delta[N_2O]$ and $\Delta\delta$ refer to the offset on the $[N_2O]$ or δ values, respectively, resulting from the difference in trace gas mole fraction between sample gas G and reference gases, denoted $\Delta[x]_G$; $[x]_G$ is the mole fraction of trace gas x (CO₂, CH₄ or CO) in sample gas G; and $[x]_{S1}$ and $[x]_{S2}$ are the mole fractions of trace gas x in reference gases S1-c_{330ppb} and S2-c_{330ppb}. It is important to note that the differences in CO₂ and CH₄ mole fractions in S1-c_{330ppb} and S2-c_{330ppb} are two orders of magnitude smaller than the differences to PA1.

Thereafter, δ values of trace gas-corrected, mole fraction-corrected (Sect.2.4.8 only) and drift-corrected measurements from the analyzers were normalized to δ values on the international isotope ratio scales using a two-point linear calibration procedure derived from values of S1-c_{330ppb} (S1) and S2-c_{330ppb} (S2) calculated using Eq. (4) (Gröning, 2018):

$$\delta_{Cal,G} = \frac{\delta_{ref,S1} - \delta_{ref,S2}}{\delta_{corr,S1} - \delta_{corr,S2}} * (\delta_{corr,G} - \delta_{corr,S1}) + \delta_{ref,S1} \quad (4)$$

where $\delta_{Cal,G}$ is the calibrated δ value for sample gas G normalized to international isotope ratio scales; $\delta_{ref,S1}$ and $\delta_{ref,S2}$ are the respective δ values assigned to reference gases S1-c_{330ppb} and S2-c_{330ppb}; $\delta_{corr,S1}$ and $\delta_{corr,S2}$ are the respective δ values measured for the reference gases S1-c_{330ppb} and S2-c_{330ppb}

which, if required, were drift-corrected; and $\delta_{corr,G}$ is the trace gas-corrected, mole fraction-corrected (Sect.2.4.8 only) and drift-corrected (if required) δ value measured for the sample gas G.

2.4 Testing of instruments

An overview of all experiments performed in this study, including applied corrections and instruments tested, is provided in Table 4.

Table 4. Overview of the experiments performed in this study.

Experiment	Sections	Aims	Corrections applied	Instruments tested	Comments
Instrumental precision (Allan deviation)	2.4.1 3.1	Short-term precision, optimal integration time/maximum precision and drift	None	OA-ICOS I CRDS I & II QCLAS I QCLAS II & III (ambient only) TREX-QCLAS I	Conducted at N ₂ O concentrations ~326, 1000, 10000 ppb
Temperature effects	2.4.2 3.2	Temperature effects on [N ₂ O] and isotope deltas	None	OA-ICOS I CRDS I & II QCLAS I	
Repeatability (short-term, ~2 hour)	2.4.3 3.3	Repeatability	Drift	OA-ICOS I CRDS I & II QCLAS I TREX-QCLAS I	Conducted at N ₂ O concentrations ~326, 1000, 10000 ppb
Repeatability (long-term, ~2 week)	2.4.3 3.3	Repeatability	Drift, delta calibration, trace gas effect ^{a)}	OA-ICOS I CRDS I & II QCLAS I TREX-QCLAS I	Conducted at ~326 ppb N ₂ O using PA1
N ₂ O mole fraction effects	2.4.4 3.4	[N ₂ O] effects on isotope deltas, and derive correction functions	Drift	OA-ICOS I CRDS I & II QCLAS I	CRDS: 300 to 1500 ppb N ₂ O, OA-ICOS, QCLAS: 300 to 90000 ppb
Gas matrix effects (N ₂ , O ₂ and Ar)	2.4.5 3.5	Gas matrix effects on [N ₂ O] and isotope deltas, and derive correction functions	Drift	OA-ICOS I CRDS I & II QCLAS I TREX-QCLAS I	Conducted at N ₂ O concentrations ~330, 660, 990 ppb
Trace gas effects (H ₂ O, CO ₂ , CH ₄ , CO)	2.4.6 3.6	Trace gas effects on [N ₂ O] and isotope deltas, and derive correction functions	Drift	OA-ICOS I CRDS I & II QCLAS I TREX-QCLAS I (except H ₂ O)	Conducted at N ₂ O concentrations ~330, 660, 990 ppb
CO ₂ and CO removal	2.4.7 3.6	Effects of removal of CO ₂ (Ascarite) and CO (Sofnocat) on [N ₂ O] and isotope deltas	Drift	OA-ICOS I CRDS I & II QCLAS I	Conducted at N ₂ O concentrations ~330 ppb
Two end-member mixing	2.4.8 3.7	Test the ability of the instruments to extrapolate a N ₂ O source using a Keeling plot approach	Drift, 3-point concentration dependence, delta calibration, trace gas effect ^{a)} , and scaled with N ₂ O ^{b)}	OA-ICOS I (exp. 1-6) CRDS I & II (exp. 1-4) QCLAS I (exp. 1-6) TREX-QCLAS I (exp. 1-2) GC [N ₂ O], IRMS [δ] (exp. 1-6)	The workflow provided in Sect. 4.3 was applied

^{a)} Derived from trace gas effect determined in Sections 3.6.

^{b)} Derived from scaling effects described in Section 3.6.2.

2.4.1 Allan precision

The precision of the laser spectrometers was determined using the Allan variance technique (Allan, 1966; Werle et al., 1993). Experiments were conducted at different $[\text{N}_2\text{O}]$: ambient, 1000 ppb, and 10000 ppb. For the Allan variance testing conducted at ambient $[\text{N}_2\text{O}]$, a continuous flow of PA1 was measured continuously for 30 h. For testing conducted at 1000 and 10000 ppb $[\text{N}_2\text{O}]$, S1-c_{90ppm} was dynamically diluted to 1000 or 10000 ppb $[\text{N}_2\text{O}]$ with matrix gas c for 10 h. CRDS I and II were disconnected for the 10000 ppb measurement because $[\text{N}_2\text{O}]$ exceeded the specified measurement range. Daily drifts were estimated using the slope of the linear regression over the measurement period normalized to 24 h (i.e. ppb d⁻¹ and % d⁻¹).

10 2.4.2 Temperature effects

To investigate instrumental sensitivities to variations in ambient temperature, PA1 was simultaneously and continuously measured by all analyzers in flow-through mode for a period of 24 h while the air conditioning of the laboratory was turned off for over 10 h. This led to a rise in temperature from 21°C to 30°C, equating to an increase in temperature of approximately 0.9°C per hour. The increase in laboratory room temperature was detectable shortly after the air conditioning was turned off due to considerable heat being released from several other instruments located in the laboratory. Thereafter, the air conditioning was restarted and the laboratory temperature returned to 21°C over the course of 16 h, equating to a decrease of roughly 0.6°C per hour, with most pronounced effects observable shortly after restart of air conditioning when temperature changes were highest.

20 2.4.3 Repeatability

Measurements of PA1 were taken twice daily over ~2 weeks prior to and following the experimental measurement period to test the long-term repeatability of the analyzers. Measurements were sequentially corrected for differences in trace gas concentrations (Eqs. 1 – 3), drift (if required), and then δ -calibrated (Eq. 4). No matrix gas corrections were applied because the N_2 , O_2 and Ar composition of PA1 was identical to that of S1-c_{330ppb} and S2-c_{330ppb}. TREX-QCLAS I measurements for long-term repeatability were collected separately from other instruments over a period of six-months. Repeatability over shorter time periods (2.5 h) was also tested for each analyzer by acquiring 10 repeated 15 min measurements at different N_2O mole fractions: ambient (PA1), 1000 ppb and 10000 ppb N_2O .

2.4.4 N_2O mole fraction dependence

30 To determine the effect of changing $[\text{N}_2\text{O}]$ on the measured δ values, S1-c_{90ppm} was dynamically diluted with matrix c to various $[\text{N}_2\text{O}]$ spanning the operational ranges of the instruments. For both CRDS analyzers mole fractions between 300 to 1500 ppb were tested, while for the OA-ICOS I and QCLAS I

5 mixing ratios ranged from 300 to 90000 ppb. Between each [N₂O] step change, the dilution ratio was systematically set to 330 ppb N₂O to perform an Anchor gas measurement. For each instrument, the effect of increasing [N₂O] on δ values was quantified by comparing the measured δ values at each step change to the mean measured δ values of the Anchor gas, and was denoted Δδ such that $\Delta\delta = \delta_{\text{measured}} - \delta_{\text{Anchor}}$ and $\Delta\delta_{\text{Anchor}} = 0$. The experiment was repeated on three consecutive days to test day-to-day variability.

2.4.5 Gas matrix effects (O₂ and Ar)

10 Gas matrix effects were investigated by determining the dependence of [N₂O] and isotope δ values on the O₂ or Ar mixing ratio of a gas mixture. For O₂ testing, Gas 1, 2 and 3 (N₂) were mixed to incrementally change mixing ratios of O₂ (0–20.5 % O₂) while maintaining a consistent [N₂O] of 330 ppb. As an Anchor gas, Gas 1 (S1-a_{90ppm}) was dynamically diluted with Gas 2 (matrix a) to produce 330 ppb N₂O in matrix a (Table 5). O₂ mole fractions in the various gas mixtures were analyzed with a paramagnetic O₂ analyzer (Servomex, UK) and agreed with expected values to within 0.3 % (relative). For Ar testing, Gas 1 (S1-b_{90ppm}) was dynamically diluted with Gas 2 (matrix b) to produce an Anchor gas with ~330 ppb N₂O in matrix b. Gas 1, 2 and 3 (N₂ + O₂) were then mixed to incrementally change mixing ratios of Ar (0.003–15 0.95 % Ar), while a consistent [N₂O] of 330 ppb was maintained. Ar compositional differences were estimated based on gas cylinder manufacturer specifications and selected gas flows. The effects of decreasing O₂ and Ar on [N₂O] and δ values were quantified by comparing the measured [N₂O] and δ values at each step change to the mean measured [N₂O] and δ values of the Anchor gas, and were denoted Δ[N₂O] and Δδ, similar to Sect. 2.4.4. Deviations in O₂ and Ar mixing ratios were quantified by 20 comparing the [O₂] and [Ar] at each step change to the mean [O₂] and [Ar] of the Anchor gas, and were denoted ΔO₂ and ΔAr such that, for example, $\Delta O_2 = O_{2 \text{ measured}} - O_{2 \text{ Anchor}}$ and $\Delta O_{2 \text{ Anchor}} = 0$. Both O₂ and Ar experiments were triplicated.

25 In addition, O₂ and Ar effects were derived for N₂O mole fractions of ~660 ppb and ~990 ppb. These experiments were undertaken in a way similar to those described above, except Anchor gas measurements were conducted once (not triplicated).

Table 5. Gas mixtures used to test effects of gas matrix (O₂, Ar) or trace gases (CO₂, CH₄, CO) on [N₂O] and isotope deltas. Gas 1 was dynamically diluted with Gas 2 to make up an Anchor gas with [N₂O] of ~330 ppb which was systematically measured throughout the experiments to (1) enable drift correction, and (2) quantify deviations of the measured [N₂O] and δ values caused by the removal of matrix gases (O₂ and Ar in Sect. 2.4.5) or addition of trace gases (CO₂, CH₄ and CO in Sect 2.4.6). Gas 1, 2 and 3 were combined in different fractions to make up sample gas with identical [N₂O] but varying mixing ratio of the target compound.

Target compound	Gas 1	Gas 2	Gas 3	Mixing range
O ₂	S1-a90ppm (N ₂ O + N ₂ + O ₂)	N ₂ + O ₂ ^a	N ₂	0-20.5 % O ₂
Ar	S1-b90ppm (N ₂ O + N ₂ + O ₂ + Ar)	N ₂ + O ₂ + Ar ^b	N ₂ + O ₂ ^a	0.003-0.95 % Ar
CO ₂	S1-b90ppm (N ₂ O + N ₂ + O ₂ + Ar)	N ₂ + O ₂ + Ar ^b	CO ₂ in N ₂ + O ₂ + Ar ^b	1.72-2030 ppm CO ₂
CH ₄	S1-b90ppm (N ₂ O + N ₂ + O ₂ + Ar)	N ₂ + O ₂ + Ar ^b	CH ₄ in N ₂ + O ₂ + Ar ^b	0.014-10.25 ppm CH ₄
CO	S1-b90ppm (N ₂ O + N ₂ + O ₂ + Ar)	N ₂ + O ₂ + Ar ^b	CO in N ₂ + O ₂ + Ar ^b	0.14-2.13 ppm CO

^a) matrix a: 20.5 % O₂ in N₂

^b) matrix b: 20.95 % O₂, 0.95 % Ar in N₂

10 2.4.6 Trace gas effects (CO₂, CH₄, CO and H₂O)

The sensitivity of [N₂O] and δ values on changing trace gas concentrations was tested in a similar way to those described in Sect. 2.4.5. In short, Gas 1 (S1-b90ppm) was dynamically diluted with Gas 2 (matrix b) to create an Anchor gas with 330 ppb N₂O in matrix b. Gas 1, 2 and 3 (either CO₂, CH₄ or CO in matrix gas b) were mixed to incrementally change the mixing ratios of the target substances (1.7 – 2030 ppm CO₂, 0.01 – 10.25 ppm CH₄ and 0.14 – 2.14 ppm CO) while maintaining a consistent gas matrix and [N₂O] of 330 ppb (Table 5). Trace gas mole fractions in the produced gas mixtures were analyzed with a Picarro G2401 (Picarro Inc., USA) and agreed with predictions within better than 2–3 % (relative). Similar to Sect. 2.4.4, the effects of increasing CO₂, CH₄ and CO on [N₂O] and δ values were quantified by comparing the measured [N₂O] and δ values at each step change to the mean measured [N₂O] and δ values of the Anchor gas, and were denoted Δ [N₂O] and $\Delta\delta$. Similar to Sect. 2.4.5, deviations in CO₂ CH₄ and CO mixing ratios were quantified by comparing the measured [CO₂], [CH₄] and [CO] at each step change to the mean measured [CO₂], [CH₄] and [CO] of the Anchor gas. Each experiment was triplicated. The interference effects were also tested at ~660 ppb and ~990 ppb N₂O.

25 The sensitivity of the analyzers to water vapor was tested by firstly diluting Gas 1 (S1-c90ppm) with Gas 2 (matrix c) to produce an Anchor gas with 330 ppb N₂O. This mixture was then combined with Gas 3 (also matrix c) which had been passed through a humidifier (customized setup by Glasbläserei Möller, Switzerland) set to 15°C (F20 Julabo GmbH, Germany) dew point. By varying the flows of Gas 2 and 3, different mixing ratios of water vapor ranging from 0 – 13800 ppm were produced and measured using a dewpoint meter (model 973, MBW, Switzerland). H₂O effects were quantified as described above, but [N₂O] results were additionally corrected for dilution effects caused by the addition of water vapor into the gas stream. Water vapor dependence testing was not performed on the TREX-QCLAS I as the instrument is equipped with a permeation dryer at the inlet.

2.4.7 CO₂ and CO removal using NaOH (Ascarite) and Sofnocat

The efficiency of NaOH and Sofnocat for removing spectral effects caused by CO₂ and CO was assessed by repeating CO₂ and CO interference tests (Sect. 2.4.6), but with the respective traps connected in-line. These experiments were triplicated but only undertaken at ~330 ppb N₂O. NaOH traps were prepared using stainless steel tubing (OD 2.54 cm, length 20 cm) filled with 14 g Ascarite (0-30 mesh, Sigma Aldrich, Switzerland) bracketed by 3g Mg(ClO₄)₂ (Alfa Aesar, Germany) each separated by glass wool. The Sofnocat trap was prepared similarly using stainless steel tubing (OD 2.54 cm, length 20 cm) filled with 50 g Sofnocat (Sofnocat 423, Molecular Products Limited, GB) and capped on each side with glass wool.

10 2.4.8 Two end-member mixing

The ability of the instruments to accurately extrapolate N₂O source compositions was tested using a simulated two end-member mixing scenario in which a gas with high N₂O concentration, considered to be a N₂O *source* gas (SG), was dynamically diluted into a gas with ambient N₂O concentration (PA2), considered to be *background* air. N₂O mole fractions were raised above ambient levels (denoted as ΔN_2O) in three different scenarios ranging from: (1) 0–30 ppb; (2) 0–700 ppb and (3) 0–10000 ppb. In each scenario, two isotopically different *source* gases with high N₂O concentration were used; one *source* gas (SG1-a_{90ppm}) ¹⁵N depleted compared to PA2; and a second *source* gas (SG2-a_{90ppm}) ¹⁵N enriched compared to PA2 (Table 3). The three different mixing scenarios and two different *source* gases resulted in a total of six mixing scenarios (referred to as Exp. 1–6). During each experiment, PA2 was alternated with PA2 + SG in four different mixing ratios to give a span of N₂O concentrations and isotopic compositions required for Keeling plot analysis. Each experiment was triplicated. OA-ICOS I and QCLAS I were used in all experiments (Exp. 1–6), CRDS was used for ΔN_2O 0–30 ppb and 0–700 ppb (Exp. 1–4) and TREX-QCLAS was only used for ΔN_2O 0–30 ppb (Exp. 1–2).

25 To test the robustness of trace gas correction equations derived for each analyzer in Sect. 3.6, NaOH and Sofnocat traps were placed in-line between the PA2 + SG mixtures and the analyzers such that we could ensure a difference in CO₂ and CO mole fractions between the measured gas mixture and reference gases (S1-c_{330ppb}, S2-c_{330ppb}). The experiments were also bracketed by two calibration phases (S1-c_{330ppb}, S2-c_{330ppb}) to allow for δ calibration, followed by two phases where the N₂O concentration dependence was determined.

Gas samples for GC-IRMS analysis were taken in the same phase (last five min of 15 min interval) used during the minute prior to the final five minutes used for averaging by the laser-based analyzers. The gas was collected at the common overflow port of the laser spectrometers using a 60 mL syringe connected

via a Luer lock three-way valve to needle and port. 200 mL samples were taken at each concentration step. 180 mL of gas sample was stored in pre-evacuated 110 mL serum crimp vials for isotopic analysis using IRMS. IRMS analyses were conducted at ETH Zürich using a gas preparation unit (Trace Gas, Elementar, Manchester, UK) coupled to an IsoPrime100 IRMS (Elementar, Manchester, UK). The remaining 20 mL were injected in a pre-evacuated 12 mL Labco exetainer for [N₂O] analysis using gas chromatography equipped with Electron Capture Detector (ECD) performed at ETH Zürich (Bruker, 456-GC, Scion Instruments, Livingston, UK). After injection, samples were separated on HayeSep D packed columns with a 5% CH₄ in Ar mixture (P5) as carrier and make-up gas. The GC was calibrated using a suite of calibration gases at N₂O concentrations of 0.393 (Carbagas AG, Switzerland), 1.02 (PanGas AG, Switzerland) and 3.17 ppm (Carbagas AG, Switzerland). For further analytical details see Verhoeven et al. (2019) and Supplementary Material 1.

For the laser-based analyzers, data was processed as described in Sect. 2.3.2 using the following sequential order: (1) analyzer-specific correction functions, determined in Sect 3.6, were applied to correct for differences in trace gas concentrations (CO₂, CO) between sample gas and calibration gases; (2) the effect of [N₂O] changes was corrected using a three-point correction; (3) a drift-correction based on repeated measurements of PA2 was applied if necessary; and (4) δ values standardized to international scales (Eq. 4) using S1-c_{330ppb} and S2-c_{330ppb}.

3 Results

Note: due to the large number of results acquired in this Section, only selected results are shown in Figs. 3 to 14. The complete datasets (including [N₂O], $\delta^{15}\text{N}^{\alpha}$, $\delta^{15}\text{N}^{\beta}$ and $\delta^{18}\text{O}$ acquired by all instruments tested) are provided in Supplementary Material 4.

3.1 Allan precision

Allan deviations (square root of Allan variance) for 5 min and 10 min averaging times, often reported in manufacturer specifications, at ~327 ppb, 1000 ppb and 10000 ppb [N₂O] are shown in Table 6.

At near-atmospheric N₂O mole fractions of ~326.5 ppb, both CRDS analyzers showed the best precision and stability for the measurement of $\delta^{15}\text{N}^{\alpha}$, $\delta^{15}\text{N}^{\beta}$ and $\delta^{18}\text{O}$ (0.32 – 0.41 ‰, 0.41 – 0.45 ‰, 0.41 – 0.46 ‰ at 300 s averaging time, respectively), while for the precision of [N₂O], the OA-ICOS I and the CRDS II showed best performance (1.7·10⁻² ppb at 300 s averaging time) (Figs. 3 and S4-1; Table 6). The Allan precision of CRDS and OA-ICOS analyzers further improved with increasing averaging times and optimal averaging times typically exceeded 1.5-3 h. The precision and daily drift of the OA-ICOS I and

both CRDS analyzers were in agreement with manufacturer specifications (ABB-Los Gatos Research Inc., 2019; Picarro Inc., 2019). The CRDS II outperformed the CRDS I for precision, presumably due to manufacturer upgrades/improvements in the newer model. The QCLAS spectrometers exhibited significant differences between instruments, which might be due to differences in the instrument hardware / design, as instruments were manufactured between 2012 – 2016, or in the parameter setting (such as cell pressure and tuning parameters) of different analyzers.

Generally, short-term (approx. up to 100 s) precision of QCLAS instruments was compatible or superior to CRDS or OA-ICOS, but data quality was decreased for longer averaging times due to drift effects. Nonetheless, the performance of QCLAS I, II and III generally agrees with Allan precision measurements executed by Yamamoto et al. (2014), who reported 1.9 – 2.6 ‰ precision for δ values at ambient N₂O mole fractions and 0.4 – 0.7 ‰ at 1000 ppb N₂O. QCLAS I, which was tested further in Sects. 3.2 – 3.7, displayed the poorest performance of all QCLAS analyzers, in particular for $\delta^{15}\text{N}^{\beta}$. The primary cause of the observed excess drift in QCLAS I was fluctuating spectral baseline structure (pers. comm. ARI), which can be significantly reduced by applying an automatic spectral correction method developed by ARI. This methodology is currently in trial phase and, thus, not yet implemented in the software that controls the QCLAS instruments. A brief overview of the methodology is provided in Supplementary Material 5, and corrected results for QCLAS I provided in Table 6. This methodology is not discussed in detail here as it is beyond the scope of this work. Nonetheless, QCLAS I achieved Allan deviations of ~0.4 ‰ at 300 s averaging time for $\delta^{15}\text{N}^{\alpha}$ and $\delta^{15}\text{N}^{\beta}$ at ambient N₂O mole fractions when this correction method was applied by ARI.

At [N₂O] of 1000 ppb, the precision of δ values measured by all analyzers, except CRDS I, significantly improved due to greater signal-to-noise ratios. Whilst the performance of OA-ICOS I was similar to that of CRDS II for $\delta^{15}\text{N}^{\alpha}$ and $\delta^{15}\text{N}^{\beta}$ (0.24‰ and 0.24‰ for CRDS II; 0.28‰ and 0.37‰ for OA-ICOS I at 300 s averaging time), CRDS II displayed the best precision for $\delta^{18}\text{O}$ (0.21‰ at 300 s averaging time). Also notable was the improved performance of the 2018 model (CRDS II) compared to the 2015 model (CRDS I). QCLAS analyzers showed the best 1 s precision for δ values, but beyond 100 s, δ -measurements were still heavily affected by instrumental drift resulting in lower precision, especially for QCLAS I. When the spectral correction method described in Supplementary Material 5 was applied, QCLAS I achieved Allan deviations of ~0.2 ‰ at 300 s averaging time for $\delta^{15}\text{N}^{\alpha}$ and $\delta^{15}\text{N}^{\beta}$ at 1000 ppb N₂O.

At [N₂O] of 10000 ppb all analyzers showed excellent precision, with QCLAS I, II and III outperforming OA-ICOS I for precision of $\delta^{15}\text{N}^{\alpha}$ and $\delta^{15}\text{N}^{\beta}$ (collectively better than 0.10 ‰ at 300 s averaging time for both $\delta^{15}\text{N}^{\alpha}$ and $\delta^{15}\text{N}^{\beta}$). QCLAS II had the best precision for [N₂O] (1.2 ppb at 300 s averaging time). OA-

ICOS I and QCLAS III were the only analyzers tested in this study that could be used to measure $\delta^{18}\text{O}$ at 10000 ppb N_2O . OA-ICOS I attained a precision of 0.17 ‰, while QCLAS III attained a precision of 0.48 ‰, both with 300 s averaging time. QCLAS I achieved Allan deviations of $\sim 0.02 - 0.03$ ‰ at 300 s averaging time for $\delta^{15}\text{N}^\alpha$ and $\delta^{15}\text{N}^\beta$ at 10000 ppb N_2O when the spectral correction method (Supplementary Material 5) was applied.

The precision of instruments on $[\text{N}_2\text{O}]$ measurements at 1000 and 10000 ppb N_2O might not be representative because of small fluctuations in the final gas mixture produced by the MFCs, which were likely amplified due to the small dilution ratios. Therefore, the indicated $[\text{N}_2\text{O}]$ precisions should be considered as a pessimistic estimate. This was most apparent for the QCLAS and the OA-ICOS analyzers, which showed the highest short-term precision, although this likely applies to all analyzers. Accordingly, the deviation of the Allan variance of mole fraction measurements by QCLAS II and III as well as OA-ICOS I at elevated $[\text{N}_2\text{O}]$ from instrumental white (Gaussian) noise was likely due to uncertainty contributions from MFCs. Therefore, it is likely that the precision of all analyzers for $[\text{N}_2\text{O}]$ measurements is better than shown in Fig. 3 and Table 6. Nonetheless, at 1000 ppb N_2O , QCLAS III showed the best precision for $[\text{N}_2\text{O}]$ ($1.0 \cdot 10^{-1}$ ppb at 300 s averaging time), which was almost one order of magnitude greater than at atmospheric N_2O mole fractions.

Table 6. Key parameters for instrument stability retrieved from Allan variance experiments for $[\text{N}_2\text{O}]$, $\delta^{15}\text{N}^\alpha$, $\delta^{15}\text{N}^\beta$ and $\delta^{18}\text{O}$: precision (1σ) at 300s and 600s averaging times, and daily drift at various N_2O concentrations. 1σ data refers to Allan deviation (square root of Allan variance).

Instrument	1σ N_2O [ppb] (300 s)	1σ N_2O [ppb] (600 s)	N_2O drift [ppb day^{-1}]	1σ $\delta^{15}\text{N}^\alpha$ [‰] (300s)	1σ $\delta^{15}\text{N}^\alpha$ [‰] (600s)	$\delta^{15}\text{N}^\alpha$ drift [‰ day^{-1}]	1σ $\delta^{15}\text{N}^\beta$ [‰] (300s)	1σ $\delta^{15}\text{N}^\beta$ [‰] (600s)	$\delta^{15}\text{N}^\beta$ drift [‰ day^{-1}]	1σ $\delta^{18}\text{O}$ [‰] (300s)	1σ $\delta^{18}\text{O}$ [‰] (600s)	$\delta^{18}\text{O}$ drift [‰ day^{-1}]
326.5 ppb N_2O												
CRDS I	$3.0 \cdot 10^{-2}$	$2.3 \cdot 10^{-2}$	$2.0 \cdot 10^{-2}$	0.41	0.27	0.22	0.45	0.38	0.18	0.46	0.34	0.03
CRDS II	$1.7 \cdot 10^{-2}$	$1.2 \cdot 10^{-2}$	$3.2 \cdot 10^{-2}$	0.32	0.23	$3.5 \cdot 10^{-3}$	0.41	0.31	0.14	0.41	0.28	0.10
OA-ICOS I	$1.7 \cdot 10^{-2}$	$1.3 \cdot 10^{-2}$	$1.5 \cdot 10^{-2}$	1.08	0.82	0.07	0.79	0.52	0.50	1.69	1.14	2.34
QCLAS I	$6.3 \cdot 10^{-2}$	$4.6 \cdot 10^{-2}$	$3.7 \cdot 10^{-2}$	1.24	1.41	6.80	3.45	4.22	15.81	n.d.	n.d.	n.d.
QCLAS I ^a	$2.1 \cdot 10^{-2}$	$2.4 \cdot 10^{-2}$	0.12	0.39	0.37	0.71	0.42	0.55	4.83	n.d.	n.d.	n.d.
QCLAS II	$9.5 \cdot 10^{-3}$	$1.1 \cdot 10^{-2}$	1.00	1.08	1.44	0.20	0.60	0.72	0.05	n.d.	n.d.	n.d.
QCLAS III	$2.5 \cdot 10^{-2}$	$3.6 \cdot 10^{-2}$	0.75	0.81	1.23	0.09	0.78	1.22	0.04	0.97	1.51	0.13
~ 1000 ppb N_2O												
CRDS I	$7.7 \cdot 10^{-1}$	$6.0 \cdot 10^{-1}$	0.29	0.88	0.67	0.67	0.89	0.73	1.39	0.81	0.67	0.32
CRDS II	$2.1 \cdot 10^{-1}$	$1.3 \cdot 10^{-1}$	0.54	0.24	0.20	0.36	0.24	0.18	0.23	0.21	0.13	0.86
OA-ICOS I	$1.7 \cdot 10^{-1}$	$1.2 \cdot 10^{-1}$	1.02	0.28	0.23	0.93	0.37	0.25	0.54	0.67	0.44	0.15
QCLAS I	$3.3 \cdot 10^{-1}$	$2.4 \cdot 10^{-1}$	1.03	0.47	0.61	7.25	0.83	1.11	8.01	n.d.	n.d.	n.d.
QCLAS I ^a	$1.4 \cdot 10^{-1}$	$1.0 \cdot 10^{-1}$	$1.2 \cdot 10^{-3}$	0.19	0.23	0.61	0.20	0.22	0.11	n.d.	n.d.	n.d.
QCLAS II	$2.0 \cdot 10^{-1}$	$2.4 \cdot 10^{-1}$	4.11	0.52	0.49	0.04	0.22	0.19	$4.3 \cdot 10^{-3}$	n.d.	n.d.	n.d.
QCLAS III	$1.0 \cdot 10^{-1}$	$1.6 \cdot 10^0$	1.61	0.81	1.37	0.06	0.72	1.18	0.03	0.38	0.54	0.05
~ 10000 ppb N_2O												
OA-ICOS I	$1.7 \cdot 10^0$	$1.3 \cdot 10^{-3}$	1.30	0.12	0.10	0.12	0.15	0.09	0.54	0.17	0.12	0.35
QCLAS I	$3.3 \cdot 10^0$	$2.3 \cdot 10^0$	3.74	0.06	0.07	1.09	0.09	0.11	0.82	n.d.	n.d.	n.d.
QCLAS I ^a	$4.6 \cdot 10^{-1}$	$3.8 \cdot 10^{-1}$	0.10	0.03	0.03	0.02	0.02	0.03	0.10	n.d.	n.d.	n.d.
QCLAS II	$1.2 \cdot 10^0$	$9.9 \cdot 10^{-1}$	35.1	0.09	0.07	$2.9 \cdot 10^{-3}$	0.09	0.08	$7.0 \cdot 10^{-3}$	n.d.	n.d.	n.d.
QCLAS III	$1.3 \cdot 10^0$	$1.6 \cdot 10^0$	66.1	0.10	0.17	$3.4 \cdot 10^{-3}$	0.10	0.13	$5.8 \cdot 10^{-3}$	0.48	0.65	$2.8 \cdot 10^{-3}$

^{a)} Data re-processed by Aerodyne Research Inc. technicians using an automatic spectral correction method. This method corrects data that was influenced by changing baseline structure. Further information on this method is provided in Supplementary Material 5.

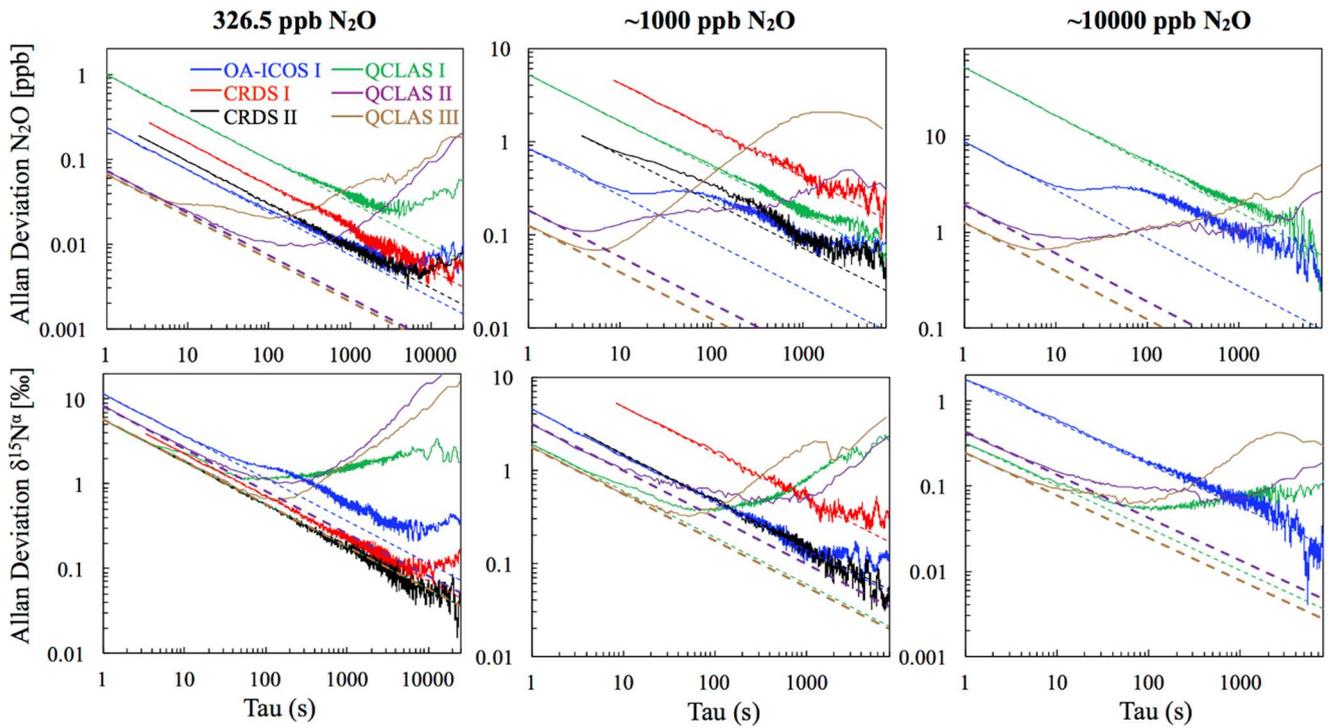


Fig. 3. Allan deviation (square root of Allan Variance) plots for the OA-ICOS I (blue), CRDS I (red), CRDS II (black), QCLAS I (green), QCLAS II (purple) and QCLAS III (brown) at different N_2O mole fractions (~327, 1000 and 10000 ppb). The dashed lines represent a slope of -0.5 (log-log scale) and indicate the expected behavior for Gaussian white noise in each analyzer. The Allan deviations of all analyzers tested were reproducible on three separate occasions prior to the test results presented here. Allan deviation plots for $\delta^{15}\text{N}^\beta$ and $\delta^{18}\text{O}$ are provided in Supplementary Material 4 (Fig. S4-1).

3.2 Temperature effects

All instruments tested showed significant effects, albeit to varying degrees, on their measurements due to the change in laboratory temperature (Figs. 4 and S4-2). The OA-ICOS I displayed no clear temperature effects for $[\text{N}_2\text{O}]$, $\delta^{15}\text{N}^\alpha$ and $\delta^{15}\text{N}^\beta$, but displayed a moderate temperature dependence for $\delta^{18}\text{O}$ measurements (up to 14‰ deviation from the mean), with measurement drift closely paralleling the laboratory temperature ($r^2 = 0.78$). Both CRDS instruments displayed smaller shifts in $[\text{N}_2\text{O}]$ (up to 0.14 ppb deviation from the mean), $\delta^{15}\text{N}^\alpha$, $\delta^{15}\text{N}^\beta$ and $\delta^{18}\text{O}$ that occurred particularly when the laboratory temperature had an acute change. QCLAS I showed a strong temperature dependence on $\delta^{15}\text{N}^\alpha$ ($r^2 = 0.85$) and $\delta^{15}\text{N}^\beta$ ($r^2 = 0.96$).

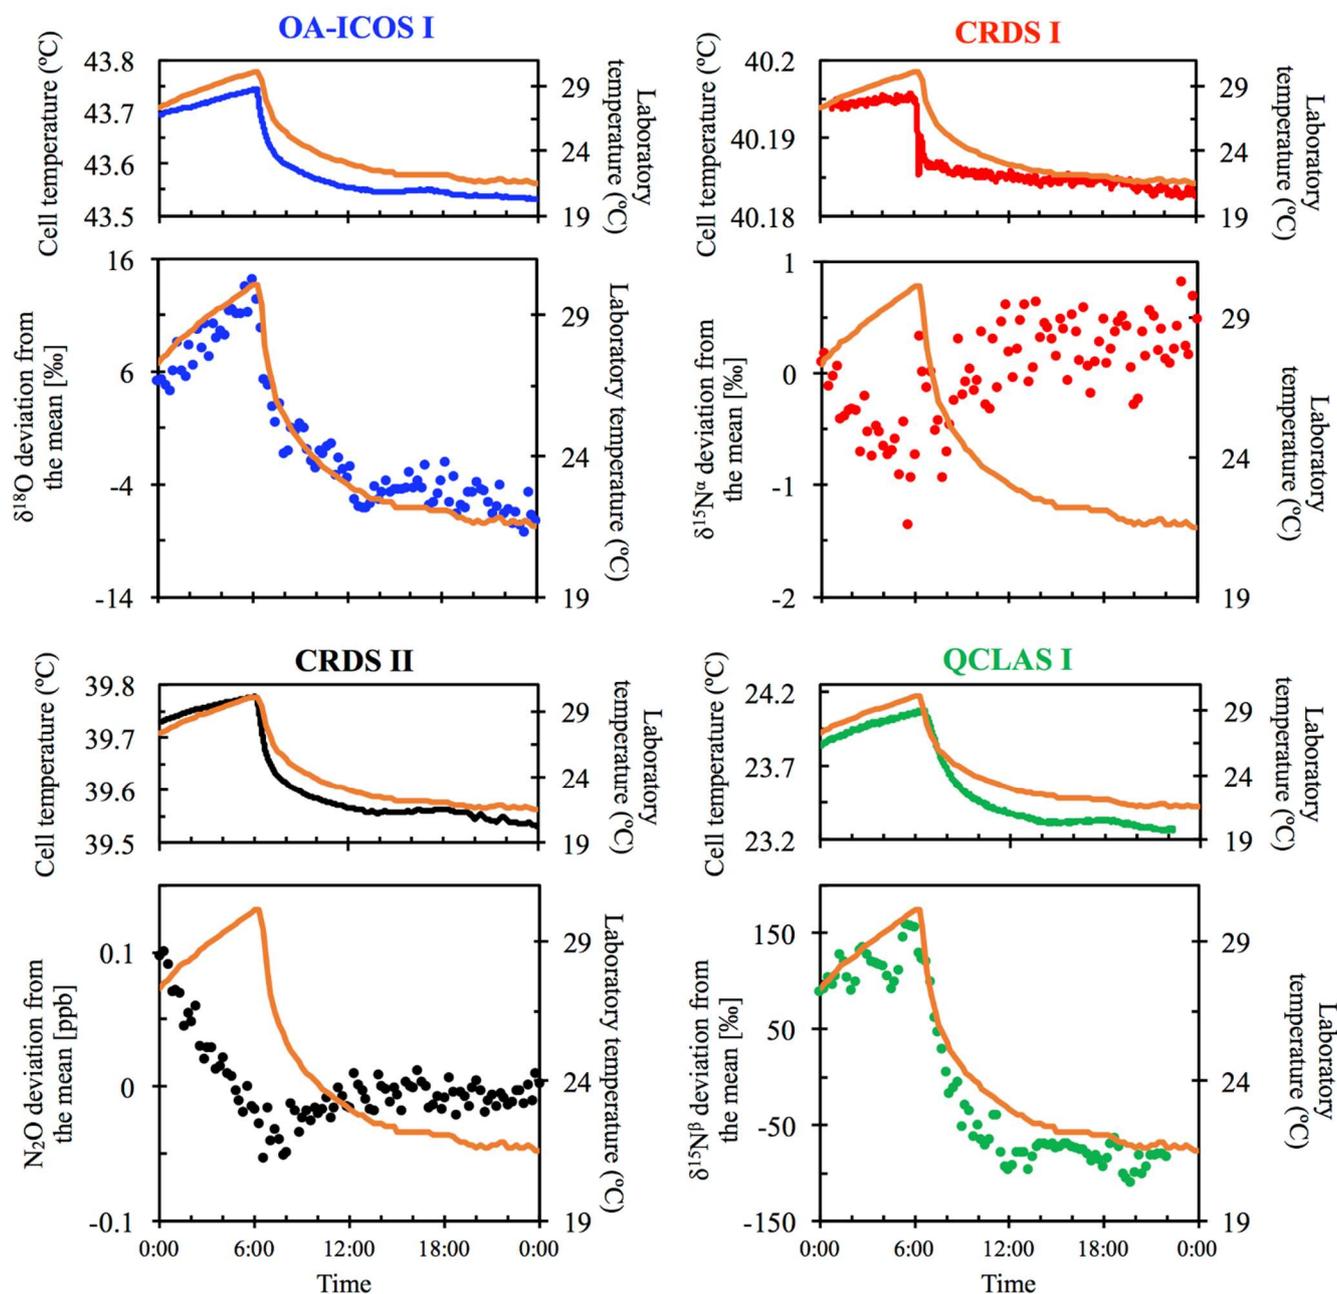


Fig. 4. Examples of the dependency of different measurements on laboratory temperature ($^{\circ}\text{C}$) for OA-ICOS I (blue), CRDS I (red), CRDS II (black) and QCLAS I (green). The complete dataset is provided in Supplementary Material 4 (Fig. S4-2). The laboratory temperature is indicated by a solid orange line and was allowed to vary over time. Cell temperatures for each instrument are also plotted for comparison. The analyzers began acquiring measurements at 00:00 on 8/07/2018, capturing the end of the rising limb of the laboratory temperature. Results are plotted as the deviation from the mean, without any anchoring to reference gases.

3.3 Repeatability

10 The best long-term repeatability for δ values was achieved by TREX-QCLAS I with 0.60 ‰ for $\delta^{15}\text{N}^{\alpha}$, 0.37 ‰ for $\delta^{15}\text{N}^{\beta}$ and 0.46 ‰ for $\delta^{18}\text{O}$, even though measurements were taken over a six-month period (Table 7). The best repeatability without preconcentration was achieved by CRDS analyzers with 0.52 – 0.75 ‰ for CRDS II and 0.79 – 0.83 ‰ for CRDS I for all δ values. OA-ICOS I achieved repeatability between 1 – 2 ‰ (1.47, 1.19 and 2.17 ‰ for $\delta^{15}\text{N}^{\alpha}$, $\delta^{15}\text{N}^{\beta}$ and $\delta^{18}\text{O}$, respectively). QCLAS I isotopic

measurements attained repeatability of 5.4 and 8.6 ‰ for $\delta^{15}\text{N}^{\alpha}$ and $\delta^{15}\text{N}^{\beta}$, respectively. Short-term repeatability results for 10 repeated 15 min measurements periods over 2.5 h are provided in Supplementary Material 6.

Table 7. Summary of the measured $[\text{N}_2\text{O}]$, $\delta^{15}\text{N}^{\alpha}$, $\delta^{15}\text{N}^{\beta}$ and $\delta^{18}\text{O}$ and associated 1σ at 300s averaging times based on repeated measurements of PA1.

Instrument	n	N_2O [ppb]	1σ N_2O [ppb]	$\delta^{15}\text{N}^{\alpha}$ [‰]	1σ $\delta^{15}\text{N}^{\alpha}$ [‰]	$\delta^{15}\text{N}^{\beta}$ [‰]	1σ $\delta^{15}\text{N}^{\beta}$ [‰]	$\delta^{18}\text{O}$ [‰]	1σ $\delta^{18}\text{O}$ [‰]
CRDS I	22	326.66	0.30	15.86	0.79	-2.30	0.83	44.48	0.81
CRDS II	22	326.72	0.26	15.71	0.52	-2.86	0.64	44.40	0.75
OA-ICOS I	22	326.49	0.07	15.29	1.47	-2.11	1.19	44.01	2.17
QCLAS I	22	326.82	0.16	13.92	5.35	-2.97	8.57	-	-
TREX-QCLAS I	28	326.70	1.29	15.72	0.60	-2.82	0.37	44.31	0.46
Empa-assigned values	3	326.51	0.06	15.81	0.07	-3.31	0.004	44.72	0.04

3.4 Dependence of isotopic measurements on N_2O mole fraction

There was an offset in measured δ values resulting from the change in $[\text{N}_2\text{O}]$ introduced to the analyzers (Figs. 5 and S4-3). A linear relationship between $\Delta\delta^{15}\text{N}^{\alpha,\beta}$ and $\Delta\delta^{18}\text{O}$ values with $[1/\text{N}_2\text{O}]$ was observed across all analyzers tested. However, examination of the residuals from the linear regression revealed varying degrees of residual curvature, highlighting that further non-linear terms would be required to adequately describe, and correct for, this mole fraction dependence. Repeated analysis of $[\text{N}_2\text{O}]$ dependencies on consecutive days showed similar trends, indicating that the structure of non-linear effects might be stable over short periods of time. Nevertheless, there were small variabilities in δ values at a given N_2O mole fraction, which could be due to the inherent uncertainty of the measurement and/or day-to-day variations in the mole fraction dependence. The standard deviation of individual 5 min averages of $\delta^{15}\text{N}^{\alpha,\beta}$ and $\delta^{18}\text{O}$ also varied according to the $[\text{N}_2\text{O}]$ measured by each analyzer due to variations in the signal:noise ratio (Supplementary Material 7).

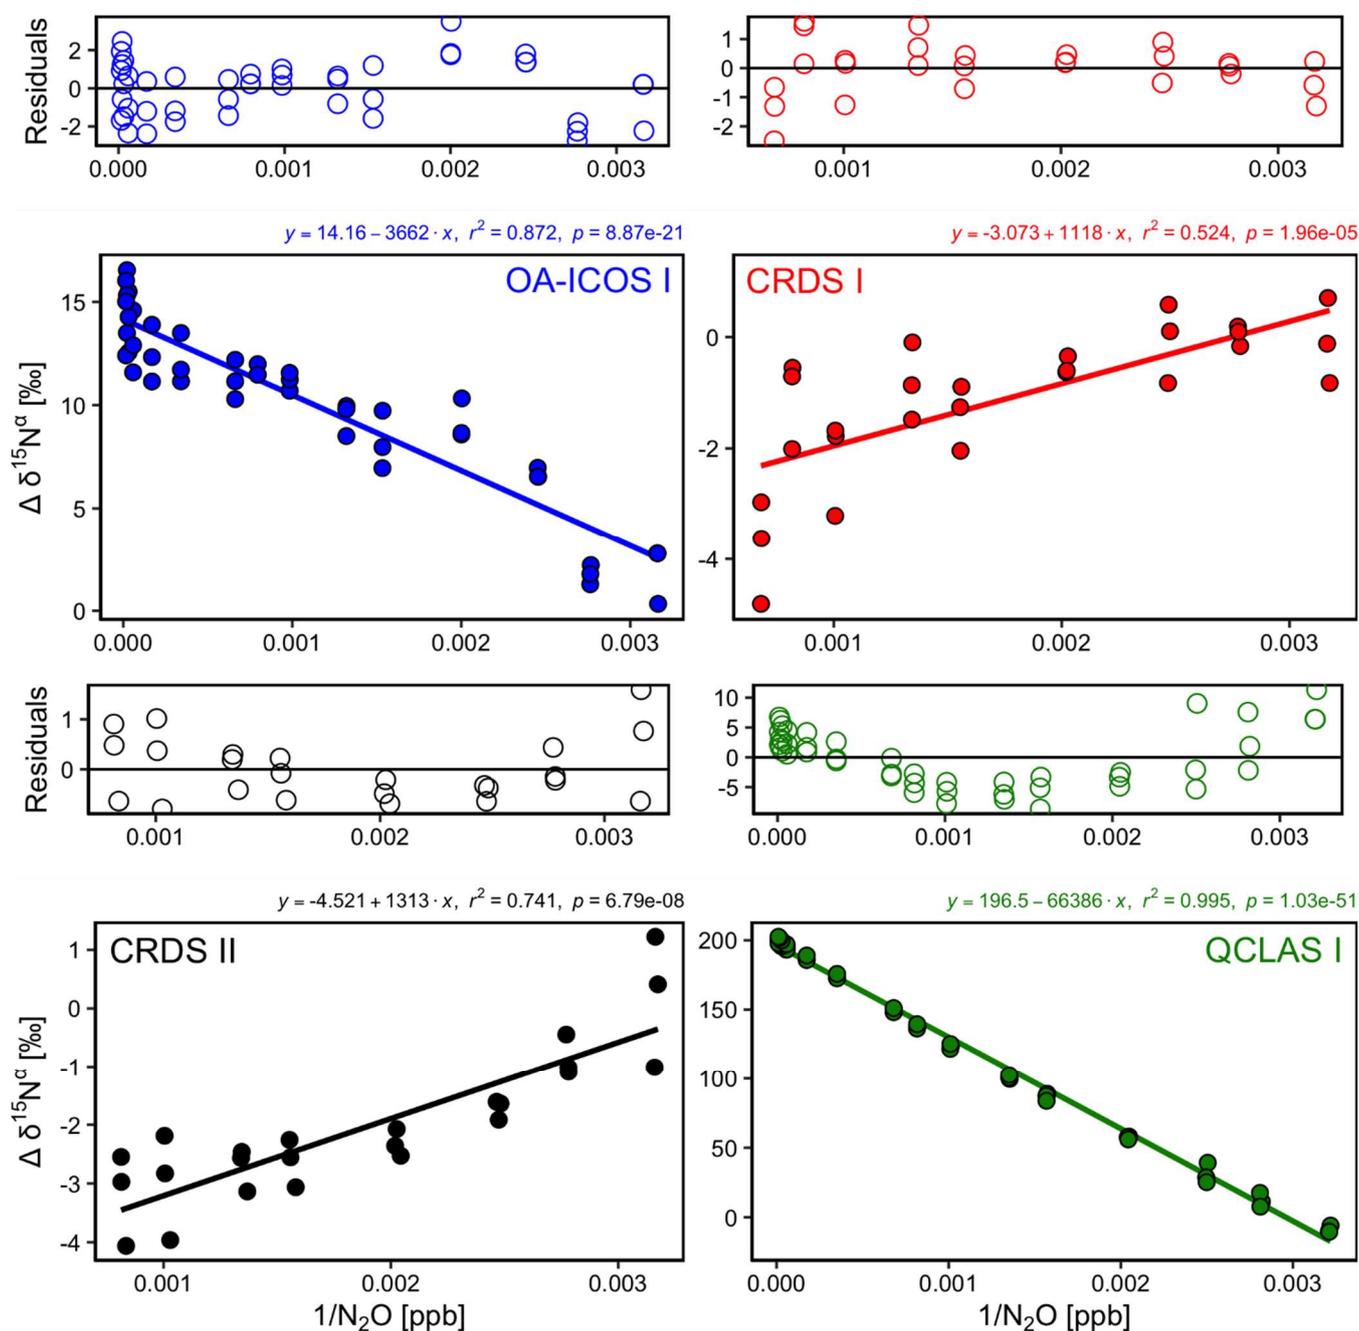


Fig. 5. Deviations of the measured $\delta^{15}\text{N}^\alpha$, $\delta^{15}\text{N}^\beta$ and $\delta^{18}\text{O}$ values according to $1/[\text{N}_2\text{O}]$ for the OA-ICOS I (blue), CRDS I (red), CRDS II (black) and QCLAS I (green). Measurements span the manufacturer-specified operational ranges of the analyzers. The experiment was repeated on three separate days. A linear regression is indicated by the solid line, and a residual plot is provided above each plot. Individual linear equations, coefficients of determination (r^2) and p -values are indicated above each plot. The remaining plots for $\delta^{15}\text{N}^\beta$ and $\delta^{18}\text{O}$ are provided in Supplementary Material 4 (Fig. S4-3).

3.5 Gas matrix effects (O_2 and Ar)

10 3.5.1 Gas matrix effects at ambient N_2O mole fractions

With the exception of TREX-QCLAS I, all instruments displayed strong O_2 dependencies for $[\text{N}_2\text{O}]$ and δ values (Figs. 6 and S4-4). For these instruments, linear regressions best described the offset of measured $[\text{N}_2\text{O}]$ and δ values resulting from the change in O_2 composition of the matrix gas. Importantly, CRDS I

and II displayed different degrees of O₂ interference on [N₂O] and δ values, suggesting that these dependencies were either analyzer-specific or differences were due to hardware/software modifications between different production years. Preconcentration prior to analysis, as performed in TREX-QCLAS I, eliminated O₂ dependencies as the gas matrix was normalized to synthetic air (20.5 % O₂).

5

The change in Ar composition of the matrix gas caused minor, yet measurable, interferences on [N₂O] and δ measurements (Fig. S4-5). The range investigated was between approximately 0 % and 0.95 % Ar, as anticipated for an N₂O in synthetic air (no Ar) reference gas versus a whole air (with Ar) sample gas. The effects observed for 0.95 % change in [Ar] were significantly smaller than that observed for O₂, but might extend to a similar range for sample and reference gases with higher differences in [Ar]. The interference effects were found to be best described by second-order polynomial functions, though we expect that a linear fit would serve equally well if a larger change in [Ar] was investigated. Although most functions to describe the dependence on Ar across all instruments were statistically significant ($p < 0.05$), maximum effects did not transgress the repeatability (1σ) of the Anchor gas measurements. TREX-QCLAS I measurements were not impaired by gas matrix effects.

15

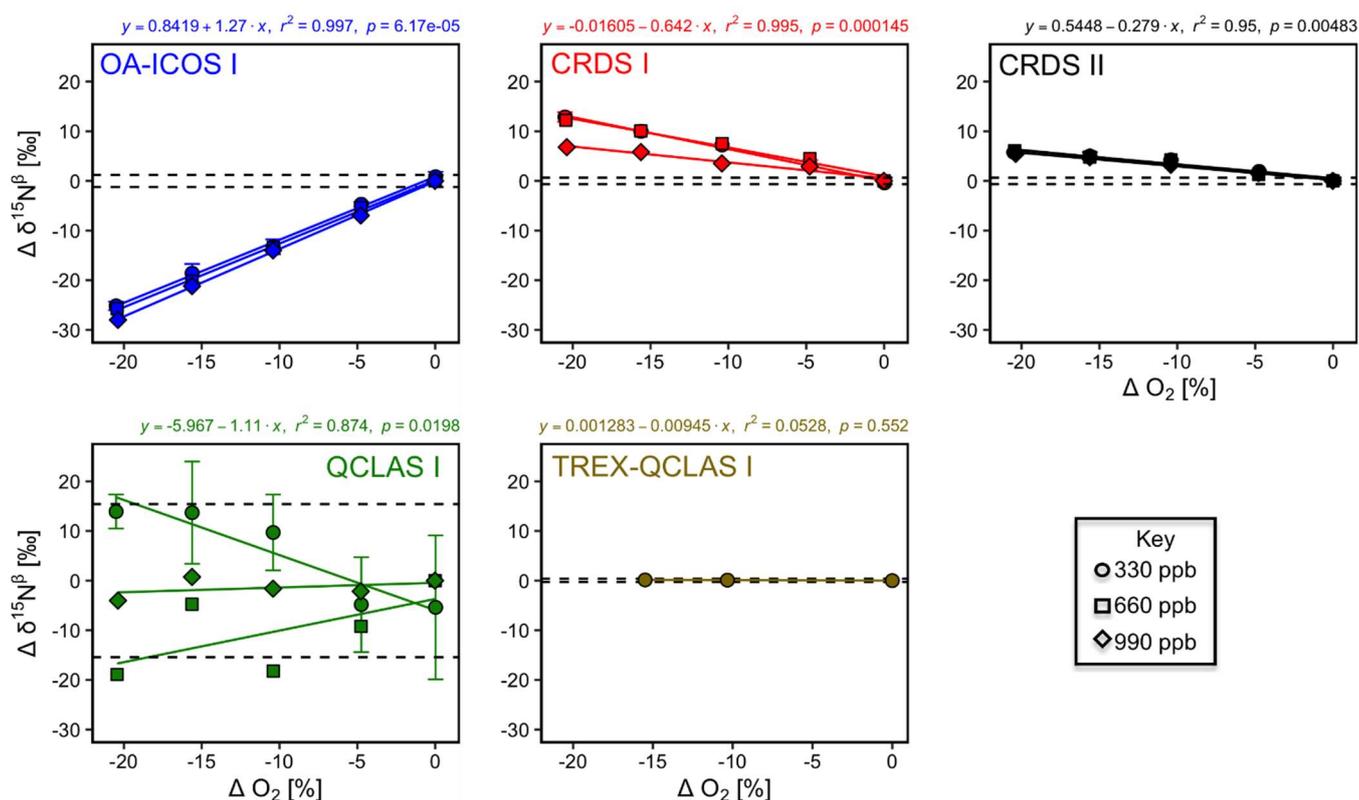


Fig. 6. Deviations of the measured [N₂O], δ¹⁵N^α, δ¹⁵N^β and δ¹⁸O values according to ΔO₂ (%) at different N₂O mole fractions (330, 660 and 990 ppb) for the OA-ICOS I (blue), CRDS I (red), CRDS II (black), QCLAS I (green) and TREX-QCLAS I (brown). The remaining plots for [N₂O], δ¹⁵N^α and δ¹⁸O are provided in Supplementary Material 4 (Fig. S4-4). The standard deviation of the Anchor gas ($\pm 1\sigma$) is indicated by dashed lines. Data points represent the mean and standard deviation (1σ) of triplicate measurements. Dependencies are best-described using linear regression, which are indicated by a solid

20

line. Individual equations, coefficients of determination (r^2) and p -values are indicated above each plot for the 330 ppb N_2O data only.

3.5.2 Continuity of gas matrix corrections at higher N_2O mole fractions

When mole fractions of 660 and 990 ppb N_2O were measured by the laser spectrometers, O_2 interference effects on $[N_2O]$ and δ values were well-described using linear regression, albeit with different slopes to those obtained for 330 ppb N_2O (Figs. 6 and S4-4; Supplementary Material 8).

We could not adequately predict the nature in which the slopes of the interference effects scaled with N_2O mole fractions. Overall, this suggests that interference effects were analyzer-specific and varied according to instrumental-specific parameters, rather than due to *bona fide* scaling of the pressure broadening effect. Therefore, to account for combined effects of $[O_2]$ and $[N_2O]$ changes on measurements, a user would be required to perform a series of laboratory tests across the range of expected $[O_2]$ and $[N_2O]$. In an exemplary approach, we applied a series of empirical equations (Eqs. 5 – 6) to predict the offset of measured $[N_2O]$ and δ values caused by changes in $[O_2]$ as a function of $[N_2O]$ introduced to the analyzers in this study:

$$\Delta[N_2O]_{meas,mix}(\Delta[O_2]_A, [N_2O]_{exp,mix}) = (A \cdot [N_2O]_{exp,mix}^2 + B \cdot [N_2O]_{exp,mix}) \cdot \Delta[O_2]_A \quad (5)$$

$$\Delta\delta_{meas,mix}(\Delta[O_2]_A, [N_2O]_{exp,mix}) = (a \cdot [N_2O]_{exp,mix}^2 + b \cdot [N_2O]_{exp,mix} + c) \cdot \Delta[O_2]_A \quad (6)$$

where $\Delta[N_2O]_{meas,mix}$ and $\Delta\delta_{meas,mix}$ are the measured offsets on $[N_2O]$ and δ values for the gas mixtures introduced to the analyzers as reported in Sect. 3.5.1, respectively; $\Delta[O_2]_A$ is the difference in O_2 mole fraction between the gas mixture and Anchor gas as reported in Sect. 3.5.1; $[N_2O]_{exp,mix}$ is the expected $[N_2O]$ of gas mixtures introduced to the analyzer, calculated based on gas flows and cylinder compositions of Gases 1, 2 and 3 as reported in Sect. 2.4.5; A and B, and a, b and c are analyzer-specific constants.

25

Using Eqs. (5) and (6) to fit values for the constants A and B for $\Delta[N_2O]_{meas,mix}$, and a, b and c for $\Delta\delta_{meas,mix}$ resulted in a total of 11 analyzer-specific values (Supplementary Material 8). With gas-specific constants established, interferences on $[N_2O]$ and δ measurements for a sample gas G for a given analyzer can be corrected using Eqs. (7–8):

$$[N_2O]_{mc,G} = \frac{-(1+B \cdot \Delta[O_2]_G) + \sqrt{(1+B \cdot \Delta[O_2]_G)^2 + 4 \cdot A \cdot \Delta[O_2]_G \cdot [N_2O]_{meas,G}}}{2 \cdot A \cdot \Delta[O_2]_G} \quad (7)$$

$$\delta_{mc,G} = \delta_{meas,G} - (a \cdot [N_2O]_{mc,G}^2 + b \cdot [N_2O]_{mc,G} + c) \cdot \Delta[O_2]_G \quad (8)$$

where $[N_2O]_{mc,G}$ and $\delta_{mc,G}$ are the matrix-corrected $[N_2O]$ and δ values of sample gas G, respectively; $\Delta[O_2]_G$ is the difference in O_2 mole fraction between sample gas G and reference gases. Correction using

Eqs. (7–8) removes the O₂ effect to a degree that corrected measurements from Sect. 3.5.1 are typically within the uncertainty bounds of the anchor (Supplementary Material 8).

Although Ar effects seemingly scaled with increased N₂O mole fractions, we did not derive scaling coefficients for Ar because the derived Ar correction equations at 330, 660 and 990 ppb N₂O were typically not statistically significant at $p < 0.05$. These interferences also did not always exceed the repeatability of Anchor gas measurements. Although we could have tested for effects for [Ar] changes greater than 0.95%, we limited our experiments to [Ar] expected in tropospheric samples.

3.6 Trace gas effects (H₂O, CO₂, CH₄ and CO)

10 3.6.1 Trace gas effects at ambient N₂O mole fractions


The apparent offset of [N₂O] and δ values resulting from the change in CO₂ composition of the matrix gas were best described by linear functions (Figs. 7 and S4-6). OA-ICOS I exhibited discrete and well-defined linear interference effects of CO₂ on [N₂O], $\delta^{15}\text{N}^{\alpha}$, $\delta^{15}\text{N}^{\beta}$ and $\delta^{18}\text{O}$ (all $r^2 > 0.95$), likely due to crosstalk between CO₂ absorption lines situated near 2192.46 cm⁻¹ and 2192.33 cm⁻¹. Both CRDS instruments showed CO₂ interference effects of smaller magnitude for [N₂O], $\delta^{15}\text{N}^{\alpha}$ and $\delta^{18}\text{O}$, presumably due to CO₂ absorption lines at 2196.21 cm⁻¹, 2195.72 cm⁻¹ and 2196.02 cm⁻¹. QCLAS I displayed less well-defined CO₂ interference effects for $\delta^{15}\text{N}^{\beta}$, which was possibly due to several overlapping absorption lines of CO₂ located near 2187.85 cm⁻¹. All linear functions derived for the TREX-QCLAS I were not statistically significant at $p < 0.05$. As shown in Figs. 7 and S4-6, the NaOH trap was effective in removing the CO₂ effect (if present) across the mole fraction ranges tested for all instruments.

Similarly, CH₄ effects on apparent [N₂O] and δ values were well-described by linear functions (Figs. 8 and S4-7). The largest effects were for CRDS I and II, which both displayed strong CH₄ dependencies for $\delta^{15}\text{N}^{\alpha}$ and $\delta^{18}\text{O}$ of similar magnitude. This might be due to crosstalk of ¹⁴N¹⁵N¹⁶O and ¹⁴N¹⁴N¹⁸O absorption lines with the respective CH₄ lines located at 2195.76 cm⁻¹ and 2195.95 cm⁻¹. For OA-ICOS I, minor CH₄ effects were observed for $\delta^{15}\text{N}^{\beta}$, due to absorption line overlap at 2192.33 cm⁻¹. QCLAS I did not display any CH₄ interference effect over the tested [CH₄] range. Linear functions derived for the TREX-QCLAS I were not statistically significant at $p < 0.05$. The similarity between the [N₂O] dependencies on CH₄ mole fractions for OA-ICOS I, CRDS I, II and QCLAS I suggests that the apparent effects may be due to small fluctuations in the gas mixtures produced by the MFCs, rather than a discrete spectral interference effect.

The CRDS analyzers showed minor interference effects for $\delta^{15}\text{N}^{\alpha}$ and $\delta^{15}\text{N}^{\beta}$ on [CO] (0.14 – 2.14 ppm) (Fig. S4-8), likely due to crosstalk with CO absorption lines located at 2195.69 cm⁻¹ and 2195.83 cm⁻¹.


The magnitude of these effects was similar for both models. QCLAS I displayed interference effects for $\delta^{15}\text{N}^\alpha$ and $\delta^{15}\text{N}^\beta$ caused by a CO absorption line located near 2187.9 cm^{-1} , although this effect did not exceed the repeatability of the Anchor gas (containing no CO) over the measurement range. The effects of [CO] on δ values acquired using OA-ICOS I and TREX-QCLAS I were not statistically significant at $p < 0.05$. Similar to CH_4 , the resemblance of [CO] effects on $[\text{N}_2\text{O}]$ measurements for OA-ICOS I, CRDS I, II and QCLAS I suggests that the apparent effects may be due to inaccuracies in the dynamic dilution process, rather than a discrete spectral interference effect. The Sofnocat trap was effective in removing CO (if present) across the mole fraction ranges tested for all instruments.

10 OA-ICOS I exhibited large effects of $[\text{H}_2\text{O}]$ (0 – 13800 ppm) on $\delta^{15}\text{N}^\beta$ (up to -10 ‰) and $\delta^{18}\text{O}$ (up to -15 ‰), and minor dependencies for $\delta^{15}\text{N}^\alpha$ (up to 4 ‰) and $[\text{N}_2\text{O}]$ (up to 1 ppb) across the range tested (Fig. S4-9). For QCLAS I, the H_2O effect was largest for $\delta^{15}\text{N}^\alpha$ (up to 20 ‰), whilst minor effects for $[\text{N}_2\text{O}]$ (up to 2 ppb) were observed in relation to the Anchor gas (no H_2O). In contrast, both CRDS instruments showed no significant effects across the range tested, which is attributable to the installation of permeation
15 dryers inside the analyzers by the manufacturer.

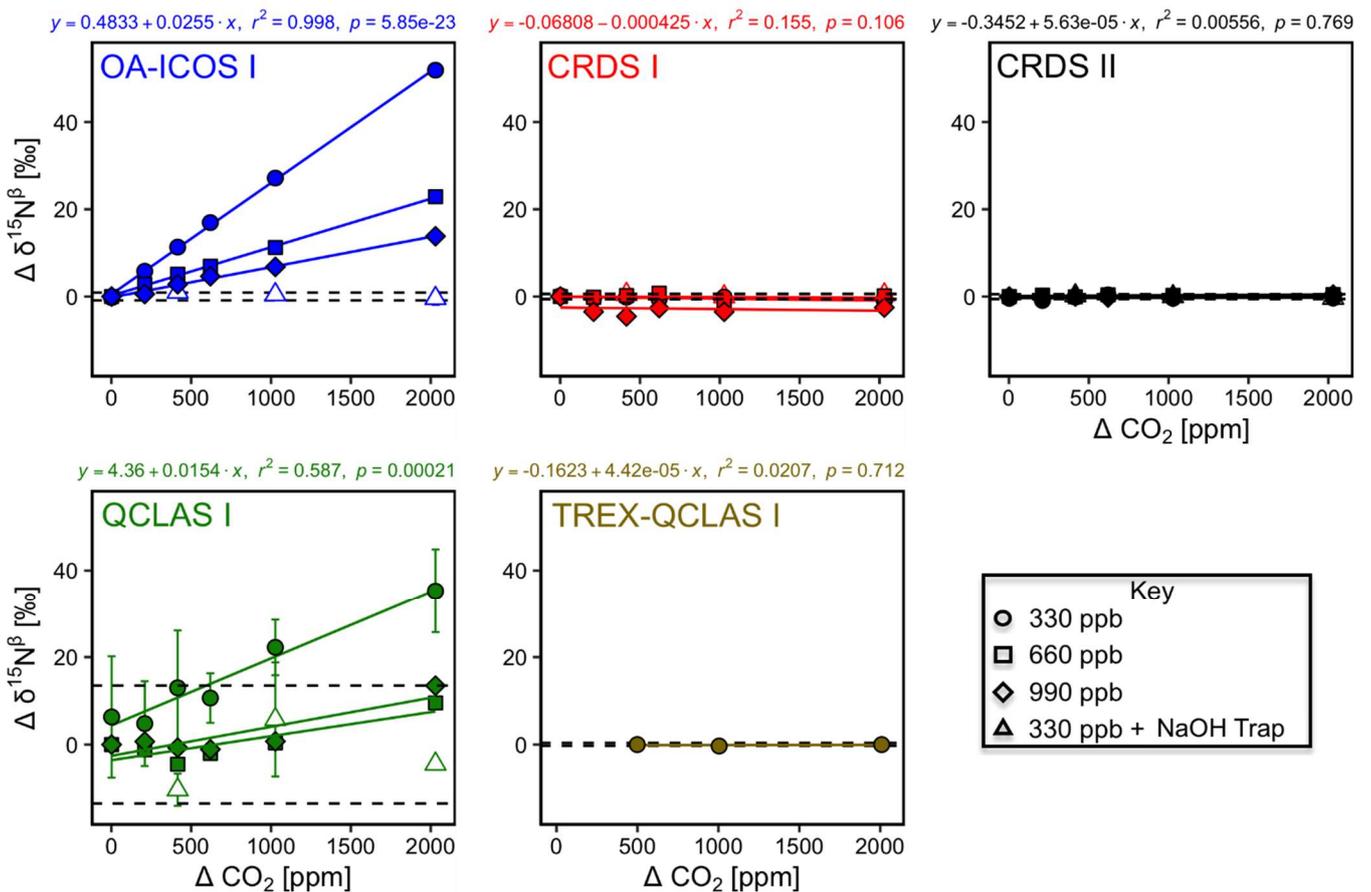

20 **Fig. 7.** Deviations of the measured $[\text{N}_2\text{O}]$, $\delta^{15}\text{N}^\alpha$, $\delta^{15}\text{N}^\beta$ and $\delta^{18}\text{O}$ values according to ΔCO_2 (ppm) at different N_2O mole fractions (330, 660 and 990 ppb) for the OA-ICOS I (blue), CRDS I (red), CRDS II (black), QCLAS I (green) and TREX-QCLAS I (brown). The remaining plots for $[\text{N}_2\text{O}]$, $\delta^{15}\text{N}^\alpha$ and $\delta^{18}\text{O}$ are provided in Supplementary Material 4 (Fig. S4-6). The standard deviation of the Anchor gas ($\pm 1\sigma$) is indicated by dashed lines. Data points represent the mean and standard deviation (1σ) of triplicate measurements. Dependencies are best-described by linear fits, which are indicated by solid lines.

Individual equations, coefficients of determination (r^2) and p -values are indicated above each plot for the 330 ppb N_2O data only.

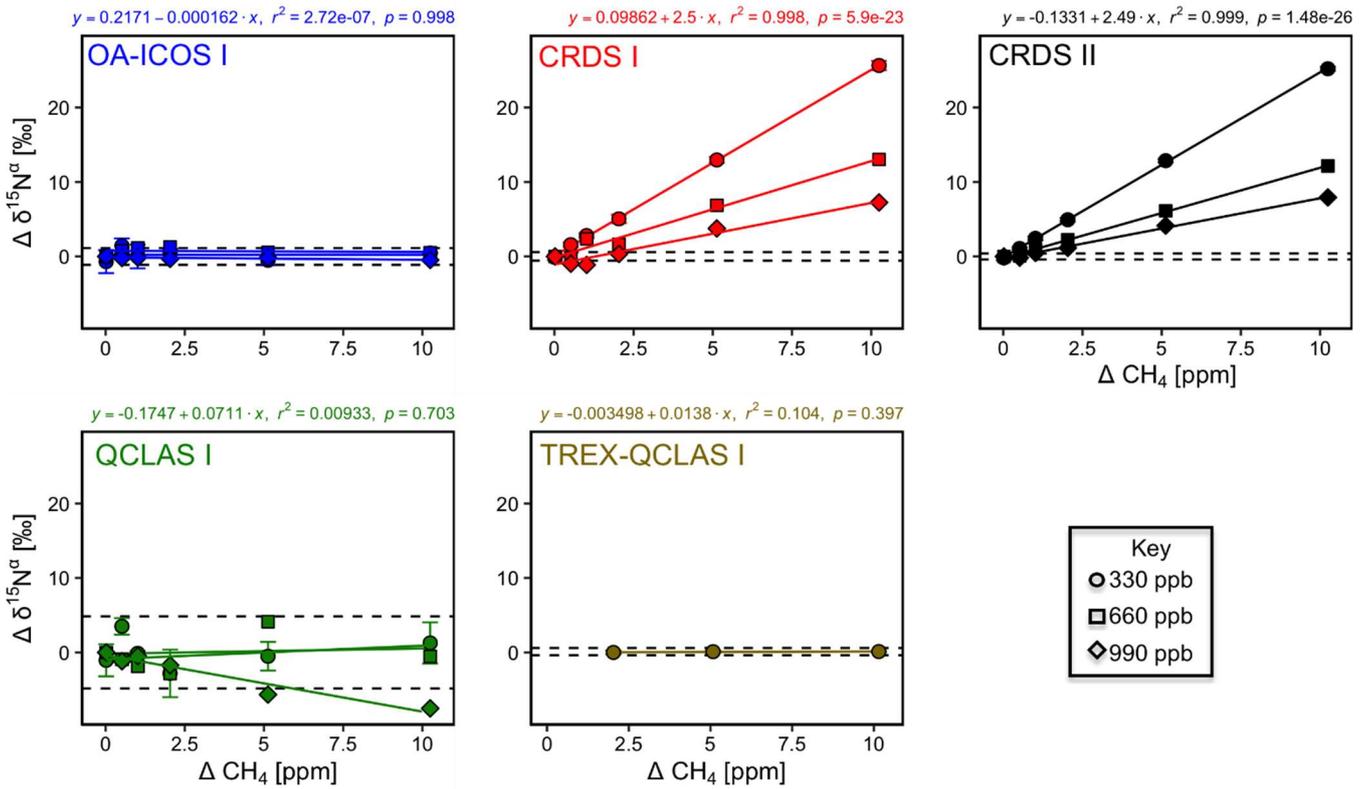

5 **Fig. 8.** Deviations of the measured $[N_2O]$, $\delta^{15}N^\alpha$, $\delta^{15}N^\beta$ and $\delta^{18}O$ values according to ΔCH_4 (ppm) at different N_2O mole fractions (330, 660 and 990 ppb) for the OA-ICOS I (blue), CRDS I (red), CRDS II (black), QCLAS I (green) and TREX-QCLAS I (brown). The remaining plots for $[N_2O]$, $\delta^{15}N^\beta$ and $\delta^{18}O$ are provided in Supplementary Material 4 (Fig. S4-7). Data points represent the mean and standard deviation (1σ) of triplicate measurements. Dependencies are best-described by linear fits, which are indicated by solid lines. Individual equations, coefficients of determination (r^2) and p -values are indicated above each plot for the 330 ppb N_2O data only.

3.6.2 Continuity of trace gas corrections at higher N_2O mole fractions

Interference effects from CO_2 , CH_4 and CO on apparent δ values, where significant, inversely scaled with increasing $[N_2O]$ (Figs. 7, 8, S4-8 and Supplementary Material 8). The scaling of trace gas effects can be explained by simple spectral overlap of the $^{14}N^{15}N^{16}O$, $^{15}N^{14}N^{16}O$ and $^{14}N^{14}N^{18}O$ lines with those of the trace gas, which results in the interference effects being inversely proportional to the mixing ratio of N_2O . However, there may be additional spectral overlap between the trace gas and the $^{14}N^{14}N^{16}O$ peak resulting in an offset for the measured $[N_2O]$, which introduces a further shift in the δ values (as shown in Sect. 3.4). The effect on the apparent $[N_2O]$ was less clear and was possibly confounded by inaccuracies during dynamic gas mixing. In this study, the scaling of interference effects from trace gases as a function of the $[N_2O]$ introduced to the analyzers could be described using Eqs. (9) and (10):

$$\Delta[N_2O]_{meas,mix}(\Delta[x]_A, [N_2O]_{exp,mix}) = \left(A_x \frac{1}{[N_2O]_{exp,mix}} + B_x \right) \cdot \Delta[x]_A \quad (9)$$

$$\Delta\delta_{meas,mix}(\Delta[x]_A, [N_2O]_{exp,mix}) = \left(a_x * \frac{1}{[N_2O]_{exp,mix}} + b_x \right) \cdot \Delta[x]_A \quad (10)$$

where $\Delta[N_2O]_{meas,mix}$ and $\Delta\delta_{meas,mix}$ are the measured offsets on $[N_2O]$ and δ values for the gas mixtures introduced to the analyzers as reported in Sect. 3.6.1, respectively; $\Delta[x]_A$ is the difference in trace gas mole fraction between the gas mixture and Anchor gas as reported in Sect. 3.6.1; and $A_x, B_x,$
 5 a_x and b_x are constants that are trace gas and instrument specific. The constant b_x only occurs when there is spectral overlap from the trace gas and $^{14}N^{14}N^{16}O$ absorption lines.

For a sample gas G, the effect can then be corrected by using Eq. (11) and Eq. (12):

$$[N_2O]_{tc,G} = [N_2O]_{meas,G} - \sum_x \left(\left(A_x \frac{1}{[N_2O]_{meas,G}} + B_x \right) \cdot \Delta[x]_G \right) \quad (11)$$

$$10 \quad \delta_{tc,G} = \delta_{meas,G} - \sum_x \left(\left(a_x \frac{1}{[N_2O]_{meas,G}} + b_x \right) \cdot \Delta[x]_G \right) \quad (12)$$

In Eqs. (11–12), the sum of the effect of all interfering gases with overlapping absorption lines is taken into account. Similar to Section 3.5.2, correction using Eqs. (11–12) removes the trace gas interference effects to the extent that corrected measurements from Sect. 3.6.1 are within the repeatability bounds of the Anchor gas (Supplementary Material 8). Similar inverse relationships have been described by
 15 Malowany et al. (2015) for H_2S interferences on $\delta^{13}C-CO_2$.

3.7 Two end-member mixing

Results for the two end-member mixing experiment were evaluated in two different ways. First, results for individual gas mixtures acquired by laser spectroscopy and GC-IRMS were compared to expected
 20 $[N_2O]$ and δ values calculated from N_2O mole fractions and isotopic composition of end-members and mixing fractions. Second, source values were extrapolated using a weighted total least squares regression analysis, known as Keeling plot analysis (Keeling, 1958), and compared to assigned δ values of the *source* gas used in each experiment.

3.7.1 Comparison with expected $[N_2O]$ and δ values

25 Triplicate measurements (mean $\pm 1\sigma$) obtained using the laser spectrometers and GC-IRMS were plotted against expected $[N_2O]$ and δ values calculated using MFC flow rates, N_2O mole fractions and isotopic composition of *background* and *source* gases (Figs. 12-15). Comparisons between individual laser spectrometer measurements and GC-IRMS are plotted in Supplementary Material 9, and are discussed only briefly below.

OA-ICOS I

Generally, there was good agreement of $[\text{N}_2\text{O}]$ between the OA-ICOS I and expected values, although the analyzer over-estimated mole fractions at higher $\Delta\text{N}_2\text{O}$ during experiments 5 and 6. There was excellent agreement between the OA-ICOS I and calculated expected δ values (all $r^2 > 0.95$; Figs. 9 and 5 S4-10). Measurements for $\delta^{15}\text{N}^\alpha$ were mostly within ± 2.4 ‰ of expected values, while $\delta^{15}\text{N}^\beta$, $\delta^{15}\text{N}^{\text{bulk}}$ and SP were all within ± 2 ‰ of expected values. $\delta^{18}\text{O}$ measurements were the poorest performing, but were typically within ± 3.6 ‰ of expected values. Similarly, there was excellent agreement between OA-ICOS I and IRMS isotope values (all $r^2 > 0.95$), which agreed within 1.7–2.4 ‰ (Fig. S9-2). The standard deviations of triplicate isotope measurements decreased dramatically with increasing $\Delta\text{N}_2\text{O}$, improving from 1 – 2 ‰ during experiments 1 and 2 to typically better than 0.1 ‰ during experiments 5 and 6. Conversely, the standard deviations of triplicate sample measurements for $[\text{N}_2\text{O}]$ increased with increasing $\Delta\text{N}_2\text{O}$, rising from < 0.1 ppb during experiments 1 through 4, to > 1 ppb during experiments 5 and 6. Nonetheless, all OA-ICOS I $[\text{N}_2\text{O}]$ measurements had better 1σ repeatability than those acquired using GC. The repeatability of the triplicate isotope measurements with OA-ICOS I was typically better than IRMS exclusively at higher $\Delta\text{N}_2\text{O}$ (> 700 ppb).

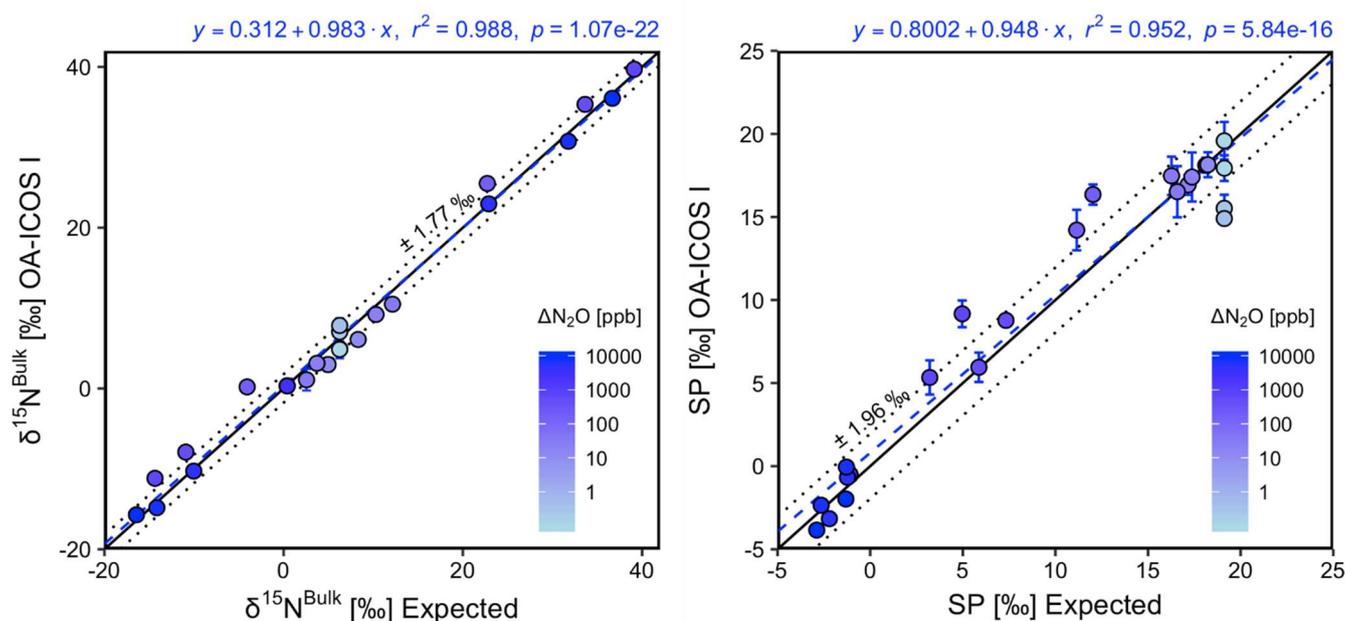


Fig. 9. Correlation diagrams for $\delta^{15}\text{N}^{\text{bulk}}$ and SP measurements at various $\Delta\text{N}_2\text{O}$ mole fractions analyzed by OA-ICOS I plotted against expected values. The remaining plots for $[\text{N}_2\text{O}]$, $\delta^{15}\text{N}^\alpha$, $\delta^{15}\text{N}^\beta$ and $\delta^{18}\text{O}$ are provided in Supplementary Material 4 (Fig. S4-10). The solid black line denotes the 1:1 line, while the dotted line indicates $\pm 1\sigma$ of the residuals from the 1:1 line. The dashed blue line represents a linear fit to the data. Individual equations, coefficients of determination (r^2) and p -values are indicated above each plot. Each data point represents the mean and standard deviation (1σ) of triplicate measurements. The inset plots indicate the standard deviation (1σ) of the triplicate measurements achieved at different $\Delta\text{N}_2\text{O}$ mole fractions, and the 1:1 line is similarly a solid line.

25 CRDS I

$[\text{N}_2\text{O}]$ acquired by CRDS I were in good agreement with expected values, although the analyzer slightly under-estimated mole fractions at higher $\Delta\text{N}_2\text{O}$ during experiments 3 and 4. There was excellent

agreement between the CRDS I and calculated expected isotope values (all $r^2 > 0.95$; Figs. 10 and S4-11). Measurements for $\delta^{15}\text{N}^\alpha$ and $\delta^{15}\text{N}^\beta$ were mostly better than ± 1.1 ‰ of expected values, while $\delta^{15}\text{N}^{\text{bulk}}$ was within ± 0.5 ‰ of expected values. SP and $\delta^{18}\text{O}$ measurements were typically within ± 1.5 ‰ of expected values. There was excellent agreement between CRDS I and IRMS isotope values (all $r^2 > 0.93$), which agreed to within 0.5 – 1.9 ‰ (Fig. S9-3). In general, the standard deviations of triplicate isotope measurements increased as a function of $\Delta\text{N}_2\text{O}$, with the lowest deviations of 0.1–1 ‰ occurring when $\Delta\text{N}_2\text{O} < 100$ ppb. However, two triplicated measurements for $\delta^{15}\text{N}^{\text{bulk}}$ had standard deviations better than 0.1 ‰. The standard deviations of triplicate measurements for $[\text{N}_2\text{O}]$ also increased with increasing $\Delta\text{N}_2\text{O}$ mole fractions, rising from 0.03–0.07 ppb when $\Delta\text{N}_2\text{O} = \sim 0$ ppb (i.e. ambient conditions) to ~ 1 ppb when $\Delta\text{N}_2\text{O} = \sim 700$ ppb. With the exception of one triplicate measurement, all CRDS I $[\text{N}_2\text{O}]$ measurements had better 1σ repeatability than those acquired using GC. Overall, IRMS had slightly better repeatability (most ranging from 0.1 – 1 ‰) than CRDS I (most ranging from 0.1 – 2 ‰) for isotopic measurements.

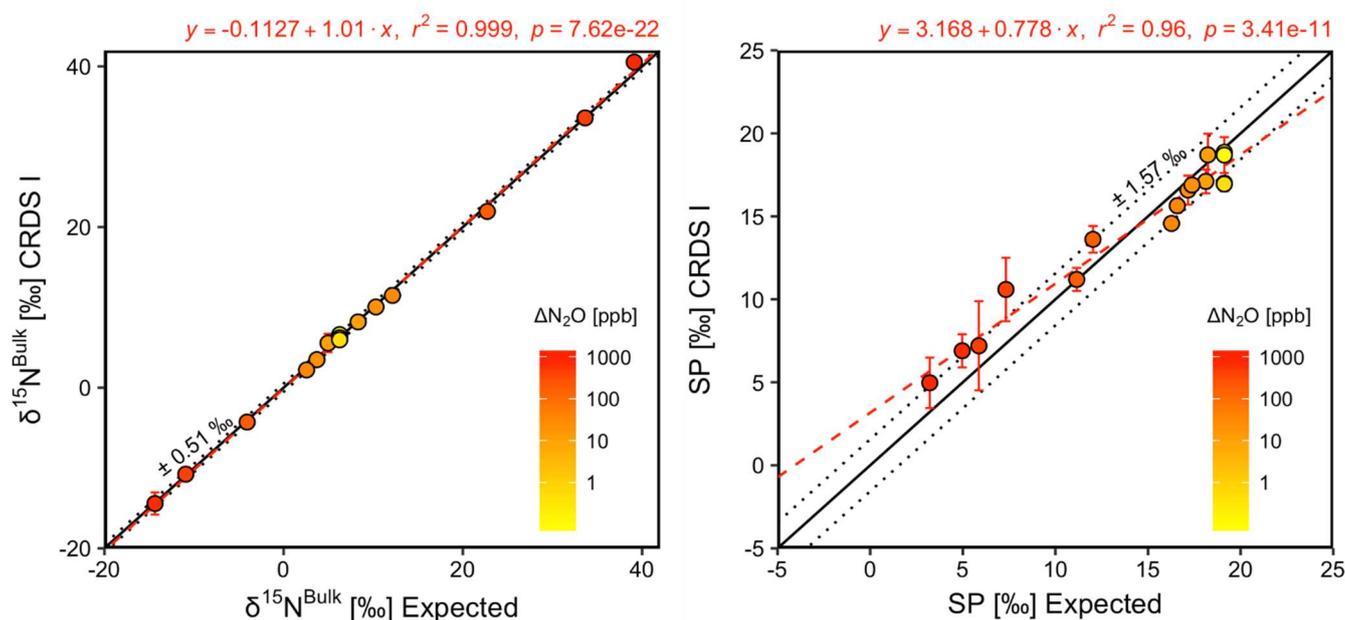


Fig. 10. Correlation diagrams for $\delta^{15}\text{N}^{\text{bulk}}$ and SP measurements at various $\Delta\text{N}_2\text{O}$ mole fractions analyzed by CRDS I plotted against expected values. The remaining plots for $[\text{N}_2\text{O}]$, $\delta^{15}\text{N}^\alpha$, $\delta^{15}\text{N}^\beta$ and $\delta^{18}\text{O}$ are provided in Supplementary Material 4 (Fig. S4-11). The solid black line denotes the 1:1 line, while the dotted line indicates $\pm 1\sigma$ of the residuals from the 1:1 line. The dashed red line represents a linear fit to the data. Individual equations, coefficients of determination (r^2) and p -values are indicated above each plot. Each data point represents the mean and standard deviation (1σ) of triplicate measurements. The inset plots indicate the standard deviation (1σ) of the triplicate measurements achieved at different $\Delta\text{N}_2\text{O}$ mole fractions, and the 1:1 line is similarly a solid line.

CRDS II

Similar to results for CRDS I, $[\text{N}_2\text{O}]$ acquired by CRDS II were in good agreement with expected values but slightly under-estimated mole fractions at higher $\Delta\text{N}_2\text{O}$ during experiments 3 and 4. There was excellent agreement between the CRDS II and calculated expected isotope values (all $r^2 > 0.99$; Figs. 11 and S4-12). Measurements for $\delta^{15}\text{N}^\alpha$ and SP were typically better than ± 0.8 ‰ of expected values, while $\delta^{15}\text{N}^\beta$, $\delta^{15}\text{N}^{\text{bulk}}$ measurements were all within ± 0.4 ‰ of expected values. $\delta^{18}\text{O}$ measurements were within

± 1.0 ‰ of expected values. There was excellent agreement between CRDS II and IRMS isotope values (all $r^2 > 0.98$), which agreed within ± 0.6–1.4 ‰ (Fig. S9-4). The standard deviations of triplicate isotope measurements typically decreased as a function of $\Delta\text{N}_2\text{O}$, with the lowest deviations of <0.1–0.3 ‰ occurring when $\Delta\text{N}_2\text{O} = \sim 700$ ppb. Conversely, the standard deviations of triplicate sample measurements for $[\text{N}_2\text{O}]$ increased with increasing $\Delta\text{N}_2\text{O}$, rising from 0.04–0.09 ppb when $\Delta\text{N}_2\text{O} = \sim 0$ ppb (i.e. ambient conditions) to ~ 0.4 ppb when $\Delta\text{N}_2\text{O} = \sim 700$ ppb. All CRDS II $[\text{N}_2\text{O}]$ measurements had better 1σ repeatability than those acquired using GC. There was no clear distinction between CRDS II and IRMS triplicate repeatability, with both achieving triplicate repeatability ranging from 0.1 to 1 ‰ for most isotopic measurements. However, the repeatability of SP CRDS II measurements was mostly better than IRMS, achieving triplicate repeatability between 0.1–0.6 ‰, compared to 0.2–1 ‰ for IRMS.

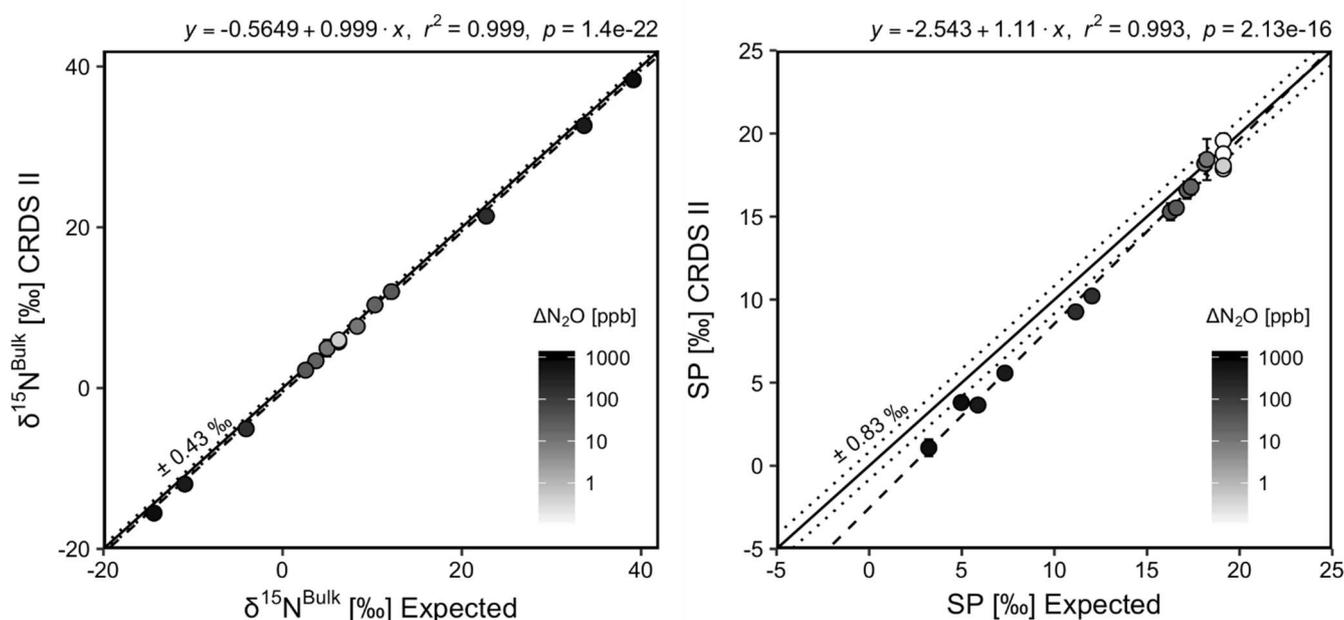


Fig. 11. Correlation diagrams for $\delta^{15}\text{N}^{\text{bulk}}$ and SP measurements at various $\Delta\text{N}_2\text{O}$ mole fractions analyzed by CRDS II plotted against expected values. The remaining plots for $[\text{N}_2\text{O}]$, $\delta^{15}\text{N}^{\alpha}$, $\delta^{15}\text{N}^{\beta}$ and $\delta^{18}\text{O}$ are provided in Supplementary Material 4 (Fig. S4-12). The solid black line denotes the 1:1 line, while the dotted line indicates $\pm 1\sigma$ of the residuals from the 1:1 line. The dashed black line represents a linear fit to the data. Individual equations, coefficients of determination (r^2) and p -values are indicated above each plot. Each data point represents the mean and standard deviation (1σ) of triplicate measurements. The inset plots indicate the standard deviation (1σ) of the triplicate measurements achieved at different $\Delta\text{N}_2\text{O}$ mole fractions, and the 1:1 line is similarly a solid line.

20 QCLAS I

There was good agreement of $[\text{N}_2\text{O}]$ between QCLAS I and expected values, however the analyzer underestimated mole fractions at higher $\Delta\text{N}_2\text{O}$ during experiments 5 and 6. Unfortunately, it is clear from the large spread of isotope values depicted in Fig. 12 that the standardized calibration scheme selected for the two end-member mixing tests was insufficient for acquiring accurate and precise isotopic measurements using QCLAS I. For this reason, we urge researchers not to over-interpret such results, as the implementation of a QCLAS-specific calibration procedure (in-line with results from Sects. 3.1 and 3.3) would improve results dramatically. Nonetheless, QCLAS I obtained accurate results at higher N_2O mole

fractions (indicated in red in Figs. 12 and S4-13), such that when $\Delta N_2O < 700$ ppb measurements were excluded, $\delta^{15}N^\alpha$, $\delta^{15}N^\beta$, $\delta^{15}N^{bulk}$ and SP were within ± 3.0 ‰, 1.4 ‰, 1.4 ‰ and 3.8 ‰ of calculated expected values, respectively. Similarly, QCLAS I showed good agreement with IRMS only at higher $\Delta N_2O (> 700$ ppb; Fig. S9-5). Similar to OA-ICOS I, the standard deviations of QCLAS I triplicate isotope measurements decreased dramatically with increasing ΔN_2O , improving from ~ 10 ‰ during experiments 1 and 2 to typically between 0.1–1 ‰ during experiments 5 and 6. Conversely, the standard deviations of triplicate sample measurements for $[N_2O]$ increased with increasing ΔN_2O , rising from < 0.1 ppb during experiments 1 through 4, to > 1 ppb during experiments 5 and 6. All QCLAS I $[N_2O]$ measurements had better 1σ repeatability than those acquired using GC. QCLAS I had triplicate isotope measurement standard deviations comparable to IRMS only at higher $\Delta N_2O (> 700$ ppb).


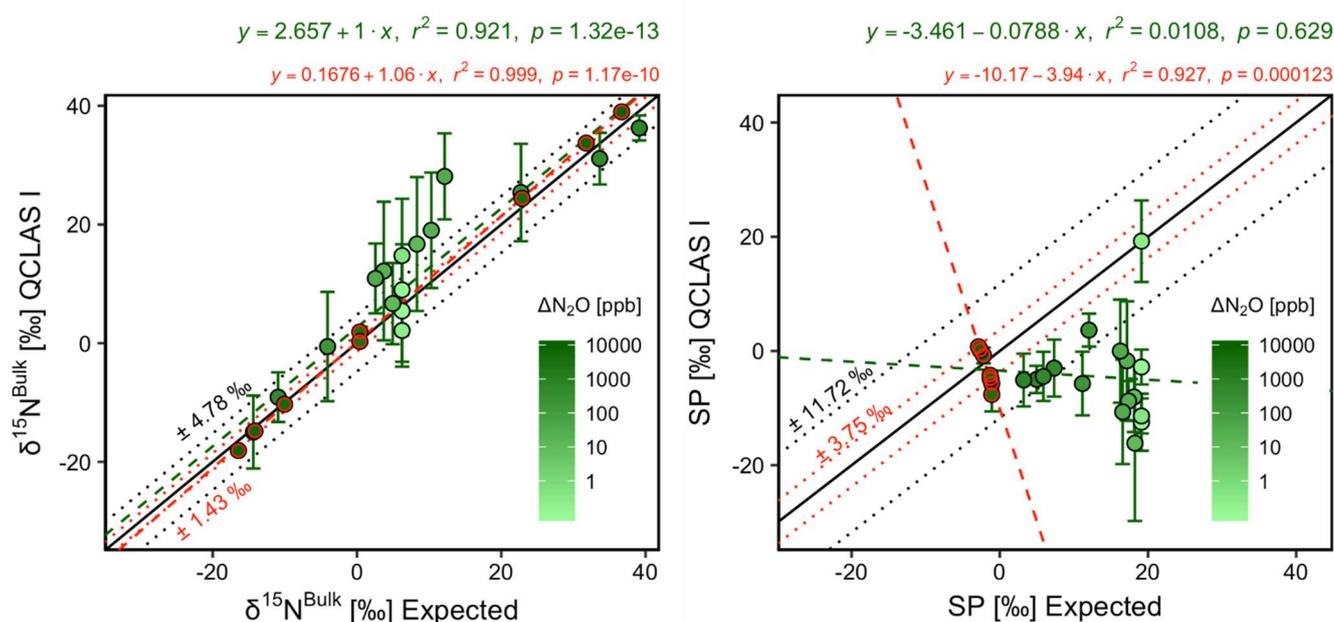


Fig. 12. Correlation diagrams for $\delta^{15}N^{bulk}$ and SP measurements at various ΔN_2O mole fractions analyzed by QCLAS I plotted against expected values. The remaining plots for $[N_2O]$, $\delta^{15}N^\alpha$, $\delta^{15}N^\beta$ and $\delta^{18}O$ are provided in Supplementary Material 4 (Fig. S4-13). The solid black line denotes the 1:1 line, while the dotted line indicates $\pm 1\sigma$ of the residuals from the 1:1 line. The dashed green line represents a linear fit to the data. Individual equations, coefficients of determination (r^2) and p -values are indicated above each plot. Each data point represents the mean and standard deviation (1σ) of triplicate measurements. The inset plots indicate the standard deviation (1σ) of the triplicate measurements achieved at different ΔN_2O mole fractions, and the 1:1 line is similarly a solid line. Results for Exp. 5-6 are highlighted in red, with the dashed red line indicating a linear fit to this data.

TREX-QCLAS I

There was good agreement of N_2O mixing ratios between the TREX-QCLAS I and expected values. Similarly, there was excellent agreement between the TREX-QCLAS I and calculated expected isotope values (all $r^2 > 0.97$; Figs. 13 and S4-14). Measurements for $\delta^{15}N^\alpha$, $\delta^{15}N^\beta$, $\delta^{15}N^{bulk}$ and SP were within ± 0.29 ‰, 0.32 ‰, 0.23 ‰ and 0.41 ‰ of expected values, respectively. $\delta^{18}O$ measurements were typically within ± 0.24 ‰ of expected values. Generally, the standard deviations of triplicate isotope measurements decreased with increasing ΔN_2O , improving from typically 0.2–0.3 ‰ at low ΔN_2O mole fractions

(ambient) to close to or better than 0.1 ‰ when $\Delta\text{N}_2\text{O}$ reached 30 ppb. Conversely, the standard deviations of triplicate sample measurements for $[\text{N}_2\text{O}]$ increased with increasing $\Delta\text{N}_2\text{O}$, rising from < 0.3 ppb to ~ 1 ppb. No comparison could be made between TREX-QCLAS I and IRMS measurements because TREX-QCLAS measurements were undertaken separately from the other instruments.

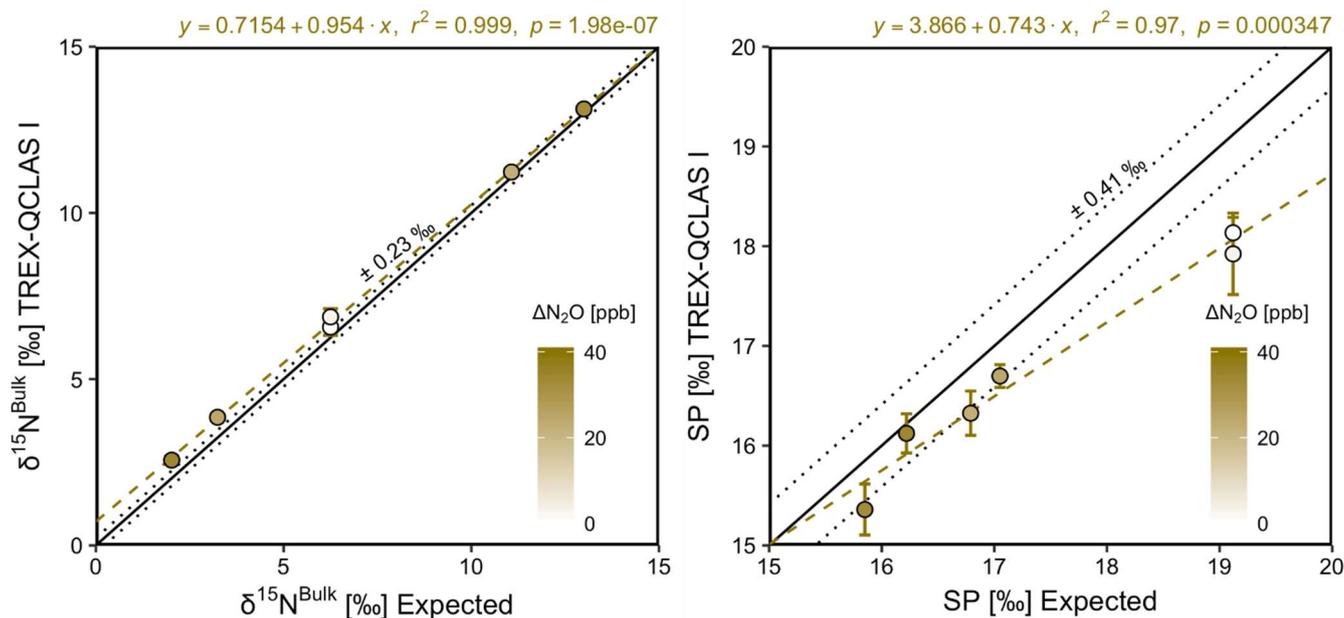

5

Fig. 13. Correlation diagrams for $\delta^{15}\text{N}^{\text{bulk}}$ and SP measurements at various $\Delta\text{N}_2\text{O}$ mole fractions analyzed by OA-ICOS I plotted against expected values. The remaining plots for $[\text{N}_2\text{O}]$, $\delta^{15}\text{N}^{\alpha}$, $\delta^{15}\text{N}^{\beta}$ and $\delta^{18}\text{O}$ are provided in Supplementary Material 4 (Fig S4-14). The solid black line denotes the 1:1 line, while the dotted line indicates $\pm 1\sigma$ of the residuals from the 1:1 line. The dashed green line represents a linear fit to the data. Individual equations, coefficients of determination (r^2) and p-values are indicated above each plot. Each data point represents the mean and standard deviation (1σ) of triplicate measurements. The inset plots indicate the standard deviation (1σ) of the triplicate measurements achieved at different $\Delta\text{N}_2\text{O}$ mole fractions, and the 1:1 line is similarly a solid line.

10


3.7.2 Source identification using Keeling analysis

15 Despite the excellent agreement between expected and measured values across all experiments for OA-ICOS I, CRDS I and II, and TREX-QCLAS I, the extrapolated *source* intercept values acquired using Keeling analysis showed large standard errors, especially for Experiments 1 and 2 ($\Delta\text{N}_2\text{O} = 30$ ppb) (Figs. 14 and S4-15; Supplementary Material 10). This was mostly due to the small mole fraction range (i.e. large inverse mole fraction range) over which the regression line was extrapolated in order to acquire the

20 intercept value. The cause of the erroneous intercept values was likely two-fold: (1) the extrapolated source was highly susceptible to measurements acquired at background levels, and due to the inherent greater uncertainty associated with measurements acquired at ambient N_2O mole fractions, intercepts can be skewed accordingly; and (2) any further non-linearity that could not be taken into account in the three-point concentration dependence correction applied. Overall, this implies that N_2O isotope source studies

25 using laser spectroscopy focusing on near-ambient N_2O variations remain a challenging undertaking, and one should expect large uncertainty in source estimates over small mole fraction changes.

For Experiments 3 through 6, however, the accuracy of the source intercept and its standard error improved dramatically for all analyzers on account of the decreasing uncertainty in measurement. OA-ICOS I and both CRDS analyzers typically achieved within $\pm 2\text{--}5\text{‰}$ of the assigned values for $\delta^{15}\text{N}^\alpha$, $\delta^{15}\text{N}^\beta$, $\delta^{15}\text{N}^{\text{bulk}}$, SP and $\delta^{18}\text{O}$, and had performance comparable to or better than the GC-IRMS approach (Figs. 14 and S4-15). Similarly, the standard error of all intercepts decreased dramatically for Experiments 3 through 6, and all analyzers typically achieved better than $\pm 1\text{‰}$ standard error on derived intercepts in Experiments 5 and 6.

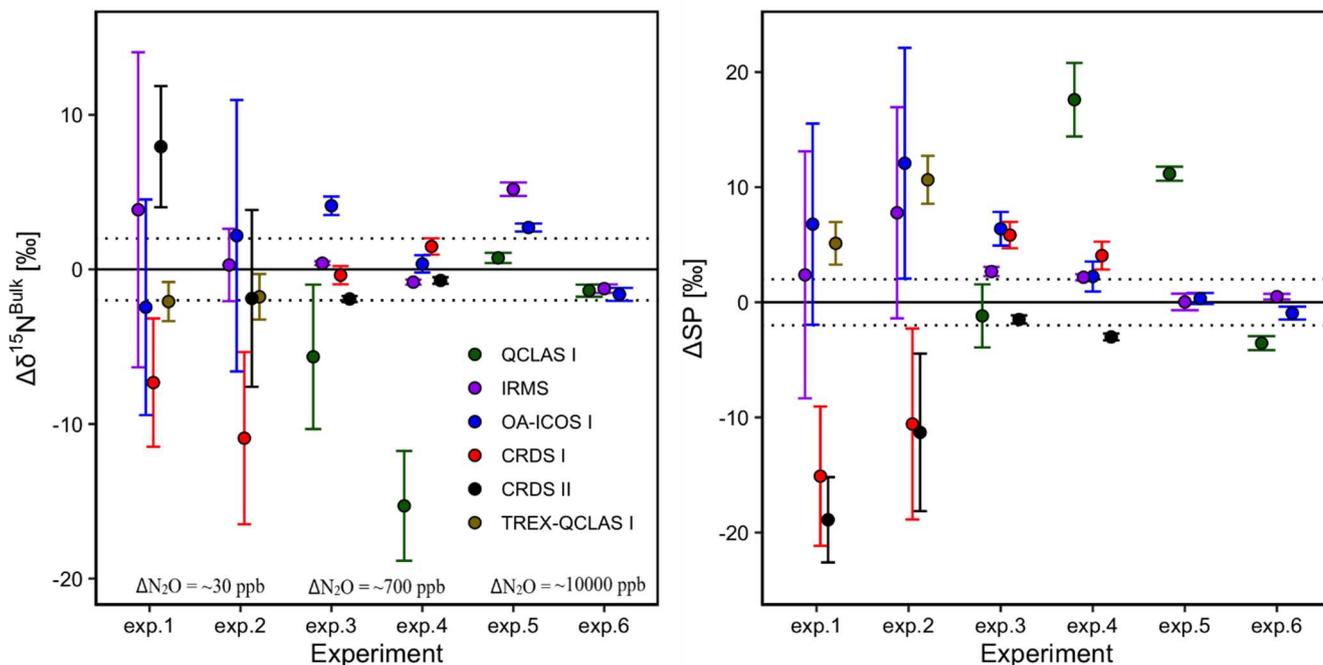

10 **Fig. 14.** $\Delta\delta^{15}\text{N}^{\text{bulk}}$ and ΔSP ($\text{Estimated}_{\text{Source}} - \text{True}_{\text{Source}}$) values derived from the OA-ICOS I (blue), CRDS I (red), CRDS II (black), QCLAS I (green) and IRMS (purple) via Keeling analysis of the two end-member mixing scenario. The remaining plots for $\delta^{15}\text{N}^\alpha$, $\delta^{15}\text{N}^\beta$ and $\delta^{18}\text{O}$ are provided in Supplementary Material 4 (Fig. S4-15). $\text{Estimated}_{\text{Source}} = \text{True}_{\text{Source}}$ is indicated by a solid black line at $y = 0$, and the dotted lines indicated $\pm 2\text{‰}$ deviation from $y = 0$. The change in concentration exceeding that of the background gas is indicated for experiments 1-2 ($\Delta\text{N}_2\text{O} = \sim 30$ ppb), 3-4 ($\Delta\text{N}_2\text{O} = \sim 700$ ppb) and 5-6 ($\Delta\text{N}_2\text{O} = \sim 10000$ ppb). Note: the QCLAS I results for experiments 1 and 2 are not depicted to maintain clarity, as they exceed the selected y-axis scale.

20 4 Discussion

4.1 Factors affecting the precision and accuracy of N_2O isotopocule measurements using laser spectroscopy

A summary of results is presented in Table 8. Our results highlight that the precision at which laser-based analyzers acquire N_2O isotopocule measurements is a function of N_2O mole fraction, the selected measuring and averaging times and calibration frequency according to measurement stability. The degree of accuracy obtained using different laser spectrometers is ultimately a function of the robustness of

corrections aimed at removing matrix and trace gas effects, and the selected calibration procedure aimed at standardizing the data to international scales.

Table 8. Summary of main findings presented in this study.

Detection scheme (model; manufacturer)	OA-ICOS I (N2OIA-30e- EP)	CRDS I & II (G5131-i)	QCLAS I (CW-QC-TILDAS- SC-D)	TREX-QCLAS I (CW-QC-TILDAS- 76-CS)
Allan precision (300 s)				
$\delta^{15}\text{N}^{\alpha}$, $\delta^{15}\text{N}^{\beta}$, $\delta^{18}\text{O}$ [‰]				
326.5 ppb N ₂ O	0.79 – 1.69	0.32 – 0.46	0.39 – 3.45 ^{a)}	n.d.
~ 1000 ppb N ₂ O	0.28 – 0.67	0.21 – 0.89	0.19 – 0.83 ^{a)}	n.d.
~ 10000 ppb N ₂ O	0.12 – 0.17	n.d.	0.02 – 0.48 ^{a)}	n.d.
Repeatability (326.5 ppb N₂O)				
N ₂ O [ppb]	0.07	0.26 – 0.30	0.16	1.29
$\delta^{15}\text{N}^{\alpha}$, $\delta^{15}\text{N}^{\beta}$, $\delta^{18}\text{O}$ [‰]	1.19 – 2.17	0.52 – 0.83	5.35 – 8.57	0.37 – 0.60
Temperature effect (326.5 ppb N₂O)				
N ₂ O [ppb K ⁻¹]	0.01	0.02	0.10	n.d.
$\delta^{15}\text{N}^{\alpha}$, $\delta^{15}\text{N}^{\beta}$, $\delta^{18}\text{O}$ [‰ K ⁻¹]	0.36 – 2.60	0.25 – 0.65	31.29 – 37.32	n.d.
N₂O mole fraction dependence				
$\delta^{15}\text{N}^{\alpha}$, $\delta^{15}\text{N}^{\beta}$, $\delta^{18}\text{O}$ [‰ ppb ($\Delta 1/\text{N}_2\text{O}$)]	-8296 – 2544	-458 – 1353	-66386 – 15833	n.d.
O₂ matrix effect (330 ppb N₂O)				
N ₂ O [ppb % ⁻¹ (ΔO_2)]	-0.044	0.24 – 0.305	0.351	n.s.
$\delta^{15}\text{N}^{\alpha}$, $\delta^{15}\text{N}^{\beta}$, $\delta^{18}\text{O}$ [‰ % ⁻¹ (ΔO_2)]	0.874 – 1.270	-0.279 – (-1.364)	-1.111	n.s.
CO₂ trace gas effects (330 ppb N₂O)				
N ₂ O [ppb ppm ⁻¹ (ΔCO_2)]	0.0011	0.0005	n.s.	n.s.
$\delta^{15}\text{N}^{\alpha}$, $\delta^{15}\text{N}^{\beta}$, $\delta^{18}\text{O}$ [‰ ppm ⁻¹ (ΔCO_2)]	-0.009 – 0.026	n.s. – (-0.0019)	n.s. – 0.0154	n.s.
CH₄ trace gas effects (330 ppb N₂O)				
N ₂ O [ppb ppm ⁻¹ (ΔCH_4)]	n.s. ^{b)}	-0.039 – (-0.056)	n.s. ^{b)}	n.s. ^{b)}
$\delta^{15}\text{N}^{\alpha}$, $\delta^{15}\text{N}^{\beta}$, $\delta^{18}\text{O}$ [‰ ppm ⁻¹ (ΔCH_4)]	0.173	0.085 – 2.50	n.s.	n.s.
CO trace gas effects (330 ppb N₂O)				
N ₂ O [ppb ppm ⁻¹ (ΔCO)]	-0.29	-0.15 – (-0.24)	-0.19	n.s.
$\delta^{15}\text{N}^{\alpha}$, $\delta^{15}\text{N}^{\beta}$, $\delta^{18}\text{O}$ [‰ ppm ⁻¹ (ΔCO)]	n.s.	-0.53 – (-2.41)	n.s. – (-4.04)	n.s.

a) Includes QCLAS I, II and III

b) Likely due to inaccuracies during dynamic dilution (see text for details)

n.d. not determined

n.s. not statistically significant at $p < 0.05$ and/or $r^2 < 0.5$

5 All spectrometers tested displayed temperature effects on isotope measurements, which can be attributed
10 to differences in the lower state energies of the probed N₂O isotopocule lines (Supplementary Material
11) (e.g. Wächter et al. 2008). The temperature sensitivities of all analyzers tested necessitates that,
especially when deployed in the field, they be operated under temperature-controlled conditions (such as
in maintained field stations).

15 The experiments performed in this study were undertaken using a standardized protocol. Calibration was
performed on isotope δ values derived from raw uncalibrated isotopocule amount fractions, thus requiring
[N₂O] dependence corrections. Alternative approaches aimed at calibrating isotopocule amount fractions

prior to deriving δ values were not included in our study, but have the potential to remove the need for this correction (e.g. Wen et al., 2013; Flores et al., 2017; Griffith, 2018) if appropriate reference materials become available. Isotopocule calibration approaches would require a set of N₂O standard gases with high accuracy mole fractions in addition to assigned δ values.

5

All analyzers tested in this study showed significant effects from changing O₂ composition of the gas matrix. Although the magnitude of this effect ultimately varied across the analysers and was dependent on N₂O mixing ratios, the effect of a change in O₂ composition of 20.5 % was typically on the order of 10 to 30 ‰ for δ values. Similar O₂ dependencies have been reported by Erler et al. (2015) for CRDS
10 N₂O isotope laser spectrometers, as well as for CRDS H₂O isotope analyzers (Johnson and Rella, 2017). The underlying reason for this effect is differences in N₂ versus O₂ (and Ar) broadening parameters of the probed N₂O isotopocule lines. In short, the N₂, O₂ (and Ar) broadening parameters depend on rotational quantum numbers of the respective N₂O lines (Henry et al., 1985; Supplementary Material 11). Thus, differences in the rotational quantum numbers for a pair of isotopocules (e.g. ¹⁴N¹⁵N¹⁶O / ¹⁴N¹⁴N¹⁶O)
15 relate to a difference in their N₂, O₂ and Ar broadening parameters. Consequently, differences in the O₂ or Ar content of the sample gas matrix and that of the reference gas affect measured isotope ratios and lead to changes in apparent delta values. Nonetheless, the magnitude of effects reported for the CRDS analyzers in this study varied across CRDS I (a 2015 model) and CRDS II (a 2018 model), as well as from those reported by Erler et al. (2015). Therefore, we recommended that in applications where O₂
20 concentrations vary, such as groundwater, estuaries, stratified waterbodies, and incubation studies, researchers test individual analyzers for their specific dependencies to allow for correction. This is especially important given that N₂O production and reduction processes in such environments are strongly controlled by O₂ availability. Although the Ar effects characterized in this study were not large, it is nonetheless recommended as a precautionary measure that researchers ensure, where possible, the
25 standard calibration gas Ar composition is similar to that of the sample gas.

The CO₂ effects for OA-ICOS and CH₄ effects for CRDS analyzers must be considered for applications of these analyzers where CO₂ and CH₄ may also co-vary, such as during diel atmospheric monitoring, in soil-flux chamber measurements, incubation studies and even waterbodies (e.g. Erler et al. 2015). These
30 effects need to be either characterized and corrected for by the user, or the interfering gas quantitatively removed. To our knowledge, there is currently no commercially-available technique to remove CH₄ from a gas stream without affecting N₂O, and therefore independent co-analysis of CH₄ is ultimately required to correct for these effects post-measurement. Similarly, while water vapor effects can in theory be characterized and corrected for all instruments, we recommend that researchers remove water vapor from
35 the gas stream prior to analysis. Although not tested here, other studies have highlighted possible spectral interference effects associated with elevated H₂S and volatile organic compounds (Erler et al., 2015;

Ostrom and Ostrom, 2017), but these may also be removed from gas streams using chemical traps (e.g. Cu and activated carbon traps, respectively).

The scaling of gas matrix and trace gas effects with $[\text{N}_2\text{O}]$ has important implications for any measurement setup that relies on post-measurement correction equations. An equation developed to correct for CH_4 effects that was derived using a $[\text{N}_2\text{O}]$ of 330 ppb should not be implemented for a sample gas containing 990 ppb N_2O . For example, as shown in Fig. 8, the measured interference effect on $\delta^{15}\text{N}^\alpha$ measurements acquired using CRDS II for 10 ppm $[\text{CH}_4]$ at 330 ppb N_2O was 24.9 ‰, while at 990 ppb N_2O it was 8.1 ‰, resulting in a 16.8 ‰ difference. The scaling of interference effects from trace gases has been reported previously for CO_2/CH_4 laser spectrometers (Assan et al., 2017; Malowany et al., 2015). This underlines the usefulness of removing H_2O , CO_2 and CO with scrubbers prior to measurement, as this removes the need for correction equations to begin with and the scaling of corrections that can ensue. We are unaware of any studies that have shown that O_2 interferences caused by pressure broadening linewidth effects change as a function of N_2O mole fraction. While we were unable to describe the scaling of the O_2 effect sufficiently using correction functions based on theoretical deductions, empirical equations based on experimental testing such as those developed in Sects. 3.5.2 and 3.6.2, could be implemented by researchers when co-variation in both O_2 and N_2O in the sample gas is expected. Alternatively, as shown in this study, matrix and/or trace gas effects can be removed by automated N_2O preconcentration devices such as TREX (Ibraim et al., 2018; Mohn et al., 2010), similar to IRMS. However, such devices are not commercially available, complex to build and operate, and restrict sample frequency.

4.2 Pre-measurement considerations

Our study clearly shows that knowledge/estimation of the matrix and trace gas composition of both reference standards and sample gases, and the differences between them, are critical for accurate N_2O isotopocule analysis using laser spectroscopy. We acknowledge, however, that this may be difficult to predict in certain applications without prior testing of the sample gas, and therefore researchers should err on the side of caution.

As a pre-requisite to acquiring measurements using N_2O isotope laser spectrometers, researchers will be required to consider the accessory gas mixtures required to characterize their instrument. For applications with significant variations in matrix (O_2 , Ar) or trace gas (CO_2 , CH_4 , CO) compositions, researchers will require gas mixtures containing the gas of interest in order to characterize the associated interference effects for their laser spectrometer. This also necessitates that appropriate interference detectors are implemented, especially O_2 and CH_4 analyzers given that these effects cannot be mitigated using chemical traps.


In this study, interference effects, and the associated scaling of these effects according to the co-measured N₂O mole fraction, were derived via dynamic dilution with various gas mixtures using MFCs. This allowed for the introduction of a wide range of gas mixtures to the analyzers for interference testing, and consequently only a small amount of gas mixtures were required for all of the experiments outlined in Sect. 2.4. In comparison, a much larger number of individual gas mixtures would have been required had they been prepared using static dilution techniques (see Erler et al. 2015). The scaling of interference effects were sufficiently distinguished by undertaking testing at three different N₂O mole fractions (N₂O = 330, 660 and 990 ppb), and we therefore recommend this as a minimum criterion for researchers wishing to characterize this effect.

Researchers should also consider the sample gas volume required for a given measurement application using a specific laser spectrometer. In our experience, ensuring that five laser cavity cell volumes have been flushed prior to measurement is *best practice* to negate any memory effects when these instruments are operated using continuous flow-through configurations (as opposed to discrete sample measurements in a closed laser cavity). By following this procedure and using the operating parameters selected in this study (Table 1), the sample gas volume required for a single 300 s measurement is approximately 80 mL for CRDS II, 150 mL for CRDS I, 600 mL for OA-ICOS I and 1200 mL for QCLAS I. By comparison, TREX-QCLAS I requires approximately 5 L of sample gas to allow for N₂O preconcentration. These sample gas volumes represent typical numbers for atmospheric applications; however, instrument parameter settings such as flow rate and cell pressure, which ultimately change the required sample volume, can be optimized depending on the measurement application. This is particularly the case for QCLAS instruments, which can be operated with different user-adjustable settings. For applications requiring discrete sample analysis (e.g. the headspace analysis of $\delta^{15}\text{N}$ and $\delta^{18}\text{O}$ in N₂O derived from dissolved NO₃⁻), high N₂O concentration gas samples with lower volumes can be introduced to these instruments using injection ports and dilution gases (e.g. Soto et al., 2015; Wassenaar et al., 2018); however we did not test these capabilities in our study.

4.3 Measurement workflow

In-line with our results, we propose a step-by-step workflow that can be followed by researchers to acquire N₂O isotopocule measurements (Fig. 15). This workflow seeks to cover all sources of potential error tested in our study. Not all steps will be applicable because interference effects vary across analyzers. For QCLAS analyzers, which offer high versatility, interference effects can also be approached by multi-line analysis, inclusion of interfering spectral lines or adaption of pressure broadening parameters in the spectral fitting algorithm. For specific applications, such as incubation experiments with He, accessory injection units and setups using TREX, related actions have to be taken. While we tested several mono-

variant (e.g. changes in [CH₄] at constant [N₂O]) and some bi-variant (e.g. changes in [CH₄] and [N₂O]) systems in our study, more complex systems (e.g. changes in [CH₄], [O₂] and [N₂O]) were not tested, and deviations from additive behavior are to be expected. Depending on the desired precision, users may vary the measurement and averaging times, and calibration frequency.

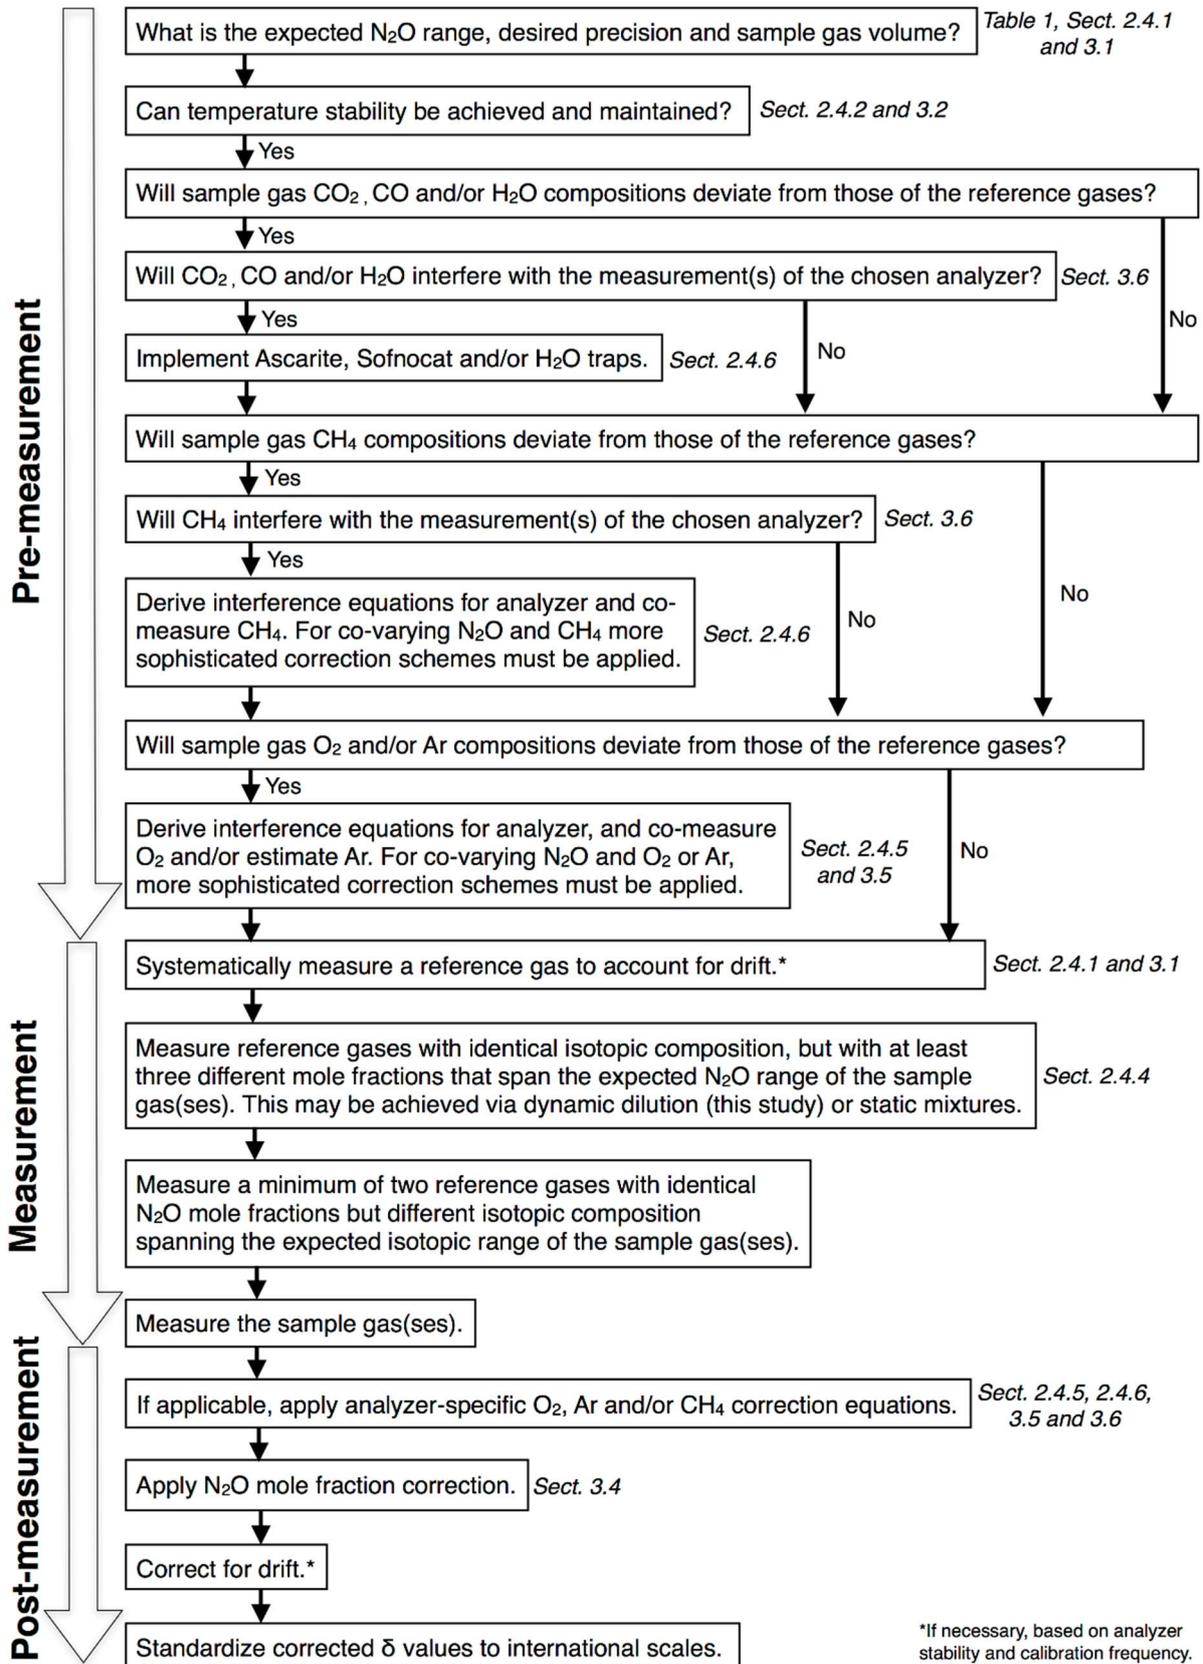

5

Fig. 15. Proposed measurement workflow for the operation of N₂O isotope laser spectrometers. Relevant sections of this study are shown next to each step.

4.4 What degree of accuracy can be achieved using this workflow?

The simulated two end-member mixing experiments conducted in this study show that, when the workflow proposed above is applied, accuracy within $\pm 0.5\%$ can be achieved for TREX-QCLAS, ± 0.4 – 1.6% for CRDS analyzers, and ± 1.6 – 3.6% for OA-ICOS analyzers. Likewise, the comparison between the laser spectrometers and IRMS highlights that cross-technique compatibility within ± 1 – 2.5% can be achieved for most N_2O isotopocule measurements. However, it is clear that the balanced (i.e. non analyzer-specific) approach applied for the purpose of this comparative study did not cater to QCLAS I. Therefore, a more specific calibration protocol for the QCLAS I will likely yield better performance, as shown in Table 6. It is worth noting that, although the results of our study are representative of the performance of the instruments tested, the magnitude of reported effects and performances are likely to vary within the same analyzer models.

Whilst the laboratory-simulated mixing experiment is not fully representative of naturally-occurring two end-member mixing *per se*, the results are useful in comparing intercept accuracy and uncertainty amongst analyzers and against IRMS. Our results show that large uncertainties exist for N_2O source apportionment using Keeling analysis performed at near-ambient N_2O mole fractions. Given the amount of corrections that are required in the experiment, we have not detailed individual analyzer uncertainty budgets to quantify individual sources of error on the intercept, as it is beyond the scope of this study. Nonetheless, the reduction of uncertainty with increasing $\Delta\text{N}_2\text{O}$ shown in experiments 1–6 in Sect. 3.7 has also been shown in previous studies (e.g. Wolf et al., 2015). Therefore, by extension, it is reasonable to assume that the current largest source of uncertainty for ambient N_2O measurements using laser spectroscopy is the inherent signal-to-noise ratio of the measurement.

5 Conclusions

In this study, we characterized and compared N_2O isotope laser-based analyzers with the three most common detection schemes, including OA-ICOS, CRDS and QCLAS. Our results show a number of factors that need to be carefully considered to ensure precise and accurate measurements of N_2O isotopocules using laser spectroscopy. The performance of N_2O isotope laser spectrometers depends on a complex interplay between instrumental precision, drift, matrix gas composition and associated spectral interferences that ultimately vary as a function of N_2O mole fraction. On this basis, we echo recommendations from Ostrom and Ostrom (2017), who cautioned not to underestimate the need for the careful consideration of analyzer-specific corrections. These analyzers clearly do not represent “plug and play” devices – instead, one needs to carefully consider the desired application, precision and accuracy, and develop appropriate calibration strategies to achieve these outcomes.

Consequently, we recommend calibration schemes that have: (1) a calibration frequency that is adequate for constraining instrument drift over experimental period/long-term measurements; (2) temperature stability during measurement, or the temperature effect adequately characterized and corrected; (3) a three-point or higher [N₂O] effect correction that spans the range of expected [N₂O] (if calibration relies on raw δ values derived from uncalibrated isotopocule amount fractions; i.e. a δ -calibration approach); and (4) accounted for the differences in matrix and trace gas composition between the sample gas and reference gases, whereby either analyzer-specific interference corrections have been carefully characterized and applied, or where possible interfering substances (CO₂, CO, H₂O) removed using chemical traps. Correcting for interference effects becomes significantly more complicated once [N₂O] exceed ambient levels, requiring a multitude of analyzer- and gas-specific constants that inevitably increase the number of gas mixtures required by the user, as well as the uncertainty of the measurement. Researchers should therefore strive to implement measurement setups that require as few corrections as possible, and this will inherently decrease the combined uncertainty in the measurement.

Author contributions. SH and JL, guided by JM, designed the study, established the setup and coordinated the experiments. Responsibilities on the analyzers were as follows: SH, BK and DC OA-ICOS; JL and TB CRDS I; LX and BW QCLAS I and CRDS II; JW and KZ TREX-QCLAS I; MB and JS QCLAS II, QCLAS III and GC-IRMS. JM prepared the non-commercial gas mixtures used in this study. LY referenced the δ values of applied gas mixtures to international scales. SH and JL performed the main data analysis and together with JM developed correction algorithms. SH and JL wrote the manuscript with input from all co-authors.

Data availability. All data are available from the corresponding author upon request.

Competing interests. The authors declare that they have no conflict of interest.

Acknowledgements. We extend our thanks to Doug Baer, Rob Provencal and Frederick Despagne from ABB Los Gatos Research Inc., Renato Winkler, Magdalena Hofmann and Paulos Getachew from Picarro Inc., and Dave Nelson and Barry McManus from Aerodyne Research Inc. for their helpful discussions and assistance concerning the analyzers. We thank Christoph Zellweger for his assistance analysing matrix gas cylinders and providing the Picarro G2401 for matrix interference testing, and the NABEL laboratory at Empa for providing the dew point generator for water vapor testing. We want to thank Kristýna Kantnerová from Empa and Daniel Zindel from ETH for the synthesis of ¹⁸O-labelled N₂O.

This study was supported by the European Metrology Programme for Innovation and Research (EMPIR) 16ENV06 project “Metrology for Stable Isotope Reference Standards (SIRS)”. The EMPIR initiative is

co-funded by the European Union's Horizon 2020 research and innovation programme and the EMPIR Participating States. Furthermore, this research was supported by grants from the Cotton Research and Development Corporation (CRDC), and was facilitated by an Endeavour Research Fellowship acquired by Stephen Harris from the Australian Government. Stephen Harris is supported by PhD scholarships
5 from the Australian Government, the Australian Institute of Nuclear Science and Engineering (AINSE), Australian Nuclear Science and Technology Organisation (ANSTO) and CRDC. The UNSW Sydney N₂OIA-30e-EP was purchased using funds from the Australian National Collaborative Research Infrastructure Strategy (NCRIS) Groundwater Infrastructure Project. Jing Wei and Longfei Yu were supported by the Swiss National Science Foundation (SNSF) within grant CRSII5_170876 and
10 200021_163075 as well as the EMPAPOSTDOCS-II programme, which received funding from the European Union's Horizon 2020 research and innovation programme under the Marie Skłodowska-Curie grant agreement number 754364.

References

ABB-Los Gatos Research Inc.: Off-Axis Integrated Cavity Output Spectroscopy (OA-ICOS), available
15 at <http://www.lgrinc.com/advantages/>, 2019.

Allan, D.: Statistics of atomic frequency standards, *Proc. IEEE*, 54, 221–230, 1966.

Anderson, B., Bartlett, K., Frohling, S., Hayhoe, K., Jenkins, J., and Salas, W.: Methane and Nitrous
20 Oxide Emissions from Natural Sources, Office of Atmospheric Programs, US EPA, EPA 430-R-10-001, Washington DC, 2010.

Assan, S., Baudic, A., Guemri, A., Ciais, P., Gros, V., and Vogel, F.R.: Characterization of interferences
25 to in situ observations of $\delta^{13}\text{C}\text{H}_4$ and C_2H_6 when using a cavity ring-down spectrometer at industrial sites, *Atmos. Meas. Tech.*, 10, 2077–2091, doi: 10.5194/amt-10-2077-2017, 2017.

Baer, D. S., Paul, J. B., Gupta, M., and O'Keefe, A.: Sensitive absorption measurements in the near-
infrared region using off-axis integrated-cavity-output spectroscopy, *Appl. Phys. B-Lasers O.*, 75, 261–
265, doi:10.1007/s00340-002-0971-z, 2002.

30 Baggs, E.M.: A review of stable isotope techniques for N₂O source partitioning in soils: recent progress, remaining challenges and future considerations, *Rapid Communications in Mass Spectrometry*, 22, 1664–1672, doi: 10.1002/rcm.3456, 2008.

- Berden, G., Peeters, R. and Meijer, G.: Cavity ring-down spectroscopy: Experimental schemes and applications, *Int. Rev. Phys. Chem.*, 19, 565–607, doi: 10.1080/014423500750040627, 2000.
- Bernard, S., Röckmann, T., Kaiser, J., Barnola, J.-M., Fischer, H., Blunier, T., and Chappellaz, J.:
5 Constraints on N₂O budget changes since pre-industrial time from new firn air and ice core isotope measurements, *Atmos. Chem. Phys.*, 6, 493–503, doi:10.5194/acp-6-493-2006, 2006.
- Bouwman, A. F., Boumans, L. J. M., and Batjes N. H.: Modeling global annual N₂O and NO emissions from fertilized fields, *Global Biogeochem. Cycles*, 16, 1080, doi:10.1029/2001GB001812, 2002.
- 10
- Bowling, D. R., Burns, S. P., Conway, T. J., Monson, R. K., and White, J. W. C.: Extensive observations of CO₂ carbon isotope content in and above a high-elevation subalpine forest, *Global Biogeochem. Cy*, 19, GB3023, doi:10.1029/2004gb002394, 2005.
- 15
- Bowling, D. R., Sargent, S. D., Tanner, B. D., and Ehleringer, J. R.: Tunable diode laser absorption spectroscopy for stable isotope studies of ecosystem-atmosphere CO₂ exchange, *Agr. Forest Meteorol.*, 118, 1–19, doi:10.1016/s0168-1923(03)00074-1, 2003.
- Brase, L., Bange, H.W., Lendt, R., Sanders, T., and Dähnke, K.: High Resolution Measurements of
20 Nitrous Oxide (N₂O) in the Elbe Estuary, *Front. Mar. Sci.*, 4, 162, doi:10.3389/fmars.2017.00162, 2017.
- Buchen, C., Lewicka-Szczebak, D., Flessa, H. and Well, R.: Estimating N₂O processes during grassland renewal and grassland conversion to maize cropping using N₂O isotopocules, *Rapid Commun Mass Spectrom*, 32, 1053–1067, doi:10.1002/rcm.8132, 2018.
- 25
- Decock, C. and Six, J.: How reliable is the intramolecular distribution of ¹⁵N in N₂O to source partition N₂O emitted from soil?, *Soil Biol. Biochem.*, 65, 114–127, doi: 10.1016/j.soilbio.2013.05.012, 2013.
- Denk, T.R., Mohn, J., Decock, C., Lewicka-Szczebak, D., Harris, E., Butterbach-Bahl, K., Kiese, R., and
30 Wolf, B.: The nitrogen cycle: A review of isotope effects and isotope modeling approaches, *Soil Biol Biochem.*, 105, 121–137, doi:10.1016/j.soilbio.2016.11.015, 2017.
- Denman, K. L., Brasseur, G., Chidthaisong, A., Ciais, P., Cox, P. M., Dickinson, R. E., Hauglustaine, D., Heinze, C., Holland, E., Jacob, D., Lohmann, U., Ramachandran, S., da Silva Dias, P. L., Wofsky, S. C.,
35 and Zhang, X.: Couplings between changes in the climate system and biogeochemistry, in: *Climate change 2007, the physical science basis, contribution of working group I to the Fourth Assessment Report*

of the Intergovernmental Panel on Climate Change, edited by: Solomon, S., Qin, D., Manning, M., Chen, Z., Marquis, M., Averyt, K. B., Tignor, M., and Miller, H. L., Cambridge University Press, Cambridge, United Kingdom and New York, NY, USA, 499–587, 2007.

- 5 Erler, D.V., Duncan, T.M., Murray, R., Maher, D.T., Santos, I.R., Gatland, J.R., Mangion, P., and Eyre, B.D.: Applying cavity ring-down spectroscopy for the measurement of dissolved nitrous oxide mole fractions and bulk nitrogen isotopic composition in aquatic systems: Correcting for interferences and field application, *Limnol Oceanogr Methods*, 13, 391–401, doi:10.1002/lom3.10032, 2015.
- 10 Eyer, S., Tuzson, B., Popa, M.E., Van Der Veen, C., Röckmann, T., Rothe, M., Brand, W.A., Fisher, R., Lowry, D., Nisbet, E.G., and Brennwald, M.S.: Real-time analysis of $\delta^{13}\text{C}$ - and $\delta\text{D-CH}_4$ in ambient air with laser spectroscopy: method development and first intercomparison results, *Atmos. Meas. Tech.*, 9, 263–280, doi:10.5194/amt-9-263-2016, 2016.
- 15 Flores, E., Viallon, J., Moussay, P., Griffith, D.W., and Wielgosz, R.I.: Calibration strategies for FT-IR and other isotope ratio infrared spectrometer instruments for accurate $\delta^{13}\text{C}$ and $\delta^{18}\text{O}$ measurements of CO_2 in air, *Anal. Chem.*, 89, 3648–3655, doi:10.1021/acs.analchem.6b05063, 2017.
- 20 Forster, P., Ramaswamy, V., Artaxo, P., Berntsen, T., Betts, R., Fahey, D. W., Haywood, J., Lean, J., Lowe, D. C., Myhre, G., Nganga, J., Prinn, R., Raga, G., Schulz, M., and Van Dorland, R.: Climate Change 2007: Changes in Atmospheric Constituents and in Radiative Forcing, The Physical Science Basis: Contribution of Working Group I to the Fourth Assessment Report of the Intergovernmental Panel on Climate Change, edited by: Solomon, S., Qin, D., Manning, M., Chen, Z., Marquis, M., Averyt, K. B., Tignor, M., and Miller, H. S., Cambridge University Press, Cambridge, UK, New York, NY, USA, 2007.
- 25 Friedrichs, G., Bock, J., Temps, F., Fietzek, P., Körtzinger, A., and Wallace, D.W.: Toward continuous monitoring of seawater $^{13}\text{CO}_2/^{12}\text{CO}_2$ isotope ratio and pCO_2 : Performance of cavity ringdown spectroscopy and gas matrix effects, *Limnol Oceanogr–Meth*, 8, 539–551, doi: 10.4319/lom.2010.8.539, 2010.
- 30 Griffis, T. J., Baker, J. M., Sargent, S. D., Tanner, B. D., and Zhang, J.: Measuring field-scale isotopic CO_2 fluxes with tunable diode laser absorption spectroscopy and micrometeorological techniques, *Agr. Forest Meteorol.*, 124, 15–29, doi:10.1016/j.agrformet.2004.01.009, 2004.

- Griffith, D. W. T., Deutscher, N. M., Caldow, C., Kettlewell, G., Riggenbach, M., and Hammer, S.: A Fourier transform infrared trace gas and isotope analyser for atmospheric applications, *Atmos. Meas. Tech.*, 5, 2481–2498, doi:10.5194/amt-5-2481-2012, 2012.
- 5 Griffith, D. W.: Calibration of isotopologue-specific optical trace gas analysers: a practical guide, *Atmos. Meas. Tech.*, 11, 6189–6201, doi:10.5194/amt-11-6189-2018, 2018.
- Gröning, M.: TEL Technical Note No. 01. SICalib User Manual (Stable Isotope Calibration for routine δ -scale measurements) Ver 2.16j, 2018.
- 10 Harris, E., Henne, S., Hüglin, C., Zellweger, C., Tuzson, B., Ibraim, E., Emmenegger L., and Mohn J.: Tracking nitrous oxide emission processes at a suburban site with semicontinuous, in situ measurements of isotopic composition, *J. Geophys. Res. Atmospheres*, 122, 1850–1870, doi: 10.1002/2016JD025906, 2017.
- 15 Harris, E., Joss, A., Emmenegger, L., Kipf, M., Wolf, B., Mohn, J. and Wunderlin, P.: Isotopic evidence for nitrous oxide production pathways in a partial nitrification-anammox reactor, *Water Res.*, 83, 258–270, doi:10.1016/j.watres.2015.06.040, 2015a.
- 20 Harris, E., Nelson, D.D., Olszewski, W., Zahniser, M., Potter, K.E., McManus, B.J., Whitehill, A., Prinn, R.G., and Ono, S.: Development of a spectroscopic technique for continuous online monitoring of oxygen and site-specific nitrogen isotopic composition of atmospheric nitrous oxide, *Anal. Chem.*, 86, 1726–1734, doi:10.1021/ac403606u, 2014.
- 25 Harris, E., Zeyer, K., Kegel, R., Müller, B., Emmenegger, L. and Mohn, J.: Nitrous oxide and methane emissions and nitrous oxide isotopic composition from waste incineration in Switzerland, *Waste Manage.*, 35, 135–140, doi:10.1016/j.wasman.2014.10.016, 2015b.
- 30 Heil, J., Wolf, B., Brüggemann, N., Emmenegger, L., Tuzson, B., Vereecken, H., and Mohn, J.: Site-specific ^{15}N isotopic signatures of abiotically produced N_2O , *Geochim. Cosmochim. Ac.*, 139, 72–82, doi: 10.1016/j.gca.2014.04.037, 2014.
- Henry, A., Margottin-Maclou, M., and Lacome, N.: N_2 - and O_2 -broadening parameters in the ν_3 band of $^{14}\text{N}_2^{16}\text{O}$, *J. Mol. Spectrosc.*, 111, 291–300, doi:10.1016/0022-2852(85)90006-2, 1985.

- Ibraim, E., Harris, E., Eyer S., Tuzson, B., Emmenegger, L., Six, J., and Mohn, J.: Development of a field-deployable method for simultaneous, real-time measurements of the four most abundant N₂O isotopocules, *Isotopes Environ Health Stud.*, 54, 1–5, doi: 10.1080/10256016.2017.1345902, 2018.
- 5 Ibraim, E., Wolf, B., Harris, E., Gasche, R., Wei, J., Yu, L., Kiese, R., Eggleston, S., Butterbach-Bahl, K., Zeeman, M., and Tuzson, B.: Attribution of N₂O sources in a grassland soil with laser spectroscopy based isotopocule analysis, *Biogeosci.*, 16, 3247–3266, doi:10.5194/bg-16-3247-2019, 2019.
- Ishijima, K., Sugawara, S., Kawamura, K., Hashida, G., Morimoto, S., Murayama, S., Aoki, S., and
10 Nakazawa, T.: Temporal variations of the atmospheric nitrous oxide mole fraction and its $\delta^{15}\text{N}$ and $\delta^{18}\text{O}$ for the latter half of the 20th century reconstructed from firn air analyses, *J Geophys. Res. Atmos.*, 112, D3, doi: 10.1029/2006JD007208, 2007.
- Ji, Q., Grundle, D.S.: An automated, laser-based measurement system for nitrous oxide isotope and
15 isotopomer ratios at nanomolar levels, *Rapid Commun Mass Spectrom.*, 33, 1553–1564, doi:10.1002/rcm.8502, 2019.
- Johnson, J. E. and Rella, C. W.: Effects of variation in background mixing ratios of N₂, O₂, and Ar on the measurement of $\delta^{18}\text{O}$ -H₂O and $\delta^2\text{H}$ -H₂O values by cavity ring-down spectroscopy, *Atmos. Meas.*
20 *Tech.*, 10, 3073-3091, <https://doi.org/10.5194/amt-10-3073-2017>, 2017.
- Keeling, C. D.: The mole fraction and isotopic abundances of atmospheric carbon dioxide in rural areas, *Geochim. Cosmochim. Acta*, 13, 322–334, doi:10.1016/0016-7037(58)90033-4, 1958.
- 25 Koba, K., Osaka, K., Tobar, Y., Toyoda, S., Ohte, N., Katsuyama, M., Suzuki, N., Itoh, M., Yamagishi, H., Kawasaki, M., and Kim, S.J.: Biogeochemistry of nitrous oxide in groundwater in a forested ecosystem elucidated by nitrous oxide isotopomer measurements, *Geochim. Cosmochim. Acta*, 73, 3115–3133, doi:10.1016/j.gca.2009.03.022, 2009.
- 30 Kong, X., Duan, Y., Schramm, A., Eriksen, J., Holmstrup, M., Larsen, T., Bol, R., and Petersen, S.O.: Mitigating N₂O emissions from clover residues by 3, 4-dimethylpyrazole phosphate (DMPP) without adverse effects on the earthworm *Lumbricus terrestris*, *Soil Biol. Biochem.*, 104, 95–107, doi:10.1016/j.soilbio.2016.10.012, 2017.

- Köster, J. R., Cárdenas, L., Senbayram, M., Bol, R., Well, R., Butler, M., Mühlhling, K. H., and Dittert, K.: Rapid shift from denitrification to nitrification in soil after biogas residue application as indicated by nitrous oxide isotopomers, *Soil Biol. Biochem.*, 43, 1671–1677, doi: 10.1002/rcm.6434, 2011.
- 5 Köster, J. R., Well, R., Tuzson, B., Bol, R., Dittert, K., Giesemann, A., Emmenegger, L., Manninen, A., Cárdenas, L., and Mohn, J.: Novel laser spectroscopic technique for continuous analysis of N₂O isotopomers – application and intercomparison with isotope ratio mass spectrometry, *Rapid Commun. Mass Spectrom.*, 27, 216–222, doi:10.1002/rcm.6434, 2013.
- 10 Lebeque, B., Schmidt, M., Ramonet, M., Wastine, B., Yver Kwok, C., Laurent, O., Belviso, S., Guemri, A., Philippon, C., Smith, J., and Conil, S.: Comparison of nitrous oxide (N₂O) analyzers for high-precision measurements of atmospheric mole fractions, *Atmos. Meas. Tech.*, 9, 1221–1238, doi:10.5194/amt-9-1221-2016, 2016.
- 15 Lee, A., Winther, M., Priemé, A., Blunier, T., and Christensen, S.: Hot spots of N₂O emission move with the seasonally mobile oxic-anoxic interface in drained organic soils, *Soil Biol. and Biochem.*, 115, 178–186, doi:10.1016/j.soilbio.2017.08.025, 2017.
- Lewicka-Szczebak, D., Well, R., Köster, J. R., Fuß, R., Senbayram, M., Dittert, K., and Flessa, H.:
20 Experimental determinations of isotopic fractionation factors associated with N₂O production and reduction during denitrification in soils, *Geochim. Cosmochim. Ac.*, 134, 55–73, doi: 10.1016/j.gca.2014.03.010, 2014.
- Lewicka-Szczebak, D., Well, R., Bol, R., Gregory, A. S., Matthews, G. P., Misselbrook, T., Whalley, W.
25 R., and Cardenas, L. M.: Isotope fractionation factors controlling isotopocule signatures of soil-emitted N₂O produced by denitrification processes of various rates, *Rapid Commun. Mass Spectr.*, 29, 269–282, doi: 10.1002/rcm.7102, 2015.
- Li, X., Sørensen, P., Olesen, J.E., and Petersen, S.O.: Evidence for denitrification as main source of N₂O
30 emission from residue-amended soil, *Soil Biol. Biochem.*, 92, 153–160, doi:10.1016/j.soilbio.2015.10.008, 2016.
- Li, P., Wang, S., Peng, Y., Liu, Y., and He, J.: The synergistic effects of dissolved oxygen and pH on N₂O production in biological domestic wastewater treatment under nitrifying conditions, *Environ. Technol.*, 36, 1623–1631, doi: 10.1080/09593330.2014.1002862, 2015.

- Malowany, K., Stix, J., Van Pelt, A., and Lucic, G.: H₂S interference on CO₂ isotopic measurements using a Picarro G1101-i cavity ring-down spectrometer, *Atmos. Meas. Tech.*, 8, 4075–4082, doi: 10.5194/amt-8-4075-2015, 2015.
- 5 Miller, J.B., and Tans, P.P.: Calculating isotopic fractionation from atmospheric measurements at various scales, *Tellus*, 55, 207–214, doi:10.1034/j.1600-0889.2003.00020.x, 2003.
- Minamikawa, K., Nishimura, S., Nakajima, Y., Osaka, K.I., Sawamoto, T., and Yagi, K.: Upward diffusion of nitrous oxide produced by denitrification near shallow groundwater table in the summer: a lysimeter experiment, *Soil Sci. Plant Nutr.*, 57, 719–732, doi: 10.1080/00380768.2011.625556, 2011.
- 10 Mohn, J., Guggenheim, C., Tuzson, B., Vollmer, M. K., Toyoda, S., Yoshida, N., and Emmenegger, L.: A liquid nitrogen-free preconcentration unit for measurements of ambient N₂O isotopomers by QCLAS, *Atmos. Meas. Tech.*, 3, 609–618, doi:10.5194/amt-3-609-2010, 2010.
- 15 Mohn, J., Tuzson, B., Manninen, A., Yoshida, N., Toyoda, S., Brand, W. A., and Emmenegger, L.: Site selective real-time measurements of atmospheric N₂O isotopomers by laser spectroscopy, *Atmos. Meas. Tech.*, 5, 1601–1609, doi:10.5194/amt-5-1601-2012, 2012.
- 20 Mohn, J., Wolf, B., Toyoda, S., Lin, C. T., Liang, C. M., Brüggemann, N., Wissel, H., Steiker, A. E., Dyckmans, J., Szwed, L., Ostrom, N. E., Casciotti, K. L., Forbes, M., Gieseemann, A., Well, R., Doucett, R. R., Yarnes, C. T., Ridley, A. R., Kaiser, J., and Yoshida, N.: Inter-Laboratory assessment of nitrous oxide isotopomer analysis of isotopomer analysis by isotope ratio mass spectrometry and laser spectroscopy: current status and perspectives, *Rapid Commun. Mass Spectr.*, 28, 1995–2007, doi: 25 10.1002/rcm.6982, 2014.
- Mosier, A., Kroeze, C., Nevison, C., Oenema, O., Seitzinger, S. and Van Cleemput, O.: Closing the global N₂O budget: nitrous oxide emissions through the agricultural nitrogen cycle, *Nutr. Cycl. Agroecosys.*, 52, 225–248, doi:10.1023/A:1009740530221, 1998.
- 30 Murray, R., Erler, D., Rosentreter, J., Maher, D., and Eyre, B.: A seasonal source and sink of nitrous oxide in mangroves: Insights from mole fraction, isotope, and isotopomer measurements, *Geochim. Cosmochim. Acta*, 238, 169–192, doi:10.1016/j.gca.2018.07.003, 2018.
- 35 Nara, H., Tanimoto, H., Tohjima, Y., Mukai, H., Nojiri, Y., Katsumata, K., and Rella, C.W.: Effect of air composition (N₂, O₂, Ar, and H₂O) on CO₂ and CH₄ measurement by wavelength-scanned cavity ring-

- down spectroscopy: calibration and measurement strategy, *Atmos. Meas. Tech.*, 5, 2689–2701, doi:10.5194/amt-5-2689-2012, 2012.
- Nikolenko, O., Orban, P., Jurado, A., Morana, C., Jamin, P., Robert, T., Knöller, K., Borges, A.V., and
5 Brouyère, S.: Dynamics of greenhouse gases in groundwater: hydrogeological and hydrogeochemical controls. *Appl Geochem.*, 105, 31–44, doi:10.1016/j.apgeochem.2019.04.009, 2019.
- NOAA/ESRL: Combined Nitrous Oxide data from the NOAA/ESRL Global Monitoring Division, 2019.
- 10 Ogawa, M., and Yoshida, N.: Intramolecular distribution of stable nitrogen and oxygen isotopes of nitrous oxide emitted during coal combustion, *Chemosphere*, 61, 877–887, doi: 10.1016/j.chemosphere.2005.04.096, 2005.
- Ostrom N., and Ostrom, P.: Mining the isotopic complexity of nitrous oxide: a review of challenges and
15 opportunities, *Biogeochemistry*, 132, 359–372, doi:10.1007/s10533-017-0301-5, 2017.
- Ostrom, N.E. and Ostrom, P.H.: The Isotopomers of Nitrous Oxide: Analytical Considerations and Application to Resolution of Microbial Production Pathways, in: *Handbook of Environmental Isotope Geochemistry Volume 1*, edited by: Baskaran, M., Springer Berlin Heidelberg, Berlin, Heidelberg, 453–
20 476, 2011.
- Ostrom, N.E., Gandhi, H., Coplen, T.B., Toyoda, S., Böhlke, J.K., Brand, W.A., Casciotti, K.L., Dyckmans, J., Gieseemann, A., Mohn, J., and Well, R.: Preliminary assessment of stable nitrogen and oxygen isotopic composition of USGS51 and USGS52 nitrous oxide reference gases and perspectives on
25 calibration needs, *Rapid Commun Mass Spectrom*, 32, 1207–1214, doi:10.1002/rcm.8157, 2018.
- Ostrom, N. E., Pitt, A., Sutka, R., Ostrom, P. H., Grandy, A. S., Huizinga, K. M., and Robertson, G. P.: Isotopologue effects during N₂O reduction in soils and in pure cultures of denitrifiers, *J. Geophys. Res.*, 112, G02005, doi:10.1029/2006JG000287, 2007.
30
- Pang, J., Wen, X., Sun, X. and Huang, K.: Intercomparison of two cavity ring-down spectroscopy analyzers for atmospheric ¹³CO₂/¹²CO₂ measurement, *Atmos. Meas. Tech.*, 9, 3879–3891, doi:10.5194/amt-9-3879-2016, 2016.

- Park, S., Croteau, P., Boering, K.A., Etheridge, D.M., Ferretti, D., Fraser, P.J., Kim, K.R., Krummel, P.B., Langenfelds, R.L., Van Ommen, T.D. and Steele, L.P.: Trends and seasonal cycles in the isotopic composition of nitrous oxide since 1940, *Nat. Geosci.*, 5, 261, doi:10.1038/NGEO1421, 2012.
- 5 Pataki, D. E., Bowling, D. R., Ehleringer, J. R., and Zobitz, J. M.: High resolution atmospheric monitoring of urban carbon dioxide sources, *Geophys. Res. Lett.*, 33, L03813, doi:10.1029/2005gl024822, 2006.
- Peng, L., Ni, B.J., Eiler, D., Ye, L., and Yuan, Z.: The effect of dissolved oxygen on N₂O production by ammonia-oxidizing bacteria in an enriched nitrifying sludge, *Water Res.*, 66, 12–21, doi:10.1016/j.watres.2014.08.009, 2014.
- 10 Picarro Inc.: Cavity Ring-Down Spectroscopy (CRDS), available at <https://www.picarro.com/company/technology/crds>, 2019.
- 15 Potter, K.E., Ono, S., and Prinn, R.G.: Fully automated, high-precision instrumentation for the isotopic analysis of tropospheric N₂O using continuous flow isotope ratio mass spectrometry, *Rapid Commun Mass Spectrom*, 27, 1723–1738, doi:10.1002/rcm.6623, 2013.
- Prokopiou, M., Martinerie, P., Sapart, C.J., Witrant, E., Monteil, G., Ishijima, K., Bernard, S., Kaiser, J., Levin, I., Blunier, T., and Etheridge, D.: Constraining N₂O emissions since 1940 using firn air isotope measurements in both hemispheres, *Atmos Chem Phys*, 17, 4539–4564, doi:10.5194/acp-17-4539-2017, 2017.
- 20 Pérez, T., Garcia-Montiel, D., Trumbore, S., Tyler, S., Camargo, P.D., Moreira, M., Piccolo, M., and Cerri, C.: Nitrous oxide nitrification and denitrification ¹⁵N enrichment factors from Amazon forest soils, *Ecol Appl*, 16, 2153–2167, doi: 10.1890/1051-0761(2006)016[2153:NONADN]2.0.CO;2, 2006.
- Pérez, T., Trumbore, S.E., Tyler, S.C., Matson, P.A., Ortiz-Monasterio, I., Rahn, T., and Griffith, D.W.T.: Identifying the agricultural imprint on the global N₂O budget using stable isotopes, *J Geophys Res Atmos.*, 106, 9869–9878, doi:10.1029/2000JD900809, 2001.
- 30 R Core Team.: R: A language and environment for statistical computing. R Foundation for Statistical Computing, Vienna, Austria. URL <https://www.R-project.org/>, 2017.
- 35 Ravishankara, A. R., Daniel, J. S., and Portmann, R. W.: Nitrous oxide (N₂O): the dominant ozone-depleting substance emitted in the 21st century, *Science*, 326, 123–125, 2009.

- Rella, C. W., Chen, H., Andrews, A. E., Filges, A., Gerbig, C., Hatakka, J., Karion, A., Miles, N. L., Richardson, S. J., Steinbacher, M., Sweeney, C., Wastine, B., and Zellweger, C.: High accuracy measurements of dry mole fractions of carbon dioxide and methane in humid air, *Atmos. Meas. Tech.*, 6, 837–860, doi:10.5194/amt-6-837-2013, 2013.
- Röckmann, T., and Levin I.: High-precision determination of the changing isotopic composition of atmospheric N₂O from 1990 to 2002, *J. Geophys. Res.*, 110, D21304, doi:10.1029/2005JD006066, 2015.
- 10 Rothman, L.S., Jacquemart, D., Barbe, A., Benner, D.C., Birk, M., Brown, L.R., Carleer, M.R., Chackerian Jr, C., Chance, K., Coudert, L.E.A., and Dana, V.: The HITRAN 2004 molecular spectroscopic database, *J Quant Spectrosc Radiat Transf.*, 96, 139–204, doi:10.1016/j.jqsrt.2004.10.008, 2005.
- 15 Soto, D.X., Koehler, G., and Hobson, K.A.: Combining denitrifying bacteria and laser spectroscopy for isotopic analyses ($\delta^{15}\text{N}$, $\delta^{18}\text{O}$) of dissolved nitrate, *Anal. Chem.*, 87, 7000–7005, doi:10.1021/acs.analchem.5b01119, 2015.
- Sutka, R. L., Ostrom, N. E., Ostrom, P. H., Breznak, J. A., Gandhi, H., Pitt, A. J., and Li, F.: Distinguishing nitrous oxide production from nitrification and denitrification on the basis of isotopomer abundances, *Appl. Environ. Microb.*, 72, 638–644, doi:10.1128/AEM.72.1.638-644.2006, 2006.
- 20 Sutka, R. L., Ostrom, N. E., Ostrom, P. H., Gandhi, H., and Breznak, J. A.: Nitrogen isotopomer site preference of N₂O produced by *Nitrosomonas europaea* and *Methylococcus capsulatus* bath, *Rapid Commun. Mass Sp.*, 17, 738–745, doi:10.1002/rcm.968, 2003.
- Tian, H., Chen, G., Lu, C., Xu, X., Ren, W., Zhang, B., Banger, K., Tao, B., Pan, S., Liu, M., Zhang, C., Bruhwiler, L., and Wofsy, S.: Global methane and nitrous oxide emissions from terrestrial ecosystems due to multiple environmental changes, *Ecosyst. Health Sustain.*, 1, 1–20, doi:10.1890/ehs14-0015.1, 30 2015.
- Tuzson, B., Mohn, J., Zeeman, M.J., Werner, R.A., Eugster, W., Zahniser, M.S., Nelson, D.D., McManus, J.B., and Emmenegger, L.: High precision and continuous field measurements of $\delta^{13}\text{C}$ and $\delta^{18}\text{O}$ in carbon dioxide with a cryogen-free QCLAS, *Appl. Phys. B*, 92, 451, doi:10.1007/s00340-008-3085-4, 2008.

- Toyoda S., Yoshida N., and Koba K.: Isotopocule analysis of biologically produced nitrous oxide in various environments, *Mass Spectrom. Rev.*, 36, 135–160, doi: 10.1002/mas.21459, 2017.
- Toyoda, S. and Yoshida, N.: Determination of nitrogen isotopomers of nitrous oxide on a modified isotope ratio mass spectrometer, *Anal. Chem.*, 71, 4711–4718, doi:10.1021/ac9904563, 1999.
- Toyoda, S., Kuroki, N., Yoshida, N., Ishijima, K., Tohjima, Y., and Machida T.: Decadal time series of tropospheric abundance of N₂O isotopomers and isotopologues in the Northern Hemisphere obtained by the long-term observation at Hateruma Island, Japan, *J. Geophys. Res. Atmos.*, 118, 3369–3381, doi:10.1002/jgrd.50221, 2013.
- Toyoda, S., Mutobe, H., Yamagishi, H., Yoshida, N., and Tanji, Y.: Fractionation of N₂O isotopomers during production by denitrifier, *Soil Biol. Biochem.*, 37, 1535–1545, doi:10.1016/j.soilbio.2005.01.009, 2005.
- Toyoda, S., Yano, M., Nishimura, S., Akiyama, H., Hayakawa, A., Koba, K., Sudo, S., Yagi, K., Makabe, A., Tobar, Y., Ogawa, N. O., Ohkouchi, N., Yamada, K., and Yoshida, N.: Characterization and production and consumption processes of N₂O emitted from temperate agricultural soils determined via isotopomer ratio analysis, *Glob. Biogeochem. Cy.*, 25, GB2008, doi: 10.1029/2009GB003769, 2011.
- Verhoeven, E., Barthel, M., Yu, L., Celi, L., Said-Pullicino, D., Sleutel, S., Lewicka-Szczebak, D., Six, J., and Decock, C.: Early season N₂O emissions under variable water management in rice systems: source-partitioning emissions using isotope ratios along a depth profile, *Biogeosci.*, 16, 383–408, doi:10.5194/bg-16-383-2019, 2019.
- Verhoeven, E., Decock, C., Barthel, M., Bertora, C., Sacco, D., Romani, M., Sleutel, S., and Six, J.: Nitrification and coupled nitrification-denitrification at shallow depths are responsible for early season N₂O emissions under alternate wetting and drying management in an Italian rice paddy system, *Soil Biol. Biochem.*, 120, 58–69, doi:10.1016/j.soilbio.2018.01.032, 2018.
- Vogel, F. R., Huang, L., Ernst, D., Giroux, L., Racki, S., and Worthy, D. E. J.: Evaluation of a cavity ring-down spectrometer for in situ observations of ¹³CO₂, *Atmos. Meas. Tech.*, 6, 301–308, doi:10.5194/amt-6-301-2013, 2013.

- Wächter, H., Mohn, J., Tuzson, B., Emmenegger, L., and Sigrist, M.W.: Determination of N₂O isotopomers with quantum cascade laser based absorption spectroscopy, *Optics express*, 16, 9239–9244, doi:10.1364/OE.16.009239, 2008.
- 5 Wassenaar, L.I., Douence, C., Altabet, M.A., and Aggarwal, P.K.: N and O isotope ($\delta^{15}\text{N}^{\alpha}$, $\delta^{15}\text{N}^{\beta}$, $\delta^{18}\text{O}$, $\delta^{17}\text{O}$) analyses of dissolved NO₃⁻ and NO₂⁻ by the Cd-azide reduction method and N₂O laser spectrometry, *Rapid Commun. Mass Spectr.*, 32, 184–194, doi:10.1002/rcm.8029, 2018.
- Wei J., Zhou M., Vereecken H., and Brüggemann N.: Large variability in CO₂ and N₂O emissions and in
10 ¹⁵N site preference of N₂O from reactions of nitrite with lignin and its derivatives at different pH. *Rapid Commun. Mass Sp.*, 31, 1333–1343, doi:10.1002/rcm.7912, 2017.
- Well, R., Eschenbach, W., Flessa, H., von der Heide, C., and Weymann, D.: Are dual isotope and isotopomer ratios of N₂O useful indicators for N₂O turnover during denitrification in nitrate-contaminated
15 aquifers? *Geochim. Cosmochim. Acta* 90, 265–282, doi:10.1016/j.gca.2012.04.045, 2012.
- Well, R. and Flessa, H.: Isotopologue signatures of N₂O produced by denitrification in soils, *J. Geophys. Res.*, 114, G02020, doi:10.1029/2008JG000804, 2009.
- 20 Well, R., Flessa, H., Jaradat, F., Toyoda, S., and Yoshida, N.: Measurement of isotopomer signatures of N₂O in groundwater, *J. Geophys. Res.* 110, G02006, doi:10.1029/2005JG000044, 2005.
- Well, R., Flessa, H., Xing, L., Xiaotang, J., and Römheld, V.: Isotopologue ratios of N₂O emitted from microcosms with NH₄⁺ fertilized arable soils under conditions favoring nitrification, *Soil Biol. Biochem.*,
25 40, 2416–2426, doi:10.1016/j.soilbio.2008.06.003, 2008.
- Wen, X.-F., Meng, Y., Zhang, X.-Y., Sun, X.-M., and Lee, X.: Evaluating calibration strategies for isotope ratio infrared spectroscopy for atmospheric ¹³CO₂/¹²CO₂ measurement, *Atmos. Meas. Tech.*, 6, 1491–1501, doi:10.5194/amt-6-1491-2013, 2013.
30
- Werle, P.O., Mücke, R., and Slemr, F.: The limits of signal averaging in atmospheric trace-gas monitoring by tunable diode-laser absorption spectroscopy (TDLAS), *Applied Physics B*, 57, 131–139, doi:10.1007/BF00425997, 1993.
- 35 Werner, R. A. and Brand, W. A.: Referencing strategies and techniques in stable isotope ratio analysis, *Rapid Commun. Mass Spectrom.*, 15, 501–519, doi:10.1002/rcm.258, 2001.

- Winther, M., Balslev-Harder, D., Christensen, S., Priemé, A., Elberling, B., Crosson, E., & Blunier, T.: Continuous measurements of nitrous oxide isotopomers during incubation experiments, *Biogeosciences*, 15, 767-780, doi:10.5194/bg-15-767-2018, 2018.
- 5
- Wolf, B., Merbold, L., Decock, C., Tuzson, B., Harris, E., Six, J., Emmenegger L., and Mohn J.: First on-line isotopic characterization of N₂O above intensively managed grassland, *Biogeosciences*, 12, 2517–2531, doi: 10.5194/bg-12-2517-2015, 2015.
- 10 Wunderlin, P., Lehmann, M. F., Siegrist, H., Tuzson, B., Joss, A., Emmenegger, L., and Mohn, J.: Isotope signatures of N₂O in a mixed microbial population system: constraints on N₂O producing pathways in wastewater treatment, *Environ. Sci. Technol.*, 47, 1339–1348, doi: 10.1021/es303174x, 2013.
- 15 Wunderlin, P., Mohn, J., Joss, A., Emmenegger, L., and Siegrist, H.: Mechanisms of N₂O production in biological wastewater treatment under nitrifying and denitrifying conditions, *Water Res.*, 46, 1027–37, doi: 10.1016/j.watres.2011.11.080, 2012.
- 20 Yamamoto, A., Uchida, Y., Akiyama, H., and Nakajima, Y.: Continuous and unattended measurements of the site preference of nitrous oxide emitted from an agricultural soil using quantum cascade laser spectrometry with intercomparison with isotope ratio mass spectrometry, *Rapid Commun. Mass Spectr.*, 28, 1444 –1452, doi:10.1002/rcm.6916, 2014.
- Yoshida, N. and Toyoda, S.: Constraining the atmospheric N₂O budget from intramolecular site preference in N₂O isotopomers, *Nature*, 405, 330–334, doi:10.1038/35012558, 2000.
- 25
- Yue, F.J., Li, S.L., Liu, C.Q., Mostofa, K.M., Yoshida, N., Toyoda, S., Wang, S.L., Hattori, S., and Liu, X.L.: Spatial variation of nitrogen cycling in a subtropical stratified impoundment in southwest China, elucidated by nitrous oxide isotopomer and nitrate isotopes, *Inland Waters*, 8, 186–195, doi: 10.1080/20442041.2018.1457847, 2018.