

## Response to RC1

This manuscript describes OH interference measurements performed using the Leeds LIF FAGE instrument with the inclusion of an inlet pre-injector during three separate field deployments. I was very interested in reviewing this manuscript due to its importance in the measurement of ambient OH. With large reported discrepancies between measured and modeled OH and the significance of accurate OH measurements, it is important for all LIF groups to conduct these tests. This manuscript is thorough and well written; however, I have concerns regarding some of the analyses which I believe can be resolved with further clarification. Nevertheless, once these changes are made, I fully recommend publication in AMT.

We thank the reviewer for their kind comments. Below we present the comments of the reviewer (blue text), then our responses to individual comments and changes made in the revised manuscript (black text).

### Specific comments

Figure 5: Do the authors have any thoughts on why there is more variability in the propane results? And why does C3F6 produce a more gradual decay?

Some of the propane results were collected when the FAGE instrument was operating with a higher background than usual, leading to more scatter in the data. Considering we are measuring on the order of <1% OH remaining, we would expect some scatter in the data. With this considered it is clear that propane and C3F6 follow the same general trend. Finally, we do not believe this affects our main point that under the IPI operating conditions used during field campaigns, >99% of ambient OH should have been scavenged away.

P11, line 367: I suggest the authors consider adding the description of the injector tip to Figure 1 for clarity. In addition, can it be clarified that this injector tip is not interrupting the sample flow?

We have added “through 1/8” stainless steel tubing” after “injected” in the revised MS. We cannot clarify that the sample flow is interrupted by the injectors and see this as a limitation to our approach for determining internal OH removal. Since the NO injector tip was only moved for the purpose of the internal removal experiment, we have chosen not to add this to Fig. 1 (in ambient HO<sub>2</sub> detection, NO is injected 7.5 cm below the pinhole).

P13, lines 464-71: I suggest the authors perform a simple modeling test to determine if SCIs are the likely cause of this interference. While it is negligible when extrapolated to ambient concentrations, acknowledgement and quantification of this interference, if it is in fact from SCIs, can be used in comparison with other FAGE instrumental overviews.

35

We agree with the reviewer that modelling the SCI decomposition and quantification of the interference would be useful for comparison to other FAGE instruments. We have added the following sentences to Section 3.2.2:

40

“Similarly, we have modelled the SCI decomposition in our FAGE cell. Assuming an ambient atmosphere containing 100 ppbv O<sub>3</sub> and 10 ppbv alkene and taking the reactions and rate coefficients from Novelli et al. (2014a), we calculate an equivalent ambient pressure OH concentration of  $\sim 4 \times 10^3$  molecule cm<sup>-3</sup> from the decomposition of SCIs at our FAGE cell residence time of 2 ms.”

45

Novelli, A., Vereecken, L., Lelieveld, J., and Harder, H.: Direct observation of OH formation from stabilised Criegee intermediates, Phys. Chem. Chem. Phys., 16, 19941–19951, 2014.

Figure 10: Do the authors have any suggestions as to why there appears to be greater variability at lower OH<sub>wave</sub> and OH<sub>chem</sub> measurements? Assuming the majority of these points are nighttime measurements, is NO<sub>3</sub> responsible? Overcorrection of O<sub>3</sub>/H<sub>2</sub>O?

50

We suggest the perceived greater variability at low OH is simply due to more datapoints being collected at low OH, thus making it more likely to see outliers. NO<sub>3</sub> interferences have been ruled out as insignificant in laboratory tests, and we believe the O<sub>3</sub>/H<sub>2</sub>O interference has been well quantified, although since this is very small it is difficult to measure accurately.

55

Section 2.3: More information about the field deployments needs to be presented. How long (#days) were each deployment? Were measurements continuous?

The text has been modified accordingly.

60

ICOZA: “Two continuous IPI sampling periods were conducted in the middle of the campaign, separated by a few days (3<sup>rd</sup>–8<sup>th</sup> July and 12<sup>th</sup>–16<sup>th</sup> July), with a total of nine days where OH<sub>chem</sub> measurements are available around midday. For other times, only measurements of OH<sub>wave</sub> are available. During the IPI sampling periods, power cuts on the nights of 3<sup>rd</sup>/4<sup>th</sup> July and 6<sup>th</sup>/7<sup>th</sup> July resulted in data loss.”

65


AIRPRO: “In winter, OH<sub>wave</sub> and OH<sub>chem</sub> were measured simultaneously for 6 days of the campaign. In summer, almost one month of near-continuous IPI data are available, with one day of interruptions due to IPI testing (see Section 3.1.2).”

The authors later mention instrumental issues such as power outages. This would be the section to provide more detail about such matters.

We have added the following sentence to the text referring to ICOZA: “During the IPI sampling periods, power cuts on the nights of 3rd/4th July and 6th/7th July resulted in data loss.”


70 P 16, lines 544-8: Did the authors compare OHint to the same parameters that were previously implicated? It seems that since there was little to no OH interference measured, that by comparing OHwave and OHchem individually to these parameters, the trend will largely be representative of actual OH.

75 We agree with this comment and have looked at correlations of OHint with other species. For ICOZA, no dependences were found on parameters previously implicated:

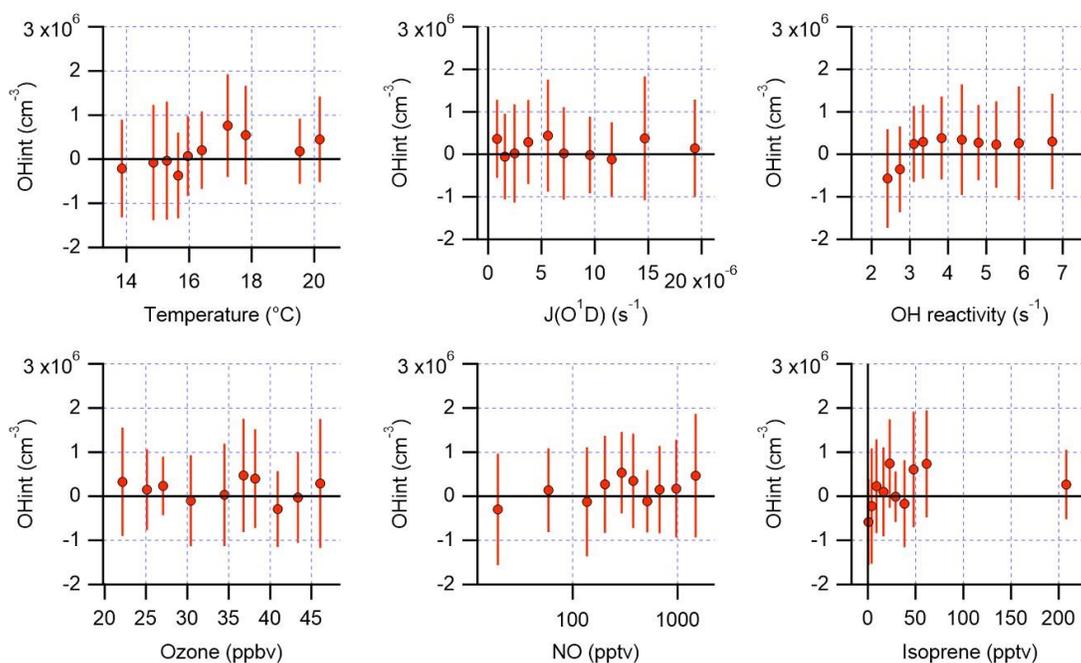

**Figure 1.** Daytime ( $J(O^1D) > 5e-7$ ) OHint binned against various parameters for the ICOZA campaign. Error bars correspond to 1 SD.

The case was similar for AIRPRO summer:

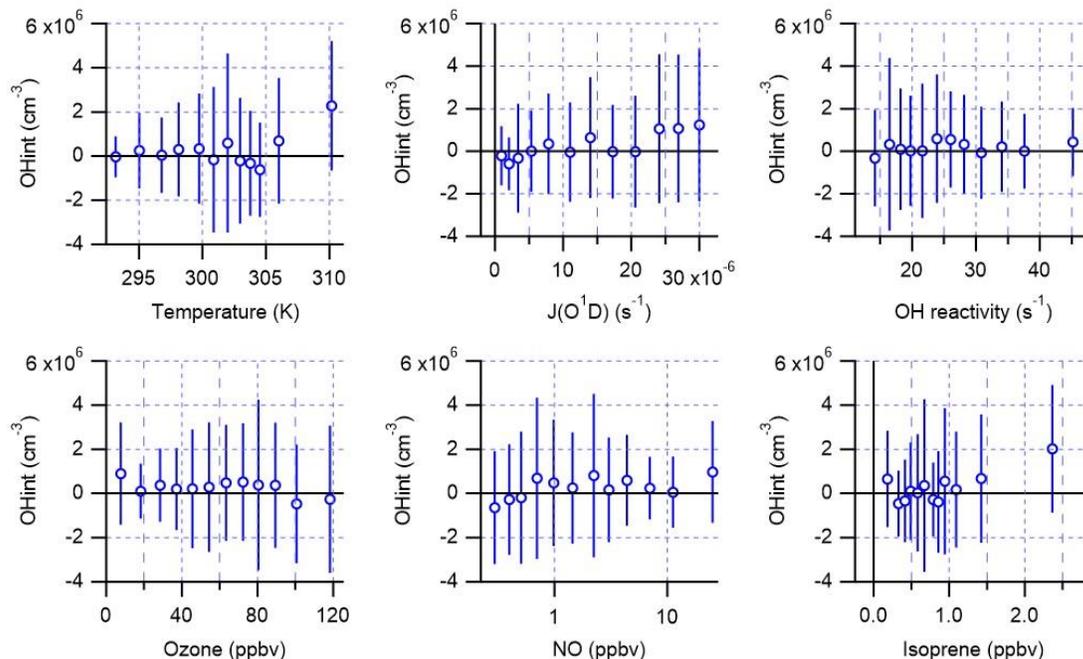

**Figure 2.** Daytime ( $J(\text{O}^1\text{D}) > 5\text{e-}7$ ) OHint binned against various parameters for the summer AIRPRO campaign. Error bars correspond to 1 SD.

80

Although, it can be seen that OHint was marginally higher in the highest temperature, JO1D, and isoprene bins. We have decided to include these figures in a supplementary information file, and referenced them in the main MS.

85

P16, lines 558-9: Are the authors convinced that an over-subtraction of O3/H2O is not occurring during the daytime as well? Figure 13 shows OHchem larger than OHwave at peak concentrations. In addition, AIRPRO summer 2017 reports a negative interference ratio (-0.09). Is this also related to an over correction of O3/H2O? The authors are encouraged to give more insight into this.

90

We believe the O3/H2O interference has been well quantified, although since this is very small it is difficult to measure accurately (see, e.g., the high scatter in Figure 7). The scaling factor in equation (E7) has a  $2\sigma$  uncertainty of  $140 \text{ molecule cm}^{-3} \text{ ppbv}^{-1} \%^{-1} \text{ mW}^{-1}$ . Subtracting this from the actual factor ( $520 \text{ molecule cm}^{-3} \text{ ppbv}^{-1} \%^{-1} \text{ mW}^{-1}$ ) yields a lower limit for the O3/H2O interference. Below shows the effect of using this lower limit interference to correct OHwave data, resulting in less negative OHint. However, in both the original and lower limit cases, OHint is still more negative than the 1 h LOD in the afternoon. OHint levels less negative than the 1 h LOD can only be achieved by reducing the O3/H2O interference to zero. It is not clear why this is the case.

95

Since the O<sub>3</sub>/H<sub>2</sub>O had to be determined at very high O<sub>3</sub>, one possibility is that, in our instrument, the dependence is nonlinear at ambient O<sub>3</sub> levels.

100

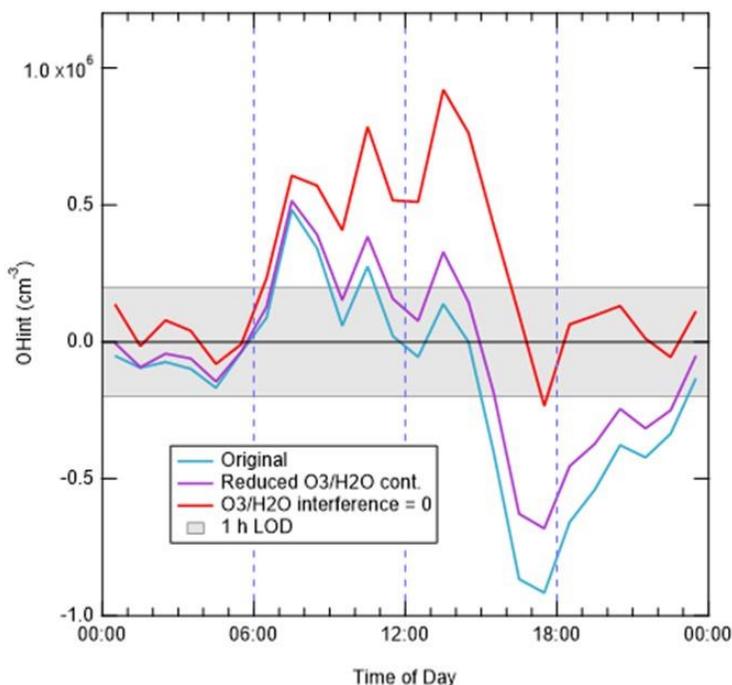


Figure 3. Effect of reducing the known interference from O<sub>3</sub>/H<sub>2</sub>O

P16, line 573: Do the authors have any suggestions for why the nighttime OH levels were so much higher during AIRPRO summer 2017 in comparison to the other two campaigns?

105 Interpretation of the chemistry is beyond the scope of this work but will be discussed in detail in forthcoming manuscripts. It is likely that the AIRPRO summer campaign had much more active NO<sub>3</sub> and ozonolysis chemistry due to high nighttime NO<sub>2</sub>, O<sub>3</sub>, and NO<sub>3</sub>, leading to increased nighttime radical production. In other field campaigns in China, significant nighttime OH concentrations have also been found. For example, in Lu et al. (2014), nighttime OH was up to 3 ×  
110 10<sup>6</sup> molecule cm<sup>-3</sup>, which is higher than the nighttime OH in our work. To reconcile such high OH levels required the inclusion of additional RO<sub>x</sub> production processes in their model.

Lu, K. D., Rohrer, F., Holland, F., Fuchs, H., Brauers, T., Oebel, A., Dlugi, R., Hu, M., Li, X., Lou, S. R., Shao, M., Zhu, T., Wahner, A., Zhang, Y. H., and Hofzumahaus, A.: Nighttime observation and chemistry of HO<sub>x</sub> in the Pearl River Delta and Beijing in summer 2006, *Atmos. Chem. Phys.*,  
115 14, 4979–4999, <https://doi.org/10.5194/acp-14-4979-2014>, 2014.

120 P17, line 578-87: While there are few points of high OH measurements, was any analysis performed on their relationship with BVOCs, O<sub>3</sub>, or temperature? Were these high concentrations measured on different days/times? While it may be limited, the authors are suggested to provide more of an analysis of these points.

Please see our relevant response above. For AIRPRO summer, no clear dependence of OH<sub>int</sub> was found on isoprene, O<sub>3</sub>, or temperature.

125 P18, lines 611-13: The sentence ‘These findings. . .in this type of environment.’ should be reworded or omitted. While one of the field sites showed high BVOC and low NO concentrations, it should not be implied as being representative of a forested environment. While the BVOC and NO conditions may have been similar, other key compounds, such as SO<sub>2</sub>, would have likely been larger, altering the environmental conditions further from that of a forest.

130 We have reworded the sentence to: “Although AIRPRO summer took place in a city, its results do provide confidence in previous measurements of OH using the same instrument, and support the hypothesis that there are unknown OH sources in the atmosphere.”

### Technical corrections

Abstract. P1, line 21: change scavenging to scavenger

135 Done

P3, line 81: either remove the word ‘by’ or change to ‘Mao et al. (2012)’

Done

140 P3, line 82: Lew et al., 2019 should be added as a reference for OH interference measurements in a forested environment

Done

P5, line 175: add reference Rickly and Stevens, 2018

145 Done

P8, line 267: move comma to read as ‘AIRPRO winter, but after’

Done

150 Figure 4: make red and blue markers consistent with graph 3

Done

P9, line 303: remove second 'reduction' in this sentence

Done

155

P12, line 398: change to 'OH removal efficiency of ~12%'

Done

P16, line 567: change 'as' to 'because'

160 Done

P17, line 590: either remove 'of' or change to 'Fittschen et al. (2019)'

Done

165 P17, lines 599-601: The authors are suggested to add 'in moderately to highly polluted environments' to the end of this sentence for clarification.

The sentence has been changed to: "The results from the three field campaigns that feature in this work demonstrate that, in moderately to highly polluted conditions, the Leeds ground-based FAGE instrument does not suffer from substantial interferences in the measurement of OH using the conventional, wavelength-modulation background technique, OHwave."

170

## Response to RC2

### General

175 The paper describes the implementation of a chemical modulation technique for the FAGE-LIF OH instrument operated by the University of Leeds. The purpose of this technical upgrade is to quantify and correct for possible OH interferences, which cannot be detected by the traditionally used laser-excitation wavelength modulation technique. Both operational methods, chemical and wavelength modulation, allow to discriminate OH signals from background that is caused by scattered laser radiation, non-resonant fluorescence, or solar radiation entering the instrument. However, only

180 chemical modulation, in which ambient OH is scavenged by an added reagent in front of the  
instrument inlet, allows the detection and subtraction of signals from OH, which is artificially  
produced inside the instrument. Over the last eight years, some LIF groups have discovered, by use  
of chemical modulation, previously unknown significant interferences due to instrumental OH,  
when measurements were performed in biogenically influenced environments. Currently, it is not  
185 clear which precursors or formation mechanisms are responsible for the observed artefacts. It is  
also not clear how much these interferences depend on the specific instrumental design and its  
operating conditions. The comparison of measured and model simulated OH concentrations in the  
real atmosphere has always been considered as an important test of our understanding of  
atmospheric chemistry. It is obvious that progress in understanding can only be achieved if  
190 atmospheric OH measurements are reliable. The implementation of the chemical modulation  
technique in LIF-FAGE instruments as in the present case is therefore an important step in the  
further development of the research field. The current paper deals with this important topic and is  
worth to be published in AMT.

The paper provides a good overview of the topic and describes in detail the implementation in the  
195 Leeds LIF-FAGE instrument. The authors present interesting results of interference tests in the  
laboratory and of applications of chemical modulation with the Leeds instrument during field  
campaigns in the UK and China. The description of the technique and results is clear and well  
structured. In agreement with laboratory work from other groups, the authors find that OH  
interferences from ozone photolysis, nitrate radicals and ozonolysis of alkenes are generally  
200 negligible at natural atmospheric conditions, or can be sufficiently well corrected (ozone  
photolysis). In relative clean air in UK and in the polluted air in Beijing, China, the authors find no  
evidence of unknown OH artefacts larger than the detection limit. This means that either the  
instrumental design of Leeds is less sensitive to OH artefacts found in other instruments, or that  
different environmental conditions have not supported the formation of such artefacts. In any case,  
205 the application of the new method increases confidence in OH field data obtained by the Leeds  
instrument. I recommend publication of the paper after the authors have addressed my comments  
below.

We thank the reviewer for their kind comments. Below we present the comments of the reviewer  
(blue text), then our responses and any changes in the revised manuscript (black text).

## 210 **Major comments**

Abstract

I am missing a quantitative statement about the possible extent of unknown interferences in the FAGE instrument of Leeds during the AIRPRO and ICOZA campaigns. Please specify upper limits as equivalent OH number densities and fractional contributions to the measured total OH signals (without scavenger) taking into account the measurement errors.

There are a number of ways to estimate an upper limit interference from the data we have presented. One approach would be to take the maximum value of OH<sub>int</sub>. For example, the maximum 1 h OH<sub>int</sub> was  $2.4 \times 10^6$  molecule cm<sup>-3</sup>, accounting for 67% of the total OH<sub>wave</sub> signal at this time. However, 1 h OH<sub>int</sub> values were scattered around zero such that the minimum OH<sub>int</sub> ( $-1.7 \times 10^6$  molecule cm<sup>-3</sup>) had almost the same absolute magnitude. For this reason, we do not think the above method is a fair way to determine upper limit interferences.

Therefore, we have chosen to estimate the upper limit interference from the data presented in Fig. 16. We have added the following sentence as the last sentence in the abstract: “The difference between OH<sub>wave</sub> and OH<sub>chem</sub> (“OH<sub>int</sub>”) was found to scale nonlinearly with OH<sub>chem</sub>, resulting in an upper limit interference of  $(5.0 \pm 1.4) \times 10^6$  molecule cm<sup>-3</sup> at the very highest OH<sub>chem</sub> concentrations measured ( $23 \times 10^6$  molecule cm<sup>-3</sup>), accounting for ~15–20% of the total OH<sub>wave</sub> signal.”

Upper limit fractional contributions (but not absolute number densities) can also be derived from the fits in Figs 10, 12, and 14. The positive 2σ limits of the slopes (i.e., slope + uncertainty) were 1.22, 1.09, and 1.12 for ICOZA, AIRPRO winter, and AIRPRO summer respectively, i.e., upper limit contributions of ~10–20%.

#### Internal OH removal efficiency

The authors present a clever idea to determine the internal removal efficiency of OH by propane. However, I think the evaluation of the data presented in Table 2 needs some revisions. The average value ( $\pm 2\sigma$ ) for the internal removal is given in the text as  $(-0.5 \pm 1.3)\%$  at a propane mixing ratio of 110 ppmv and  $(-2.8 \pm 2.3)\%$  at 1100 ppmv. I believe that the stated errors are too small. The number of experiments mentioned for both cases (Table 2) is rather low (n=3). The calculated standard deviation from such small statistical sample underestimates the error of the mean value. I suggest to calculate weighted means with their standard errors (using error propagation). This would yield  $(0.0 \pm 4.0)\%$  at 110 ppmv propane and  $(2.9 \pm 6.6)\%$  at 1100 ppmv. While the mean values are not much different from the ones given in Table 2, the larger errors seem more plausible.

We agree with the method of error estimation suggested by the reviewer and have amended Table 2 accordingly.

245

An internal OH removal of 12% is theoretically calculated for the case that the sampled OH is exposed to the scavenger (1100 ppmv) for 2 ms on the way from pinhole to laser axis. The experimental value of 2.8% (Table 2) cannot be directly compared with this theoretical estimate, as is done in the paper. In the instrument, OH is built up gradually (in this case linearly) by HO<sub>2</sub> conversion along the line from pinhole to the laserbeam, followed by OH reaction with propane (and NO). In this sequential reaction system, the effective scavenging efficiency is about half the efficiency for OH radicals exposed to the reactant over the entire distance from the inlet to the laser beam. Thus, the experimental value has to be approximately doubled to be comparable with the theoretical estimate. A value of  $2 \times (2.9 \pm 6.6)\% = (5.8 \pm 13)\%$  would not be much different from the theoretical value of 12%. My conclusion is that 10% internal OH loss at 1100 ppmv of propane cannot be ruled out by these laboratory experiments.

250

255

We thank the reviewer for pointing out the flaws in our internal removal experiment and how to better compare the measured and theoretical internal removal. We have added the following discussion to Section 3.1.3:

260

265

“In the internal removal experiment, OH is not formed instantly at the pinhole but is built up linearly by HO<sub>2</sub>/NO conversion along the line from the pinhole to the laser axis. Therefore, the experimental internal removal may not be directly compared with the theoretical estimate. In such a sequential reaction system, the OH scavenging is about half as efficient as that for the case where OH is formed as an instant point source at the pinhole. Thus, the experimental value should be doubled to  $(5.8 \pm 13)\%$ , which is in reasonable agreement with the theoretical value. From this, we cannot rule out a small internal OH removal on the order of 10% at the higher propane level used for the AIRPRO summer campaign. However, no such corrections were applied to the ambient data featured in this work.”

270

#### Intercomparison OHwave and OHchem

In Figure 10, 12 and 14, OHwave is higher than OHchem by 16%, 5%, and 10%, respectively. The discrepancy is statistically significant (i.e., larger than the  $\pm 2\sigma$  statistical errors of the fitted slopes). There must be reasons for the systematic deviations which should be discussed in more detail. I am not satisfied by the statement that the discrepancies can be explained by the instrumental

275 uncertainties (26%,  $\pm 2\sigma$ ). Two measurements are compared which actually use the same  
calibration. Thus, uncertainties of parameters used to quantify the OH production in the wand  
cannot be responsible for the differences between OHwave and OHchem. How much of the  
discrepancy between OHwave and OHchem can be explained by the uncertainty of the O3-H2O  
interference correction in OHwave? Are there other possible reasons? Finally, the differences could  
280 indicate an uncorrected bias due to an unknown interference in OHwave, which, I agree, would be  
smaller than the instrumental uncertainty of 26%.

We agree with the reviewer in that, although the slopes in Figs 10, 12, and 14 indicate small  
contributions from interferences, we cannot rule unknown interferences out since the slopes are all  
significantly greater than 1. We believe the O3/H2O interference has been well characterised and  
285 thus is not the reason for the differences seen between OHwave and OHchem. Therefore, the  
differences must be due to unknown interferences, although these are smaller than the instrumental  
uncertainty of 26% at  $2\sigma$ .

To accommodate the reviewer's suggestions, we have amended the first paragraph in the discussion  
section to:

290 "The results from the three field campaigns that feature in this work demonstrate that, in moderately  
to highly polluted conditions, the Leeds ground-based FAGE instrument does not suffer from  
substantial interferences in the measurement of OH using the conventional, wavelength-modulation  
background technique, OHwave. This is illustrated best by the slopes of the overall measurement  
intercomparison plots (Figures 10, 12, and 14), which ranged from 1.05–1.16. However, while the  
295 deviations of these slopes from 1 are small, they are still significant, suggesting the presence of  
unknown OH interferences. Nonetheless, such unknown interferences are well within the  
instrumental uncertainty of  $\sim 26\%$  at  $2\sigma$ ."

### Minor comments

300 Line 125. SI unit should be used for pressure (e.g., hPa) instead of Torr.

Done

Line 149. initially to HO2 and subsequently to OH ?

In the ROxLIF flow tube, RO<sub>2</sub> is converted all the way to OH using NO, then reconverted back to HO<sub>2</sub> using CO. Inside the FAGE cell, the HO<sub>2</sub> is then converted once more to OH using NO. To clarify this, we have modified the sentence as follows:

“Although not reported here, RO<sub>2</sub> radicals are measured using the RO<sub>x</sub>LIF method (Fuchs et al., 2008; Whalley et al., 2013), in which their reactions with NO and CO (BOC, 5% in N<sub>2</sub> and Messer, 10% in N<sub>2</sub>) result in conversion initially to OH (using NO; RO<sub>2</sub> → HO<sub>2</sub> → OH) and subsequently back to HO<sub>2</sub> (using CO; OH → HO<sub>2</sub>) that is then detected as described above (via addition of NO inside the FAGE cell; HO<sub>2</sub> → OH).”

Line 290-295. It should be explicitly stated that the determination of OH<sub>wave</sub> and OH<sub>chem</sub> uses the same calibration, which is carried out without IPI under the assumption of negligible transmission losses with IPI.

We have added the following sentence to Section 3.1.1:

“In other words, we assume negligible transmission losses within the IPI and the OH calibration factor we applied to ambient data was the same for (1) OH<sub>wave</sub> without IPI sampling, (2) OH<sub>wave</sub> during IPI sampling, and (3) OH<sub>chem</sub> during IPI sampling. However, it should be noted that in the field, calibrations are normally carried out without the IPI system present.”

Line 290-295. For the given IPI conditions, I calculate a Reynolds number of 2290. This value is close to the critical point where laminar flow becomes turbulent. The state of the flow is expected to influence the mixing of the scavenger in the IPI flow and the loss rate of OH at the walls. Have the authors tested, how sensitive the scavenging efficiency and tube transmission depends on the IPI flow rate?

In preliminary experiments, it was found that the OH transmission through the IPI increased with sheath flow rate (range: 0–25 slm) until the air sent through the wand (max 40 slm) was no longer sufficient to overflow the inlet (sheath flow = 25 slm, total flow through IPI = 32 slm). The increase in transmission with flow is likely due to reduced contact with the walls at faster flow, despite the increased turbulence. Since we observed maximum transmission at the limits of our experimental setup, we settled on those experimental conditions for all future experiments and ambient studies.

335 Similarly, although we did not test whether the sheath flow rate affected scavenging efficiency, we did test the N<sub>2</sub> dilution flow. Again, the maximum scavenging efficiency was observed at the maximum of the MFC used (500 sccm), so we used these flow conditions for all further tests.

Line 345. I assume you mean (0.030±0.091)% instead of 0.030±0.091% ? Check also other instances in the paper.

340 All instances corrected

Line 387. The number for the internal removal of  $-0.5 \pm 1.3\%$  is not consistent with the value in Table 2 showing  $-0.2 \pm 1.1\%$ .

This was corrected to  $(0.0 \pm 4.4)\%$  based on the discussion of weighted averages above.

345

Line 413. I assume, the water level is given as a volume mixing ratio and not as relative humidity. Please clarify.

We mean volume mixing ratio, this has been clarified.

350 Line 435. How long is the reaction time for isoprene and ozone before the gas is entering the pinhole of the FAGE cell?

Line 444. Which material was used for the additional 30cm flow tube?

Line 445. What is the meaning of ' $\tau = 0.15 \text{ s}$ ' ?

We have amended the relevant paragraph to (changes highlighted):

355 “To test for interferences from isoprene (ISO) ozonolysis products, isoprene (~16 ppmv) and ozone (~1.8 ppmv) were mixed in the calibration wand and the scavenger (propane, PROP) was injected into the IPI flow tube. The propane concentrations were set to those used for ambient OHchem measurements, such that the tests were representative of normal atmospheric sampling (i.e., to test whether an interference signal would remain in ambient data). However, to generate sufficient OH  
360 signal for quantitative analysis, ozone and isoprene were introduced at concentrations that far exceeded their typical ambient levels (Table 3). Unlike previous tests of interferences from alkene ozonolysis (Novelli et al., 2014b), low [O<sub>3</sub>]:[ISO] ratios were used to suppress the signal

contribution from the atmospheric (real) OH generated by ozonolysis (i.e., isoprene acted as an additional OH scavenger). To allow sufficient time for steady-state conditions to develop, the IPI did not sample from the calibration wand directly, but instead a 30 cm flow tube (polycarbonate, ID ~ 19 mm) was used to extend the IPI (which sampled wand gas at the normal IPI flow rate of ~32 slm, residence time for O<sub>3</sub> + isoprene reaction ~ 0.15 s).”

370 Table 1, footnotes. Labels are missing in the table body.

Amended

Table 3. Column width of 'Obs' needs reformatting.

375 Table reformatted

Table 4. What is the meaning of the \* symbol for the daytime contribution in the CalNexLA study?

The \* symbol means that the interference was consistent with the known O<sub>3</sub>/H<sub>2</sub>O interference; we have added a footnote to clarify this.

380 Nighttime column: what is the conceptual difference between ~ 0 (e.g., PROPHET, AIRPRO summer) and 'Nighttime OH almost always < LOD' (AIRPRO Winter)?

For this column in the table, we put values of ~ 0 for campaigns in which OH was measured above the LOD at night, but OH<sub>wave</sub> and OH<sub>chem</sub> were virtually the same. For AIRPRO winter, this was not the case and so it cannot be explicitly stated that the nighttime contribution was 0.

385 The reported OH interferences in the PRIDE-PRD2014 campaign made contributions up to 8% during daytime and up to 20% at sunset and nighttime.

The daytime contribution has been amended to <8%.

390 Fig. 4, 6, 7c, and 9. Error bars are much larger than the scatter of the shown data. Therefore, the error bars do not seem to represent the precision of the shown data. If you show mean values of

repeat experiments, you may want to display the statistical error of the mean rather than of single measurements.

The error bars in Figs. 4, 6, 7 (a, b, and c) and 9 have all been reduced from  $2\sigma$  to  $1\sigma$  to better reflect the apparent precision of the data. Please note, that since weighted fits were used in Fig. 7, this has  
395 changed the slope in Fig. 7A and hence the scaling factor in equation (E7).

Figure 1. Insert a scale to illustrate the size of the IPI.

Scale added

400 Figure 4. Consider to include the diurnal profile of jO1D scaled to OH; as jO1D and OH often correlate extremely well, it could help to visualise the expected trend of OH while the IPI switches between modes.

jO1D profile added

405

Figure 6. For better understanding, you could add in the figure caption the information that OH is internally formed in the cell by the conversion of HO<sub>2</sub> with added NO.

Caption amended to:

Time series of the LIF signal during internal OH removal experiments. The raw 1 s data are given  
410 by the grey line. NO was continuously added to the FAGE cell during these experiments (to form OH internally), and points where propane was added to the IPI flow tube are indicated by the orange shaded panels, with the corresponding signal averages ( $\pm 1\sigma$ ) shown as markers (see text for details). The first experiment (left-hand side) corresponds to the propane mixing ratio used for ICOZA, while the second (right-hand side) corresponds to that used for AIRPRO summer. The results of  
415 the internal OH removal experiments are summarised in Table 2.

Figure 8. The y-axis is labelled 'HOx' cell signal. Please clarify: was the sum of OH and HO<sub>2</sub> measured (i.e., with added NO), or only OH (without added NO) ?

NO was not added in these experiments. The HOx label is used to discriminate the fluorescence  
420 cell normally used for ambient OH and HO2 measurements from the reference cell. Since HO2 is  
not relevant to this experiment, we have modified the label to “OH cell”.

425

430

435

440

# Implementation of a chemical background method for atmospheric OH measurements by laser-induced fluorescence: characterisation and observations from the UK and China

Robert Woodward-Massey<sup>1,a</sup>, Eloise J. Slater<sup>1</sup>, Jake Alen<sup>1</sup>, Trevor Ingham<sup>1,2</sup>, ~~Daniel~~Danny R. Cryer<sup>1</sup>, Leanne M. Stimpson<sup>1</sup>, Chunxiang Ye<sup>1,a</sup>, Paul W. Seakins<sup>1</sup>, Lisa K. Whalley<sup>1,2</sup> and Dwayne E. Heard<sup>1</sup>

<sup>1</sup>School of Chemistry, University of Leeds, Leeds, LS2 9JT, UK

<sup>2</sup>National Centre for Atmospheric Science, University of Leeds, Leeds, LS2 9JT, UK

<sup>a</sup>now at: College of Environmental Sciences and Engineering, Peking University, Beijing, 100871, China

*Correspondence to:* L. K. Whalley (l.k.whalley@leeds.ac.uk) and D. E. Heard (d.e.heard@leeds.ac.uk)

**Abstract.** Hydroxyl (OH) and hydroperoxy (HO<sub>2</sub>) radicals are central to the understanding of atmospheric chemistry. Owing to their short lifetimes, these species are frequently used to test the accuracy of model predictions and their underlying chemical mechanisms. In forested environments, laser-induced fluorescence–fluorescence assay by gas expansion (LIF–FAGE) measurements of OH have often shown substantial disagreement with model predictions, suggesting the presence of unknown OH sources in such environments. However, it is also possible that the measurements have been affected by instrumental artefacts, due to the presence of interfering species that cannot be discriminated using the traditional method of obtaining background signals via modulation of the laser excitation wavelength (“OHwave”). The interference hypothesis can be tested by using an alternative method to determine the OH background signal, via the addition of a chemical ~~scavenging~~scavenger prior to sampling of ambient air (“OHchem”). In this work, the Leeds FAGE instrument was modified to include such a system to facilitate measurements of OHchem, in which propane was used to selectively remove OH from ambient air using an inlet pre-injector (IPI). The IPI system was characterised in detail, and it was found that the system did not reduce the instrument sensitivity towards OH (<5% difference to conventional sampling), and was able to efficiently scavenge external OH (>99%) without the removal of OH formed inside the fluorescence cell (<5%). Tests of the photolytic interference from ozone in the presence of water vapour revealed a small but potentially significant interference, equivalent to an OH concentration of  $\sim 4 \times 10^5$  molecule cm<sup>-3</sup> under typical atmospheric conditions of [O<sub>3</sub>] = 50 ppbv and [H<sub>2</sub>O] = 1%. Laboratory experiments to investigate potential interferences from products of isoprene ozonolysis did result in interference signals, but these were negligible when extrapolated down to ambient ozone and isoprene levels. The interference from NO<sub>3</sub> radicals was also tested but was found to be insignificant in our system. The Leeds IPI module was deployed during three separate field intensives that took place in summer at a coastal site in the UK, and both in summer and winter in the megacity Beijing, China, allowing for investigations of ambient OH interferences under a wide range of chemical and meteorological conditions. Comparisons of ambient OHchem measurements to the traditional OHwave method showed excellent agreement, with OHwave vs OHchem slopes of 1.05–1.16 and

480 identical behaviour on a diel basis, consistent with laboratory interference tests. The difference between OHwave and OHchem (“OHint”) was found to scale nonlinearly with OHchem, resulting in an upper limit interference of  $(5.0 \pm 1.4) \times 10^6$  molecule  $\text{cm}^{-3}$  at the very highest OHchem concentrations measured ( $23 \times 10^6$  molecule  $\text{cm}^{-3}$ ), accounting for ~15–20% of the total OHwave signal.

## 1 Introduction

485 The removal of pollutants and greenhouse gases in the troposphere is dominated by reactions with the hydroxyl radical (OH), which is closely coupled to the hydroperoxy radical ( $\text{HO}_2$ ). Comparisons of the levels of OH and  $\text{HO}_2$  observed during field campaigns to the results of detailed chemical box models serve as a vital tool to assess our understanding of the underlying chemical mechanisms involved in tropospheric oxidation. Laser-induced fluorescence–fluorescence assay by gas expansion (LIF–FAGE) measurements of  
490 OH in forested environments have often been considerably higher than those predicted by models (Carslaw et al., 2001; Lelieveld et al., 2008; Ren et al., 2008; Hofzumahaus et al., 2009; Stone et al., 2011; Whalley et al., 2011; Wolfe et al., 2011). The difficulty in simulating radical concentrations in such environments has prompted a multitude of theoretical (Peeters et al., 2009; da Silva et al., 2010; Nguyen et al., 2010; Peeters and Muller, 2010; Peeters et al., 2014), laboratory (Dillon and Crowley, 2008; Hansen et al., 2017), and  
495 chamber (Paulot et al., 2009; Crouse et al., 2011; Crouse et al., 2012; Wolfe et al., 2012; Fuchs et al., 2013; Fuchs et al., 2014; Praske et al., 2015; Teng et al., 2017; Fuchs et al., 2018) studies to help explain the sources of the measurement–model discrepancy, through detailed investigations of the mechanism of isoprene oxidation under low  $\text{NO}_x$  conditions, as well as other biogenic volatile organic compounds (BVOCs) (Novelli et al., 2018). However, another hypothesis is that the LIF measurements have, at least in part, suffered from  
500 an instrumental bias in these environments due to interfering species.

Early LIF measurements of OH suffered from significant interferences due to laser-generated OH from ozone photolysis in the presence of water vapour (Hard et al., 1984). While this effect has been reduced in going from 282 to 308 nm laser excitation of OH, it may still be significant, especially at night or with the use of multi-pass laser setups (e.g., up to  $\sim 4 \times 10^6$  molecule  $\text{cm}^{-3}$  in Griffith et al. (2016)). Laboratory  
505 experiments conducted by Ren and co-workers using the Pennsylvania State University (PSU) LIF instrument showed negligible interferences in OH detection for a range of candidate species:  $\text{H}_2\text{O}_2$ , HONO, HCHO,  $\text{HNO}_3$ , acetone, and various  $\text{RO}_2$  radicals (Ren et al., 2004). Observations of OH during the PROPHET (Program for Research on Oxidants: PHotochemistry, Emissions and Transport) field campaign in summer 1998, located in a mixed deciduous forest in Michigan, USA, revealed unusually high nighttime OH  
510 concentrations ( $\sim 1 \times 10^6$  molecule  $\text{cm}^{-3}$ ) but measurement interferences were ruled out (Faloona et al., 2001).

However, the results of more recent studies conducted in forested environments have meant that interferences in the measurement of OH by LIF–FAGE have been revisited. The usual background method of this technique, where the laser wavelength is scanned off-resonance from an OH transition (“OHwave”), does not discriminate between ambient (i.e., “real”) OH and either OH formed inside the FAGE cell (e.g.,  
515 laser- or surface-generated OH, or via unimolecular decomposition in the gas phase to form OH), or

fluorescence from other species at  $\lambda \sim 308$  nm (e.g., naphthalene,  $\text{SO}_2$ ), although it is possible to correct for such effects providing the interference has been previously characterised (Martinez et al., 2004; Ren et al., 2004; Griffith et al., 2013; Fuchs et al., 2016). There is an alternative, chemical method (“OHchem”) for obtaining the OH background signal in LIF instruments that allows for interference signals to be determined without their prior characterisation, to rule out possible artefacts from unknown species. The OHchem method involves the addition of a high concentration of an OH scavenger, such as perfluoropropene ( $\text{C}_3\text{F}_6$ ) or propane, just before the FAGE inlet. Ambient OH is quickly titrated away by fast reaction with the scavenger, but any interference should remain in the fluorescence signal, although this must be corrected for reaction of any internally generated OH with the scavenger inside the FAGE cell.

Several LIF–FAGE groups have now made efforts to validate ambient OH measurements through incorporation of the alternative OHchem technique, which was first applied for continuous OH measurements by (Mao et al., 2012). Since then, field studies of OH measurement interferences have been conducted in forested (Griffith et al., 2013; Novelli et al., 2014a; Feiner et al., 2016; Novelli et al., 2017; [Lew et al., 2019](#)), rural (Fuchs et al., 2017; Tan et al., 2017), suburban (Tan et al., 2018; Tan et al., 2019), urban (Ren et al., 2013; Brune et al., 2016; Griffith et al., 2016), and coastal (Novelli et al., 2014a; Mallik et al., 2018) locations. Substantial improvement in measurement–model agreement has been possible when OH backgrounds were determined chemically, especially in forested environments, suggesting that understanding of tropospheric oxidation processes in such regions may be better than previously thought (Mao et al., 2012; Hens et al., 2014; Feiner et al., 2016). This is further supported by the positive identification of two new OH interference candidates in laboratory experiments, namely intermediates in alkene ozonolysis reactions, which may (Novelli et al., 2014b; Novelli et al., 2017; Rickly and Stevens, 2018) or may not (Fuchs et al., 2016) be related to stabilised Criegee intermediates (SCIs), and the  $\text{NO}_3$  radical (Fuchs et al., 2016) although for all cases the observed interferences cannot explain the magnitudes of the OH background signals under ambient conditions. The trioxide species, ROOOH, has also been postulated to explain elevated OH backgrounds in LIF–FAGE measurements made in forested regions (Fittschen et al., 2019).

However, it is not known whether other LIF instruments suffer the same levels of interference, which are likely highly dependent on cell design and operating parameters, especially the residence time of air between sampling and detection (Novelli et al., 2014a; Fuchs et al., 2016; Rickly and Stevens, 2018). Considering the bespoke nature of LIF–FAGE instruments, those of different groups share the same main features but differ in many aspects, such as inlet size and shape, or whether the laser crosses the detection axis once (i.e., single-pass) or multiple times (multi-pass). As a result, the magnitude of any interference is likely to vary significantly between different instruments. Because of this, a general recommendation of the 2015 International  $\text{HO}_x$  Workshop (Hofzumahaus and Heard, 2016) was that different groups should incorporate their own chemical scavenger system for use in ambient OH measurements, and to test interferences in the laboratory.

Following this recommendation, the Leeds ground-based FAGE instrument was modified to incorporate a chemical scavenger system, through the addition of an inlet pre-injector (IPI). In this work, we describe the

design of the IPI system and its thorough characterisation in terms of sensitivity and the degree of external and internal OH removal. Following this, we present the results of interference testing experiments performed using the IPI system, in which we investigated interferences from  $O_3 + H_2O$ , isoprene ozonolysis, and  $NO_3$  radicals. Finally, we demonstrate the use of the optimised IPI system for measurements of ambient OH made during three separate field campaigns in the UK and China, which encompassed a wide range of chemical and meteorological conditions.

## 2 Methodology

### 2.1 Overview of the Leeds ground-based FAGE instrument

The University of Leeds ground-based FAGE instrument, described in detail elsewhere (Creasey et al., 1997a; Whalley et al., 2010; Whalley et al., 2013), has participated in 24 intensive field campaigns since its initial deployment in 1996. Measurements of OH,  $HO_2$ , and, more recently,  $RO_2$  radicals (Whalley et al., 2013), have been made in a variety of locations, ranging from pristine marine boundary layer (Creasey et al., 2003; Whalley et al., 2010), tropical rainforest (Whalley et al., 2011), and polar (Bloss et al., 2007) environments, to coastal (Smith et al., 2006) and semi-polluted regions (Creasey et al., 2001), as well as urban areas (Heard et al., 2004; Emmerson et al., 2007) including a highly polluted megacity (Lee et al., 2016; Whalley et al., 2016).

Ambient OH is measured using laser-induced fluorescence. Briefly, ambient air is drawn through a 1.0 mm diameter pinhole in a conical turret inlet (4 cm length, 3.4 cm ID; Figure 1) at  $\sim 7$  slm into a stainless steel fluorescence cell, held at  $\sim 1.5$  Torr (2 hPa) using a Roots blower (Leybold RUVAC WAU 1001) backed by a rotary pump (Leybold SOGEVAC SV200). An all solid-state laser system is used to excite OH via the  $A^2\Sigma^+(v' = 0) \leftarrow X^2\Pi_{3/2}(v'' = 0)$  electronic transition at  $\lambda = 308$  nm ( $HO_2$  is measured by conversion to OH using NO, details below). The resultant fluorescence at 308 nm is detected by a micro-channel plate photomultiplier (MCP, Photek PMT325/Q/BI/G with 10 mm diameter photocathode) equipped with a 50 ns gating unit (Photek GM10-50) and a 2 GHz 20 dB gain amplifier (Photek PA200-10), and the signal analysed by gated photon counting (Whalley et al., 2010). The background signal is normally obtained by scanning the laser wavelength off-resonance from the OH transition line, yielding the measurement commonly referred to as OHwave:

$$\begin{aligned} [\text{OHwave}] &= C_{\text{OH}} \times (S_{\text{online}}^{\text{OH}} - S_{\text{offline}}^{\text{OH}}) \\ &= C_{\text{OH}} \times S^{\text{OH}} \end{aligned} \quad (1)$$

where  $C_{\text{OH}}$  is the instrument calibration factor for OH, and  $S_{\text{online}}^{\text{OH}}$  and  $S_{\text{offline}}^{\text{OH}}$  are the OH LIF signals at on- and off-resonance wavelengths, respectively. Similarly, the alternative measurement known as OHchem is defined as:

$$[\text{OHchem}] = C_{\text{OH}} \times (S_{\text{online}}^{\text{OH}} - S_{\text{online, scavenger}}^{\text{OH}})$$

$$= C_{\text{OH}} \times S_{\text{scavenger}}^{\text{OH}} \quad (2)$$

590 where  $S_{\text{online, scavenger}}^{\text{OH}}$  is the OH signal measured at an on-resonance wavelength but in the presence of a scavenger.

HO<sub>2</sub> is detected via its conversion to OH following the addition of NO (BOC, 99.95% and Messer, 99.95%). Although not reported here, RO<sub>2</sub> radicals are measured using the RO<sub>x</sub>LIF method (Fuchs et al., 2008; Whalley et al., 2013), in which their reactions with NO and CO (BOC, 5% in N<sub>2</sub> and Messer, 10% in N<sub>2</sub>) result in conversion initially to OH (using NO; RO<sub>2</sub> → HO<sub>2</sub> → OH) and subsequently back to HO<sub>2</sub> (using CO; OH → HO<sub>2</sub>) that is then detected as described above- (via addition of NO inside the FAGE cell; HO<sub>2</sub> → OH). The NO and CO are delivered using mass flow controllers (MFC, MKS Instruments 1179A series), which, unless otherwise stated, were also used to control all other gas flows described in this work. The Leeds FAGE instrument features two fluorescence cells, where laser light (~10–20 mW at 308 nm, supplied at a pulse repetition frequency of 5 kHz via an optical fibre) enters each cell in series. For normal operation in the field, the first cell (HO<sub>x</sub>) measures OH and HO<sub>2</sub> (low NO flow, 5 sccm; RO<sub>2</sub> interference minimised) sequentially, while the second cell (RO<sub>x</sub>) measures HO<sub>2</sub>\* (high NO flow, 50 sccm; RO<sub>2</sub> interference maximised) and then total RO<sub>2</sub> (Fuchs et al., 2008; Whalley et al., 2013).

600 Calibration of the FAGE instrument is achieved by supplying known radical concentrations via a turbulent flow tube (known in Leeds as the “wand”) held at ~45° to the instrument inlet, where OH and HO<sub>2</sub> are formed in a 1:1 ratio (Fuchs et al., 2011) by the photolysis of water vapour at 184.9 nm using a Hg(Ar) pen-ray lamp (LOT LSP035) in an excess flow (40 slm) of humidified ultra-high purity air (BOC, BTCA 178 and Messer, 20.5% O<sub>2</sub> in N<sub>2</sub>). Chemical actinometry is performed via the photolysis of N<sub>2</sub>O (BOC, medical grade 98%) to measure the product of lamp flux and photolysis exposure time to enable calculation of radical concentrations (Edwards et al., 2003; Faloon et al., 2004). The calibration of OH using the water vapour photolysis method has been validated by comparison with other methods, for example the kinetic decay of hydrocarbons (Winiberg et al., 2015).

## 2.2 Inlet pre-injector (IPI) design

615 The Leeds inlet pre-injector (Figure 1) is similar in concept to the design of Mao et al. (2012) and consists of a 4.0 cm length, 1.9 cm ID perfluoroalkoxy (PFA) cylinder embedded inside an aluminium housing, which seals to the FAGE cell via an O-ring base. The scavenger is injected into the centre of the PFA flow tube via four 0.25 mm ID needles, 4.0 cm above the FAGE inlet. The low bore capillary tubing increases the pressure inside the needles, which facilitates mixing of the scavenger into the ambient air stream. In this work propane (BOC, research grade 99.95% and Messer, 99.995%) was used as the main OH chemical scavenger, with similar results (see section 3.1.2) obtained for C<sub>3</sub>F<sub>6</sub> (Sigma-Aldrich, 99%). Based on previous investigations of OH interferences (Stevens et al., 1994; Dubey et al., 1996; Faloon et al., 2001; Ren et al., 2004; Mao et al., 2012; Griffith et al., 2013; Rickly and Stevens, 2018), C<sub>3</sub>F<sub>6</sub> was used initially as it reacts quickly and selectively with OH ( $k_{298} = 2.2 \times 10^{-12} \text{ cm}^3 \text{ molecule}^{-1} \text{ s}^{-1}$  (Sander et al., 2011)), and does not contain any

hydrogen atoms which could serve as a source of laser-generated OH via abstraction by O(<sup>1</sup>D) atoms (Stevens et al., 1994; Dubey et al., 1996). However, C<sub>3</sub>F<sub>6</sub> must be diluted in an inert gas before it can be flowed through MFCs, and its availability in the UK became limited in 2015. Following Novelli et al. (2014a), we therefore used propane for most laboratory experiments and all ambient measurements, despite the fact that it reacts more slowly with OH ( $k_{298} = 1.1 \times 10^{-12} \text{ cm}^3 \text{ molecule}^{-1} \text{ s}^{-1}$  (Sander et al., 2011)).

As shown in Figure 2, the scavenger (0–50 sccm) is diluted in a flow of N<sub>2</sub> (500 sccm, BOC, 99.998%) prior to injection, which is controlled using a solenoid valve (Metron Semiconductors). Any dead volume after the valve is purged continuously by the N<sub>2</sub> dilution flow, using a narrow-bore injector inserted through the tee after the valve, with the injector tip placed as close to the valve orifice as possible. This enables fast flushing of the system to optimise the response time before and after scavenger injection. Incorporation of the purge system resulted in pre- and post-injection stabilisation times on the order of seconds (data not shown), minimising data loss. The valve state and scavenger flow over the course of the data acquisition cycle are controlled using a custom program nested within the FAGE software.

To reduce radical wall losses, excess ambient air is drawn through the IPI to generate a sheath flow, via four ports spaced evenly around the flow tube housing as shown in Figure 1. This minimises the FAGE sampling of air from near the walls of the cylinder, housing, and turret. The total flow rate through the IPI is 32 slm, of which 7 slm is sampled by the FAGE cell and the remainder of the flow is maintained by a vacuum pump (Agilent Technologies IDP-3 Dry Scroll Pump) and measured volumetrically using a rotameter (Brooks 2520, 4–50 L min<sup>-1</sup>).

During interference testing experiments using the IPI system (section 3.2), ozone and water vapour concentrations were measured using a commercial UV absorption instrument (Thermo Environmental Instruments Inc. 49C) and a chilled mirror dew point hygrometer (General Eastern 1311DR sensor and 4×4 Optica), respectively.

### 2.3 Field measurement sites

Ambient measurements of OHwave and OHchem were made using the Leeds IPI–FAGE instrument during three separate intensive field campaigns, in different locations and seasons. This allowed for the investigation of potential OH interferences under markedly contrasting conditions. For all three field campaigns, measurements of OH, HO<sub>2</sub>, and partially speciated RO<sub>2</sub> were made using the Leeds FAGE instrument (4 m above ground level), operated in the sequential detection modes described in section 2.1 (Whalley et al., 2013). Total OH reactivity,  $k'_{\text{OH}}$ , was also measured, using the laser flash photolysis–LIF instrument described in detail by (Stone et al., 2016). A range of supporting chemical, aerosol, and meteorological parameters were measured, with instruments situated either in buildings or shipping containers at each of the two sites. Gas phase chemical observations included water vapour, NO<sub>x</sub>, NO<sub>y</sub>, O<sub>3</sub>, CO, SO<sub>2</sub>, HONO, HCHO (Cryer, 2016), ClNO<sub>2</sub>, VOCs, and OVOCs. Photolysis rates ( $J$ ) for a variety of species, including O<sub>3</sub> (→ O(<sup>1</sup>D)), NO<sub>2</sub>, HCHO, HONO, and ClNO<sub>2</sub>, were measured using a 2π spectral radiometer (2π actinic receiver optic (Meteorologie Consult GmbH) coupled to an Ocean Optics QE Pro spectrometer), and  $J(\text{O}^1\text{D})$  was also

660 measured using a  $2\pi$  filter radiometer (Meteorologie Consult GmbH) (Bohn et al., 2008). The meteorological  
and chemical conditions, including some example VOCs, encountered during each campaign are summarised  
in Table 1 and discussed in further detail below.

The first deployment of the Leeds IPI was during the ICOZA (Integrated Chemistry of OZone in the  
Atmosphere) project, which took place in July 2015, at the Weybourne Atmospheric Observatory (WAO),  
665 Weybourne, located on the North Norfolk Coast, UK ( $52^{\circ}57'02''\text{N}$ ,  $1^{\circ}07'19''\text{E}$ , 15 m asl). The WAO is a  
Global Atmospheric Watch (GAW) Regional station, and the site is impacted by a range of contrasting air  
masses, from clean Arctic air to processed emissions from the UK (e.g., London, which is located  $\sim 180$  km  
SSW of the observatory) and Northern Europe. The aim of this field campaign was to improve understanding  
of ozone chemistry through integrated measurements of  $P(\text{O}_3)$ , the chemical or *in situ* ozone production rate  
670 (OPR) (Cazorla and Brune, 2010; Cazorla et al., 2012), with comparisons to a range of other observational  
and model approaches. Two continuous IPI sampling periods were conducted in the middle of the campaign,  
separated by a few days (3<sup>rd</sup>–8<sup>th</sup> July and 12<sup>th</sup>–16<sup>th</sup> July), with a total of nine days where OHchem  
measurements are available around midday. For other times, only measurements of OHwave are available.  
During the IPI sampling periods, power cuts on the nights of 3<sup>rd</sup>/4<sup>th</sup> July and 6<sup>th</sup>/7<sup>th</sup> July resulted in data loss.

675 In general, the ICOZA campaign was characterised (Table 1) by moderate temperatures ( $16^{\circ}\text{C}$  median),  
high humidity (RH  $\sim 80\%$ ), and strong wind speeds ( $\sim 6\text{ m s}^{-1}$ ), as might be expected at a temperate, coastal  
location in the summertime. The predominant wind sector, based on wind direction measurements at the site,  
was westerly ( $\sim 30\%$ ), followed by southwesterly ( $\sim 20\%$ ) and southerly ( $\sim 15\%$ ). Back-trajectory analysis  
showed that during IPI sampling periods, the site was predominantly under the influence of Atlantic air  
680 (Cryer, 2016). These air masses had spent a considerable amount of time ( $\sim 1$  day) over the UK, often  
encountering emissions from urban areas, which underwent photochemical aging during their transport to the  
WAO site. Overall, the levels of pollution observed at the site were moderate, and the lowest of the three  
field campaigns discussed in this work (Table 1), and levels of isoprene were low. However, ozone mixing  
ratios were relatively high, with a diel-average maximum of  $\sim 40$  ppbv, driven in part by strong UV and near-  
685 UV radiation.

The Leeds IPI was deployed during another two campaigns at the Institute of Atmospheric Physics (IAP,  
 $39^{\circ}58'36.06''\text{N}$ ,  $116^{\circ}22'53.69''\text{E}$ ), an urban site in Beijing, China, during winter (November–December)  
2016 and summer (May–June) 2017, as part of the AIRPRO (an integrated study of AIR pollution PROCesses  
in Beijing) project. AIRPRO is part of the wider APHH (Air Pollution and Human Health in a Chinese  
megacity) project (Shi et al., 2018), a joint UK–China programme. The aims of AIRPRO included the  
690 assessment of how pollutants are transformed and removed through transport, chemical, and photolytic  
processes, with a particular emphasis on the identification of the dominant oxidative degradation pathways  
(i.e., the relative importance of reactions with OH,  $\text{NO}_3$ , and  $\text{O}_3$ ). The AIRPRO project allowed for the  
assessment of OH measurement interferences under the highly polluted conditions of the megacity Beijing,  
695 situated in the heavily industrialised North China Plain. In winter, the site is impacted by urban and regional  
anthropogenic emissions, in particular those from the combustion of fossil fuels for residential heating.

During summer, the site is subject to additional biogenic influences, and strong photochemical activity results in high rates of ozone production. In winter, OHwave and OHchem were measured simultaneously for 6 days of the campaign. In summer, almost one month of near-continuous IPI data are available, with one day of interruptions due to IPI testing (see Section 3.1.2).

For both AIRPRO field intensives, the predominant wind sectors were westerly and southerly/southeasterly, which generally result in higher pollutant concentrations (Chen et al., 2015). Indeed, the two campaigns were subject to high pollutant concentrations, as illustrated by the elevated levels of NO<sub>2</sub>, CO, propane, benzene, and  $k'_{\text{OH}}$ , many of which were over an order of magnitude higher than ICOZA (Table 1). In addition, the biogenic influence during summer is clear from the relatively high isoprene concentrations observed, ~0.4 ppbv on average but reaching up to 7.9 ppbv, a level considerably higher than those observed in some forested environments. Despite similar  $J(\text{O}^1\text{D})$  values between ICOZA and AIRPRO summer, the higher VOC loadings during the latter resulted in increased production of ozone (90 ppbv diurnally-averaged maximum). In contrast, AIRPRO winter was characterised by small ozone mixing ratios (15 ppbv diurnal maximum), as a consequence of high NO levels (median 22 ppbv) and weak UV radiation. In summer, NO levels were high in the morning (~14 ppbv at 06:00 China Standard Time (CST)) but surprisingly low in the afternoon, with diel-average median levels of ~0.5 ppbv (15:00–18:00 CST).

For all ambient observation periods, the IPI data acquisition cycle consisted of 5 minutes of online wavelength and 30 seconds of offline wavelength (spectral background) integration, where the online period was split into 2 minutes of OH measurements and 2 minutes of propane addition to the IPI flow tube (chemical background), followed by 1 minute of HO<sub>2</sub> measurements (by the addition of NO to the FAGE cell). In terms of instrumental operation, the only difference between ICOZA and the AIRPRO campaigns was the use of different propane flows in the IPI. The propane concentration in the IPI flow tube was ~110 ppmv ( $k'_{\text{OH}} \sim 3000 \text{ s}^{-1}$ ,  $\tau_{\text{OH}} \sim 0.3 \text{ ms}$ ) during ICOZA and AIRPRO winter, but, after internal removal experiments revealed that the propane level could be increased further (see section 3.1.3), a ten-fold higher concentration (~1100 ppmv), resulting in a concomitant reduction in the OH lifetime, was used for the AIRPRO summer campaign. On one day with high ozone (up to ~80 ppbv) and moderate isoprene (~0.5–1 ppbv) levels, the propane mixing ratio was reduced to ~110 ppmv, but this had no observable effect on the background signals obtained for the summer data. All ambient OHwave data presented here have been corrected for the known interference from O<sub>3</sub> in the presence of H<sub>2</sub>O vapour (see section 3.2.1).

## 3 Results

### 3.1 IPI characterisation

#### 3.1.1 Sensitivity

The presence of additional surfaces in the IPI system may result in radical wall losses and therefore reduce the overall FAGE instrument sensitivity. To test for potential OH losses in the IPI flow tube, OH radicals were generated using a 184.9 nm Hg lamp placed at ~19 cm from the instrument inlet, so that ambient air

with elevated radical concentrations ( $\sim 2-7 \times 10^7$  molecule  $\text{cm}^{-3}$ ) was sampled, alternating between IPI and non-IPI sampling (Figure 3), where for the latter the entire IPI assembly was removed. The dominant source of OH was the photolysis of ambient water vapour at 184.9 nm. In these experiments, the Hg lamp was placed sufficiently far away from each inlet within a large tent enclosure on the container roof, such that it could be assumed that OH concentrations were uniform in the region the inlet sampled from. Otherwise, the difference in inlet height between IPI and non-IPI sampling may have resulted in different OH concentrations being sampled, e.g., due to differences in  $\text{O}_3$  absorption at 184.9 nm ( $\text{O}_3$  has a high cross-section at this wavelength), which would affect the light flux at the point of sampling and hence the concentration of OH generated. Since ambient variability (e.g., in  $\text{NO}_x$  levels) also affects the atmospheric radical concentrations, the IPI/non-IPI cycle was repeated several tens of times on three different days within the tent enclosure to ensure sufficient averaging of the results. Any differences in wind speed or direction during the different days are not important because of the tent enclosure. Based on the averages for each set of repeat measurements in Figure 3, these experiments yield a mean  $\pm 2\sigma$  IPIoff/IPIon ratio of  $1.043 \pm 0.023$ , i.e., a  $<5\%$  sensitivity reduction due to the presence of the IPI. While  $\text{HO}_2$  loss was not tested, the relative sensitivity is assumed to be closer to unity since it is less reactive than OH. In either case, the correction is smaller than the total instrumental uncertainty ( $\sim 26\%$  at  $2\sigma$ ), and as such no corrections were applied to OH or  $\text{HO}_2$  calibration factors for the final workup of ambient data collected during IPI sampling periods. In other words, we assume negligible transmission losses within the IPI and the OH calibration factor we applied to ambient data was the same for (1) OHwave without IPI sampling, (2) OHwave during IPI sampling, and (3) OHchem during IPI sampling. However, it should be noted that in the field, calibrations are normally carried out without the IPI system present.

The lack of OH loss in the IPI system is further supported by another test conducted in the field during the summer 2017 AIRPRO campaign, where on one day of the campaign, sequential measurements of OHwave were taken with and without the IPI assembly present. While this was not a formal intercomparison, the summer 2017 campaign provided ideal conditions to assess IPI losses, considering the very high radical concentrations observed (OH frequently  $>1 \times 10^7$  molecule  $\text{cm}^{-3}$ ) in Beijing and thus a good signal-to-noise ratio. The results of this experiment are shown for OH in Figure 4. It can be seen that if no correction for a reduction in sensitivity ~~reduction~~ is applied, adjacent IPIoff and IPIon periods of data are qualitatively in agreement, with no discontinuities in the temporal profile, implying that IPI sensitivity loss is close to zero under field operating conditions. Similar results were obtained for  $\text{HO}_2$  (data not shown).

### 3.1.2 External OH removal

The external OH removal efficiency in the IPI system is controlled by the injection height, the choice of scavenger (i.e., the rate coefficient of the reaction of scavenger with OH), the scavenger and  $\text{N}_2$  dilution gas flows delivered to the injectors, as well as the sheath flow. A key requirement here is efficient mixing of the scavenger into the ambient air stream, which is difficult considering the fast flow rate and hence short residence time of air in the IPI flow tube. Additionally, it is important to consider that some reaction of the scavenger may occur inside the fluorescence chamber (internal OH removal, section 3.1.3). This would give

rise to a positive bias in ambient OH concentration measurements made using the OHchem method, as internal OH removal could result in loss of interfering OH and therefore an apparent reduction in the true background signal.

770

External OH removal experiments were performed by supplying known concentrations of OH and HO<sub>2</sub> to the instrument using the calibration wand described in section 2.1. However, in contrast to normal calibration procedures, where the wand is held at 45° to the pinhole (to overfill the pinhole and minimise sampling of pockets of air which may have been in contact with the metal pinhole surface), IPI characterisation experiments were performed with the wand positioned parallel to the direction of flow within the IPI (i.e., 90° relative to the plane of the pinhole), with a distance of ~3 cm between the wand exit and the PFA flow tube. The high flow through the calibration wand (40 slm) ensured that an excess of calibration gas was delivered to the IPI system (sample flow ~ 32 slm).

775

The external OH removal efficiency ( $RE_{\text{external}}^{\text{OH}}$ ) may be calculated from the proportion of OH remaining ( $R_{\text{external}}^{\text{OH}}$ ) after injection of the scavenger, obtained from the ratio of the OH signals in the presence ( $S_{\text{scavenger}}^{\text{OH}}$ ) and absence ( $S^{\text{OH}}$ ) of the scavenger:

780

$$R_{\text{external}}^{\text{OH}} (\%) = 100 \times S_{\text{scavenger}}^{\text{OH}} / S^{\text{OH}} \quad (3)$$

$$RE_{\text{external}}^{\text{OH}} (\%) = 100 - R_{\text{external}}^{\text{OH}} \quad (4)$$

785

Initial tests included variation of the N<sub>2</sub> dilution flow, however the OH removal efficiency was generally low (data not shown), likely due to poor mixing of the scavenger into the sampled air when the flow rate from the injector is small. As a result, the N<sub>2</sub> dilution was set to the maximum flow of the MFC used (0.5 slm) for all subsequent experiments. Any further dilution of the ambient air stream would result in a loss of sensitivity towards the detection of radicals, however, at 0.5 slm the dilution flow is virtually negligible compared to the total flow rate in the IPI system (32 slm). In other preliminary experiments, the scavenger was injected closer to the FAGE inlet (1.0 and 2.5 cm), but this also resulted in poor external OH removal owing to the shorter residence time between scavenger injection and FAGE sampling.

790

The scavenging efficiency was determined for both propane and C<sub>3</sub>F<sub>6</sub>, with good agreement between the two scavengers. Figure 5 shows the remaining OH signal as a function of the OH reactivity ( $k'_{\text{OH}} = k_{\text{OH+scavenger}}$  [scavenger]) calculated in the flow tube, which normalises the scavenger concentrations according to their different reaction rates with OH. The observed removal efficiency is in broad agreement with the theoretical scavenging efficiency, based on the residence time in the flow tube (~20 ms, assuming plug flow) and assuming perfect mixing, suggesting that in the Leeds IPI system the scavenger is well mixed into the gas sampled by the FAGE cell. An optimum removal of virtually 100% (OH remaining  $\pm 2\sigma = (0.030 \pm 0.091\%)$ ) was observed at  $k'_{\text{OH}} \sim 3000 \text{ s}^{-1}$ , equivalent to ~110 ppmv ( $2.7 \times 10^{15} \text{ molecule cm}^{-3}$ ) propane. This scavenger concentration was used for measurements of OHchem during the summer 2015 ICOZA project and winter 2016 AIRPRO project. For the summer 2017 AIRPRO project, a ten-fold higher scavenger

800

concentration was used (~1100 ppmv propane), after internal removal experiments revealed no loss of  
805 internal OH at this higher concentration, as discussed in detail in the next section.

### 3.1.3 Internal OH removal

Internal removal of OH was quantified by Mao et al. (2012) after forming OH inside the PSU ground-FAGE  
cell using a Hg lamp, and comparing the OH signal with and without the presence of the scavenger (C<sub>3</sub>F<sub>6</sub>),  
added externally in the IPI system. It was found that most of the internal removal occurred in the instrument  
810 inlet, rather than in the OH detection axis, with a total loss of ~20%. Internal removal was not tested in the  
laboratory by Novelli et al. (2014a) for the Max Planck Institute for Chemistry (MPIC) FAGE instrument,  
but instead they limited the scavenger (propene and propane) concentration such that the external OH removal  
efficiency was < 95%, to minimise possible reaction of the scavenger with OH inside the fluorescence cell.  
However, during ambient, nighttime tests (constant atmospheric OH concentration assumed), no change in  
815 the OH background signal was observed after increasing the scavenger concentration by a factor of seven,  
providing evidence for a lack of internal removal (Novelli et al., 2014a).

In the present study, a novel approach was devised to quantify internal removal of OH in the Leeds IPI–  
FAGE instrument. First, under otherwise identical experimental conditions to those for external OH removal  
tests, sufficient CO (75 sccm, 95 ppmv) was added to the calibration wand to verify that the OH formed  
820 (alongside HO<sub>2</sub>) from the photolysis of water vapour was almost quantitatively converted to HO<sub>2</sub> ((98.0 ±  
0.4%-%, data not shown). Secondly, in addition to the calibration wand CO flow, a high flow of NO (50  
sccm) was injected through 1/8" stainless steel tubing inside the FAGE cell, with the injector tip positioned  
centrally just below the turret pinhole, to reconvert the HO<sub>2</sub> back to OH for LIF detection; these experimental  
conditions ensured a fairly high HO<sub>2</sub>-to-OH conversion efficiency of approximately 30%. In this manner,  
825 OH was only generated inside the FAGE cell, and not in the IPI flow tube, such that any change in the  
fluorescence signal could be attributed to internal reaction of OH with propane, rather than reaction in the  
flow tube. The procedure for determination of internal OH removal bears some resemblance to that used for  
ambient detection of RO<sub>2</sub> using the RO<sub>x</sub>LIF technique (Fuchs et al., 2008; Whalley et al., 2013), i.e., the  
external conversion of all radical species to HO<sub>2</sub> before internal conversion to OH within the fluorescence  
830 cell.

The internal OH removal efficiency ( $RE_{\text{internal}}^{\text{OH}}$ ) was quantified in an analogous manor to the external  
scavenging efficiency, using the total fluorescence signal in the presence ( $S^{\text{HOx}}_{\text{scavenger}}$ ) and absence ( $S^{\text{HOx}}$ ) of  
the scavenger:

$$835 \quad R_{\text{internal}}^{\text{OH}} (\%) = 100 \times S^{\text{HOx}}_{\text{scavenger}} / S^{\text{HOx}} \quad (5)$$

$$RE_{\text{internal}}^{\text{OH}} (\%) = 100 - R_{\text{internal}}^{\text{OH}} \quad (6)$$

Figure 6 shows a time series of the LIF signal during two example internal removal experiments. Here, the  
LIF signal represents the sum of signals from OH and HO<sub>2</sub>, since they are produced in a 1:1 ratio (Fuchs et

840 al., 2011) in the calibration wand. For both of the propane mixing ratios used, which were shown to result in  
near complete external OH removal in section 3.1.2, there was no obvious decrease in the LIF signal,  
indicating no significant internal removal of OH. The average  $\pm 2\sigma$  internal OH removal observed for repeat  
experiments was  $\underline{-(0.5 \pm 1.3\% \pm 4.0)\%}$  (Table 2) at a propane mixing ratio of  $\sim 110$  ppmv (ICOZA and  
845 AIRPRO winter conditions). For repeat experiments at the higher propane mixing ratio used during the  
AIRPRO summer field campaign ( $\sim 1100$  ppmv), the internal removal was still very small, and almost  
insignificant  $\underline{((2.8 \pm 2.3\% \pm 9 \pm 6.6)\%}$ , Table 2). The observed internal OH removal may be compared to that  
which might be expected theoretically. In the ambient pressure flow tube, a propane mixing ratio of 1100  
ppmv equates to  $k'_{\text{OH}} = 30,000 \text{ s}^{-1}$ , but this is a factor of 760/1.5 lower in the detection cell (i.e., the ratio of  
850 ambient to cell pressure),  $59 \text{ s}^{-1}$  (assuming constant gas density and no change in the OH + propane rate  
coefficient). Under normal operation, NO injection occurs 10.5 cm below the pinhole, and 7.5 cm away from  
the laser axis (i.e., total of 18 cm between the pinhole and detection volume), with a residence time of 0.9 ms  
between NO injection and OH detection (Creasey et al., 1997b; Whalley et al., 2013). The gas likely slows  
down between pinhole sampling and NO injection, but assuming a constant gas velocity, the residence time  
855 between the pinhole and the laser axis is estimated at  $\sim 2$  ms. Based on this, an internal OH removal ~~of~~  
efficiency of  $\sim 12\%$  is calculated, which is higher than observed, likely because the assumption of constant  
gas velocity is invalid (i.e., the real residence time is closer to  $\sim 1$  ms) and mixing between HO<sub>2</sub> and NO from  
the injector is not instantaneous. However, it should be noted that this calculation also neglects the fact that  
the density is higher in the jet, or the perturbation to normal flow caused by moving the NO injector close to  
the pinhole.

860 In the internal removal experiment, OH is not formed instantly at the pinhole but is built up linearly by  
HO<sub>2</sub>/NO conversion along the line from the pinhole to the laser axis. Therefore, the experimental internal  
removal may not be directly compared with the theoretical estimate. In such a sequential reaction system, the  
OH scavenging is about half as efficient as that for the case where OH is formed as an instant point source at  
the pinhole. Thus, the experimental value should be doubled to  $(5.8 \pm 13)\%$ , which is in reasonable agreement  
865 with the theoretical value. From this, we cannot rule out a small internal OH removal on the order of 10% at  
the higher propane level used for the AIRPRO summer campaign. However, no such corrections were applied  
to the ambient data featured in this work.

### 3.2 Interference testing experiments

#### 3.2.1 O<sub>3</sub> + H<sub>2</sub>O vapour

870 In LIF-FAGE instruments, there is a known interference due to laser-generated OH from ozone photolysis  
in the presence of water vapour (Fuchs et al., 2016; Griffith et al., 2016; Tan et al., 2017). This interference  
was quantified by (Whalley et al., 2018) and characterised in further detail in the present work. In these  
experiments, ozone was generated from the 184.9 nm photolysis of oxygen in a 12–20 slm flow of zero air  
using a Hg(Ar) pen-ray lamp (LOT LSP035). Another 12–20 slm of zero air was humidified using a water  
875 (HPLC grade) bubbler. The two zero air flows were combined and delivered to the calibration wand, from

which the IPI sampled in a manner analogous to the experiments conducted to investigate external and internal OH removal discussed above. Ozone mixing ratios in the range 0–2.5 ppmv were generated by varying the Hg lamp current (0–21 mA), while water vapour levels volume mixing ratios in the range 0.1–1.0% were produced by varying the flow through the bubbler, or by bypassing it completely, and the total flow (32 slm) was compensated by changing the dry zero air flow. Laser power (LP) at 308 nm was varied in the range 3–17 mW by varying the ratio of acetone:water in a cuvette placed before the fibre launcher that is used to send laser light to the detection cells.

Figure 7 shows the results of O<sub>3</sub> + H<sub>2</sub>O vapour interference tests. It can be seen that the interference signal (OH<sub>int</sub> = OH<sub>wave</sub> – OH<sub>chem</sub>) is linear in both ozone (panel (a)) and water vapour (panel (b)) mixing ratios. The quadratic dependence of the interference signal on laser power (panel (c)) in terms of raw count rates indicates that the interference originates from a two-photon process, as expected. However, since OH data are normalised to laser power, the equivalent OH concentrations are linear with respect to laser power. Thus overall, OH<sub>int</sub> is linear in ozone, water vapour, and laser power. Normalisation of the slope in panel (a) yields the relation:

$$[\text{OH}_{\text{int}}] = (520 \pm 140565 \pm 42) \text{ molecule cm}^{-3} \text{ ppbv}^{-1} \%^{-1} \text{ mW}^{-1} \times [\text{O}_3] \times [\text{H}_2\text{O}] \times \text{LP} \quad (7)$$

where [O<sub>3</sub>], [H<sub>2</sub>O], and LP are in units of ppbv, %, and mW, respectively. Under typical atmospheric conditions of [O<sub>3</sub>] = 50 ppbv and [H<sub>2</sub>O] = 1%, and a typical instrument laser power of 15 mW, the interference signal is equivalent to an OH concentration of 3.9 × 10<sup>5</sup> molecule cm<sup>-3</sup>. This signal is slightly smaller than the instrumental limit of detection (LOD) of ~7 × 10<sup>5</sup> molecule cm<sup>-3</sup> at a signal-to-noise ratio (SNR) of 2, but nonetheless it was used to correct the ambient OH<sub>wave</sub> data presented in section 3.3, using co-located measurements of ozone and water vapour.

### 3.2.2 Isoprene ozonolysis

To test for interferences from isoprene (ISO) ozonolysis products, isoprene (~16 ppmv) and ozone (~1.8 ppmv) were mixed in the calibration wand and the scavenger (propane, PROP) was injected into the IPI flow tube. The propane concentrations were set to those used for ambient OH<sub>chem</sub> measurements, such that the tests were representative of normal atmospheric sampling (i.e., to test whether an interference signal would remain in ambient data). However, to generate sufficient OH signal for quantitative analysis, ozone and isoprene were introduced at concentrations that far exceeded their typical ambient levels (Table 3). Unlike previous tests of interferences from alkene ozonolysis (Novelli et al., 2014b), low [O<sub>3</sub>]:[ISO] ratios were used to suppress the signal contribution from the atmospheric (real) OH generated by ozonolysis (i.e., isoprene acted as an additional OH scavenger). To allow sufficient time for steady-state conditions to develop, the IPI did not sample from the calibration wand directly, but instead a 30 cm flow tube (polycarbonate, ID ~ 19 mm) was used to extend the IPI (which sampled wand gas at the normal IPI flow rate of ~32 slm, residence time for O<sub>3</sub> + isoprene reaction ~ 0.15 s).

Time series of the interference testing experiments conducted using the IPI are shown in Figure 8. In panel (a), no isoprene is added, but due to ozone photolysis in the presence of high [H<sub>2</sub>O] (0.73%) an interference signal (OH<sub>int</sub>) is observed (i.e., signal in the presence of propane is higher than the offline signal). The magnitude of this signal (OH<sub>int</sub> ~ 1.0 × 10<sup>7</sup> molecule cm<sup>-3</sup>) yields a scale factor of 510 ± 270 molecule cm<sup>-3</sup> ppbv<sup>-1</sup> %<sup>-1</sup> mW<sup>-1</sup> when linearly extrapolated down from the measured [O<sub>3</sub>], [H<sub>2</sub>O], and LP, in agreement with the 520 ± 140 565 ± 42 molecule cm<sup>-3</sup> ppbv<sup>-1</sup> %<sup>-1</sup> mW<sup>-1</sup> in equation (E7).

In panel (b), ozone and isoprene react under dry conditions, and an interference signal is observed again. The low H<sub>2</sub>O (0.07%) suppressed the O<sub>3</sub> + H<sub>2</sub>O interference, such that this cannot explain the magnitude of OH<sub>int</sub> (~1.9 × 10<sup>7</sup> molecule cm<sup>-3</sup>, Table 3), suggesting that OH was formed internally from a reaction other than O<sup>1</sup>D + H<sub>2</sub>O. Under high-humidity (H<sub>2</sub>O ~ 1%) conditions (panel (c)), OH<sub>int</sub> (~1.6 × 10<sup>7</sup> molecule cm<sup>-3</sup>) was similar, but in this case the signal can be explained almost entirely by the O<sub>3</sub> + H<sub>2</sub>O interference. Under dry conditions but with a ten-fold higher concentration of propane (as used for the AIRPRO summer campaign, panel (c)), the interference signal from panel (b) was reduced but remained elevated relative to the offline signal (OH<sub>int</sub> ~ 1.4 × 10<sup>7</sup> molecule cm<sup>-3</sup>), where again the contribution from O<sub>3</sub> + H<sub>2</sub>O cannot explain the discrepancy. The decrease in OH<sub>int</sub> between panels (b) and (d) may be attributed to the suppression of steady-state OH generated from ozonolysis, but the remaining signal implies that OH was also formed internally in both cases. For the dry, low-propane experiment (panel (b)), the magnitude of the OH signal is much higher than that calculated from a steady-state model (~1.4 × 10<sup>6</sup> molecule cm<sup>-3</sup>).

The suppression of the interference signal attributable to O<sub>3</sub>/isoprene only (i.e., O<sub>3</sub> + H<sub>2</sub>O corrected) by the addition of water vapour (panel (c), H<sub>2</sub>O ~ 1%) suggests that the internal OH may have been formed from SCIs. The simplest C1 and C2 SCIs are known to react quickly with the water vapour dimer ( $k \sim 4\text{--}7 \times 10^{-12}$  cm<sup>3</sup> molecule<sup>-1</sup> s<sup>-1</sup> at 298 K for CH<sub>2</sub>OO (Chao et al., 2015; Lewis et al., 2015)) and monomer ( $k \sim 1\text{--}2 \times 10^{-14}$  cm<sup>3</sup> molecule<sup>-1</sup> s<sup>-1</sup> for *anti*-CH<sub>3</sub>CHOO (Taatjes et al., 2013; Sheps et al., 2014; Lin et al., 2016)), respectively. Reaction with the water vapour monomer was also shown to be relatively fast ( $k \sim 1.2 \times 10^{-15}$  cm<sup>3</sup> molecule<sup>-1</sup> s<sup>-1</sup>,  $k_{\text{loss}} \sim 300$  s<sup>-1</sup> at ~1% H<sub>2</sub>O) for the ensemble of SCIs, including the C1 SCI, generated from isoprene ozonolysis (Newland et al., 2015).


However, regardless of whether the signal observed at high propane is due to internally formed OH, which may have originated from SCIs, the equivalent OH concentrations are negligible when extrapolated back to ambient chemical conditions (Table 3). Assuming a linear dependence of the interference signal on both ozone and isoprene, the interference (after O<sub>3</sub> + H<sub>2</sub>O correction) is equivalent to <10<sup>2</sup> molecule cm<sup>-3</sup> at the ozone (10 ppbv) and isoprene (3.5 ppbv) levels measured in a low-NO<sub>x</sub>, biogenic environment during the Oxidants and Particle photochemical processes (OP3) campaign in Borneo, 2008 (Hewitt et al., 2010). Similarly, the interference is calculated to be higher for the ozone (90 ppbv) and isoprene (7.9 ppbv) levels during the summer AIRPRO campaign, but it is still <10<sup>3</sup> molecule cm<sup>-3</sup>. Similarly, we have modelled the SCI decomposition in our FAGE cell. Assuming an ambient atmosphere containing 100 ppbv O<sub>3</sub> and 10 ppbv alkene and taking the reactions and rate coefficients from Novelli et al. (2014a), we calculate an equivalent ambient pressure OH concentration of ~4 × 10<sup>3</sup> molecule cm<sup>-3</sup> from the decomposition of SCIs at our FAGE

cell residence time of 2 ms. The insignificance of the interference signal for atmospherically relevant O<sub>3</sub>/alkene concentrations is consistent with the results of previous interference experiments, for which equivalent OH concentrations of  $\sim 3\text{--}4 \times 10^4$  (Novelli et al., 2014b; Fuchs et al., 2016) and  $\sim 4 \times 10^5$  molecule cm<sup>-3</sup> (Rickly and Stevens, 2018) can be derived.

### 3.2.3 NO<sub>3</sub> radicals

Fuchs et al. (2016) found that, despite the absence of a hydrogen atom, NO<sub>3</sub> radicals were responsible for a small OH interference signal in the Forschungszentrum Jülich (FZJ) LIF-FAGE instrument, equivalent to an OH concentration of  $1.1 \times 10^5$  molecule cm<sup>-3</sup> per 10 pptv NO<sub>3</sub>. The OH interference scaled linearly with observed NO<sub>3</sub> mixing ratios but showed no dependence on inlet length, cell pressure, laser power, or humidity, and the background signal did not change significantly in the presence of CO scavenger, suggesting the OH was indeed being formed internally. It was postulated that the interference was a result of a heterogeneous process involving NO<sub>3</sub> and H<sub>2</sub>O adsorbed on instrument walls. Interference signals were also observed in the detection of HO<sub>2</sub> and RO<sub>2</sub> radicals, equivalent to  $1.0 \times 10^7$  and  $1.7 \times 10^7$  molecule cm<sup>-3</sup>, respectively, per 10 pptv NO<sub>3</sub>.

To test for an NO<sub>3</sub> interference in OH measurements made by the Leeds FAGE instrument, NO<sub>3</sub> was generated from the reaction of ozone and NO<sub>2</sub>:



In these experiments, ozone was generated by flowing zero air (15 slm) past a Hg lamp (LOT LSP035). A constant 0.5 slm flow of NO<sub>2</sub> (BOC, 2 ppmv) was diluted in 25 slm zero air and mixed with the zero air/ozone flow as well as an additional zero air dilution flow of 10 slm, to yield a final mixing ratio of 20 ppbv. Gas was delivered to the IPI system using the calibration wand, with a total residence time of 3.7 s for the O<sub>3</sub> + NO<sub>2</sub> reaction. Ozone mixing ratios in the range 0–2.8 ppmv (after dilution) were generated by varying the current supplied to the Hg lamp. NO<sub>3</sub> radical mixing ratios in the range 0–90 pptv were calculated based on a box model with rate constants taken from the Master Chemical Mechanism (MCM; <http://mcm.leeds.ac.uk/MCM>) version 3.3.1 ( $k_{\text{R1}} = 3.52 \times 10^{-17}$  cm<sup>3</sup> molecule<sup>-1</sup> s<sup>-1</sup>,  $k_{\text{R2}} = 1.24 \times 10^{-12}$  cm<sup>3</sup> molecule<sup>-1</sup> s<sup>-1</sup>, and  $k_{\text{R3}} = 0.045$  s<sup>-1</sup>). These experiments were performed under dry conditions (H<sub>2</sub>O ~ 0.07%), such that only a small correction was applied for the O<sub>3</sub>/H<sub>2</sub>O interference.

The results of the NO<sub>3</sub> radical interference tests are shown in Figure 9. It can be seen that the equivalent OH signals were all  $< 8 \times 10^5$  molecule cm<sup>-3</sup>, and almost always below the instrument LOD of  $6.3 \times 10^5$  molecule cm<sup>-3</sup> (SNR = 2). Unlike the dependence found by Fuchs et al. (2016), the interference signal does not increase linearly with NO<sub>3</sub>. However, based on the point at the highest NO<sub>3</sub> mixing ratio of ~90 pptv, the interference is equivalent to an insignificant  $\sim 6 \times 10^4$  molecule cm<sup>-3</sup> at 10 pptv NO<sub>3</sub>, or approximately half

985 of that observed by Fuchs et al. (2016). These experiments suggest that an interference from NO<sub>3</sub> radicals is not significant for the detection of OH using the Leeds ground-based FAGE instrument.

### 3.3 Ambient observations of OH<sub>wave</sub> and OH<sub>chem</sub>

#### 3.3.1 ICOZA 2015

990 Figure 10 shows the overall intercomparison of OH<sub>wave</sub> (with O<sub>3</sub> + H<sub>2</sub>O interference as given in Equation 7 subtracted) and OH<sub>chem</sub> measurements made during the ICOZA 2015 campaign. It is evident that the raw data (averaged for 4 minute periods) are quite noisy, but averaging to 1 h improves the precision and reveals a tight correlation, with the majority of points scattered around the line of 1:1 agreement. An orthogonal distance regression (ODR) fit (Boggs et al., 1987), which accounts for errors in both the y- and x- directions, to the hourly data yields a slope of  $1.160 \pm 0.058$  ( $2\sigma$ ) and a negative intercept on the order of the instrumental precision. In a similar manner, an unweighted least squares linear fit (not shown) gives a slope of  $1.060 \pm 0.065$ , an intercept of  $(0.5 \pm 1.5) \times 10^5$  molecule cm<sup>-3</sup>, and a correlation coefficient ( $R^2$ ) of 0.992. Regardless of the fit method, these results show that on average, the two OH measurements agree within the instrumental uncertainty of ~26% at  $2\sigma$ .

1000 Median hourly diurnal profiles of OH<sub>wave</sub>, OH<sub>chem</sub>, and  $J(\text{O}^1\text{D})$ , averaged over both IPI sampling periods, are shown in Figure 11. The two OH measurements exhibit virtually identical profiles, with peak values of  $\sim 3 \times 10^6$  molecule cm<sup>-3</sup> slightly before solar noon, and relatively high concentrations ( $\sim 1\text{--}2 \times 10^6$  molecule cm<sup>-3</sup>) persisting into the early evening despite the concomitant falloff in  $J(\text{O}^1\text{D})$ . Nighttime levels were generally below  $5 \times 10^5$  molecule cm<sup>-3</sup>. The variability in OH concentrations, shown only for OH<sub>chem</sub> for clarity, was high during both day and nighttime periods.

1005 In Figure 10 it can be seen that some points lie substantially above the 1:1 line, especially for the 4 minute averaged raw data. It is possible that, despite the good overall agreement between the median diurnal profiles of OH<sub>wave</sub> and OH<sub>chem</sub> in Figure 11, OH<sub>hint</sub> may have exhibited its own distinct diurnal profile, independent of atmospheric OH concentrations, for example if the interference signal was generated from a particular chemical species. However, the median diurnal profile of individual OH<sub>hint</sub> measurements (= OH<sub>wave</sub> – OH<sub>chem</sub>) in Figure 11 exhibits no obvious structure, with values scattered around zero and a mean  $\pm 2\sigma$  value of  $(0.3 \pm 3.3) \times 10^5$  molecule cm<sup>-3</sup>, which is well below the LOD for individual OH measurements. Similarly, the average (OH<sub>wave</sub> – OH<sub>chem</sub>)/OH<sub>wave</sub> ratio (i.e., the contribution of interferences to the total OH<sub>wave</sub> signal) was zero within error (mean  $\pm 2$  standard errors (SE) =  $0.03 \pm 0.12$ ).

1015 Furthermore, ~~OH<sub>wave</sub> and OH<sub>chem</sub>~~ OH<sub>hint</sub> does not exhibit ~~virtually identical behaviour~~ any dependence when binned against various parameters (Woodward Massey, 2018 Fig. S1), including those previously implicated in LIF-FAGE measurement interferences, such as  $J(\text{O}^1\text{D})$  (Feiner et al., 2016), temperature (Mao et al., 2012; Novelli et al., 2017), OH reactivity  $k_{\text{OH}}$  (Mao et al., 2012), ~~OH reactivity due to VOCs~~, and O<sub>3</sub> (Feiner et al., 2016; Novelli et al., 2017), ~~isoprene~~ (Feiner et al., 2016), and NO (Feiner et al., 2016) mixing ratios.

### 1020 3.3.2 AIRPRO winter 2016

The overall agreement between the two measurements is presented in the correlation plot in Figure 12. As with ICOZA (Figure 10), a tight correlation is revealed after averaging the data to one hour, and all points are distributed evenly around the line of 1:1 agreement. ODR fitting yields an overall slope of  $1.051 \pm 0.039$  and a negative intercept of a similar magnitude to the instrumental precision. An unweighted least squares linear fit (not shown) gives a slope of  $0.997 \pm 0.038$ , an intercept of  $(5.1 \pm 7.3) \times 10^4$  molecule  $\text{cm}^{-3}$ , and an  $R^2$  of 0.97.

The two measurements exhibit the same profile on a diurnal basis (Figure 13), with a diel maximum of  $\sim 3 \times 10^6$  molecule  $\text{cm}^{-3}$  occurring in the late morning due to the build-up of HONO overnight. At night, OHchem concentrations were close to the LOD ( $< \sim 2 \times 10^5$  molecule  $\text{cm}^{-3}$ ), while OHwave measurements were frequently negative, possibly as a result of over-subtraction of the  $\text{O}_3/\text{H}_2\text{O}$  interference as this is subject to high uncertainty (Figure 7). The diurnal profile of OHint is scattered around zero with a mean  $\pm 2\sigma$  difference of  $(-0.9 \pm 2.7) \times 10^5$  molecule  $\text{cm}^{-3}$ , and the mean  $\pm 2$  SE contribution of interferences to the total signal was  $-0.02 \pm 0.07$ .

### 3.3.3 AIRPRO summer 2017

1035 The intercomparison of OHwave and OHchem measurements for the AIRPRO summer campaign is shown in Figure 14. Consistent with ICOZA and the AIRPRO winter results, the 1 h data are scattered around the 1:1 line, with an overall ODR slope of  $1.103 \pm 0.017$ . However, the intercept is more negative than for the other campaigns, which suggests that the  $\text{O}_3/\text{H}_2\text{O}$  interference may have been overestimated, [asbecause](#) it is during this campaign that the highest ozone mixing ratios ( $\sim 90$  ppbv diurnally-averaged maximum, Table 1) were encountered. Similarly, an unweighted least squares linear fit to the data (not shown) yields a slope of  $1.111 \pm 0.029$ , an intercept of  $(-3.8 \pm 1.7) \times 10^5$  molecule  $\text{cm}^{-3}$ , and an  $R^2$  of 0.92 (data not shown).

1045 Again, the two measurements follow the same diurnal profile (Figure 15), peaking in the afternoon at  $\sim 1 \times 10^7$  molecule  $\text{cm}^{-3}$  with relatively high nighttime levels of  $\sim 1-2 \times 10^6$  molecule  $\text{cm}^{-3}$ . As with ICOZA and the AIRPRO winter campaign, the OHint diurnal profile does not exhibit any obvious structure, with values scattered around zero and a mean  $\pm 2\sigma$  difference of  $(-1.6 \pm 4.1) \times 10^5$  molecule  $\text{cm}^{-3}$ . The mean  $\pm 2$  SE (OHwave - OHchem)/OHwave ratio was  $-0.09 \pm 0.10$ . During AIRPRO, measured  $\text{NO}_3$  mixing ratios reached up to  $\sim 100$  pptv, such that the lack of significant nighttime OH interference signals is consistent with the results of  $\text{NO}_3$  interference tests (section 3.2.3).

1050 It can be seen from Figure 14 that there is a small cluster of points that lie significantly away from both the 1:1 and ODR regression lines, which are characterised by high OHwave concentrations of  $> 1.5 \times 10^7$  molecule  $\text{cm}^{-3}$ . This finding was investigated further, with the results summarised in Figure 16. Above an OHchem threshold of  $\sim 1.0-1.5 \times 10^7$  molecule  $\text{cm}^{-3}$ , the OHint signal becomes significantly greater than zero and the instrument LOD, reaching  $\sim 3-5 \times 10^6$  molecule  $\text{cm}^{-3}$  at OHchem levels of around  $\sim 2 \times 10^7$  molecule  $\text{cm}^{-3}$ . However, these results should be treated with caution, since only a few points are available for which OHchem was present at such high concentrations. The same behaviour was not observed for either

the AIRPRO winter or ICOZA campaigns, since OHchem levels did not surpass  $1 \times 10^7$  molecule  $\text{cm}^{-3}$ , but the analogous mean values at low OHchem concentrations are in agreement with the AIRPRO summer results.

The above results suggest that in the Beijing summertime, the Leeds FAGE instrument is subject to an interference(s) at the highest OH levels, although its contribution of ~15–20% (Figure 16) is still below the instrumental accuracy of 26% at  $2\sigma$ . This finding is consistent with the suggestion of (Fittschen et al., (2019) that ROOOH species, formed from  $\text{RO}_2 + \text{OH}$  reactions, generate an OH interference in LIF-FAGE instruments, since high OH levels would generate high  $\text{RO}_2$  concentrations and favour this class of reaction. It is also possible that, for high ambient OH production rates, the scavenger cannot react with the sampled OH sufficiently quickly, leading to elevated but spurious OHchem background signals. Although a modelling study of the inlet chemistry would be required to fully assess this hypothesis, it is likely not the case considering that the propane concentration used during AIRPRO results in an OH lifetime of ~0.03 ms in the IPI flow tube, in comparison to a residence time of ~20 ms (i.e., ~700 OH lifetimes).

No clear dependences were found when OHint was binned against various parameters previously implicated in OH measurement interferences (Fig. S2), although it can be seen that OHint was marginally higher in the highest temperature,  $J(\text{O}^1\text{D})$ , and isoprene bins.

#### 4 Discussion

The results from the three field campaigns that feature in this work demonstrate that, in moderately to highly polluted conditions, the Leeds ground-based FAGE instrument does not suffer from substantial interferences in the measurement of OH using the conventional, wavelength-modulation background technique, OHwave. This is illustrated best by the slopes of the overall measurement intercomparison plots (Figures 10, 12, and 14), which ranged from 1.05–1.16. However, while the deviations of these slopes from 1 are small, they are still significant, suggesting the presence of unknown OH interferences. Nonetheless, such unknown interferences are well within the instrumental uncertainty of ~26% at  $2\sigma$ .

With respect to previous studies during which OH has been measured by a LIF instrument equipped with a scavenger injector, the significance of interferences during the campaigns that feature in this work are amongst the lowest observed (Table 4). This can likely be attributed to two main factors: environment and instrumental. In terms of the former, none of the studies described in the present study took place in forested environments, where the most significant interferences have been observed (Mao et al., 2012; Novelli et al., 2014a; Feiner et al., 2016). However, as mentioned previously, the AIRPRO summer campaign did share some characteristics, in that high BVOC and low NO mixing ratios were observed in the afternoon. Despite this, OHwave and OHchem were in good agreement. These findings ~~Although AIRPRO summer took place in a city, its results do~~ provide confidence in previous measurements of OH using the same instrument, ~~particularly those in a forested region (Whalley et al., 2011),~~ and support the hypothesis that there are unknown OH sources in this type of environmentthe atmosphere.

The insignificance of daytime interferences during the AIRPRO campaigns are consistent with results of another urban study, CalNex-LA (Research in California at the Nexus of Air Quality and Climate Change) (Griffith et al., 2016). The  $\text{O}_3/\text{H}_2\text{O}$  interference is much higher (up to  $\sim 4 \times 10^6$  molecule  $\text{cm}^{-3}$  OH equivalent during CalNex-LA) in the Indiana University (IU) LIF instrument (Dusanter et al., 2009), such that the  
1095 daytime contributions of  $\sim 33\%$  can be explained entirely by this known interference. However, measurements made at a nearby site during the same study (CalNex-SJV) showed daytime contributions of  $\sim 20\%$  (Brune et al., 2016), although this may be related to instrumental differences as discussed below. On average, interferences were not observed in the daytime during ICOZA, but they were observed in other coastal campaigns, namely DOMINO (Diel Oxidants Mechanisms In relation to Nitrogen Oxide)  $\text{HO}_x$   
1100 ( $\sim 50\%$ ) (Novelli et al., 2014a) and CYPHEX (CYprus PHotochemistry EXperiment,  $\sim 45\%$ ) (Mallik et al., 2018), as well as in rural regions, HOPE (Hohenpeißenberg Photochemistry Experiment, 20–40%) (Novelli et al., 2014a). Studies in the North China Plain have revealed small interferences on the order of 0–10% (Tan et al., 2017; Tan et al., 2018), with slightly higher but variable contributions of 0–20% in the Pearl River Delta (Tan et al., 2019).

1105 The second major reason for the differences in contributions between the studies listed in Table 4 is likely instrumental effects. For the campaigns in which the highest OH interferences have been observed (Mao et al., 2012; Novelli et al., 2014b; Feiner et al., 2016), OH measurements were made using the Max Planck Institute (MPI) (Martinez et al., 2010) and PSU (Faloona et al., 2004) LIF instruments. These instruments feature laser-multi-pass detection cells, which give rise to larger detection volumes and increased UV fluence,  
1110 although this may not be relevant considering that the interference signals did not display any laser power dependence for these instruments. The Leeds instrument also differs in terms of cell geometry, where the  $\text{HO}_x$  cell is composed of a short (5 cm) turreted inlet on top of a large fluorescence cell (additional  $\sim 8$  cm to laser axis,  $\sim 13$  cm total length, and a cell diameter of 25 cm). In contrast, the MPI and PSU instruments feature flow tube-like inlets (14–17 cm from the pinhole to laser axis) mounted on smaller fluorescence cells,  
1115 facilitating the interaction of sampled gas with the cell walls, which may promote the generation of internal OH. For the measurements listed in Table 4, the Peking University (PKU) instrument (Tan et al., 2017) is most similar to the Leeds FAGE (i.e., single-pass detection,  $\sim 10$  cm total length from sampling inlet to laser axis), for which similar daytime interferences on the order of  $\sim 0$ –20% were observed.

For the ICOZA campaign, nothing could be inferred about the origin of the OH interference signal when  
1120 one was observed, as it did not exhibit any characteristic diurnal profile (Figure 11), and showed no obvious dependences on a variety of meteorological and chemical parameters. This finding is in contrast to previous studies in which diel profiles (Mao et al., 2012; Feiner et al., 2016) and dependences (Mao et al., 2012; Feiner et al., 2016; Novelli et al., 2017) of the interference have been observed. The occurrence of large (i.e.,  $> 1 \times 10^6$  molecule  $\text{cm}^{-3}$ ) background OH signals ( $\text{OH}_{\text{int}} = \text{OH}_{\text{wave}} - \text{OH}_{\text{chem}}$ ) after instrumental problems (e.g.,  
1125 power cuts, data not shown) implies that the differences may have been instrumental rather than as a result of a species present in ambient air, although the data at these times did pass all quality control filters and therefore could not be rejected. Nonetheless, any differences are still a concern, regardless of their cause; the

IPI system thus serves as an additional check on measurement accuracy and operational stability, and is perhaps most useful for fieldwork sites where power supplies are unreliable, for example in more remote areas.

It is possible that, even though the background OH had a flat diurnal profile in each field campaign, the species responsible for any interference observed were different between day and nighttime periods. Thus, analysis of the day and nighttime data separately, as a function of the same parameters, might reveal more information. Considering the recent identification of NO<sub>3</sub> radicals as an internal OH source in LIF instruments (Fuchs et al., 2016), and that OH concentrations have often been underpredicted at night (Faloona et al., 2001; Mao et al., 2012; Ren et al., 2013; Hens et al., 2014; Lu et al., 2014; Tan et al., 2017), this is perhaps the most interesting period for further study. However, for the data presented in this work, robust quantitative nighttime analyses are not possible due to OH measurements being below or close to the instrument LOD.

In this work, there are several key findings that stand out. First, OHwave and OHchem were in good agreement even at the very low NO concentrations of < 100 pptv during ICOZA, and the moderate afternoon levels (~500 pptv on average but often < 100 pptv (Shi et al., 2018)) during the AIRPRO summer campaign. While the role of isoprene could not be assessed for ICOZA, due to the limited range of concentrations observed (< 0.2 ppbv), it reached high levels during AIRPRO summer (up to 7.9 ppbv, larger than seen in some forested regions) but did not seem to perturb the agreement between the two measurements. In addition, very high levels of aromatic VOCs were observed during both AIRPRO winter and summer, where the agreement between OHwave and OHchem suggests that the intermediates of aromatic oxidation, such as exotic bicyclic species (Birdsall et al., 2010) and highly-oxygenated molecules (HOMs) (Wang et al., 2017; Molteni et al., 2018; Hammes et al., 2019), do not give rise to OH interferences, which is postulated to be the case for intermediates (SCIs) in the ozone-oxidation of alkenes (Novelli et al., 2014b; Novelli et al., 2017; Rickly and Stevens, 2018). However, the large alkene and ozone concentrations observed during AIRPRO summer should favour the formation of these SCIs, but significant interferences were not observed, consistent with laboratory investigations of the isoprene interference and casting doubt on the SCI hypothesis. Although, the AIRPRO SCI concentrations also depend on the magnitude of the SCI loss rates, which could be high if elevated levels of SO<sub>2</sub> (Welz et al., 2012; Sheps et al., 2014) or organic acids (Welz et al., 2014) were present.

Considering the success of the first three field deployments of the IPI system, and given that it does not reduce the instrument sensitivity towards OH, it is suggested that the system is adopted for permanent use in ambient studies, although conventional sampling should still be performed from time-to-time to check for potential artefacts caused by the IPI system itself. Another advantage of the IPI system is that it reduces the amount of solar light entering the pinhole, which reduces the size and variability of daytime background signals and therefore improves signal-to-noise and hence detection limits. It is recommended that the IPI propane concentration is kept the same as the summer AIRPRO campaign, as it is possible that the slightly poorer agreement between OHwave and OHchem during ICOZA was because of the lower propane flow used (i.e., the flow was not sufficient to ensure that OH generated from all steady-state sources was removed), although this cannot be verified.

1165 Future field campaigns using the IPI will allow for the assessment of interferences in the Leeds FAGE  
instrument for a range of different environments. From these, the contribution of interferences for previous  
studies in similar environments, where measurements were made prior to the discovery of significant  
interferences in the LIF measurement of OH reported by others, may be inferred. The measurement-model  
comparisons may then be reassessed in light of any new information regarding the accuracy of OH  
1170 measurements. Regardless of the reasons for any differences between the two measures of OH (i.e., chemical  
interferences or instrumental problems such as during recovery periods after power cuts), the IPI system  
serves as an additional check on OH observations, increasing confidence in the validity of the data obtained.

## 5 Conclusions

The addition of an IPI system to the Leeds ground-based FAGE instrument allowed for a comprehensive  
1175 investigation of OH measurement interferences in both the laboratory and the field. Following its  
optimisation and thorough characterisation in terms of sensitivity and external and internal OH removal  
efficiency, laboratory experiments were conducted to assess potential interferences from (1) the photolysis  
of O<sub>3</sub> in the presence of H<sub>2</sub>O vapour, (2) the intermediates and products of isoprene ozonolysis, and (3) NO<sub>3</sub>  
radicals. For O<sub>3</sub> + H<sub>2</sub>O, a small but potentially significant interference (at high O<sub>3</sub> levels) was found, but  
1180 interferences from isoprene ozonolysis products and NO<sub>3</sub> radicals were shown to be insignificant under  
typical atmospheric conditions.

Field campaigns conducted in the UK and China showed that, on average, the Leeds ground-based FAGE  
instrument does not suffer from significant interferences in the detection of OH. It was only under the very  
high OH levels of  $> 1.5 \times 10^7$  molecule cm<sup>-3</sup> sometimes observed during the AIRPRO summer campaign  
1185 that interferences were found consistently, although their contributions (~15–20%) were smaller than the  
instrumental accuracy of 26% at 2 $\sigma$ . Large interference signals ( $> 1 \times 10^6$  molecule cm<sup>-3</sup>) were occasionally  
observed during the ICOZA campaign, but always after instrumental problems such as power cuts, suggesting  
that the OHchem method serves as an additional tool for verifying instrument stability and validating  
measurements. The Leeds IPI system will find continued use in future fieldwork.

1190

*Data availability.* Data presented in this study are available from the authors upon request  
(d.e.heard@leeds.ac.uk).

*Competing interests.* The authors declare that they have no conflict of interest.

1195

## Acknowledgements

We are grateful to the Natural Environment Research Council for funding (grant numbers NE/K012029/1,  
NE/K012169/1, NE/N007115/1 and NE/N006895/1). RWM, DRC and EJS are grateful to NERC for funding  
PhD studentships. We would like to acknowledge Brian Bandy, Grant Forster, David Oram and Claire Reeves  
1200 (University of East Anglia), William Bloss, Leigh Crilley and Louisa Kramer (University of Birmingham),

and Rachel Dunmore, Jacqui Hamilton, James Hopkins, James Lee, Chris Reed and Freya Squires (University of York) for provision of some of the data used to generate the averages in Table 1. We would also like to thank other participants in the ICOZA and AIRPRO field campaigns. We are grateful for technical support from the University of Leeds mechanical and electronics workshops,

## 1205 **References**

- Birdsall, A. W., Andreoni, J. F., and Elrod, M. J.: Investigation of the role of bicyclic peroxy radicals in the oxidation mechanism of toluene, *Journal of Physical Chemistry A*, 114, 10655-10663, 10.1021/jp105467e, 2010.
- Bloss, W. J., Lee, J. D., Heard, D. E., Salmon, R. A., Bauguitte, S. J. B., Roscoe, H. K., and Jones, A. E.: Observations of OH and HO<sub>2</sub> radicals in coastal Antarctica, *Atmospheric Chemistry and Physics*, 7, 4171-4185, 10.5194/acp-7-4171-2007, 2007.
- 1210 Boggs, P. T., Byrd, R. H., and Schnabel, R. B.: A Stable and Efficient Algorithm for Nonlinear Orthogonal Distance Regression, *Siam Journal on Scientific and Statistical Computing*, 8, 1052-1078, 10.1137/0908085, 1987.
- Bohn, B., Corlett, G. K., Gillmann, M., Sanghavi, S., Stange, G., Tensing, E., Vrekoussis, M., Bloss, W. J., Clapp, L. J., Kortner, M., Dorn, H. P., Monks, P. S., Platt, U., Plass-Dulmer, C., Mihalopoulos, N., Heard, D. E., Clemmshaw, K. C., 1215 Meixner, F. X., Prevot, A. S. H., and Schmitt, R.: Photolysis frequency measurement techniques: results of a comparison within the ACCENT project, *Atmospheric Chemistry and Physics*, 8, 5373-5391, 10.5194/acp-8-5373-2008, 2008.
- Brune, W. H., Baier, B. C., Thomas, J., Ren, X., Cohen, R. C., Pusede, S. E., Browne, E. C., Goldstein, A. H., Gentner, D. R., Keutsch, F. N., Thornton, J. A., Harrold, S., Lopez-Hilfiker, F. D., and Wennberg, P. O.: Ozone production chemistry in the presence of urban plumes, *Faraday Discussions*, 189, 169-189, 10.1039/c5fd00204d, 2016.
- 1220 Carslaw, N., Creasey, D. J., Harrison, D., Heard, D. E., Hunter, M. C., Jacobs, P. J., Jenkin, M. E., Lee, J. D., Lewis, A. C., Pilling, M. J., Saunders, S. M., and Seakins, P. W.: OH and HO<sub>2</sub> radical chemistry in a forested region of north-western Greece, *Atmospheric Environment*, 35, 4725-4737, 10.1016/S1352-2310(01)00089-9, 2001.
- Cazorla, M., and Brune, W. H.: Measurement of Ozone Production Sensor, *Atmospheric Measurement Techniques*, 3, 545-555, 10.5194/amt-3-545-2010, 2010.
- 1225 Cazorla, M., Brune, W. H., Ren, X., and Lefer, B.: Direct measurement of ozone production rates in Houston in 2009 and comparison with two estimation methods, *Atmospheric Chemistry and Physics*, 12, 1203-1212, 10.5194/acp-12-1203-2012, 2012.
- Chao, W., Hsieh, J. T., Chang, C. H., and Lin, J. J.: Atmospheric chemistry. Direct kinetic measurement of the reaction of the simplest Criegee intermediate with water vapor, *Science*, 347, 751-754, 10.1126/science.1261549, 2015.
- 1230 Chen, W., Tang, H. Z., and Zhao, H. M.: Diurnal, weekly and monthly spatial variations of air pollutants and air quality of Beijing, *Atmospheric Environment*, 119, 21-34, 10.1016/j.atmosenv.2015.08.040, 2015.
- Creasey, D. J., HalfordMaw, P. A., Heard, D. E., Pilling, M. J., and Whitaker, B. J.: Implementation and initial deployment of a field instrument for measurement of OH and HO<sub>2</sub> in the troposphere by laser-induced fluorescence, *Journal of the Chemical Society-Faraday Transactions*, 93, 2907-2913, 10.1039/a701469d, 1997a.
- 1235 Creasey, D. J., Heard, D. E., Pilling, M. J., Whitaker, B. J., Berzins, M., and Fairlie, R.: Visualisation of a supersonic free-jet expansion using laser-induced fluorescence spectroscopy: Application to the measurement of rate constants at ultralow temperatures, *Applied Physics B: Lasers and Optics*, 65, 375-391, 10.1007/s003400050285, 1997b.
- Creasey, D. J., Heard, D. E., and Lee, J. D.: OH and HO<sub>2</sub> measurements in a forested region of north-western Greece, *Atmospheric Environment*, 35, 4713-4724, 10.1016/S1352-2310(01)00090-5, 2001.
- 1240 Creasey, D. J., Evans, G. E., Heard, D. E., and Lee, J. D.: Measurements of OH and HO<sub>2</sub> concentrations in the Southern Ocean marine boundary layer, *Journal of Geophysical Research: Atmospheres*, 108, D15, 4475, 10.1029/2002JD003206, 2003.
- Crouse, J. D., Paulot, F., Kjaergaard, H. G., and Wennberg, P. O.: Peroxy radical isomerization in the oxidation of isoprene, *Physical Chemistry Chemical Physics*, 13, 13607-13613, 10.1039/c1cp21330j, 2011.
- 1245 Crouse, J. D., Knap, H. C., Ornsø, K. B., Jorgensen, S., Paulot, F., Kjaergaard, H. G., and Wennberg, P. O.: Atmospheric fate of methacrolein. 1. Peroxy radical isomerization following addition of OH and O<sub>2</sub>, *Journal of Physical Chemistry A*, 116, 5756-5762, 10.1021/jp211560u, 2012.

- Cryer, D. R.: Measurements of hydroxyl radical reactivity and formaldehyde in the atmosphere, PhD thesis, School of Chemistry, University of Leeds, 2016.
- 1250 da Silva, G., Graham, C., and Wang, Z. F.: Unimolecular beta-hydroxyperoxy radical decomposition with OH recycling in the photochemical oxidation of isoprene, *Environmental Science and Technology*, 44, 250-256, 10.1021/es900924d, 2010.
- Dillon, T. J., and Crowley, J. N.: Direct detection of OH formation in the reactions of HO<sub>2</sub> with CH<sub>2</sub>C(O)O<sub>2</sub> and other substituted peroxy radicals, *Atmospheric Chemistry and Physics*, 8, 4877-4889, 10.5194/acp-8-4877-2008, 2008.
- 1255 Dubey, M. K., Hanisco, T. F., Wennberg, P. O., and Anderson, J. G.: Monitoring potential photochemical interference in laser-induced fluorescence measurements of atmospheric OH, *Geophysical Research Letters*, 23, 3215-3218, 10.1029/96gl03008, 1996.
- Dusanter, S., Vimal, D., Stevens, P. S., Volkamer, R., and Molina, L. T.: Measurements of OH and HO<sub>2</sub> concentrations during the MCMA-2006 field campaign - Part 1: Deployment of the Indiana University laser-induced fluorescence instrument, *Atmospheric Chemistry and Physics*, 9, 1665-1685, 10.5194/acp-9-1665-2009, 2009.
- 1260 Edwards, G. D., Cantrell, C. A., Stephens, S., Hill, B., Goyea, O., Shetter, R. E., Mauldin, R. L., 3rd, Kosciuch, E., Tanner, D. J., and Eisele, F. L.: Chemical ionization mass spectrometer instrument for the measurement of tropospheric HO<sub>2</sub> and RO<sub>2</sub>, *Analytical Chemistry*, 75, 5317-5327, 10.1021/ac034402b, 2003.
- 1265 Emmerson, K. M., Carslaw, N., Carslaw, D. C., Lee, J. D., McFiggans, G., Bloss, W. J., Gravestock, T., Heard, D. E., Hopkins, J., Ingham, T., Pilling, M. J., Smith, S. C., Jacob, M., and Monks, P. S.: Free radical modelling studies during the UK TORCH Campaign in Summer 2003, *Atmospheric Chemistry and Physics*, 7, 167-181, 10.5194/acp-7-167-2007, 2007.
- Faloona, I., Tan, D., Brune, W., Hurst, J., Barket, D., Couch, T. L., Shepson, P., Apel, E., Riemer, D., Thornberry, T., Carroll, M. A., Sillman, S., Keeler, G. J., Sagady, J., Hooper, D., and Paterson, K.: Nighttime observations of anomalously high levels of hydroxyl radicals above a deciduous forest canopy, *Journal of Geophysical Research-Atmospheres*, 106, 24315-24333, 10.1029/2000jd900691, 2001.
- 1270 Faloona, I. C., Tan, D., Leshner, R. L., Hazen, N. L., Frame, C. L., Simpas, J. B., Harder, H., Martinez, M., Di Carlo, P., Ren, X. R., and Brune, W. H.: A laser-induced fluorescence instrument for detecting tropospheric OH and HO<sub>2</sub>: Characteristics and calibration, *Journal of Atmospheric Chemistry*, 47, 139-167, 10.1023/B:JOCH.0000021036.53185.0e, 2004.
- 1275 Feiner, P. A., Brune, W. H., Miller, D. O., Zhang, L., Cohen, R. C., Romer, P. S., Goldstein, A. H., Keutsch, F. N., Skog, K. M., Wennberg, P. O., Nguyen, T. B., Teng, A. P., DeGouw, J., Koss, A., Wild, R. J., Brown, S. S., Guenther, A., Edgerton, E., Baumann, K., and Fry, J. L.: Testing Atmospheric Oxidation in an Alabama Forest, *Journal of the Atmospheric Sciences*, 73, 4699-4710, 10.1175/Jas-D-16-0044.1, 2016.
- 1280 Fittschen, C., Al Ajami, M., Batut, S., Ferracci, V., Archer-Nicholls, S., Archibald, A. T., and Schoemaeker, C.: ROOOH: a missing piece of the puzzle for OH measurements in low-NO environments?, *Atmospheric Chemistry and Physics*, 19, 349-362, 10.5194/acp-19-349-2019, 2019.
- Fuchs, H., Holland, F., and Hofzumahaus, A.: Measurement of tropospheric RO<sub>2</sub> and HO<sub>2</sub> radicals by a laser-induced fluorescence instrument, *Review of Scientific Instruments*, 79, 084104, 10.1063/1.2968712, 2008.
- 1285 Fuchs, H., Bohn, B., Hofzumahaus, A., Holland, F., Lu, K. D., Nehr, S., Rohrer, F., and Wahner, A.: Detection of HO<sub>2</sub> by laser-induced fluorescence: calibration and interferences from RO<sub>2</sub> radicals, *Atmospheric Measurement Techniques*, 4, 1209-1225, 10.5194/amt-4-1209-2011, 2011.
- Fuchs, H., Hofzumahaus, A., Rohrer, F., Bohn, B., Brauers, T., Dorn, H. P., Haseler, R., Holland, F., Kaminski, M., Li, X., Lu, K., Nehr, S., Tillmann, R., Wegener, R., and Wahner, A.: Experimental evidence for efficient hydroxyl radical regeneration in isoprene oxidation, *Nature Geoscience*, 6, 1023-1026, 10.1038/Ngeo1964, 2013.
- 1290 Fuchs, H., Acir, I. H., Bohn, B., Brauers, T., Dorn, H. P., Haseler, R., Hofzumahaus, A., Holland, F., Kaminski, M., Li, X., Lu, K., Lutz, A., Nehr, S., Rohrer, F., Tillmann, R., Wegener, R., and Wahner, A.: OH regeneration from methacrolein oxidation investigated in the atmosphere simulation chamber SAPHIR, *Atmospheric Chemistry and Physics*, 14, 7895-7908, 10.5194/acp-14-7895-2014, 2014.
- 1295 Fuchs, H., Tan, Z. F., Hofzumahaus, A., Broch, S., Dorn, H. P., Holland, F., Kunstler, C., Gomm, S., Rohrer, F., Schrade, S., Tillmann, R., and Wahner, A.: Investigation of potential interferences in the detection of atmospheric RO<sub>x</sub> radicals by laser-induced fluorescence under dark conditions, *Atmospheric Measurement Techniques*, 9, 1431-1447, 10.5194/amt-9-1431-2016, 2016.
- 1300 Fuchs, H., Tan, Z. F., Lu, K. D., Bohn, B., Broch, S., Brown, S. S., Dong, H. B., Gomm, S., Haseler, R., He, L. Y., Hofzumahaus, A., Holland, F., Li, X., Liu, Y., Lu, S. H., Min, K. E., Rohrer, F., Shao, M., Wang, B. L., Wang, M., Wu,

- Y. S., Zeng, L. M., Zhang, Y. S., Wahner, A., and Zhang, Y. H.: OH reactivity at a rural site (Wangdu) in the North China Plain: contributions from OH reactants and experimental OH budget, *Atmospheric Chemistry and Physics*, 17, 645-661, 10.5194/acp-17-645-2017, 2017.
- 1305 Fuchs, H., Albrecht, S., Acir, I., Bohn, B., Breitenlechner, M., Dorn, H. P., Gkatzelis, G. I., Hofzumahaus, A., Holland, F., Kaminski, M., Keutsch, F. N., Novelli, A., Reimer, D., Rohrer, F., Tillmann, R., Vereecken, L., Wegener, R., Zaytsev, A., Kiendler-Scharr, A., and Wahner, A.: Investigation of the oxidation of methyl vinyl ketone (MVK) by OH radicals in the atmospheric simulation chamber SAPHIR, *Atmospheric Chemistry and Physics*, 18, 8001-8016, 10.5194/acp-18-8001-2018, 2018.
- 1310 Griffith, S. M., Hansen, R. F., Dusanter, S., Stevens, P. S., Alaghmand, M., Bertman, S. B., Carroll, M. A., Erickson, M., Galloway, M., Grossberg, N., Hottle, J., Hou, J., Jobson, B. T., Kamrath, A., Keutsch, F. N., Lefer, B. L., Mielke, L. H., O'Brien, A., Shepson, P. B., Thurlow, M., Wallace, W., Zhang, N., and Zhou, X. L.: OH and HO<sub>2</sub> radical chemistry during PROPHET 2008 and CABINEX 2009-Part 1: Measurements and model comparison, *Atmospheric Chemistry and Physics*, 13, 5403-5423, 10.5194/acp-13-5403-2013, 2013.
- 1315 Griffith, S. M., Hansen, R. F., Dusanter, S., Michoud, V., Gilman, J. B., Kuster, W. C., Veres, P. R., Graus, M., de Gouw, J. A., Roberts, J., Young, C., Washenfelder, R., Brown, S. S., Thalman, R., Waxman, E., Volkamer, R., Tsai, C., Stutz, J., Flynn, J. H., Grossberg, N., Lefer, B., Alvarez, S. L., Rappenglueck, B., Mielke, L. H., Osthoff, H. D., and Stevens, P. S.: Measurements of hydroxyl and hydroperoxy radicals during CalNex-LA: Model comparisons and radical budgets, *Journal of Geophysical Research-Atmospheres*, 121, 4211-4232, 10.1002/2015jd024358, 2016.
- 1320 Hammes, J., Tsiligiannis, E., Mentel, T. F., and Hallquist, M.: Effect of NO<sub>x</sub> on 1,3,5-trimethylbenzene (TMB) oxidation product distribution and particle formation, *Atmospheric Chemistry and Physics*, 2019, 19, 15073-15086, 10.5194/acp-19-15073-2019, 2019.
- Hansen, R. F., Lewis, T. R., Graham, L., Whalley, L. K., Seakins, P. W., Heard, D. E., and Blitz, M. A.: OH production from the photolysis of isoprene-derived peroxy radicals: cross-sections, quantum yields and atmospheric implications, *Phys Chem Chem Phys*, 19, 2332-2345, 10.1039/c6cp06718b, 2017.
- 1325 Hard, T. M., O'Brien, R. J., Chan, C. Y., and Mehrabzadeh, A. A.: Tropospheric Free-Radical Determination by fluorescence by gas expansion, *Environmental Science & Technology*, 18, 768-777, 10.1021/es00128a009, 1984.
- Heard, D. E., Carpenter, L. J., Creasey, D. J., Hopkins, J. R., Lee, J. D., Lewis, A. C., Pilling, M. J., Seakins, P. W., Carslaw, N., and Emmerson, K. M.: High levels of the hydroxyl radical in the winter urban troposphere, *Geophysical Research Letters*, 31, L18112, 10.1029/2004GL020544, 2004.
- 1330 Hens, K., Novelli, A., Martinez, M., Auld, J., Axinte, R., Bohn, B., Fischer, H., Keronen, P., Kubistin, D., Nolscher, A. C., Oswald, R., Paasonen, P., Petaja, T., Regelin, E., Sander, R., Sinha, V., Sipila, M., Taraborrelli, D., Ernest, C. T., Williams, J., Lelieveld, J., and Harder, H.: Observation and modelling of HO<sub>x</sub> radicals in a boreal forest, *Atmospheric Chemistry and Physics*, 14, 8723-8747, 10.5194/acp-14-8723-2014, 2014.
- 1335 Hewitt, C. N., Lee, J. D., MacKenzie, A. R., Barkley, M. P., Carslaw, N., Carver, G. D., Chappell, N. A., Coe, H., Collier, C., Commane, R., Davies, F., Davison, B., DiCarlo, P., Di Marco, C. F., Dorsey, J. R., Edwards, P. M., Evans, M. J., Fowler, D., Furneaux, K. L., Gallagher, M., Guenther, A., Heard, D. E., Helfter, C., Hopkins, J., Ingham, T., Irwin, M., Jones, C., Karunaharan, A., Langford, B., Lewis, A. C., Lim, S. F., MacDonald, S. M., Mahajan, A. S., Malpass, S., McFiggans, G., Mills, G., Misztal, P., Moller, S., Monks, P. S., Nemitz, E., Nicolas-Perea, V., Oetjen, H., Oram, D. E., Palmer, P. I., Phillips, G. J., Pike, R., Plane, J. M. C., Pugh, T., Pyle, J. A., Reeves, C. E., Robinson, N. H., Stewart, D., Stone, D., Whalley, L. K., and Yin, X.: Overview: oxidant and particle photochemical processes above a south-east Asian tropical rainforest (the OP3 project): introduction, rationale, location characteristics and tools, *Atmospheric Chemistry and Physics*, 10, 169-199, 10.5194/acp-10-169-2010, 2010.
- 1340 Hofzumahaus, A., Rohrer, F., Lu, K., Bohn, B., Brauers, T., Chang, C. C., Fuchs, H., Holland, F., Kita, K., Kondo, Y., Li, X., Lou, S., Shao, M., Zeng, L., Wahner, A., and Zhang, Y.: Amplified trace gas removal in the troposphere, *Science*, 324, 1702-1704, 10.1126/science.1164566, 2009.
- 1345 Hofzumahaus, A., and Heard, D. E.: Assessment of Local HO<sub>x</sub> and RO<sub>x</sub> Measurement Techniques: Achievements, Challenges, and Future Directions - Outcomes of the 2015 International HO<sub>x</sub> Workshop, *IGAG News*, 55, 20-21, 2015.
- Lee, J. D., Whalley, L. K., Heard, D. E., Stone, D., Dunmore, R. E., Hamilton, J. F., Young, D. E., Allan, J. D., Laufs, S., and Kleffmann, J.: Detailed budget analysis of HONO in central London reveals a missing daytime source, *Atmospheric Chemistry and Physics*, 16, 2747-2764, 10.5194/acp-16-2747-2016, 2016.
- 1350 Lelieveld, J., Butler, T. M., Crowley, J. N., Dillon, T. J., Fischer, H., Ganzeveld, L., Harder, H., Lawrence, M. G., Martinez, M., Taraborrelli, D., and Williams, J.: Atmospheric oxidation capacity sustained by a tropical forest, *Nature*, 452, 737-740, 10.1038/nature06870, 2008.

- 355 [Lew, M. L., Rickly, P. S., Bottorff, B. P., Sklaveniti, S., Léonardis, T., Locoge, N., Dusanter, S., Kundu, S., Wood, E., and Stevens, P. S.: OH and HO<sub>2</sub> radical chemistry in a midlatitude forest: Measurements and model comparisons, \*Atmos. Chem. Phys. Discuss.\*, 2019, 1-35, \[10.5194/acp-2019-726\]\(#\), 2019.](#)
- Lewis, T. R., Blitz, M. A., Heard, D. E., and Seakins, P. W.: Direct evidence for a substantive reaction between the Criegee intermediate, CH<sub>2</sub>OO, and the water vapour dimer, *Phys Chem Chem Phys*, 17, 4859-4863, [10.1039/c4cp04750h](#), 2015.
- 1360 Lin, L. C., Chao, W., Chang, C. H., Takahashi, K., and Lin, J. J.: Temperature dependence of the reaction of anti-CH<sub>3</sub>CHO with water vapor, *Phys Chem Chem Phys*, 18, 28189-28197, [10.1039/c6cp05171e](#), 2016.
- Lu, K. D., Rohrer, F., Holland, F., Fuchs, H., Brauers, T., Oebel, A., Dlugi, R., Hu, M., Li, X., Lou, S. R., Shao, M., Zhu, T., Wahner, A., Zhang, Y. H., and Hofzumahaus, A.: Nighttime observation and chemistry of HO<sub>x</sub> in the Pearl River Delta and Beijing in summer 2006, *Atmospheric Chemistry and Physics*, 14, 4979-4999, [10.5194/acp-14-4979-2014](#), 2014.
- 1365 Mallik, C., Tomsche, L., Bourtsoukidis, E., Crowley, J. N., Derstroff, B., Fischer, H., Hafermann, S., Huser, I., Javed, U., Kessel, S., Lelieveld, J., Martinez, M., Meusel, H., Novelli, A., Phillips, G. J., Pozzer, A., Reiffs, A., Sander, R., Taraborrelli, D., Sauvage, C., Schuladen, J., Su, H., Williams, J., and Harder, H.: Oxidation processes in the eastern Mediterranean atmosphere: evidence from the modelling of HO<sub>x</sub> measurements over Cyprus, *Atmospheric Chemistry and Physics*, 18, 10825-10847, [10.5194/acp-18-10825-2018](#), 2018.
- 1370 Mao, J., Ren, X., Zhang, L., Van Duin, D. M., Cohen, R. C., Park, J. H., Goldstein, A. H., Paulot, F., Beaver, M. R., Crounse, J. D., Wennberg, P. O., DiGangi, J. P., Henry, S. B., Keutsch, F. N., Park, C., Schade, G. W., Wolfe, G. M., Thornton, J. A., and Brune, W. H.: Insights into hydroxyl measurements and atmospheric oxidation in a California forest, *Atmospheric Chemistry and Physics*, 12, 8009-8020, [10.5194/acp-12-8009-2012](#), 2012.
- 1375 Martinez, M., Harder, H., Ren, X., Leshner, R. L., and Brune, W. H.: Measuring atmospheric naphthalene with laser-induced fluorescence, *Atmospheric Chemistry and Physics*, 4, 563-569, [10.5194/acp-4-563-2004](#), 2004.
- Martinez, M., Harder, H., Kubistin, D., Rudolf, M., Bozem, H., Eerdeken, G., Fischer, H., Klupfel, T., Gurk, C., Konigstedt, R., Parchatka, U., Schiller, C. L., Stickler, A., Williams, J., and Lelieveld, J.: Hydroxyl radicals in the tropical troposphere over the Suriname rainforest: airborne measurements, *Atmospheric Chemistry and Physics*, 10, 3759-3773, [10.5194/acp-10-3759-2010](#), 2010.
- 1380 Molteni, U., Bianchi, F., Klein, F., El Haddad, I., Frege, C., Rossi, M. J., Dommen, J., and Baltensperger, U.: Formation of highly oxygenated organic molecules from aromatic compounds, *Atmospheric Chemistry and Physics*, 18, 1909-1921, [10.5194/acp-18-1909-2018](#), 2018.
- Newland, M. J., Rickard, A. R., Vereecken, L., Munoz, A., Rodenas, M., and Bloss, W. J.: Atmospheric isoprene ozonolysis: impacts of stabilised Criegee intermediate reactions with SO<sub>2</sub>, H<sub>2</sub>O and dimethyl sulfide, *Atmospheric Chemistry and Physics*, 15, 9521-9536, [10.5194/acp-15-9521-2015](#), 2015.
- 1385 Nguyen, T. L., Vereecken, L., and Peeters, J.: HO<sub>x</sub> regeneration in the oxidation of isoprene III: theoretical study of the key isomerisation of the Z-delta-hydroxy-peroxy isoprene radicals, *Chemphyschem*, 11, 3996-4001, [10.1002/cphc.201000480](#), 2010.
- 1390 Novelli, A., Hens, K., Ernest, C. T., Kubistin, D., Regelin, E., Elste, T., Plass-Dulmer, C., Martinez, M., Lelieveld, J., and Harder, H.: Characterisation of an inlet pre-injector laser-induced fluorescence instrument for the measurement of atmospheric hydroxyl radicals, *Atmospheric Measurement Techniques*, 7, 3413-3430, [10.5194/amt-7-3413-2014](#), 2014a.
- Novelli, A., Vereecken, L., Lelieveld, J., and Harder, H.: Direct observation of OH formation from stabilised Criegee intermediates, *Phys Chem Chem Phys*, 16, 19941-19951, [10.1039/c4cp02719a](#), 2014b.
- 1395 Novelli, A., Hens, K., Ernest, C. T., Martinez, M., Nolscher, A. C., Sinha, V., Paasonen, P., Petaja, T., Sipila, M., Elste, T., Plass-Dulmer, C., Phillips, G. J., Kubistin, D., Williams, J., Vereecken, L., Lelieveld, J., and Harder, H.: Estimating the atmospheric concentration of Criegee intermediates and their possible interference in a FAGE-LIF instrument, *Atmospheric Chemistry and Physics*, 17, 7807-7826, [10.5194/acp-17-7807-2017](#), 2017.
- 1400 Novelli, A., Kaminski, M., Rolletter, M., Acir, I. H., Bohn, B., Dorn, H. P., Li, X., Lutz, A., Nehr, S., Rohrer, F., Tillmann, R., Wegener, R., Holland, F., Hofzumahaus, A., Kiendler-Scharr, A., Wahner, A., and Fuchs, H.: Evaluation of OH and HO<sub>2</sub> concentrations and their budgets during photooxidation of 2-methyl-3-butene-2-ol (MBO) in the atmospheric simulation chamber SAPHIR, *Atmospheric Chemistry and Physics*, 18, 11409-11422, [10.5194/acp-18-11409-2018](#), 2018.
- 1405 Paulot, F., Crounse, J. D., Kjaergaard, H. G., Kurten, A., St Clair, J. M., Seinfeld, J. H., and Wennberg, P. O.: Unexpected epoxide formation in the gas-phase photooxidation of isoprene, *Science*, 325, 730-733, [10.1126/science.1172910](#), 2009.

- Peeters, J., Nguyen, T. L., and Vereecken, L.: HO<sub>x</sub> radical regeneration in the oxidation of isoprene, *Physical Chemistry Chemical Physics*, 11, 5935-5939, 10.1039/b908511d, 2009.
- 1410 Peeters, J., and Muller, J. F.: HO(x) radical regeneration in isoprene oxidation via peroxy radical isomerisations. II: experimental evidence and global impact, *Physical Chemistry Chemical Physics*, 12, 14227-14235, 10.1039/c0cp00811g, 2010.
- Peeters, J., Muller, J. F., Stavrou, T., and Nguyen, V. S.: Hydroxyl radical recycling in isoprene oxidation driven by hydrogen bonding and hydrogen tunneling: the upgraded LIM1 mechanism, *Journal of Physical Chemistry A*, 118, 8625-8643, 10.1021/jp5033146, 2014.
- 1415 Praske, E., Crounse, J. D., Bates, K. H., Kurten, T., Kjaergaard, H. G., and Wennberg, P. O.: Atmospheric fate of methyl vinyl ketone: peroxy radical reactions with NO and HO<sub>2</sub>, *Journal of Physical Chemistry A*, 119, 4562-4572, 10.1021/jp5107058, 2015.
- Ren, X. R., Harder, H., Martinez, M., Faloona, I. C., Tan, D., Leshner, R. L., Di Carlo, P., Simpas, J. B., and Brune, W. H.: Interference testing for atmospheric HO<sub>x</sub> measurements by laser-induced fluorescence, *Journal of Atmospheric Chemistry*, 47, 169-190, 10.1023/B:Joch.0000021037.46866.81, 2004.
- 1420 Ren, X. R., Olson, J. R., Crawford, J. H., Brune, W. H., Mao, J. Q., Long, R. B., Chen, Z., Chen, G., Avery, M. A., Sachse, G. W., Barrick, J. D., Diskin, G. S., Huey, L. G., Fried, A., Cohen, R. C., Heikes, B., Wennberg, P. O., Singh, H. B., Blake, D. R., and Shetter, R. E.: HO<sub>x</sub> chemistry during INTEX-A 2004: Observation, model calculation, and comparison with previous studies, *Journal of Geophysical Research-Atmospheres*, 113, D05310, Art. D0531010.1029/2007jd009166, 2008.
- 1425 Ren, X. R., van Duin, D., Cazorla, M., Chen, S., Mao, J. Q., Zhang, L., Brune, W. H., Flynn, J. H., Grossberg, N., Lefer, B. L., Rappengluck, B., Wong, K. W., Tsai, C., Stutz, J., Dibb, J. E., Jobson, B. T., Luke, W. T., and Kelley, P.: Atmospheric oxidation chemistry and ozone production: Results from SHARP 2009 in Houston, Texas, *Journal of Geophysical Research-Atmospheres*, 118, 5770-5780, 10.1002/jgrd.50342, 2013.
- 1430 Rickly, P., and Stevens, P. S.: Measurements of a potential interference with laser-induced fluorescence measurements of ambient OH from the ozonolysis of biogenic alkenes, *Atmospheric Measurement Techniques*, 11, 1-16, 10.5194/amt-11-1-2018, 2018.
- Sander, S. P., Abbatt, J., Barker, J. R., Burkholder, J. B., Friedl, D. M., Golden, D. M., Huie, R. E., Kolb, C. E., Kurylo, M. J., Moortgat, G. K., Orkin, V. L., and Wine, P. H.: *Chemical Kinetics and Photochemical Data for Use in Atmospheric Studies*, Evaluation No. 17, 2011.
- 1435 Sheps, L., Scully, A. M., and Au, K.: UV absorption probing of the conformer-dependent reactivity of a Criegee intermediate CH<sub>3</sub>CHOO, *Physical Chemistry Chemical Physics*, 16, 26701-26706, 10.1039/c4cp04408h, 2014.
- 1440 Shi, Z., Vu, T., Kotthaus, S., Grimmond, S., Harrison, R. M., Yue, S., Zhu, T., Lee, J., Han, Y., Demuzere, M., Dunmore, R. E., Ren, L., Liu, D., Wang, Y., Wild, O., Allan, J., Barlow, J., Beddows, D., Bloss, W. J., Carruthers, D., Carslaw, D. C., Chatzidiakou, L., Crilley, L., Coe, H., Dai, T., Doherty, R., Duan, F., Fu, P., Ge, B., Ge, M., Guan, D., Hamilton, J. F., He, K., Heal, M., Heard, D., Hewitt, C. N., Hu, M., Ji, D., Jiang, X., Jones, R., Kalberer, M., Kelly, F. J., Kramer, L., Langford, B., Lin, C., Lewis, A. C., Li, J., Li, W., Liu, H., Loh, M., Lu, K., Mann, G., McFiggans, G., Miller, M., Mills, G., Monk, P., Nemitz, E., O'Connor, F., Ouyang, B., Palmer, P. I., Percival, C., Popoola, O., Reeves, C., Rickard, A. R., Shao, L., Shi, G., Spracklen, D., Stevenson, D., Sun, Y., Sun, Z., Tao, S., Tong, S., Wang, Q., Wang, W., Wang, X., Wang, Z., Whalley, L., Wu, X., Wu, Z., Xie, P., Yang, F., Zhang, Q., Zhang, Y., Zhang, Y., and Zheng, M.: Introduction to Special Issue – In-depth study of air pollution sources and processes within Beijing and its surrounding region (APHH-Beijing), *Atmospheric Chemistry Physics*, 19, 7519–7546, 2019, 10.5194/acp-19-7519-2019, 2019..
- 1445 Smith, S. C., Lee, J. D., Bloss, W. J., Johnson, G. P., Ingham, T., and Heard, D. E.: Concentrations of OH and HO<sub>2</sub> radicals during NAMBLEX: measurements and steady state analysis, *Atmospheric Chemistry and Physics*, 6, 1435-1453, 10.5194/acp-6-1435-2006, 2006.
- 1450 Stevens, P. S., Mather, J. H., and Brune, W. H.: Measurement of Tropospheric OH and HO<sub>2</sub> by Laser-Induced Fluorescence at Low-Pressure, *Journal of Geophysical Research-Atmospheres*, 99, 3543-3557, 10.1029/93jd03342, 1994.
- 1455 Stone, D., Evans, M. J., Edwards, P. M., Commane, R., Ingham, T., Rickard, A. R., Brookes, D. M., Hopkins, J., Leigh, R. J., Lewis, A. C., Monks, P. S., Oram, D., Reeves, C. E., Stewart, D., and Heard, D. E.: Isoprene oxidation mechanisms: measurements and modelling of OH and HO<sub>2</sub> over a South-East Asian tropical rainforest during the OP3 field campaign, *Atmospheric Chemistry and Physics*, 11, 6749-6771, 10.5194/acp-11-6749-2011, 2011.
- Stone, D., Whalley, L. K., Ingham, T., Edwards, P. M., Cryer, D. R., Brumby, C. A., Seakins, P. W., and Heard, D. E.: Measurement of OH reactivity by laser flash photolysis coupled with laser-induced fluorescence spectroscopy, *Atmospheric Measurement Techniques*, 9, 2827-2844, 10.5194/amt-9-2827-2016, 2016.

- 1460 Taatjes, C. A., Welz, O., Eskola, A. J., Savee, J. D., Scheer, A. M., Shallcross, D. E., Rotavera, B., Lee, E. P., Dyke, J. M., Mok, D. K., Osborn, D. L., and Percival, C. J.: Direct measurements of conformer-dependent reactivity of the Criegee intermediate  $\text{CH}_3\text{CHOO}$ , *Science*, 340, 177-180, 10.1126/science.1234689, 2013.
- Tan, Z., Lu, K., Hofzumahaus, A., Fuchs, H., Bohn, B., Holland, F., Liu, Y., Rohrer, F., Shao, M., Sun, K., Wu, Y., Zeng, L., Zhang, Y., Zou, Q., Kiendler-Scharr, A., Wahner, A., and Zhang, Y.: Experimental budgets of OH,  $\text{HO}_2$ , and  $\text{RO}_2$  radicals and implications for ozone formation in the Pearl River Delta in China 2014, *Atmospheric Chemistry and Physics*, 19, 7129-7150, 10.5194/acp-19-7129-2019, 2019.
- 1465 Tan, Z. F., Fuchs, H., Lu, K. D., Hofzumahaus, A., Bohn, B., Broch, S., Dong, H. B., Gomm, S., Haseler, R., He, L. Y., Holland, F., Li, X., Liu, Y., Lu, S. H., Rohrer, F., Shao, M., Wang, B. L., Wang, M., Wu, Y. S., Zeng, L. M., Zhang, Y. S., Wahner, A., and Zhang, Y. H.: Radical chemistry at a rural site (Wangdu) in the North China Plain: observation and model calculations of OH,  $\text{HO}_2$  and  $\text{RO}_2$  radicals, *Atmospheric Chemistry and Physics*, 17, 663-690, 10.5194/acp-17-663-2017, 2017.
- 1470 Tan, Z. F., Rohrer, F., Lu, K. D., Ma, X. F., Bohn, B., Broch, S., Dong, H. B., Fuchs, H., Gkatzelis, G. I., Hofzumahaus, A., Holland, F., Li, X., Liu, Y., Liu, Y. H., Novelli, A., Shao, M., Wang, H. C., Wu, Y. S., Zeng, L. M., Hu, M., Kiendler-Scharr, A., Wahner, A., and Zhang, Y. H.: Wintertime photochemistry in Beijing: observations of  $\text{RO}_x$  radical concentrations in the North China Plain during the BEST-ONE campaign, *Atmospheric Chemistry and Physics*, 18, 12391-12411, 10.5194/acp-18-12391-2018, 2018.
- 1475 Teng, A. P., Crounse, J. D., and Wennberg, P. O.: Isoprene Peroxy Radical Dynamics, *Journal of the American Chemical Society*, 139, 5367-5377, 10.1021/jacs.6b12838, 2017.
- 1480 Wang, S., Wu, R., Berndt, T., Ehn, M., and Wang, L.: Formation of Highly Oxidized Radicals and Multifunctional Products from the Atmospheric Oxidation of Alkylbenzenes, *Environmental Science & Technology*, 51, 8442-8449, 10.1021/acs.est.7b02374, 2017.
- Welz, O., Savee, J. D., Osborn, D. L., Vasu, S. S., Percival, C. J., Shallcross, D. E., and Taatjes, C. A.: Direct kinetic measurements of Criegee intermediate ( $\text{CH}_2\text{OO}$ ) formed by reaction of  $\text{CH}_2\text{I}$  with  $\text{O}_2$ , *Science*, 335, 204-207, 10.1126/science.1213229, 2012.
- 1485 Welz, O., Eskola, A. J., Sheps, L., Rotavera, B., Savee, J. D., Scheer, A. M., Osborn, D. L., Lowe, D., Murray Booth, A., Xiao, P., Anwar, H. K. M., Percival, C. J., Shallcross, D. E., and Taatjes, C. A.: Rate coefficients of C(1) and C(2) Criegee intermediate reactions with formic and acetic Acid near the collision limit: direct kinetics measurements and atmospheric implications, *Angewandte Chemie International Edition English*, 53, 4547-4550, 10.1002/anie.201400964, 2014.
- 1490 Whalley, L. K., Furneaux, K. L., Goddard, A., Lee, J. D., Mahajan, A., Oetjen, H., Read, K. A., Kaaden, N., Carpenter, L. J., Lewis, A. C., Plane, J. M. C., Saltzman, E. S., Wiedensohler, A., and Heard, D. E.: The chemistry of OH and  $\text{HO}_2$  radicals in the boundary layer over the tropical Atlantic Ocean, *Atmospheric Chemistry and Physics*, 10, 1555-1576, 10.5194/acp-10-1555-2010, 2010.
- 1495 Whalley, L. K., Edwards, P. M., Furneaux, K. L., Goddard, A., Ingham, T., Evans, M. J., Stone, D., Hopkins, J. R., Jones, C. E., Karunaharan, A., Lee, J. D., Lewis, A. C., Monks, P. S., Moller, S. J., and Heard, D. E.: Quantifying the magnitude of a missing hydroxyl radical source in a tropical rainforest, *Atmospheric Chemistry and Physics*, 11, 7223-7233, 10.5194/acp-11-7223-2011, 2011.
- 1500 Whalley, L. K., Blitz, M. A., Desservettaz, M., Seakins, P. W., and Heard, D. E.: Reporting the sensitivity of laser-induced fluorescence instruments used for  $\text{HO}_2$  detection to an interference from  $\text{RO}_2$  radicals and introducing a novel approach that enables  $\text{HO}_2$  and certain  $\text{RO}_2$  types to be selectively measured, *Atmospheric Measurement Techniques*, 6, 3425-3440, 10.5194/amt-6-3425-2013, 2013.
- Whalley, L. K., Stone, D., Bandy, B., Dunmore, R., Hamilton, J. F., Hopkins, J., Lee, J. D., Lewis, A. C., and Heard, D. E.: Atmospheric OH reactivity in central London: observations, model predictions and estimates of in situ ozone production, *Atmos. Chem. Phys.*, 16, 2109-2122, 10.5194/acp-16-2109-2016, 2016.
- 1505 Whalley, L. K., Stone, D., Dunmore, R., Hamilton, J., Hopkins, J. R., Lee, J. D., Lewis, A. C., Williams, P., Kleffmann, J., Laufs, S., Woodward-Massey, R., and Heard, D. E.: Understanding in situ ozone production in the summertime through radical observations and modelling studies during the Clean air for London project (ClearfLo), *Atmospheric Chemistry and Physics*, 18, 2547-2571, 10.5194/acp-18-2547-2018, 2018.
- 1510 Winiberg, F. A. F., Smith, S. C., Bejan, I., Brumby, C. A., Ingham, T., Malkin, T. L., Orr, S. C., Heard, D. E., and Seakins, P. W.: Pressure-dependent calibration of the OH and  $\text{HO}_2$  channels of a FAGE  $\text{HO}_x$  instrument using the Highly Instrumented Reactor for Atmospheric Chemistry (HIRAC), *Atmospheric Measurement Techniques*, 8, 523-540, 10.5194/amt-8-523-2015, 2015.
- Wolfe, G. M., Thornton, J. A., Bouvier-Brown, N. C., Goldstein, A. H., Park, J. H., McKay, M., Matross, D. M., Mao, J., Brune, W. H., LaFranchi, B. W., Browne, E. C., Min, K. E., Wooldridge, P. J., Cohen, R. C., Crounse, J. D., Faloona, I.

1515 C., Gilman, J. B., Kuster, W. C., de Gouw, J. A., Huisman, A., and Keutsch, F. N.: The Chemistry of Atmosphere-Forest Exchange (CAFE) Model - Part 2: Application to BEARPEX-2007 observations, *Atmospheric Chemistry and Physics*, 11, 1269-1294, 10.5194/acp-11-1269-2011, 2011.

Wolfe, G. M., Crounse, J. D., Parrish, J. D., St Clair, J. M., Beaver, M. R., Paulot, F., Yoon, T. P., Wennberg, P. O., and Keutsch, F. N.: Photolysis, OH reactivity and ozone reactivity of a proxy for isoprene-derived hydroperoxyenals (HPALDs), *Physical Chemistry Chemical Physics*, 14, 7276-7286, 10.1039/c2cp40388a, 2012.

520 ~~Woodward Massey, R.: Observations of radicals in the atmosphere: measurement validation and model comparisons, School of Chemistry, University of Leeds, 2018.~~

## Tables

1525

**Table 1.** Overall meteorological and chemical conditions encountered during each field campaign, including example VOCs. Values are given as the median of all points that coincide with IPI sampling periods, except for  $J(\text{O}^1\text{D})$  and  $\text{O}_3$ , which are reported as diurnally-averaged maxima.

	<b>ICOZA<sup>a</sup>ICOZA</b>	<b>AIRPRO<sup>b</sup>AIRPRO winter</b>	<b>AIRPRO summer</b>
<i>Dates (IPI sampling)</i>	3–8 and 12–16 Jul, 2015	2–7 Dec, 2016	23 May–25 Jun, 2017
<i>Location</i>	52°57'02''N, 1°07'19''E	39°58'28''N, 116°22'16''E	
<i>Meteorological</i>			
Temperature (°C)	16	6.1	26
H <sub>2</sub> O (%)	1.5	0.4	1.6
Wind speed (ms <sup>-1</sup> )	5.8	0.9	0.4
$J(\text{O}^1\text{D})$ (10 <sup>-6</sup> s <sup>-1</sup> )	16	3.5	19
<i>Chemical</i>			
O <sub>3</sub> (ppbv)	42	15	90
NO (ppbv)	0.19	22	0.81
NO <sub>2</sub> (ppbv)	2.2	33	17
CO (ppbv)	100	1120	460
Propane (ppbv)	0.26	6.2	3.8
Isoprene (ppbv)	0.02	0.07	0.38
Benzene (ppbv)	0.03	1.4	0.46
$k'_{\text{OH}}$ (s <sup>-1</sup> )	4.4	38	25

<sup>a</sup>Integrated Chemistry of OZone in the Atmosphere

<sup>b</sup>an integrated study of AIR pollution PROCesses in Beijing (Shi et al., 2019)

1530

**Table 2.** Internal removal of OH ( $\%$ ,  $\pm 2\sigma$ ) as a function of propane mixing ratio in the IPI flow tube, determined as shown in Figure 6 (see text for details).

Propane (ppmv)	Experiment no.	Internal removal (%)
110 (used for ICOZA and AIRPRO winter)	1	$-0.1 \pm 4.8$
	2	$0.3 \pm 7.7$
	3	$-0.9 \pm 16$
	<i>Average <math>\pm 2</math> SD</i> <i>Weighted average <math>\pm 2\sigma</math></i>	<i><math>0.2 \pm 1.10 \pm 4.0</math></i>
550	1	$1.0 \pm 9.6$
1100 (used for AIRPRO summer)	1	$1.9 \pm 12$
	2	$4.2 \pm 11$
	3	$2.5 \pm 11$
	<i>Average <math>\pm 2</math> SD</i> <i>Weighted average <math>\pm 2\sigma</math></i>	<i><math>2.8 \pm 2.39 \pm 6.6</math></i>

1535

**Table 3.** Summary of interference tests with O<sub>3</sub> and isoprene (ISO) in the presence of propane (PROP), based on the data in Figure 8.

Test	O <sub>3</sub> (ppmv)	H <sub>2</sub> O (%)	ISO (ppmv)	PROP (ppmv)	OHint (molecule cm <sup>-3</sup> )			
					Obs.	<sup>a</sup> O <sub>3</sub> /H <sub>2</sub> O corr.	<sup>b</sup> OP3 levels	<sup>c</sup> AIRPRO 2017 levels
A	1.64	0.73	0	110	$1.0 \times 10^7$	0	N/A	N/A
B	1.86	0.07	16	110	$1.9 \times 10^7$	$1.8 \times 10^7$	21	430
C	1.83	0.98	16	110	$1.6 \times 10^7$	$8.0 \times 10^5$	1	19
D	1.85	0.07	16	1100	$1.4 \times 10^7$	$1.3 \times 10^7$	15	310

<sup>a</sup>Corrected using equation (E7)

<sup>b</sup>Oxidant and Particle photochemical processes field campaign in Borneo, 2008: average O<sub>3</sub> = 10 ppbv, ISO = 3.5 ppbv

<sup>c</sup>Diurnally-averaged maximum O<sub>3</sub> = 90 ppbv, overall maximum ISO = 7.9 ppbv

1540


**Table 4.** Average contributions of FAGE background signals to the total OH measured (= (OHwave – OHchem)/OHwave) during ambient air studies where a chemical modulation technique was employed.


Study	Year	Location	Environment Type	Contribution (%)		Reference(s)
				Daytime	Nighttime	
PROPHET	1998	N Michigan	Forest, isoprene dominated	Not tested	~0	Faloona et al (2001)
BEARPEX	2009	NE California	Forest, <sup>a</sup> MBO dominated	40–60	50	Mao et al (2012)
CABINEX	2009	N Michigan	Forest, isoprene dominated	Not tested	50–100	Griffith et al (2013)
SHARP	2009	Houston, Texas	Urban	30	50	Ren et al (2013)
CalNex-LA	2010	Pasadena, California	Urban, downwind of LA	33*	Not reported	Griffith et al (2016)
CalNex-SJV	2010	Bakersfield, California	Urban	20	80	Brune et al (2016)
DOMINO	2010	El Arenosillo, near Huelva, SW Spain	Coastal, close to petrochemical industry	50	100	Novelli et al (2014)
HUMPPA-COPEC	2010	Hyytiälä, SW Finland	Boreal forest, terpene dominated	60–80	100	Hens et al (2014); Novelli et al (2014); Novelli et al (2017)
HOPE	2012	Hohenpeissenberg, S Germany	Rural	20–40	100	Novelli et al (2014); Novelli et al (2017)
SOAS	2013	near Brent, Alabama	Forest, isoprene dominated	80	>70	Feiner et al (2016)
Wangdu	2014	North China Plain	Rural, urban influenced	10	Not reported	Fuchs et al (2017); Tan et al (2017)
CYPHEX	2014	NW Cyprus	Coastal, influenced by processed European emissions	45	100	Mallik et al (2018)
PRIDE-PRD2014	2014	Pearl River Delta	Suburban, 60 km SW of Guangzhou	<del>0–20</del> <8	0–20	Tan et al (2019)
BEST-ONE	2016	North China Plain	Suburban, 60 km NE of Beijing	~0	~0	Tan et al (2018)
ICOZA	2015	N Norfolk Coast, UK	Coastal, London outflow	~0	~0	This work
AIRPRO <i>Winter</i>	2016	Beijing, China	Urban	~0	Nighttime OH almost always <LOD	This work
AIRPRO <i>Summer</i>	2017	Beijing, China	Urban	~0	~0	This work

<sup>a</sup>MBO = 2-methyl-3-buten-2-ol, a biogenic volatile organic compound


\*Consistent with known O<sub>3</sub>/H<sub>2</sub>O interference

# Figures

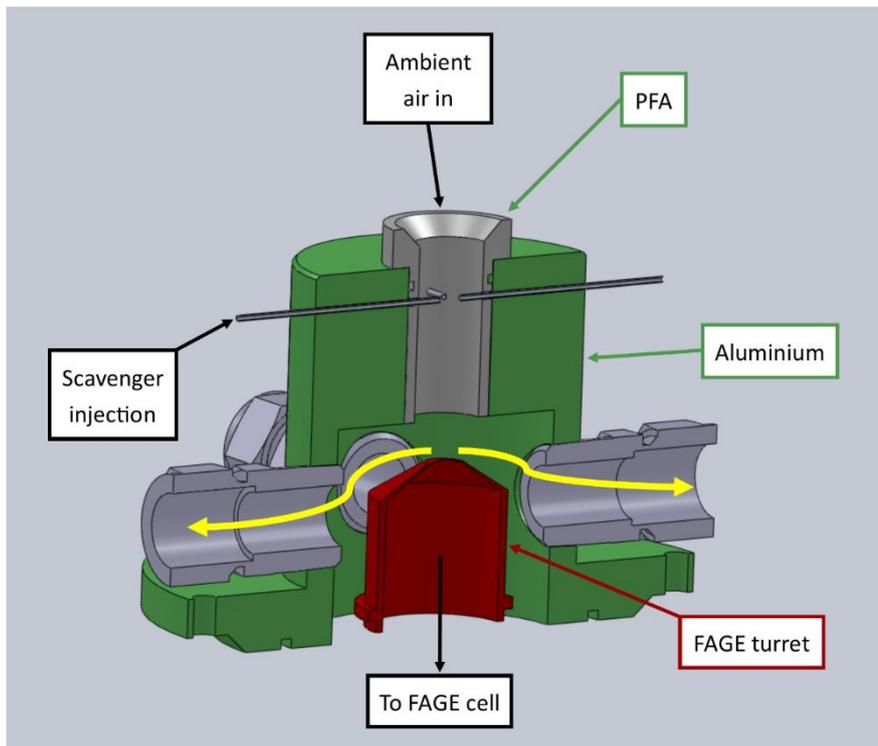


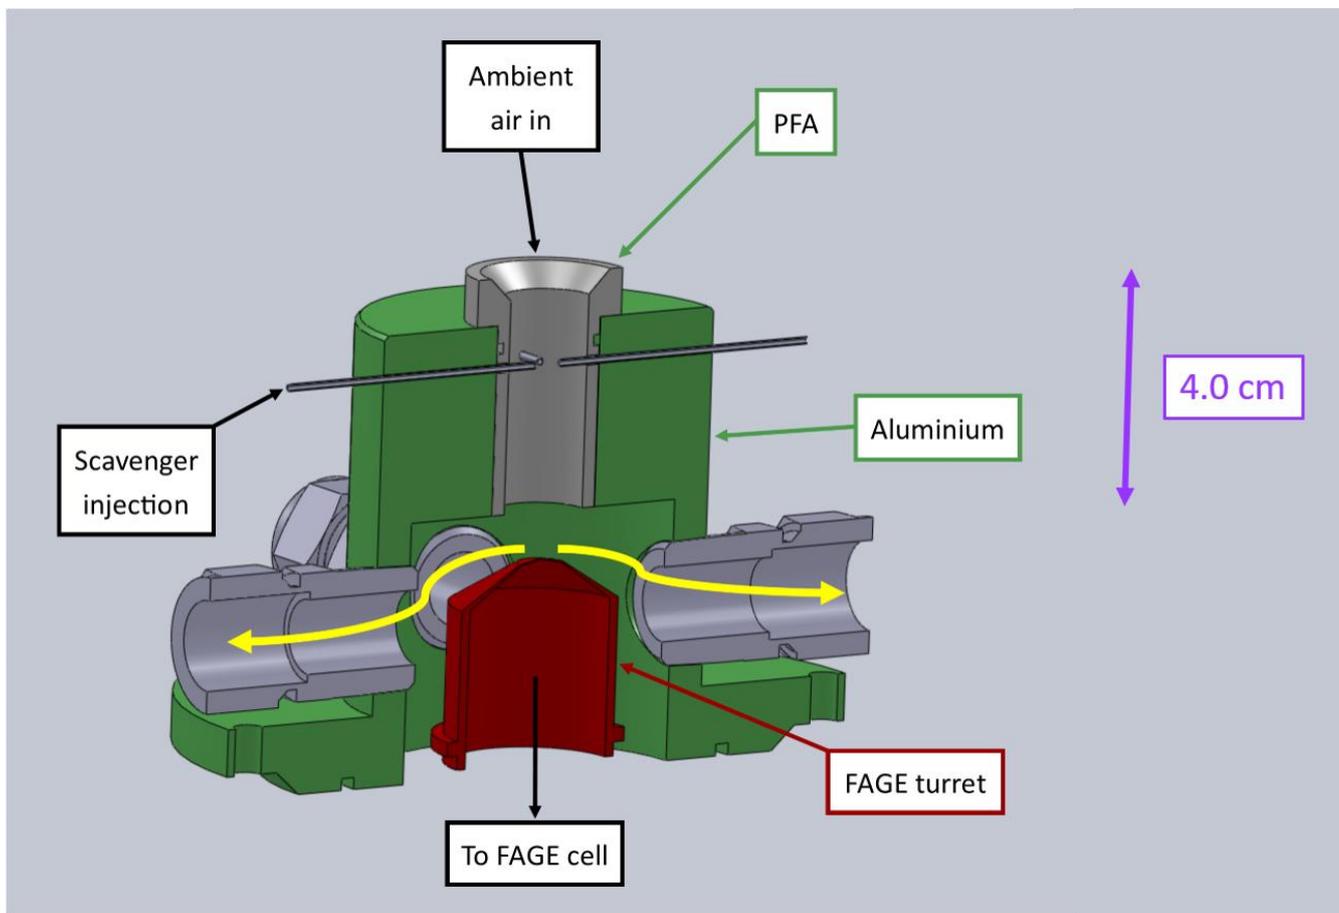



**Figure 1.** Labelled SolidWorks model of the Leeds inlet pre-injector (IPI). The scavenger is injected into the centre of the perfluoroalkoxy (PFA) flow tube via four 0.25 mm ID needles. The thick yellow arrows indicate the direction of the sheath flow.

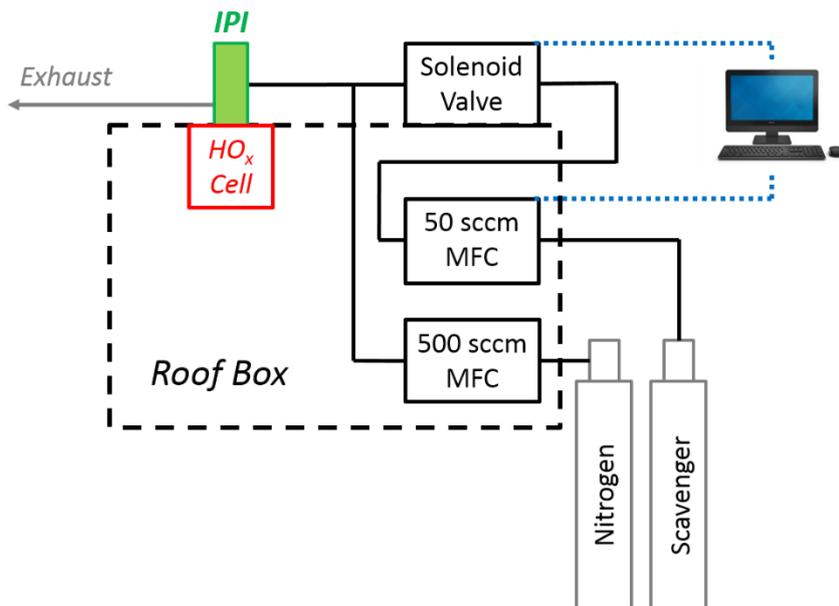


**Figure 2.** Diagram of the gas flows involved in IPI scavenger injection (not to scale). The two mass flow controllers (MFCs) are housed in the roof box, where the scavenger MFC (0–50 sccm) and injection valve (in a weatherproof housing on top of the roof box) are controlled using the main FAGE PC situated in the container laboratory.

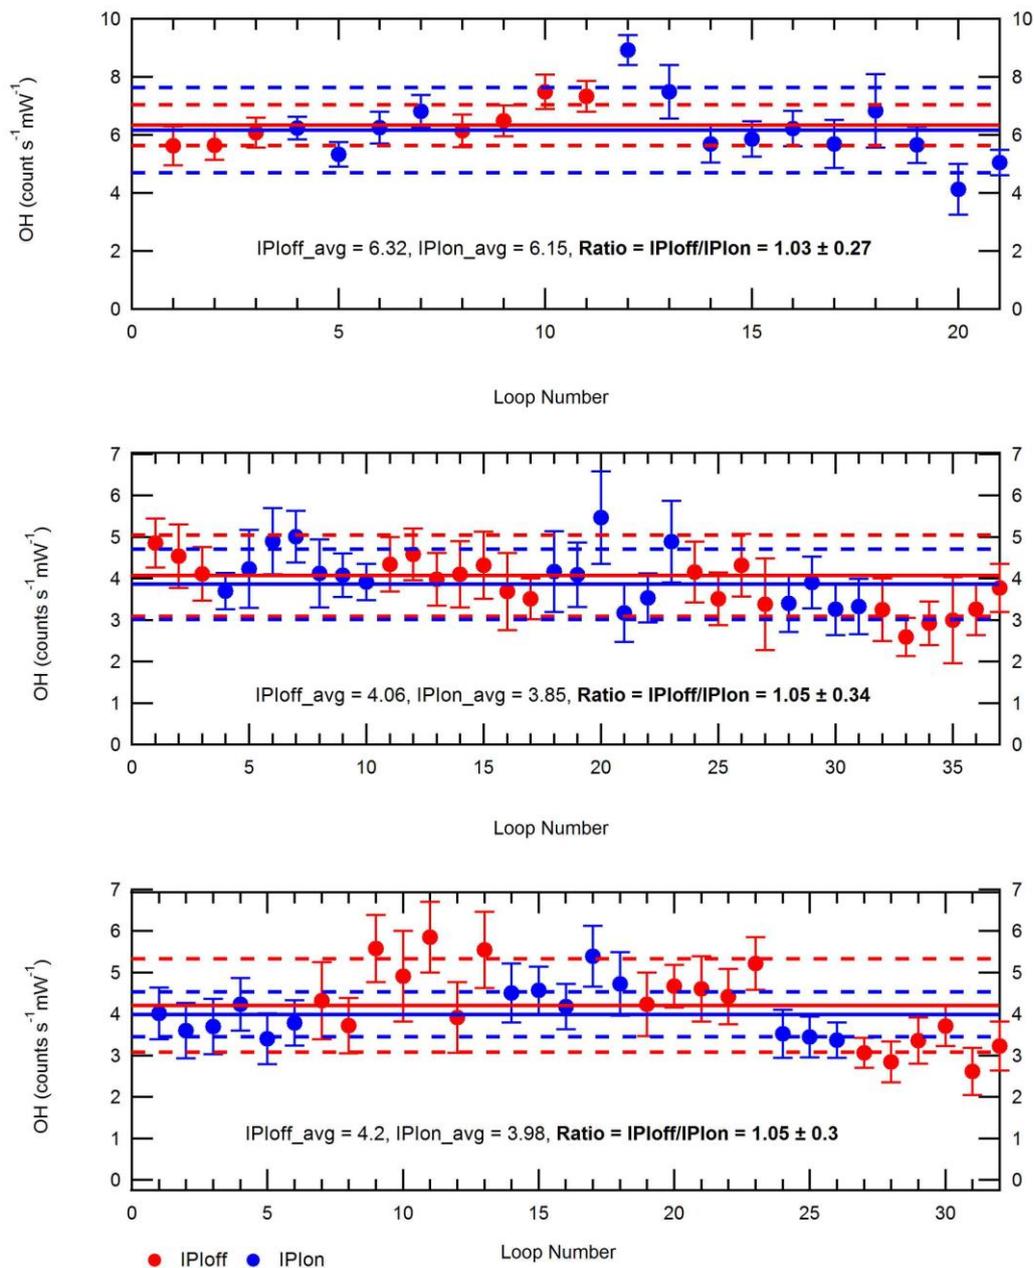

**Figure 3.** Testing of OH losses in the IPI system. Each panel shows repeat measurements of OH signals ( $\pm 2\sigma$ ) over the course of one day, where high OH concentrations were generated using a 184.9 nm Hg lamp placed near the instrument inlet. Blue and red markers denote individual measurements (one measurement “loop”, i.e., one wavelength online–offline cycle) performed with (“IPIon”) and without (“IPIoff”) the IPI system, respectively. Solid lines correspond to the average signals for each day, with  $2\sigma$  standard deviations (SD) shown by the dashed lines.

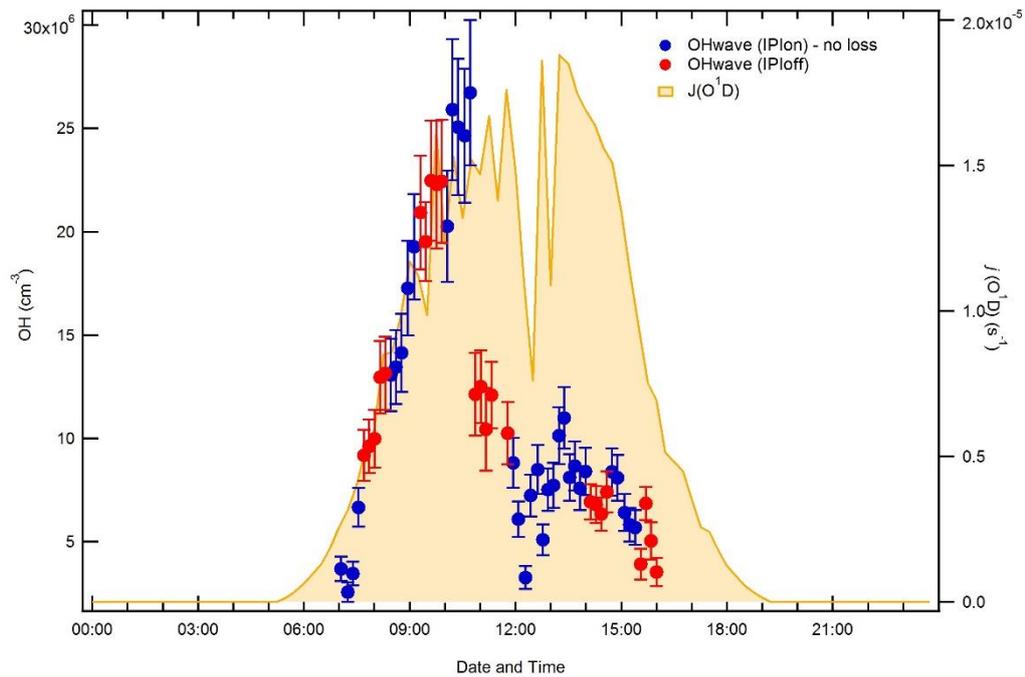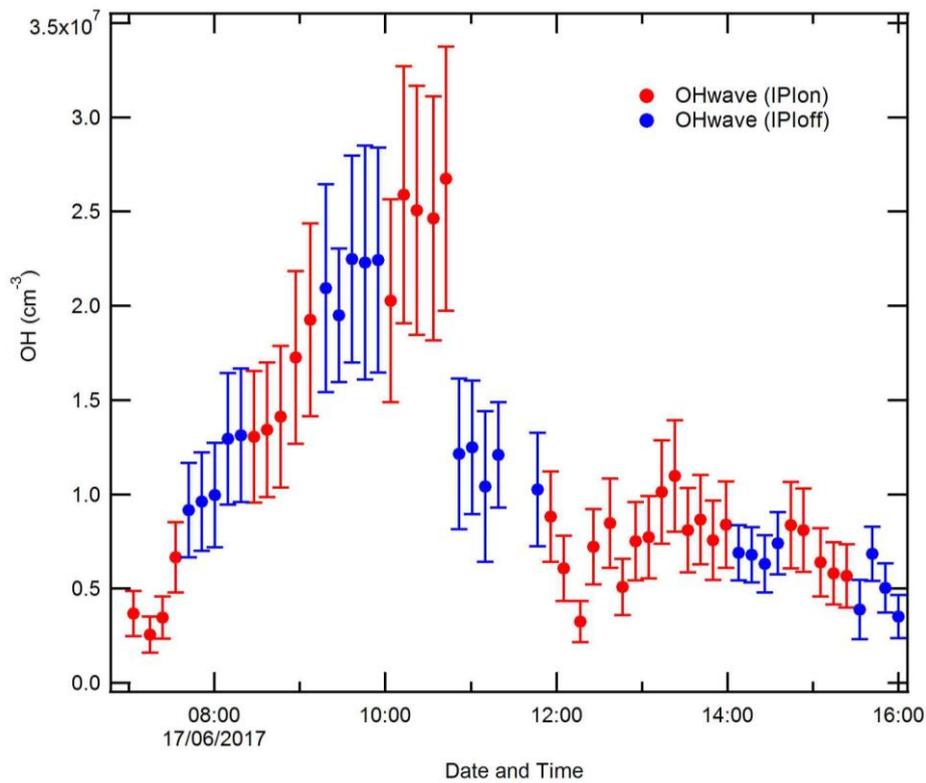


**Figure 4.** Time series of OH concentrations in Beijing on 17<sup>th</sup> June 2017, a period of high OH levels in the summer 2017 AIRPRO (an integrated study of AIR pollution PROCesses in Beijing) campaign. Blue and red markers ( $\pm 2\sigma$ ) denote observations made with and without the IPI system, respectively.

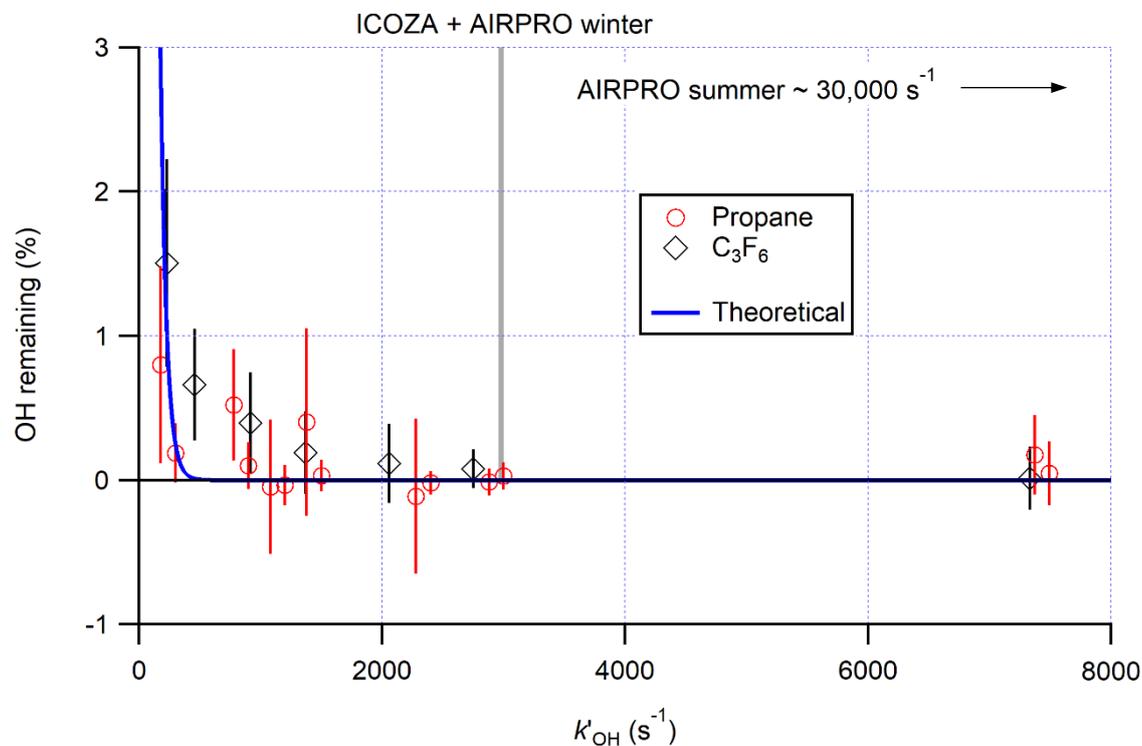




5


**Figure 5.** Proportion of the OH signal remaining (i.e., external OH removal efficiency) after addition of increasing concentrations of propane and perfluoropropene ( $C_3F_6$ ) scavengers to the IPI flow tube, converted to equivalent OH reactivities ( $k'_{OH}$ ) to account for the different rate constants for the reaction of each scavenger with OH. Error bars denote the  $2\sigma$  SD of repeat experiments. The blue curve corresponds to the theoretical scavenging efficiency assuming perfect mixing, using the estimated residence time,  $\tau \sim 20$  ms. The propane OH reactivity used for the ICOZA (Integrated Chemistry of OZone in the Atmosphere) and AIRPRO winter campaigns is given, but that used for AIRPRO summer is off-scale.

10

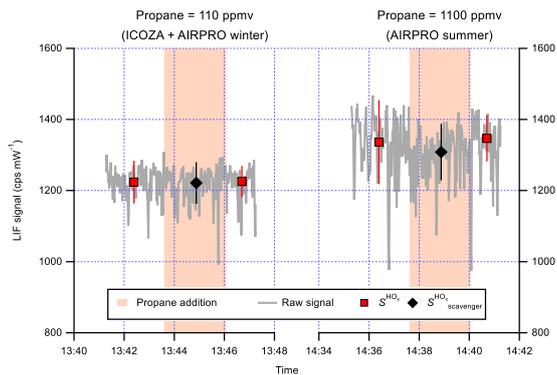





5 **Figure 6.** Time series of the LIF signal during internal OH removal experiments. The raw 1 s data are given by the grey line. NO was continuously added to the FAGE cell during these experiments, (to form OH internally), and points where propane was added to the IPI flow tube are indicated by the orange shaded panels, with the corresponding signal averages ( $\pm 1\sigma$ ) shown as markers (see text for details). The first experiment (left-hand side) corresponds to the propane mixing ratio used for ICOZA, while the second (right-hand side) corresponds to that used for AIRPRO. The results of the internal OH removal experiments are summarised in Table 2.

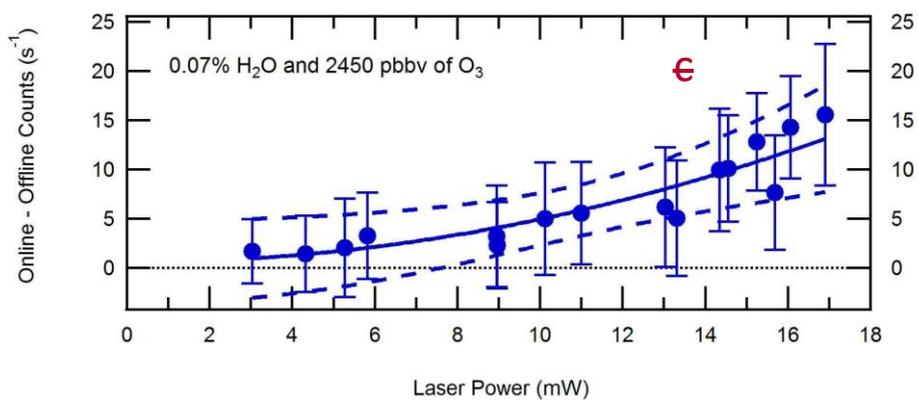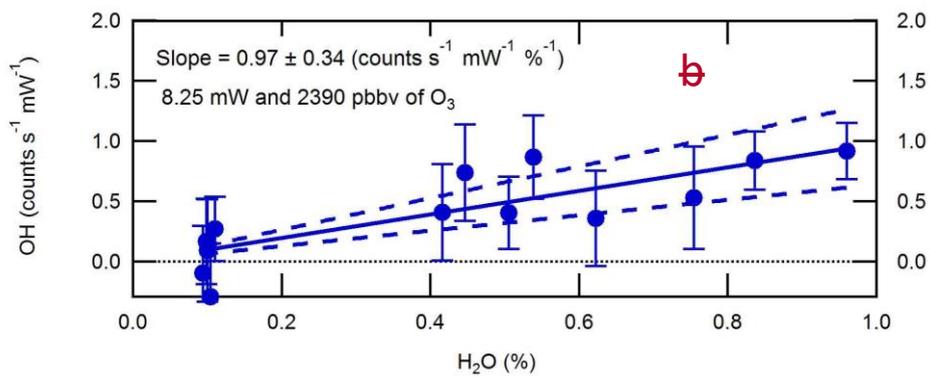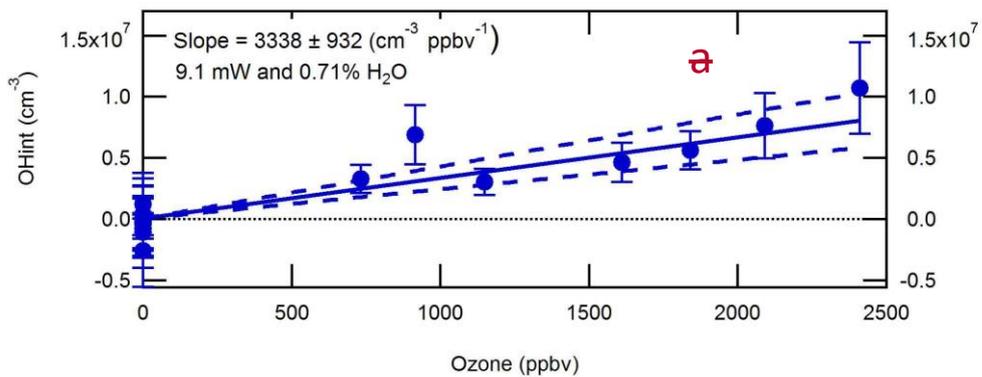


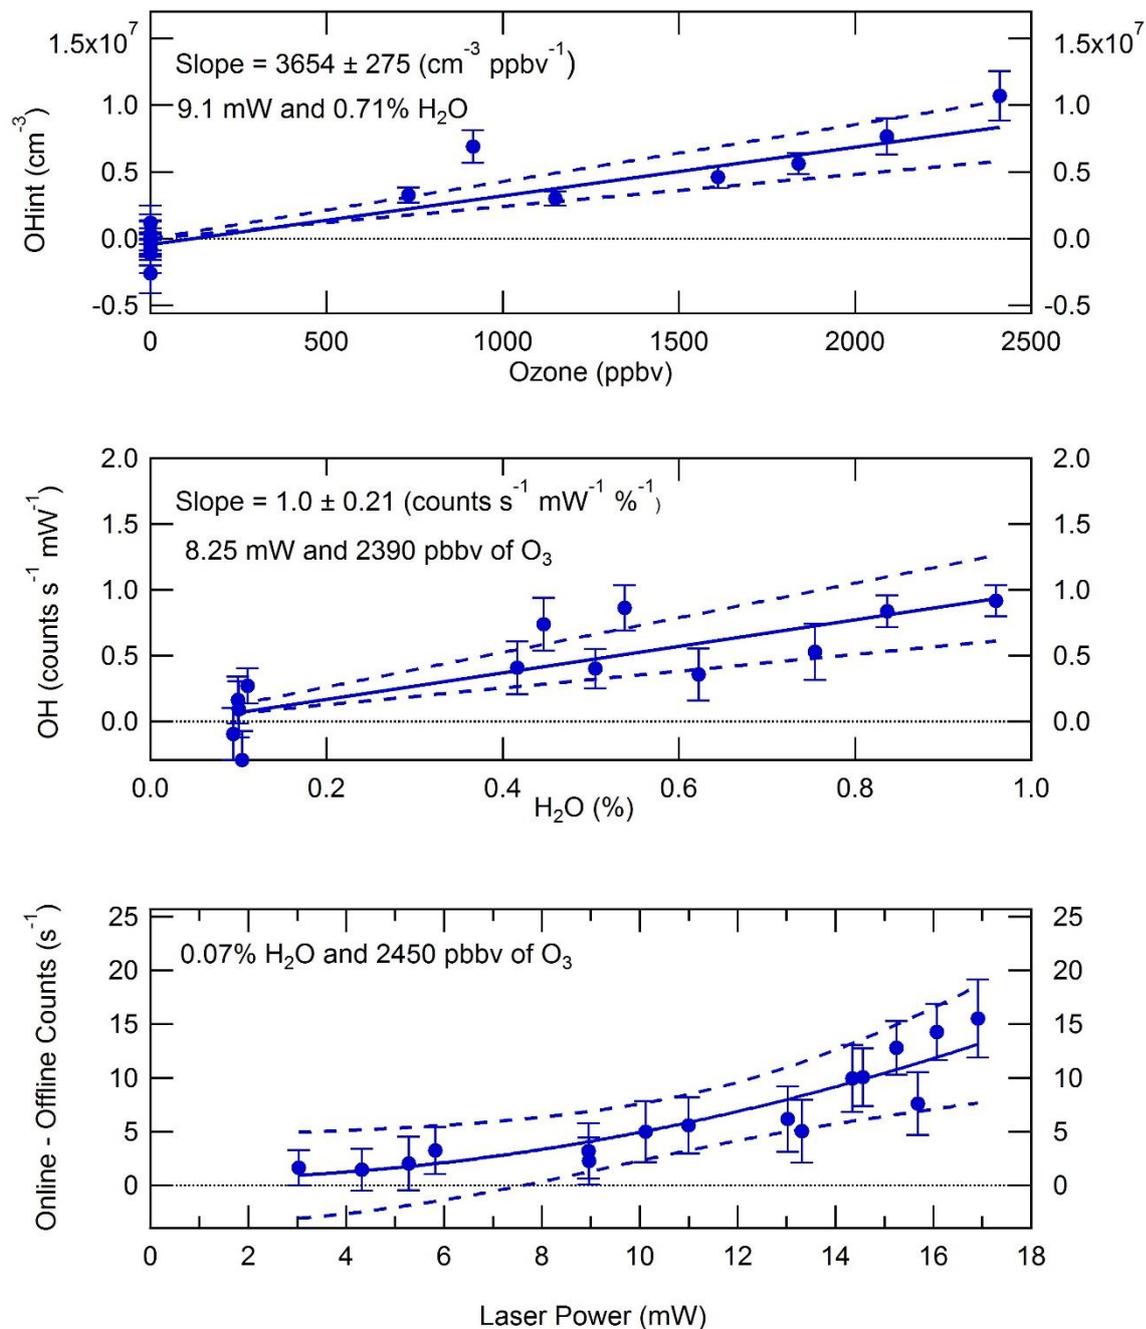


**Figure 7.** OH interference ( $\pm 2\sigma$ ) from O<sub>3</sub> + H<sub>2</sub>O as a function of (a) O<sub>3</sub>, (b) H<sub>2</sub>O, and (c) laser power. The interference signal is linear in O<sub>3</sub> and H<sub>2</sub>O mixing ratios and quadratic in laser power, confirming the two-photon nature of the process. Normalising the slope in panel (a) to O<sub>3</sub> = 1 ppbv, H<sub>2</sub>O = 1%, and laser power = 1 mW yields an OH interference equivalent to a concentration of  $520 \pm 140565 \pm 42$  molecule cm<sup>-3</sup>.

5

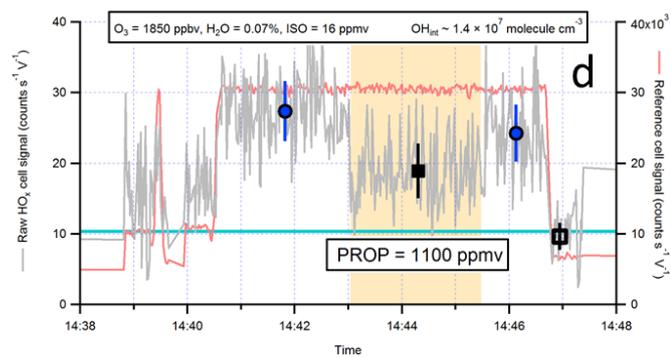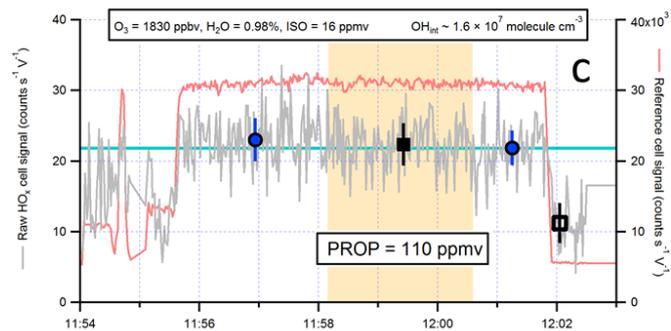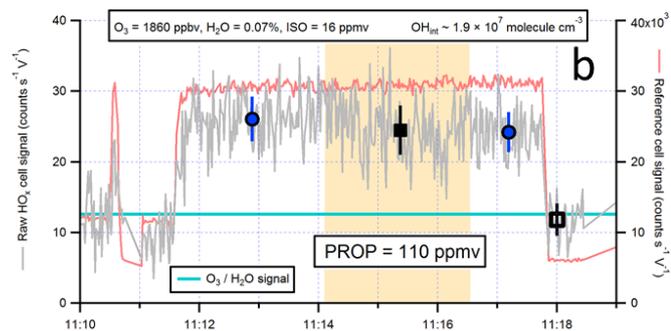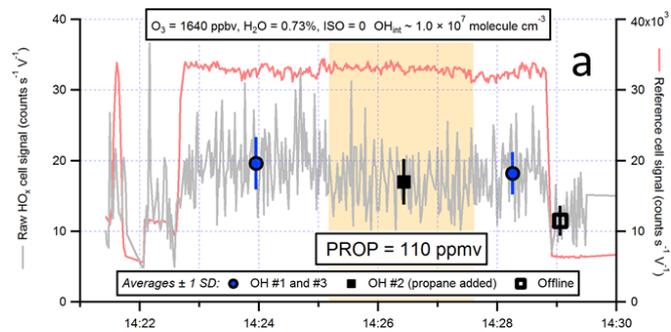


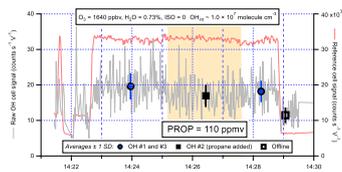


a

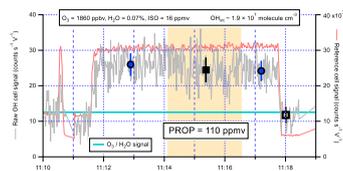

b

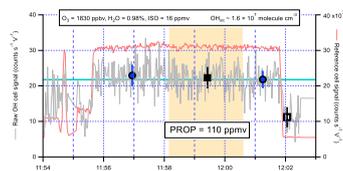



c

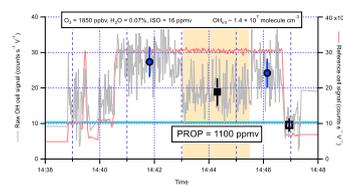


d

**Figure 8.** Isoprene (ISO) ozonolysis interference tests: (a) O<sub>3</sub>/H<sub>2</sub>O only, (b) O<sub>3</sub> and ISO under dry conditions, (c) O<sub>3</sub> and isoprene with H<sub>2</sub>O added, and (d) O<sub>3</sub> and isoprene under dry conditions, but with a higher concentration of propane (PROP) to remove any steady-state generated OH. Shaded areas are periods of propane addition, and the light blue lines correspond to the calculated signals from O<sub>3</sub> + H<sub>2</sub>O only (for

experiments with isoprene present). The interference signals (“OH #2” – “offline”) were used to derive equivalent OH concentrations ( $\text{OH}_{\text{int}}$ ), which are on the order of  $\sim 1\text{--}2 \times 10^7$  molecule  $\text{cm}^{-3}$ . These experiments are summarised in Table 3. See text for further details.

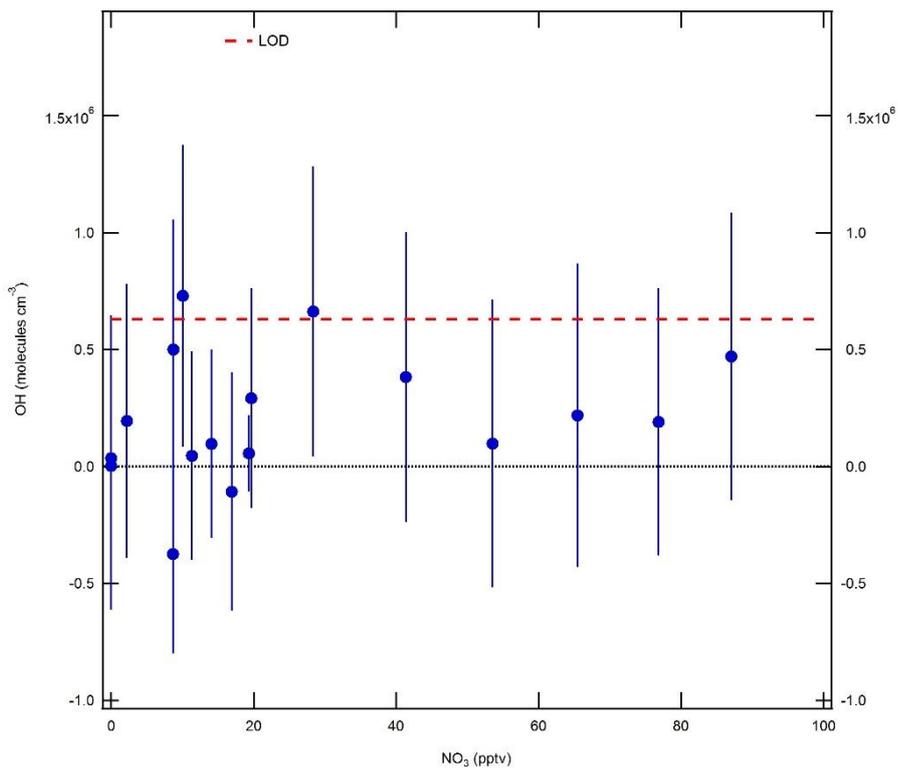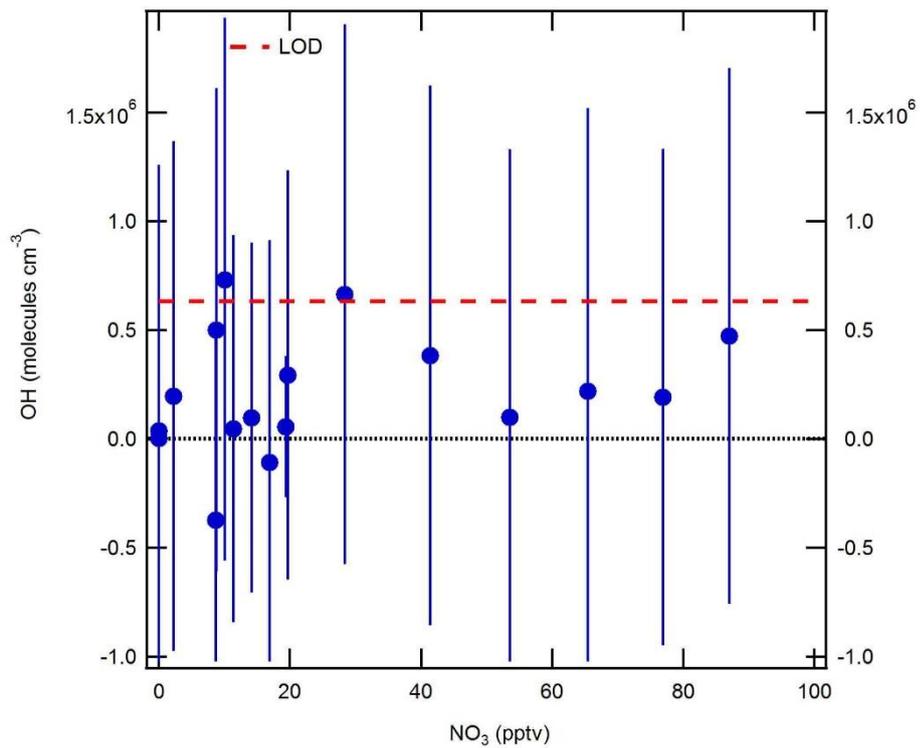


**Figure 9.** Equivalent OH concentrations ( $\pm 2\sigma$ ) measured during  $\text{NO}_3$  radical interference tests.  $\text{NO}_3$  concentrations were calculated using a box model and OH interference signals were corrected for the interference from  $\text{O}_3 + \text{H}_2\text{O}$ . The OH limit of detection (LOD,  $6.3 \times 10^5$  molecule  $\text{cm}^{-3}$ , SNR = 2) is denoted by the red dashed line.

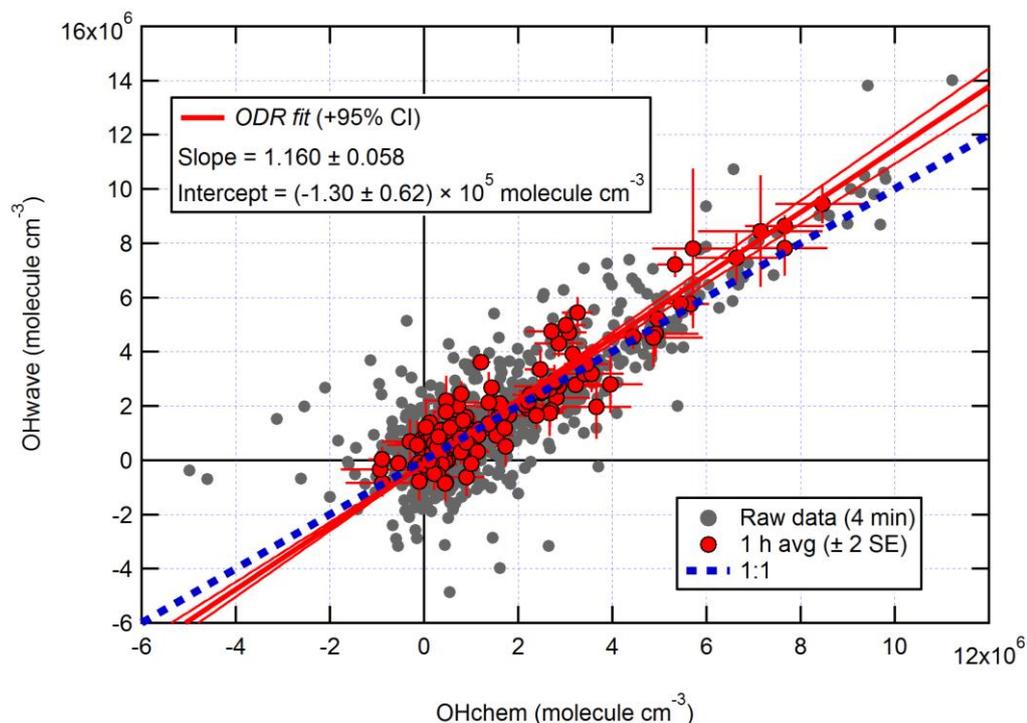

5


**Figure 10.** Overall intercomparison of OHwave and OHchem observations from the ICOZA campaign. Grey markers represent raw data (4 min), with 1 h averages ( $\pm 2$  standard errors (SE)) in red. The thick red line is the orthogonal distance regression (ODR) fit to the hourly data, with its 95% confidence interval (CI) bands given by the thin red lines; fit errors given at the  $2\sigma$  level. For comparison, 1:1 agreement is denoted by the blue dashed line. OHwave data were corrected for the known interference from  $\text{O}_3 + \text{H}_2\text{O}$ .

10

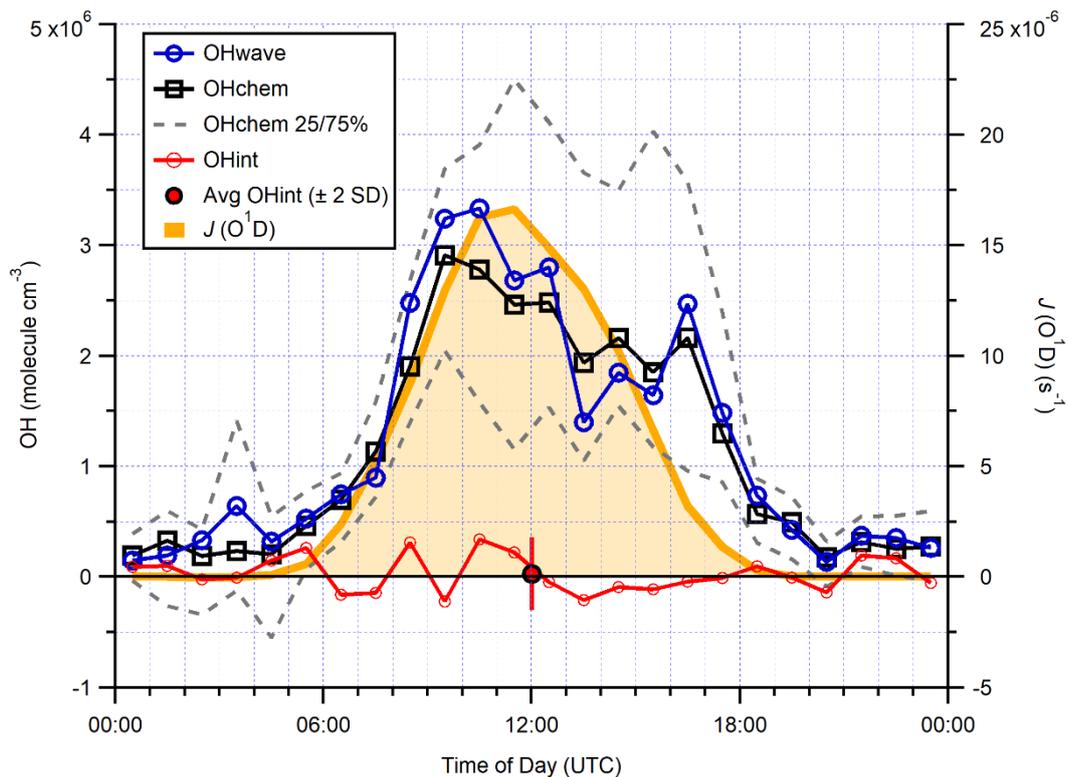


**Figure 11.** Hourly median diurnal profiles of OHwave, OHchem, and  $J(O^1D)$  (right axis) from the ICOZA campaign. Also shown (red line and markers) is the hourly median diurnal profile of OHint (= OHwave – OHchem), calculated from individual 4 min data points; the single red marker corresponds to the average ( $\pm 2\sigma$ ) of this trace. The variability (interquartile range, IQR) in OHchem measurements is denoted by the grey dashed lines, not shown for others for clarity. OHwave data were corrected for the known interference from  $O_3 + H_2O$ .

5

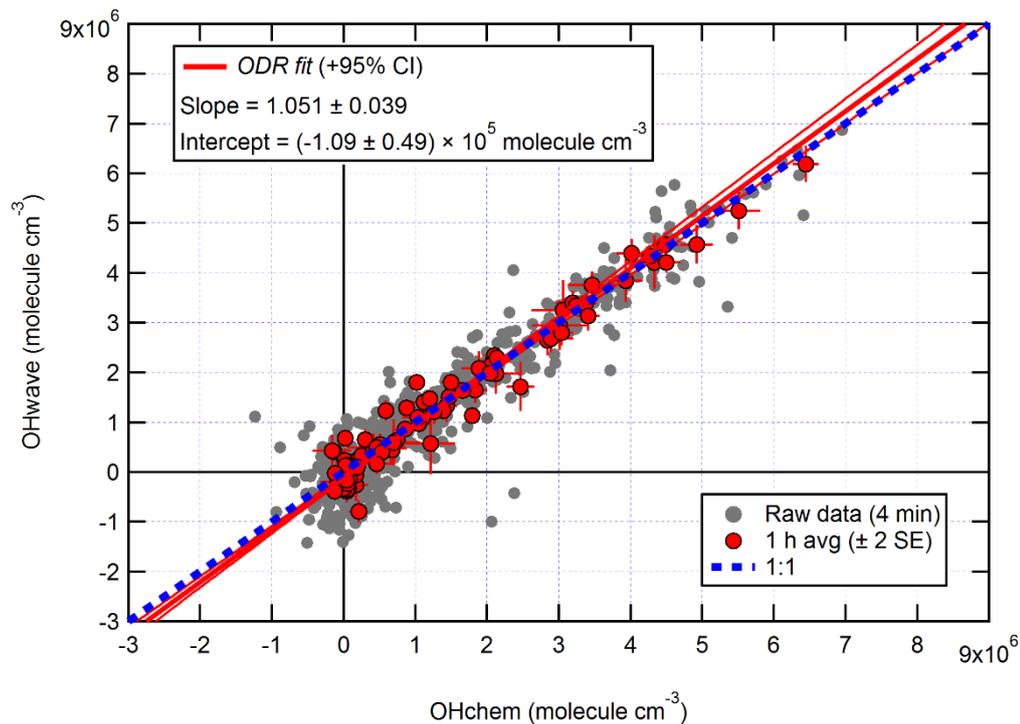


**Figure 12.** Overall intercomparison of OHwave and OHchem observations from the winter 2016 AIRPRO campaign. Grey markers represent raw data (4 min), with 1 h averages ( $\pm 2 \text{ SE}$ ) in red. The thick red line is the ODR fit to the hourly data, with its 95% CI bands given by the thin red lines; fit errors given at the  $2\sigma$  level. For comparison, 1:1 agreement is denoted by the blue dashed line. OHwave data were corrected for the known interference from  $\text{O}_3 + \text{H}_2\text{O}$ .

5

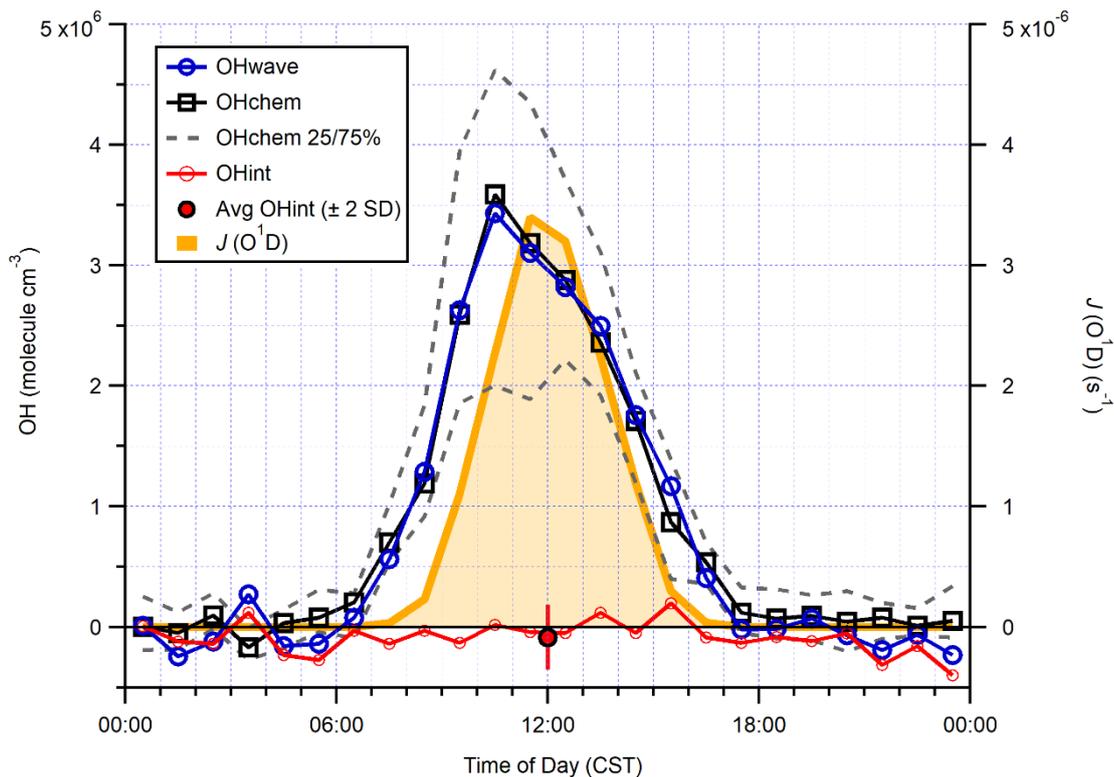


**Figure 13.** Hourly median diurnal profiles of OHwave, OHchem, and  $J(O^1D)$  (right axis) from the winter 2016 AIRPRO campaign. Also shown (red line and markers) is the hourly median diurnal profile of OHint, calculated from individual 4 min data points; the single red marker corresponds to the average ( $\pm 2\sigma$ ) of this trace. The variability (IQR) in OHchem measurements is denoted by the grey dashed lines, not shown for others for clarity. OHwave data were corrected for the known interference from  $O_3 + H_2O$ .

5

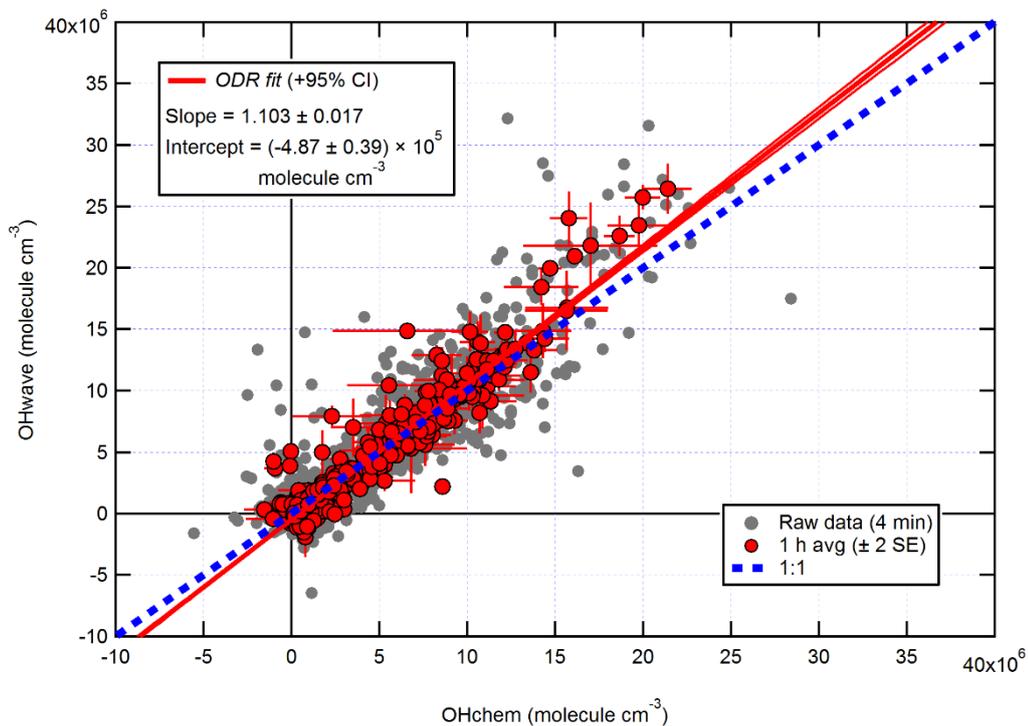


**Figure 14.** Overall intercomparison of OHwave and OHchem observations from the summer 2017 AIRPRO campaign. Grey markers represent raw data (4 min), with 1 h averages ( $\pm 2$  SE) in red. The thick red line is the ODR fit to the hourly data, with its 95% CI bands given by the thin red lines; fit errors given at the  $2\sigma$  level. For comparison, 1:1 agreement is denoted by the blue dashed line. OHwave data were corrected for the known interference from  $\text{O}_3 + \text{H}_2\text{O}$ .

5

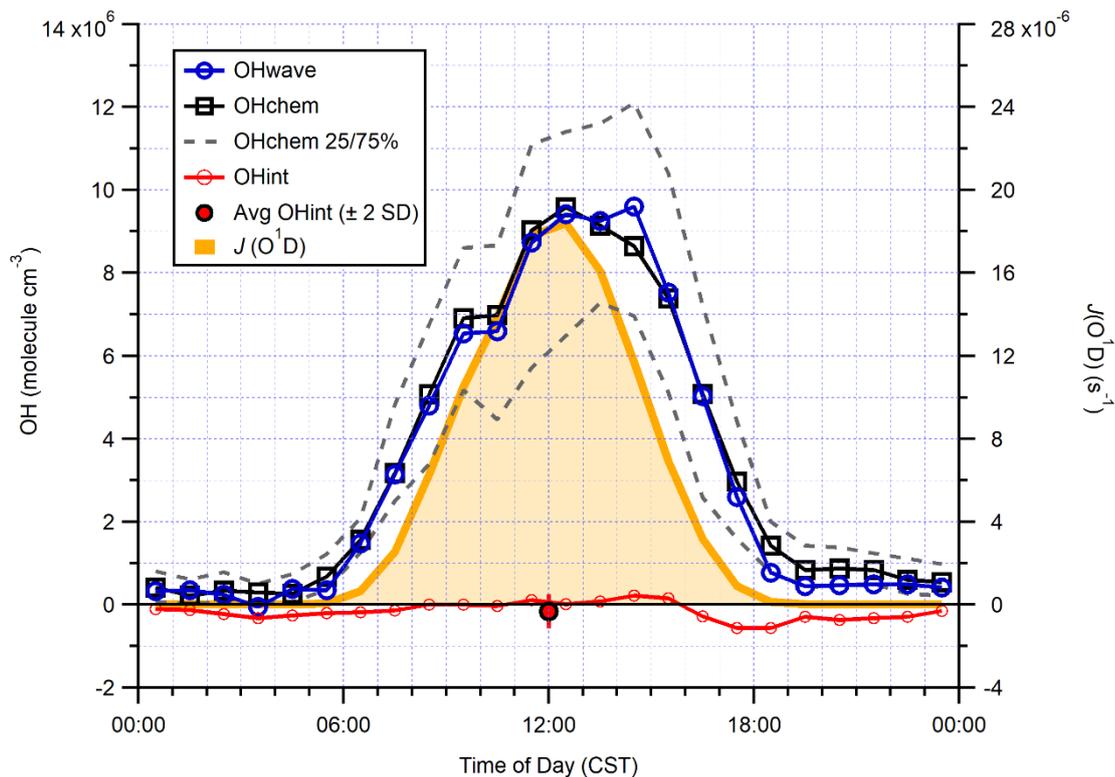

**Figure 15.** Hourly median diurnal profiles of OHwave, OHchem, and  $J(O^1D)$  (right axis) from the summer 2017 AIRPRO campaign. Also shown (red line and markers) is the hourly median diurnal profile of OHint, calculated from individual 4 min data points; the single red marker corresponds to the average ( $\pm 2\sigma$ ) of this trace. The variability (IQR) in OHchem measurements is denoted by the grey dashed lines, not shown for others for clarity. OHwave data were corrected for the known interference from  $O_3 + H_2O$ .

5

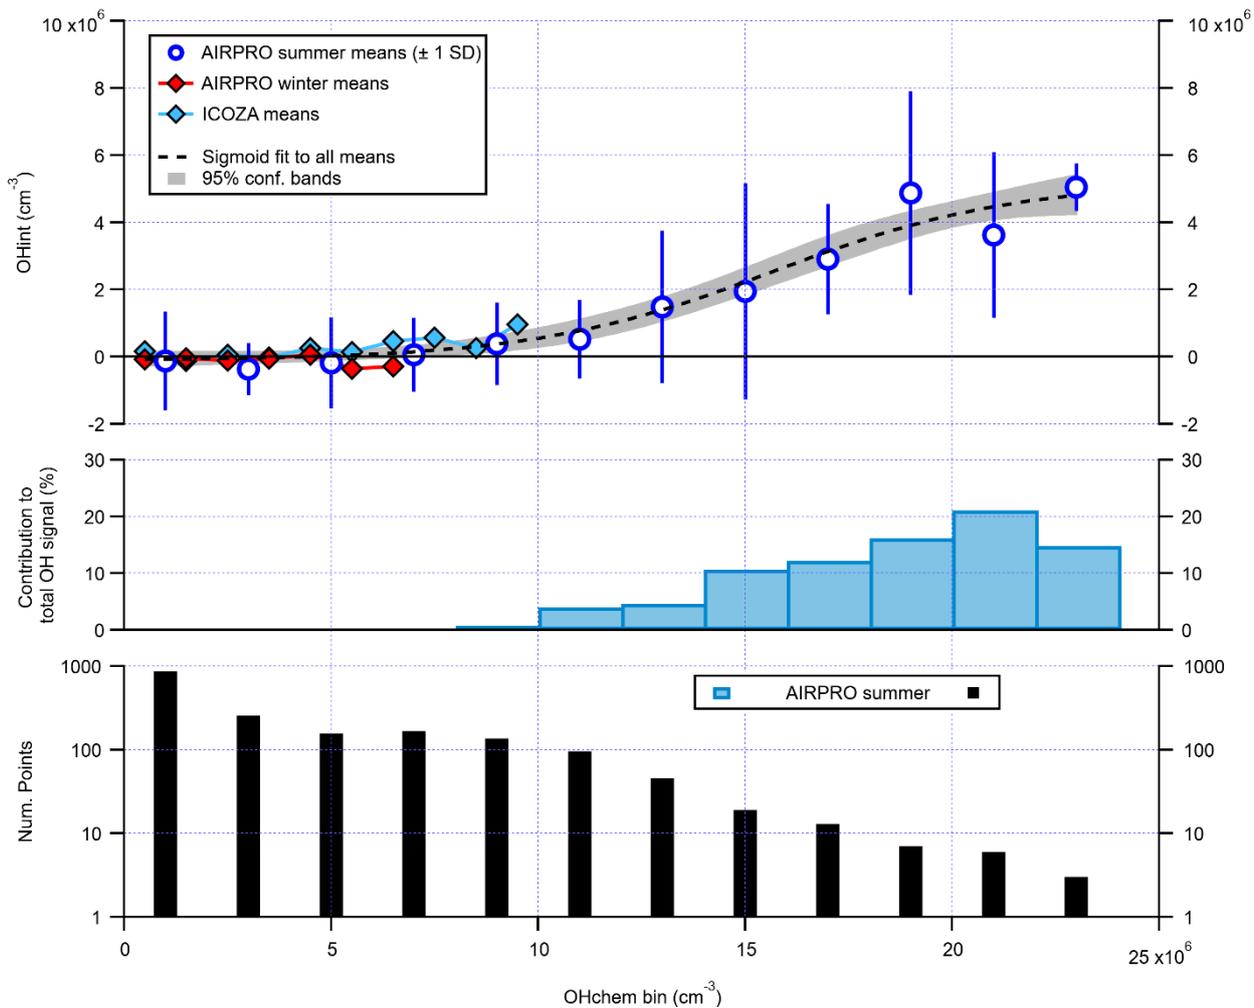

**Figure 16.** Relationship between OHint and OHchem using binned data. The error bars for AIRPRO summer (upper panel, blue markers) denote 1 SD, not shown for AIRPRO winter and ICOZA for clarity. The black dashed line corresponds to a sigmoid fit used to guide the eye only. The contribution of interferences to the total OHwave signal ( $= \text{OHint}/\text{OHwave} \times 100\%$ ) for the AIRPRO summer campaign is shown in the middle panel, with the number of points in each bin shown in the lower panel. All OHint data used here have been corrected for the known interference from  $\text{O}_3 + \text{H}_2\text{O}$ .

5