

Coupling a gas chromatograph simultaneously to a flame ionization detector and chemical ionization mass spectrometer for isomer-resolved measurements of particle-phase organic compounds

Chenyang Bi¹, Jordan E. Krechmer², Graham O. Frazier¹, Wen Xu², Andrew T. Lambe², Megan S. Claflin², Brian M. Lerner², John T. Jayne², Douglas R. Worsnop², Manjula R. Canagaratna², Gabriel Isaacman-VanWertz¹

¹Department of Civil and Environmental Engineering, Virginia Tech, Blacksburg, Virginia, 24060, USA

²Aerodyne Research Inc, Billerica, Massachusetts, 01821, USA

Correspondence to: Gabriel Isaacman-VanWertz (ivw@vt.edu)

Supporting Information

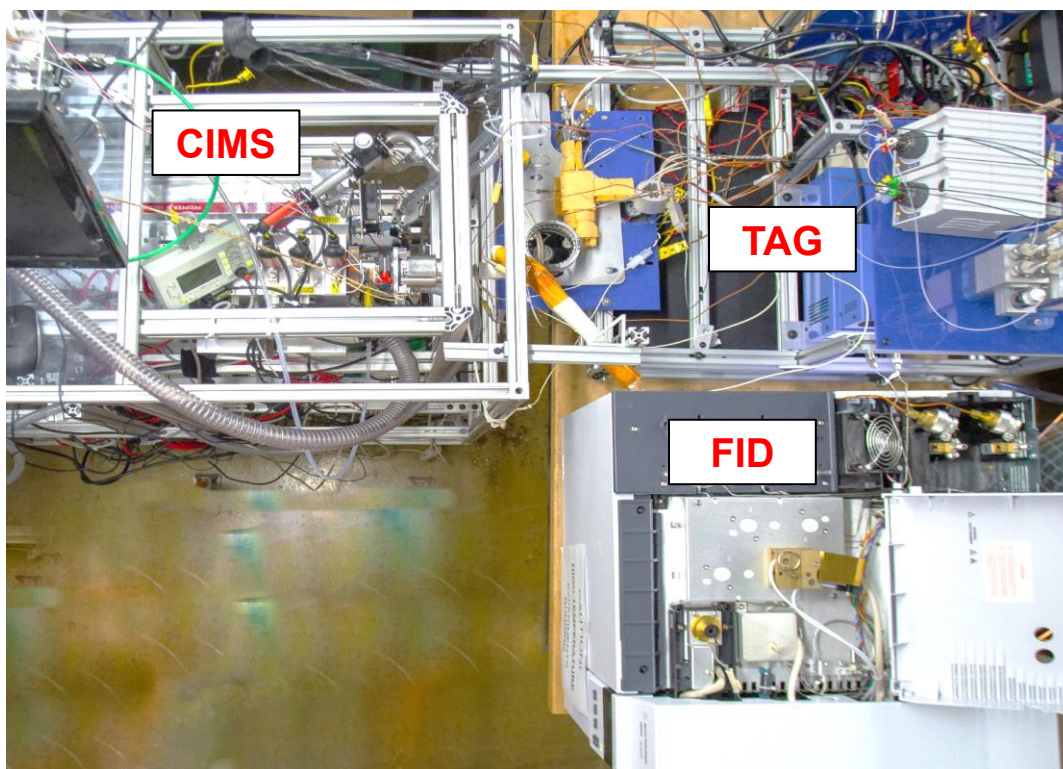


Figure S1. Plan view of the TAG-CIMS/FID

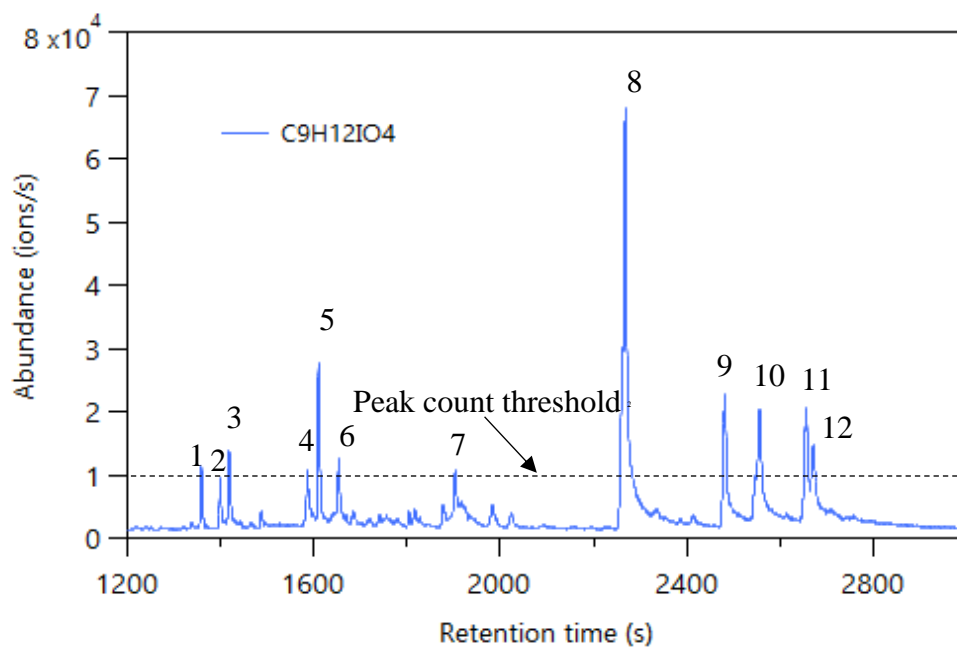


Figure S2. Single ion chromatograph of C₉H₁₂IO₄. Peaks marked with numbers are those having abundance higher than the peak count threshold.