

Dear Dr. Joanna Joiner and Dr. Thomas F. Hanisco,

We sincerely thank you and both reviewers for reviewing our manuscript and valuable suggestions. We have revised the manuscript following suggestions from the reviewers. Our detailed responses to both reviewers are included in two separate documents, also attached in the following pages. The changes in the manuscript are shown with track changes in the marked-up version of the manuscript, attached in the end of this file. Furthermore, we revised all the Figures according to the reviewers' suggestions.

I hereby declare that the revision of this paper was checked by all coauthors. We hope that our revision and responses will satisfy you and the reviewers, and that the manuscript is now acceptable for a publication in AMT.

Yours sincerely,

Shujiro Komiya, Ph.D. (First author, Corresponding author)

Postdoctoral Researcher

Max Planck Institute for Biogeochemistry, Jena, Germany

(e-mail: [skomiya@bgc-jena.mpg.de](mailto:skomiya@bgc-jena.mpg.de) )

## Response to Reviewer #1

Please note: the original reviewer's comments are printed in black, while our response is printed in orange.

Review of "Characterising water vapour concentration dependence of commercial cavity ring-down spectrometers for continuous onsite atmospheric water vapour isotope measurements in the tropics" Komiya et al. AMT

Cavity ring-down spectrometers have been increasingly used in water cycle dynamics studies that employ stable water isotopes as tracers for moist processes in the atmosphere and at the land-atmosphere interface. This paper presents an interesting evaluation of the water vapour mixing ratio dependency of cavity ring-down laser spectrometers focusing on the high specific humidity range that is encountered in tropical regions such as the Amazon.

In general, I found this paper interesting and mostly well written, with some instances, where it was more difficult to follow in particular in Section 2.3 about the calibration strategy of the water vapour mixing ratio dependence as well as the results part. I very much liked the precise description of the self-made calibration unit and find the approach of the authors very nice. Maybe they could add a bit more information on the long-term stability of their calibration system as mentioned in my minor comments below.

I recommend publication of this manuscript after the following three major comments and several minor comments below have been adequately addressed.

**Response:** We sincerely appreciate your support and comments for our study. We have revised our manuscript following your comments and suggestions. The revised parts of the manuscript are shown with track changes in the marked-up version. We also revised all the Figures.

### Major comment:

- 1) The description of the calibration strategy in Section 2.3, especially with respect to Figures 2 and 3 was very difficult to follow. It would help if Figure 3 had panel numbers to which the captions could refer to. In general the figure captions could be improved to help the reader understand the Figures. Also the text should guide the reader better in understanding Figs. 2 and 3.

**Response:** We revised the Figs. 2 and 3, and also the captions. Following the revised Figs. 2 and 3, we revised section 2.3 (see pp. 8-9, Figure 2; pp. 10-11, Figure 3; pp. 5-6, section 2.3 in the marked manuscript).

- 2) The results would benefit from a better structure within the sections. In particular, I would find it nice if the general findings valid for both instruments would be presented first and then the details about the L1102 and L2130.

**Response:** Following your suggestions here and in the Minor comments section, we revised the paragraphs in section 3.1 (see pp. 11-12 in the marked manuscript). In addition, we rearranged the paragraphs in section 3.3 (see pp. 14-16 in the marked manuscript), also suggested by the RC2 reviewer's minor comment. Regarding section 3.2, we decided not to rearrange the paragraphs because in our opinion this would impact negatively the narrative flow.

- 3) The final recommendation of the paper to perform weekly or even more regular water vapour mixing ratio calibrations is surprising (e.g. P 16, L1-3), because an overwhelming majority of studies until now found that the water vapour mixing ratio dependencies of cavity ring-down systems from Picarro remain relatively constant in

time and only occasional full water vapour mixing ratio dependency experiments were necessary, mainly for monitoring purposes. I therefore think the authors should discuss their recommendation and finding in this context of the existing literature. How much do you gain in permil uncertainty reduction for d18O and d2H (and maybe dexcess) with performing regular water vapour mixing ratio dependent calibrations compared to just applying a drift correction and a water vapour mixing ratio dependency correction that is constant in time? This is important because a lot of ambient measurement time is lost with the time consuming calibration scheme proposed by the authors.

**Response:** Thank you for your suggestion, with which we agree. Our final recommendation in the original manuscript “to conduct the [H<sub>2</sub>O]-dependence calibration **at 28 h or less interval.**” (see p. 16, LL. 1-3 in the original manuscript) may indeed be too conservative and would not improve significantly the quality of the measurement, while taking away precious measurement time. As you correctly point out, recent studies show that “new CRDS models (e.g., L2130i and L2140i) did not show any significant changes for [H<sub>2</sub>O]-dependence from ~500 to 25,000 ppm over several months up to 2 years.” (see p. 15, LL. 11-13 in the marked manuscript). However, there was to our knowledge no study prior to ours that assessed the [H<sub>2</sub>O]-dependence consistency above 25,000 ppm H<sub>2</sub>O over several months. According to the results of our laboratory experiments, we decided that “one [H<sub>2</sub>O]-dependence calibration per week is sufficient for correcting moisture-biased isotopic accuracy of the CRDS analysers.” (see p. 19, L. 1 in the marked manuscript). Therefore, we discussed this part in section 3.3 in Results and Discussion as follows: “According to the recent studies (Bonne et al., 2019; Weng et al., 2020), new CRDS models (e.g., L2130i and L2140i) did not show any significant changes for [H<sub>2</sub>O]-dependence from ~500 to 25,000 ppm over several months up to 2 years. The consistency of [H<sub>2</sub>O]-dependence may be extended to higher concentrations than 25,000 ppm, but based on our laboratory experiments, we decided to conduct the [H<sub>2</sub>O]-dependence calibration at weekly or less interval with the DI1-2\*2Pairs strategy. After we continuously run the ambient measurement and calibration systems at the ATTO site over several months, we will try to reduce the [H<sub>2</sub>O]-dependence calibration frequency to maximize the ambient sampling period while maintaining high measurement accuracy of both CRDS analysers.” (see p. 15, LL. 11-17 in the previous manuscript). Base on the revised discussion, we also revised the last sentences in section 4: Conclusion (see pp. 18-19 in the previous manuscript).

#### **Minor comments:**

P 1, L 15: “including...” I would slightly rephrase to “which includes the correction of the H<sub>2</sub>O concentration dependence of isotope measurements”

**Response:** We revised the text according to your suggestion (see p. 1, L. 15 in the marked manuscript).

P 1, L16: “past studies have assessed **the** [H<sub>2</sub>O]-dependence...”

**Response:** We revised the text according to your suggestion (see p. 1, L. 16 in the marked manuscript).

P 1, L23: “... two pairs of a two point calibration with four different H<sub>2</sub>O concentration levels” sounds a bit obscure to me in an abstract. I think I see what you mean after having read the paper several times, but, maybe a more explicit formulation would be helpful

**Response:** We revised this sentence as follows: “The best strategy required conducting a two-point calibration with four different H<sub>2</sub>O concentration levels, carried out at the beginning and end of the calibration interval.” (see p. 1, LL. 24-25 in the marked manuscript).

P 1, L29: Overall very clear and nice abstract. I would find it nice to finish it with a less technical and more general sentence on a scientific level. This could be for example that this study shows that measurements in the tropics are in principle possible also at very high humidity levels, which has promising implications for water cycle studies focusing on tropical regions. But maybe the authors have a better idea for such a final zoom out sentence.

**Response:** Agreed. We added a general sentence on a scientific level as follows; “This study shows that the CRDS analysers, appropriately calibrated for [H<sub>2</sub>O]-dependence, allow the detection of natural signals of stable water vapour isotopes at very high humidity levels, which has promising implications for water cycle studies in areas like the central Amazon rainforest and other tropical regions.” (see pp. 1, LL. 30-32 in the marked manuscript).

P 1, L 35: Maybe Dansgaard 1964 and Craig and Gordon 1965 would be good studies to cite here in addition to the more recent review by Galewsky et al. 2016.

**Response:** Agreed - we added the suggested two references (see p. 1, L. 38 in the marked manuscript).

P 1, L36: Here maybe specific modelling studies would be good to cite: Risi et al. 2010, Werner et al. 2011, Pfahl and Wernli 2012 instead of a review paper. I think the statement “has also improved simulations of hydrometeorological fields” could potentially be misunderstood. Isotopes are implemented in different global and regional circulation models to improve our understanding of how stable water isotopes are transported in the atmosphere and affected by phase changes in clouds, below the clouds and how they behave in different situation of surface-atmosphere interactions. Of course, the idea is to learn more about these moist processes through these isotope modelling studies. But, stable water isotopes are implemented as *passive* tracers in these models and do not directly impact other hydrometeorological fields.

**Response:** Following your suggestion, we used the suggested three references, and also revised this sentence as follows: “Incorporating water vapour isotopic information into global and regional circulation models has also improved our understanding of how stable water isotopes are transported in the atmosphere and affected by phase changes in- and below-clouds, and how they behave in different situation of surface-atmosphere interactions (Risi et al., 2010; Werner et al., 2011; Pfahl et al., 2012).” (see p. 1, L. 39 – p. 2, L. 3 in the marked manuscript).

Based on this revision, in the next sentence we also corrected “hydrometeorological cycles” to “the atmospheric hydrological system” (see p. 2, L. 5 in the marked manuscript).

P 2, L6: Maybe here the polar regions, midlatitudes and subtropics/tropics could be mentioned separately. There are many studies based on water vapour isotope measurements available in polar and midlatitude regions, some in the subtropics (e.g. Gonzalez et al. 2016, Bailey et al. 2013) but only very few in the tropics (e.g. Tremoy et al. 2012, Aemisegger et al. 2020). In particular studies over tropical continental regions are rare.

**Response:** According to your suggestion, we revised this sentence as follows: “So far, there are many studies based on field water isotopic measurements available in polar and midlatitude regions, some in the subtropics (e.g., Bailey et al., 2013; Gonzalez et al., 2016) but only very few in the tropics (e.g., Tremoy et al., 2012; Aemisegger et al., 2020). Particularly studies in tropical continental regions, such as the Amazon basin region, are rare.” (see p. 2, LL. 11-15 in the marked manuscript).

P 2, L16: Replace “confirmed” by “showed” because this was not shown before, and remove s in “an older model”.

**Response:** We replaced it with ‘demonstrated’ because this revision more fits here. (see p. 2, L. 25 in the marked manuscript).

P 2, L 26: This statement about the diel cycle comes a bit abruptly after the discussion about older studies of water vapour isotopes in different humidity ranges. Maybe a new paragraph would help and a smoother transition from mainly instrument technical aspects to previous observations in nature.

**Response:** Based on your and RC2 reviewer suggestions, we added ‘in addition’ before this sentence (see p. 2, L. 37 in the marked manuscript). Additionally, we started a new paragraph from “However, H<sub>2</sub>O concentrations within the Amazon...” based on the context (see p. 2, LL. 35-42 in the marked manuscript).

P 2, L 33: ATTO is a new abbreviation to me

**Response:** The abbreviation is mentioned for the first time and explained at p. 2 L. 23 of the original manuscript (and LL. 35-36 on p.2 in the marked version of the revised manuscript).

P 2, L35: Old and new instead of older and newer, the latter would require a “with respect to what” statement

**Response:** According to your suggestion, we revised as follows: “an old (L1102i) and a new CRDS models (L2130i)” (see p. 3, L.4 in the marked manuscript).

In addition, regarding “the latter would require a “with respect to what” statement”, we added “both” before “an old (L1102i) and a new CRDS models (L2130i)” to clearly state it (see p. 3, L. 4 in the marked manuscript).

P 2, L42: “sufficiently detect...” sounds a bit awkward. Maybe something like “based on the uncertainty quantification presented, we discuss whether the CRDS analysers can detect natural signals of ...”.

**Response:** According to your suggestion, we revised the sentence as follows: “Based on the uncertainty quantification presented, we discussed whether the CRDS analysers with our calibration setup can sufficiently detect natural signals of stable water vapour isotopes expected at the ATTO site.” (see p. 3, LL. 11-13 in the marked manuscript).

P 3, L16: To which water vapour mixing ratio level does this dew point correspond?

**Response:** We revised here as follows: “dew point temperature of -32 °C or below (~300 ppm of H<sub>2</sub>O or below)” (see p. 3, L. 37 in the marked manuscript).

P 3, Section 2.1: In general: very nice self-made setup and description of it! I would be curious to see it in operation. A picture of the full setup next to the schematic in Fig. 1 would be great! Also could the authors comment on the long-term stability of their system? Are there any failure-prone parts in this system? E.g. how about the Syringe pump?

**Response:** Thank you for your support. We added two photos showing the main part of the dry air and calibration units (see p. 7, Figs. 1b and 1c in the marked manuscript). Also following the detailed information about the 3-way solenoid valves in Fig. 1c., we revised the solenoid valves' information in Fig. 1a, concisely presented in the previous manuscript. In addition, regarding the long-term stability, we added maintenance information for the syringe-pump and membrane dryer (see p. 3, LL. 26-28 and LL. 33-35 in the marked manuscript).

P 3, L 26: Could you indicate the total flow rate of the CRDS instruments? A recent study has shown that the water vapour mixing ratio dependency is actually depending on the instrument's flow rate (see supplement of Thurnherr et al. 2020)

**Response:** Yes, we added the total flow rate of the two CRDS analysers as follows: "... the suction flow rates of the two CRDS analyzers (~50 mL min<sup>-1</sup> in total)." (see p. 4, L. 8 in the marked manuscript). In addition, Thurnherr et al. (2020) found that L2130i's isotope dependence with humidity dependence occurred by not the high suction flow rate (300 mL min<sup>-1</sup>) but the low suction flow rate (50 mL min<sup>-1</sup>) like our study. So we cited this finding to explain why our L2130i analyzer detected the isotope dependence of  $\delta^2\text{H}$  accuracy in section 3.2 in Results and Discussions as follows: "Additionally, the isotope dependence of  $\delta^2\text{H}$  accuracy may have related to the low suction flow rate of the L2130i (Thurnherr et al., 2020)." (see p. 13, LL. 20-21 in the marked manuscript).

P 3, L35: Could the authors shortly mention how this correction is implemented? Were the two CRDS instruments also connected to a dew point generator at different dew point temperatures to ensure that no bias affects their water vapour concentration?

**Response:** Unfortunately we were not able to connect a dew point generator to the CRDS analysers during the experiment period. So, we used a nonlinear calibration fitting, determined by Winderlich et al., (2010) and recommended for old CRDS models (e.g., G1301 CO<sub>2</sub>/CH<sub>4</sub>/H<sub>2</sub>O analyser) of H<sub>2</sub>O measurement by Rella (2010), in order to correct for H<sub>2</sub>O concentration by the old CRDS model (e.g., L1102i). Therefore, we revised this sentence as follows:

"Since H<sub>2</sub>O concentration values measured by old CRDS models (e.g., L1102i) are biased due to the self-broadening effect of water vapour (Winderlich et al., 2010), H<sub>2</sub>O concentration measuring by the L1102i were corrected by a nonlinear calibration fitting, determined by Winderlich et al., (2010) and recommended for old CRDS models (e.g., G1301 CO<sub>2</sub>/CH<sub>4</sub>/H<sub>2</sub>O analyser) by Rella (2010)." (see p. 4, LL. 15-18 in the marked manuscript).

P 4, L13: Also use humidity or water vapour mixing ratio level and not "moisture level"

**Response:** We replaced "moisture level" with "concentration level" (see p. 4, L. 35 in the marked manuscript), and revised the corresponding parts throughout the manuscript.

P7: I had difficulties to understand Fig. 2. Is this actually a Figure or a Table? Maybe the caption could be a bit more detailed. And why does the DI1 strategy contain Cali. ID 1 to 3 and not only 1 and 3? Same for DI2, why is it not 2 & 4? And why do I see Cali IDs such as 43-47 at the 14h calibration interval. So in short, I think, I get the general idea, but I was confused by some details. The text and Figure/Table could also speak a bit more together to help the reader here.

**Response:** Since we combined the top diagram with a table at the bottom, we assigned those as a Figure. To make it clearer, we added a figure letter to each part (see p. 8, Figs. 2a and 2b in the marked manuscript).

We are sorry that the Cali. ID information in the DI1, DI2 and DI1-DI2\*1Pair strategies in the bottom table was misleading to readers, so we revised the corresponding parts (see p. 8, Fig. 2b in the marked manuscript).

P 9, L 20: At these water vapour mixing ratio levels, the instrument is measuring at its uppermost limits. So, I am not sure if the larger variability in H<sub>2</sub>O concentrations should be attributed to the calibration unit or a saturation effect within the cavity. Are the instruments used here optimized factory-wise (e.g. absorption peak scanning strategy) for high water vapour mixing ratio ranges? If yes, then it would be good to mention this in the methods section.

**Response:** Agreed. We revised this sentence as follows: “In addition, the larger variation in H<sub>2</sub>O concentration at 41,000 ppm may have been influenced by instability of the calibration system and a saturation effect inside the cavity measuring H<sub>2</sub>O concentration near the upper limit (50,000 ppm).” (see p. 11, LL. 22-24 in the marked manuscript).

Our CRDS analysers just have a factory standard setting for absorption peak scanning strategy, so we did not mention it in the Material and Methods.

P 9, L24-25: I was confused here: variability in H<sub>2</sub>O concentration higher than what?

**Response:** We revised here as follows: “...even though variability in H<sub>2</sub>O concentration measurement was higher at 29,000 ppm (H<sub>2</sub>O- $\sigma \geq 578.6$  ppm) than at 21,500 ppm (H<sub>2</sub>O- $\sigma \leq 253.5$  ppm).” (see p. 11, LL. 36-37 in the marked manuscript).

P 9, L27: The higher d<sup>18</sup>O and d<sup>2</sup>H precision at higher H<sub>2</sub>O levels is a bit surprising. I would have expected a saturation effect at some point.

**Response:** Indeed, we also did not expect it at first, yet this is what we have observed in our experiment (see p. 11, L. 34 – p. 12, L. 2 in the marked manuscript). Future work may provide an explanation.

P 9, L34: This is what I would have expected, maybe a slight rearrangement of paragraphs would be good here first discussion statements that are valid for both instruments and then discussing the individual instrument versions.

**Response:** Following your suggestion, we rearranged the second and last paragraphs in section 3.1 (see p. 11, L. 27 – p. 12, L. 2 in the marked manuscript). We did not rearrange the first paragraph because the first paragraph does not describe anything about Table 1. In the second paragraph, based on Table 1’s results we described the general findings for both analysers, and then discussed more detailed parts in the third paragraph.

P 9, L37: I would make it clear that you mean the absorption peak fitting algorithm and you could add the “absorption peak scanning strategy”.

**Response:** Our CRDS analysers just have a factory standard setting for absorption peak scanning strategy, so we did not mention it here.

P 11, L 9: Replace “checked” by “tested”

**Response:** I revised here (see p. 13, L. 36 in the marked manuscript).

P 11, L 12: Replace “confirmed” by “showed”

**Response:** I revised here according to your suggestion (see p. 13, L. 38 in the marked manuscript).

P 12, L 6: Aren't the lower RMSE values for the L2130 compared to the L1102 mainly due to the higher precision of the L2130?

**Response:** Yes, the lower RMSE values for the L2130i is mainly due to the higher precision of the L2130i compared to the L1102i. We revised this sentence as follows: “The lower RMSE values of the L2130i analyser are mainly due to the higher precision of the L2130i analyser compared to the L1102i analyser.” (see p. 14, LL. 16-18 in the marked manuscript).

P 15, L 9: And in other tropical areas to make it more general?

**Response:** According to your suggestion, we replaced here as follows: “in the Amazon rainforest and other tropical areas” (see p. 18, L. 10 in the marked manuscript).

P 15, L13: Also here I would rather use “water vapour mixing ratio level” instead of moisture (moisture is more general and could also for instance imply liquid water).

**Response:** Here, we replaced “moisture conditions” with “H<sub>2</sub>O concentration levels” (see p. 18, L. 14 in the marked manuscript). In addition, in the next sentence we replaced “moisture content” with “H<sub>2</sub>O concentration” (see p. 18, LL. 15-16 in the marked manuscript).



## References

- Aemisegger, F., Vogel, R., Graf, P., Dahinden, F., Villiger, L., Jansen, F., Bony, S., Stevens, B., and Wernli, H.: How Rossby wave breaking modulates the water cycle in the North Atlantic trade wind region, *Weather Clim. Dynam. Discuss.*, <https://doi.org/10.5194/wcd-2020-51>, in review, 2020.
- Craig, H. and Gordon, L. I.: Deuterium and oxygen 18 variations in the ocean and the marine atmosphere, 1965.
- Bailey, A., Toohey, D., and Noone, D.: Characterizing moisture exchange between the Hawaiian convective boundary layer and free troposphere using stable isotopes in water, *J. Geophys. Res. Atmos.*, 118, 8208–8221, doi:10.1002/jgrd.50639, 2013
- Dansgaard, W.: Stable isotopes in precipitation. *Tellus*, 16: 436-468. <https://doi.org/10.1111/j.2153-3490.1964.tb00181.x>, 1964.
- Galewsky, J., Steen-Larsen, H. C., Field, R. D., Worden, J., Risi, C., and Schneider, M.: Stable isotopes in atmospheric water vapor and applications to the hydrologic cycle, *Rev. Geophys.*, 54, 809–865, doi:10.1002/2015RG000512, 2016.
- González, Y., Schneider, M., Dyroff, C., Rodríguez, S., Christner, E., García, O. E., Cuevas, E., Bustos, J. J., Ramos, R., Guirado-Fuentes, C., Barthlott, S., Wiegele, A., and Sepúlveda, E.: Detecting moisture transport pathways to the subtropical North Atlantic free troposphere using paired H<sub>2</sub>O- $\delta$ D in situ measurements, *Atmos. Chem. Phys.*, 16, 4251–4269, <https://doi.org/10.5194/acp-16-4251-2016>, 2016.
- Pfahl, S., Wernli, H., and Yoshimura, K.: The isotopic composition of precipitation from a winter storm – a case study with the limited-area model COSMOiso, *Atmos. Chem. Phys.*, 12, 1629–1648, <https://doi.org/10.5194/acp-12-1629-2012>, 2012.
- Risi, C., Bony, S., Vimeux, F., and Jouzel, J.: Water stable isotopes in the LMDZ4 general circulation model: Model evaluation for present day and past climates and applications to climatic interpretation of tropical isotopic records, *J. Geophys. Res.*, 115, D12118, doi:10.1029/2009JD013255, 2010.
- Tremoy, G., Vimeux, F., Mayaki, S., Souley, I., Cattani, O., Risi, C., Favreau, G., and Oi, M.: A 1-year long  $\delta^{18}\text{O}$  record of water vapor in Niamey (Niger) reveals insightful atmospheric processes at different timescales, *Geophys. Res. Lett.*, 39, L08805, doi:10.1029/2012GL051298, 2012.
- Thurnherr, I., Kozachek, A., Graf, P., Weng, Y., Bolshiyarov, D., Landwehr, S., Pfahl, S., Schmale, J., Sodemann, H., Steen-Larsen, H. C., Toffoli, A., Wernli, H., and Aemisegger, F.: Meridional and vertical variations of the water vapour isotopic composition in the marine boundary layer over the Atlantic and Southern Ocean, *Atmos. Chem. Phys.*, 20, 5811–5835, <https://doi.org/10.5194/acp-20-5811-2020>, 2020.
- Werner, M., Langebroek, P. M., Carlsen, T., Herold, M., and Lohmann, G.: Stable water isotopes in the ECHAM5 general circulation model: Toward high-resolution isotope modeling on a global scale, *J. Geophys. Res.*, 116, D15109, doi:10.1029/2011JD015681, 2011.

## Response to Reviewer #2

Please note: the original reviewer's comments are printed in black, while our response is printed in orange.

### Review of 'Characterising water vapour concentration dependence of commercial cavity ring-down spectrometers for continuous onsite atmospheric water vapour isotope measurements in the tropics' by Komiya *et al.*, submitted to AMT

This manuscript presents a characterisation of concentration dependence of 2 commercial cavity ring-down spectrometers at 4 high water concentration levels between 21500 and 41000 ppm. The authors assessed the calibration results using 4 different calibration strategies, and for each calibration strategy using 5 different fitting functions. The authors concluded with identifying the most appropriate calibration strategy and fitting choice for their two specific instruments.

The relative new aspects of the study are the focus of the calibration at high water concentration levels (21500 to 41000 ppm) and the assessment of different calibration strategies (including fitting choices). The manuscript is relatively well written. Below I have detailed 2 major points, and some minor issues with suggestions.

**Response:** Thank you for your support and suggestions. We have revised our manuscript following your comments and suggestions. The revised parts are shown with track changes in the marked-up version of the manuscript. We also revised all the Figures.

#### Major comments

1. One key aspect of the study is to test the 5 calibration strategies. A general question would be: what motivates the authors to choose *these specific* calibration strategies in the first place? In other words, what is the purpose or hypothesis, advantage, and disadvantage behind each specific strategy? It would be more clear and helpful if the authors could briefly clarify these questions before presenting the methods and results.

**Response:** Regarding “to test the 5 calibration strategies”, actually we tested the 4 calibration strategies. Following your suggestion, we explained why we used the 4 calibration strategies in the first paragraph in section 2.3 as follows: “...The DI1 and DI2 calibration strategies used a single standard water (DI1 or DI2) to correct for [H<sub>2</sub>O]-dependence. In contrast, the DI1-DI2\*1Pair and DI1-2\*2Pairs strategies used the two standard waters (DI1 and DI2) for calibrating [H<sub>2</sub>O]-dependence because we considered that [H<sub>2</sub>O]-dependence might change between the two standard waters according to recent studies (Bonne *et al.*, 2019; Weng *et al.*, 2020). In addition, the DI1-2\*2Pairs strategy used more calibration data than the DI1-DI2\*1Pair strategy to obtain more robust calibration fittings of [H<sub>2</sub>O]-dependence.” (see p. 5, LL. 20-25 in the marked manuscript).

2. The authors have described a custom-built calibration unit. The unit's working principle is similar to the commercially available (since 2013?) Picarro Standards Delivery Module (A0101). What is the specific motivation for the authors to build their own calibration unit? What main differences or advantages do the authors achieve?

**Response:** The Picarro officially guarantees that the operational H<sub>2</sub>O concentration range of A0101 is between 200 and 30,000 ppm, which does not cover our aimed H<sub>2</sub>O concentration over 30,000 ppm. In addition, according to discussion with Picarro's staff, there is no easy way to run A0101 off with the L1102i model. Based on these reasons, we built up the calibration unit for ourselves.

Based on these reasons, we revised the beginning of section 2.1 as follows: “A setup with a commercial vaporizer coupled with a standard delivery module (A0211 and SDM, A0101, respectively; Picarro Inc., Santa Clara, CA, USA), guarantees the delivery of standard water vapour samples up to 30,000 ppm of H<sub>2</sub>O, which does not cover the H<sub>2</sub>O concentration range we are expecting for the Amazon rainforest. In addition, according to discussion with Picarro's technicians, there is no easy way to run an A0101 with the L1102i model.

Therefore, we built a calibration system to routinely and automatically conduct onsite-calibration of CRDS analysers (Fig. 1).” (see p. 3, LL. 18-21 in the marked manuscript).

In addition, due to the customization, we were able to achieve “The customized heating system and buffer reservoir enabled us to produce a high moisture stream of standard water vapour samples” (see p. 3, L. 41 – p. 4, L. 1 in the marked manuscript).

## Detailed comments

Page 1, Line 12: ‘isotope ratios’ is confusing here since it normally refers to R and not delta-notation. It may be replaced with ‘isotope compositions’. The term ‘isotope ratios’ has been used in many places in the manuscript, and all should be reconsidered or replaced.

**Response:** Following your suggestions, we replaced ‘isotope ratios’ with ‘isotope compositions’ throughout the manuscript.

P 2, L 17: ‘models’ replaced to ‘model’

**Response:** Following your suggestion, we revised here (see p. 2, L. 26 in the marked manuscript).

P 2, L 26: To make the structure more clear, suggest to add ‘In addition,’ before ‘Moreira et al.’.

**Response:** We added ‘In addition,’ before ‘Moreira et al.’ (see p. 2, L. 37 in the marked manuscript). Additionally, based on RC1 suggestion and the context we made a new paragraph from “However, H<sub>2</sub>O concentrations within the Amazon...” (see p. 2, LL. 35-42 in the marked manuscript).

P 2, L 37: To make the sentence more clear, suggest to remove ‘expected based on past measurement at the ATTO site’ or place it in a new sentence.

**Response:** Agreed. We removed it (see p. 3, LL. 6-7 in the marked manuscript).

P 3, L25: Maybe remove ‘(Fig. 1)’. This is already referred to in the beginning.

**Response:** Following your suggestions, we removed it (see p. 4, L. 7 in the marked manuscript).

P 3, L40: Is the purpose to remove ‘salt compounds’? I would suppose that there is very low salt contents in the fresh water (if the original water is fresh water and not sea water, otherwise it should be stated). I think the purpose is to in general remove contaminants.

**Response:** Yes, the original water is fresh water. We replaced ‘salt compounds’ with ‘contaminants’ (see p. 4, L. 22 in the marked manuscript).

P4, L21: The statement is very strong here so that it requires proof. If it is/can not be proved, it is rather a hypothesis or speculation. Also, this statement is in contradicted to the statement in P9, L15. Maybe replace ‘any’ to ‘to a large extent the’ or something like this.

**Response:** It is difficult to clearly prove that the rinsing and drying steps prevented **any** residual memory effects. Therefore, we revised the text as follows: ‘These rinsing and drying steps were introduced to minimize the residual memory effect’ (see p. 5, LL. 1-2 in the marked manuscript).

P4, L26: Not really common in the literature to use “[H<sub>2</sub>O]” as abbreviation. “[H<sub>2</sub>O]” has appeared in many places to represent ‘water concentration level’. I personally feel it hinders the reading flow. Maybe it is better to use ‘WCL’ or simply ‘concentration’?

**Response:** Following your suggestion, we did not abbreviate concentration level (see p. 5, L. 7 in the marked manuscript), and revised the corresponding parts throughout the manuscript.

P4, L29: 'Thus, the isotopic deviation values at 21,500 ppm are set to 0.' Personally think this sentence is redundant and can be removed with no harm.

**Response:** We removed this sentence (see p. 5, LL. 10-11 in the marked manuscript).

P4, L29: '(Fig. 2)' can be removed here.

**Response:** We cannot find '(Fig. 2)' at L. 29 on p. 4 in the previous manuscript, but we assumed it to be placed at L. 42 on p. 4 in the previous manuscript. After the revision following the RC1 reviewer, we did not remove here but changed here with "(Fig. 2b)" to help readers to find the place with the assigned Figure 2's letter (b) (see p. 5, LL. 31 in the marked manuscript).

P5, L7: '(Fig. 3)'. It is better to assign each subplot with a letter, and refer the description to the exact subfigure, for example '(Fig. 3a)'. With this context, suggest to add letters for all the subplots in Fig 3, 4, 6, and 7, as you have done for other figures.

**Response:** According to your suggestion, we assigned a figure letter to each subplot in Fig. 3 (see p. 10 in the marked manuscript), and revised here as follows: '(Figs. 3i and 3j)' (see p. 5, L. 40 in the marked manuscript). In addition, we assigned a figure letter to each subplot in Figs. 4, 6 and 7 (see p. 12 and p. 16-17 in the marked manuscript).

P5, L16: 'For example,'

**Response:** Done (see p. 6, L. 8 in the marked manuscript).

P5, L16: Suggest to remove '=', also for the other occasions throughout the manuscript.

**Response:** Done.

P5, L26: Suggest to remove 'For instance,'.

**Response:** Since we explain how many pairs the DII-2\*2Pairs strategy formed at 28 h interval as an example, we left 'For instance' here (see p. 6, L. 20 in the marked manuscript).

P5, L35-38: The sentence is redundant. Suggest to change to 'For each calibration strategy, we also calculated RMSE value for each of the [H 2 O]-dependence 2D or 3D fittings'.

**Response:** Done (see p. 6, LL. 29-30 in the marked manuscript).

P6, Table 1: Remove the bold title.

**Response:** Done (see p. 8, Table 1 in the marked manuscript).

P9, L12: '(1.1%)' to '(1.1 %)'.

**Response:** We revised here and also added space between '~1.5' and '%' in the end of this sentence (see p. 11, LL. 17-18 in the marked manuscript).

P9, L12: Suggest to remove '( > 40,000 ppm)'.

**Response:** We removed it (see p. 11, L. 21 in the marked manuscript).

P9, L125: Should be 'lower' precision? I can see the standard deviation becomes larger at high concentrations.

**Response:** Due to the revision in this section suggested by the RC1 reviewer, this sentence is no longer used.

P9, L126: Following above, should it be 'decrease'?

**Response:** We found "both analysers had the highest  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  measurement precision for DI1 at 29,000 ppm even though variability in  $\text{H}_2\text{O}$  concentration measurement was higher at 29,000 ppm ( $\text{H}_2\text{O}-\sigma = 578.6$  ppm) than at 21,500 ppm ( $\text{H}_2\text{O}-\sigma = 243.6$ )." (see p. 11, LL. 35-37 in the marked manuscript). Therefore, we revised "The increase in measurement precision of L2130i and L1102i with  $[\text{H}_2\text{O}]$ , despite larger  $[\text{H}_2\text{O}]$  variability," in the previous manuscript as follows: "The high measurement precision of L2130i and L1102i even with the larger  $\text{H}_2\text{O}$  concentration variability..." (see p. 11, LL. 37-38 in the marked manuscript).

P9, L133: Remove 'At all H 2 O concentration levels, and '.

**Response:** We removed it (see p. 11, L. 28 in the marked manuscript).

P9, L137: Again, the statement here sounds strong. It seems that it has been proved, but actually not in the manuscript. Therefore, I would say it is more like a speculation or hypothesis. Suggest to change 'mainly be' to 'is likely' or something similar.

Same applies to P11, L17.

**Response:** Following your suggestion, we revised the corresponding parts (see p. 11, L. 29 and p. 14, L. 2 in the marked manuscript).

P10, L8: Add space before unit '%' and check all other units to be consistent.

**Response:** We revised the corresponding parts throughout the manuscript.

P10, L16: Should be 'Fig. 5a-d'.

**Response:** In this sentence, we mention the results only about the L2130i analyser. So, the Figure letters are correct, but to make it clear we added "L2130i's" before "...deviation of each isotope from reference" (see p. 13, L. 14 in the marked manuscript).

P10, L17: Should be 'Fig. 5b'.

**Response:** We revised here (see p. 13, L. 16 in the marked manuscript).

P10, L18-19: This is an interesting observation. There is recently also a systematic study on concentration dependence that emphasizes this isotope-dependency. Probably this is something worthy to be discussed?

*Weng, Y., Touzeau, A., and Sodemann, H.: Correcting the impact of the isotope composition on the mixing ratio dependency of water vapour isotope measurements with cavity ring-down spectrometers, Atmos. Meas. Tech., 13, 3167–3190, <https://doi.org/10.5194/amt-13-3167-2020>, 2020.*

**Response:** Following your suggestion, we revised here as follows: "This finding indicates that the L2130i's  $\delta^2\text{H}$  accuracy for high moisture like 41,000 ppm is dependent on the isotopic composition, such as has been found for low moisture conditions below 4,000 ppm (Weng et al., 2020). This further indicates that more than one

standard water needs to be used in the field under not only low moisture but also high moisture conditions.” (see p. 13, LL. 16-21 in the marked manuscript).

P12, L10: Refer exactly to subfigures such as (Fig 6e, j).

**Response:** We revised here as follows: “(Fig. 6h)” (see p. 14, L. 22 in the marked manuscript).

P12, L23: It would be helpful to explain the method before instead of going directly to the results. It is not clear for the readers what have been calculated here and how they are calculated.

**Response:** Following your suggestion, we revised this sentence as follows: “Hence, for the DI1-2\*2Pairs strategy we obtained a [H<sub>2</sub>O]-dependence fitting method, which only obtained minimum RMSE values of  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$ , from each two calibration pairs at each interval and then calculated a contribution rate of the respective five [H<sub>2</sub>O]-dependence fittings (i.e., linear, quadratic, cubic, quartic, linear surface fitting methods) to the total calibration pairs at each interval (Fig. 7).” (see p. 15, LL. 25-29 in the marked manuscript).

P12, L39: ‘smaller sample numbers for calculating RMSE (28 h: n=43, 196 h: n=19; c.f., Fig. 2)’. It is confusing here because it seems to me the short-interval calibration has larger sample numbers (n=43).

**Response:** We are sorry that the description in the previous manuscript was misleading. The sample number for obtaining each RMSE value corresponds to the sample number during the assigned measurement cycles. For example, a 28 h interval using the DI1-2\*2Pairs strategy with ID-[3,4] & [7,8] used 8 samples from two measurement cycles (i.e., DI1: 5, DI2: 6) for calculating RMSE value of each fitting method. (8 samples = 4 samples  $\times$  2 measurement cycles). Therefore, we revised the information in the parentheses as follows: “(e.g., 28 h with ID-[3,4] & [7,8]: n=8 (4 samples  $\times$  2 measurement cycles, i.e., ID-5,6), 196 h with ID-[3,4] & [31,32]: n=104 (4 samples  $\times$  26 measurement cycles, i.e., ID-5-30); c.f., Fig. 2b).” (see p. 15, LL. 21-22 in the marked manuscript).

P12, L31-39: This paragraph jumps back to Fig. 6. Suggest to move it up after L19, before presenting Fig 7.

**Response:** Following your suggestion, we moved this paragraph before presenting Figure 7, and also divided this paragraph into two paragraphs to make the context clearer (see p. 15, LL. 8-22 in the marked manuscript).

P16, L2: Replace ‘the CRDS’ to ‘CRDS’.

**Response:** Following your suggestions, we revised here (see p. 19, L. 5 in the marked manuscript).

Fig S1: delta<sup>2</sup>H instead of delta<sup>18</sup>O in first line.

**Response:** We revised here (see p. 2, Fig. S1 caption’s first line in the marked supplement).

# Characterising water vapour concentration dependence of commercial cavity ring-down spectrometers for continuous onsite atmospheric water vapour isotope measurements in the tropics

Shujiro Komiya<sup>1</sup>, Fumiyoshi Kondo<sup>2</sup>, Heiko Moossen<sup>1</sup>, Thomas Seifert<sup>1</sup>, Uwe Schultz<sup>1</sup>, Heike Geilmann<sup>1</sup>, David Walter<sup>1,3</sup>, and Jost V. Lavric<sup>1</sup>

<sup>1</sup>Max Planck Institute for Biogeochemistry, Jena, 07745, Germany

<sup>2</sup>Japan Coast Guard Academy, Kure, 737-8512, Japan

<sup>3</sup>Max Planck Institute for Chemistry, Mainz, 55128, Germany

\* Correspondence to: Shujiro Komiya (skomiya@bgc-jena.mpg.de)

**Abstract.** The recent development and improvement of commercial laser-based spectrometers have expanded in situ continuous observations of water vapour (H<sub>2</sub>O) stable isotope ratios/compositions (e.g.,  $\delta^{18}\text{O}$ ,  $\delta^2\text{H}$ , etc.) in a variety of sites worldwide. However, we still lack continuous observations in the Amazon, a region that significantly influences atmospheric and hydrological cycles on local to global scales. In order to achieve accurate on-site observations, commercial water isotope analysers require regular in situ calibration, which includesing the correction of H<sub>2</sub>O concentration dependence ([H<sub>2</sub>O]-dependence) of isotopic measurements accuracy. Past studies have assessed the [H<sub>2</sub>O]-dependence for air with H<sub>2</sub>O concentrations up to 35,000 ppm, a value that is frequently surpassed in tropical rainforest settings like the central Amazon where we plan continuous observations. Here we investigated the performance of two commercial analysers (L1102i and L2130i models, Picarro, Inc., USA) for measuring  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  in atmospheric moisture at four different H<sub>2</sub>O levels from 21,500 to 41,000 ppm. These H<sub>2</sub>O levels were created by a custom-built calibration unit designed for regular in situ calibration. Measurements on the newer analyser model (L2130i) had better precision for  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  and demonstrated less influence of H<sub>2</sub>O concentration on the measurement accuracy at each concentration/moisture level compared to the older L1102i. Based on our findings, we identified the most appropriate calibration strategy for [H<sub>2</sub>O]-dependence, adapted to our calibration system. The best strategy required conducting a two-point calibration with four different H<sub>2</sub>O concentration levels, carried out at the beginning and end of the calibration interval. The smallest uncertainties in calibrating [H<sub>2</sub>O]-dependence of isotopic accuracy of the two analysers were achieved using a linear-surface fitting method and a 28 h calibration interval, except for the  $\delta^{18}\text{O}$  accuracy of the L1102i analyser for which the cubic fitting method gave best results. The uncertainties in [H<sub>2</sub>O]-dependence calibration did not show any significant difference using calibration intervals from 28 h up to 196 h; this suggested that one [H<sub>2</sub>O]-dependence calibration per week for the L2130i and L1102i analysers is sufficient. This study shows that the CRDS analysers, appropriately calibrated for [H<sub>2</sub>O]-dependence, allow the detection of natural signals of stable water vapour isotopes at very high humidity levels, which has promising implications for water cycle studies in areas like the central Amazon rainforest and other tropical regions.

## 1 Introduction

Ongoing climate change has affected various aspects of global and local climate, including the hydrological cycle (Intergovernmental Panel on Climate Change, 2014). Further and more detailed understanding on how climate change affects the atmospheric hydrological system is required. Water vapour isotope ratios/compositions (e.g.,  $\delta^{18}\text{O}$ ,  $\delta^2\text{H}$ ,  $\delta^{17}\text{O}$ ) have been used in meteorology and hydrology to disentangle the water vapour transport, mixing and phase changes such as evaporation and condensation that govern processes of the atmospheric hydrological cycle (Dansgaard, 1964; Craig and Gordon, 1965; Galewsky et al., 2016). Incorporating water vapour isotopic information into global and regional circulation models has also

improved ~~our understanding of how stable water isotopes are transported in the atmosphere and affected by phase changes in- and below-clouds, and how they behave in different situation of surface-atmosphere interactions~~ ~~simulations of hydrometeorological fields~~ (Risi et al., 2010; Werner et al., 2011; Pfahl et al., 2012; Galewsky et al., 2016). The increase in field observation of water vapour isotope ~~ratios~~ ~~compositions~~ therefore is expected to improve our process understanding and thereby models simulating the interactions between ~~the atmospheric hydrological system~~ ~~hydrometeorological cycles~~ and global climate change.

Until around 10-15 years ago, *in-situ* water vapour isotope measurements were limited due to the laborious and error-prone sampling techniques using cryogenic traps, molecular sieves, vacuum flasks, etc. (Helliker and Noone, 2010). Recent development and improvement of laser-based spectrometers have made continuous water vapour isotope ratio measurements at a high temporal resolution possible. The number of onsite measurements of stable water vapour isotope ~~ratios~~ ~~compositions~~ across the world has increased in the last decade (Wei et al., 2019). So far, ~~there are many studies based on field water isotopic measurements available in polar and midlatitude regions, some in the subtropics (e.g., Bailey et al., 2013; Gonzalez et al., 2016) but only very few in the tropics (e.g., Tremoy et al., 2012; Aemisegger et al., 2020). Particularly studies in tropical continental regions, have been frequently conducted in North America, Europe, Africa, Asia, Oceania, Arctic and Antarctic regions (Wei et al., 2019), but not in South America such as the Amazon basin region, are rare. Yet,~~ ~~U~~ understanding the hydrological processes in the Amazon basin is crucial as it significantly influences the atmospheric convective circulation in the tropics and beyond (Coe et al., 2016; Galewsky et al., 2016b). Thus, *in-situ* ~~continuous~~ measurements of water vapour isotope ~~ratios~~ ~~compositions~~ in the Amazon region will improve our comprehension of the Amazonian hydro-climatological system and its interaction with global climate (Coe et al., 2016; Galewsky et al., 2016).

Recent field observations for water vapour isotopes have mainly utilized two commercial laser-based instruments: Picarro cavity ring-down spectroscopy (CRDS) and ~~Los Gatos Research~~ ~~GR~~-off-axis integrated cavity output spectroscopy (OA-ICOS) analysers (Galewsky et al., 2016; Wei et al., 2019). The CRDS analysers have been used in most of the field sites that are registered in the Stable Water Vapor Isotopes Database (SWVID) website that archives onsite high-frequency ~~ncy~~ water vapour isotope data (Wei et al., 2019). Globally, five ~~Picarro~~ CRDS models (i.e., L1102i, L1115i, L2120i, L2130i, L2140i sorted by oldest to newest) are in operation at various field sites, ~~and~~ Aemisegger et al. (2012) ~~confirmed~~ ~~demonstrated~~ that a ~~newer-recent~~ model (L2130i) has better precision and accuracy compared to an older model ~~s~~ (L1115i) due to the improved spectroscopic fitting algorithms.

Even with improved analysers, CRDS instruments still require regular calibration (e.g., 3-24 hour frequency) (Aemisegger et al., 2012; Delattre et al., 2015; Wei et al., 2019). The main calibration issue is that the measurement quality of water vapour isotopic ~~ratios~~ ~~compositions~~ depends on water vapour ( $\text{H}_2\text{O}$ ) concentration (hereinafter called “[ $\text{H}_2\text{O}$ ]-dependence”; Schmidt et al., 2010; Tremoy et al., 2011; Aemisegger et al., 2012; Bailey et al., 2015; Delattre et al., 2015). The [ $\text{H}_2\text{O}$ ]-dependence of Picarro analysers has been assessed over a  $\text{H}_2\text{O}$  concentration range spanning 200 to 35,000 ppm (Schmidt et al., 2010; Aemisegger et al., 2012; Steen-Larsen et al., 2014; Bailey et al., 2015; Delattre et al., 2015), and only rarely above 35,000 ppm (Tremoy et al. 2011).

However,  $\text{H}_2\text{O}$  concentrations within the Amazon tropical rainforest canopy (e.g., the Amazon Tall Tower Observatory (ATTO) site; see Andreae et al., 2015) ~~normally~~ exceed 35,000 ppm on a daily basis ~~and occasionally, with maximum concentrations reaching 404,000 ppm. In addition,~~ Moreira et al. (1997) observed the diel variation pattern in  $\text{H}_2\text{O}$  concentration in the Amazon tropical rainforest was mostly similar to that in  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  of water vapour. The diel relationship between  $\text{H}_2\text{O}$  concentration and isotopes may lead to over- or under-estimation of isotopic values measured by CRDS analysers in the Amazon tropical rainforest. Thus, ~~assuming for~~ *in-situ* water vapour isotope measurements by CRDS analysers in the Amazon tropical rainforest, the [ $\text{H}_2\text{O}$ ]-dependence of CRDS analysers under high moisture conditions ( $> 35,000$  ppm  $\text{H}_2\text{O}$ ) needs to be assessed and corrected.



The primary aim of this study was to characterise two CRDS analysers (L1102i and L2130i) for measuring  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  of water vapour in high atmospheric moisture expected at the ATTO site ([~ 150 km NE of Manaus, Brazil](#)), where we intend to conduct continuous in-situ observations. Over a two week periods, we examined the effects of  $\text{H}_2\text{O}$  concentration on isotopic measurement precision and accuracy for [both an older \(L1102i\) and a newer CRDS models \(L2130i\)](#). [They were both connected to our](#)~~We used a~~ custom-made calibration system that regularly supplied standard water vapour samples at four different  $\text{H}_2\text{O}$  concentrations covering high moisture conditions (21,500 to 41,000 ppm)~~expected based on past measurement at the ATTO site~~. Standard water vapour samples were made from two standard waters, almost covering the previously reported isotopic ranges ( $\delta^{18}\text{O} = -19.4$  to  $-6.7$  ‰ and  $\delta^2\text{H} = -151$  to  $-42$  ‰) for water vapour samples ~~in from~~ Manaus ~~located near the ATTO site, or in from~~ the Ducke Reserve near Manaus (Matsui et al., 1983; Moreira et al., 1997; IAEA/WMO, 2020). We also assessed which  $[\text{H}_2\text{O}]$ -dependence calibration strategy ~~based on the two week operation~~, can [best](#) reduce measurement uncertainty of the two CRDS models ~~the most~~. ~~According to~~ [Based on the uncertainty quantification presented](#)~~determined best calibration strategy~~, we discussed whether the CRDS analysers [with our calibration setup](#) can sufficiently detect natural signals of stable water vapour isotopes, expected at the ATTO site.

## 2 Materials and Methods

### 2.1 Calibration system

[A setup with a commercial vaporizer coupled with a standard delivery module \(A0211 and SDM, A0101, respectively; Picarro Inc., Santa Clara, CA, USA\), guarantees the delivery of standard water vapour samples up to 30,000 ppm of  \$\text{H}\_2\text{O}\$ , which does not cover the  \$\text{H}\_2\text{O}\$  concentration range we are expecting for the Amazon rainforest. In addition, according to discussion with Picarro's technicians, there is no easy way to run an A0101 with the L1102i model. Therefore, w](#)~~We~~ built a calibration system to routinely and automatically conduct onsite-calibration of CRDS analysers (Fig. 1). The main units of the calibration system are a syringe-pump, a vaporizer and a dry-air supply unit ([Fig. 1a](#)). The syringe-pump (Pump 11 Pico Plus Elite, Harvard Apparatus, Holliston, MA, USA) takes 3.3 mL standard water from a 2L reservoir bag (Cali-5-Bond<sup>TM</sup>, Calibrated Instruments, Inc., Ardsley, New York, USA), and delivers the standard water into a vaporizer unit with a constant water flow of  $1.9 \mu\text{L min}^{-1}$  ([Figs. 1a and 1b](#)). [To maintain accuracy of the syringe-pump's infusion over a long term, two guide rods and a lead screw of the syringe pump need to be properly lubricated every 100 hours of operation for injecting and withdrawing](#). The vaporizer unit [that was modified from an A0211](#) is comprised of a heater, vaporization chamber and buffer reservoir, which is enclosed in a copper pipe and heated at  $140$  °C, covered by insulation material to reduce heat dissipation and help to reduce the memory effects between different water vapour isotopic measurements. Dried ambient air, recommended as a carrier gas for calibration by Aemisegger et al. (2012), was supplied into the heated vaporizer unit from a dry-air unit made up of a compressor, water separator, mist separators, membrane dryer (IDG60SAM4-F03C, SMC, Tokyo, Japan), precision regulator (IR1000, SMC, Tokyo, Japan) and flow regulator ([Figs. 1a and 1c](#)). [We chose the SMC's membrane dryer because SMC guarantees a long-term operation \(e.g., 10 years or more by 10 hours/day operation\) without replacing the membrane module](#). The dry-air unit and mass flow controller 1 (MFC1) (1179B, MKS GmbH, Munich, Germany) provide the vaporizer unit with a steady flow of dried ambient air with a dew point temperature of  $-32$  °C or below ([~300 ppm of  \$\text{H}\_2\text{O}\$  or below](#)), operated at  $50 \text{ mL min}^{-1}$  flow rate and 17.2-20.7 kPa flow pressure. The dry air entering the vaporizer is heated through the heater line, speeding up the evaporation of the infused standard water inside the vaporization chamber without fractionation. Furthermore, the heated carrier gas also [helps reduc](#)~~ing~~[es](#) the memory effect of ~~f~~ the measurements. The subsequent standard water vapour was well mixed inside a [bigger](#) buffer reservoir [compared to A0211](#). [The customized heating system and buffer reservoir enabled us to produce a high moisture stream of standard water vapour](#)

samples, and then delivered through the multiposition valve (Model EMTMA-CE, VICI Corp., Houston, TX, USA), switching flow paths between the calibration and routine analysis mode of the two CRDS analysers: L1102i and L2130i. To minimise tubing memory effects on water vapour isotopic measurements, we connected the vaporizer unit and CRDS analysers with stainless steel tubing constantly held at 45 °C with heating tapes to avoid condensation inside the tubes (c.f., Schmidt et al., 2010, Tremoy et al., 2011). Before reaching the CRDS analysers, the transported standard water vapour was diluted with the dried ambient air via a dilution line and adjusted to an intended concentration level by regulating the dilution dry air flow rate using MFC2 (Fig. 1). The total flow rate of both the calibration and dilution lines exceeded the suction flow rates of the two CRDS analysers (~50 mL min<sup>-1</sup> in total). The excess air was exhausted through an overflow port.

## 2.2 Water vapour concentration dependence experiment

We conducted a continuous operation of the L1102i and L2130i analysers over a two-week period in June 2019 in an air-conditioned laboratory at Max Planck Institute for Biogeochemistry (MPI-BGC, Jena, Germany). The two CRDS analysers measured water vapour (H<sub>2</sub>O) concentration,  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  of outside/room air samples from a profile gas-stream switching system (not shown in this article here) or H<sub>2</sub>O concentration,  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  of water vapour samples supplied from the calibration system (Fig. 1). Since H<sub>2</sub>O concentration values measured by old CRDS models (e.g., L1102i) are biased due to the self-broadening effect of water vapour (Rella et al., 2013), H<sub>2</sub>O concentration measuring by the L1102i were corrected by a nonlinear calibration fitting, determined by following Winderlich et al., (2010) and recommended for old CRDS models (e.g., G1301 CO<sub>2</sub>/CH<sub>4</sub>/H<sub>2</sub>O analyser) by Rella (2010) and Rella et al., (2013).

We also simulated regular automated calibration operation designed for field operations over the two-week period to regularly supply the two CRDS analysers with standard water vapour samples at four different concentration levels from 21,500 to 41,000 ppm. We prepared two different working standard waters (DI1 and DI2) made of deionized water to avoid clogging the heated tubes and chamber inside the vaporizer unit with contaminants/salt compounds. Stable water isotope ratios/compositions ( $\delta^{18}\text{O}$  and  $\delta^2\text{H}$ ) of the DI1 and DI2 standards were analysed at the MPI-BGC stable isotope laboratory (BGC-IsoLab) of the MPI-BGC (BGC-IsoLab) using Isotope Ratio Mass Spectrometry (IRMS). For details on the IRMS technique/analysis, we refer readers to Gehre et al., (2004). The DI1 and DI2 standards were calibrated against VSMOW and SLAP via in-house standards: DI1- $\delta^{18}\text{O}$  = -25.07 ± 0.16 ‰, DI1- $\delta^2\text{H}$  = -144.66 ± 0.60 ‰, DI2- $\delta^{18}\text{O}$  = -3.69 ± 0.15 ‰, DI2- $\delta^2\text{H}$  = -34.30 ± 1.00 ‰ (also see the section S1 in the Supplement). The isotopic span of the DI1 and DI2 almost covers the previously reported range of  $\delta^{18}\text{O}$  (-19.4 to -6.7 ‰) and  $\delta^2\text{H}$  (-151 to -42 ‰) for water vapour samples in the Ducke Reserve near Manaus or in Manaus, located near the ATTO site (Matsui et al., 1983; Moreira et al., 1997; IAEA/WMO, 2020). For calibration, we alternated between the two standard waters. One calibration run required 75 minutes, of which the first 30 minutes were used for stabilizing the produced standard water vapours at the highest concentration level and delivering it to the CRDS analysers. Subsequently the calibration system created stepwise lower concentration levels of the standard water vapour every 15 minutes by regulating the dilution flow rate. One calibration run consisted of a 4-point concentration calibration at approximately 41,000 ppm, 36,000 ppm, 29,000 ppm, and 21,500 ppm. The actual measured mean and standard deviation of H<sub>2</sub>O concentration at the respective four concentration/moisture level for all the calibration cycles during the two-week operation are shown in Table 1. The dilution flow rates for the different concentration/moisture levels were set to 9 sccm (41,000 ppm), 14 sccm (36,000 ppm), 21 sccm (29,000 ppm) and 28 sccm for 21,500 ppm. The set-point values were not changed during the 2-week test, thus simulating remote automatic onsite calibration runs. We used the last 7-minutes of data collected at each concentration level for the calibration assessment of the CRDS analysers. Immediately after a calibration cycle, the syringe-pump drained the remaining standard water inside the tube between the vaporization chamber and 3-way solenoid valve 6+ (SV6+) through the waste line and then washed the inner space between the vaporization chamber and the SV12 valve 3 times with the standard water scheduled for the next calibration cycle (Fig. 1).

Subsequently, the rinsed vaporization chamber was fully dried with air from the dry-air unit for 2 to 4 hours. These rinsing and drying steps were introduced to minimize the residual memory effect from the last calibration cycle on standard water vapour isotopic compositions during the next calibration run. We started the next calibration cycle seven hours after the start time of the last calibration cycle (i.e., the interval of the same working standard was 14 hours). Throughout the entire experimental period, the calibration system conducted automatically 24 calibration runs for each standard water, which used 160 mL each standard water in total.

We calculated isotopic deviations at each concentration level (hereinafter called “[H<sub>2</sub>O]”) for each calibration cycle to evaluate [H<sub>2</sub>O]-dependence on isotopic measurement accuracy. The isotopic deviations at each concentration level [H<sub>2</sub>O] were obtained from the difference between measured isotopic values at each concentration level [H<sub>2</sub>O] during each calibration cycle and assigned reference values at 21,500 ppm on each calibration. Thus, the isotopic deviation values at 21,500 ppm are set to 0. We selected the 21,500 ppm level as the reference H<sub>2</sub>O condition because Picarro guarantees high  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  precision of CRDS analysers between 17,000 – 23,000 ppm of H<sub>2</sub>O, and to make the results comparable with a similar past study (Tremoy et al., 2011) that assigned 20,000 ppm as the reference level. The assignment of reference values for each calibration cycle enabled us to assess isotopic biases that were mainly due to [H<sub>2</sub>O]-dependence but not for other effects (e.g., drift effects on  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  accuracy between each calibration cycle).

### 2.3 Calibration for water vapour concentration dependence

We devised four strategies, referred to here as DI1, DI2, DI1-DI2\*1Pair, DI1-2\*2Pairs, to use the automated calibration system to determine and correct for [H<sub>2</sub>O]-dependence, and used the two-week operation to assess which calibration strategy decreased the uncertainties in  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  measurements the most. The DI1 and DI2 calibration strategies used a single standard water (DI1 or DI2) to correct for [H<sub>2</sub>O]-dependence. In contrast, the DI1-DI2\*1Pair and DI1-2\*2Pairs strategies used the two standard waters (DI1 and DI2) for calibrating [H<sub>2</sub>O]-dependence because we considered that [H<sub>2</sub>O]-dependence might change between the two standard waters according to recent studies (Bonne et al., 2019; Weng et al., 2020). In addition, the DI1-2\*2Pairs strategy used more calibration data than the DI1-DI2\*1Pair strategy to obtain more robust calibration fittings of [H<sub>2</sub>O]-dependence.

Figure 2 summarises the overview of the four calibration strategies. DI1 and DI2 refer to the two standard waters, measured at the four different concentration levels [H<sub>2</sub>O], and an identity number is assigned to the respective 48 calibration cycles (ID: 1 – 48), ordered by time during the experimental period (Fig. 2a). Hereinafter, we explain how to obtain calibration fittings and assess uncertainties of obtained calibration fittings by using the DI1-2\*2Pairs strategy as an example. For example, the DI1-2\*2Pairs strategy uses two pairs of DI1 and DI2 calibration cycles (e.g., ID-[3,4] & [7,8] at 28 h interval) for obtaining calibration fittings of [H<sub>2</sub>O]-dependence at intervals from 28 h to 196 h (Fig. 2b). The DI1-2\*2Pairs strategy utilized four two-dimensional (2D) and a three-dimensional (3D) fitting methods (i.e., linear, quadratic, cubic, quartic, and linear-surface fitting methods) to obtain [H<sub>2</sub>O]-dependence calibration fitting parameters. For instance, the DI1-2\*2Pairs strategy at 28 h interval with ID-[3,4] & [7,8] obtained total 5 [H<sub>2</sub>O]-dependence calibration fittings for each isotope accuracy.

As an example, Figure 3 illustrates five calibration fittings for [H<sub>2</sub>O]-dependence of  $\delta^{18}\text{O}$  accuracy for each CRDS analyser, acquired from two pairs of DI1 and DI2 calibration cycles (e.g., 3,4 and 7,8) following the DI1-2\*2Pairs strategy at a 28 h interval (also c.f., Fig. 2b). The respective 2D fitting is acquired from a relationship between H<sub>2</sub>O concentrations, measured at 4 different levels, and  $\delta^{18}\text{O}$  deviation at each of the 4-point levels [H<sub>2</sub>O] (the blue dots in Figs. 3a-h). The linear-surface fitting also involves measuring the  $\delta^{18}\text{O}$  value at each concentration level [H<sub>2</sub>O] as an independent variable (Figs. 3i and 3j). The procedure for calculating isotopic deviations at each concentration level [H<sub>2</sub>O] was the same as described in section 2.2.

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

The quantitative evaluation of uncertainties in [H<sub>2</sub>O]-dependence calibration was conducted by means of root mean square error (RMSE) between actual observed and predicted isotopic deviation values by obtained [H<sub>2</sub>O]-dependence fittings. We calculated RMSE value for each of the [H<sub>2</sub>O]-dependence 2D or 3D fittings as follows:

$$RMSE = \sqrt{\frac{1}{n} \sum_{i=1}^n (\delta_{(obs)} - \delta_{(pred)})^2} \quad (1)$$

where  $\delta_{(obs)}$  is the actual observed deviation value of  $\delta^{18}\text{O}$  or  $\delta^2\text{H}$  at each concentration level [H<sub>2</sub>O] from measurement cycles,  $\delta_{(pred)}$  is the predicted deviation value of  $\delta^{18}\text{O}$  or  $\delta^2\text{H}$  at each [H<sub>2</sub>O] concentration level, and n is the sample number. The measurement cycles represent calibration cycles that were not used for estimating [H<sub>2</sub>O]-dependence, over an interval period between one or two calibration pairs. For example, in the case of the DI1-2\*2Pairs strategy at 28 h interval with ID [3,4] & [7,8], Figs. 2 and 3 show a 28 h interval using the DI1-2\*2Pairs strategy with ID [3,4] [7,8], where a DI1 and DI2 calibration cycles (i.e., DI1: 5, DI2: 6) occurring in between are regarded as measurement cycles (Fig. 2). The measured  $\delta^{18}\text{O}$  deviation value at each concentration level [H<sub>2</sub>O] during the measurement cycles (e.g. red dots: DI1, ID-5; green dots: DI2, ID-6; Fig. 3) (i.e., DI1: 5, DI2: 6) represents the value of  $\delta_{(obs)}$  at each concentration level [H<sub>2</sub>O] (the red and green dots in Fig. 3). The predicted isotopic deviation value ( $=\delta_{(pred)}$ ) at each concentration level [H<sub>2</sub>O] during the measurement cycles (e.g., DI1: 5, DI2: 6) is calculated by each of the [H<sub>2</sub>O]-dependence 2D or 3D fittings, applied to measured value of H<sub>2</sub>O concentration at each concentration level [H<sub>2</sub>O] (the open triangles in Figs. 3a-3h) or to measured values of both H<sub>2</sub>O concentration and  $\delta^{18}\text{O}$  at each concentration level [H<sub>2</sub>O] during the measurement cycles (the open triangles in Figs. 3i and 3j). The example of calculated  $\delta^{18}\text{O}$  RMSE of each fitting method for each CRDS analyser is shown on each plot in Fig. 3.

We conducted  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  RMSE evaluation for all the [H<sub>2</sub>O]-dependence fittings that were obtained from all the respective two pairs of DI1 and DI2 calibration cycles at each interval period (28 - 196 h) following the DI1-2\*2Pairs strategy over the entire two-week period (c.f., Fig. 2b). For instance, since the DI1-2\*2Pairs strategy at 28 h interval formed 43 two pairs in total (i.e., [1,2]-[5,6], [2,3]-[6,7], [3,4]-[7,8] ~ [42,43]-[46,47], [43,44]-[47,48]) (c.f., Fig. 2b), we calculated  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  RMSE values for each of 43 [H<sub>2</sub>O]-dependence linear, quadratic, cubic, quartic, or linear-surface fittings.

Compared with the DI1-2\*2Pairs strategy, the DI1, DI2, and DI1-DI2\*1Pair calibration strategies used a pair of only DI1 calibrations, a pair of only DI2 calibrations, and a pair of DI1 and DI2 calibrations, respectively, for acquiring [H<sub>2</sub>O]-dependence fittings at intervals from 14 h to 196 h (DI1, DI2 calibration strategies) or from 21 h to 203 h (DI1-DI2\*1Pair calibration strategy) (Fig. 2b). The DI1 and DI2 calibration strategies utilized the four 2D fitting methods for obtaining [H<sub>2</sub>O]-dependence calibration fittings, whereas the DI1-DI2\*1Pair calibration strategy used the four 2D and one 3D fitting methods as with the DI1-2\*2Pairs strategy. For each calibration strategy, we also calculated RMSE value for each of the [H<sub>2</sub>O]-dependence 2D or 3D fittings, obtained from each of all the pairs of only DI1 calibrations (DI1 calibration strategy), all the pairs of only DI2 calibrations (DI2 calibration strategy), or all the pairs of DI1 and DI2 calibrations (DI1-DI2\*1Pair calibration strategy) at each interval period as well as the DI1-2\*2Pairs strategy.

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold


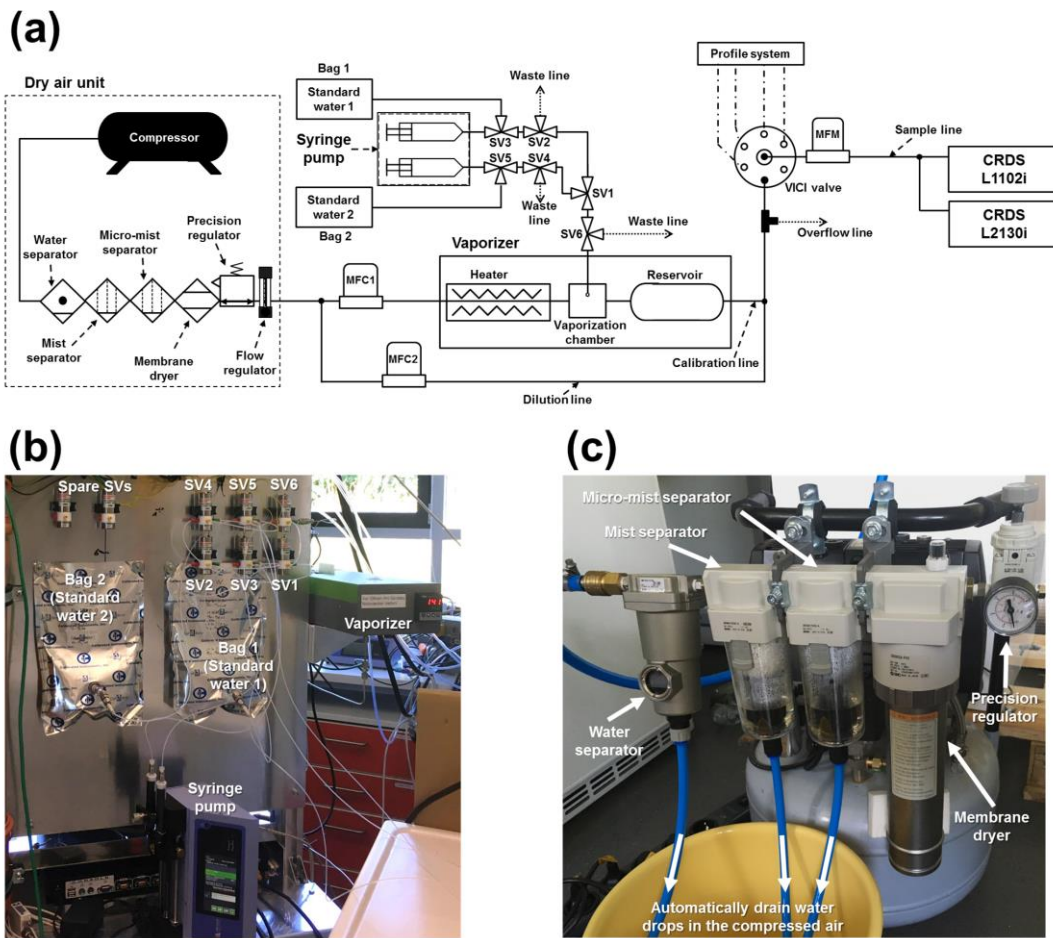


Figure 1 (a) Schematic diagram of the calibration system, including the dry air unit. MFC, MFM and SV denote mass flow controller, mass flow meter, and 3-way solenoid valve, respectively. The profile system, prepared for in situ observation at the Amazon Tall Tower Observatory site (c.f., Andreae et al. 2015) in the Amazon tropical forest, is not described in this article. The diagram is not to scale. Panel (b) shows the photo of the main part of the calibration system: a vaporizer, syringe pump, 2L reservoir bags, and solenoid valves. Panel (c) shows the photo of the main part of the dry air unit: a water separator, mist separators, membrane dryer, precision regulator, and drain lines for water drops in the compressed air.

10 **Table 1** Standard deviations of  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  at each concentration level from all 24 calibration runs for the respective DI1 and DI2 standard waters. The standard deviations were calculated from all 24 data set of raw 7-min average values, obtained by L2130i and L1102i on each calibration run. The mean values of  $\text{H}_2\text{O}$  concentration at each concentration level were also calculated from all 24 data set of raw 7-min average values, obtained by L2130i and L1102i on each calibration run.

Picarro	Standard water					
	DI1 (n=24)			DI2 (n=24)		
	H <sub>2</sub> O concentration (ppm)	δ <sup>18</sup> O (‰)	δ <sup>2</sup> H (‰)	H <sub>2</sub> O concentration (ppm)	δ <sup>18</sup> O (‰)	δ <sup>2</sup> H (‰)
L2130i	21656.2 ± 243.6	0.09	0.45	21289.8 ± 220.0	0.08	0.55
	29144.1 ± 578.6	0.08	0.35	28473.0 ± 514.7	0.11	0.59
	36593.8 ± 676.2	0.13	0.68	35701.3 ± 565.7	0.12	0.68
	41803.0 ± 653.9	0.13	0.68	40744.4 ± 543.1	0.12	0.71
L1102i	20967.1 ± 253.5	0.14	1.01	20563.2 ± 244.9	0.11	0.99
	28957.3 ± 634.2	0.12	0.72	28244.0 ± 545.4	0.15	1.08
	37250.0 ± 756.5	0.18	0.90	36246.2 ± 690.1	0.20	1.06
	43387.8 ± 759.8	0.23	0.79	42172.1 ± 695.9	0.21	0.95



(b)

Calibration strategy	Interval (h)							
	14	21	28	35	42	~	196	203
DI1	[1,3] [3,5] [5,7] ~ [43,45] [45,47] (n = 23)	NA	[1,5] [3,7] [5,9] ~ [41,45] [43,47] (n = 22)	NA	[1,7] [3,9] [5,11] ~ [39,45] [41,47] (n = 21)	~	[1,29] [3,31] [5,33] ~ [17,45] [19,47] (n = 10)	NA
DI2	[2,4] [4,6] [6,8] ~ [44,46] [46,48] (n = 23)	NA	[2,6] [4,8] [6,10] ~ [42,46] [44,48] (n = 22)	NA	[2,8] [4,10] [6,12] ~ [40,46] [42,48] (n = 21)	~	[2,30] [4,32] [6,34] ~ [18,46] [20,48] (n = 10)	NA
DI1-DI2*1Pair	NA	[1,4] [2,5] [3,6] ~ [44,47] [45,48] (n = 45)	NA	[1,6] [2,7] [3,8] ~ [42,47] [43,48] (n = 43)	NA	~	NA	[1,30] [2,31] [3,32] ~ [18,47] [19,48] (n = 19)
DI1-DI2*2Pairs	NA	NA	[1,2] & [5,6] [2,3] & [6,7] [3,4] & [7,8] ~ [42,43] & [46,47] [43,44] & [47,48] (n = 43)	NA	[1,2] & [7,8] [2,3] & [8,9] [3,4] & [9,10] ~ [40,41] & [46,47] [41,42] & [47,48] (n = 41)	~	[1,2] & [29,30] [2,3] & [30,31] [3,4] & [31,32] ~ [18,19] & [46,47] [19,20] & [47,48] (n = 19)	NA

5

Figure 2 Overview of the four different [H<sub>2</sub>O]-dependence calibration strategies (DI1, DI2, DI1-DI2\*1Pair, DI1-2\*2Pairs) for assessing [H<sub>2</sub>O]-dependence uncertainties of the L2130i and L1102i analysers related to the length of the calibration interval. (a) The top diagram shows a part of the total 48 calibration cycles, including both the DI1 and DI2 standard waters, with 7-hour interval and identity number (ID: 1 – 48) as an example. (b) The bottom table presents a part of which calibration cycles the four calibration strategies utilize for obtaining [H<sub>2</sub>O]-dependence calibration fittings at different intervals as an example. The respective DI1 and DI2 strategies used a pair of only DI1 calibration cycles and a pair of only DI2 calibration cycles for obtaining calibration fittings of [H<sub>2</sub>O]-dependence at intervals from 14 h to 196 h. For example, the DI1 calibration strategy at 14 h interval with ID-[1,3] used data sets from a pair of DI1 calibration cycles (ID-1 and ID-

10

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

3) to obtain [H<sub>2</sub>O]-dependence calibration fittings. The DI1-DI2\*1Pair and DI1-2\*2Pairs strategies used a pair of DI1 and DI2 calibration cycles, and two pairs of DI1 and DI2 calibration cycles, respectively, for obtaining calibration fittings of [H<sub>2</sub>O]-dependence at intervals from 21 h to 203 h (DI1-DI2\*1Pair strategy) or from 28 h to 196 h (DI1-DI2\*2Pairs strategy). At each interval, the respective calibration strategy made all the pairs of each set calibration cycles (e.g., 43 two pairs at 28 h interval for the DI1-DI2\*2Pairs strategy)-, and then obtained calibration fittings from each pair of calibration cycles. For instance, as the DI1-DI2\*2Pairs strategy utilized four two-dimensional (2D) and a three-dimensional (3D) fitting methods (i.e., linear, quadratic, cubic, quartic, and linear-surface fitting methods) (c.f., section 2.3), the DI1-DI2\*2Pairs strategy at 28 h interval obtained 215 calibration fittings in total (= 5 fitting methods × 43 two pairs) for the respective  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  accuracy. The procedure for assessing uncertainties in the obtained [H<sub>2</sub>O]-dependence calibration fittings is described in section 2.3.

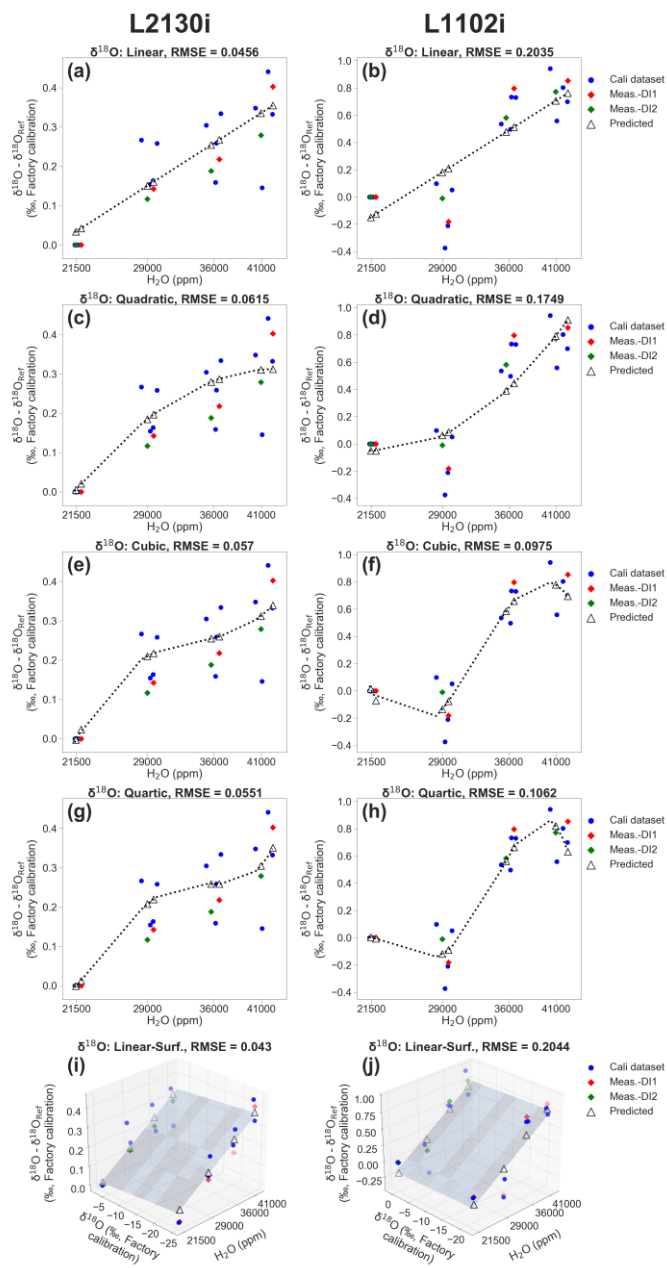


Figure 3 Example of calibrating  $[H_2O]$ -dependence of  $\delta^{18}O$  accuracy for the respective (a) L2130i and (b) L1102i analysers by using four two-dimensional (2D) and a three-dimensional (3D) fitting methods (i.e., linear, quadratic, cubic, quartic, and linear-surface fitting methods) according to the DI1-2\*2Pairs calibration strategy at 28 h interval with ID-[3,4] & -[7,8] (c.f., Fig. 2b). Calibrating (a) L2130i's and (b) L1102i's  $[H_2O]$ -dependence by using the linear fitting method. Calibrating (c) L2130i's and (d) L1102i's  $[H_2O]$ -dependence by using the quadratic fitting method. Calibrating (e) L2130i's and (f) L1102i's  $[H_2O]$ -dependence by using the cubic fitting method. Calibrating (g) L2130i's and (h) L1102i's  $[H_2O]$ -dependence by using the quartic fitting method. Calibrating (i) L2130i's and (j) L1102i's  $[H_2O]$ -dependence by using the linear-surface fitting method. The blue dots on each plot represent data sets from two pairs of DI1 and DI2 calibration cycles (i.e., [3,4] and [7,8]) for obtaining each of the five calibration fittings. The respective 2D  $[H_2O]$ -dependence calibration fitting

Formatted: Font: Not Bold

Formatted: Font: (Default) Arial

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: (Default) Arial

Formatted: Font: Not Bold



derives from a relationship between measured H<sub>2</sub>O concentration and  $\delta^{18}\text{O}$  deviation, equivalent to a difference between a measurement value of  $\delta^{18}\text{O}$  at each of four concentration levels and that at 21,500 ppm level ( $=\delta^{18}\text{O}_{\text{Ref}}$ ) on each calibration (a-h). The 3D [H<sub>2</sub>O]-dependence calibration fitting also involves a measurement value of  $\delta^{18}\text{O}$  value at each concentration level as an independent variable (i-j). The red and green diamonds denote the actual observed  $\delta^{18}\text{O}$  deviations from unused DI1 (ID-5) and DI2 (ID-6) calibration cycles, respectively. The predicted  $\delta^{18}\text{O}$  deviations, denoted as open triangles, on each plot were calculated from each [H<sub>2</sub>O]-dependence calibration fitting, applied to measured H<sub>2</sub>O concentrations (2D fitting methods: a-h) or to both measured H<sub>2</sub>O concentration and  $\delta^{18}\text{O}$  (3D fitting method: i-j) during the unused calibration cycles. The RMSE value on each plot was calculated from a difference between actual observed and predicted deviation values of  $\delta^{18}\text{O}$ .

Formatted: Font: Not Bold

Formatted: Font: Not Bold

### 3 Results and Discussions

#### 3.1 Measurement precision over the two-week period

Figure 4 shows example times series of 7-min mean H<sub>2</sub>O concentration,  $\delta^{18}\text{O}$ , and  $\delta^2\text{H}$ , calculated from raw L2130i measurement data for the highest and lowest H<sub>2</sub>O concentrations (i.e., ~41,000 and ~21,500 ppm) over the entire DI1 standard water calibration runs for the two week period. The precision is defined as the standard deviation ( $\sigma$ ) of all the raw 7-min average values over the 24 calibrations. The temporal changes in measured H<sub>2</sub>O concentration at 21,500 ppm varied with  $\text{H}_2\text{O}-\sigma = 243.6$  ppm (1.1%) over the whole period, whereas the highest moisture condition (~41,000 ppm) had larger variation of H<sub>2</sub>O concentration ( $\text{H}_2\text{O}-\sigma: 653.9$  ppm or ~1.5%; Fig. 4). The larger variability at 41,000 ppm likely derived from difficulty in establishing and delivering a stable high moisture stream from the calibration unit to L2130i, and possibly residual memory effects inside the tube line and L2130's measurement cell even with the well-heated condition (cell temperature = 80 °C) due to the extremely high moisture (~40,000 ppm). One solution of the possible residual memory effects would be an increase in the tube-heater's temperature above 45 °C. In addition, the larger variation in H<sub>2</sub>O concentration at 41,000 ppm may have been influenced by instability of the calibration system and a saturation effect inside the cavity measuring H<sub>2</sub>O concentration near the upper limit (50,000 ppm). Moreover, the less stable H<sub>2</sub>O signal at the highest concentration level [H<sub>2</sub>O] results in lower precisions of  $\delta^{18}\text{O}$  ( $\sigma = 0.13\%$ ) and  $\delta^2\text{H}$  ( $\sigma = 0.68\%$ ) compared with at the lowest concentration level [H<sub>2</sub>O] ( $\delta^{18}\text{O}-\sigma = 0.09\%$  and  $\delta^2\text{H}-\sigma = 0.45\%$ ) (Fig. 4).

Table 1 summarizes the precision of  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  for each concentration level on each standard water for the L2130i and L1102i analysers. For both standard waters, the L2130i analyser had higher  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  precision than the L1102i analyser, likely due to the improved fitting algorithm used for the L2130i analyser (Aemisegger et al., 2012). In addition, the L2130i analyser had higher  $\delta^{18}\text{O}$  ( $\sigma < 0.11\%$ ) and  $\delta^2\text{H}$  ( $\sigma < 0.59\%$ ) precision under 30,000 ppm than over 30,000 ppm:  $\delta^{18}\text{O}-\sigma \geq 0.12\%$  and  $\delta^2\text{H}-\sigma \geq 0.68\%$  (Table 1). The L1102i analyser also had higher precision below 30,000 ppm relative to over 30,000 ppm except  $\delta^2\text{H}$  precision for DI2 (Table 1). These findings indicate that both analysers can measure stable water isotopes more precisely for water vapour samples below 30,000 ppm.

Across concentration levels for DI2, both analysers had the highest  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  measurement precision at 21,500 ppm level with the lowest H<sub>2</sub>O variation ( $\text{H}_2\text{O}-\sigma \leq 244.9$  ppm) except  $\delta^2\text{H}$  precision of L1102i. In contrast, for DI1, both analysers had the highest  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  measurement precision at 29,000 ppm even though variability in H<sub>2</sub>O concentration measurement was higher at 29,000 ppm ( $\text{H}_2\text{O}-\sigma \geq 578.6$  ppm) than at 21,500 ppm ( $\text{H}_2\text{O}-\sigma \leq 253.5$  ppm). The high measurement precision of L2130i and L1102i even with the larger H<sub>2</sub>O concentration variability indicates that the measurement precision of the L2130i and L1102i analysers was not largely influenced by the instability of the calibration unit. Furthermore, the L1102i's  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  precision at 21,500 ppm ( $\delta^{18}\text{O}-\sigma = 0.11\text{-}0.14\%$  and  $\delta^2\text{H}-\sigma = 0.99\text{-}1.01\%$ ) were similar or better than those reported by Delattre et al. (2015) at 20,000 ppm for the L1102i ( $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  precision of 0.08-0.19% and 1.5-2.0%

respectively based on 40 calibration data over 35 days). This proves that the calibration system has a negligible effect on the isotopic measurement precision for L2130i and L1102i analysers.

The larger variation in H<sub>2</sub>O concentration at 41,000 ppm also implies instability of the calibration system, which possibly induces a decline in measurement precision of δ<sup>18</sup>O and δ<sup>2</sup>H values for the CRDS analysers at high humidity. Table 1 summarizes the precision of δ<sup>18</sup>O and δ<sup>2</sup>H for each [H<sub>2</sub>O] on each standard water for the L2130i and L1102i analysers. The L2130i analyser has the highest precision of δ<sup>18</sup>O measurement for the DI1 standard water at 29,000 ppm even though variability in H<sub>2</sub>O concentration measurement was higher (H<sub>2</sub>O σ = 578.6 ppm at 29,000 ppm versus H<sub>2</sub>O σ = 243.6 at 21,000 ppm). Additionally, the L1102i analyser had higher δ<sup>18</sup>O and δ<sup>2</sup>H measurement precision at higher moisture conditions (≥ 29,000 ppm) than at the lowest moisture condition (= 21,500 ppm) for both the standard waters. The increase in measurement precision of L2130i and L1102i with [H<sub>2</sub>O], despite larger [H<sub>2</sub>O] variability, indicates that the instability of the calibration unit did not inherently exert a large influence on the measurement precision of the L2130i and L1102i analysers. Furthermore, the L1102i's δ<sup>18</sup>O and δ<sup>2</sup>H precision at 21,500 ppm (δ<sup>18</sup>O σ = 0.11–0.14‰ and δ<sup>2</sup>H σ = 0.99–1.01‰) were similar or better than those reported by Delattre et al. (2015) at 20,000 ppm for the L1102i (δ<sup>18</sup>O and δ<sup>2</sup>H precision of 0.08–0.19‰ and 1.5–2.0‰ respectively based on 40 calibration data over 35 days). This proves that the calibration system has a negligible effect on the isotopic measurement precision for L2130i and L1102i analysers.

At all H<sub>2</sub>O concentration levels, and for both standard waters, the L2130i analyser had higher δ<sup>18</sup>O (σ ≤ 0.11‰) and δ<sup>2</sup>H (σ ≤ 0.59‰) precision under 30,000 ppm than over 30,000 ppm: δ<sup>18</sup>O σ ≥ 0.12‰ and δ<sup>2</sup>H σ ≥ 0.68‰ (Table 1). This indicates that the L2130i analyser can measure stable water isotopes more precisely for water vapour samples below 30,000 ppm. Compared to the L2130i analyser, the L1102i analyser had higher precision for only δ<sup>18</sup>O below 30,000 ppm relative to over 30,000 ppm (Table 1). The different behaviour of both analysers described above would mainly be due to the old fitting algorithm used for the L1102i analyser (Aemisegger et al., 2012).

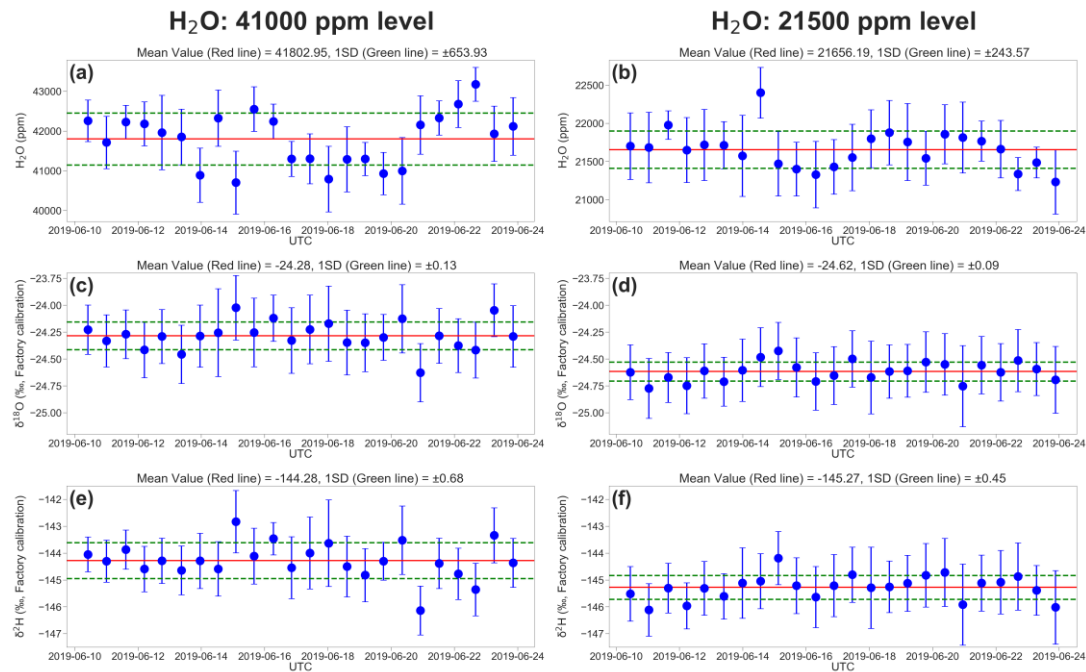


Figure 4 Two-week evolution of the L2130i's measurements for the DI1 standard water in (a) H<sub>2</sub>O concentration at 41,000 ppm level, (b) H<sub>2</sub>O concentration at 21,500 ppm level, (c) δ<sup>18</sup>O at 41,000 ppm level, (d) δ<sup>18</sup>O at 21,500 ppm level, (e) δ<sup>2</sup>H at

41,000 ppm level (a), and (f)  $\delta^2\text{H}$  at 21,500 ppm level (b). Each value is a 7-minute average of raw measurement data from the L2130i, and error bars are one standard deviation of 7-minutes. The red and green lines show the average and standard deviation through the 2-week measurement period.

### 5 3.2 Accuracy of isotope values for water vapour concentration dependence

For the L2130i analyser, the  $\delta^{18}\text{O}$  deviation of both standard waters from reference values at 21,500 ppm gradually increased with  $\text{H}_2\text{O}$  concentration, reaching a maximum median value of 0.32 ‰ for DI1 and of 0.28 ‰ for DI2 (Fig. 5a). For  $\delta^{18}\text{O}$ , these differences were significant for both standard waters between 41,000 and 36,000 or 29,000 ppm (Fig. 5a, Welch's t-test,  $p < 0.01$ ), but differences between 36,000 and 29,000 ppm were not significant (Fig. 5a, Welch's t-test,  $p > 0.09$ ). As with  $\delta^{18}\text{O}$ , the values of  $\delta^2\text{H}$  measured with the L2130i for both standard waters differed significantly between 41,000 ppm and the lower  $\text{H}_2\text{O}$  concentrations (Fig. 5b, Welch's t-test,  $p < 0.05$ ), without a significant difference between 29,000 ppm and 36,000 ppm (Fig. 5b, Welch's t-test,  $p > 0.86$ ). These results indicate accurate measurement of both  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  using the L2130i analyser require correction for  $[\text{H}_2\text{O}]$ -dependence under high moisture conditions ( $> 36,000$  ppm  $\text{H}_2\text{O}$ ).

The differences in the L2130i's deviation of each isotope from reference values at 21,500 ppm were similar for the two standard waters at all concentration levels except 41,000 ppm (Figs. 5a and 5b, Welch's t-test,  $p > 0.05$ ), where the L2130i indicated differences in  $\delta^2\text{H}$  deviation for the two different standard waters (Figs. 5a and 5b, Welch's t-test,  $p < 0.05$ ). This finding indicates that the L2130i's  $\delta^2\text{H}$  accuracy for high moisture like 41,000 ppm is dependent on the isotopic composition, such as has been found for low moisture conditions below 4,000 ppm (Weng et al., 2020). This result further indicates that more than one standard water needs to be used in the field under not only low moisture but also high moisture conditions. Additionally, the isotope dependence of  $\delta^2\text{H}$  accuracy may have related to the low suction flow rate of the L2130i (Thurnherr et al., 2020).

The  $[\text{H}_2\text{O}]$ -dependence of  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  accuracy also gives rise to uncertainty in deuterium excess (hereinafter called d-excess,  $\text{d-excess} = \delta^2\text{H} - 8\delta^{18}\text{O}$ ) values, estimated with the uncorrected  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  values (Figs. 5c and 5f). The d-excess deviation of the L2130i analyser significantly increased in a negative direction with concentration level on each standard water, and reached a maximum negative median value of -1.62 ‰ for DI1 and of -1.70 ‰ for DI2 (Fig. 5c). According to the calculation of d-excess, the decrease in d-excess with  $\text{H}_2\text{O}$  concentration mostly stemmed from the increase in the L2130i's  $\delta^{18}\text{O}$  values with  $\text{H}_2\text{O}$  concentration (Figs. 5a and 5c), which underlines the need for correcting for the  $[\text{H}_2\text{O}]$ -dependence, especially for  $\delta^{18}\text{O}$  accuracy at high concentration moisture levels using the L2130i analyser.

The L1102i also had strong  $[\text{H}_2\text{O}]$ -dependence for both isotopes, larger than that of the L2130i (Figs. 5a-b and 5d-e). The larger variations also led to large deviations in the d-excess values (Fig. 5f). In addition, both  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  accuracy for the L1102i depend on isotopic compositions ( $\delta^{18}\text{O}$ : 36,000 ppm,  $\delta^2\text{H}$ : all concentration levels  $[\text{H}_2\text{O}]$ ; Figs. 5d and 5e, Welch's t-test,  $p < 0.05$ ), different from the L2130i analyser. The above findings indicate that for the L1102i both  $\delta^2\text{H}$  and  $\delta^{18}\text{O}$  accuracy depend on  $\text{H}_2\text{O}$  concentration and the isotopic compositions, thus making the  $[\text{H}_2\text{O}]$ -dependence correction for both the  $\delta^2\text{H}$  and  $\delta^{18}\text{O}$  accuracy using different standard waters necessary.

The L1102i's result of  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  deviations were comparable with those reported by Tremoy et al. (2011) who checked  $[\text{H}_2\text{O}]$ -dependence on  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  accuracy for L1102i up to 39,000 ppm against the reference  $\text{H}_2\text{O}$  concentration at 20,000 ppm. However, Tremoy et al. (2011) observed negative  $\delta^{18}\text{O}$  deviations at 39,000 ppm with a range between -2 and 0 ‰, different from this study. In addition, they showed a smaller increase in  $\delta^2\text{H}$  deviations with  $\text{H}_2\text{O}$  concentration from 20,000 to 39,000 ppm than this study. The above differences in  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  deviations between Tremoy et al. (2011) and this study shows that  $[\text{H}_2\text{O}]$ -dependence of  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  accuracy must be evaluated for each individual analyser (Aemisegger et al., 2012; Bailey et al., 2015).

In summary, the measurement accuracy for in  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  is more dependent on  $\text{H}_2\text{O}$  concentration for the L1102i than the L2130i, mainly likely due to the older fitting algorithm for the initial version of the L1102i. In other words, the accuracy of  $[\text{H}_2\text{O}]$ -dependence of  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  for the L2130i has been improved due to the updated/corrected fitting algorithm (Aemisegger et al., 2012), but our results still remind us of the importance of correcting for the  $[\text{H}_2\text{O}]$ -dependence of  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  accuracy for the L2130i analyser, particularly for high moisture condition at 36,000 ppm and above.

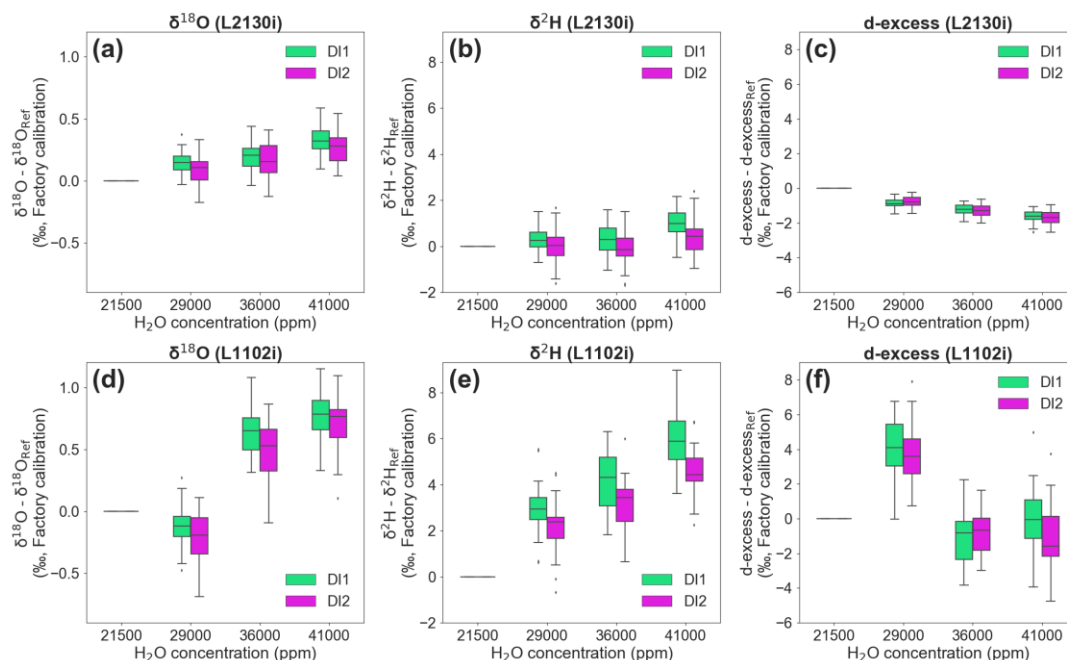


Figure 5 Deviations of stable isotopic compositions ( $\delta^{18}\text{O}$ ,  $\delta^2\text{H}$  and d-excess) for each standard water (DI1 and DI2) at three different  $\text{H}_2\text{O}$  concentrations compared to the 21,500 reference  $\text{H}_2\text{O}$  concentration. Boxplots of (a)  $\delta^{18}\text{O}$ , (b)  $\delta^2\text{H}$ , and (c) d-excess deviations, measured by L2130i. Boxplots of (d)  $\delta^{18}\text{O}$ , (e)  $\delta^2\text{H}$ , and (f) d-excess deviations, measured by L1102i. The  $\delta^{18}\text{O}$ ,  $\delta^2\text{H}$  and d-excess values at 21,500 ppm are assigned a value of 0, and  $[\text{H}_2\text{O}]$ -dependence for each isotope can be observed as the deviation between the value at each concentration level  $[\text{H}_2\text{O}]$  from the value measured at 21,500 ppm.

### 3.3 Strategy for calibration of isotope values for water vapour concentration dependence

The four calibration strategies for correcting isotope values using measured  $\text{H}_2\text{O}$  concentrations are compared in Figure 6. Across methods, the L2130i analyser usually displays lower median  $\delta^{18}\text{O}$  RMSE values compared to the L1102i analyser (Fig. 6). This tendency is also found in  $\delta^2\text{H}$  RMSE results on each calibration strategy (see Fig. S1 in the Supplement). The lower RMSE values of the L2130i analyser are mainly due to the higher precision of the L2130i analyser compared to the L1102i analyser, indicate that a  $[\text{H}_2\text{O}]$  dependence calibration increases accuracy of water vapour isotope measurements more for the L2130i analyser than the L1102i analyser. The lowest median RMSE for the L1102i analyser is the cubic fitting method (Figs. 6b, 6d, 6f and 6h). Among all the calibration strategies of the L1102i analyser, the DI1-2\*2Pairs calibration strategy with the cubic fitting method usually shows the minimum median RMSE value for  $\delta^{18}\text{O}$  accuracy (Fig. 6h). For  $\delta^2\text{H}$  accuracy of the L1102i analyser, the DI1-2\*2Pairs calibration strategy also usually displays lower median RMSE values relative to the other strategies. These results indicate that this calibration strategy is most appropriate for correcting  $[\text{H}_2\text{O}]$ -dependence and improving the accuracy of isotope measurements with the L1102i analyser.

Compared with the L1102i analyser, the DI1-2\*2Pairs calibration strategy of the L2130i analyser does not show clearly reduced isotopic RMSE values relative to the other calibration strategies, but still displays low RMSE values with a small distribution from each fitting method at each interval (Figs. 6a, 6c, 6e, 6g and S1). This indicates that the DI1-2\*2Pairs strategy can be utilized for correcting [H<sub>2</sub>O]-dependence of the L2130i analyser as well as the L1102i analyser. Since the calibration system uses the same tube line between the vaporizer and the branch point before the inlet port of each CRDS analysers (Fig. 1a), we decided to utilize the DI1-2\*2Pairs strategy for the L2130i analyser in the same way as the L1102i analyser.

Each CRDS analyser using the DI1-2\*2Pairs strategy shows the lowest median RMSE values of isotopic accuracy at the shortest interval (28 h), which only slightly increases with interval over 8 days (Figs. 6g and 6h). This indicates that one [H<sub>2</sub>O]-dependence calibration per week is enough to maintain good isotopic measurement of the CRDS analysers for an in-situ continuous observation remotely. According to the recent studies (Bonne et al., 2019; Weng et al., 2020), new CRDS models (e.g., L2130i and L2140i) did not show any significant changes for [H<sub>2</sub>O]-dependence from ~500 to 25,000 ppm over several months up to 2 years. The consistency of [H<sub>2</sub>O]-dependence may be extended to higher moisture conditions than 25,000 ppm, but based on our laboratory experiments, we decided to conduct the [H<sub>2</sub>O]-dependence calibration at weekly or less interval with the DI1-2\*2Pairs strategy. After we continuously run the ambient measurement and calibration systems at the ATTO site over several months, we will try to reduce the [H<sub>2</sub>O]-dependence calibration frequency to maximize the ambient sampling period while maintaining high measurement accuracy of both CRDS analysers. For both analysers using the DI1-2\*2Pairs strategy, the RMSE distribution of isotopic accuracy gradually gets smaller with interval over 8 days (Figs. 6g and 6h). The smaller RMSE distributions at long intervals result from larger sample numbers for calculating RMSE values at long intervals, whereas the larger RMSE distributions at short intervals are attributed to smaller sample numbers for calculating RMSE (e.g., 28 h with ID-[3,4] & [7,8]: n=8 (4 samples × 2 measurement cycles, i.e., ID-5,6), 196 h with ID-[3,4] & [31,32]: n=104 (4 samples × 26 measurement cycles, i.e., ID-5-30); c.f., Fig. 2b).

The respective CRDS analyser with the DI1-2\*2Pairs strategy also shows a similar range of RMSE among the five curve-fitting methods (Figs. 6g-h and S1g-h). The results do not clearly indicate which fitting method most frequently obtains the lowest RMSE values for each [H<sub>2</sub>O]-dependence calibration interval. Hence, for the DI1-2\*2Pairs strategy we obtained a [H<sub>2</sub>O]-dependence fitting method, which only obtained minimum RMSE values of δ<sup>18</sup>O and δ<sup>2</sup>H, from each two calibration pairs at each interval and then calculated a contribution rate of the respective five [H<sub>2</sub>O]-dependence fittings (i.e., linear, quadratic, cubic, quartic, linear surface fitting methods) to the total calibration pairs at each interval~~we report differences among fitting methods in detail only for the DI1-2\*2Pairs strategy~~ (Fig. 7). The linear-surface fitting method most frequently gives the lowest isotopic RMSE values, except δ<sup>18</sup>O accuracy of the L1102i analyser (i.e., cubic fitting method), at 28 h interval (Fig. 7). This indicates that the linear-surface fitting method at 28 h interval reduces uncertainties in correcting [H<sub>2</sub>O]-dependence on isotopic accuracy most effectively, except for δ<sup>18</sup>O accuracy of the L1102i analyser. Compared with 28 h interval, the 2D fitting methods are the most appropriate for calibrating [H<sub>2</sub>O]-dependence on isotopic accuracy over long intervals, excluding δ<sup>2</sup>H accuracy of the L1102i analyser (Fig. 7). The difference in fitting methods between 28 h and longer intervals suggests that the 28 h interval strategy can correct for both [H<sub>2</sub>O]- and isotope-dependent errors by using the 3D fitting method, whereas the long interval strategies can correct for only [H<sub>2</sub>O]-dependent errors with the 2D fitting methods.

~~Each CRDS analyser using the DI1-2\*2Pairs strategy shows the lowest median RMSE values of isotopic accuracy at the shortest interval (= 28 h), which only slightly increases with interval over 8 days (Fig. 6). This suggests that more frequent [H<sub>2</sub>O]-dependence calibrations in high moisture environments can improve δ<sup>18</sup>O and δ<sup>2</sup>H accuracy unless the frequent calibrations use up standard water on site. However, at remote field sites where logistics is restricted, the above findings for the interval period also support that one [H<sub>2</sub>O]-dependence calibration per week is enough to maintain good isotopic measurement of the CRDS analysers for an in situ continuous observation remotely. Additionally, the RMSE distribution of~~

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Font: Not Bold

isotopic accuracy gradually gets smaller with interval over 8 days (Fig. 6). The smaller RMSE distributions at long intervals result from larger sample numbers for calculating RMSE values at long intervals, whereas the larger RMSE distributions at short intervals is attributed to smaller sample numbers for calculating RMSE (28 h: n=43, 196 h: n=19; e.f., Fig. 2). Although our results suggest one [H<sub>2</sub>O] dependence calibration per week is enough, to be on the safe side, we decided to conduct the [H<sub>2</sub>O] dependence calibration at 28 h or less interval with the DI1-2\*2Pairs strategy. Figure 8 presents the corrected isotope deviations by the best fitting methods (L2130i-δ<sup>18</sup>O: linear fitting, L2130i and L1102i-δ<sup>2</sup>H: linear surface quadratic fitting, L1102i-δ<sup>18</sup>O: cubic fitting, L1102i-δ<sup>2</sup>H: linear-surface fitting) at weekly (i.e., 168~~28~~ h) interval by assuming the continuous operation at the ATTO site, discussed above. The isotope deviations of each CRDS analysers do not substantially vary with H<sub>2</sub>O concentration. This indicates the calibrations successfully corrected [H<sub>2</sub>O]-dependence of isotope accuracy for each analysers. Based on Moreira et al. (1997), water vapour isotope values in Amazon rainforest is expected to change diurnally by up to 2‰ (δ<sup>18</sup>O) or 4-8‰ (δ<sup>2</sup>H) with H<sub>2</sub>O concentration. The diel isotope variations are higher than the corrected deviation values of each CRDS analyser (Fig. 8). This supports that both the CRDS analysers will detect diel or probably seasonal/interannual variations in water vapour isotopes in Amazon rainforest.

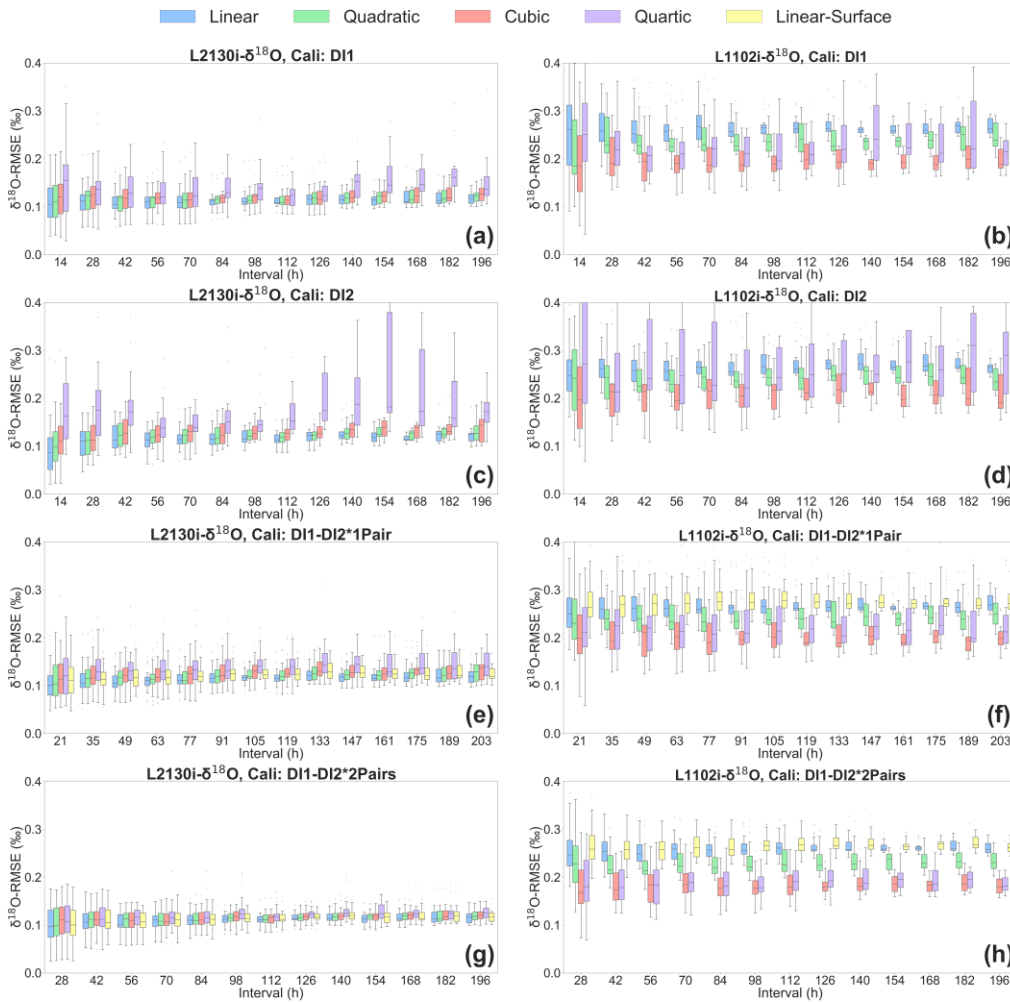


Figure 6 Boxplots of root mean square error (RMSE) of  $\delta^{18}\text{O}$ , derived from calibrating  $[\text{H}_2\text{O}]$ -dependence of  $\delta^{18}\text{O}$  measurements by each of five fitting methods (i.e., linear, quadratic, cubic, quartic, linear surface fitting methods) for each of four calibration strategies: DI1, DI2, DI1-DI2\*1Pair, DI1-2\*2Pairs. Boxplots of (a) L2130's and (b) L1102's  $\delta^{18}\text{O}$  RMSE for the DI1 strategy, depending on interval length (i.e., the time period used for calibrating  $[\text{H}_2\text{O}]$ -dependence). Boxplots of (c) L2130's and (d) L1102's  $\delta^{18}\text{O}$  RMSE for the DI2 strategy, depending on interval length. Boxplots of (e) L2130's and (f) L1102's  $\delta^{18}\text{O}$  RMSE for the DI1-DI2\*1Pair strategy, depending on interval length. Boxplots of (g) L2130's and (h) L1102's  $\delta^{18}\text{O}$  RMSE for the DI1-2\*2Pairs strategy, depending on interval length. The left hand figures present boxplots of RMSE of  $\delta^{18}\text{O}$  measurements by the L2130i, depending on interval length (i.e., the time period used for calibrating  $[\text{H}_2\text{O}]$ -dependence). The right hand figures display boxplots of RMSE of  $\delta^{18}\text{O}$  measurements by the L1102i, depending on interval length. The procedure for assessing  $[\text{H}_2\text{O}]$ -dependence uncertainties ( $\Rightarrow$ RMSE) is described in section 2.3.

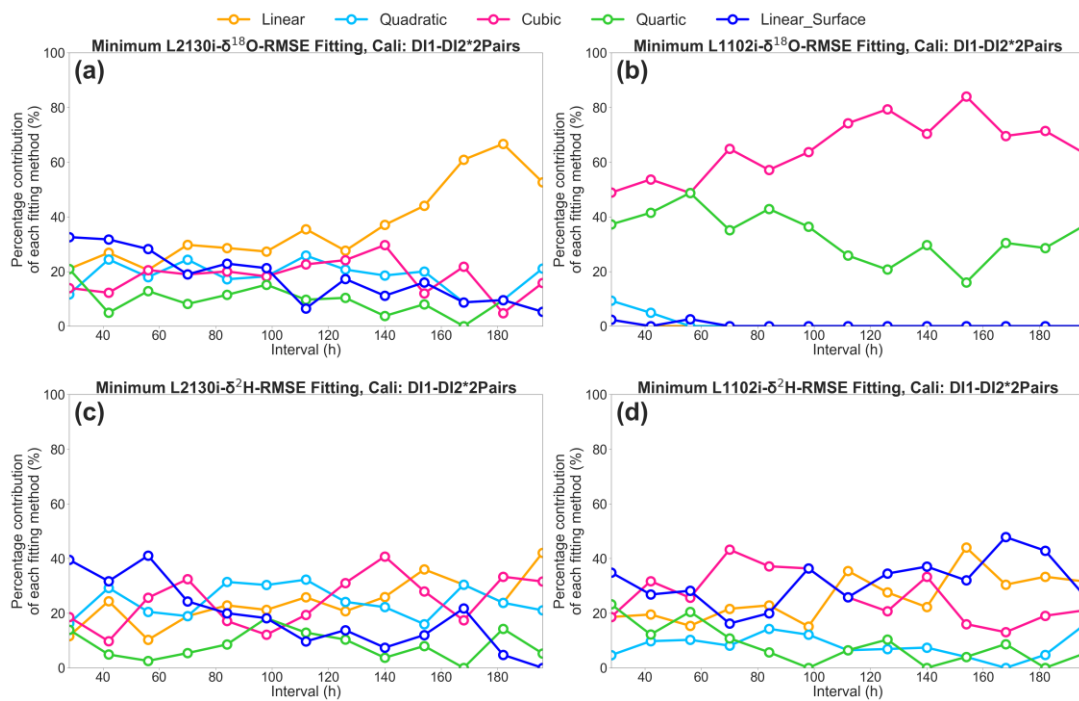


Figure 7 Percentage contribution of the respective five  $[\text{H}_2\text{O}]$ -dependence fittings (i.e., linear, quadratic, cubic, quartic, linear surface fitting methods) to the total calibration pairs, which only obtained minimum RMSE values of  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$ , at each interval for the DI1-2\*2Pairs calibration strategy. (a) L2130i's and (b) L1102i's results for  $\delta^{18}\text{O}$  RMSE. (c) L2130i's and (d) L1102i's results for  $\delta^2\text{H}$  RMSE. The left hand and right hand figures present results of the L2130i, and of the L1102i, respectively. The top and bottom figures present results of  $\delta^{18}\text{O}$  RMSE, and of  $\delta^2\text{H}$  RMSE, respectively.

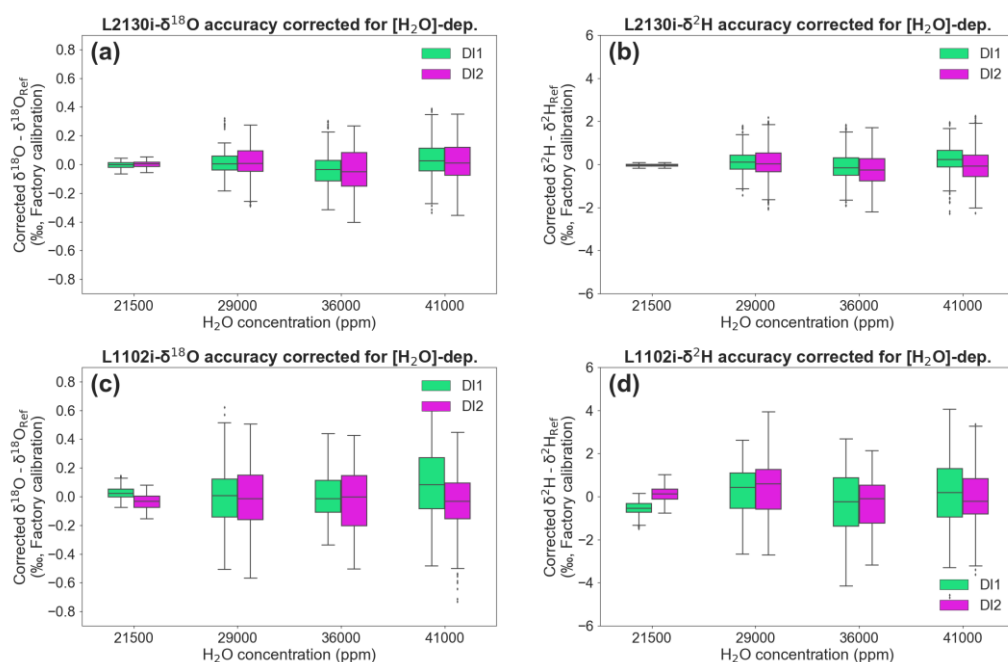


Figure 8 Deviations of  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$ , both corrected for [H<sub>2</sub>O]-dependence, for each standard water (DI1 and DI2) at four different H<sub>2</sub>O concentrations. Boxplots of (a)  $\delta^{18}\text{O}$  and (b)  $\delta^2\text{H}$  deviations, corrected for [H<sub>2</sub>O]-dependence of L2130i. Boxplots of (c)  $\delta^{18}\text{O}$  and (d)  $\delta^2\text{H}$  deviations, corrected for [H<sub>2</sub>O]-dependence of L1102i. The [H<sub>2</sub>O]-dependence of each CRDS analysers was corrected by the DI1-2\*2Pairs calibration strategy with the best fitting methods ([L2130i- \$\delta^{18}\text{O}\$ : linear fitting](#), [L2130i- \$\delta^2\text{H}\$ : quadratic fitting](#), [L1102i- \$\delta^{18}\text{O}\$ : cubic fitting](#), [L1102i- \$\delta^2\text{H}\$ : linear-surface fitting](#)) ([L2130i and L1102i- \$\delta^2\text{H}\$ : linear surface fitting](#), [L1102i- \$\delta^{18}\text{O}\$ : cubic fitting](#)) at 16828 h interval.

#### 4 Conclusions

This study extends previous work documenting water vapour concentration dependence of Picarro CRDS analysers to high moisture (> 35,000 ppm H<sub>2</sub>O) likely to be measured in the Amazon rainforest [and other tropical areas](#). We assessed the precision and accuracy of two CRDS analysers (i.e., model L1102i and L2130i) for concentration and isotopic measurements by using a custom-made calibration unit that regularly supplied standard water vapour samples at four different H<sub>2</sub>O concentrations between 21,500 and 41,000 ppm to the CRDS analysers. Our results demonstrate that the newer version of the analyser (L2130i) has better precision for both  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  measurements under all [H<sub>2</sub>O concentration levels](#) [moisture conditions](#) compared to the older model (L1102i). In addition, isotope measurements in both analysers varied with [H<sub>2</sub>O concentration](#) [moisture content](#), especially at [H<sub>2</sub>O concentration over](#)  $>36,000$  ppm. The concentration dependence of the L1102i analyser was stronger than the L2130i analyser. These findings indicate that calibrating the [H<sub>2</sub>O]-dependence of  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  measurements for both the CRDS analysers during field deployment in high atmospheric moisture areas such as tropical forests is important.

Assuming continuous in situ observation together with regular calibration in tropical Amazon rainforest, we devised four calibration strategies, adjusted to our custom-made calibration system, and then evaluated which [H<sub>2</sub>O]-dependence calibration procedure best improved the accuracy of  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  measurements for both the L2130i and L1102i analysers. The best [H<sub>2</sub>O]-dependence strategy was the DI1-2\*2Pairs strategy that required two pairs of a two-point calibration with different [concentration](#) [moisture](#) levels from 21,500 to 41,000 ppm. The 28 h interval strategy with the linear-surface fitting method leads to the most accurate measurements for both the CRDS analysers, except  $\delta^{18}\text{O}$  accuracy of the L1102i analyser



that required the cubic fitting method. In addition, [H<sub>2</sub>O]-dependence calibration uncertainties hardly changed at any interval over 8 days. That indicates one [H<sub>2</sub>O]-dependence calibration per week is sufficient for correcting moisture-biased isotopic accuracy of the CRDS analysers. ~~Nevertheless, to stay on the safe side~~ ~~Therefore, we decided to conduct the [H<sub>2</sub>O]-dependence calibration at weekly 28 h or less interval.~~ The best calibration strategy at weekly 28 h interval also supported that both ~~the~~ CRDS analysers can sufficiently distinguish temporal variations of water vapour isotopes in the aimed ATTO site. In addition, since the recent studies indicate the consistency of the [H<sub>2</sub>O]-dependence for the CRDS analysers over several months up to 2 years, we intend to determine the appropriate frequency for calibrating [H<sub>2</sub>O]-dependence under high moisture conditions after a continuous operation over several months at the ATTO site to maximize the ambient sampling period.

## 10 Data availability

All the data used in this publication are freely available at the “<https://dx.doi.org/10.17617/3.4n>.”

## Author contribution

The calibration system was designed and developed by SK, JL, TS and US. The laboratory experiments were conducted by SK with assistance from JL, TS, US and FK. The IRMS analysis was done by HM and HG. DW helped us to check water vapour concentration in the ATTO site. SK conducted the data-analysis and wrote the manuscript with assistance from JL, FK, and HM. SK wrote the manuscript with contributions from all co-authors.

## Competing interests

The authors declare that they have no conflict of interest.

## Acknowledgements

This research was supported by German-Brazilian project ATTO, supported by the German Federal Ministry of Education and Research (BMBF contracts 01LB1001A and FKR 01LK1602A) and the Brazilian Ministério da Ciência, Tecnologia e Inovação (MCTI/FINEP contract 01.11.01248.00) as well as the Max-Planck Society. We are grateful to Susan Trumbore (MPI-BGC) for reviewing the earlier manuscript and her valuable feedback, to Stefan Wolff and Matthias Sörgel (MPI-Chemistry) for helping us to check H<sub>2</sub>O concentration in the ATTO site, and also to Jürgen M. Richter (MPI-BGC) for helping us to prepare the DI1 and DI2 standard waters.

## References

- Aemisegger, F., Sturm, P., Graf, P., Sodemann, H., Pfahl, S., Knohl, A. and Wernli, H.: Measuring variations of  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  in atmospheric water vapour using two commercial laser-based spectrometers: An instrument characterisation study, *Atmospheric Measurement Techniques*, 5(7), 1491–1511, doi:10.5194/amt-5-1491-2012, 2012.
- [Aemisegger, F., Vogel, R., Graf, P., Dahinden, F., Villiger, L., Jansen, F., Bony, S., Stevens, B. and Wernli, H.: How Rossby wave breaking modulates the water cycle in the North Atlantic trade wind region, \*Weather and Climate Dynamics Discussions\*, 1–47, doi:10.5194/wcd-2020-51, 2020.](#)

- Andreae, M. O., Acevedo, O. C., Araújo, A., Artaxo, P., Barbosa, C. G. G., Barbosa, H. M. J., Brito, J., Carbone, S., Chi, X., Cintra, B. B. L., da Silva, N. F., Dias, N. L., Dias-Júnior, C. Q., Ditas, F., Ditz, R., Godoi, A. F. L., Godoi, R. H. M., Heimann, M., Hoffmann, T., Kesselmeier, J., Könemann, T., Krüger, M. L., Lavric, J. V., Manzi, A. O., Lopes, A. P., Martins, D. L., Mikhailov, E. F., Moran-Zuloaga, D., Nelson, B. W., Nölscher, A. C., Santos Nogueira, D., Piedade, M. T. F., Pöhlker, C., Pöschl, U., Quesada, C. A., Rizzo, L. V., Ro, C.-U., Ruckteschler, N., Sá, L. D. A., de Oliveira Sá, M., Sales, C. B., dos Santos, R. M. N., Saturno, J., Schöngart, J., Sörgel, M., de Souza, C. M., de Souza, R. A. F., Su, H., Targhetta, N., Tóta, J., Trebs, I., Trumbore, S., van Eijck, A., Walter, D., Wang, Z., Weber, B., Williams, J., Winderlich, J., Wittmann, F., Wolff, S. and Yáñez-Serrano, A. M.: The Amazon Tall Tower Observatory (ATTO): overview of pilot measurements on ecosystem ecology, meteorology, trace gases, and aerosols, *Atmos. Chem. Phys.*, 15(18), 10723–10776, doi:10.5194/acp-15-10723-2015, 2015.
- Bailey, A., Tooney, D. and Noone, D.: [Characterizing moisture exchange between the Hawaiian convective boundary layer and free troposphere using stable isotopes in water, \*Journal of Geophysical Research: Atmospheres\*, 118\(15\), 8208–8221, doi:10.1002/jgrd.50639, 2013.](#)
- Bailey, A., Noone, D., Berkelhammer, M., Steen-Larsen, H. C. and Sato, P.: The stability and calibration of water vapor isotope ratio measurements during long-term deployments, *Atmos. Meas. Tech.*, 8(10), 4521–4538, doi:10.5194/amt-8-4521-2015, 2015.
- Coe, M. T., Macedo, M. N., Brando, P. M., Lefebvre, P., Panday, P. and Silvério, D.: The Hydrology and Energy Balance of the Amazon Basin, in *Interactions Between Biosphere, Atmosphere and Human Land Use in the Amazon Basin*, edited by L. Nagy, B. R. Forsberg, and P. Artaxo, pp. 35–53, Springer, Berlin, Heidelberg., 2016.
- Craig, H. and Gordon, L. I.: [Deuterium and oxygen 18 variations in the ocean and the marine atmosphere, 1965.](#)
- Dansgaard, W.: [Stable isotopes in precipitation, \*Tellus\*, 16\(4\), 436–468, doi:10.1111/j.2153-3490.1964.tb00181.x, 1964.](#)
- Delattre, H., Vallet-Coulomb, C. and Sonzogni, C.: Deuterium excess in the atmospheric water vapour of a Mediterranean coastal wetland: regional vs. local signatures, *Atmos. Chem. Phys.*, 15(17), 10167–10181, doi:10.5194/acp-15-10167-2015, 2015.
- Galewsky, J., Steen-Larsen, H. C., Field, R. D., Worden, J., Risi, C. and Schneider, M.: Stable isotopes in atmospheric water vapor and applications to the hydrologic cycle: ISOTOPES IN THE ATMOSPHERIC WATER CYCLE, *Rev. Geophys.*, 54(4), 809–865, doi:10.1002/2015rg000512, 2016.
- Gehre, M., Geilmann, H., Richter, J., Werner, R. A. and Brand, W. A.: Continuous flow  $^2\text{H}/^1\text{H}$  and  $^{18}\text{O}/^{16}\text{O}$  analysis of water samples with dual inlet precision, *Rapid Communications in Mass Spectrometry*, 18(22), 2650–2660, doi:10.1002/rcm.1672, 2004.
- González, Y., Schneider, M., Dyroff, C., Rodríguez, S., Christner, E., García, O. E., Cuevas, E., Bustos, J. J., Ramos, R., Guirado-Fuentes, C., Barthlott, S., Wiegele, A. and Sepúlveda, E.: [Detecting moisture transport pathways to the subtropical North Atlantic free troposphere using paired  \$\text{H}\_2\text{O}\$ - \$\delta\text{D}\$  in situ measurements, \*Atmospheric Chemistry and Physics\*, 16\(7\), 4251–4269, doi:10.5194/acp-16-4251-2016, 2016.](#)
- Helliker, B. R. and Noone, D.: Novel Approaches for Monitoring of Water Vapor Isotope Ratios: Plants, Lasers and Satellites, in *Isoscapes: Understanding movement, pattern, and process on Earth through isotope mapping*, edited by J. B. West, G. J. Bowen, T. E. Dawson, and K. P. Tu, pp. 71–88, Springer Netherlands, Dordrecht., 2010.
- IAEA/WMO: <https://nucleus.iaea.org/wiser>, last access: 30 July 2020.
- Intergovernmental Panel on Climate Change, Ed.: *Detection and attribution of climate change: From global to regional*, in *Climate change 2013 - the physical science basis*, pp. 867–952, Cambridge University Press, Cambridge., 2014.
- Matsui, E., Salati, E., Ribeiro, M. N. G., Reis, C. M., Tancredi, A. C. S. N. F. and Gat, J. R.: Precipitation in the Central Amazon basin:-The isotopic composition of rain and atmospheric moisture at Belém and Manaus, *Acta Amaz.*, 13(2), 307–369, doi:10.1590/1809-43921983132307, 1983.

Moreira, M., Sternberg, L., Martinelli, L., Victoria, R., Barbosa, E., Bonates, L. and Nepstad, D.: Contribution of transpiration to forest ambient vapour based on isotopic measurements. *Global Change Biology*, 3(5), 439-450, doi: 10.1046/j.1365-2486.1997.00082.x, 1997.

~~Schmidt, M., Maseyk, K., Bariac, T. and Seibt, U.: Concentration effects on laser based  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  measurements and implications for the calibration of vapour measurements with liquid standards, *Rapid Commun. Mass Spectrom.*, 9, doi:10.1002/rcm.4813, 2010.~~

Steen-Larsen, H. C., Sveinbjörnsdóttir, A. E., Peters, A. J., Masson-Delmotte, V., Guishard, M. P., Hsiao, G., Jouzel, J., Noone, D., Warren, J. K. and White, J. W. C.: Climatic controls on water vapor deuterium excess in the marine boundary layer of the North Atlantic based on 500 days of in situ, continuous measurements, *Atmos. Chem. Phys.*, 14(15), 7741–7756, doi:10.5194/acp-14-7741-2014, 2014.

Pfahl, S., Wernli, H. and Yoshimura, K.: The isotopic composition of precipitation from a winter storm – a case study with the limited-area model COSMO<sub>iso</sub>, *Atmos. Chem. Phys.*, 12(3), 1629–1648, doi:10.5194/acp-12-1629-2012, 2012.

Rella, C. W.: Accurate Greenhouse Gas Measurements in Humid Gas Streams Using the Picarro G1301 Carbon Dioxide/Methane/Water Vapor Gas Analyzer, Picarro, Inc., Santa Clara, CA, USA, available at: [https://www.picarro.com/support/library/documents/accurate\\_greenhouse\\_gas\\_measurements\\_in\\_humid\\_gas\\_streams\\_using\\_the\\_g1301](https://www.picarro.com/support/library/documents/accurate_greenhouse_gas_measurements_in_humid_gas_streams_using_the_g1301) (last access: 11 December 2020), 2010.

Rella, C. W., Chen, H., Andrews, A. E., Filges, A., Gerbig, C., Hatakka, J., Karion, A., Miles, N. L., Richardson, S. J., Steinbacher, M., Sweeney, C., Wastine, B. and Zellweger, C.: High accuracy measurements of dry mole fractions of carbon dioxide and methane in humid air, *Atmospheric Measurement Techniques*, 6(3), 837–860, doi:10/gb8sm2, 2013.

Risi, C., Bony, S., Vimeux, F. and Jouzel, J.: Water-stable isotopes in the LMDZ4 general circulation model: Model evaluation for present-day and past climates and applications to climatic interpretations of tropical isotopic records, *Journal of Geophysical Research: Atmospheres*, 115(D12), doi:10.1029/2009JD013255, 2010.

~~Schmidt, M., Maseyk, K., Bariac, T. and Seibt, U.: Concentration effects on laser-based  $\delta^{18}\text{O}$  and  $\delta^2\text{H}$  measurements and implications for the calibration of vapour measurements with liquid standards, *Rapid Commun. Mass Spectrom.*, 9, doi:10.1002/rcm.4813, 2010.~~

Steen-Larsen, H. C., Sveinbjörnsdóttir, A. E., Peters, A. J., Masson-Delmotte, V., Guishard, M. P., Hsiao, G., Jouzel, J., Noone, D., Warren, J. K. and White, J. W. C.: Climatic controls on water vapor deuterium excess in the marine boundary layer of the North Atlantic based on 500 days of in situ, continuous measurements, *Atmos. Chem. Phys.*, 14(15), 7741–7756, doi:10.5194/acp-14-7741-2014, 2014.

Thurnherr, I., Kozachek, A., Graf, P., Weng, Y., Bolshiyarov, D., Landwehr, S., Pfahl, S., Schmale, J., Sodemann, H., Steen-Larsen, H. C., Toffoli, A., Wernli, H. and Aemisegger, F.: Meridional and vertical variations of the water vapour isotopic composition in the marine boundary layer over the Atlantic and Southern Ocean, *Atmospheric Chemistry and Physics*, 20(9), 5811–5835, doi:10.5194/acp-20-5811-2020, 2020.

Tremoy, G., Vimeux, F., Cattani, O., Mayaki, S., Souley, I. and Favreau, G.: Measurements of water vapor isotope ratios with wavelength-scanned cavity ring-down spectroscopy technology: New insights and important caveats for deuterium excess measurements in tropical areas in comparison with isotope-ratio mass spectrometry, *Rapid Commun. Mass Spectrom.*, 25(23), 3469–3480, doi:10.1002/rcm.5252, 2011.

[Tremoy, G., Vimeux, F., Mayaki, S., Souley, I., Cattani, O., Risi, C., Favreau, G. and Oi, M.: A 1-year long  \$\delta^{18}\text{O}\$  record of water vapor in Niamey \(Niger\) reveals insightful atmospheric processes at different timescales. \*Geophysical Research Letters\*, 39\(8\), doi:10.1029/2012GL051298, 2012.](#)

Wei, Z., Lee, X., Aemisegger, F., Benetti, M., Berkelhammer, M., Casado, M., Caylor, K., Christner, E., Dyrhoff, C., García, O., González, Y., Griffis, T., Kurita, N., Liang, J., Liang, M.-C., Lin, G., Noone, D., Gribanov, K., Munksgaard, N. C., Schneider, M., Ritter, F., Steen-Larsen, H. C., Vallet-Coulomb, C., Wen, X., Wright, J. S., Xiao, W. and Yoshimura, K.: A global database of water vapor isotopes measured with high temporal resolution infrared laser spectroscopy, *Sci Data*, 6(1), 180302, doi:10.1038/sdata.2018.302, 2019.

[Werner, M., Langebroek, P. M., Carlsen, T., Herold, M. and Lohmann, G.: Stable water isotopes in the ECHAM5 general circulation model: Toward high-resolution isotope modeling on a global scale. \*Journal of Geophysical Research: Atmospheres\*, 116\(D15\), doi:10.1029/2011JD015681, 2011.](#)

[Weng, Y., Touzeau, A. and Sodemann, H.: Correcting the impact of the isotope composition on the mixing ratio dependency of water vapour isotope measurements with cavity ring-down spectrometers. \*Atmospheric Measurement Techniques\*, 13\(6\), 3167–3190, doi:10.5194/amt-13-3167-2020, 2020.](#)

## S1 IRMS methodology

The  $\delta^2\text{H}$  and  $\delta^{18}\text{O}$  measurements were done on a Delta<sup>+</sup>XL isotope ratio mass spectrometer coupled to a high-temperature conversion reactor (HTC) via a ConFloIII. The analysis method is described in Gehre et al. (2004). A daily sequence consisted of the DI1 or DI2 water samples, an in-house reference standard www-j1 (Willi Working Water-Jena1;  $\delta^2\text{H}$ :  $-66.45 \pm 1.0$  ‰,  $\delta^{18}\text{O}$ :  $-9.78 \pm 0.10$  ‰), an in-house scaling standard BGP-j1 (Brand Greenland Precipitation-Jena1;  $\delta^2\text{H}$ :  $-187.94 \pm 1.0$  ‰,  $\delta^{18}\text{O}$ :  $-24.46 \pm 0.10$  ‰), and an in-house quality control RWB-j1 (ReinstWasser Brand-Jena1;  $\delta^2\text{H}$ :  $-1 \pm 1.0$  ‰,  $\delta^{18}\text{O}$ :  $7.8 \pm 0.10$  ‰). The daily average standard deviation of www-j1 was better than 0.16 ‰ (n = 44) for  $\delta^{18}\text{O}$ , and better than 0.7 ‰ (n = 41) for  $\delta^2\text{H}$  measurements. All in-house standards are regularly calibrated and checked against the international IAEA standards VSMOW2 and SLAP2. Thus the DI1 and DI2 isotope values are given on the VSMOW/SLAP scale.

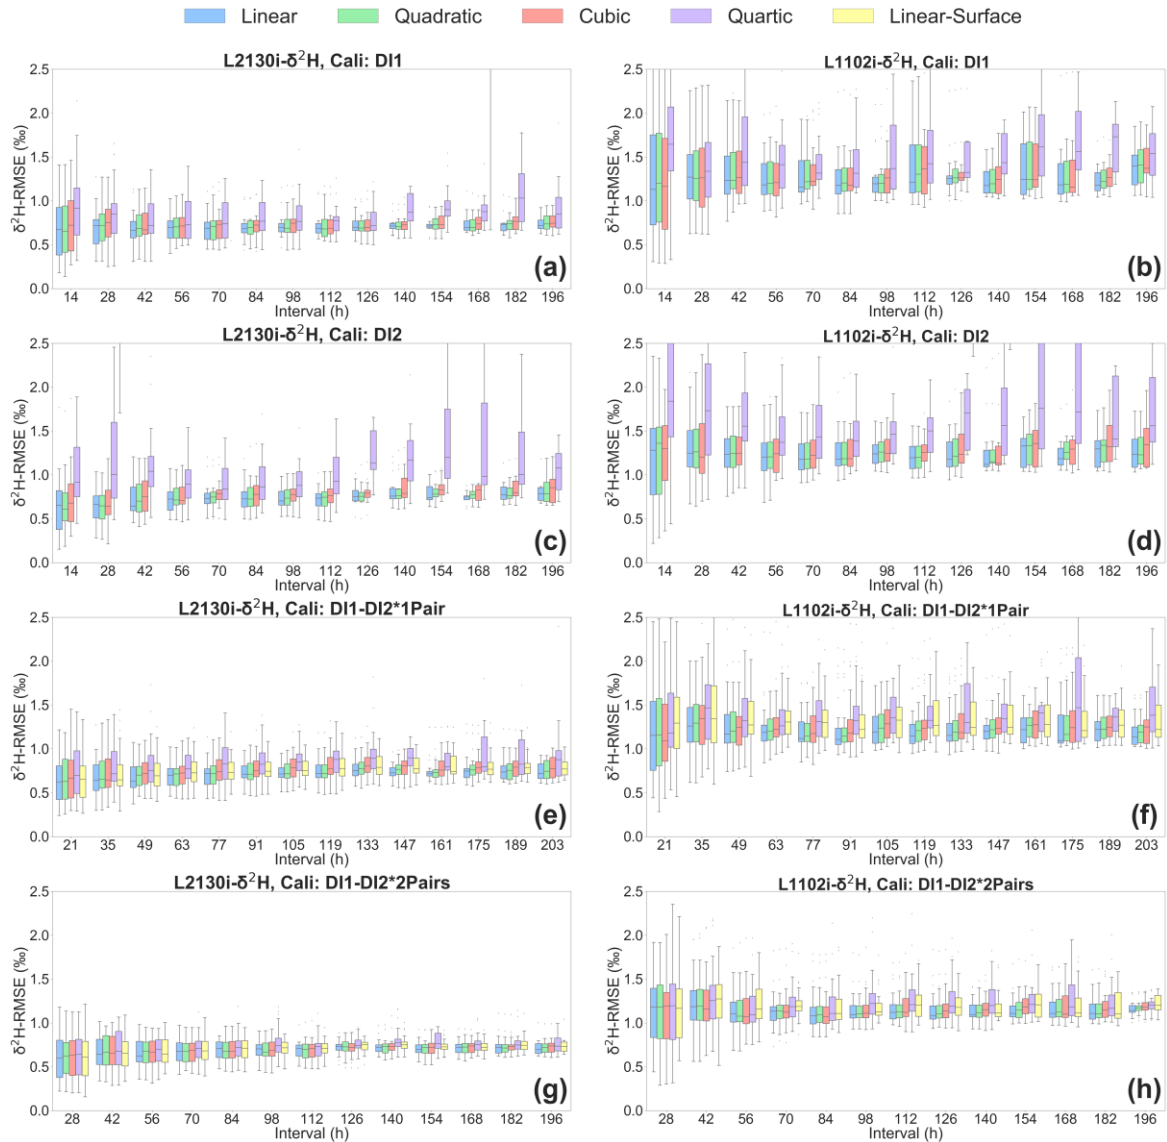


Figure S1 Boxplots of root mean square error (RMSE) of  $\delta^{2\text{H}}_{\text{OH}}$ , derived from calibrating  $[\text{H}_2\text{O}]$ -dependence of  $\delta^{2\text{H}}$  measurements by each of five fitting methods (i.e., linear, quadratic, cubic, quartic, linear surface fitting methods) for each of four calibration strategies: DI1, DI2, DI1-DI2\*1Pair, DI1-DI2\*2Pairs. Boxplots of (a) L2130's and (b) L1102's  $\delta^{2\text{H}}$  RMSE for the DI1 strategy, depending on interval length (i.e., the time period used for calibrating  $[\text{H}_2\text{O}]$ -dependence). Boxplots of (c) L2130's and (d) L1102's  $\delta^{2\text{H}}$  RMSE for the DI2 strategy, depending on interval length. Boxplots of (e) L2130's and (f) L1102's  $\delta^{2\text{H}}$  RMSE for the DI1-DI2\*1Pair strategy, depending on interval length. Boxplots of (g) L2130's and (h) L1102's  $\delta^{2\text{H}}$  RMSE for the DI1-DI2\*2Pairs strategy, depending on interval length. The left hand figures present boxplots of RMSE of  $\delta^{2\text{H}}$  measurements by the L2130i, depending on interval length (i.e., the time period used for calibrating  $[\text{H}_2\text{O}]$ -dependence). The right hand figures display boxplots of RMSE of  $\delta^{18}\text{O}$  measurements by the L1102i, depending on interval length. The procedure for assessing  $[\text{H}_2\text{O}]$ -dependence uncertainties (= RMSE) is described in section 2.3.

## References

Gehre, M., Geilmann, H., Richter, J., Werner, R. A. and Brand, W. A.: Continuous flow  $^2\text{H}/^1\text{H}$  and  $^{18}\text{O}/^{16}\text{O}$  analysis of water samples with dual inlet precision, *Rapid Communications in Mass Spectrometry*, 18(22), 2650–2660, doi:10.1002/rcm.1672, 2004.