

A dedicated robust instrument for water vapor generation at low-humidity for use with a laser water isotope analyzer in cold and dry polar regions.

Christophe Leroy-Dos Santos¹, Mathieu Casado^{1,2}, Frédéric Prié¹, Olivier Jossoud¹, Erik Kerstel³, Morgane Farradèche¹, Samir Kassi³, Elise Fourré¹, Amaëlle Landais^{1,*}

¹ Laboratoire des Sciences du Climat et de l'Environnement, CEA-CNRS-UVSQ-Paris Saclay-IPSL, Gif-sur-Yvette, France

² Alfred Wegener Institut, Helmholtz Center for Polar and Marine Research, Potsdam, Germany

³ Laboratoire Interdisciplinaire de Physique, CNRS - Université Grenoble Alpes, Grenoble, France

* corresponding author: amaelle.landais@lsce.ipsl.fr

Abstract

Obtaining precise continuous measurements of water vapor isotopic composition in dry places (polar or high-altitude regions) is an important challenge. The current limitation is the strong influence of humidity on the measured water isotopic composition by laser spectroscopy instruments for low-humidity levels (below 3,000 ppmv). This problem is addressed by determining the relationships between humidity and measured $\delta^{18}\text{O}$ and δD of known water standards. We present here the development of a robust field instrument able to generate water vapor, down to 70 ppmv, at very stable humidity levels (average 1σ lower than 10 ppmv). This instrument, operated by a Raspberry interface, can be coupled to a commercial laser spectroscopy instrument. We checked the stability of the system as well as its accuracy when expressing the measured isotopic composition of water vapor on the VSMOW-VSLAP scale. It proved to be highly stable during autonomous operation over more than one year at the East Antarctic Concordia and Dumont d'Urville stations.

1. Introduction

The recent development of laser spectroscopy instruments now enables the continuous measurement of the isotopic composition of water vapor at many observation stations all around the world (Bailey et al., 2015; Bastrikov et al., 2014; Schmidt et al., 2010; Sodemann et al., 2017; Tremoy et al., 2011). In particular, the isotopic composition of the water vapor has proven to be a very useful tool to document moist synoptic events in many locations (Bonne et al., 2014; Guilpart et al., 2017). In polar regions, the water vapor isotopic signal is not only useful to detect the origin of moist air (Bréant et al., 2019; Kopec et al., 2014) but also to improve the interpretation of the isotopic composition of water in surface snow and ice core archives (Steen-Larsen et al., 2014). Indeed, exchanges are occurring after deposition between the surface

snow and the water vapor leading to modifications of the isotopic composition of the former and hence of the archived ice (Casado et al., 2016, 2018; Ritter et al., 2016).

Obtaining continuous and accurate measurements of the water vapor isotopic composition expressed on the VSMOW-VSLAP scale measurements of the water vapor isotopic composition at Concordia station in central Antarctica is a key scientific challenge since the deep ice core drilled there, EPICA Dome C, provides the oldest continuous water isotopic record expressed on the VSMOW-VSLAP scale to date (Jouzel et al., 2007). It is thus a key reference for the study of past climate, and a correct interpretation of the isotopic record relies on the quantification of the transfer function between climate parameters and water isotopic composition in ice, itself influenced by exchanges with water vapor in the upper layers of the firn (Casado et al., 2018). Such knowledge is also of uttermost importance for the interpretation of water isotope records from the starting deep drilling project “Beyond EPICA-Oldest Ice” (<https://www.beyondepica.eu>), whose aim is to drill a 1.5-million-year old ice core at the Little Dome C site located 40 km away from Concordia station, hence with similar low temperature and humidity conditions.

One of the main limitations of the current commercial instruments when deployed in polar regions is their relatively poor performance at low water vapor concentration. Generally, the precision of the measured isotopic ratios $\delta^{18}\text{O}$ and δD rapidly worsens when the water mixing ratio decreases to humidity levels below 3,000-5,000 ppmv (part-per-million per volume) (Bonne et al., 2014; Weng et al., 2020). However, in remote continental areas in Greenland and Antarctica, temperatures in winter can drop to very low values, leading to humidity levels down to 10 ppmv (Genthon et al., 2017). Arguably one of the most extreme experiments for continuous measurement of the water vapor isotopic composition was the deployment of a commercial Picarro L2130-i instrument at the East Antarctic French-Italian station of Concordia where the mean annual temperature is around -54°C and the humidity barely exceeds 1,000 ppmv during the warmest summer days (Casado et al., 2016). For such applications, there are two major impacts of low-humidity on the raw isotopic signal: first, we generally observe an apparent increase in the $\delta^{18}\text{O}$ and δD with decreasing humidity level and second, the standard deviation associated with the continuous measurements of $\delta^{18}\text{O}$ and δD of the water vapor increases. This can lead to overall uncertainties of several ‰ for $\delta^{18}\text{O}$ and tens of ‰ for δD . It is thus of uttermost importance to have a correct determination of the humidity dependency of the water vapor isotopic ratios.

Commercial instruments from Picarro Inc. are usually associated with a Picarro Standard Delivery Module (SDM) designed to generate humidity at stable levels between 5,000 and 30,000 ppmv. Using such a set-up for humidity levels below 5,000 ppmv leads to large uncertainties in the determination of the humidity influence on the water vapor isotopic composition (e.g. Guilpart et al., 2017). These uncertainties are due both to the instability of the water vapor generation using the SDM (in terms of water concentration – humidity – and/or isotopic composition) and to the analytical noise in the spectroscopy measurements when the absorption signals are weak. An alternative commercial device is the LGR (Los Gatos Research)

calibration system (Water Vapor Isotope Standard Source, WVISS), which uses a nebulizer to instantaneously evaporate micro-droplets of liquid water from a standard reservoir into a large (1 L) vaporizing chamber (Dong and Baer, 2010). This system is very stable and well adapted for a humidity range between 2,500 and 25,000 ppmv (Aemisegger et al., 2012).

Several home-made water vapor injection systems have been developed with the specific aim to achieve a better stability of the generated humidity at low-humidity levels. A first approach is to use a dew point generator injecting small amounts of water into dry air (Lee et al., 2005; Wang et al., 2009). This approach is time consuming as it takes long to reach equilibrium and relies on a very precise knowledge of the temperature to quantify the isotopic fractionation. A method using a piezoelectric microdroplet generator into a dry air stream could generate water mixing ratios between 12 and 3,500 ppmv (Iannone et al., 2009; Sturm and Knohl, 2009; Sayres et al., 2009). However, adjustment of humidity level and long-term stability were difficult to obtain with such devices. Systems relying on the use of syringe pumps were also built by Gkinis et al. (2010) and Tremoy et al. (2011): a small fraction of the input stream of liquid water is introduced into a hot oven where water is vaporized in the presence of a dry air flow. These systems cover humidity range between 2,000 and 30,000 ppmv. Finally, bubbler systems, in which dry air flows through a large volume of water to create saturated vapor, are very robust but can only produce water vapor at high-humidity levels (Ellehoj et al., 2013). The aforementioned devices are unfortunately not well suited for automatic long-term operation at low-humidity levels. During the 2014-2015 summer field season at Concordia station in Antarctica, a home-made humidity generator specifically designed for low-humidity levels (Landsberg, 2014) has been deployed (Casado et al., 2016). The device used dual high-precision, low-volume, syringe pumps to generate stable humidity levels at two different isotopic compositions over the range from 100 to 800 ppmv (Casado et al., 2016). Unfortunately, we observed quite a large scattering among the isotopic values measured at similar humidity levels, as well as a large discrepancy between the humidity dependency of the water isotopic ratios measured in the field and the one measured in the laboratory. Upon return to the laboratory, these defaults were traced primarily to tiny leaks in the water supply lines to the syringes.

Therefore, we re-engineered the prototype by Landsberg (2014) in order to develop a robust and autonomous device for stable low-level humidity generation for the purpose of precise humidity calibration of spectroscopic instruments. Such devices have now been operating with minimum manual intervention for more than one year at two polar stations in Antarctica, Dumont d'Urville and Concordia, coupled to Picarro laser spectroscopy instruments. We detail here the technical description of the instrument and show key performance characteristics, enabling, for instance, a discussion of small amplitude signals such as the diurnal variability of the water vapor isotopic composition in remote dry sites in East Antarctica.

2. New vapor generator for low-humidity levels

The low-humidity level generator (LHLG) developed here relies on the same principle as the one developed by Landsberg (2014), i.e., a steady, undersaturated evaporation of a liquid water droplet at the tip of a needle into a dry air stream inside a small evaporation chamber. Based on this first prototype, the instrument has been remodeled including a specific hardware and software design.

2-1-Physical principle

The LHLG is based on undersaturated evaporation of a small droplet at the tip of a needle (Figure 1). Liquid water is pushed through a needle around which dry air is flowing. Dry air is obtained from a bottle of high purity synthetic air with pressure regulation through two manometers connected in series. The mass flux of water f_L is kept low compared to the air mass flow f_A so that the relative humidity RH of the downstream moist air flow remains low ($RH < 0.1$). Therefore, the air stays largely undersaturated and its humidity is controlled only by the flow of liquid water in the needle and that of the dry air upstream of it. The mixing ratio (or humidity) of the air as classically provided by a Picarro instrument is given by:

$$MR = \frac{d_{H_2O} \times f_L \times R \times T_{st}}{f_A \times P_{st} \times M_{H_2O}} \quad (\text{eq. 1})$$

where $d_{H_2O} = 1000 \text{ kg m}^{-3}$ is the density of water, $R = 8.314 \text{ J mol}^{-1} \text{ K}^{-1}$ is the universal gas constant, $T_{st} = 293.15 \text{ K}$ and $P_{st} = 1013.25 \text{ hPa}$ are standard conditions of temperature and pressure and $M_{H_2O} = 18.10^{-3} \text{ kg mol}^{-1}$.

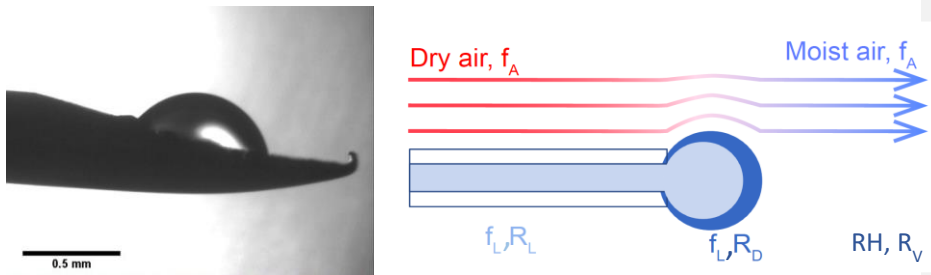


Figure 1: Evaporation of a droplet in the humidity generator chamber: left, picture from the prototype from Landsberg (2014); right, schematics of the water molecules being transferred to the air flow (Casado, 2016).

Physically, when the flux of water or air is changed, there is first a transient regime during which the radius

of the droplet changes, modifying the evaporative surface and therefore the humidity of the outgoing air. Once a stationary regime is reached, the radius of the droplet is stabilized and the humidity is given by equation 1. In this regime, there is no accumulation of water molecules in the system and therefore the isotopic composition of the vapor produced is equal to the isotopic composition of the liquid water injected in the needle: $R_V = R_L$ (note that because of the fractionation during the transition phase, the isotopic composition of the droplet R_D is different from R_L and R_V , see Kerstel, 2020). When changing the flux of evaporating water, we modify the size of the evaporating surface and therefore the radius of the drop. The evolution of the radius of the drop can be obtained from the resolution of a non-linear differential equation of the volume V of the drop:

$$dV/dt = f_L - f_{evap} \quad (\text{eq. 2})$$

where $f_{evap} = k_e \times S$ is the evaporation flux depending of k_e , the evaporation rate, and S , the surface area of the drop exposed to the dry air. A good approximation is to consider the shape of the drop as a fraction of a sphere of variable radius intercepted by the surface of a disk of constant radius (the syringe tip). By solving numerically the differential equation (2), it is possible to faithfully simulate the behavior of the device under changing conditions (Kerstel, 2020). This numerical approach validates the theoretical explanation of the undersaturated evaporation of the droplet. Importantly, it is noted that in steady-state as is the case for our application, the isotopic composition of the generated humid air is identical to that of the injected water stream, and therefore does not depend on the infusion rate, nor on the specific humidity.

2-2- Instrument conception

- Technical realization

As the LHLG relies on operating in a stationary regime, it is important that the dry air input and the water input are steady. Thus, the air and water fluxes, as well as the air pressure in the evaporation chamber are controlled by electronic PID regulators. Temperature intervenes through its effect on fractionation and the evaporation rate (apart from a negligible effect on the flow controller stability), which could lead to a departure from steady-state operation. For these reasons, the temperature of the evaporation chambers was maintained at 20°C (within 1°C over 24 hours).

The dry air flux is regulated by a high-precision mass flow controller (Vögtlin GSC-A9TS-DD22), that has an operating range from 6 to 600 sccm (std cm³ min⁻¹) and an accuracy of 3.3 sccm. The water flux is regulated by a high-precision syringe pump (Harvard Apparatus Pump 11 Pico Plus Elite Dual), which can produce a water flow down to 10.8 pL min⁻¹ with an accuracy of 0.35 % using syringes with a volume ranging from

168 10 μL to 250 μL . We operate in the routine mode with a dry air flow of 300 sccm and a water flow between
 169 0.02 to 0.5 $\mu\text{L min}^{-1}$ using mainly 50 or 100 μL syringes. A syringe pump is equipped with two syringes that
 170 provide two water flows into two evaporation chambers in parallel (Figure 2). Each syringe is connected
 171 to a water reservoir and to an evaporation chamber by a double 3-way liquid valve (Rheodyne MXX777603)
 172 switching from an “infuse” mode to a “withdraw” mode to refill the syringes. The water in the water
 173 reservoirs is sampled every month to check its isotopic composition and renewed when the level of water
 174 is below half the maximum level. A maximum evolution of the isotopic composition of the lab-standard
 175 filling the water reservoirs has been observed as 0.05‰ and 0.5‰ respectively for $\delta^{18}\text{O}$ and δD over a 2-
 176 month period.
 177 A major change to the instrument designed by Landsberg (2014) is the introduction of the double 3-way
 178 valve with leak-tight connections and an internal volume of 1.9 μL . This modification is an important
 179 improvement as it enables automatic handling of the lab-standards from a reservoir to the evaporation
 180 chamber with a robust connection, avoiding in particular potential air bubbles in the water flow. Indeed,
 181 the compressibility of air bubbles trapped in the water flow can lead to flow irregularities by amplification
 182 of small non-linearities in the progression of the syringe plunger. This would lead to non-steady state
 183 operation, which in turn would create artefacts in the humidity and isotopic composition, reducing the
 184 performance of the calibration device (see Kerstel 2020). In addition, the 3-way valve provides the
 185 opportunity of a “withdrawn” mode in which the syringes draw lab-standard water from a reservoir. When
 186 equipped with 100- μL syringes, the instrument can operate for several hours up to one day between refills.
 187 With the addition of the auto-refill option and the effective suppression of bubbles, the instrument can be
 188 used unattended for many months, as required for an Antarctic winter field campaign.
 189

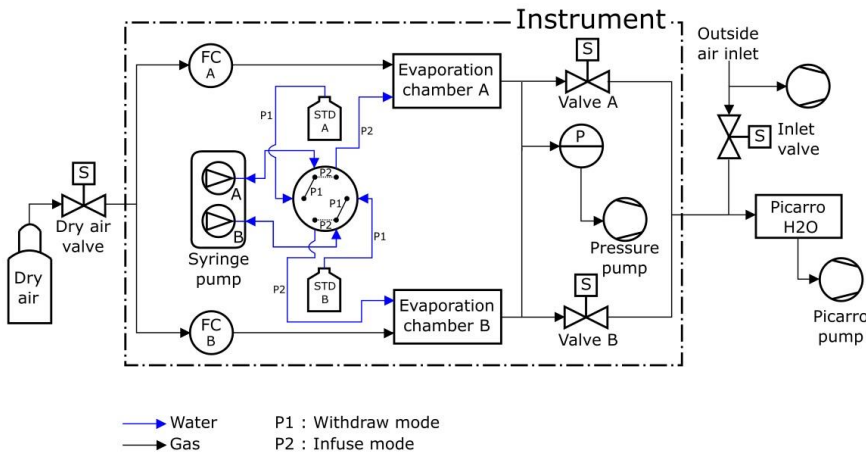


Figure 2: Humidity generator schematic diagram (see supplementary Table S1 for details on the different elements)

The evaporation chambers are stainless steel cylinders equipped with specific connectors (Swagelok Ultra-Torr SS-4CD-TW-25) holding silicon rubber septa through which needles are inserted toward the middle of the chamber. The pressure in both chambers is regulated by a pressure controller (Bronkhorst P-702CV-1K1A-AAD-22-V) with a precision of 3 mbar in a range from 0 to 1,000 mbar. This pressurization of the two chambers combined with the relatively high flow (higher than required by the infrared spectrometers) enables maintaining a steady state whether or not the infrared spectrometer is connected, and increases the time efficiency of calibration procedures. The spectrometer is not sensitive to the inlet pressure, the precision of the pressure controller is not an essential aspect. On the contrary, the precision of the flow controller is key for the precision of the humidity level produced by the instrument: it is of 1% for the air flow which is comparable to the precision of the measurement of the humidity level with the optical spectrometer. When the instrument is connected to the infrared spectrometer, the excess humid air flow is exhausted to the room through the pressure pump and the spectrometer only pumps what is required (Figure 2).

The control of the instrument is ensured by a Raspberry Pi that can be interfaced to a Picarro water analyzer (L2130-i in our case) in sequencer mode (see below). The hardware has been designed to meet the specifications dictated by field conditions: 1) All components are fixed in a transportable case (except the dry air bottle), isolated from vibration by an anti-vibration foam. 2) A panel of connectors (HDMI, USB, Ethernet, etc.) ensures the accessibility to the instrument when it is closed. 3) The electrical and electronic parts (e.g. power supply, Raspberry Pi) are separated from the rest of the instrument (e.g. sensors, gauges). Both the electrical and electronic parts are fully and easily accessible in case of failure.

- **Software details**

The control software has been developed using open source Python libraries and homemade drivers, including a user interface displaying the state of relevant components and the value of the different sensors. The software (HumGen) can be downloaded on line (<https://github.com/ojsd/humgen>; <https://doi.org/10.5281/zenodo.4003465>).

The LHLG can operate in eight different states, each state representing a specific setup for each element (valves position, syringe pump infusion rate, dry air flow rate, pressure). Those eight states can be divided into three categories: a routine mode, an expert mode and a humidity dependence calibration mode. The simple mode is composed of six predefined states referring to the classic isotopic calibration in everyday routine operation (Table 1): 1) measurement of the outside air water vapor isotopic composition; 2) drying of the cavities; 3) "humidity boost", in order to reach faster the desired humidity level in the cavities; 4)

226 injection of the standard A in the corresponding evaporation chamber at a set humidity level; 5) injection
 227 of the standard B in the corresponding evaporation chamber; 6) refill of the syringes. The expert mode is
 228 useful to adjust each parameter manually: flow rates on the controllers FCA and FCB, opening of the
 229 electrovalves A and B, mode (infuse or withdraw) and infused rate for the syringe pump, pressure
 230 regulation, state of the double three-way valve, activation of the pressure pump at the exhaust, opening
 231 of external electrovalves from the dry air tank and to the inlet (Figure 2). The humidity dependence
 232 calibration mode produces a scale of increasing humidity steps in the evaporation chambers (e.g. from 100
 233 ppmv to 1000 ppmv, through steps of 100 ppmv for 50 minutes for each standard). The details of the
 234 sequence (standard type, humidity level and duration of each step) is defined in a text file by the operator
 235 from the Raspberry interface, the Raspberry being itself connected to Ethernet for remote access.
 236 The Picarro L2130-i analyser has an External Valve Sequencer, which is able to turn on/off up to six
 237 electrovalves and create loop sequences with defined durations for each step of the sequence. This tool
 238 can be diverted from its original purpose by using it as a 6-digit code: each of the humidity generator state
 239 is associated with a code. When the Picarro Valve Sequencer matches one of the state code, this state is
 240 triggered on the humidity generator. This eases both the operator's activities and the data post-treatment,
 241 because the current valve status - thus the calibration instrument state - is saved in the analyzer output
 242 data file, in the "ValveMask" column. The Raspberry inside the LHLG reads the Valve Sequencer state code
 243 using the Picarro's Remote Control Interface (a RS232 serial connection through one of the rear-face DB9
 244 connector).

245

States (min)	Flow FCA (sccm)	Flow FCB (sccm)	Valve A	Valve B	Syringe Pump (μ L/min)	Inlet Valve	Dry air Valve	Pressure controller (mbar)	Pressure Pump for exhaust	Double 3-way valve
Outside air (1100)	0	0	Closed	Closed	0	Open	Closed	Off	Off	To chamber
Drying (20)	400	400	Open	Open	0	Closed	Open	Off	Off	To chamber
Boost (0.7)	300	300	Open	Open	Infuse at 2.5	Closed	Open	905	On	To chamber
Standard A (50)	300	150	Open	Closed	Infuse at 0.25	Closed	Open	905	On	To chamber

Standard B (50)	150	300	Closed	Open	Infuse at 0.25	Closed	Open	905	On	To chamber
Reset (1)	Closed	Closed	Closed	Closed	Withdraw max speed	Open	Closed	Off	Off	From standard

Table 1: Typical routine sequence of measurements + calibration for two standards A and B at 1000 ppmv for a measurement site located at sea level. No mixing occurs between standards A and B during steps “Standard A” and “Standard B” (see supplementary text S1).
Note that the humidity dependence mode and the expert mode can also be included in the valve sequencer but are not used in a daily calibration routine.

A set of tools has been developed to quickly check daily calibration. In the field, analyzer and LHLG data are archived daily and sent to the laboratory, i.e. at LSCE, Gif sur Yvette. They are checked semi-automatically once a week to warn maintenance personnel in the event of a malfunction.

3- Performance of the instrument

The stability of the instrument has been tested over a large range of parameters. We show an example in Table 2. We modified the air flow associated with standard A (the same results can be obtained with standard B) between 200 and 400 sccm with an air flow on channel B of half the value of channel A. The infusion rate was varied between 0.03 and 0.14 $\mu\text{L}/\text{min}$ in order to produce humidity levels of 400 and 800 ppmv. The 1σ standard deviations observed over 10 minutes plateaus are comparable to the standard deviation obtained when the air flow is set to 300 sccm.

Air flow (sccm)	Infusion rate ($\mu\text{L}/\text{min}$)	Humidity (ppmv)	10 minutes 1σ standard deviation for humidity (ppmv)	$\delta^{18}\text{O}$ (‰)	10 minutes 1σ standard deviation for $\delta^{18}\text{O}$ (‰)
200	0.07	808	1	-7.88	0.89
300	0.11	851	2	-7.73	0.85
400	0.14	818	2	-7.95	0.90
200	0.03	374	1	-8.45	1.92
300	0.05	411	2	-9.16	1.64
400	0.07	415	3	-9.05	1.59

Table 2 : Evolution and stability of humidity and $\delta^{18}\text{O}$ (same water used for the different tests) for different syringe infusion rates and dry air flows.

For routine measurement, while the stability of the instrument has been tested over a large range of parameters (supplementary Table S2), air flow and infusion rate have been adjusted to optimize the stability of the generated vapor while minimizing the dry air consumption. The LHLG is thus able to generate stable levels of humidity (drift lower than 20 ppmv over one hour and 1σ below 10 ppmv over 10 minutes) from 70 ppmv to 2,400 ppmv following the optimal set-points shown in Table 32.

Humidity (ppmv)	Infusion rate ($\mu\text{L}/\text{min}$)	Dry Air flow (sccm)
80	0.01	300
160	0.02	300
320	0.04	300
800	0.1	300
1200	0.15	300
1600	0.2	300
2400	0.3	300

Table 32: Set-points for water infusion rate and dry air flow at a temperature of 20°C.

3-1- No fractionation during water vaporization in the cavity

We have checked that there was no fractionation of the water during its transfer from the bottles to the syringe pump, then from the syringe to the moist air generated in the vaporization chamber through the following tests.

First, the isotopic composition of three different lab-standards calibrated against VSMOW at LSCE (H_2O - CO_2 equilibration followed by IRMS for $\delta^{18}\text{O}$; Cavity RingDown Spectroscopy for δD ; calibrated every 3 years using VSMOW and VSLAP provided by IAEA) have been compared, after their generation by the present LHLG and by the commercial SDM, both at a humidity of 2,000 ppmv over 50-min time spans. The measured $\delta^{18}\text{O}$ and δD values agreed to within 0.5‰ and 2‰, respectively, for the 3 lab-standard waters calibrated against VSMOW: EPB ($\delta^{18}\text{O} = -6.24$ ‰; $\delta\text{D} = -43.6$ ‰), NEEM ($\delta^{18}\text{O} = -33.50$ ‰; $\delta\text{D} = -257.2$ ‰), FP5 ($\delta^{18}\text{O} = -48.33$ ‰; $\delta\text{D} = -383.5$ ‰). Second, the measured isotopic composition of the same standard (FP5) generated at different humidity levels between 1,000 and 2,400 ppmv by the SDM and the LHLG show the same $\delta^{18}\text{O}$ (δD) evolution with humidity within respective uncertainties (Supplementary Figure S1).

3-2- Stability of the water vapor delivery and associated water isotopic composition

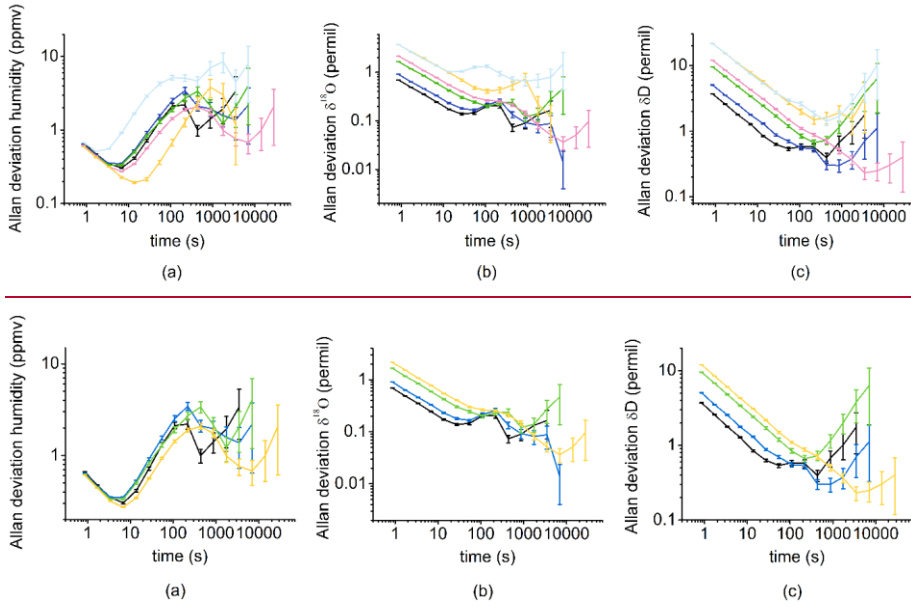


Figure 3: Allan deviation over 4 hours for different humidity levels (black 1,080 ppmv; dark blue 770 ppmv; green 400 ppmv; pink/yellow 320 ppmv; yellow and light blue 170 ppmv) for humidity (a), $\delta^{18}\text{O}$ (b) and δD (c).

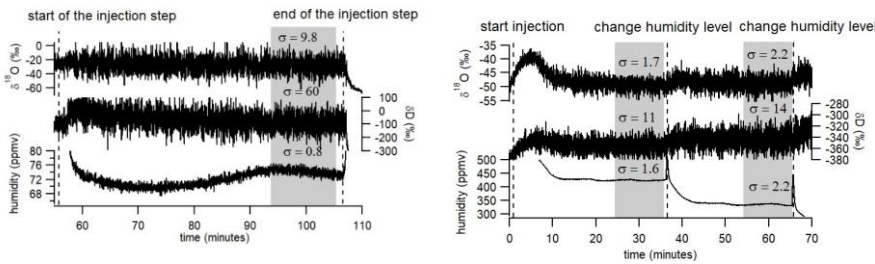


Figure 4: Records of $\delta^{18}\text{O}$, δD and humidity over 3 humidity plateaus (72 ppmv on the left, 425 and 335 ppmv on the right) obtained with the LHLG. The grey rectangles indicate the period (10 min) over which the average values are kept for calibrating the data generated by a L2130-i analyzer.

A proper approach to quantify the stability of our system is to use the Allan variance defined as:

$$\sigma_y^2(t) = \frac{1}{2} \langle (y_{n+1} - y_n)^2 \rangle \quad (\text{eq. 3})$$



where y_n are the successive measurements over a period t .

An Allan variance plot as a function of averaging time is indeed useful to determine the optimal time over which the sample humidity and the isotopic composition should be averaged to obtain a precise determination (low standard deviation) and avoid drift. Figure 3 displays the Allan deviation (square root of the Allan variance) in $\delta^{18}\text{O}$, δD and humidity obtained by running a long plateau of standard A or standard B in the “infuse” mode. Figure 3 displays the Allan variance in $\delta^{18}\text{O}$, δD and humidity over 4 hours for different humidity levels. The humidity variance always stays below 10 ppmv over the 4 hours test and the $\delta^{18}\text{O}$ and δD Allan deviations display minimum values below 0.1 ‰ and 70.8 ‰ respectively. The minimum value for (the Allan variance of $\delta^{18}\text{O}$ and δD Allan deviation is generally obtained for about 15 minutes of measurement. While the Allan deviation of $\delta^{18}\text{O}$ and δD is are however strongly dependent on the analyzer used, we observe that the Allan deviation at 1000 s (17 minutes) for $\delta^{18}\text{O}$ and δD also depends to some extent and on the humidity level: the lowest levels are obtained for humidity levels of 770-1,080 ppmv and the highest levels are obtained for humidity level of 170 ppmv.

In the routine mode (Figure 4), we perform plateaus of 30 to 50 minutes (50 minutes when the instrument is unattended since the time to reach the plateau varies between a few minutes to 30 minutes). We then select the last 10 minutes before the following switch of the instrument to measure the average level of humidity and the isotopic ratios, $\delta^{18}\text{O}$ and δD . We also calculate the associated standard deviations and reject the values if the humidity standard deviation exceeds 30 ppmv over these last 10 minutes. In Figure 4, one observes that the standard deviations for humidities generated in the routine mode are actually much lower. The corresponding standard deviations for the isotopic ratios ($\delta^{18}\text{O}$ and δD , see values indicated in Figure 4) increase with decreasing humidity, reflecting the decrease of the molecular absorption signal recorded by the L2130-i laser analyzers. This has an obvious impact on the determination of the relationship between humidity and water vapor isotopic composition.

The performance of the present LHLG can be compared to the performance of the SDM (see Supplementary Figures S1 and S2). First (Figure S2), a comparison has been performed at a humidity level of 800 ppmv, for which we have numerous daily calibrations performed with a SDM from a 4.5 years field deployment in Svalbard (Leroy-Dos Santos et al., 2020). The best SDM performance displays a standard deviation 1σ of 31 ppmv, which is significantly worse than the performance of the LHLG (standard deviation 1σ lower than 10 ppmv on average and down to 2 ppmv for 30% of the generated humidity plateaus). Second (Figure S1), while we measure the same influence of humidity on measured $\delta^{18}\text{O}$ and δD either with the SDM or with the LHLG, the 1σ values on humidity levels are much larger for the SDM than for the LHLG.

341 **3-3- Determination of the influence of humidity on water vapor isotopic composition**

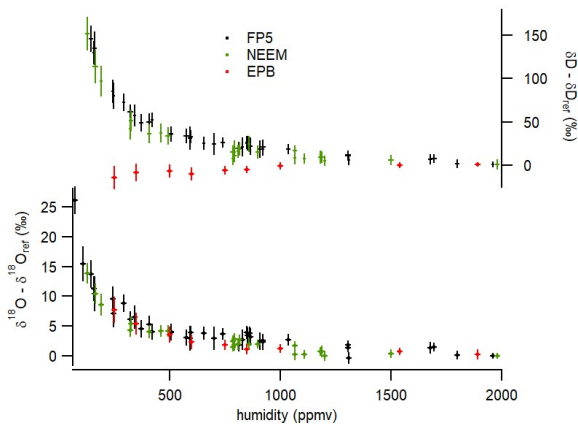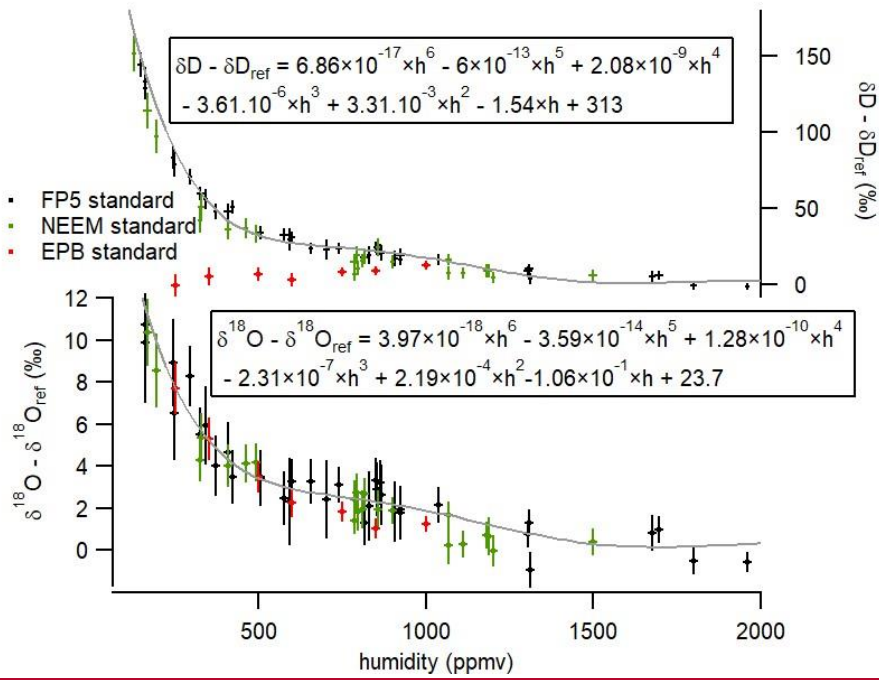

344 **Figure 5:** Influence of humidity on the isotopic composition ($\delta^{18}O$ and δD) of the vapor obtained with the
 345 LHLG with 3 water lab-standards. The error bars are calculated as the standard deviation (1σ) over the
 346 generated values by the L2130-i instrument during 10 minutes at 1 second resolution (i.e. without any pre-
 347 averaging of the raw dataseries). The $\delta^{18}O_{ref}$ and δD_{ref} are the values of the injected water standards at

2,000 ppmv. *The grey lines represent the polynomial fits for the influence of humidity on the water isotopic composition (equations 4 and 5 also written on the graph).*

Contrary to the commercial SDM, which hardly produces stable and reproducible humidity levels below 500 ppmv, the LHLG was able to daily produce stable 10-minute humidity plateaus over the range from 70 ppmv to 2,400 ppmv with an associated standard deviation of the order of 10 ppmv over more than one year at the Concordia and Dumont d'Urville stations (installation in December 2018). The stability of the LHLG allows a robust quantification of the L2130-i analyzer drift thanks to a daily measurement of the same water isotopic standard reference (see Table S2S3 showing actually no measurable drift over a 3-week period). It also permits the characterization of the measurement non-linearities observed at low-humidity (Figure 5). The more than one-year long Concordia and Dumont d'Urville datasets showed that the humidity dependence of $\delta^{18}\text{O}$ and δD did not vary measurably. The uncertainty of the obtained calibration curve can be attributed entirely to the L2130-i $\delta^{18}\text{O}$ and δD measurements. In other words, the uncertainty bars in the horizontal (x-) axis in Figure 5, associated with the LHLG, are negligible.

Our data show a result already observed in Weng et al. (2020): while the dependency of $\delta^{18}\text{O}$ and δD to humidity is similar for low $\delta^{18}\text{O}$ and δD lab-standards (NEEM and FP5), we observe a different behavior for the δD vs humidity relationship for the high $\delta^{18}\text{O}$ and δD lab-standard EPB. This result strengthens the recommendation of Weng et al. (2020) to use two water standards in the range of the measured water vapor isotopic composition to best calibrate our final data. In our case, our applications were in Antarctica, so that we used our two lowest lab-standards (NEEM and FP5). For the two standards and for this particular Picarro L2130-i (results are expected to depend on the instrument), the same dependency of isotopic composition vs humidity is observed. We express this dependency as the relationship between the difference in δD or $\delta^{18}\text{O}$ between the measured value at the given humidity and the value of the same standard measured at a humidity of 2,000 ppmv. The experimental data for NEEM and FP5 from Figure 5 are fitted through polynomial functions with respect to humidity h (in ppmv):

$$\delta^{18}\text{O} - \delta^{18}\text{O}_{\text{ref}} = 3.97 \times 10^{-18} \times h^6 - 3.58631559 \times 10^{-14} \times h^5 + 1.284364599428 \times 10^{-10} \times h^4 - 2.308775344509434 \times 10^{-7} \times h^3 + 2.185728535047310049 \times 10^{-4} \times h^2 - 0.10603325432255400000 \times h - 1.06 \times 10^{-3} \times h + 23.7 \quad (\text{eq. 43})$$

$$\delta\text{D} - \delta\text{D}_{\text{ref}} = 6.85986 \times 10^{-17} \times h^6 - 6.004770900 \times 10^{-13} \times h^5 + 2.079033134908 \times 10^{-9} \times h^4 - 3.61319302207374 \times 10^{-6} \times h^3 + 3.30716141498371 \times 10^{-3} \times h^2 - 1.5365164511470154 \times h + 313 \quad (\text{eq. 54})$$

These curves are valid only for a given Picarro analyzer and for humidity lower than 70 ppmv and higher than 2,000 ppmv. Outside this calibration range, the extrapolation of the polynomial function may lead to anomalous corrections.

Mis en forme : Police :NimbusSanL-Regu

Mis en forme : Police :NimbusSanL-Regu

Mis en forme : Police :NimbusSanL-Regu

Mis en forme : Police :NimbusSanL-Regu

Mis en forme : Gauche, Interligne : simple, Ne pas ajuster l'espace entre le texte latin et asiatique, Ne pas ajuster l'espace entre le texte et les nombres asiatiques

Mis en forme : Police :NimbusSanL-Regu

Mis en forme : Police :NimbusSanL-Regu

Mis en forme : Police :NimbusSanL-Regu

Mis en forme : Police :NimbusSanL-Regu

Mis en forme : Gauche, Interligne : simple, Ne pas ajuster l'espace entre le texte latin et asiatique, Ne pas ajuster l'espace entre le texte et les nombres asiatiques

Mis en forme : Police :NimbusSanL-Regu

Mis en forme : Police :NimbusSanL-Regu

Mis en forme : Police :NimbusSanL-Regu, Exposant

Mis en forme : Police :NimbusSanL-Regu

Mis en forme : Police :NimbusSanL-Regu

Mis en forme : Police :NimbusSanL-Regu

Mis en forme : Police :NimbusSanL-Regu, Exposant

Mis en forme : Police :NimbusSanL-Regu

Mis en forme : Police :NimbusSanL-Regu

Mis en forme : Police :NimbusSanL-Regu

Mis en forme : Police :NimbusSanL-Regu

385
 386 After this correction, the measured values corrected from humidity dependence are corrected using the
 387 comparison of the measured values of the 2 standards at 2,000 ppmv to their VSMOW calibrated values
 388 as explained in section 3.5 below.

389
 390 **3.5- Accuracy of the system and calibration on the VSMOW-VSLAP scale**

391 The accuracy of the system has been addressed performing a 2-standard calibration and measuring a third
 392 standard treated as an unknown. We used two lab-standards calibrated vs VSMOW on the VSMOW-VSLAP
 393 scale with large $\delta^{18}\text{O}$ and δD differences (EPB and FP5) and used the lab-standard NEEM, also
 394 independently calibrated against VSMOW. The 3 lab-standards have been vaporized at 800 ppmv and
 395 measured by the same L2130-i analyzer.

396

Standard	VSMOW calibrated value	Measured value at 800 ppmv	Measured value corrected from humidity dependence (Equation 1)
EPB	-6.24 ‰	-8.27 ‰	-10.78 ‰
NEEM	-33.5 ‰	-34.48 ‰	-36.99 ‰
FP5	-48.33 ‰	-49.02 ‰	-51.53 ‰

397
 398 **Table 43:** Comparison of measured vs VSMOW calibrated $\delta^{18}\text{O}$ values for 3 standards measured with a
 399 Picarro analyzer after generation of water vapor using the LHLG.


Mis en forme : Police :Non Italique

400
 401 We used the measured and true values of EPB and FP5 to estimate the $\delta^{18}\text{O}$ value of the NEEM standard
 402 from its measured value (Table 43). Using the linear relationship obtained from VSMOW calibrated EPB
 403 and FP5 $\delta^{18}\text{O}$ vs measured EPB and FP5 $\delta^{18}\text{O}$ values (Figure S3) following the recommendations of the
 404 National Institute of Standards and Technology (NIST, reference material 8535a) leads to an estimated
 405 NEEM $\delta^{18}\text{O}$ of -33.31 ‰ to be compared to the independently VSMOW calibrated value of -33.5 ‰.
 406 Given the uncertainty of about 0.8-1 ‰ when measuring $\delta^{18}\text{O}$ around 800 ppmv, we can conclude that
 407 the system is accurate.

408
 409 **4- Application**

410 The main application of this device is the interpretation of water isotopic profiles at dry sites, in particular
 411 in polar regions. As shown in Figure 5, the influence of humidity on the measurement of the water vapor
 412 isotopic composition with the L2130-i analyzer is large when humidity is below 1,000 ppm and increases
 413 when humidity decreases. Even though the precise isotope ratio-humidity calibration curve is likely to be
 414 different from one analyzer to another, all laser-based water isotope analyzers investigated to date have

415 shown a strongly non-linear response at low-humidity levels (Guilpart et al., 2017; Leroy Dos-Santos, 2020;
 416 Weng et al., 2020). At the Concordia station, even in summer, humidity is generally below 1,000 ppmv
 417 (Figure 6) so that the interpretation of the diurnal variability of the water vapor isotopic composition is
 418 strongly affected by the dependency of the measured $\delta^{18}\text{O}$ and δD signals on humidity. Figure 6 displays
 419 such diurnal variabilities during austral summer 2018-2019 at Concordia and the consequently large
 420 correction of the isotopic records (uncorrected in grey and corrected in black).

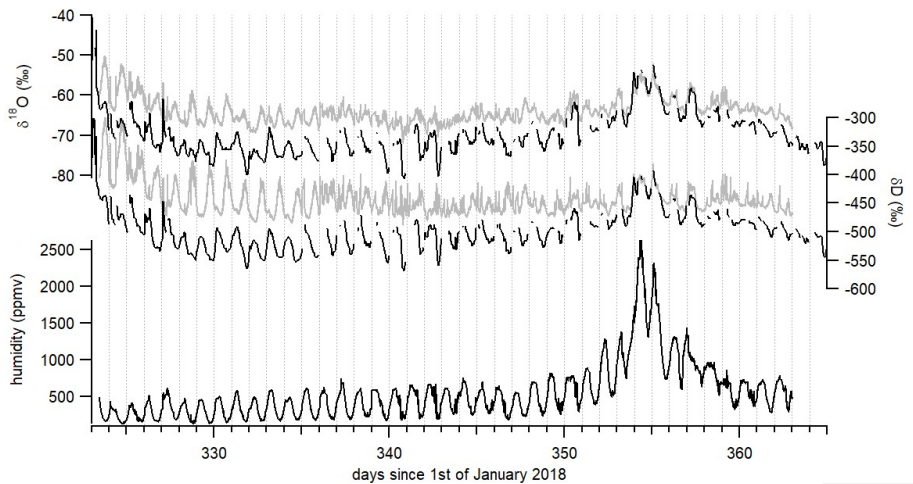

421
 422 **Figure 6:** $\delta^{18}\text{O}$, δD and humidity records over December 2018 and beginning of January 2019. Raw isotopic
 423 values are in grey. Corrected isotopic values at hourly resolution are in black after correction of the
 424 influence of humidity on the water isotopic ratios and adjustment of $\delta^{18}\text{O}$ and δD values on the VSMOW-
 425 VSLAP scale using relationships between measured lab-standard values and known VSMOW calibrated lab-
 426 standard values.

427
 428 The data clearly demonstrate the importance of the humidity correction which shifts the curves generally
 429 to lower isotopic ratio values. However, the difference between uncorrected and corrected data is
 430 particularly important in the observation of the diurnal variability, illustrated even better when zooming
 431 in on a section of the data, as in Figure 7. When looking in detail at the diurnal variability in the raw $\delta^{18}\text{O}$
 432 and δD isotope data, some periods stand out with two identified daily peaks, one in phase with the
 433 humidity peak (marked in red in Figure 7) and one occurring during the period of minimum humidity
 434 (marked in blue in Figure 7). The strong non-linearity of the calibration curve of Figure 5 suggests that
 435 artificial peaks in $\delta^{18}\text{O}$ and δD could be due to changing humidity levels. Indeed, after correcting the data
 436 for the humidity dependence of the analyzer (black curve in Figure 7), the isotopic peaks occurring during
 437 humidity minima are diminished or disappear altogether, while the peaks occurring during humidity

maxima are amplified. More strikingly, the phase of the signal changes by practically 180° over some periods. Whereas the raw isotope signal peaks during the night, the corrected record shows higher isotope ratios during daytime. The diurnal variability recorded on both raw and corrected isotopic values during a period with higher humidity level, hence when the isotope ratio-humidity correction is smaller (around day 355 in figure 6), also shows that the $\delta^{18}\text{O}$ (δD) diurnal cycles are indeed in-phase with the humidity cycle. This result confirms the correlation between humidity cycles and $\delta^{18}\text{O}$ and δD of the water vapor at the daily scale at Concordia as reported by Casado et al. (2016). We thus conclude that the anticorrelation observed between $\delta^{18}\text{O}$ (δD) and humidity in the raw data (highlighted in blue in Figure 7) during periods of low-humidity is an artefact due to the influence of the humidity level on the vapor isotopic measurements by the L2130-i analyzer.

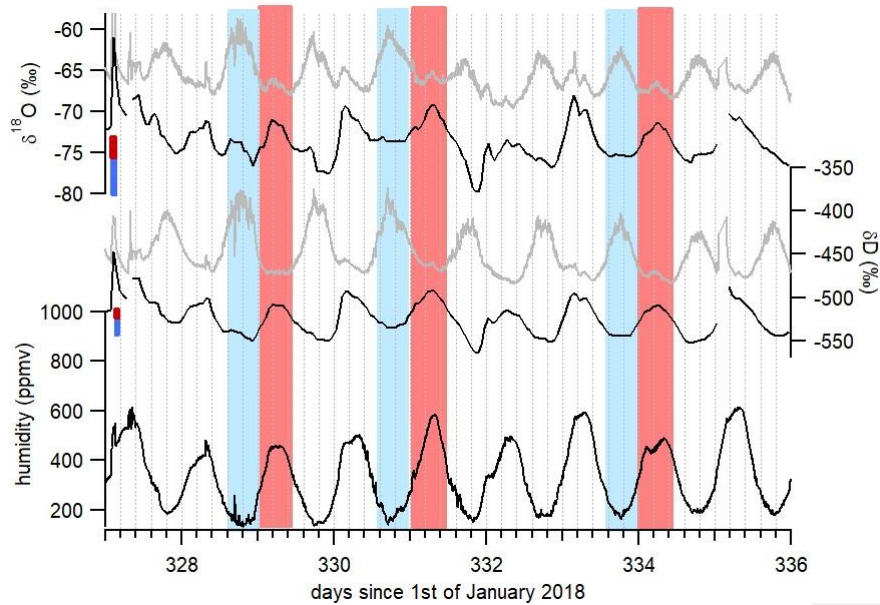


Figure 7: Focus on diurnal variability of $\delta^{18}\text{O}$, δD and humidity recorded at Concordia. Grey curves show the raw measurements and black curves the corrected records. The red (blue) bars indicate the calculated uncertainty due to the isotopic ratio vs humidity dependence (Figure 5) on the corrected $\delta^{18}\text{O}$ and δD values during periods with maximum (minimum) humidity. The red (blue) rectangles indicate half day with maximum (minimum) humidity.

5- Conclusion

We have developed an autonomous instrument for low-humidity generation (70 to 2,400 ppmv) with controlled water vapor isotopic composition specifically aimed at carrying out continuous measurements

of the water vapor isotopic composition using a laser-based spectrometer in regions characterized by very low-humidity, such as polar regions. If needed, an interface permits to conveniently connect the new LHLG to the valve sequencer port of commercial Picarro instruments. After more than one year of routine operation on two Antarctic sites (Dumont d'Urville and Concordia), this instrument has proven to be very reliable and robust. It consistently generates stable humidity levels with a 1σ variability lower than 10 ppmv over more than 10 minutes. Besides, its performance is significantly better than that of the Picarro SDM at low humidity.

We used this instrument for the calibration of our water isotopic data with a special focus on accurately quantifying the influence of humidity on the measured isotopic composition of the water vapor. This effect is huge at low-humidity. We showed that this has an important impact on the interpretation of the diurnal cycles of $\delta^{18}\text{O}$ and δD in the water vapor at the Concordia station at humidity below 1,500 ppmv. We were able to confirm that, at this site, the diurnal $\delta^{18}\text{O}$ and δD variability is actually correlated with humidity variability, which would not have been possible without the new LHLG instrument.

Finally, the development of such an instrument is an important step forward to a better understanding of the transfer function between climate parameters and the isotopic composition of deep ice cores from the remote East Antarctic plateau, especially in the context of the new program "Beyond EPICA". It should be completed by ongoing development of laser spectrometers better adapted to low-humidity levels, such as those based on the technique of Optical Feedback Cavity Enhanced Absorption Spectroscopy (OFCEAS) (Casado et al., 2016; Landsberg, 2014; Landsberg et al., 2014).

Code availability

The software (HumGen) can be downloaded on line (<https://github.com/ojsd/humgen>; <https://doi.org/10.5281/zenodo.4003465>).

Competing interests

The authors declare that they do not have any competing interest.

Author contributions

CLDS, MC, FP and EK designed and built the instrument. OJ realized the software interface development. CLDS, MC and AL installed the instrument in Antarctica and tested it extensively. EK, SK, MF, AL and EF tested the instrument in the laboratory. AL wrote the manuscript with the help of all co-authors.

Acknowledgments

The development presented in this manuscript is largely inspired from the initial PhD work of Janek Landsberg which we gratefully acknowledge here. The research leading to these results has received

493 funding from the Antarctic Snow program of the Fondation Prince Albert II de Monaco, the ANR EAIIST and
494 CNRS-LEFE program ADELISE. The deployment of this instrument in the field was made possible through
495 the logistic support of the NIVO2 & ADELISE IPEV programs. We thank the two reviewers for their useful
496 comments which greatly improved the manuscript.

497

498 **References**

499 Aemisegger, F., Sturm, P., Graf, P., Sodemann, H., Pfahl, S., Knohl, A. and Wernli, H.: Measuring variations
500 $\delta^{18}\text{O}$ and $\delta^2\text{H}$ in atmospheric water vapour using two commercial laser-based spectrometers: an
501 instrument characterisation study, *Atmos. Meas. Tech.*, 5(7), 1491–1511, doi:10.5194/amt-5-1491-2012,
502 2012.

503 Bailey, H. L., Kaufman, D. S., Henderson, A. C. G. and Leng, M. J.: Synoptic scale controls on the $\delta^{18}\text{O}$ in
504 precipitation across Beringia, *Geophys. Res. Lett.*, 42(11), 4608–4616, doi:10.1002/2015GL063983, 2015.

505 Bastrikov, V., Steen-Larsen, H. C., Masson-Delmotte, V., Griбанov, K., Cattani, O., Jouzel, J. and Zakharov,
506 V.: Continuous measurements of atmospheric water vapour isotopes in western Siberia (Kourovka),
507 *Atmos. Meas. Tech.*, 7(6), 1763–1776, doi:10.5194/amt-7-1763-2014, 2014.

508 Bonne, J.-L., Masson-Delmotte, V., Cattani, O., Delmotte, M., Risi, C., Sodemann, H. and Steen-Larsen, H.
509 C.: The isotopic composition of water vapour and precipitation in Ivittuut, southern Greenland, *Atmos.*
510 *Chem. Phys.*, 14(9), 4419–4439, doi:10.5194/acp-14-4419-2014, 2014.

511 Bréant, C., Leroy Dos Santos, C., Agosta, C., Casado, M., Fourré, E., Goursaud, S., Masson-Delmotte, V.,
512 Favier, V., Cattani, O., Prié, F., Golly, B., Orsi, A., Martinerie, P. and Landais, A.: Coastal water vapor isotopic
513 composition driven by katabatic wind variability in summer at Dumont d'Urville, coastal East Antarctica,
514 *Earth Planet. Sci. Lett.*, 514, 37–47, doi:10.1016/j.epsl.2019.03.004, 2019.

515 Casado, M., Landais, A., Masson-Delmotte, V., Genthon, C., Kerstel, E., Kassi, S., Arnaud, L., Picard, G., Prie,
516 F., Cattani, O., Steen-Larsen, H.-C., Vignon, E. and Cermak, P.: Continuous measurements of isotopic
517 composition of water vapour on the East Antarctic Plateau, *Atmos. Chem. Phys. Discuss.*, 1–26,
518 doi:10.5194/acp-2016-8, 2016.

519 Casado, M., Landais, A., Picard, G., Münch, T., Laepple, T., Stenni, B., Dreossi, G., Ekaykin, A., Arnaud, L.,
520 Genthon, C., Touzeau, A., Masson-Delmotte, V. and Jouzel, J.: Archival processes of the water stable
521 isotope signal in East Antarctic ice cores, *Cryosphere*, 12(5), doi:10.5194/tc-12-1745-2018, 2018.

522 Dong, F. and Baer, D. Development and Deployment of a Portable Water Isotope Analyzer for Accurate,
523 Continuous and High-Frequency Oxygen and Hydrogen Isotope Measurements in Water Vapor and Liquid
524 Water, in *Geophysical Research Abstracts*, 12:EGU2010-5571, 2010.

525 Ellehoj, M. D., Steen-Larsen, H. C., Johnsen, S. J. and Madsen, M. B.: Ice-vapor equilibrium fractionation
526 factor of hydrogen and oxygen isotopes: Experimental investigations and implications for stable water
527 isotope studies, *Rapid Commun. Mass Spectrom.*, 27(19), 2149–2158, doi:10.1002/rcm.6668, 2013.

528 Genthon, C., Piard, L., Vignon, E., Madeleine, J.-B., Casado, M. and Gallée, H.: Atmospheric moisture
529 supersaturation in the near-surface atmosphere at Dome C, Antarctic Plateau, *Atmos. Chem. Phys.*, 17(1),
530 691–704, doi:10.5194/acp-17-691-2017, 2017.

531 Gkinis, V., Popp, T. J., Johnsen, S. J. and Blunier, T.: A continuous stream flash evaporator for the calibration
532 of an IR cavity ring-down spectrometer for the isotopic analysis of water, *Isotopes Environ. Health Stud.*,

46(4), 463–475, doi:10.1080/10256016.2010.538052, 2010.

Guilpart, E., Vimeux, F., Evan, S., Brioude, J., Metzger, J., Barthe, C., Risi, C. and Cattani, O.: The isotopic composition of near-surface water vapor at the Maïdo observatory (Reunion Island, southwestern Indian Ocean) documents the controls of the humidity of the subtropical troposphere, *J. Geophys. Res. Atmos.*, 122(18), 9628–9650, doi:10.1002/2017JD026791, 2017.

Iannone, R., Romanini, D., Kassi, S., Meijer, H. A. J. and Kerstel, E.: A Microdrop Generator for the Calibration of a Water Vapor Isotope Ratio Spectrometer, *J. Atmos. Ocean. Technol.*, 26, doi:10.1175/2008JTECHA1218.1, 2009.

Jouzel, J., Masson-Delmotte, V., Cattani, O., Dreyfus, G., Falourd, S., Hoffmann, G., Minster, B., Nouet, J., Barnola, J. M., Chappellaz, J., Fischer, H., Gallet, J. C., Johnsen, S., Leuenberger, M., Loulergue, L., Luthi, D., Oerter, H., Parrenin, F., Raisbeck, G., Raynaud, D., Schilt, a, Schwander, J., Selmo, E., Souchez, R., Spahni, R., Stauffer, B., Steffensen, J. P., Stenni, B., Stocker, T. F., Tison, J. L., Werner, M. and Wolff, E. W.: Orbital and millennial Antarctic climate variability over the past 800,000 years., *Science*, 317(5839), 793–796, doi:10.1126/science.1141038, 2007.

Kerstel, E. Modeling the Dynamic Behavior of a Droplet Evaporation Device for the Delivery of Isotopically Calibrated Low-Humidity Water Vapor, *Atmospheric Measurement Techniques Discussions*, 1–19. <https://doi.org/10.5194/amt-2020-428>, 2020.

Kopeck, B., Lauder, A., Posmentier, E. and Feng, X.: The diel cycle of water vapor in west Greenland, *J. Geophys. Res. Atmos.*, 119(15), 9386–9399, 2014.

Landsberg, J.: Développement d'un spectromètre laser OF-CEAS pour les mesures des isotopes de la vapeur d'eau aux concentrations de l'eau basses. [online] Available from: <http://www.theses.fr/2014GRENY052/document>, 2014.

Landsberg, J., Romanini, D. and Kerstel, E.: Very high finesse optical-feedback cavity-enhanced absorption spectrometer for low concentration water vapor isotope analyses., *Opt. Lett.*, 39(7), 1795–1798, doi:10.1364/OL.39.001795, 2014.

Lee, X., Sargent, S., Smith, R. and Tanner, B.: In Situ Measurement of the Water Vapor $^{18}\text{O}/^{16}\text{O}$ Isotope Ratio for Atmospheric and Ecological Applications, *J. Atmos. Ocean. Technol.*, 22(5), 555–565, doi:10.1175/JTECH1719.1, 2005.

Leroy Dos Santos, C., Masson-Delmotte, V., Casado, M., Fourré, E., Steen-Larsen, H-C, Maturilli, M., Orsi, A., Berchet, A., Cattani, O., Minster, B., Gherardi, J. and Landais, A., A 4.5 year-long record of Svalbard water vapor isotopic composition documents winter air mass origin, *J. Geophys. Research*, 125 (23), (10.1029/2020JD032681), 2020.

Ritter, F., Steen-larsen, H. C., Werner, M., Masson-Delmotte, V., Orsi, A., Behrens, M., Birnbaum, G., Freitag, J., Risi, C. and Kipfstuhl, S.: Isotopic exchange on the diurnal scale between near-surface snow and lower atmospheric water vapor at Kohnen station , East Antarctica, *J. Geophys. Research* (February), 1–35, doi:10.5194/tc-2016-4, 2016.

Sayres, David S, E J Moyer, T F Hanisco, J M St Clair, F N Keutsch, A O'Brien, N T Allen, et al., A New Cavity Based Absorption Instrument for Detection of Water Isotopologues in the Upper Troposphere and Lower Stratosphere. *Review of Scientific Instruments* 80 (4): 44102–14. <http://link.aip.org/link/?RSI/80/044102/1>, 2009.

Schmidt, M., Maseyk, K., Lett, C., Biron, P., Richard, P., Bariac, T. and Seibt, U.: Concentration effects on

574 laser-based $\delta^{18}\text{O}$ and $\delta^2\text{H}$ measurements and implications for the calibration of vapour measurements with
575 liquid standards, *Rapid Commun. Mass Spectrom.*, 24(24), 3553–3561, doi:10.1002/rcm.4813, 2010.

576 Sodemann, H., Aemisegger, F., Pfahl, S., Bitter, M., Corsmeier, U., Feuerle, T., Graf, P., Hankers, R., Hsiao,
577 G., Schulz, H., Wieser, A. and Wernli, H.: The stable isotopic composition of water vapour above Corsica
578 during the HyMeX SOP1 campaign: Insight into vertical mixing processes from lower-tropospheric survey
579 flights, *Atmos. Chem. Phys.*, 17(9), 6125–6151, doi:10.5194/acp-17-6125-2017, 2017.

580 Steen-Larsen, H. C., Masson-Delmotte, V., Hirabayashi, M., Winkler, R., Satow, K., Prié, F., Bayou, N., Brun,
581 E., Cuffey, K. M., Dahl-Jensen, D., Dumont, M., Guillevic, M., Kipfstuhl, S., Landais, A., Popp, T., Risi, C.,
582 Steffen, K., Stenni, B. and Sveinbjörnsdóttir, A. E.: What controls the isotopic composition of Greenland
583 surface snow?, *Clim. Past*, 10(1), 377–392, doi:10.5194/cp-10-377-2014, 2014.

584 Sturm, P. and Knohl, A.: Water vapor $\delta^2\text{H}$ and $\delta^{18}\text{O}$ measurements using off-axis integrated cavity output
585 spectroscopy, *Atmos. Meas. Tech. Discuss.*, 2(4), 2055–2085, doi:10.5194/amtd-2-2055-2009, 2009.

586 Tremoy, G., Vimeux, F., Cattani, O., Mayaki, S., Souley, I. and Favreau, G.: Measurements of water vapor
587 isotope ratios with wavelength-scanned cavity ring-down spectroscopy technology: new insights and
588 important caveats for deuterium excess measurements in tropical areas in comparison with isotope-ratio
589 mass spectrometry, *Rapid Commun. Mass Spectrom.*, 25(23), 3469–3480, doi:10.1002/rcm.5252, 2011.

590 Wang, L., Caylor, K. and Dragoni, D.: On the calibration of continuous, high-precision $\delta^{18}\text{O}$ and $\delta^2\text{H}$
591 measurements using an off-axis integrated cavity output spectrometer, *Rapid Commun. Mass Spectrom.*,
592 23, 530–536, doi:10.1002/rcm.3905, 2009.

593 Weng, Y., Touzeau, A. and Sodemann, H.: Impact of isotope composition on the humidity dependency
594 correction of water vapour isotope measurements with infra-red cavity ring-down spectrometers, *Atmos.*
595 *Meas. Tech.*, 13, 3167–3190, <https://doi.org/10.5194/amt-13-3167-2020>, 2020.

596

597

598

599