

# Absorption instruments inter-comparison campaign at the Arctic Pallas station

Eija Asmi<sup>1</sup>, John Backman<sup>1</sup>, Henri Servomaa<sup>1</sup>, Aki Virkkula<sup>1</sup>, Maria Gini<sup>2</sup>, Kostas Eleftheriadis<sup>2</sup>, Thomas Müller<sup>3</sup>, Sho Ohata<sup>4,5</sup>, Yutaka Kondo<sup>6</sup>, and Antti Hyvärinen<sup>1</sup>

<sup>1</sup>Finnish Meteorological Institute, Helsinki, Finland

<sup>2</sup>ERL Institute of Nuclear and Radiological Science & Technology, NCRS Demokritos, Attiki, Greece

<sup>3</sup>Leibniz Institute for Tropospheric Research e.V. (TROPOS), Leipzig, Germany

<sup>4</sup>Institute for Space–Earth Environmental Research, Nagoya University, Nagoya, Aichi, Japan

<sup>5</sup>Institute for Advanced Research, Nagoya University, Nagoya, Aichi, Japan

<sup>6</sup>National Institute of Polar Research, Tachikawa, Japan

**Correspondence:** Eija Asmi (eija.asmi@fmi.fi)

**Abstract.** Aerosol light absorption was measured during one month field campaign in June–July 2019 at the Pallas Global Atmospheric Watch (GAW) station in northern Finland. Very low aerosol concentrations prevailed during the campaign which imposed a challenge for the instruments detection capabilities. The campaign provided a real-world test for different absorption measurement techniques supporting the goals of the EMPIR BC metrology project in developing aerosol absorption standard and reference methods. In this study we compare the results from five filter-based absorption techniques: Aethalometer models AE31 and AE33, Particle Soot Absorption Photometer (PSAP), Multi Angle Absorption Photometer (MAAP) and Continuous Soot Monitoring System (COSMOS), and from one indirect technique called Extinction Minus Scattering (EMS). The ability of the filter-based techniques was shown to be adequate to measure aerosol light absorption coefficients down to around 0.01 Mm<sup>-1</sup> levels when data was averaged to 1–2 hours. The hourly-averaged atmospheric absorption measured by the reference MAAP was 0.09 Mm<sup>-1</sup> (at wavelength of 637 nm). When data was averaged for >1 hours, the filter-based methods agreed to around 15–20%. COSMOS measured systematically the lowest absorption coefficient values, which was expected due to the sample pre-treatment in COSMOS inlet. PSAP showed the best linear correlation with MAAP (slope = 0.95, R<sup>2</sup> = 0.78), followed by AE31 (slope=0.93). Scattering correction applied to PSAP data improved the data accuracy but also generated a higher noise and led to an under-estimation of the absorption at very high scattering values. The AE31 data had the highest noise and the correlation with MAAP was the lowest (R<sup>2</sup> = 0.65). Statistically the best correlations with MAAP were obtained for AE33 and COSMOS, but biases at around the zero values led to slopes clearly below one. In COSMOS, also the sample pre-treatment could affect on the correlation slope. In contrast to the filter-based techniques, the sensitivity of the indirect EMS method to measure aerosol absorption was not adequate at such low concentrations levels for such highly scattering aerosol. An absorption coefficient on the order of >0.1 Mm<sup>-1</sup> was estimated as the lowest limit, to reliably distinguish the EMS signal from the noise at 1–2 hours averaging times. The mass absorption cross-section (MAC) value for the measured absorption coefficient range 0 – 0.3 Mm<sup>-1</sup> was calculated based on MAAP and SP2 as a reference instrument, leading to a MAC value of

16.0 m<sup>2</sup> g<sup>-1</sup>. Overall, our results demonstrate the challenges encountered in the aerosol absorption measurements in pristine environments and provide some useful guidelines for instruments selection and measurement practices.

## 1 Introduction

25 The development of a filter-based absorption measurement method began with an experiment by Rosen et al. (1978). The Raman spectral measurements confirmed that the light attenuation is proportional to the graphitic soot content on a filter. After this discovery the development continued by Hansen et al. (1982, 1984), and today, the various filter-based techniques are commonly used in aerosol absorption measurements (Tørseth et al., 2019). The filter-based methods are sensitive, simple and robust, and therefore widely applicable.

30 Meanwhile, it has become evident that the filter-based methods are prone to several filter artifacts. These include the dependence of light attenuation on the filter tape loading and the interference of aerosol light scattering with the absorption measurement (Müller et al., 2011). Aerosol size affects the penetration depth in a filter adding another size dependent measurement artifact (Kondo et al., 2009; Nakayama et al., 2010). Additional sources of uncertainties are the variations in filter spot size and the non-idealities of light source (Bond et al., 1999). Various algorithms to correct for these artifacts have been developed (Bond et al., 1999; Weingartner et al., 2003; Arnott et al., 2005; Schmid et al., 2006; Virkkula et al., 2007; Nakayama et al., 2010; Ogren, 2010; Virkkula, 2010; Collaud Coen et al., 2010). The diverse use of these algorithms complicates a direct comparison of aerosol absorption values from different studies. The measured aerosol light absorption is frequently reported as equivalent black carbon (eBC) mass [in units: ng m<sup>-3</sup>] which relies on a specific wavelength dependent mass absorption cross section (MAC) coefficient (Bond and Bergstrom, 2006; Petzold et al., 2013).

40 Alternative absorption measurement methods exist. They are less prone to measurement artifacts and have been used for development of algorithms to remedy the uncertainties associated with the filter-based techniques. Photoacoustic techniques have the advantage to measure particle absorption in their natural atmospheric state suspended in air (Arnott et al., 1999). However, they suffer from artifacts related to the gas composition and are less robust and sensitive than the filter-based techniques. An individual particle analysis with a laser-induced incandescence (LII) technique is to date the most accurate and sensitive method to measure the absorbing mass content, the so called refractory black carbon (rBC) mass, of the aerosol. The existing LII techniques are expensive and complex, and converting the rBC signal to atmospheric absorption is not straightforward (Schulz et al., 2006; Schwarz et al., 2006). A simultaneous measurement of the aerosol extinction and scattering is yet another alternative that allows to derive the aerosol absorption indirectly (Strawa et al., 2003; Virkkula et al., 2005). A review of methods with their common pros and cons is provided by Moosmuller et al. (2009).

50 The different methods to measure aerosol light absorption have been compared and verified in previous laboratory (Saathoff et al., 2003; Slowik et al., 2007; Müller et al., 2011) and field (Reid et al., 1998; Schmid et al., 2006; Kanaya et al., 2008; Kondo et al., 2011; Backman et al., 2017; Laing et al., 2020) campaigns. The campaigns have focused on characterizing uncertainties of the different absorption techniques and examined their response to varying absorbing aerosol sources. Reid et al. (1998) measured Brazilian biomass burning aerosol using six different techniques, concluding about 20% convergence

55 between them. Kanaya et al. (2008) found an overall good agreement between the results of different instruments, but the discrepancies increased at high Organic Carbon (OC) content. Schmid et al. (2006) measured the Amazon biomass burning aerosol using various methods and estimated 15% and 20% accuracy, for PSAP and Aethalometer measurement, respectively. Better agreement, in terms of eBC mass, can be expected when solely non-volatile absorbing particle is analyzed avoiding any artifacts from volatile light scattering particles (Kondo et al., 2011).

60 Accuracy of the aerosol absorption measurement methods needs to be improved to reduce the uncertainties associated with their climate impacts. Absorbing aerosol has an accelerating impact on the global temperature rise, which is further intensified over the Polar Regions due to the regional strong climate feedbacks. The aerosol light absorption, and its spatial and temporal variability, are therefore of specific concern in the Arctic. Absorption measurements in the Arctic require sensitive and robust techniques. Previous work have presented data analysis techniques aimed to improve the detection capabilities of the absorption  
65 instruments (Springston et al., 2007; Hagler et al., 2011; Backman et al., 2017), yet the instruments inter-comparisons are view. The co-located PSAP and CLAP instruments showed a good agreement in a real-world Arctic inter-comparison (Ogren et al., 2017), but the study did not include Aethalometer or MAAP instruments, which are slightly different techniques. The co-located aethalometers in the Arctic showed relatively more discrepancies, which were discussed by Mölders and Edwin (2018). However, to the best of our knowledge, comprehensive studies of co-located parallel filter-based instruments inter-comparisons  
70 in pristine field environments are lacking and that is one reason for the poorly quantified Arctic absorption baseline. Recently, Backman et al. (2017); Schmeisser et al. (2018) found significant spatial differences in aerosol light absorption seasonal characteristics in the Arctic. All long-term aerosol absorption data series from the Arctic are measured using filter-based methods. Backman et al. (2017) used the co-located measurements to construct a homogeneous dataset for multiple Arctic sites, but the instruments were never applied all in parallel. Such a parallel comparison in the Arctic would assist to estimate  
75 the uncertainties associated to these measurements.

The EMPIR BC project develops metrology for light absorption by atmospheric aerosols. It aims at finding standard reference materials that mimic the atmospheric absorbing aerosol and a traceable, primary method to determine the aerosol absorption coefficients. An additional goal of the EMPIR BC project is to develop a validated transfer standard for field calibrations. The Pallas campaign was the first field campaign in the project. The goal was to test the stability, accuracy and  
80 detection capabilities of the commonly available absorption measurement methods focusing on the filter-based techniques, and to conclude on their applicability in pristine environments. To our knowledge, this is the most comprehensive absorption and BC mass measurement instrument parallel field comparison done in the Arctic.

## 2 Methodology

### 2.1 The Pallas site description

85 The Pallas atmosphere ecosystem supersite is located in the northern Finland inside the Arctic. It is part of the Pallas-Sodankylä Global Atmospheric Watch (GAW) station and contributes to various national and international networks and programmes. Important in this context is the Aerosols, Clouds, and Trace gases Research InfraStructure (ACTRIS) to which Pallas provides

quality controlled and continuous data on aerosol number, size and optical properties. The main station for aerosol measurements at Pallas is on top of the Sammallunturi fell (67° 58 N', 24° 07' E, 560 m a.g.l.) where also the EMPIR BC field campaign was organized. A detailed description of the site, its surroundings and on-going measurement programmes were published earlier by Hatakka et al. (2003); Lohila et al. (2015).

The EMPIR BC field campaign took place during the Nordic summer, between 19.6 – 17.7.2019. A summary of the instrumentation used with corresponding settings during the campaign are presented in Table 1. Each instruments operational principle and respective data corrections are presented in detail below.

## 95 2.2 Aerosol optical properties

Table A1 summarizes the quantities that frequently appear in this manuscript text. All the filter-based instruments target to achieve aerosol light absorption coefficients  $\sigma_{AP,\lambda}$  at instrument specific wavelengths  $\lambda$ , which are acquired from the measured light attenuation using signal post-processing.  $\sigma_{AP,\lambda}$  is a measure of the absolute magnitude of atmospheric absorption, or the cross-section of light-absorbing material (BC) available in a volume of air in which this material exists. This cross-section can be normalized to particle mass by a simple factor called mass absorption cross-section (MAC) (Bond and Bergstrom, 2006). Some applications, such as atmospheric modeling, favor the use of BC mass over the absorption coefficient, for which the value of MAC needs to be known.

Here, when referring to a corrected absorption coefficient measured using a particular technique, a notation  $\sigma_{INST,\lambda}$ , where INST is an abbreviation of the technique, is used. When referring to an aerosol light absorption coefficient value directly reported by the instrument,  $\sigma_{0,\lambda}$  is used instead.

A typical measure of aerosol "brightness" is the ratio of aerosol scattering  $\sigma_{SP,\lambda}$  to aerosol extinction  $\sigma_{EP,\lambda}$ , a parameter called single-scattering albedo

$$\omega_{0,\lambda} = \frac{\sigma_{SP,\lambda}}{\sigma_{EP,\lambda}} = \frac{\sigma_{SP,\lambda}}{\sigma_{SP,\lambda} + \sigma_{AP,\lambda}}, \quad (1)$$

which is of great significance when assessing the radiative forcing of the aerosols. The scattering wavelength dependence is described as

$$\sigma_{SP,\lambda_1} / \sigma_{SP,\lambda_2} = (\lambda_1 / \lambda_2)^{-\alpha_{SP,\lambda}}, \quad (2)$$

where  $\alpha_{SP,\lambda}$  is called the Ångström exponent of scattering and is related with the aerosol optical size. A similar wavelength dependent parameter,  $\alpha_{AP,\lambda}$ , can be defined for aerosol absorption.

Interpolation of  $\sigma_{SP,\lambda}$  to any wavelength  $\lambda$  was done by applying the calculated Ångström exponent at the nearest available wavelengths (Anderson and Ogren, 1998). Interpolation of  $\sigma_{AP,\lambda}$  to a wavelength  $\lambda$  was done by assuming a simple relation between the wavelengths and variation in  $\alpha_{AP,\lambda}$  was not accounted for due to high noise in data.

## 2.3 Instruments

Data from five filter-based absorption photometers, two instruments that measure aerosol scattering, two instruments that measure aerosol extinction and one instrument that measure refractory BC are used in this paper. The data were corrected with the best practices considered for each particular instrument independently, following the global guidelines, literature citations and earlier work done at the station.

The flow rate of each instrument was measured at the beginning and at the end of the campaign with a Gilian flow calibrator (volumetric flow rate), and converted to standard (STP) conditions (0°C, 1013hPa) after which the flow correction based on the equation 5 in Bond et al. (1999) was applied. Instrument flow rates are shown in Table 1.

### 2.3.1 AE31

Aethalometer model AE31 (Magee Scientific Inc.) is part of the permanent installation at Pallas site since year 2005 (Lihavainen et al., 2015). It measures the aerosol absorption coefficient at seven wavelengths: 370 nm, 470 nm, 520 nm, 590 nm, 660 nm, 880 nm and 950 nm. The measurement principle is based on the observed light attenuation caused by the particles that are continuously collected on a filter tape (Hansen et al., 1982, 1984). The aerosol attenuation coefficient is then calculated as

$$\sigma_{0,\lambda} = \frac{A}{Q * 100} * \frac{\Delta ATN}{\Delta t}, \quad (3)$$

where A is the filter spot size, Q is the flow rate and  $\Delta ATN$  is the measured change in the attenuation during the time interval  $\Delta t$  (e.g. Backman et al. (2017) Eq. (1)). AE31 changed the filter spot automatically when a pre-set limit value of  $ATN = 60$  was reached. The instrument reports data in eBC mass concentration which is simply the measured aerosol absorption coefficient corrected with a wavelength dependent specific attenuation.

The AE31 data measured at Pallas was corrected for the multiple scattering of light by filter fibers by dividing  $\sigma_{0,\lambda}$  with a multiple scattering enhancement factor,  $C_0 = 3.5$ , which is selected according to the global recommendation of the Global Atmospheric Watch's World Calibrations Centre for Aerosol Physics (GAWReport No. 227; <http://wmo-gaw-wcc-aerosol-physics.org/wmo-gaw-reports.html>), and is also very close to the  $C_0$  factor for the Arctic given by Backman et al. (2017). The filter loading artifact was corrected using the method by Virkkula et al. (2007, 2015), and the Pallas station specific correction factor  $k = 0.0038$  (Backman et al., 2017). Note that this correction is a loading correction only, unlike the algorithms of Arnott et al. (2005) and Collaud Coen et al. (2010) in which a fraction of scattering coefficient is subtracted from  $\sigma_{0,\lambda}$ .

### 2.3.2 AE33

An updated version of the AE31 is the dual-spot aethalometer model AE33 (Drinovec et al., 2015). The instrument reports an aerosol light absorption coefficient based on the measured attenuation on two parallel filter spots with different particle loadings. It applies a real-time loading effect compensation algorithm that is essentially based on the work by Virkkula et al. (2007). The Pallas AE33 uses an internal multiple scattering correction factor  $C_0 = 1.39$  (Drinovec et al., 2015). This was corrected to a value  $C_0 = 3.5$  in order to comply with the global recommendation (GAWReport No. 227; <http://wmo-gaw-wcc-aerosol->

physics.org/wmo-gaw-reports.html). No clear consensus or published recommendation for the AE33 specific global scattering correction factor  $C_0$  yet exist, although it is clear that the correction by the manufacturer is too low for most atmospheric

150 aerosols (Laing et al., 2020). The AE33 at Pallas was programmed to change the filter spot automatically every 24h.

### 2.3.3 MAAP

The Multi Angle Absorption Photometer (MAAP) model 5012 (Thermo Scientific) has been frequently used as an absorption reference for the filter-based absorption instrument techniques (Müller et al., 2011). It internally corrects for the scattering artifact by using a simultaneous back-scattering measurement of the filter tape at multiple angles. In general, the data need  
155 very little post-processing. MAAP measures absorption at a wavelength of 637 nm. A wavelength shift from the nominal value was reported by Müller et al. (2011), and requires a correction with a multiplier 1.05. This correction was applied also here. Pallas MAAP was set to report eBC directly at STP conditions and no further corrections were thus applied. In polluted environments the MAAP internal data averaging procedure can lead to an artifact that needs to be corrected as suggested by Hyvärinen et al. (2013).

### 160 2.3.4 PSAP

The Particle Soot Absorption Photometer (PSAP; Radiance Research) measures aerosol light attenuation at wavelengths 467, 530, and 660 nm (Bond et al., 1999). The PSAP, in contrast to the other filter-based techniques used, requires a manual filter spot change. This was done when the transmittance reported by the instrument decreased from the initial value of 1.0 to a range of 0.8–0.7. The flow rate of PSAP was set at 1 LPM.

165 PSAP records the signal, reference and dark count data at 4s time resolution, which was hourly averaged to calculate the absorption coefficients. The data were corrected with the measured filter spot size and flow rate as suggested by Bond et al. (1999); Ogren (2010). An average of five spot sizes was determined to be  $A = 18.63 \text{ mm}^2$ . The volumetric flow rate was measured at 15 different adjusted flow rate settings at the beginning and at the end of the campaign. The results were converted to standard flow rate and a linear fit was made to the data, resulting in a flow correction factor of 1.12.

170 The obtained aerosol absorption coefficient was corrected for the filter-tape loading and scattering artifacts using the correction scheme by Virkkula (2010)

$$\sigma_{\text{PSAP},\lambda} = (k_0 + k_1(h_0 + h_1 * \omega_{0,\lambda}) \ln(\text{Tr}_\lambda)) \sigma_{0,\lambda} - s * \sigma_{\text{SP},\lambda}, \quad (4)$$

where  $k_0$ ,  $k_1$ ,  $h_0$ ,  $h_1$  and  $s$  are wavelength dependent constants given by Virkkula (2010).  $\text{Tr}_\lambda$  is the transmittance measured by PSAP at a wavelength  $\lambda$  and  $\sigma_{\text{SP},\lambda}$  are the corresponding scattering coefficients. The scattering coefficients were measured  
175 with a nephelometer (TSI Inc. model 3563) and interpolated to the three PSAP wavelengths using the calculated Ångström exponent values  $\alpha_{\text{SP},\lambda}$ . The single scattering albedo  $\omega_{0,\lambda}$  in Equation 4 was iterated until no significant change in  $\sigma_{\text{PSAP},\lambda}$  was observed. At large values of  $\omega_{0,\lambda}$  such as here, this correction scheme approaches the widely applied Bond-Ogren correction scheme (Bond et al., 1999; Ogren, 2010). However, it should be noted that at high  $\omega_{0,\lambda}$  values the corrected  $\alpha_{\text{AP},\lambda}$  becomes

uncertain and should be interpreted with caution, as shown in Backman et al. (2014) Figure 7: inter-comparison of correction algorithms.

### 2.3.5 COSMOS

The continuous soot monitoring system (COSMOS) measures light attenuation at a wavelength of 565 nm. The measurement principle is similar to the other filter-based absorption photometers but differs in a sample pre-treatment (Miyazaki et al., 2008; Kondo et al., 2009). In the COSMOS inlet the volatile non-refractory aerosol components are removed by heating the sample to 300°C (Kondo et al., 2009). The COSMOS mechanical and optical design with the determined instrument detection limit and measurement uncertainties are presented by Miyazaki et al. (2008). Due to efficient elimination of the aerosol scattering related artifacts this method is typically found in good agreement with the thermal-optical and the laser-induced incandescence techniques (Kondo et al., 2009, 2011), and not directly comparable to other filter-based absorption measurements. Each COSMOS is calibrated against a standard COSMOS instrument using ambient absorbing aerosol within an accuracy of about 5%. The standard COSMOS, in turn, is calibrated by SP2 using ambient absorbing aerosol and applying an aerosol specific MAC. At Pallas, we applied a MAC of  $8.73 \text{ m}^2 \text{ g}^{-1}$  to calculate the absorption coefficient from the COSMOS data (Sinha et al., 2017). Detailed comparison of COSMOS and SP2 measurements at several sites in Asia and the Arctic have demonstrated that the overall accuracy in the absorbing aerosol mass concentration measurement is about 10% (Sinha et al., 2017; Ohata et al., 2019, 2020). The stability of MAC is explained by the elimination of the artifacts from aerosol scattering. At Pallas, COSMOS was operated at 0.7 LPM flow rate (STD) and the data was saved every 1-min.

### 2.3.6 SP2

The single particle soot photometer (SP2, Droplet Measurement Technologies Inc.) measures refractory black carbon (rBC) mass in particles  $>70 \text{ nm}$  in diameter (Schwarz et al., 2006). The measurement principle is based on a laser-induced incandescence where the particle is heated up to the point of incandescence which is picked up by the instruments detectors (Stephens et al., 2003). The incandescence signal is proportional to the mass of the refractory black carbon which is calculated particle-by-particle to obtain the rBC mass concentration (Laborde et al., 2012). This technique is both sensitive and accurate and is here used as a reference for the rBC mass concentration in the field.

### 2.3.7 CAPS

The cavity attenuated phase shift light extinction monitor (CAPS PMex, Aerodyne Research Inc.) instrument measures total light extinction by aerosol particles ( $\sigma_{EP,\lambda}$ ) utilizing a cavity attenuated phase shift principle (Kebabian et al., 2007; Massoli et al., 2010; Petzold et al., 2013; Perim de Faria et al., 2017). An updated model of CAPS is the CAPS PMssa (CAPSssa, Aerodyne Research Inc.). CAPSssa additionally measures the aerosol light scattering allowing the single scattering albedo to be determined with a single instrument (Onasch et al., 2015; Modini et al., 2021). The scattering measurement technique is similar to an integrating nephelometer, and utilizes a Lambertian integrating sphere in the sample cell. The aerosol light

210 scattering measurement by CAPSssa is affected by background, truncation and light-source related uncertainties for which calibration is needed.

Aerosol extinction measurement with CAPS is nearly a calibration free technique as long as frequent baseline measurements are performed. A potential source of systematic bias is the geometry correction factor. This is generally a stable constant but has been shown to vary between instruments of even the same model (Petzold et al., 2013; Onasch et al., 2015). An accurate  
215 aerosol extinction measurement thus requires calibration against a calibrated scattering instrument, generally a nephelometer.

CAPSex and CAPSssa that were operated at Pallas both measure at a wavelength of 630 nm. They were calibrated in the beginning, middle and end of the campaign using ammonium sulfate aerosol generated with an atomizer.

### 2.3.8 Nephelometer

Aerosol light scattering is continuously monitored at Pallas Sammaltunturi site with an integrating nephelometer (TSI3; TSI,  
220 model 3563) (Anderson and Ogren, 1998; Heintzenberg et al., 2006). It measures aerosol total scattering and back-scattering fraction at three wavelengths: 450 nm, 550 nm and 700 nm. Nephelometer data were corrected for truncation as suggested by Anderson and Ogren (1998) and converted to standard atmospheric conditions (STP).

During the EMPIR campaign the aerosol light scattering was also measured with an Aurora integrating polar nephelometer (AUR4; Ecotech, model 4000) at two angles: 90 and 180. In this setup, the Aurora nephelometer measures the total scattering  
225 (180) and back-scattering (90) of the aerosol in similar manner as the TSI nephelometer. The Aurora 4000 measures scattering at wavelengths of 450 nm, 525 nm, and 635 nm. Data were corrected for truncation based on Müller et al. (2011) and converted to STP.

A zero check was performed daily for both nephelometers and they were calibrated with CO<sub>2</sub> gas in the beginning and in the end of the campaign.

### 230 2.3.9 Extinction Minus Scattering (EMS)

An indirect technique to determine the aerosol light absorption is based on separately measured aerosol extinction and aerosol scattering (Strawa et al., 2003; Virkkula et al., 2005; Modini et al., 2021). This extinction minus scattering (EMS) -method relies on those aerosol optical properties that can be accurately determined using existing techniques. It is also traceable to SI units. The EMS method avoids the artifacts encountered with filter-based techniques.

235 In Pallas the aerosol light scattering was measured with two integrating nephelometers and the extinction with CAPSex and CAPSssa instruments. Two instrument "pairs" were formed: (1) Aurora 4000 polar nephelometer and CAPSssa (both were part of campaign instrumentation) and (2) CAPSex and the TSI nephelometer (permanent instrumentation at site). These methods here are referred to as EMS<sub>1</sub> and EMS<sub>2</sub>, respectively. The CAPSssa scattering and extinction measurement alone was also used to determine aerosol absorption, which is here referred to as method EMS<sub>3</sub>.

240 In the beginning, middle and end of the campaign the CAPS instruments data were calibrated against the nephelometers. Purely scattering ammonium sulphate aerosol was produced with an atomizer (TOPAS, model ATM230). The aerosol losses in the sampling lines and in the instruments are size dependent and the  $\alpha_{SP,\lambda}$  reflects the optical size of the aerosol. In Pallas



summer atmosphere a typical value of  $\alpha_{SP,\lambda} = 1.5 - 1.7$  (Lihavainen et al., 2015). The ammonium sulphate calibrations were performed at this  $\alpha_{SP,\lambda}$  range so that the calibrations will be valid for the ambient aerosol as well. A summary of the three calibrations proposed multipliers of 1.21 (EMS<sub>1</sub>) and 1.04 (EMS<sub>2</sub>) for CAPS data (Figure S1). These correction factors were applied to all CAPS data in this manuscript. The different correction factors for the CAPSex and CAPSssa could be explained by the different individual geometry correction factors. The two CAPS were having identical flow rates and inlet settings, and the two nephelometers (reference points) had a small difference in flow rates and in inlet tubing sizes which could to a minor part also explain the differences in correction factors. However, the discrepancies in nephelometers were very minor in comparison to those in CAPS.

## 2.4 Sampling

The bulk of the instruments were connected to a common inlet which was equipped with a Particulate Matter (PM) 10  $\mu\text{m}$  cut-size aerosol inlet head and a nafion permapure model MD-700-48 aerosol drier. The relative humidity (RH) of the sample in the entrance of the inlet was monitored to remain  $<40\%$  throughout the campaign. The total flow of 18.3 LPM was divided for the instruments via a self-made flow-divider that consisted of six cylinder symmetric exit tubes. One of the exits was further divided using a TSI laminar flow-divider into two flows, one for each extinction monitor (CAPSex and CAPSssa, see Table 1). In addition, two instruments (SP2 and AE31, see Table 1) were connected to a slightly heated, total aerosol inlet about 3 m apart from the PM10 line. The AE31 is measuring in this inlet year-round and the SP2 has a limited measurement size range for which the inlet cut-size does not affect the result in cloud-free conditions.

## 260 3 Results

### 3.1 Allan variance analysis on absorption methods stability and detection limits

Detection limits and optimal averaging times for the absorption measurement instruments were defined using Allan variance analysis. Allan variances describe the time-averaged stability of a series of consecutive measurements and can be used to estimate noise processes (Allan, 1966; Werle et al., 1993). They determine the data variability by analyzing the sum of the squared differences between the measurements subsets in such a way that if N is the number of subsets of  $y_j$  measurements, the Allan variance for a time period t is defined as

$$\sigma_y^2(t) = \frac{1}{2(N-1)} \sum_{j=1}^{N-1} (y_{j+1} - y_j)^2. \quad (5)$$

The Allan variances can be used to find the optimal averaging time that minimizes the noise without sacrificing the signal. For a white noise dominated system the square root of the variance, called Allan deviation, is equal to the standard deviation of the mean and gives directly the  $1\sigma$  detection limit (Werle et al., 1993).

Noise in the measured absorption signal was determined during a 6 hours period of clean, particle-free measurements. Allan deviation for the different absorption methods in this study was calculated for data averaging times from 1 minute to 6 hours

(Figure 1). The lowest Allan deviation minimum was measured by PSAP, and followed by AE33, COSMOS, MAAP and AE31, in the order from lowest to highest (Figure 1a). The absorption coefficients measured by the three EMS methods were about an order of magnitude higher in Allan deviation when compared to the values determined for the filter-based methods (Figure 1b). The minimum Allan deviation in PSAP data was obtained with an averaging time of about an hour, after which a strong increase ( $1/t$ -dependence) in noise occurred. Deviation from the typical behavior of a white noise dominated system (i.e.  $1/\sqrt{t}$ -dependence) can be expected for PSAP as was shown by Springston et al. (2007). The increasing Allan deviation of the absorption at the averaging times of  $>1$  hour that was observed in PSAP indicates system drifts. A similar drift-effect could be interpreted to take place in AE33 and COSMOS instruments at  $>2.5$  hours data averaging times. The EMS methods showed a constant decrease of a white noise signal from 10 minutes to longer averaging times. Out of the three EMS methods used, the EMS3 that measured both extinction and scattering with a single instrument, here presented the lowest noise. While it is known that the EMS method is very sensitive to error amplification, the accuracy of this result can still be compromised (Modini et al., 2021).

The  $1\sigma$  detection limits of different  $\sigma_{AP,637nm}$  measurement methods were calculated as an average of the Allan deviation between 1–2 hours averaging times and are presented in Table 2. The lowest detection limit of  $0.002 \text{ Mm}^{-1}$  was calculated for PSAP, while it was  $0.01 \text{ Mm}^{-1}$  for MAAP,  $0.1 \text{ Mm}^{-1}$  for EMS3 and  $0.8 \text{ Mm}^{-1}$  for EMS2. Qualitatively and in comparison to each others, the instruments detection limits followed those provided by the instrument manufacturers, although the determined  $1\sigma$  absolute values were all slightly lower than predetermined (Table 1).

The above stability analysis is used to justify our choice to use hourly-averaged absorption data in the further analysis of this work.

### 3.2 Aerosol absorption coefficient values measured in Arctic air masses

The absorption instruments were used in parallel to measure atmospheric aerosol in Pallas campaign. Arctic air masses prevailed during all the campaign and correspondingly very low aerosol concentrations were measured (Figure 2). The aerosol was highly scattering, with an average single-scattering albedo of 0.97. These conditions challenged the detection capabilities of the absorption measurement methods used. The aerosol absorption coefficient  $\sigma_{AP,630nm}$  measured with filter-based instruments varied between 0 and  $0.3 \text{ Mm}^{-1}$  (Figure 2a). The variability of  $\sigma_{AP,630nm}$  with time measured by the EMS methods differed 10-fold in absolute numbers giving a range between 0 and  $3 \text{ Mm}^{-1}$  (Figure 2b). In qualitative terms they assembled the extinction and scattering time series (Figure 2c). A plausible explanation for this clear over-estimation of absorption by the EMS method is that it is calculated by taking the difference of two large and noisy numbers.

Both absorption and scattering increased slightly on a second half of the campaign from July 7 onwards (Figure 2c). The maximum  $\sigma_{EX,630nm}$  of around  $25 \text{ Mm}^{-1}$  were observed on July 8 and on July 16. During these high-concentration episodes PSAP seemed to under-estimate the absorption, when compared to the other filter-based instruments and especially the reference MAAP. Particularly high  $\omega_0$  of  $>0.99$  was measured on both these cases. The wavelength dependent scattering correction function that was applied to PSAP data could thus overestimate the correction when extremely high scattering values are measured and in particular at the higher wavelengths. Essentially an opposite behavior was observed on July 14 when PSAP and

MAAP coincided in absorption while the other filter-based instruments under-estimated the absorption. In this case the  $\omega_0$  was in range 0.85 – 0.95, which is rather low for Pallas.

The median aerosol absorption coefficients  $\sigma_{AP,635nm}$  measured by the five filter-based methods during the campaign were within the limits from 0.07 to 0.09  $Mm^{-1}$  (Table 3). The overall median using data from all instruments was 0.08  $Mm^{-1}$  and the 25th and the 75th percentiles were 0.06 and 0.10  $Mm^{-1}$  (Figure 3). The measured atmospheric absorption coefficient values with their standard deviation range exceeded the instruments detection limits for all the five filter-based methods (Table 2). The lowest average  $\sigma_{AP,\lambda}$  was measured with COSMOS instrument along with the lowest standard deviation of data (Figure 3). This is expected since the sample pre-treatment in the COSMOS heated inlet effectively removes the particle light scattering coating thereby eliminating the related artifacts. Heating also decreases fluctuations caused by possible sample RH variations. However, the sample modification also changes the aerosol interaction with light which then no longer corresponds to its dry atmospheric state. Therefore, this method is primarily used to determine the mass of the absorbing refractory particles, rather than the aerosol light absorption in the atmosphere. A low standard deviation around the average was also measured by the AE33. The highest average  $\sigma_{AP,\lambda}$  was measured by the AE31 instrument. This could be explained by this methods' sensitivity to various artifacts and thus, a significant dependence on the aerosol characteristics.

The EMS methods systematically overestimated the aerosol absorption coefficient, giving a campaign-average medium of 0.59  $Mm^{-1}$  and the 25th and the 75th percentiles of 0.44 and 0.74  $Mm^{-1}$  when considering all EMS data (Figure 3). The absorption values measured at Pallas are clearly below the detection capabilities of the EMS methods, as already suggested by the results from the previous section. The baseline drift and the error amplification are known to affect the EMS methods detection limits (Modini et al., 2021). The calculated standard deviation around the average  $\sigma_{AP,\lambda}$  was more significant than the signal height in all three EMS methods (Table 3).

### 3.3 Representativeness of the measured absorption values

The measured absorption coefficient values are in the lower end of that typically observed at Pallas site. Lihavainen et al. (2015) long-term analysis showed that the  $\sigma_{AP,50nm}$  in Pallas during summer ranges between 0.05–1  $Mm^{-1}$  (10 – 90 percentile range), where the lowest values correspond to the clean Arctic air flows. Summer is also the season of the highest  $\omega_0$  in all the year, with values ranging from 0.90 to 0.98 (Lihavainen et al., 2015). Both the Arctic marine and the continental air masses are observed during summer season, and typically with similar probability of occurrence. Thus, having our campaign-time air masses 100% from the Arctic was rather unexpected and focuses our conclusions to pristine environments.

Indeed, the  $\sigma_{AP,\lambda}$  values measured during the Pallas campaign are well representative of those observed at around the Arctic during summer (Schmeisser et al., 2018). In a majority of the Arctic region, a minimum in absorption is observed during summer and early autumn when the monthly median  $\sigma_{AP,550nm}$  remains below 0.1  $Mm^{-1}$  for 4–5 months (Schmeisser et al., 2018). Quantification of this Arctic absorption concentration baseline thus requires well calibrated, accurate techniques. An additional measurement challenge is that the Arctic aerosol is particularly bright with  $\omega_0$  typically exceeding 0.95 (Schmeisser et al., 2018). The filter-based techniques and correction schemes are known to be particularly sensitive and noisy at high values of  $\omega_0$  (Backman et al., 2014; Ogren et al., 2017).

### 3.4 Accuracy of the measured absorption

The accuracy of the filter-based methods was further investigated by comparing them between each others using MAAP as a main campaign-time reference. MAAP is known to be essentially an artifact-free technique to measure aerosol absorption on a filter and has been widely utilized as a practical field reference method also in the past.

345 Linear correlation between the absorption coefficients measured with different techniques was calculated using the Williamson-York bivariate fitting method provided by Cantrell (2008). This method is less sensitive to outliers than the standard least-squares method, and considers that uncertainties can exist in both fitting variables which here is the case. The correlation statistics ( $R^2$ , slope and intercept with their corresponding standard errors) for the filter-based techniques are presented in Table 4. All correlations were statistically highly significant.

350 The best correlation was obtained with  $\sigma_{\text{AE33},\lambda}$  and  $\sigma_{\text{MAAP},\lambda}$ , followed by  $\sigma_{\text{COSMOS},\lambda}$  and  $\sigma_{\text{MAAP},\lambda}$  ( $R^2 = 0.87$  and  $0.85$ , respectively). Correlation between  $\sigma_{\text{AE31},\lambda}$  and  $\sigma_{\text{MAAP},\lambda}$  was noisy and resulted in the lowest  $R^2 = 0.65$ . Both AE31 and PSAP compared to MAAP showed nearly a linear correlation of  $\sigma_{\text{AP},\lambda}$ , with a slope of 0.95 and 0.93, respectively, and an offset of 0.01. The scattering correction that was done for PSAP data is a plausible explanation for the lower  $R^2 = 0.78$ . The AE33 appeared to overestimate the  $\sigma_{\text{AP},\lambda}$  at the lowest measured absorption values, while it slightly underestimated at the  
355 other end of the scale. This led to a correlation slope significantly below one, as compared to MAAP. Both COSMOS and AE33 correlations were low, 0.68 and 0.62, respectively, but in COSMOS this is explained by the sample pre-treatment in inlet which modifies the sample composition. The low correlation slope of AE33 seems to be rather explained by the deviation of data near the zero values. Overestimation of  $\sigma_{\text{AP},\lambda}$  at values close to zero as compared to MAAP was notable in all instruments data, except in AE31 (Figure 4).

360 Figure 4 additionally shows that aerosol absorption increases with decreasing single scattering albedo  $\omega_0$ . This can be a real effect but can also partly relate with the decreasing accuracy in  $\sigma_{\text{AP},\lambda}$  result at the edge of the instruments detection limits, affecting the scattering to absorption ratio. In case of PSAP this is in agreement with the discrepancies observed in time series analysis at high  $\omega_0$  values.

Given that the measured absorption coefficients are close to the detection limits of the instruments the obtained correlations  
365 are reasonably good. Slopes and intercepts could be modified with a different selection of data outliers which at such low concentrations can be a sensitive choice. Comparison of  $\sigma_{\text{AP},\lambda}$  measured with EMS methods to the hourly-averaged values from MAAP did not lead to statistically highly significant correlations.

### 3.5 Mass absorption cross-section of Arctic aerosol

The absorbing particle mass based on the measured absorption coefficient can be calculated with a suitable selection of the mass  
370 absorption cross-section (MAC). We defined the average MAC during our campaign by comparing the measured absorption by MAAP with the measured rBC mass by SP2, extending the range from zero to  $18 \text{ ng m}^{-3}$  (Figure 2d). This analysis resulted in a MAC value of  $16.0 \text{ m}^2 \text{ g}^{-1}$  (Figure 5). The default MAC in MAAP is  $6.6 \text{ m}^2 \text{ g}^{-1}$ , which gives a ratio of 2.4 between the black carbon mass equivalent and the refractory black carbon mass.

375 The MAC is not a constant value and can depend on various factors such as the absorbing aerosol source and the aerosol mixing state that is subject to its atmospheric aging (Jacobson , 2001; Slowik et al., 2007; Petzold et al., 2013; Ohata et al., 2020). Recently, a comprehensive characterization of the Arctic MAC values was published by Ohata et al. (2020). Their results were calculated for a dataset covering a broad range of absorption values measured around the Arctic using COSMOS as a reference mass monitor. The overall average MAC in their study was  $14.0 \text{ m}^2 \text{ g}^{-1}$ , and thus on the same order of magnitude as obtained here for Pallas site when comparing MAAP directly with the SP2.

#### 380 4 Discussion and conclusions

Absorbing aerosol characteristics were measured by various methods and instruments in an EMPIR BC month long measurement campaign at remote Pallas station in northern Finland. Arctic air masses prevailed and consequently very clean and highly scattering aerosol persisted throughout the campaign. This was a challenge for the absorption instrumentation in terms of their accuracy and detection limits.

385 We determined the  $1\sigma$  -detection limits of  $\sigma_{AP,637nm}$  for five filter-based absorption monitors: MAAP, AE31, AE33, PSAP, COSMOS, and for the extinction minus scattering (EMS) method with three different instrument pairs using Allan variance analysis by data averaging at 1–2 hours interval. The detection limits of filter-based instruments were in range  $0.002 \text{ Mm}^{-1}$  –  $0.014 \text{ Mm}^{-1}$ . The lowest detection limit was calculated for PSAP and the highest for AE31. The detection limits of EMS methods were an order of magnitude higher, ranging from  $0.38$  to  $0.11 \text{ Mm}^{-1}$ . As a general rule our results suggest that the filter-based absorption instruments can be applied down to  $\sigma_{AP,\lambda} = 0.01 \text{ Mm}^{-1}$  and **the EMS methods are not applicable at  $\sigma_{AP,\lambda} < 0.1 \text{ Mm}^{-1}$ , at least in these high  $\omega_0$  values as in this study.**

The aerosol absorption coefficient measured at Pallas ranged from  $0.06$  to  $0.10 \text{ Mm}^{-1}$  (representing the 25th to 75th percentiles) and the different filter-based instruments agreed approximately within 15–20%. This was at a lower edge of the absorption coefficients typically measured at the site, but is well representative for Arctic summer conditions. AE33 showed the best linear correlation with MAAP ( $R^2 = 0.87$ ), followed by COSMOS ( $R^2 = 0.85$ ) and PSAP ( $R^2 = 0.78$ ). **The scattering correction that was applied to PSAP data at the measured low absorption values improved the correlation with MAAP at low  $\omega_0$  values but led to an under-estimation and increased noise at extremely high  $\omega_0$  values  $> 0.99$ .** The noisy data of AE31 resulted in a slightly lower, yet a highly significant, correlation ( $R^2 = 0.65$ ). A positive bias at low  $\sigma_{AP,\lambda}$  values near zero levels was observed in AE33, PSAP and COSMOS. The correlation slope with MAAP was close to one in PSAP and AE31, but clearly below one in COSMOS and AE33. It has to be kept in mind that these results were calculated for a very clean environment and at a relatively narrow  $\sigma_{AP,\lambda}$  range from 0 to  $0.3 \text{ Mm}^{-1}$ . Thus the biases observed at around zero concentrations can affect significantly the correlation slopes.

405 Finally, we determined the aerosol MAC value during the campaign using SP2 as a mass reference and MAAP as an absorption reference. The MAC, determined as a slope of the correlation between those two, was  $16.0 \text{ m}^2 \text{ g}^{-1}$  and is thus in good agreement with previous similar Arctic MAC studies.

Overall, the filter-based absorption instruments are shown to be a robust and sensitive method to measure absorption in pristine environments, such as the Arctic. A sufficient averaging of data to reach at least the minimum of instruments detection limit and an utilization of co-located instruments as transfer standards to better estimate data precision are recommended. Co-located scattering measurements for data post-correction was shown to be beneficial. Special caution in data analysis when highly scattering aerosol is present is required. In addition, our results suggest that modernization of instrumentation can provide clear benefits in data quality. Future studies should focus on providing the means for field instruments reference and calibration methods to further improve the accuracy of the filter-based methods.

*Data availability.* Pallas WMO Global Atmospheric Watch (GAW) station, part of the Aerosols, Clouds, and Trace gases Research Infrastructure (ACTRIS), submits aerosol number, size, scattering and absorption measurement data annually to EBAS database operated at the Norwegian Institute for Air Research (NILU) (<http://ebas.nilu.no>). These data are available at no cost and can be used in agreement with the ACTRIS Data Policy statement. The specific data measured during EMPIR BC campaign are available for scientific use upon request. Aurora 4000 data are available at TROPOS, CAPS data at DEMOKRITOS and all other data at FMI by contacting the corresponding data owner and co-author in this manuscript.

*Author contributions.* EA, HS, JB, MG, KE, TM and AH participated in planning the campaign. EA, JB, HS and MG made the measurements. EA analysed the filter-based instrument absorption data and all auxiliary data with contributions from AV and JB. JB analysed SP2 data. MG and KE analysed CAPS data. TM analysed Aurora nephelometer data. SO, YK and HS analysed COSMOS data. EA prepared the paper with contributions from all authors.

*Competing interests.* Authors do not declare any competing interests.

*Acknowledgements.* We greatly acknowledge the funding from the 16ENV02 Black Carbon project of the European Union through the European Metrology Programme for Innovation and Research (EMPIR). The financial support of the ACTRIS by the European Union's Horizon 2020 research and innovation programme under grant agreement no. 654109 is also gratefully acknowledged. This research was also supported by Academy of Finland via project NABCEA (grant no. 29664) and by Business Finland via project BC Footprint (grant no. 49402-201040). This work was also supported by the Environmental Research and Technology Development Fund (2-2003), and the Arctic Challenge for Sustainability II (ArCS II) project of Japan.

## 430 References

- Allan, D. W.: Statistics of Atomic Frequency Standards, *Proc. IEEE*, 54, 221–230, 1966.
- Anderson, T. L., and Ogren, J. A.: Determining aerosol radiative properties using the TSI 3563 integrating nephelometer, *Aerosol Sci. Tech.*, 29, 57–69, <https://doi.org/10.1080/02786829808965551>, 1998.
- Arnott, W. P., Moosmüller, H., Rogers, C. F., Jin, T., and Bruch, R.: Photoacoustic spectrometer for measuring light absorption by aerosol:  
435 Instrument description, *Atmos. Environ.*, 33, 2845–2852, [https://doi.org/10.1016/S1352-2310\(98\)00361-6](https://doi.org/10.1016/S1352-2310(98)00361-6), 1999.
- Arnott, W. P., Hamasha, K., Moosmüller, H., Sheridan, P. J., and Ogren, J. A.: Towards aerosol light-absorption measurements with a 7-wavelength aethalometer: evaluation with a photoacoustic instrument and 3-wavelength nephelometer, *Aerosol Sci. Tech.*, 39(1), 17–29, <https://doi.org/10.1080/027868290901972>, 2005.
- Backman, J., Virkkula, A., Vakkari, V., Beukes, J. P., Van Zyl, P. G., Josipovic, M., Piketh, S., Tiitta, P., Chiloane, K., Petäjä, T., Kulmala,  
440 M., and Laakso, L.: Differences in aerosol absorption Ångström exponents between correction algorithms for a particle soot absorption photometer measured on the South African Highveld, *Atmos. Meas. Tech.*, 7, 4285–4298, <https://doi.org/10.5194/amt-7-4285-2014>, 2014.
- Backman, J., Schmeisser, L., Virkkula, A., Ogren, J. A., Asmi, E., Starkweather, S., Sharma, S., Eleftheriadis, K., Uttal, T., Jefferson, A., Bergin, M., Makshtas, A., Tunved, P., and Fiebig, M.: On Aethalometer measurement uncertainties and an instrument correction factor for the Arctic, *Atmos. Meas. Tech.*, 10, 5039–5062, <https://doi.org/10.5194/amt-10-5039-2017>, 2017.
- 445 Bond, T. C., Anderson, T. L., and Campbell, D.: calibration and intercomparison of filter-based measurements of visible light absorption by aerosols, *Aerosol Sci. Tech.*, 30(6), 582–600, <https://doi.org/10.1080/027868299304435>, 1999.
- Bond, T. C., and Bergstrom, R. W.: Light Absorption by Carbonaceous Particles: An Investigative Review, *Aerosol Sci. Technol.*, 40, 27–67, 2006.
- Cantrell, C. A.: Technical Note: Review of methods for linear least-squares fitting of data and application to atmospheric chemistry problems,  
450 *Atmos. Chem. Phys.*, 8, 5477–5487, <https://doi.org/10.5194/acp-8-5477-2008>, 2008.
- Collaud Coen, M., Weingartner, E., Apituley, A., Ceburnis, D., Fierz-Schmidhauser, R., Flentje, H., Henzing, J. S., Jennings, S. G., Moerman, M., Petzold, A., Schmid, O., and Baltensperger, U.: Minimizing light absorption measurement artifacts of the Aethalometer: evaluation of five correction algorithms, *Atmos. Meas. Tech.*, 3, 457–474, <https://doi.org/10.5194/amt-3-457-2010>, 2010.
- Drinovec, L., Močnik, G., Zotter, P., Prévôt, A. S. H., Ruckstuhl, C., Coz, E., Rupakheti, M., Sciare, J., Müller, T., Wiedensohler, A., and  
455 Hansen, A. D. A.: The "dual-spot" Aethalometer: an improved measurement of aerosol black carbon with real-time loading compensation, *Atmos. Meas. Tech.*, 8, 1965–1979, <https://doi.org/10.5194/amt-8-1965-2015>, 2015.
- Hagler, G., Vedantham, R., and Turner, J.: Post-processing Method to Reduce Noise while Preserving High Time Resolution in Aethalometer Real-time Black Carbon Data. *Aerosol Air Qual. Res.*, 11, 539–546, 2011.
- Hansen, A. D. A., Rosen, H., and Novakov, T.: Real-time measurement of the absorption coefficient of aerosol particles, *Appl. Opt.*, 21,  
460 3060–3062, <https://doi.org/10.1364/AO.21.003060>, 1982.
- Hansen, A. D. A., Rosen, H., and Novakov, T.: The aethalometer – An instrument for the real-time measurement of optical absorption by aerosol particles, *Sci. Total Environ.*, 36, 191, [https://doi.org/10.1016/0048-9697\(84\)90265-1](https://doi.org/10.1016/0048-9697(84)90265-1), 1984.
- Hatakka J., Aalto T., Aaltonen V., Aurela M., Hakola H., Komppula M., Laurila T., Lihavainen H., Paatero J., Salminen K., and Viisanen Y.: Overview of the atmospheric research activities and results at Pallas GAW station, *Boreal Env. Res.*, 8, 365–383, 2003.


- 465 Heintzenberg, J., Wiedensohler, A., Tuch, T. M., Covert, D. S., Sheridan, P., Ogren, J. A., Gras, J., Nessler, R., Kleefeld, C., Kalivitis, N., Aaltonen, V., Wilhelm, R. T., and Havlicek, M.: Intercomparisons and aerosol calibrations of 12 commercial integrating nephelometers of three manufacturers, *J. Atmos. Oceanic. Technol.*, 23(7), 902–914, <https://doi.org/10.1175/JTECH1892.1>, 2006.
- Hyvärinen, A.-P., Vakkari, V., Laakso, L., Hooda, R. K., Sharma, V. P., Panwar, T. S., Beukes, J. P., van Zyl, P. G., Josipovic, M., Garland, R. M., Andreae, M. O., Pöschl, U., and Petzold, A.: Correction for a measurement artifact of the Multi-Angle Absorption Photometer (MAAP) at high black carbon mass concentration levels, *Atmos. Meas. Tech.*, 6, 81–90, <https://doi.org/10.5194/amt-6-81-2013>, 2013.
- 470 Jacobson, M. Z.: Strong radiative heating due to the mixing state of Black Carbon in atmospheric aerosols, *Nature*, 409, 695–697, 2001.
- Kanaya, Y., Komazaki, Y., Pochanart, P., Liu, Y., Akimoto, H., Gao, J., Wang, T., and Wang, Z.: Mass concentrations of black carbon measured by four instruments in the middle of Central East China in June 2006, *Atmos. Chem. Phys.*, 8, 7637–7649, <https://doi.org/10.5194/acp-8-7637-2008>, 2008.
- 475 Kebejian, P. L., Robinson, W. A., and Freedman, A.: Optical extinction monitor using cw cavity enhanced detection, *Rev. Sci. Instrum.*, 78(6), 063102, <https://doi.org/10.1063/1.2744223>, 2007.
- Kondo, Y., Sahu, L., Kuwata, M., Miyazaki, Y., Takegawa, N., Moteki, N., Imaru, J., Han, S., Nakayama, T., Kim Oanh, N. T., Hu, M., Kim, Y. J., and Kita, K.: Stabilization of the mass absorption cross section of black carbon for filter-based absorption photometry by the use of a heated inlet, *Aerosol Sci. Tech.*, 43(8), 741–756, <https://doi.org/10.1080/02786820902889879>, 2009.
- 480 Kondo, Y., Sahu, L., Moteki, N., Khan, F., Takegawa, N., Liu, X., Koike, M., and Miyakawa, T.: Consistency and traceability of black carbon measurements made by laser-induced incandescence, thermal-optical transmittance, and filter-based photo-absorption techniques, *Aerosol Sci. Tech.*, 45(2), 295–312, <https://doi.org/10.1080/02786826.2010.533215>, 2011.
- Laborde, M., Schnaiter, M., Linke, C., Saathoff, H., Naumann, K.-H., Möhler, O., Berlenz, S., Wagner, U., Taylor, J. W., Liu, D., Flynn, M., Allan, J. D., Coe, H., Heimerl, K., Dahlkötter, F., Weinzierl, B., Wollny, A. G., Zannata, M., Cozic, J., Laj, P., Hitznerberger, R., Schwarz, J. P. and Gysel, M.: Single Particle Soot Photometer intercomparison at the AIDA chamber, *Atmos. Meas. Tech.*, 5(12), 3077–3097, doi:10.5194/amt-5-3077-2012, 2012.
- 485 Laing, J.R., Jaffe, D.A., and Sedlacek, III, A.J.: Comparison of filter-based absorption measurements of biomass burning aerosol and background aerosol at the Mt. Bachelor Observatory. *Aerosol Air Quality Research* 20, 663–678, 2020. doi: 10.4209/aaqr.2019.06.0298.
- Lihavainen, H., Hyvärinen, A., Asmi, E., Hatakka, J., and Viisanen, Y.: Long-term variability of aerosol optical properties in northern Finland, *Boreal Env. Res.*, 20, 526–541, <http://hdl.handle.net/10138/228289>, 2015.
- 490 Lohila A., Penttilä T., Jortikka S., Aalto T., Anttila P., Asmi E., Aurela M., Hatakka J., Hellén H., Henttonen H., Hänninen P., Kilkki J., Kyllönen K., Laurila T., Lepistö A., Lihavainen H., Makkonen U., Paatero J., Rask M., Sutinen R., Tuovinen J.-P., Vuorenmaa J., and Viisanen Y.: Preface to the special issue on integrated research of atmosphere, ecosystems and environment at Pallas, *Boreal Env. Res.*, 20, 431–454, <http://hdl.handle.net/10138/228278>, 2015.
- 495 Massoli, P., Kebejian, P. L., Onasch, T. B., Hills, F. B., and Freedman, A.: Aerosol Light Extinction Measurements by Cavity Attenuated Phase Shift (CAPS) Spectroscopy: Laboratory validation and field deployment of a compact aerosol particle extinction monitor, *Aerosol Sci. Tech.*, 44, 428–435, <https://doi.org/10.1080/02786821003716599>, 2010.
- Miyazaki, Y., Kondo, Y., Sahu, L. K., Imaru, J., Fukushima, N., and Kanno, A.: Performance of a newly designed continuous soot monitoring system (COSMOS), *J. Environ. Monitor.*, 10, 1195–1201, <https://doi.org/10.1039/B806957C>, 2008.
- 500 Modini, R. L., Corbin, J. C., Brem, B. T., Irwin, M., Bertò, M., Pileci, R. E., Fetfatzis, P., Eleftheriadis, K., Henzing, B., Moerman, M. M., Liu, F., Müller, T., and Gysel-Beer, M.: Detailed characterization of the CAPS single-scattering albedo monitor (CAPS PM<sub>ssa</sub>) as a




- field-deployable instrument for measuring aerosol light absorption with the extinction-minus-scattering method, *Atmos. Meas. Tech.*, 14, 819–851, <https://doi.org/10.5194/amt-14-819-2021>, 2021.
- Moosmuller, H., Chakrabarty, R.K., and Arnott, W.: Aerosol light absorption and its measurement: A review, *J. Quant. Spectrosc. Radiat. Transf.*, 110, 844–878, <https://doi.org/10.1016/j.jqsrt.2009.02.035>, 2009.
- Mölders, N., and Edwin, S.: Review of Black Carbon in the Arctic—Origin, Measurement Methods, and Observations. *Open J. Air Pollut.*, 7, 181–213. doi: 10.4236/ojap.2018.72010, 2018.
- Müller, T., Henzing, J. S., de Leeuw, G., Wiedensohler, A., Alastuey, A., Angelov, H., Bizjak, M., Collaud Coen, M., Engström, J. E., Gruening, C., Hillamo, R., Hoffer, A., Imre, K., Ivanow, P., Jennings, G., Sun, J. Y., Kalivitis, N., Karlsson, H., Komppula, M., Laj, P., Li, S.-M., Lunder, C., Marinoni, A., Martins dos Santos, S., Moerman, M., Nowak, A., Ogren, J. A., Petzold, A., Pichon, J. M., Rodriguez, S., Sharma, S., Sheridan, P. J., Teinilä, K., Tuch, T., Viana, M., Virkkula, A., Weingartner, E., Wilhelm, R., and Wang, Y. Q.: Characterization and intercomparison of aerosol absorption photometers: result of two intercomparison workshops, *Atmos. Meas. Tech.*, 4, 245–268, <https://doi.org/10.5194/amt-4-245-2011>, 2011a.
- Müller, T., Laborde, M., Kassell, G., and Wiedensohler, A.: Design and performance of a three-wavelength LED-based total scatter and backscatter integrating nephelometer, *Atmos. Meas. Tech.*, 4, 1291–1303, <https://doi.org/10.5194/amt-4-1291-2011>, 2011b.
- Nakayama, T., Kondo, Y., Moteki, N., Sahu, L. K., Kinase, T., Kita, K., and Matsumi, Y.: Size-dependent correction factors for absorption measurements using filter-based photometers: PSAP and COSMOS, *J. Aerosol Sci.*, 41, 333–343, <https://doi.org/10.1016/j.jaerosci.2010.01.004>, 2010.
- Ogren, J. A.: Comment on ‘Calibration and intercomparison of filter-based measurements of visible light absorption by aerosols’, *Aerosol Sci. Tech.*, 44(8), 589–591, <https://doi.org/10.1080/02786826.2010.482111>, 2010.
- Ogren, J.A., Wendell, J., Andrews, E., and Sheridan, P.J.: Continuous Light Absorption Photometer for Long-Term Studies. *Atmos. Meas. Tech.*, 10, 4805–4818. <https://doi.org/10.5194/amt-10-4805-2017>, 2017.
- Ohata, S., Kondo, Y., Moteki, N., Mori, T., Yoshida, A., Sinha, P. R., and Koike, M.: Accuracy of black carbon measurements by a filter-based absorption photometer with a heated inlet, *Aerosol Sci. Tech.* 53(9), 1079–91, <https://doi.org/10.1080/02786826.2019.1627283>, 2019.
- Ohata, S., Mori, T., Kondo, Y., Sharma, S., Hyvärinen, A., Andrews, E., Tunved, P., Asmi, E., Backman, J., Servomaa, H., Veber, D., Koike, M., Kanaya, Y., Yoshida, A., Moteki, N., Zhao, Y., Matsushita, J., and Oshima, N.: Estimates of mass absorption cross sections of black carbon for filter-based absorption photometers in the Arctic, *Atmos. Chem. Phys. Discuss.* [preprint], <https://doi.org/10.5194/acp-2020-1190>, 2020.
- Onasch, T. B., Massoli, P., Kebejian, P. L., Hills, F. B., Bacon, F. W., and Freedman, A.: Single Scattering Albedo Monitor for Airborne Particulates, *Aerosol Sci. Tech.*, 49, 267–279, <https://doi.org/10.1080/02786826.2015.1022248>, 2015.
- Perim de Faria, J., Bundke, U., Berg, M., Freedman, A., Onasch, T. B., and Petzold, A.: Airborne and laboratory studies of an IAGOS instrumentation package containing a modified CAPS particle extinction monitor, *Aerosol Sci. Tech.*, 1–14, <https://doi.org/10.1080/02786826.2017.1355547>, 2017.
- Petzold, A., Ogren, J. A., Fiebig, M., Laj, P., Li, S.-M., Baltensperger, U., Holzer-Popp, T., Kinne, S., Pappalardo, G., Sugimoto, N., Wehrli, C., Wiedensohler, A., and Zhang, X.-Y.: Recommendations for reporting "black carbon" measurements, *Atmos. Chem. Phys.*, 13, 8365–8379, <https://doi.org/10.5194/acp-13-8365-2013>, 2013a.
- Petzold, A., Onasch, T., Kebejian, P., and Freedman, A.: Intercomparison of a Cavity Attenuated Phase Shift-based extinction monitor (CAPS PMex) with an integrating nephelometer and a filter-based absorption monitor, *Atmos. Meas. Tech.*, 6, 1141–1151, <https://doi.org/10.5194/amt-6-1141-2013>, 2013b.

- 540 Reid, J. S., Hobbs, P. V., Liousse, C., Martins, J. V., Weiss, R. E. and Eck, T. F.: Comparisons of techniques for measuring short-wave absorption and black carbon content of aerosols from biomass burning in Brazil. *J. Geophys. Res.-Atmos.* 103, 32031–32040, <https://doi.org/10.1029/98JD00773>, 1998.
- Rosen, H., Hansen, A. D. A., Gundel, L., and Novakov, T.: Identification of the optically absorbing component in urban aerosols, *Appl. Opt.*, 17, 3859–3861, <https://doi.org/10.1364/AO.17.003859>, 1978.
- 545 Saathoff, H., Naumann, K. H., Schnaiter, M., Schock, W., Weingartner, E., Baltensperger, U., Kramer, L., Bozoki, Z., Pöschl, U., Niessner, R., and Schurath, U.: Carbon mass determinations during the AIDA soot aerosol campaign 1999, *J. Aerosol Sci.*, 34(10), 1399–1420, [https://doi.org/10.1016/S0021-8502\(03\)00365-3](https://doi.org/10.1016/S0021-8502(03)00365-3), 2003.
- Schmeisser, L., Backman, J., Ogren, J. A., Andrews, E., Asmi, E., Starkweather, S., Uttal, T., Fiebig, M., Sharma, S., Eleftheriadis, K., Vratolis, S., Bergin, M., Tunved, P., and Jefferson, A.: Seasonality of aerosol optical properties in the Arctic, *Atmos. Chem. Phys.*, 18, 11599–11622, <https://doi.org/10.5194/acp-18-11599-2018>, 2018.
- 550 Schmid, O., Artaxo, P., Arnott, W. P., Chand, D., Gatti, L. V., Frank, G. P., Hoffer, A., Schnaiter, M., and Andreae, M. O.: Spectral light absorption by ambient aerosols influenced by biomass burning in the Amazon Basin. I: Comparison and field calibration of absorption measurement techniques, *Atmos. Chem. Phys.*, 6, 3443–3462, <https://doi.org/10.5194/acp-6-3443-2006>, 2006.
- Schulz, C., Kock, B., Hofmann, M., Michelsen, H.A., Will, S., Bougie, B., Suntz, R., and Smallwood, G.: Laser-induced incandescence: Recent trends and current questions, *J. Appl. Phys. B.*, 83, 333–354, <https://doi.org/10.1007/s00340-006-2260-8>, 2006.
- 555 Schwarz, J. P., Gao, R. S., Fahey, D. W., Thomson, D. S., Watts, L. A., Wilson, J. C., Reeves, J. M., Darbeheshti, M., Baumgardner, D. G., Kok, G. L., Chung, S. H., Schulz, M., Hendricks, J., Lauer, A., Kaercher, B., Slowik, J. G., Rosenlof, K. H., Thompson, T. L., Langford, A. O., Loewenstein, M. and Aikin, K. C.: Single-particle measurements of midlatitude black carbon and light scattering aerosols from the boundary layer to the lower stratosphere, *J. Geophys. Res.-Atmos.*, 111, D16, <https://doi.org/10.1029/2006JD007076>, 2006.
- 560 Sinha, P. R., Kondo, Y., Koike, M., Ogren, J. A., Jefferson, A., Barrett, T. E., Sheesley, R. J., Ohata, S., Moteki, N., Coe, H., Liu, D., Irwin, M., Tunved, P., Quinn, P. K., and Zhao, Y.: Evaluation of ground-based black carbon measurements by filter-based photometers at two Arctic sites, *J. Geophys. Res. Atm.*, 122(6), 3544–3572, 2017. <https://doi.org/10.1002/2016JD025843>
- Slowik, J. G., Cross, E. S., Han, J-H, Davidovits, P., Onasch, T. B., Jayne, J. T., Williams, L. R., Canagaratna, M. R., Worsnop, D. R., Chakrabarty, R. K., Moosmüller, H., Arnott, W. P., Schwarz, J. P., Gao, R-S., Fahey, D. W., David W. Kok, G. L., and Petzold, A.: An inter-comparison of instruments measuring black carbon content of soot particles, *Aerosol Sci. Tech.*, 41(3), 295–314, <https://doi.org/10.1080/02786820701197078>, 2007.
- 565 Springston, S. R., and Sedlacek III, A. J.: Noise Characteristics of an Instrumental Particle Absorbance Technique, *Aerosol Sci. Tech.*, 41(12), 1110–1116, 2007. DOI: 10.1080/02786820701777457
- Stephens, M., Turner, N., and Sandberg, J.: Particle identification by laser-induced incandescence in a solid-state laser cavity, *Appl. Opt.*, 42, 3726–3736, <https://doi.org/10.1364/AO.42.003726>, 2003.
- 570 Strawa, A., Castaneda, R., Owano, T., Baer, D., Paldus, B., and Gore, W.: The measurement of aerosol optical properties using continuous wave cavity ring-down techniques, *J. Atmos. Oceanic Technol.*, 20(4), 454–465, [https://doi.org/10.1175/1520-0426\(2003\)20<454:TMOAOP>2.0.CO;2](https://doi.org/10.1175/1520-0426(2003)20<454:TMOAOP>2.0.CO;2), 2003.
- Tørseth, K., Andrews, E., Asmi, E., Eleftheriadis, K., Fiebig, M. Herber, A., Lin, H., Kylling, A., Lupi, A., Massling, A., Mazzola, M., Nøjgaard, J.K., Popovicheva, O., Schichtel, B., Schmale, J., Sharma, S., Skov, H., Stebel, K., Vassel, B., Vitale, V., Whaley, C., Yttri, K.E., and Zanatta, M.: Review of Observation Capacities and Data Availability for Black Carbon in the Arctic Region: EU Action on Black Carbon in the Arctic – Technical Report 1, 2019.


- Virkkula, A., Ahlquist, N. C., Covert, D. S., Sheridan, P. J., Arnott, W. P., and Ogren, J. A.: A three-wavelength optical extinction cell for measuring aerosol light extinction and its application to determining light absorption coefficient, *Aerosol Sci. Tech.*, 39, 52–67, <https://doi.org/10.1080/027868290901918>, 2005.
- 580 Virkkula, A., Mäkelä, T., Yli-Tuomi, T., Hirsikko, A., Koponen, I. K., Hämeri, K., and Hillamo, R.: A simple procedure for correcting loading effects of aethalometer data, *J. Air Waste Manag. Assoc.*, 57, 1214–1222, <https://doi.org/10.3155/1047-3289.57.10.1214>, 2007.
- Virkkula, A.: Correction of the calibration of the 3-wavelength particle soot absorption photometer (3 $\lambda$  PSAP), *Aerosol Sci. Tech.*, 44(8), 706–712, <https://doi.org/10.1080/02786826.2010.482110>, 2010.
- 585 Virkkula, A., Chi, X., Ding, A., Shen, Y., Nie, W., Qi, X., Zheng, L., Huang, X., Xie, Y., Wang, J., Petäjä, T., and Kulmala, M.: On the interpretation of the loading correction of the aethalometer, *Atmos. Meas. Tech.*, 8, 4415–4427, <https://doi.org/10.5194/amt-8-4415-2015>, 2015.
- Weingartner, E., Saathof, H., Schnaiter, M., Streit, N., Bitnar, B., and Baltensperger, U.: Absorption of light by soot particles: determination of the absorption coefficient by means of aethalometers, *J. Aerosol Sci.*, 34, 1445–1463, [https://doi.org/10.1016/S0021-8502\(03\)00359-8](https://doi.org/10.1016/S0021-8502(03)00359-8), 590 2003.
- Werle, P., Mücke, R., and Slemr, F.: The limits of signal averaging in atmospheric trace-gas monitoring by tunablediode-laser absorption spectroscopy (TDLAS). *Appl. Phys. B*, 57, 131–139, 1993.

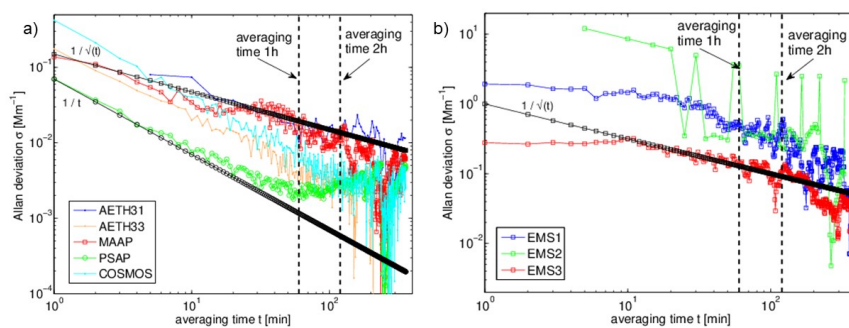


**Figure 1.** Allan deviation of aerosol absorption  $\sigma_{AP,637nm}$  measured with a) the filter-based instruments and with b) the EMS technique. Averaging times between 1min and 6h are shown in x-axis. The black lines with slope -0.5 in a) and b) demonstrate white noise and in a) noise with slope -1.0 is added to guide the eye due to better fit with some instruments. Averaging times until 1h (marked with black dash line) improve signal-to-noise in all instruments but averaging 2h or more (marked with the second black dashed line) does not always lead to improvement.

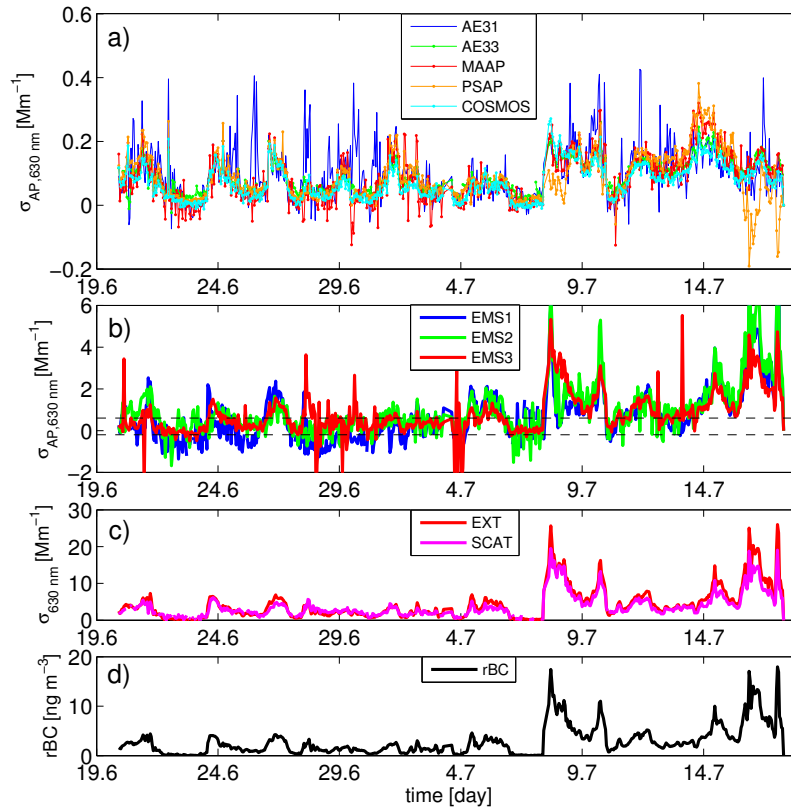


**Figure 2.** The 1h-averaged absorption coefficients at  $\lambda=630$  nm during the whole campaign period measured with a) the filter-based instruments and b) the EMS-technique. To guide the eye, in b) are also depicted the lower and upper limits of panel a) with dash black lines. Simultaneously measured extinction and scattering coefficients and the residual-BC concentration are presented in lower panels c) and d). The extinction and scattering presented were measured with AUR4 and CAPSssa instruments, and the rBC was measured with SP2.

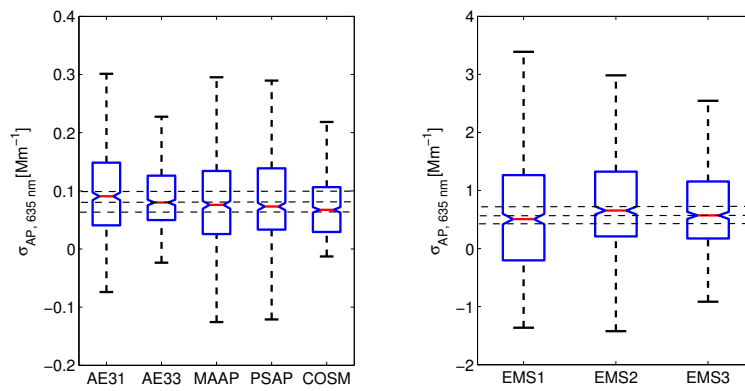

**Figure 3.** The vertical black lines show the range of 1h-averaged absorption coefficient values measured with the eight different techniques labeled in the x-axis. The red lines show the medians and the blue boxes the 25th and 75th percentiles. The horizontal dotted black lines present the overall medians  $\pm 25\%$ .

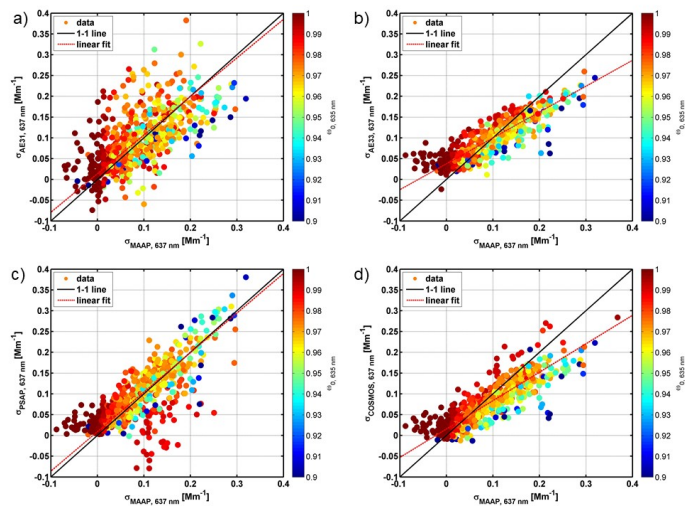

**Figure 4.** Bi-variate correlation of the 1h-averaged absorption coefficient measured by MAAP (x-axis) and by a) AE31, b) AE33, c) PSAP, and d) COSMOS at 637 nm. For each data value also 1h-averaged  $\omega_{0,635nm}$  is presented as color. The corresponding correlation coefficients, their standard errors and the  $R^2$ -statistics are presented in Table 4.

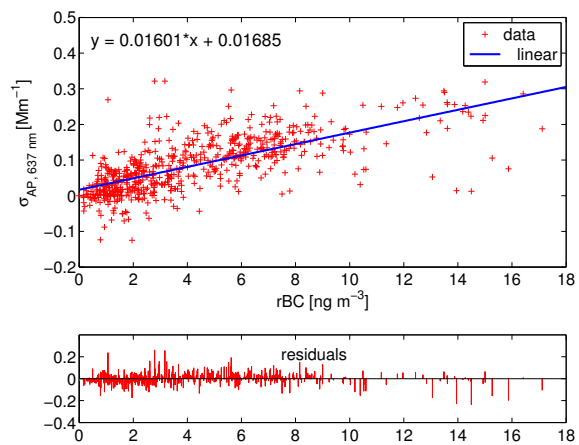

**Figure 5.** The absorption coefficient measured with MAAP as a function of the rBC concentration measured with SP2. The linear regression slope provides the corresponding mass absorption cross-section ( $\text{MAC} = 16.0 \text{ m}^2 \text{ g}^{-1}$ ) value for MAAP and the lower panel presents the residuals of the correlation.



**Table 1.** The campaign instrumentation presented in columns: (1) instrument abbreviation, (2) variable measured (scattering = sca; extinction = ext; refractory Black Carbon = rBC; equivalent Black Carbon = eBC; particle number concentration = PN), (3) measurement time resolution, (4) flow rate, (5) instrument inlet (cut-size 10  $\mu\text{m}$  = PM10 or Total inlet = TOT), and (6) lower detection limit based on manufacturer info.

Instrument	Variable	Time res [s]	Volumetric Flow [LPM]	Inlet	Lower det limit [ $\text{Mm}^{-1}$ ]
AE31	eBC	300	4.5	TOT	<2.22
AE33	eBC	60	5.8	PM10	<0.05 (1h)
MAAP	eBC	60	8.0	PM10	<0.13 (30-min)
PSAP	eBC	1	1.0	PM10	<0.1 (1-min)
COSMOS	rBC	60	0.7	PM10	
SP2	rBC	1	0.1	TOT	
CAPSex	ext	5	0.8	PM10	<0.5 (1-min)
CAPSssa	ext	1	0.9	PM10	<0.5 (1-min)
NEPH AUR4	sca	10	5.8 (via AE33)	PM10	<0.3 (1-min)
NEPH TSI3563	sca	300	8.0 (via MAAP)	PM10	<0.1 (30s)

**Table 2.** The Allan deviation  $\sigma$  of absorption coefficient  $\sigma_{AP,637nm}$  measured with different methods between 1–2hs averaging time (average  $\pm$  standard deviation).

Method	$\sigma$ ave $\pm$ std [Mm] <sup>-1</sup>
AE31	0.014 $\pm$ 0.004
AE33	0.003 $\pm$ 0.001
MAAP	0.012 $\pm$ 0.003
PSAP	0.002 $\pm$ 0.000
COSMOS	0.005 $\pm$ 0.002
EMS <sub>1</sub>	0.379 $\pm$ 0.104
EMS <sub>2</sub>	0.806 $\pm$ 1.100
EMS <sub>3</sub>	0.107 $\pm$ 0.030

**Table 3.** Average  $\pm$  standard deviation and median absorption coefficient  $\sigma_{AP,635nm}$  measured with different methods.

Method	$\sigma_{AP,635nm}$ ave $\pm$ std [Mm] <sup>-1</sup>	$\sigma_{AP,635nm}$ median [Mm] <sup>-1</sup>
AE31	0.101 $\pm$ 0.082	0.091
AE33	0.090 $\pm$ 0.050	0.080
MAAP	0.085 $\pm$ 0.074	0.076
PSAP	0.088 $\pm$ 0.074	0.073
COSMOS	0.073 $\pm$ 0.054	0.067
EMS <sub>1</sub>	0.709 $\pm$ 1.312	0.507
EMS <sub>2</sub>	0.952 $\pm$ 1.303	0.654
EMS <sub>3</sub>	0.785 $\pm$ 1.015	0.570

**Table 4.** Linear regression statistics (correlation coefficients and standard error, SE) and  $R^2$ -values for 1h-average absorption coefficient measured with filter-based instruments  $y=m+bx$ , where  $x=MAAP$  and  $y=AE31, AE33, PSAP$  or  $COSMOS$ . All presented correlations are statistically highly significant ( $p<0.001$ ) and calculated at  $\lambda = 637\text{nm}$ .

Instrument	slope = m (SE)	offset = b (SE)	$R^2$
AE31	0.93 (0.035)	0.01 (0.004)	0.65
AE33	0.62 (0.014)	0.04 (0.002)	0.87
PSAP	0.95 (0.027)	0.01 (0.003)	0.78
COSMOS	0.68 (0.016)	0.02 (0.002)	0.85

## Appendix A: Symbols and abbreviations

**Table A1.** Summary of symbols and abbreviations frequently used in the manuscript text.

Symbol	Explanation
$\lambda$	Wavelength of light.
$\sigma_{SP,\lambda}$	Scattering coefficient at wavelength $\lambda$ .
$\sigma_{AP,\lambda}$	Absorption coefficient at wavelength $\lambda$ .
$\sigma_{EP,\lambda}$	Extinction coefficient at wavelength $\lambda$ .
$\sigma_{0,\lambda}$	Absorption coefficient at wavelength $\lambda$ as directly reported by instrument.
$\sigma_{INST,\lambda}$	Absorption coefficient at wavelength $\lambda$ after corrections measured with INST.
INST	Abbreviation of the absorption measurement instrument (see section 2 Methodology for a complete list of instruments used).
$\omega_{0,\lambda}$	Single-scattering albedo at wavelength $\lambda$ .
$\alpha_{SP,\lambda}$	Ångström exponent of scattering at wavelength $\lambda$ .
$\alpha_{AP,\lambda}$	Ångström exponent of absorption at wavelength $\lambda$ .
EMS <sub>n</sub>	Extinction minus scattering technique to measure absorption, where n = 1, 2 or 3, referring to a pair of instruments used (see section 2 Methodology for details).