

Improvements to a laser-induced fluorescence instrument for measuring SO₂: impact on accuracy and precision

Pamela S. Rickly^{1,2}, Lu Xu³, John D. Crounse³, Paul O. Wennberg^{3,4}, and Andrew W. Rollins²

¹Cooperative Institute for Research in Environmental Sciences, University of Colorado, Boulder, CO 80309, USA

²Chemical Sciences Laboratory, National Oceanic and Atmospheric Administration, Boulder, CO 80305, USA

³Division of Geological and Planetary Sciences, California Institute of Technology, Pasadena, CA 91125, USA

⁴Division of Engineering and Applied Science, California Institute of Technology, Pasadena, CA 91125, USA

Abstract. This work describes **key** improvements made to the *in-situ* laser induced fluorescence instrument for measuring sulfur dioxide (SO₂) that was originally described by Rollins et al. (2016). Here we report measurements of the SO₂ fluorescence emission spectrum. These measurements allow for the determination of the most appropriate bandpass filters to optimize the fluorescence signal while reducing the instrumental background. Because many aromatic species fluoresce in the same spectral region as SO₂, fluorescence spectra were also measured for naphthalene and anisole to determine if ambient SO₂ measurements could be biased in the presence of such species. Improvement in the laser system resulted in better tunability, and a significant reduction in the 216.9 nm laser linewidth. This increases the online/offline signal ratio which in-turn improves the precision and specificity of the measurement. The effects of these improvements on the instrumental sensitivity were determined by analyzing the signal and background of the instrument using varying optical bandpass filter ranges and cell pressures and calculating the resulting limit of detection. As a result, we report an improvement to the instrumental sensitivity by as much as 50%.

1 Background

Sulfur dioxide (SO₂) is responsible for a number of health and environmental impacts. Through reaction with the hydroxyl radical (OH), SO₂ produces sulfuric acid which affects the pH of aqueous particles and leads to acid deposition. Sulfuric acid also condenses onto organic and black carbon particles producing sulfate which increases the aerosol hygroscopicity and influences the accumulation of aerosol liquid water (Fiedler et al., 2011; Carlton et al., 2020). Sulfuric acid is believed to be the most important source gas globally for homogeneous nucleation and growth of new aerosol particles, which may occur primarily in the tropical upper troposphere (Brock et al., 1995; Dunne et al., 2016; Williamson et al. 2019). SO₂ and sulfate particles can be transported long distances driving the production of haze pollution in areas downwind of SO₂ emissions (Andreae et al., 1988). Both the direct radiative forcing from aerosol and the indirect forcing from aerosol cloud interactions are important for climate. While both tend to produce an offset to greenhouse gas induced warming by reducing incoming shortwave radiation, the effect of aerosol cloud interactions is complicated and produces large uncertainties in climate models (Finlayson-Pitts and Pitts, 1999; IPCC, 2018). Changing emissions distributions coupled with incomplete understanding of the chemistry and microphysics associated with sulfur and aerosol formation in the atmosphere necessitates further studies which require precise and accurate measurements of SO₂ throughout the troposphere and lower stratosphere.

Regulation of anthropogenic emissions has resulted in decreased atmospheric SO₂ concentrations in the United States and Europe since the 1970's. However, during the early 21st century, emissions began increasing dramatically in Asia as a result of increased fossil fuel burning (Smith et al., 2011; Hoesly et al., 2018). The main source of SO₂ to the troposphere is through direct emission, followed by oxidation of DMS. The remaining pathways of SO₂ formation, H₂S, CS₂, and OCS oxidation, contribute negligible fluxes (Feinberg et al., 2019). As of 2014, global emission rates of SO₂ were reported to be approximately 113 Tg S yr⁻¹ - more than double the flux during the 1950's (Hoesly, et al., 2018). Anthropogenic sources of sulfur, mainly from fossil fuel combustion and smelting, are the largest global sources of SO₂ to the atmosphere and as of year 2000 comprised around 67% of total global SO₂ emissions (Feinberg et al., 2019; Lee et al., 2011; Smith et al., 2011). Biogenic sources make up a small, but significant fraction of SO₂ emissions with the majority derived from marine phytoplankton, in the form of

Deleted: SO₂

Deleted: as

Deleted: in

Deleted: W

Deleted: may

Deleted: In addition,

Deleted: was decreased in order to

Deleted: increases

Deleted: It

Deleted: some areas of the world

Deleted: ;

Deleted: h

Deleted: concentrations

Deleted: ed

Deleted: ,

Formatted: Subscript

Deleted: , with

Deleted: ing

Formatted: Subscript

Deleted: T

Deleted: of biogenic sources are

dimethyl sulfide which exhibits a global source rate that is approximately 26% of total global SO₂ input (Lee et al., 2011, Feinberg et al., 2019).

75 Although global emission rates of SO₂ have continued to decrease since the early 21st century, atmospheric sulfur concentrations are expected to be affected by continued climate change and could represent feedback mechanisms within the climate system. Due to reductions of sulfur deposition, Hinckley et al. (2020) has found that farmers are needing to apply sulfur containing fertilizer to croplands to enhance nitrogen uptake to plants at a rate of 20-300 kg S yr⁻¹. In addition, Kesselmeier et al. (1993) have reported that terrestrial sources of sulfur exhibit behavior similar to monoterpenes in that they are light and temperature dependent. This suggests that increasing sulfur emissions are likely to occur as global temperatures continue to rise. Lastly, the effect of climate warming on the variability of moisture conditions, as well as increased land use change, is expected to increase both the frequency and duration of biomass burning events which is expected to further increase sulfur emissions (Westerling et al., 1990; Heyerdahl et al., 2002). In combination, while fossil fuel burning sources of SO₂ are continuing to decrease, it is likely that these climate-related and additive sources may keep SO₂ emission from returning to pre-industrial levels.

85 Even small SO₂ mixing ratios can produce important effects. Remote regions, including much of the equatorial marine boundary layer, exhibit mixing ratios of SO₂ on the order of 100 ppt. Still, in these regions, the biogenic SO₂ may be the primary source of cloud condensation nuclei. In addition, convective transport from these regions into the tropical tropopause layer can allow these small sources to reach the lower stratosphere. Sulfate aerosol lifetimes in the stratosphere are approximately 100 times that of aerosol within the lower troposphere allowing them to persist for 1-2 years (Holton et al., 1995). As a result, sources of sulfate aerosol and aerosol precursor species reaching the UT/LS are disproportionately important for climate compared to short lived aerosols in the lower troposphere. However, to date, few studies have reported measurements of SO₂ in the UT/LS (Inn and Veder, 1981; Georgii and Meixner, 1980; Rollins et al., 2017, 2018). Understanding in detail the impact that SO₂ has on the stratosphere is only becoming increasingly important as discussions of albedo modification by injection of SO₂ into the stratosphere is becoming more common (National Research Council, 2015).

90 Despite the potential implications that changing SO₂ concentrations present in the UT/LS and the remote lower troposphere, few in situ measurements are routinely made in either of these areas. Most direct measurements have been made through the use of pulsed fluorescence instruments, which are available commercially; however, this technique tends to exhibit interferences from other fluorescent species and limited precision. Most measurements of SO₂ with pptv precision have been made using chemical ionization mass spectrometry (CIMS). Many CIMS SO₂ ionization chemistry schemes can be sensitive to variations in ambient water vapor, complicating tropospheric measurements (Huey et al., 2004; Eger et al., 2019). Operation of CIMS instruments on unpressurized aircraft capable of reaching the tropical lower stratosphere (>17 km) is also challenging from an engineering perspective.

105 As an alternative, the development of a compact *in situ* laser induced fluorescence (LIF) based SO₂ instrument was recently reported by Rollins et al. (2016) with a 1σ precision of 2 ppt over a 10 s integration period. That technique was developed and originally used to quantify SO₂ in the UT/LS region on two NASA WB-57F missions; VIRGAS (Volcano Investigation Readiness and Gas and Aerosol Sulfur) in 2015 and POSIDON (Pacific Oxidants Sulfur Ice and DehydratiON) in 2016. In the UT/LS where potentially interfering fluorescent species (e.g. aromatic compounds) are in negligible concentrations, the instrument was used in a mode where the excitation laser was maintained on an SO₂ resonance and the optical background was determined using periodic SO₂-free zero-air additions. However, it is expected that LIF measurements of SO₂ in the more complex chemical environment of the troposphere, and especially in areas where fossil fuel combustion is occurring and through biomass burning plumes might result in interferences from species including aromatics that are also formed during these processes. Prior to the deployment of the instrument on a NASA Global Hawk mission in 2017 (HOPE-EPOCH), the LIF instrument was improved to allow for rapid dithering of the excitation laser on and off of an SO₂ resonance, to allow for continuous discrimination of SO₂ from other fluorescent species. It was also operated this way during the NASA ATom-4 mission (Atmospheric Tomography Mission) in 2018 and the NASA/NOAA Fire Influence on Regional to Global Environments Experiment – Air Quality experiment in 2019 (FIREX-AQ). Following ATom-4, it has been investigated how further improvements to the detection of SO₂ might be accomplished by quantifying the spectral region of SO₂ fluorescence for separation from scattering and identification of fluorescence emissions from potentially interfering aromatic species. Here we report on these recent improvements and use of the instrument.

125 2 Laser induced fluorescence

2.1 SO₂ spectroscopy

Deleted: ,

Deleted: ing

Formatted: Superscript

Formatted: Subscript

Deleted: limit

Deleted: reduction

Deleted: reaching

Deleted: in situ

Deleted: instrumental

Fluorescence occurs during the radiative relaxation of a molecule after its absorption of a photon. Thus, the LIF signal is proportional to the molecular absorption cross section at the laser wavelength and the quantum yield for fluorescence. A study by Manatt and Lane (1993) compiled numerous measurements of SO₂ absorption cross-sections over varying wavelengths to find six absorption bands between 100 and 400 nm. Because strong absorption by oxygen (O₂) occurs below 200 nm, the three spectral regions between 200 and 400 nm are most appropriate for atmospheric measurements of SO₂. Excitation into the $\tilde{C}(^1B_2)$ state with a wavelength region of 170-235 nm, is typically chosen for SO₂ fluorescence detection due to the higher absorption cross-section and fluorescence quantum yield compared to longer wavelengths. Pumping into the B or A bands ($\lambda > 240$ nm), while useful for absorption measurements, results in negligible fluorescence. Another consideration is the predissociation threshold near 218.7 nm (Bludsky et al., 2000). As a result, pumping at wavelengths less than ~215 nm results in negligible fluorescence. Considering the absorption cross section and fluorescence quantum yields, excitation at 220.6 nm is theorized to produce the maximum detectable signal using LIF (Rollins et al., 2016).

Deleted: of

Due to the limited availability of practical laser technology for airborne instrumentation, Rollins et al. (2016) targeted a band-head at 216.9 nm through the use of the fifth harmonic produced from a tunable 1084.5 nm fiber-amplified diode laser. The detected fluorescence was selected using a long-pass filter (Thorlabs FGUV5) in combination with a bandpass filter (Asahi XUV0400) allowing transmission of the red-shifted fluorescence in the wavelength region of 240-400 nm. A more detailed description of the LIF SO₂ instrument can be found in Rollins et al. (2016). Generally, while precision sufficient for measurements in the UT/LS was achieved (2 ppt over 10 s integration period), the detection limit was primarily controlled by the background from scattered photons, and it was anticipated that in polluted regions where other fluorescent species exist, the detection limit might be further degraded due to these additional sources of background.

Deleted: determined

2.2 Laser subsystem improvements

The SO₂ instrument uses a custom-built fiber laser system. Pulses from a fiber coupled tunable diode laser near 1084.5 nm are used to seed a fiber amplifier system. Originally, the seed laser operated in a gain-switching mode where short pulses of current injected into the seed laser generated the ~1 ns optical output pulses. In the present design, the seed laser is instead operated in a constant current mode, and its output is modulated using a fiber-coupled electro-optic modulator (EOM). The EOM can produce pulses of less than 1 ns full width at half maximum, and with an extinction ratio of 40 dB. While the original design was somewhat simpler to operate than the present design, gain-switching of the seed laser significantly broadened the laser spectrum and eliminated the possibility of tuning the laser wavelength by modulating the seed laser injection current. Rather, the wavelength of the system was tuned by adjusting the temperature of the seed laser, which had a settling time on the order of seconds. The new design is also operated at a laser repetition-rate of 200 kHz instead of the 25 kHz of the original design. This reduces the peak power leading to less spectral broadening within the fibers and also increases the dynamic range of the single-photon counting LIF signal to 200 kHz rather than 25 kHz. While less UV laser power is achieved with the higher repetition rate and lower pulse energy, the overall sensitivity to SO₂ improves because the SO₂ spectrum can now be fully resolved which increases the convolution of the SO₂ spectrum with the laser spectrum.

Deleted: s

Output from the fiber amplifier is passed through three nonlinear crystals (KTP, LBO, BBO) in the same configuration as described by Rollins et al. (2016) to produce the fifth harmonic of the fiber output at 216.9 nm with typically 1 mW of power. Overall, injecting the seed laser at constant current and operating the amplifier with lower peak powers results in a significantly narrower laser linewidth. Due to the narrower laser linewidth, the Doppler broadened SO₂ spectrum can now be fully resolved (Fig. 1). This significantly increases the effective SO₂ absorption cross-section. The laser wavelength can also be tuned rapidly to measure on and off of an SO₂ resonance many times each second which eliminates spectral interferences from other fluorescent species (Fig. 2).

Deleted: producing

Deleted: the new system has

Deleted: , due to the reduced peak power

Deleted: , such that

2.2 Fluorescence background

Signal on the detector may result from SO₂ fluorescence, or from a suite of other sources. These include Rayleigh, Raman, or aerosol scattering, or fluorescence from the LIF chamber or windows, and red-shifted fluorescence from other gases and aerosols in the sample. Because the SO₂ absorption spectrum has fine structure, the signal from SO₂ can selectively be reduced by more than one order of magnitude by tuning the laser less than 10 pm off of an SO₂ resonance (Fig. 1). All other sources of photons, however, are expected to have no appreciable structure at this spectral resolution. Therefore, the signal from SO₂ can accurately be distinguished from other photon sources by constantly tuning the laser on and off of an SO₂ resonance.

200 The instrumental precision, however, is determined by the Poisson counting statistics of the sum of the SO₂ fluorescence and background signals which, at low SO₂ mixing ratios, is dominated by the non-SO₂ count rate. Therefore, the detection limit is determined by these background sources of photons.

205 Knowledge of the SO₂ emission spectrum is key for choosing detection bandpass filters to maximize the SO₂ signal while minimizing detection of photons from non-SO₂ sources. While the Rayleigh and Raman scatter by N₂ and O₂ occur at constant and known wavelengths, red-shifted fluorescence from other gases and aerosols may vary by compound. Many aromatic species have been reported to have non-negligible absorption cross-sections and fluorescence quantum yields when pumped near 216.9 nm. Because aromatics and SO₂ are co-emitted during combustion of many fuels, it is important to understand the affect they may produce on ambient LIF SO₂ measurements.

210 While many aromatics are released during combustion, two compounds reported as having large emission ratios and significant absorption cross-sections at 216.9 nm are naphthalene and anisole (Grosch et al., 2015; Koss et al., 2018; Mangini et al., 1967; Warneke et al., 2011). Emission ratios of these compounds are dependent on the type of combustion, fossil fuel or biomass, and the elements involved in the combustion. Naphthalene is released through both fossil fuel combustion and biomass burning with the latter producing an emission ratio of greater than 1 ppb/ppm CO (Warneke et al., 2011). Anisole is primarily released through biomass burning with an emission ratio reported in combination with cresol as 1.5 ppb/ppm CO (Koss et al., 2018). The absorption cross-sections reported for these compounds near 216.9 nm are 2.6×10^{-17} cm² molecule⁻¹ for naphthalene (Grosch et al., 2015) and 2.1×10^{-17} cm² molecule⁻¹ for anisole (Mangini et al., 1967). With the emission ratio of SO₂ being similar to these aromatics, in addition to similar absorption cross-sections, it is anticipated that aromatics could significantly interfere with ambient SO₂ measurements. To optimize the detection of the fluorescence spectral region for SO₂, we measured the spectral distributions of the fluorescence emission from SO₂, naphthalene, and anisole.

3 Measurement of scattering and fluorescence spectra

225 The optical bench used for the LIF SO₂ detection is shown in Fig. 3. The 216.9 nm laser, approximately 1 mW, enters the cell perpendicular to the entrance of the sampled air. Sampled air (2500 sccm) enters the system through a custom butterfly valve machined from PEEK (polyether ether ketone) that reduces the pressure to 170 mbar which shows minimal change through the sample cell. The majority of the gas exits the sample cell opposite of the inlet, while 250 sccm is exhausted through each of the cell side arms to eliminate dead space in the flow system.

230 Detection of the fluorescence is then measured orthogonally to both the sample flow and laser axes. A UV fused silica aspheric lens (Edmund Optics, NA = 0.5) is used to collect approximately 10% of the solid angle relative to the center of the cell. After passing through the measurement cell, the beam passes through a LIF reference cell with a similar arrangement to the measurement cell. A constant flow with a mixing ratio near 500 ppb SO₂ is maintained in the reference cell. Feedback from the reference cell is used to ensure that the laser is tuned to the SO₂ resonance peak, and to quantify any changes in the instrument sensitivity due to changes in the laser spectrum. The exhausts of the measurement and reference cells are tied together such that small perturbations in the system pressure will also be equally observed in the two cells. [A National Instruments cRIO computer system is used for controlling all timing requirements. This includes the timing of the seed laser pulses, amplification, and photon counting and gating.](#)

240 For measurements of the fluorescence emission spectra of SO₂ and aromatic compounds, the entrance of a round-to-linear fiber optic bundle (ThorLabs FG105UCA) was placed at the focal point of the lens where the fluorescence detecting PMT is typically located. The emission from the linear end of the fiber bundle was focused by a collimating lens (74-series Ocean Optics) onto the entrance slit of a scanning monochromator (Acton Research Corporation VM-502). Measurements were made with the monochromator in the V configuration with slit sizes of 4 mm wide using a Hamamatsu photomultiplier tube (H12386-210) connected at the exit of the monochromator.

245 In order to measure the SO₂ fluorescence spectrum, a flow of 46 sccm from a 5 ppm SO₂ gas cylinder (Scott Marrin) was mixed with 2500 sccm zero air producing a concentration of approximately 90 ppb that was sampled into the cell. Figure 4 shows the observed spectrum in the presence (red) and absence (orange) of SO₂. The signal observed at 202-236 nm in the absence of SO₂ is primarily from Rayleigh scatter of the laser and the observed width is a measure of the spectral resolution of the experimental setup. The figure to the right shows just the SO₂ fluorescence calculated after the subtraction of the background.

250 To verify the calibration and spectral resolution of the monochromator, a [low-pressure](#) double-bore mercury (Hg) capillary lamp (Jelight) was positioned in front of the fiber as a spectral reference. The atomic Hg emission spectrum from 200 – 500 nm was measured using the monochromator to calibrate the monochromator and show that the monochromator-fiber setup produces a spectral resolution with a full width-half max (FWHM) of

Deleted: low pressure

approximately 20 nm. Figure 4 shows that the SO₂ fluorescence emission spectrum appears to occur in two regions. The main peak is centered around 302 nm and produces a FWHM value of 63 nm in our setup. A second peak may exist between 350-360 nm; however, it is not possible to accurately determine the peak position nor the width in this setup. Using the monochromator with relatively wide slits was necessary to achieve enough signal to measure the fluorescence emission spectrum in our setup, and somewhat exaggerates the width of the emission spectrum in figures 4 – 6.

Deleted: s

Measurements were similarly made with the aromatic compounds. Zero-air was passed through the head-space of a vial containing a sample of pure (>99%) crystalline naphthalene (Aldrich), which has a vapor pressure of 0.04 mbar at 298K. This resulted in a naphthalene concentration of approximately 3.6 ppm when the flow through the vial was 100 sccm and the total flow through the instrument was 1300 sccm. Liquid anisole (Sigma-Aldrich), with a vapor pressure of 5 mbar at 298K, was similarly used to produce a concentration of approximately 26 ppm when the flow through the vial was 10 sccm and the total flow was 2260 sccm (Ambrose et al., 1976). A comparison of the fluorescence spectra of the aromatic compounds to the SO₂ fluorescence spectrum is shown in Fig. 5.

Anisole produces a similar fluorescence spectrum as the main SO₂ emission peak with a maximum at 304 nm. The FWHM of 46 nm occurs between 286 and 332 nm, the latter half of the largest SO₂ fluorescence peak. Similarly, naphthalene produces a fluorescence spectrum peaking around 340 nm with a FWHM value of 46 nm, which slightly overlaps with the tail end of the largest SO₂ fluorescence peak and nearly completely overlaps with the second SO₂ region.

Deleted: between 320 and 366 nm,

Figure 5 shows that aromatic compounds could produce significant signal in the SO₂ instrument during measurements in polluted environments. While naphthalene has a similar absorption cross section and rate of collisional quenching as SO₂, its low-pressure fluorescence quantum yield has been reported to be 2-3 times larger due to a lower expected rate of photodissociation as a result of a larger dissociation energy threshold (Hui and Rice, 1973; Martinez et al., 2004; Reed and Kass, 2000; Suto et al., 1992). However, the observed naphthalene signal in our experiment is approximately 30 times lower than SO₂. Because of its reduced rate of photodissociation, the fluorescence lifetime of naphthalene (340 ns) is much greater than that of SO₂ (30 ns) (Hui and Rice, 1973; Martinez et al., 2004). Therefore, the short counting gate used in this work for SO₂ detection (25 ns) discriminates the majority of the naphthalene signal from that of SO₂.

Deleted: As a result,

No difference in the fluorescence emission (intensity or spectral distribution) was observed for the aromatic compounds with the laser tuned on or off of the SO₂ resonance. This is consistent with expectations based on the literature absorption cross sections for those compounds showing no fine structure comparable to the features in the SO₂ spectrum (refs xx). Therefore, these compounds would only increase the instrument background resulting in reduced precision, but would result in unbiased ambient SO₂ measurements in areas of high aromatic concentrations.

4 Implementation of bandpass filters

In order to achieve the highest sensitivity and lowest limit of detection, the impact of the fluorescence detection bandpass filters was further investigated. With the instrument in its normal configuration for measuring SO₂ (PMT photocathode located at focal point of fluorescence collection lens), different bandpass filters were used in front of the detection cell PMT to directly measure the SO₂ fluorescence signal and quantify the background scatter over a few discrete regions of the spectrum. Figure 6 shows the fluorescence spectrum (red) and background (orange) observed using the monochromator scaled to the count rates observed with each of the tested filters. It was observed that the background increases with wavelength until around 300 nm. After this point, the background slowly decreases reaching a minimum around 400 nm before increasing again near 420 nm. The boxes and closed circles are indicative of the filter measurements. The heights of the boxes indicate the fluorescence signal observed and the width shows the range in which transmission was achievable with the filter. The closed circles indicate the background observed with the filter of the corresponding color.

Deleted: use of varying bandpass filters was investigated.

To optimize the SO₂ detection limit in zero air, the detection limit was calculated from the scaled SO₂ fluorescence and background spectra using a theoretical bandpass filter assuming a low pass of 246 nm and a variable high pass limit where 100% transmission is observed in the pass band and 0% transmission elsewhere. The detection limit was calculated with the filter high pass limit at 270 nm and in increasing increments of 10 nm to the full spectrum at 500 nm. Figure 7 shows the results of this calculation as a function of the high pass filter limit. As the upper end of the pass band is initially increased from 250 to 300 nm, the calculated detection limit rapidly decreases due to significant gains in signal relative to background here. A minimum in the SO₂ detection limit occurs over the range of 350-450 nm with a theoretical detection limit as low as 1.8 ppt over a 1 second integration

Deleted: instrumental

Deleted: is

Formatted: Subscript

Deleted: with a

Deleted: The detection limit increases significantly at wavelengths below 300 nm due to the larger background in combination with the decreasing SO₂ emission observed in this region of the fluorescence spectrum

period. For polluted environments where 1 ppb of naphthalene may be present, the detection limit would increase by 20% within this detection range due to the increased background from naphthalene fluorescence.

The dielectric bandpass filter that we have used previously for SO₂ measurements in the atmosphere (Asahi XUV0400) efficiently reduces signal from Rayleigh scatter, and we find that the additional inclusion of the absorptive glass filter (Thorlabs FGUV5) originally used with this instrument is no longer necessary. Removal of the FGUV5 filter allows for greater transmission within the SO₂ fluorescence spectrum range and provides the largest signal to noise ratio of the sampled bandpass filters. However, the transmission is still limited to 80-95% with the Asahi XUV0400 filter alone in comparison to the theoretical filter. This results in a detection limit of approximately 3.4 ppt over a 1 second integration period, as shown by the marker in Fig. 7. Testing showed that the detection limit decreases with increasing pressure up to at least 250 mbar (Fig. 8). Because predissociation limits the SO₂ fluorescence lifetime to ~5 ns, the fluorescence quantum yield is rather insensitive to pressure in this regime, and therefore the signal increases linearly with pressure due to the increased number density of SO₂. While these measurements were performed under dry conditions, ambient measurements are expected to produce similar results because the short fluorescence lifetime will also limit the importance of collisional quenching by water vapor (Rollins et al., 2016). As a result, the detection limit can be reduced by approximately 15% by increasing the cell pressure to around 250 mbar. While this is beneficial for measurements in the lower troposphere, UT/LS measurements will require the cell pressure to remain less than 100 mbar in order for the instrument to maintain an adequate flow rate.

5 Effect of Ozone

Typical mixing ratios of ozone that can be encountered during stratospheric sampling are not anticipated to affect the SO₂ LIF signal. However, due to the relatively high quantum yield for SO₂ photolysis at 216.9 nm forming primarily sulfur monoxide (SO), the possibility of significantly enhancing the LIF signal through the chemiluminescent reaction of SO with ozone was investigated using higher ozone mixing ratios (Hui and Rice, 1972; Okabe et al., 1971; Ryerson et al., 1994). Figure 9 shows the observed LIF signal in the presence of significant additions of ozone to the inlet. At ozone additions up to 2000 ppm, small increases in LIF signal were observed with increasing O₃ (2 % LIF signal / ppm O₃). This further demonstrates that at stratospheric O₃ mixing ratios accessible by aircraft (< 5 ppm), the signal changes by < 10 %. At O₃ above 2000 ppm, significant decreases in the LIF signal were observed. We attribute these decreases to photolysis of O₃ at 216.9 nm followed by destruction of SO₂ by fast reaction (2.2 × 10⁻¹⁰ cm³ molecule⁻¹ s⁻¹) with the atomic oxygen produced by O₃ photolysis (Sander et al., 2011).

6 Field performance

With the instrument configured with the typical bandpass filter (Asahi XUV0400) and at a pressure of 170 mbar, calibrations were performed to assess the impact of the improvements on the precision of the SO₂ measurement. Calibrations of the instrument are performed in which a mixture of zero air and SO₂ standard are introduced to the instrument with a mixing ratio range of around 1.6-8 ppb SO₂. This mixture is comprised of a flow of 1-5 sccm of 5 ppm SO₂ with 3000 sccm zero air which has passed through a KMnO₄ scrubber removing any SO₂ that may be present in the zero air.

An example of the new calibration is shown in Fig. 10. Typical sensitivity is 26 counts per second (CPS) ppt⁻¹ for SO₂ and 1000 CPS of background. Thus, the background is a photon count rate equivalent to 38 ppt of SO₂. In our previous work (Rollins et al. 2016) we reported in-flight background of 480 CPS and sensitivity of 4.1 CPS ppt⁻¹, or a background equivalent to 114 ppt of SO₂. Therefore, the signal relative to background has increased threefold, which we attribute primarily to the narrower laser linewidth in the new configuration. With the new signal level, the 1σ detection limit for 1 Hz measurements is 3.4 ppt. For 10 seconds of integration time the detection limit would be 1.1 ppt, which is nearly half of what we previously stated for 10 s of integration.

During the NASA ATom-4 field campaign, measurements of SO₂ were acquired by both the LIF instrument as well as the California Institute of Technology CIMS instrument (CIT CIMS). ATom-4 sampled primarily pristine air masses with a limited number of measurements of ship emissions, biomass burning plumes, and volcanic emissions. This allowed for the first in-situ comparison between the current LIF technique and another SO₂ measurement method. CIT CIMS uses fluoride ion transfer chemistry from CF₃O⁻ reagent ion (e.g. SO₂ + CF₃O⁻ → SO₂F⁻ + CF₂O) followed by mass spectral analysis using a compact time of flight mass spectrometer (CToF) with typical mass resolution of m/Δm = 1,200. The precision of CIMS measurements degrades with increasing water vapor concentration because of rising interference of formic acid signal (CH₂O₂:H₂O:CF₃O⁻) which has a mass that

- Deleted: As the
- Deleted: the long-pass
- Deleted: was found to be
- Deleted: unnecessary
- Deleted: long-pass
- Deleted: ; h
- Deleted: Furthermore
- Deleted: shows a decreasing trend
- Deleted: the
- Deleted: collisional quenching of the
- Deleted: is limited as a result of its
- Deleted: short fluorescence lifetime (
- Deleted:)
- Deleted: of
- Deleted: molecules
- Deleted: due to a linear increase in fluorescence signal in this regime.
- Deleted: 70
- Deleted: (< 10 ppm)
- Deleted: Instrument
- Deleted: al
- Deleted: , a detection limit

400 differs from SO₂ by only 0.054 Da. In the marine boundary layer when water vapor was > 20 × 10³ ppm, the CIMS
SO₂ precision (1σ standard deviation over a 1 s integration period) is larger than 130ppt, a value greater than the
typical SO₂ concentration (<100 pptv) as reported by LIF instrument. Therefore, CIMS measurements when water
vapor was > 20 × 10³ ppm are excluded from the comparison. Figure 11a shows an orthogonal regression of both
405 the two instruments (R² = 0.99). Furthermore, measurements during FIREX-AQ acquired during smoke plume
penetration again show excellent correlation between the CIT CIMS and SO₂ LIF instruments (Fig. 11b). This
indicates that aromatic compounds are not biasing the SO₂ LIF measurements. The CIMS instrument reported 12%
and 10% lower SO₂ than the LIF during the ATom-4 and FIREX-AQ missions, respectively. While these are within
410 the combined uncertainties of the measurements, it indicates a systematic calibration error with one or both of the
instruments that has not been resolved at this time.

7 Summary

415 Rollins et al. (2016) reported a new *in situ* method of measuring SO₂ in the UT/LS using LIF. Here we report
improvements to the technique that allow for measurements in polluted areas containing other fluorescent species
and an overall reduction in the detection limit. This was accomplished by limiting non-SO₂ fluorescence
background sources and by improvements in the linewidth and tunability of the laser system. Similar to SO₂,
aromatic species are largely emitted during combustion processes, many of which have large absorption cross-
sections near 216.9 nm and significant fluorescence quantum yields. To determine the effect of these compounds on
420 measuring SO₂, the fluorescence spectra of SO₂ and two aromatic compounds, naphthalene and anisole, were
measured. While strong overlap was exhibited in the fluorescence spectra of these aromatic species with SO₂, the
excitation spectrum of SO₂ has fine structure near 216.9 nm while the excitation spectra of the aromatics is relatively
invariant near 216.9 nm. Therefore, these compounds will only increase the background, slightly reducing the
precision of the instrument, but will not result in biased SO₂ measurements. Similar consequences on the LIF SO₂
425 measurements are expected from other aromatic species since those species generally do not have fine structure in
their excitation spectra.

The SO₂ fluorescence spectrum was also used to determine the bandpass filter application that would best
limit the amount of scatter observed and provide the best limit of detection. Using a theoretical bandpass filter with
transmission beginning at 246 nm, the ending transmission range in which the lowest detection limit is expected is
430 350–450 nm. This is expected to result in a detection limit of 1.8 ppt. Using the Asahi XUV0400 bandpass filter,
we are able to reach a detection limit of 3.4 ppt.

Improvements in the laser system are responsible for significant performance improvements over our
previous work. Here, we reduced the laser linewidth which increased the LIF signal by nearly a factor of three. The
laser wavelength is now controlled by current tuning of the laser, which can be performed rapidly allowing for
435 measurements of online and offline fluorescence signals many times in a second. This eliminates the possibility of
spectral interferences from other species such as aromatics. Increasing the laser repetition rate from 25 kHz to 200
kHz also greatly increased the dynamic range.

While it is shown that increasing the cell pressure to around 250 mbar would reduce the limit of detection
by approximately 25%, this higher cell pressure can only be used in the lower troposphere. Measurements in the
440 UT/LS will require the cell pressure to be operated near 40–50 mbar. It was also demonstrated that increased ozone
concentrations observed in the UT/LS would not significantly influence LIF SO₂ measurements. The resulting
production of O(¹D) does not become large enough to decrease SO₂ within the sampling cell until reaching ozone
concentrations greater than 4000 ppm, more than two orders of magnitude greater than stratospheric ozone
concentrations.

445 The culmination of these changes to the LIF SO₂ instrument has resulted in an increased instrumental
sensitivity and lower limit of detection. Calibrations suggest that the instrumental sensitivity has improved by
approximately 3x relative to the background from that reported in Rollins et al. (2016). Comparison with
measurements performed by the CIT CIMS instrument during the NASA ATom-4 campaign demonstrated good
agreement, including in polluted environments. These results suggest that the LIF SO₂ instrument is highly suitable
450 for measurements in both polluted and pristine environments.

Acknowledgements. This research was funded by the ATom investigation under NASA's Earth Venture program
and the FIREX-AQ investigation under NASA's Upper Atmospheric Composition Observations program program
(Caltech grants NNX15AG61A and 80NSSC18K0660, respectively). We would like to thank the NASA DC-8 crew

Deleted: this is

Deleted: the SO₂ online resonance signals were equivalent to the offline signals for both aromatic species

Deleted: Rayleigh

and management team for support during ATom-4 and FIREX-AQ integration and flights. We thank Michelle Kim and Hannah Allen for their efforts in operating Caltech's CIMS instrument during ATom-4. Data from ATom-4 are available on a NASA online archive (<https://espo.nasa.gov/atom/archive/browse/atom/id14>). Data from FIREX-AQ are available at (<https://www-air.larc.nasa.gov/cgi-bin/ArcView/firexaq>).

Deleted: .

Deleted: .


Deleted: the

8 References


- 465 Ambrose, D., Ellender, J. H., Sprake, C. H. S., and Townsend, R.: Thermodynamic properties of organic oxygen compounds XLIII. Vapour pressures of some ethers, *J. Chem. Therm.*, 8, 165-178, [https://doi.org/10.1016/0021-9614\(76\)90090-2](https://doi.org/10.1016/0021-9614(76)90090-2), 1976.
- Andreae, M. O., Browell, E. V., Garstang, M., Gregory, G. L., Harriss, R. C., Hill, G. F., Jacob, D. J., Pereira, M. C., Sachse, G. W., Setzer, A. W., Silva Dias, P. L., Talbot, R. W., Torres, A. L., and Wofsy, S. C.: Biomass-burning emissions and associated haze layers over Amazonia, *J. Geophys. Res.*, 93(D2), 1509-1527, <https://doi.org/10.1029/JD093iD02p01509>, 1988.
- 470 Bludský, O., Nachtigall, P., Hrušák, J., and Jensen, P.: The calculation of the vibrational states of SO₂ in the C¹B₂ electronic state up to the SO(³Σ)+O(²P) dissociation limit, *Chem. Phys. Letters*, 318, 607-613, [https://doi.org/10.1016/S0009-2614\(00\)00015-4](https://doi.org/10.1016/S0009-2614(00)00015-4), 2000.
- 475 Brock, C. A., Hamill, P., Wilson, J. C., Jonsson, H. H., and Chan, K. R.: Particle Formation in the Upper Tropical Troposphere: A Source of Nuclei for the Stratospheric Aerosol, *Science*, 270(5242), 1650-1653, <https://doi.org/10.1126/science.270.5242.1650>, 1999.
- 480 Carlton, A.G., Christiansen, A. E., Flesch, M. M., Hennigan, C. J., and Sareen, N. Multiphase Atmospheric Chemistry in Liquid Water: Impacts and Controllability of Organic Aerosol. *Accounts of Chemical Research* 2020 53 (9), 1715-1723. DOI: 10.1021/acs.accounts.0c00301, 2020.
- Dunne, E. M., Gordon, H., Kurten, A. et al.: Global atmospheric particle formation from CERN CLOUD measurements, *Science*, 354(6316), <https://doi.org/10.1126/science.aaf2649>, 2016.
- Eger, P. G., Helleis, F., Schuster, G., Phillips, G. J., Lelieveld, J., and Crowley, J. N.: Chemical ionization quadrupole mass spectrometer with an electrical discharge ion source for atmospheric trace gas measurement, *Atmos. Meas. Tech.*, 12, 1935-1954, <https://doi.org/10.5194/amt-12-1935-2019>, 2019.
- 485 Feinberg, A., Sukhodolov, T., Luo, B. P., Rozanov, E., Winkel, L. H. E., Peter, T. and Stenke, A.: Improved tropospheric and stratospheric sulfur cycle in the aerosol-chemistry-climate model SOCOL-AERv2, *Geosc. Model Dev.*, 12, 3863-3887, <https://doi.org/10.5194/gmd-12-3863-2019>, 2019.
- 490 Fiedler, V., Arnold, F., Ludmann, S., Minikin, A., Hamburger, T., Pirjola, L., Dörnbrack, A., and Schlager, H.: African biomass burning plumes over the Atlantic: aircraft based measurements and implications for H₂SO₄ and HNO₃ mediated smoke particle activation, *Atmos. Chem. Phys.*, 11, 3211-3225, <https://doi.org/10.5194/acp-11-3211-2011>, 2011.
- Finlayson-Pitts B.J. and Pitts J.N., Jr.: *Chemistry of the Upper and Lower Atmosphere: Theory, Experiments, and Applications* (Academic, San Diego), 1999.
- 495 Georgii, H. W. and Meixner, F. X.: Measurement of the tropospheric and stratospheric SO₂ distribution, *J. Geophys. Res.*, 85(C12), 7433-7438, doi: 10.1029/JC085iC12p07433, 1980.
- Grosch, H., Sárosy, Z., Egsgaard, H., and Fateev, A.: UV absorption cross-sections of phenol and naphthalene at temperatures up to 500 °C, *J. Quant. Spectrosc. Radiat. Transfer* 156, 17-23, doi: 10.1016/j.jqsrt.2015.01.021, 2015.
- 500 Heyerdahl, E. K., Brubaker, L. B., and Agee, J. K.: Annual and decadal climate forcing of historical fire regimes in the interior Pacific Northwest, USA, *The Holocene*, 12(5), 597-604, <https://doi.org/10.1191/0959683602hl570rp>, 2002.
- Hinckley, E.S., Crawford, J.T., Fakhraei, H. et al. A shift in sulfur-cycle manipulation from atmospheric emissions to agricultural additions. *Nat. Geosci.* 13, 597–604 (2020). <https://doi.org/10.1038/s41561-020-0620-3>

- 510 Hoesly, R. M., Smith, S. J., Feng, L., Klimont, Z., Janssens-Maenhout, G., Pitkanen, T., Seibert, J. J., Vu, L., Andres, R. J., Bolt, R. M., Bond, T. C., Dawidowski, L., Kholod, N., Kurokawa, J.-I., Li, M., Liu, L., Lu, Z., Moura, M. C. P., O'Rourke, P. R., and Zhang, Q.: Historical (1750–2014) anthropogenic emissions of reactive gases and aerosols from the Community Emissions Data System (CEDS), *Geosci. Model Dev.*, 11, 369–408, <https://doi.org/10.5194/gmd-11-369-2018>, 2018.
- Holton, J. R., Haynes, P. H., McIntyre, M. E., Douglass, A. R., Rood, R. B., Pfister, L.: Stratosphere-troposphere exchange, *Reviews of Geophysics*, 33(4), 403–439, 1995.
- 515 Huey, L. G., Tanner, D. J., Slusher, D. L., Dibb, J. E., Arimoto, R., Chen, G. Davis, D., Buhr, M. P., Nowak, J. B., MauldinIII, R. L., Eisele, F. L., and Kosciuch, E.: CIMS measurements of HNO₃ and SO₂ at the South Pole during ISCAT 2000, *Atm. Env.*, 38(32), 5411–5421, <https://doi.org/10.1016/j.atmosenv.2004.04.037>, 2004.
- Hui, M-H and Rice, S. A.: Decay of fluorescence from single vibronic states of SO₂, *Chem. Phys. Letters*, 17(4), 474–478, [https://doi.org/10.1016/0009-2614\(72\)85083-8](https://doi.org/10.1016/0009-2614(72)85083-8), 1972.
- 520 Hui, M-H and Rice, S. A.: Comment on “Decay of fluorescence from single vibronic states of SO₂,” *Chem. Phys. Letters*, 20(5), 411–412, [https://doi.org/10.1016/0009-2614\(73\)85186-3](https://doi.org/10.1016/0009-2614(73)85186-3), 1973.
- IPCC, 2018: Global warming of 1.5°C. An IPCC Special Report on the impacts of global warming of 1.5°C above pre-industrial levels and related global greenhouse gas emission pathways, in the context of strengthening the global response to the threat of climate change, sustainable development, and efforts to eradicate poverty [V. Masson-Delmotte, P. Zhai, H. O. Pörtner, D. Roberts, J. Skea, P.R. Shukla, A. Pirani, W. Moufouma-Okia, C. Péan, R. Pidcock, S. Connors, J. B. R. Matthews, Y. Chen, X. Zhou, M. I. Gomis, E. Lonnoy, T. Maycock, M. Tignor, T. Waterfield (eds.)]. In Press.
- 525 Inn, E. C. Y., Vedder, J. F., and O'Hara, D.: Measurement of stratospheric sulfur constituents, *Geophys. Res. Lett.*, 8(1), 5–8, doi:10.1029/GL008i001p00005, 1981.
- 530 Kesselmeier, J., Meixner, F. X., Hofmann, U., Ajavon, A., Leimbach, S., and Andreae, M. O.: Reduced sulfur compound exchange between the atmosphere and tropical tree species in southern Cameroon, *Biogeochemistry*, 23(1), 23–45, <https://doi.org/10.1007/BF00002921>, 1993.
- 535 Koss, A. R., Sekimoto, K., Gilman, J. B., Selimovic, V., Coggon, M. M., Zarzana, K. J., Yuan, B., Lerner, B. M., Brown, S. S., Jimenez, J. L., Krechmer, J., Roberts, J. M., Warneke, C., Yokelson, R. J., and de Gouw, J.: Non-methane organic gas emissions from biomass burning: identification, quantification, and emission factors from PTR-ToF during the FIREX 2016 laboratory experiment, *Atmos. Chem. Phys.*, 18, 3299–3319, <https://doi.org/10.5194/acp-18-3299-2018>, 2018.
- Kremser, S., et al.: Stratospheric aerosol—Observations, processes, and impact on climate, *Rev. Geophys.*, 54, 278–335, doi:10.1002/2015RG000511, 2016.
- 540 Lee, C., Martin, R. V., van Donkelaar, A., Lee, H., Dickerson, R. R., Hains, J. C., Krotkov, N., Richter, A., Vinnikov, K., and Schwab, J. J.: SO₂ emissions and lifetimes: Estimates from inverse modeling using in situ and global, space-based (SCIAMACHY and OMI) observations, *J. Geophys. Res.*, 116(D06304), 1–13, doi:10.1029/2010JD014758, 2011.
- Manatt, S. L. and Lane, A. L.: A Compilation of the Absorption Cross-Sections of SO₂ from 106 to 403 nm, *J. Quant. Spectrosc. Radiat. Transfer*, 50(3), 267–276, [https://doi.org/10.1016/0022-4073\(93\)90077-U](https://doi.org/10.1016/0022-4073(93)90077-U), 1993.
- 545 Mangini, A., Trombetti, A., and Zauli, C. Vapour phase spectra in the near-ultraviolet of some monosubstituted benzenes, *J. Chem. Soc. B*, 153–165; doi: 10.1039/J29670000153, 1967.
- Martinez, M., Harder, H., Ren, X., Leshner, R. L., and Brune, W. H.: Measuring atmospheric naphthalene with laser-induced fluorescence, *Atmos. Chem. Phys.*, 4, 563–569, <https://doi.org/10.5194/acp-4-563-2004>, 2004.
- 550 National Research Council. 2015. Climate Intervention: Reflecting Sunlight to Cool Earth. Washington, DC: The National Academies Press. <https://doi.org/10.17226/18988>.
- Okabe, H.: Fluorescence and predissociation of sulfur dioxide, *J. Am. Chem. Soc.*, 93(25), 7095–7096, <https://doi.org/10.1021/ja00754a072>, 1971.


- 555 Reed, D. R. and Kass, S. R., Experimental determination of the α and β C—H bond dissociation energies in naphthalene, *J. Mass Spectrom.*, 35, 534-539, [https://doi.org/10.1002/\(SICI\)1096-9888\(200004\)35:4<534::AID-JMS964>3.0.CO;2-T](https://doi.org/10.1002/(SICI)1096-9888(200004)35:4<534::AID-JMS964>3.0.CO;2-T), 2000.
- Rollins, A. W., Thornberry, T. D., Ciciora, S. J., McLaughlin, R. J., Watts, L. A., Hanisco, T. F., Baumann, E., Giorgetta, F. R., Bui, T. V., Fahey, D. W., and Gao, R.-S.: A laser-induced fluorescence instrument for aircraft measurements of sulfur dioxide in the upper troposphere and lower stratosphere, *Atmos. Meas. Tech.*, 9, 4601-4613, <https://doi.org/10.5194/amt-9-4601-2016>, 2016.
- 560 Rollins, A. W., Thornberry, T. D., Watts, L. A., Yu, P., Rosenlof, K. H., Mills, M., Baumann, E., Giorgetta, F. R., Bui, T. V., Höpfner, M., Walker, K. A., Boone, C., Bernath, P. F., Colarco, P. R., Newman, P. A., Fahey, D. W., Gao, R.S.: The role of sulfur dioxide in stratospheric aerosol formation evaluated by using in situ measurements in the tropical lower stratosphere, *Geophys. Res. Lett.*, 44, 4280–4286, doi:10.1002/2017GL072754, 2017.
- 565 Rollins, A. W., Thornberry, T. D., Atlas, E., Navarro, M., Schauffler, S., Moore, F., Elkins, J. W., Ray, E., Rosenlof, K., Aquila, V., Gao, R.S.: SO₂ Observations and Sources in the Western Pacific Tropical Tropopause Region, *J. Geophys. Res. Atmos.*, 123(23), 13,549-13,559, doi.org/10.1029/2018JD029635, 2018.
- Ryerson, T. B., Dunham, A. J., Barkley, R. M., and Sievers, R. E.: Sulfur-Selective Detector for Liquid Chromatography Based on Sulfur Monoxide-Ozone Chemiluminescence, *Anal. Chem.*, 66(18), 2841-2851, <https://doi.org/10.1021/ac00090a009>, 1994.
- 570 Sander, S. P., Abbatt, J., Barker, J. R., Burkholder, J. B., Friedl, R. R., Golden, D. M., Huie, R. E., Kolb, C. E., Kurylo, M. J., Moortgat, G. K., Orkin, V. L., and Wine, P. H.: Chemical kinetics and photochemical data for use in atmospheric studies, evaluation no. 17, JPL Publication 10-6, Jet Propulsion Laboratory, Pasadena, California, USA, <http://jpldataeval.jpl.nasa.gov/>, 2011.
- 575 Smith, S. J., van Aardenne, J., Klimont, Z., Andres, R. J., Volke, A., and Delgado Arias, S.: Anthropogenic sulfur dioxide emissions: 1850–2005, *Atmos. Chem. Phys.*, 11, 1101-1116, <https://doi.org/10.5194/acp-11-1101-2011>, 2011.
- Suto, M., Wang, X., Shan, J., and Lee, L.C. Quantitative photoabsorption and fluorescence spectroscopy of benzene, naphthalene, and some derivatives at 106–295 nm, *J. Quant. Spectrosc. Radiat. Transfer*, 48, 79-89, [https://doi.org/10.1016/0022-4073\(92\)90008-R](https://doi.org/10.1016/0022-4073(92)90008-R), 1992.
- 580 Warneke, C., Roberts, J. M., Veres, P., Gilman, J., Kuster, W. C., Burling, I., Yokelson, R., de Gouw, J. A.: VOC identification and inter-comparison from laboratory biomass burning using PTR-MS and PIT-MS. *Intern. J. Mass Spec.*, 303, 6-14, <https://doi.org/10.1016/j.ijms.2010.12.002>, 2011.
- 585 Westerling, A. L., Hidalgo, H. G., Cayan, D. R., and Swetnam, T. W.: Warming and Earlier Spring Increase Western U.S. Forest Wildfire Activity, *Science*, 313(5789), 940-943, <https://doi.org/10.1126/science.1128834>, 2006.
- Williamson, C.J., Kupc, A., Axisa, D. et al.: A large source of cloud condensation nuclei from new particle formation in the tropics. *Nature* 574, 399–403, doi:10.1038/s41586-019-1638-9, 2019.

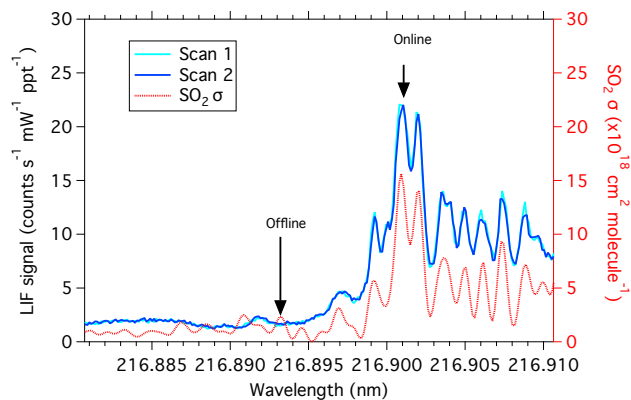


590 **Figure 1. SO₂ absorption cross-section (red, right axis) in comparison to laser scans by the LIF SO₂ instrument (blue and cyan, left axis). The online wavelength is identified as the largest absorption cross-section peak.**

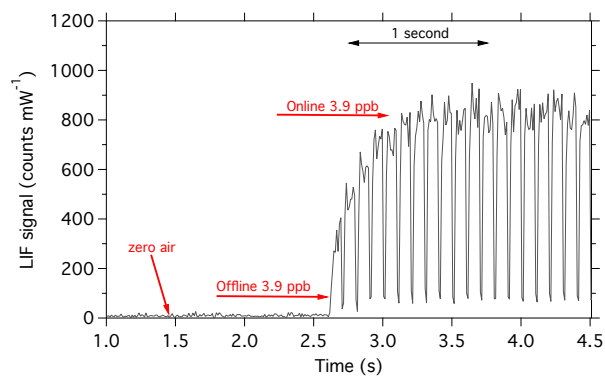


595 **Figure 2. SO₂ measurements performed at 10 Hz showing a large distinction between online and offline signals. Background measurements with zero air show the signal to be negligible in the absence of SO₂.**

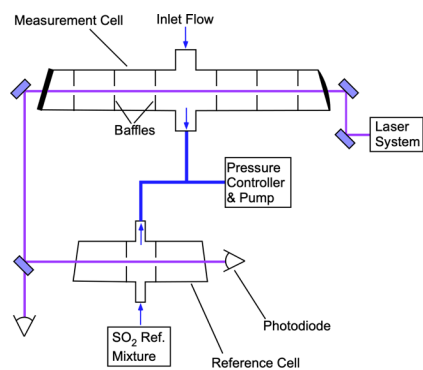


600 **Figure 3. LIF SO₂ detection optical bench. PMTs are located above the plane of this schematic and oriented to collect fluorescence from the center of each cell.**

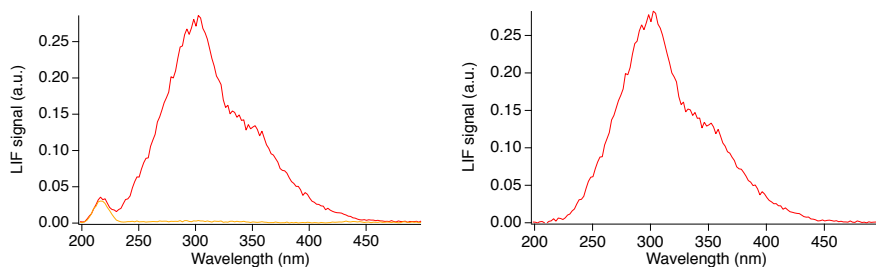

605 **Figure 4. Fluorescence spectrum observed from SO₂ (red) in addition to Rayleigh scattering and background (orange) (left) and the absolute SO₂ fluorescence after subtraction of the background (right).**

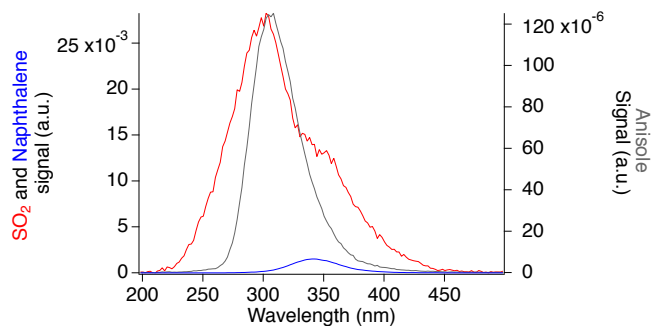


610 **Figure 5. Fluorescence spectra of SO₂ (red), naphthalene (blue), and anisole (grey) normalized by the calculated concentrations.**

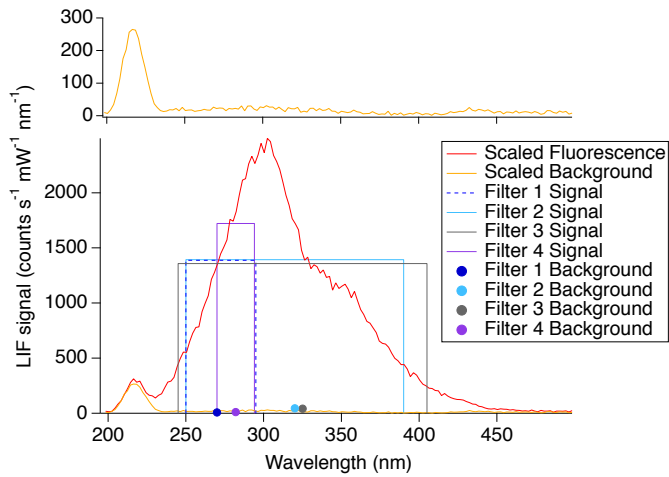


615

Figure 6. Adjusted SO₂ fluorescence spectrum (red line) and background (orange line, top and bottom panels). The filter measurements (boxes and solid circles) show the filter range by the width of the box and the height indicates the observed signal. The solid circles indicate the background observed for the corresponding filter. Filter 1 is the Semrock 300/SP-25 plus the Semrock 244RS-25. Filter 2 is the Schott UG11 plus the Semrock 244RS-25. Filter 3 is the Asahi XUV0400 plus the Thorlabs FGUV5. Filter 4 is the Semrock 280/10-25 plus the Semrock 244RS-25.

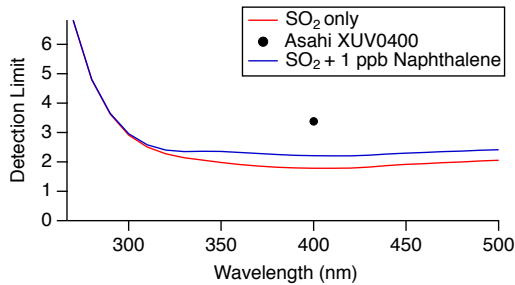


620


Figure 7. Calculated detection limit of the LIF SO₂ instrument (red line), with the addition of 1 ppb naphthalene (blue line), and the measured detection limit of Asahi XUV0400 bandpass filter (black marker) with a 1 second integration period.

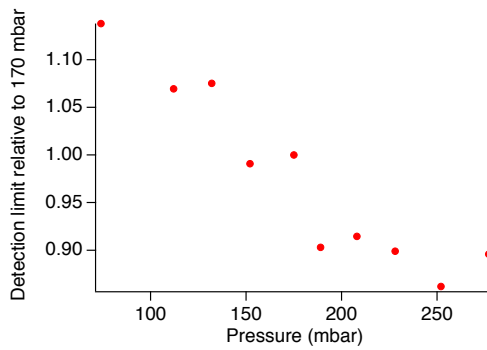

625 **Figure 8. Measured LIF SO₂ detection limit over a pressure range of 74-277 mbar.**

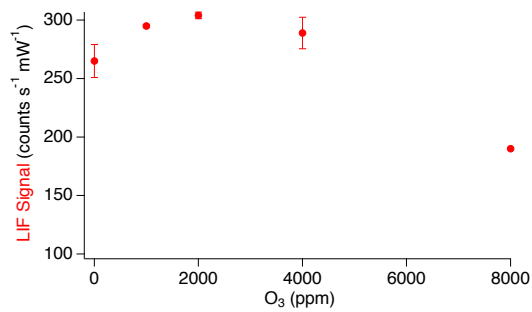

630 **Figure 9. LIF signal as a result of ozone addition in the range of 0-8000 ppm.**

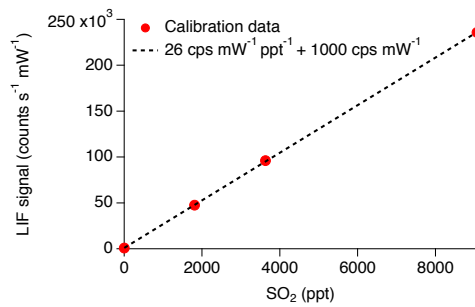

635 **Figure 10. Closed circles indicate the linearized count rate divided by measured laser power observed during calibration. Dashed line represents the fit to the calibration data indicating a sensitivity of 26 cps mW⁻¹ ppt⁻¹ and background of 1000 cps mW⁻¹.**

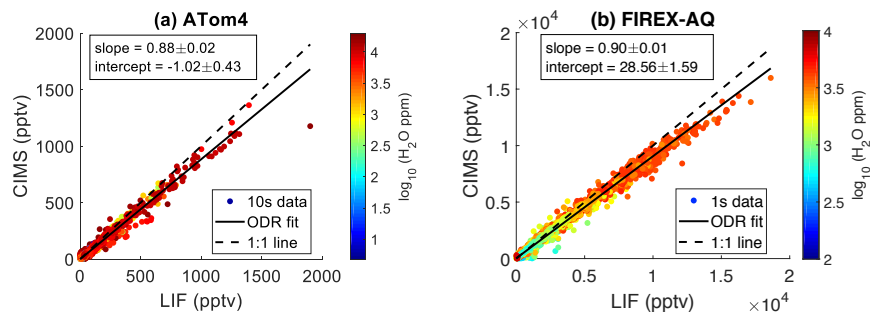


Figure 11. Correlation between CIT CIMS and LIF SO₂ during (a) all 12 of the NASA ATom-4 flights and (b) one FIREX-AQ flight on 08/03/2019. The dashed line represents the 1:1 ratio and the solid line represents the orthogonal fit. 10-second averaged data are used in the ATom-4 comparison to improve the signal/noise and 1-second averaged data are used in the FIREX-AQ comparison.

640

Response to the reviewers for the “Improvements to a laser-induced fluorescence instrument for measuring SO₂: impact on accuracy and precision” study by Pamela S. Rickly et al.

We thank the reviewers for their insightful comments which has helped to improve the manuscript. Below are our replies to each comment in blue.

Anonymous Referee #1

Comment #1: Line 44-64: The discussion of SO₂ emissions is rather confusing. The author should be clearer in the discussion of increases and decreases of emissions specifically which time and emission sector is referred to.

Response: We have changed the text within the paragraph to reflect a clearer discussion of the emissions.

Comment #2: Line 135: What is meant by "simpler design"?

Response: This was meant to indicate a simpler mode of operation. Clarification has been made.

Comment #3: Line 139: Why exactly can the system now be operated at 200kHz instead of 25kHz?

Response: Previously, the lower repetition rate was used to achieve higher energy pulses and more UV laser power. Now, we have re-optimized the system at a higher repetition rate. Some additional text has been added to describe this.

Comment #4: Line 144: What exactly is the reason why the laser linewidth is now narrower compared to the previous system?

Response: As mentioned in this section, the seed laser is operated at a constant current mode instead of very short pulses. This, along with lower peak powers resulting in less spectral broadening in the fibers has reduced the laser linewidth. Some text has been added in section 2.2 to better explain this.

Comment #5: Line 175: Please state the wavelengths for the stated absorption cross sections.

Response: Done.

Comment #6: Line 208- 227: Does the calculation of FWHM takes the resolution of 20nm of the experimental set-up into account? Does this include the second red-shifted peak in the case of SO₂? Was there an effort to de-convolute the spectrum taking these effects into account?

Response: We did not do any de-convolution of the spectrum. Now we explain more clearly how the observed emission spectrum is impacted by the resolution of our experiment.

Comment #7: Line 235: Because the timing of the fluorescence detection becomes important in the discussion, this should be explained in more detail in the instrument description.

Response: This has been added at Line 237-239.

Comment #8: Line 237-240: The authors may want to make the point that not only fluorescence is required for an interference, but also that the excitation spectrum must be similar. The author may want to consider showing excitation spectra of the aromatic compounds in addition. There is no comparison about fluorescence and excitation spectra found in literature. This should be added.

Response: A comment and citations have been added here.

Comment #9: Section 4: This entire section is rather confusing. The motivation for testing different bandpass filters should be made clear. Why are there only the results from one filter shown in Fig 7? A clear discussion of Fig 7 and conclusions with respect to the different filters is missing.

Response: The bandpass filter results shown in Figure 7 represent the detection limit of the bandpass filter that was found to be most optimal for measurements of SO₂. This section has been edited for clarity.

Anonymous Referee #2

Comment #10: L123-126: “. . . while precision sufficient for measurements in the UT/LS was achieved, the detection limit was determined by the background from scattered photons . . .” - Please indicate the precision reached on this version of the instrument and the main sources of noise contributing to the background signal.

Response: This has been added.

Comment #11: L269-270: “Furthermore, the detection limit shows a decreasing trend with increasing pressure (Fig. 8) due to a linear increase in fluorescence signal in this regime.” – When the pressure increases in the measurement cell, wouldn't we expect a reduction of the fluorescence yield due to an increase of collisional quenching. If so, why is the fluorescence signal increasing linearly with the pressure?

Response: The reviewer has made a good suggestion about the need to further explain the fluorescence signal trend with pressure. While collisional quenching is an important consideration for LIF detection of other molecules, the short SO₂ lifetime (~5 ns) limits the importance of fluorescence quenching by surrounding molecules. Instead, the fluorescence signal continues to increase linearly as the number of SO₂ molecules increases with pressure. This discussion has been added.

Comment #12: Section 6: It seems that calibrations were performed under dry conditions. Could the SO₂ fluorescence signal be impacted by quenching from ambient water vapor?

Response: It is expected that water vapor will not create additional fluorescence quenching due to the short fluorescence lifetime of SO₂ as further explained in response to comment #11. This was demonstrated in our prior work (Rollins et al., 2016) and is now noted in section 4.

Comment #13: Figure 11 (right panel: FIREX-AQ): not discussed in the text

Response: This has been added.

Comment #14: Figure 11 (insert): Please add significant figures for the uncertainty reported on the slope

Response: This has been added.