

Supplement of

Calibration and assessment of electrochemical low-cost sensors in remote alpine harsh environments

Federico Dallo^{1,2}

¹Institute of Polar Sciences (CNR-ISP), Via Torino, 155, 30172, Venice, ITALY

²University Ca' Foscari of Venice, Dorsoduro 3246, 30123, Venice, ITALY

Correspondence: Federico Dallo (federico.dallo@unive.it)

S1 Technical Specifications

Purpose of the study is to assess the reliability of low cost sensors for the environmental monitoring of tropospheric Ozone. The low-cost monitoring station is located in a remote alpine area, where comparison of data harvested by low cost sensors can be compared with state-of-art instrumentations. The sensors evaluated are the Alphasense OX-B431, calibrated prior to field
5 installation at CNR-ISAC headquarted in Bologna.

The dimension of the IP56 box is 300x220x120 mm, the total dimension of the wooden cover is 360x290x180 mm. Three arrows on the bottom of the box indicate where the Ozone sensors are located.

S1.1 Components

To open the box it is necessary a ≈ 10 mm flat-blade screwdriver. Inner object are:

- 10 1. AC power wires (red and black are phase and neutral, yellow/green is the Ground),
2. ethernet wire to bring internet connection to the Raspberry Pi (7b),
3. power supply, AC input and 12 VDC out, where black is V- ad red V+,
4. charge regulator, 12 VDC input from power supply into the “Solar” socket, VDC input/output from the 12 V “Battery” and 12 VDC output from “Load” to the DC/DC (6). Black is V- ad red V+.
- 15 5. 12 V, 2,3 Ah battery that acts as an UPS in case of AC failure. It is connected to the “Battery” on the charge regulator using black as V- and red as V+.
6. DC/DC. 12 VDC input from che charge regulator and 5 VDC output to the Raspberry Pi,
7. a) USB power wire for the b) Raspberry Pi,

8. Data acquisition board. This board contains the circuit that performs analog to digital conversion of the sensor's measurements and then send digital data to the Raspberry Pi using i2c protocol.
9. Ozone sensor made by Alphasense,
10. sensor plug for ease the change of the sensor,
11. this is a spare sensor which is not measuring. It is calibrated like the others.

S1.2 Wiring Raspberry Pi with the acquisition board

The most tricky operation in case of maintenance could be the correct wiring of the acquisition board and the T&RH sensors to the Raspberry Pi. In Figure S1.1, Figure S1.2 and Figure S1.3 are shown the wires that goes to the Raspberry Pi, while Figure S1.4 shows the pins scheme of the Raspberry Pi. Here is the list of connection from acquisition board to Raspberry Pi:

- RED on 5 V, pin04
- BROWN on GND, pin06
- GREEN on SDA, pin03
- BLUE on SCL, pin05

Here is the list of connection from T&RH on the top of sensor 1 (it has a 1 on it) to Raspberry Pi:

- RED on 3.3 V, pin01
- WHITE on GND, pin09
- YELLOW on GPIO22, pin15

Here is the list of connection from T&RH on the top of the acquisition board (it has a 4 on it) to Raspberry Pi:

- RED on 3.3 V, pin17
- WHITE on GND, pin30
- YELLOW on GPIO23, pin16

S1.3 Mounting the sensors

Each sensor is fastened with eight Phillips screws, four from the inside and four from the outside. In Figure S1.5 you can see that each sensor is provided of four spacers and stainless steel flat washers. From the outside there are four rubber gaskets to protect from humidity that may come into the box.

The main hole that get the sensor in contact with air is also provided with a gasket ring.

Mounting and unmounting the sensor is easy, just remove the sensor plug and then unscrew from outside the box.

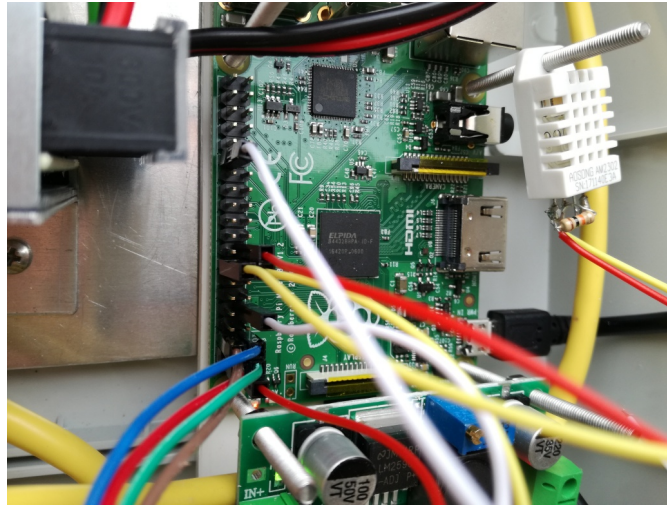


Figure S1.1. The Raspberry Pi with the GPIO on the left. The schematic of the pins are shown in Figure S1.4.

S1.4 Wiring sensors with the acquisition board

As shown in Figure S1.5, sensors are wired using a numbered plug. In case of need to change the sensor the procedure should be straightforward; unplug the sensor, unscrew it using the Phillips screwdriver and the wrench, replace it with the new sensor and plug it.

50 S1.5 Replacing the power supply

First remove the power connector from the outer left side of the box, in order to avoid 220 VAC. Then it is possible to detach the power supply from its support, removing the two flat-blade screws that are beneath it. After removing the power supply, it should be easy to remove all the wires (phase input, neutral input, ground, V+ output and V- output) with the Phillips screwdriver. At this point, replace the power supply with the spare part and rewire. Prior to wire the power supply to the charge
55 regulator, be sure that the V+ output don't exceed 13.5 V and is not less than 12.5 V. Voltage output can be adjusted with the Phillips screwdriver.

S1.6 Replacing the charge regulator

Remove all the red(V+) and black(V-) wires from the terminal blocks "mammuth", only the regulator side has to be released. Then remove the two Phillips screws and replace the charge regulator with its spare part.

60 S1.7 Replacing the battery

Remove the red(V+) and black(V-) wires from the terminal blocks "mammuth" from the battery side. Cut the cable ties and then the battery can be changed with a new one.

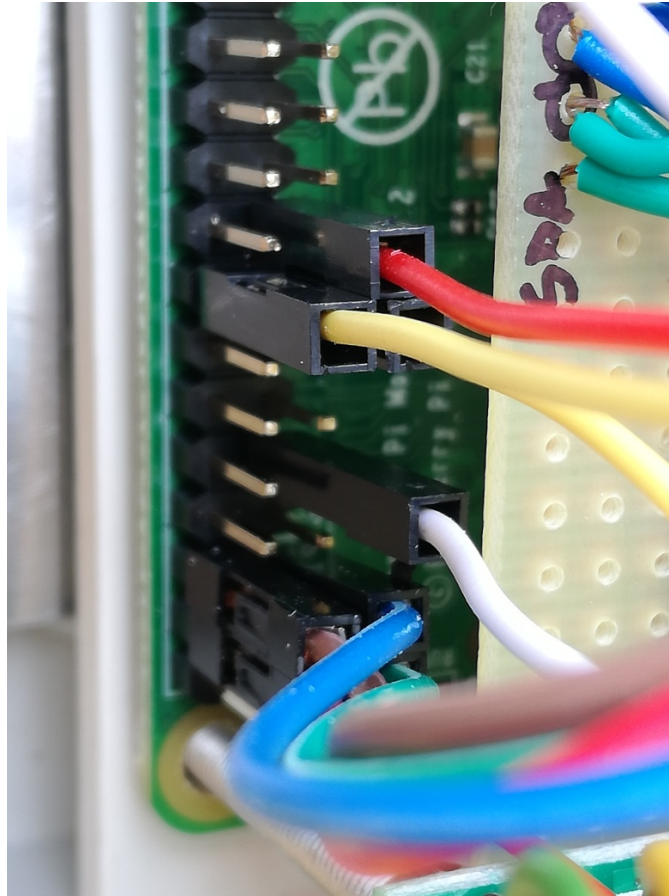


Figure S1.2. A detail of the wiring between the acquisition board and T&RH sensors to the GPIO of the Raspberry Pi. Here are shown the GPIO pins from 1 (bottom-right) to 24 (top-left).

S1.8 Replacing the DC/DC

The DC/DC is fixed with dices. It is sufficient to remove the dice and then pull out the board. Release the wires using the
65 Phillips screwdriver and then replace the DC/DC with the new one.

WARNING: before to give power to the Raspberry Pi, check that the VDC output is 5.0 VDC ($4.75V < V_{out} < 5.25V$ is fine)!!! You can regulate output voltage with the screw on the blue resistor.

S1.9 Replacing the Raspberry Pi USB power wire

Release the wire from the DC/DC output then remove the μ USB from the Raspberry Pi and replace with the new cable.



Figure S1.3. A detail of the wiring between the acquisition board and T&RH sensors to the GPIO of the Raspberry Pi. Here are shown the GPIO pins from 9 (GND with white wire on bottom-right of the pic) to 30 (GND with white wire on top-left of the pic).

70 **S1.10 Replacing the acquisition board**

Hoping that you'd never arrive to this... To remove the acquisition board first remove each sensors plug. Then remove all the wires from the Raspberry Pi pins. Once free, remove the T&RH sensor and then the dices that keep the acquisition board in place. Then replace the board with the new one and follow the subsection S1.2 to rewire everything.

S1.11 Replacing the Raspberry Pi

75 To remove the Raspberry Pi you have to remove its power USB wire and the ethernet wire, then remove the T&RH sensor and the acquisition board. Therefore you can remove the dices that lock the Raspberry Pi. The new Raspberry Pi has everything preinstalled so that, once repowered and connected to the Internet, it should automatically be part of the VPN that allows for remote control.

Raspberry Pi2 GPIO Header					
Pin#	NAME		NAME	Pin#	
01	3.3v DC Power	⬇	DC Power 5v	02	
03	GPIO02 (SDA1 , I ² C)	⬇	DC Power 5v	04	
05	GPIO03 (SCL1 , I ² C)	⬇	Ground	06	
07	GPIO04 (GPIO_GCLK)	⬇	(TXD0) GPIO14	08	
09	Ground	⬇	(RXD0) GPIO15	10	
11	GPIO17 (GPIO_GEN0)	⬇	(GPIO_GEN1) GPIO18	12	
13	GPIO27 (GPIO_GEN2)	⬇	Ground	14	
15	GPIO22 (GPIO_GEN3)	⬇	(GPIO_GEN4) GPIO23	16	
17	3.3v DC Power	⬇	(GPIO_GEN5) GPIO24	18	
19	GPIO10 (SPI_MOSI)	⬇	Ground	20	
21	GPIO09 (SPI_MISO)	⬇	(GPIO_GEN6) GPIO25	22	
23	GPIO11 (SPI_CLK)	⬇	(SPI_CE0_N) GPIO08	24	
25	Ground	⬇	(SPI_CE1_N) GPIO07	26	
<hr/>					
	27	⬇	(PC ID EEPROM) ID_SC	28	
	29	⬇	Ground	30	
	31	⬇	GPIO12	32	
	33	⬇	Ground	34	
	35	⬇	GPIO16	36	
	37	⬇	GPIO20	38	
	39	⬇	GPIO21	40	

Early Models
Late Models

Rev. 1
 26/01/2014

<http://www.element14.com>

Figure S1.4. This is the scheme of the Raspberry Pi GPIO pins. Check if you're looking with the right orientation (in Figure S1.1 the pin 1 is on the bottom-right). This "table showing all 26 pins on the P1 header, including any special function they may have," was made by SparkFun and can be reused under the CC BY licence.



Figure S1.5. These are the three working sensors, and the T and RH sensor close to Sensor 1.

S1.12 Approximate cost of the sensing system

80 The sensing system cost is around 700 EU. Considering the following prices:

- O3 Alphasense sensors 3*150 EU;
- Lead acid battery 20 EU;
- charge regulator 20 EU;
- DHT22 sensor 2*20 EU;
- 85 – DC/DC step down 10 EU;
- ADS1115 ADC 16 bit 2*15 EU;
- Raspberry Pi 40 EU
- IP56 box 40 EU
- Breadboard and wires about 50 EU

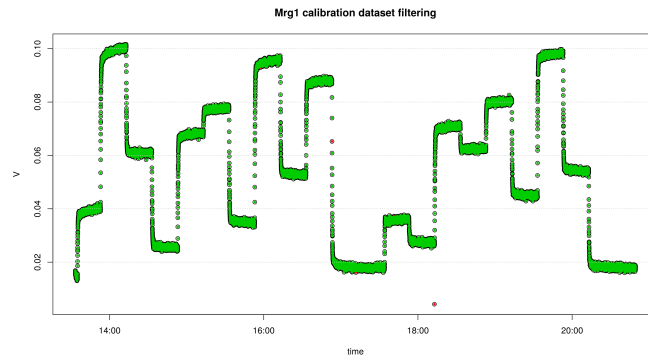


Figure S2.1. Example of the automatic filter to detect outliers in the dataset collected during laboratory calibration.

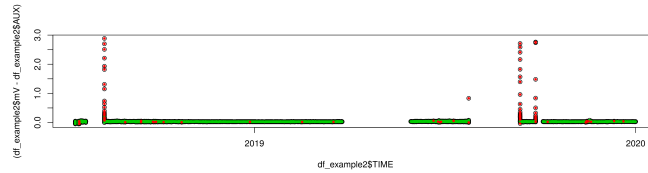


Figure S2.2. Example of the automatic filter to detect outliers in the field dataset.

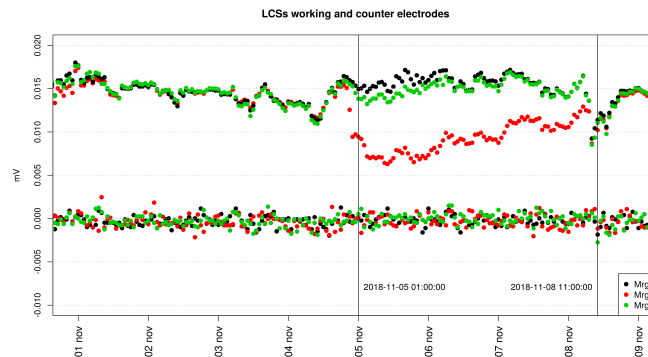


Figure S2.3. The behaviour of the Mrg2 sensor was not consistent in respect to the others LCSs from 1AM November 5 to 11PM November 8. We were not able to identify the cause of this temporary malfunction, but it represents an interesting event proving the importance of considering low-cost sensors redundancy. The data from Mrg2 flagged as erroneous readings were excluded from the dataset and statistical analysis

S3 Electrical noise

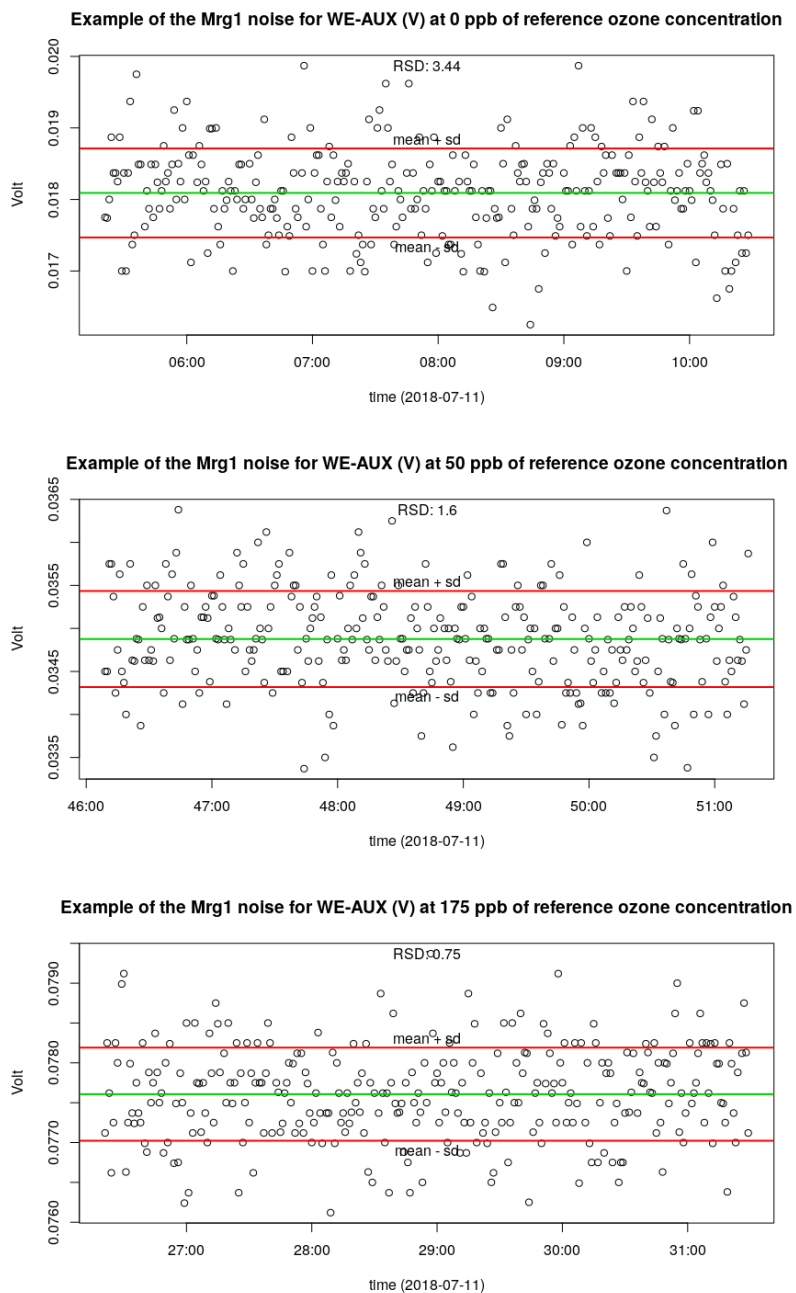


Figure S3.1. Electrical noise of the LCSs.

S4 RSD as function of the ozone concentration

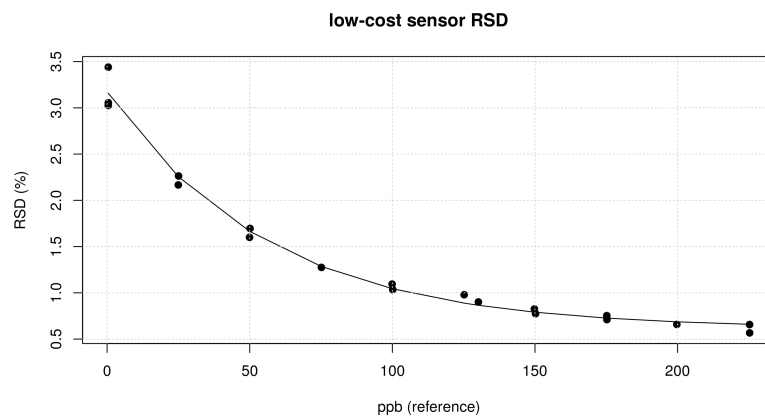


Figure S4.1. The RSD for the LCSs is lower for higher ozone concentration.

S5 Ozone measurements and meteorological variables in Col Margherita

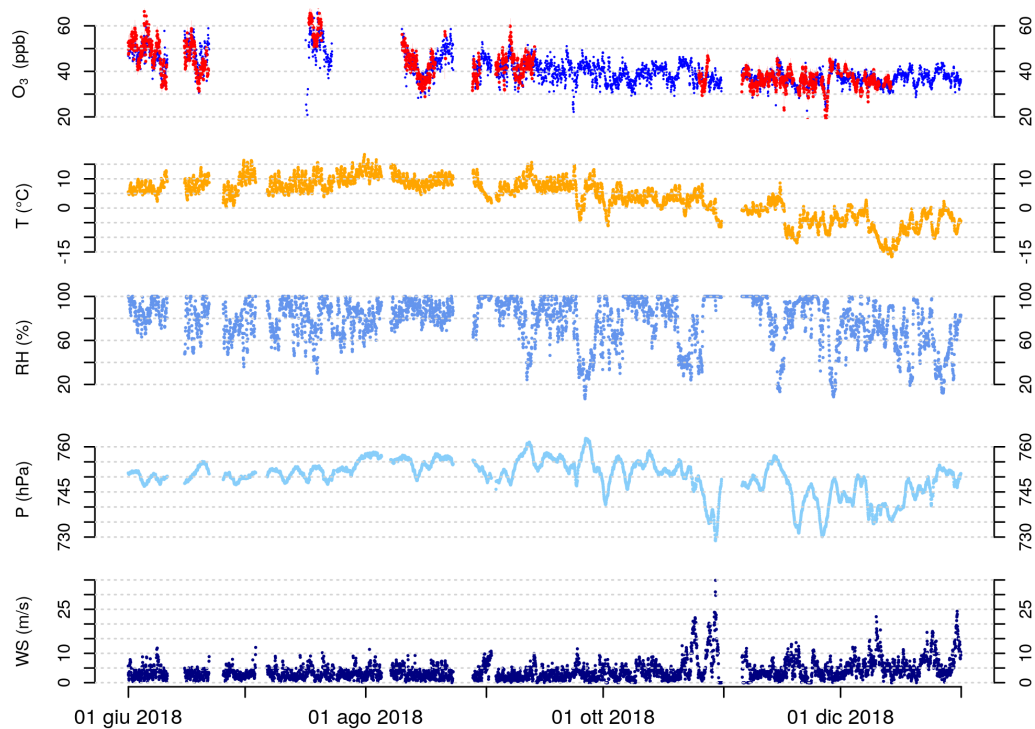


Figure S5.1. Time series of ozone concentration measurements and meteorological variables for the period June-December 2018. The first plot from the top show the LCSs ozone concentration (ppb) in blue and the reference ozone concentration (ppb) in red. The second plot shows the external air Temperature (T). The third plot shows the Relative Humidity (RH). The third plot shows the Atmospheric Pressure (P) and the fourth plot shows the Wind Speed (WS). It is clearly visible the Vaia storm event that hit the North-eastern Italy on 29th October.

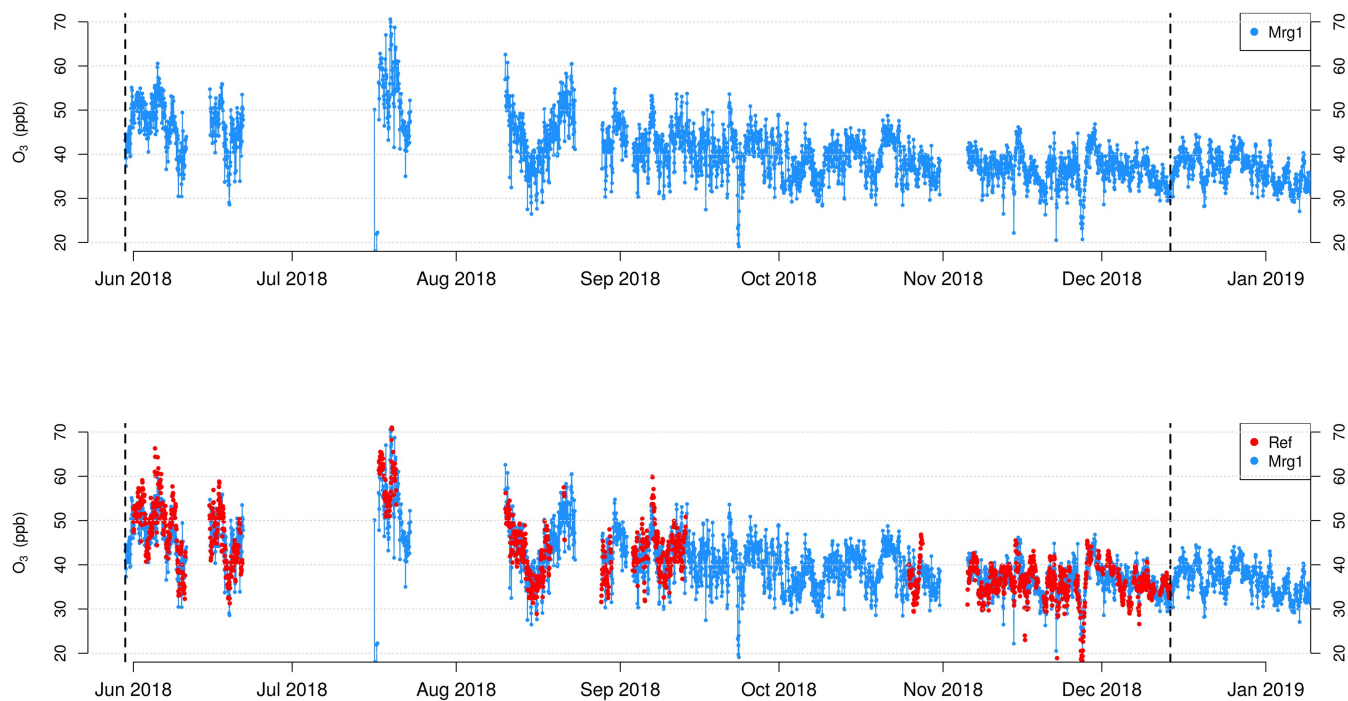


Figure S5.2. Time series of ozone concentration measurements and meteorological variables for the period June–December 2018. The first plot from the top show the Mrg1 ozone concentration (ppb) in blue and the reference ozone concentration (ppb) in red.

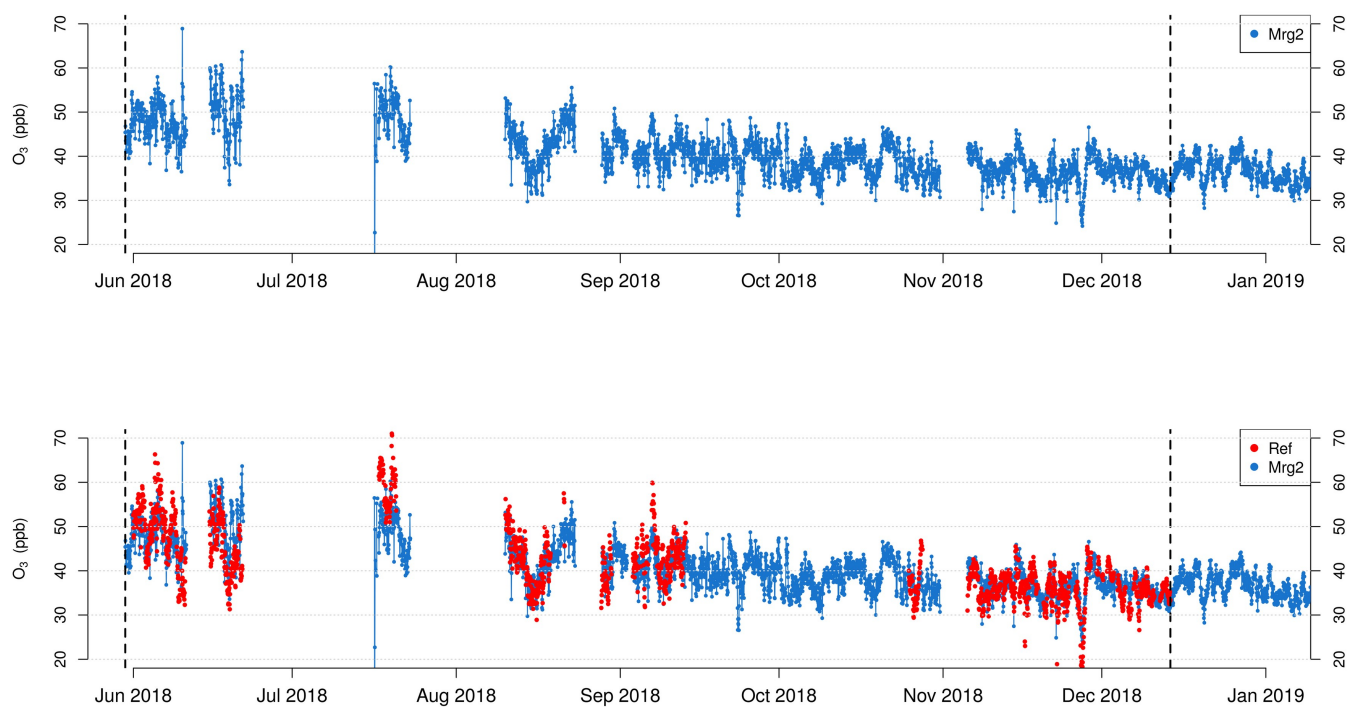


Figure S5.3. Time series of ozone concentration measurements and meteorological variables for the period June-December 2018. The first plot from the top show the Mrg2 ozone concentration (ppb) in blue and the reference ozone concentration (ppb) in red.

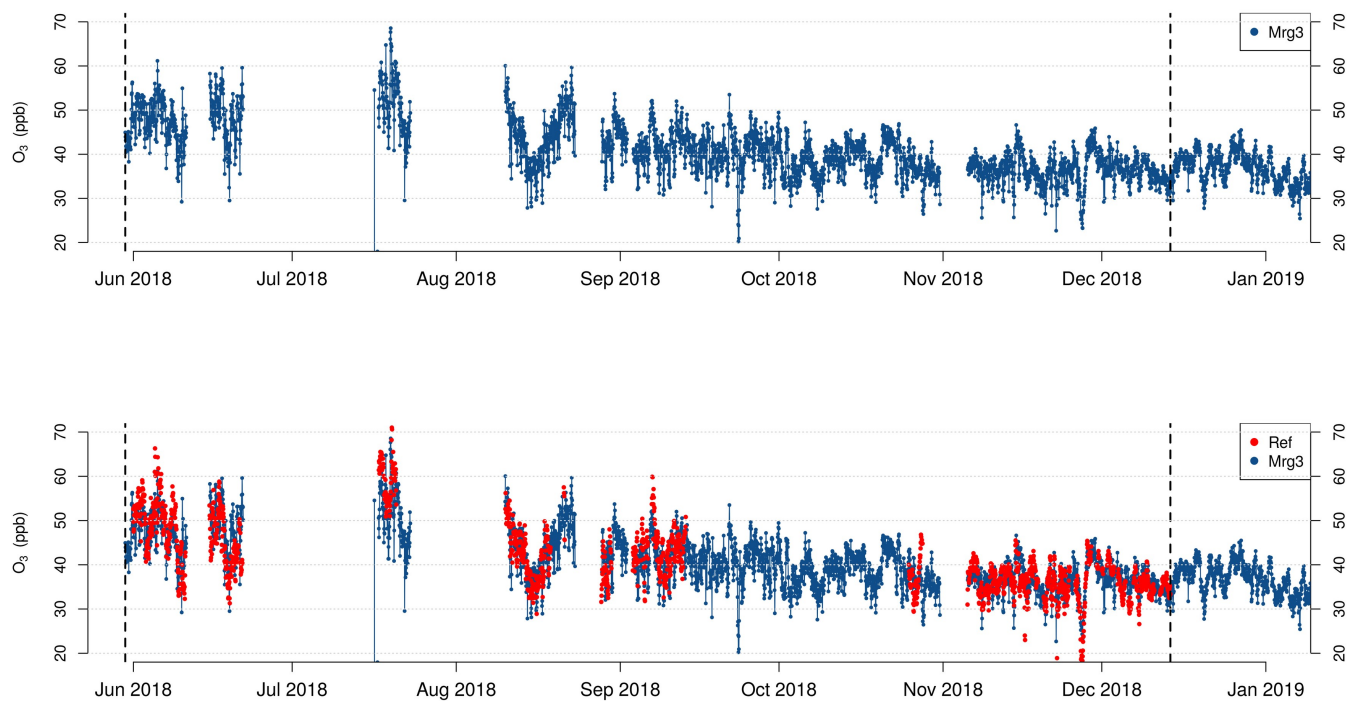


Figure S5.4. Time series of ozone concentration measurements and meteorological variables for the period June–December 2018. The first plot from the top show the Mrg3 ozone concentration (ppb) in blue and the reference ozone concentration (ppb) in red.

S5.1 Non correlating environmental variables

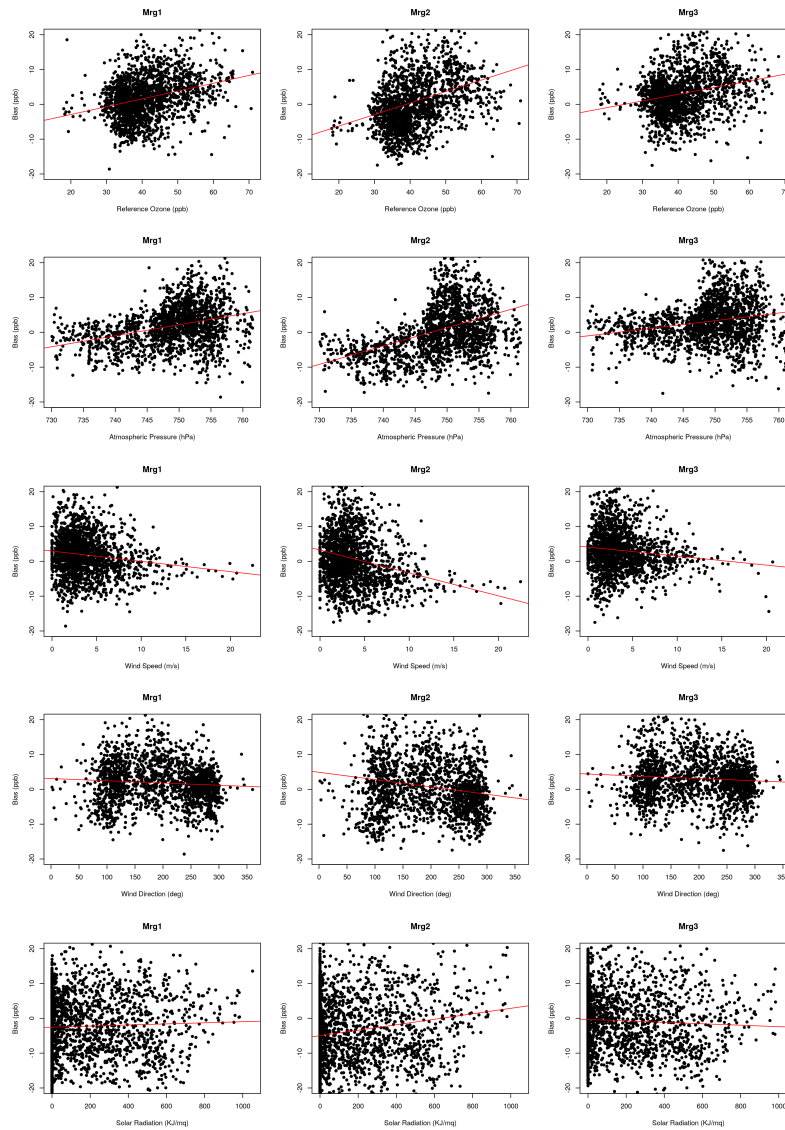


Figure S5.5. Non correlating variables. No evidence of correlation was found among the bias ($O_3^{LCS} - O_3^R$) and the incident solar radiation (PCC ≈ 0.05 , p-value ≈ 0.1), the atmospheric pressure (PCC ≈ 0.24 , p-value ≈ 0.3), the wind speed (PCC ≈ -0.22 , p-value ≈ 0.1) and the wind direction (PCC ≈ -0.10 , p-value ≈ 0.4).