



# Calibration and evaluation of broad supersaturation scanning (BS2) cloud condensation nuclei counter for rapid measurement of particle hygroscopicity and CCN activity

5 Najin Kim<sup>1</sup>, Yafang Cheng<sup>2</sup>, Nan Ma<sup>3</sup>, Mira L. Pöhlker<sup>1</sup>, Thomas Klimach<sup>1</sup>, Thomas. F. Mentel<sup>4</sup>, Ovid  
O. Krüger<sup>1</sup>, Ulrich Pöschl<sup>1</sup> and Hang Su<sup>1\*</sup>

<sup>1</sup>Multiphase Chemistry Department, Max Planck Institute for Chemistry, Mainz, 55128, Germany

<sup>2</sup>Minerva Research Group, Max Planck Institute for Chemistry, Mainz, 55128, Germany

10 <sup>3</sup>Center for Air Pollution and Climate Change Research (APCC), Institute for Environmental and Climate Research (ECI),  
Jinan University, Guangzhou, 511443, China

<sup>4</sup>Institute of Energy and Climate Research, IEK-8: Troposphere, Forschungszentrum Jülich GmbH, Jülich, 52425, Germany

*Correspondence to:* Dr. Hang Su (h.su@mpic.de)

**Abstract.** For understanding and assessing aerosol-cloud interactions and their impact on climate, reliable measurement data  
15 of aerosol particle hygroscopicity and cloud condensation nuclei (CCN) activity are required. The CCN activity of aerosol  
particles can be determined by scanning particle size and supersaturation ( $S$ ) in CCN measurements. Compared to the existing  
differential mobility analyzer (DMA)-CCN activity measurement, a broad supersaturation scanning CCN (BS2-CCN) system,  
in which particles are exposed to a range of  $S$  simultaneously, can measure the CCN activity with a high time-resolution. Based  
on a monotonic relation between the activation supersaturation of aerosol particles ( $S_{aerosol}$ ) and the activated fraction ( $F_{act}$ )  
20 of the BS2-CCN measurement, we can derive  $\kappa$ , a single hygroscopicity parameter, directly. Here, we describe how the BS2-  
CCN system can be effectively calibrated and which factors can affect the calibration curve ( $F_{act} - S_{aerosol}$ ). For calibration,  
size-resolved CCN measurements with ammonium sulfate and sodium chloride particles are performed under the three  
different thermal gradient (dT) conditions (dT=6, 8, and 10 K). We point out key processes that can affect the calibration curve  
and thereby need to be considered as follows: First, the shape of the calibration curve is primarily influenced by  $S_{max}$ , the  
25 maximum  $S$  in the activation tube. We need to determine appropriate  $S_{max}$  depending on particle size and  $\kappa$  to be investigated.  
To minimize the effect of multiply charged particles, small geometric mean diameter ( $D_g$ ) and  $\sigma_g$  geometric standard deviation  
( $\sigma_g$ ) in number size distribution are recommended when generating the calibration aerosols. Last,  $F_{act}$  is affected by particle  
number concentration and has a decreasing rate of  $0.02/100cm^{-3}$  due to the water consumption in the activation tube. For  
30 evaluating the BS2-CCN system, inter-comparison experiments between typical DMA-CCN and BS2-CCN measurement were  
performed with the laboratory-generated aerosol mixture and ambient aerosols. Good agreements of  $\kappa$  values between DMA-  
CCN and BS2-CCN measurements for both experiments show that the BS2-CCN system can measure CCN activity well  
compared to the existing measurement, and can measure a broad range of hygroscopicity distribution with a high time-



35 resolution (~1 second vs. few minutes for a standard CCN activity measurement). As the hygroscopicity can be used as a proxy for the chemical composition, our method can also serve as a complementary approach for fast and size-resolved detection/estimation of aerosol chemical composition.

## 1 Introduction

Atmospheric aerosol particles affect global climate change in that aerosols alter the radiative balance by scattering and absorbing shortwave and longwave radiation directly. Additionally, by serving as cloud condensation nuclei (CCN), atmospheric aerosol particles influence the radiative budget by modulating the microphysical structure, lifetime, and coverage of the clouds. Although the direct and indirect effects of aerosols on climate change are widely accepted within the scientific community, the assessment of aerosol-cloud interactions and the quantification of their effect on climate still remain largely uncertain (IPCC 2013). Notably, one of the underlying challenges is to determine the ability of aerosol particles that act as cloud droplet, CCN activity, which has come up as a rising issue over the past years (McFiggans et al., 2006; Andreae and Rosenfeld, 2008; Hiranuma et al., 2011; Paramonov et al., 2013).

45 The CCN activity, the fraction at which aerosol particles can be activated to become CCN, can be determined by particle size and chemical composition at a given water vapor supersaturation (Charlson et al., 2001; Andreae et al., 2005, 2007; McFiggans et al., 2006; Cai et al., 2018) and can be parameterized by a single parameter,  $\kappa$  (Petters and Kreidenweis, 2007). The activation  $S$  of aerosol particles can be estimated from dry particle diameter ( $D_d$ ) and water activity (Kohler, 1936; Su et al., 2010). Once determined, the parameter  $\kappa$  can greatly simplify the descriptions of chemical composition effect in models.

50  $\kappa$  is closely linked to the chemical compositions of aerosol particles, especially the ratio of organic to inorganic compositions. Thus,  $\kappa$  is expected to and has been demonstrated to show a size dependence due to the change of chemical compositions at different size ranges. However, size-resolved  $\kappa$  data are still limited due to the relatively slow response of the commercial instrument when scanning both  $S$  and  $D_d$  (Robert and Nenes 2005; Dusek et al., 2006; Moore and Nenes 2009a; Petters et al., 2009; Svenningsson et al., 2005; Wex et al., 2009; Rose et al., 2011; Zhao et al., 2015). For example, measurements based on the continuous-flow streamwise thermal-gradient CCN-Counter (CCNC) from Droplet Measurement Technologies (DMT) complete a cycle of size-resolved  $\kappa$  in about an hour due to the slow temperature stabilization (about few minutes to stabilize) for changing new  $S$ . To solve the low-time resolution problem, other techniques have been developed such as “Scanning Flow CCN Analysis” (SFCA) that changes flow rate over time in the growth chamber under the constant temperature gradient (Moore and Nenes, 2009) and an instantaneous CCN spectrometer with more than 40 channels of supersaturation resolution from 0.01% to 1.0% (Hudson, 1989).

60 Su et al. (2016) introduce a new concept for the design of CCN counter, the broad supersaturation scanning (BS2) approach, for the rapid measurement of particle hygroscopicity and CCN activity. Compared to the measurement system of DMT-CCNC that applies a single  $S$  at the centerline, aerosol particles of the BS2-CCN system are introduced with a wider inlet at a low sheath-to-aerosol flow ratio (SAR) and are exposed to a range of  $S$  simultaneously. Through this new design of CCNC, we can



65 obtain a monotonic relation between the activated fraction of aerosols ( $F_{act}$ ) and critical activation supersaturation ( $S_{aerosol}$ )  
and thereby calculate the size-resolved  $S_{aerosol}$  as well as  $\kappa$  directly. A decrease in time required for scanning  $S$  of BS2-CCN  
system makes it possible to derive the  $\kappa$  with a high temporal and size resolution. Additionally, a constant temperature  
difference minimizes the bias from the potential volatilization of aerosols in the instrument (Moore and Nenes, 2009).  
In this study, we introduce the experimental setup of materialized BS2-CCN system, including the newly designed inlet, and  
70 describe how the BS2-CCN system can be effectively calibrated. To validate the performance of the BS2-CCN system, we  
perform the inter-comparison with the existing DMA-CCN measurement using the laboratory-generated aerosol mixture and  
ambient aerosols.

## 2 Method

### 2.1 Concept of BS2-CCNC

75 The BS2-CCN counter, a modified commercial DMT-CCNC with a newly designed inlet system, measures the activation of  
size-resolved CCN with a high-time resolution (Su et al. 2016). Aerosol particles are introduced with a low SAR by wider  
inlet and distributed over a continuous range of  $S$  in the activation tube whereas aerosol particles of a commercial DMT-CCNC  
are forced onto the centerline facing a single  $S$ . The BS2-CCN system reduces the time required for scanning  $S$  and thereby  
obtains the  $\kappa$  with a high temporal and size resolution by using a monotonic  $F_{act} - S_{aerosol}$  relation. Figure S1 shows the  
80 comparison of supersaturation distribution in the activation tube of CCNC, denoted by  $S_{tube}$ , between typical CCNC and a  
modified CCNC for the BS2-CCN system.  $S_{tube}(r)$  is a function of  $r$ , the radial distance to the centerline of the activation  
unit, and is the highest in the centerline ( $r=0$ ). For a typical CCNC, aerosol particles pass through the centerline in the activation  
tube by narrow inlet and laminar sheath flow (Fig. S1a). Particles can be activated as CCN (i.e.,  $F_{act} = 1$ ) when  $S_{aerosol}$  of  
particles is lower than  $S_{tube}(r = 0)$  or cannot be activated (i.e.,  $F_{act} = 0$ ) when  $S_{aerosol}$  is higher than  $S_{tube}(r = 0)$ . For the  
85 modified CCNC for the BS2-CCN system, aerosol particles are introduced in a broad cross-section of the activation tube  
through a wider inlet of a low sheath-to-aerosol flow ratio (Fig. S1b). Therefore, aerosol particles show a monotonic  
dependence between  $F_{act}$  and  $S_{aerosol}$  based on  $S_{tube}$  distribution as they are simultaneously exposed to a wide range of  $S$ .  
The  $\kappa$  value of certain  $D_d$  can be derived by the  $F_{act} - S_{aerosol}$  relation directly based on  $\kappa$ -Köhler theory. This relation  
implies that  $S_{aerosol}$  can be directly determined depending on  $F_{act}$  and therefore, it is essential to get an accurate calibration  
90 curve (i.e.,  $F_{act} - S_{aerosol}$  relation).

### 2.2 Experimental setup

Figure 1 shows the schematic plot of the instrumental setup for the BS2-CCN system. The setup consists of an aerosol  
classifier, a condensation particle counter (CPC), a modified DMT-CCNC, and other components to maintain and monitor the  
working system. The aerosol sample is firstly dried to  $RH < 30\%$  with an aerosol dryer before entering the aerosol classifier



95 (TSI classifier 3080). A sensor to monitor the temperature (T), pressure (P), and RH of the aerosol sample is placed in the aerosol flow pathway. A Y-shaped splitter is mounted at the outlet of the aerosol classifier to split the selected monodispersed aerosols into two aerosol flows, CPC (TSI CPC 3772) and modified DMT-CCNC (CCN 100, DMT).

Compared to the commercial DMT-CCNC, a modified DMT-CCNC has a redesigned inlet and flow maintaining system. The newly designed diffusive inlet is used to distribute aerosol samples widely in the activation tube, as detailed in Appendix A.  
100 This new inlet allows for maintaining stable low sheath-to-aerosol flow ratios (SAR), for which monotonic  $F_{act} - S_{aerosol}$  relation can then be obtained. Compressed air is used to provide the sheath flow with a HEPA filter in-line to remove all particles in the flow. Its volume flow rate is controlled by a mass flow controller (MFC, Bronkhorst). The aerosol and sheath flows are set to  $0.46 \text{ L min}^{-1}$  and  $0.04 \text{ L min}^{-1}$ , respectively. The calibration curves with the different flow set in Fig. S2 show that, if the sample flow is set low, the slope between  $F_{act}$  and  $S_{aerosol}$  gradually decreases due to the narrow  $S$  distribution in  
105 the activation tube, making it difficult to obtain a monotonic relationship. It is noted that the total flow in the modified DMT-CCNC is maintained at  $0.5 \text{ L min}^{-1}$  by vacuum pump with MFC and filter.

For avoiding the water depletion in the activation tube by high particle number concentration, an aerosol humidifier is placed in the aerosol flow pathway to pre-humidify the monodispersed aerosols before it enters the activation tube (dashed line in Fig. 1). Pure water is circulated between the humidifier and a water reservoir by the Bath circulator (Thermo Scientific).

110  $N_{CCN}$  is recalculated with bin counts data and sample flow as  $N_{CCN}$  values recorded in the instrument software are different from what we measure due to the separated flow control system in modified DMT-CCNC. It can be calculated as follows:

$$N_{CCN} = \text{Sum of Bin counts} / \text{Sample flow} \times 60 \quad (1)$$

The 60 is a unit conversion factor since bin counts are given in particle per second while sample flow is in  $\text{cm}^{-3} \text{ min}^{-1}$ . Particle number concentration (i.e., Number concentration of condensation nuclei,  $N_{CN}$ ) is measured by CPC.  $F_{act}$  is calculated as the ratio of  $N_{CN}$  and  $N_{CCN}$ . Although each of  $N_{CN}$  and  $N_{CCN}$  data has 1s time resolution and thereby  $F_{act}$  data with 1s time  
115 resolution are initially available, we use 1-min average data to calculate  $F_{act}$  value corresponding to each  $D_d$  for the calibration curve.

### 3 Results and discussion

#### 3.1 Calibrations

120 For the calibration of the BS2-CCN system, the goal is to determine the monotonic  $F_{act} - S_{aerosol}$  relation, as discussed above. This can be obtained from the size-resolved CCN measurement with pure calibration aerosols, e.g., ammonium sulfate and sodium chloride, in which hygroscopic properties are well known. A specific  $S_{aerosol}$  corresponding to each  $D_d$  can be calculated from an approximate solution in Eq. (2).

$$S_{aerosol} \approx 100\% \times \left( \exp \left( \sqrt{\frac{4A^3}{27\kappa D_d^3}} \right) - 1 \right) \quad (2)$$



125 The  $F_{act}$  value of each  $D_d$  can be measured by the size-resolved CCN measurement, and thereby we can get a calibration curve,  $F_{act} - S_{aerosol}$  relation. Figure 2 and 9 show exemplary of calibration curves obtained in this study. We investigate the impact of several factors that may affect the calibration results.

### 3.1.1 $S_{tube}$ distribution

130  $S_{tube}$  distribution in the activation tube shows the maximum in the centerline (i.e.,  $S_{max}$ ) and the minimum at the edge (Fig. S1). Depending on the temperature gradient, controlled by the temperature difference ( $dT$ ) between the top and the heated bottom of the activation tube, the distribution of  $S_{tube}$  varies, resulting in different shapes of the calibration curve. Figure 2 shows the calibration curves depending on temperature gradients ( $dT= 6, 8, \text{ and } 10 \text{ K}$ ). For calibration experiments, we used an aerosol atomizer to generate particles with diameters of 20 – 300 nm of ammonium sulfate (purity > 99.5%, VWR Chemicals) and sodium chloride (purity > 99.5%, Sigma-Aldrich) solutions. According to Fig. 2, monotonic  $F_{act} - S_{aerosol}$  relation is confirmed by the investigated aerosol systems. Good agreements between two calibration aerosols for all three  $dT$  conditions show the reproducibility and stability of the BS2-system in measurement CCN activity, supporting its application in the real atmosphere. Large standard deviations at high  $F_{act}$  range is mainly caused by the low particle counts  $N_{CN}$  at large diameters (e.g., less than  $20 \text{ cm}^{-3}$ ).

140 Although the calibration curve covers the whole range of  $F_{act}$ , we suggest using only the center part of the curve, from 0.1 to 0.9 of  $F_{act}$ . This is because steeper slope at low  $F_{act}$  and aforementioned low  $N_{CN}$  at high  $F_{act}$  can introduce large uncertainties in the retrieved  $S_{aerosol}$  and  $\kappa$ . Moreover, it is essential to determine an appropriate  $dT$ , so that the supersaturation at the centerline,  $S_{max}$ , is higher than the highest  $S_{aerosol}$  of aerosol particles for investigated size range and environment. For the dependence of  $S_{aerosol}$ ,  $\kappa$  and  $D_d$ , please refer to the  $\kappa$ –Köhler equation (Petters and Kreidenweis, 2007) and exemplary of Fig. 2 in Wang et al. (2015).

### 145 3.1.2 Minimize the effect of doubly/multiply charged aerosols

Particles of given electrical mobility passed through the DMA are not all singly charged as a DMA extracts particle with a narrow range of electrical mobility rather than a geometric diameter. Multiply (mostly doubly) charged particles with a larger size also penetrate the DMA, accompanying the singly charged particles with a targeted diameter. As the CCN activation of a particle strongly depends on its size, a high fraction of doubly charged particles can directly affect the calibration curve (i.e.,  $F_{act} - S_{aerosol}$  relation).

150 For solving this problem, Frank et al. (2006) suggested a correction method that subtracts the doubly charged particle distribution in the number size distribution of polydisperse calibration aerosol from  $N_{CCN}/N_{CN}$  under the assumption of a bipolar equilibrium charge distribution. Rose et al. (2008) proposed the simple alternative method that calculates the fraction of activated doubly charged particles from the lower level of the plateau in the CCN spectrum, assuming a constant fraction over the whole particle size range. However, these methods are for the CCN efficiency spectra of typical CCNC using a single



$S$  in the center line of the activation tube. As BS2-CCNC has a wide range of  $S$  simultaneously in the activation tube and the number concentration of activated particles is different depending on  $S$ , it is quite complicated to apply existing methods to experimental data. Here, we compare CCNC responses with and without considering doubly charged aerosol particles and how it depends on the size distribution of calibration aerosols through calculation and experiment results.

160 We use an activation model that describes the CCNC response to the transferred polydisperse charge-equilibrated particles through an ideal DMA, similar to Petters et al. (2007). Considering electrical mobilities of particles classified by DMA and the fraction of particles carrying  $n$  charges (+1, +2) at charge equilibrium, this model calculates an idealized CCN instrument response with an assumed log-normal particle size distribution. When calculating the number of particles that activate as CCN, we need to consider the activation fraction for each aerosol particle size. As the aerosol particles in the BS2-CCN system are  
165 distributed in a broad cross section of activation tube, the activation fraction is calculated by integrating the activation fraction function and flow velocity over the cross-section of the aerosol flow. The detailed calculation procedure is described in Supplement S1.

Figure 3 shows the calculated activation fraction ( $F_{act\_total} = F_{act\_single} + F_{act\_double}$ ) for ammonium sulfate aerosols and the ratio of [+2]/[+1] charges at charge equilibrium of an assumed a log-normal size distribution with  $N = 2000\text{ cm}^{-3}$ ,  $D_g =$   
170  $50\text{ nm}$ , and  $\sigma_g = 1.4$ . Sheath flow ( $Q_{sh}$ ), and aerosol flow ( $Q_a$ ) of DMA were set to 10 lpm and 1.5 lpm, respectively, which are the same as the calibration experiment. It is noted that we used the physico-chemical properties of ammonium sulfate for the calculation and set 0.63% for  $S_{max}$  for the  $S$  distribution in the activation tube when calculating the activation fraction of aerosol particles. A small plateau exists in an area where the  $F_{act}$  is low ( $D_p < 40\text{ nm}$ ) due to doubly charged particles, however the overall effect of multiply charged particles on  $F_{act}$  is not significant and has only a small effect. The maximum  
175  $F_{act\_double}$  in the assumed particle size distribution is about 0.04. According to Fig. 4, the  $F_{act\_double}$  varies depending on the particle size distribution. The  $F_{act\_double}$  not only increases as the value of  $D_g$  increases, but also increases as the  $\sigma_g$  increases, even if the  $D_g$  is the same. As the  $F_{act}$  directly affects the calculation of  $\kappa$  for the BS2-CCN system, the effect of particle size distribution still needs to be considered even though  $F_{act\_double} < 0.1$  for  $D_g = 60\text{ nm}$  case. Therefore, when generating calibration aerosols, small  $D_g$  and  $\sigma_g$  in number size distribution are recommended to minimize the effect of multiply charged  
180 particles on the calibration curve. These effects can also be seen in the calibration experiment using sodium chloride. Figure 5 presents the calibration curves and number size distribution of  $N_{CN}$  and  $N_{CCN}$  of sodium chloride particles for  $dT = 10$  and 8 K. Sodium chloride that has a high  $\kappa$  value ( $\kappa = 1.28$ ) shows variant calibration curves depending on the particle number size distribution, whereas ammonium sulfate shows only small change in the calibration curves (Fig. S3). The  $F_{act}$  in calibration curve is higher for larger peak diameter ( $D_{peak}$ ), and accordingly, the gap in the calibration curve between the ammonium sulfate and sodium chloride increases. Specifically, according to Fig. 5a ( $dT = 10\text{ K}$ ), the calibration curve of sodium chloride particle with  $D_{peak}$  of 31 nm matches well with that of ammonium sulfate. However, the calibration curve of sodium chloride  
185 with  $D_{peak}$  of 37 nm and 52 nm are inconsistent with that of ammonium sulfate. This effect is more pronounced at higher supersaturation conditions. Both calculation and experiment results imply that the number size distribution of the generated



190 particles should be considered, especially when using sodium chloride during calibration, and it is recommended to generate aerosols with  $D_{peak}$  corresponding to an  $F_{act}$  less than 0.3. The number size distribution of generated calibration aerosols can be controlled by adjusting the particle concentration.

### 3.1.3 Effect of particle number concentration

As the modified CCNC enlarges the cross-section of aerosol flow, more particles can enter the column compared to a in the standard DMT-CCNC. The consumption of water vapor in the column by a large number of particles can change the  
195 distribution of the supersaturation and thereby influence the measured number fraction of activated particles. Therefore, as a simple test, the  $F_{act}$  values of three different sizes of ammonium sulfate particles (60, 80, and 120 nm) are measured under the different particle number concentrations. In this experiment,  $dT$  is set to be 7.7 ( $S = 0.6\%$ ). According to Fig. 6, we can see that  $F_{act}$  decreases with a rate of about  $0.02/(100 \text{ cm}^{-3})$  with the increase of the particle number concentration. Specifically,  $F_{act}$  decreases by about 2.6% (60 nm), 1.6% (80 nm) and 1.1% (120 nm) per increase of  $100 \text{ cm}^{-3}$  in the number of particles.  
200 It is noted that the decrease with particle number is calculated for a particle number concentration of  $300 \text{ cm}^{-3}$  of ammonium sulfate, and the decrease is expected to be greater if the number concentration increases. The decreasing rate increases slightly as the particle size decreases. These results imply that the number concentration of calibration aerosols can affect the calibration result, and we can get consistent results even in very low number concentrations from this BS2-CCNC setup.

For examining the necessity of a humidifier to avoid water consumption in the activation tube, an aerosol humidifier is installed  
205 additionally in the aerosol flow pathway. The setup is described in Fig. 1, and the part is marked by the blue dashed line. Monodispersed aerosols are pre-humidified by the humidifier that is composed of a Nafion tube and a bath circulator before the aerosol flow enters the BS2-CCN system. Particle number concentrations are controlled within the range of  $\sim 300 \text{ cm}^{-3}$ . Figure 7 shows the calibration curves for three  $dT$  conditions ( $dT=6, 8, \text{ and } 10 \text{ K}$ ) with a humidifier (blue dots) and without a humidifier (black dots). For  $dT=6 \text{ K}$ , the calibration curves with the humidifier system (WH) and without the humidifier system  
210 (NH) are almost identical. Although  $F_{act}$  values of WH are slightly higher than those of NH under higher  $dT$  conditions (i.e.,  $dT= 8 \text{ and } 10 \text{ K}$ ), differences are not significant as number concentrations of calibration aerosol are not so high. In other words, a compact instrumental setup without the pre-humidifier system is sufficient for the BS2-CCNC calibration experiment as well as the measurement if aerosol particles are kept below  $\sim 3 \times 10^2 \text{ cm}^{-3}$ . Otherwise, we need a pre-humidifier system for high aerosol number concentration condition to avoid the decrease of  $F_{act}$ . It is noted that particle concentrations below  $\sim 3 \times 10^3$   
215  $\text{cm}^{-3}$  are recommended to avoid counting error for calibration experiment of typical DMT-CCNC (Rose et al., 2008). We usually observe the low number concentration for aerosol particles during the size-resolved CCN measurement and  $F_{act}$  is not highly variable within that range. However, we still need to consider this effect, especially for the region of high number concentration and/or high-number concentration cases like new particle formation (NPF) events and the transport of pollution.



### 220 3.2 Fitting procedure of calibration curve

As selected diameters for calibration are limited and cannot cover the whole  $F_{act}$  values, the curve fitting procedure is necessary. The equation for curve fitting (Eq.3), the relationship between  $F_{act}$  and  $S_{aerosol}$ , can be derived based on Eq. (S8) and cosine function of  $S_{tube}$  distribution in Supplement S1.

$$F(x) = a \times \text{acos}(b \times x) - c \quad (3)$$

225 where  $F(x)$  and  $x$  correspond to  $S_{aerosol}$  and  $F_{act}$ , respectively. Coefficients of  $a$ ,  $b$ , and  $c$  are what we need to be obtained from the curve-fitting procedure. They are calculated using a non-linear least square method (MATLAB curve fitting toolbox 3.5.8). It is noted that the data less than 0.05 of  $F_{act}$ , showing the large discrepancy between reference curves and experimental data, are excluded for curve fitting.

Figure 8 shows fitting curves and experimental data from ammonium sulfate particles for three dT conditions (dT = 6, 8, and  
230 10 K). Coefficients and goodness of fit for each curve are presented in Table 1. For assessing the goodness of fit, three statistical parameters were used: Error sum of squares (SSE), coefficient of determination ( $R^2$ ), and root mean square error (RMSE). According to Fig. 8 and Table 1, fitting curves cover most of the experiment data, and good fitting results are shown for all three dT conditions. It implies that Eq. (3) covers the experimental data well and appears suitable for the calibration curve of the BS2-CCN system. Also,  $S_{aerosol}$  corresponding to the  $F_{act}$  can be directly obtained through this curve. Furthermore, we  
235 can calculate the effective particle hygroscopicity parameter,  $\kappa$ , based on  $\kappa$  – Köhler theory (Petters and Kreidenweis, 2007). Figure S4 presents  $\kappa$  values, which correspond to the  $F_{act}$  values of a particle ranged from 50 nm to 150 nm. They are calculated with a fitting curve equation of dT=8 K condition shown in Fig. 8 and Table 1.

As  $F_{act}$  values obtained from the size-resolved CCN measurement use 1-min average data, the calibration curve could have the range, not a single curve line. To consider the range of  $F_{act}$ , we add two more calibration curve lines applying data points  
240 of  $F_{act\_low}$  (average - standard deviation,  $\mu - \sigma$ ) and  $F_{act\_high}$  ( $\mu + \sigma$ ). Figure 9 shows the range of the calibration curve for the dT=8 K condition. All of the calibration curves are obtained using Eq. (3) for curve fitting. When the  $F_{act}$  is measured at a certain  $D_p$ , three  $\kappa$  values, denoted as  $\kappa_{high}$ ,  $\kappa_{avg}$  and  $\kappa_{low}$ , can be calculated based on these three curves. Specifically,  $\kappa_{high}$  is derived from the curve that is obtained from data points of  $F_{act\_low}$ , and vice versa.

### 4. Evaluation and application of BS2-CCN system

245 To evaluate the BS2-CCN system, we performed two inter-comparison experiments between BS2-CCN and standard DMA-CCN measurement (denoted as ‘DMA-CCN’) with a laboratory-generated aerosol mixture and ambient aerosols. The DMA-CCN measurement is widely used for the size-resolved CCN measurement in the aerosol community to examine the CCN activity (Cai et al., 2018; Deng et al., 2011; Moore et al., 2011; Rose et al., 2011; Pöhlker et al., 2016, 2018; Thalman et al., 2017 and references therein). For DMA-CCN measurement, critical diameter ( $D_c$ ) that  $F_{act}$  becomes 0.5 is determined by  
250 scanning  $D_p$  under a given constant supersaturation (i.e.,  $D_p$  scan) and  $\kappa$  can be calculated with a given S and  $D_c$  based on  $\kappa$  –



Köhler theory (Petters and Kreidenweis, 2007). In other words, in DMA-CCN measurement, we can obtain single  $D_c$  value for each  $D_p$  scan and convert it to single  $\kappa$ , but in BS2-CCN measurement, we can obtain  $\kappa$  values at all selected particle sizes of each  $D_p$  scan by converting  $F_{act}$  values using the calibration curve. Figure S5 presents the schematic plot of the instrumental setup for inter-comparison experiments. Specifically, selected monodisperse aerosol flows by the DMA (TSI classifier 3080) are split into three parallel lines and fed into CPC, modified CCNC (CCN-100, DMT for BS2-CCNC), and DMT-CCNC (CCN-200, DMT for DMA-CCNC). Before entering the DMA, all aerosol particles are dried ( $RH < 30\%$ ) by the Nafion tube aerosol dryer and neutralized by Krypton-85 (Kr 85) bipolar charger. All instruments were installed in the laboratory at the Max Planck Institute for Chemistry, Mainz, Germany. A detailed set of experiments for each inter-comparison experiment is described in the following section.

#### 4.1 Ammonium sulfate and succinic acid mixture

We used an atomizer to generate nanoparticles with diameters of 30 – 160 nm by spraying a mixed solution of succinic acid and ammonium sulfate. This mixture was chosen to mimic a typical atmospheric aerosol composed of ammonium sulfate and organic acids. For the mixture, molar ratios of ammonium sulfate and succinic acid used in this study were 1:1, 3:1, and 1:3. The experiments were performed under  $dT=8$  K (0.63 %  $S$ ) condition. The sample flow rates of CCNCs were 0.04 lpm and 0.46 lpm for the DMA-CCN and BS2-CCN measurements, respectively. The total flow rate (sample + sheath) was 0.5 lpm for both instruments. As the  $\kappa$  of ammonium sulfate is higher than that of succinic acid (i.e., more hygroscopic), a mixture of ammonium sulfate and succinic acid in a ratio of 3:1 shows the highest  $\kappa$  value among three mixtures and vice versa. Table 2 presents details of the comparison for all three solutions. The  $\kappa$  values of the DMA-CCN measurement for all three solutions are within the range of  $\kappa$  for the BS2-CCN measurement, but is slightly lower (less than about 10 % of relative deviation) than the  $\kappa_{avg}$ . These results infer that we can measure  $\kappa$  of aerosol mixture quantitatively well from the BS2-CCN measurement compared to the existing measurement method, DMA-CCN measurement.

#### 4.2 Ambient aerosol measurement

An inter-comparison experiment with ambient aerosols was performed from 13 July to 16 July 2020. The instrumental setup and flow system were the same as in Section 3.1. For  $D_p$  scan (fixed  $S$ ), 19 dry diameters of 40 – 250 nm were selected for each scan. Each scan took a total of 22 minutes, including 1 min for each diameter and 3 min for stabilization. The  $S$  of CCNC was set to be 0.63 % ( $dT=8$  K) for BS2-CCN measurement and 0.4% for DMA-CCN measurement. The  $S$  of DMA-CCN measurement was set slightly lower because the comparison with  $\kappa$  of BS2-CCN measurement is difficult if the critical diameter is too small, which is obtained from the DMA-CCN measurement. It is noted that  $\kappa$  values from BS2-CCN measurement were calculated based on the fitting curve for  $dT=8$  K, as shown in Fig. 9 and Table 1. Figure 10 shows the times series of  $F_{act}$  and  $\kappa$  distribution of BS2-CCN measurement. Here  $\kappa_{avg}$ , derived from  $F_{act,avg}$ , is referred to as  $\kappa$ . For  $\kappa$  calculation, high  $F_{act}$  ( $> 0.85$ ) and low  $F_{act}$  ( $< 0.1$ ) data are excluded.  $F_{act}$  distribution showed a clear size-dependency, low



$F_{act}$  for small particles and high  $F_{act}$  for large particles. Since the  $\kappa$  value is calculated based on the  $F_{act}$  value, the  $\kappa$  value appeared to be increasing at the time when the  $F_{act}$  was increased, and vice versa. The average  $\kappa$  values of particles for the BS2-CCN measurement exhibit diurnal variability that increases during the daytime and decreases at nighttime within the range of 0.11 to 0.32 (Fig. 10 and Fig. S6) and has an average value of 0.18. For DMA-CCN measurement, average  $D_c$  and  $\kappa$  was about 80 nm and 0.17, respectively, during the measurement under the 0.4 %  $S$  condition. Figure S7 presents the average CCN efficiency spectra and the cumulative particle hygroscopicity distribution,  $H(\kappa, D_d)$ , of DMA-CCN measurement. Particularly, the  $\kappa$  values of a significant portion of particles were distributed between 0.1 and 0.3, which was consistent with the result of the BS2-CCN measurement. Figure 11 presents the hourly-averaged  $\kappa$  value of BS2-CCN and DMA-CCN measurement. Unlike BS2-CCN measurement results, which show  $\kappa$  distribution of various particle sizes, DMA-CCN measurement allows a single  $\kappa$  value to be produced per each  $D_p$  scan cycle. Therefore, as shown in Fig. 11, we used  $\kappa$  value of BS2-CCN measurement by selecting the particle diameter close to the average  $D_c$  of the DMA-CCN measurement for the inter-comparison. Compared to the  $\kappa$  values of the DMA-CCN measurement, those from the BS2-CCN measurement showed a good agreement, keeping up with the increasing and decreasing variability. Additionally, a direct inter-comparison was carried out through the 1:1 scatterplot between the  $\kappa$  of BS2-CCN and DMA-CCN measurements in Fig. 12. All the detailed inter-comparison results, including the ratio between  $\kappa$  of DMA-CCN and BS2-CCN measurement and goodness of fit of the linear regression line for each scatter plot, are presented in Table 3. It is noted that  $\kappa_{high}$ , showing excessively high value compared to that of DMA-CCN measurement, are excluded in Fig. 11 and 12. We can conclude through the good agreements of  $\kappa$  value as well as results of three different statistical values to judge the goodness of fitting, including a residual sum of squares, Pearson's  $r$ , and  $R^2$  that we can obtain reliable and quantitative  $\kappa$  data, as well as the  $\kappa$  variability from BS2-CCN measurement compared to the existing DMA-CCN measurement. The possible reason for the discrepancy of  $\kappa$  between BS2-CCN and DMA-CCN measurement is the multimode  $\kappa$  distribution. According to Fig. S7, we can infer that aerosols were externally mixed, not a single mode. The BS2-CCN system alone cannot resolve bimodal or multimodal  $\kappa$  distribution, and thereby when particles at a certain size are externally mixed, lower  $F_{act}$ , resulting in lower  $\kappa$ , can be observed. In particular,  $\kappa$  values of BS2-CCN measurement are slightly higher than those of DMA-CCN measurement between 15 and 16 July when externally mixed aerosols were frequently observed. Su et al. (2016) pointed out through the simulation that BS2-CCN measurement can underestimate  $\kappa$  when particles are externally mixed. The uncertainty of  $F_{act}$  values for each measurement caused by the uncertainty of each CCNC can be another possible reason for the discrepancy. The  $F_{act}$  value is essential for both measurements as  $\kappa$  is directly determined by  $F_{act}$  for BS2-CCN and  $D_c$  of a DMA-CCN measurement can be changed depending on  $F_{act}$ . The selected diameters of BS2-CCN measurement for comparison in Fig. 11 and Fig. 12 do not perfectly match with the  $D_c$  of DMA-CCN measurement because  $D_c$  in this study is not fixed due to the ' $D_p$  scan' method, scanning  $D_p$  with a constant  $S$ . The difference of time resolution can also be a cause of the discrepancy, although the impact may not be significant in this study. As we use 1 min average data per particle size, we can obtain  $\kappa$  values for every 1 minute for the BS2-CCN measurement but only every 19 minutes for the DMA-CCN measurement. Therefore, a difference  $\kappa$  is expected if there



315 are fast changes of the aerosol. Nevertheless, good correlation and correspondence of  $\kappa$  values between DMA-CCN and BS2-  
CCN measurement from both inter-comparison experiments infer that we can obtain a high time resolution with reliable  
hygroscopicity data from the BS2-CCN system. These powerful advantages allow for applying the BS2-CCN system  
preferably to ship and aircraft measurements requiring high time-resolution, as well as ground-based measurements for  $\kappa$   
distribution with a broad particle size range.

## 320 **5 Summary and conclusion**

In this study, we implement a new concept for the design of CCN counters, a broadening supersaturation scanning BS2-CCN  
system, for rapid hygroscopicity measurement and describe how to calibrate this system. Compared to the typical CCN  
counters, particles are exposed to a range of  $S$  simultaneously in an activation tube with a newly designed inlet and low sheath-  
to-aerosol flow ratio (SAR). Through this system, we can obtain a monotonic relation between  $F_{act}$  and  $S_{aerosol}$ . Based on the  
325  $\kappa - Köhler$  theory,  $\kappa$  can be derived directly through the calibration curve (i.e.,  $F_{act} - S_{aerosol}$  relation) when we measured  
the  $F_{act}$  value at a certain  $S$ .

For calibration, ammonium sulfate and sodium chloride, representative calibration aerosols for CCNC, are used under three  
different dT conditions. It can be inferred from consistent results between two calibration aerosols as well as reference curves  
for all three dT conditions that the experimental setting of the BS2-CCN system, suggested in this study, is appropriate and  
330 can apply to the real measurement. We also examine factors that can affect the calibration curves. In the first,  $S_{max}$ , the  
maximum  $S$  in the activation tube, determine  $S_{tube}$  distribution in the activation tube and the shape of the calibration curve  
changes accordingly. The range of particle size and  $\kappa$  value that we can measure depends on the  $S_{max}$  value. Specifically, a  
high  $S_{max}$  can cover the wide range of particle size and  $\kappa$ , but the steeper slope of the calibration curve can lead to high  
sensitivity of  $S_{aerosol}$  corresponding to the measured  $F_{act}$ . Therefore, depending on the particle size and environment to be  
335 investigated, we need to determine an appropriate  $S_{max}$ . Calculation and experimental results confirm that multiply charged  
particles have a small but measurable effect on the  $F_{act}$  value and show that the effect depends on the size distribution of the  
particles. For minimizing the effect of multiply charged particles, small  $D_g$  and  $\sigma_g$  in number size distribution are  
recommended when generating calibration particles. This effect is more pronounced for sodium chloride with very high  
hygroscopicity and/or higher dT conditions. Lastly, we examine the effect of particle number concentration on the calibration  
340 curve. The activated particle number fraction decreases with a rate of about  $0.02/(100 \text{ cm}^{-3})$  within  $\sim 300 \text{ cm}^{-3}$  of ammonium  
sulfate particles, and the decreasing rate is expected to be much higher when the concentration is higher due to the water  
consumption in the activation tube. It implies that we need to generate fewer particles for the calibration experiment of the  
BS2-CCN system compared to that of typical CCNC. Particles below  $\sim 3 \times 10^2 \text{ cm}^{-3}$  are recommended for generating  
calibration aerosols. If the number of particles is high, the pre-humidifier system is helpful to avoid decreasing  $F_{act}$ .

345 As selected particles for the calibration experiment cannot cover the whole  $F_{act}$  range, the curve fitting procedure is essential.  
We propose the equation for curve fitting (Eq.3) based on the equation of  $S_{tube}$  distribution. It is noted that the data lower than



0.05 of  $F_{act}$  are excluded. Good results of statistical parameters to judge the goodness of fit is shown for all three different  $dT$  conditions. With these curves, we performed two inter-comparison experiments between DMA-CCN and BS2-CCN measurement for evaluation; Laboratory generated aerosol mixture and ambient aerosol measurement. Firstly,  $\kappa$  values of the mixture of ammonium sulfate and succinic acid with three different molar ratios were compared. The  $\kappa$  values of the BS2-CCN measurements agree well with those of DMA-CCN measurement. For ambient aerosol measurement,  $S$  of CCNC was set to be 0.63 % ( $dT=8$  K) for BS2-CCN measurement and 0.4% for DMA-CCN measurement. For BS2-CCN measurement,  $\kappa$  distribution between 70 nm and 120 nm in diameter showed a size-dependency, low  $\kappa$  at small particle and high  $\kappa$  at the large particle, and a distinct diurnal variability that increases during the daytime and decreases during the nighttime. Also, the  $\kappa$  values of BS2-CCN measurement corresponded and correlated well with those from DMA-CCN measurement. It can be concluded from these results that the BS2-CCN system can measure  $\kappa$  quantitatively well compared to the existing measurement method and even can measure a broad range of  $\kappa$  distribution with high-time resolution.

The BS2-CCN system, a simple modification of the commercial design of CCNC, uses constant supersaturation and flow during the measurement, so it is technically simple, and thereby we can obtain stable data with a high-time resolution. And low SAR of the BS2-CCN system provides sufficient counting statistics for size-resolved measurement, in which particle concentrations are generally low. Besides, the calibration of the BS2-CCN system is not complicated and has many similarities compared to the existing method, so it is easy to apply. The advantages of the fast response and stability, as well as the relatively simple calibration method of the BS2-CCN system, make it possible to apply not only to long-term observation but also extensive measurements including aircraft, ship, and ground. Lastly, as the hygroscopicity can be used as a proxy for the chemical composition, our method can also serve as a complementary approach for fast and size-resolved estimation of aerosol chemical composition.



### **Data availability**

Data can be accessed by contacting the corresponding author.

### 370 **Author contributions**

HS and YC had the initial idea, and HS, YC, and NM designed the BS2 instrument. TFM provided the CCNC instrument and discussed the new system. NK organized and performed all experiments. MP provided the instrument for the inter-comparison experiment. OK supported inter-comparison experiment. TK provided technical support for experiments. NK wrote the paper. All coauthors discussed and results and commented on the paper.

### 375 **Competing interests**

The authors declare that they have no conflict of interest.

### **Acknowledgments**

This work was supported by the Max Planck Society (MPG).



## 380 References

- Andreae, M. O., Hegg, D., Feichter, J., Kloster, S., Levin, Z., Liousse, C., Radke, L., and Stier, P.: Sources and nature of atmospheric aerosols, in: Scientific assessment of the effects of aerosols on precipitation, edited by: Levin, Z. and Cotton, W., World Meteorological Organization, 2007.
- Andreae, M. O., Jones, C. D., and Cox, P. M.: Strong present-day aerosol cooling implies a hot future, *Nature*, 435, 1187–  
385 1190, 2005.
- Andreae, M. O. and Rosenfeld, D.: Aerosol-cloud-precipitation interactions. Part 1. The nature and sources of cloud-active aerosols, *Earth Sci. Rev.*, 89, 13–41, 2008.
- Cai, M., Tan, H., Chan, C. K., Qin, Y., Xu, H., Li, F., Schurman, M. I., Liu, L., and Zhao, J.: The size-resolved cloud condensation nuclei (CCN) activity and its prediction based on aerosol hygroscopicity and composition in the Pearl Delta  
390 River (PRD) region during wintertime 2014, *Atmos. Chem. Phys.*, 18, 16419–16437, <https://doi.org/10.5194/acp-18-16419-2018>, 2018.
- Charlson, R. J., Seinfeld, J. H., Nenes, A., Kulmala, M., Laaksonen, A., and Facchini, M. C.: Reshaping the theory of cloud formation, *Science*, 292, 2025–2026, 2001.
- Deng, Z. Z., Zhao, C. S., Ma, N., Liu, P. F., Ran, L., Xu, W. Y., Chen, J., Liang, Z., Liang, S., Huang, M. Y., Ma, X. C., Zhang,  
395 Q., Quan, J. N., Yan, P., Henning, S., Mildenberger, K., Sommerhage, E., Schäfer, M., Stratmann, F., and Wiedensohler, A.: Size-resolved and bulk activation properties of aerosols in the North China Plain, *Atmos. Chem. Phys.*, 11, 3835–3846, <https://doi.org/10.5194/acp-11-3835-2011>, 2011.
- Dusek, U., Frank, G. P., Hildebrandt, L., Curtius, J., Schneider, J., Walter, S., Chand, D., Drewnick, F., Hings, S., Jung, D., Bor-  
400 rmann, S., and Andreae, M. O.: Size Matters More Than Chemistry for Cloud-Nucleating Ability of Aerosol Particles, *Science*, 312, 1375–1378, doi:10.1126/science.1125261, 2006.
- Frank, G. P., Dusek, U., and Andreae, M. O. (2006). Technical Note: A Method for Comparing Size-Resolved CCN in the Atmosphere, *Atmos. Chem. Phys. Discuss.* 6:4879–4895.
- Hiranuma, N., Brooks, S. D., Gramann, J., and Auvermann, B. W.: High concentrations of coarse particles emitted from a cattle feeding operation, *Atmos. Chem. Phys.*, 11, 8809–8823, <https://doi.org/10.5194/acp-11-8809-2011>, 2011.
- 405 Hudson, J. G.: An Instantaneous CCN Spectrometer, *J. Atmos. Ocean. Tech.*, 6, 1055–1065, 1989.
- IPCC: Climate Change: the physical science basis, Working Group I Contribution to the Fifth Assessment Report of the Intergovernmental Panel on Climate Change, Cambridge University Press, Cambridge, UK, New York, NY, USA 2013, 2013.
- Kohler, H.: The nucleus in the growth of hygroscopic droplets, *T. Faraday Soc.*, 32, 1152–1161, 1936.
- McFiggans, G., Artaxo, P., Baltensperger, U., Coe, H., Facchini, M. C., Feingold, G., Fuzzi, S., Gysel, M., Laaksonen, A.,  
410 Lohmann, U., Mentel, T. F., Murphy, D. M., O’Dowd, C. D., Snider, J. R., and Weingartner, E.: The effect of physical and chemical aerosol properties on warm cloud droplet activation, *Atmos. Chem. Phys.*, 6, 2593–2649, 2006, <http://www.atmos-chem-phys.net/6/2593/2006/>.



- Moore, R. H. and Nenes, A.: Scanning Flow CCN Analysis – A Method for Fast Measurements of CCN Spectra, *Aerosol Sci. Tech.*, 43, 1192–1207, doi:10.1080/02786820903289780, 2009.
- 415 Moore, R. H., Bahreini, R., Brock, C. A., Froyd, K. D., Cozic, J., Holloway, J. S., Middlebrook, A. M., Murphy, D. M., and Nenes, A.: Hygroscopicity and composition of Alaskan Arctic CCN during April 2008, *Atmos. Chem. Phys.*, 11, 11807–11825, <https://doi.org/10.5194/acp-11-11807-2011>, 2011.
- Paramonov, M., Aalto, P. P., Asmi, A., Prisle, N., Kerminen, V.-M., Kulmala, M., and Petäjä, T.: The analysis of size-segregated cloud condensation nuclei counter (CCNC) data and its implications for cloud droplet activation, *Atmos. Chem. Phys.*, 13, 10285–10301, <https://doi.org/10.5194/acp-13-10285-2013>, 2013.
- 420 Petters, M. D. and Kreidenweis, S. M.: A single parameter representation of hygroscopic growth and cloud condensation nucleus activity, *Atmos. Chem. Phys.*, 7, 1961–1971, doi:10.5194/acp-7-1961-2007, 2007.
- Petters, M. D., Carrico, C. M., Kreidenweis, S. M., Prenni, A. J., DeMott, P. J., Collett Jr., J. L., and Moosmuller, H.: Cloud condensation nucleation activity of biomass burning aerosol, *J. Geophys. Res.*, 114, D22205, doi:10.1029/2009jd012353, 425 2009.
- Petters, M. D., A. J. Prenni, S. M. Kreidenweis, and P. J. DeMott.: On measuring the critical diameter of cloud condensation nuclei using mobility selected aerosol, *Aerosol. Sci. Technol.*, 41, 907–913, 2007.
- Pöhlker, M. L., Pöhlker, C., Ditas, F., Klimach, T., Hrabe de Angelis, I., Araújo, A., Brito, J., Carbone, S., Cheng, Y., Chi, X., Ditz, R., Gunthe, S. S., Kesselmeier, J., Könemann, T., Lavric, J. V., Martin, S. T., Mikhailov, E., Moran-Zuloaga, D., Rose, 430 D., Saturno, J., Su, H., Thalman, R., Walter, D., Wang, J., Wolff, S., Barbosa, H. M. J., Artaxo, P., Andreae, M. O., and Pöschl, U.: Longterm observations of cloud condensation nuclei in the Amazon rain forest – Part 1: Aerosol size distribution, hygroscopicity, and new model parametrizations for CCN prediction, *Atmos. Chem. Phys.*, 16, 15709–15740, <https://doi.org/10.5194/acp-16-15709-2016>, 2016.
- Pöhlker, M. L., Ditas, F., Saturno, J., Klimach, T., Hrabe de Angelis, I., Araújo, A. C., Brito, J., Carbone, S., Cheng, Y., Chi, 435 X., Ditz, R., Gunthe, S. S., Holanda, B. A., Kandler, K., Kesselmeier, J., Könemann, T., Krüger, O. O., Lavric, J. V., Martin, S. T., Mikhailov, E., Moran-Zuloaga, D., Rizzo, L. V., Rose, D., Su, H., Thalman, R., Walter, D., Wang, J., Wolff, S., Barbosa, H. M. J., Artaxo, P., Andreae, M. O., Pöschl, U., and Pöhlker, C.: Long-term observations of cloud condensation nuclei over the Amazon rain forest – Part 2: Variability and characteristics of biomass burning, long-range transport, and pristine rain forest aerosols, *Atmos. Chem. Phys.*, 18, 10289–10331, <https://doi.org/10.5194/acp-18-10289-2018>, 2018.
- 440 Roberts, G. C. and Nenes, A.: A Continuous-Flow Streamwise Thermal-Gradient CCN Chamber for Atmospheric Measurements, *Aerosol Sci. Tech.*, 39, 206–221, 2005.
- Rose, D., Gunthe, S. S., Mikhailov, E., Frank, G. P., Dusek, U., Andreae, M. O., and Pöschl, U.: Calibration and measurement uncertainties of a continuous-flow cloud condensation nuclei counter (DMT-CCNC): CCN activation of ammonium sulfate and sodium chloride aerosol particles in theory and experiment, *Atmos. Chem. Phys.*, 8, 1153–1179, 445 <https://doi.org/10.5194/acp-8-1153-2008>, 2008.



- Rose, D., Gunthe, S. S., Su, H., Garland, R. M., Yang, H., Berghof, M., Cheng, Y. F., Wehner, B., Achtert, P., Nowak, A., Wiedensohler, A., Takegawa, N., Kondo, Y., Hu, M., Zhang, Y., Andreae, M. O., and Pöschl, U.: Cloud condensation nuclei in polluted air and biomass burning smoke near the mega-city Guangzhou, China – Part 2: Size-resolved aerosol chemical composition, diurnal cycles, and externally mixed weakly CCN-active soot particles, *Atmos. Chem. Phys.*, 11, 2817–2836, doi:10.5194/acp-11-2817-2011, 2011.
- 450 Su, H., Cheng, Y., Ma, N., Wang, Z., Wang, X., Pöhlker, M. L., Nillius, B., Wiedensohler, A., and Pöschl, U.: A broad supersaturation scanning (BS2) approach for rapid measurement of aerosol particle hygroscopicity and cloud condensation nuclei activity, *Atmos. Meas. Tech.*, 9, 5183–5192, <https://doi.org/10.5194/amt-9-5183-2016>, 2016.
- Su, H., Rose, D., Cheng, Y. F., Gunthe, S. S., Massling, A., Stock, M., Wiedensohler, A., Andreae, M. O., and Pöschl, U.: Hygroscopicity distribution concept for measurement data analysis and modeling of aerosol particle mixing state with regard to hygroscopic growth and CCN activation, *Atmos. Chem. Phys.*, 10, 7489–7503, <https://doi.org/10.5194/acp-10-7489-2010>, 2010.
- 455 Svenningsson, B., Rissler, J., Swietlicki, E., Mircea, M., Bilde, M., Facchini, M. C., Decesari, S., Fuzzi, S., Zhou, J., Mønster, J., and Rosenørn, T.: Hygroscopic growth and critical supersaturations for mixed aerosol particles of inorganic and organic compounds of atmospheric relevance, *Atmos. Chem. Phys. Discuss.*, 5, 2833–2877, 2005.
- Thalman, R., de Sá, S. S., Palm, B. B., Barbosa, H. M. J., Pöhlker, M. L., Alexander, M. L., Brito, J., Carbone, S., Castillo, P., Day, D. A., Kuang, C., Manzi, A., Ng, N. L., Sedlacek III, A. J., Souza, R., Springston, S., Watson, T., Pöhlker, C., Pöschl, U., Andreae, M. O., Artaxo, P., Jimenez, J. L., Martin, S. T., and Wang, J.: CCN activity and organic hygroscopicity of aerosols downwind of an urban region in central Amazonia: seasonal and diel variations and impact of anthropogenic emissions, *Atmos. Chem. Phys.*, 17, 11779–11801, <https://doi.org/10.5194/acp-17-11779-2017>, 2017.
- 465 Wang, Z., Su, H., Wang, X., Ma, N., Wiedensohler, A., Pöschl, U., and Cheng, Y.: Scanning supersaturation condensation particle counter applied as a nano-CCN counter for size-resolved analysis of the hygroscopicity and chemical composition of nanoparticles, *Atmos. Meas. Tech.*, 8, 2161–2172, <https://doi.org/10.5194/amt-8-2161-2015>, 2015.
- Wex, H., Petters, M. D., Carrico, C. M., Hallbauer, E., Massling, A., McMeeking, G. R., Poulain, L., Wu, Z., Kreidenweis, S. M., and Stratmann, F.: Towards closing the gap between hygroscopic growth and activation for secondary organic aerosol: Part 1 – Evidence from measurements, *Atmos. Chem. Phys.*, 9, 3987–3997, doi:10.5194/acp-9-3987-2009, 2009.
- 470 Wiedensohler, A. (1988). An Approximation of the Bipolar Charge-Distribution for Particles in the Sub-Micron Size Range, *J. Aerosol Sci.* 19(3):387–389.
- Zhao, D. F., Buchholz, A., Kortner, B., Schlag, P., Rubach, F., Kiendler-Scharr, A., Tillmann, R., Wahner, A., Flores, J. M., Rudich, Y., Watne, Å. K., Hallquist, M., Wildt, J., and Mentel, T. F.: Size-dependent hygroscopicity parameter ( $\kappa$ ) and chemical composition of secondary organic cloud condensation nuclei, *Geophys. Res. Lett.*, 42, 10920–10928, <https://doi.org/10.1002/2015GL066497>, 2015



### Appendix A: Newly designed diffusive inlet

480 The newly designed diffusive inlet is comprised of the main body (**101**) and a sheath flow straightener (**102**), as shown in Fig. A1. The main body of the diffusive inlet is constructed from the conductive material. An aerosol inlet (**103**) is placed at the center top of the main body. Downstream of the aerosol inlet has a funnel-shaped region (**105**) where the cross-section of the aerosol is smoothly expanded. The angle (**106**) of the wall of the funnel-shaped region is small enough to keep a laminar flow. The wall of the funnel-shaped region is polished to minimize air turbulence and particle deposition. The inlet of sheath air  
485 (**104**) is placed at the side of the main body. A flow straighter (**102**), located at the down-stream of the sheath air inlet, is made up of a single or double screen of fine nylon mesh to straighten the sheath flow and lead to a laminar flow. This inlet is mounted at the top of the column of the activation tube. At the lower end of the main body, there are two rubber O-rings (**107**) to keep the activation tube air-tight.



490 **Table 1. Coefficients and goodness of fit for calibration curves for three different dT conditions (dT= 10, 8, and 6 K). Three different statistical values, including Error sum of squares (SSE), coefficient of determination (R<sup>2</sup>), and root mean square error (RMSE), are used to judge the goodness of fit.**

Equation	$F(x) = a \times \text{acos}(b \times x) - c$		
dT	dT=10	dT=8	dT=6
*Coefficients (with 95% confidence bounds)	a =0.5097 (0.501, 0.5183) b =0.9912 (0.987, 0.9954) c =9.133e-13 (fixed at bound)	a =0.3895 (0.3601, 0.419) b =0.9892 (0.9635, 1.015) c =-0.005699 (-0.04233, 0.03093)	a =0.3221 (0.3013, 0.343) b =0.9722 (0.9429, 1.002) c =0.05177 (0.02362, 0.07991)
*Goodness of fit	SSE = 0.002435 R <sup>2</sup> = 0.9961 RMSE = 0.01274	SSE = 0.00135 R <sup>2</sup> = 0.9967 RMSE = 0.009187	SSE = 0.0002855 R <sup>2</sup> = 0.9987 RMSE = 0.004363

\*Coefficients and goodness of fit were calculated by MATLAB curve fitting toolbox 3.5.8.




495 **Table 2.**  $\kappa_{avg}$  from DMA-CCN and  $\kappa_{low}$ ,  $\kappa_{avg}$ , and  $\kappa_{high}$  from BS2-CCN measurement for  $dT=8$  K ( $S = 0.63\%$ ) condition for mixtures of ammonium sulfate and succinic acid.  $\kappa_{low}$ , and  $\kappa_{high}$  are derived from the range of calibration curves in Fig. 9.

	DMA-CCN		BS2-CCN	
	$\kappa_{avg}$	$\kappa_{low}$	$\kappa_{avg}$	$\kappa_{high}$
<b>AS:Su = 1:1</b>	0.176	0.168	0.186	0.200
<b>AS:Su = 3:1</b>	0.255	0.253	0.285	0.311
<b>AS:Su = 1:3</b>	0.121	0.118	0.132	0.143




500 **Table 3.** The average and standard deviation of ratio between  $\kappa$  of DMA-CCN and BS2-CCN measurement and goodness of fit for linear regression line. Three different statistical values, residual sum of squares, Pearson correlation coefficient and coefficient of determination ( $R^2$ ), are used to evaluate the goodness of fit.


	<b>F<sub>fact_low</sub></b> <b>(<math>\mu-\sigma</math>)</b>	<b>F<sub>fact_mean</sub></b> <b>(<math>\mu</math>)</b>	<b>F<sub>fact_high</sub></b> <b>(<math>\mu+\sigma</math>)</b>
<b>Ratio</b> <i>(<math>\kappa_{BS2-CCN} / \kappa_{DMA-CCN}</math>)</i>	1.17±0.17	1.05±0.12	0.98±0.10
<b>Residual Sum of Squares</b>	0.04	0.02	0.02
<b>Pearsons's r</b>	0.75	0.83	0.86
<b>R<sup>2</sup></b>	0.57	0.70	0.74

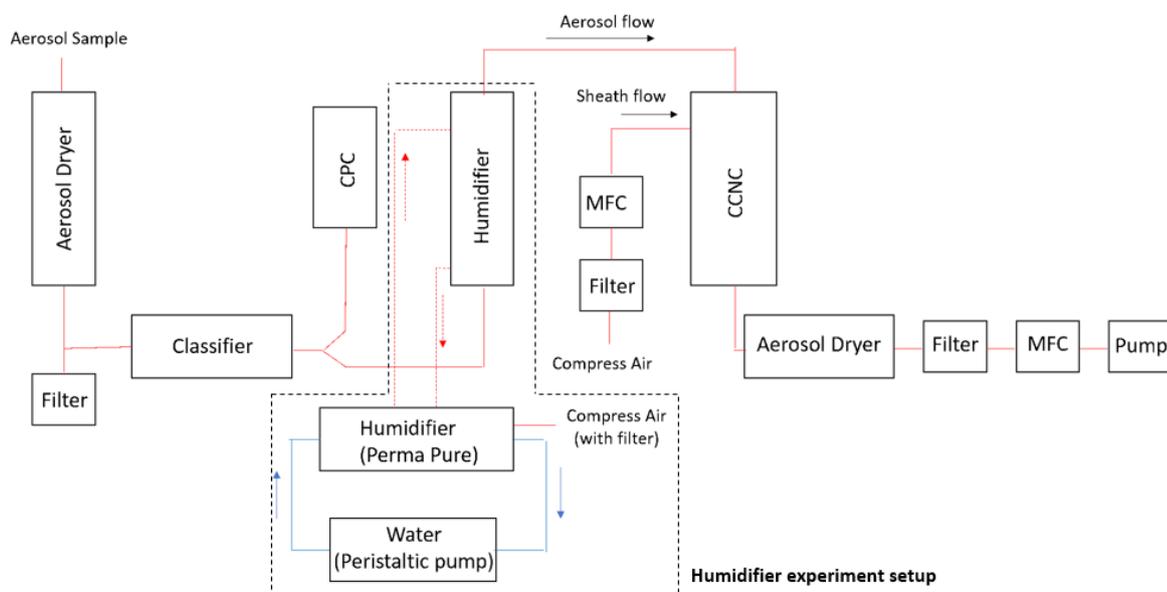


505 **Figure 1: Schematic plot of a broad scanning supersaturation cloud condensation nuclei counter (BS2-CCN) system. An additional setup marked with dashed line is for a humidifier experiment.**

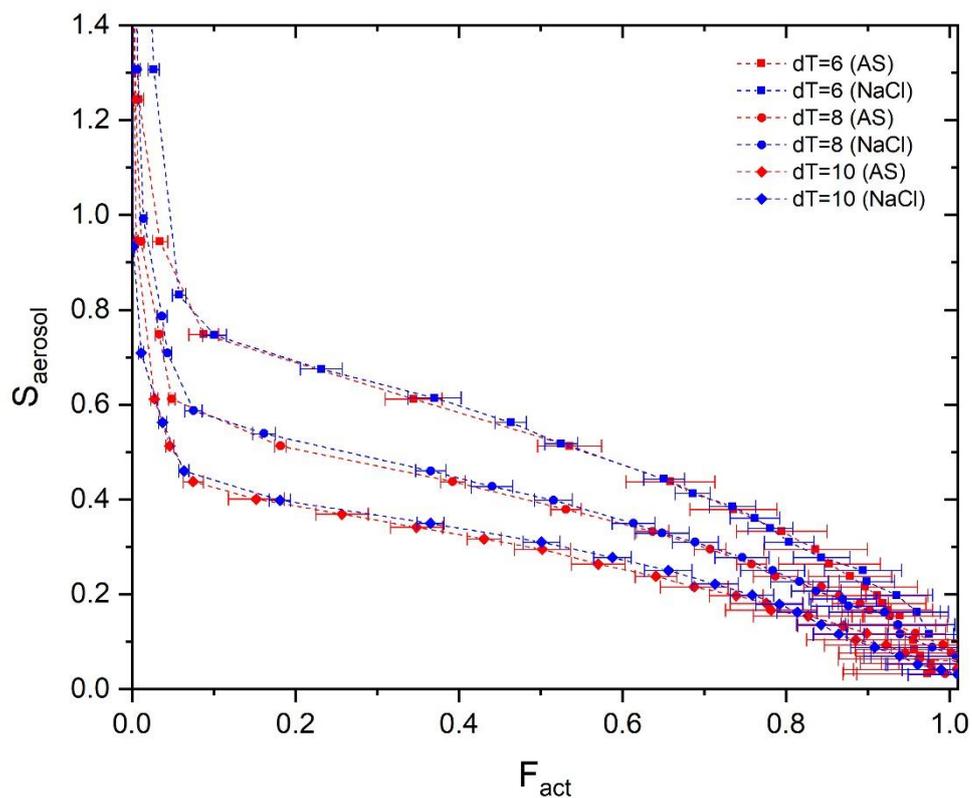


510 **Figure 2: Calibration curves ( $F_{act} - S_{aerosol}$ ) for three different T gradients ( $dT = 6, 8,$  and  $10$  K) with ammonium sulfate (red) and sodium chloride (blue) particles.**

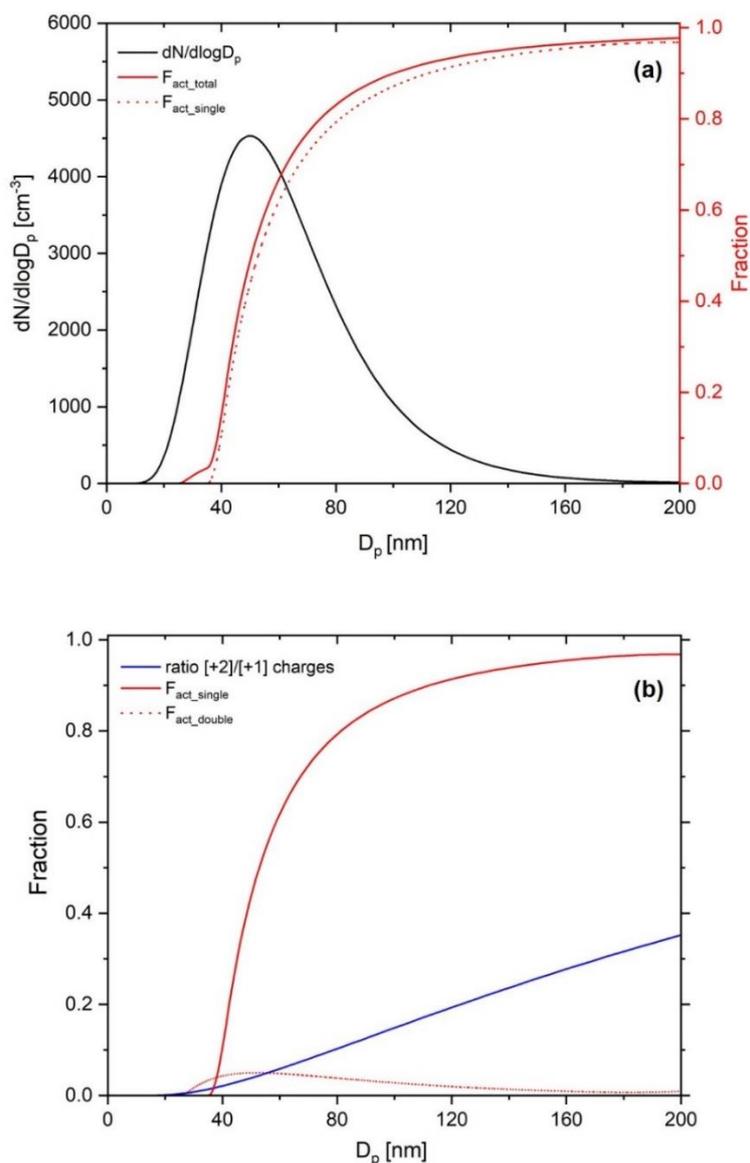

515 **Figure 3: Calculated ideal activation fraction for log-normally distributed, charge-equilibrated particles transmitted BS2-CCNC system. Shown are (a) assumed log-normal particle size distribution (black solid line, left ordinate,  $N = 2000 \text{ cm}^{-3}$ ,  $D_g = 50 \text{ nm}$ , and  $\sigma_g = 1.4$ ), total activation fraction (red solid line), activation fractions by singly charged particles (red dashed line) and (b) activation fraction by singly charged particle (red solid line) and doubly charged particles (red dashed line), and the ratio of [+2]/[+1] charges (blue solid line), which refers to  $f(D, n = +2)/f(D, n = +1)$  with mobility diameter at charge equilibrium.  $f(D, n)$  is the fraction of particle carrying  $n$  charges at charge equilibrium by Wiedensohler (1988).**

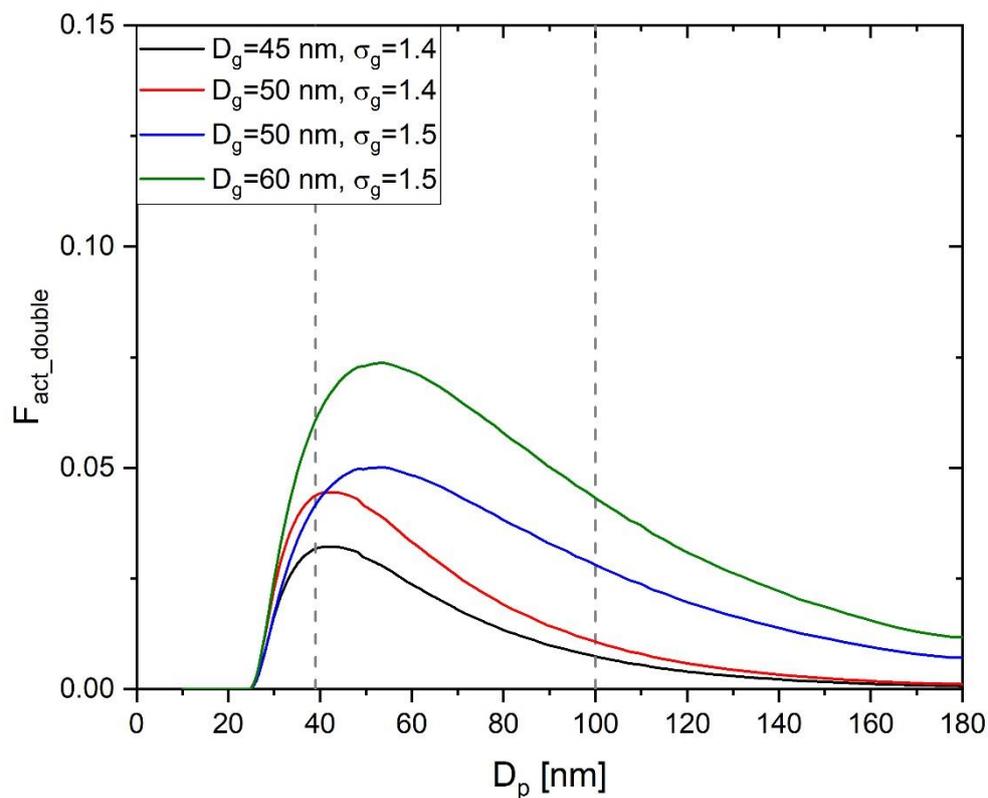

520 **Figure 4: Activation fractions by doubly charged particles ( $F_{act\_double}$ ) for variant particle size distributions. Information of each particle size distribution is presented in the legend of the figure.**

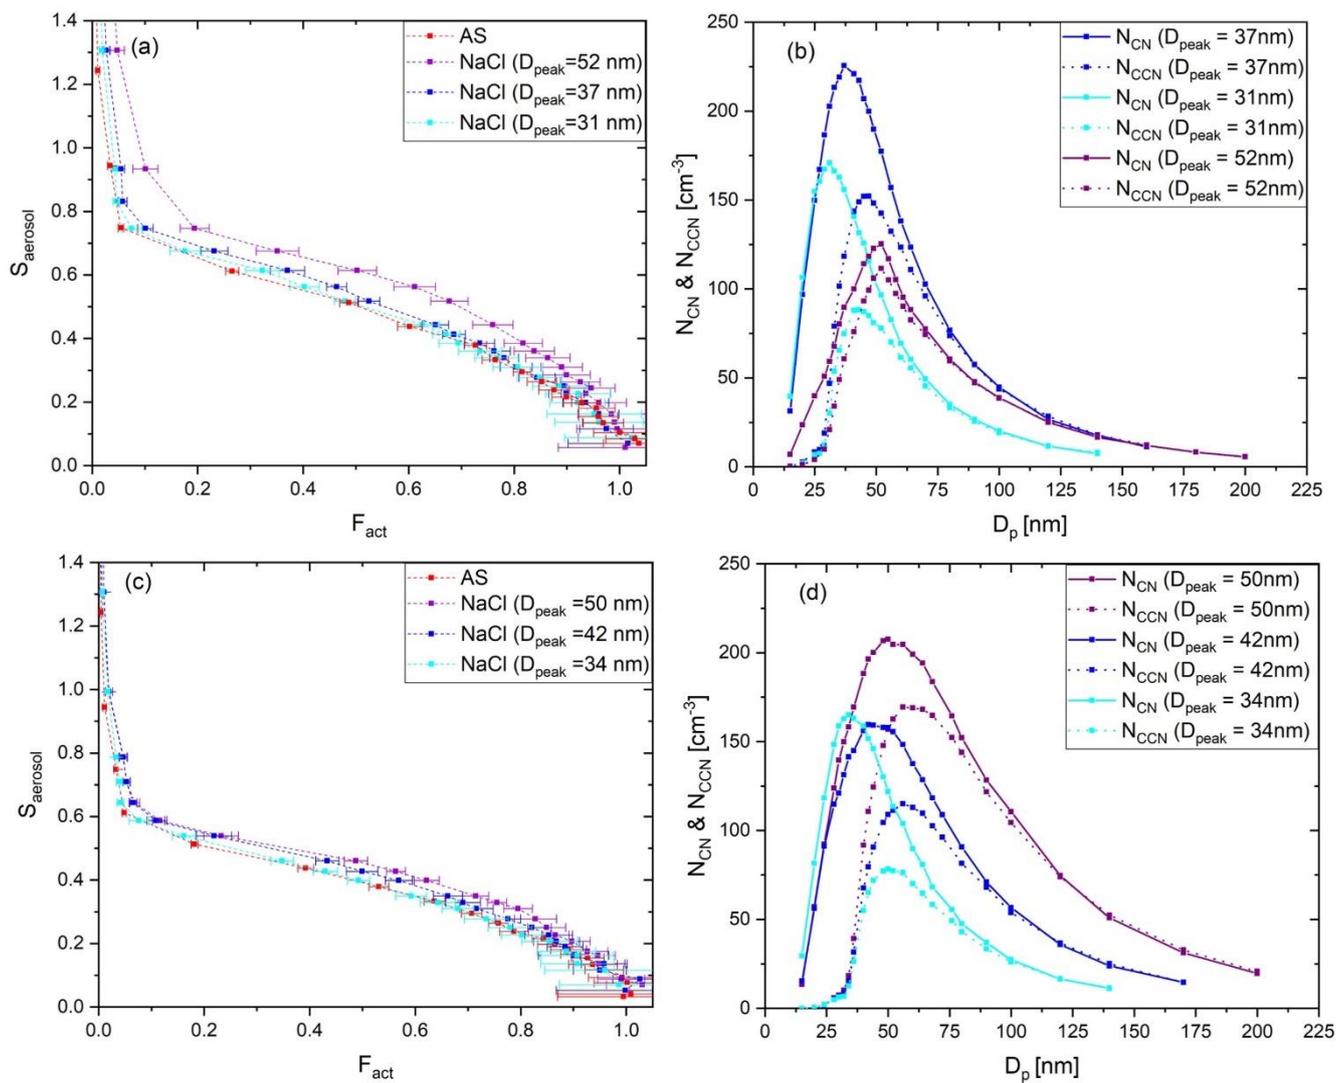

525 **Figure 5: Calibration curves of ammonium sulfate and sodium chloride for (a)  $dT=10$  K and (c)  $dT=8$  K and number size distribution of  $N_{\text{CN}}$  and  $N_{\text{CCN}}$  for sodium chloride particle for (b)  $dT=10$  K and (d)  $dT=8$  K.**

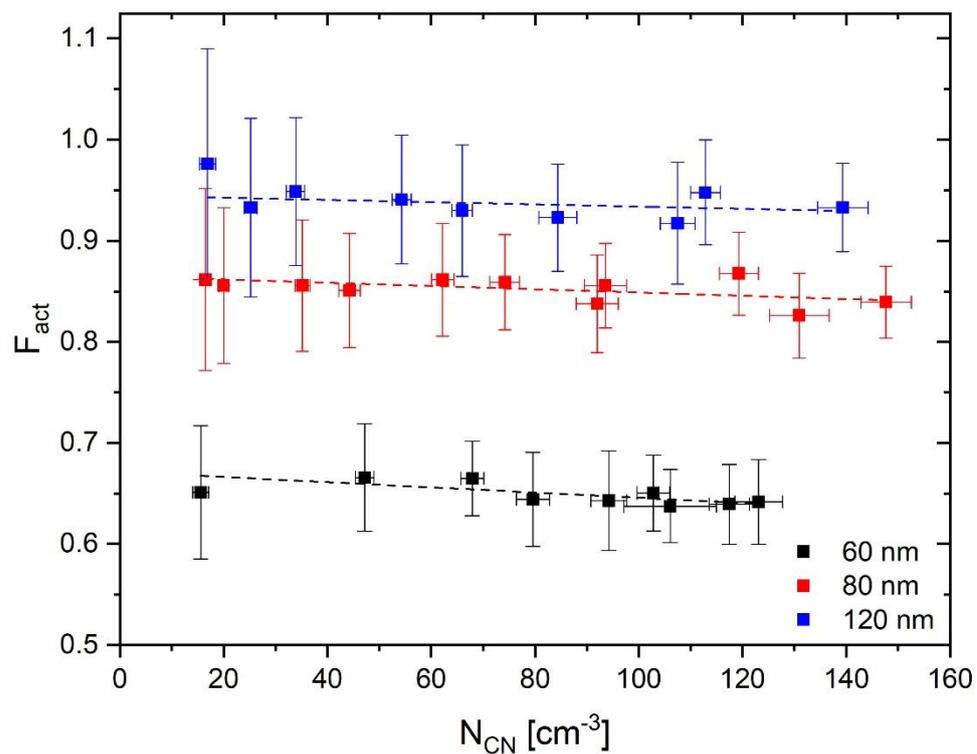
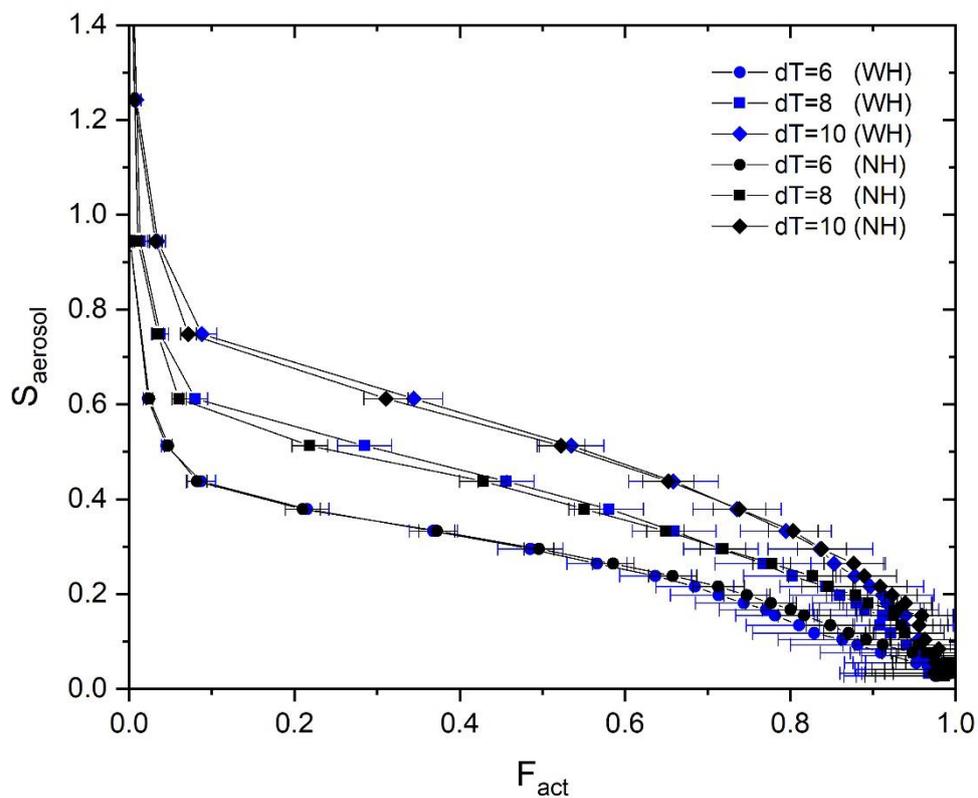
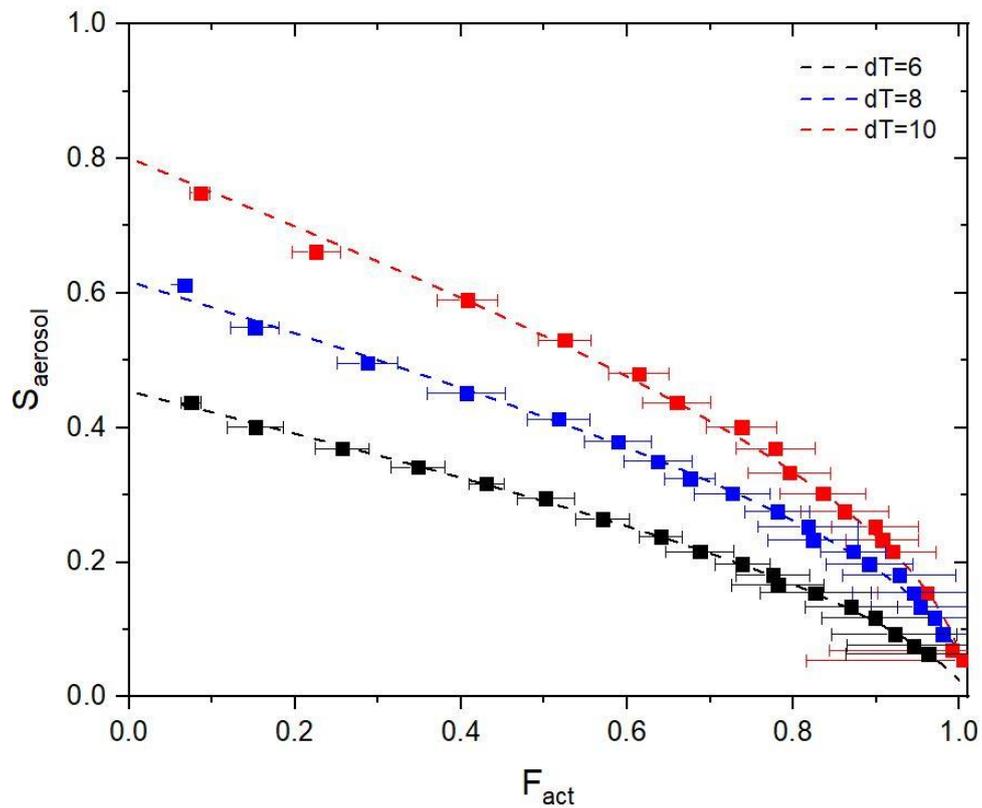


Figure 6: Average and standard deviation (error bar) of  $F_{act}$  depending on the number concentration  $N_{CN}$  for 60 nm (black), 80 nm (red) and 120 nm (blue) of ammonium sulfate particle under the  $dT=7.7$  K (0.6% S) condition. Dashed lines indicate linear regression lines.


530



**Figure 7:** Calibration curves ( $F_{act} - S_{aerosol}$ ) for three different T gradients (dT = 6 (circle), 8 (square), and 10 (diamond) K) with humidifier system (WH) and without humidifier system (NH).




**Figure 8: Experimental data (square dot with error bar) and fitting curves (dashed lines) for three different  $dT$  conditions ( $dT = 6$  (black), 8 (blue), and 10 K (red)). Ammonium sulfate particles are used for calibration.**

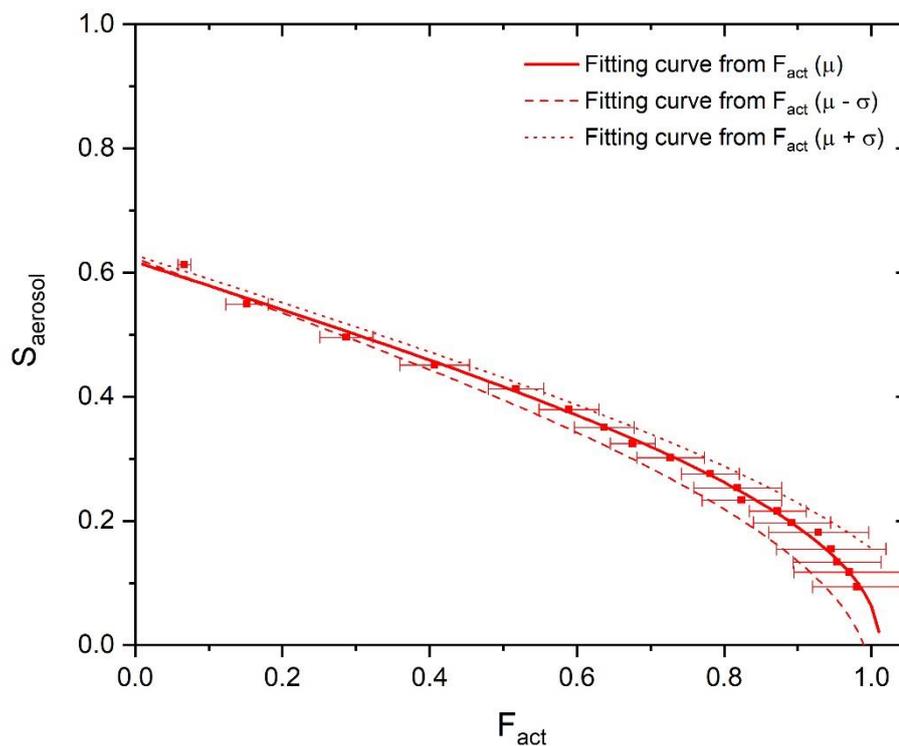


540

**Figure 9:** Experimental data point (square dot with error bar) and fitting curves for  $dT=8$  K ( $S=0.63\%$ ) condition. Solid line is obtained from data of  $F_{act}(\mu)$ . Dotted and dashed fitted line are obtained from data of  $F_{act\_high}(\mu + \sigma)$  and  $F_{act\_low}(\mu - \sigma)$ .  $\mu$  and  $\sigma$  indicate average and standard deviation of  $F_{act}$ , respectively.

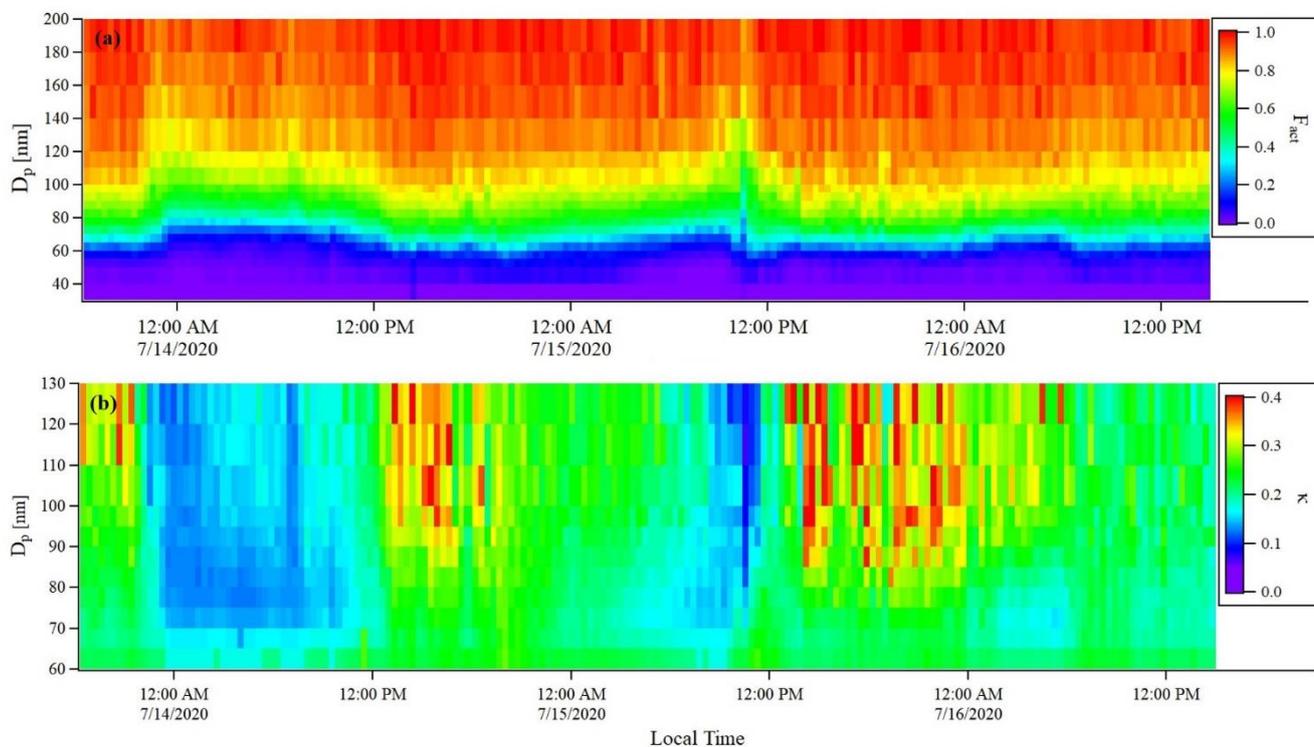


545

**Figure 10: Time series of (a)  $F_{act}$  and (b)  $\kappa$  distribution of BS2-CCN measurement for 0.63% S ( $dT=8$  K) condition. Measurement period was 13 July – 16 July 2020.**

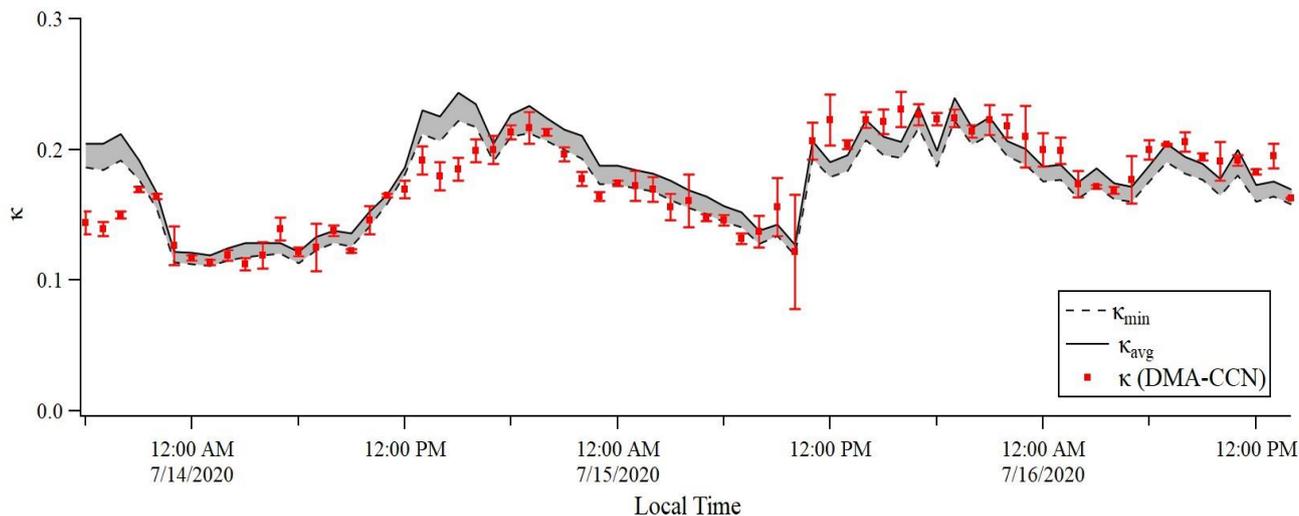


550 **Figure 11:** Time series of hourly averaged  $\kappa$  values for DMA-CCN (red dots, bar indicates the standard deviation of  $\kappa$ ) and BS2-CCN (grey shaded area for the range between  $\kappa_{avg}$  (black solid line) and  $\kappa_{low}$  (black dashed line)) measurements. The  $\kappa_{high}$  is excluded in this figure.

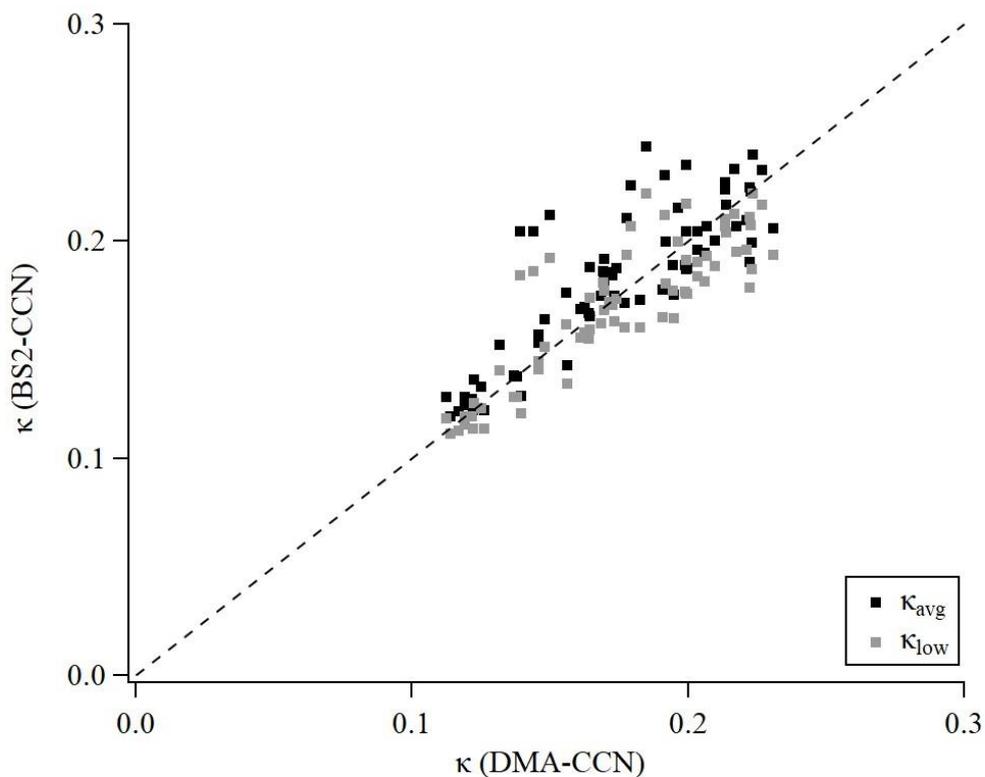

555 **Figure 12:** Scatterplot of  $\kappa$  between DMA-CCN and BS-CCN measurement. Black square and grey square dots indicate  $\kappa_{avg}$  (calculated from the calibration curve of  $F_{act}(\mu)$ ) and  $\kappa_{low}$  (calculated from the calibration curve of  $F_{act\_high}(\mu + \sigma)$ ) for the BS2-CCN measurement, respectively. The  $\kappa$  value of BS2-CCN measurement was selected for that in the diameter adjacent to the critical diameter of DMA-CCN measurement for the comparison. The black dashed line is a 1:1 line for clarity.



560

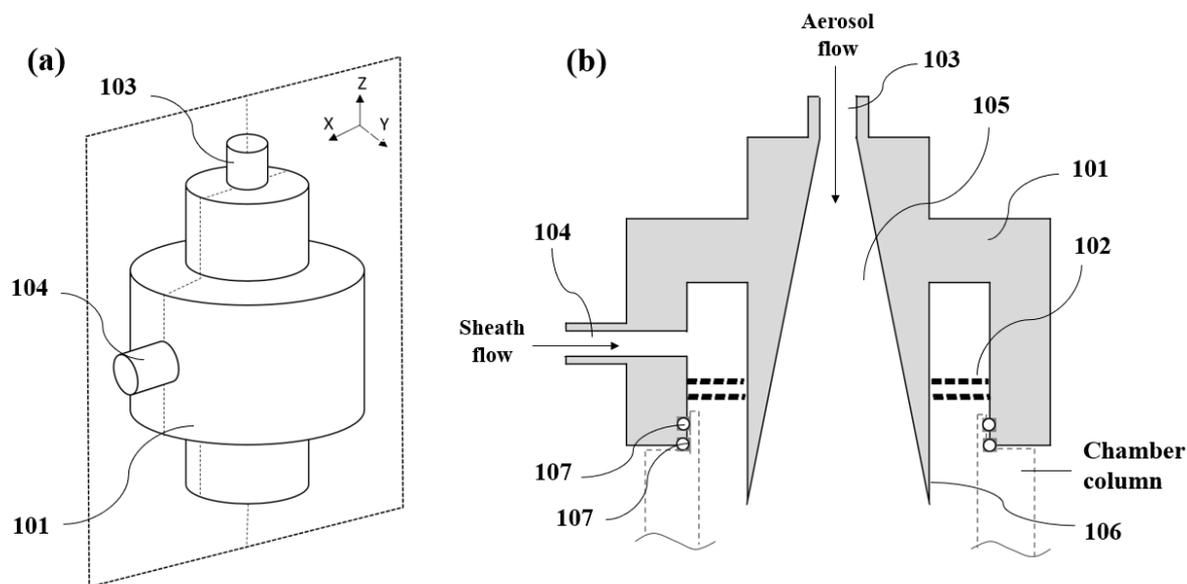

565

**Figure A1:** (a) Front perspective view of an embodiment of the diffusive inlet. (b) Longitudinal sectional (the cross section in X-Z surface) view of Fig.A1 (a). Each of numbers in the figure is as follows: main body (101), a sheath flow straightener (102), an aerosol inlet (103), a funnel-shaped region (105) where the cross-section of the aerosol is smoothly expanded, the angle (106) of the wall of the funnel-shaped region, the inlet of sheath air (104) at the side of the main body and two rubber O-rings (107) at the lower end of the main body to keep the activation tube air-tight.