The Aerosol Research Observation Station (AEROS)

Karin Ardon-Dryer¹, Mary C. Kelley¹, Xia Xueting^{1*}, and Yuval Dryer¹

1. Department of Geosciences, Atmospheric Science Group, Texas Tech University, TX * Now at Department of Statistics, Ohio State University, Columbus, OH, USA

5 Correspondence to: Karin Ardon-Dryer (Karin.ardon-dryer@ttu.edu)

Abstract. Information on atmospheric particles' concentration and sizes are important for environmental and human health reasons. Air quality monitor stations (AQMSs) for measuring Particulate Matter (PM) concentrations are found across the United States, but only three AQMSs measure $PM_{2.5}$ concentrations (mass of particles with an aerodynamic diameter of <2.5 µm) in the Southern High Plains of -West Texas (area $\ge 1.8 \times 10^5$ km²). This area is prone to many dust events (~21 per year), yet no information is available on other PM sizes, total particle <u>number</u> concentration, or size distribution during these events. The Aerosol Research Observation Station (AEROS) was designed to continuously measure these particles' (mass and number) concentrations using three optical particle sensors (Grimm 11-D, OPS, and DustTrak) to better understand the impact of dust events on local air quality. The AEROS aerosol measurements unit features a temperature-controlled shed with a dedicated inlet and custom-built dryer for each of the three aerosol instruments used. This article provides a description of

- 15 AEROS as well as an intercomparison of the different instruments using laboratory and atmospheric particles, which shows that the instruments used provided <u>a</u> similar <u>range</u> (within a factor of 3) of mass and number concentration measurements. <u>Grimm 11-D and OPS show compatibility for comparison of number concentration and size distribution, and agreement in PM₁₀ concentrations (mass of particles with an aerodynamic diameter of <10 µm). Overall Grimm 11-D and DustTrak had a good agreement in mass concentration, comparison using laboratory particles was better than that with atmospheric particles.</u>
- 20 <u>Overall, DustTrak measured lower mass concentrations compared to Grimm 11-D for larger particle sizes, and higher mass</u> <u>concentrations for lower PM sizes.</u> Measurement with AEROS can distinguish between various pollution events (natural dust <u>events</u> vs anthropogenic-haze) <u>based on their mass concentration and size distribution which will help</u> to improve knowledge of the air quality in this region.

1. Introduction

10

25 Particulate matter (PM) comprises microscopic solid and liquid particles suspended in the atmosphere, which can be generated by anthropogenic or natural sources. PM is categorized by the size of the particle, with PM₁₀ representing <u>a mass of particles</u> with an aerodynamic diameter of up to 10 μm₂₅ and PM₄, PM_{2.5}, and PM₁ representing <u>a mass of particles</u> with an aerodynamic diameter of up to 4, 2.5, and 1 μm, respectively. <u>In general, PM measurements define as measurements where 50% of the</u> <u>particles with the defined diameter (e.g., PM_{2.5}) will pass through a size-selective inlet.</u> Smaller PMs can stay in the atmosphere

- 30 for a long time and travel far from their source. PM in the atmosphere determines air quality levels and has been found to degrade human health (World Health Organization, 2016; Shiraiwa et al., 2017). The health impact is associated with particles smaller than PM₁₀, as particles ranging from 5 to 10 μm can settle in the upper respiratory system when inhaled, and smaller particles, such as PM_{2.5}, can penetrate deep into the lungs (Ling and van Eeden, 2009; Goudie, 2014). The latter has been identified as a leading contributor to the global burden of disease (Cohen et al., 2017; Lim et al., 2012).
- 35

40

45

In the United States_(US), the Environmental Protection Agency (EPA)_uses air quality monitoring stations (AQMSs) to monitors ambient PM₁₀ and PM_{2.5} as hourly and daily average mass_concentrations, but these stations generally have sparse geographic coverage, are-located in fixed sites (mainly in large population centerscentres) and are lacking in smaller cities and underdeveloped regions. Additional monitoring networks provide information on PM_{2.5} and PM₁₀ in the US, including the Interagency Monitoring of Protected Visual Environments (IMPROVE) network, which provides an additional 150 remote and rural sites nationwide, but the PM_{2.5} and PM₁₀ samples are collected only every third day and provide only daily values (Prenni et al., 2019). The EPA Chemical Speciation Monitoring Network (CSN) provides information on PM_{2.5} and the chemical composition of ambient fine particles across 150 US urban sites (Solomon et al., 2014; EPA, 2022). The Surface PARTiculate mAtter Network (SPARTAN) also provides information on PM_{2.5} and PM₁₀ concentrations, but it has only two sites in the US and none in the south-central part of the country (Snider et al., 2015). Low-cost sensors, such as PurpleAir, are also increasingly used across the US, but their efficiency is still under investigation (Ardon-Dryer et al., 2020; Barkjohn et al., 2021). None of the monitoring units mentioned above provides information on total particle number concentrations or particle size distribution. The National Oceanic and Atmospheric Administration Earth System Research Laboratory (NOAA/ESRL)

Federated Aerosol Network provides this information, but it is stretched very thin, with only a few units across the US 50 (Andrews et al., 2019).

Most of these monitoring methods are not affordable, with prices ranging from \$50,000 to \$250,000, but newer methods based on optical particle sensors are becoming increasingly popular. These sensors rely on the principle of single-particle elastic light scattering following Mie scattering theory, which enables determining the size and number of particles within a unit volume of air (Masic et al., 2020). While some of these low-cost sensors (prices lower than \$500) <u>are gaining popularity</u>, their efficiency and accuracy compared to reference sensors are still in doubt (Masic et al., 2020; Ardon-Dryer et al., 2020). Midprice optical particle sensors (\$10,000 – \$20,000) have the advantage of a slightly more affordable price (than those of reference units) as well as better accuracy than the low-cost units. Among the advantages of these units, they can provide various types of measurement; for example, the Grimm 11-D (Grimm Aerosol Technik GmbH & Co. KG, Germany; Grimm

60 11-D, 2021) provides information on total particle <u>number</u> concentration and size distribution as well as information on <u>mass</u> concentrations of various PMs. Some of these units can provide information on multiple mass fractions of PM simultaneously, which is an advantage to the gravimetric system which provides the <u>mass</u> concentration of only a single fraction (Masic et al., 2020). Several studies have found mid-price optical particle sensors to be comparable to high-priced reference units as long as

65 al., 2018; Vasilatou et al., 2021).

The Southern High Plains in West Texas host <u>a</u> few of thes<u>e reference</u> monitoring methods. The West Texas region (an area larger than 1.8×10^5 km²) has only a few, widespread AQMSs operated by the Texas Commission on Environmental Quality (TCEQ) (TCEQ, 2021) which measure only PM_{2.5} concentrations and provide no information on other PM sizes, total particle <u>number</u> concentrations, or size distribution. While the air quality in this region is considered good overall (Kelley et al., 2020), the region experiences many dust events (~21 per year) that reduce the air quality (Kelley and Ardon-Dryer, 2021). Therefore, routine_± and long-term measurements are required for comprehensive monitoring of diverse pollution events in this region, including dust events (Tong et al., 2012; Mahowald et al., 2014), so-therefore, there is a need to monitor particle mass

concentrations (of various PM sizes) and size distribution to understand how they change under distinct metrological and pollution conditions. The Aerosol Research Observation Station (AEROS) was designed to address this need. This article provides information on each of its aerosol instruments and compares the units using standard particles in the laboratory as well as atmospheric measurements. Examples of aerosol measurements in various atmospheric conditions are presented to highlight AEROS's acuity in distinguishing between anthropogenic and natural pollution events.

2. Research Area and Measurement Station

80 2.1 Research Area

70


Measurements were taken in Lubbock, Texas₁ located in the Southern High Plains of West Texas (Fig. 1). This area is rural, flat, and approximately 1 km above sea level, with an urban area surrounded by extensive agriculture fields, including cotton (30% of national production) and cattle. It is a semi-arid environment with an average annual rainfall of 463 mm from 2000 through 2019, while the average annual rainfall for the same period in the US was 789 mm (Jaganmohan, 2021). The bare soil,

85 low soil moisture, and strong winds typical of this region are important factors in dust formation (Stout, 1989). Several studies have found that this area is among the most prominent regions of dust events in the US (Orgill and Sehmel, 1976; Deane and Gutmann, 2003).

2.2. AEROS

AEROS was installed 9.8 m above the ground on the rooftop of the Electrical Engineering building at Texas Tech University 90 (33°35'12.5"N 101°52'31.3"W; Fig. 1). AEROS's design followed World Meteorology Organization Global Atmosphere Watch (WMO/GAW) aerosol measurement procedures, guidelines, and recommendations (WMO, 2016). It includes two units: an aerosol measurements unit and Harvard Impactor (HI) filter sampler unit.

- 95 The <u>HI</u> filter sampler unit has two setups with three HI units in each (Fig. 1). The HI units collect daily <u>gravimetric</u> PM_{2.5} and PM₁₀ particles on filters substrate (Marple et al., 1987) in 24-hour cycles (midnight to midnight). The HIs are designed to sample particles of 2.5 µm and 10 µm at flow rates of 16.7 and 10.0 <u>liters perL</u> min⁻¹, respectively, using impactor stages in series with polyurethane foam (PUF) impaction substrates (Lee et al., 2011). The 37-mm filters are pre- and post-weighed using an electronic microbalance (XRP2U Microbalance) to provide gravimetric measurements. <u>Filter are kept in the filter</u>
- 100 room which follows U.S. EPA (EPA, 1997) regulation conditions of temperature in the range of 20-23 °C and relative humidity in the range of 30-40%. To assure filter weight post sampling will not be impacted by hysteresis effect, filters post-aerosol collections are kept in a Dry-Keeper Auto-Desiccator Cabinet for 48 hours until weight. The filter sampler unit was fully operational only after September 2019 and therefore is not discussed in this article.
- 105 The aerosol measurements unit has been operational since March 14, 2019. It includes a shed that is temperature controlled by an air conditioning unit (Pioneer inverted WAS/WYS Series) that maintains a continuous temperature of 22 °C. Four rain-protected sampling inlet units are installed at 2.9 m from the rooftop floor (1 ± 0.01 m from AEROS rooftop) to minimize influences from the surrounding area. Each rain-protected inlet unit collects total suspended particles and is connected to a stainless steel tube (0.013 m diameter; 0.5 inches). Inside the station, each stainless steel inlet tube (from the outside) is connected to a custom-built in-line dryer unit that removes condensed-phase water from the collected particles (Fig. 1). Each
- dryer is 0.5 m long and contains a 0.013 m diameter metal wire mesh screen. A Swagelok reducer connects the dryers to a 0.0064 m diameter (1/4 inch) stainless steel tube. Conductive silicone tubes connect the small stainless steel tubes to the various instruments. The average distance from the dryer to the instrument is about 0.24 m. Figure S1A provides a schematic design of the inlet to the instruments. There are no bends tubes in any part of the inlet tubes from the inlet to the instrument, and the
- entire sampling tube was kept to a minimum to minimize diffusion losses. Also, all the inlet tubes are aligned with the dryer and with the instrument to minimize particle loss. A calculation of the Reynolds number (Re) of each inlet and its instrument indicated that the aerosol flow in the inlets tubes is laminar (Re < 850). Calculation of particle loss in inlets (from rain protector to instrument) was performed using the particle loss calculator (von der Weiden et al., 2009). Calculations were made for particles in the size range of 0.25 to 41 µm (based on particle size measured by instrument), using different particle types of different density and shape factors (based values in Table 1 in Ardon-Dryer et al., 2015). Particle loss was below 5% for particles of 0.25 um and below 0.01% for particles in the size range of 1-2 um.</p>

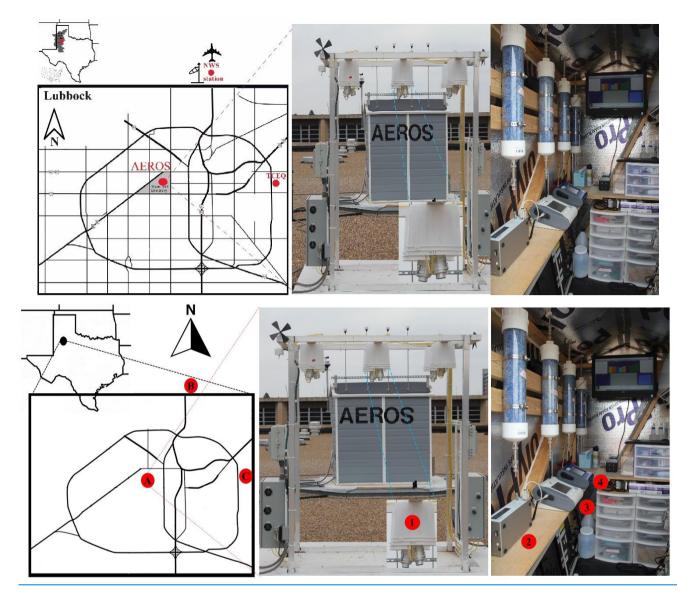

125 Figure 1. Location of AEROS (A) in the South High Plains of West Texas with locations of meteorological station (B) and <u>TCEQ PM_{2.5} station (C)</u>. The photos show the filter sampler unit with Harvard Impactor 4(HI:1) units and the aerosol measurements unit (outside and inside view with dryers and instruments 2-Grimm 11-D, 3-OPS, and 4-DustTrak).

2.2.1 Instruments used in the aerosol measurements unit

Each of the three inlets is connected to a separate aerosol instrument, and an additional inlet is kept available for aerosol collection using a filter holder (see Fig. 1). Three distinct particle instruments monitor PM concentrations, total particle number concentrations, and size distributions. The three instruments include TSI 3330 Optical Particle Sizer (OPS) (TSI, <u>OPS3330</u> Shoreview, MN, USA2012), a DustTrak DRX aerosol monitor (TSI 8533EP, Shoreview, MN, USA), and Grimm 11-D system

Portable Aerosol Spectrometer (Grimm Aerosol Technik GmbH & Co. KG, Germany). The three instruments are on a build shelf at the same height and at sufficient distance from one another to avoid interference (Fig. 1).

135

The OPS unit measures total particle number concentration as well as particle size distributions in 16 channels (bins) from 0.3 to 10 um. It works on the principle of optical scattering from single particles. Particles are illuminated using a laser beam shaped to a thin sheath that is focused below the inlet nozzle. As particles pass through this light sheath, they scatter light in the form of pulses that are counted and sized simultaneously. The OPS time resolution is $\frac{60 \text{ see}1}{100}$ min, with a flow rate is 1.0 L min⁻¹, which can reach a particle number concentration of up to 3,000 particle cm⁻³ with a size resolution of < 5% at 0.5 µm 140 and with measurements error of 0.001 # cm⁻³ (TSI, personal communication). There is an option to calculate total mass concentration for particles of up to 10 μ m (representing PM₁₀). The OPS is calibrated by the manufacturer using different sizes of polystyrene latex sphere particles (PSL). In the operation of the OPS, the particle density is assumed as 1 g cm⁻³, and no information on the reflective index is added, as there is very limited knowledge of the atmospheric particle chemical and 145 mineralogical composition in this region (Gill et al., 2000; 2009) and, therefore, no way to correctly capture the particles' density or refractive index, which are needed to convert the particle concentrations which are based on optical diameterconcentration to aerodynamic sizes. The OPS has been used previously in many laboratory settings (Ardon-Dryer et al., 2015; Yamada et al., 2015; Hsiao et al., 2016) and indoor experiments (Mølgaard et al., 2015; Maragkidou et al., 2018; Wang et al., 2020). Several studies that examined the performance of the OPS under diverse laboratory conditions have found 150 it to be comparable with various reference units (Ardon-Dryer et al., 2015; Vasilatou et al., 2021). To the best of our knowledge, the OPS has not previously been used for atmospheric measurements or for monitoring atmospheric dust events.

The DustTrak DRX measures aerosol mass concentrations at various sizes (PM₁, PM_{2.5}, PM₄, and PM₁₀) at a time resolution of $\frac{60 \text{ see}1}{1000}$ min, using a flow rate of 1.0 L min⁻¹. Its detection ranges from 1 to 150,000 µg em⁻³, with a mass resolution of 1 µg 155 em⁻³ (TSI Inc., 2019). Measurements are made with a diode laser wavelength of 655 nm (Wang et al., 2009). The DustTrak combines the photometric measurements of the group particles in the chamber with the optical sizing of single particles in the optical system and thus reports the concentration of various size fractions simultaneously. The unit is used with an external pump designed for continuous operation. The DustTrak is calibrated by the manufacturer using Arizona Road Dust/ISO 12103-1, and the default calibration factor ("Factory Cal") of 1.0 was used (TSI Inc., 2019). No information is provided by the 160 manufacturer on the calculation or measurements error of the DustTrak. The DustTrak DRX (and previous versions) have been widely used in numerous studies (Holstius et al., 2014; Wang et al., 2020; Javed and Guo, 2021), mainly for monitoring outdoor PM due to its sensitivity to a diverse range of aerosols, fast response time, and high temporal resolution (Rivas et al., 2017). While some studies have reported high correlations of PM values between the DustTrak and a reference method (McNamara et al., 2011; Viana et al., 2015), others have found large differences between the two (Holstius et al., 2014; Javed and Guo, 165 2021). A better comparison can be achieved when relative humidity is taken into account with the use of a dryer (Javed

and Guo, 2021).

The Grimm 11-D measures particle count and mass distribution by light scattering over the size range of 0.25 - 35.15 um in 31 predefined size channels (bins). It provides measurements of total particle number concentrations, size distribution,

170

and mass concentration (e.g., PM₁, PM_{2.5}, PM₄ and PM₁₀). Data are recorded at 1 min intervals (it is also possible to save data every 6 see). Particle mass concentration can reach up to $100,000 \,\mu g \, mg \, em^{-3}$, while number concentration can reach up to 53,000,000 # em^{-3} L⁻¹. The Grimm 11-D tolerance ranges are $\pm 3\%$ for particle concentration $\geq 500 \text{ # cm}^{-3}$, and $\pm 2 \mu \text{g m}^{-3}$ (Grimm, personal communication). The sample volume flow is automatically regulated to the set point of 1.2 L min⁻¹. The air is drawn in via a radially symmetrical suction head and directed straight into an optical measuring cell with a diode laser 175 wavelength of 655 nm (Peters et al., 2006). The signal from the scattered light is classified by size and count, and these counts are then converted to mass concentrations. These are made available through a Grimm proprietary algorithm, but the manufacturer does not share information about it, or the refractive index, density, and weighting factors used for the calculations. The Grimm 11-D is calibrated by the manufacturer using PSL particles according to ISO 21501-1, calibration factor ("Factory Cal") of 1.0 was used (Grimm 11-D, 2020). The Grimm 11-D and previous versions have been used in various 180 indoor (Mølgaard et al., 2015) and atmospheric studies (Mukherjee et al., 2017; Stavroulas et al., 2020; Masic et al., 2020),

including under dusty conditions (Jaafari et al., 2018). Several studies examining the performance of the Grimm 11-D unit under diverse atmospheric and laboratory conditions have found it to be comparable to various reference units (Masic et al., 2020; Vasilatou et al., 2021). For example, Masic et al. (2020) found that it performed well under diverse atmospheric and pollution conditions; when equipped with a dryer, it performed at a level comparable to that of a reference unit (a beta-Beta 185 attenuation Attenuation monitor).

The three instruments used in AEROS (Grimm 11-D, OPS, and DustTrak) have been found to perform similarly to reference instruments (Viana et al., 2015; Masic et al., 2020; Vasilatou et al., 2021) and to one another (Crilley et al., 2018; Wang et al., 2020); some studies have even used them as reference instruments (Mølgaard et al., 2015; Crilley et al., 2018; 2020). The 190 rationale for using these three instruments is the overlap in measurements between them. For example, similar PM sizes are measured by the DustTrak and Grimm 11-D, and total number concentration and size distribution (at least for the size range of 0.3-10.0) are measured by both the OPS and Grimm 11-D. The usage of these three different distinct instruments as part of the AEROS aerosol measurements unit was planned to overcome times of common instrument problems, e.g., connection issues, broken units, or the need for repair. Both the Grimm 11-D and OPS are connected to a computer that saves their data, 195 while the DustTrak data are saved on the instrument. Those data were downloaded and saved every week after the silica gel replacement, the 1-min values were then calculated using a MATLAB code to determine the values based on various time intervals (e.g., 10-min, hourly, and daily average values). All instrument time was synchronized and converted to local Central

Standard Time (CST).

Each aerosol instrument is connected to a dedicated dryer to minimize the airflow passing through each dryer and to allow for longer use of each dryer (one-week duration). The dryers impede any hygroscopic growth, as the relative humidity after the dryer is low (24 ± 0.5%). The instruments and station underwent standard maintenance operations each week, including replacing the used silica gel in each dryer with freshly baked ones, cleaning each inlet and tubing, and replacing paper filters in each instrument. In addition, each instrument was examined to verify that it counted 0 particles with a clean purge zero count filter, which enabled testing for leakage. Additional zero offset calibrations were performed on the DustTrak, based on the manufacturer's advice. When no particles were detected, the freshly baked dryer was connected to each instrument with a clean filter at the inlet, and measurements of particles were performed to verify the dryer background particle level (PM, size distribution, and total number concentration). These background values were subsequently subtracted from the instruments' atmospheric measurements. The contribution of particles due to the use of the dryers was minimal; for example, the PM₁₀ particle mass concentration was 0.3 ± 0.16 µg m⁻³ (average ± standard deviation, SD values), while the <u>number concentration</u> of particles in the size range of 253 - 298 nm was 15.4 ± 8.9 # cm⁻³.

2.3. Measurements of PM_{2.5} concentration from TCEQ

215

There only reference AQMS unit in this region belongs to the TCEQ (TCEQ, 2021). This unit located 8.2 km from AEROS (Fig. 1), measures only hourly gravimetric PM_{2.5} concentrations (local conditions at local CST) using a Met One BAM-1022 Beta Attenuation Mass monitor unit. The BAM-1022 measure PM_{2.5} concentrations ranging from -15 to 10,000 μ g m⁻³ with a resolution of 0.1 μ g m⁻³ and a precision of < 2.4 μ g m⁻³ per hour. Additional information on this unit can be found in Kelley et al. (2020).

2.4. Comparison of aerosol instrumentation under laboratory and atmospheric conditions

A comparison of the three aerosol instruments was performed using known particles under controlled laboratory conditions as well as under atmospheric conditions.

2.4.1. Comparison of aerosol instrumentation using known particles in the lab

Although the three instruments were received from the manufacture<u>r</u> after factory calibration, we performed calibration tests of the OPS and Grimm 11-D using diverse monodisperse polystyrene <u>latex</u>-sphere particles (0.25, 0.5, and 0.95 μ m)- to verify their performance in identifying particle size at the corrected size bins. (data not shown). The PSL particles were wet generated

225 <u>using a Brechtel Manufacturing, Inc. (BMI) 9200 Aerosol Generator (BMI, 2022), the atomized particles entered integrated in-line dryers where they evaporated, leaving anhydrous crystalline particles before reaching OPS and Grimm 11-D.</u>

A laboratory comparison was performed using an experimental setup designed specifically for this comparison (Fig. 2). For this comparison, Arizona Test Dust (ATD) particles (Nominal 0 - 3 mm, Powder Technology Inc. <u>MN, US</u>) with 100 μm
 Bronze Beads (TSI 3400) were generated using a 3D printed dust generator (<u>PRinted FluidIZed bed gEnerator- 3D dust</u>)

generator, PRIZE; Roesch et al., 2017). The dry dust particles were suspended in the dry generator using a 4 L min⁻¹ nitrogen flow. The particles were then measured by each of the three instruments, and any excess flow not drawn into the instruments was filtered and vented to a hood. A Brechtal Y-shaped flow splitter was used to split the flow, and conductive silicone tubing carried the particles between all components to minimize particle loss to the tubing by electrostatic forces.

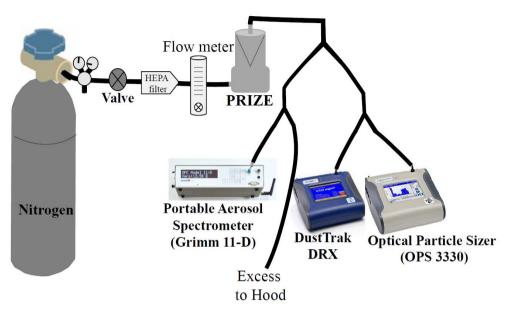


Figure 2. Experimental setup: <u>Arizona Test Dust (ATD)</u> particles were generated using <u>PRinted FluidIZed bed gEnerator- 3D</u> <u>dust generator (PRIZE)</u> and measured by the various instruments (DustTrak, OPS, and Grimm 11-D).

2.4.2. Comparison of aerosol instrumentation using atmospheric particles

- 240 Two types of atmospheric measurements were performed using the three instruments. In the first, a comparison of the aerosol instruments in AEROS was performed for 78 days from mid-March to the end of May 2019. In the second comparison, which took place in the same period, aerosol measurements by AEROS were compared to measurements taken at ground level and outside the station shed (on the rooftop).
- 245 To evaluate the similarities and differences of the three instruments (or locations), a set of calculations and comparisons was performed using MATLAB and Excel. The evaluation and comparisons were based on R-squared (R²), root-mean-square error (RMSE), and mean absolute error (MAE) values as well as the best fit information (including the slope and intercept). After the comparisons were performed, additional measurements of different meteorological and atmospheric conditions were made to observe the behavior of AEROS and examine its ability to observe diverse pollution conditions and to distinguish between
- 250 natural (e.g., dust) and anthropogenic (e.g., haze) pollution.

2.5. Meteorological measurements

Meteorological information, such as 5-min to hourly ambient temperature, relative humidity, wind speed, direction, and gust as well as visibility, pressure, and precipitation were retrieved from the local National Weather Service (NWS) Automated Surface Observation System (ASOS), available via the METeorological Aerodrome Reports (METARs) station located ~9.8

255 km northeast of AEROS (33° 39' 48.96" N, 101° 49' 22.8" W, Fig. 1). The data were retrieved from March to May 2019, and all times were converted to CST. Observations of meteorological conditions (e.g., thunderstorms, rain, haze, and dust) were retrieved for that period using the "Present Weather Code", which is provided in the METAR.

3. Results and Discussion

3.1. Laboratory intercomparison of aerosol instrumentation using ATD-known particles

260Analysis of OPS and Grimm 11-D using PSL particles was performed to identify if the instrument can detect particles at the correct sizes. Three different PSL sizes were examined, these PSL had nominal sizes of 0.25, 0.5, and 0.95 µm with a size range of 0.24-0.26, 0.48-0.52, and 0.93-0.97 nm, respectively. The results of the PSL test can be found in Fig. S2, on average 16 measurements were taken for each size and instrument. Overall, OPS and Grimm 11-D identified particles of similar sizes and concentrations. Both instruments, when examining 0.25 um particles (Fig. S2A), had the highest concentration at the 265 smallest (first) bin size, Grimm 11-D identified the 0.25 µm PSL at a bin size of 0.253 to 0.298 µm, while OPS detect the highest concentration at a bin size of 0.3 to 0.374 µm. When 0.5 µm PSL particles were examined (Fig. S2B), both units identified monodisperse distribution with a narrow maximum at the expected size range. The OPS identified the PSL at size range (bins) of 0.465 to 0.579 µm while Grimm 11-D identified most of the particles in two bins of 0.414 to 0.488 µm and 0.488 to 0.576 um, the particles examined were in the range of 0.48-0.52 um, and therefore identified in the correct detected 270sizes of Grimm 11-D. For the 0.95 µm particles (Fig. S2C), both instruments behave similarly and had bimodal distribution with two maxima, one at the smallest bin and another one at larger particle size. We suspected that this PSL solution was contaminated leading to this high concentration of small particles. OPS identified the 0.95 um particles in size bins of 0.897-1.117 µm, while Grimm 11-D identified most of the particles in bin size of 0.679 to 0.8 µm, much lower than the PSL size range. More recently, when only Grimm 11-D was used (Fig. S2D) while using a new solution of 0.95 um PSL particles. 275 Grimm 11-D identified most of the particles in two bins 0.679 to 0.8 and 0.8 to 0.943 µm, the latter was in the PSL size range yet slightly lower than size expected. The detection of particles of that size range ($\sim 1 \mu m$) at smaller sizes was observed in previous studies that used Grimm 11-D, yet it seems as if this size was in the detected size range according to ISO 21501-4 (Vasilatou et al., 2021). The behavior of the OPS came as no surprise as it was similar to previous studies that used sizeselected ammonium sulfate particles (Ardon-Drver et al., 2015).

280

<u>Arizona Test Dust</u><u>ATD</u> particles were generated and measured by each instrument every minute for 30 min. A comparison of total particle number concentration and size distribution was made between the OPS and the Grimm 11-D, while a comparison

of PM was performed between the DustTrak and Grimm 11-D. Overall, similar measurements were found between the various instruments as shown in Fig. 3. Full information on the statistics of each comparison including R², RMSE, and MAE, slope, intercepts, and the number of parallel measurements can be found in Table S1. The OPS and Grimm 11-D had a similar particle 285 size distribution in most of the overlapping particle sizes, mainly for particle sizes ranging from 0.8 µm to 9 µm. For small particle sizes (<0.8 µm), however, the Grimm 11-D measured a higher particle number concentration than the OPS (Fig. 3A). Similar values of total particle number concentration were measured by the OPS and Grimm 11-D when similar particle size ranges were used (0.3-10 μ m; Fig. 3B). A high R² value (R² - 0.97) was measured during this experiment, and no statistical 290 difference (based on one-way ANOVA) was detected between the two units. A comparison of the DustTrak and Grimm 11-D was performed using various PM sizes (Table S1 and Fig. 3C). Overall, both instruments measured similar PM concentrations, but the Grimm 11-D measured higher mass concentrations for the larger particle sizes (PM₁₀, PM₄, PM_{2.5}), while the DustTrak measured higher mass concentrations than the Grimm 11-D for the smaller PM_1 -sizes. The R² for the PM concentration comparison was high (range: 0.94.85 - 1.0, see Table S1), and there was no statistical difference between the measurements of 295 these instruments based on one-way ANOVA.

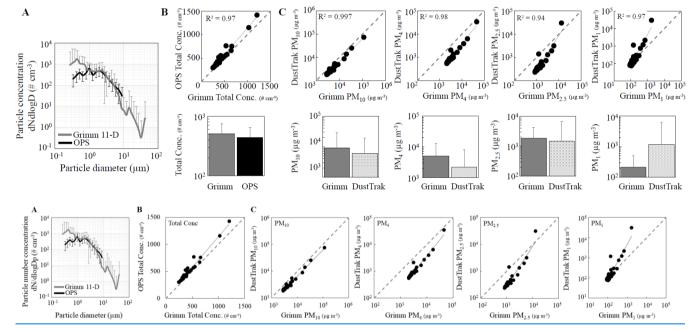


Figure 3. Comparison of the particle size distribution for optical diameter between the OPS and Grimm 11-D (A) as well as total number concentration (B), and comparison of PM concentration between the DustTrak and Grimm 11-D for PM₁₀, PM₄. $PM_{2.5}$, and $PM_1(C)$ using Arizona Test DustATD particles. Error bars represent SD values for measurement duration.


300

3.2. Intercomparison of aerosol instruments using atmospheric particles

305

310

A comparison of atmospheric measurements was performed using hourly average values measured from mid-March to the end of May 2019 (a total of 78 days). During this period, PM and total number concentration varied, as shown in Fig. 4. The <u>hourly</u> PM_{2.5} values ranged from $< 1 \mu g$ em⁻³ to more than 300 μg em⁻³, while the total number concentration ranged from 0.5 to 220 # cm⁻³. The time comparison in Fig. 4 shows that, while two instruments (OPS and Grimm 11-D) measured similar total number concentration values, the three instruments that measured PM_{2.5} values (Grimm 11-D, DustTrak, and TCEQ) had large variabilities in their PM values. The Grimm 11-D measured higher PM_{2.5} values on some days while on others, the DustTrak measured higher PM_{2.5} concentrations. For that difference, a full comparison was performed between all the instruments for diverse PM sizes as well as for the total number concentration (Fig. 5). It should be noted that during the examined period the DustTrak reported no jumps in PM concentrations or negative or 0 values under low PM concentrations (as presented in Rivas et al., 2017), perhaps due to the weekly calibration (zero offset).

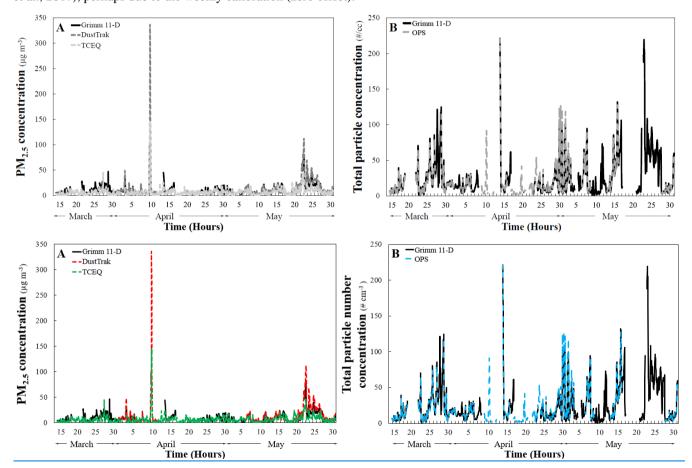

315 Figure 4. (A) Hourly values OF of PM_{2.5} from THE the Grimm 11-D (black), DustTrak (dark grayred), and TCEQ station (light graygreen) and (B) total number concentrations from THE the Grimm 11-D (black) and OPS (graylight blue) as measured during March-May 2019.

320

A comparison of atmospheric measurements was performed for PM_{10} between the Grimm 11-D and OPS (Fig. 5A). This comparison, which had 867 hours of parallel measurements, returned a high R² value (0.95) and low RSME and MAE values (3.3 and 2.1 µg em⁻³, respectively). When the PM_{10} values from the OPS were compared to those of the DustTrak (Fig. 5B), the comparison had a lower R² value (0.79) and higher RSME and MAE values (24.3 and 8.0 µg em⁻³, respectively). Although this comparison was low, previous studies have shown that the OPS and DustTrak measure similar PM_{10} values, under laboratory conditions (Wang et al., 2020)

325

The PM concentration for sizes PM₁₀, PM₄, PM_{2.5}, and PM₁ were compared between the Grimm 11-D and DustTrak; there were 671 parallel hours. The R² values ranged from 0.63 (for PM₁₀; Fig. 5C) to 0.86 (for PM_{2.5}; Fig. 5D), while the RSME values ranged from 5.3 µg em⁻³ to 10.6 µg em⁻³, and the MAE values ranged from 3.3 µg em⁻³ to 6.6 µg em⁻³. On average, the Grimm 11-D measured higher PM₁₀ and PM₄ values (9.3 ± 19.1 and 2.8 ± 8.4 µg em⁻³, respectively) than the DustTrak, similar to the results of Javed and Guo (2021), who found that the DustTrak measured lower mass_concentrations at larger particle sizes. For PM_{2.5} and PM₁, however, the DustTrak measured higher values on average (2.4 ± 6.5 and 5.3 ± 8.2 µg em⁻³, respectively) than the Grimm 11-D. These findings are similar to those of Holstius et al. (2014), who compared the DustTrak and a Grimm unit and recorded higher PM_{2.5} (Javed and Guo, 2021).

335

In a comparison of PM_{2.5} hourly values between the Grimm 11-D and DustTrak and to the local TCEQ station (Figs. 5E, 5F) the AEROS instruments (Grimm 11-D and DustTrak) measured higher PM_{2.5} values (with averages of 3.5 ± 5.5 and 6.1 ± 15.1 µg em⁻³, respectively) than those measured by the TCEQ. When PM_{2.5} values from the TCEQ were compared with those measured by the DustTrak, the comparison had a high R² value (0.8) and low RSME and MAE values (4.8 and 3.3 µg em⁻³, respectively). A lower R² value (0.55) and RSME and MAE values (3.5 and 2.5 µg em⁻³, respectively) were measured when the TCEQ values were compared with those of the Grimm 11-D. Although the overall R² values were high and the RSME and MAE values were low overall, there were differences between the units. The differing PM_{2.5} values between the TCEQ and the Grimm 11-D and DustTrak could be attributed to two causes. First, the TCEQ unit is not located near AEROS but ~8.2 km away meaning it was most likely exposed to slightly different conditions (e.g., due to its location near an agriculture field, while AEROS is located on campus in an urban setting) and therefore had different particle mass_concentrations. Second, several of the TCEQ PM_{2.5} values were below zero (down to -8 µg em⁻³), and the TCEQ zero setting is below 0 µg em⁻³, which could impact the comparison by lowering the overall TCEQ values.

A comparison of total particle number concentration between the OPS and Grimm 11-D for particles 0.3 µm to 10 µm yielded

a high R^2 value (0.98) and low RSME and MAE values (3.5 and 2.5 $\mu g \# cm^{-3}$, respectively), with a slope of 1.0 (Fig. 5I) emphasizing the compatibility of the two units. It should be noted that although overall these two instruments show high comparability a close look at the distribution of the total concentration shows a difference between the OPS and Grimm 11-D over some periods. A comparison was performed between the units based on different periods, where each period represents the time between silica gel replacement and filter change in instruments (see Fig. S3). For two out of the nine periods (for


355 <u>unknown reasons) OPS measured much higher number concentration values compared to Grimm 11-D, leading to much higher difference values between the two units (Fig. S3B) and therefore shift of the 1:1 line (Fig. 5I).</u>

Overall, \pm the OPS and Grimm 11-D are more comparable based on their total number concentration and PM₁₀ values, but the Grimm 11-D and DustTrak had high comparison values (relatively high R² values) for the diverse PM sizes, so the difference 360 was not consistent. Larger PM sizes (PM₁₀ and PM₄) were higher in the Grimm 11-D than in the DustTrak, while smaller PM sizes (PM_{2.5} and PM₁) were higher in the DustTrak than in Grimm 11-D. Some of these differences in mass concentration in the atmospheric measurements could be attributed to slight changes in the method used by each instrument for particle detection. For example, according to Wang et al. (2020), the OPS uses a more focused laser beam and a nozzle with a smaller inner diameter to sample particles compared to the one used in the DustTrak, while the DustTrak single scattering measurement 365 has a larger minimum detectable size (~0.5 um) yields more coincidence errors than the OPS. Another factor lav with the fact that the instruments are calibrated by the manufacturer using different particle types, both OPS and Grimm 11-D calibrated using PSL particles while the DustTrak is calibrated with Arizona Road Dust. Calibration using different particle types could cause different detection or reading. Previous studies indicated that optical responses of different particles may vary significantly, depending on the particles type or the pollution level (McNamara et al., 2011; Sousan et al., 2016; Masic et al., 370 2020). For example, irregular particles, like dust particles, will scatter more light which may overestimate the optical diameter of the particles (Chien et al., 2016). According to Zhang et al. (2018), the relationship between PM mass concentration and

- light scattering is strongly dependent on particle size and, to a lesser extent, on PM composition. Atmospheric particles, as the one used in this comparison, contain different types of particles which will be varied by their refractive indexes, densities, and shapes leading to slightly different interpretations by each of the instruments and to different readings (Cheng et al., 2010).
- 375 Since there is very limited information about the atmospheric particle chemical and mineralogical composition in this region no correction (e.g., different refractive indexes, densities values) could be made, and instruments were used as default from the manufacture with manufacture correction factors.

380

Some of these differences could be attributed to slight changes in the method each instrument uses to detect the particles. Unlike when defined ATD particles are used, atmospheric particles vary in size, shape, and density, which may be interpreted slightly differently by each of the three instruments' optical methods, leading to slightly different PM readings.

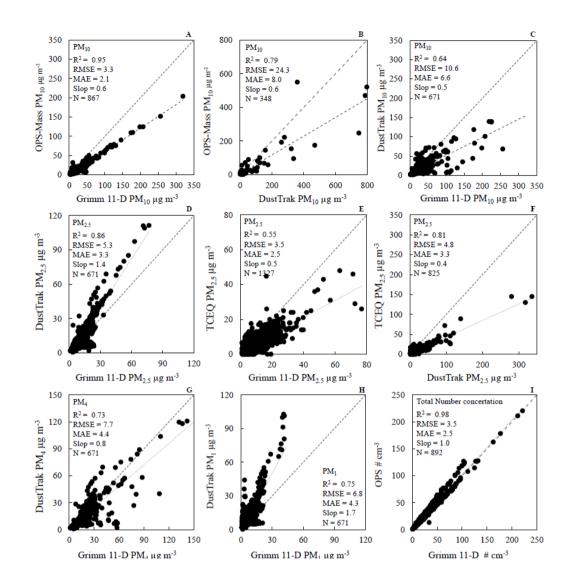

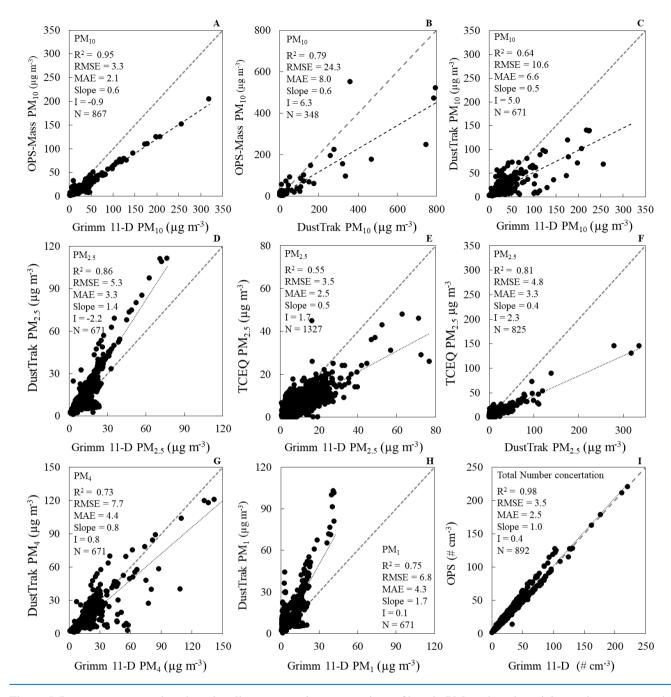


Figure 5. Instrument comparison based on linear regression, comparison of hourly PM, and total particle number concentration values as measured by the Grimm 11-D, OPS, DustTrak, and TCEQ. Dashed gray lines represent a 1:1 line. The statistics of each case include the R², RMSE, and MAE, as well as the slope, intercepts (I), and N, which represent the number of parallel measurement points. Shown are comparisons of the Grimm 11-D and OPS (A) and Grimm 11-D and DustTrak (B) for PM₁₀

and between the OPS and DustTrak for PM_{10} (C). The Grimm 11-D and DustTrak (A) and Grimm 11-D and TCEQ (B) for $PM_{2.5}$, and between TCEQ and DustTrak for $PM_{2.5}$ (E). Comparison between the Grimm 11-D and DustTrak for PM_4 (G) and PM_1 (H), and between Grimm 11-D and OPS for total particle number concentration (I).

390

395

400

3.3. Comparison of aerosol-particle concentration based on different locations

A comparison of <u>aerosol-particle</u> concentration (mass and number) based on instrument location was performed (using identical rental units). For this comparison, one Grimm 11-D unit was located in AEROS, while the second (rental) unit was located outside the shed on the rooftop floor. One DustTrak and one OPS unit were kept in AEROS, while two other (rental) units were located on the ground floor. Each measurement in each location was taken every 1-min for 1-hour. The instruments in AEROS used the sampling design and inlet length described in Section 2.2 and shown in Fig. 1, while the units at the two other locations (rooftop and ground floor) were used as is, without a dryer or inlet. These comparisons were taken under atmospheric conditions with a temperature of 26 ± 5.4 °C and relative humidity of 48.9 ± 16.7 % (as measured by the NWS station). The measurements were taken under conditions of a temperature of 26 ± 5.4 °C and relative humidity of 48.9 ± 16.7 % (as measured by the NWS station). The measurements were taken under conditions of a temperature of 26 ± 5.4 °C and relative humidity of 48.9 ± 16.7 % (as measured by the NWS station). The measurements pair (near each other) showed that both units measured similar overall particle


concentrations (number and mass, (data not shown).

Overall, similar particle concentrations were found at all three locations (Fig. 6). The average particle size distribution measured in AEROS, when compared to those taken on the rooftop floor (using the Grimm 11-D; (Fig. 6A)) showed similar

- 405 number concentrations for all particle sizes. For the comparison between measured in AEROS and the ground floor using OPS (Fig. 6B), we found higher particle number concentration in size range of 0.3 to 2 μ m (with difference up to 350 # cm⁻³ for 0.3 μ m) at the ground level. The measurements at the ground floor were higher most likely due to people walking near the instruments and kicking particles from the sidewalk, and the fact the ground sampling location was near a parking lot that was active during the sampling period.- or the ground floor (using OPS; Fig. 6B), showed similar concentrations for particles ≥ 0.5
- 410 μ m. For particles $\leq 0.5 \mu$ m, measurements at the ground floor were higher (up to 350 # cm⁻³), most likely due to people walking near the instruments and kicking particles from the sidewalk that were detected by the OPS instrument. Although higher number concentrations were measured at the ground, the comparison between the two OPS measurements (in the AEROS shed and on the ground floor) had a high R² value (0.99) and low RMSE and MAE values (0.8 and 0.6 # cm⁻³, respectively). The difference between the two Grimm 11-D measurements (in the AEROS shed and on the rooftop floor) also had a good
- 415 comparison, with a high R^2 value (0.99) but with slightly higher RMSE and MAE values (7.7 and 3.4 # cm⁻³, respectively).

Similar measurements were obtained for PM concentration using the Grimm 11-D and DustTrak in different locations. The PM concentration measured using the Grimm 11-D in the AEROS shed were slightly higher (with an average of $2.3 \pm 1.3 \mu g$ m⁻³ for all PM sizes) than the measurements taken on the rooftop floor (Fig. 6C), while the measurements with the DustTrak

420 at ground level were also slightly higher (an average of $1.3 \pm 1.1 \,\mu g \,m^{-3}$ for all PM sizes) than those measured in the AEROS shed (Fig. 6D). Although there were differences in PM concentrations, these were relatively small-(1.3 - 2.3 $\mu g \,m^{-3}$) and within the range of difference found between the two instruments when they were measured at the same location and timebetween the two instruments. In addition, in both cases, the RMSE and MAE were relatively low (≤ 1.8 and $1.2 \,\mu g \,m^{-3}$, respectively). There was no statistical difference (based on one-way ANOVA) between the measurements from these locations (in the 425 AEROS shed vs. the rooftop floor and-or the ground floor). Overall, this comparison showed that measurements using AEROS (with the current setup in the shed) reflect measurements at ground level, at least for the condition tested. It is possible to assume that different meteorological and atmospheric conditions would cause some differences.

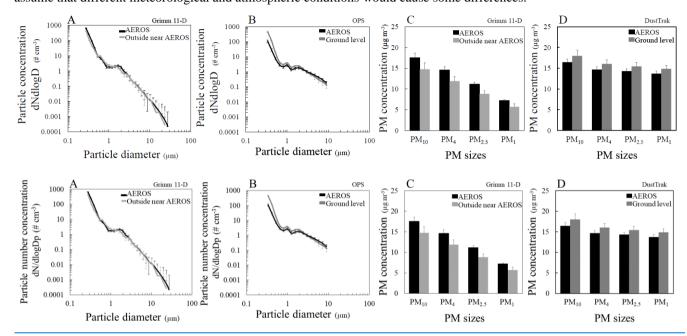

- 430 Figure 6. Comparison of measurements taken in the AEROS shed with measurements taken on the ground level or on the rooftop floor outside the AEROS shed. (A) Particle size distribution <u>(optical diameter)</u> measured by the Grimm 11-D unit in the AEROS shed (black) and outside on the rooftop floor (light gray). (B) Particle size distribution <u>(optical diameter)</u> measured by the OPS in AEROS (black) and <u>ON-on</u> the ground floor (dark gray). (C) PM concentration at various sizes as measured by the Grimm 11-D unit in AEROS (black) and outside AEROS on the rooftop floor (gray). (D) PM concentration at various sizes
- 435 as measured by DustTrak in AEROS (black) and on the ground floor (dark gray). Error bars represent SD values of the measured period.

3.4. Observation and identification of different pollution events (anthropogenic vs. natural)

Observations using AEROS's aerosol instruments were used to distinguish between different pollution events attributed to anthropogenic causes (haze) or natural causes (dust events). Ideally, the identification of particle chemistry confirms the type of particles, but that was impossible at the time of the measurements, so observations of particle concentrations (total number and <u>PM-mass</u> concentrations) and particle size distribution were used to distinguish between these different events. It is expected that pollution events will have high emissions of particles with a high particle concentration, as an anthropogenic event has more small particles than a natural event (e.g., dust), which has larger particles (Kulkarni et al., 2011).

445

470

Observations of anthropogenic and natural events were made on March 28 - 30, 2019, when two haze events and one dust event were captured. Figure 7 presents the total number concentrations, PM mass concentrations, and size distribution at these times. During the morning hours of March 28, the local NWS reported a haze event. The visibility (based on measurements taken from the meteorological station) decreased from 16 to 8 km (from 5:00 to 10:00). At 10:00, the hourly average value based on total particle number concentration was $122.5 \pm 14.1 \, \text{# cm}^{-3}$ (Fig. 7A), and the hourly PM concentration at the same 450 time did not exceed 45 µg m⁻³ (PM₁₀ was 44 ± 5.9 µg m⁻³, PM_{2.5} was 27 ± 1.4 µg m⁻³, and PM₁ was 23.8 ± 1.2 µg m⁻³; Fig. 7B). The size distribution at the same time showed a very high number concentration of small particles $<1\mu m$ (more than $\frac{10^5}{10^3}$ # cm⁻³ for particles ranging from 0.25 - 0.3 µm; Fig. 7C). Haze was reported again the next morning beginning at 5:00, and the visibility from 10:00 to 11:00 dropped from 16 to 8 km. The total number concentration (hourly averaged) at that time was $126 \pm 13.8 \, \mu \, \text{cm}^{-3}$ (Fig. 7A). The PM hourly concentrations did not exceed 30 $\mu \, \text{gm}^{-3}$ (the hourly PM₁₀ was 29.6 $\pm 3 \, \mu \, \text{gm}^{-3}$. 455 $PM_{2.5}$ was $23.0 \pm 1.6 \mu g$ m⁻³ and PM_1 of $20.8 \pm 1.5 \mu g$ m⁻³; Fig. 7B), while as observed the previous day, the size distribution showed very high number concentrations of small particles of $<1\mu$ m (Fig. 7C). These two haze events had lower (by an order of magnitude) particle mass and total number concentrations compared to several large haze events measured in China (Gou et al., 2014; Wang et al., 2014; Li et al., 2019). Some of the differences in particle concentration in the haze events measured here compared to those measured in China may be attributed to the different particle sizes used. -The particle size range used 460 in Gou et al. (2014) was smaller (from 10 nm to 0.6 μ m) than the one used in this work (particles \geq 0.25 μ m were detected). Using similar particle sizes, Wang et al. (2014) still measured higher particle number concentrations than the two presented here, but the haze event in their work had a higher magnitude than the one measured in this work. It is possible to assume that since measurements taken in this region which has much smaller cities compared to those measured in China, therefore there will be differences in the emissions rate and type which will attribute to the differences of number and mass concentrations 465

observed here compared to those from China.

On March 30 at midnight, a dust event (blowing dust) was reported by the local NWS station (reports observed between 0:35 to 0:45). The wind speed reached 12 m s⁻¹, wind gusts of 17 m s⁻¹ were reported, and the visibility dropped to 9.6 km. During that hour, lower total number concentrations were measured ($28.3 \pm 2.3 \# \text{ cm}^{-3}$) than those measured in the two haze events

mentioned above. Higher PM concentrations were reported during the hour with the dust event, with hourly values of 319.3 ± 192.2 , 46.7 ± 29.9 , and $6.6 \pm 3.5 \,\mu g \,\mathrm{m}^{-3}$ for PM₁₀, PM_{2.5}, and PM₁, respectively (Fig. 7B). This dust event had much lower PM concentrations than those measured in Saudi Arabia (Alghamdi et al., 2015), Israel (Ardon-Dryer and Levin, 2014), Crete (Polymenakou et al., 2008), and other locations in the US, such as Arizona (Hyde et al., 2018). During the dust event, higher number concentrations of larger particles (>1µm) were observed (Fig. 7C). The size distribution of the particles had a bimodal distribution, with high number concentrations at sizes 0.28 µm and 3 µm. Previous studies also measured lower number concentrations of small particles with an increase in large particles during several dust events (Ardon-Dryer and Levin, 2014; Niu et al., 2016).

- 480 An increase in particle <u>number</u> concentration during the dust event compared to the two haze events was observed for particles ≥ 0.8 µm. Observations based on the differences or ratio between PM₁₀ and PM_{2.5} have been used to distinguish between dust and non-dust events (Alghamdi et al., 2015; Sugimoto et al., 2016). For the dust event, PM₁₀ PM_{2.5} was 277.6 µg m⁻³, which was an order of magnitude higher than in the two haze events (17 and 7.6 µg m⁻³ for March 28 and 29, respectively). The PM_{2.5}/PM₁₀ ratio for the dust event was 0.15, while the values for the haze events were higher (0.61 and 0.74 for March 28 and 485 29, respectively). It has been suggested that a lower PM_{2.5}/PM₁₀ ratio (<0.35) indicates a contribution from natural sources</p>
- (e.g., dust event), while a higher ratio suggested that a lower TM_{2,5}/TM₁₀ ratio ((0.55)) indicates a contribution from natural sources (e.g., dust event), while a higher ratio suggests a larger contribution from anthropogenic sources (Sugimoto et al., 2016; Tong et al., 2012). The PM_{2.5}/PM₁₀ ratio helps to distinguish between natural and anthropogenic events, but according to Lei and Wang (2014), this ratio may suffer from intrinsic deficiency as an identification criterion for dust events because the ratio for normal days may have already been very low. Therefore, additional measurements such as particle size distribution can support such observation.

As described above, continuous measurements of <u>aerosol-particle_concentrations (number and mass)</u> and particle size distribution enable distinguishing between dust and anthropogenic events in this area, which emphasizes the ability of AEROS's aerosol instruments to distinguish between different pollution events. The additional information of different PM sizes provided by AEROS, as well as total number concentrations and particle size distribution, can better explain the impact of different pollution events on air quality in this region. Although the atmospheric measurements presented in this work were based on an hourly basis, each of the three instruments measures at a 1-_min time resolution, allowing the observation of changes of particle concentration at short time intervals (e.g., 10 min). Measurements of such short duration will allow observation of short-term events that would have been missed when using the regular hourly average basis.

500

475

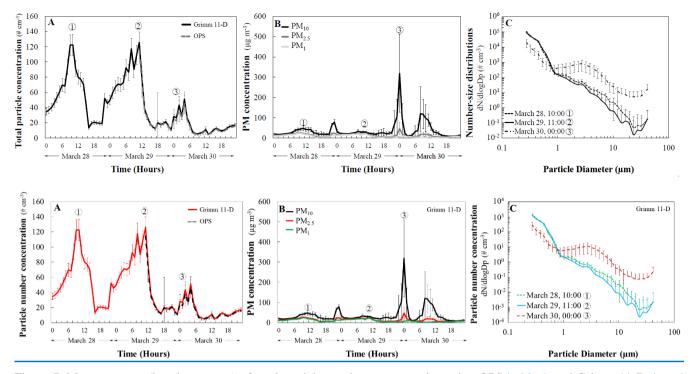


Figure 7. Measurements (hourly average) of total particle number concentration using OPS in black and Grimm 11-D, in red (A), measurements of PM mass concentration from Grimm 11-D (B), and particle size distribution of optical diameter (C)
using Grimm 11-D for March 28 - 30, 2019. The numbers on the plots represent different events (1 and 2 for the haze events and 3 for the dust event). Error bars represent SD values of hourly measurements.

3.5. AEROS limitations

Although AEROS provides crucial information on long-term measurements of various PM sizes, total particle <u>number</u> 510 concentration, and particle size distribution under diverse meteorological and pollution conditions, it has some limitations. Some of these arise from the maintenance of AEROS, which requires weekly checks and calibrations, including cleaning of the instruments and inlets, and replacement of the silica gel in the dryers. The fact that all the instruments used are based on optical size allows for comparison between the instruments, but also mean these instruments require examination and calibration by the manufacturer every year which could be a financial burden as the calibration cost for each unit can range from ~\$3000 to ~\$5000. While AEROS contain grammatic measurements for PM_{2.5} and PM₁₀, those were not available at the time of this comparison and no access was available to reference units such as Beta Attenuation Mass (BAM) monitor or a Tapered Element Oscillating Microbalance (TEOM), therefore additional measurements. Another limitation is that our station provides information for only one site and is unable to capture the spatial variability of particles conversation,

- 520 but even information from this one site is critical for this region, which does not have much information on atmospheric particles number concentrations, different PM sizes mass concentration or and particle size distribution. The fact that all the instruments used are based on optical size allows for comparison between the instruments; ideally, information on particle density or refractive index would allow us to convert the particle sizes, to aerodynamic sizes but such information is not yet available in this region, so particle sizes are based only on optical size. Another limitation is that our station only provides
- 525 information for only one site and is unable to capture the spatial variability of particles, but even information from even this one site is critical for this region, which does not have much information on atmospheric particle concentrations and sizes.

4. Summary

The lack of AQMSs in the Southern High Plains inspired the design and building of AEROS, which provides continuous
measurements of PM mass_concentrations of various sizes, total particle number concentrations, and particle size distribution
from three separate optical aerosol instruments (OPS, Grimm 11-D, and DustTrak). The three aerosol instruments provided
overlapping measurements with similar mass and number_concentrations of atmospheric and laboratory particles. Both the
OPS and Grimm 11-D provided information on total number concentration and size distribution (at least for the size range of
0.3 – 10 µm) and a comparison showed that they are very similar. The DustTrak and Grimm 11-D provided similar PM sizes;
their comparison showed some differences depending on the PM sizes, but although those differences were small, an additional examination will be required, ideally while using a reference PM measurement. Continuous measurement of aerosol-particle concentrations and particle size distribution using AEROS allows demonstrating between dust and anthropogenic events

demonstrating AEROS's ability to identify different pollution events, which will help us to better understand the impact of diverse pollution events (mainly dust) on the air quality in this region.

540

Author contribution. KAD designed and <u>build_built</u> AEROS, designed the experiments, supervised the entire process, and performed most of the analysis, in addition to writing the manuscript. MK performed the experiments. XX helped with the data analysis. YD wrote all the MATLAB codes used for the analysis. All authors were actively involved in interpreting results and in discussions on the manuscript.

545

Declaration of competing interest. The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper.

Acknowledgment. This research did not receive any specific grant from funding agencies in the public, commercial, or notfor-profit sectors. The authors would like to thank Livingston Jeff and Wilks Lee from National Wind Institute, and to James Browning and Darren Hedrick from the Department of Geosciences for all their help assembling AEROS. To Dr. Frank Drewnick for his help and guidance, while using the Particle Loss Calculator (PLC), The authors would like to thank_-Texas Tech University for the support of Mary Kelley and Xia Xueting's scholarship and financial support.

Reference

575

https://doi.org/10.5194/amt-11-709-2018, 2018.

555 Alghamdi, M. A., Almazroui, M., Shamy, M., Redal, M. A., Alkhalaf, A. K., Hussein, M. A., and Khoder, M. I.: Characterization and elemental composition of atmospheric aerosol loads during springtime dust storm in western Saudi Arabia, Aerosol Air Qual. Res., 15, 440–453, https://doi.org/10.4209/aaqr.2014.06.0110, 2015.

Andrews, E., Sheridan, P. J., Ogren, J. A., Hageman, D., Jefferson, A., Wendell, J., Alástuey, A., Alados-Arboledas, L., Bergin, M., Ealo, M., Hallar, A. G., Hoffer, A., Kalapov, I., Keywood, M., Kim, J., Kim, S., Kolonjari, F., Labuschagne, C., Lin, N.,

560 Macdonald, A., Mayol-Bracero, O. L., McCubbin, I. B., Pandolfi, M., Reisen, F., Sharma, S., Sherman, J. P., Sorribas, M., & Sun, J.: Overview of the NOAA/ESRL Federated Aerosol Network, Bull. Am. Meteorol. Soc., 100(1), 123-135, https://doi.org/10.1175/BAMS-D-17-0175.1, 2019.

Ardon-Dryer, K. and Levin, Z.: Ground-based measurements of immersion freezing in the eastern Mediterranean, Atmos. Chem. Phys., 14, 5217–5231, https://doi.org/10.5194/acp-14-5217-2014, 2014.

Ardon-Dryer, K., Garimella, S., Huang, Y.-W., Christopoulos, C., and Cziczo, D: Evaluation of DMA size selection of dry dispersed mineral dust particles, Aerosol Sci. Technol., 49, 828–841,<u>http://dx.doi.org/10.1080/02786826.2015.1077927</u>,2015.
 Ardon-Dryer, K., Dryer, Y., Williams, J. N., and Moghimi, N.: Measurements of PM2.5 with PurpleAir under atmospheric conditions, Atmos. Meas. Tech., 13, 5441–5458, https://doi.org/10.5194/amt-13-5441-2020, 2020.

Barkjohn, K. K., Gantt, B., and Clements, A. L.: Development and application of a United States-wide correction for
PM2.5 data collected with the PurpleAir sensor, Atmos. Meas. Tech., 14, 4617–4637, https://doi.org/10.5194/amt-14-4617-2021, 2021.

BMI.: Brechtel Manufacturing Incorporated Model 9200 Aerosol Generation System. Brechtel Manufacturing Inc., Hayward, CA, 2022.

Cheng, Y.H. and Lin, Y.L.: Measurement of Particle Mass Concentrations and Size Distributions in an Underground Station. Aerosol Air Qual. Res. 10: 22-29. https://doi.org/10.4209/aaqr.2009.05.0037, 2010.

- Chien, C.H., Theodore, A., Wu, C.Y., Hsu, Y.M., and Birky, B.: Upon correlating diameters measured by optical particle counters and aerodynamic particle sizers. J. Aerosol Sci., 101, 77–85, https://doi.org/10.1016/j.jaerosci.2016.05.011, 2016.
 Cohen, A., Anderson, R., Ostro, B., Pandey, K. D., Krzyzanowski, M., Künzli, N, Gutschmidt, K., Pope, C. A., Romieu, I., Samet J. M., and Smith K. R.: Urban ambient air pollution, in: Comparative Quantification of Health Risks: Global and
- Regional Burden of Disease Attributable to Selected Major Risk Factors, edited by: Ezzati, M., Lopez, A.D., Rodgers, A., and Murray, C.J.L, World Health Organization, Geneva, Switzerland, 1353-1433, 2004.
 Crilley, L. R., Shaw, M., Pound, R., Kramer, L. J., Price, R., Young, S., Lewis, A. C., and Pope, F. D.: Evaluation of a low-cost optical particle counter (Alphasense OPC-N2) for ambient air monitoring, Atmos. Meas. Tech., 11, 709–720,
- 585 Crilley, L. R., Singh, A., Kramer, L. J., Shaw, M. D., Alam, M. S., Apte, J. S., Bloss, W. J., Hildebrandt Ruiz, L., Fu, P., Fu, W., Gani, S., Gatari, M., Ilyinskaya, E., Lewis, A. C., Ng'ang'a, D., Sun, Y., Whitty, R. C. W., Yue, S., Young, S., and Pope,

F. D.: Effect of aerosol composition on the performance of low-cost optical particle counter correction factors, Atmos. Meas. Tech., 13, 1181–1193, https://doi.org/10.5194/amt-13-1181-2020, 2020.

Deane, G. and Gutmann, M. P.: Blowin' Down the Road: Investigating Bilateral Causality Between Dust Storms and 590 Population in the Great Plains, Popul. Res. Policy Rev., 22, 297–331, https://doi.org/10.1023/A:1027374330129, 2003.

EPA. Appendix L to part 50—reference method for the determination of fine particulate matter as PM_{2.5} in the atmosphere.
 Federal Register, 62:57–95, 1997.

EPA. Chemical Speciation Network (CSN). https://www.epa.gov/amtic/chemical-speciation-network-csn, 2022.

Gill, T. E., Reynolds, R. L., and Zobeck, T. M.: Measurements of current and historic settled dusts in west Texas, in:
Proceedings of the 93rd Air and Waste Management Association (AWMA) Annual Conference and Exhibition, Salt Lake City, Utah, June 2000, 175, 15, 2000.

Gill, T. E., Stout, J. E., and Peinado, P.: Composition and characteristics of aerosols in the Southern High Plains of Texas (USA), in: Proceedings of Application of Accelerators in Research and Industry: Twentieth International Conference, Fort Worth, Texas, 10-15 August 2008, 255-258, 2009.

600 Goudie, A. S.: Desert dust and human health disorders, Environ. Int., 63, 101-113, https://doi.org/10.1016/j.envint.2013.10.011, 2014.

Grimm 11-D.: Portable Aerosol Spectrometer MODEL 11-D manual, Grimm Aerosol Technik Ainring GmbH & Co.KG, Germany, 2020.

Grimm 11-D: https://www.grimm-aerosol.com/products-en/dust-monitors/the-dust-decoder/11-d/, last access: 5 August 2021.

 Guo, S., H, M., Zamora, M. L., Peng, J., Shang, D., Zheng, J., Du, Z., Wu, Z., Shao, M., Zeng, L., Molina, M. J., and Zhang,
 R.: Haze in China, in: Proceedings of the National Academy of Sciences, December 2014, 111, 17373-17378, https://doi.org/10.1073/pnas.1419604111, 2014.

Holstius, D. M., Pillarisetti, A., Smith, K. R., and Seto, E.: Field calibrations of a low-cost aerosol sensor at a regulatory monitoring site in California, Atmos. Meas. Tech., 7, 1121–1131, https://doi.org/10.5194/amt-7-1121-2014, 2014.

610 Hsiao, T. C., Lee, Y. C., Chen, K. C., Ye, W. C., Sopajaree, K., and Tsai, Y. I.: Experimental Comparison of Two Portable and Real-Time Size Distribution Analyzers for Nano/Submicron Aerosol Measurements, Aerosol Air Qual. Res., 16, 919-929, https://doi.org/10.4209/aaqr.2015.10.0614, 2016.

Hyde, P., Mahalov, A., and Li, J.: Simulating the meteorology and PM10 concentrations in Arizona dust storms using the Weather Research and Forecasting model with Chemistry (Wrf-Chem), J. Air Waste Manag. Assoc., 68, 177-195, https://doi.org/10.1080/10962247.2017.1357662, 2018.

- Jaafari, J., Naddafi, K., Yunesian, M., Nabizadeh, R., Hassanvand, M. S., Ghozikali, M. G., Nazmara, S., Shamsollahi, H. R., and Yaghmaeian, K.: Study of PM10, PM2.5, and PM1 levels in during dust storms and local air pollution events in urban and rural sites in Tehran, Hum. Ecol. Risk Assess.: Int. J., 24, 482-493, https://doi.org/10.1080/10807039.2017.1389608, 2018. Jaganmohan. M.: Annual amount of precipitation in the United States from 1900 2020, to
- 620 https://www.statista.com/statistics/504400/volume-of-precipitation-in-th e-us/, access: 9 May 2021.

615

Javed, W. and Guo, B.: Performance Evaluation of Real-time DustTrak Monitors for Outdoor Particulate Mass Measurements in a Desert Environment, Aerosol Air Qual. Res., 21, 200631, https://doi.org/10.4209/aaqr.200631, 2021.

Kelley, M. C., Brown, M. M., Fedler, C. B., and Ardon-Dryer, K.: Long-term Measurements of PM2.5 Concentrations in Lubbock, Texas, Aerosol Air Qual. Res., 20, 1306-1318, https://doi.org/10.4209/aaqr.2019.09.0469, 2020.

Kelley, M. C. and Ardon-Dryer, K.: Analyzing two decades of dust events on the Southern Great Plains region of West Texas, Atmos. Pollut. Res., 12, 101091, https://doi.org/10.1016/j.apr.2021.101091, 2021.
Kulkarni, P., Baron, P. A., and Willeke, K. (Eds.): Aerosol Measurement: Principles, Techniques, and Applications, third edition, John Wiley & Sons Inc., 2011.

Lee, H. G., Gent, J. F., Leaderer, B. P., Koutrakis, P.: Spatial and temporal variability of fine particle composition and source 630 types in five cities of Connecticut and Massachusetts, Sci. Total Environ., 409, 2133–2142, https://doi.org/10.1016/j.scitotenv.2011.02.025, 2011.

- Lei, H. and Wang, J. X. L.: Observed characteristics of dust storm events over the western United States using meteorological, satellite, and air quality measurements, Atmos. Chem. Phys., 14, 7847–7857, https://doi.org/10.5194/acp-14-7847-2014, 2014. Li, Y., Zheng, C., Ma, Z., and Quan, W.: Acute and Cumulative Effects of Haze Fine Particles on Mortality and the Seasonal
- Characteristics in Beijing, China, 2005-2013: A Time-Stratified Case-Crossover Study, Int J Environ Res Public Health, 16, 2383, https://doi.org/10.3390/ijerph16132383, 2019.
 - Lim, S. S., Vos, T., Flaxman, A. D., Danaei, G., Shibuya, K., Adair-Rohani, H., AlMazroa, M. A., Amann, M., Anderson, H.
 R., Andrews, K. G., Aryee, M., Atkinson, C., Bacchus, L. J., Bahalim, A. N., Balakrishnan, K., Balmes, J., Barker-Collo, S.,
 Baxter, A., Bell, M. L., Blore, J. D., Blyth, F., Bonner, C., Borges, G., Bourne, R., Boussinesq, M., Brauer, M., Brooks, P.,
- Bruce, N. G., Brunekreef, B., Bryan-Hancock, C., Bucello, C., Buchbinder, R., Bull, F., Burnett, R. T., Byers, T. E., Calabria, B., Carapetis, J., Carnahan, E., Chafe, Z., Charlson, F., Chen, H., Chen, J. S., Cheng, A. T.-A., Child, J. C., Cohen, A., Colson, K. E., Cowie, B. C., Darby, S., Darling, S., Davis, A., Degenhardt, L., Dentener, F., Des Jarlais, D. C., Devries, K., Dherani, M., Ding, E. L., Dorsey, E. R., Driscoll, T., Edmond, K., Ali, S. E., Engell, R. E., Erwin, P. J., Fahimi, S., Falder, G., Farzadfar, F., Ferrari, A., Finucane, M. M., Flaxman, S., Fowkes, F. G. R., Freedman, G., Freeman, M. K., akidou, E., Ghosh, S.,
- Giovannucci, E., Gmel, G., Graham, K., Grainger, R., Grant, B., Gunnell, D., Gutierrez, H. R., Hall, W., Hoek, H. W., Hogan, A., Hosgood III, H. D., Hoy, D., Hu, H., Hubbell, B. J., Hutchings, S. J., Ibeanusi, S. E., Jacklyn, G. L., Jasrasaria, R., Jonas, J. B., Kan, H., Kanis, J. A., Kassebaum, N., Kawakami, N., Khang, Y.-H., Khatibzadeh, S., Khoo, J.-P., Kok, C., Laden, F., Lalloo, R., Lan, Q, Lathlean, T., Leasher, J. L., Leigh, J., Li, Y., Lin, J. K., Lipshultz, S. E., London, S., Lozano, R., Lu, Y., Mak, J., Malekzadeh, R., Mallinger, L., Marcenes, W., March, L., Marks, R., Martin, R., McGale, P., McGrath, J., Mehta, S.,
- 650 Mensah, G. A., Merriman, T. R., Micha, R., Michaud, C., Mishra, V., Mohd Hanafiah, K.,Mokdad, A. A., Morawska, L., Mozaffarian, D., Murphy, T., Naghavi, M., Neal, B., Nelson, P. K., Nolla, J. M., Norman, R., Olives, C., Omer, S. B., Orchard, J., Osborne, R., Ostro, B., Page, A., Pandey, K. D., Parry, C. D., Passmore, E., Patra, J., Pearce, N., Pelizzari, P.M., Petzold, M., Phillips, M. R., Pope, D., Pope, C. A., Powles, J., Rao, M., Razavi, H., Rehfuess, E. A., Rehm, J. T., Ritz, B., Rivara, F. P., Roberts, T., Robinson, C., Rodriguez-Portales, J. A., Romieu, I., Room, R., Rosenfeld, L. C., Roy, A., Rushton, L.,

- Salomon, J. A., Sampson, U., Sanchez-Riera, L., Sanman, E., Sapkota, A., Seedat, S., Shi, P., Shield, K., Shivakoti, R., Singh, G. M., Sleet, D. A., Smith, E., Smith, K. R., Stapelberg, N. J., Steenland, K., Stockl, H., Stovner, L. J., Straif, K., Straney, L., Thurston, G. D., Tran, J. H., Van Dingenen, R., van Donkelaar, A., Veerman, J. L., Vijayakumar, L., Weintraub, R., Weissman, M. M., White, R. A., Whiteford, H., Wiersma, S. T., Wilkinson, J. D., Williams, H. C., Williams, W., Wilson, N., Woolf, A. D., Yip, P., Zielinski, J. M., Lopez, A. D., Murray, C. J., Ezzati, M., AlMazroa, M. A., and Memish, Z. A.: A comparative risk
- 660 assessment of burden of disease and injury attributable to 67 risk factors and risk factor clusters in 21 regions, 1990–2010: a systematic analysis for the Global Burden of Disease Study 2010, Lancet, 380, 2224–2260, https://doi.org/10.1016/S0140-6736(12)61766- 8, 2012.

Ling, S. H., and van Eeden, S. F.: Particulate matter air pollution exposure: Role in the development and exacerbation of chronic obstructive pulmonary disease, Int. J. Chron. Obstruct. Pulmon. Dis., 4, 233-243, <u>DOI: 10.2147/copd.s5098</u>, 2009.

Mahowald, N., Albani, S., Kok, J. F., Engelstaeder, S., Scanza, R., Ward, D. S., and Flanner, M. G.: The size distribution of desert dust aerosols and its impact on the Earth system, Aeolian Res., 15, 53-71, https://doi.org/10.1016/j.aeolia.2013.09.002, 2014.

Maragkidou, A., Jaghbeir, O., Hämeri, K., and Hussein, T.: Aerosol particles (0.3 – 10 μm) inside an educational workshop -Emission rate and inhaled deposited dose, Build. Environ., 140, 80–89, https://doi.org/10.1016/j.buildenv.2018.05.031, 2018.

- Marple, V. A., Rubow, K. L., Turner, W., Spengler, J.: Low flow rate sharp cut impactors for indoor air sampling: design and calibration, JAPCA, 37, 1303–1307, https://doi.org/10.1080/08940630.1987.10466325, 1987.
 Masic, A., Bibic, D., Pikula, B., Blazevic, A., Huremovic, J., and Zero, S.: Evaluation of optical particulate matter sensors under realistic conditions of strong and mild urban pollution, Atmos. Meas. Tech., 13, 6427–6443, https://doi.org/10.5194/amt-13-6427-2020, 2020.
- McNamara, M. L., Noonan, C. W., and Ward, T. J.: Correction factor for continuous monitoring of wood smoke fine particulate matter, Aerosol Air Qual. Res., 11, 315–322, http://doi.org/ 10.4209/aaqr.2010.08.0072, 2011.
 Mølgaard, B., Viitanen, A. K., Kangas, A., Huhtiniemi, M., Larsen, S. T., Vanhala, E., Hussein, T., Boor, B. E., Hämeri, K., and Koivisto, A. J.: Exposure to Airborne Particles and Volatile Organic Compounds from Polyurethane Molding, Spray Painting, Lacquering, and Gluing in a Workshop, Int. J. Environ. Res. Public Health, 12, 3756–3773,
- https://doi.org/10.3390/ijerph120403756, 2015.
 Mukherjee, A., Stanton, L. G., Graham, A. R., Roberts, P. T.: Assessing the Utility of Low-Cost Particulate Matter Sensors over a 12-Week Period in the Cuyama Valley of California, Sensors, 17, 1805, https://doi.org/10.3390/s17081805, 2017.
 Niu, H., Zhang, D., Hu, W., Shi, J., Li, R., Gao, H., Pian, W., and Hu, M.: Size and elemental composition of dry-deposited particles during a severe dust storm at a coastal site of Eastern China, J. Environ. Sci., 40, 161-168, https://doi.org/10.1016/j.jes.2015.09.016, 2016.
- Orgill, M. M. and Sehmel, G. A.: Frequency and diurnal variation of dust storms in the contiguous U.S.A., Atmos. Environ., 10, 813-825, https://doi.org/10.1016/0004-6981(76)90136-0, 1976.

Peters, T. M., Ott. D., and O'Shaughnessy, P. T.: Comparison of the Grimm 1.108 and 1.109 Portable Aerosol Spectrometer to the TSI 3321 Aerodynamic Particle Sizer for Dry Particles, Ann. Occup. Hyg., 50, 8, 843–

Polymenakou, P. N., Mandalakis, M., Stephanou, E. G., and Tselepides, A.: Particle size distribution of airborne microorganisms and pathogens during an Intense African dust event in the eastern Mediterranean, Environ. Health Perspect., 116, 292-6, https://doi.org/10.1289/ehp.10684, 2008.

690

850, https://doi.org/10.1093/annhyg/mel067, 2006.

- Prenni, A. J., Hand, J. L., Malm, W. C., Copeland, S., Luo, G., Yu, F., Taylor, N., Russell, L. M., and Schichtel, B. A.: An examination of the algorithm for estimating light extinction from IMPROVE particle speciation data, Atmos. Environ., 214, 116880, https://doi.org/10.1016/j.atmosenv.2019.116880, 2019.
- Rivas, I., Mazaheri, M., Viana, M., Moreno, T., Clifford, S., He, C., Bischof, O. F., Martins, V., Reche, C., Alastuey, A., Alvarez-Pedrerol, M., Sunyer, J., Morawska, L., and Querol, X.: Identification of technical problems affecting performance of DustTrak DRX aerosol monitors, Sci. Total Environ., 584-585, 849-855, https://doi.org/10.1016/j.scitotenv.2017.01.129, 2017.
 - Roesch, M., Roesch, C., and Cziczo, D. J.: Dry particle generation with a 3-D printed fluidized bed generator, Atmos. Meas. Tech., 10, 1999-2007, https://doi.org/10.5194/amt-10-1999-2017, 2017.
 - Shiraiwa, M., Ueda, K., Pozzer, A., Lammel, G., Kampf, C. J., Fushimi, A., Enami, S., Arangio, A. M., Frohlich-Nowoisky, J., Fujitani, Y., Furuyama, A., Lakey, P. S. J., Lelieveld, J., Lucas, K., Morino, Y., Poschl, U., Takaharna, S., Takami, A.,
- Tong, H. J., Weber, B., Yoshino, A., and Sato, K.: Aerosol Health Effects from Molecular to Global Scales, Environ. Sci. Technol., 51, 13545–13567, https://doi.org/10.1021/acs.est.7b04417, 2017.
 Snider, G., Weagle, C. L., Martin, R. V., van Donkelaar, A., Conrad, K., Cunningham, D., Gordon, C., Zwicker, M., Akoshile, C., Artaxo, P., Anh, N. X., Brook, J., Dong, J., Garland, R. M., Greenwald, R., Griffith, D., He, K., Holben, B. N., Kahn, R., Koren, I., Lagrosas, N., Lestari, P., Ma, Z., Vanderlei Martins, J., Quel, E. J., Rudich, Y., Salam, A., Tripathi, S. N., Yu, C.,
- 710 Zhang, Q., Zhang, Y., Brauer, M., Cohen, A., Gibson, M. D., and Liu, Y.: SPARTAN: a global network to evaluate and enhance satellite-based estimates of ground-level particulate matter for global health applications, Atmos. Meas. Tech., 8, 505– 521, https://doi.org/10.5194/amt-8-505-2015, 2015.

<u>Solomon, P. A., Crumpler, D., Flanagan, J. B., Jayanty, R. K. M., Rickman, E. E., and McDade, C. E.: U.S. National PM2.5</u>
 <u>Chemical Speciation Monitoring Networks</u>— CSN and IMPROVE: Description of Networks. J. Air Waste Manag. Assoc.,
 64:1410–1438. DOI: 10.1080/10962247.2014.956904, 2014

- Stavroulas, I., Grivas, G., Michalopoulos, P., Liakakou, E., Bougiatioti, A., Kalkavouras, P., Fameli, K. M., Hatzianastassiou, N., Mihalopoulos, N., Gerasopoulos, E.: Field Evaluation of Low-Cost PM Sensors (Purple Air PA-II) Under Variable Urban Air Quality Conditions, in Greece, Atmos., 11, 926, https://doi.org/10.3390/atmos11090926, 2020.
 <u>Sousan, S., Koehler, K., Hallett, L., and Peters, T. M.: Evaluation of the Alphasense optical particle counter (OPC-N2) and the</u>
- 720 Grimm portable aerosol spectrometer (PAS-1.108), Aerosol Sci. Tech., 50, 1352–1365, https://doi.org/10.1080/02786826.2016.1232859, 2016.

Stout, J. E.: Effect of averaging time on the apparent threshold for aeolian transport, J. Arid Environ., 39, 395-401, https://doi.org/10.1006/jare.1997.0370, 1998.

Sugimoto, N., Shimizu, A., Matsui, I., and Nishikawa, M.: A method for estimating the fraction of mineral dust in particulate matter using PM2.5-to-PM10 ratios, Particuology, 28, 114–120, https://doi.org/10.1016/j.partic.2015.09.005, 2016.

Texas Commission on Environmental Quality: AQI and Data Reports, Texas Commission on Environmental Quality, https://www.tceq.texas.gov/airquality/monops/data-reports, last access: 4 June 2020.

725

750

Tong, D. Q., Dan, M., Wang, T., and Lee, P.: Long-term dust climatology in the western United States reconstructed from routine aerosol ground monitoring, Atmos. Chem. Phys., 12, 5189–5205, https://doi.org/10.5194/acp-12-5189-2012, 2012.

TSI: DUSTTRAK[™] DRX Aerosol Monitor Model 8533/8534/8533EP, Operation and Service Manual, P/N 6001898 Revision
 S, https://www.tsi.com/getmedia/3699890e-4adf-452f-9029-f3725612d5d1/8533-8534-DustTrak_DRX-6001898-Manual-US?ext=.pdf, 2019.

Vasilatou, K., Wälchlia, C., Koust, S., Horender, S., Iida, K., Sakurai, H., Schneider, F., Spielvogel, J., Wu, T. Y., and Auderset, K.: Calibration of optical particle size spectrometers against a primary standard: Counting efficiency profile of the

735 TSI Model 3330 OPS and Grimm 11-D monitor in the particle size range from 300 nm to 10 μm, J. Aerosol Sci., 157, 105818, https://doi.org/10.1016/j.jaerosci.2021.105818, 2021.

Viana, M., Rivas, I., Reche, C., Fonseca, A. S., Pérez, N., Querol, X., Alastuey, A., Álvarez-Pedrerol, M., and Sunyer, J.: Field comparison of portable and stationary instruments for outdoor urban air exposure assessments, Atmos. Environ., 123, 220–228, http://dx.doi.org/10.1016/j.atmosenv.2015.10.076, 2015.

 von der Weiden, S.-L., Drewnick, F., and Borrmann, S.: Particle Loss Calculator – a new software tool for the assessment of the performance of aerosol inlet systems, Atmos. Meas. Tech., 2, 479–494, https://doi.org/10.5194/amt-2-479-2009, 2009.
 Wang, X., Chancellor, G., Evenstad, J., Farnsworth, J. E., Hase, A., Olson, G. M., Sreenath, A., Agarwal, J. K., 2009. A novel

optical instrument for estimating size segregated aerosol mass concentration in real time. Aerosol Sci. Technol. 43:939–950. http://dx.doi.org/10.1080/02786820903045141.2009.

745 Wang, X. M., Chen, J. M., and Cheng, T. T.: Particle number concentration, size distribution and chemical composition during haze and photochemical smog episodes in Shanghai, J. Environ. Sci., 26, 1894–1902, https://doi.org/10.1016/j. jes.2014.07.003, 2014.

Wang, X., Zhou, H., Arnott, W. P., Meyer, M. E., Taylor, S., Firouzkouhi, H., Moosmüller, H., Chow, J. C., and Watson, J. G.: Evaluation of gas and particle sensors for detecting spacecraft-relevant fire emissions, Fire Saf. J., 113, 102977, https://doi.org/10.1016/j.firesaf.2020.102977, 2020.

WMO: WMO/GAW aerosol measurement procedures, guidelines, and recommendations. 2nd ed, World Meteorological Organization GAW, Rep. 227, 93 pp., https://library.wmo.int/opac/doc_num.php?explnum_id=3073, 2016.

World Health Organization: Ambient Air Pollution: A Global Assessment of Exposure and Burden of Disease, World Health Organization, Geneva, Switzerland, 2016.

Yamada, M., Takaya, M., and Ogura, I.: Performance evaluation of newly developed portable aerosol sizers used for nanomaterial aerosol measurements. Ind. Health, 53, 511–516, https://doi.org/10.2486/indhealth.2014-0243, 2015.
 Zhang, J., Marto, J. P., and Schwab, J. J.: Exploring the applicability and limitations of selected optical scattering instruments for PM mass measurement, Atmos. Meas. Tech., 11, 2995–3005, https://doi.org/10.5194/amt-11-2995-2018, 2018.