

Traceable total ozone column retrievals from direct solar spectral irradiance measurements in the ultraviolet

Luca Egli¹, Julian Gröbner¹, Gregor Hülsen¹, Herbert Schill¹ and René Stübi²

¹Physikalisch-Meteorologisches Observatorium Davos (PMOD/WRC), 7260 Davos Dorf, Switzerland

5 ²MeteoSwiss, Payerne, Switzerland

Correspondence to: L. Egli (luca.egli@pmodwrc.ch)

Abstract Total column ozone (TCO) is commonly measured by Brewer and Dobson spectroradiometers. Both types of instruments are using solar irradiance measurements at four wavelengths in the ultraviolet radiation range to derive TCO. For the calibration and quality assurance of the measured TCO both instrument types require periodic field comparisons with a reference instrument.

This study presents traceable TCO retrievals from direct solar spectral irradiance measurements with the portable UV reference instrument QASUME. TCO is retrieved by a spectral fitting technique derived by a minimal least square fit algorithm using spectral measurements in the wavelength range between 305 nm and 345 nm. The retrieval is based on an atmospheric model accounting for different atmospheric parameters such as effective ozone temperature, aerosol optical depth, Rayleigh scattering, SO₂, ground air pressure, ozone absorption cross sections and top-of-atmosphere solar spectrum. Traceability is achieved by fully characterizing and calibrating the QASUME spectroradiometer in the laboratory to SI standards (International System of Units). The TCO retrieval method from this instrument is independent from any reference instrument and does not require periodic in situ field calibration.

The results show that TCO from QASUME can be retrieved with a relative standard uncertainty of less than 0.8%, when accounting for uncertainties from the measurements and the retrieval model, such as different ozone absorption cross sections, different reference top-of-the atmosphere solar spectra, uncertainties from effective ozone temperature or other atmospheric parameters. The long-term comparison of QASUME TCO with TCO derived from a Brewer and a Dobson in Davos, Switzerland, reveals, that all three instruments are consistent within 1% when using the ozone absorption cross section from the University of Bremen. From the results and method presented here, other absolute SI calibrated cost effective solar spectroradiometers, such as array spectroradiometers, may be applied for traceable TCO monitoring.

1 Introduction

Since the 1970's the depletion of the stratospheric ozone layer is reported in many international scientific publications (e.g. Molina and Rowland 1974, Solomon 1999, Staehlin et al. 2001) and regularly summarized in the Word Meteorological Organisation (WMO) assessment of ozone depletion (e.g. WMO (2018) or <https://www.esrl.noaa.gov/csd/assessments/ozone>). It has been shown that the ozone layer in the stratosphere was reduced by anthropogenic emissions of ozone depleting substances, which have been controlled since the 1980s by the Montreal protocol. In order to monitor the effect of the decisions by the Montreal protocol and its amendments, the temporal development of the ozone layer needs to be observed worldwide with accurate instrumentations. Furthermore, the mutual interactions between the ozone layer and climatic change on Earth's surface are currently investigated and require long-term consistent observations of total ozone column in the atmosphere (e.g. Bais et al., 2015, Bais et al., 2019; Seckmeyer et al., 2018, Young et al., 2021).

The atmospheric shield of total column ozone (TCO) is important for the incoming UV radiation at the Earth's surface and its impact on human health (Zerefos, 2002) due to changing UV exposure on the ground with decreasing TCO. Since the ozone layer absorbs effectively the radiation in the UV band at wavelengths shorter than 350 nm, accurate direct sun measurements

of the UV radiation allow retrieving TCO at the earth surface by measuring the UV radiation in that wavelength band (Kerr et al., 1988).

Since the beginning of the 1920s, total ozone column has been measured by the Dobson sun spectroradiometer (Dobson, 1931; Dobson, 1968, Basher 1982, Komhyr et al. 2002) to form a global network. The Dobson instruments were operated manually and required substantial manpower and maintenance and were difficult to operate at remote sites. In order to monitor the aforementioned depletion of TCO and its impact on climatic change and the UV exposure on the ground, the Brewer spectrometer (Kerr et al., 1981, Kerr et al. 1985) was introduced in the 1980s as an automatic device measuring direct solar UV radiation and global UV irradiance with then state-of-the-art technology using gratings instead of prisms. Contrary to the Dobson instruments, the Brewer also allowed measuring absolute intensities, in contrast to the Dobson instruments, which provide relative measurements of the different UV wavelength bands. Both, the Brewer and the Dobson instruments are considered as the standard instruments for TCO monitoring on the ground by WMO in the framework of the Global Atmosphere Watch program (GAW).

The Dobson as well as the Brewer are operationally using solar irradiance measurements at four specific wavelengths in the UV band between 300 nm and 340 nm for the retrieval of ozone with the double ratio technique (Kerr et al, 1988) and have to be calibrated for TCO against a regional standard instrument via on-site intercomparisons (Köhler et al. 2002, Redondas et al. 2018). Systematic biases and seasonal dependency were observed when comparing both instruments (Kerr et al., 1988, Köhler et al., 2018, Stählin et al., 2018, Vanicek et al., 2012, Redondas et al., 2014, Gröbner et al., 2021), displaying biases in estimating TCO with the Dobson or the Brewer. Recently, Gröbner et al. 2021 showed that these systematic biases between Brewer and Dobson can be reduced by using the temperature dependent ozone absorption cross sections from the University of Bremen (IUP, Serdyuchenko et al, 2014) calculated with the effective ozone temperature from balloon soundings.

In recent years, TCO was also retrieved from the Earth's surface accounting for the solar spectrum between 300 nm and 340 nm, e.g. with the Phaeton system (Gkertsi et al. 2018), the Pandora system (Herman et al. 2017) or the BTS array spectroradiometer (Zuber et al. 2018a,b, Zuber et al. 2021).

In this study a scanning double monochromator is used to retrieve TCO from direct solar UV spectral irradiance measurements between 305 nm and 345 nm at a wavelength increment of 0.25 nm. The retrieval of TCO is named here as "full spectrum" retrieval of TCO. Therefore, this retrieval includes a larger amount of spectral information in the atmospheric ozone absorption band compared to the standard four wavelengths of the Dobson and Brewer.

The main objective of this study is to introduce traceable TCO measurements from the world portable reference spectroradiometer for UV radiation QASUME (Gröbner et al. 2005) as a reference for TCO. Traceability is achieved by fully characterizing and calibrating the QASUME spectroradiometer in the laboratory with sources that are traceable to primary SI standards with an unbroken calibration chain and a comprehensive uncertainty analysis for the entire calibration chain. Since TCO cannot be measured directly, but only from ground remote sensing, a retrieval model algorithm is needed to derive TCO from the solar UV irradiance measurements. The uncertainty of the retrieval algorithm is also investigated for the various parameters of the retrieval model. We define here "model traceability" with respect to the retrieval as a standardized, reproducible and comprehensible process to derive TCO from the solar UV spectrum. Both, the uncertainty of the spectral measurements and the uncertainties of the retrieval algorithm result in an overall uncertainty of traceable TCO observations. The sensitivity of the retrieval model is determined for various atmospheric input parameters and then optimized for robust TCO estimations. The presented method can also be considered as a reference algorithm for other instruments measuring UV spectra from calibrated direct sun irradiance as e.g. array spectroradiometers (Zuber et al. 2021).

Finally, the results of the traceable TCO measurements from QASUME are compared with long-term observations from two instruments of MeteoSwiss, a double monochromator Brewer and a Dobson spectroradiometer operated at the World Radiation Center (PMOD/WRC), in Davos, Switzerland, between 20 September 2018 and 15 November 2020. This long-term intercomparison allows validating and investigating the reproducibility of the TCO measurements from QASUME.

2 Instrument and Retrieval Algorithm

2.1 QASUME portable UV reference instrument

85

The transportable reference spectroradiometer QASUME was built for quality assurance of spectral ultraviolet measurements in Europe, as described in Gröbner et al. (2005). Since 2001, QASUME has been deployed at more than 33 stations worldwide to assure the quality of global UV irradiance measurements from other spectroradiometers such as e.g. the Brewer spectroradiometer. A thorough revised uncertainty budget for the QASUME instrument was calculated and presented in Hülsen et al. (2016). The uncertainty budget will be used for the estimation of the overall uncertainty budget of TCO in section 3.1.

90

The QASUME instrument is a scanning double monochromator consisting of a commercially available Bentham DM-150 with a focal length of 150 mm and a grating with 2400 lines/mm. The spectral range covers the wavelength region between 250 nm and 550 nm. The slit function is almost triangular with a full width half maximum resolution of 0.78 nm. The entrance optic is connected by an optical fiber to the monochromator entrance slit and is mounted at the end of a collimating tube of 1000 mm length, providing a full field of view of approximately 2°. The collimating tube with the global entrance optic is mounted on a sun tracker which follows the sun during daytime to measure direct solar irradiance. The system is embedded in a temperature stabilized box, while the entrance optics is heated to a temperature above 28°C to exclude temperature effects of the entrance optics.

95

For this study, direct solar UV irradiance measurements were collected with QASUME between 20 September 2018 and 15 November 2020 at the measurement platform at PMOD/WRC, Davos, Switzerland at 1560 m a.s.l. (coordinates: 46.81 N, 9.83 E) during all seasons, but with some missing periods, when the system was in the laboratory or participated at field measurement campaigns. Spectral measurements of QASUME are traceable to the primary spectral irradiance standard of the Physikalisch Technische Bundesanstalt (PTB) (Gröbner and Sperfeld, 2005) via secondary standard tungsten halogen 1 kW FEL lamps. The stability of QASUME is monitored in the field with 250 W tungsten halogen lamps on a regular schedule on the measurement platform.

105

The spectra were recorded regularly on an interval of 30 minutes and occasionally on an interval of 20 min. Since the instrument is a scanning spectroradiometer, the time interval between each wavelength increment of 0.25 nm is less than or equal to 1.5 seconds, therefore the measurement of the spectrum between 305 nm and 345 nm requires a maximum of 4.5 minutes. More than 3200 spectra, valid for TCO retrieval, were recorded from morning to evening at different solar zenith angles (SZA) ranging between 23° and 76° (ozone air mass between 1.1 and 4.0) during 20 September 2018 and 15 November 2020. The measured spectra were used for the TCO retrieval algorithm as described in the following section.

110

2.2 Total ozone column retrieval algorithm

The post processing of the calibrated solar UV irradiance spectra from QASUME was performed off-line in two steps: a) wavelength shift correction and homogenisation of the spectra with the MatSHIC software developed at PMOD/WRC, b) retrieving TCO with a least square fit (LSF) minimization algorithm according to Huber et al. (1995).

The post-processing chain described here displays an algorithm routine, which ensures consistent and comparable TCO measurements derived from spectral solar measurements:

120

a) MatSHIC algorithm

The MatSHIC algorithm is based on the concepts of the SHICrivism algorithm developed by Slaper et al. (1995) and implemented in Matlab. The algorithm convolves a high spectral resolution solar spectrum (ETS) with the slit function of QASUME and determines the spectral shift for each wavelength of the measured spectrum until the best agreement to the

125 convolved ETS is found. The so detected wavelength shift is then applied to each wavelength of the measured spectrum to
 provide consistency to this reference solar spectrum. In a second step, the algorithm adjusts the high resolution ETS to the
 wavelength corrected measurements. Since the ETS is a high-resolution spectrum with 0.01 nm wavelength steps and around
 0.05 nm full width half maximum slit function, the resulting spectrum can be homogenized by convolution with a triangular
 130 slit function to a selectable wavelength increment and slit function, equal or larger than the wavelength-increment and slit
 function of the ETS. For this study, the resulting spectra were homogenized to 0.01 nm wavelength-increment and **convolved**
 to 0.5 nm full width half maximum with a triangular slit function. These selected specifications have been shown to be the best
 homogenization settings for the TCO retrieval in terms of overall uncertainty.

b) *Total ozone column retrieval algorithm from full solar UV irradiance spectrum*

135 For the full **solar UV irradiance** spectrum TCO retrieval the LSF algorithm presented by Huber et al. (1995) and applied by
 Vaskuri et al. (2018) and further described in Zuber et al. (2021) is refined and optimized here for traceable TCO measurements
 with QASUME.

The LSF algorithm is using a spectral **non-linear least squares fitting procedure** in the main UV ozone absorption wavelength
 range between 305 nm to 345 nm and **implements** an atmospheric model based on the Beer-Lambert law:

140

$$I_{\lambda} = I_0 \exp[-\tau_{\lambda} m] \quad \text{Eq.1}$$

I_{λ} denotes the measured spectral irradiance from QASUME and homogenized by MatSHIC at the wavelength λ . I_0 indicates
 the ETS at the top of the atmosphere. For the standard retrieval presented here, the new composite hybrid solar reference
 145 spectrum TSIS (Coddington et al., 2021) is used for I_0 . m is the airmass **from the surface of Earth** the top of the atmosphere.
 The atmospheric model accounts for the effect of ozone absorption **at** each wavelength and **furthermore** the attenuation by the
 atmosphere including aerosols, Rayleigh scattering and **Sulfur Dioxide (SO₂)**. The resulting attenuated **modelled** solar
 spectrum **using Eq.(2)** is then compared with the measured **solar** spectrum on **the Earth's** surface. The LSF algorithm
 minimizes the **spectral** residuals between the modelled and measured solar spectrum and returns the corresponding model
 150 parameters. Figure 1 shows the residuals **at** each wavelength for **three sample solar spectra measured on 27th** of June 2020. The
 figure shows that the residuals **of the fitting parameters in Eq 1-3 are besides the high frequency variations almost** spectrally
 flat with a high spectral variation between 300 nm and 305 nm and a slight increase at wavelengths larger than 345 nm. The
 spectral **high frequency** variation of up to 2% seen **in Figure 1 are residuals from the convolution of the high resolution ETS**
with the QASUME slit function during the MatSHIC procedure.

155 An important parameter of the model **shown** in Eq.1 is the airmass m , denoting the path length of radiation through the
 atmosphere. The airmass m **furthermore** depends on the geographical location and time of the day and thus on the solar zenith
 angle during a day and over the seasons. The airmass is calculated based on the geometry between the Earth, atmosphere and
 the sun for each time stamp and corresponding wavelength of the measured spectrum individually. The absorption through the
 atmosphere is summarized by the term $\tau(T, p)_{\lambda} m$ in Eq. 2. The term $\tau(T, p)_{\lambda} m$ indicates the attenuation of direct irradiance
 160 by ozone, aerosols, sulfur dioxide (SO₂) and Rayleigh scattering during its path through the standard atmosphere. The airmass
 for the ozone (m_{λ}^{O3}), aerosol (m_{λ}^{AOD}) and Rayleigh (m_{λ}^R) and SO₂ (m_{λ}^{SO2}) is calculated from the standard US atmosphere
 profile for mid-latitudes *afglus* (NOAA, 1976) and Eq. 1 can be written in more detail as Eq. 2.

$$\tau_{\lambda}(T, p) \cdot m_{\lambda} = \tau_{\lambda}^{O3}(T) \cdot m_{\lambda}^{O3} + \tau_{\lambda}^{AOD} \cdot m_{\lambda}^{AOD} + \tau_{\lambda}^R(p) \cdot m_{\lambda}^R + \tau_{\lambda}^{SO2} \cdot m_{\lambda}^{SO2} \quad \text{Eq.2}$$

165

For the ozone attenuation term $\tau_{\lambda}^{O3}(T) \cdot m_{\lambda}^{O3}$ the IUP ozone absorption cross section (Serduychenko et al. 2014) for different
 effective ozone temperatures (T) parametrized with a quadratic polynomial fit is applied for the standard retrieval algorithm.

This cross section has been selected by the WMO as the new reference **ozone absorption** cross sections for the Brewer and Dobson (M. Tully, personal communication in Gröbner et al. (2021)) and the best consistency between Brewer and Dobson is found for the IUP cross section (Redondas et al. 2014, Gröbner et al. (2021)). However, the effect of other available **ozone absorption** cross sections will be analysed and discussed in section 3 addressing the overall uncertainty budget. The dependency of the ozone absorption **cross sections** on temperature implies, that the effective ozone temperature is required **as input** for the TCO retrieval algorithm. In analogy to Gröbner et al. (2021), the effective ozone temperature measurements from balloon sounding at the nearest sounding station in Payerne, Switzerland is taken as input for the retrieval algorithm. **As in Gröbner et al. (2021), days without ozone-sonde launches were calculated from linearly interpolating the effective ozone temperature between successive measurements. To reduce the day-to-day noise, the interpolated dataset was smoothed with a 10-days running mean.**

The term $\tau_{\lambda}^{AOD} \cdot m_{\lambda}^{AOD}$ in Eq. 2 denotes the attenuation by aerosol optical depth. The wavelength dependence of the aerosol optical depth (AOD) for $\tau_{\lambda}^{AOD} \cdot m_{\lambda}^{AOD}$ is defined with a linear parametrization normalized to 340 nm as follows

$$\tau_{\lambda}^{AOD} = \alpha + \beta \cdot (\lambda - 340\text{nm}) \quad \text{Eq. 3}$$

where α and β are the other two free parameters besides TCO for the LSF retrieval. The linear **dependence** of AOD **with wavelength** is also **assumed** in the double ratio technique for the Brewer retrieval (Kerr et al. 1985). **Note that AOD calculated by the Angstrom law result in similar TCO as when using Eq.3.**

The third term in Eq. 2 $\tau_{\lambda}^R(p) \cdot m_{\lambda}^R$ accounts for the **effect of Rayleigh-scattering** in the atmosphere. **The scattering by air molecules** is parametrized according to Bodhaine et al. (1999). This parametrization **uses** the air-pressure p **in order to calculate the Rayleigh optical depth**. Finally, the attenuation by SO_2 is also considered in the overall attenuation equation (Eq.2), **even though the amount of SO_2 in the atmosphere above Davos is so small that it can be neglected here (Gröbner et al., 2021).** **Nitrogen dioxide and other atmospheric trace gases are not considered as their absorption is negligible in this wavelength range. Finally, Recalculation TCO with other standard atmospheres than *afglus* revealed neglectable changes of TCO in Davos.**

Accounting for all four terms of attenuation in the Beer-Lambert atmospheric model, the LSF approach derives the best fit to determine TCO.

In summary, the standard full spectrum TCO retrieval with QASUME consists of the following settings:

- MatSHIC spectrum homogenization: 0.5 nm FWHM, 0.01 nm wavelength increment
- Wavelength range: 305 nm – 345 nm
- Ozone absorption cross section: IUP (Serduyschenko et al. 2014)
- Extraterrestrial solar Spectrum: TSIS (Coddington et al. 2021)
- Aerosol optical depth (AOD): Linear spectral function
- Rayleigh scattering: Bodhaine (Bodhaine et al. 1999)
- SO_2 : **HITRAN (Hermans et al., 2009)**
- Effective ozone temperature: Input parameter from balloon soundings (Gröbner et al. 2021)
- Atmospheric model: Beer-Lambert law (Eq.1), with US standard atmosphere (NOAA, 1976)

3 Uncertainty Budget

3.1 TCO Uncertainty from measurement Uncertainty

The measurement uncertainty of QASUME is reported in Hülsen et al. (2016) for global solar UV irradiance measurements and recalculated for direct solar irradiance in Gröbner et al. (2017). The different contributions for the direct solar UV irradiance measurement uncertainty are separately listed in the publication resulting in an overall relative standard uncertainty of 0.91% (Gröbner et al. (2017), Vaskuri et al. 2018). Vaskuri et al. (2018) stated an uncertainty of 0.38% for TOC retrievals when considering this random noise of 0.91% from the measurements. The uncertainty assessment in Gröbner et al. (2017) does not report any spectral correlation of the uncertainty from spectral measurements. The effects of potential spectral correlations on full spectrum retrievals are investigated and discussed in Vaskuri et al. (2018) applying sinusoidal spectral correlations of different degrees. Depending on the degree of spectral correlation, the uncertainty for TCO from full spectrum originating from the measurements can result in uncertainties of TCO between 0.72% (full correlation), 0.42% (unfavorable correlation) and 0.38% (no correlation) (Vaskuri et al. 2018). Effects of potential spectral correlations are included and discussed in this study in the uncertainty assessment of two different solar spectra (section 3.3). Therefore, we state a conservative uncertainty contribution to TCO originating from spectral measurements from QASUME of 0.42%, $k=1$, (Table 1).

Note that here and in the following sections, the standard uncertainty, $k=1$, indicates that for a normal distribution the uncertainty corresponds to a coverage probability of about 68%, while $k=2$ (expanded uncertainty) corresponds to a coverage probability of approximately 95%.

3.2 Uncertainty from ozone absorption cross section

The authors of the IUP cross-section reported an uncertainty of 1.5% ($k=1$) for the measurements. Applying this uncertainty randomly by adding gaussian noise within 1.5% to the cross-section and retrieving TCO from the modified cross-section, a variation of TCO of less than 0.2 DU or 0.06% is observed. This low uncertainty is attributed to the convolution of the high-resolution cross-section to the FWHM of 0.5 nm and the use of a large number of measurements (305 nm to 345 nm with 0.01 nm yields 4000 fitting points).

A more pragmatic method to estimate the uncertainty regarding the cross-sections is the comparison of retrieved TCO with other available ozone absorption cross sections in the wavelength range between 305 nm and 345 nm. In order to estimate the uncertainty derived from the use of different ozone absorption cross sections, we compare TCO retrieved with the standard settings but with four other available cross sections. For comparability, the same cross sections with the same quadratic or linear parametrizations of the effective ozone temperature as in Gröbner et al. (2021) and available from the IGACO webpage (http://igaco-o3.fmi.fi/ACSO/cross_sections.html) are used and summarised as follows:

IGQ The Bass&Paur (Bass and Paur, 1985) ozone absorption cross sections from the IGACO web-page, with a quadratic parametrisation of cross section temperature (file bp.par).

DBM Daumont et al. (1993), Brion et al. (1993), and Malicet et al. (1995) published a high resolution dataset of at five temperatures between 218 K and 295 K. As in Gröbner et al. (2021) a linear parametrisation of the ozone temperature is applied, due to the lack of measurements at temperatures below 218 K.

IUPA This absorption cross sections measured by the University of Bremen in 2017 (M. Weber, personal communication in Gröbner et al, 2021) during the project European Metrology Research Program ATMOZ (Traceability of atmospheric total column ozone). The IUPA (ATMOZ) cross section was measured between 295 nm and 350 nm with improved noise characteristics in this wavelength region compared to the IUP cross section from Serdyuchenko et al. (2014).

250 However, IUP was selected by the WMO as new reference cross-section for the Dobson and Brewer network before IUPA was measured. Here and in Gröbner et al. (2021) the quadratic polynomial temperature approximation is used.

ACS Birk et al. (2018) measured a new cross section in the frame of the ESA project SEOM-IAS between 243 nm and 346 nm. The temperature range is at 193 K, 213 K, 233 K, 253 K, 273 K, and 293 K. As for IUP a quadratic polynomial temperature dependence fit is applied to parametrise the temperature dependency.

255

Figure 2 presents the relative differences between TCO retrievals with the aforementioned specific cross sections and the resulting TCO derived with the IUP cross section. Figure 2 shows the relative difference of over 3200 TCO data recorded between 20 September 2018 and 15 November 2020. The subfigures display the mean of the relative differences, indicated as offset, the standard deviation, and the seasonal variation in terms of a sinusoidal fit. TCO derived when using the different cross sections deviate in average between -0.43% and +0.31% for IGQ, DBM and IUPA cross sections respectively. The results of the ACS cross section shows that this new cross section produces a large offset in TCO compared with the other ozone absorption cross-sections. This fact is also mentioned in Gröbner et al. (2021). When comparing this cross-section with the other cross-sections, an increasing spectral variability is seen at wavelengths longer than 320 nm, thus affecting the ozone retrieval of QASUME and Dobson, while the Brewer is less affected since his longest wavelength is at 320 nm. Therefore, ACS is excluded here for the uncertainty analysis origination from cross section.

265

To account for the variability of each individual measurement and the offset, all relative differences from the three cross sections (IGQ, DBM and IUPA) are merged and the mean and standard deviation is calculated resulting in an offset of -0.15% and a standard deviation of 0.38%. Since the standard deviation is larger than the bias, we state and note in Table 1 a relative standard uncertainty of TCO retrieval from the cross sections of 0.38%.

270

3.3 Uncertainty from top of the atmosphere solar spectrum

The top of the atmosphere spectrum chosen as the standard ETS, TSIS, has an uncertainty of 1.3% at wavelengths shorter than 400 nm (Coddington, 2021). Applying this uncertainty as a gaussian noise to the ETS during the TCO retrieval process a variation of less than 0.18 DU or smaller than 0.06% of resulting TCO is obtained (again, mainly due to the large number of points used in the retrieval).

275

Since the above approach does not take into account systematic spectral uncertainties, we estimated the uncertainty in TCO retrieval by using different independent solar spectra. As in the previous section, the other standard parameters are kept constant for the TCO retrieval. The second ETS that was used is called QASUMEFTS and was at the Izana Observatory, Tenerife, Spain during September 2016 and fully described in Gröbner et al (2017) and compared in Coddington et al. (2021) with the TSIS solar spectrum. The QASUMEFTS solar spectrum has an overall uncertainty of around 1% (k=1) for the wavelength range between 310 nm and 350 nm and gradually about 2.0% (k=1) between 300 nm and 310 nm as reported in Gröbner et al. (2017) and is therefore comparable with the uncertainty from TSIS with an uncertainty of 1.3% at wavelengths shorter than 400 nm (Coddington et al., 2021).

280

Figure 3 presents the comparison of TCO retrievals from TSIS versus QASUMEFTS resulting in an offset of 0.68% in retrieved TCO with a standard deviation of -0.24%. The resulting uncertainty component is therefore 0.196% ($=0.68/2/\sqrt{3}$), assuming a rectangular uncertainty distribution with width 0.68% (Table 1). The resulting bias of 0.68% between TSIS and QASUMEFTS may be caused by spectral correlations of the QASUME measurements and the solar spectrum TSIS which are not explicitly known. This bias is in the order of 0.72%, as reported in Vaskuri et al. (2018), when a full correlation of measurement uncertainties between the spectral measurement and the extraterrestrial spectrum is assumed. Here we have chosen

285

290 “unfavorable” correlation for the measurement uncertainty, while potential larger spectral correlations of the measurement are therefore reflected here by the comparison of QASUMEFTS and TSIS resulting in an uncertainty of 0.196%.

3.4 Uncertainty from effective ozone temperature

Figure 4 shows the temperature dependency of the QASUME TCO retrieval algorithm normalized to 228 K which is taken as a climatological value by the Brewer procedure. The calculated temperature dependency shows that the sensitivity of TCO is about 0.1 %/K for IGQ, IUPA and IUP cross sections and about 0.08%/K for ASC and only 0.04%/K for DBM cross section. These values are comparable with the temperature sensitivity of the Dobson of also about 0.1%/K (Gröbner et al. 2021, Redondas et al. 2014), while the Brewer has almost no temperature dependency (e.g. for the IUP cross section).

Due to the sensitivity of TCO on effective temperature, one may assume that the temperature could be retrieved by the LSF algorithm. In this case the temperature would serve as a fitting parameter. An expanded algorithm was developed and tested. However, the retrieved effective temperature showed unreasonable variation of more than 7 K and the resulting TCO exhibit large invalid TCO for large number of spectra. Since the effective temperature cannot be retrieved by this algorithm, the temperature needs to be included as input parameter to the algorithm. Note that the effective temperature can be retrieved by the Brewer as proposed in Kerr (2002). However, in order to be independent of the Brewer, we have chosen the effective ozone temperature for Davos derived from balloon soundings in Payerne Switzerland, 220 km distant from Davos. The effective temperature input for the retrieval is measured on a two- or three days schedule and linearly interpolated for daily values. Note that the uncertainty of the ozone sondes and their traceability is not known. However, an estimate of the uncertainty is given as follows: Gröbner et al. (2021) stated a seasonal variability of the effective temperature of amplitude of 11.4 K and a mean value of 225.2 K between 2016 and 2020. This would result in an uncertainty of about 5.7 K if a constant effective ozone temperature of 225.2 K is used as a constant climatological value for the TCO retrieval. To reduce the uncertainty of TCO from this dependence on effective ozone temperature, we included the temperature in the retrieval instead of a fixed climatological value. Gröbner et al. (2021) also compared the effective ozone temperature from balloon soundings with ECMWF reanalysis data from (<https://www.temis.nl/climate/efftemp/overpass.php>) with daily data and revealed a standard deviation of 2.5 K for the period between 2016 to 2020. The differences between the two datasets are not correlated within the seasons and we therefore pragmatically consider the uncertainty of observing the temperature as 2.5 K, when using either balloon soundings or ECMWF reanalysis data. Considering this sensitivity on effective temperature of 0.1K/% for QASUME TCO measurements and the estimated uncertainty of measuring the effective ozone temperature, a general standard uncertainty for TCO of 0.25% can be stated from effective ozone temperature and included in Table 1.

3.5 Air mass

320 The standard retrieval algorithm includes the US standard atmosphere *afglus* with defined ozone profile. However, balloon soundings from Payerne, Switzerland, show that the effective ozone height can change by about 3.6 km within the seasons (Gröbner et al., 2021), resulting in a change in TCO of 0.3%. Therefore, the standard uncertainty in TCO for this parameter is estimated at $0.086\% = 0.3/2/\sqrt{3}$ (see Table 1).

3.6 Uncertainty from atmospheric pressure

325 The sensitivity of retrieved TCO on pressure changes is about 0.2% when pressure changes of 100 hPa are included in the TCO retrieval algorithm. On average, the pressure in Davos was around 840 hPa and varied between +/-7 hPa during the period of comparison, which results in a variation of TCO of 0.014%. Due to this small sensitivity of TCO on air pressure and to simplify the standard algorithm, a constant air pressure of 840 hPa was used as input parameter for the algorithm. The resulting variation of TCO is here considered as an TCO uncertainty of 0.014% from Rayleigh scattering parametrization with variable

330 ground air pressure (Table1). For locations with higher variations of air pressure, the measured pressure can be taken as the input for the algorithm, if necessary.

3.7 Uncertainty from Least Square Fit Algorithm (Computational)

As a criterion for valid TCO retrieval, residuals of the Jacobian matrix from the in-built Matlab function “lsqnonlin” are calculated indicating the 95% confidence interval of the retrieved TCO. If the value is less than 0.7 DU (or about 0.23 % at 300 DU) then the retrieval is considered as valid. If the value exceeds 0.7 DU, the measurement could have been disturbed by moving clouds, overcast sky or other atmospheric effects. The criterion of 0.7 DU indicates that TCO varies by less than 0.25% (at 300 DU). Therefore, we define the relative **standard** uncertainty of the least square fit retrieval model as $0.25\%/2=0.125\%$. (Table 1).

3.8 Overall Uncertainty

340 In section 3.1 to 3.7 the individual **uncertainty components relevant for the TOC retrieval from solar UV irradiance measurements were described and calculated. The summary and the combined uncertainty are** listed in Table 1. In order to estimate **the combined** uncertainty two methods are chosen:

a) Arithmetic calculation of overall uncertainty

345 Assuming no correlation of the individual **uncertainty components** as listed in Table 1, the **combined standard** uncertainty can be calculated by the square root of the sum of the **squares of the** individual uncertainties, **according to the Guide to the expression of uncertainty in measurement (GUM, ISO (2009)):**

$$\hat{u} = \sqrt{\sum u_i^2} \quad \text{Eq. 4}$$

350 Equation 4 results in a **combined uncertainty of 0.67%** when including all uncertainty contributions (Table 1).

b) Monte Carlo Simulation

Since TCO is derived by an atmospheric model as described in section 2.2 the **combined** uncertainty of the model and the corresponding input parameters can also be determined by a Monte Carlo simulation (Vaskuri et al., 2018). Monte Carlo simulation means that all the input parameters of the model, such as measurement, cross sections, effective ozone temperature, solar spectrum, pressure and airmass are varied within their specific uncertainties **using the specific type of distribution** as listed in Table 1. Each variation displays a realization of possible TCO retrievals. Specifically, the TCO time series between 20 September 2018 and 15 November 2020 is recalculated for each of the 3200 individual measurements by a random variation of the different retrieval model parameters. **Each data point of the** entire time series is recalculated 10 times to obtain a total number of randomly varied realizations of more than 32,000.

Figure 5a presents the standard deviation over 10 realizations for a single measurement (blue points). The black line indicates the mean **standard deviation of** all 3200 measurements of $0.62 \pm 0.16\%$ (black dashed lines). Since the **standard deviation** may be dependent on solar zenith angle and the corresponding air mass change, the **standard deviation** of each measurement is displayed as a function of air mass (Figure 5b). The cubic fit highlights **that there is a negligible dependence of the standard deviation with air mass of 0.16%, which is slightly larger at lower air masses.** Figure 6 presents the frequency distribution of the differences between TCO from the standard algorithm and **TCO from all varied input parameters resulting in $10 \times 3200 = 32,000$ realizations.** The mean of the distribution if this large number of realizations is around 0.33% with a standard deviation of 0.80%. **The bias of 0.33% (= approx. $0.68\%/2$) originates from the differences between the two selected ETS's (Figure 3), which differ by 0.68% (see section 3.3).**

370 Combining the two statistical analysis of the Monte Carlo simulation (Figures 5 and 6), we achieve an average **standard deviation** of 0.71%. **The standard deviation indicates the standard uncertainty of 0.8% retrieved from MC simulations. This estimation is in good agreement with the previous uncertainty estimation using uncorrelated quantities of 0.67 %.** The similarity of the uncorrelated and the Monte Carlo **derived** uncertainties indicates that the individual uncertainties are weakly correlated. However, they are slightly depending on the airmass. **Therefore, a standard relative uncertainty of 0.8% or expanded**
375 **uncertain of 1.6% can be used as a maximum value for TCO retrievals from solar UV irradiance measurements, based on the two independent uncertainty estimations presented here.**

4 Discussion

380 *Comparison with Dobson and Brewer:* Gröbner et al. (2021) presented a long-term comparison between automated Dobson (Stübi et al. 2020) and Brewer from the Lichtklimatologische Observatorium Arosa (LKO) and PMOD/WRC Davos TCO time series. The comparison accounted for the **same ozone absorption** cross sections as used **in our study**, the physical characteristics of the instruments (e.g. measured slit functions) and the **effective ozone temperature from balloon soundings**. The comparison revealed that the best agreement can be found when using the IUP ozone absorption cross section (Serdyuchenko et al., 2014,
385 **Gröbner et al., 2021**) showed that the comparison of TCO from Brewer and Dobson with other ozone absorption cross sections, however, revealed variation of up to 5% between these two instruments. **The comparison included however only two instrument types.** With QASUME we have introduced a third independent type of instrument for measuring TCO.

In analogy to Gröbner et al. (2021), Figure 7 presents the comparisons of the Brewer 156 double monochromator and Dobson 101 with QASUME TCO for five different cross sections. The results show that **averaged relative differences of TCO** ranges
390 between -4.06% (DBM) and 0.98% (IGQ), when comparing QASUME with the Brewer 156. **These large differences of up to 5% between the use of different ozone absorption cross sections is consistent with the findings reported by Gröbner et al. 2021 for the comparison between Brewer and Dobson.**

On the other hand, the comparison between Dobson and QASUME ranges between -1.01% (IUP) to - 0.72% (DBM), which is significantly smaller than the variation **seen between Brewer and QASUME**. The variability of 5.04% for the Brewer-
395 QASUME comparison and the much lower variability of 0.29% for the Dobson-QASUME comparison **indicate that the TCO retrieval by Dobson and QASUME have a similar response to the cross sections studied here.** The Brewer is more sensitive to some of the ozone absorption cross sections (e.g. DBM, ACS and IUPA) than on IGQ and IUP. It remains speculative if the sensitivity originates from the instrument characteristics or the cross section at the specific wavelength or both. We only can conclude that the response on the cross sections is similar for the Dobson as for QASUME, which might lead to a lower
400 **sensitivity to spectral errors in the ozone absorption cross-sections.**

Additionally, Figure 8 presents the dependency of the differences of TCO **retrieved with the IUP cross section with respect to the ozone** slant path column, which is defined as the multiplication of air mass and TCO. **While Brewer and QASUME show the same slant path dependency, the comparison between QASUME and Dobson shows a slight roll-off at larger slant path, with the Dobson measuring lower TCO values. This is probably caused by spectral stray light contamination in the Dobson**
405 **monochromator, as reported in (Komhyr et al., 1986). Similar slant path dependencies for the Brewer and the Dobson are found also when retrieving TCO with other cross sections indicating that the slant path dependency is less sensitive on the selected cross section than the offset of the averaged differences.**

As concluded by Gröbner et al. (2021), the IUP cross section shows the best consistency between Brewer and Dobson of less than 0.21%. However, Figure 7 shows that QASUME over-estimates TCO by about 1% (Dobson) and 1.2% (Brewer), **which**
410 **is 1% and 0.8% larger than the comparison between Dobson and Brewer, respectively. We clearly see that the independent instrument and retrieval procedure, which is a distinct different retrieval approach compared to the double ratio technique for Brewer and Dobson, agree with the ground based TCO retrieval from the established instruments to within 1% as shown in**

Figure 7. The observed offset of 1% in the TCO retrieved by QASUME with respect to the Brewer (using IUP cross section for both) is also confirmed by preliminary comparisons performed at the Observatory in Izãna, Tenerife, Spain in September 2016 and in El Arenosillo in June 2019 in Southern Spain. The final approved results are foreseen to be published in a WMO report (Nr. 274, in preparation). One may assume that ground based TCO observations may result in same values independent on the instrument and retrieval algorithm if the effect of the different cross sections is negligible as seen for the Dobson (Figure 7). We have undertaken many efforts to detect the potential source (e.g. Angstrom parametrization instead of linear parametrization) of this bias, but we could not explain the observed bias of 1%. However, the offset of 1% between the TCO from QASUME relative to Brewer and Dobson is well within the uncertainties of the TCO retrieval of 1.6% (expanded uncertainty, with 95% coverage interval) of QASUME. If the uncertainties of the Dobson and Brewer TCO retrieval are assumed to be 1%, then the combined uncertainty of 1.9% clearly demonstrates the consistency of the three instruments to within their uncertainties.

5 Conclusion

We have introduced traceable TCO ground based retrievals from direct solar spectral UV irradiance measurements in the wavelength range between 305 nm and 345 nm. The QASUME spectroradiometer used for this study is calibrated in the laboratory based on an unbroken traceability chain to SI and the TCO retrieval algorithm is standardized. The combined standard uncertainty of 0.8% is quantified by the uncertainties from the radiometric quantities, the instrument characteristics and the various uncertainties of the retrieval model. The expanded relative uncertainty is 1.6% ($k=2$, representative for a coverage interval of 95%). The Monte Carlo simulation of the uncertainties revealed that the parameters affecting the uncertainty are weakly correlated and the combined uncertainty can therefore be calculated by the square root of the sum of the squares of the individual uncertainty parameters according to GUM (ISO, 2009):

The calibration and stability of QASUME is regularly verified in the field and in the laboratory using proven radiometric calibration techniques (Hülse et al., 2016), thereby allowing a TCO retrieval with known uncertainties without requiring recalibrations with respect to other reference instruments, as is the case for the Brewer and Dobson networks.

The Arosa/Davos time series consist of a triad of Dobson and a triad of Brewer (Stählin et al. 2018). This triad of two instrument types is now complemented with an instrument traceable to the SI providing independent traceable TCO values from a distinct different TCO retrieval algorithm with well established uncertainties. When using the IUP ozone absorption cross sections, QASUME agrees with Brewer and Dobson within 1% in a long-term comparison in Davos, which is within their combined uncertainties. Further studies are necessary to validate the TCO retrieval using this method at other locations worldwide with different atmospheric compositions such as higher aerosol loads and different effective ozone temperatures.

Competing interests. The authors declare that they have no conflict of interest.

Acknowledgement: We thank the two anonymous reviewers for the helpful comment, who substantially improved this publication.

This research has been supported by the ESA project QA4EO, grant no. QA4EO/SER/SUB/09) and by GAW-CH MeteoSwiss (project INFO3RS, grant no. 123001926).

Author contributions: LE and JG developed the QASUME retrieval algorithm, analysed the data and have written the manuscript. GH operated QASUME at PMOD/WRC. HS and RS were responsible for the Brewer and Dobson measurements used in this study.

Data availability: The data is available from the main author (LE) on request.

Code availability: The MatSHIC and TCO retrieval algorithm is available from the main author (LE) on request.

References

- 460 Bais, A. F., McKenzie, R. L., Bernhard, G., Aucamp, P. J., Ilyas, M., Madronich, S., and Tourpali, K.: Ozone depletion and climate change: impacts on UV radiation, *Photochemical & Photobiological Sciences*, 14, 19-52, 10.1039/C4PP90032D, 2015.
- Bais, A. F., Bernhard, G., McKenzie, R. L., Aucamp, P. J., Young, P. J., Ilyas, M., Jöckel, P., and Deushi, M.: Ozone–climate interactions and effects on solar ultraviolet radiation, *Photochemical & Photobiological Sciences*, 18, 602-640, 10.1039/C8PP90059K, 2019.
- 465 Basher, R. E.: Review of the Dobson spectrophotometer and its accuracy, WMO Global Ozone Research and Monit, Project, Report No. 13., Geneva, 1982.
- Bass, A. M. and Paur, R. J.: The ultraviolet cross-sections of ozone, I – The measurements, II – Results and temperature dependence, in: Atmospheric Ozone, edited by: Zerefos, C. S. and Ghazi, A., Springer, Dordrecht, The Netherlands, 606–616, https://doi.org/10.1007/978-94-009-5313-0_120, 1985.
- 470 Birk, M. and Wagner, G.: ESA SEOM-IAS – Measurement and ACS database O3 UV region, Version I, [Data set], Zenodo, <https://doi.org/10.5281/zenodo.1485588>, 2018.
- 475 Bodhaine, B. A., Wood, N. B., Dutton, E. G., and Slusser, J. S.: On Rayleigh Optical Depth Calculations, *J. Atmos. Ocean. Tech.*, 16, 1854–1861, 1999.
- Brion, J., Chakir, A., Daumont, D., Malicet, J., and Parisse, C.: High-resolution laboratory absorption cross section of O₃, Temperature effect, *Chem. Phys. Lett.*, 213, 610–612, 1993.
- 480 Coddington, O. M., Richard, E. C., Harber, D., Pilewskie, P., Woods, T. N., Chance, K., et al. (2021). The TSIS-1 Hybrid Solar Reference Spectrum. *Geophysical Research Letters*, 48, e2020GL091709. <https://doi.org/10.1029/2020GL091709>, 2021
- 485 Daumont, D., Brion, J., Charbonnier, J., and Malicet, J.: Ozone UV spectroscopy I: Absorption cross-sections at room temperature, *J. Atmos. Chem.*, 15, 145–155, 1992.
- Dobson G M B 1968 Forty years research on atmospheric ozone at Oxford – a history *Appl. Optics* 387-405
- 490 Dobson G M B 1931 A photoelectric spectrophotometer for measuring the amount of atmospheric ozone *Proceedings of the Physical Society* 43 324
- Gkertsi, F., Bais, F. A., Kouremeti, N., Drosoglou, T., Fountoulakis, I., and Fragkos, K.: DOAS-based total column ozone retrieval from Phaethon system, *Atmospheric Environment*, 2018
- 495 Gröbner J., Schreder J., Kazadzis S., Bais A. F., Blumthaler M., Görts P., Tax R., Koskela T., Seckmeyer G., Webb A. R., and Rembges D.: Traveling reference spectroradiometer for routine quality assurance of spectral solar ultraviolet irradiance measurements, *Appl. Opt.*, 44, 5321–5331, 2005.
- 500 Gröbner, J. and Peter Sperfeld: Direct traceability of the portable QASUME irradiance scale to the primary irradiance standard of the PTB, *Metrologia* 42 134, 2005
- 505 Gröbner, J., Kröger, I., Egli, L., Hülsen, G., Riechelmann, S., and Sperfeld, P.: A high resolution extra-terrestrial solar spectrum determined from ground-based solar irradiance measurements, *Atmos. Meas. Tech.*, 10, 3375–3383, 2017, <https://doi.org/10.5194/amt-10-3375-2017>, 2017.
- Gröbner, J., Schill, H., Egli, L., and Stübi, R.: Consistency of total column ozone measurements between the Brewer and Dobson spectroradiometers of the LKO Arosa and PMOD/WRC Davos, *Atmos. Meas. Tech.* 3319–3331, <https://doi.org/10.5194/amt-14-3319-2021>, 2021
- 510 Huber, M., Blumthaler, M., Ambach, W., and Staehelin, J.: Total atmospheric ozone determined from spectral measurements of direct solar UV irradiance, 22, 53-56, 10.1029/94gl02836, 1995.
- 515 Herman, J., Evans, R., Cede, A., Abuhassan, N., Petropavlovskikh, I., McConville, G., Miyagawa, K., and Noiro, B.: Ozone comparison between Pandora #34, Dobson #061, OMI, and OMPS in Boulder, Colorado, for the period December 2013–December 2016, *Atmos. Meas. Tech.*, 10, 3539–3545, <https://doi.org/10.5194/amt-10-3539-2017>, 2017.

- 520 Hermans, C., Vandaele, A.C., and Fally, S.: Fourier Transform measurements of SO₂ absorption cross sections: I. Temperature dependence in the 24 000 - 29 000 cm⁻¹ (345-420 nm) region. *Journal of Quantitative Spectroscopy and Radiative Transfer*. 110. 756-765. 2019.
- Hülsen, G., Gröbner, J., Nevas, S., Sperfeld, P., Egli, L., Porrovecchio, G., and Smid, M.: Traceability of solar UV measurements using the QASUME reference spectroradiometer, *Appl. Optics*, 55, 7265–7275, 2016
- 525 *ISO/IEC Guide 98-1:2009: Guide to the expression of uncertainty in measurement (GUM)*, <https://www.iso.org/standard/46383.html>, 2009.
- 530 Kerr, J. B., Asbridge, I. A., Evans, W. F. J.: Intercomparison of total ozone measured by the Brewer and Dobson Spectrophotometers at Toronto *J. Geophys. Res.*, 93(D9), 11,129– 11,140, 1988
- Kerr, J. B., McElroy, C. T., Olafson, R. A.: Measurements of total ozone with the Brewer spectrophotometer *Proc. Quad. Ozone Symp.*, 1980, J. London (ed.), Natl. Cent. for Atmos. Res., Boulder CO, 74-79, 1981
- 535 Kerr, J. B., McElroy, C. T., Wardle, D. I., Olafson, R. A., Evans, W. F.J.: The automated Brewer Spectrophotometer *Proceed. Quadr. Ozone Symp.* in Halkidiki, C.S. Zerefos and A. Ghazi (Eds.), D. Reidel, Norwell, Mass., pp. 396-401, 1985
- 540 *Kerr, J. B.: New methodology for deriving total ozone and other atmospheric variables from Brewer spectrophotometer direct sun spectra, J. Geophys. Res.*, 107(D23), 4731, <https://doi.org/10.1029/2001JD001227>, 2002.
- Komhyr, W. D., Grass, R. D., and Leonard, R. K.: Dobson Spectrophotometer 83: A Standard for Total Ozone Measurements, 1962–1987, *J. Geophys. Res.*, D7(94), 9847–9861, 1989.
- 545 Köhler U 2002 Europäisches Dobson Kalibrierzentrum Hohenpeißenberg garantiert hohe Datenqualität Ozonbulletin des Deutschen Wetterdienstes Nr. 87
- Köhler, U., Nevas, S., McConville, G., Evans, R., Smid, M., Stanek, M., Redondas, A., and Schönenborn, F.: Optical characterisation of three reference Dobsons in the ATMOZ Project – verification of G. M. B. Dobson’s original specifications, *Atmos. Meas. Tech.*, 11, 1989-1999, <https://doi.org/10.5194/amt-11-1989-2018>, 2018.
- 550 Molina, M. J., and F. S. Rowland: Stratospheric sink for chlorofluoromethanes-Chlorine atom catalyzed destruction of ozone, *Nature*, 249, 810– 812, 1974.
- 555 NOAA: National Oceanic and Atmospheric Administration (NOAA), US Standard Atmosphere, NOAA-S/T 76-1562, 1976.
- Redondas A, Evans R, Stübi R, Köhler U and Weber M 2014 Evaluation of the use of five laboratory-determined ozone absorption cross sections in Brewer and Dobson retrieval algorithms *Atmos. Chem. Phys.*, 14, 1635–1648
- 560 Seckmeyer, G., L., L. R., C., G., W., H. J., and M., S.: Biologische und medizinische Wirkungen solarer Bestrahlung - Biological and medical effects of solar radiation, *promet Meteorologische Fortbildung DWD*, 2018.
- Stahelin, J., N. Harris, C. Appenzeller, and J. Eberhard: Ozone trend: A review, *Rev. Geophys.*, 39(2), 231– 290, 2001.
- 565 Stahelin, J., Viatte, P., Stübi, R., Tummon, F., and Peter, T.: Stratospheric ozone measurements at Arosa (Switzerland): history and scientific relevance, *Atmos. Chem. Phys.*, 18, 6567–6584, <https://doi.org/10.5194/acp-18-6567-2018>, 2018.
- Stübi, R., Schill, H., Klausen, J., Maillard Barras, E., and Haefele, A.: A fully Automated Dobson Sun Spectrophotometer for total column ozone and Umkehr measurements, *Atmos. Meas. Tech. Discuss.* [preprint], <https://doi.org/10.5194/amt-2020-391>, in review, 2020.
- 570 Serdyuchenko, A., Gorshchev, V., Weber, M., Chehade, W., and Burrows, J. P.: High spectral resolution ozone absorption crosssections–Part 2: Temperature dependence, *Atmos. Meas. Tech.*, 7, 625–636, <https://doi.org/10.5194/amt-7-625-2014>, 2014.
- 575 Solomon, S.: Stratospheric ozone depletion: A review of concepts and history, *Rev. Geophys.*, 37, 275–316, 1999
- Slaper, H., Reinen, H., Blumthaler, M. Huber, M. Kuik, F. 1995. Comparing Ground-Level Spectrally Resolved Solar UV Measurements Using Various Instruments: A Technique Resolving Effects of Wavelength Shift and Slit Width. *Geophysical Research Letters - GEOPHYS RES LETT*. 22. 2721-2724. [10.1029/95GL02824](https://doi.org/10.1029/95GL02824).
- 580 Thompson, D., Seidel, D., Randel, W. et al. The mystery of recent stratospheric temperature trends. *Nature* 491, 692–697 (2012). <https://doi.org/10.1038/nature11579>
- Vaniček, K., Metelka, L., Skřivánková, P., and Staněk, M.: Dobson, Brewer, ERA-40 and ERA-Interim original and merged total ozone data sets – evaluation of differences: a case study, Hradec Králové (Czech), 1961–2010, *Earth Syst. Sci. Data*, 4, 91–100, <https://doi.org/10.5194/essd-4-91-2012>, 2012.
- 585 Vaskuri, A., Kärhä, P., Egli, L., Gröbner, J., and Ikonen, E.: Uncertainty analysis of total ozone derived from direct solar irradiance spectra in the presence of unknown spectral deviations, *Atmos. Meas. Tech.*, 11, 3595-3610, [10.5194/amt-11-3595-2018](https://doi.org/10.5194/amt-11-3595-2018), 2018.
- 590 WMO (World Meteorological Organization), *Scientific Assessment of Ozone Depletion: 2018*, Global Ozone Research and Monitoring Project – Report No. 58, 588 pp., Geneva, Switzerland, 2018.

Young, P.J., Harper, A.B., Huntingford, C. et al. The Montreal Protocol protects the terrestrial carbon sink. *Nature* 596, 384–388 (2021). <https://doi.org/10.1038/s41586-021-03737-3>

595

Zerefos, C. S.: Long-term ozone and UV variations at Thessaloniki, Greece, *Phys. Chem. Earth A/B/C*, 27, 455–460, doi: 10.1016/S1474-7065(02)00026-8, 2002.


600

Zuber, R., Ribnitzky, M., Tobar, M., Lange, K., Kutscher, D., Schrepf, M., Niedzwiedz, A., and Seckmeyer, G.: Global spectral irradiance array spectroradiometer validation according to WMO, *Measurement Science and Technology*, 2018a.

605


Zuber, R., Sperfeld, P., Riechelmann, S., Nevas, S., Sildoja, M., and Seckmeyer, G.: Adaption of an array spectroradiometer for total ozone column retrieval using direct solar irradiance measurements in the UV spectral range, *Atmos. Meas. Tech.*, 11, 2477–2484, <https://doi.org/10.5194/amt-11-2477-2018>, 2018, 1–12, 10.5194/amt-2017-240, 2018b

Zuber, R., Köhler, U., Egli, L., Ribnitzky, M., Steinbrecht, W., and Gröbner, J.: Total ozone column intercomparison of Brewers, Dobsons, and BTS-Solar at Hohenpeißenberg and Davos in 2019/2020, *Atmos. Meas. Tech.*, 14, 4915–4928, <https://doi.org/10.5194/amt-14-4915-2021>, 2021.

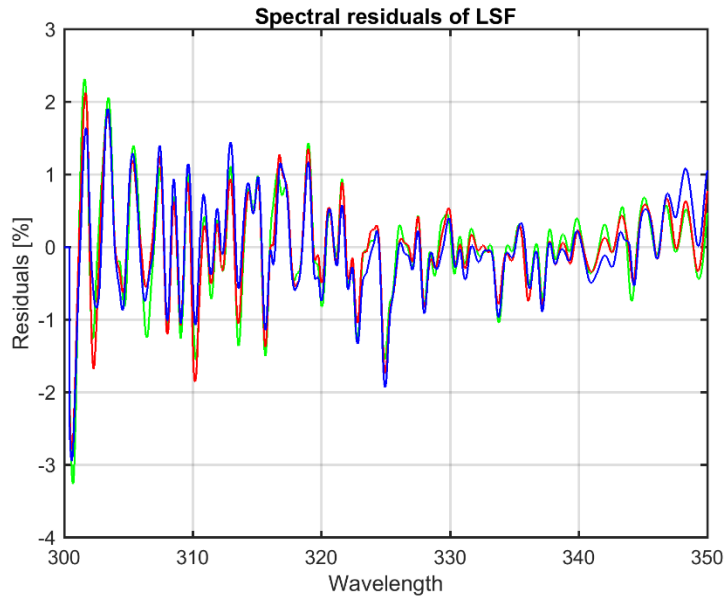

610

Figure 1: Spectral residuals of the measured and the modelled spectra of the best fit from the LSF algorithm. The exemplary figure shows three spectra at local noon and retrieved TCO of 303 DU. The average of the residuals of the irradiance over all wavelengths are less than 0.5%.

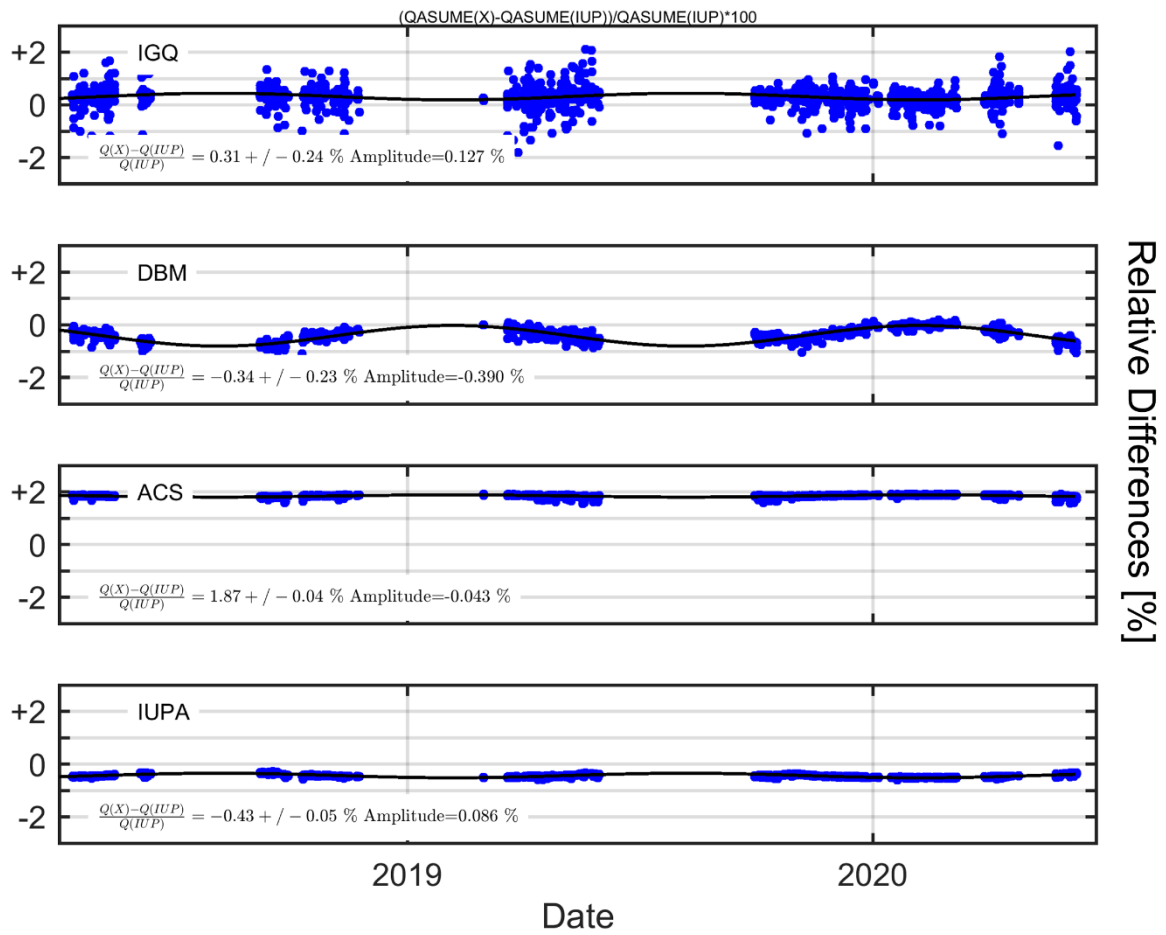

615

Figure 2: Differences (in %) of systematic offset, point to point variability (+/-) and seasonal variation (amplitude) of TCO retrieval of different cross sections compared with the IUP standard cross section.

620

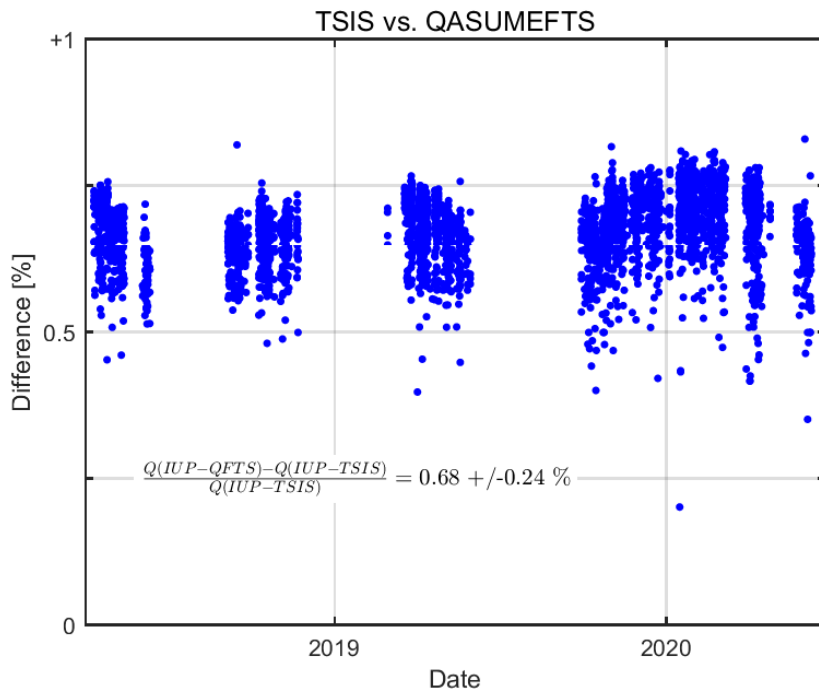


Figure 3: Differences between TSIS extraterrestrial spectrum and QASUMEFTS with IUP cross section displaying the uncertainty originating from the selection of the solar spectrum.

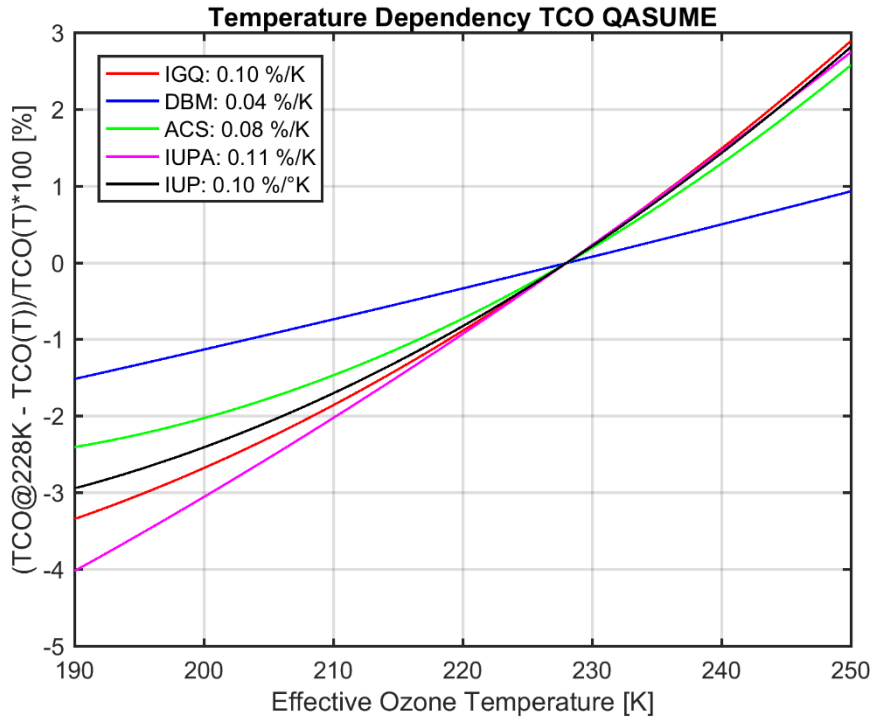


Figure 4: Dependency on effective ozone temperature of five different cross sections



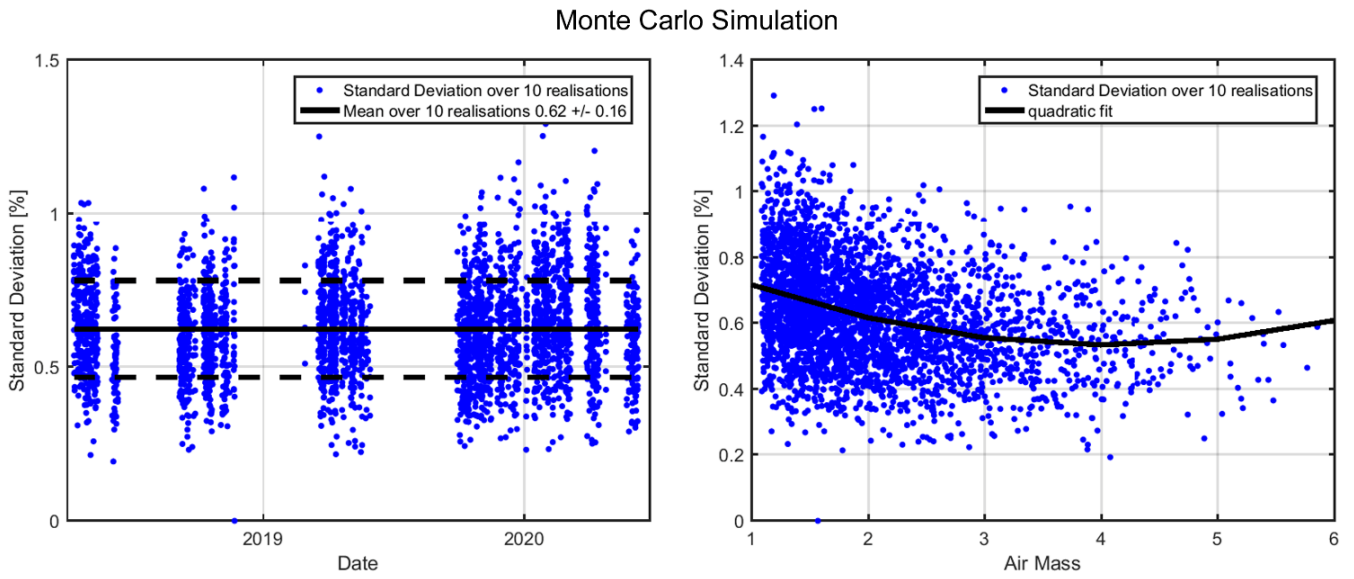


Figure 5: Results of the 32'000 realisations of TCO from Monte Carlo simulation (MC). The left panel shows the standard deviation of 10 realizations for each measurement points and the right panel indicates the dependency on airmass

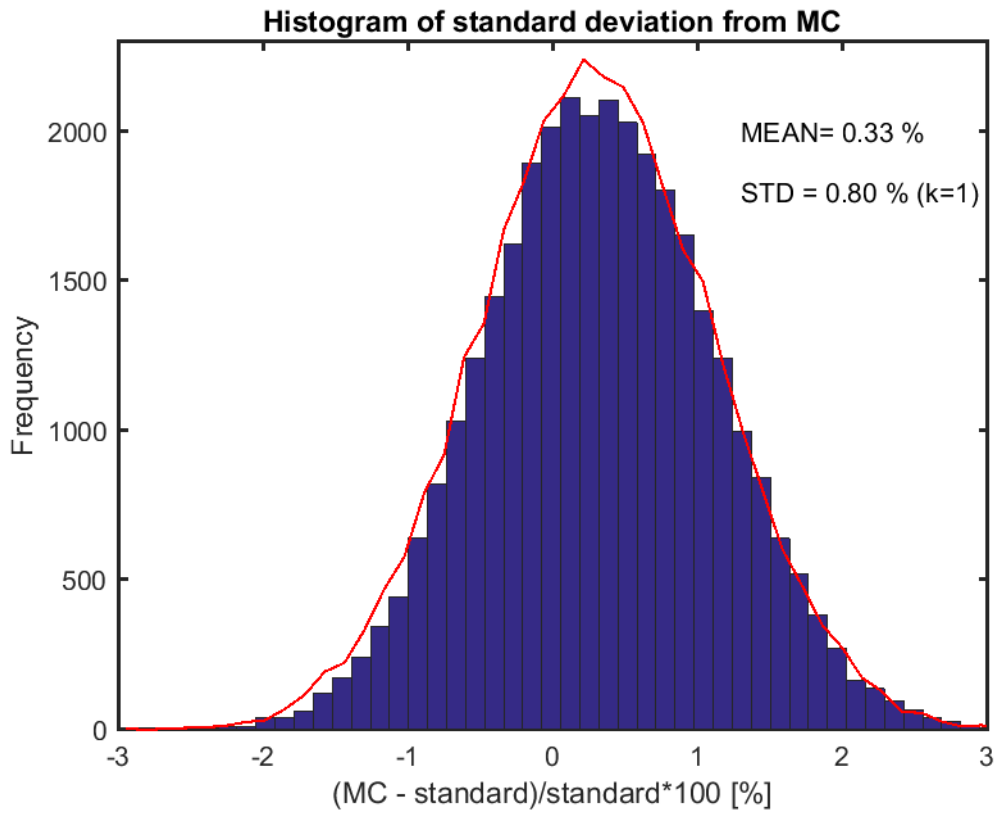


640

Figure 6: Histogram of all realizations from the Monte Carl Simulation indicating an overall uncertainty of 0.8% (standard deviation of differences) of traceable TCO measurements with QASUME. The red line indicates a randomly generated gaussian distribution.

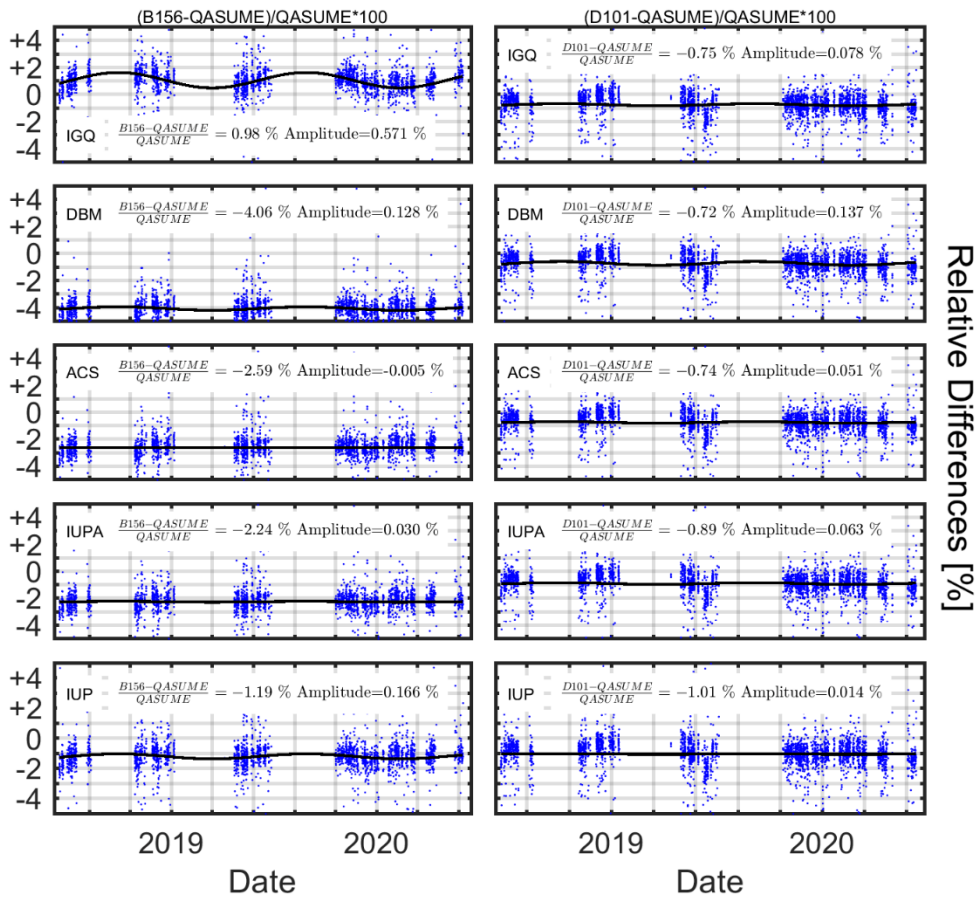

645

Figure 7: Comparison of TCO from Brewer 156 (left panels) and Dobson 101 (right panel) with TCO from traceable QASUME TCO retrieval for five different cross sections.

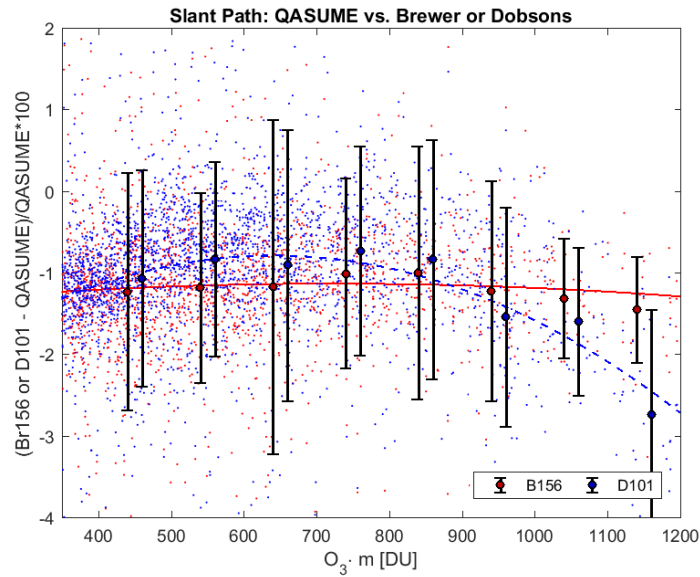

650 Figure 8: Differences of Brewer 156 and Dobson 101 retrieved with IUP cross section compared with QASUME TCO depending on the ozone slant path. The comparison with Brewer shows neglectable straylight effects.

Uncertainty Parameter	Type / distribution	Input Uncertainty (k=1)	Standard relative Uncertainty of TCO in %
Measurement	normal	0.91%	$u_1 = 0.42\%$
Ozone absorption cross section	Rectangular	4 cross sections	$u_2 = 0.38\%$
Effective Ozone Temperature	normal	0.1%/K for +/-2.5°K	$u_3 = 0.25\%$
Computational	Rectangular	<0.125%	$u_4 = < 0.125\%$
ETS	Rectangular	0.68%	$u_5 = 0.196\%$
Pressure	normal	0.002%/hPa for +/- 7 hPa	$u_6 = 0.014\%$
Ozone air mass	Rectangular	0.15%	< 0.085%
Total combined standard uncertainty (k=1)	$\hat{u} = \sqrt{\sum u_i^2}$		$\hat{u} = 0.67\%$
Expanded uncertainty (k=2)			1.3 %

655 Table 1: Uncertainty budget for the TCO retrieval by the LSF Algorithm applied to the QASUME spectroradiometer.