



A Method for Liquid Spectrophotometric Measurement of Various Forms of Iron and Copper in Ambient Aerosols

Yuhan Yang¹, Dong Gao², Rodney J. Weber¹

¹Earth and Atmospheric Sciences, Georgia Institute of Technology, Atlanta, 30331, USA

5 ²Department of Environmental Health Sciences, School of Public Health, Yale University, New Haven, 06510, USA

Correspondence to: Professor Rodney J. Weber, Ph.D. (rodney.weber@eas.gatech.edu)

Abstract. Determination of transition metals in ambient aerosols is important due to their toxicity to human health. However, the traditional measurement techniques for metal analysis are often costly and require sophisticated instruments. In this study, we developed and verified relatively low-cost liquid spectrophotometric methods for the measurements of iron (Fe) and copper
10 (Cu), often the two most abundant transition metals in ambient fine particulate matter (PM_{2.5}). For Fe analysis, we utilized a ferrozine based colorimetric method, which has been frequently used for water-soluble (WS) Fe determination, and further extended this approach for the measurement of total Fe (water-soluble + water-insoluble). In this method, Fe is quantified through the formation of a light-absorbing ferrozine-Fe(II) complex (absorbance at 562 nm). A similar colorimetric method, which forms a bathocuproine-Cu(I) complex absorbing light at 484 nm, was developed and examined for measurement of WS
15 and total Cu. These methods were applied to 24-hour integrated filter samples collected in urban Atlanta. Based on PM_{2.5} ambient aerosols, total and water-soluble Fe and Cu concentrations were in good agreement with inductively coupled plasma mass spectrometry (ICP-MS) measurements (slopes 1.0 ± 0.1 , $r^2 > 0.89$). The water-soluble components, operationally defined as those species in the aqueous filter extract that pass through a 0.45 μm pore filter, were further characterized by ultrafiltration, which showed that roughly 85 % of both the Fe and Cu in the water-soluble fraction was composed of components smaller
20 than nominally 4 nm.

1 Introduction

Transition metals are known to contribute to airborne particle toxicity and can cause a wide range of adverse health effects (Chen et al., 2018; Gonet and Maher, 2019). Iron (Fe) and copper (Cu) are often two of the most abundant transition metals in ambient fine particles (PM_{2.5}) and have been linked to a number of human diseases associated with the respiratory,
25 cardiovascular, and central nervous systems (Calderón-Garcidueñas et al., 2019; Dreher et al., 1997; Wang et al., 2007). They have also been associated with other organ damage (Kim et al., 2013; Schrand et al., 2010). Transition metals in ambient aerosols are emitted in a variety of chemical forms, such as metal oxides, metal sulfates, metal halides, metal organics, and reactive nano-metalloid particles (Gonet and Maher, 2019; Sutto, 2018). Fe and Cu nanoparticles ($< 0.1 \mu\text{m}$) may be especially toxic due to unique surface properties, combined with their small sizes that allow them to pass through cellular membranes



30 and ability to be translocated to other organs (Bongaerts et al., 2020; Lee et al., 2020; Moreno-Ríos et al., 2021). Water-soluble species are operationally defined and are obtained through aqueous dissolution of collected aerosols followed by liquid filtration of the extract solution (typical filter pore sizes of 0.22 or 0.45 μm), which is roughly analogous to the process particles undergo when deposited in the respiratory tract lining fluid. Metals measured in this fraction can include molecules and colloidal nanoparticles that are more readily bioavailable than insoluble species. Studies have found that water-soluble transition metals, including WS Fe and Cu, have stronger adverse health associations than the corresponding water-insoluble components (Costa and Dreher, 1997; Frampton et al., 1999; Huang et al., 2003; Ye et al., 2018). Transition metal ions that can form dissolution of aerosol components, such as Fe(II) and Fe(III) and Cu(I) and Cu(II), are highly redox-active components of $\text{PM}_{2.5}$. These ions can trigger and sustain catalytic reaction cycles, such as Fenton reactions, generating reactive oxygen species (ROS; OH, O_2^- , HO_2 , O_3 , and H_2O_2) *in vivo* (Brewer, 2007; Lakey et al., 2016), which can induce oxidative stress and further lead to inflammatory responses and a subsequent host of adverse health effects (Brook et al., 2010; Donaldson et al., 2001; Ghio et al., 2012; Nel, 2005).

Transition-metal-bearing particles are emitted by a wide variety of sources. Major Fe sources include resuspended mineral and road dust (tire and brake wear), and combustion of biomass and fossil fuels (Khillare and Sarkar, 2012; See et al., 2007; Wang et al., 2016). Cu sources are often dominated by traffic road dust and in certain locations by industrial sources (Adachi and Tainosho, 2004; Khillare and Sarkar, 2012; Kulshrestha et al., 2009; Lee and Hieu, 2011; Wang et al., 2016). Water-soluble transition metals may originate from primary emissions, such as combustion (e.g., WS Fe), but secondary processing is likely the major source. This can occur by dissolution of the various insoluble forms of the metals emitted as primary emissions, for example, dissolution of metal oxides to soluble forms as the particles age in the atmosphere (Alves et al., 2020; Fang et al., 2015; Galon-Negru et al., 2019; Ito et al., 2019; Meskhidze et al., 2005; See et al., 2007; Wong et al., 2020).

50 Measuring transition metals in ambient aerosols is challenging due to their low concentrations (10's of ng m^{-3} or less). Various analytical methods have been utilized. X-ray fluorescence (XRF) and particle-induced X-ray emission analysis (PIXE) are non-destructive but can be influenced by matrix effects that result in major interferences (Lin and Luo, 1979). Inductively coupled plasma mass spectrometry (ICP-MS) is widely used for quantifying trace elements and is included in some federal reference methods for the identification of metals in water and ambient PM in the US (e.g. Method IO-3.5, USEPA Method 1640) (Ammann, 2007; Chow, 1995; Danadurai et al., 2011). Overall, these instruments tend to be expensive, making it challenging to do routine analysis of large numbers of aerosol particle samples in modestly equipped laboratories.

An alternative approach is liquid-based colorimetric methods, which can provide precise and accurate measurements of specific metal species based on the assumption that the ligand used reacts exclusively with the target metal (i.e., in this case Fe or Cu) to form a light-absorbing complex. Stookey (1970) developed a spectrophotometric method for the analysis of Fe(II) based on Fe(II) complexing with a ferrozine ligand (3-(2-pyridyl)-5,6-bis(4-phenylsulfonic acid)-1,2,4-triazine) that absorbs light at 562 nm. Smith and Wilkins (1953) reported a colorimetric reagent, bathocuproine (2,9-dimethyl-4,7-diphenyl-1,10-phenanthroline), that can selectively chelate with Cu(I). The absorption spectra of the bathocuproine-Cu(I) complex display a maximum value at 484 nm. Both techniques have been developed and used to detect Fe and Cu in natural waters (Moffett et



al., 1985; Viollier et al., 2000), however, use of the Fe-ferrozine approach is much more common and has also been utilized
65 for measurements of ambient aerosols (Kuang et al., 2019; Majestic et al., 2006; Oakes et al., 2010; Rastogi et al., 2009; Zhu
et al., 1997; Zhuang et al., 1992). These analytical techniques can be applied to relatively small liquid spectrophotometers that
utilize a long path Liquid Waveguide Capillary Cell (LWCC) for high sensitivity. Although only able to measure a specific
compound per analysis, in contrast to mass spectrometer methods, the instrument is small, portable, and relatively low cost
and can be used for offline measurements of sample extracts or for online measurement when connected to a particle-into-
70 liquid sampler (PILS) or similar system (Oakes et al., 2010; Rastogi et al., 2009). Here we report on the development,
verification and application of liquid spectrophotometers for measurement of Fe and Cu in ambient aerosols collected on filters.

2 Methods

2.1 Collection of Ambient PM_{2.5} filters

One-year of filter collection was conducted throughout 2017 at the Jefferson Street (JST) site located ~ 4 km northwest of
75 downtown Atlanta, Georgia. The JST site is surrounded by a mixed commercial/residential area and has a characteristic urban
signature (Hansen et al., 2003). A total of 355 PM_{2.5} filter samples were collected with high-volume (Hi-Vol) samplers (Thermo
Anderson, flow rate normally 1.13 m³/min), each filter collected over a 24 h period (midnight to midnight) using prebaked
(maximum T = 550 °C) quartz filters (Pallflex® Tissuquartz™, 8×10 inches) with an effective collection area of 516.13 cm²
(20.32 cm by 25.40 cm). Samples were immediately wrapped in prebaked aluminum foil and stored at -18 °C until analysis.
80 A selection of these filters are included in the following analyses. A suite of other air quality sampling instruments was also
operational during the filter sampling period. Portions of these filters have already been utilized in studies on aerosol oxidative
potential (Gao et al., 2020; Gao et al., 2019).

2.2 Reagents and standards

All acids and sodium hydroxide (NaOH) used were trace metal grade obtained from VWR International LLC (Radnor, PA,
85 USA). Standard stock solutions for Fe and Cu calibrations were prepared by dilution of commercially available standards
(1000 ppm in 2 % HCl obtained from RCCA chemical company, Arlington, TX, USA) and stored in a refrigerator (T = 4 °C).
Calibration with these standards was performed at the beginning of every measurement day. Ammonium acetate (C₂H₇NO₂)
was obtained from Fisher Scientific International Inc. (Fair Lawn, New Jersey, USA), and ferrozine (3-(2-pyridyl)-5,6-bis (4-
phenylsulfonic acid)-1,2,4-triazine) from the HACH company (Loveland, CO, USA). Bathocuproine (2,9-dimethyl-4,7-
90 diphenyl-1,10-phenanthroline), sodium citrate dihydrate (HOC(COONa)(CH₂COONa)₂·2H₂O) and hydroxylamine
hydrochloride (HONH₂·HCl) were obtained from Sigma Aldrich (St. Louis, MO, USA). Details of the chemical preparations
are provided in the Supplement.



2.3 Spectrophotometer and LWCC system

Similar spectrophotometric instruments were used for all measurements (WS and total Fe and Cu). The final mixture containing
95 the light-absorbing complexes were pushed into a Liquid Waveguide Capillary Cell (LWCC-3250/ LWCC-3100, World
Precision Instrument, Sarasota, FL). The waveguide was coupled at one end to a dual deuterium and tungsten halogen light
source (DT-Mini-2, Ocean Optics, Dunedin, FL), which produced light over the wavelength range of 200 to 800 nm, and at
the other end to a multi-wave light detector (USB4000, Ocean Optics, Dunedin, FL), using 400 μm fiber core-diameter fiber
optic cables (QP400-2-SR, Ocean Optics, Dunedin, FL). The light absorbance was recorded with a data requisition software
100 (SpectraSuite). For Fe analysis, the light absorption over the wavelength range between 557 nm and 567 nm was measured
and averaged as the absorbance of the Fe complex in the sample (Abs_{562}). Average absorption between wavelengths of 479
nm to 489 nm was recorded and referenced to as the absorbance for Cu measurements (Abs_{484}). In both measurements, the
average absorbance measured over the wavelength range of 695 nm to 705 nm (Abs_{700}) was chosen as the baseline absorbance.
Since the light absorption efficiencies of Fe(II)-ferrozine and Cu(I)-bathocuproine complexes differed, the optical path lengths
105 of the LWCC for Fe and Cu measurements were 100 cm (LWCC-3100) and 250 cm (LWCC-3250), respectively. To keep the
light absorption within an optimal range, the recommended Fe(II) and Cu(I) liquid concentrations detected by the system are
up to 40 and 50 ppb, respectively.

The metal concentrations in the liquid (C) were determined based on the light absorbances by:

$$C = \frac{1}{b} [(Abs_{\lambda} - Abs_{700}) - a]. \quad (1)$$

110 Where Abs_{λ} represents the average light absorption of the sample (or blank) for the ranges given above, which encompasses
the wavelength (λ) at which maximum optical absorption occurs; for Fe, $\lambda = 562 \text{ nm}$, and for Cu, $\lambda = 484 \text{ nm}$. Abs_{700}
represents the average light absorption between 695 to 705 nm, a (arbitrary units) and b ($1/\text{ng mL}^{-1}$) are the intercept and slope
of the calibration curve, respectively.

The final ambient concentration of each element, C_{air} (ng m^{-3}), was calculated by:

$$115 \quad C_{air} = (C_{sample} - C_{blank}) \frac{V_l}{V_s} \times \frac{V_e}{V_{air}} \times \frac{A_{filter}}{A_{punch}}. \quad (2)$$

Where C_{sample} and C_{blank} are the liquid sample and blank concentrations of the specific element (ng mL^{-1}), determined by
Eq. (1), V_e (mL) is the liquid volume of the sample (or blank) extract, V_s (mL) is the liquid extract volume used for the actual
measurement, and V_l (mL) is the volume of liquid sample solution after being diluted by all the chemicals (i.e. $V_l = V_s +$
 $V_{chemicals}$). V_{air} (m^3) is the volume of air drawn through the filter during sampling. A_{filter} (cm^2) and A_{punch} (cm^2) are the
120 total areas of the Hi-Vol filter and the filter punches used for analysis, respectively.



2.4 Filter extraction

2.4.1 Extraction for water-soluble metals and ultrafiltration

For measurements of the water-soluble Fe and Cu collected on the filters, one circular filter punch (1 inch in diameter, $A_{punch} = 5 \text{ cm}^2$) was extracted in 7 mL (V_e) of de-ionized water (DI water, Nanopure Infinity™ ultrapure water system; >18 MΩ cm⁻¹) in a sterile polypropylene centrifuge tube (VWR International LLC, Suwanee, GA, USA) via 30-min sonication (Ultrasonic Cleanser, VWR International LLC, West Chester, PA, USA). The extract was filtered using a 0.45 μm PTFE syringe filter (Fisherbrand™) and then acidified using 6 M high purity HCl to a pH of 1 to preserve the Fe or Cu in solution. A schematic of the extraction is shown in Figure 1.

The filterable metal fraction in the extracts, defined as water-soluble metals in this paper, will include all dissolved metal forms and any colloidal particles with a diameter less than 0.45 μm, assuming that all colloidal particles < 0.45 μm can penetrate through the syringe filter and the retention efficiency of particles > 0.45 μm is 100 %.

To assess the contribution of colloidal particles to the operationally defined WS Fe and WS Cu, a subset of the collected filters (N = 69) were further filtered by ultrafiltration (Amicon™ ultra centrifugal filter units, Merck Millipore Ltd., Tullagreen, Carrigtwohill, Co. Cork, IRL). Two filter sizes, 30,000 Daltons (Da) and 3,000 Da, were used for size fractionation, which roughly correspond to colloidal particles of 4 nm and 2 nm diameter, respectively (Erickson, 2009). Details of the conversion of particle mass in Da to particle diameter and the effects of ultrafiltration membrane rejection are discussed in the Supplement. The particles were separated within the 30 kDa and 3 kDa ultrafiltration units at ~ 3000g (4000 rpm) centrifugation for 30-min and 60-min, respectively. The filtrate was then pH adjusted to 1 and measured for WS Fe and WS Cu.

The soluble metal fraction may be affected by the degree of dilution of the samples in the extraction process. The ratio of extraction water volume to the volume of air sampled on the analyzed filter portion, denoted as P , is ~ 0.5 in this study. This implies that Fe- and Cu-containing substances with solubility higher than roughly 10⁻³ g L⁻¹ under conditions close to neutral pH will likely be fully dissolved, while species with water solubility as low as 10⁻⁶ g L⁻¹ may be partially soluble but still contribute to the WS Fe and WS Cu measured with our method. Details of the effect of P on Fe or Cu solubility are discussed in the Supplement.

2.4.2 Extraction for total metal analysis

The extraction procedures for the determination of total Fe and Cu (shown in Fig. 1) follow the method conducted by Aller et al. (1986). To increase the solubility of metals, filter punches (1.5 cm² for Fe and 3 cm² for Cu) were digested with 1.5 mL and 2 mL of 6 M HCl for total Fe and Cu measurements, respectively. The filter was incubated in acid at 99°C and shaken at a rotational frequency of 350 rpm using a ThermoMixer (Eppendorf North America, Inc., Hauppauge, NY, USA) for 24 h. This extraction method has been demonstrated to remove >96 % of Fe from the PACS1 international sedimental standards and > 98 % of Fe from standard rocks and inner shelf muds (Poulton and Canfield, 2005). The effect of extraction time, heating temperature and rotation rate on extraction efficiency were tested and are discussed below. The extract was diluted to 10 mL



(V_e) using DI and then filtered by a 0.45 μm pore PTFE syringe filter. The volume of the sample extract used for the measurement (V_s) differed between samples and was determined by the ambient concentration of each sample. The pH of sample extract was adjusted to 1 using 5 M NaOH, and the sample volume was adjusted to 2.5 mL with DI water.

A total of 10 blank filters were collected throughout the one year of sampling, and these were used randomly to assess the blank levels (i.e., multiple punches were taken from the blank filters for a blank analysis on different days). The same tools and type of filter were used for blanks and samples to track all possible contamination. The concentration of blanks was calculated using Eq. (1) assuming V_a was equal to the volume of air drawn through actual ambient filter samples.

160 2.5 Colorimetric Methods

2.5.1 Colorimetric Method for Fe

A ferrozine based method, which has been previously established and discussed (Oakes et al., 2010; Rastogi et al., 2009), was adopted and modified in this study for Fe measurement. Briefly, excessive amount of reducing agent, hydroxylamine hydrochloride (0.1 mL; 1.5 M), was added to 2.5 mL (V_s) of sample solution to reduce all soluble forms of Fe (e.g., Fe(III) to Fe(II). The vial was sealed and stored overnight (roughly 18 hours) at room temperature to ensure complete reduction (Bengtsson et al., 2002; Rozan et al., 2002). After the overnight redox reaction, the sample pH was adjusted to 4 ~ 5 using ammonium acetate buffer. 0.2 mL of 5 mM ferrozine-acetate reagent was added to the solution to form the colored ferrozine-Fe(II) complex that absorbs light at 562 nm. The total volume of sample solution after addition of all the chemicals (V_t) was 2.85 mL.

The reaction between Fe(II) and ferrozine is found to be pH-dependent; the absorption of the complex increases rapidly when pH is above 0 and becomes steady within the pH range of 3 to 6 (Gibbs, 1976; Stookey, 1970). Under the conditions of the original method, when the pH of the sample was approximately 1, the absorbance of the complex was sensitive to small fluctuations in pH, adding uncertainty to the analysis. A further disadvantage is that at lower pH (pH = 1), the reaction rate of Fe(II) and ferrozine was much slower relative to higher pH (3-5). Therefore, we tested a modification to the method by raising the pH of the sample to 4 ~ 5 during the colorimetric reaction using ammonium acetate buffer to increase the precision of the Fe measurement (Fig. 1). Part of the WS Fe samples was analysed both ways, with low and higher pH, whereas all total Fe measurements were done with the buffered (higher pH) samples.

2.5.2 Colorimetric Method for Cu

For the determination of Cu concentrations, a bathocuproine assay was used. Bathocuproine can selectively chelate with Cu(I) and form complexes absorbing light at 464 nm. To convert other soluble Cu forms (e.g., Cu(II)) to Cu(I), 0.5 mL of 1.6 M hydroxylamine hydrochloride was added to 2.5 mL (V_a) sample extracts at pH 1 (as described above) and allowed to react for 30 minutes (Imamura and Fujimoto, 1975; Tomat and Rigo, 1975). The reaction between Cu(I) and bathocuproine is also pH-



185 dependent, and so a set of controlled trials were performed with different pH conditions ranging from 0.5 to 6 to assess the optimal pH for forming the colored complex (Fig. S1). The light absorption of the complex remained low at $\text{pH} < 1.5$ and exhibited a rapid increase above $\text{pH} 2$ and became steady when pH was within the range of 5 to 6. Based on these results, 1 mL of 1 M sodium citrate was added to the sample solution to maintain the pH within the range of 5 to 6, followed by 1 mL of 2.8 mM bathocuproine ($V_l = 5.05 \text{ mL}$). After 15-min reaction, the light absorption of the bathocuproine-Cu(I) complex was measured.

190 The colorimetric methods can provide insights on the forms of metal ions present, such as Fe(II) and Fe(III), or Cu(I) and Cu(II). For example by first measuring the reduced species, Fe(II) or Cu(I), then adding the reducing agent to measure the total (Fe(II)+Fe(III), or Cu(I)+Cu(II)). We do not attempt to speciate the WS Fe and WS Cu in this study since reduction-oxidation processes during the sampling, storage or extraction procedures may alter the valence states of airborne metals from what existed in the ambient particles.

2.6 Metal analysis by ICP-MS

195 Both total and water-soluble elements, which included magnesium (Mg), aluminum (Al), potassium (K), manganese (Mn), and zinc (Zn) in addition to Fe and Cu, were also measured by inductively coupled plasma mass spectrometry (ICP-MS) (Agilent 7500a series, Agilent Technologies, Inc., CA, USA). The sample preparation procedures have been described in detail in Gao et al. (2019). The sample preparation for WS metal analysis followed the same extraction procedures as those described above for WS Fe and Cu. The filtered extract was then acid-preserved with concentrated nitric acid (70 %) to a final concentration of 2 % (v/v). For total metal analysis, aqua regia, a more powerful acid than HCl, was used for filter digestion. 200 The acid-digested sample was then diluted and filtered for ICP-MS analysis.

3 Results and Discussions

3.1 Evaluation of the colorimetric measurement method

3.1.1 Calibration of the Detection Methods

205 The analytical systems were calibrated and assessed with a series of standards diluted from the standard stocks of Cu(II) and Fe(III). The calibration curves for the reduced form of metals (Cu(I) and Fe(II)) are illustrated in Fig. 2. York regression (Wu and Yu, 2018) was applied and demonstrated a strong linear relationship between the element concentrations and the detected light absorbance with the coefficient of determination (R^2) of 1.00. The slopes of calibration curves from multiple calibration runs were 0.033 ± 0.004 for Cu (coefficient of variation, CV = 12 %, N = 22) and 0.053 ± 0.005 for Fe (CV = 9 %, N = 5), 210 indicating the stable performance of the systems. Repeated measurements (N = 20) of a $35 \mu\text{g L}^{-1}$ standard solution had a relative standard deviation for both Cu and Fe of $< 10 \%$. These results indicated good precision and the robustness of this method for quantifying both Cu and Fe.



3.1.2 Blanks, Detection Limit and Uncertainty

Field blanks were analyzed on each test day in parallel with samples to assess the overall system background. The limits of
215 detection (LODs) of the spectroscopic systems, determined as three times the standard deviation of the filter blanks, were 3.07
ng m⁻³ (N = 34) for WS Fe, 14.79 ng m⁻³ (N = 6) for total Fe, 3.04 ng m⁻³ (N = 29) for WS Cu, and 3.23 ng m⁻³ (N = 6) for
total Cu. The overall uncertainties of the sampling system ranged from 7 % to 14 %, calculated from the combination of the
analytical uncertainty, uncertainty of blank measurements and quadrature sum of square of various relative uncertainties (such
as uncertainties caused by calibrations, blank filters, flow rates, liquid extract volumes, etc.). The detection limits and
220 uncertainties were comparable to the measurement using ICP-MS, indicating that LWCC has an equally good performance as
ICP-MS, especially for the WS Fe measurement. A summary of LOD, blank and uncertainty are shown in Table 1.

3.1.3 Interference

In the spectrophotometric method, species in ambient aerosol particles, such as black carbon (BC, or also called refractory
BC), light-absorbing organic species (i.e., Brown Carbon, BrC) or inorganic species (i.e., components of mineral dust), can
225 also absorb light at 482 or 562 nm, potentially resulting in measurement interference. However, these interferences are not
accounted for in the blanks since no particles are collected as part of the blank measurement. To assess the interference, the
light absorption at 484 or 562 nm of the individual liquid samples was measured without adding the colorimetric reagents (see
X in Fig 1). The interference was measured for the ambient samples collected in this study and in an extreme case (sampling
wildfire smoke). By comparing the interference corrected and non-corrected data, it is found that the average interference was
230 less than 20 % for WS Fe and 1 % for total Fe. For total and WS Cu, a correction of about 24 % and 30 % was found,
respectively. For the extreme case, samples from within wildfire plumes, for WS Cu an average correction of 50 % was needed
(see supplemental Fig. S2). The impact of this correction also depends on the concentrations of the Fe or Cu, which in smoke
plumes can be at low concentrations relative to high level of light-absorbing aerosol species (i.e., BC and BrC) and so the
correction, in this case, is important. The magnitude of the interference also depends on the extraction method; methods that
235 more effectively extract solid particles (e.g., BC) or solubilize light-absorbing species at low pH (e.g., mineral dust) could
produce higher interferences. Black carbon absorbs light over all wavelengths, whereas BrC and mineral dust absorb
preferentially at lower wavelengths and so would be a potentially larger interference for the Cu method since the Cu complex
is measured at 484 nm compared to 562 nm for Fe. Since incomplete combustion is the main source for BC and BrC, tests for
this interference are most important when these types of emissions make a large contribution to the overall aerosol sources,
240 such as sampling in regions highly influenced by biomass burning or vehicle tailpipe emissions. Interference from light
absorbing mineral dust species is most likely when sampling under dry conditions and high winds.

We also used a series of metal mixtures, which contained different levels of Fe and Cu, to test the possible interferences from
the formation of colored complexes with other metals. For the Cu measurement, no interference from Fe was observed with
up to 100 ppb of Fe present. Similarly, Cu did not interfere with the Fe measurement with Cu concentrations in the liquid up



245 to 100 ppb. In this study, the liquid concentrations of Cu and Fe from ambient samples were much lower than 100 ppb, therefore, no interference between Cu and Fe for the colorimetric methods. All measurements for ambient samples in this study were blank and interference corrected.

3.1.4 Comparison to ICP-MS Measurements and influence of experimental conditions

250 To further evaluate the accuracy of the new detection method, the concentrations determined by the colorimetric methods were compared to ICP-MS measurements. WS Fe and WS Cu were measured with the colorimetric methods using the LWCC system on all collected filters (N = 355), but only a portion of the 355 filters was used for the measurement of total Fe and total Cu using the same LWCC system (Fe: N = 23, Cu: N = 21). All filters (N = 355) were used for the ICP-MS measurements of both WS and total elements.

255 **Water-soluble Fe and Cu:** Regression analysis between the colorimetric methods and ICP-MS measurements showed good quantitative agreement for WS Fe and WS Cu with R^2 greater than 0.89. The differences between the LWCC and ICP-MS measured concentrations were 6 %, and 12 % for WS Fe and WS Cu (Fig. 3a and 3c) with the offsets (intercepts) less than 1 ng m^{-3} . Considering measurement uncertainty, most points overlap the 1:1 line except for several WS Fe measurements. The difference in WS Fe between these two methods was possibly due to the acidic conditions (pH ~1) of the colored complex forming solution used in the original approach of the colorimetric method. As noted above, to improve the method, some of the samples (N = 69) was re-analyzed with sample pH adjusted to 4 ~ 5, which resulted in a higher correlation to the ICP-MS measurement, consistent with less sensitivity of the complex to pH when in the higher pH range ($r^2 = 0.92$, slope 1.02, intercept -0.42 ng m^{-3}) (Fig. 4). Considering the overall uncertainties of these two methods, the LWCC and ICP-MS measurements of the water-soluble metals were in agreement.

265 **Total Fe and Cu:** Similar results were found between the LWCC and ICP-MS methods for the measurement of total element concentration. For total Fe, York regression between LWCC and ICP-MS yields a slope of 1.07, with an intercept of 3.09 ng m^{-3} and $r^2 = 0.97$, see Fig. 3b. For Cu, the slope was 0.96, intercept = -1.86 ng m^{-3} and $r^2 = 0.95$ (Fig. 3d).

As noted, in the colorimetric methods description above, the filters for the total Fe and total Cu analysis were extracted for a 24 h period with the assistance of shaking and high temperature. The effect of extraction time, heating temperature and rotation rate on extraction efficiency were tested (with N = 3 filters for each condition). It was found that for total Fe extraction, there was a 5 % decrease when the extraction time was shortened from 24 to 2.5 hours and a 5 % increase when extraction time was increased from 24 to 120 hours. For Cu, the concentration decreased by 15 % when the extraction time was changed from 24 to 2.5 hours and decreased by 5 % when the extraction time was extended to 120 hours. An extraction time of 24 hours was concluded to be optimal for both Fe and Cu. Extract temperature had a small impact, with a 5 % and 10 % decrease for Fe and Cu extraction, respectively, when the temperature decreased from 99°C to 50°C. The rotational shaking was found to significantly affect the extraction efficiency. Compared to shaking at a rate of 350 rpm, extraction without rotational shaking reduced the extraction efficiency by 98 % and 89 % for Fe and Cu, respectively.



3.2 Characteristics of Fe and Cu in Urban Atlanta

3.2.1 Water-soluble, Total and Fractional Solubility

280 The annual average concentrations of total Fe measured by ICP-MS and WS Fe measured by LWCC was 203.7 ng m^{-3} and 20.2 ng m^{-3} , respectively. Mass concentrations of WS Fe spanned a wide range, from the detection limit (3.07 ng m^{-3}) to 169 ng m^{-3} . The average concentrations of total Cu and WS Cu were 30.7 ng m^{-3} and 13.8 ng m^{-3} , respectively. Mass concentration of WS Cu ranged from the detection limit (3.04 ng m^{-3}) to 132 ng m^{-3} . Table 2 and Table S1 provide a more complete summary. The statistics of the LWCC measurement and ICP-MS measurement of total metals were different since only a fraction of all
285 the 2017 filter samples were analyzed for total metals using the LWCC system (Fe: $N = 23$, Cu: $N = 21$). These concentrations were comparable with a previous study conducted in Atlanta, GA, and in the range reported for many other regions globally (Table 3).

As expected the total Fe concentration was much higher than total Cu since Fe is a common element in the Earth's crust (mass fraction of 5.63 %) (Taylor, 1964) and ubiquitous in mineral dust, while $\text{PM}_{2.5}$ Cu in urban environments is mainly derived
290 from vehicle brake and tire wear, and motor-oil impurities resulting in tail-pipe emissions; both of these sources are associated with traffic (Fang et al., 2015; Marcazzan et al., 2003). Other industrial sources of $\text{PM}_{2.5}$ Cu are also possible. Despite much higher total concentrations, the concentrations of WS Fe were comparable with WS Cu. This is due to a much lower solubility of Fe than Cu. The average soluble fraction of Fe and Cu are 14.6 % and 50.7 %, respectively (Table 2).

3.2.2 Components of Water-Soluble Fe and Cu Based on Ultrafiltration

295 Ultrafiltration of WS Fe and WS Cu was used to assess contributions of colloidal particles to the concentrations of water-soluble metals. The size fractionation results are given in Fig. 5. Based on medians of all ultrafiltration data, approximately 82 % of the WS Fe had a nominal diameter smaller than 4 nm, passing through the 30k Dalton filter; 56 % of the WS Fe were nominally smaller than 2 nm in diameter, which passed through the 3k Dalton filter. The fractions for the sizes in between were calculated by taking the difference, and a rough distribution of Fe in the overall WS Fe was: 56 % smaller than 2 nm, 26
300 % between 2 and 4 nm, and 18 % between 4 nm and $0.45 \mu\text{m}$. For WS Cu, most (82 %) of WS Cu passed through the 3k Dalton filter and had a nominal diameter less than 2 nm, with 2 % between 2 and 4 nm and 16 % between 4 nm and $0.45 \mu\text{m}$. The 2 to 4 nm fraction of Fe colloidal particles (23 %) was higher than that found in WS Cu (4 %, which was practically zero). Laboratory studies find that ambient particles undergoing pH cycling from low pH (~ 2) in deliquesced particles to circumneutral pH of ~ 5 -6 when activated in cloud drops leads to the formation of nanoparticles of highly reactive ferrihydrite
305 of a few nm diameter ($\sim 5 \text{ nm}$) (Shi et al., 2011). The pH of the bulk $\text{PM}_{2.5}$ aerosol in this region is estimated to be in the range $1.63 \sim 2.31$ (25th and 75th percentiles throughout the year (Wong et al., 2020)), which would rise rapidly to pH between 5 and 7 in the extraction solution (based on measurements). Rapid increase to circumneutral pH leads to a supersaturated soluble Fe(III) which then precipitates out of the solution. Thus, either from pH cycling experienced by the ambient aerosol, or changes due to the filter extraction process, the colloidal particles of WS Fe observed in the 2 to 4 nm range are consistent with the



310 ferrihydrite reported by Shi et al. (2011). Acid driven solubility of Cu occurs rapidly at higher pH's and so may not reach supersaturation like that of Fe when pH increases to circumneutral, accounting for the lack of colloidal particles in the nominal 2 to 4 nm size range WS Cu.

For both Fe and Cu, the fraction of Fe and Cu in the 4 nm to 0.45 μm range may be insoluble chemical forms from primary emissions, like metal oxides that had been extracted from the filter and had passed through the syringe filter, making them not a “true” water-soluble species (i.e., not unique from the insoluble fraction). More research needs to be done to determine what caused the variability in the various fractions separated by ultrafiltration and to characterize the forms of the metals in the various size fractions of what we operationally define as overall water-soluble metal. These results have implications for aerosol toxicity and health effects.

4 Conclusion

320 In this study, a new approach for the measurement of WS Cu and total Cu has been developed and tested based on liquid spectrophotometry. It follows a similar method for quantifying WS Fe. All measurements can be performed with a single relatively inexpensive spectrophotometer. Utilizing daily $\text{PM}_{2.5}$ filters collected in Atlanta during 2017, the spectrophotometer methods were assessed by comparing with elements measured by ICP-MS on the same ambient filter samples. Calibrations with liquid standards produced by serial dilutions were highly linear and stable over periods of days. The spectrophotometric method detection limits in this study were 3.07 ng m^{-3} for WS Fe, and 14.8 ng m^{-3} for total Fe, 3.04 ng m^{-3} for WS Cu, and 3.23 ng m^{-3} for total Cu with measurement uncertainties ranging from 7 to 14 %. The detection limit and uncertainties are comparable to ICP-MS measurement. Possible interferences from other light-absorbing species, such as black and brown carbon should be considered, especially for the Cu measurement and in situations where emissions of light-absorbing aerosols are high (e.g., BC, BrC, mineral dust). From comparisons with ICP-MS measurements, in all cases (WS Fe, total Fe, WS Cu and total Cu) the spectrophotometry data were in good agreement (slopes ranged between 0.88 and 1.07 and $r^2 > 0.89$).

330 In Atlanta, total Fe concentration was much higher than total Cu, whereas the level of WS Fe was comparable with WS Cu, due to a higher soluble fraction of $\text{PM}_{2.5}$ Cu (45.6 %) compared to Fe (14.6 %). The composition of what is operationally defined as WS Fe and WS Cu (i.e., the aerosol filter extracted in pure water and extract passed through 0.45 μm pore liquid filter) was investigated with ultrafiltration Fe and Cu in the filtrate measured with the spectrophotometric (LWCC) method.

335 Ultrafiltration showed that roughly 82 % of WS Fe and 84 % of WS Cu was composed of dissolved species or colloidal particles smaller than nominally 4 nm diameter. Fe and Cu are two important redox-active metals that have been linked to reactive oxygen species (ROS) formed *in vivo* and lead to adverse health effects through oxidative stress. These spectrophotometric methods allow analyses of the various physical forms of Fe and Cu in ambient aerosol particles and are directly applicable to aerosol toxicity studies and their contribution to aerosol oxidative potential (OP).



340 Data availability

The data used in this paper are publicly available at [https://github.com/yhyang611/A-Method-for-Liquid-Spectrophotometric-Measurement-of-Variou-Forms-of-Iron-and-Copper-in-Ambient-Ae/blob/main/summaryofdata\(1\).xlsx](https://github.com/yhyang611/A-Method-for-Liquid-Spectrophotometric-Measurement-of-Variou-Forms-of-Iron-and-Copper-in-Ambient-Ae/blob/main/summaryofdata(1).xlsx) and can also be obtained from the corresponding author upon request.

Author contribution

345 YY is responsible for the study design, experiment using LWCC, data analysis and manuscript writing. RJW supervised the study and participated in the writing and revision of the paper. DG provided ICP-MS data and interpretation of the results.

Competing interests

The authors declare that they have no conflict of interest.

Acknowledgements

350 This work was supported by the NSF under grant number 1927778 and by the Georgia Tech EAS Jefferson Street Funds through a generous gift from Georgia Power-Southern Company.

Thanks are given to Linghan Zeng for his kind guidance in experiment and many interesting discussions about data analysis. We would also like to thank Allison Weber for her help in conducting the IC measurements.

355 References

- Adachi, K. and Tainosho, Y.: Characterization of heavy metal particles embedded in tire dust, *Environment international*, 30, 1009-1017, 2004.
- Aller, R. C., Mackin, J. E., and Cox Jr, R. T.: Diagenesis of Fe and S in Amazon inner shelf muds: apparent dominance of Fe reduction and implications for the genesis of ironstones, *Continental Shelf Research*, 6, 263-289, 1986.
- 360 Alves, D. D., Riegel, R. P., Klauck, C. R., Ceratti, A. M., Hansen, J., Cansi, L. M., Pozza, S. A., de Quevedo, D. M., and Osório, D. M. M.: Source apportionment of metallic elements in urban atmospheric particulate matter and assessment of its water-soluble fraction toxicity, *Environmental Science and Pollution Research*, 2020. 1-13, 2020.
- Ammann, A. A.: Inductively coupled plasma mass spectrometry (ICP MS): a versatile tool, *Journal of mass spectrometry*, 42, 419-427, 2007.
- 365 Bengtsson, G., Fronæus, S., and Bengtsson-Kloo, L.: The kinetics and mechanism of oxidation of hydroxylamine by iron (III), *Journal of the Chemical Society, Dalton Transactions*, 2002. 2548-2552, 2002.
- Bongaerts, E., Nawrot, T. S., Van Pee, T., Ameloot, M., and Bové, H.: Translocation of (ultra) fine particles and nanoparticles across the placenta; a systematic review on the evidence of in vitro, ex vivo, and in vivo studies, *Particle and fibre toxicology*, 17, 1-26, 2020.



- 370 Brewer, G. J.: Iron and copper toxicity in diseases of aging, particularly atherosclerosis and Alzheimer's disease, *Experimental Biology and Medicine*, 232, 323-335, 2007.
- Brook, R. D., Rajagopalan, S., Pope, C. A., 3rd, Brook, J. R., Bhatnagar, A., Diez-Roux, A. V., Holguin, F., Hong, Y., Luepker, R. V., Mittleman, M. A., Peters, A., Siscovick, D., Smith, S. C., Jr., Whitsel, L., and Kaufman, J. D.: Particulate matter air pollution and cardiovascular disease: An update to the scientific statement from the American Heart Association, *Circulation*, 121, 2331-2378, 2010.
- 375 Calderón-Garcidueñas, L., González-Maciel, A., Mukherjee, P. S., Reynoso-Robles, R., Pérez-Guillé, B., Gayosso-Chávez, C., Torres-Jardón, R., Cross, J. V., Ahmed, I. A. M., and Karloukovski, V. V.: Combustion-and friction-derived magnetic air pollution nanoparticles in human hearts, *Environmental research*, 176, 108567, 2019.
- Chen, Y., Luo, X.-S., Zhao, Z., Chen, Q., Wu, D., Sun, X., Wu, L., and Jin, L.: Summer–winter differences of PM_{2.5} toxicity to human alveolar epithelial cells (A549) and the roles of transition metals, *Ecotoxicology and environmental safety*, 165, 505-509, 2018.
- 380 Chow, J. C.: Measurement methods to determine compliance with ambient air quality standards for suspended particles, *Journal of the Air & Waste Management Association*, 45, 320-382, 1995.
- Costa, D. L. and Dreher, K. L.: Bioavailable transition metals in particulate matter mediate cardiopulmonary injury in healthy and compromised animal models, *Environmental health perspectives*, 105, 1053-1060, 1997.
- 385 Danadurai, K. S. K., Chellam, S., Lee, C.-T., and Fraser, M. P.: Trace elemental analysis of airborne particulate matter using dynamic reaction cell inductively coupled plasma–mass spectrometry: Application to monitoring episodic industrial emission events, *Analytica chimica acta*, 686, 40-49, 2011.
- Donaldson, K., Stone, V., Seaton, A., and MacNee, W.: Ambient particle inhalation and the cardiovascular system: potential mechanisms, *Environmental health perspectives*, 109, 523-527, 2001.
- 390 Dreher, K. L., Jaskot, R. H., Lehmann, J. R., Richards, J. H., Ghio, J. K. M. A. J., and Costa, D. L.: Soluble transition metals mediate residual oil fly ash induced acute lung injury, *Journal of toxicology and environmental health part a*, 50, 285-305, 1997.
- Erickson, H. P.: Size and shape of protein molecules at the nanometer level determined by sedimentation, gel filtration, and electron microscopy, *Biological procedures online*, 11, 32, 2009.
- 395 Fang, T., Guo, H., Verma, V., Peltier, R. E., and Weber, R. J.: PM_{2.5} water-soluble elements in the southeastern United States: automated analytical method development, spatiotemporal distributions, source apportionment, and implications for health studies, *Atmospheric Chemistry and Physics*, 15, 11667-11682, 2015.
- Frampton, M. W., Ghio, A. J., Samet, J. M., Carson, J. L., Carter, J. D., and Devlin, R. B.: Effects of aqueous extracts of PM₁₀ filters from the Utah Valley on human airway epithelial cells, *American Journal of Physiology-Lung Cellular and Molecular Physiology*, 277, L960-L967, 1999.
- 400 Galon-Negru, A. G., Olariu, R. I., and Arsene, C.: Size-resolved measurements of PM_{2.5} water-soluble elements in Iasi, north-eastern Romania: Seasonality, source apportionment and potential implications for human health, *Science of The Total Environment*, 695, 133839, 2019.
- 405 Gao, D., Mulholland, J. A., Russell, A. G., and Weber, R. J.: Characterization of water-insoluble oxidative potential of PM_{2.5} using the dithiothreitol assay, *Atmospheric Environment*, 224, 117327, 2020.
- Gao, D., Pollitt, K. J., Mulholland, J. A., Russell, A. G., and Weber, R. J.: Characterization and comparison of PM_{2.5} oxidative potential assessed by two acellular assays, *Atmospheric Chemistry and Physics*, doi: 10.5194/acp-2019-941, 2019. 2019.
- Ghio, A. J., Carraway, M. S., and Madden, M. C.: Composition of air pollution particles and oxidative stress in cells, tissues, and living systems, *J Toxicol Environ Health B Crit Rev*, 15, 1-21, 2012.
- 410 Gibbs, C. R.: Characterization and application of ferrozine iron reagent as a ferrous iron indicator, *Analytical Chemistry*, 48, 1197-1201, 1976.
- Gonet, T. and Maher, B. A.: Airborne, vehicle-derived Fe-bearing nanoparticles in the urban environment: A review, *Environmental Science & Technology*, 53, 9970-9991, 2019.
- 415 Huang, Y.-C. T., Ghio, A. J., Stonehuerner, J., McGee, J., Carter, J. D., Grambow, S. C., and Devlin, R. B.: The role of soluble components in ambient fine particles-induced changes in human lungs and blood, *Inhalation toxicology*, 15, 327-342, 2003.
- Imamura, T. and Fujimoto, M.: Kinetics and Mechanism of the Reaction of Copper (II) with Hydroxylamine in the Presence of Bathocuproine Disulfonate, *Bulletin of the Chemical Society of Japan*, 48, 2971-2972, 1975.



- 420 Ito, A., Myriokefalitakis, S., Kanakidou, M., Mahowald, N. M., Scanza, R. A., Hamilton, D. S., Baker, A. R., Jickells, T., Sarin, M., and Bikkina, S.: Pyrogenic iron: The missing link to high iron solubility in aerosols, *Science advances*, 5, eaau7671, 2019.
- Khillare, P. S. and Sarkar, S.: Airborne inhalable metals in residential areas of Delhi, India: distribution, source apportionment and health risks, *Atmospheric pollution research*, 3, 46-54, 2012.
- 425 Kim, J. S., Peters, T. M., O'Shaughnessy, P. T., Adamcakova-Dodd, A., and Thorne, P. S.: Validation of an in vitro exposure system for toxicity assessment of air-delivered nanomaterials, *Toxicology in Vitro*, 27, 164-173, 2013.
- Kuang, X. M., Gonzalez, D. H., Scott, J. A., Vu, K., Hasson, A., Charbouillot, T., Hawkins, L., and Paulson, S. E.: Cloud Water Chemistry Associated with Urban Aerosols: Rapid Hydroxyl Radical Formation, Soluble Metals, Fe (II), Fe (III), and Quinones, *ACS Earth and Space Chemistry*, 4, 67-76, 2019.
- 430 Kulshrestha, A., Satsangi, P. G., Masih, J., and Taneja, A.: Metal concentration of PM_{2.5} and PM₁₀ particles and seasonal variations in urban and rural environment of Agra, India, *Science of the Total Environment*, 407, 6196-6204, 2009.
- Lakey, P. S., Berkemeier, T., Tong, H., Arangio, A. M., Lucas, K., Poschl, U., and Shiraiwa, M.: Chemical exposure-response relationship between air pollutants and reactive oxygen species in the human respiratory tract, *Sci Rep*, 6, 32916, 2016.
- Lee, B.-K. and Hieu, N. T.: Seasonal variation and sources of heavy metals in atmospheric aerosols in a residential area of Ulsan, Korea, *Aerosol and Air Quality Research*, 11, 679-688, 2011.
- 435 Lee, Y., Chun, H.-S., Moon, J.-Y., Choi, J. S., Park, D., and Lee, Y.-C.: Correlation of α/γ -Fe₂O₃ nanoparticles with the toxicity of particulate matter originating from subway tunnels in Seoul stations, Korea, *Journal of hazardous materials*, 382, 121175, 2020.
- Lin, T.-L. and Luo, C.-s.: Matrix effects in PIXE analysis on liquid samples with an external beam, *Nuclear Instruments and Methods*, 159, 387-393, 1979.
- 440 Majestic, B. J., Schauer, J. J., Shafer, M. M., Turner, J. R., Fine, P. M., Singh, M., and Sioutas, C.: Development of a wet-chemical method for the speciation of iron in atmospheric aerosols, *Environmental science & technology*, 40, 2346-2351, 2006.
- Marcazzan, G. M., Ceriani, M., Valli, G., and Vecchi, R.: Source apportionment of PM₁₀ and PM_{2.5} in Milan (Italy) using receptor modelling, *Science of the Total Environment*, 317, 137-147, 2003.
- 445 Meskhidze, N., Chameides, W. L., and Nenes, A.: Dust and pollution: A recipe for enhanced ocean fertilization?, *Journal of Geophysical Research: Atmospheres*, 110, 2005.
- Moffett, J. W., Zika, R. G., and Petasne, R. G.: Evaluation of bathocuproine for the spectrophotometric determination of the copper(I) in copper redox studies with applications in studies of natural waters, *Analytical Chimica Acta.*, 175, 171-179, 1985.
- 450 Moreno-Ríos, A. L., Tejada-Benítez, L., and Bustillo-Lecompte, C.: Sources, characteristics, toxicity, and control of ultrafine particles: An overview, *Geoscience Frontiers*, 2021. 101147, 2021.
- Nel, A.: Air pollution-related illness: effects of particles, *Science*, 308, 804-806, 2005.
- 455 Oakes, M., Rastogi, N., Majestic, B. J., Shafer, M., Schauer, J. J., Edgerton, E. S., and Weber, R. J.: Characterization of soluble iron in urban aerosols using near-real time data, *Journal of Geophysical Research: Atmospheres*, 115, 2010.
- Poulton, S. W. and Canfield, D. E.: Development of a sequential extraction procedure for iron: implications for iron partitioning in continentally derived particulates, *Chemical geology*, 214, 209-221, 2005.
- Rastogi, N., Oakes, M. M., Schauer, J. J., Shafer, M. M., Majestic, B. J., and Weber, R. J.: New technique for online measurement of water-soluble Fe (II) in atmospheric aerosols, *Environmental science & technology*, 43, 2425-2430, 2009.
- 460 Rozan, T. F., Taillefert, M., Trouwborst, R. E., Glazer, B. T., Ma, S., Herszage, J., Valdes, L. M., Price, K. S., and Luther III, G. W.: Iron-sulfur-phosphorus cycling in the sediments of a shallow coastal bay: Implications for sediment nutrient release and benthic macroalgal blooms, *Limnology and Oceanography*, 47, 1346-1354, 2002.
- Schrand, A. M., Rahman, M. F., Hussain, S. M., Schlager, J. J., Smith, D. A., and Syed, A. F.: Metal-based nanoparticles and their toxicity assessment, *Wiley interdisciplinary reviews: Nanomedicine and Nanobiotechnology*, 2, 544-568, 2010.
- 465 See, S. W., Wang, Y. H., and Balasubramanian, R.: Contrasting reactive oxygen species and transition metal concentrations in combustion aerosols, *Environmental Research*, 103, 317-324, 2007.
- Shi, Z., Bonneville, S., Krom, M. D., Carslaw, K. S., Jickells, T. D., Baker, A. R., and Benning, L. G.: Iron dissolution kinetics of mineral dust at low pH during simulated atmospheric processing, *Atmospheric Chemistry and Physics*, 11, 995-1007, 2011.



- 470 Smith, G. F. and Wilkins, D. H.: New Colorimetric Reagent Specific for Cooper, *Anal. Chem.*, 25, 510-511, 1953.
Stookey, L. L.: Ferrozin-a new spectrophotometric reagent for iron, *Anal. Chem.*, 42, 779-781, 1970.
Sutto, T. E.: Magnetite fine particle and nanoparticle environmental contamination from industrial uses of coal, *Environmental pollution*, 243, 528-533, 2018.
- 475 Taylor, S. R.: Abundance of chemical elements in the continental crust: a new table, *Geochimica et cosmochimica acta*, 28, 1273-1285, 1964.
- Tomat, R. and Rigo, A.: Kinetic study of the reduction of hydroxylamine by Cu (I), *Journal of Electroanalytical Chemistry and Interfacial Electrochemistry*, 59, 191-194, 1975.
- Viollier, E., Inglett, P. W., Hunter, K., Roychoudhury, A. N., and Van Cappellen, P.: The ferrozine method revisited: Fe (II)/Fe (III) determination in natural waters, *Applied geochemistry*, 15, 785-790, 2000.
- 480 Wang, B., Feng, W. Y., Wang, M., Shi, J. W., Zhang, F., Ouyang, H., Zhao, Y. L., Chai, Z. F., Huang, Y. Y., and Xie, Y. N.: Transport of intranasally instilled fine Fe₂O₃ particles into the brain: micro-distribution, chemical states, and histopathological observation, *Biological trace element research*, 118, 233-243, 2007.
- Wang, Y., Jia, C., Tao, J., Zhang, L., Liang, X., Ma, J., Gao, H., Huang, T., and Zhang, K.: Chemical characterization and source apportionment of PM_{2.5} in a semi-arid and petrochemical-industrialized city, Northwest China, *Science of the Total Environment*, 573, 1031-1040, 2016.
- 485 Wong, J. P. S., Yang, Y., Fang, T., Mulholland, J. A., Russell, A., Sarnat, S. E., Nenes, A., and Weber, R. J.: Fine Particle Iron in Soils and Road Dust is Modulated by Coal-Fired Power Plant Sulfur, *Environmental Science & Technology*, 2020. 2020.
- Wu, C. and Yu, J. Z.: Evaluation of linear regression techniques for atmospheric applications: the importance of appropriate weighting, *Atmospheric Measurement Techniques*, 11, 1233-1250, 2018.
- 490 Ye, D., Klein, M., Mulholland, J. A., Russell, A. G., Weber, R., Edgerton, E. S., Chang, H. H., Sarnat, J. A., Tolbert, P. E., and Ebel Sarnat, S.: Estimating Acute Cardiovascular Effects of Ambient PM_{2.5} Metals, *Environ Health Perspect*, 126, 027007, 2018.
- Zhu, X. R., Prospero, J. M., and Millero, F. J.: Diel variability of soluble Fe (II) and soluble total Fe in North African dust in the trade winds at Barbados, *Journal of Geophysical Research: Atmospheres*, 102, 21297-21305, 1997.
- 495 Zhuang, G., Yi, Z., Duce, R. A., and Brown, P. R.: Link between iron and sulphur cycles suggested by detection of Fe (n) in remote marine aerosols, *Nature*, 355, 537-539, 1992.



500 **Table 1:** Limits of detection, blanks and uncertainties for WS Fe, WS Cu and total Cu for the liquid spectrophotometric (LWCC) and ICP-MS measurement

	LWCC		ICP-MS	
	LOD, ng m ⁻³	Overall uncertainty, %	LOD, ng m ⁻³	Overall uncertainty, %
WS Fe	3.07	12.5	4.38	18.0
WS Cu	3.04	13.8	2.86	6.3
Total Fe	14.79	7.2	14.80	7.2
Total Cu	3.23	9.9	9.67	6.3

505 **Table 2:** Statistical summary of transition metal concentrations in PM_{2.5} measured in Atlanta in 2017 based on liquid spectrophotometric (LWCC) measurement.

	Total Fe (N = 23)	Total Cu (N = 21)	WS Fe (N = 355)	WS Cu (N = 355)	Fe solubility (N = 23)	Cu solubility (N = 21)
Mean (ng m ⁻³)	478.9	61.8	20.2	13.8	14.6 %	45.6 %
Median (ng m ⁻³)	388.4	45.4	11.4	10.8	16.3 %	44.0 %
Maximum (ng m ⁻³)	1535.2	247.1	169.3	131.5	32.5 %	> 100 %
Minimum (ng m ⁻³)	22.1	4.4	LOD	LOD	0.2 %	3.3 %
RSD	0.76	0.87	1.25	0.98	0.76	0.82

510 **Table 3:** Concentration of PM_{2.5} particulates (□g m⁻³) and transition metals (ng m⁻³) in the ambient air of urban and suburban areas in different parts of the world.

	PM _{2.5} mass	Total Fe	WS Fe	Total Cu	WS Cu
Present study, Atlanta (USA)	10.4	203.7*	20.2**	30.7*	13.8**
Previous study, Atlanta (USA) ^a			21.1		13.8
Patras (Greece) ^b	17.4	124	11.9	7.28	2.67
Megalopolis (Greece) ^b	23.0	87	8.51	4.02	0.94
Po Valley (Italy) ^c		103		4.7	
Tampa (USA) ^d	12.7	790		2.4	
Hong Kong (China) ^e	29	160		15	
Agra (India) ^f	104.9	1900		200	

^a Fang et al. (2015), ^b Manousakas et al. (2014), ^c Canepari et al. (2014), ^d Olson et al. (2008), ^e Hagler et al. (2007), ^f Kulshrestha et al. (2009)


515

* Based on ICP-MS measurement.

** Based on LWCC measurement



520

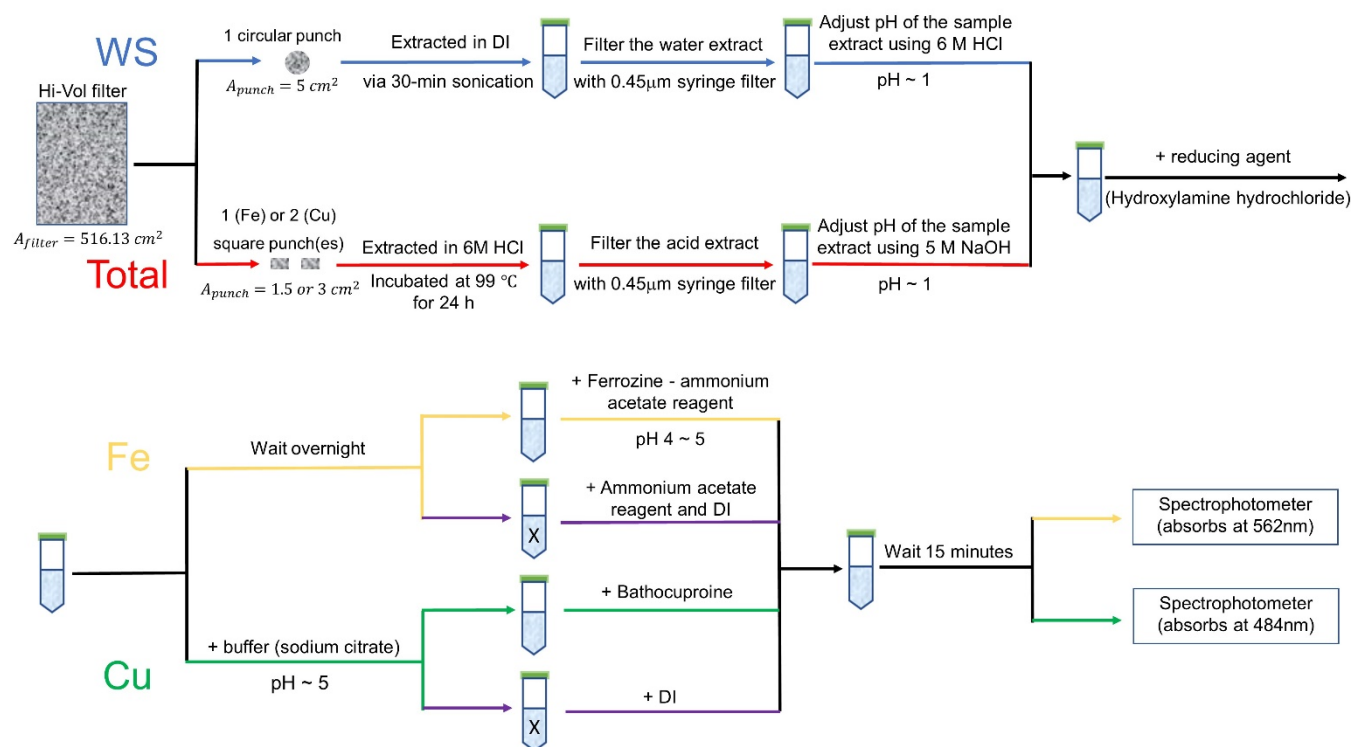


525

Figure 1: Schematic of the experimental procedures for the measurement of water-soluble (blue line) and total (red line) Fe and Cu. The upper schematic shows the processes common to both methods. The sample vial from this process is then analysed for Fe or Cu via the process illustrated in the bottom schematic. In the bottom schematic the process for Fe (yellow line) or Cu (green line) is given. The black line is common to both the WS and total measurement (in the upper schematic) or common to both the Fe and Cu measurement (in the lower schematic). X refers to the liquid samples used to assess the interference of other light-absorbing species at 562 or 484 nm (purple line).



530

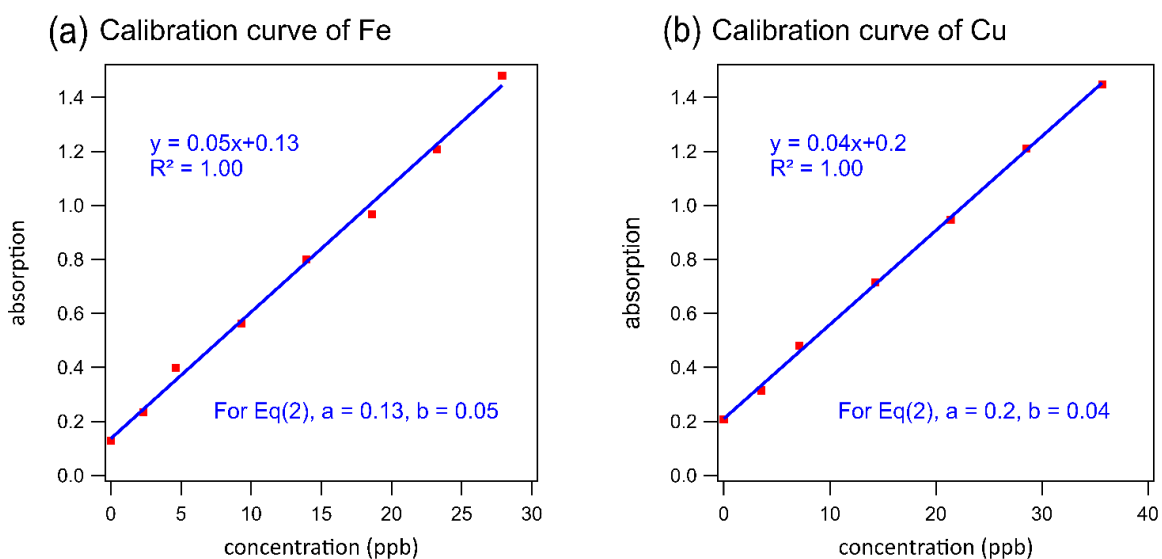

535 **Figure 2:** Calibration curves for (a) Fe(II) and (b) Cu(I) measurement by the LWCC system. Results of York regression are shown.



540


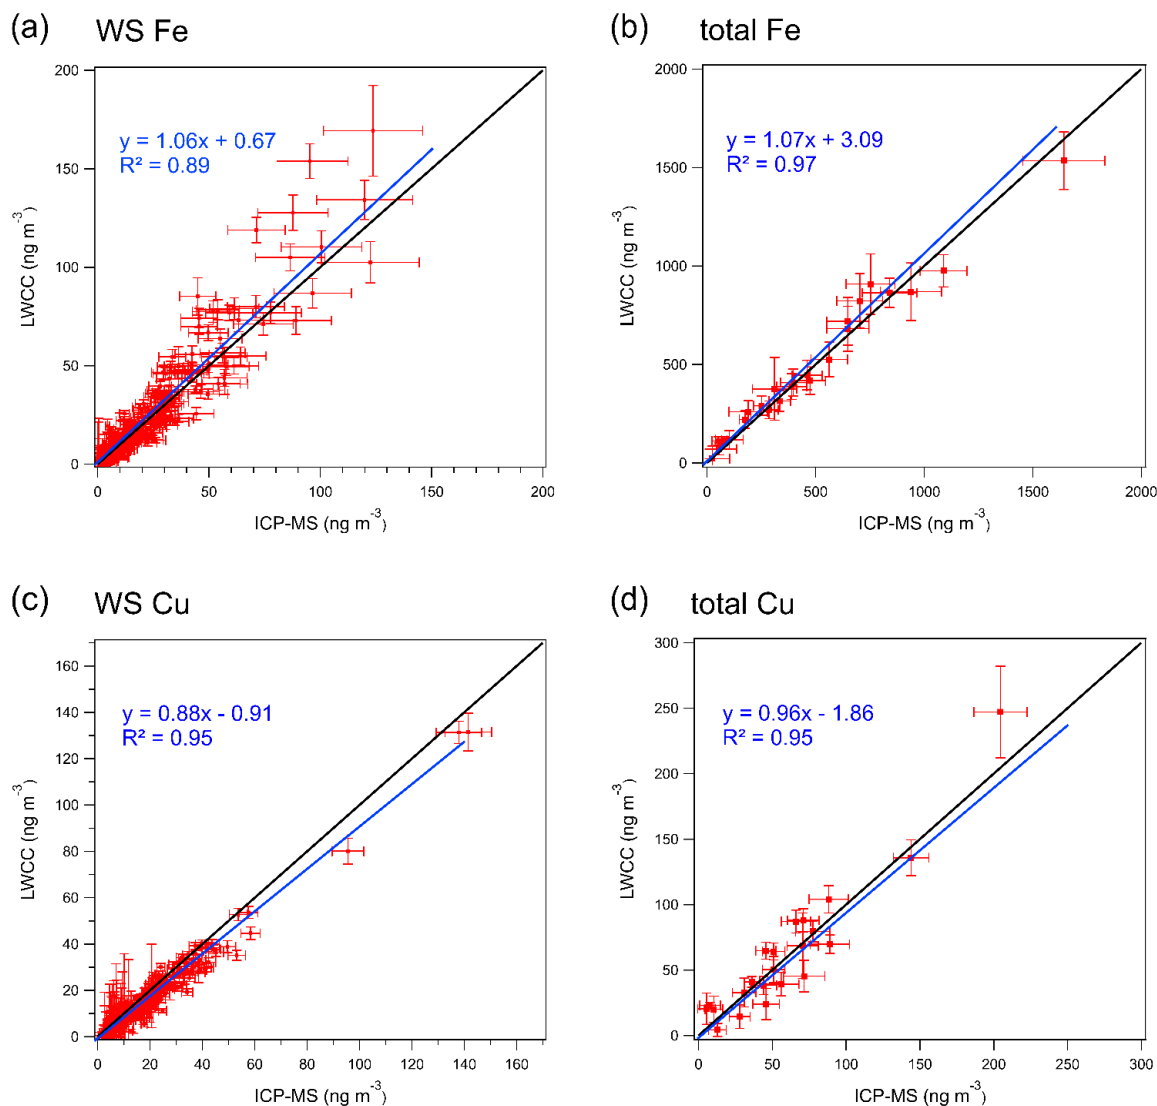


Figure 3: Comparison between LWCC method and ICP-MS method for (a) WS Fe, (b) total Fe, (c) WS Cu and (d) total Cu (results of York regression are shown, along with 1:1 ratio by black line). Bars represent the uncertainties of measurements.



545

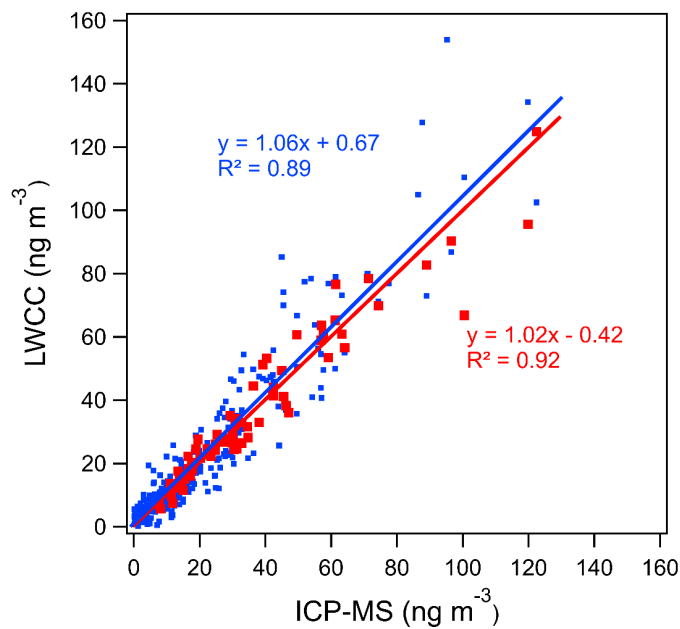


550 **Figure 4:** Comparison between LWCC method and ICP-MS method for WS Fe with pH adjustment of the light absorbing sample. The blue points and line represent the original method without ammonium acetate with pH of ~ 1. The red points and line refer to the improved method with ammonium acetate with pH 4 ~ 5 (results of York regression are shown).




555

(a) Fe

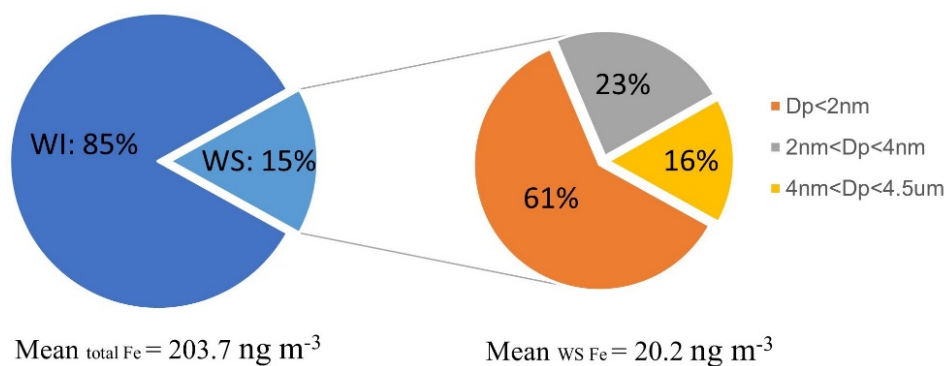

(b) Cu

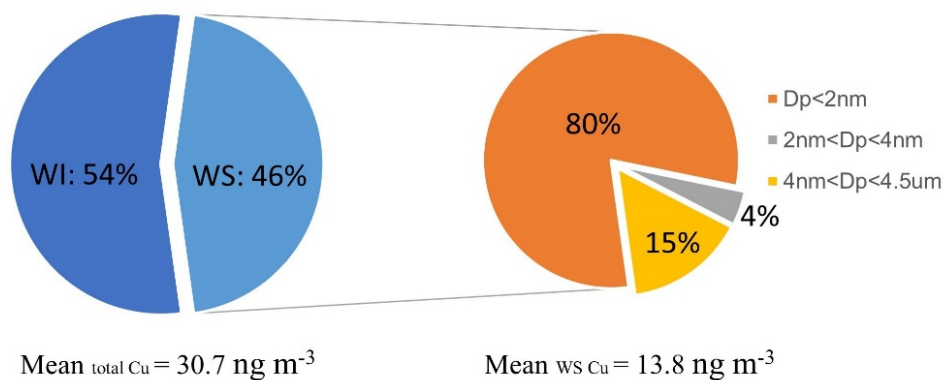

560 **Figure 5:** Components of PM_{2.5} (a) Fe and (b) Cu. Water-soluble (WS) species are operationally defined by samples that pass through a 0.45 μm pore syringe filter (shown in light blue). Water-insoluble (WI) are defined by the difference of all (total) species of that metal and WS species (shown in dark blue). WS Fe (a) and WS Cu (b) concentrations were further separated in ultrafiltration via 30,000 or 3,000 Dalton ultrafiltration filters (roughly corresponding to particle sizes of 4 and 2 nm, respectively). Concentrations in different size ranges were determined by difference (statistics calculated on the differences).