



Design and fabrication of an electrostatic precipitator for infrared spectroscopy

Nikunj Dudani¹ and Satoshi Takahama¹

¹ENAC/III, Laboratory for Atmospheric Processes and Their Impacts (LAPI), École Polytechnique Fédérale de Lausanne (EPFL), 1015 Lausanne, Switzerland

Correspondence: Satoshi Takahama (satoshi.takahama@epfl.ch)

Abstract. Infrared (IR) spectroscopy is a direct measurement technique for chemical characterization of aerosols that can be applied without solvent extraction thermal treatment a priori. This technique has been used for chemical speciation, source apportionment, and detailed characterization of the complex organic fraction of atmospheric particles. Currently, most of the IR analysis is performed by transmission through porous membranes on which the particles are collected via filtration. The membrane materials interfere with the IR spectra through scattering and absorption that not only makes extracting the chemical information of aerosol harder but also limits the lower extent of detection. An alternative IR measurement method that does not inherit such limitations aerosol is to collect the particles on an IR transparent material. We present an electrostatic precipitator design that enables such measurements by collection on a Zinc Selenide (ZnSe) crystal. Through numerical simulations and rapid prototyping with 3D-printing, we design and fabricate a device which is tested with poly-dispersed ammonium sulfate particles to evaluate the quantitative chemical composition estimates against particle count reference. Furthermore, with an image analysis procedure and using variable aperture of the IR spectrometer, we analyze the radial mass distribution. The collector has high collection efficiency ($82\% \pm 8\%$) and linear response to mass loading ($R^2 > 0.94$) with a semi-uniform deposition. The method of design and fabrication is transferable to other applications and the current ESP collector can provide directions for further design improvements.

Keywords: Design, fabrication, collector, quantitative, IR, FT-IR, ESP.

1 Introduction

Mid-infrared (IR) spectroscopy is a non-destructive technique that can be used to directly probe the chemical signature of particles without solvent extraction or similar transformations for sample preparation. Absorbance signatures of major components of $PM_{2.5}$ (organic matter, elemental carbon, mineral dust, and inorganic salts) (Ivlev and Popova, 1973; Cunningham et al., 1974; Bogard et al., 1982; Mcclenny et al., 1985; Pollard et al., 1990; Debus et al., 2021) and tracer species (Yazdani et al., 2021) can be found in the IR spectrum. To obtain an IR spectrum of the particles, they must first be isolated from the surrounding vapor as they also absorb IR and are present in comparable or greater concentrations as particle constituents.

Capability for quantification of chemical concentrations and source contributions have been demonstrated in transmission mode analysis on particles isolated on “optically thin” polytetrafluoroethylene (PTFE) membrane filters with the judicious



25 use of appropriate calibration standards and algorithms (Maria, 2003; Reff et al., 2007; Russell et al., 2009; Takahama et al.,
2013; Ruthenburg et al., 2014; Takahama et al., 2019). However, this approach suffers from measurement uncertainties due to
spectroscopic interferences from the substrate, as PTFE filters have strong absorption peaks in the fingerprint region and also
scatters radiation (Mcclenny et al., 1985), which are partially handled by statistical algorithms for removal (Kuzmiakova et al.,
2016; Yazdani et al., 2021). Reflectance spectra of particles collected on quartz or glass fiber filters or reflective foils vary in
30 magnitude of interferences but essentially require nonlinear calibration functions for quantitative analysis (Tsai and Kuo, 2006;
Hopey et al., 2008; Parks et al., 2021).

One solution to this problem is to collect particles directly onto optical crystals transparent to IR for transmission mode
analysis, but no method exists to achieve high collection efficiency on such substrates. Filtration is not amenable with conven-
tional IR transparent crystals. Impaction has been used for collection onto such crystals in the past (Fischer, 1975; Allen et al.,
35 1994; Blando et al., 1998; Sax et al., 2005), but have material-dependent bounce off effects, size stratification, and undesirable
deposition characteristics for spectroscopy (Marple, 2004; Blando et al., 2001; Virtanen et al., 2010). ESP is a versatile method
and has low pressure drop unlike both the other methods, and is selected for this application.

ESP geometry for particle collection generally fall into two broad categories: a translationally symmetric design (linear ESP)
(Harrick and Beckmann, 1974; Ofner et al., 2009) or a radially symmetric design (radial ESP) (Dixkens and Fissan, 1991; Fierz,
40 2007; Kala et al., 2012). In both systems, the electric field is perpendicular to the fluid flow that is parallel to the collection
surface. Additionally, in most radial ESPs, the fluid enters the collection region through a tube perpendicular to the collection
surface, before moving radially outwards. ESPs can also be categorized by single-stage or two-stage configurations, depending
on whether the charging and collection is handled with the same or different set of electrodes — the former is simpler in
design, while the latter permits better control in deposition. However, existing designs across these categories either require
45 high electric field strengths for operation that can cause chemical modification of the aerosol, or have high size-segregation in
deposition.

We therefore introduce a new two-stage radial ESP for collection of particles on IR transparent crystals, and report on its
capability for quantitative IR analysis. A charger with low chemical interference is selected from the existing literature, while
a new radial collector is designed to permit high collection efficiency and mass throughput. The choice of charger is germane
50 since the strong ionization in the chargers result in formation of reactive molecules such as O_2^+ , O^+ , N_2^+ , N^+ , NO^+ , and H_3O^+
(Volckens and Leith, 2002; Arnold et al., 1997), leading to changes in particle composition through ozone reactions and gas-to-
particle conversion (Volckens and Leith, 2002). Numerous chargers have been developed and use either through direct corona
discharge to charge the particles (Hewitt, 1957; Liu and Pui, 1975; Biskos et al., 2005; Whitby, 1961; Tsai et al., 2010), or
indirect corona discharge where charged ions in gas flow are generally mixed with the particle flow separately (Medved et al.,
55 2000; Marquard et al., 2006; Kimoto et al., 2010). Indirect chargers have higher charge levels but leads to diluted particle
concentrations after mixing, which reduces mass throughput. Direct or indirect photoelectric discharge (Burtscher et al., 1982;
Grob et al., 2014; Nishida et al., 2018; Shimada et al., 1999) — especially with UV photoionization (Hontañón and Kruijs,
2008; Grob et al., 2013) — leads to less chemical artifacts, but generally have strong dependence on the conductivity of the
particle (which varies by composition). Two different unipolar chargers with minimal ozone generation suitable for chemical



60 sampling have been proposed: one using carbon fiber ionizer technology Han et al. (2008) and another using a wire-to-wire configuration of metal electrodes Han et al. (2017). We adapt the latter for this work.

The radial collector design, numerical simulation, and novel methods for fabrication using 3D printing and post-treatment (together with the rest of the ESP) are described in the rest of the manuscript. The remaining portion of the manuscript describe the methods and results for characterization of collected mass and its relationship to apparent IR absorbance.

65 2 Method

In this section, we describe the design objectives and constraints (Section 2.1), numerical simulations for virtual performance characterization (Section 2.2), and 3D printing (Section 2.3) with acrylonitrile butadiene styrene (ABS). The fabricated device and an aerosol flow system (Section 2.4) was used to collect ammonium sulfate particles on a 25.4 mm diameter ZnSe crystal, which has desirable chemical, electrical, and optical properties for this application. The IR spectra of this crystal is
70 acquired before and after sampling (Section 2.5). The spatial deposition pattern on this crystal was also characterized using optical microscopy, electron microscopy and IR analysis (Section 2.6). All of these measurements are combined to evaluate the quantitative response of the IR measurement with particle loading (Section 2.7).

2.1 Design of a radial ESP

A two-stage radially symmetric (radial) ESP was selected for geometry and flow design. Separating the charging and collection
75 permits greater control over the conditions for charging and collection within each stage. The radial collector configuration does not have flow and collection directionality that is inherent in a linear ESP, which could theoretically result in some directional dependence in the particle deposition based on particle size and flow rate; and the radial symmetry in deposition profile is consistent with the transmission IR beam. The resulting design blueprint has a particle charger connected to an ESP where the flow enters perpendicular to the collection surface and moves radially outward and subsequently collected, illustrated in the
80 device schematic (Figure 1a).

One of the critical requirements in the design is to limit the high electric field strength and voltage in the vicinity of the particles, mainly because regions of high electric field facilitate ion production that modifies the chemical composition of the particles (Ofner et al., 2009). For the charging stage, another application where ozone production is an undeniable consideration is personal bio-aerosol sampling and the PEBS's wire-to-wire electrode arrangement in the charger (Han et al., 2017) was
85 specifically designed to maintain a low ozone concentration (< 10 ppb). In this work, we employ a similar wire-to-wire charger and design the collector stage with the following desired features (1) Low electric field strength (lower than 1 kV/mm, with a factor of safety 3 over the theoretical breakdown field of air at 3 kV/mm); (2) Low electrode voltage (lower than 10 kV); (3) High collection efficiency (greater than 70%); (4) High flow rate (for example, a 1.7 LPM (2.8×10^{-5} m³/s) flow rate would result in a 1 μ g total mass collection in 1 hour for an ambient concentration of 10 μ g/m³).

90 In the collector, the combination of an electric field limit to 1 kV/mm and a voltage limit of 5 kV imposed a minimum electrode separation distance of 5 mm. For conditions where inertial effects and diffusion effects can be neglected, the collection



in the radial ESP is a result of the trade-off between the drag force on the particle parallel to the collection surface (r -direction) and the electrostatic force into the surface ($-z$ -direction). For a given flow conditions, a stronger electric field will result in a more efficient particle collection making closest 5 mm separation the most desirable as any larger separation distance would either require that the voltage be higher or E_0 be lower than 1 kV/mm.

Based on these design constraints, prototypes were developed using 3D-CAD software (Section S1 Figures S2a, b, c), simulated for particle collection (Section 2.2), and assembled after 3D-printing and post-treating (Section 2.3 and Section S1 Figure S2d). The charger (modeled after Han et al. (2017)) was 3D printed using ABS and had the same dimensions of a 25.4 mm diameter tube, with the circular ground electrode wire made from 0.5 mm diameter stainless steel wire, and the ionizer was a 0.075 mm diameter Tungsten wire, 25.4 mm in length sitting symmetrically about the ground electrode while held rigidly in place at the ends through two thin glass tubes (1 mm outer diameter) that were connected to the ABS housing. The total length of the flow channel was 60 mm, and had a further gradually expanding and contracting part at either ends (40 mm in length and having 10 mm diameter at the other ends, where stainless steel tubes were used to connect the charger to the inlet and the collector).

2.2 Numerical simulations

Particle trajectories were numerically simulated in an electrostatic and flow field using COMSOL Multiphysics software. 2D-axisymmetric simulations allow much faster simulations and the fluid flow was simulated using laminar flow physics. The simulation was made with dimensions and materials replicating the actual fabricated device. A radial ESP collector (made of ABS) was simulated with a tubular inlet facing the substrate (ZnSe crystal) resting on the ground electrode, while the high voltage electrodes were placed near the outlet of the tube and at a fixed distance above the collection surface (Section S1 Figure S1a) using an extremely fine physics-controlled mesh. The electrostatic field (Section S1 Figure S1b) and the fluid flow field (Section S1 Figure S1c) were simulated using a stationary solver with 10^{-3} relative tolerance for convergence. Despite large scale eddies in the laminar flow simulations, no turbulent simulation was required mainly because mesh-refinement analysis yielded identical laminar flow results (for example, changing the mesh to a finer grid resulted in similar flow fields). This was confirmed using mesh-refinement in a 3D simulation of the device design with laminar flow field. The in-variance to mesh-refinement suggests that the obtained calculations were indeed resolved with laminar physics alone and did not represent a scrupulous flow field.

Time-dependent particle trajectories were simulated in the two stationary fields (Section S1 Figure S1d) with convergence at 10^{-5} relative tolerance. No coupling of the perturbations of the particles on the stationary fields is employed as the particles are very small to cause substantial change. 1000 charged particles were released uniformly spaced at the top of the inlet tube at $t = 0$ till it collected on the surface, collided with another surface or ran-off. The charge levels on the particle was assumed to be proportional to particle diameter (as assumed for diffusion charging) with around one elementary charge for every 20 nm diameter (Biskos et al., 2005). A couple of additional charge values around the linear value were also simulated for each particle size as the charge can be expected to be higher on larger particles if particle charge is a combined effect of field and diffusion charging (Marquard, 2007). The particle diameter D_p was manually adjusted for the slip corrected factor



$C_c = 1 + Kn [1.142 + 0.558 \exp(-0.999/Kn)]$ (Allen and Raabe, 1985), where Kn is the Knudsen number, in the drag force calculations for the particle simulation.

An iterative simulation process was used to explore geometries and operating parameters to find a configuration permitting high flowrates (for high throughput), and long residence time of particles between the electrodes (to improve collection efficiency) within electric field constraints described above. At the end of each simulation, the position of the particles on the crystal are used to calculate the histogram of the relative frequency at different radial positions (Figure 1b) as it represents the spatial distribution. Collection efficiency was calculated using the number of particles out of the 1000 that were collected on the surface (i.e till $r < 12.7$ mm) – measured through the cumulative frequency from the histogram in Figure 1b. A device with inlet radius of 10 mm and flow rate of 2.1 LPM, and $E = 1$ kV/mm was estimated to have a collection efficiency of 75% (for 200 nm particles with 8 elementary charges) for D_p of 100, 200, 400, 600, and 800 nm. An additional increase in collection efficiency of 5% was estimated for incorporating a protrusion that extended the inlet tube closer to the collection surface while keeping the electrodes at a farther distance (Section S1 Figure S1a). We satisfied with this design for fabrication.

The resulting device is a radial ESP with the particles entering through a 10 mm diameter tube, perpendicular to a 25.4 mm diameter and 5 mm thick ZnSe crystal, which sits on the ground electrode, and the top electrode is positioned at 5 mm above the top crystal surface and at a diameter of 36 mm around the crystal (such that the minimum separation between the crystal surface and the electrode is 5 mm). Furthermore, the entry tube is extended by 4 mm (referred as "protrusion") and brought closer to have the exit of the tube 1 mm above the crystal. The electrodes are made using Ag or Cu materials, and the other parts of the device are 3D printed with ABS (including the tube extension). The device is operated to maintain an $E_0 = 1$ kV/mm, voltage difference of $V_0 = 5$ kV, and operating at a flow rate $Q = 2.1$ LPM.

This work was completed prior to the publication of an analytical radial electrostatic collector model by Preger et al. (2020). Their model estimates collection spot size as a function of flowrate and electric field strength in a radial collector with parallel plates and small inlet radii, which could now be used in selection of collector plate or operating parameters for devices which follow these geometric constraints.

2.3 Fabrication via 3D printing

We discuss three considerations for fabrication: material selection, printing protocol, and post-printing assembly and treatment. For rapid-prototyping there are limited materials that can be 3D-printed reliably: nylon, ABS and polylactic acid (PLA); these materials have tradeoffs in print reliability, durability, chemical interferences, and electrical properties. PLA is not stable to heat, less durable, and has known outgassing issues, limiting its application for aerosol chemical analysis. Nylon is a stronger material than ABS but lies higher in the triboelectric series, making it prone to more electrostatic losses of particles near the surface. Moreover, in our observations the main source of leaks in the initial prototypes was through the in-layer-space between each print layer. The spacing was much higher in nylon as it can absorb moisture during and after printing and results in larger printing defects and layer-separation. The additional strength of nylon comes with cost of being more brittle and harder to seal, leaving ABS as our choice of material for this application. The strength of ABS is sufficient for inherently low pressure drop



ESP applications as it has a yield strength of 25 MPa, which is much higher than the expected hoop stress of 1.7 MPa acting
160 on a 50 mm internal diameter cylinder design with a thin 2 mm ABS body operated with an extreme 1 atm pressure.

The 3D Systems CubePro 3D printer was used to fabricate all printed parts. Warping, cracking, curling and stringing was
reduced with proper printing speed, temperature and layer spacing adjustment. The print bed was regularly leveled to better
adjust to the filament feed rate, leading to smoother printed objects. The feed-rate and temperature was self-controlled by the
CubePro 3D printer and the print chamber was kept heated generally up to 55 °C (failure in the chamber heating results in
165 poor print quality due to spatially uneven cooling). Using a pre-heated print chamber along with a water soluble glue that was
applied on the print surface and dried completely before starting each print job substantially improved bed-adhesion, which can
be problematic in longer ABS printing jobs. Finally, the ESP was printed with as few parts as possible to have higher structural
stability and avoid forced turbulence because of material discontinuity at the joints. This strategy required fabrication of parts
with complex overhangs. Using filler materials with dual head printers is a possible solution, but has limited application for
170 larger parts — as the printing volume and time scales cubically to the size on top of which printing the entire hollow part
with a filler substantially increases the chances of print failure. We instead pursued an alternate strategy of printing the parts
tilted at 45°. The parts which have an angle of 90° or lower ranged within $\pm 45^\circ$ with respect to the bed and hence were all
inter-supported, and further strengthened by using simple line or point supports on the surfaces. Increasing the size of the base
on the print bed promoted bed-adhesion, and further use of side supports enabled reliable printing of surfaces supported at the
175 largest theoretical angle (45°).

Further post-assembly and treatment strategies were necessary to reduce gas leak through 1) areas where two parts join and
2) the layer spacing in the print surface. The junctions where two parts assemble were sealed by extending the joining surfaces
outward to act as larger flanges, and were sealed using an o-ring placed in a groove designed for the static axial (face) assembly
where the pressure is lower on the interior. The flanges and the greased (Using GE Bayer Silicones Baysilon grease) o-ring
180 were assembled together using multiple screws along the circumference, using latches, magnets, or clips. In our observation,
even using a calculated number of screws based on the theoretical bite angle sometimes resulted in leaks. A reliable solution
was to use a series of magnets arranged in a circumferential Halbach array that directs the field in the axial direction. Two
such arrays of 16 magnets were designed where each array was housed in a single 3D printed part shaped as a leaf spring to
redirect the axial force evenly over the flange. The combined force applied was around 1 kN and was sufficient to eliminate all
185 leaks. Another practical advantage of using this design was that despite the very strong force, opening the flange was possible
by rotating one of the arrays such that opposite polarities align - resulting in an easy disassembly and reassembly, useful for
changing the ZnSe crystal between experiments.

The inter-layer spacing in the 3D prints was sealed along with smoothening the rough 3D-printed surface by manually
rubbing the outside surface with acetone while pressing down on the surface until no spots were left. Since ABS dissolves
190 in acetone, surfaces are sometimes smoothed by suspending an ABS part in a chamber above an acetone vapor bath. In our
observation, the method resulted in overly softened parts or unsealed portions numerous times due to the sensitivity to the
bath time and the acetone amount. Therefore, the surface and joint sealing procedure was repeated until the assembled device
could hold vacuum at levels of -10 kPa for over 5 minutes. To locate sources of leaks, positive pressure was created using



195 a compressed air flow through the assembly (static pressure in closed system to avoid a pressure buildup inside 3D printed parts, which is a safety concern) and a soap solution was applied over the entire printed surface and joint areas. Leak locations were identified by the resulting bubbles and then sealed. Sealing larger gaps in nylon parts required a coat of epoxy solution thinned using acetone for easier application, which required longer preparation times and higher chances of smaller holes remaining after treatment because of the higher surface tension of the epoxy solution, further enforcing advantages of ABS for prototyping.

200 2.4 Aerosol flow system

Laboratory-generated ammonium sulphate ($(\text{NH}_4)_2\text{SO}_4$) particles were used for ESP performance evaluation. Two flow system setups were used: one to characterize the generated and collected particle size distribution using a scanning mobility particle sizer (SMPS) (Figure 2a), and another to measure the total particle counts collected at higher time resolution over the course of each experiment with a condensation particle counter (CPC) (Figure 2b).

205 Ammonium sulphate particles were continuously nebulized from freshly prepared 5 g/L concentration solutions in milli-Q water with TSI, Inc., 3076 atomizer and dried using silica gel denuder (machined in-house). The particles were passed through a cyclone to remove supermicron particles and the concentration was adjusted with a dilution system before introducing the particles into the ESP. Different bypass lines (red-dotted flow lines) were setup to measure the size-distribution or particle count at different flow-line points. A mass flow controller (MFC, MKS) with a vacuum pump (GAST) was used to maintain
210 the desired ESP flow (2.1 LPM).

The charger was operated at a 6 kV voltage on the Tungsten wire, and the ESP was operated at 5 kV voltage difference between the top electrode and the top surface of the ZnSe crystal. We used a positively biased ground electrode in the ESP (at 1 kV) to avoid potential negative voltage in any part of the assembly. Moreover, as the ZnSe crystal is not perfectly conducting, we observed that the top surface of the ZnSe crystal was around 1 kV voltage higher than the ground electrode voltage, resulting
215 in a top electrode voltage of 7 kV for maintaining the 5 kV voltage difference. The entire assembly was operated at 2.1 LPM flow rate, maintained using two pumps - one connected through the CPC and the other through a mass flow controller.

Particle size distributions $n^\# = dN^\# / d \log D_p$ between 17.5 nm to 982 nm were measured with a scanning phase of 210 s and a down-sampling time of 30 s with an aerosol flow rate of 0.7 LPM and a sheath flow rate of 2 LPM. Size measurements were obtained with 6, 20 and 33 scans at three points of interest: at the inlet of the ESP ($n_{in}^\#$), the outlet of the charger
220 ($n_{ch,out}^\#$) and the outlet of the collector ($n_{col,out}^\#$). Additionally, $n_{ch,out}^\#$ and $n_{in}^\#$ were measured again at the end of the experiment, with 6 and 13 scans respectively. The mean volume of collected particles \bar{V}_p was computed from the collected distribution $(n_{ch,out}^\# - n_{col,out}^\#)Qt$ with flowrate Q and collection interval t .

The transient raw particle count experiment (Figure 2b) was conducted for different collection intervals, t (from 5 minutes to 3 hrs) and adjusting the particle concentration $N_{ch,out}^\#$ to around 9000 – 10000 particles/cm³ i.e. below the operating limit
225 of the CPC. The flow line is switched from measuring $N_{ch,out}^\#$ from the bypass to $N_{col,out}^\#$ in the main line at a resolution of one measurement per second. Because the particle number may drift during the duration of the experiment, the average and deviation in number concentrations over this period ($\bar{N}_{ch,out}^\#$ and $\delta \bar{N}_{ch,out}^\#$, respectively) are characterized for calculation. The



corresponding difference in the concentrations between charger and collector outlet is used to estimate the number of particles collected (N^*) and its error (δN^*).

$$230 \quad N^* = \left(N_{\text{ch,out}}^{\#} - N_{\text{col,out}}^{\#} \right) Qt, \quad \delta N^* = \delta N_{\text{ch,out}}^{\#} Qt \quad (1)$$

N^* and \bar{V}_p are used to calculate the collected mass (Section 2.7).

2.5 Infrared spectroscopy

The IR absorbance spectra of the particle loaded and clean ZnSe crystal were measured with the Vertex 80 with Deuterated Lanthanum α Alanine doped TriGlycine Sulphate (DLaTGS) detector. Each spectrum was measured after purging the measurement chamber for 3 minutes with dry, compressed air (from Bruker gas generator) after introducing the sample, and was measured with an average of 64 scans over $4000 - 400 \text{ cm}^{-1}$ with 4 cm^{-1} resolution. The purged chamber was used as the background for measurement of the sample and clean crystal spectra. The default aperture (Jacquinot stop) setting of 6 mm diameter was used, except for a set of experiments to study the spatial distribution of deposited particles (VAIRS, Section 2.6). The beam spot is approximately 80% greater in diameter than the aperture setting (Bruker rep., personal communication, 240 2018). Two identical ZnSe collection crystals (WG71050 from Thorlabs Inc.) were used for all the experiments. The crystal was cleaned between each loading and IR measurement by alternating between rubbing with a clean wipe (Kimberly Clark 7552) dampened with iso-propyl-alcohol (IPA, =99.8% (GC grade) Sigma Aldrich) and another with milli-Q water.

The raw IR spectra is processed to correct small deviations in the baseline which can arise from changes in background conditions in the IR chamber. In this work, $(\text{NH}_4)_2\text{SO}_4$ was the only test material and a method that automatically corrects the baseline is employed. First, the absorbance spectra of the cleaned collection crystal is subtracted from the particle-loaded absorption spectra. The slope of absorbance values is used in combination with the moving mean of absorbance to identify non-absorbing baseline points (Section S2). A smoothing spline was fitted to interpolate the baseline through absorption regions and then subtracted from the original spectrum. 245

2.6 Spatial profiling

The spatial profile is primarily assessed using optical image analysis, and supported by electron microscopy and a method we refer to as variable aperture infrared spectroscopy (VAIRS) in this work. A top-view image of the ZnSe crystal was taken with an optical camera after each deposition experiment. Using a dark background to contrast the bright ammonium sulfate particles, we took an image of the particle loaded crystal under diffused light using a digital camera (Firefly DE300, focal dept of 35mm with 2048×1536 pixel resolution) kept at a fixed height of 30 cm. The image was analyzed by converting to gray scale (0 to 255 pixel intensity), and finding the radial change in pixel intensity from the analyzed center and periphery of the crystal. 255

Scanning electron microscopy (SEM) analysis was performed to qualitatively assess the particle distribution at different radial positions using the FEI Teneo microscope. Secondary electrons were detected using the Everhart-Thornley detector



detector while using a 5 kV voltage and low 50 pA current to prevent charge build up on the particles. The crystal was
260 introduced in the SEM chamber without any conductive coating and images were taken from a working distance of 6 mm.

For VAIRS analysis, IR absorbance intensities for different apertures (0.25 to 8 mm) were used to compute the surface mass
distribution. By varying the aperture setting, and consequently the beam spot size on the surface (which is around 80% larger
than the aperture), the observed change in absorbance intensity of the peak near 1410 cm^{-1} was representative of the areal mass
density of the deposition under the beam. From the difference in intensities among successive beam areas, the mass per unit
265 annulus area was estimated.

2.7 Quantitative evaluation

The quantitative analysis of spectra outlined in this work is enabled through the condition that small particles are spaced far
apart (weak scattering approximation) on the collecting crystal. Further details for the following statements are provided in
Section S4 and S5. The absorbance contribution from particles is obtained from subtracting the absorbance of the clean crystal
270 from that of the sample. The transmittance T of the sample used for calculation of absorbance is obtained by ratioing the
sample spectrum to single-beam background of the purged chamber, and transmittance T_c of the clean crystal is obtained
prior to the experiments by ratioing a clean ZnSe crystal to the purged chamber background. Neglecting scattering interactions
between particle and crystal and among particles, the absorbance A is related to the mass of deposited particles per unit area
of a disc, $m_a^*(r_b)$, inscribed by the beam radius r_b , substance density ρ , and the decadic volume attenuation coefficient $\alpha_{10,v}$
275 (the Napierian volume attenuation coefficient divided by $\ln 10$) (Adamson, 1979; Bohren and Huffman, 1983; Hapke, 2012):

$$A(\tilde{\nu}) = -\log_{10} T(\tilde{\nu}) + \log_{10} T_c(\tilde{\nu}) = \alpha_{10,v}(\tilde{\nu}) \frac{m_a^*(r_b)}{\rho}. \quad (2)$$

$\alpha_{10,v}/\rho$ is the decadic form of the mass attenuation coefficient, which can be related to the molar attenuation coefficient
previously used to characterize IR response (Allen et al., 1994; Maria, 2003), and also the molecular absorption cross section
used in other applications. Alternatively, the areal mass density $m_a^*(r_b)/\rho$ can be conceptualized as the equivalent thickness of
280 the sample in the form of a void-free film (without coherent interferences).

The mean areal density over the entire crystal $m_a^*(R)/\rho$ is calculated from the total deposited volume m^*/ρ , estimated from
the product of the SMPS and CPC measurement outputs:

$$\frac{m_a^*(R)}{\rho} = \frac{m^*}{\rho\pi R^2}, \text{ where } \frac{m^*}{\rho} = \bar{V}_p N^*. \quad (3)$$

N^* is the cumulative number of particles deposited from the CPC (Eq. 1 and Section 3.1), \bar{V}_p is the mean volume obtained
285 from the measured size distribution from the SMPS (Section 3.1), and ρ is the mass density of the substance (ammonium
sulfate). The mean areal density under the beam is calculated through an adjustment factor $\phi_R(r_b)$:

$$m_a^*(r_b) = \phi_R(r_b) m_a^*(R). \quad (4)$$



The value of this adjustment factor is calculated from the scattered intensity I^* (Section 3.2) integrated over various radii, which is interpreted as being proportional to mass loading:

$$290 \quad \phi_r(r_b) = \frac{m_a^*(r_b)}{m_a^*(R)} \approx \frac{I^*(r_b)/r_b^2}{I^*(R)/R^2}. \quad (5)$$

From measurement, $\alpha_{10,v}(\tilde{\nu})$ is estimated from individual experiments by dividing the apparent absorbance $A(\tilde{\nu})$ by $m_a^*(r_b)/\rho$, or collectively determined by calibration for specific wavenumbers at peak apexes. These values are compared against theoretical values obtained from previously reported refractive indices of ammonium sulfate. Given the size range of particles used in our study (Rayleigh regime), absorption is the dominant process leading to attenuation of IR radiation by particles. In the electrostatics approximation (van de Hulst, 1957), the volume attenuation coefficient of such small particles is related to the vacuum wavenumber $\tilde{\nu}$ and complex refractive index \tilde{n} of the substance comprising the particles (Bohren and Huffman, 1983):

$$295 \quad \alpha_{10,v}(\tilde{\nu}) = \frac{6\pi\tilde{\nu}}{\ln 10} \operatorname{Im} \left\{ \frac{\tilde{n}^2(\tilde{\nu}) - 1}{\tilde{n}^2(\tilde{\nu}) + 2} \right\}. \quad (6)$$

In contrast, the decadic linear absorption coefficient α_{10} that would be used in place of $\alpha_{10,v}$ in Eq. 2 for a homogeneous medium follows a different relation with the refractive index and is also used as a point of comparison:

$$300 \quad \alpha_{10}(\tilde{\nu}) = \frac{4\pi\tilde{\nu}}{\ln 10} \operatorname{Im}\{\tilde{n}(\tilde{\nu})\}. \quad (7)$$

For a collection of tenuous particles (Rayleigh-Gans-Debye approximation), the volume absorption coefficient and linear absorption coefficient are related in the weak absorption limit as $\alpha_{10,v} \approx \alpha_{10}$ (Bohren and Huffman, 1983), but this condition does not strictly apply here due to the sharp contrast in the refractive index of ammonium sulfate and that of the surrounding medium (air). $\alpha_{10,v}$ is evaluated in Section 3.3. The deviation from 1 between the ratio of $\alpha_{10,v}$ to α_{10} is significant especially near the absorption peaks, calculated from reference spectra of Ammonium Sulfate (Earle et al., 2006) (Section S3 Figure S5a).

3 Results and discussions

We discuss the generated and collected particle size distributions (Section 3.1) and spatial deposition profiles (Section 3.2) used to estimate the mass deposited within the probing area of the IR beam, and then evaluate how spectral absorbance relates to this estimated mass (Section 3.3).

310 3.1 Particle size distributions and collection efficiency

The measured average particle size distributions at the charger inlet ($\bar{n}_{in}^\#$), charger outlet ($\bar{n}_{ch,out}^\#$) and collector outlet ($\bar{n}_{col,out}^\#$) according to the described method (Section 2.4) shows a charger penetration of $78\% \pm 6\%$ (over the particle size range $D_p < 982$ nm); and a collection efficiency of $82\% \pm 8\%$ on the fraction of particles at the charger outlet (Figure 3a). The charger efficiency was in accordance with the ones reported in the charger design (between 75% and 90%) at the operating voltage of 6 kV but measured only for higher flow rates (Han et al., 2017). The mass mean diameter of the collector fraction was 207 nm and an additional 5% mass was estimated to have been present in the system, using a log-normal fit extension of the measured



volume distribution (which is limited till 982 nm). The log-normal distribution fit was used to obtain a tail that extended further from 982 nm and was scaled to match the volume distribution at the last bin (982 nm).

320 The Figure 3b shows corresponding normalized number size distribution, where the charger inlet distribution at both the start and at the end of the experiment are included to provide an estimate of expected change in the distribution over the long sampling experiment. The collector did collect some larger particles preferentially but qualitatively there was no large shift in size distribution because of the charger or the collector. Contrary to the observed nominally higher collection for larger particles, COMSOL simulations showed a nominally decreasing collection efficiency with increasing particle size (as the electrical mobility was decreasing) for a charge level proportional to the diameter. The discrepancy is mostly because of larger
325 fraction of larger particles getting charged vs. un-charged in the charger. Numerical simulations had a similar 80% collection efficiency for $D_p = 100, 200, 400, 600,$ and 800 nm with 4, 8, 20, 36, and 48 elementary charges respectively. Qualitatively, the particle distribution imaged by the SEM (Section S1 Figure S3a, b, c) is similar at the three positions and support the idea that there is lower size segregation in collection. Particles were spatially separated, as expected below $5\text{--}20 \mu\text{g}/\text{cm}^2$ (Casuccio et al., 2004), and supports the independent scattering assumption (Drolen and Tien, 1987) over the range of areal mass densities in
330 our experiment ($< 3.15 \mu\text{g}/\text{cm}^2$).

3.2 Spatial mass distribution

The three methods of evaluating the spatial profile (Section 2.6) show that the deposition is semi-uniform. The radial dependence of pixel intensity computed from optical images (Figure 4a) show a general trend for prominent mound near the point where the device inlet tube extrudes towards the surface ($r = 5$ mm), as predicted by simulation (Figure 1b). The presence of
335 the mound is supported by qualitative SEM image analysis which has nominally different particle densities for the different images at different radial positions (1, 6 and 9 mm) (Section S1 Figure S3a, b, c), despite having low qualitative variation in the size distribution. However, there are some observed variations in the relative height of the mound and whether the deposited mass is increasing or decreasing with radial distance. The VAIRS analysis (Section 2.6) of the IR absorbance spectra with different aperture sizes, also closely follows the image analysis profile (Figure 4), though it is much coarser because of limited
340 number of aperture points. These variations across experiments, especially the relative mound intensity, likely results from small perturbations in the vertical position of the crystal placed in the collector disc housing (Section S1 Figure S2a)

The scattered integrated over the entire crystal $I^*(R)$ for each experiment scales with the total mass areal density m_a^* calculated using image analysis (Section S3 Figure S7a) and supports its use for resolving the spatial distribution of deposited mass (albeit making use of variations in intensity over a single experiment). The estimated density scaling factor $\phi_R(r_b)$ for a
345 beam radius of 5.4 mm corresponding to the aperture of 6 mm diameter is ratio of $I^*(r_b)/\pi r_b^2$ to $I^*(R)/\pi R^2$ (Figure 4b), and its deviation from unity (1:1 line in the Figure) is mostly $\pm 10\%$ (with two points at $+20\%$ and $+25\%$). $\phi_R(r_b)$ is systematically higher for the intensity profiles that increases sharply with radius and lower for profiles which have decreasing radial intensities (Figure 4a). The non negligible deviation in $\phi_R(r_b)$ in conjunction with it conserving some detail about the distribution profile, we employ the density scaling factor to estimate the mass, m_a^* , in this work (Section 3.3). A concurrent analysis is done in
350 Supplementary material without the image analysis correction i.e. with a value of $\phi_R(r_b) = 1$ for all samples.



3.3 Absorbance with mass loading

We first examine features of the measured volume attenuation coefficient (effectively, its absorption profile) over the entire range of scanned wavenumbers. Then, we examine the magnitude of the volume attenuation coefficient at two of the major peaks. These quantities are compared against reference values derived from previously reported refractive indices of ammonium sulfate obtained by different methods.

The experimentally-determined volume attenuation coefficient are shown in Figure 5a. The absorbance peak locations and their magnitudes are generally consistent, indicating that the method of measurement and baseline correction does not introduce major chemical or spectroscopic artifacts. Some absorption peaks for aliphatic C-H (2800 - 3150 cm^{-1}) is visible, likely due to impurities on the crystal originating from the o-ring sealing grease in the crystal housing during manual removal of the sample, or condensed vapors on optical components, or impurities in the solvent used for cleaning the crystal (resulting in negative peaks). The o-ring sealing grease most likely contaminates each experiment as most silicone greases use polydimethylsiloxane (PDMS) and absorption bands for both Si-CH₃ (800 cm^{-1} and 1260 cm^{-1}) are visible for all experiments. PDMS IR spectra (Myers et al., 2001) also has a Si-O-Si band (1130 - 1100 cm^{-1}) that can potentially interfere with the SO₄²⁻ absorption peak near 1090 cm^{-1} , but does not appear to materially affect SO₄²⁻ quantification (Section S3 Figure S5a and S6b) and is therefore not further considered in the analysis. The spectra does not appear to contain peaks related to nitrates or other additional artifacts that may be caused by spark discharge and formation of reactive molecules near regions of high electrical potential in the charger or collector. (Such peaks in initial stages of ESP-development were observed where needle electrodes and high voltages were used for charging and collection in a single stage design.) Moreover, no physical heating of the ZnSe crystal was observed after each experiment, which also suggests the absence of sparking and substantial production of reactive gases.

Overlaid on Figure 5a are $\alpha_{10,v}$ and α_{10} calculated from refractive indices measured by (Earle et al., 2006) using ammonium sulfate particles suspended in nitrogen gas in an aerosol flow tube. In our experiments, we observed a consistent peak positions of $\nu_3(\text{SO}_4^{2-}) = 1090 \text{ cm}^{-1} (\pm 0.2\%)$ and $\nu_4(\text{NH}_4^+) = 1415 \text{ cm}^{-1} (\pm 0.08\%)$, which are consistent with reported values for homogeneous samples (Toon et al., 1976) [$\nu_3(\text{SO}_4^{2-}) = 1090 \text{ cm}^{-1}$, $\nu_4(\text{NH}_4^+) = 1415 \text{ cm}^{-1}$] and (Torrie et al., 1972) [$\nu_3(\text{SO}_4^{2-}) = 1093 \text{ cm}^{-1}$, $\nu_4(\text{NH}_4^+) = 1417 \text{ cm}^{-1}$] — though the lack of wavenumber resolution in the older measurements made on dispersive spectrometers prevent a more precise comparison. Blue shifting of peaks on the order of $\sim 10 \text{ cm}^{-1}$ can be expected for small particles (Bohren and Huffman, 1983; Maidment et al., 2018), with asphericity and increasing particle size reducing the extent of this shift (Mishchenko, 1990; Segal-Rosenheimer et al., 2009). Blue-shifts have been reported in extinction spectra of ammonium sulfate in aerosol flow tubes (Weis and Ewing, 1996; Earle et al., 2006; Segal-Rosenheimer et al., 2009; Laskina et al., 2014), though observations are often below that predicted by Mie theory. Such shifts are not observed in our experiments, though the extent of peak shifts, spectral profiles, and the underlying refractive indices vary among various studies (Laskina et al., 2014; Johnson et al., 2020; Myers et al., 2020) and are attributed to some extent on differences arising from sample morphology.

Figure 5b shows the absorbance against the effective deposition thickness for the $\nu_3(\text{SO}_4^{2-})$ peak near 1110 cm^{-1} and $\nu_4(\text{NH}_4^+)$ peak near 1410 cm^{-1} , the slope of which can be compared to $\alpha_{10,v}$ and α_{10} calculated from the refractive indices of



385 (Earle et al., 2006). The reference values are calculated for their respective peaks which vary by a few wavenumbers from our
experiments, as mentioned previously. The experimental absorbance and effective deposition thickness estimates are strongly
correlated (R^2 of 0.95 and 0.94, respectively). While weak bands are typically recommended for quantification of analytes of
inorganic substances (Mayo et al., 2004) due to possibility for signal saturation, for low loadings (low optical depths) for which
single scattering approximation applies, this work confirms that even the strongest absorbance band of $\nu_3(\text{SO}_4^{2-})$ at 1110 cm^{-1}
390 exhibits high linearity and can also be for quantification. The slope values of $1.32 \times 10^4\text{ cm}^{-1}$ (95% confidence interval (CI) of
[1.11, 1.52] $\times 10^4\text{ cm}^{-1}$) for the peak near 1110 cm^{-1} and $5.89 \times 10^3\text{ cm}^{-1}$ (95% CI of [4.87, 6.93] $\times 10^3\text{ cm}^{-1}$) for the peak near
 1410 cm^{-1} vary from the reference values within 20% and -8%, which is within the uncertainty due to variations in reported
refractive indices (Laskina et al., 2014; Johnson et al., 2020; Myers et al., 2020). The variation of the slope from the α_{10} (for
homogeneous medium) is consistent (+20%) for both the peaks. The higher slope of the peak near 1110 cm^{-1} (as also evident
395 from its higher values in Figure 5a) is not because of Si-O-Si band ($1130 - 1100\text{ cm}^{-1}$) from the silicone grease, removing
which the slope still varies by 18% (Section S3 Figure S6b). In our experiments the peak height ratio of $\nu_3(\text{SO}_4^{2-})$ to $\nu_4(\text{NH}_4^+)$
was 2.1 ($\pm 10\%$); consistent with spectra acquired from nebulized and dried polydisperse ammonium sulphate solution (4.8
g/L) with mass mean diameter of 200 nm studied under conditions close to our experiments (Weis and Ewing, 1996). The
consistency of peak height ratios and similarly higher slopes from the linear absorption coefficient (for homogeneous medium)
400 further strengths the observation that the particles deposited on the crystal behave more like a homogeneous medium.

In the analysis above, the ZnSe crystal was not assumed to play a role. Nonmetallic particles collected on the surface of a
substrate can behave optically different from suspended particles due to multiple far-field scattering interactions, van der Waals-
like interactions, and superposition of incident and reflected electromagnetic fields between particle and surface (Quinten,
2011). Scattering power of IR radiation by submicron particles is reasonably small (though increasingly important in the region
405 above 1500 cm^{-1} for larger particles within this range), so these far-field (incoherent) interactions are not considered to be
substantial. Otherwise, deviations in our measurements were within uncertainty of past reference measurements, and systematic
influences of near-field optical effects or physical interactions were not detected within the precision of our technique.

We also evaluate the value of optical microscopy experiments (and corresponding image analysis) in our quantification by
considering a case where a constant density scaling factor is employed — i.e. $\phi_R(r_b) = 1$ for all samples (Section S3 Figure
410 S6a), which results in a shift of the points along the abscissa for each experiment compared to Figure 5b. The correlation with
absorbance remains almost the same (R^2 of 0.96 and 0.95) for the 1110 and 1410 cm^{-1} , respectively. The estimated slope also
remains statistically indifferent, at $1.3 \times 10^4\text{ cm}^{-1}$ (95% CI of [1.14, 1.51] $\times 10^4\text{ cm}^{-1}$) for the peak near 1110 cm^{-1} and 5.9×10^3
 cm^{-1} , (95% CI of [4.95, 6.84] $\times 10^3\text{ cm}^{-1}$) for the peak near 1410 cm^{-1} . The results of the analysis are effectively the same
regardless of whether image analysis is incorporated, because $\phi_R(r_b)$ was effectively close to unity (Section S3 Figure S7b).

415 Finally, we estimate a limit of qualification (LOQ) of $m_a^*(r_b) = 0.012\text{ }\mu\text{g}/\text{cm}^2$ for ammonium sulphate based on the threshold
at which the absorption at 1410 cm^{-1} is ten-fold greater than root mean square of noise (Section S6). This threshold is at least
an order of magnitude lower than for PTFE filters based on reported accounts for other substances or peaks (Russell et al.,
2009; Debus et al., 2021), which is an expected result due to low substrate interferences and baseline uncertainties. For our
current ESP device operating at a flowrate of 2.1 LPM with overall efficiency of 0.64 (for charger and collector), this LOQ



420 translates into a required average airborne concentration threshold of $1.5 \mu\text{g}/\text{m}^3$ of ammonium sulphate over a sampling time of
30 minutes. PTFE sampling can potentially achieve similar time resolutions for quantification of airborne concentrations due
to high particle collection efficiency and flow rate (at the cost of greater pressure drop) than our ESP, which is limited by the
applicable voltage to maintain the strength of electrostatic forces that facilitate particle deposition. However, greater sensitivity
to deposited mass on the optical crystal through ESP collection may confer benefits when the flow rate or total sampled volume
425 is limited, such as in cases of co-sampling from manifolds, environmental chambers, flow reactors, or denuders. Furthermore,
the lower pressure drop and face velocity in the ESP is expected to reduce evaporation artifacts from semivolatile substances
reported for filter sampling (McDow and Huntzicker, 1990; Zhang and McMurry, 1991).

4 Conclusions

This work demonstrates the possibility of using a 3D printed radial ESP for quantitative IR spectroscopy with minimal optical
430 interferences. Rapid prototyping to achieve the presented design was achieved through numerical simulations and 3D-printing
with ABS. To enable 3D-printing of parts for a flow system, the number of joints were minimized by printing with a 45° rotation
to allow fabrication of parts with overhangs, and a small amount of acetone was used for press-sealing surfaces after printing.
Polydisperse ammonium sulfate particles were atomized from solution and studied over 11 experiments with varying particle
loading. The collection area and spatial distribution of particles on the crystal were analyzed using optical image analysis
435 and IR absorbance measured across variable aperture sizes. The mass distribution was estimated to be semiuniform due to the
variation in electrode distances and electric field strengths within the collector. We observed the IR absorbance at $\nu_3(\text{SO}_4^{2-})$ and
 $\nu_4(\text{NH}_4^+)$ peaks at ~ 1410 and $\sim 1110 \text{ cm}^{-1}$ to scale linearly ($R^2 > 0.94$) with particle loading over two orders of magnitude,
with an estimated limit of quantification of 61 ng of collected mass, corresponding to an average airborne concentration of
 $1.5 \mu\text{g}/\text{m}^3$ for a 30 minute sampling interval. The peak positions and peak heights of the extinction spectra were within the
440 variability of previous studies using particles suspended in an inert gas, and particle-substrate effects were not discernable.
While particle extinction should follow the electrostatic approximation for small, separated particles (for areal mass densities
< $3 \mu\text{g}/\text{cm}^2$ and size < $1 \mu\text{m}$ in this work), we find that modeling the particle deposits formed in this work as homogeneous
medium of equivalent mass also provided a reasonable prediction of the apparent absorbance. The advances presented in this
work permit higher sensitivity and chemical resolution for aerosol measurement, and encourage 1) further investigation of this
445 design and analysis strategy for collector design, and 2) use of such a device in studies of aerosol composition for various
applications.



Figures

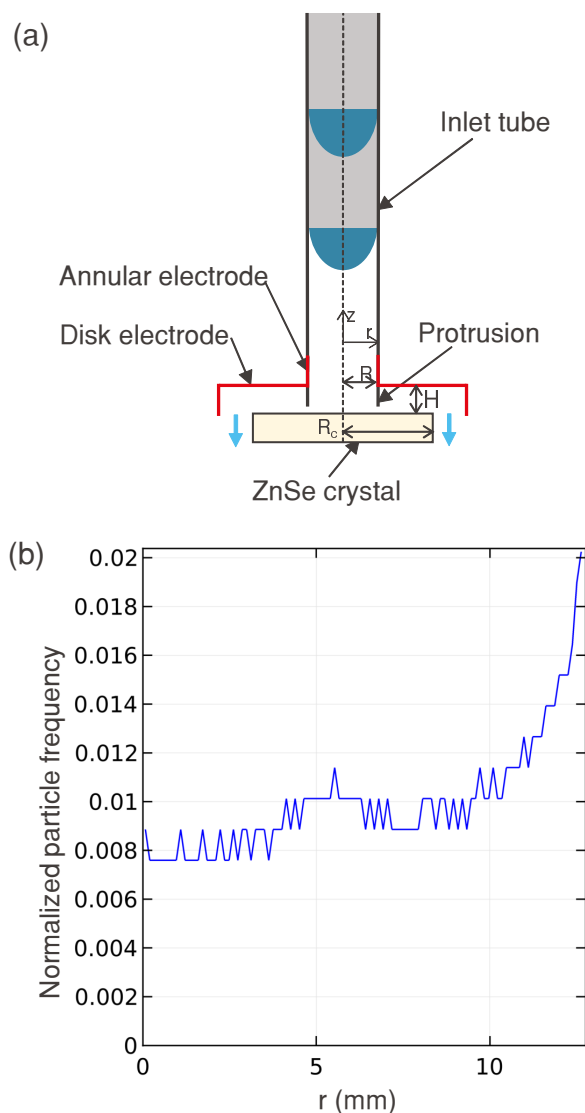


Figure 1. (a) A schematic representation of the radial ESP where particles enter through an inlet tube that is extended closer to the collection crystal through a protrusion. The particles are focused on the crystal using high voltage electrodes near the exit of the tube, and above and around the crystal. (b) Radial particle deposition profile as obtained from COMSOL simulation of velocity, electrostatics and particle tracing on the device in part a - the mound of particles near $r = 5$ mm corresponds to the position of the protrusion.

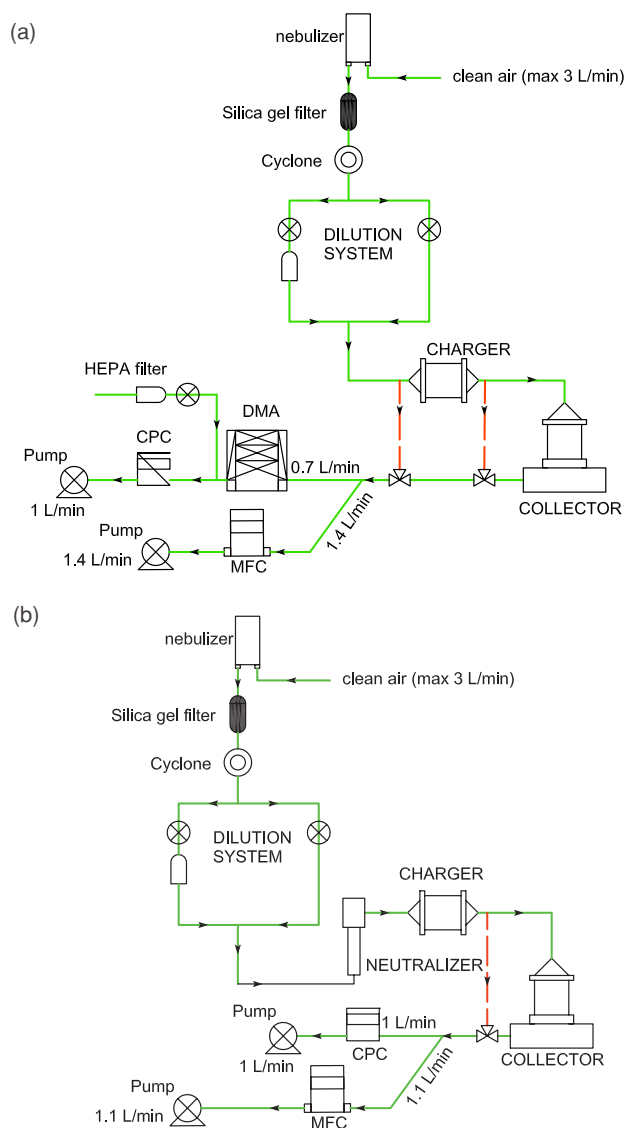


Figure 2. Diagram of the aerosol flow system experiments (green line is the main flow line and the red-dotted lines are the alternate bypass lines) for (a) obtaining the particle size distribution, and (b) obtaining the mass loading reference through the CPC particle counts.

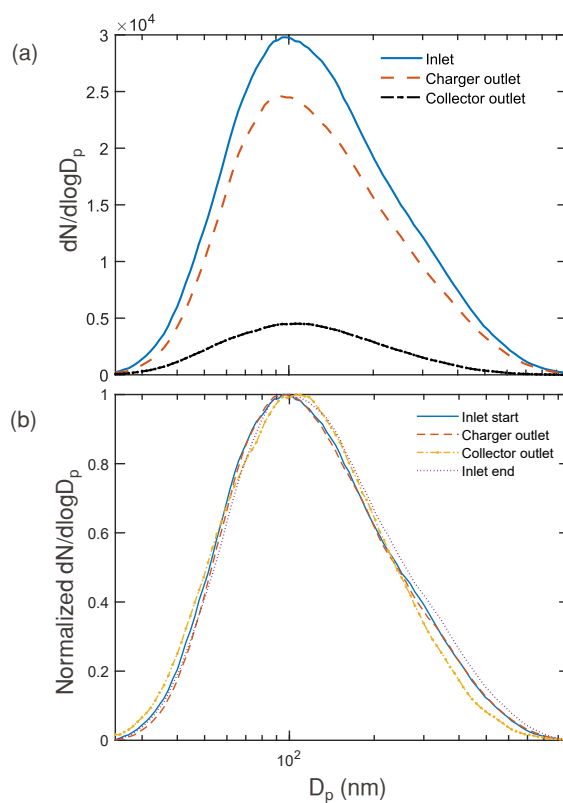


Figure 3. (a) Particle size distribution measured at the inlet averaged from that before and after collection, at the charger outlet averaged from that before and after collection and at the outlet of the collector, and (b) normalized particle size distribution measured for the inlet before starting the experiment, at the outlet of the charger, at the outlet of the collector, and the inlet at the end of the experiment (to determine any bias in the inlet).

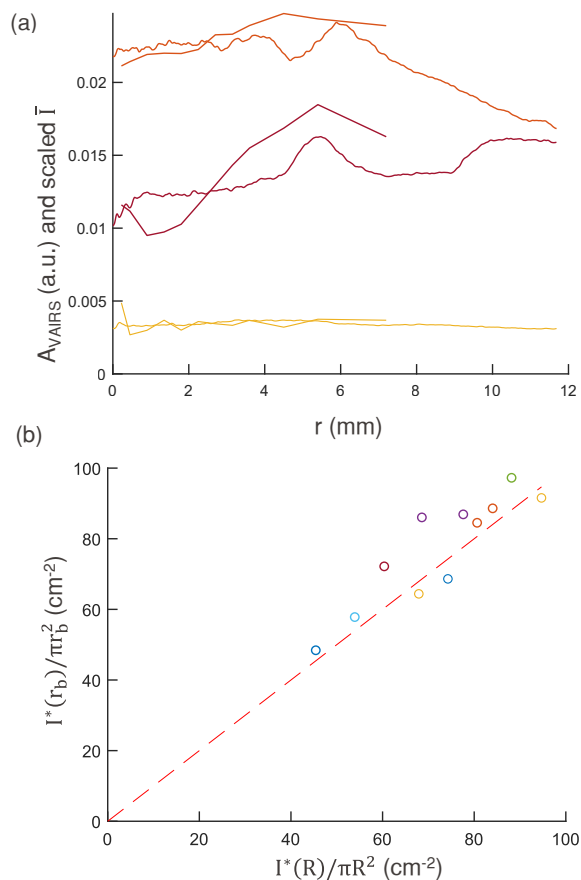


Figure 4. (a) Radial profile of scattered intensities ($\bar{I}(r)$), obtained from image analysis (Section S5) and from VAIRS analysis (A_{VAIRS}). $\bar{I}(r)$ values range to a higher r and have higher resolution than A_{VAIRS} values and are scaled differently for each sample to display it together with the corresponding A_{VAIRS} profile. (b) Calculated $I^*(r_b)/\pi r_b^2$ and $I^*(R)/\pi R^2$ from image analysis for the experiments with different $m_a^*(R)$ and a 1:1 reference line (red-dotted line).

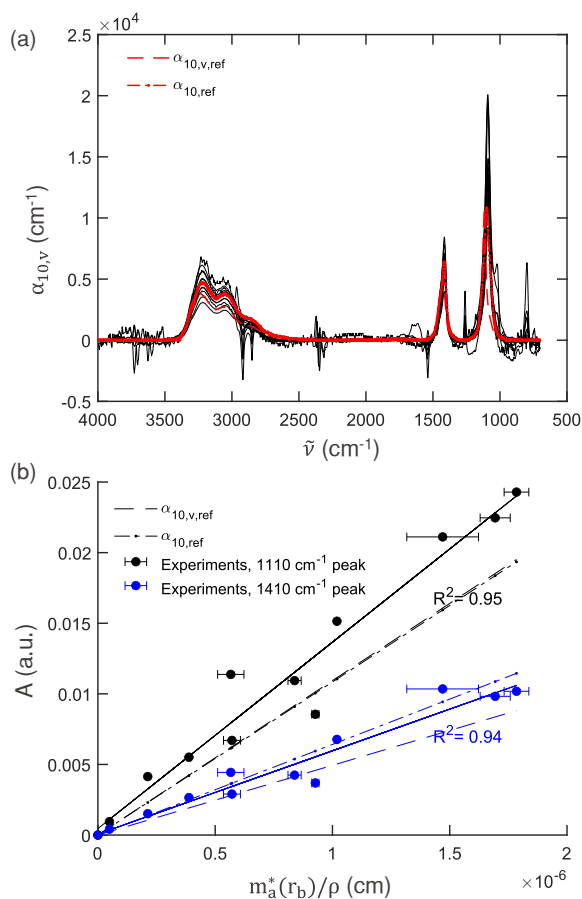


Figure 5. (a) Comparison of volume absorption coefficient (α_v) from the experiments for IR measurement with an aperture of 6mm against the reference linear absorption coefficient (α_{ref}) and volume absorption coefficient ($\alpha_{v,\text{ref}}$) for ammonium sulfate calculated using n and k (Earle et al., 2006). (b) Response of IR absorbance (A) against the effective deposition thickness (cm) of the total particle collected reference from CPC calculated using image analysis, for absorbance at the peak near 1110 cm^{-1} (for $\nu_3(\text{SO}_4^{2-})$) and at the peak near 1410 cm^{-1} (for $\nu_4(\text{NH}_4^+)$).



Author contributions. ND designed and fabricated the device, ran the simulations, prepared and performed the experiments, and performed the data analysis. ST conceived of, acquired funding for, and provided supervision of the project, and provided feedback on the analysis. ND and ST wrote the manuscript.

Competing interests. We declare that no competing interests are present.

Acknowledgements. We thank Dr. Jiannong Fang for discussions on numerical simulations and SNF 200021_172923 for funding.



References

- Adamson, A.: A Textbook of Physical Chemistry, Elsevier Science Techn., https://www.ebook.de/de/product/21133459/arthur_adamson_a_textbook_of_physical_chemistry.html, 1979.
- 455 Allen, D. T., Palen, E. J., Haimov, M. I., Hering, S. V., and Young, J. R.: Fourier transform infrared spectroscopy of aerosol collected in a low pressure impactor (LPI/FTIR): Method development and field calibration, *Aerosol Science and Technology*, 21, 325–342, <https://doi.org/10.1080/02786829408959719>, 1994.
- Allen, M. D. and Raabe, O. G.: Slip Correction Measurements of Spherical Solid Aerosol Particles in an Improved Millikan Apparatus, *Aerosol Science and Technology*, 4, 269–286, <https://doi.org/10.1080/02786828508959055>, 1985.
- 460 Arnold, S. T., Viggiano, A. A., and Morris, R. A.: Rate Constants and Branching Ratios for the Reactions of Selected Atmospheric Primary Cations with n-Octane and Isooctane (2,2,4-Trimethylpentane), *The Journal of Physical Chemistry A*, 101, 9351–9358, <https://doi.org/10.1021/jp972106v>, 1997.
- Biskos, G., Reavell, K., and Collings, N.: Unipolar diffusion charging of aerosol particles in the transition regime, 36, 247–265, <https://doi.org/10.1016/j.jaerosci.2004.09.002>, 2005.
- 465 Blando, J. D., Porcja, R. J., Li, T. H., Bowman, D., Liroy, P. J., and Turpin, B. J.: Secondary formation and the Smoky Mountain organic aerosol: An examination of aerosol polarity and functional group composition during SEAVS, *Environmental Science and Technology*, 32, 604–613, <https://doi.org/10.1021/es970405s>, 1998.
- Blando, J. D., Porcja, R. J., and Turpin, B. J.: Issues in the Quantitation of Functional Groups by FTIR Spectroscopic Analysis of Impactor-
470 Collected Aerosol Samples, *Aerosol Science and Technology*, 35, 899–908, <https://doi.org/10.1080/02786820126852>, 2001.
- Bogard, J. S., Johnson, S. A., Kumar, R., and Cunningham, P. T.: Quantitative analysis of nitrate ion in ambient aerosols by Fourier-transform infrared spectroscopy, *Environmental Science & Technology*, 16, 136–140, <https://doi.org/10.1021/es00097a004>, 1982.
- Bohren, C. and Huffman, D.: *Absorption and Scattering of Light by Small Particles*, Wiley Science Series, Wiley, 1983.
- Burtscher, H., Scherrer, L., Ott, H. C. S. S., Federer, B., Burtscher, H., Scherrer, L., and Siegmann, H. C.: Probing aerosols by photoelectric
475 charging, 3787, <https://doi.org/10.1063/1.331120>, 1982.
- Casuccio, G. S., Schlaegle, S. F., Lersch, T. L., Huffman, G. P., Chen, Y., and Shah, N.: Measurement of fine particulate matter using electron microscopy techniques, *Fuel Processing Technology*, 85, 763–779, <https://doi.org/10.1016/j.fuproc.2003.11.026>, 2004.
- Cunningham, P. T., Johnson, S. A., and Yang, R. T.: Variations in chemistry of airborne particulate material with particle size and time, *Environmental Science & Technology*, 8, 131–135, <https://doi.org/10.1021/es60087a002>, 1974.
- 480 de Rooij, J. J. and Eilers, P. H.: Mixture models for baseline estimation, *Chemometrics and Intelligent Laboratory Systems*, 117, 56–60, <https://doi.org/10.1016/j.chemolab.2011.11.001>, 2012.
- Debus, B., Weakley, A. T., Takahama, S., George, K. M., Schichtel, B., Copleland, S., Wexler, A. S., and Dillner, A. M.: Quantification of major particulate matter species from a single filter type using infrared spectroscopy – Application to a large-scale monitoring network, *Atmospheric Measurement Techniques Discussions*, 2021, 1–29, <https://doi.org/10.5194/amt-2021-382>, 2021.
- 485 Dixkens, J. and Fissan, H.: Electrostatic particle sampler for total-reflection X-ray fluorescence analysis, *Journal of Aerosol Science*, 22, S375–S378, [https://doi.org/10.1016/s0021-8502\(05\)80116-8](https://doi.org/10.1016/s0021-8502(05)80116-8), 1991.
- Drolen, B. and Tien, C.: Absorption and scattering of agglomerated soot particulate, *Journal of Quantitative Spectroscopy and Radiative Transfer*, 37, 433–448, [https://doi.org/10.1016/s0022-4073\(87\)90090-2](https://doi.org/10.1016/s0022-4073(87)90090-2), 1987.



- 490 Earle, M. E., Pancescu, R. G., Cosic, B., Zsetsky, A. Y., and Sloan, J. J.: Temperature-Dependent Complex Indices of Refraction for Crystalline (NH₄)₂SO₄, *The Journal of Physical Chemistry A*, 110, 13 022–13 028, <https://doi.org/10.1021/jp064704s>, 2006.
- Fierz, M.: Theoretical and Experimental Evaluation of a Portable Electrostatic TEM Sampler, *Aerosol Science and Technology*, 41, 520–528, <https://doi.org/10.1080/02786820701253327>, 2007.
- Fischer, K.: Mass absorption indices of various types of natural aerosol particles in the infrared, *Applied Optics*, 14, 2851, <https://doi.org/10.1364/ao.14.002851>, 1975.
- 495 Grob, B., Burtscher, H., and Niessner, R.: Charging of ultra-fine aerosol particles by an ozone-free indirect uv photo-charger, *Aerosol Science and Technology*, 47, 1325–1333, <https://doi.org/10.1080/02786826.2013.840357>, 2013.
- Grob, B., Wolf, J. C., Kiwull, B., and Niessner, R.: Calibration system with an indirect photoelectric charger for legislated vehicle number emission measurement counters in the single counting mode, *Journal of Aerosol Science*, 70, 50–58, <https://doi.org/10.1016/j.jaerosci.2014.01.001>, 2014.
- 500 Haedel, G.: Radiation budget of the boundary layer. II- Simultaneous measurement of mean solar volume absorption and extinction coefficients of particles, *Beiträge zur Physik der Atmosphäre*, 60, 241–254, http://scholar.google.com/scholar_lookup?hl=en&volume=60&publication_year=1987&pages=241-247&author=G.+H%C3%A4nel&title=Radiation+budget+of+the+boundary+layer%3A+Part+II%2C+Simultaneous+Measurement+of+Mean+Solar+Volume+Absorption+and+Extinction+Coefficients+of+Particles, 1987.
- Han, B., Kim, H.-j., Kim, Y.-j., Sioutas, C., Han, B., Kim, H.-j., Kim, Y.-j., and Sioutas, C.: Unipolar Charging of Fine and Ultra-Fine Particles Using Carbon Fiber Ionizers Unipolar Charging of Fine and Ultra-Fine Particles Using Carbon Fiber Ionizers, 6826, <https://doi.org/10.1080/02786820802339553>, 2008.
- 505 Han, T. T., Thomas, N. M., and Mainelis, G.: Design and development of a self-contained personal electrostatic bioaerosol sampler (PEBS) with a wire-to-wire charger, *Aerosol Science and Technology*, 51, 903–915, <https://doi.org/10.1080/02786826.2017.1329516>, 2017.
- Hapke, B.: Bidirectional reflectance spectroscopy 7, *Icarus*, 221, 1079–1083, <https://doi.org/10.1016/j.icarus.2012.10.022>, 2012.
- 510 Harrick, N. J. and Beckmann, K. H.: *Internal Reflection Spectroscopy*, pp. 215–245, Springer US, Boston, MA, https://doi.org/10.1007/978-1-4613-4490-2_11, 1974.
- Hewitt, G. W.: The charging of small particles for electrostatic precipitation Part I: Communication and Electronics, *Transactions of the American Institute of Electrical Engineers*, 76, 300–306, <https://doi.org/10.1109/TCE.1957.6372672>, 1957.
- Hontañón, E. and Kruis, F. E.: Single Charging of Nanoparticles by UV Photoionization at High Flow Rates, *Aerosol Science and Technology*, 515 42, 310–323, <https://doi.org/10.1080/02786820802054244>, 2008.
- Hopey, J., Fuller, K., and Krishnaswamy, V.: Fourier transform infrared spectroscopy of size-segregated aerosol deposits on foil substrates, *Applied optics*, 47, 2266–74, 2008.
- Ivlev, L. S. and Popova, S. I.: The Complex Refractive Indices of Substances in The Atmospheric-Aerosol Dispersed Phase, 9, 1034–1043, 1973.
- 520 Johnson, T. J., Diaz, E., Hughey, K. D., Myers, T. L., Blake, T. A., Dohnalkova, A. C., and Burton, S. D.: Infrared Optical Constants from Pressed Pellets of Powders: I. Improved n and k Values of (NH₄)₂SO₄ from Single-Angle Reflectance, *Applied Spectroscopy*, 74, 851–867, <https://doi.org/10.1177/0003702820930009>, 2020.
- Kala, S., Rouenhoff, M., Theissmann, R., and Kruis, F. E.: Synthesis and Film Formation of Monodisperse Nanoparticles and Nanoparticle Pairs, in: *Nanoparticles from the Gasphase*, pp. 99–119, Springer Berlin Heidelberg, https://doi.org/10.1007/978-3-642-28546-2_4, 2012.
- 525 Kimoto, S., Saiki, K., Kanamaru, M., and Adachi, M.: A small mixing-type unipolar charger (SMUC) for nanoparticles, *Aerosol Science and Technology*, 44, 872–880, <https://doi.org/10.1080/02786826.2010.498796>, 2010.



- Kuzmiakova, A., Dillner, A. M., and Takahama, S.: An automated baseline correction protocol for infrared spectra of atmospheric aerosols collected on polytetrafluoroethylene (Teflon) filters, *Atmospheric Measurement Techniques*, 9, 2615–2631, <https://doi.org/10.5194/amt-9-2615-2016>, 2016.
- 530 Laskina, O., Young, M. A., Kleiber, P. D., and Grassian, V. H.: Infrared Optical Constants of Organic Aerosols: Organic Acids and Model Humic-Like Substances (HULIS), *Aerosol Science and Technology*, 48, 630–637, <https://doi.org/10.1080/02786826.2014.904499>, 2014.
- Liland, K. H., Alm-Åy, T., and Mevik, B.-H.: Optimal Choice of Baseline Correction for Multivariate Calibration of Spectra, *Applied Spectroscopy*, 64, 1007–1016, <https://www.osapublishing.org/as/abstract.cfm?uri=as-64-9-1007>, 2010.
- Liu, B. Y. H. and Pui, D. Y. H.: LIU and DAVID, 6, 1975.
- 535 Maidment, L., Schunemann, P. G., Clewes, R. J., Bowditch, M. D., Howle, C. R., and Reid, D. T.: Systematic spectral shifts in the mid-infrared spectroscopy of aerosols, *Optics Express*, 26, 18 975, <https://doi.org/10.1364/oe.26.018975>, 2018.
- Maria, S. F.: Source signatures of carbon monoxide and organic functional groups in Asian Pacific Regional Aerosol Characterization Experiment (ACE-Asia) submicron aerosol types, *Journal of Geophysical Research*, 108, <https://doi.org/10.1029/2003jd003703>, 2003.
- Marple, V. A.: History of Impactors—The First 110 Years, *Aerosol Science and Technology*, 38, 247–292, <https://doi.org/10.1080/02786820490424347>, 2004.
- 540 Marquard, A.: Unipolar Field and Diffusion Charging in the Transition Regime—Part I: A 2-D Limiting-Sphere Model, *Aerosol Science and Technology*, 41, 597–610, <https://doi.org/10.1080/02786820701272053>, 2007.
- Marquard, A., Meyer, J., and Kasper, G.: Characterization of unipolar electrical aerosol chargers-Part II: Application of comparison criteria to various types of nanoaerosol charging devices, *Journal of Aerosol Science*, 37, 1069–1080, <https://doi.org/10.1016/j.jaerosci.2005.09.002>, 2006.
- 545 Mayo, D. W., Miller, F. A., and Hannah, R. W., eds.: *Course Notes on the Interpretation of Infrared and Raman Spectra*, John Wiley & Sons, Inc., <https://doi.org/10.1002/0471690082>, p.333, 2004.
- Mcclenny, W., Childers, J., Röhl, R., and Palmer, R.: FTIR transmission spectrometry for the nondestructive determination of ammonium and sulfate in ambient aerosols collected on teflon filters, *Atmospheric Environment* (1967), 19, 1891–1898, [https://doi.org/10.1016/0004-6981\(85\)90014-9](https://doi.org/10.1016/0004-6981(85)90014-9), 1985.
- 550 McDade, C. E., Dillner, A. M., and Indresand, H.: Particulate Matter Sample Deposit Geometry and Effective Filter Face Velocities, *Journal of the Air & Waste Management Association*, 59, 1045–1048, <https://doi.org/10.3155/1047-3289.59.9.1045>, 2009.
- McDow, S. R. and Huntzicker, J. J.: Vapor adsorption artifact in the sampling of organic aerosol: Face velocity effects, *Atmospheric Environment*. Part A. General Topics, 24, 2563–2571, [https://doi.org/10.1016/0960-1686\(90\)90134-9](https://doi.org/10.1016/0960-1686(90)90134-9), 1990.
- 555 Medved, A., Dorman, F., Kaufman, S., and Pöcher, A.: A new corona-based charger for aerosol particles, *Journal of Aerosol Science*, 31, 616–617, [https://doi.org/10.1016/S0021-8502\(00\)90625-6](https://doi.org/10.1016/S0021-8502(00)90625-6), 2000.
- Milosevic, M.: *Internal Reflection and ATR Spectroscopy*, *Chemical Analysis: A Series of Monographs on Analytical Chemistry and Its Applications*, John Wiley & Sons, Inc., 2012.
- Mishchenko, M. I.: Extinction of light by randomly-oriented non-spherical grains, *Astrophysics and Space Science*, 164, 1–13, <https://doi.org/10.1007/bf00653546>, 1990.
- 560 Myers, T. L., Tonkyn, R. G., Oeck, A. M., Danby, T. O., Loring, J. S., Taubman, M. S., Sharpe, S. W., Birnbaum, J. C., and Johnson, T. J.: online, <https://webbook.nist.gov/cgi/cbook.cgi?ID=C63148629&Mask=80#Refs>, 2001.



- Myers, T. L., Blake, T. A., Yokosuk, M. O., Fortin, G., and Johnson, T. J.: Improved Infrared Optical Constants from Pressed Pellets: II. Ellipsometric n and k Values for Ammonium Sulfate with Variability Analysis, *Applied Spectroscopy*, 74, 868–882, <https://doi.org/10.1177/0003702820928358>, 2020.
- 565 Nishida, R. T., Boies, A. M., and Hochgreb, S.: Measuring ultrafine aerosols by direct photoionization and charge capture in continuous flow, *Aerosol Science and Technology*, 52, 546–556, <https://doi.org/10.1080/02786826.2018.1430350>, 2018.
- Northrop, R. B.: *Signals and Systems Analysis in Biomedical Engineering*, CRC Press, Boca Raton, FL, 2nd edn., 2011.
- Ofner, J., Krüger, H.-U., Zetzsch, C., and Grothe, H.: Direct Deposition of Aerosol Particles on an ATR Crystal for FTIR Spectroscopy Using an Electrostatic Precipitator, *Aerosol Science and Technology*, 43, 794–798, <https://doi.org/10.1080/02786820902946612>, 2009.
- 570 Parks, D. A., Griffiths, P. R., Weakley, A. T., and Miller, A. L.: Quantifying elemental and organic carbon in diesel particulate matter by mid-infrared spectrometry, *Aerosol Science and Technology*, 55, 1014–1027, <https://doi.org/10.1080/02786826.2021.1917764>, 2021.
- Petzold, A. and Schönlinner, M.: Multi-angle absorption photometry—a new method for the measurement of aerosol light absorption and atmospheric black carbon, *Journal of Aerosol Science*, 35, 421–441, <https://doi.org/10.1016/j.jaerosci.2003.09.005>, 2004.
- 575 Pollard, M., Jaklevic, J., and Howes, J.: Analysis of Carbon Particle Deposition on Teflon Filters Using Fourier Transform Infrared Spectroscopy, *Aerosol Science and Technology*, 12, 182–193, <https://doi.org/10.1080/02786829008959338>, 1990.
- Preger, C., Overgaard, N. C., Messing, M. E., and Magnusson, M. H.: Predicting the deposition spot radius and the nanoparticle concentration distribution in an electrostatic precipitator, *Aerosol Science and Technology*, pp. 1–11, <https://doi.org/10.1080/02786826.2020.1716939>, 2020.
- 580 Quinten, M.: *Optical Properties of Nanoparticle Systems: Mie and Beyond*, Wiley-VCH Verlag & Co. KGaA, Weinheim, 2011.
- Reff, A., Turpin, B. J., Offenberg, J. H., Weisel, C. P., Zhang, J., Morandi, M., Stock, T., Colome, S., and Winer, A.: A functional group characterization of organic PM_{2.5} exposure: Results from the RIOPA study RID C-3787-2009, *Atmospheric Environment*, 41, 4585–4598, <https://doi.org/10.1016/j.atmosenv.2007.03.054>, 2007.
- Russell, L. M., Takahama, S., Liu, S., Hawkins, L. N., Covert, D. S., Quinn, P. K., and Bates, T. S.: Oxygenated fraction and mass of organic aerosol from direct emission and atmospheric processing measured on the R/V Ronald Brown during TEXAQS/GoMACCS 2006, *Journal of Geophysical Research*, 114, <https://doi.org/10.1029/2008jd011275>, 2009.
- 585 Ruthenburg, T. C., Perlin, P. C., Liu, V., McDade, C. E., and Dillner, A. M.: Determination of organic matter and organic matter to organic carbon ratios by infrared spectroscopy with application to selected sites in the IMPROVE network, *Atmospheric Environment*, 86, 47–57, <https://doi.org/10.1016/j.atmosenv.2013.12.034>, 2014.
- 590 Sax, M., Zenobi, R., Baltensperger, U., and Kalberer, M.: Time Resolved Infrared Spectroscopic Analysis of Aerosol Formed by Photo-Oxidation of 1,3,5-Trimethylbenzene and α -Pinene, *Aerosol Science and Technology*, 39, 822–830, <https://doi.org/10.1080/02786820500257859>, 2005.
- Scanlon, K., Laux, L., and Overend, J.: The Determination of Absolute Infrared Intensities with a Fourier Transform Spectrometer, *Applied Spectroscopy*, 33, 346–348, <https://doi.org/10.1366/0003702794925552>, 1979.
- 595 Segal-Rosenheimer, M., Dubowski, Y., and Linker, R.: Extraction of optical constants from mid-IR spectra of small aerosol particles, *Journal of Quantitative Spectroscopy and Radiative Transfer*, 110, 415–426, <https://doi.org/10.1016/j.jqsrt.2009.01.005>, 2009.
- Shimada, M., Okuyama, R. K., Inoue, Y., S, M. A., and T, T. F.: Removal of Airborne Particles By a Device Using Uv / Photoelectron Method Under Reduced Pressure Conditions, 30, 341–353, 1999.
- Takahama, S., Johnson, A., and Russell, L. M.: Quantification of Carboxylic and Carbonyl Functional Groups in Organic Aerosol Infrared Absorbance Spectra, *Aerosol Science and Technology*, 47, 310–325, <https://doi.org/10.1080/02786826.2012.752065>, 2013.
- 600



- Takahama, S., Dillner, A. M., Weakley, A. T., Reggente, M., Bürki, C., Lbadaoui-Darvas, M., Debus, B., Kuzmiakova, A., and Wexler, A. S.: Atmospheric particulate matter characterization by Fourier transform infrared spectroscopy: a review of statistical calibration strategies for carbonaceous aerosol quantification in US measurement networks, *Atmospheric Measurement Techniques*, 12, 525–567, <https://doi.org/10.5194/amt-12-525-2019>, 2019.
- 605 Toon, O. B., Pollack, J. B., Khare, B. N., and Owen: The optical constants of several atmospheric aerosol species: Ammonium sulfate, aluminum oxide, and sodium chloride, *Journal of Geophysical Research*, 81, 5733–5748, <https://doi.org/10.1029/jc081i033p05733>, 1976.
- Torrie, B., Lin, C., Binbrek, O., and Anderson, A.: Raman and infrared studies of the ferroelectric transition in ammonium sulphate, *Journal of Physics and Chemistry of Solids*, 33, 697–709, [https://doi.org/10.1016/0022-3697\(72\)90078-9](https://doi.org/10.1016/0022-3697(72)90078-9), 1972.
- Tsai, C.-j., Lin, G.-y., Chen, H.-l., Huang, C.-h., Tsai, C.-j., Lin, G.-y., Chen, H.-l., Huang, C.-h., and Alonso, M.: Enhancement of Extrinsic
610 Charging Efficiency of a Nanoparticle Charger with Multiple Discharging Wires Enhancement of Extrinsic Charging Efficiency of a Nanoparticle Charger with Multiple Discharging Wires, 6826, <https://doi.org/10.1080/02786826.2010.492533>, 2010.
- Tsai, Y. I. and Kuo, S.-C.: Development of diffuse reflectance infrared Fourier transform spectroscopy for the rapid characterization of aerosols, vol. 40, pp. 1781–1793, <https://doi.org/10.1016/j.atmosenv.2005.11.023>, 2006.
- van de Hulst, H. C.: *Light Scattering by Small Particles*, Dover Publications Inc., 1957.
- 615 Villares, G., Hugi, A., Blaser, S., and Faist, J.: Dual-comb spectroscopy based on quantum-cascade-laser frequency combs, *Nature Communications*, 5, <https://doi.org/10.1038/ncomms6192>, 2014.
- Virtanen, A., Joutsensaari, J., Koop, T., Kannosto, J., Yli-Pirila, P., Leskinen, J., Makela, J. M., Holopainen, J. K., Poeschl, U., Kulmala, M., Worsnop, D. R., and Laaksonen, A.: An amorphous solid state of biogenic secondary organic aerosol particles, *Nature*, 467, 824–827, <https://doi.org/10.1038/nature09455>, 2010.
- 620 Volckens, J. and Leith, D.: Electrostatic Sampler for Semivolatile Aerosols: Chemical Artifacts, *Environmental Science & Technology*, 36, 4608–4612, <https://doi.org/10.1021/es0207100>, 2002.
- Weis, D. D. and Ewing, G. E.: Infrared spectroscopic signatures of (NH₄)₂SO₄ aerosols, *Journal of Geophysical Research: Atmospheres*, 101, 18 709–18 720, <https://doi.org/10.1029/96jd01543>, 1996.
- Whitby, K. T.: Generator for Producing High Concentrations of Small Ions, *Review of Scientific Instruments*, 32, 1351–1355,
625 <https://doi.org/10.1063/1.1717250>, 1961.
- Yazdani, A., Dudani, N., Takahama, S., Bertrand, A., Prévôt, A. S. H., Haddad, I. E., and Dillner, A. M.: Characterization of primary and aged wood burning and coal combustion organic aerosols in an environmental chamber and its implications for atmospheric aerosols, *Atmospheric Chemistry and Physics*, 21, 10 273–10 293, <https://doi.org/10.5194/acp-21-10273-2021>, 2021.
- Zhang, X. and McMurry, P. H.: Theoretical analysis of evaporative losses of adsorbed or absorbed species during atmospheric aerosol
630 sampling, *Environmental Science & Technology*, 25, 456–459, <https://doi.org/10.1021/es00015a012>, 1991.