

Applicability of the ~~low-cost optical particle counter~~ Low-Cost Optical Particle Counter OPC-N3 for ~~microphysical measurements~~ Microphysical Measurements of fog. Fog

Katarzyna Nurowska¹, Moein Mohammadi¹, Szymon Malinowski¹, and Krzysztof Markowicz¹

¹Institute of Geophysics, Faculty of Physics, University of Warsaw, Warsaw, Poland

Correspondence: Katarzyna Nurowska (knurowska@fuw.edu.pl)

Abstract. Low-cost devices for particulate matter measurements are characterized by small dimensions and a light weight. This advantage makes them ideal for UAV measurements, where those parameters are crucial. However, they also have some issues; ~~like the~~. The values of particulate matter from low-cost optical particle counters can be biased by high ambient humidity. In this article, we ~~are evaluating~~ evaluate low-cost optical particle counter Alphasense OPC-N3 for measuring the microphysical properties of fog. This study aimed to show that OPC-N3 not only registers aerosols or humidified aerosols but also registers fog droplets.

The study was ~~done~~ carried out on the rooftop of the Institute of Geophysics, University of Warsaw, Poland, during autumn-winter 2021. To validate the results, the data from OPC-N3 were compared with the data obtained from the reference instrument, ~~which was the~~ Oxford Laser VisiSize D30. VisiSize D30 is a shadowgraph device able to register photos of individual droplets.

~~Taking into consideration~~ Considering the effective radius of droplets, it is possible to differentiate low-visibility situations between fog conditions (which are not hazardous for people) from haze events, when highly polluted air can cause health risks to people.

The compared microphysical properties were liquid water content (LWC), number concentration (N_c), effective radius $\langle r_{eff} \rangle$ r_{eff} and statistical moments of radius. The Pearson correlation coefficient between both devices for LWC was ~~0.94~~ 0.92, N_c was ~~0.94~~ 0.95, and for $\langle r_{eff} \rangle$ r_{eff} was 0.63. Overall, these results suggest ~~a~~ good compliance between ~~devices~~ instruments. However, the OPC-N3 has to be corrected ~~in reference to~~ regarding professional equipment. ~~To conclude, our study provides the foundation for a new application of the optical particle counter Alphasense OPC-N3 within UAV to measure the vertical profiles of the microphysical properties of fog.~~

20 1 Introduction

Fog is defined as a layer of water droplets (or ice crystals) near the Earth's surface, which reduces visibility to below 1 km. ~~There are several different types of fog, depending~~ (Gultepe, 2007). Depending on the cause which helps in forming it, there are different types of fog, e.g., radiation fog, advection fog, and valley fog. Radiation fog forms in the evening when the heat absorbed by the Earth's surface during the day is radiated into the air. The ~~cold surface cools down~~ air near the ground cools

25 ~~down when the air reaches saturation, and the air-causing condensation of water forming the~~ first layer of fog forms. Fog phenomenon can affect from the small scale (valley fog) to size region of the whole country.

~~It~~ Fog is a dangerous phenomenon for transport safety (Gultepe et al., 2015; Bartok et al., 2012), which causes ~~not only~~ increased road accidents ~~, but also as well as~~ downtime of aircraft flights. This phenomenon affects the carriage of goods by land, air and maritime transport, causing financial losses similar to those caused by extreme weather events (Kulkarni et al., 30 2019; Price et al., 2018).

The research by Vautard et al. (2009) shows that ~~fogs in Europe have~~ fog in Europe has decreased significantly in the last 30 years. This can be the outcome of an increase in air temperature (Klemm and Lin (2016)). However, the fog decrease trend is spatially and temporally correlated with a negative trend in sulphur dioxide emissions, indicating that air quality policies ~~have a significant impact on fog occurrence~~ significantly impact fog occurrence (Vautard et al., 2009).

35 ~~Particle~~ Particulate matter (PM) is a suspension of ~~particles of solids or liquids~~ solid or liquid particles in the air ~~such as dust, , such as, for example, dust or~~ soot. Aerosol is ~~an important a critical~~ component that contributes to fog formation. ~~Decrease of~~ A decrease in PM can cause changes in fog occurrence or its microphysics. Fog is generated with relatively low ~~super saturation~~ super saturation (SS). Mazoyer et al. (2022) showed that the amount of activated aerosol depends more on the aerosol size than ~~on~~ its chemical composition. Numerical simulations conducted by Tsai et al. (2021) show that for urban aerosols (~~similar to the~~ 40 ~~marine aerosol~~), a higher ~~number~~ density of aerosols resulted in more ~~, but~~ smaller droplets and increased liquid water content (LWC). The effect of urban aerosols was more pronounced near the surface, where the aerosols were most concentrated. ~~This result is consistent with Maalick et al. (2016), however, they also show that absorbing aerosols can lead to a decrease in LWC resulting in a shallower fog.~~

The decrease ~~of in~~ fog events in Europe coincides with the reduction of particulate matter. Between 1998 and 2010, Barm- 45 padimos et al. (2012) found that in Europe, the concentration of PM₁₀ (particulate matter of sizes less than 10 µm) decreased, the mean trends were -0.4 µg m⁻³ per year. According to Colette and Rouil (2021) the median annual concentration of PM₁₀ decreased by 40 % in Europe from 2000 to 2017. The decrease in PM_{2.5} after 2008 was visible, but less pronounced. PM concentrations decrease due to the reduction of primary PM emissions, but also due to the reduction of PM precursors, such as SO_x, NO_x and NH₃. The mentioned studies agree with ~~with~~ Beloconi and Vounatsou (2021) where it was shown that ~~during~~ 50 ~~over a span of~~ 14 years (2006-2019), the concentrations of PM₁₀ and PM_{2.5} decreased by 36.5% and 39.1%, respectively.

The decrease in PM₁₀ and PM_{2.5} is thanks to social awareness. Many countries have introduced restrictions on the amount of PM₁₀ and PM_{2.5} emitted during the day and year. ~~Due~~ Thanks to the growing awareness of the community, the networks measuring the concentration of PM₁₀ and PM_{2.5} are growing (Considine et al., 2021; Feinberg et al., 2019). Consequently, ~~there~~ are increasingly inexpensive and simple PM sensors are available on the market.

55 Low-cost optical particle counters (OPC) are based on measuring light scattering on suspended particles in the air. Light scattering can be enhanced by water droplets. Thus, the reported values of PM are overestimated because of the water uptake by the particles. It is shown that for some low-cost OPCs, the measured PM is dependent on ambient humidity (e.g., Liu et al., 2019; Wang et al., 2015; Badura et al., 2018; Jayaratne et al., 2018). To remove the bias, the air should be dehumidified or correction methods should be applied, as proposed by Crilley et al. (2018).

60 Most ~~of the~~ fog studies focus on ground measurements or numerical ~~modelling~~ modeling. Current weather forecasts have a problem with ~~the~~ high precision of fog forecasting. ~~It~~ ~~This~~ is due to many processes in the lower boundary layer that are involved in its evolution. The processes that influence the development and duration of fog are, for example, droplet microphysics, aerosol hygroscopicity or radiation and turbulent processes (Gultepe et al., 2007). ~~Fog is also affected by local surface conditions, as it develops in the immediate vicinity~~ ~~The local surface fluctuations of temperature or humidity have a high impact~~
65 ~~on the model prediction of fog conditions~~ (Hu et al., 2017).

Microphysical models are based on microphysical parameters such as the total droplet number concentration (N_c), ~~the mean droplet diameter (\bar{D}) and LWC~~, ~~mean volume droplet diameter \bar{D}_V , LWC~~ (Gultepe et al., 2017). Based on in situ measurements, many works provide the range for LWC: $0.01 - 0.5 \text{ g m}^{-3}$ (although the value typically does not exceed 0.2 g m^{-3}); N_c : $10 - 500 \text{ cm}^{-3}$ and \bar{D} : $10 - 20 \text{ }\mu\text{m}$ (e.g., Pruppacher and Klett, 2010; Liu et al., 2011; Tsai et al., 2021; Mazoyer et al., 2019, 2022)
70 . However, these parameters show a large variability (e.g., Pruppacher and Klett, 2010; Liu et al., 2011; Tsai et al., 2021; Mazoyer et al., 20

The ~~standard device used to measure fog microphysics is the~~ Fog Monitor FM-120 from Droplet Measurement Technologies ~~is the standard device for measuring fog microphysics~~. It is an optical spectrometer that can measure the droplet size distribution (DSD(r)) from $2 \text{ }\mu\text{m}$ to $50 \text{ }\mu\text{m}$ ~~in 23 channels (size bins)~~, ~~FM-120 can generate particle-by-particle files~~. It can be used to obtain
75 information on N_c , LWC, and visibility. This instrument is widely used to measure fog, ~~allowing a consistent comparison of the results with those obtained in other studies~~ ~~and allows for consistent comparison based on various field observations~~ (e.g., Weston et al., 2022; Gultepe et al., 2021; Mazoyer et al., 2019; Degefie et al., 2015; Gultepe et al., 2009).

Another in situ device is Cloud Droplet Probe 2 (CDP-2) ~~that~~, ~~which~~ illuminates the droplets and measures the intensity of the forward-scattered light. ~~Droplets are measured in the range of $2 \text{ }\mu\text{m}$ to $50 \text{ }\mu\text{m}$ and N_c to 2000 cm^{-3}~~ . This device was
80 used, ~~inter alia among other things~~, during two campaigns oriented towards fog microphysics: High Energy Laser in Fog ~~project~~ (HELFOG) ~~project~~ and the Toward Improving Coastal Fog Prediction ~~project~~ (C-FOG) ~~project~~ (Wang et al., 2021). ~~Droplets are measured in the range of 2 to 50 and N_c to 2000~~. (Wang et al., 2021; Gultepe et al., 2021).

The alternative device used to retrieve the aerosol and fog particle size distribution is the Palas Welas-2000 particle counter. ~~The~~ Palas Welas-2000 is a system capable of ~~the~~ analysis of light scattering by a single particle. The device can measure
85 particles in four ranges: $0.2 - 10 \text{ }\mu\text{m}$, $0.3 - 17 \text{ }\mu\text{m}$, $0.6 - 40 \text{ }\mu\text{m}$ or $2 - 100 \text{ }\mu\text{m}$. ~~The~~ Palas Welas-2000 spectrometer was used in the ParisFog fog campaign ~~Haefelin et al. (2010)~~ (Haefelin et al., 2010). ParisFog lasted 6 months between October 2006 and March 2007. The measurements were taken at the SIRTA observatory 20 km south of Paris and a total of 154 hours of fog were recorded. The articles Elias et al. (2009a) and Elias et al. (2009b) focus on the amount of extinction caused by each particle mode in clear sky, haze (pre-fog) conditions and after fog onset. ~~In clear sky, the extinction is caused in equal parts by the~~
90 ~~ultrafine and accumulation mode, during haze, the main role in the extinction plays the hydrated aerosol of the accumulation mode, and the fog droplet mode contributes 40 to the extinction.~~

Optical devices, such as the lidar or the ceilometer, cannot penetrate thick fog to retrieve information about their vertical structure. On the contrary, radars based on ~~micrometre~~ micrometer wavelengths can penetrate the fog and measure the reflectivity and velocity structure (Hamazu et al., 2003). The HATPRO microwave radiometer (MWR) registers a vertical brightness

95 temperature ~~;~~ where the highest resolution (200 m) is in the range of 0 to 2 km. Based on several brightness channels, the HATPRO artificial neural network algorithm inverts the radiance to estimate the vertical profiles of atmospheric temperature (T), relative humidity (RH), integrated water ~~vapour~~vapor, liquid water path (LWP) and liquid water content (LWC) vertical profile. SOFOG3D (SOUth west FOGs 3D experiment) was a project that was conducted from October 2019 to April 2020 in France over 300×300 km, where eight MWRs were used. The data from this campaign have been presented at scientific 100 conferences ~~so far~~ (e.g., Martinet et al., 2021; Vishwakarma et al., 2021; Burnet et al., 2020). The reason for the use of MWR during the SOFOG3D campaign was the article Martinet et al. (2020), which showed the improvement of numerical weather prediction models by the assimilation of MWR data.

The microphysical properties of fog are not the only ones that influence the life cycle of fog. Radiative heating and cooling are crucial to the development and decay of radiation fog. Wærsted et al. (2017) showed that for fog that has no cloud above 105 and its liquid water path exceeds 30 g m^{-2} , the cooling of the fog by long-wave radiation can produce $40 - 70 \text{ g m}^{-2} \text{ h}^{-1}$ liquid water by condensation. Furthermore, the heating of short-wave radiation can contribute significantly to the evaporation by $10 - 15 \text{ g m}^{-2} \text{ h}^{-1}$ in thick fog in the middle of the day (winter). ~~These results were obtained using MWR, cloud radar and~~ ~~cehliometer.~~

~~Motivation~~ The motivation for this work is a lack of devices that can perform in situ microphysical measurements of the 110 vertical structure of the fog. For this purpose, miniature devices are needed that can be mounted on the Unnamed Aircraft Vehicle (UAV), balloons or cable cars. In this study, we propose a novel application of Alphasense OPC-N3 optical particulate matter. We postulate that OPC-N3 can be used to observe the microphysical properties of fog.

During this study, we observed fog near the city ~~centre of Warsaw~~, center of Warsaw at the Institute of Geophysics, University of Warsaw. Parameters such as LWC, N_c and the effective radius (~~$\langle r_{eff} \rangle$~~ r_{eff}) are examined. The results from 115 Alphasense OPC-N3 were validated ~~with using~~ the Oxford Laser VisiSize D30 (ShadowGraph instrument), which has already been successfully used to study cloud/fog microphysics (Nowak et al., 2021; Mohammadi et al., 2022).

The rest of this article is organized as follows: ~~Sect. 3 describes data acquisition~~, Section 2 describes the data acquisition ~~and~~ and Section 3 describes data processing. Section 4 shows the results of the comparison between OPC-N3 and ShadowGraph. Section 5 reports a case study of fog evolution during ~~a~~ night observation. Section 6 discusses the 120 applicability of OPC-N3 to perform fog microphysics measurements.

2 ~~Instrumentation and Methods~~ Instruments

2.1 ~~Apparatus~~

2.1 Data acquisition

The measurements were conducted ~~in situ during the occurrence of fog on the roof (20 m above ground) of the~~ at the Institute 125 of Geophysics (52.21°N , 20.98°E , 115 m a.s.l.), Faculty of Physics, University of Warsaw, Poland. The ~~OPC-N3 was mounted next to the Oxford Laser ViSize D30. In vicinity to those devices~~ Radiation Transfer Laboratory is located on the rooftop of

Table 1. ~~Days analysed~~ General information of the measurement cases analyzed in this study, including the date, time and length of measurements.

Referred as	Measurement start [UTC]	Measurement stop [UTC]	Day / Night	Total minutes of fog
D-12.11	12.11.2021 19:11	13.11.2021 04:43	Night	150
D-16.11	16.11.2021 22:00	17.11.2021 07:21	Night	470
D-13.12	13.12.2021 09:03	13.12.2021 10:34	Day	50
D-14.12	14.12.2021 16:07	15.12.2021 08:20	Night	230
D-15.12	15.12.2021 17:58	16.12.2021 08:41	Night	130

~~Institute are mounted~~ the Faculty of Physics, where measurements of the optical and microphysical properties of atmospheric aerosols and clouds are continuously conducted (i.e., by nephelometer Ecotech Aurora4000,-), as well as components of radiation fluxes and sensible and latent heat fluxes at the Earth's surface (CGR4 for incoming ~~longwave-long-wave~~ (infrared) flux, CMP22 total incoming ~~shortwave-short-wave~~ (solar) flux~~and~~). Basic atmospheric parameters are collected by Vaisala weather station WXT 520. ~~Fog~~The platform is located 20 m above the ground. Some devices, such as Oxford Laser VisiSize D30, are mounted solely for a given period of time.

The fog observations were carried out in the ~~fall-autumn~~ - winter period of 2021. As ShadowGraph has a waterproof case, it was mounted on the platform for the duration of the observation. The OPC-N3 was mounted next to it in case of high probability of fog events without any protection. The Figure1 presents the mounting of both devices at The Radiation Transfer Laboratory. A total of five days with fog were recorded, most of the fog occurred at night, and Table 1 summarises these events. During D-16.11, the ~~longest-most extended~~ period of fog occurred and was ~~analysed-in-detail~~ analyzed in detail in Section 5.

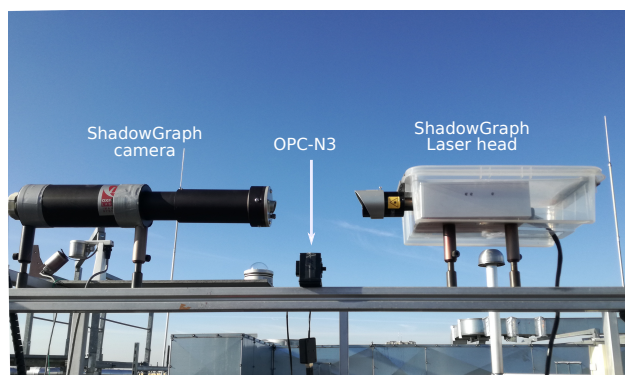


Figure 1. OPC-N3 and ShadowGraph at the Radiation Transfer Laboratory, Institute of Geophysics, Faculty of Physics, University of Warsaw, Poland

2.1.1 ~~ShadowGraph~~VisiSize D30

The VisiSize D30 is a ~~ShadowGraph~~shadowgraph system manufactured by Oxford Lasers Ltd. ~~ShadowGraph captures the photographs~~The VisiSize D30 (hereafter called ShadowGraph) captures the shadow images of particles passing through a measurement volume between a laser head and a ~~high-speed camera. This device is capable of distinguishing high-resolution camera. It can detect particles of~~ different sizes and shapes ~~of particles~~ in various suspensions in ~~real-time~~real-time. The images are ~~created~~acquired by backlight illumination of a ~~specific volume~~. ~~The source of light is~~ measurement volume using an infrared diode laser (808 nm). The ~~maximum speed for capturing the droplets is defined by the camera, with the maximum frame rate being~~ camera is triggered in time with the laser pulses so that a single pulse of laser light occurs in each exposure ~~of the camera. It can capture shadow images of particles with a maximum rate of 30 fps. The manufacturer provides software for particle~~frames per second. The size and velocity of the captured particles are then measured by the ShadowGraph using ~~software provided by the manufacturer based on the Particle/droplet image analysis. Detailed information on VisiSize D30 is described in two articles (Kashdan et al., 2003, 2004)~~Droplet Image Analysis (PDIA) method. The PDIA was first introduced ~~by (Kashdan et al., 2003, 2004) to measure industrial sprays.~~ The system allows for retrieving microphysical properties such as shape, size, DSD(r), total droplet number concentration (N_c) and LWC.

The ShadowGraph camera is equipped with different lens ~~magnifications~~magnification settings, and this adjustment can change the resolution of the sample volume. The manufacturer provides ~~three calibrations~~calibration for three settings: $\times 1$, $\times 2$, $\times 4$. For this study, the magnification setting of $\times 4$ was used, as it allows ~~one to measure for measuring~~ the smallest ~~droplets.~~ The effective pixel size for this magnification is $0.9 \mu\text{m}$. The ShadowGraph collects data in runs; one run was set to last 10 minutes. ~~There is a pause of around 1 second between runs to save the data.~~ Table 2 presents ~~further information~~ more details on the ShadowGraph ~~specification. VisiSize D30 specifications.~~ The ShadowGraph has already been ~~successfully used~~used successfully to study cloud microphysics in ~~the laboratory (Nowak et al., 2021)~~ both laboratory and in situ ~~, in~~ measurements. The droplet detection and sizing system of the ShadowGraph were described by Nowak et al. (2021) in detail. The data collected with ShadowGraph on orographic clouds, i.e. in fog conditions over the mountains (Mohammadi et al., 2022), were analyzed by Mohammadi et al. (2022).

2.1.2 OPC-N3

OPC-N3 is an optical particle counter developed by Alphasense Ltd. The device is constructed of a diode laser light (wavelength 658 nm) and an elliptical mirror that reflects the laser to a detector. The flow is perpendicular to the laser beam. By using a ~~fan to force the flow, the device can operate continuously without the need to periodically replace the pump filters.~~ OPC-N3 measures the particle number concentration (PNC) in 24 bins, in a diameter range of 0.35 to $40 \mu\text{m}$. The PNC measured by the on-board algorithm is converted to PM_{10} , $\text{PM}_{2.5}$ and $\text{PM}_{1.0}$. OPC-N3 can measure the mass concentrations of particles up to $2000 \mu\text{g m}^{-3}$. The sensor returns information about the internal temperature and relative humidity. More information on the Alphasense OPC-N3 specification is provided in Table 2, more details about OPC-N3 can be found in Hagan and Kroll (2020).

Table 2. ~~ShadowGraph specification~~ Technical specifications for the two instruments provided by ~~Oxford Lasers Ltd. and the manufacturers;~~ by Nowak et al. Nowak et al. (2021) - ~~Alphasense OPC-N3 specification provided by Alphasense Ltd. and from~~ Hagan et al. Hagan and Kroll (2020).

ShadowGraph		Lens magnification <u>setting</u> ×4	
Camera sensor [pix × pix]	1952 × 1112	Magnification	6.12
Frame rate [fps]	30	Effective pixel size [μm]	0.90
Laser wavelength [nm]	808	Resolution [μm]	2.0
Laser pulse duration [μs]	0.1-5.0	Field of view [mm × mm]	1.75 × 1.00
Sampling	10 minutes	Depth of field [mm]	5.2
		Sample volume [cm ³]	0.0092
		Typical flow rate [cm ³ s ⁻¹]	0.28
Alphasense OPC-N3			
Particle range	0.35-40	Laser wavelength [nm]	658
Bins	24	Viewing angle	32° – 88°
Sampling	1 minute <u>10 sec.</u>	Refractive Index	1.5 + 0i
Weight [g]	105	Typical flow rate [cm ³ s ⁻¹]	5.5

170 2.2 ~~Data processing~~

3 Methods

3.0.1 ~~Fog detection~~

3.1 Fog detection

To automatically retrieve data concerning fog events, calculations were performed to obtain the minimum concentration of
 175 droplets needed to create a fog. The Koschmieder formula (Equation 1) relates visibility (VIS) to the scattering coefficient σ .

$$\text{VIS} = \frac{\ln 50}{\sigma} \quad (1)$$

The scattering coefficient for spherical particles σ is defined by the equation:

$$\sigma = \pi \int r^2 Q_e \text{DSD}(r) dr \quad (2)$$

where r - droplet radius, $\text{DSD}(r)$ - droplet size distribution and Q_e is the efficiency coefficient for extinction. To estimate the
 180 minimum N_c , it was assumed that fog consists of a monodisperse distribution of droplets with ~~radius a radius of~~ 9.76 μm
 (effective radius of droplets measured by ShadowGraph). From the Mie theory for the radius of 9.76 μm the Q_e was calculated
 to be 2.17.

Based on Equations 1) and 2) the minimum concentration of droplets necessary to cause fog was ~~obtained~~ 6.03 cm^{-3} . For calculations of the microphysical properties of fog, data from ShadowGraph for which the droplet concentration is greater than or equal to 6.03 cm^{-3} were taken into account. During five days, 103 runs (each of 10 min) with detected fog were obtained.

3.1.1 ~~ShadowGraph depth-of-field~~

~~To calculate the droplet~~

3.2 ShadowGraph depth-of-field

When a droplet is at a distance from the camera's focal plane (i.e., a defocused droplet), the generated shadow image consists of a gray halo area around a dark interior circle. If the defocus distance increases, the halo area will grow faster than the total image area. It reaches point where it takes over almost the whole particle image and eventually fades into the background. A criterion was set in the ShadowGraph software algorithm called focus rejection to avoid the sizing error that occurs in the above mentioned situation. The particles with a halo area equal to or larger than 95% of the total particle area are rejected based on this criterion.

To precisely calculate the sample volume in which the droplet can be detected, and subsequently the total droplet number concentration, ~~ShadowGraph needs information on an accurate measurement of the depth of field (DOF)~~. ~~Kashdan et al. (2003) proposed a linear dependence of the DOF for the particle diameter in the range 18–145 μm is essential.~~ The DOF, which is equal to the maximum defocus distance, is assumed by Kashdan et al. (2003) to be linearly dependent on the particle size for a diameter range between 18 and 145 microns.

However, Nowak et al. (2021) showed that for smaller droplets, ~~focus rejection criteria play a role and must be taken into account in the DOF formula. In this study, to obtain results depending on the DOF, (e.g. cloud-size droplets), the focus rejection criterion plays a key role by imposing a significant constraint on the acceptable DOF. In such cases, the formula of Nowak et al. (2021) was used.~~ $z_{95|D_i}$ is DOF proposed by Nowak et al. (2021) which depends on the diameter of the droplet, a_i are the parameters, respectively, of the lens magnification given by the manufacturer.

$$z_{95|D_i} = \frac{0.95}{(1 - 0.95a_3)(a_1D_i + a_2)} \frac{\pi (D_i + a_4 + a_5)^2}{4 \pi x^2}$$

halo area around the droplet exceeds the focus rejection limit at a defocus distance shorter than the linearly size-dependent DOF assumed by Kashdan et al. (2003). Consequently, the relevant sample volume is affected by the focus rejection, which results in an underestimation of the total droplet number concentration.

Nowak et al. (2021) developed a correction method based on the focus rejection criterion in which the DOF for droplet diameter D_i is calculated as follows:

$$z_{95|D_i} = \frac{0.95}{(1 - 0.95a_3)(a_1D_i + a_2)} \frac{\pi (D_i + a_4 + a_5)^2}{4 \pi x^2}, \quad (3)$$

The total volume measured for each droplet is the following: where the constants a_1 and a_2 are calibration constants for a given lens magnification, while constants a_3 , a_4 , and a_5 refer to the halo blurring, pixelization, and diffraction. In addition, pix represents the effective pixel size equal to $0.9\mu\text{m}$ for x4 lens magnification setting.

215 Subsequently, the sample volume for individual droplet i is calculated by multiplying the above DOF and ShadowGraph field of view (FOV) as follows:

$$V_i^{ind} = 2z_{95|D_i}(L_x - D_i)(L_y - D_i), \quad (4)$$

where i denotes the iterations of the measured droplets, D_i its diameter in μm , L_x and L_y denote the size of the effective area of the camera sensor are respectively the horizontal and vertical length of FOV in μm . Eventually, to calculate the N_c , a sum over 220 multiplicative inverse values of V_{ind} must be divided by the total frame numbers F as shown below:

$$N_c = \frac{1}{F} \sum_i \frac{1}{V_i^{ind}}. \quad (5)$$

3.3 Uncertainty of the measurement

The data from ShadowGraph were integrated every 10 minutes. To calculate the uncertainty of the values (LWC, N_c , mean radius) calculated from ShadowGraph, it was assumed that the uncertainty is only influenced by the effective pixel size of 225 ShadowGraph of $0.9\mu\text{m}$ and by the Poisson statistics. The formula for the DOF depends on the diameter of the droplet. The uncertainty of a given variable was calculated using the formula for the propagation of uncertainty.

Data from OPC-N3 were collected every 10 seconds, averaged to 1 minute and then averaged every 10 minutes to compare them with ShadowGraph. As the uncertainty of the OPC-N3 data, the standard deviation was used, obtained by averaging the data over 10-minute periods and the Poisson statistics.

230 3.3.1 Scope of compliance between OPC-N3 and ShadowGraph

3.4 Scope of compliance between OPC-N3 and ShadowGraph

ShadowGraph samples around 1000 cm^3 of air over the period of one hour. To obtain a smooth droplet size distribution spectrum from ShadowGraph, the data needs to be averaged for a period longer than 10 minutes. The minimum averaging time needs to be chosen in such a way that the spectrum is smooth and the time of averaging still allows for the analysis of 235 spectrum changes over time. The data were averaged over one hour¹. Figure 2 (a) shows the volume droplet size distribution (vDSD(r)) and (b) droplet size distribution (DSD(r)) of OPC-N3 and ShadowGraph. The data was averaged over one hour. Aphasense OPC-N3 manual specifies that OPC-N3 record records droplet radiuses in the range of 0.175 to $20.000\mu\text{m}$. On the Fig. 2 can be seen shows that the last bin of OPC-N3 registers a much greater-greater mass of droplets than it would appear from the distribution. This indicates that the last bin has not been properly assigned its right edge. In the last bin of OPC-N3 240 the particles of radiuses larger than $20.00\mu\text{m}$ are also counted.

¹As there is an interval of around 1 second between ShadowGraph runs, the data are averaged over one hour plus around 6-10 seconds

The last OPC-N3 bin contains a significant part of LWC, ~~for this reason therefore~~ it was not excluded from the analysis. However, a new mean radius ($\langle r \rangle$) for this bin was estimated based on ShadowGraph data. ~~From~~ One histogram of DSD was created from all ShadowGraph data of fog ~~was created one histogram of DSD, the events. The~~ mean volume radius ($\langle r_v \rangle_{rv}$) was calculated for droplets bigger than 18.5 μm . The obtained $\langle r_v \rangle_{rv}$ is 21.76 μm . Based on this calculation the lower boundary of OPC-N3 last bin is set as 18.5 μm , the mean radius is set to 21.76 μm and the upper boundary is set as 25.02 μm (the upper limit is set in such a way that the center of the bin falls on the mean radius). ~~The~~ Fig. 2 (c) shows ~~how the vDSD looks the vDSD~~ after adjustment of the last bin of OPC-N3.

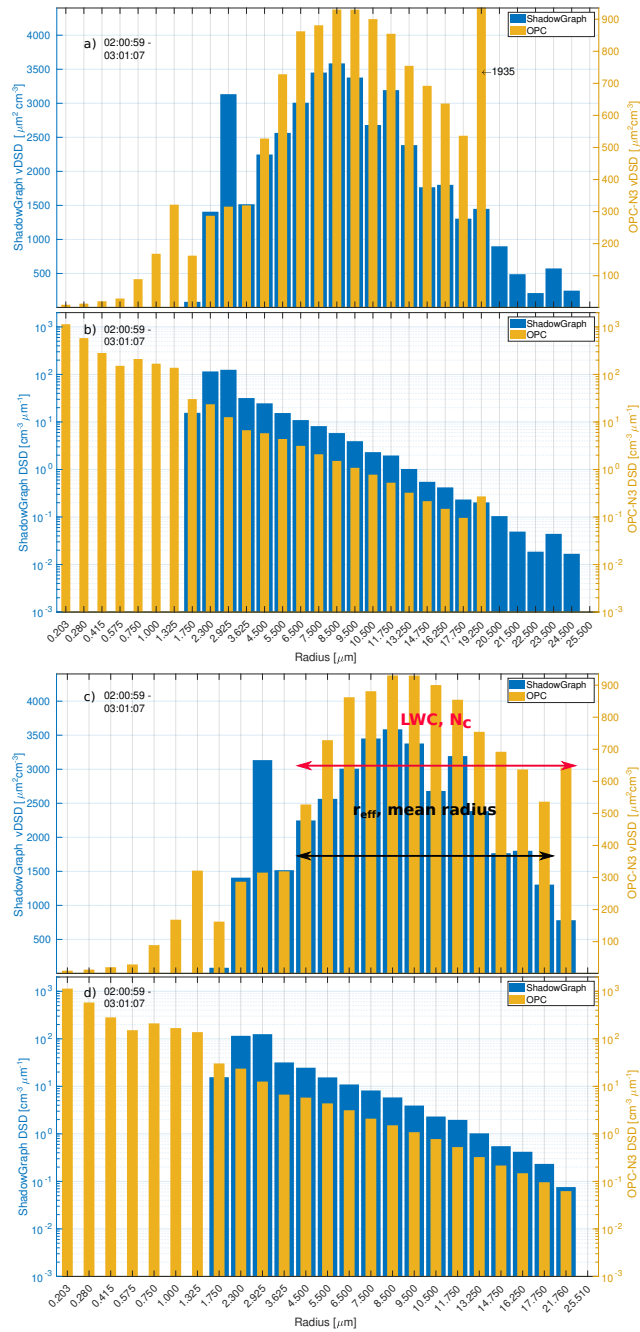


Figure 2. The droplet size distribution $\text{DSD}(r)$ - Fig. (b) and (d) and volume droplet size distribution $\text{vDSD}(r)$ - Fig. (a) and (c) of OPC-N3 and ShadowGraph. In yellow are shown the values obtained for each bin of OPC-N3, in blue are shown ShadowGraph data, aggregated into the same bins as OPC-N3 are shown in blue. The data were averaged by one hour (17-November 17, 2021, 02:00:59 - 03:01:07). The right axis corresponds to OPC-N3. Fig. (a) and (b) represent the bins from OPC-N3 as they are provided by the manufacturer. In Fig. (c) and (d), the last bin of OPC-N3 has been adjusted and its range is $(18.5 - 25.02) \mu\text{m}$. In Fig. (c), in red the range of OPC-N3 bins taken into account for the calculations of LWC and N_c is shown, and in black for $\langle r_{\text{eff}} \rangle$ and mean radius. The number 1935 on Fig. (a) indicates the value of the last bin of OPC-N3.

Oxford Lasers state that the minimum value of the diameter that can be imaged by the ShadowGraph for a magnification of $\times 4$ is $2\ \mu\text{m}$. The minimum diameter of fog ~~droplet droplets~~ registered by ShadowGraph was $3.47\ \mu\text{m}$.

250 ShadowGraph spectrum has a peak in the bin of ~~droplet droplets~~ mean radius $2.925\ \mu\text{m}$. This ~~pick-peak~~ is not visible in the OPC-N3 data. It appears to be a problem in ~~recognising-recognizing~~ the actual size of small droplets by ~~the~~ algorithm. The pixel size of ShadowGraph is $0.9\ \mu\text{m}$, leading to ~~a~~ misinterpretation of droplets ~~of-size-of-2-3 pixels in size~~. In the article of Kashdan et al. (2003) there is a peak in the droplet distribution function for the bin with the smallest droplets. This is explained by the misclassification of small unfocused droplets. Identification of the droplets and their size is done by distinguishing the
255 brightness between the shadow of the drop and the brightness of the background pixels. For fuzzy droplets, the difference is small, making it difficult to classify the droplets to the correct size. In our analysis, the droplets below ~~a~~ radius of $4\ \mu\text{m}$ ~~where~~ ~~were~~ excluded.

During the five days of the study, fog was observed for 17.2 hours. Microphysical parameters such as N_c , LWC, ~~$\langle r_{eff} \rangle$~~ ~~r_{eff}~~ and mean radius were calculated. For those calculations, droplets from ~~range-the range of~~ $4\ \mu\text{m}$ to $25.024\ \mu\text{m}$ ~~where-were~~
260 taken into account for both devices. In the case of OPC-N3, it corresponds to bins from 12 to 24. ~~The bin-Bin~~ 24 was taken into account as it contains a significant amount of LWC, but after adjusting its mean radius to $21.76\ \mu\text{m}$. Droplets smaller than $4\ \mu\text{m}$ ~~where-were~~ excluded from the comparison as ShadowGraph has problems ~~in-classifying-them-correctly-correctly~~ ~~classifying them~~.

For the comparison of ~~$\langle r_{eff} \rangle$~~ ~~r_{eff}~~ and mean radius, only the droplets from ~~range-the range of~~ $4\ \mu\text{m}$ to $18.5\ \mu\text{m}$ were taken
265 into account for ShadowGraph and OPC-N3 (bins 12 to 23 of OPC-N3), as in this range, the registered sizes of droplets from both devices overlap without any adjustments. The droplet radius range, taken into account for each microphysic parameter, is shown in ~~Appendix A~~ Table A1.

~~The range of droplet radiuses which was taken into account for the calculation of microphysical properties of fog- LWC, N_c , $\langle r_{eff} \rangle$, $\langle r \rangle$, $\langle r_s \rangle$, $\langle r_v \rangle$ droplet radii 4.00 - 25.02 4.00 - 18.50-~~

270 ~~Fig. 2 shows that the values of DSD for OPC-N3 are smaller than for ShadowGraph. Appendix A presents a study regarding whether correcting the OPC-N3 data based on RI allows for better data compliance with ShadowGraph.~~

Particles in OPC-N3 are assigned to the size bins based on the amount of light scattered. In Mie theory, the amount of light scattered can be linked to a specific size of a particle; to be able to use Mie theory, one needs to assume an appropriate refractive index (RI) of a particle. In OPC-N3, the manufacturer set the RI_{OPC} at $1.500 + 0.00i$. The refractive index of pure
275 water - $RI_{water} = 1.331 + 0.000i$ (Hale and Query, 1973) - is different from the one assumed in OPC-N3, which can lead to ~~an~~ incorrect assignment of the droplets to the correct bin based on ~~its radius-We analysed their radius~~.

~~We analyzed~~ the effect of recalculating the assignment of droplets to specific bins using RI_{water} . As a result, we ~~have~~ ~~obtained-found out~~ that the vDSD spectrum of OPC-N3 and ShadowGraph after RI correction does not overlap as well as when it was assumed RI_{OPC} , however, due to the greater representation of bigger droplets, a better comparison of LWC between
280 the devices was obtained. ~~In this study, the refractive index is the default OPC-N3 RI_{OPC} in the Appendix the comparison to values calculated using RI_{water} is shown.~~

3.4.1 OPC-N3 temperature and relative humidity

3.5 OPC-N3 temperature and relative humidity

Alphasense OPC-N3 reports temperature (T) and relative humidity (RH). The sensors are mounted inside the device. The registered values were compared with Vaisala WXT520, which is mounted on the roof of the Institute of Geophysics and measures ambient T and RH. As seen ~~on-in~~ Fig. 3 (a) the T inside OPC-N3 is approximately 6°C higher than that of Vaisala WXT520. ~~Probably the~~ The circuit board system is most probably heating the inside of the device. This causes a drop in humidity within OPC-N3. When comparing the RH of OPC-N3 with Vaisala WXT520, it is seen that the RH within OPC-N3 is lower by around 20 %. The measurements presented were taken during the night and early morning. During the night, the value from OPC-N3 seems to be shifted by a constant value in comparison with Vaisala WXT520. The temperature and RH registered by OPC-N3 ~~start rapidly changing~~ rapidly change after sunrise (6:00 UTC). The OPC-N3 is made of black plastic ~~which probably is~~, which is probably heated by sunlight; the higher temperature of the body affects the inside humidity. This leads to the conclusion that the T and RH reported by OPC-N3 cannot be used as the values of ambient conditions and ~~can not~~ cannot be easily corrected. Furthermore, a higher T and lower RH within OPC-N3 may ~~have an~~ impact on the droplet size due to the evaporation process.

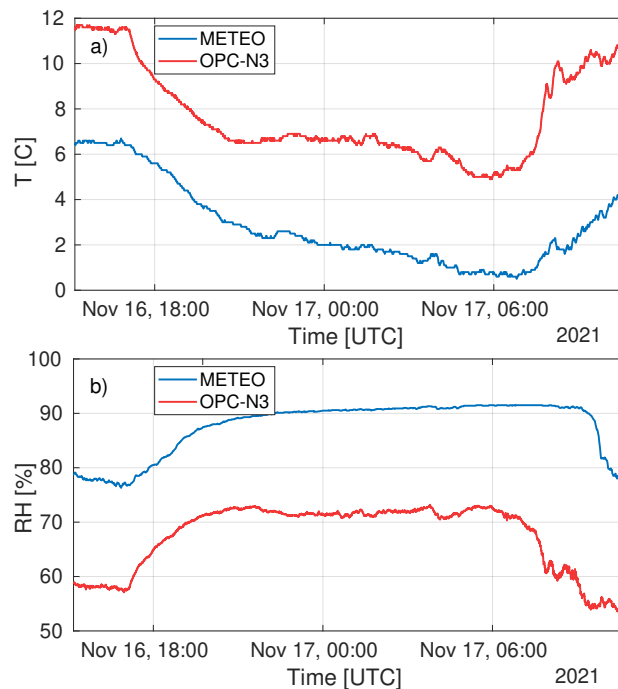


Figure 3. Comparison between OPC-N3 (red line) with Vaisala WXT520 (blue line) of (a) temperature (T) and (b) relative humidity (RH). Devices mounted on the roof of the Institute of Geophysics, sunrise at 6:00 UTC.

4 Results

4.1 Microphysical properties of fog

4.1.1 Liquid water content

LWC results are shown ~~on~~in Fig. 4 (a). The LWC calculated from ShadowGraph ranges from 0 to 0.2 g m^{-3} . The comparison
300 between OPC-N3 and ShadowGraph shows a linear relationship between devices. The OPC-N3 values are almost two times
lower than those from ShadowGraph. The Pearson correlation coefficient (PCC) is ~~0.91~~0.92.

Values such as LWC, N_c , droplet diameter statistics obtained from OPC-N3 can be corrected using a linear regression curve
of the form $y = ax + b$, where x is the measured value from OPC-N3, a and b are calculated coefficients and y is the measured
value from ShadowGraph. The linear regression coefficients, PCC and RMSE for LWC are presented in Appendix B Table B1.

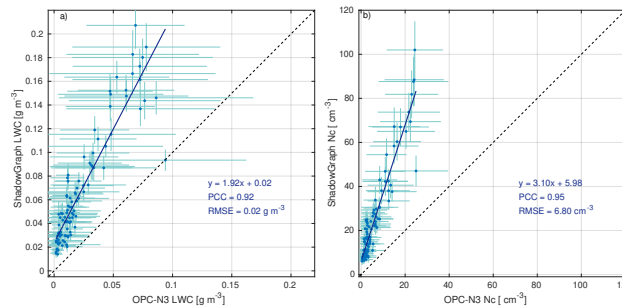


Figure 4. Comparison between ShadowGraph and OPC-N3 of (a) liquid water content (LWC) (b) total droplet number concentration (N_c).
Each point ~~represent~~represents a value measured over ~~a 10 minutes~~minute period. Blue points represent data retrieved from the devices,
solid deep blue ~~line-lines~~line represent linear fit to the data, ~~and~~bars represent the estimation of ~~standard deviation~~uncertainty.

305 4.1.2 Total number concentration

The droplet number concentration is shown in Fig. 4 (b), the values span ~~almost from~~from below 10 to around 100 cm^{-3} for
ShadowGraph. There is a high Pearson correlation coefficient equal to ~~0.94~~0.95 for the comparison with OPC-N3. The values
obtained from OPC-N3 are lower than those obtained from ShadowGraph. The linear regression coefficients, PCC and RMSE
for N_c are presented in Appendix B Table B1.

310 4.1.3 Droplet diameter

Four different droplet diameter statistical moments were calculated. The arithmetic mean ~~$\langle r \rangle$~~ $\langle r \rangle$, the surface mean ~~$\langle r_s \rangle$~~ $\langle r_s \rangle$,
the volume mean ~~$\langle r_v \rangle$~~ $\langle r_v \rangle$ ~~and the~~and the ~~$\langle r_{eff} \rangle$~~ $\langle r_{eff} \rangle$ ~~and the effective radius~~and the effective radius r_{eff} . The values were calculated using a formula for

statistical moments. To calculate $\langle r_{eff} \rangle_{r_{eff}}$, the following formula was used:

$$\langle r_{eff} \rangle = \left(\sum_{i=1}^m r_i^3 \cdot N_i \right) \cdot \left(\sum_{i=1}^m r_i^2 \cdot N_i \right)^{-1}, \quad (6)$$

315 where N_i in the case of OPC-N3 is the concentration of droplets in the volume of the bin, m denotes the number of bins. For ShadowGraph, m denotes the number of droplets and $N_i = V_i^{-1}$ where $V_i = (FV_i^{ind})^{-1}$ where V_i^{ind} is the volume in which the droplet was droplets were measured.

Figure 5 shows the $\langle r_{eff} \rangle_{r_{eff}}$ and Fig. 6 (a) the mean radius, (b) the mean surface radius and (c) the mean volume radius. The $\langle r_{eff} \rangle_{r_{eff}}$ is between 8.05 and 11.71 μm for ShadowGraph. There is a modest correlation coefficient between the devices for all mean radiuses. The linear regression coefficients, PCC and RMSE for $\langle r_{eff} \rangle_{r_{eff}}$ are presented in Appendix B Table B1.

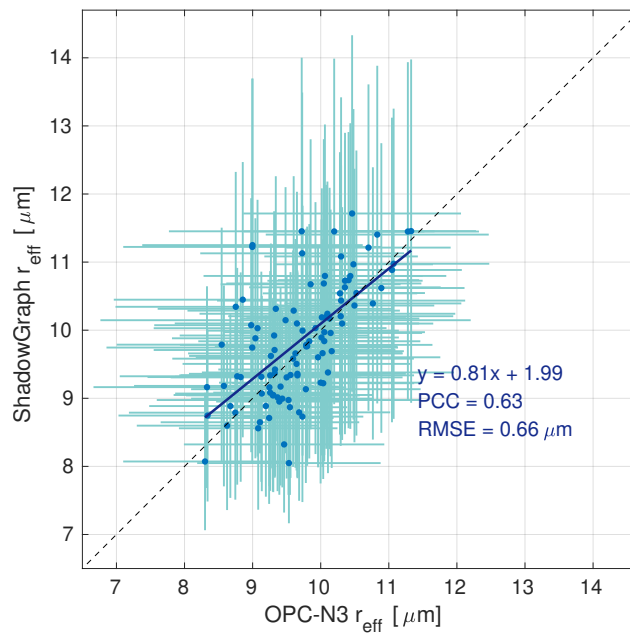


Figure 5. Comparison between ShadowGraph and OPC-N3 of $\langle r_{eff} \rangle_{r_{eff}}$ [μm]. Each point represent represents a value averaged over 10 minutes, and the bars represent the estimation of standard deviation uncertainty. Blue points and lines represent data retrieved from the devices, and solid deep blue line lines represent the linear fit to the data.

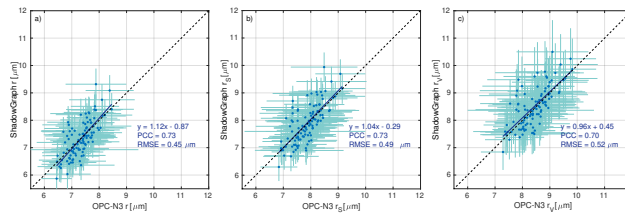


Figure 6. Comparison between ShadowGraph and OPC-N3 for (a) mean radius [μm], (b) mean surface radius [μm], (c) mean volume radius [μm]. Each point ~~represent~~ represents a value averaged over 10 minutes, and the bars represent the estimation of standard deviation uncertainty. Blue points and lines represent data retrieved from the devices, and solid deep blue line-lines represent linear fit to the data, bars represent the estimation of standard deviation.

5 Case study

5.1 Overview of weather conditions

~~In this section, the evolution of fog which~~ During the measurements, five fog events were registered. Most of them lasted less
 325 than two and a half hours. The longest event occurred at night from November 16 to 17, 2021. As this case of fog lasted for
almost eight hours, it was chosen for the case study in this section.

5.1 Overview of weather conditions

On November 16, 2021 is studied. On 16 November 2021, Poland was in the saddle region, between two highs over the North Atlantic and Ukraine. The anticyclone above Ukraine moved towards the Caspian Sea, causing the pressure to drop from
 330 1008 hPa at 18:00 UTC to 1004 hPa around 07:00 UTC on November 17, 2021. Atmospheric conditions at the saddle point resulted in a decrease in wind speed during the measurements. The wind blowing from the direction of 150° was on average 2.2 m s^{-1} , which favoured the formation of fog.

Fog started to form around 21:15 UTC. The sky was clear before fog occurrence (infrared incoming surface flux was around 250 W m^{-2} before 20 UTC). Infrared flux started to rise around 21 UTC, and ~~it~~ dropped around 22:16, suggesting a temporary
 335 disappearance of fog. Approximately at At approximately 4:00 UTC, the infrared flux started to decrease, and after sunrise the total flux ~~was increasing~~ increased - the line representing the total flux is jagged, which suggests that in the ~~morning above the fog~~ said morning, there was a layer of thin clouds above the fog.

From 18:00 UTC, on ~~16 November~~ November 16, 2021, the air temperature decreased from 5.4°C to a minimum of 0.5°C just before 07:00 UTC the next day. The temperature then started to increase, and the process of dissipating the fog started.
 340 ~~In~~ Appendix C Fig. C1 shows ~~in detail~~ the atmospheric situation on the measurement site in detail and Appendix C Fig. C2 presents the radiosounding from 00 UTC ~~17 November~~ November 17, 2021 from Legionowo, which is near Warsaw city.

In Appendix C Fig. C1 (a) shows the scattering coefficient at 525 nm measured by Aurora 4000 nephelometer at dry conditions (the humidity inside Aurora 4000 during the measurements was below 30 %). The values increased from 178 Mm^{-1}

at 18:00 UTC to 250 at 19:30 UTC, then oscillated between 250-260 Mm^{-1} until 23:15 UTC, then continuously decreased
 345 to 170 Mm^{-1} at 07:00 UTC. Values above 200 Mm^{-1} suggest moderate smog conditions. The increase in the scattering
 coefficient after 18:00 UTC was probably due to air pollution caused by the activation of the house heating system and traffic
 emissions.

The PM values obtained from OPC-N3 are presented in Fig. 7. The PM_1 was around $17 \mu g m^{-3}$ at 18:00 UTC and increased
 to $125 \mu g m^{-3}$ at 23:00 UTC, then the PM_1 value decreased. PM_{10} data exhibit a different behaviour from PM_1 . Between
 350 21:00 and 22:30 UTC, 22:45 and 04:00 UTC, 04:20 and 06:10 UTC, episodes of significant increase and decay in PM_{10} value
~~have been were~~ observed. For each episode, PM_{10} reached, respectively (14960, 12550, 6897 $\mu g m^{-3}$). A similar pattern ~~is~~
~~was~~ observed in $PM_{2.5}$ but less pronounced (1354, 1148, 893 $\mu g m^{-3}$). Such values are unrealistic for ~~Warsaw City the City of~~
~~Warsaw~~, the values are biased due to high humidity and fog droplet contamination. These episodes correspond to three periods
 of fog events. In Fig. 7 (b) the estimated values of LWC are presented for OPC-N3 and ShadowGraph.

355 The data collected from OPC-N3 allows to calculate the effective radius. ~~In Appendix C Fig. C17 (b) it is shown shows~~ the
 effective radius calculated from ~~all~~ the droplets that have a radius bigger than $1.15 \mu m$ ($r_{eff}^{1.15}$). The $r_{eff}^{1.15}$ rapidly increases after
 the fog onset. ~~This parameter can be used as an automatic detection of fog events.~~ When there are high concentrations of PM ,
 based on $r_{eff}^{1.15}$, it is possible to distinguish an episode of haze from an episode of fog.

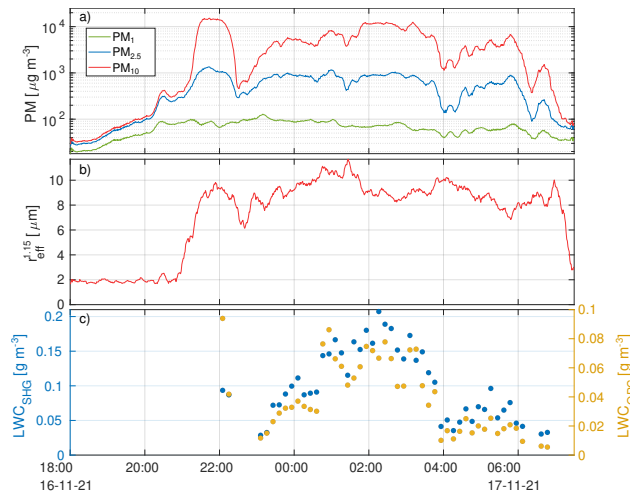


Figure 7. Situation ~~over during~~ the night of November 16, 2021: (a) PM_1 , $PM_{2.5}$ and PM_{10} obtained from Alphasesnse OPC-N3. The data
 from this instrument ~~is was~~ collected every ~~minute~~ ~~10 seconds~~, and later a running mean over a ten minute window was applied to smooth the
 data. (b) Effective radius calculated from OPC-N3 for droplets (radiuses from $1.15 \mu m$ ~~where were~~ taken into account). (c) LWC obtained
 from ShadowGraph and OPC-N3. The values were calculated every ten minutes. LWC was calculated only for fog occurrence (set as droplet
 concentration ~~is higher than or equal to~~ $9.73 cm^{-3}$).

5.2 Evolution of the droplet spectrum

360 In this subsection, the evolution of the droplet spectrum is shown for the period between 22:00 UTC on November 16 and
07:00 UTC on November 17. Figure 8 shows the $vDSD(r)$ for OPC-N3 and ShadowGraph. In one plot, the data for the average
of one hour are shown.

Figure 8 shows a relatively good agreement between devices on the behaviour of the droplet spectrum. During the night
of ~~16 November~~ November 16, the first fog event occurred from 21:00 to 22:20 UTC. Due to some connection errors, the
365 ShadowGraph was set at 22:00 UTC. Moreover, during the first 10 minute run, ~~probably due to the steamed lens~~, it did not
recognise all the droplets that passed through it, probably due to the steamed lens.

The spectrum obtained from OPC-N3 consists of a two-mode distribution. The first mode has a maximum for bin mean
radius $1.33 \mu\text{m}$ and its location remains steady at night. The second mode ~~pick~~ peaked during hours 23:00 - 02:00 UTC moves
from $11.75 \mu\text{m}$ to $14.75 \mu\text{m}$. During this time, the fog ~~evolves~~ evolved and the value of the $vDSD(r)$ ~~increases~~ increased. The
370 maximum intensity of the fog ~~is~~ was observed at 02:00 - 03:00 UTC and the ~~pick~~ peak of the second mode rapidly ~~changes~~
changed to $8.50 \mu\text{m}$. After 3:00 UTC, the second mode of droplet distribution ~~flattens~~ flattened out and the fog ~~starts~~ started to
disappear. The data obtained from ShadowGraph ~~follow~~ followed the same pattern and the values obtained from ShadowGraph
~~are greater~~. During ~~were greater~~. From 02:00 ~~-to~~ 03:00 UTC, the maximum value of the $vDSD(r)$ was $930 \mu\text{m}^2 \text{cm}^{-3}$ for
OPC-N3 and $3586 \mu\text{m}^2 \text{cm}^{-3}$ for ShadowGraph.

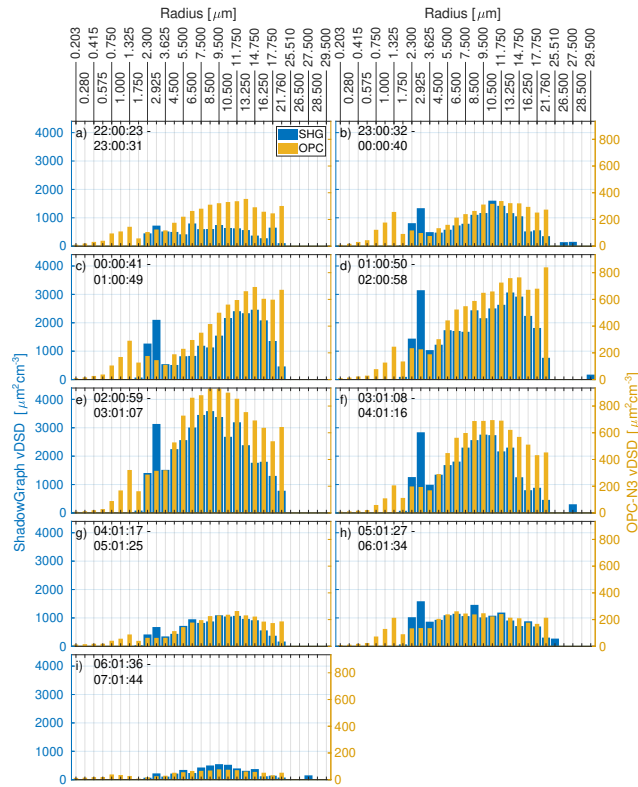


Figure 8. Volume droplet size distribution ($vDSD(r)$). In blue are shown data obtained from ShadowGraph, and in yellow-blue, from OPC-N3 in yellow. Figures from (a) to (i) represent consecutive hours between 22:00 UTC on November 16 and 07:00 UTC on November 17.

375 6 Conclusions

The low-cost optical particle counter Alphasense OPC-N3 was tested for its application in the measurement of fog droplets and compared to Oxford Lasers VisiSize D30 ShadowGraph. There were some limitations in comparing the radius ranges of both devices. The manual provided by Oxford Lasers reports that the minimum radius resolution of ShadowGraph is 1.01. However, during the measurements, ShadowGraph did not record droplets smaller than 1.73. Interestingly, the results reveal that there were non-physical concentrations of droplets in bin (2.6–3.24). As we stated in Sec. 3.4 this peak probably comes from noise and problems with the wrong diameter assignment of small defocused droplets. We conclude that the minimal practical radius that can be measured by ShadowGraph is approximately 3.5–4 for lens magnification $\times 4$.

The range of comparison between the devices ranged from a radius of approximately 4 to 18.5/25.02. To better illustrate the data, we present the results as a $vDSD(r)$. An interesting aspect that has emerged from this analysis is that the last bin (diameter 18.5–20) of

385

- ~~In this article, we have shown that OPC-N3 counts not only drops to 20, but also larger. We estimated based on ShadowGraph data that the last bin of OPC-N3 for this analysis collects droplets from 18.5–25.02. Because this instrument is used mainly for aerosol measurements, which are usually not present at this size, this problem has not been described before.~~

390 registers fog droplets. Badura et al. (2018) showed that the previous version of Alphasense OPC overestimates PM values in high humidity. Our results are in line with this article, OPC-N3 in the case of high humidity $RH = 80 - 90 \%$ can overestimate PM values. During this study, the value of PM_{10} reached ~~15185~~ above 15 mg m^{-3} . Such high values cannot be explained only by the hygroscopic growth of aerosols. The high PM values are associated with fog occurrence and are a result of the count of fog droplets by OPC-N3. The main point of this article was to verify the hypothesis that

395 the values are overestimated because OPC-N3 counts fog droplets.

~~The~~

- OPC-N3 can be used to automatically detect the fog. After fog onset, the effective radius for particles bigger than aerosol (only droplets from bins 7 and higher taken into account) drastically increases (from a value of 2 μm to around 6-10 μm) and stays high for the duration of the fog.

400 - The last bin (diameter 18.5 – 20 μm) of OPC-N3 counts not only drops to 20 μm , but also larger. Because this instrument is used mainly for aerosol measurements, which are usually not present at this size, this problem has not been described before. This fact was possible to observe by presenting the results from ShadowGraph and OPC-N3 as the volume droplet size distribution $vDSD(r)$. We estimated based on ShadowGraph data that the last bin of OPC-N3 for this analysis collects droplets from 18.5 – 25.02 μm .

405 - The minimal practical radius that can be measured by ShadowGraph is approximately 3.5-4 μm for lens magnification $\times 4$. The manual provided by Oxford Lasers reports that the minimum radius resolution of ShadowGraph is 1.01 μm . However, during the measurements, ShadowGraph did not record droplets smaller than 1.73 μm . Interestingly, the results reveal that there were non-physical concentrations of droplets in bin (2.6 -3.24 μm). As we stated in Sec. 3.4 this peak probably comes from noise and problems with the wrong diameter assignment of small defocused droplets. As there

410 were some limitations in comparing the radius ranges of both devices, the range of radius taken for comparison in this article was from 4 μm to 18.5 / 25.02 μm .

- The LWC, N_c , $\langle r_{eff} \rangle$, r_{eff} and the statistical moments of radius were calculated based on the data obtained from OPC-N3. The values were compared with those retrieved from ShadowGraph. Overall, these results suggest that there is a high correlation between OPC-N3 and ShadowGraph. OPC-N3 can be used to measure fog microphysics; however,
- 415 the values reported by OPC-N3 need to be corrected.

- We have shown that the measured T and RH by OPC-N3 are biased. As shown in Section 3.5 OPC-N3 T is higher by 6°C and RH is lower by 20 % compared to ambient T and RH . After sunrise, those values change, probably because

of device case heating by solar radiation, and because of this it is not possible to propose a correction of the measured T and RH by OPC-N3.

420 – The OPC-N3 lowers the values compared to ShadowGraph; in the case of LWC the values are 1.92 times lower and in the case of N_c 3.10 times lower. As OPC-N3 uses a default RI index for radius calculations, it was investigated whether applying the correction of the RI index would improve the compatibility of the instruments (this issue was addressed in Appendix A). After correction, an improvement in LWC was observed; OPC-N3 data were ~~1.15~~ 0.88 times smaller than the ShadowGraph values. ~~As shown in Sect. 3.5 within~~ However, applying the RI correction caused the shifting of the assigned radius of droplets registered by OPC-N3 T is higher by $6^\circ C$ and RH is lower by 20 compared to ambient T and RH . Inside OPC-N3, there are favourable conditions for droplet evaporation, which may be the reason for the observed lower LWC and N_c .

425 to higher values. This resulted in a better compliance between OPC-N3 and Shadowgraph in LWC, however it decreased compliance in the effective radius. Applying RI correction does not appear to improve the consistency of the results.

430 It might be that Alphasense has a built-in processing of the data while assigning it to the bin size. The underestimated results from OPC-N3 appear to be due to the fact that OPC-N3 counts fewer droplets than the ShadowGraph and not from their wrong assignment to the correct bin size. The reason for less droplets maybe their evaporation due to the fact that inside the OPC-N3 is higher temperature and lower humidity than environmental values. The second possibility could be that the open path inside of OPC-N3 allows the flow to expand and this changes the droplet number concentration.

435 The third reason could be that when the fan speed, which drives the flow inside the OPC-N3 changes, the algorithm does not properly adjust the amount of sampled air.

OPC-N3, due to its dimensions and low weight, can be mounted on UAVs, cable cars or balloons. Such works have been performed with small OPCs by Posyniak et al. (2021); Habeck et al. (2022); Girdwood et al. (2020). The main objective of that research was to investigate changes in PM in the vertical profile. Our work presents a new applicability of OPC-N3 within ~~UAV~~

440 UAVS (Unmanned Aerial ~~Vehicle~~ Vehicles) to measure the vertical profiles of the microphysical properties of fog. Additionally, using the AE-51 device on flying platforms, it would allow to estimate the impact of smog on the development of fog. Another application of our study could be to produce ~~cheap~~ inexpensive fog detection systems in airports or automatic fog monitoring systems on roads. Taking ~~into consideration~~ the effective radius of droplets received from OPC-N3 into consideration, it is possible to differentiate the low-visibility situations between fog conditions (which are not hazardous for people) from haze

445 events, when highly polluted air can cause health risks to people.

Code and data availability. The results presented in this study were obtained with the use of the Oxford Lasers VisiSize D30 software version 6.5.39 and code developed by the authors in the MATLAB environment. The latter are available from the authors upon request. The data presented in this study are available from the authors on request.

Appendix A

450 A0.1 Correction of OPC-N3 due to refractive index

Optical particulate matter devices operate by measuring the light scattered by a particle. The Mie theory allows one to relate the amount of light scattered by a particle to its size, assuming particle sphericity. OPC-N3 has an elliptical mirror that sums up the amount of light scattered between angles $32 - 88^\circ$ (Hagan and Kroll, 2020).

The proposed correction of the refractive index changes the bin edges of OPC-N3. First, the theoretical scattering cross section (C_{scat}) was calculated for two RIs, one assumed in the OPC-N3 and one for water. The theoretical values of Mie scattering were calculated for 6000 points of logarithmic spaced radiuses. The curve was then smoothed by running the mean function (the mean was taken over 100 points). Later, for each mean radius of an OPC-N3 bin (r_{old}), C_{scat} was found on the calibration curve derived for RI_{OPC} (brown line with red dots in Fig. A1). Then the obtained C_{scat} values were transferred on the curve for RI_{water} (deep blue line) and their corresponding radius (r_{new}) - blue points in Fig. A1. In the following figures,

460 the microphysical properties were calculated for the uncorrected radiuses r_{old} and the corrected ones r_{new} .

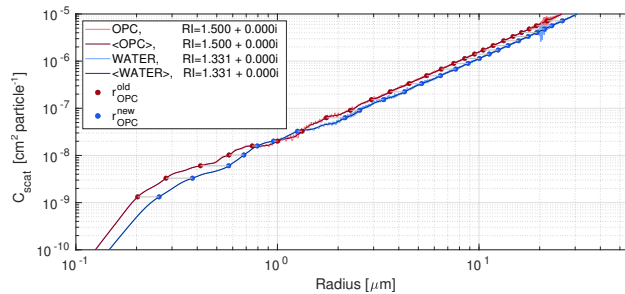


Figure A1. Theoretical scattering cross section C_{scat} calculated by the Mie theory for refractive index assumed by Alphasense in OPC-N3 ($1.500 + 0.00i$) and RI for pure water ($1.331 + 0.000i$) integrated for scattering angles $32^\circ - 88^\circ$. Curves were smoothed by running mean (lines denoted as <OPC> and <WATER>). Points indicate the C_{scat} values at each middle radius of the bin (red dots) and blue dots for corrected radius values assuming RI of water.

In the main text, droplets with radiuses from $4 \mu\text{m}$ to $18.5 \mu\text{m}$ (for r_{eff} , r , r_s , r_V) or $25.02 \mu\text{m}$ (for LWC, N_c) were taken into account. In this section, we show figures that compare the data not corrected (RI_{OPC} , represented in blue) to the data after the RI correction (RI_{water} , depicted in red). In the case of RI_{water} , the bin edges of OPC-N3 where shifted. The edge $18.5 \mu\text{m}$ was shifted to $22.03 \mu\text{m}$ and $25.02 \mu\text{m}$ was shifted to $28.31 \mu\text{m}$. In the case of RI_{water} , the range of droplet radius taken into

465 account for comparison between OPC-N3 and ShadowGraph was from $3.82 \mu\text{m}$ to $23.51 \mu\text{m}$ (for r_{eff} , r , r_s , r_V or $28.31 \mu\text{m}$ (for LWC, N_c), the appropriate ranges are listed in Table A1.

A0.2 Microphysical properties of fog

Table A1. The range of droplet radius which was taken into account for the calculation of microphysical properties of fog.

<u>droplet radii [μm]</u>	<u>LWC, N_c</u>	<u>r_{eff}, r_e, r_v, r_X</u>
<u>no RI corr. (RI_{OPC}):</u>	<u>4.00 - 25.02</u>	<u>4.00 - 18.50</u>
<u>RI corr. (RI_{water}):</u>	<u>3.82 - 28.31</u>	<u>3.82 - 23.51</u>

LWC results are shown in Fig. A2 (a). Applying the RI correction reduces the difference in LWC between devices; OPC-N3 shows values 0.88 smaller than those from ShadowGraph. The droplet number concentration is shown in Fig. A2 (b), the proposed RI correction does not make a significant improvement in the N_c data. In the case of LWC and N_c PCC and RMSE are similar regardless of whether the correction was applied or not. The linear regression coefficients, PCC and RMSE for LWC are presented in Appendix B Table B1.

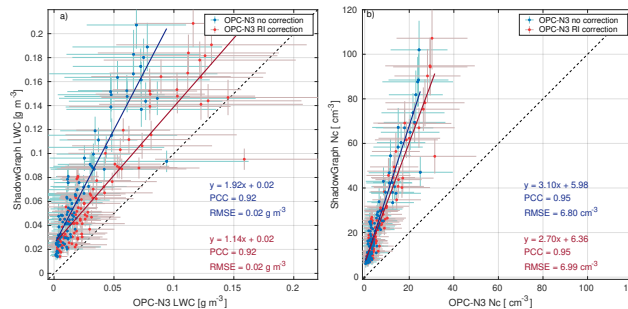


Figure A2. Comparison between ShadowGraph and OPC-N3 of (a) liquid water content (LWC) (b) total droplet number concentration (N_c). Each point represents a value measured over 10 minutes. Solid blue and red lines represent linear fit to the data. Blue points and lines represent data retrieved from the devices, red points and lines represent data after correction of the refractive index for OPC-N3.

The r_{eff} is shown in Fig. A3. The correction of RI index is applied only to OPC-N3, however, however, the RI correction affects the bin boundaries, which also has an impact on the data from ShadowGraph (the droplet radius range taken into account is wider after RI correction)

Applying the RI correction caused the shifting of the assigned radiuses of droplets registered by OPC-N3 compared to ShadowGraph (Fig. A3). The RMSE is higher between OPC and ShadowGraph than without correction. As the droplets are assumed to be larger, the LWC obtained is higher.

Figure A4 shows the evolution of the vDSD during D-16,11 fog case. The vDSD obtained from OPC-N3 is less consistent with the vDSD obtained from ShadowGraph than it was in the case without RI correction. The OPC-N3 vDSD consists of two modes, one with a peak around $0.8 \mu\text{m}$ and other around $14 \mu\text{m}$. The second mode is shifted towards bigger droplet diameters compared to the distribution from ShadowGraph. Applying such a correction does not appear to improve the consistency of the results. It might be that Aphasense has a built-in processing of the data while assigning the bin size. The underestimated

485 results from OPC-N3 appear to be due to the fact that OPC-N3 counts fewer droplets than the ShadowGraph and not from their wrong assignment to the correct bin size.

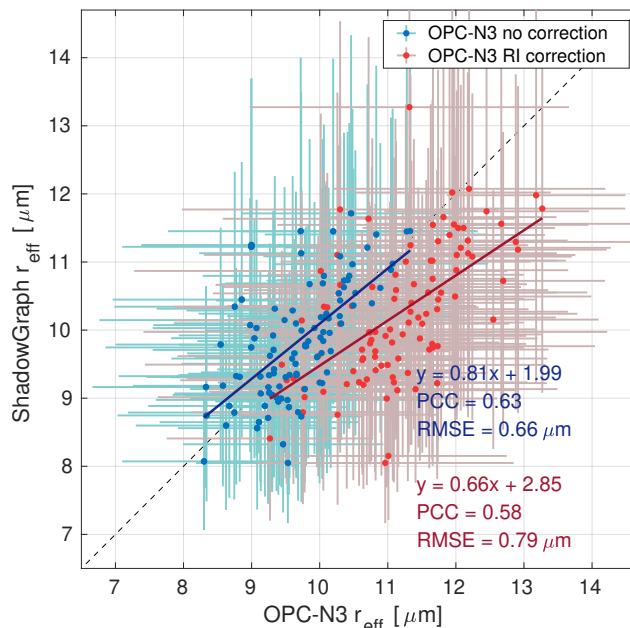


Figure A3. Comparison between ShadowGraph and OPC-N3 of $\langle r_{eff} \rangle$ [μm]. Each point represents values averaged over ten minutes, the bars represent the estimation of uncertainty. Solid blue and red lines represent linear fit to the data. Blue points and lines represent data retrieved from the devices, red points and lines represent data after correction of the refractive index for OPC-N3.

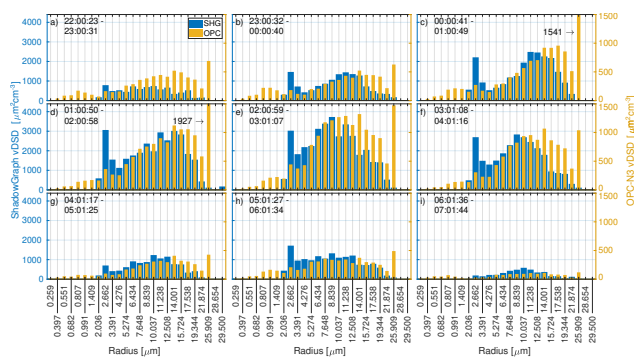


Figure A4. Volume droplet size distribution (vDSD(r)) after applying RI correction to the data from OPC-N3. The bin mean radiuses are different in comparison to Fig. 8. The data obtained from ShadowGraph are shown in blue, from OPC-N3 in yellow. Figures from (a) to (i) represent consecutive hours between 22:00 UTC on November 16 and 07:00 UTC on November 17. The bin value which is out of range has an assigned numerical value.

Appendix B

Table B1. The linear regression coefficients, Pearson's correlation coefficient (PCC) and the root mean square error (RMSE) for LWC, N_c , r_{eff} , r , r_s , r_v . The linear regression was obtained for data without RI correction and with RI correction applied.

	No RI correction			RI correction		
LWC	a	1.923 <u>1.921</u> \pm 0.085 <u>0.084</u>		a	1.148 <u>1.144</u> \pm 0.050	
	b	0.024 \pm 0.003	[gm^{-3}]	b	0.024 <u>0.025</u> \pm 0.003	[gm^{-3}]
	PCC	0.914 <u>0.916</u>		PCC	0.915 <u>0.916</u>	
	RMSE	0.020 <u>0.019</u>	[gm^{-3}]	RMSE	0.020	[gm^{-3}]
N_c	a	3.098 <u>3.100</u> \pm 0.108 <u>0.106</u>		a	2.702 \pm 0.090 <u>0.089</u>	
	b	5.989 <u>5.979</u> \pm 0.942 <u>0.930</u>	[cm^{-3}]	b	6.350 <u>6.361</u> \pm 0.967 <u>0.955</u>	[cm^{-3}]
	PCC	0.944 <u>0.945</u>		PCC	0.948 <u>0.949</u>	
	RMSE	6.890 <u>6.803</u>	[cm^{-3}]	RMSE	7.073 <u>6.991</u>	[cm^{-3}]
r_{eff}	a	0.816 <u>0.810</u> \pm 0.099		a	0.668 <u>0.663</u> \pm 0.088 <u>0.092</u>	
	b	1.939 <u>1.994</u> \pm 0.959 <u>0.960</u>	[μm]	b	2.694 <u>2.848</u> \pm 0.981 <u>1.032</u>	[μm]
	PCC	0.635 <u>0.632</u>		PCC	0.605 <u>0.583</u>	
	RMSE	0.655 <u>0.657</u>	[μm]	RMSE	0.751 <u>0.791</u>	[μm]
r	a	1.124 <u>1.118</u> \pm 0.104		a	0.894 \pm 0.083 <u>0.084</u>	
	b	-0.915 <u>-0.874</u> \pm 0.766 <u>0.765</u>	[μm]	b	0.125 <u>0.137</u> \pm 0.663 <u>0.670</u>	[μm]
	PCC	0.731 <u>0.730</u>		PCC	0.730 <u>0.726</u>	
	RMSE	0.452 <u>0.453</u>	[μm]	RMSE	0.472 <u>0.478</u>	[μm]
r_s	a	1.047 <u>1.041</u> \pm 0.098		a	0.837 \pm 0.080 <u>0.082</u>	
	b	-0.335 <u>-0.294</u> \pm 0.773 <u>0.772</u>	[μm]	b	0.613 <u>0.643</u> \pm 0.695 <u>0.708</u>	[μm]
	PCC	0.728 <u>0.727</u>		PCC	0.721 <u>0.714</u>	
	RMSE	0.487 <u>0.488</u>	[μm]	RMSE	0.520 <u>0.531</u>	[μm]
r_v	a	0.961 <u>0.955</u> \pm 0.096		a	0.772 <u>0.77</u> \pm 0.080 <u>0.083</u>	
	b	0.403 <u>0.446</u> \pm 0.808	[μm]	b	1.291 <u>1.358</u> \pm 0.758 <u>0.780</u>	[μm]
	PCC	0.707 <u>0.705</u>		PCC	0.692 <u>0.680</u>	
	RMSE	0.522 <u>0.523</u>	[μm]	RMSE	0.568 <u>0.587</u>	[μm]

Appendix C

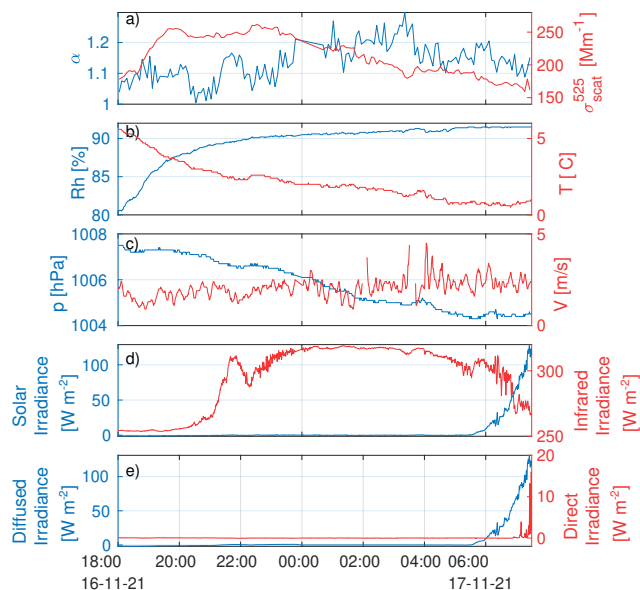


Figure C1. Situation over during the night of November 16, 2021: (a) Scattering coefficient (σ_{scat}^{525} and Ångström exponent obtained from Ecotech Aurora 4000. The data from this instrument is was collected every five minutes. (b) Temperature (T) and relative humidity (RH) obtained from Vaisala WXT520. The data from this instrument is was collected every minute. (c) Local pressure (p) and mean wind velocity (V) obtained from Vaisala WXT520. (d) Total and infrared irradiance, (e) diffused and direct irradiance. The data came from apparatus mounted in the Radiation Transfer Laboratory, Faculty of Physics, University of Warsaw, Poland.

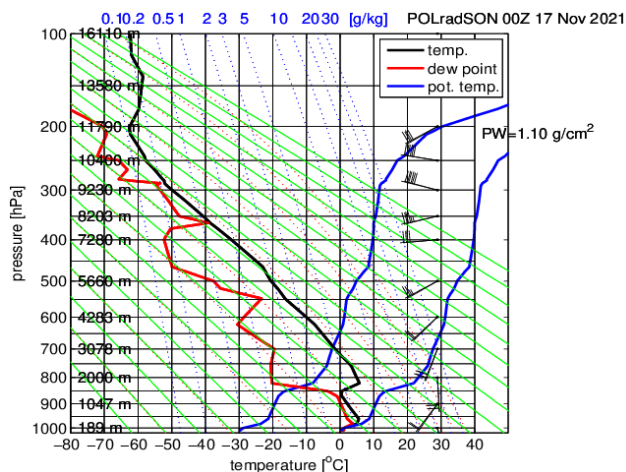


Figure C2. Radio sounding from 00 UTC November 17 Nov., 2021 from Legionowo (near Warsaw), Poland.

Author contributions. SM and KM planned the campaign; KN, MM, KM performed the measurements; KN analyzed the data; KN wrote the manuscript draft; KN, MM, SM, KM reviewed and edited the manuscript.

490 *Competing interests.* Some authors are members of the editorial board of journal Atmospheric Measurement Techniques. The peer-review process was guided by an independent editor, and the authors have also no other competing interests to declare.

Acknowledgements. This research was funded by the National Science Centre (NCN), Poland, grant number UMO-2017/27/B/ST10/00549.

References

- Badura, M., Batog, P., Drzeniecka-Osiadacz, A., and Modzel, P.: Evaluation of Low-Cost Sensors for Ambient PM_{2.5} Monitoring, *Journal of Sensors*, 2018, <https://doi.org/10.1155/2018/5096540>, 2018.
- 495
- Barmpadimos, I., Keller, J., Oderbolz, D., Hueglin, C., and Prévôt, A. S. H.: One decade of parallel fine (PM_{2.5}) and coarse (PM₁₀-PM_{2.5}) particulate matter measurements in Europe: trends and variability, *Atmospheric Chemistry and Physics*, 12, 3189–3203, <https://doi.org/10.5194/acp-12-3189-2012>, 2012.
- Bartok, J., Bott, A., and Gera, M.: Fog Prediction for Road Traffic Safety in a Coastal Desert Region, *Boundary-Layer Meteorology*, 145, <https://doi.org/10.1007/s10546-012-9750-5>, 2012.
- 500
- Beloconi, A. and Vounatsou, P.: Substantial Reduction in Particulate Matter Air Pollution across Europe during 2006–2019: A Spatiotemporal Modeling Analysis, *Environmental Science & Technology*, 55, 15 505–15 518, <https://doi.org/10.1021/acs.est.1c03748>, PMID: 34694135, 2021.
- Burnet, F., Lac, C., Martinet, P., Fourrié, N., Haeffelin, M., Delanoë, J., Price, J., Barrau, S., Canut, G., Cayez, G., Dabas, A., Denjean, C., Dupont, J.-C., Honnert, R., Mahfouf, J.-F., Montmerle, T., Roberts, G., Seity, Y., and Vié, B.: The SOUTh west FOGs 3D experiment for processes study (SOFOG3D) project, in: EGU General Assembly 2020, Online, 4–8 May 2020, EGU2020-17836, <https://doi.org/https://doi.org/10.5194/egusphere-egu2020-17836>, 2020.
- 505
- Colette, A. and Rouil, L.: ETC/ATNI Report 16/2019: Air Quality Trends in Europe: 2000–2017. Assessment for surface SO₂, NO₂, Ozone, PM₁₀ and PM_{2.5}—Eionet Portal., Eionet Report - ETC/ATNI 2019/16, <https://www.eionet.europa.eu/etcs/etc-atni/products/etc-atni-reports/etc-atni-report-16-2019-air-quality-trends-in-europe-2000-2017-assessment-for-surface-so2-no2-ozone-pm10-and-pm2-5-1>, 2021.
- 510
- Considine, E. M., Reid, C. E., Ogletree, M. R., and Dye, T.: Improving accuracy of air pollution exposure measurements: Statistical correction of a municipal low-cost airborne particulate matter sensor network, *Environmental Pollution*, 268, 115 833, <https://doi.org/10.1016/j.envpol.2020.115833>, 2021.
- 515
- Crilley, L. R., Shaw, M., Pound, R., Kramer, L. J., Price, R., Young, S., Lewis, A. C., and Pope, F. D.: Evaluation of a low-cost optical particle counter (Alphasense OPC-N2) for ambient air monitoring, *Atmospheric Measurement Techniques*, 11, 709–720, <https://doi.org/10.5194/amt-11-709-2018>, 2018.
- Degefie, D., El-Madany, T.-S., Hejkal, J., Held, M., Dupont, J.-C., Haeffelin, M., and Klemm, O.: Microphysics and energy and water fluxes of various fog types at SIRTa, France, *Atmospheric Research*, 151, 162–175, <https://doi.org/10.1016/j.atmosres.2014.03.016>, sixth International Conference on Fog, Fog Collection and Dew, 2015.
- 520
- Elias, T., Haeffelin, M., Drobinski, P., Gomes, L., Rangognio, J., Bergot, T., Chazette, P., Raut, J., and Colomb, M.: Extinction of Light during the Fog Life Cycle: a Result from the ParisFog Experiment, *AIP Conference Proceedings*, 1100, 165–168, <https://doi.org/10.1063/1.3116939>, 2009a.
- Elias, T., Haeffelin, M., Drobinski, P., Gomes, L., Rangognio, J., Bergot, T., Chazette, P., Raut, J.-C., and Colomb, M.: Particulate contribution to extinction of visible radiation: Pollution, haze, and fog, *Atmospheric Research*, 92, 443–454, <https://doi.org/10.1016/j.atmosres.2009.01.006>, 2009b.
- 525
- Feinberg, S. N., Williams, R., Hagler, G., Low, J., Smith, L., Brown, R., Garver, D., Davis, M., Morton, M., Schaefer, J., and Campbell, J.: Examining spatiotemporal variability of urban particulate matter and application of high-time resolution data from a network of low-cost air pollution sensors, *Atmospheric Environment*, 213, 579–584, <https://doi.org/10.1016/j.atmosenv.2019.06.026>, 2019.

- 530 Girdwood, J., Smith, H., Stanley, W., Ulanowski, Z., Stopford, C., Chemel, C., Doungeris, K.-M., Brus, D., Campbell, D., and Mackenzie, R.: Design and field campaign validation of a multi-rotor unmanned aerial vehicle and optical particle counter, *Atmospheric Measurement Techniques*, 13, 6613–6630, <https://doi.org/10.5194/amt-13-6613-2020>, 2020.
- Gultepe, I.: Fog and Boundary Layer Clouds: Fog Visibility and Forecasting, Birkhäuser, <https://doi.org/10.1007/978-3-7643-8419-7>, 2007.
- Gultepe, I., Tardif, R., Michaelides, S., Cermak, J., Bott, A., Muller, M., Pagowski, M., Hansen, B., Ellrod, G., Jacobs, W., Toth, G., and
535 Cober, S.: Fog research: A review of past achievements and future perspectives., *Pure and Applied Geophysics*, 164, 1121–1159, 2007.
- Gultepe, I., Pearson, G., Milbrandt, J. A., Hansen, B., Platnick, S., Taylor, P., Gordon, M., Oakley, J. P., and Cober, S. G.: The Fog Remote Sensing and Modeling Field Project, *Bulletin of the American Meteorological Society*, 90, 341 – 360, <https://doi.org/10.1175/2008BAMS2354.1>, 2009.
- Gultepe, I., Zhou, B., Milbrandt, J., Bott, A., Li, Y., Heymsfield, A., Ferrier, B., Ware, R., Pavolonis, M., Kuhn, T.,
540 Gurka, J., Liu, P., and Cermak, J.: A review on ice fog measurements and modeling, *Atmospheric Research*, 151, 2–19, <https://doi.org/10.1016/j.atmosres.2014.04.014>, sixth International Conference on Fog, Fog Collection and Dew, 2015.
- Gultepe, I., Milbrandt, J. A., and Zhou, B.: Marine Fog: A Review on Microphysics and Visibility Prediction, pp. 345–394, Springer International Publishing, Cham, https://doi.org/10.1007/978-3-319-45229-6_7, 2017.
- Gultepe, I., Heymsfield, A., Fernando, H., Pardyjak, E., Dorman, C., Wang, Q., Creegan, E., Hoch, S., Flagg, D., Yamaguchi, R., Krishna-
545 murthy, R., Gabersek, S., Perrie, W., Perelet, A., Singh, D., Chang, R., Nagare, B., Wagh, S., and Wang, S.: A Review of Coastal Fog Microphysics During C-FOG, *Boundary-Layer Meteorology*, 181, 1–39, <https://doi.org/10.1007/s10546-021-00659-5>, 2021.
- Habeck, J. B., Hogan, C. J., Flaten, J. A., and Candler, G. V.: Development of a calibration system for measuring aerosol particles in the stratosphere, in: *AIAA SCITECH 2022 Forum*, p. 1582, 2022.
- Haeffelin, M., Bergot, T., Elias, T., Tardif, R., Carrer, D., Chazette, P., Colomb, M., Drobinski, P., Dupont, E., Dupont, J.-C., Gomes,
550 L., Musson-Genon, L., Pietras, C., Plana-Fattori, A., Protat, A., Rangognio, J., Raut, J.-C., Rémy, S., Richard, D., Sciare, J., and Zhang, X.: Parisfog: Shedding new Light on Fog Physical Processes, *Bulletin of the American Meteorological Society*, 91, 767 – 783, <https://doi.org/10.1175/2009BAMS2671.1>, 2010.
- Hagan, D. H. and Kroll, J. H.: Assessing the accuracy of low-cost optical particle sensors using a physics-based approach, *Atmospheric Measurement Techniques*, 13, 6343–6355, <https://doi.org/10.5194/amt-13-6343-2020>, 2020.
- 555 Hale, G. M. and Querry, M. R.: Optical Constants of Water in the 200-nm to 200- μ m Wavelength Region, *Appl. Opt.*, 12, 555–563, <https://doi.org/10.1364/AO.12.000555>, 1973.
- Hamazu, K., Hashiguchi, H., Wakayama, T., Matsuda, T., Doviak, R. J., and Fukao, S.: A 35-GHz Scanning Doppler Radar for Fog Observations, *Journal of Atmospheric and Oceanic Technology*, 20, 972 – 986, [https://doi.org/10.1175/1520-0426\(2003\)20<972:AGSDRF>2.0.CO;2](https://doi.org/10.1175/1520-0426(2003)20<972:AGSDRF>2.0.CO;2), 2003.
- 560 Hu, H., Sun, J., and Zhang, Q.: Assessing the Impact of Surface and Wind Profiler Data on Fog Forecasting Using WRF 3DVAR: An OSSE Study on a Dense Fog Event over North China, *Journal of Applied Meteorology and Climatology*, 56, 1059 – 1081, <https://doi.org/10.1175/JAMC-D-16-0246.1>, 2017.
- Jayarathne, R., Liu, X., Thai, P., Dunbabin, M., and Morawska, L.: The influence of humidity on the performance of a low-cost air particle mass sensor and the effect of atmospheric fog, *Atmospheric Measurement Techniques*, 11, 4883–4890, <https://doi.org/10.5194/amt-11-4883-2018>, 2018.
- 565

- Kashdan, J. T., Shrimpton, J. S., and Whybrew, A.: Two-Phase Flow Characterization by Automated Digital Image Analysis. Part 1: Fundamental Principles and Calibration of the Technique, *Particle & Particle Systems Characterization*, 20, 387–397, <https://doi.org/10.1002/ppsc.200300897>, 2003.
- Kashdan, J. T., Shrimpton, J. S., and Whybrew, A.: Two-Phase Flow Characterization by Automated Digital Image Analysis. Part 2: Application of PDIA for Sizing Sprays, *Particle & Particle Systems Characterization*, 21, 15–23, <https://doi.org/10.1002/ppsc.200400898>, 2004.
- Klemm, O. and Lin, N.-H.: What Causes Observed Fog Trends: Air Quality or Climate Change?, *Aerosol and Air Quality Research*, 16, 1131–1142, <https://doi.org/10.4209/aaqr.2015.05.0353>, 2016.
- Kulkarni, R., Jenamani, R. K., Pithani, P., Konwar, M., Nigam, N., and Ghude, S. D.: Loss to Aviation Economy Due to Winter Fog in New Delhi during the Winter of 2011–2016, *Atmosphere*, 10, <https://doi.org/10.3390/atmos10040198>, 2019.
- Liu, D., Yang, J., Niu, S., and Li, Z.: On the Evolution and Structure of a Radiation Fog Event in Nanjing, *Advances in Atmospheric Sciences*, 28, 223–237, <https://doi.org/10.1007/s00376-010-0017-0>, 2011.
- Liu, H.-Y., Schneider, P., Haugen, R., and Vogt, M.: Performance Assessment of a Low-Cost PM_{2.5} Sensor for a near Four-Month Period in Oslo, Norway, *Atmosphere*, 10, <https://doi.org/10.3390/atmos10020041>, 2019.
- Maalick, Z., Kühn, T., Korhonen, H., Kokkola, H., Laaksonen, A., and Romakkaniemi, S.: Effect of aerosol concentration and absorbing aerosol on the radiation fog life cycle, *Atmospheric Environment*, 133, 26–33, <https://doi.org/10.1016/j.atmosenv.2016.03.018>, 2016.
- Martinet, P., Cimini, D., Burnet, F., Ménérier, B., Michel, Y., and Unger, V.: Improvement of numerical weather prediction model analysis during fog conditions through the assimilation of ground-based microwave radiometer observations: a 1D-Var study, *Atmospheric Measurement Techniques*, 13, 6593–6611, <https://doi.org/10.5194/amt-13-6593-2020>, 2020.
- Martinet, P., Burnet, F., Bell, A., Kremer, A., Letillois, M., Löhnert, U., Antoine, S., Caumont, O., Cimini, D., Delanöe, J., Hervo, M., Huet, T., Georgis, J.-F., Orlandi, E., Price, J., Raynaud, L., Rottner, L., Seity, Y., , and Unger, V.: Benefit of microwave radiometer and cloud radar observations for data assimilation and fog process studies during the SOFOG3D experiment, in: EMS Annual Meeting 2021, online, 6–10 Sep 2021, EMS2021-232, <https://doi.org/https://doi.org/10.5194/ems2021-232>, 2021.
- Mazoyer, M., Burnet, F., Denjean, C., Roberts, G. C., Haeffelin, M., Dupont, J.-C., and Elias, T.: Experimental study of the aerosol impact on fog microphysics, *Atmospheric Chemistry and Physics*, 19, 4323–4344, <https://doi.org/10.5194/acp-19-4323-2019>, 2019.
- Mazoyer, M., Burnet, F., and Denjean, C.: Experimental study on the evolution of droplets size distribution during the fog life cycle, *Atmospheric Chemistry and Physics Discussions*, 2022, 1–28, <https://doi.org/10.5194/acp-2021-1027>, 2022.
- Mohammadi, M., Nowak, J. L., Bertens, G., Moláček, J., Kumala, W., and Malinowski, S. P.: Cloud microphysical measurements at a mountain observatory: comparison between shadowgraph imaging and phase Doppler interferometry, *Atmospheric Measurement Techniques*, 15, 965–985, <https://doi.org/10.5194/amt-15-965-2022>, 2022.
- Nowak, J. L., Mohammadi, M., and Malinowski, S. P.: Applicability of the VisiSize D30 shadowgraph system for cloud microphysical measurements, *Atmospheric Measurement Techniques*, 14, 2615–2633, <https://doi.org/10.5194/amt-14-2615-2021>, 2021.
- Posyniak, M., Markowicz, K., Czyzewska, D., Chilinski, M., Makuch, P., Zawadzka-Manko, O., Kucieba, S., Kulesza, K., Kachniarz, K., Mijal, K., and Borek, K.: Experimental study of smog microphysical and optical vertical structure in the Silesian Beskids, Poland, *Atmospheric Pollution Research*, 12, 101 171, <https://doi.org/10.1016/j.apr.2021.101171>, 2021.
- Price, J. D., Lane, S., Boutle, I. A., Smith, D. K. E., Bergot, T., Lac, C., Duconge, L., McGregor, J., Kerr-Munslow, A., Pickering, M., and Clark, R.: LANFEX: A Field and Modeling Study to Improve Our Understanding and Forecasting of Radiation Fog, *Bulletin of the American Meteorological Society*, 99, 2061 – 2077, <https://doi.org/10.1175/BAMS-D-16-0299.1>, 2018.

- Pruppacher, H. and Klett, J.: Microstructure of Atmospheric Clouds and Precipitation, pp. 10–73, Springer Netherlands, Dordrecht, 605 https://doi.org/10.1007/978-0-306-48100-0_2, 2010.
- Tsai, I.-C., Hsieh, P.-R., Cheung, H. C., and Chung-Kuang Chou, C.: Aerosol impacts on fog microphysics over the western side of Taiwan Strait in April from 2015 to 2017, *Atmospheric Environment*, 262, 118 523, <https://doi.org/10.1016/j.atmosenv.2021.118523>, 2021.
- Vautard, R., Yiou, P., and Van Oldenborgh, G. J.: Decline of fog, mist and haze in Europe over the past 30years, *Nature Geoscience - NAT GEOSCI*, 2, 115–119, <https://doi.org/10.1038/ngeo414>, 2009.
- 610 Vishwakarma, P., Delanoë, J., Le Gac, C., Bertrand, F., Dupont, J.-C., Haeffelin, M., Martinet, P., Burnet, F., Lac, C., Bell, A., Vignelles, D., Toledo, F., Jorquera, S., and Vinson, J.-P.: Fog Analysis during SOFOG3D Experiment, in: vEGU General Assembly 2021, online, 19–30 Apr 2021, EGU21-9941, <https://doi.org/https://doi.org/10.5194/egusphere-egu21-9941>, 2021.
- Wang, Q., Yamaguchi, R. T., Kalogiros, J. A., Daniels, Z., Alappattu, D. P., Jonsson, H., Alvarenga, O., Olson, A., Wauer, B. J., Ortiz-Suslow, D. G., and Fernando, H. J.: Microphysics and Optical Attenuation in Fog: Observations from Two Coastal Sites, *Boundary-Layer* 615 *Meteorology*, 181, 267–292, <https://doi.org/10.1007/s10546-021-00675-5>, 2021.
- Wang, Y., Li, J., Jing, H., Zhang, Q., Jiang, J., and Biswas, P.: Laboratory Evaluation and Calibration of Three Low-Cost Particle Sensors for Particulate Matter Measurement, *Aerosol Science and Technology*, 49, 1063–1077, <https://doi.org/10.1080/02786826.2015.1100710>, 2015.
- Weston, M., Francis, D., Nelli, N., Fonseca, R., Temimi, M., and Addad, Y.: The First Characterization of Fog Microphysics 620 in the United Arab Emirates, an Arid Region on the Arabian Peninsula, *Earth and Space Science*, 9, e2021EA002 032, <https://doi.org/10.1029/2021EA002032>, e2021EA002032 2021EA002032, 2022.
- Wærsted, E., Haeffelin, M., Dupont, J.-C., Delanoë, J., and Dubuisson, P.: Radiation in fog: Quantification of the impact on fog liquid water based on ground-based remote sensing, *Atmospheric Chemistry and Physics*, 17, 10 811–10 835, [https://doi.org/10.5194/acp-17-10811-](https://doi.org/10.5194/acp-17-10811-2017) 2017, 2017.