

Performance evaluation of the Alphasense OPC-N3 and Plantower PMS5003 sensor in measuring dust events in the Salt Lake Valley, Utah

Kamaljeet Kaur¹, Kerry E. Kelly¹

¹Department of Chemical Engineering, University of Utah, SLC, 84102, USA

Correspondence to: Kerry Kelly (kerry.kelly@utah.edu)

Abstract. As the changing climate expands the extent of arid and semi-arid lands, the number, severity of, and health effects associated with dust events are likely to increase. However, regulatory measurements capable of capturing dust (PM₁₀, particulate matter smaller than 10 µm in diameter) are sparse, sparser than measurements of PM_{2.5} (PM smaller than 2.5 µm in diameter). Although low-cost sensors could supplement regulatory monitors, as numerous studies have shown for PM_{2.5} concentration, most of these sensors are not effective at measuring PM₁₀ despite claims by sensor manufacturers. This study focuses on the Salt Lake Valley, adjacent to the Great Salt Lake, which recently reached historic lows exposing 1865 km² of dry lakebed. It evaluated the field performance of the Plantower PMS 5003, a common low-cost PM sensor, and the Alphasense OPC-N3, a promising candidate for low-cost measurement of PM₁₀, against a federal equivalent method (FEM, beta attenuation) and research measurements (GRIMM aerosol spectrometer model 1.109) at three different locations. During a month-long field study that included five dust events in the Salt Lake Valley with PM₁₀ concentrations reaching 311 µg/m³, the OPC-N3 exhibited strong correlation with FEM PM₁₀ measurements ($R^2 = 0.865$, RMSE = 12.4 µg/m³) and GRIMM ($R^2 = 0.937$, RMSE = 17.7 µg/m³). The PMS sensor exhibited poor to moderate correlations ($R^2 < 0.49$, RMSE = 33-45 µg/m³) with reference/research monitors and severely underestimated the PM₁₀ concentrations (slope <0.099) for PM₁₀. We also evaluated a PM-ratio-based correction method to improve the estimated PM₁₀ concentration from PMS sensors. After applying this method, PMS PM₁₀ concentrations correlated reasonably well with FEM measurements ($R^2 > 0.63$) and GRIMM measurements ($R^2 > 0.76$), and the RMSE decreased to 15-25 µg/m³. Our results suggest that it may be possible to obtain better resolved spatial estimates of PM₁₀ concentration using a combination of PMS sensors (often publicly available in communities) and measurements of PM_{2.5} and PM₁₀, such as those provided by FEMs, research-grade instrumentation, or the OPC-N3.

1 Introduction

Our changing climate is expanding the extent of arid and semi-arid lands globally; these lands currently cover approximately 1/3rd of the Earth's land surface (Williams et al., 2022; Huang et al., 2016). Recent studies suggest that this expansion of arid lands is linked to increases in the number and severity of dust events (Clifford et al., 2019; Tong et al., 2017; Ardon-Dryer and Kelley, 2022). Dust events can transport particulate matter (PM), particle-bound air toxics, and allergens over thousands of kilometers (Goudie, 2014). The suspended PM affects regional climate by

impacting cloud formation, precipitation processes, and convection activity (Cai et al., 2021; Kumar et al., 2021; Mallet et al., 2009). Dust events significantly affect the regional air quality (Chakravarty et al., 2021; Akinwumiju et al., 2021; Liu et al., 2020), decrease atmospheric visibility (Jayaratne et al., 2011) and have adverse effects on human health, including being linked to increased incidence of asthma, pneumonia, bronchitis, stroke, adverse birth outcomes, influenza, meningitis, and valley fever (Dastoorpoor et al., 2018; Jones, 2020; Bogan et al., 2021; Soy, 2016; Trianti et al., 2017; Diokhane et al., 2016; Schweitzer et al., 2018).

During dust events, the majority of PM is greater than 2.5 μm in diameter (Tam et al., 2012). Government organizations, such as the World Health Organization (WHO), measure and/or provide guidelines for ambient PM₁₀ concentrations (PM₁₀, particles with aerodynamic diameter <10 μm). PM smaller than 10 μm in diameter is of particular interest because it is inhalable. The WHO has set guidelines for 24-hour and annual average PM₁₀ concentration at 45 and 15 $\mu\text{g}/\text{m}^3$, respectively (WHO, 2022). The US EPA's national ambient air quality standard for PM₁₀ concentration and are 150 and 50 $\mu\text{g}/\text{m}^3$ for the 24-hour and annual average, respectively. One challenge with 24-hour standards/guidelines is that dust events often last a few hours, and these events are obscured when reporting only the PM₁₀ 24-hour average or comparing these averages to the 24-hour guidelines (Ardon-Dryer and Kelley, 2022).

PM₁₀ concentrations tend to be more spatially heterogenous than PM_{2.5} concentrations because PM₁₀ settles more quickly (Keet et al., 2018). In addition, regulatory measurements of PM₁₀ are spatially and temporally sparser than PM_{2.5} measurements. For example, the US EPA reports measurements from 1,370 active PM_{2.5} sites versus 800 active PM₁₀ sites (EPA, 2022). Approximately half of these PM₁₀ sites only report 24-hour averages (USA EPA, 2022). Furthermore, many dust-prone areas of the US lack any PM monitoring (USA EPA, 2022). More highly resolved measurements of PM₁₀ concentration would aid communities and researchers in understanding and addressing the effects of windblown dust and dust events.

More recent studies of PM have leveraged low-cost PM measurements and mobile measurements to obtain higher spatial and temporal resolution PM_{2.5} estimates (Bi et al., 2020; Caplin et al., 2019; Lim et al., 2019; Caubel et al., 2019; Kelly et al., 2021). With appropriate calibration, low-cost sensors have been demonstrated to be generally effective at measuring PM_{2.5}; however, the most common low-cost PM sensors that employ a laser, and a photodiode to estimate particle concentration (Plantower PMS, Nova SDSS011, Sensirion SPS30, Shineyi PPD42NS, and Samyoung DSM501A) are ineffective at measuring PM₁₀ and dust (Kosmopoulos et al., 2020; Mei et al., 2020; Sayahi et al., 2019, Kuula et al. 2020) primarily due to truncation of the forward scattering coefficient for larger particles and in potentially due to the sensors' inability to aspirate the larger particles into the device (Ouimette et al., 2022). Kuula et al. (2020) tested several low-cost PM sensors using monodisperse di-octyl sebacate particles (0.5 – 10 μm) and observed a constant particle size distribution for particle sizes >0.5 μm and indicated that these sensors are incapable of measuring coarse-mode particles (2.5-10 μm).

The Alphasense OPC-N series is a promising low-cost sensor for measuring PM₁₀. It is larger and more expensive (~\$500) than many of the low-cost PM sensors (<\$50) with a greater flow rate (total flow of 5.5 LPM and sample flow rate of 0.28 L/min) and a mirror that allows collection of light scattering from broader array of angles than typical low-cost PM sensors, which have flow rates on the order of 0.1 LPM (Sayahi et al., 2019; Ouimette et al., 2022; Alphasense Ltd, 2022). The OPC-N3 allows particle counting in 24-size bins for sizes ranging from 0.35-40 µm. The working principle of Alphasense OPC-N3 and its previous version (OPC-N2) is similar to an aerosol spectrometer; it measures scattering from single particles (Vogt et al., 2021). Studies have used the Alphasense OPCs for indoor and ambient PM monitoring (Kaliszewski et al., 2020; Chu et al., 2021; Dubey et al., 2022b; Feenstra et al., 2019; Pope et al., 2018; Nor et al., 2021; Alhasa et al., 2018; Mohd Nadzir et al., 2020), to monitor PM_{2.5} personal exposure (Harr et al., 2022a), to identify PM sources (Harr et al., 2022b; Bousiotis et al., 2021), and to monitor occupational PM_{2.5} and PM₁₀ exposure (Runström Eden et al., 2022; Bächler et al., 2020). The Alphasense OPCs correlate well ($R^2 = 0.93-0.99$) with PM₁₀ in laboratory studies (Sousan et al., 2021, 2016; Samad et al., 2021; Dubey et al., 2022a). The field-based studies have reported somewhat lower correlations ($R^2: 0.53 - 0.8$) (Bílek et al., 2021; Dubey et al., 2022b, a; Crilley et al., 2018), due to the variable ambient meteorological conditions and changing PM compositions. The ambient PM ratios (PM_{2.5}/PM₁₀) in these previous studies were greater than 0.6, indicating the main contributions to PM levels were from the fine PMs, rather than coarser PMs. The ratio of PM_{2.5}/PM₁₀ can provide crucial information about particle origin and formation process (Xu et al., 2017; Speranza et al., 2014). Duvall et al. (2021) have suggested evaluating the performance of PM₁₀ sensors for varying PM_{2.5}/PM₁₀ ratios, and dust events provide a great opportunity to evaluate PM₁₀ sensor performance at ambient PM ratios <0.3.

Few studies have evaluated the performance of Alphasense OPCs for measuring PM₁₀ concentration during dust events. Gomes et al. (2022) measured hourly PM₁₀ concentration exceeding 300 µg/m³ using the OPC-N3 during Saharan dust events in western Portugal. In Sarajevo, Bosnia-Herzegovina, Masic, et al. (2020) reported that for the Aralkum Desert dust event, the OPC-N2 tracked GRIMM-11D PM₁₀ measurements but at a lower magnitude. Fewer studies have compared the Alphasense OPCs with the regulatory monitors during dust events. Vogt et al. (2021) reported that the OPC-N3 captures the long-range transported dust well, but slightly overestimates PM₁₀ concentration (<120 µg/m³) compared to a FIDAS (EN 16450 approved regulatory instrument). They also reported a moderate correlation with PM₁₀ compared to FIDAS ($R^2 = 0.58-0.64$, and RMSE between 12-13 µg/m³) and compared to a gravimetric method ($R^2 = 0.71-0.74$, and RMSE between 9-11 µg/m³). Mukherjee et al. (2017) evaluated the OPC-N2 performance against a Met One beta attenuation monitor (BAM) over 12 weeks in the Cuyama Valley of California, where PM concentrations are impacted by wind-blown dust events and regional transport; they reported a moderate to good degree of correlation ($R^2 = 0.53-0.81$, depending on sampling orientation) for PM₁₀ (<750 µg/m³). In general, the studies report that the OPC-N2/N3 tracks the temporal variation of research/reference measurements but with varying correlation factors.

A high PM_{2.5}/PM₁₀ ratio represents fine-dominated aerosols, likely corresponding to anthropogenic or other combustion sources. Low ratios represent coarser particles (aerodynamic size between 2.5-10 µm) that tend to

correspond to wind-blown dust (Sugimoto et al., 2016). Sugimoto et al. (2016) classified aerosols as local dust when the $PM_{2.5}/PM_{10}$ ratio was less than 0.1 and as transported dust when $PM_{2.5}/PM_{10}$ ratios were between 0.1 to 0.3. During dust events, low-cost sensors like the Plantower PMSs can detect only a small portion of a particle size distribution, and its response greatly depends on the particle size distribution and particle optical properties (Vogt et al., 2021). This study explores the possibility of using a size-segregated correction factor ($PM_{2.5}/PM_{10}$ ratio) to infer PM_{10} concentration from low-cost sensors that typically respond poorly to particles larger than 2.5 μm in diameter. If successful, this technique could leverage the large number of existing low-cost sensor measurements that use the Plantower PMS (and similar sensors) and improve spatial estimates of PM_{10} concentration.

This study aims to evaluate the Alphasense OPC-N3 to complement common low-cost PM measurements to understand PM_{10} concentrations during dust events in the Salt Lake Valley. The Salt Lake Valley is particularly well suited to studying dust events because it is affected by both regional dust events from the playas located to the west of the valley and from the drying Great Salt Lake bed, which has reached historic lows with more than 1865 km^2 of exposed lakebed (Perry et al., 2019). Under appropriate meteorological conditions, portions of this exposed lakebed produce substantial dust plumes, and the winds can transport this dust directly into the populated areas of the Salt Lake Valley (Perry et al., 2019).

2 Methods

This study focused on April of 2022 in the Salt Lake Valley, when it experienced five dust events (summarized in Table 1). It relies on low-cost sensors and reference/research measurements at three different locations (Fig. 1): the Utah Division of Air Quality (UDAQ)'s Hawthorne monitoring station (HW), the UDAQ's Environmental Quality (EQ) station and surroundings, and a residential site (RS) in the northeast quadrant of the Salt Lake Valley. This period included an hourly average FEM (Federal Equivalent Method) PM_{10} concentration that reached 311 $\mu g/m^3$.



Figure 1: Study locations in Salt Lake County: EQ (UDAQ Environmental Quality) site, HW (Hawthorne UDAQ) site, and RS (residential site). The distance between EQ to HW, HW to RS, and EQ to RS is 7.8 km, 4.3 km, and 7.35 km, respectively. The OPC and PMS sensors were collocated at RS and HW sites. Two PurpleAir II were located within 2 km of the EQ monitoring station.

152 **Table 1:** PM measurements at the three different study locations.

153

Site	Measurement type	Working principle	#	Sensor ID	Distance from a reference monitor	Hours of operation*
HW	OPC-N3	Light Scattering (optical particle counter)	1	OPC-HW	Collocation	633 ^a
	PurpleAir II	Light Scattering- (nephelometry)	2	PMS-HW-1A, PMS-HW-1B, PMS-HW-2A, PMS-HW-2B	Collocation	697
	Thermo Scientific Model 5030 SHARP analyzer	Light scattering (nephelometry) + BAM	1	PM _{2.5} FEM-HW	Federal equivalent method	697
	MetOne E-BAM PLUS	BAM	1	PM ₁₀ FEM-HW	Federal equivalent method	695
EQ	PurpleAir II	Light Scattering- (nephelometry)	2	PMS-EQ-1A, PMS-EQ-1B, PMS-EQ-2A, PMS-EQ-2B	480 m and 1.82 km	697
	Thermo Scientific Model 5030 SHARP analyzer	Light scattering (nephelometry) + BAM		PM _{2.5} FEM-EQ	Federal equivalent method	697
	MetOne E-BAM PLUS	BAM		PM ₁₀ FEM-EQ	Federal equivalent method	697
RS	OPC-N3	Light Scattering (optical particle counter)	1	OPC-RS	Collocation	425 ^c
	PurpleAir II	Light Scattering- (nephelometry)	2	PMS-RS-1A, PMS-RS-1B, PMS-RS-2A, PMS-RS-2B	Collocation	302 ^d
	GRIMM 1.109	Light Scattering (optical particle counter)		GRIMM	Research monitor	452

154 *Total number of available hours = 711. Measurements between 4/11/2022 8:00 pm – 4/12/22 5:00 am were not
155 available for HW, and subsequently removed for all sensors. Measurements corresponding to relative humidity
156 >85%, i.e., 14 hrs, were excluded.

157 ^aOPC-HW measurements were not available between 4/12/2022 6:00 pm – 4/14/2022 7:00 pm due to connectivity
158 issues.

159 ^cThe measurements for OPC-RS were available starting 9 April 2022. OPC-RS measurements between 4/14/2022
160 10:00 am – 4/17/2022 20:00 pm were not available due to connectivity issues.

161 ^dThe measurements from all the PurpleAir II at RS were available starting on 18 April 2022

2.1 Low-cost sensors

The low-cost sensors tested in this study include the Alphasense optical particle counter (OPC-N3, Alphasense Ltd, \$500) and the Plantower PMS5003 (\$20) integrated into the PurpleAir II (~\$259). The Alphasense OPC-N3 uses a class 1 laser (~658 nm) to detect, size, and count particles in the size range 0.35-40 μm in 24 bins, which is translated, using the embedded algorithm, into estimated PM_{10} , $\text{PM}_{2.5}$, and PM_1 mass concentrations. The default setting for the OPC-N3's refractive index is 1.5 (real part) and for density is 1.65 g/cm^3 , and these default settings were used throughout this study. The OPC-N3 uses an internal fan to create flow and reports a sample flow rate (~0.28 L/min and a total flow rate of 5.5 LPM). Each OPC-N3 was connected to a laptop and used the manufacturer-provided software. The OPC-N3 was set to store measurements every 1 min. The measurements included the date, size bins and counts, pump flow, relative humidity (RH), temperature, and PM_1 , $\text{PM}_{2.5}$, and PM_{10} concentration.

The PMS 5003 is a low-cost sensor (~\$20, Plantower Technology, China), which has been integrated into a variety of low-cost air quality sensor packages, such as TSI BlueSky, PurpleAir, etc. It uses a fan to create a flow (~0.1 L/min), and it is equipped with a red laser (~680 $\pm$ 10 nm), a scattering angle of 90°, and a photo-diode detector to convert the scattered light to a voltage pulse (Sayahi et al., 2019; Ouimette et al. 2022). The PMS sensor converts light scattering into several different air quality parameters, including particle counts (0.3-10 μm), PM_1 , $\text{PM}_{2.5}$, and PM_{10} , although these different metrics are all based on this single measurement, total light scattering. The PMS 5003 has been evaluated extensively in the laboratory and the field, and the measurements tend to correlate well with PM_1 or $\text{PM}_{2.5}$ concentration although it performs poorly for larger PM sizes, such as $\text{PM}_{2.5}$ - PM_{10} (Sayahi et al., 2019; Vogt et al., 2021; Kuula et al., 2020; Ouimette et al., 2022). In this study, we used two PurpleAir PA-II at the HW and RS sites, each PA-II has two PMS sensors per node. PM_{10} mass concentration corresponding to correction factor (CF) = 1 and a data collection rate of every 2 minutes were used. The data were downloaded from the PurpleAir website. In addition, we evaluated two PurpleAir PA-II sensors located within 2 km of the EQ monitoring station.

All the OPC-N3 were placed inside a custom build housing to protect the sensor from rain and insects. The details of housing can be found in the supplementary material (Section S3).

2.2 Site descriptions

The study includes measurements from the two UDAQ sites (HW and EQ) in Salt Lake County that provide both hourly $\text{PM}_{2.5}$ and PM_{10} measurements (Fig. 1). UDAQ uses a Thermo Scientific Model 5030 SHARP analyzer for measuring hourly $\text{PM}_{2.5}$ concentration and a MetOne E-BAM (Beta Attenuation Monitoring) PLUS for measuring PM_{10} concentration. We placed two PurpleAir PA-II (containing four Plantower PMS 5003s, named: PMS-HW-1A, PMS-HW-1B, PMS-HW-2A, PMS-HW-2B) and one OPC-N3 (named: OPC-HW) at the HW site (Table 1). The PurpleAir PA-IIs and the OPC-N3 were mounted on poles that extend above the roof of the HW monitoring station. The HW monitoring station is located in an urban residential area (AQS: 49-035-3006, Lat: 40.7343, Long: -111.8721) at an elevation of 1308m. This site was established to represent population exposure in the Salt Lake City area, and it is often the controlling monitor for the county. The average of PMS-HW-1A, PMS-HW-2A, and PMS-HW-2B PM_{10}

concentrations at HW were named PMS-HW. PMS-HW-2B was excluded from the PMS-HW average because of its moderate correlation with the other three sensors (Fig. S2).

We also evaluated two PurpleAir II (containing four Plantower PMS 5003s, named PMS-EQ-1A, PMS-EQ-1B, PMS-EQ-2A, PMS-EQ-2B) sensors located near the UDAQ EQ site. One of the sensors was 480 m away (PMS-EQ-1), while the other was 1.82 km away (PMS-EQ-2). The EQ monitoring station (AQS: 49-035-3015, Lat: 40.777028, Long: -111.94585, elevation 1284 m) is located approximately 14 km southeast of the Great Salt Lake dry lake bed. In addition to PM concentrations, we accessed relative humidity (RH), temperature, wind speed, and wind direction data from the two UDAQ monitoring sites on EPA's AirNow Tech website. EPA-flagged measurements were excluded from this study. UDAQ uses RM Young Ultrasonic Anemometer Model 86004 to measure the wind speed and wind direction and an instrument based on a hygroscopic plastic film to measure relative humidity.

The RS was located in the northeast quadrant of the Salt Lake Valley at an elevation of 1383 m (40.771938, -111.861290). Measurements at this site included four Plantower PMS 5003s (labeled as PMS-RS-1A, PMS-RS1B, PMS-RS-2A, PMS-RS-2B) in two PurpleAir PA-IIs, one OPC-N3 (labeled as OPC-RS) and one GRIMM (model 1.109 Aerosol Technik Ainring, Germany). The GRIMM employs an internal pump to create a flow of 1.2 L/min and measures the number concentration of particles of size 0.265 μm – 34 μm in 31 size bins, and reports estimated PM_{10} , $\text{PM}_{2.5}$, and PM_{10} concentrations. The GRIMM measurements were stored every minute in an internal storage card. The GRIMM measurements were not available between 4/24/2022 6:00PM -4/26/2022 2:00 PM MDT (Mountain Day Time). The PurpleAir PA-IIs and the GRIMM were mounted on the east side of a small outbuilding.

2.3 Data Analysis

The measurements from the low-cost sensors and the research monitor (GRIMM) were converted to hourly average concentrations and time-synchronized to MDT. Two EPA-flagged measurements corresponding to unexplainable high hourly PM_{10} concentrations ($>800 \mu\text{g}/\text{m}^3$) from FEM-HW were removed. The low-cost sensors used in this study were not supplemented with dryers, and therefore their performance is affected by high humidity conditions, which can result in condensation and droplet formation (Samad et al., 2021). Consequently, the measurements corresponding to relative humidity greater than 85% were excluded from the study ($<2\%$ of total measurements).

Using the HW and EQ meteorological measurements, we defined dust events as periods with PM_{10} concentrations exceeding $100 \mu\text{g}/\text{m}^3$ accompanied by winds exceeding 5 m/s at either site. These high winds were either observed at the beginning or during dust events. Each dust event typically included a period of time when PM_{10} concentrations began increasing before reaching peak values. After wind speeds began to decrease, PM_{10} concentration decreased gradually. The dust events in this study included the entire time period when wind/ PM_{10} levels decreased until PM_{10} concentrations reached background levels ($<50 \mu\text{g}/\text{m}^3$). Table 2 (for HW) and Table 1S (for EQ) provide the

meteorological parameters (wind speed, wind direction, temperature, and RH), PM_{2.5} and PM₁₀ concentrations, and PM_{2.5}/PM₁₀ ratios for each event.

We performed a linear regression to relate the PM₁₀ concentration measurements of the low-cost sensors to reference monitors at HW and EQ and a research monitor at the RS. Performance guidelines for low-cost PM₁₀ measurements are not yet available. For discussion purposes, we use EPA guidelines for low-cost PM_{2.5} sensors, which include acceptable performance as a slope of 1 ± 0.35 , intercept of $0 \pm 5 \mu\text{g}/\text{m}^3$, root mean square error (RMSE) $\leq 7 \mu\text{g}/\text{m}^3$, normalized root mean square error (NRMSE) $\leq 30\%$, and $R^2 > 0.7$ (when compared with the reference monitor) (Rachelle M. Duvall et al., 2021). RMSE and NRMSE were calculated using the following equations:

$$RMSE = \sqrt{\frac{1}{N} \sum_{t=1}^N (low\ cost\ sensor_t - Ref_t)^2}$$

$$NRMSE = \frac{RMSE}{\overline{Ref}} \times 100$$

where, *low cost sensor* represents the low-cost sensor measurement, $\overline{Ref}$ represents the reference/regulatory measurements, and $\overline{Ref}$ represents the average of the reference or regulatory monitor measurements.

We also explored a PM_{2.5}/PM₁₀ ratio-based calibration strategy for correcting PMS sensor readings. Based on the ratio of FEM-HW PM_{2.5}/PM₁₀, we segregated the FEM-HW and PMS-HW PM₁₀ measurements into six bins: PM_{2.5}/PM₁₀: <0.2, 0.2-0.3, 0.3-0.4, 0.4-0.5, 0.5-0.7, and >0.7. For each bin, the co-located PMS-HW PM₁₀ concentrations were linearly regressed against the FEM-HW PM₁₀ concentrations to obtain correction factors (slope and intercept). These correction factors were later used to correct the PMS PM₁₀ concentrations at the other two locations (RS and EQ). The PM_{2.5}/PM₁₀ ratios from the GRIMM and OPC-RS at the RS were calculated for use in the in selecting the appropriate PM-ratio-based correction factor and subsequent correction of the collocated PMS sensors. At the EQ site, the PM_{2.5}/PM₁₀ ratio from the FEM-EQ was used to select the appropriate PM-ratio-based correction factor and subsequent correction of the nearby PMS sensors.

Table 2: Meteorological and PM characteristics during the non-dust and dust events at the HW monitoring site. The number in the parenthesis represents the minimum and maximum of the parameter. Parameters for the EQ site can be found in Table S1 (supplementary material).

Start	Duration (hr)	Wind Speed (m/s)	Relative humidity %	Temperature (°C)	PM _{2.5} /PM ₁₀	PM ₁₀ (μg/m ³)
All non-dust duration	658	1.93 [0.26, 6.07]	39.7 [9, 92]	9.58 [-2.78, 23.3]	0.47 [0.056, 1]	165.47 [1.9, 99*]
4/9/22 5:00 AM	7	3.13 [1.13, 4.16]*	37.9 [28, 46]	10.4 [8.3, 13.8]	0.14 [0.10, 0.27]	81.3 [36, 140]

4/11/22 10:00 AM	9	4.12 [2.11, 5.91]	20.9 [12, 37]	12.4 [7.2, 15.6]	0.2 [0.13, 0.36]	67.6 [44, 101]
4/19/22 9:00 AM	10	3.75 [1.64, 5.60]	23.4 [17,32]	16.7 [13.3, 18.3]	0.24 [0.13, 0.36]	96.5 [54, 161]
4/21/22 11:00 AM	23	3.54 [1.02, 6.73]	37.6 [10, 79]	15.6 [7.2,23.9]	0.15 [0.08, 0.24]	141 [51, 274]
4/28/22 9:00 PM	4	3.17 [1.54, 5.14]	36.5 [28, 45]	14.4 [11.1, 17.2]	0.2 [0.10, 0.38]	79.5 [26, 128]

#a single measurement with high PM₁₀ concentration (99 µg/m³) was observed at 4/5/2022 12:00 am. The measurement did not meet the dust event criteria and hence was not included in the dust events.

*a wind speed of 6.27 m/s was observed at the EQ site.

3 Results and Discussion

Figure 2 shows the hourly average PM₁₀ concentration at the three different sites, with the dust events highlighted in grey. The five dust events were observed at all three locations, and they occurred at approximately the same time. Four of the dust events lasted less than 10 hours, and the event on 21 April 2022 lasted 23 hours. The PM_{2.5}/PM₁₀ ratio (Table 1) remained less than 0.3 during all the events, indicating the predominant contribution of coarser particles to PM₁₀. For each event, the PM₁₀ concentrations reached at least 100 µg/m³. During the 21st April event, hourly average PM₁₀ concentrations reached 275 µg/m³ at HW, 311 µg/m³ at EQ, and 173 µg/m³ at the RS site (Table 1 and Table 1S). The lower PM₁₀ concentration at the RS may be due to its residential location, its higher altitude, and its greater distance from dust sources. The OPC-HW and OPC-RS PM₁₀ concentration estimates followed the temporal pattern of the reference/research monitors including during the dust events. Previous studies have observed similar response for OPC-N3 and OPC-N2 (previous version of the OPC-N3) for dust events (Masic et al., 2020; Vogt et al., 2021). Vogt et al. (2021) found that the OPC-N3 tracked PM₁₀ concentrations from a FIDAS (EN 16450 approved regulatory instrument) for long-range transport dust events (PM₁₀ range 60 – 125 µg/m³). The PMS sensors followed the temporal pattern of the reference/research monitors except during the dust events when the PMS sensors substantially underestimated PM₁₀ concentration (Fig. 2). Vogt et al. (2021) also found that the PMS5003 underestimated the PM₁₀ concentration during dust events. In addition, Masic et al. (2020) reported that during the Aralkum Desert dust event (PM₁₀ reached 160 µg/m³), the PM₁₀ reported by OPC-N2 agreed well with the GRIMM 11-D (research-grade optical particle sizer), whereas the PMS5003 was not able to detect a large fraction of coarse particles correctly. Most of these studies recorded one dust event during their sampling duration, whereas this study found that the OPC-N3 tracked multiple dust events.

Figure 3 shows wind roses for April 2022 and each of the dust events. During the month of April, winds exceeding 5 m/s were observed at HW during 2.5% of the hours (1.81 % south predominant and 0.69% west predominant). For

dust events observed on 11th April and 21-22nd April, the high winds came from the south, whereas, for the rest of the events, high winds predominantly came from the west. The different wind directions could be transporting dust from different sources, such as the playas to the south and west of the Salt Lake Valley, the exposed playas of the Great Salt Lake, or local sources, such as mine tailing, gravel operations, unpaved roads, and an open-pit copper mine (Hahnenberger and Nicoll, 2012; Perry et al., 2019). All study monitoring sites are located west and southwest of the Great Salt Lake (Perry et al., 2019). Identifying the sources of the wind-blown dust and the effects of these differences on sensor performance would require a thorough analysis of the meteorology, the PM composition, and size distribution during the study period.

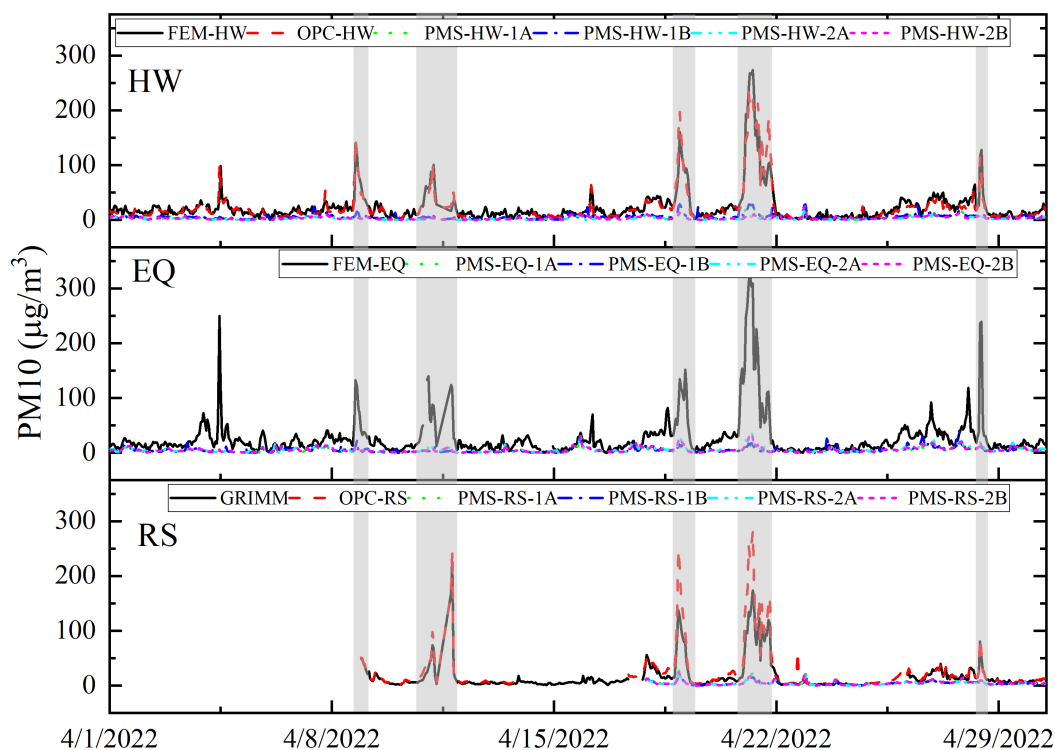


Figure 2: Hourly averaged PM₁₀ concentrations from the FEM, research monitors and low-cost sensors at the three different sites: HW, EQ, and RS. Black solid lines represent reference/research monitors; red dash represents OPC-N3; green dot, blue dash-dot, turquoise dash-dot-dot, and pink short-dash represent PMS sensors. The shaded peaks on 4/9/2022, 4/11/2022, 4/19/2022, 4/21/2022, and 4/28/2022 correspond to dust events. More details on these events can be found in Table 2.

3.1 OPC-N3 performance

Figure 4 illustrates the strong correlation between the OPC-N3 and the PM₁₀ concentration measured by the FEM at the HW site and the GRIMM monitor at the RS where the coefficient of determination ranges from 0.865 and 0.937. The intercept, slope, and R² were within the guidelines suggested by the EPA for low-cost PM_{2.5} sensors, although the RMSE and NRMSE (uncorrected measurements) exceeded the guidelines, 12.4 µg/m³ and 53.5 %, respectively (Fig.

4). Vogt et al. (2021) also observed a similar slope ($0.84\text{--}0.9\ \mu\text{g}/\text{m}^3$) and RMSE ($12\text{--}13\ \mu\text{g}/\text{m}^3$) for OPC-N3 hourly PM_{10} compared to FIDAS, but with a lower correlation ($R^2\ 0.58\text{--}0.64$) and for lower concentrations than this study. Vogt et al. (2021) did not correct the PM_{10} measurements for relative humidity, and approximately 20—30% of their measurements corresponded to high humidity conditions ($\text{RH} > 85\%$), and the inclusion of elevated RH conditions may have affected their correlations. The coefficient of determination in this study dropped to 0.81 after the inclusion of measurements corresponding to RH above 85%, which corresponded to just 2% of the total measurements (Fig. S1). Mukherjee et al. (2017) also reported correlations as high as 0.81 for OPC-N2 compared to BAM PM_{10} measurements in the Cuyama Valley of California, with OPC-N2 reporting PM_{10} concentrations of as high as $750\ \mu\text{g}/\text{m}^3$. Mukherjee et al. (2017) also did not correct the OPC data for relative humidity, which may have affected their correlations. Our study as well as previous studies suggest that the OPC-N3/OPC-N2 tends to underestimate the PM_{10} concentrations compared to the BAM (Mukherjee et al., 2017; Imami et al., 2022). The operating principle of the BAM and OPC-N3 differ. The BAM PM_{10} measurements are based on beta attenuation and do not require assumptions about particle properties or particle size distribution. In contrast, OPCs rely on the measured particle size distribution and assumed or measured particle properties (i.e., refractive index, shape, and density that can be size dependent) to estimate mass concentration. In addition, particles $< 0.3\ \mu\text{m}$ in diameter do not scatter light sufficiently. Consequently, some deviation from the mass measured by the FEM is expected. The assumptions about refractive index and shape affect how particles are size classified, and in addition assumptions about density, affect estimates of mass concentration.

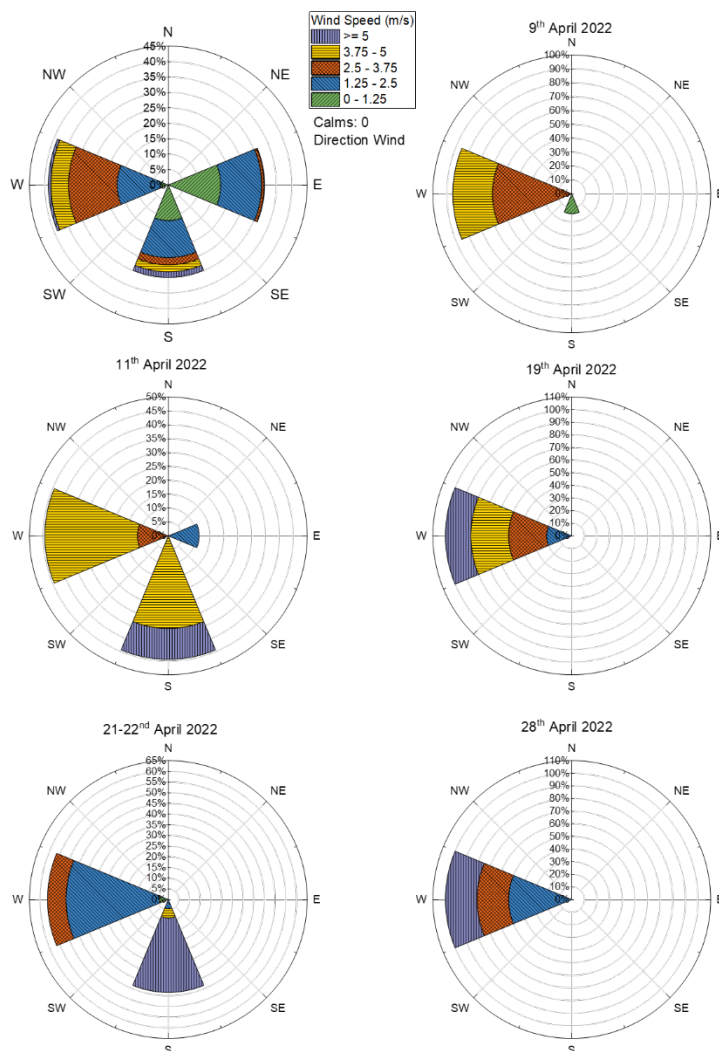


Figure 3: Wind roses for April 2022 and individual dust events, observed at HW. The wind roses for the EQ site can be found in the supplementary material (Fig. S13).

At the RS site, the OPC-RS showed a strong correlation with the GRIMM ($R^2 > 0.9$) and somewhat overestimated the PM_{10} concentration (slope = 1.45) compared to the GRIMM's default settings (Fig. 4). Such behavior from OPC-N3 and its predecessor model OPC-N2 has been observed previously. Crilley et al. (2018) also observed this same behavior for PM_{10} for the OPC-N2 versus the GRIMM (1.108) and reported that the OPC-N2 estimated two to five times greater PM_{10} mass than the GRIMM. Sousan et al. (2016) observed a slope of 1.6 for the Alphasense OPC-N2 compared to a GRIMM (1.108) for Arizona Road Dust. They attributed this behavior to the higher detection efficiency of OPC-N2 for particles $> 0.8 \mu m$ compared to the GRIMM, and the effect of aerosol composition on OPC-N2 readings. Unlike Sousan et al. (2016), Bezantakos et al. (2018), using polystyrene spheres (size: 0.8, 1, 2.5, 5.1, 7.2, and $10.2 \mu m$), reported that the OPC-N2 overestimated particle number concentrations, compared to GRIMM (1.109), for all sizes, not just size $> 1 \mu m$.

Crilley et al.(2018) considered high relative humidity as a controlling factor behind the overestimation by the OPC-N2. Badura et al. (2018) also reported a strong effect of relative humidity on the OPC-N2 measurements. We excluded measurement corresponding to $RH > 85\%$ because we focus on dust events, and RH is low during these events. We investigated the effect of RH (after excluding values $> 85\%$) by performing a multilinear regression with the FEM-HW as the dependent variable and the OPC-HW PM_{10} concentration and RH as independent variables. Adding RH did not significantly improve the correlation coefficient (not including RH: $R^2 = 0.865$, $RMSE = 12 \mu g/m^3$; including RH: $R^2 = 0.872$, $RMSE = 11.7 \mu g/m^3$; Section S1, Supplementary material). Hygroscopic growth changes with PM composition (Masic et al. 2020), and correcting measurements using a constant humidity coefficient can inject noise into the results. In addition, the Salt Lake Valley is in an arid region, and 82% of PM measurements corresponded to an RH of less than 60%. Consequently, the measurements were not corrected for the relative humidity for this study.

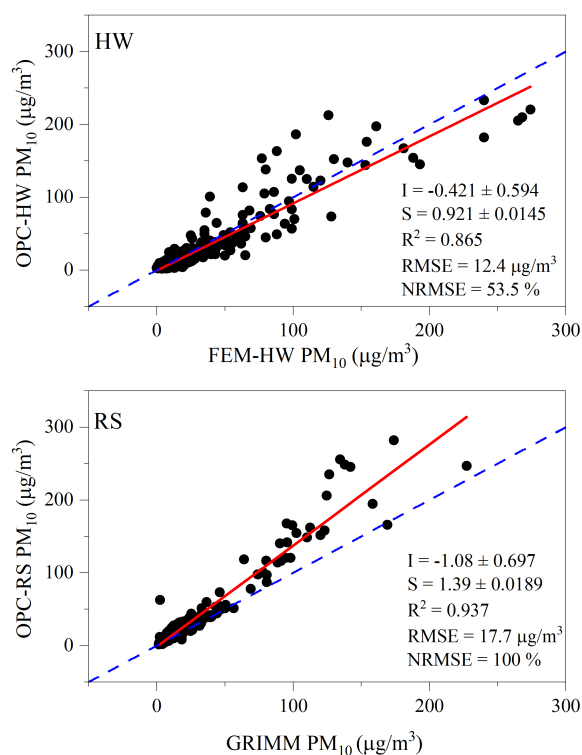


Figure 4: Hourly averaged PM_{10} concentration (top) OPC-HW vs. FEM-HW PM_{10} concentration for the period between 04/1/2022-04/30/2022, (bottom) OPC-RS vs. GRIMM PM_{10} concentration at the RS for the sampling period 04/09/2022-04/30/2022. The red solid line represents linear fit, and the blue dashed line represents the 1:1 line. I: intercept; S: slope.

3.2 Performance of the PMS5003

Figure 5, Figure 7 (top), and Figure 8 (top) illustrate the PMS sensors' poor-to-moderate correlations (R^2 between 0.128 and 0.482) with reference/research measurements of PM_{10} concentration; these sensors underestimate the PM_{10} concentration (slope < 0.09), particularly during dust events. These sensors also show high RMSEs ($> 30 \mu g/m^3$). Poor performance of PMS sensors for PM_{10} has been reported previously (Masic et al., 2020; Sayahi et al., 2019). Unlike

the OPC-N3, PMS sensors are nephelometers (Ouimette et al., 2022) and not optical particle counters, and their response decreases with increasing size. Previous studies reported decreased response from PMS 5003 sensors for particles larger than 0.5 μm (He et al., 2020; Kuula et al., 2020; Tryner et al., 2020). Kuula et al. (2020) and Tryner et al. (2020) observed constant particle size distributions from the PMS 5003 regardless of actual particle size (exposed monodisperse particles from polystyrene latex spheres, 0.1 – 2 μm , or generated with di-octyl sebacate 0.5– 10 μm). The PMS sensors' inability to aspirate particles larger 2.5 μm is a significant cause of these sensors' inability to detect coarse particles (aerodynamic size between 2.5 – 10 μm), such as those that dominate dust events (Ouimette et al. 2021).

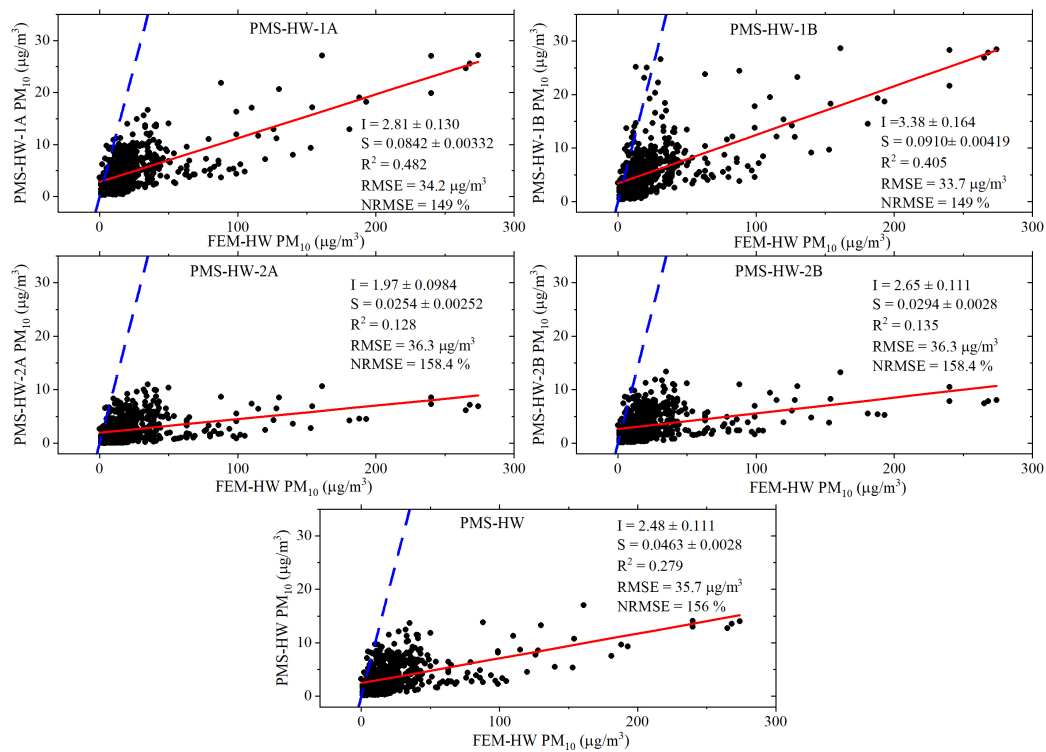


Figure 5: PMS PM_{10} concentration vs. FEM-HW PM_{10} concentration. PMS-HW represents the average of three PMS sensors (PMS-HW-1A, PMS-HW-2A, and PMS-HW-2B). The red solid line represents linear fit, and the blue line represents the 1:1 line. The plot includes measurements recorded between 04/1/2022 – 04/30/2022. I: intercept, and S: slope. Each measurement represents hourly averaged PM_{10} concentrations.

The PMS sensors also exhibited some inter-sensor variability during this study (Fig. S2). One sensor, PMS-HW-1B, exhibited a fair correlation with the other three PMS sensors ($R^2 = 0.53$ - 0.55 with slopes differing by more than 50%). The remaining three sensors (when compared to each other) had R^2 greater than 0.7, although their slopes differed by 40% (slope: PMS-HW-2A vs. PMS-HW-1A = 0.504; PMS-HW-2B vs. PMS-HW-1A = 0.577). In terms of response

to PM₁₀ and correlation with the reference monitor, PMS-HW-1(A and B) performed somewhat better than PMS-HW-2 (A and B) (RMSE < 35 µg/m³ and R² > 0.4, compared to RMSE < 36 and R² > 0.15).

Sensor-to-sensor variability has been reported in previous studies of PMS sensors, particularly for PM_{2.5} concentration (Sayahi et al., 2019; Tagle et al., 2020). The two PurpleAir II sensors (four PMS sensors) at the HW site were deployed on different dates. PMS-HW-1 was deployed on 4/24/2020, whereas the PMS-HW-2 was deployed on 9/20/2019. These sensors could be from different manufacturing batches, and they experienced different amounts of time in the field. Sensor aging can cause differences in PMS sensor performance (Tryner et al., 2020). In addition, because the PMS sensors are inefficient at measuring particles larger than PM_{2.5} µm in diameter, as evidenced by the low slopes in Figure 5, small differences (potentially due to sensor orientation and inherent differences in the sensors themselves) can magnify sensor to sensor variability. Mukherjee et al. (2017) and Duvall et al. (2021) discuss the importance of sampler positioning for PM₁₀ measurements. For presentation purposes, we have excluded the PMS-HW-1B, which exhibited poor correlation with the other PMS sensors (PMS-HW-1A, PMS-HW-2A, and PMS-HW-2B), and averaged the remaining three PMS PM₁₀ concentrations at HW and compared the average of the three sensors to the PM₁₀ concentrations measured by the FEM. Figure 5 shows the poor R² between the average of all PMS sensors and FEM PM₁₀ (R² = 0.279), and how the PMS-HW underestimates the PM₁₀ composition (slope of 0.0463).

3.3 Using PM_{2.5}/PM₁₀ ratios to obtain size-segregated PMS correction factors

The effect of correcting the PMS measurements with PM_{2.5}/PM₁₀ ratio-based factors on PMS performance was explored as a strategy to obtain correction factors that could enable the PMS measurements to infer PM₁₀ concentrations. The PM_{2.5}/PM₁₀ ratio, calculated using the PM_{2.5} and PM₁₀ concentrations reported by the FEM-HW, was used to segregate the PMS-HW measurements into six bins: PM_{2.5}/PM₁₀: <0.2, 0.2-0.3, 0.3-0.4, 0.4-0.5, 0.5-0.7, >0.7. For all the binned ratios (Figure 6), the PMS showed a consistent R² of greater than 0.6 (compared to R² values of 0.128 – 0.482 prior to binning), but with very different slopes for the different PM_{2.5}/PM₁₀ bins. The slope varied between 17 – 1.07, with the magnitude decreasing with the PM_{2.5}/PM₁₀ ratio. Note that Figures 4 and 5 show the FEM on the x axes, whereas Figure 6 shows the regression equations used for correcting the PMS measurements (with FEM on the y axes). During the dust events, the PM_{2.5}/PM₁₀ ratio was less than 0.3, supporting the large contribution from dust and the corresponding large magnitude of PM₁₀ concentration. The PM₁₀ concentrations were lowest for the high PM_{2.5}/PM₁₀ ratios (>0.7), and most PM₁₀ concentrations were below 5 µg/m³, which is close to the BAM's lower limit of detection (Met One Technical Bulletin BAM-1020 Detection Limit, 2022) and likely contributes to the low correlation observed for this ratio.

The slope and intercept for each bin were used as correction factors, called PM-ratio-based correction factors, to correct the PMS PM₁₀ measurements at the other two locations, i.e., RS and EQ.

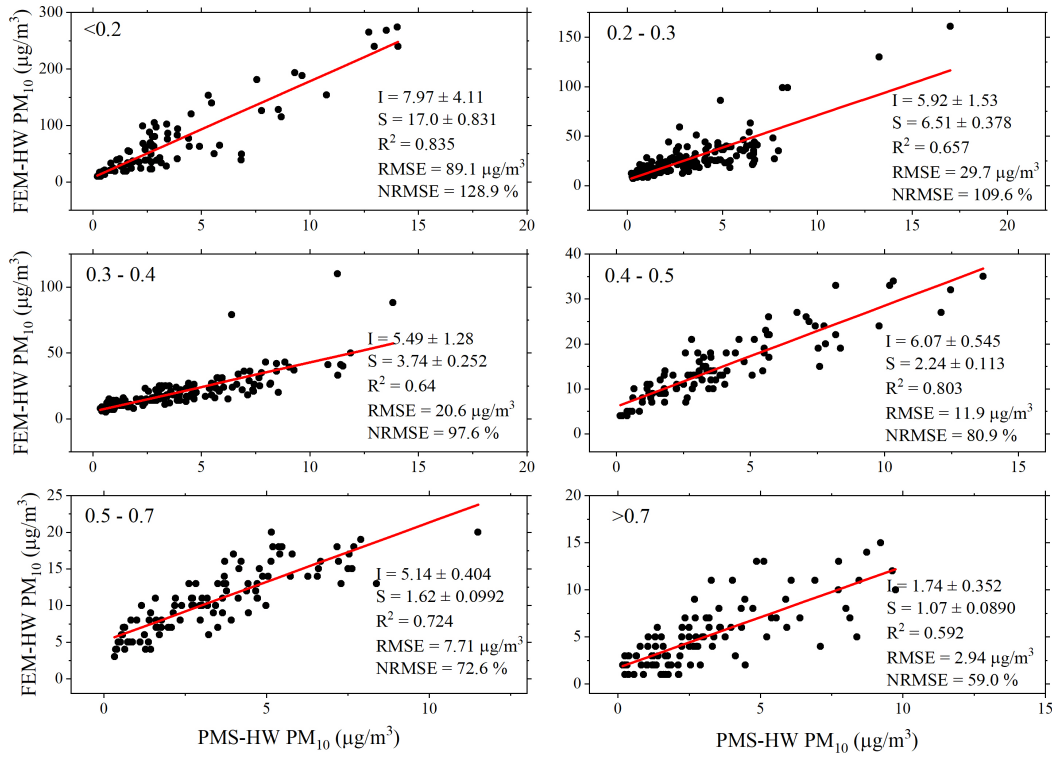


Figure 6: PMS-HW PM₁₀ concentration (average of three PMS sensors at HW) vs. FEM-HW PM₁₀ concentration for different PM_{2.5}/PM₁₀ bins. The RMSE and NRMSE has units μg/m³ and %, respectively. **Each measurement represents hourly averaged PM₁₀ concentrations.**

3.4 Correcting PMS data at RS and EQ sites

Similar to the HW site, the PMS PM₁₀ concentration measurements at the RS (Fig. 7, top) exhibited poor-to-moderate correlation (R² between 0.32-0.49, RMSE > 33 μg/m³) compared to the research monitor and underestimated the PM₁₀ concentrations (slope <0.099). We corrected the raw PMS PM₁₀ concentration measurements using the PM-ratio-based correction factors obtained from the HW site and the PM_{2.5}/PM₁₀ ratio from the GRIMM or the OPC to select a correction factor for each of the six PM_{2.5}/PM₁₀ bins. Using the GRIMM provided ratios, Figure 7 (middle) shows that at the RS, after PM-ratio-based correction of the PM₁₀ measurements, the correlation for all the PMS sensors improved significantly (R² > 0.77) and the RMSEs decreased (< 18 μg/m³). The R² varied between 0.773-0.810, and the slopes varied between 0.526-0.717. The intercept was a little higher (7-10 μg/m³) than the EPA suggested guideline for low-cost PM_{2.5} sensors. All the PMS sensors at RS were freshly deployed and were all mounted on the east side of a small building. These sensors exhibited good inter-sensor correlation (Fig. S4, R² > 0.97, slope > 0.77) and therefore exhibited very similar improvement all the sensors using the PM-ratio-based correction. The correlations between PMS PM₁₀ and GRIMM PM₁₀ concentrations were also good (R² > 0.7) when considering PM₁₀ < 50 μg/m³.

(Fig. S8 vs. Fig. S9), indicating that PM-ratio-based correction factors are applicable during more typical ambient levels of PM₁₀ (without dust events).

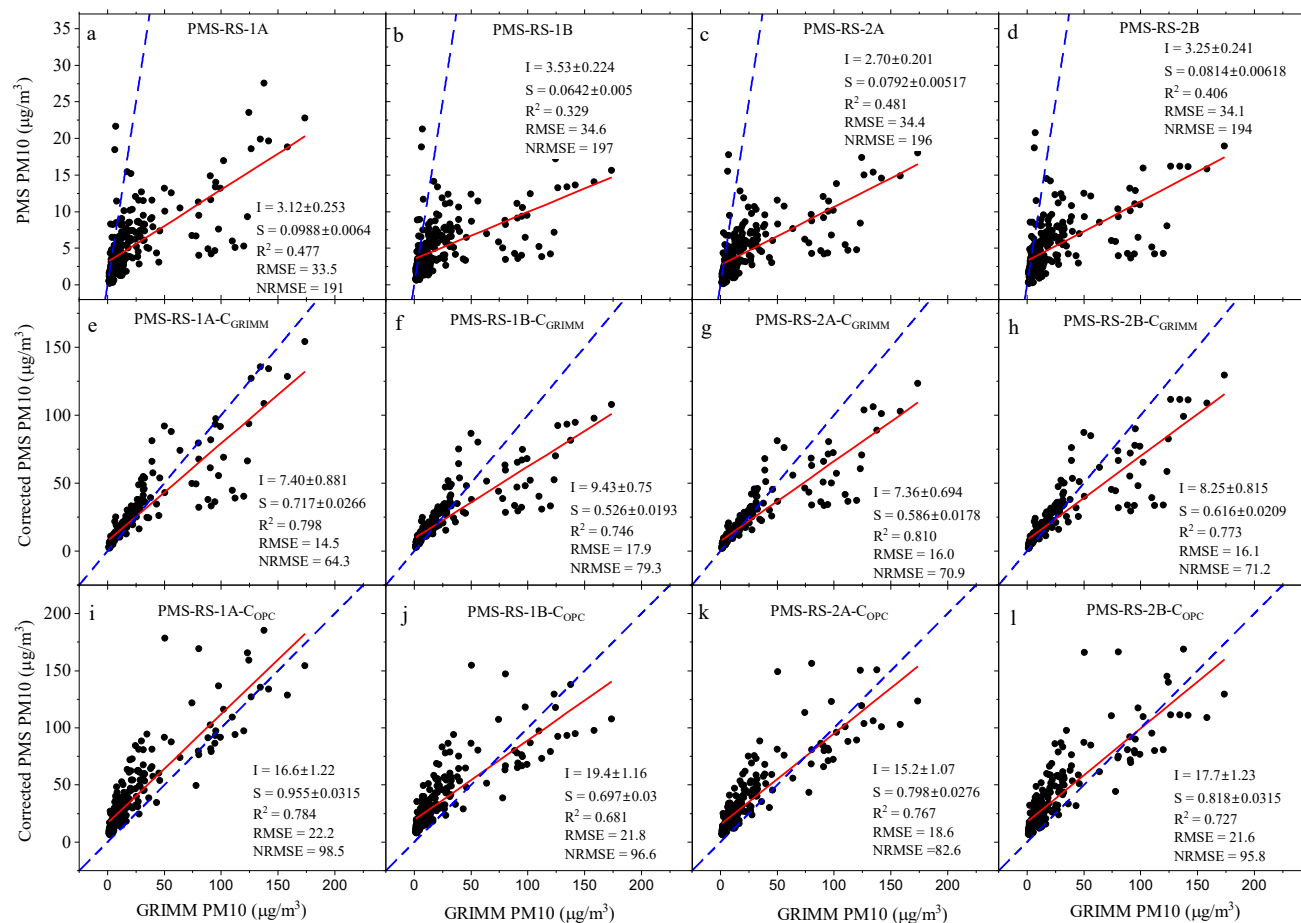


Figure 7: (Top: a, b, c, and d) Uncorrected PMS PM₁₀ concentration vs. GRIMM PM₁₀ concentration at RS the site. (Middle: e, f, g, and h) Corrected PM₁₀ concentrations using the PM-ratio-based correction factors developed at HW and the PM_{2.5}/PM₁₀ ratios provided by the GRIMM at the RS. (Bottom: i, j, k, and l) Corrected PM₁₀ concentrations using the PM-ratio-based correction factors developed at HW and the PM_{2.5}/PM₁₀ ratios provided by the OPC-RS at the RS. The solid red line represents the linear fit and the blue dash line represents the 1:1 line. The plots include measurements recorded between 04/18/2022 – 04/30/2022. I: intercept; S: slope. The RMSE and NRMSE has units μg/m³ and %, respectively. Each measurement represents hourly averaged PM₁₀ concentrations.

Figure 7 (bottom) illustrates a similar strategy at the RS site but using the OPC-RS to provide the PM_{2.5}/PM₁₀ ratio. It also shows that the correlation for PMS sensors improved after applying the PM-ratio-based correction using the OPC-RS for the ratio ($R^2 = 0.681 - 0.784$). After correction, the slope also increased and varied between 0.589-0.813. The corrected RMSE (18.6 – 22.2 μg/m³) and intercept (15.2-19.4 μg/m³) were somewhat higher than that observed when using GRIMM-reported PM ratios (Fig. 7 (middle)). From Figure 7 (bottom), the PM-ratio-based corrected PMS PM₁₀ concentration for PM₁₀ < 50 μg/m³ was always above the 1:1 line, i.e., the PMS PM₁₀ concentration was overestimated. The OPC-RS efficiency in counting particles smaller than 0.8 μm is lower than the GRIMM (Bezantakos et al., 2018;

Sousan et al., 2016), and therefore underestimates PM_{2.5} mass. Figure S5 also illustrates this overestimation in our study, where for low PM_{2.5} and PM₁₀ concentrations (90% of the measurements when PM_{2.5} < 12 µg/m³ and PM₁₀ < 40 µg/m³) the OPC-RS underestimated the PM_{2.5} mass compared to the GRIMM, although the OPC-RS PM₁₀ concentrations were similar to those of the GRIMM. The underestimated PM_{2.5} measurements from the OPC affected the PM_{2.5}/PM₁₀ ratios, which for the OPC-RS remained lower than those reported by the GRIMM (Fig. S6). The magnitude of the PM-ratio-based correction factors (Fig. 6) was inversely related to the PM_{2.5}/PM₁₀ ratio. Since the OPC-RS reported ratios were always low, the corrected PM₁₀ measurements below 50 µg/m³ were overestimated (Fig S10).

At the EQ site, we used the PM_{2.5}/PM₁₀ ratios from FEM measurements at the EQ site coupled with the PM-ratio-based correction factors developed at the HW site to correct the PMS PM₁₀ concentrations from sensors located near the EQ site. Correcting the PMS PM₁₀ concentrations using this approach did improve the correlation with FEM-EQ (Fig. 8). Before the correction, all the PMS sensors has poor correlation with the FEM ($R^2 < 0.342$ and slope < 0.0737). The R^2 improved to 0.617 - 0.797, and the slope increased to 0.602-1.38 after PM-ratio-based correction. The RMSE decreased and ranged between 21.5 – 35.6 µg/m³. The intercept increased and varied between 6.06-15.4. The sensors at this site showed moderate inter-sensor correlation (Fig. S7), which was expected as these sensors were not collocated. The different correlations with respect to FEM-EQ for the two PurpleAir II were also expected as these sensors were not collocated with the FEM-EQ.

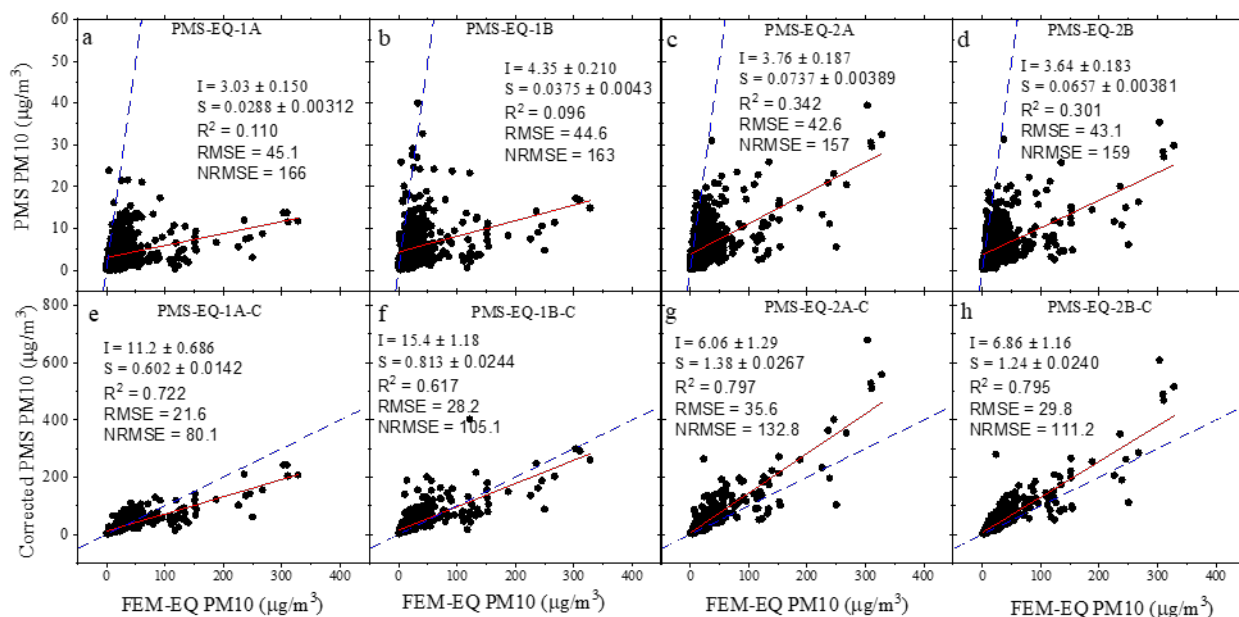


Figure 8: (top: a, b, c, and d) Uncorrected PMS PM₁₀ concentration vs. FEM-EQ PM₁₀ concentrations at the EQ site. (bottom: e, f, g, and h) Corrected PM₁₀ concentrations using the correction factors developed at HW and the PM_{2.5}/PM₁₀ ratios calculated using FEM-EQ PM₁₀ and PM_{2.5} concentrations. The solid red line represents the linear fit and the blue dash line represents the 1:1 line. The plots include measurements recorded between 04/1/2022 – 04/30/2022. I: intercept; S: slope. The RMSE and NRMSE has units µg/m³ and %, respectively. Each measurement represents hourly averaged PM₁₀ concentrations.

4 Limitations

This study has several limitations. The sensor's performance was evaluated for a month-long period in April 2022 and focused primarily on dust events, which commonly occur during this month. Understanding the OPC-N3 performance and whether using a $PM_{2.5}/PM_{10}$ ratio-based correction could improve correction factors for PMS sensors in other seasons and under different environmental conditions, like, wildfires, cold air pools, etc., would require a longer period of evaluation. This study used four PMS5003 sensors at the HW site and unlike the RS site, the sensors at HW were deployed at different times. These sensors showed moderate inter-sensor correlation, suggesting the need for further investigation of sensor age, sensor siting for PM_{10} measurements, and potentially recalibration. This study occurred in an arid region, with RH generally less than 60%. This study did not find a significant improvement by adding RH to a calibration model between the OPC-N3 and the FEM. However, this study excluded measurements with a RH > 85% (<2% of total measurements), a range where previous studies have identified a significant effect of RH (Crilley et al., 2018), and the applicability of this study's results to other, more humid, regions would need to be evaluated. The correction factors derived in this study used an average of three co-located PMS sensor measurements at a single site. In absence of detailed information about ambient particle properties, this study used default constant density for all the size-bins for OPC-N3. The Alphasense OPC-N3 allows the user to change the size-bin specific density for better estimates of PM_{10} , and if size-bin density and refractive index were available, the OPC measurements could potentially be improved. Our proposed PM-ratio-based calibration method relies on local measurements of the $PM_{2.5}/PM_{10}$ ratio. This requires FEM or other accurate measurements of $PM_{2.5}$ and PM_{10} concentration, and the needed spatial distribution of these accurate $PM_{2.5}$ and PM_{10} concentrations would need to be determined.

5 Conclusions

This study evaluated the performance of Alphasense OPC-N3 PM_{10} measurements compared to FEM and GRIMM measurements during multiple dust events at two locations (HW and RS). The OPC-N3 tracked all the dust events at the two locations and exhibited a strong correlation with reference measurements ($R^2 = 0.865 - 0.937$), RMSE of 12.4-17.7 $\mu g/m^3$, and NRMSE of 53.5 - 100 %. Uncorrected PMS5003 PM_{10} measurements showed poor to moderate correlation ($R^2 < 0.49$) with the reference/research monitors at three locations (HW, RS, and EQ), with a RMSE of 33-45 $\mu g/m^3$ and a NRMSE of 145-197 %. The PMS measurements severely underestimated the PM_{10} concentrations (slope <0.099). We evaluated a PM-ratio-based correction method to improve estimates of PM_{10} concentration from PMS sensors. After applying this method, PMS PM_{10} concentrations correlated reasonably well with FEM measurements ($R^2 > 0.63$) and GRIMM measurements ($R^2 > 0.76$), the RMSE decreased to 15-25 $\mu g/m^3$ and NRMSE decreased to 64 - 132 %. Our results suggest that it may be possible to leverage measurements from existing networks relying on low-cost $PM_{2.5}$ sensors to obtain better resolved spatial estimates of PM_{10} concentration using a combination of PMS sensors and measurements of $PM_{2.5}$ and PM_{10} , such as those provided by FEMs, research-grade instrumentation, or the OPC-N3.

Data Availability:

The raw and processed data used in the manuscript can be found at: <https://doi.org/10.7278/S50d-xbns-3ge3>

Authors Contribution:

KEK and KK conceptualized the research, collected, and analysed the data. KK developed the original draft and KEK reviewed the original draft. KEK provided the supervision and acquired the funding.

Competing interests:

Dr. Kerry Kelly has a financial interest in the company Tellus Networked Solutions, LCC, which commercializes solutions for environmental monitoring. Their technology was not used as part of this work.

Acknowledgements:

This material is based upon work supported by the National Science Foundation under Grant No. 2012091 Collaborative Research Network Cluster: Dust in the Critical Zone and under Grant No. 2228600 CIVIC-PG: TRACK A: Community Resilience through Engaging, Actionable, Timely, High-Resolution Air Quality Information (CREATE-AQI). Thanks to PurpleAir for donating two PAIIs to the project.

References:

- Akinwumiju, A. S., Ajisafe, T., and Adelodun, A. A.: Airborne Particulate Matter Pollution in Akure Metro City, Southwestern Nigeria, West Africa: Attribution and Meteorological Influence, *Journal of Geovisualization and Spatial Analysis*, 5, 11, <https://doi.org/10.1007/s41651-021-00079-6>, 2021.
- Alhasa, K., Mohd Nadzir, M., Olalekan, P., Latif, M., Yusup, Y., Iqbal Faruque, M., Ahamad, F., Abd. Hamid, H., Aiyub, K., Md Ali, S., Khan, M., Abu Samah, A., Yusuff, I., Othman, M., Tengku Hassim, T., and Ezani, N.: Calibration Model of a Low-Cost Air Quality Sensor Using an Adaptive Neuro-Fuzzy Inference System, *Sensors*, 18, 4380, <https://doi.org/10.3390/s18124380>, 2018.
- WHO: [https://www.who.int/news-room/fact-sheets/detail/ambient-\(outdoor\)-air-quality-and-health](https://www.who.int/news-room/fact-sheets/detail/ambient-(outdoor)-air-quality-and-health), last access: 5 October 2022.
- Ardon-Dryer, K. and Kelley, M. C.: Particle size distribution and particulate matter concentrations during synoptic and convective dust events in West Texas, *Atmos Chem Phys*, 22, 9161–9173, <https://doi.org/10.5194/acp-22-9161-2022>, 2022.
- Bächler, P., Szabadi, J., Meyer, J., and Dittler, A.: Simultaneous measurement of spatially resolved particle emissions in a pilot plant scale baghouse filter applying distributed low-cost particulate matter sensors, *J Aerosol Sci*, 150, <https://doi.org/10.1016/j.jaerosci.2020.105644>, 2020.

Badura, M., Batog, P., Drzeniecka-Osiadacz, A., and Modzel, P.: Evaluation of low-cost sensors for ambient PM_{2.5} monitoring, *J Sens*, 2018, <https://doi.org/10.1155/2018/5096540>, 2018.

Bezantakos, S., Schmidt-Ott, F., and Biskos, G.: Performance evaluation of the cost-effective and lightweight Alphasense optical particle counter for use onboard unmanned aerial vehicles, *Aerosol Science and Technology*, 52, 385–392, <https://doi.org/10.1080/02786826.2017.1412394>, 2018.

Bi, J., Wildani, A., Chang, H. H., and Liu, Y.: Incorporating Low-Cost Sensor Measurements into High-Resolution PM_{2.5} Modeling at a Large Spatial Scale, *Environ Sci Technol*, 54, 2152–2162, <https://doi.org/10.1021/acs.est.9b06046>, 2020.

Bílek, J., Bílek, O., Maršolek, P., and Buček, P.: Ambient air quality measurement with low-cost optical and electrochemical sensors: An evaluation of continuous year-long operation, *Environments - MDPI*, 8, <https://doi.org/10.3390/environments8110114>, 2021.

Bogan, M., Al, B., Kul, S., Zengin, S., Oktay, M., Sabak, M., Gümüşboğa, H., and Bayram, H.: The effects of desert dust storms, air pollution, and temperature on morbidity due to spontaneous abortions and toxemia of pregnancy: 5-year analysis, *Int J Biometeorol*, 65, 1733–1739, <https://doi.org/10.1007/s00484-021-02127-8>, 2021.

Bousiotis, D., Singh, A., Haugen, M., Beddows, D. C. S., Diez, S., Murphy, K. L., Edwards, P. M., Boies, A., Harrison, R. M., and Pope, F. D.: Assessing the sources of particles at an urban background site using both regulatory instruments and low-cost sensors – a comparative study, *Atmos Meas Tech*, 14, 4139–4155, <https://doi.org/10.5194/amt-14-4139-2021>, 2021.

Cai, H., Yang, Y., Luo, W., and Chen, Q.: City-level variations in aerosol optical properties and aerosol type identification derived from long-term MODIS/Aqua observations in the Sichuan Basin, China, *Urban Clim*, 38, 100886, <https://doi.org/10.1016/j.uclim.2021.100886>, 2021.

Caplin, A., Ghandehari, M., Lim, C., Glimcher, P., and Thurston, G.: Advancing environmental exposure assessment science to benefit society, *Nat Commun*, 10, 1236, <https://doi.org/10.1038/s41467-019-09155-4>, 2019.

Caubel, J. J., Cados, T. E., Preble, C. v., and Kirchstetter, T. W.: A Distributed Network of 100 Black Carbon Sensors for 100 Days of Air Quality Monitoring in West Oakland, California, *Environ Sci Technol*, 53, 7564–7573, <https://doi.org/10.1021/acs.est.9b00282>, 2019.

Chakravarty, K., Vincent, V., Vellore, R., Srivastava, A. K., Rastogi, A., and Soni, V. K.: Revisiting Andhi in northern India: A case study of severe dust-storm over the urban megacity of New Delhi, *Urban Clim*, 37, 100825, <https://doi.org/10.1016/j.uclim.2021.100825>, 2021.

Chu, M. D. T., Gillooly, S. E., Levy, J. I., Vallarino, J., Reyna, L. N., Cedeño Laurent, J. G., Coull, B. A., and Adamkiewicz, G.: Real-time indoor PM_{2.5} monitoring in an urban cohort: Implications for exposure disparities and source control, *Environ Res*, 193, <https://doi.org/10.1016/j.envres.2020.110561>, 2021.

Clifford, H. M., Spaulding, N. E., Kurbatov, A. v., More, A., Korotkikh, E. v., Sneed, S. B., Handley, M., Maasch, K. A., Loveluck, C. P., Chaplin, J., McCormick, M., and Mayewski, P. A.: A 2000 Year Saharan Dust Event Proxy Record from an Ice Core in the European Alps, *Journal of Geophysical Research: Atmospheres*, 124, 12882–12900, <https://doi.org/10.1029/2019JD030725>, 2019.

Crilley, L. R., Shaw, M., Pound, R., Kramer, L. J., Price, R., Young, S., Lewis, A. C., and Pope, F. D.: Evaluation of a low-cost optical particle counter (Alphasense OPC-N2) for ambient air monitoring, *Atmos Meas Tech*, 11, 709–720, <https://doi.org/10.5194/amt-11-709-2018>, 2018.

Dastoorpoor, M., Idani, E., Goudarzi, G., and Khanjani, N.: Acute effects of air pollution on spontaneous abortion, premature delivery, and stillbirth in Ahvaz, Iran: a time-series study, *Environmental Science and Pollution Research*, 25, 5447–5458, <https://doi.org/10.1007/s11356-017-0692-9>, 2018.

Met One Technical Bulletin BAM-1020 Detection Limit: https://metone.com/wp-content/uploads/2019/04/bam-1020_detection_limit.pdf, last access: 5 October 2022.

Diokhane, A. M., Jenkins, G. S., Manga, N., Drame, M. S., and Mbodji, B.: Linkages between observed, modeled Saharan dust loading and meningitis in Senegal during 2012 and 2013, *Int J Biometeorol*, 60, 557–575, <https://doi.org/10.1007/s00484-015-1051-5>, 2016.

Dubey, R., Patra, A. K., Joshi, J., Blankenberg, D., Kolluru, S. S. R., Madhu, B., and Raval, S.: Evaluation of low-cost particulate matter sensors OPC N2 and PM Nova for aerosol monitoring, *Atmos Pollut Res*, 13, <https://doi.org/10.1016/j.apr.2022.101335>, 2022a.

Dubey, R., Patra, A. K., Joshi, J., Blankenberg, D., and Nazneen: Evaluation of vertical and horizontal distribution of particulate matter near an urban roadway using an unmanned aerial vehicle, *Science of the Total Environment*, 836, <https://doi.org/10.1016/j.scitotenv.2022.155600>, 2022b.

Duvall, R. M., Hagler, G. S. W., Clements, A. L., Benedict, K., Barkjohn, K., Kilaru, V., Hanley, T., Watkins, N., Kaufman, A., Kamal, A., Reece, S., Fransioli, P., Gerboles, M., Gillerman, G., Habre, R., Hannigan, M., Ning, Z., Papapostolou, V., Pope, R., Quintana, P. J. E., and Lam Snyder, J.: Deliberating Performance Targets: Follow-on workshop discussing PM10, NO2, CO, and SO2 air sensor targets, in: *Atmospheric Environment*, <https://doi.org/10.1016/j.atmosenv.2020.118099>, 2021.

EPA: <https://www.epa.gov/outdoor-air-quality-data/interactive-map-air-quality-monitors>, last access: 5 October 2022.

USA EPA: https://aq5.epa.gov/aq5web/airdata/download_files.html, last access: 4 October 2022.

Feenstra, B., Papapostolou, V., Hasheminassab, S., Zhang, H., Boghossian, B. der, Cocker, D., and Polidori, A.: Performance evaluation of twelve low-cost PM2.5 sensors at an ambient air monitoring site, *Atmos Environ*, 216, <https://doi.org/10.1016/j.atmosenv.2019.116946>, 2019.

Gomes, J., Esteves, H., and Rente, L.: Influence of an Extreme Saharan Dust Event on the Air Quality of the West Region of Portugal, *Gases*, 2, 74–84, <https://doi.org/10.3390/gases2030005>, 2022.

Goudie, A. S.: Desert dust and human health disorders, *Environ Int*, 63, 101–113, <https://doi.org/10.1016/j.envint.2013.10.011>, 2014.

Hahnenberger, M. and Nicoll, K.: Meteorological characteristics of dust storm events in the eastern Great Basin of Utah, U.S.A., *Atmos Environ*, 60, 601–612, <https://doi.org/10.1016/J.ATMOSENV.2012.06.029>, 2012.

Harr, L., Sinsal, T., Simon, H., Konter, O., Dreiseitl, D., Schulz, P., and Esper, J.: PM2.5 exposure differences between children and adults, *Urban Clim*, 44, <https://doi.org/10.1016/j.uclim.2022.101198>, 2022a.

Harr, L., Sinsel, T., Simon, H., and Esper, J.: Seasonal Changes in Urban PM_{2.5} Hotspots and Sources from Low-Cost Sensors, *Atmosphere (Basel)*, 13, <https://doi.org/10.3390/atmos13050694>, 2022b.

He, M., Kuerbanjiang, N., and Dhaniyala, S.: Performance characteristics of the low-cost Plantower PMS optical sensor, *Aerosol Science and Technology*, 54, 232–241, <https://doi.org/10.1080/02786826.2019.1696015>, 2020.

Huang, J., Ji, M., Xie, Y., Wang, S., He, Y., and Ran, J.: Global semi-arid climate change over last 60 years, *Clim Dyn*, 46, 1131–1150, <https://doi.org/10.1007/s00382-015-2636-8>, 2016.

Imami, A. D., Driejana, Villegas, E. R., and McFiggans, G.: Evaluation of Alphasense OPC-N2 sensor for PM₁₀ measurement in the North Jakarta, *ASEAN Engineering Journal*, 12, 243–248, <https://doi.org/10.11113/aej.V12.17853>, 2022.

Jayaratne, E. R., Johnson, G. R., McGarry, P., Cheung, H. C., and Morawska, L.: Characteristics of airborne ultrafine and coarse particles during the Australian dust storm of 23 September 2009, *Atmos Environ*, 45, 3996–4001, <https://doi.org/10.1016/j.atmosenv.2011.04.059>, 2011.

Jones, B. A.: After the Dust Settles: The Infant Health Impacts of Dust Storms, *J Assoc Environ Resour Econ*, 7, 1005–1032, <https://doi.org/10.1086/710242>, 2020.

Kaliszewski, M., Włodarski, M., Młyńczak, J., and Kopczyński, K.: Comparison of low-cost particulate matter sensors for indoor air monitoring during covid-19 lockdown, *Sensors (Switzerland)*, 20, 1–17, <https://doi.org/10.3390/s20247290>, 2020.

Keet, C. A., Keller, J. P., and Peng, R. D.: Long-Term Coarse Particulate Matter Exposure Is Associated with Asthma among Children in Medicaid, *Am J Respir Crit Care Med*, 197, 737–746, <https://doi.org/10.1164/rccm.201706-1267OC>, 2018.

Kelly, K. E., Xing, W. W., Sayahi, T., Mitchell, L., Becnel, T., Gaillardon, P.-E., Meyer, M., and Whitaker, R. T.: Community-Based Measurements Reveal Unseen Differences during Air Pollution Episodes, *Environ Sci Technol*, 55, 120–128, <https://doi.org/10.1021/acs.est.0c02341>, 2021.

Kosmopoulos, G., Salamalikis, V., Pandis, S. N., Yannopoulos, P., Bloutsos, A. A., and Kazantzidis, A.: Low-cost sensors for measuring airborne particulate matter: Field evaluation and calibration at a South-Eastern European site, *Science of the Total Environment*, 748, <https://doi.org/10.1016/j.scitotenv.2020.141396>, 2020.

Kumar, S., Singh, A., Srivastava, A. K., Sahu, S. K., Hooda, R. K., Dumka, U. C., and Pathak, V.: Long-term change in aerosol characteristics over Indo-Gangetic Basin: How significant is the impact of emerging anthropogenic activities?, *Urban Clim*, 38, 100880, <https://doi.org/10.1016/j.uclim.2021.100880>, 2021.

Kuula, J., Mäkelä, T., Aurela, M., Teinilä, K., Varjonen, S., González, Ó., and Timonen, H.: Laboratory evaluation of particle-size selectivity of optical low-cost particulate matter sensors, *Atmos Meas Tech*, 13, 2413–2423, <https://doi.org/10.5194/amt-13-2413-2020>, 2020.

Lim, C. C., Kim, H., Vilcassim, M. J. R., Thurston, G. D., Gordon, T., Chen, L.-C., Lee, K., Heimbinder, M., and Kim, S.-Y.: Mapping urban air quality using mobile sampling with low-cost sensors and machine learning in Seoul, South Korea, *Environ Int*, 131, 105022, <https://doi.org/10.1016/j.envint.2019.105022>, 2019.

Liu, L., Duan, Y., Li, L., Xu, L., Yang, Y., and Cu, X.: Spatiotemporal trends of PM_{2.5} concentrations and typical regional pollutant transport during 2015–2018 in China, *Urban Clim*, 34, 100710, <https://doi.org/10.1016/j.uclim.2020.100710>, 2020.

Mallet, M., Tulet, P., Serça, D., Solmon, F., Dubovik, O., Pelon, J., Pont, V., and Thouron, O.: Impact of dust aerosols on the radiative budget, surface heat fluxes, heating rate profiles and convective activity over West Africa during March 2006, *Atmos Chem Phys*, 9, 7143–7160, <https://doi.org/10.5194/acp-9-7143-2009>, 2009.

Masic, A., Bibic, D., Pikula, B., Blazevic, A., Huremovic, J., and Zero, S.: Evaluation of optical particulate matter sensors under realistic conditions of strong and mild urban pollution, *Atmos Meas Tech*, 13, 6427–6443, <https://doi.org/10.5194/amt-13-6427-2020>, 2020.

Mei, H., Han, P., Wang, Y., Zeng, N., Liu, D., Cai, Q., Deng, Z., Wang, Y., Pan, Y., and Tang, X.: Field evaluation of low-cost particulate matter sensors in Beijing, *Sensors (Switzerland)*, 20, 1–17, <https://doi.org/10.3390/s20164381>, 2020.

Mohd Nadzir, M. S., Ooi, M. C. G., Alhasa, K. M., Bakar, M. A. A., Mohtar, A. A. A., Nor, M. F. F. M., Latif, M. T., Hamid, H. H. A., Ali, S. H. M., Ariff, N. M., Anuar, J., Ahamad, F., Azhari, A., Hanif, N. M., Subhi, M. A., Othman, M., and Nor, M. Z. M.: The Impact of Movement Control Order (MCO) during Pandemic COVID-19 on Local Air Quality in an Urban Area of Klang Valley, Malaysia, *Aerosol Air Qual Res*, 20, 1237–1248, <https://doi.org/10.4209/aaqr.2020.04.0163>, 2020.

Mukherjee, A., Stanton, L. G., Graham, A. R., and Roberts, P. T.: Assessing the utility of low-cost particulate matter sensors over a 12-week period in the Cuyama valley of California, *Sensors (Switzerland)*, 17, <https://doi.org/10.3390/s17081805>, 2017.

Nor, N. S. M., Yip, C. W., Ibrahim, N., Jaafar, M. H., Rashid, Z. Z., Mustafa, N., Hamid, H. H. A., Chandru, K., Latif, M. T., Saw, P. E., Lin, C. Y., Alhasa, K. M., Hashim, J. H., and Nadzir, M. S. M.: Particulate matter (PM_{2.5}) as a potential SARS-CoV-2 carrier, *Sci Rep*, 11, 2508, <https://doi.org/10.1038/s41598-021-81935-9>, 2021.

Ouimette, J. R., Malm, W. C., Schichtel, B. A., Sheridan, P. J., Andrews, E., Ogren, J. A., and Arnott, W. P.: Evaluating the PurpleAir monitor as an aerosol light scattering instrument, *Atmos Meas Tech*, 15, 655–676, <https://doi.org/10.5194/amt-15-655-2022>, 2022.

Perry, K. D., Crosman, E. T., and Hoch, S. W.: Results of the Great Salt Lake Dust Plume Study (2016–2018), 2019.

Pope, F. D., Gatari, M., Ng’ang’a, D., Poynter, A., and Blake, R.: Airborne particulate matter monitoring in Kenya using calibrated low-cost sensors, *Atmos Chem Phys*, 18, 15403–15418, <https://doi.org/10.5194/acp-18-15403-2018>, 2018.

Rachelle M. Duvall, Andrea L. Clements, Gayle Hagler, Ali Kamal, Vasu Kilaru, Laura Goodman, Samuel Frederick, Karoline K. (Johnson) Barkjohn, Ian VonWal, Danny Greene, and Tim Dye: Performance Testing Protocols, Metrics, and Target Values for Fine Particulate Matter Air Sensors: Use in Ambient, Outdoor, Fixed Site, Non-Regulatory Supplemental and Informational Monitoring Applications, 2021.

Runström Eden, G., Tinnerberg, H., Rosell, L., Möller, R., Almstrand, A. C., and Bredberg, A.: Exploring Methods for Surveillance of Occupational Exposure from Additive Manufacturing in Four Different Industrial Facilities, *Ann Work Expo Health*, 66, 163–177, <https://doi.org/10.1093/annweh/wxab070>, 2022.

Samad, A., Mimiaga, F. E. M., Laquai, B., and Vogt, U.: Investigating a low-cost dryer designed for low-cost PM sensors measuring ambient air quality, *Sensors (Switzerland)*, 21, 1–18, <https://doi.org/10.3390/s21030804>, 2021.

Sayahi, T., Butterfield, A., and Kelly, K. E.: Long-term field evaluation of the Plantower PMS low-cost particulate matter sensors, *Environmental Pollution*, 245, 932–940, <https://doi.org/10.1016/j.envpol.2018.11.065>, 2019.

Schweitzer, M. D., Calzadilla, A. S., Salamo, O., Sharifi, A., Kumar, N., Holt, G., Campos, M., and Mirsaedi, M.: Lung health in era of climate change and dust storms, *Environ Res*, 163, 36–42, <https://doi.org/10.1016/j.envres.2018.02.001>, 2018.

Sousan, S., Koehler, K., Hallett, L., and Peters, T. M.: Evaluation of the Alphasense optical particle counter (OPC-N2) and the Grimm portable aerosol spectrometer (PAS-1.108), *Aerosol Science and Technology*, 50, 1352–1365, <https://doi.org/10.1080/02786826.2016.1232859>, 2016.

Sousan, S., Regmi, S., and Park, Y. M.: Laboratory evaluation of low-cost optical particle counters for environmental and occupational exposures, *Sensors*, 21, <https://doi.org/10.3390/s21124146>, 2021.

Soy, F. K.: The effects of dust storms on quality of life of allergic patients with or without asthma, *The Turkish Journal of Ear Nose and Throat*, 26, 19–27, <https://doi.org/10.5606/kbbihtisas.2016.56254>, 2016.

Speranza, A., Caggiano, R., Margiotta, S., and Trippetta, S.: A novel approach to comparing simultaneous size-segregated particulate matter (PM) concentration ratios by means of a dedicated triangular diagram using the Agri Valley PM measurements as an example, *Natural Hazards and Earth System Sciences*, 14, 2727–2733, <https://doi.org/10.5194/nhess-14-2727-2014>, 2014.

Sugimoto, N., Shimizu, A., Matsui, I., and Nishikawa, M.: A method for estimating the fraction of mineral dust in particulate matter using PM_{2.5}-to-PM₁₀ ratios, *Particuology*, 28, 114–120, <https://doi.org/10.1016/j.partic.2015.09.005>, 2016.

Tagle, M., Rojas, F., Reyes, F., Vásquez, Y., Hallgren, F., Lindén, J., Kolev, D., Watne, Å. K., and Oyola, P.: Field performance of a low-cost sensor in the monitoring of particulate matter in Santiago, Chile, *Environ Monit Assess*, 192, 171, <https://doi.org/10.1007/s10661-020-8118-4>, 2020.

Tam, W. W. S., Wong, T. W., Wong, A. H. S., and Hui, D. S. C.: Effect of dust storm events on daily emergency admissions for respiratory diseases, *Respirology*, 17, 143–148, <https://doi.org/10.1111/j.1440-1843.2011.02056.x>, 2012.

Alphasense Ltd: https://www.alphasense.com/wp-content/uploads/2022/09/Alphasense_OPC-N3_datasheet.pdf, last access: 12 October 2022.

Tong, D. Q., Wang, J. X. L., Gill, T. E., Lei, H., and Wang, B.: Intensified dust storm activity and Valley fever infection in the southwestern United States, *Geophys Res Lett*, 44, 4304–4312, <https://doi.org/10.1002/2017GL073524>, 2017.

Trianti, S.-M., Samoli, E., Rodopoulou, S., Katsouyanni, K., Papiris, S. A., and Karakatsani, A.: Desert dust outbreaks and respiratory morbidity in Athens, Greece, *Environmental Health*, 16, 72, <https://doi.org/10.1186/s12940-017-0281-x>, 2017.

Tryner, J., Mehaffy, J., Miller-Lionberg, D., and Volckens, J.: Effects of aerosol type and simulated aging on performance of low-cost PM sensors, *J Aerosol Sci*, 150, 105654, <https://doi.org/10.1016/j.jaerosci.2020.105654>, 2020.

Vogt, M., Schneider, P., Castell, N., and Hamer, P.: Assessment of low-cost particulate matter sensor systems against optical and gravimetric methods in a field co-location in norway, *Atmosphere (Basel)*, 12, <https://doi.org/10.3390/atmos12080961>, 2021.

Williams, A. P., Cook, B. I., and Smerdon, J. E.: Rapid intensification of the emerging southwestern North American megadrought in 2020–2021, *Nat Clim Chang*, 12, 232–234, <https://doi.org/10.1038/s41558-022-01290-z>, 2022.

Xu, G., Jiao, L., Zhang, B., Zhao, S., Yuan, M., Gu, Y., Liu, J., and Tang, X.: Spatial and temporal variability of the PM_{2.5}/PM₁₀ ratio in Wuhan, Central China, *Aerosol Air Qual Res*, 17, 741–751, <https://doi.org/10.4209/aaqr.2016.09.0406>, 2017.