

# A versatile water vapor generation module for vapor isotope calibration and liquid isotope measurements

Hans Christian Steen-Larsen<sup>1</sup>, Daniele Zannoni<sup>1,2</sup>

<sup>1</sup>Geophysical Institute, University of Bergen and Bjerknes Centre for Climate Research, Bergen, Norway

5 <sup>2</sup>Department of Environmental Sciences, Informatics and Statistics, University Ca' Foscari of Venice, Venice, Italy

*Correspondence to:* Hans Christian Steen-Larsen ([Hans.Christian.Steen-Larsen@uib.no](mailto:Hans.Christian.Steen-Larsen@uib.no))

## Abstract.

10 A versatile vapor generation module has been developed for both field-based water vapor isotope calibrations and laboratory-based liquid water isotope measurements. The vapor generation module can generate a stream of constant vapor at a wide variety of humidity levels spanning 300 ppmv to 30 000 ppmv and is fully scalable allowing in principle an unlimited number of standards or samples to be connected. This versatility opens up the possibility for calibrating with multiple standards during field deployment including examining instrument isotope-humidity dependence. Utilizing the ability to generate an  
15 uninterrupted constant stream of vapor we document an Allan Deviation for <sup>17</sup>O-excess ( $\Delta^{17}\text{O}$ ) of less than 2 per meg for an approximate 3-hour averaging time. For similar averaging time the Allan Deviation for  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$ ,  $\delta\text{D}$ , d-excess is 0.004, 0.005, 0.01, 0.04 ‰. Measuring unknown samples shows that it is possible to obtain an average standard deviation of 3 per meg for  $\Delta^{17}\text{O}$  and an average standard error (95 % confidence limit) of 5 per meg.

Using the vapor generation module, we document that an increase in the Allan Deviation above the white noise level for  
20 integration times between 10 minutes and 1 hour is caused by cyclic variations in the cavity temperature, which if improved upon could result in an improvement in liquid sample measurement precision of up to a factor of 2. We further argue that increases in Allan Deviation for longer averaging times could be a result of memory effects and not only driven by instrumental drifts as it is often interpreted.

The vapor generation module as a calibration system has been documented to generate a constant water vapor stream for more  
25 than 90 hours showing the feasibility of being used to integrate measurements over much longer periods than achievable with syringe-based injections as well as allowing the analysis of instrument performance and noise. Using clean in-house standards, we have operated the vapor generation module daily for 1-3 hours for more than 6 months without the need for maintenance, illustrating the potential as a field-deployed autonomous vapor isotope calibration unit. When operating the vapor generation module for laboratory-based liquid water isotope measurements we document a more than 2 times lower memory effect  
30 compared to a standard autosampler system.

## 1 Introduction

Water samples from the atmospheric hydrological cycle in the states of liquid, solid, and vapor offer an extraordinary tool for understanding how meteorological and hydrological processes drive the climate system. The isotopic composition of meteoric water represents integrated information of the water cycle from evaporation at the ocean and land surface along the air mass trajectory until the water molecules in the end fall back to the surface either as liquid or solid precipitation (e.g. Galewsky et al., 2016).

The relative abundance of HD<sup>16</sup>O and H<sub>2</sub><sup>18</sup>O compared to H<sub>2</sub><sup>16</sup>O of meteoric water samples have routinely been measured for the last more than 60 years (e.g. Craig and Gordon, 1965; Dansgaard, 1964) and in recent decades also along with the relative abundance of H<sub>2</sub><sup>17</sup>O (e.g. Steig et al., 2014; Luz and Barkan, 2005). The relative abundance of HD<sup>16</sup>O, H<sub>2</sub><sup>17</sup>O, H<sub>2</sub><sup>18</sup>O compared to H<sub>2</sub><sup>16</sup>O, referred to using the  $\delta$ -notation (Craig, 1961), is classically understood through the first order principle of temperature-driven distillation during transport in the atmosphere (Dansgaard, 1964). To account for kinetic processes during phase transition for example during ocean evaporation (Merlivat and Jouzel, 1979), formation of snow crystals (Jouzel and Merlivat, 1984), sublimation from snow (Wahl et al., 2021), and plant transpiration (Landais et al., 2006), second order parameters such as the d-excess (Dansgaard, 1964) and the <sup>17</sup>O-excess ( $\Delta^{17}\text{O}$ ) (Landais et al., 2008) are defined as:

$$d - excess = \delta D - (8 \times \delta^{18}O)$$

$$\Delta^{17}O = \text{Ln}(\delta^{17}O + 1) - 0.528 \text{Ln}(\delta^{18}O + 1)$$

The number of atmospheric water vapor isotope measurements has over the last decade increased rapidly thanks to the availability of commercial water vapor isotope laser spectroscopy analysers. Similarly, the number of laboratories that carry out routine measurements of liquid water samples for their isotopic composition has increased thanks to the lowering in costs of acquiring a laser spectroscopy analyser and the ease of use compared to isotope ratio mass spectrometry (IRMS). This development has allowed the scientific community to enhance the understanding of the hydrological cycle by not only using collected precipitation samples but also measuring the exchange and transport of water vapor in the climate system. However, the availability of high-accuracy water vapor isotope measurements has hinged on the ability to make robust and reliable field measurements of water vapor with known isotopic composition based on laboratory standards referenced against the international VSMOW-SLAP scale. Similarly, the availability of second-order parameters such as the d-excess or the  $\Delta^{17}\text{O}$  is dependent on the ability to make high accuracy measurements of  $\delta^{18}\text{O}$ ,  $\delta^{17}\text{O}$ , and  $\delta D$ .

Commercial systems including the Water Vapor Isotope Standard Source (WVISS) from Los Gatos Research and the Standard Delivery Module (SDM) from Picarro inc. have been developed together with commercial water vapor isotope analysers. However, challenges in the calibration of measurements using these systems for long deployments (Bonne et al., 2014; Steen-Larsen et al., 2015) or deployments in low humidity regions (Guilpart et al., 2017) have been documented. Custom-made

changes to the SDM system have been carried out to facilitate long-term deployments (Bastrikov et al., 2014). While the SDM  
65 system allows two standards to be used, the WVISS system only allows a single standard to be measured without manually  
changing the standard. For the WVISS this implies that a VSMOW-SLAP scale calibration cannot be performed automatically.  
For the SDM this implies that the accuracy of the calibration cannot be assessed using a third known standard as is standard  
protocol for liquid water isotope measurements (e.g. Van Geldern and Barth, 2012).

70 To overcome some of these challenges custom-made calibration systems have been developed, specifically targeting the  
conditions of the field deployment. The simplest and to date most robust calibration system in terms of long-term deployment  
is the bubbler system, which has been used continuously at the water vapor isotope monitoring station in Bermuda for more  
than 10 years (Zannoni et al., 2022; Steen-Larsen et al., 2014). The versatility of the system lies in the wide humidity range  
(1000 ppm to 30 000 ppm) and the minimal need for manual intervention to operate (e.g. Bailey et al., 2015; Ellehoj et al.,  
75 2013). However, for the system to operate with low uncertainty (providing calibration pulses with an uncertainty of +/- 0.1/1.0  
‰ for  $\delta^{18}\text{O}/\delta\text{D}$ ) it is a requirement that temperature stability to within half a degree is obtained. In addition, large quantities  
(3-5 litre depending on deployment period) of water standards are needed and it is not practical to transport. These constraints  
mean that the bubbler system is not feasible for many field campaigns.

80 Besides bubbler-systems, custom-made calibration systems have been developed on the principle of either complete  
evaporation of small water droplets or steady-state evaporation of a sub-millimeter-size droplet. To the former group of  
calibration systems count the use of a dew point generator (Lee et al., 2005), dripper-systems (Tremoy et al., 2011; Lee et al.,  
2005), nebulizer-systems (Jones et al., 2017), and piezoelectric microdrop generators (Iannone et al., 2009). While these  
systems have been proven to work under field conditions, they require significant time to equilibrate and may potentially be  
85 sensitive to room temperature fluctuations. For the operation of the nebulizer-system, the system needs in the order of 5 L/min  
dry air to achieve low humidity levels, which provides additional need for bringing a high-performing dry air generator into  
the field, which adds logistical challenges of organizing field campaigns.

To the group of calibration systems operating on the principles of steady-state evaporation belongs a field deployable system  
90 developed by Gkinis et al. (2011) for continuous ice core water isotope analysis directly in the field and a dedicated low-  
humidity calibration system developed by Leroy-Dos Santos et al. (2021). The system developed by Gkinis et al. (2011) used  
a combination of a peristaltic pump and tuned back-pressure to push water through a silica capillary into a micro-Tee heated  
to 170 deg C. A similar system has also been deployed and used for calibration of water vapor isotope measurements (Benetti  
et al., 2017; Steen-Larsen et al., 2014). A similar system has also been shown to be reliable for  $\Delta^{17}\text{O}$  measurements in  
95 continuous-flow analysis of ice core samples (Davidge et al., 2022).

To achieve atmospheric water vapor and liquid sample data of highest quality it is crucial to address the sources of measurement uncertainty arising through both the measurement protocol and the instrumental drift. Several published protocols exist for liquid samples (e.g. Hutchings and Konecky, 2023; Penna et al., 2012; Van Geldern and Barth, 2012) and atmospheric water vapor (e.g. Bailey et al., 2015; Steen-Larsen et al., 2013) along with a multitude of laboratory-specific protocols. However, improvement of liquid measurement protocols for better precision and accuracy has been restricted to adjusting the number of injections, the amount of injected liquid, and to a small degree changes in integration time. For measurement protocols of water vapor isotopes, improvements have been restricted by the lack of a possibility of generating a continuous vapor stream with constant and known isotopic composition at different humidity levels using more than 2 standards.

Our goal was to not only develop a field-deployable water vapor isotope calibration system targeting the shortcomings described above, but also developing a system for liquid sample measurements exceeding available systems in throughput and accuracy. To achieve this we have further developed the vapor generation module, for which a patent application was filed in 2015 and published in Steen-Larsen (2016). Our target for the water vapor isotope calibration needs were:

- Field deployable i.e. robust, transportable, and easy to operate
- Multiple standard measurement capability
- High humidity span from 300 to 30 000 ppmv
- High flow rate span of vapor with a constant known isotopic composition
- Possibility to calibrate with sufficient high accuracy for  $\Delta^{17}\text{O}$  data

Our target for the liquid measurements were:

- Scalable system in terms of the number of unknown samples
- Improvement in sample measurement time compared to discrete injections for similar precision
- User-defined choice of integration time and hence measurement accurateness and precision.
- Comparable sample material use as discrete measurements/Small quantity of sample material required.

The developed system should have the ability to be used both for liquid measurements and for calibration of water vapor isotope measurements. In addition, the system should have sufficient stability to function as a benchmark tester for isotope analyzer performance by supplying a constant stream of water vapor with a known isotopic composition over multiple days.

To further demonstrate the fulfillment of all the proposed targets, we report two case studies as representative of water isotope calibration and liquid measurement applications:

- A humidity-isotope characterization curve performed during a field campaign in the Arctic,

130 - The liquid analysis of  $\Delta^{17}\text{O}$  of artificial samples generated from mixing of two reference waters with known  $\Delta^{17}\text{O}$  values.

## 2 Materials and Methods

### 2.1 Vapor Generation Module description

135 The vapor generation module is an improved and revised version of an original prototype developed in 2014 for which a patent application was filed in 2015 (Steen-Larsen, 2016). The previous prototype was reengineered at the beginning of 2021 and its schematic with a generic number of ovens ( $n$ ) is reported in Fig. 1. A four-oven version was used in this study. The focus of the improvements compared to the original prototype is the control of the liquid going into the oven and control on stopping the flow of liquid into the oven.

140 The operating principle of the vapor generation module is based upon the *flash evaporator* method, which is adopted in the water stable isotopes community for continuous flow analysis of ice-cores and for atmospheric water vapor analysis (e.g. Gkinis et al., 2011; Leroy-Dos Santos et al., 2021). In the flash evaporator, a droplet of water continuously evaporates on the tip of a needle/capillary inside an evaporation chamber at high temperature. The temperature of the evaporation chamber is precisely controlled well above the boiling point (in this work at  $170^\circ\text{C}$ ) and the volume is continuously flushed with dry air  
145 to produce a water vapor stream with the same isotopic composition of the water source in the needle. As recently demonstrated, no fractionation occurs during operation in steady state, and back diffusion from the tip through the capillary line is not sufficient to affect the water vapor isotopic composition inside the water reservoir (Kerstel, 2021; Leroy-Dos Santos et al., 2021). To push the water through the capillary, previous studies used syringe pumps or combinations of tubings of different size to generate sufficient back pressure (Gkinis et al., 2011; Landsberg et al., 2014; Leroy-Dos Santos et al., 2021).  
150 In this study, we used compressed dry air, with headspace pressure precisely controlled by an electronic pressure regulator (ALICAT PCD-5PSIG, resolution 0.01 PSI), as proposed in Steen-Larsen (2016).

The main improvements from the original design are the presence of:

1. A vacuum pump that can be connected to the vial headspace via a three-way valve and a vacuum valve to halt vapor  
155 generation in the oven.
2. A proportional-integral-derivative PID control loop to control and stabilize humidity level.
3. An additional mixing tee connected (2<sup>nd</sup> stage mixing) to a secondary mass flow controller (MFC2) to ensure a larger dynamic humidity range.
4. The use of a dual valve pressure controller flow meter to enable seamless control of humidity level.
- 160 5. Use of stainless steel capillaries instead of fused silica capillary tubes.
6. The option of using a single oven connected to a selector valve connected to individual vials.

These main improvements compared to the original patent application (Steen-Larsen, 2016) were implemented with the following operations in mind: (1) the purpose of the vacuum pump is to create a small vacuum in the vials' headspace, which reverses the flow of the water in the capillaries out of each oven and back into the vials. The benefit of this is that water is immediately removed from the capillary and the oven dries out immediately, minimizing cross-contamination of the samples and build-up of water inside the oven. (2) A custom humidity sensor probe is installed in the tube where the vapor is flowing to the analyser and internally looped to the primary MFC to control the humidity level. This is necessary because of the potential for a slowly decreasing trend of humidity during long injection time (several hours). The decrease in injection performance during long runs is attributed to the build-up of salt deposits inside the capillary during evaporation (further discussed in Section 4.3). (3) The secondary MFC allows for a second dry air stream to be mixed into the flow of vapor from the oven at a higher flow rate than the primary MFC and without influencing the production of vapor in the oven. This way, the vapor generation module can generate humidity levels at a much lower level compared to using only mixing in the oven setup and can also generate vapor with a higher flow rate. (4) The dual valve pressure controller flow meter installed to regulate the pressure in the vials' headspace is chosen to ensure that the pressure can both be increased and decreased. (5) As discussed in Section 4.3 one of the main issues with the operation of a flash evaporator of this type is clogging of the capillaries. We observed that the use of stainless steel capillaries reduced the frequency of clogging compared to when using fused silica capillaries. (6) Instead of having individual oven and valve circuits for each sample vial we installed a selector valve similar to Jones et al. (2017) for the purpose of cost optimization. Unfortunately, the use of a selector valve comes at the cost of increased memory effect between samples and hence we opt for a combination of individual oven and valve circuits and the use of a 10-port selector valve. For generating a stream of water vapor from standards we use the individual oven and valve circuits while liquid samples are measured using the selector valve and single oven circuit.

## 2.2 Technical realization of the vapor generation module

For the technical realization of the vapor generation module, a 2 ml sample vial commonly used in autosamplers for liquid water isotope analysis is used as the water reservoir, as shown in Fig. 2 panel a. A PTFE capillary (1.59 mm outer diameter (OD), 0.150 mm inner diameter (ID)) is passed through a tee assembly and 3.18 mm OD stainless steel tubing (ID > 1.59 mm) toward the bottom of the vial which is kept in place with a Swagelok UltraTorr fitting. The PTFE capillary is sealed only at the very top of the tee assembly with a PTFE ferrule and a PTFE nut to minimize the deformation of the PTFE capillary. The pressure inside the tee assembly is equal to the pressure in the vial headspace and can be precisely controlled with a combination of a manual pressure regulator (model 8286, Parker) and an electronic dual valve pressure controller (PCD-5PISG-D-SV, ALICAT), which includes an advanced PID control of the pressure. Any change of the pressure in the headspace (positive or negative) will produce a flow of water through the PTFE capillary. In this study, the headspace pressure was regulated between 0.5 and 3.5 PSI.

195 The PTFE capillary is connected with a 1.59 mm PEEK union to a 100 mm long stainless-steel capillary with 0.127 mm ID (T10C5, VICI) and fitted into one end of a stainless steel tee (ZT1M, VICI) which is kept in place over a 200W heating element (860-6912, RS-PRO) with a custom aluminium assembly, as shown in Fig 2 panel b. The stainless-steel tee and the heating block are placed into an aluminium diecast enclosure (Hammond Mfg.) and thermally insulated with machinable glass ceramic rods (Cornic) and wrapped in fiberglass liner. As mentioned before, in this study we used a 4 elements version of the oven,  
200 but the module is highly scalable in terms of number of heated tee units.

The water vapor produced in the oven is routed toward the output of the system through the stainless steel valve manifold and a copper tube where the vapor is measured using a custom humidity sensor probe to monitor the temperature and the humidity of the outflow gas (AD22100STZ, Analog Device and HIH-4000-004, Honeywell inside a SS-400-3-4TTF tee, Swagelok). The humidity sensor probe is used to control the flow rate of the first MFC (GFC17A, 0-500 ml/min, AALBORG) with a PID,  
205 to keep a steady humidity level at the output of the vapor generation module during long injections. A data acquisition module (USB-6001, National Instrument) was used to control valves and MFCs. The control software was written in LabView 16.

### 2.2.1 Continuous injections of different samples

In a subsequent modification of the vapor generation module, we used a single oven connected with the stainless-steel capillary to a multiport selector (C25-3180EUHA, VICI) to inject samples from the different vial holders continuously, without needing  
210 to switch the oven. This second modification was introduced to analyse samples of unknown isotopic composition in a similar fashion to continuous flow analysis of ice cores. The possibility of changing between water sources without affecting the water vapor production enables both measurements of individual unknown samples and the possibility of running long stability tests (>24h) since switching between samples containing the same standard occur seamlessly.

### 2.3 Standards and samples used for testing the vapor generation module

215 A wide range of isotopic values were used to test the calibration module, spanning approximately the VSMOW-SLAP2 range (Coplen, 1988; Gonfiantini, 1978). Laboratory standards with known isotopic composition for this study were provided by Laboratoire des Sciences du Climat et de l'Environnement, Centre for Ice and Climate at the Niels Bohr Institute, and the Stable Isotope Laboratory at the Institute of Arctic and Alpine Research, University of Colorado. The  $\Delta^{17}\text{O}$  values of the standards provided by the Stable Isotope Laboratory were provided by  $\Delta^*$ IsoLab, University of Washington. An overview of  
220 all the standards used are listed in supplementary material Table S1, while Table 1 shows the most frequently used standards for analysing stability and memory effects. Moreover, four more samples (Supplementary material Table S2) were prepared at the University of Bergen by weighting precise amounts of SW and WW standards (Table S1) with an uncertainty of 0.01g to test the reproducibility of the  $\Delta^{17}\text{O}$  measurements. For these four samples, the uncertainty associated to  $\Delta^{17}\text{O}$  value is assumed to be half the maximum span obtained by mixing SW +/- 0.01g with WW +/- 0.01g, which is approximately 0.013  
225 ‰ (13 per meg).

## 2.4 Isotopic water vapor analyzer

Most of the laboratory characterization tests for the vapor generation module were performed using a L2140-i Cavity Ring-Down Spectroscopy (CRDS) water isotope analyser by Picarro (s.n. HKDS2156). In one occasion, to identify the source of measurement noise, the analyser was run simultaneously with another Picarro L2140-i (s.n. HKDS2092). The HKDS2092 model was also used for the field activity mentioned in this work (see Section 3.4). Chronologically, the HKDS2092 is the oldest manufactured instrument that was used while HKDS2156 is the most recent one. Both the HKDS2092 and the HKDS2156 have an acquisition rate of  $\sim 1$  Hz, which is a typical value for this type of instrument. The reader is referred to previous studies for detailed description of the technology and performances of such analyzers (e.g. Steig et al., 2014).

## 3 Results

### 3.1 Long term injection and long-term stability

To demonstrate the long-term stability of the vapor generation system, a 92 hour test was performed during the fall 2022, from Oct 10<sup>th</sup> 16:20 to Oct 14<sup>th</sup> 12:25 (LST). During the test, a 2 ml aliquot of SP standard (1 vial) and 26 ml aliquot of BER (13 vials) were injected using the four available vial holders and routed to a single oven using a multiport selector. The consumption rate was  $\sim 1.5 \mu\text{l}/\text{min}$ . To prevent contamination between SP and BER standards, the first holder was used only for SP standards while the remaining three were cycled every 24 hours using fresh BER standards. Sequence, timing and relevant statistics of the injections are reported in supplement material Table S3. The PID control loop was set to 17300 ppmv and the final averaged humidity recorded was  $17229 \pm 340$  ppmv with no observable trend, as shown in Fig. 3 panel a. For  $\sim 80\%$  of injections the standard deviation of H<sub>2</sub>O is between 113 - 353 ppmv, yielding an RSD in the range 0.7 - 2%. There is apparently no pattern in the variability of H<sub>2</sub>O signal among the different holders. At the working humidity between 15000 and 20000 ppmv the humidity-isotope response curve is almost flat for  $\delta^{17}\text{O}$  and  $\delta^{18}\text{O}$ . The temporal evolution in the humidity,  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$ ,  $\delta\text{D}$ , d-excess, and  $\Delta^{17}\text{O}$  are shown in supplementary material Fig. S1. A small dependency was observed between H<sub>2</sub>O and  $\delta\text{D}$ , as reported in supplementary material Fig. S2, but we do not correct for this.

The Allan Deviation plots in Fig. 3 panel b and c (solid lines) show a constant improvement of the two-sample variance, consistent with a nearly flat noise spectrum (white noise). For ideal white noise, a slope of  $-0.5 \sigma_{\text{Allan}}/\tau$  is expected. Observed slopes between averaging time 1 to  $10^4$  seconds are -0.42, -0.33, -0.31 and -0.38 ‰/s for  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$ ,  $\delta\text{D}$  and d-excess,



respectively, and  $-0.42$  ppm/s for  $\Delta^{17}\text{O}$ . A slope smaller than the one predicted for pure white noise implies that the non-flat spectral characteristic of the measurement noise can be due to the instability of the analyser as well as from the instability of the vapor generation module. We note that for some ranges of averaging times, the measurement noise can be seen to be pure white noise. For example, white noise is observed for d-excess and  $\Delta^{17}\text{O}$  in the ranges 1 to  $10^2$  and 1 to  $10^1$ , and again in the ranges  $10^3$  to  $2 \cdot 10^4$  and  $2 \cdot 10^2$  to  $10^4$  seconds, respectively. In the range  $\sim 10^2$  to  $10^3$  and  $\sim 10^1$  to  $2 \cdot 10^2$  seconds for respectively d-excess and  $\Delta^{17}\text{O}$  it can be noted that instabilities of the analyser exist, which has consequences for the optimal choice of averaging time when weighing precision up against averaging time. It is worth noting that the Allan Deviation plot presented in this study shows better isotopic analyser performances than previously published in other studies (e.g. Sturm and Knohl, 2010; Steig et al., 2014; Leroy-Dos Santos et al., 2021; Aemisegger et al., 2012), yielding 0.004, 0.005, 0.01, 0.04 ‰  $\sigma_{\text{Allan}}$  for  $10^4$  seconds averaging time for  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$ ,  $\delta\text{D}$ , d-excess respectively and 2 per meg  $\sigma_{\text{Allan}}$  for  $10^4$  seconds averaging time for  $\Delta^{17}\text{O}$ . Albeit for  $10^3$  seconds, we show similar  $\Delta^{17}\text{O}$   $\sigma_{\text{Allan}}$  as Davidge et al. (2022). We argue that the apparent better performance to not only be dependent on the isotope analyser quality, even though instrumental performance improved with the introduction of the Picarro L2140-i series, but dependent on the management of memory effect during Allan Deviation tests, such as priming the system for up to 12 hours using the same standard. As mentioned above, the 92-hour test started with a large positive isotopic step change in the water vapor source ( $\sim 55\%$  for  $\delta^{18}\text{O}$ ) and the following 16 hours were removed from the Allan Deviation analysis to minimize the memory effect. If the extra 16 hours of data is used to compute the Allan Deviation, the plateau is reached already at  $4 \times 10^3$  s and the  $\sigma_{\text{Allan}}$  is larger (dashed lines in Fig. 3 panel b). Most notably, an apparent drift effect shows up for  $\delta\text{D}$  after an averaging time of  $10^2$  s. Interestingly, the  $\Delta^{17}\text{O}$  quantity seems to be unaffected by this memory effects issue. To test the long-term stability and reproducibility of the Allan Deviation characterization, an independent characterization was carried out 8 months later. The test revealed a similar result as presented in Fig. 3.

### 3.2 Isotope step change and reduced memory effect

Assuming 24 hours of continuous injection of the same water standard are enough to completely remove the memory effect of the previous sample, we show in Fig. 4 the temporal evolution of the SP-BER normalized isotopic step change curve for fractions of the normalized target value larger than 0.90. For comparison, we ran a similar step-change test using the liquid injection mode of the Picarro L2140-i instrument ( $^{17}\text{O}$ , high precision mode) coupled to the A0235 autosampler and A0211 vaporizer. For the liquid injections test the standards were analysed as follows: 2 vials of SP (25 injection each) followed by 9 vials of BER (25 injection each), for a total number of 275 injections and a running time of  $\sim 41$  hours. Results clearly show that the vapor generation module is faster than the vaporizer using the autosampler system for reaching the target value after the step change. For instance, using the vapor generation system the 0.995 level is reached after 24, 23 and 47 minutes for  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$  and  $\delta\text{D}$ , respectively. The same level is reached with the vaporizer using the autosampler system after 54, 54 and 152 minutes. However, the liquid injections with the vaporizer using an autosampler are evenly spaced by cleaning cycles of the vaporizer, robotic arm movements, etc. All such operations require a considerable amount of time, which is mentioned

hereafter as dead time. The large difference in memory effect is discussed further in section 4.4. Fig. 4 shows that timings for calibration system and vaporizer using autosampler are comparable for  $\delta^{17}\text{O}$  and  $\delta^{18}\text{O}$  when dead time is ruled out. However, when theoretically removing the dead time, the vaporizer using the autosampler requires  $\sim 77$  minutes to reach the 0.995 level of target value for  $\delta\text{D}$ , which is still considerably longer by about  $\sim 60\%$  than the time required by the presented vapor generation system.

### 295 3.3 Short-term stability

The vapor generation module was tested by injecting the BER standard at 12 different humidity levels with injection times ranging from 3.5 to 8.7 hours (see Fig. 5 and supplement material SM table S4).

Such humidity levels cover almost completely the mixing ratio variability of the Earth's lower troposphere, with the exception of very dry regions like Antarctica (Casado et al., 2016), and warm-wet regions like tropical areas (e.g. Laskar et al., 2014). The stability of water vapor signal was evaluated with three metrics for each level:

**Metric 1: The spread-variability of H<sub>2</sub>O signal.** Results in Fig. 5 show that the 1-second standard deviation ranges between 18 and 110 ppmv and is independent of the humidity level. If a smaller variability is required, the vapor generation module can be locked to a humidity level and a second dry airflow can be used to dilute the water vapor concentration at TEE2 (Figure 1). The application study in Section 3.4 reports an example of usage of the second stage mixing and the associated 1-second standard deviation between humidity levels 500 - 3500 ppmv.

**Metric 2: The short-term trend of the H<sub>2</sub>O signal ( $\Delta\text{H}_2\text{O}/\Delta t$ ).** Results in Fig. 5 show that the trend, evaluated between 3.5 - 8.7 hours is limited in a narrow variation range, from -24 ppmv/h to 29 ppmv/h. Positive trends were observed always below 9000 ppmv, while positive and negative trends above 11000 ppmv. A linear fit of the observed trend vs humidity reveals that a trend of  $\sim 0$  ppmv/h is achievable at  $\sim 12500$  ppmv, which can be considered the most stable region of the calibration module in terms of drift of mixing ratio level.

**Metric 3: The overlapping Allan Deviation of  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$ ,  $\delta\text{D}$  and  $\Delta^{17}\text{O}$ .** In general, a significant improvement of the two-sample variance can be observed above 5000 ppmv (Appendix 1 Figure A1). As expected, the largest Allan Deviation with averaging time of 600 seconds is the one measured at 584 ppmv level (0.04, 0.05 and 0.17 ‰ for  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$  and  $\delta\text{D}$ , respectively). Between 5000 and 20000 ppmv, the 600 s Allan Deviation is characterized in general by small variability ( $0.013 \pm 0.002$ ,  $0.014 \pm 0.004$  and  $0.02 \pm 0.01$  ‰ for  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$  and  $\delta\text{D}$ , respectively). For unknown reasons the worst performances in terms of Allan Deviation are observed at 11584 ppmv (0.02, 0.03, and 0.06 ‰ for  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$  and  $\delta\text{D}$ , respectively for 600 s averaging time). This is in contrast with the analysis above, which shows the smallest short-term trend of the H<sub>2</sub>O signal in

the ~12500 ppmv region, which is ~0 ppmv/h. Similar to  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$  and  $\delta\text{D}$ , the overlapping Allan Deviation of  $\Delta^{17}\text{O}$  follows in general the same pattern, as shown in Fig. 6. However, the decrease of performances observed for  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$  and  $\delta\text{D}$  at 11584 ppmv is limited for  $\Delta^{17}\text{O}$ . The optimal working region of the Picarro L2140i coupled to the vapor generation module is  
325 between 14000 and 18000 ppmv.

### 3.4 Application study 1: Humidity - isotope characterization of water vapor analyzer for the lower polar troposphere (WIFVOS)

Obtaining accurate vertically resolved profiles of water vapor isotopic composition is challenging because of the large isotopic (~30‰ for  $\delta^{18}\text{O}$ ) and humidity span (~10 000 ppmv) in the atmospheric column. This is even more extreme in the polar  
330 regions, where humidity can easily be < 1000 ppmv near the ground (e.g. Casado et al., 2016; Wahl et al., 2021; Rozmiarek et al., 2021). Here we show how the calibration system can be successfully used to fully characterize the humidity-isotope response of CRDS water vapor analysers between 500 - 3500 ppm, where commercially available calibration systems notoriously have issues generating stable humidity signal (Ritter et al., 2016; Guilpart et al., 2017). The data of this application study was acquired during the Water vapour Isotopologue Flask sampling for the Validation Of Satellite data (WIFVOS) field  
335 campaign in Sodankylä, Finland, for the characterization of the HKDS2092 analyser used in the field to measure the isotopic composition of water vapor collected with flasks between ground level and ~8000 m ASL. Following the procedure by e.g. Steen-Larsen et al. (2013), the vapor generation module was used to provide a stream of known and constant water vapor isotopic composition at different humidity steps (from ~500 ppm to ~3500 ppmv). Since the characterization is time-consuming, the duration of each step was set to ~15 minutes, and only the last 5 minutes of the signal was used to compute the  
340 humidity-isotope response curve. The response curves were repeated for three different laboratory standards (FL0, FL1, FL2; most enriched to most depleted, see Table S1 in supplementary material). For this application, the second MFC and the second mixing tee (MFC2 and 2<sup>nd</sup> stage mixing in Fig. 1) were used while the humidity feedback and the PID control were not used as the calibration system provided a very stable humidity signal to estimate correction curves for the CRDS analyser at very low humidity, as shown in Fig. 7 Panel a and b. The second mixing tee contributes significantly in producing very small H<sub>2</sub>O  
345 variability for all steps, yielding a minimum and a maximum standard deviation of 6 and 58 ppmv (22 ppmv, on average). The main disadvantage of the second mixing tee is, however, the use of a large amount of dry air to dilute the signal coming from the oven unit (up to 1 l/min). When using the second mixing tee it is important to pay attention to the internal diameter of the tubing as too large back pressure will inhibit injection of water in the oven through the capillary. For extreme dry conditions (< 300 ppmv) a dedicated low humidity calibration system such as the one proposed in Leroy-Dos Santos et al. (2021) should  
350 be adopted.

Interestingly, the CRDS analyser showed slightly different patterns of  $\delta^{18}\text{O}$  for the different standards used and a very different pattern is observed for  $\delta\text{D}$  for the very depleted standard as also reported earlier by Weng et al. (2020). Importantly we note that the precision of the CRDS analyser is not affected by the isotopic composition of the standards, as shown in Fig. 7 panel

c and d. Users of CRDS analysers at very low humidity must be aware of the different humidity-isotope sensitivity for different isotopic composition, which might be due to issues in fitting of the spectra and could be instrument-dependent.

### 3.5 Application study 2: $\Delta^{17}\text{O}$ analysis of liquid samples

The two reference waters SW and WW, with known  $\Delta^{17}\text{O}$  values, were mixed in three different aliquots to obtain three solutions with known  $\Delta^{17}\text{O}$  of 20 ml each (see Table S2 in supplementary material for details on aliquots). The solutions of reference waters were weighted using a laboratory scale with 0.01 g resolution. Half of the maximum span obtained by mixing SW +/- 0.01g with WW +/- 0.01g yields a 13 per meg variation of the final  $\Delta^{17}\text{O}$  value, which can be considered a conservative estimate of the sample uncertainty due to weighting. A typical analysis run consisted of injecting the two standard waters (SW and WW) followed by injections of the two solutions (~15000 ppmv). Each injection lasted for 3 hours, and a typical run consisted of 7 - 12 injections, for a total time of approximately 21 - 36 hours per run. For both reference waters and solutions, the first 2 hours of each injection were discarded to limit the memory effect introduced by the injection of the previous sample. A linear calibration was performed by using reference SW and WW's value for  $\delta^{18}\text{O}$  and  $\delta^{17}\text{O}$ . Since the standards were measured from 2 to 4 times for each measurement session, and the solutions were measured on different days, we applied both an average and independent calibration. The average calibration factors for the former were estimated by averaging the raw observations of the standards injected for all the runs. While, the independent calibration factors were calculated for each couple of reference standards and then applied only to the following couple of solutions (2 standards followed by 2 samples). The results of the experiment are reported in Table 2.

Despite the analysis was performed on 3 different samples only, Table 2 clearly shows that the reproducibility of sample measurement is very high: 4 and 5 per meg on average for average and independent calibration, respectively. Such reproducibility is comparable to precision achieved with IRMS (e.g. Barkan and Luz, 2005; Steig et al., 2014) and to the total error obtained within the latest development in continuous flow analysis of ice cores (Davidge et al., 2022), but better than analysis performed with optimal settings of vaporizer and autosampler from Picarro, which is 8 per meg following Schauer et al. (2016). The root mean squared error is 8 per meg and in general the measured  $\Delta^{17}\text{O}$  is 5-6 per meg higher than the expected values, but within the expected uncertainty due to the weighting uncertainty, which could produce an off set of up to 13 per meg. Memory effect was estimated to have a limited impact on  $\Delta^{17}\text{O}$ , as further discussed in Section 4.4, and we argue the systematic difference can be due to measurement error of the weighing scale, degraded quality of the reference waters due to long storage or biases in assigned  $\Delta^{17}\text{O}$ -values of reference waters. Despite the small bias, this analysis represents a line of evidence that the calibration module can successfully be used to analyse  $\Delta^{17}\text{O}$  in liquid water given its ability to measure a sample potentially for extended time.

#### 4.1 Drivers of measurement noise

To investigate the origin of the water isotope measurement noise we placed two Picarro L2140 instruments (HKDS2092 and HKDS2156) in parallel in a configuration that they measured the same output generated by the water vapor generator module at 14500 ppmv level for 10 hours with BER standard. A 1 m length 3.125 mm OD copper tube coming from the water vapor generation module was connected to a stainless steel tee (SS-200-3, Swagelok). Two nearly identical 0.75 m 3.125 mm OD copper tube segments were connected to the tee, carrying the sample gas to each analyser. The instrument connection at the gas inlet was reproduced as similarly as possible for both instruments, to achieve the same gas transport resistance. Both instruments were connected to the inlet line in open split mode and each instrument was pulling the gas sample at its nominal flow rate (~40 sccm/min). The water vapor generation module was configured to keep at least a flow rate of 100 sccm/min at its output, to compensate for the requirements of two instruments measuring at the same time. The excess gas sample was released into the room air.

The newer HKDS2156 instrument is performing better than the HKDS2092 in terms of noise and precision, as shown in Fig. 8 panel A. In the figure “bumps” in the Allan Deviation plot for both instruments are seen at different timings for different isotopes and with differences, which are instrument-dependent. This supports the hypothesis that the main driver of the noise in  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$  and  $\delta\text{D}$  is related to the analysers’ characteristics and not to the vapor generation module. A simple correlation analysis of the synchronized and resampled (1 Hz)  $\text{H}_2\text{O}$  signal between the two analysers yielded  $r = 0.91$ . An insignificant correlation ( $<0.01$ ) was observed for  $\delta^{18}\text{O}$ , showing that even though  $\text{H}_2\text{O}$  variability due to vapor generator fluctuations is captured by the two instruments, no co-varying isotopic composition change can be detected by the two instruments during the test (for completeness,  $\delta^{17}\text{O}$  and  $\delta\text{D}$  measured with the two analysers have correlation  $<0.01$  and  $\sim 0.01$ , respectively). Since the variability of the isotopic composition of the signal is independent of the mixing ratio variability, the main sources of isotope variability in the measurement must be investigated in the analyser performances. The isotope data recorded at ~1 Hz by both analysers do not correlate with any of the following parameters recorded in the log file of the analyser: cavity temperature, cavity pressure, internal computer temperature referenced as DAS temperature, warmbox temperature. However, a wavelet analysis reveals significant power in periods with 10 to 60 minutes periodicity in  $\delta^{18}\text{O}$  and cavity temperature. When performing a wavelet coherence analysis (Grinsted et al., 2004) we find a significant in-phase coherence between  $\delta^{18}\text{O}$  and cavity temperature for periods in the range of 10 to 60 minutes for the HKDS2092 and in the range 10 to 30 minutes for the HKDS2156 instrument (See Appendix Figure B2). When a low-pass Butterworth filter is applied to the data, as shown in Figure 8 panel B we detect a significant correlation between  $\delta^{18}\text{O}$  and cavity temperature. For instance, a Butterworth low-pass filter with a cut-off of periods less than 600 s yielded  $r=0.68$  for HKDS2092 and  $r=0.59$  for HKDS2156. Correlations also increase for  $\delta^{17}\text{O}$  and  $\delta\text{D}$ , but not as much as for  $\delta^{18}\text{O}$  (e.g., with the same time window, the correlation between  $\delta^{17}\text{O}$  and cavity temperature is only 0.31 for HKDS2156). It is important to note that the cavity temperature control is precisely tuned

using a PID loop and it is not accessible at user level. We note that a similar “bump” can be seen in Allan Deviation analyses presented in previous studies (e.g. Leroy-Dos Santos et al., 2021; Steig et al., 2014) and we hence speculate if the observed significant periodicity in cavity temperature in the range 12 to 30 minutes is consistent across instruments. Should this hypothesis be correct, it would imply that  $\delta^{18}\text{O}$  precision for measurements averaged between  $10^2$  and  $10^3$  seconds could be improved by up to a factor 2 if the PID driven cavity-temperature cycles were to be dampened. We also further notice that this increase in Allan Deviation occurs at similar integration times as used for liquid measurements, which makes it even more important to improve on.

## 4.2 Isotope calibration pulses

To test the repeatability of the calibration system for producing calibration cycles suitable for water vapor analysis, the standards BER and SP were used to autonomously produce 100-minute pulse trains spaced every 3 hours for 48 hours continuously. The test was performed with the multiple oven configuration using two different lines to stream from the two different standard 2 ml vials. The mixing ratio level was kept constant at 10 000 ppmv in order to have enough water inside the vials to allow repeated injections for 48 hours. The isotopic composition variability of the injected water for each pulse centered around the mean, calculated as the average  $\pm 1$  standard deviation of the last 5 minutes of the  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$ ,  $\delta\text{D}$ , d-excess and  $\Delta^{17}\text{O}$  signals, is reported in Fig. 9.

The calibration system successfully injected both SP and BER standards autonomously, reporting no failed injections for 48 hours. No large change in isotopic composition of the injected standards were observed for 48 hours for the multiple oven configuration. However, as can be observed in Fig. 9 there appears to be slight enrichment in the two standards throughout the experiment as indicated by the decrease of the d-excess value ( $\sim -0.6$  ‰ for both standards).. This drift (increase in delta values) of the measurements could be a result of instrumental drift, but we understand the enrichment to be a result of the long exposure of the liquid sample to the dry push gas inside the vial leading to evaporation and hence enrichment. The dry push gas from the headspace of the vial being replaced after each injection when stopping the flow of water into the capillary. This observed drift means that whenever a sample in a vial will be measured for a continuous long period of time it is important to use a relative larger sample holder to limit the relative influence of evaporation. The variability in the mean of the last 5 minutes of the injection is relatively small, with standard errors ranging in the order of 0.01‰, 0.01‰, 0.02‰, 0.1‰ and 11 per meg for  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$ ,  $\delta\text{D}$ , d-excess and  $\Delta^{17}\text{O}$  respectively. To illustrate the repeatability of the injections the standard deviation of the mean values from the individual pulses is 0.02‰, 0.02‰, 0.09‰ and 0.13‰ for  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$ ,  $\delta\text{D}$ , d-excess respectively when linearly correcting for the long-term drift likely induced by evaporation.  $\Delta^{17}\text{O}$  shows no significant change with time and the standard deviation of the mean values from the individual pulses is 16 per meg.

This experiment illustrates the potential of the system to be used as a calibration unit for atmospheric water vapor isotope measurements in the field. As we will discuss below the most often occurring issue when using the vapor generation module

was clogging of the capillary providing water to the flash evaporator oven. The operator of the system for field calibration of water vapor isotope measurements therefore needs to use relatively clean (such as milli-Q water) standards to allow for extended operation. As illustrated in the long-term stability experiment in Fig. 3 we have carried out a successful ~90 hours long injection of a single standard. We have used the calibration system in the laboratory and during field campaigns for about 455 2 years now and found that a stable performance of the vapor generation module is dependent on using clean standards. When using in-house generated standards consisting of a mixture of melted Greenland snow and milli-Q water from Bermuda we have successfully operated the vapor generation module daily (roughly 1-3 hours every day) in the laboratory for more than 6 months without changing the capillaries.

### 4.3 Capillary issues

460 To control the flow of water into the oven as precisely as possible it is beneficial to use a capillary with a small internal diameter between 50um and 350um. However, as a consequence of the flash evaporation at the tip of the capillary inside the oven residue from dissolved and non-dissolved impurities in the water is building up ultimately leading to clogging of the capillary. Typical signs of clogging are a gradual decrease in humidity and enhanced variability in the humidity, which occur within a few days of operation when using non-clean standards. Following Gkinis et al. (2011) we started out using a silica 465 capillary but discovered that using a stainless steel capillary (T10C5, VICI) resulted in enhanced performance in terms of length of operation before signs of clogging appeared. We also observed that using a stainless steel capillary had the advantage that it could be placed the same way every time, while due to the flexibility of the silica capillary it occurred that the capillary would touch the nut of the oven leading to a non-uniform heating at the tip. Such cases of non-uniform heating were often seen as increased variability in the generated humidity. We do not have an explanation for why the stainless steel capillary was 470 performing better. From experience we observed that using a capillary with an ID of 127 um created the overall best performance. Once a capillary was clogged, we had partial success to unclog it by placing it in an ultrasonic bath with deionized water. We were able to extend the life time of the clogged capillaries by cutting the last 2 cm off. As we will discuss in details below, the clogging of the capillary had consequences of changing the memory effect. While our experience using our in-house clean standards shows stable performance by the vapor generation module, we have also used standards, which were 475 provided to us by other labs. In those cases, we observed that the capillary would get clogged more frequently and had to be replaced every 2-4 weeks. To extend the lifetime of the capillaries it is possible to use a larger ID, but this can potentially result in less stable humidity values.

### 4.4 Memory effect

As documented in Section 3.2 memory effects need to be considered, when using the vapor generation module for 480 measurements of samples with a large spread in water isotopic composition. The vapor generation module shows an approximate factor four reduction in memory effect for  $\delta D$  compared to liquid injections using an autosampler and vaporizer. However, in the work-mode applied here, the control software will automatically adjust the dry air dilution to maintain a

targeted humidity setpoint. The consequence of this is that during a build-up of non-dissolved impurities less water will be delivered at the tip of the capillary, and the control software will reduce the flow of dry air. Less water and air molecules will therefore flow through the system leading to a reduction in removal of water molecules from the previous sample. An example of such situation is illustrated in supplementary material Fig. S3 for a similar pulse train of standard injections as discussed in Section 4.2 with an approximate jump of 55‰/435‰ in  $\delta^{18}\text{O}/\delta\text{D}$  obtained by injecting the BER and SP standards. We do not know of similar published tests with other types of vapor generation modules, but we expect that similar variability in memory effect must also be present for other modules. Our presented example therefore stands as a lesson in the need for quantifying and tracking the performance of every aspect when measuring standards and unknown samples. When using the vapor generation module in automatic measurement mode, one must therefore characterize the memory effect of the setup as a function of dilution flow rate and have the control system log the flow rate for post memory correction of the sample and standard measurement.

The difference in memory effect for the individual isotopes as documented in Fig. 4 illustrates the need to reject relatively longer measurement time to obtain accurate  $\delta\text{D}$  measurements compared to  $\delta^{18}\text{O}$ . We speculate that the difference in memory effect between  $\delta\text{D}$  and  $\delta^{18}\text{O}$  originates from the difference in polarity of the  $\text{HD}^{16}\text{O}$  and  $\text{H}_2^{18}\text{O}$  molecules with the  $\text{HD}^{16}\text{O}$  adhering relatively stronger to the sides of the tubing. This difference in memory effect of  $\delta^{18}\text{O}$  compared to  $\delta\text{D}$  is not only important for obtaining the most accurate isotope values, but also means that care needs to be taken when calculating the d-excess. Interesting, the memory effect for  $\delta^{18}\text{O}$  and  $\delta^{17}\text{O}$  is nearly identical (e.g.  $\tau_{95} = 335$  and  $333$  seconds for  $\delta^{18}\text{O}$  and  $\delta^{17}\text{O}$ , respectively). Due to the relatively high measurement uncertainty (e.g.  $\sigma_{\text{Allan}} = 9$  per meg @ 15 minutes) and relatively small changes in  $\Delta^{17}\text{O}$  observed in natural waters ( $\sim 90$  per meg), it is not the memory effect, which is the limiting factor influencing the  $\Delta^{17}\text{O}$  measurements. As documented in Fig. 10 showing the memory effect for a  $\Delta^{17}\text{O}$  step change of approximately 90 per meg, already within the first hour of measurements the memory effect is producing an error that is  $\sim$ five times smaller than the analytical error. Hence, the vapor generation module is highly capable of  $\Delta^{17}\text{O}$  measurements as it can provide integration times over multiple hours of both standards and samples allowing optimal treatment of memory effects and measurement noise to be reduced to a minimum.

#### 4.5 Potential future updates

We developed the vapor generation module system with 4 ovens allowing 4 individual vials to be measured without interference from an operator. However, by connecting one of the ovens to a 10-port selector valve we were able to run the system for liquid measurements using 3 known standards and 10 unknown samples. We are now in the process of setting up the system for a standard daily operating procedure measuring  $\Delta^{17}\text{O}$  of ice core samples. To increase further throughput by reducing the memory effect, one could also configure the N-oven system to initiate the vapor generation of the subsequent vial while the previous vial is being measured. It would then be a matter of simply switching to an already existing vapor stream



515 from the next oven in line. We invite readers, who plan to build a similar module to contact us for the latest update on  
measurement procedure and control software.

## 5 Conclusion

The water vapor generation module presented here represents a stand-alone modular system for water vapor isotope  
calibrations in the field and high precision liquid water isotope measurements in the laboratory. The system is completely  
520 scalable from one sample/standard vial up to N vials. The vapor generation module is designed to be connected directly with  
a water vapor isotope analyser without the need for additional auxiliary systems. There are several advantages of the system  
compared to existing systems for vapor calibration and liquid sample measurements for water stable isotopes, most notably  
the possibility of calibrating using several standards, the high dynamic range of humidity generation, significant reduction in  
memory effect, and the possibility to, in principle, measure indefinitely the same sample.

525 We have used the vapor generation module to characterize the performance of two water isotope analysers, and documented  
that a key driver of the measurement noise for averaging times between 10 minutes and 1 hour is driven by temperature  
fluctuations of the optical cavity inside the analyzer. This result provides guidance on optimal measurement integration times  
as well as points to the need for stabilizing the cavity temperature on these time scales. We argue that previously published  
increases in Allan Deviation for longer averaging times could be a result of memory effects and not only driven by instrumental  
530 drifts as it is often interpreted. We document Allan Deviation of the water vapor isotope analyser yielding 0.004, 0.005, 0.01,  
0.04 ‰  $\sigma_{\text{Allan}}$  for  $10^4$  seconds averaging time for  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$ ,  $\delta\text{D}$ , d-excess respectively and 2 per meg  $\sigma_{\text{Allan}}$  for  $10^4$  seconds  
averaging time for  $\Delta^{17}\text{O}$ .

Despite the memory effect of the vapor generation module being respectively 2 and 3 times smaller compared to injections  
using an autosampler for  $\delta^{18}\text{O}/\delta^{17}\text{O}$  and  $\delta\text{D}$ , it is still possible to detect the memory effect after more than ~20 hours, thanks  
535 to the high measurement precision on the instrument. This result indicates that for achieving measurements with very low  
uncertainty as for example needed for ice core analysis of million-year-old ice, dedicated efforts on developing measurements  
systems with minimal memory effect is needed. We find however, that measurements of  $\Delta^{17}\text{O}$  is limited by the integration  
time of the vapor measurements and to a lesser extend the memory effect. By measuring an unknown liquid sample for  $\Delta^{17}\text{O}$   
for a three-hour period (rejecting the first two hours due to memory effect) we document an average standard deviation of 4  
540 per meg for  $\Delta^{17}\text{O}$  and an average standard error (95 % confidence limit) of 5 per meg.

We hypothesized that the measurement uncertainty using laser spectroscopy instruments would increase for more depleted  
values due to the lower number of heavy water isotopologues. Using standards spanning of 55‰/435‰ in  $\delta^{18}\text{O}/\delta\text{D}$  we do  
not find any evidence that measuring more depleted values results in higher uncertainty.

Using sufficiently clean water we have been able to continuously measure a constant vapor stream from a single standard over  
545 a period of more than 90 hours. This documents the feasibility of using the vapor generation module as an autonomous field

calibration system. The PID control system ensuring stable humidity levels along with the large range of possible humidity levels make the vapor generation module truly versatile both in the field and in the laboratory.

550

## 555 **6 Appendices**

### **Appendix A: Stability at different humidity levels**

### **Appendix B: Squared Wavelet Coherence analysis between $\delta^{18}\text{O}$ and cavity temperature**

#### **Author Contributions**

560 HCSL conceptualizes this study. HCSL and DZ carried out the development of the methodology and investigation. DZ led with HCSL the formal analysis. DZ carried out the visualization. DZ carried out data curation. HCSL and DZ wrote the original draft, edited, and reviewed the submitted version. HCSL acquired funding for this study and administrated the project.

#### **Competing Interests**

The authors declare that they have no conflict of interest.

## 565 **Acknowledgements**

This work has received funding from the European Research Council (ERC) under the European Union's Horizon 2020 research and innovation program: Starting Grant SNOWISO (Grant Agreement no. 759526).

We are grateful to Laboratoire des Sciences du Climat et de l'Environnement, Centre for Ice and Climate at the Niels Bohr Institute, and the Stable Isotope Laboratory at the Institute of Arctic and Alpine Research, University of Colorado for providing 570 samples of their internal standards for use in this study. The  $\Delta^{17}\text{O}$  values of the standards provided by the Stable Isotope Laboratory were provided by  $\Delta^*\text{IsoLab}$ , University of Washington. DZ acknowledges funding from the European Union's

Horizon 2020 Research and Innovation program under Grant 821868 and from the European Space Agency under EO science for society permanently open call Grant 4000134119/21/I-DT-Ir. HCSL acknowledges funding from the Research Council of Norway under Grant 325681 Isotopic Transfer Rates During Water Phase Changes – iTRANSFER. We are grateful for the many who have provided input to earlier versions of the prototype of the vapor generation module used during SNOWISO field campaigns in Greenland. We thank Picarro Inc. for the instrument support making the instrument comparison analysis possible. We thank 6 reviewers for providing insightful comments, which have greatly improved the paper.

## References

- Aemisegger, F., Sturm, P., Graf, P., Sodemann, H., Pfahl, S., Knohl, A., and Wernli, H.: Measuring variations of delta O-18 and delta H-2 in atmospheric water vapour using two commercial laser-based spectrometers: an instrument characterisation study, *Atmos Meas Tech*, 5, 1491-1511, 10.5194/amt-5-1491-2012, 2012.
- Bailey, A., Noone, D., Berkelhammer, M., Steen-Larsen, H. C., and Sato, P.: The stability and calibration of water vapor isotope ratio measurements during long-term deployments, *Atmos Meas Tech*, 8, 4521-4538, 10.5194/amt-8-4521-2015, 2015.
- Barkan, E. and Luz, B.: High precision measurements of O-17/O-16 and O-18/O-16 ratios in H<sub>2</sub>O, *Rapid Commun Mass Sp*, 19, 3737-3742, 10.1002/rcm.2250, 2005.
- Bastrikov, V., Steen-Larsen, H. C., Masson-Delmotte, V., Gribanov, K., Cattani, O., Jouzel, J., and Zakharov, V.: Continuous measurements of atmospheric water vapour isotopes in western Siberia (Kourovka), *Atmos Meas Tech*, 7, 1763-1776, 10.5194/amt-7-1763-2014, 2014.
- Benetti, M., Steen-Larsen, H. C., Reverdin, G., Sveinbjornsdottir, A. E., Aloisi, G., Berkelhammer, M. B., Bourles, B., Bourras, D., De Coetlogon, G., Cosgrove, A., Faber, A. K., Grelet, J., Hansen, S. B., Johnson, R., Legoff, H., Martin, N., Peters, A. J., Popp, T. J., Reynaud, T., and Winther, M.: Stable isotopes in the atmospheric marine boundary layer water vapour over the Atlantic Ocean, 2012-2015, *Sci Data*, 4, 10.1038/sdata.2016.128, 2017.
- Bonne, J. L., Masson-Delmotte, V., Cattani, O., Delmotte, M., Risi, C., Sodemann, H., and Steen-Larsen, H. C.: The isotopic composition of water vapour and precipitation in Ivittuut, southern Greenland, *Atmos Chem Phys*, 14, 4419-4439, 10.5194/acp-14-4419-2014, 2014.
- Casado, M., Landais, A., Masson-Delmotte, V., Genthon, C., Kerstel, E., Kassi, S., Arnaud, L., Picard, G., Prie, F., Cattani, O., Steen-Larsen, H. C., Vignon, E., and Cermak, P.: Continuous measurements of isotopic composition of water vapour on the East Antarctic Plateau, *Atmos Chem Phys*, 16, 8521-8538, 10.5194/acp-16-8521-2016, 2016.
- Coplen, T. B.: Normalization of Oxygen and Hydrogen Isotope Data, *Chem Geol*, 72, 293-297, Doi 10.1016/0168-9622(88)90042-5, 1988.
- Craig, H.: Isotopic Variations in Meteoric Waters, *Science*, 133, 1702-&, DOI 10.1126/science.133.3465.1702, 1961.
- Craig, H. and Gordon, L. I.: Deuterium and oxygen 18 variations in the ocean and the marine atmosphere, *Stable Isotopes in Oceanographic Studies and Paleotemperatures*, Consiglio Nazionale delle Ricerche, Laboratorio de Geologia Nucleare Pisa, 9-130 pp.1965.
- Dansgaard, W.: Stable Isotopes in Precipitation, *Tellus*, 16, 436-468, 1964.
- Davidge, L., Steig, E. J., and Schauer, A. J.: Improving continuous-flow analysis of triple oxygen isotopes in ice cores: insights from replicate measurements, *Atmos Meas Tech*, 15, 7337-7351, 10.5194/amt-15-7337-2022, 2022.
- Ellehoj, M. D., Steen-Larsen, H. C., Johnsen, S. J., and Madsen, M. B.: Ice-vapor equilibrium fractionation factor of hydrogen and oxygen isotopes: Experimental investigations and implications for stable water isotope studies, *Rapid Commun Mass Sp*, 27, 2149-2158, 10.1002/rcm.6668, 2013.
- Galewsky, J., Steen-Larsen, H. C., Field, R. D., Worden, J., Risi, C., and Schneider, M.: Stable isotopes in atmospheric water vapor and applications to the hydrologic cycle, *Rev Geophys*, 54, 809-865, 10.1002/2015rg000512, 2016.
- Gkinis, V., Popp, T. J., Blunier, T., Bigler, M., Schupbach, S., Kettner, E., and Johnsen, S. J.: Water isotopic ratios from a continuously melted ice core sample, *Atmos Meas Tech*, 4, 2531-2542, 10.5194/amt-4-2531-2011, 2011.
- Gonfiantini, R.: Standards for Stable Isotope Measurements in Natural Compounds, *Nature*, 271, 534-536, DOI 10.1038/271534a0, 1978.
- Grinsted, A., Moore, J. C., and Jevrejeva, S.: Application of the cross wavelet transform and wavelet coherence to geophysical time series, *Nonlin. Processes Geophys.*, 11, 561-566, 10.5194/npg-11-561-2004, 2004.
- Guilpart, E., Vimeux, F., Evan, S., Brioude, J., Metzger, J. M., Barthe, C., Risi, C., and Cattani, O.: The isotopic composition of near-surface water vapor at the Mado observatory (Reunion Island, southwestern Indian Ocean) documents the controls of the humidity of the subtropical troposphere, *J Geophys Res-Atmos*, 122, 9628-9650, 10.1002/2017jd026791, 2017.
- Hutchings, J. A. and Konecky, B. L.: Optimization of a Picarro L2140-i cavity ring-down spectrometer for routine measurement of triple oxygen isotope ratios in meteoric waters, *Atmos Meas Tech*, 16, 1663-1682, 10.5194/amt-16-1663-2023, 2023.

- 620 Iannone, R. Q., Romanini, D., Kassi, S., Meijer, H. A. J., and Kerstel, E. R. T.: A Microdrop Generator for the Calibration of a Water Vapor Isotope Ratio Spectrometer, *J Atmos Ocean Tech*, 26, 1275-1288, 10.1175/2008jtecha1218.1, 2009.
- Jones, T. R., White, J. C., Steig, E. J., Vaughn, B. H., Morris, V., Gkinis, V., Markle, B. R., and Schoenemann, S. W.: Improved methodologies for continuous-flow analysis of stable water isotopes in ice cores, *Atmos Meas Tech*, 10, 617-632, 10.5194/amt-10-617-2017, 2017.
- 625 Jouzel, J. and Merlivat, L.: Deuterium and O-18 in Precipitation - Modeling of the Isotopic Effects during Snow Formation, *J Geophys Res-Atmos*, 89, 1749-1757, DOI 10.1029/JD089iD07p11749, 1984.
- Kerstel, E.: Modeling the dynamic behavior of a droplet evaporation device for the delivery of isotopically calibrated low-humidity water vapor, *Atmos Meas Tech*, 14, 4657-4667, 10.5194/amt-14-4657-2021, 2021.
- Landais, A., Barkan, E., and Luz, B.: Record of delta O-18 and O-17-excess in ice from Vostok Antarctica during the last 150,000 years, *Geophys Res Lett*, 35, Artn L02709, 10.1029/2007gl032096, 2008.
- 630 Landais, A., Barkan, E., Yakir, D., and Luz, B.: The triple isotopic composition of oxygen in leaf water, *Geochim Cosmochim Ac*, 70, 4105-4115, 10.1016/j.gca.2006.06.1545, 2006.
- Landsberg, J., Romanini, D., and Kerstel, E.: Very high finesse optical-feedback cavity-enhanced absorption spectrometer for low concentration water vapor isotope analyses, *Opt Lett*, 39, 1795-1798, 10.1364/Ol.39.001795, 2014.
- 635 Laskar, A. H., Huang, J. C., Hsu, S. C., Bhattacharya, S. K., Wang, C. H., and Liang, M. C.: Stable isotopic composition of near surface atmospheric water vapor and rain-vapor interaction in Taipei, Taiwan, *J Hydrol*, 519, 2091-2100, 10.1016/j.jhydrol.2014.10.017, 2014.
- Lee, X. H., Sargent, S., Smith, R., and Tanner, B.: In situ measurement of the water vapor O-18/O-16 isotope ratio for atmospheric and ecological applications, *J Atmos Ocean Tech*, 22, 555-565, Doi 10.1175/Jtech1719.1, 2005.
- 640 Leroy-Dos Santos, C., Casado, M., Prie, F., Jossoud, O., Kerstel, E., Farradeche, M., Kassi, S., Fourre, E., and Landais, A.: A dedicated robust instrument for water vapor generation at low humidity for use with a laser water isotope analyzer in cold and dry polar regions, *Atmos Meas Tech*, 14, 2907-2918, 10.5194/amt-14-2907-2021, 2021.
- Luz, B. and Barkan, E.: The isotopic ratios O-17/O-16 and O-18/O-16 in molecular oxygen and their significance in biogeochemistry, *Geochim Cosmochim Ac*, 69, 1099-1110, 10.1016/j.gca.2004.09.001, 2005.
- 645 Merlivat, L. and Jouzel, J.: Global Climatic Interpretation of the Deuterium-Oxygen-18 Relationship for Precipitation, *J Geophys Res-Oceans*, 84, 5029-5033, DOI 10.1029/jc084ic08p05029, 1979.
- Penna, D., Stenni, B., Sanda, M., Wrede, S., Bogaard, T. A., Michellini, M., Fischer, B. M. C., Gobbi, A., Mantese, N., Zuecco, G., Borga, M., Bonazza, M., Sobotkova, M., Cejkova, B., and Wassenaar, L. I.: Technical Note: Evaluation of between-sample memory effects in the analysis of delta H-2 and delta O-18 of water samples measured by laser spectrometers, *Hydrol Earth Syst Sc*, 16, 3925-3933, 10.5194/hess-16-3925-2012, 2012.
- 650 Ritter, F., Steen-Larsen, H. C., Werner, M., Masson-Delmotte, V., Orsi, A., Behrens, M., Birnbaum, G., Freitag, J., Risi, C., and Kipfstuhl, S.: Isotopic exchange on the diurnal scale between near-surface snow and lower atmospheric water vapor at Kohnen station, East Antarctica, *Cryosphere*, 10, 1647-1663, 10.5194/tc-10-1647-2016, 2016.
- Rozmiarek, K. S., Vaughn, B. H., Jones, T. R., Morris, V., Skorski, W. B., Hughes, A. G., Elston, J., Wahl, S., Faber, A. K., and Steen-Larsen, H. C.: An unmanned aerial vehicle sampling platform for atmospheric water vapor isotopes in polar environments, *Atmos Meas Tech*, 14, 7045-7067, 10.5194/amt-14-7045-2021, 2021.
- 655 Schauer, A. J., Schoenemann, S. W., and Steig, E. J.: Routine high-precision analysis of triple water-isotope ratios using cavity ring-down spectroscopy, *Rapid Commun Mass Sp*, 30, 2059-2069, 10.1002/rcm.7682, 2016.
- Steen-Larsen, H. C.: An Automated Calibration Or Measurement Device Adapted For The Determination Of Water Isotopic Composition Of An Unknown Liquid And Vapor Sample, Associated Automated Measurement Process, European Patent Application, EP3109634A1, 1-23, <https://worldwide.espacenet.com/patent/search/family/054252207/publication/EP3109634A1?q=pn=EP3109634A1>, 2016.
- 660 Steen-Larsen, H. C., Sveinbjornsdottir, A. E., Jonsson, T., Ritter, F., Bonne, J. L., Masson-Delmotte, V., Sodemann, H., Blunier, T., Dahl-Jensen, D., and Vinther, B. M.: Moisture sources and synoptic to seasonal variability of North Atlantic water vapor isotopic composition, *J Geophys Res-Atmos*, 120, 5757-5774, 10.1002/2015jd023234, 2015.
- Steen-Larsen, H. C., Sveinbjornsdottir, A. E., Peters, A. J., Masson-Delmotte, V., Guishard, M. P., Hsiao, G., Jouzel, J., Noone, D., Warren, J. K., and White, J. W. C.: Climatic controls on water vapor deuterium excess in the marine boundary layer of the North Atlantic based on 500 days of in situ, continuous measurements, *Atmos Chem Phys*, 14, 7741-7756, 10.5194/acp-14-7741-2014, 2014.
- 665 Steen-Larsen, H. C., Johnsen, S. J., Masson-Delmotte, V., Stenni, B., Risi, C., Sodemann, H., Balslev-Clausen, D., Blunier, T., Dahl-Jensen, D., Ellehoj, M. D., Falourd, S., Grindsted, A., Gkinis, V., Jouzel, J., Popp, T., Sheldon, S., Simonsen, S. B., Sjolte, J., Steffensen, J. P., Sperlich, P., Sveinbjornsdottir, A. E., Vinther, B. M., and White, J. W. C.: Continuous monitoring of summer surface water vapor isotopic composition above the Greenland Ice Sheet, *Atmos Chem Phys*, 13, 4815-4828, 10.5194/acp-13-4815-2013, 2013.
- 670 Steig, E. J., Gkinis, V., Schauer, A. J., Schoenemann, S. W., Samek, K., Hoffnagle, J., Dennis, K. J., and Tan, S. M.: Calibrated high-precision O-17-excess measurements using cavity ring-down spectroscopy with laser-current-tuned cavity resonance, *Atmos Meas Tech*, 7, 2421-2435, 10.5194/amt-7-2421-2014, 2014.

- 675 Sturm, P. and Knohl, A.: Water vapor delta H-2 and delta O-18 measurements using off-axis integrated cavity output spectroscopy, Atmos Meas Tech, 3, 67-77, DOI 10.5194/amt-3-67-2010, 2010.
- Tremoy, G., Vimeux, F., Cattani, O., Mayaki, S., Souley, I., and Favreau, G.: Measurements of water vapor isotope ratios with wavelength-scanned cavity ring-down spectroscopy technology: new insights and important caveats for deuterium excess measurements in tropical areas in comparison with isotope-ratio mass spectrometry, Rapid Commun Mass Sp, 25, 3469-3480, 10.1002/rcm.5252, 2011.
- 680 van Geldern, R. and Barth, J. A. C.: Optimization of instrument setup and post-run corrections for oxygen and hydrogen stable isotope measurements of water by isotope ratio infrared spectroscopy (IRIS), Limnology and Oceanography: Methods, 10, 1024-1036, <https://doi.org/10.4319/lom.2012.10.1024>, 2012.
- Wahl, S., Steen-Larsen, H. C., Reuder, J., and Horhold, M.: Quantifying the Stable Water Isotopologue Exchange Between the Snow Surface and Lower Atmosphere by Direct Flux Measurements, J Geophys Res-Atmos, 126, 10.1029/2020JD034400, 2021.
- 685 Weng, Y. B., Touzeau, A., and Sodemann, H.: Correcting the impact of the isotope composition on the mixing ratio dependency of water vapour isotope measurements with cavity ring-down spectrometers, Atmos Meas Tech, 13, 3167-3190, 10.5194/amt-13-3167-2020, 2020.
- Zannoni, D., Steen-Larsen, H. C., Peters, A. J., Wahl, S., Sodemann, H., and Sveinbjornsdottir, A. E.: Non-Equilibrium Fractionation Factors for D/H and O-18/O-16 During Oceanic Evaporation in the North-West Atlantic Region, J Geophys Res-Atmos, 127, 10.1029/2022JD037076, 2022.

690 **Tables:**

**Table 1: Standards used for stability and memory effect analysis in this study.**

Name	$\delta D$ (‰)	$\delta^{17}O$ (‰)	$\delta^{18}O$ (‰)	d-excess (‰)	$\Delta^{17}O$ (per meg)
BER (Bermuda water)	-2.10	-0.05	-0.25	4	82
SP (South Pole water)	-435.31	-29.6497	-55.39	8	-11


695 **Table 2: Analysis of  $\Delta^{17}O$  of liquid samples using the vapor generation module. All  $\Delta^{17}O$  values in per meg. Analytical precision is standard error multiplied by Student's t-factor for a 95% confidence limit. \*indicate independent calibrations for each run.**

Sample	Measured $\Delta^{17}O$ ( $\pm 1\sigma$ )	Expected $\Delta^{17}O$	Analytical precision	# replicates (dates Dec 2022)
<b>M20</b>	24 $\pm$ 3 *24 $\pm$ 3	21	3 *2	<b>5</b> (3 on 9 <sup>th</sup> 1 on 11 <sup>th</sup> 1 on 12 <sup>th</sup> )
<b>M50</b>	17 $\pm$ 5 *17 $\pm$ 4	12	6 *5	<b>4</b> (2 on 9 <sup>th</sup> 1 on 11 <sup>th</sup> 1 on 12 <sup>th</sup> )
<b>M85</b>	24 $\pm$ 5 *24 $\pm$ 8	18	5 *8	<b>4</b> (1 on 12 <sup>th</sup> 2 on 13 <sup>th</sup> 1 on 14 <sup>th</sup> )


700

705

Figures:

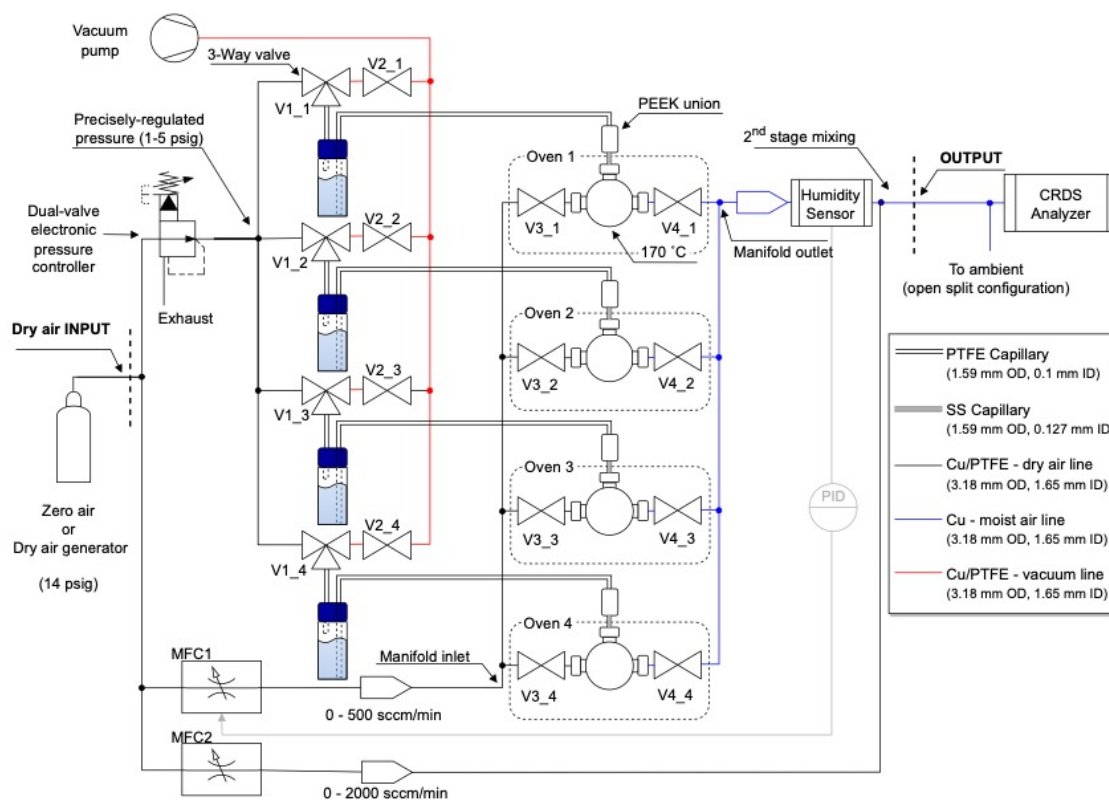


710 **Figure 1:** Sketch of the vapor generation module equipped with multiple ovens. The gas analyser must be connected at the OUTPUT of the vapor generation module in open-split mode to allow the part of the vapor stream that is not going into the Picarro instrument to escape. Pictures of the physical realization of the vapor generation module are shown in the Supplement material Image 1. Reference to product numbers of the labelled components is reported in Supplementary material text T1.

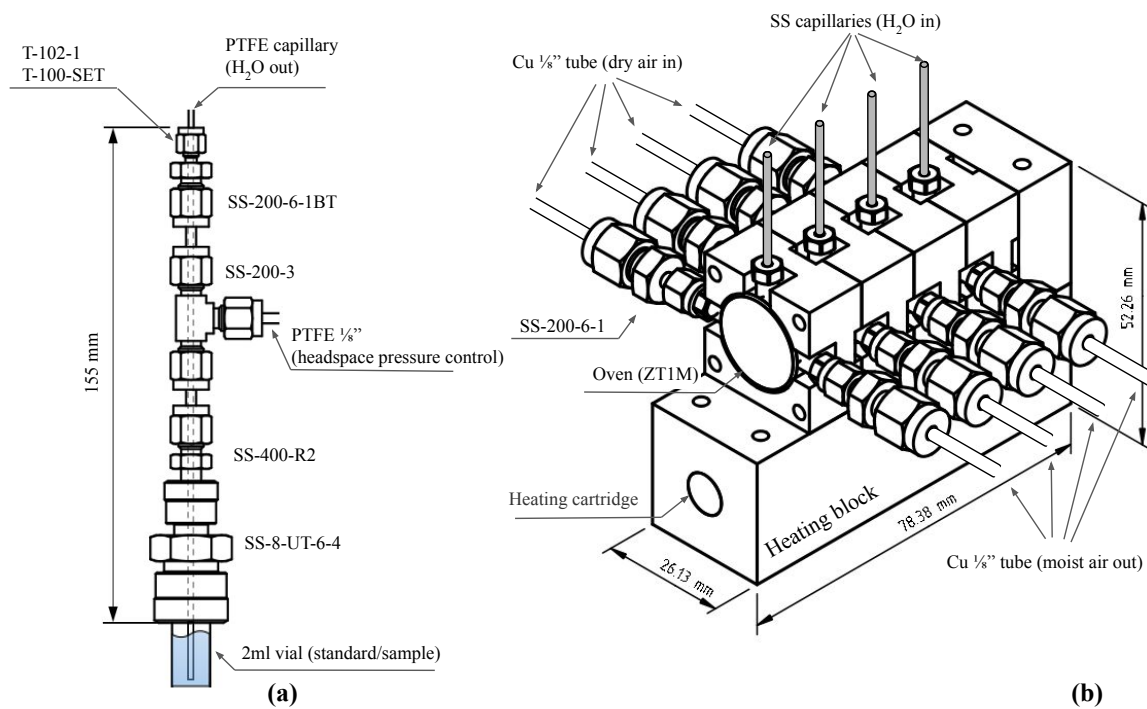

715

**Figure 2:** Technical drawings of the components used to produce the water vapor stream. (a) Detail of the custom vial holder (Swagelok part numbers). (b) Detail of the compact 4 ovens assembly (Swagelok and VICI part numbers). For both panels, white arrows indicate push gas/dry air, blue arrows indicate water flow, and gray arrow indicates moist air flow.

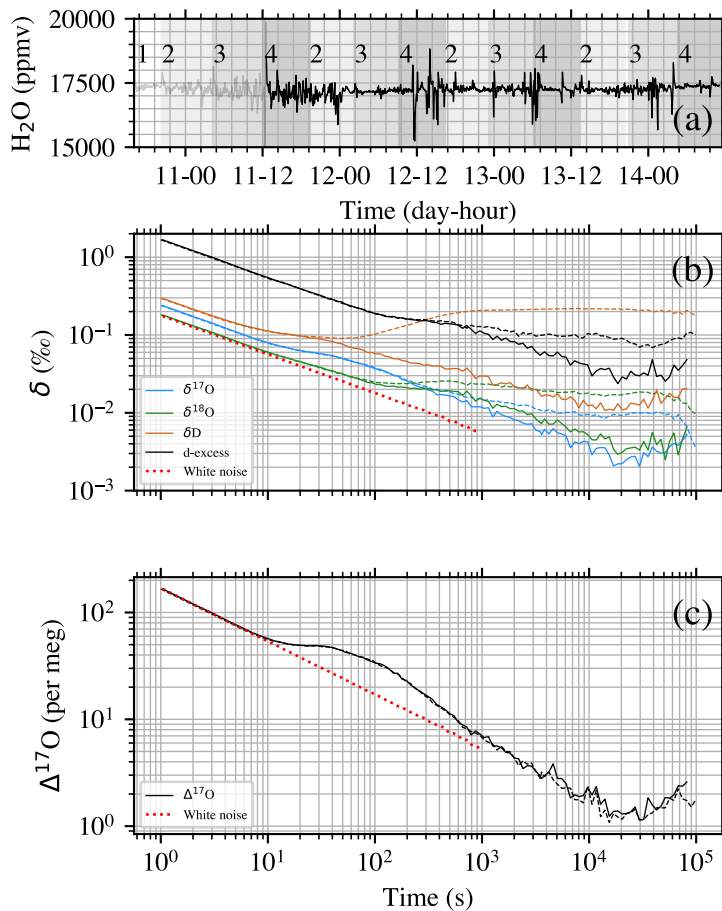


720

**Figure 3:** Flash evaporator 92-hours stability test of BER standard. (a) Timeseries of H<sub>2</sub>O signal ( $17229 \pm 340$  ppmv). The signal used to calculate the Allan Deviation is reported as a solid black line. On the x-axis: day (October 2022) and hour (LST). Gray shading used to distinguish among injections from different vials. The ID of vial holders are reported on the top of the plot. (b) Allan Deviation of  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$ ,  $\delta\text{D}$  and d-excess during the long-term stability test, including the full 92 hours dataset (dashed lines) and discarding the first 16 hours (solid lines). The Allan deviation of white noise is reported as a red dotted line for reference. (c) Similar to b but for  $\Delta^{17}\text{O}$ .

725




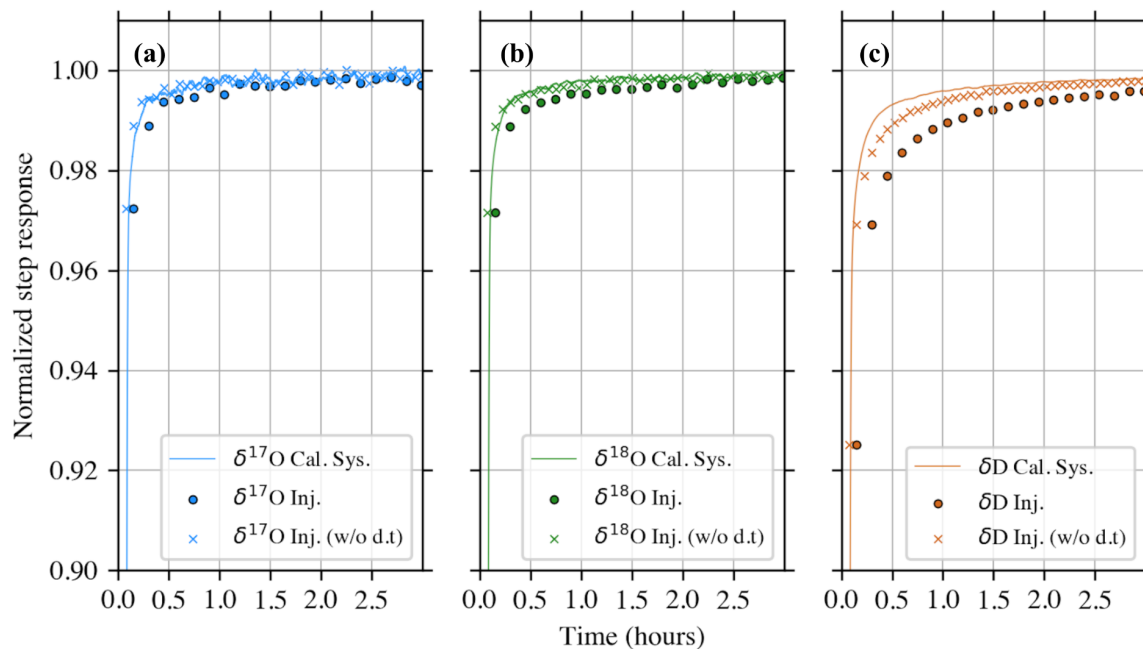


**Figure 4:** Normalized step change between standard SP and BER for  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$ , and  $\delta\text{D}$  in (a), (b), and (c), respectively. Solid lines: continuous signal acquired from the calibration system (moving average 270s). Coloured circles: injections performed with the Picarro autosampler and vaporizer including dead time. Coloured crosses: injections performed with the Picarro autosampler and vaporizer removing dead time.

730


735

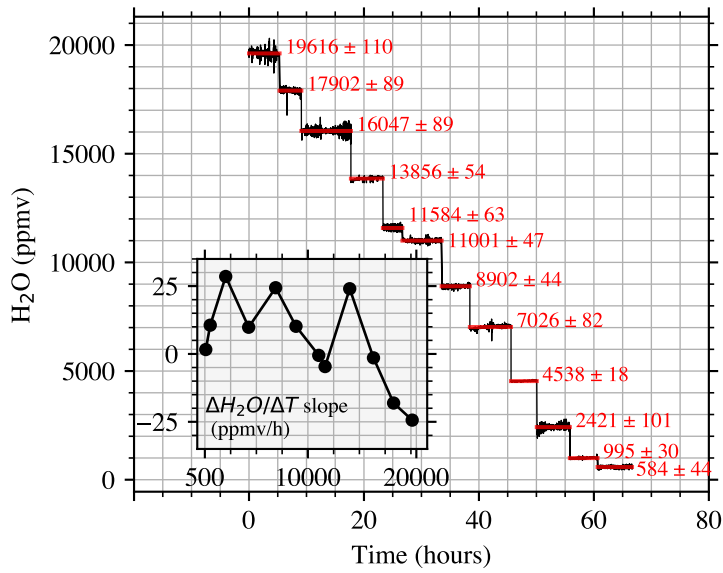

**Figure 5:** Humidity levels selected to test the short-term performances of the vapor generation module. H<sub>2</sub>O 1 $\sigma_{1-s}$  is one standard deviation calculated at a standard sampling rate (~1 Hz). The trend in the humidity level during each level is shown in the insert.

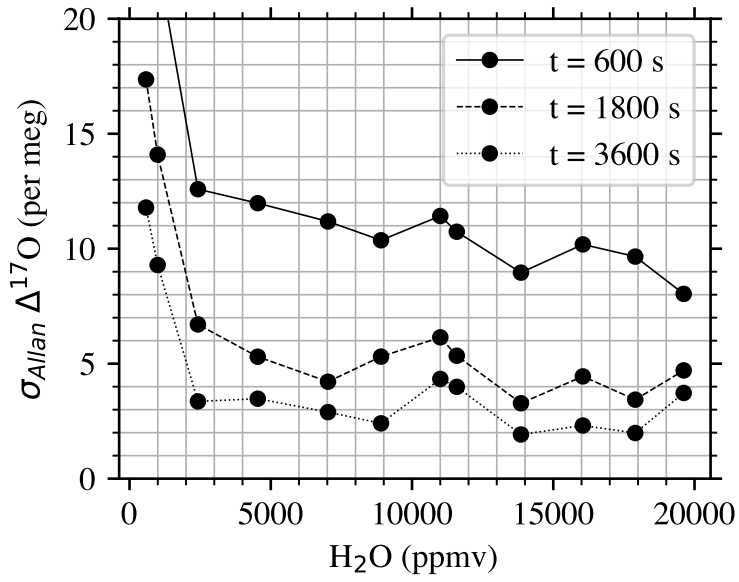


745 **Figure 6:** Overlapping Allan Deviation of  $\Delta^{17}\text{O}$  measured at different humidity levels and for different integration times.

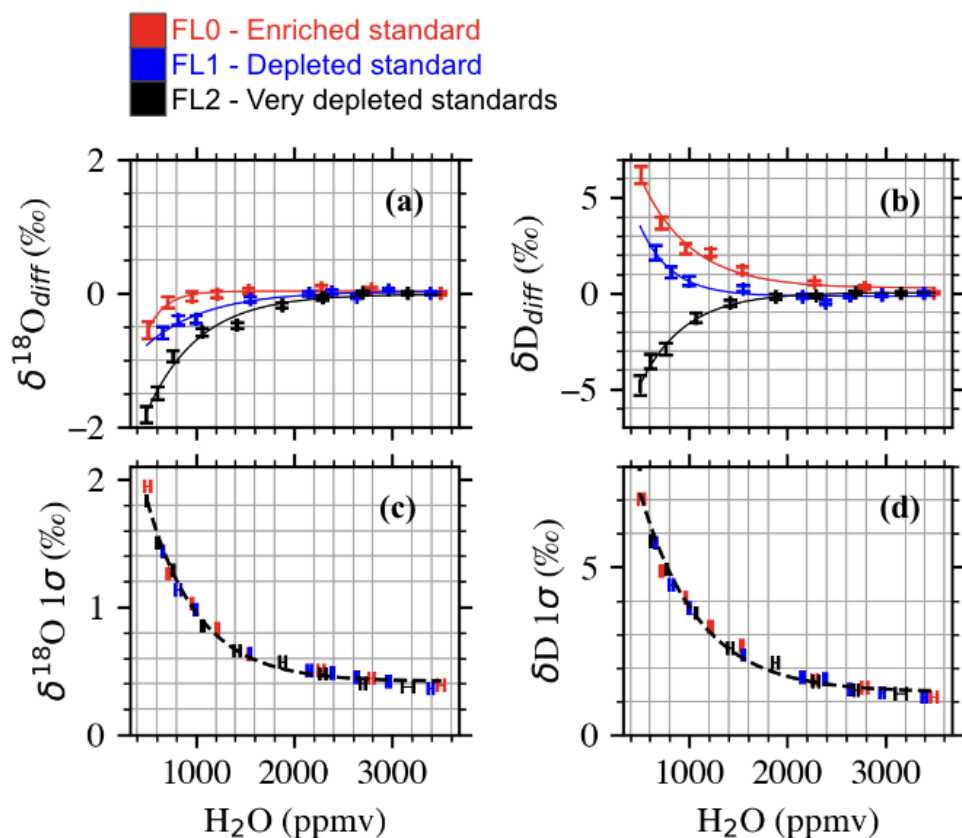


**Figure 7:** Humidity-isotope characterization of the HKDS2092 analyzer between 500-3500 ppmv using three different isotopic standards. (a) and (b) humidity - isotope dependency for  $\delta^{18}\text{O}$  and  $\delta\text{D}$ , respectively. Dependency reported as the difference between the isotopic composition at 3500 ppmv and isotopic composition for each humidity step. Error bars are standard errors of the mean. Lines are exponential decay models that best fit the observations of each isotope standard. (c) and (d) standard deviation of  $\delta^{18}\text{O}$  and  $\delta\text{D}$  for each humidity step and different standards. Error bars on the horizontal axis are standard deviations. For all panels, results of the best fits are reported in supplementary material Table S5.

750

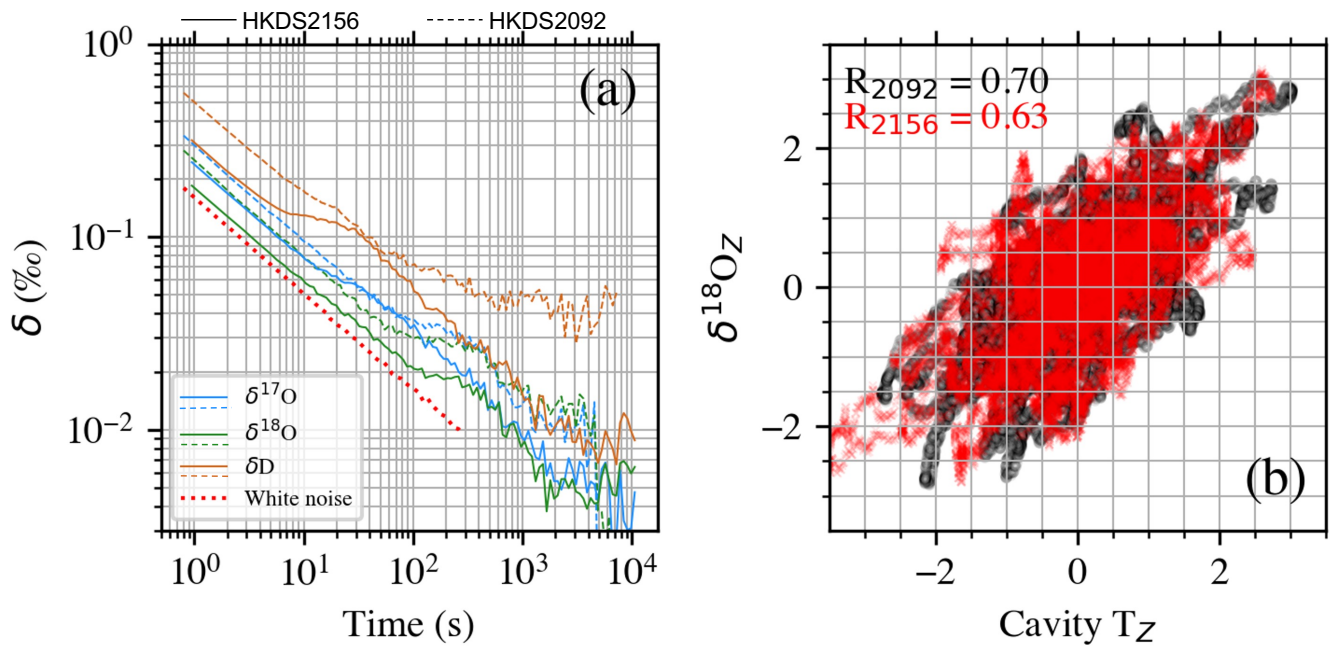


755 **Figure 8:** 10 hours analysis of the same water vapor source using two water isotope analyzers (HKDS2092, HKDS2156). (a) Allan Deviations of the two analyzers showing “bumps” at different averaging times for the two instruments. The Allan deviation of white noise is reported as a red dotted line for reference. (b) Z-scores of  $\delta^{18}\text{O}$  vs z-scores of cavity temperature of the two instruments (HKDS2092 in black, HKDS2156 in red). Standard deviations of  $\delta^{18}\text{O}$  are 0.02‰ and 0.01‰ for HKDS2092 and HKDS2156, respectively. Standard deviations of cavity temperature are 0.002 and 0.001 K for HKDS2092 and HKDS2156, respectively.

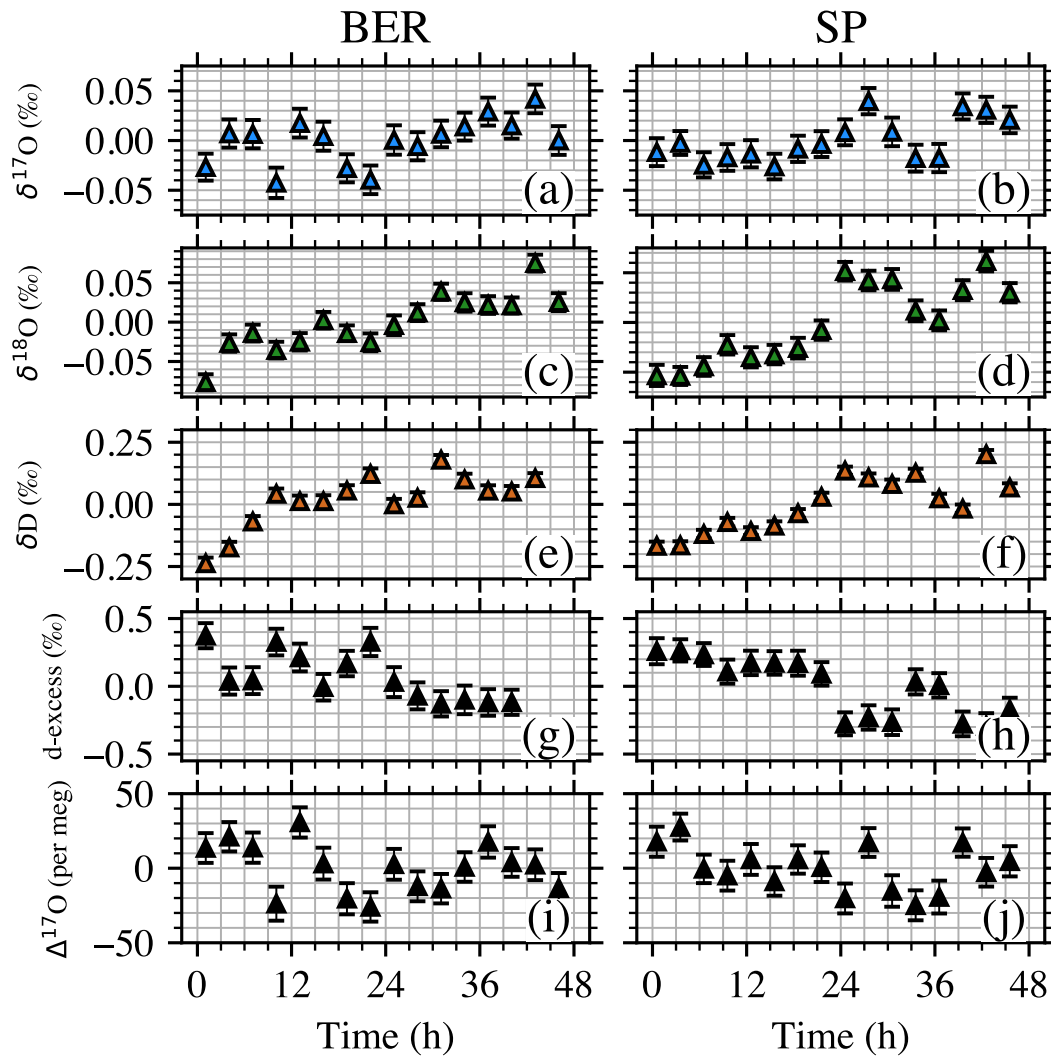

760

**Figure 9:** Variability of repeated injections of BER and SP standards using the multiple ovens configuration (raw data). Results reported as average  $\pm$  standard error calculated for the last 5 minutes of  $\delta^{17}\text{O}$  (a and b),  $\delta^{18}\text{O}$  (c and d),  $\delta\text{D}$  (e and f), d-excess (g and h) and  $\Delta^{17}\text{O}$  (i and j) signals. The results are centred around the mean value of all the injections to improve visualization.


765

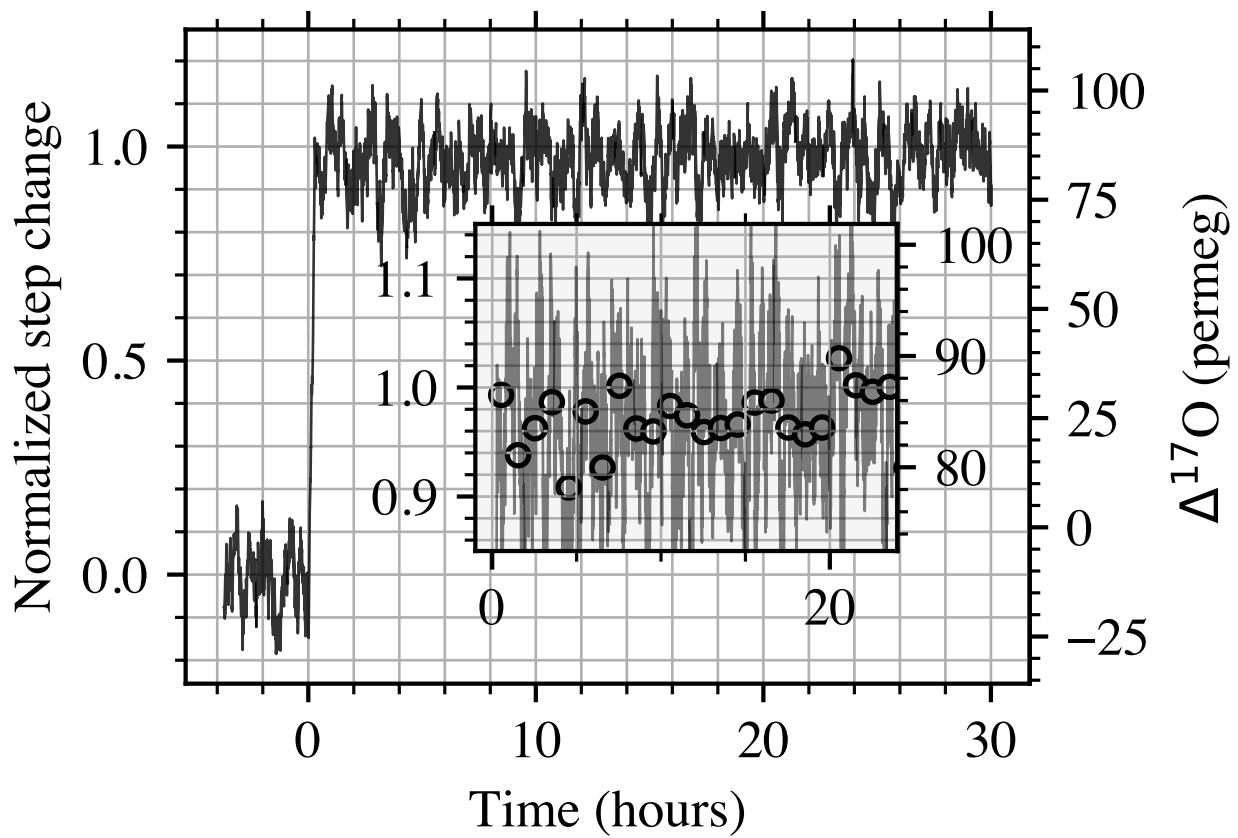


**Figure 10:** Calibrated and normalized step change for  $\Delta^{17}\text{O}$ . Black line is a 15-minute window moving average. Inset plot: detail of the 0-24h region. Grey line is the same as in the main plot. Circles are 1-hour averaged sample mean.

770

775

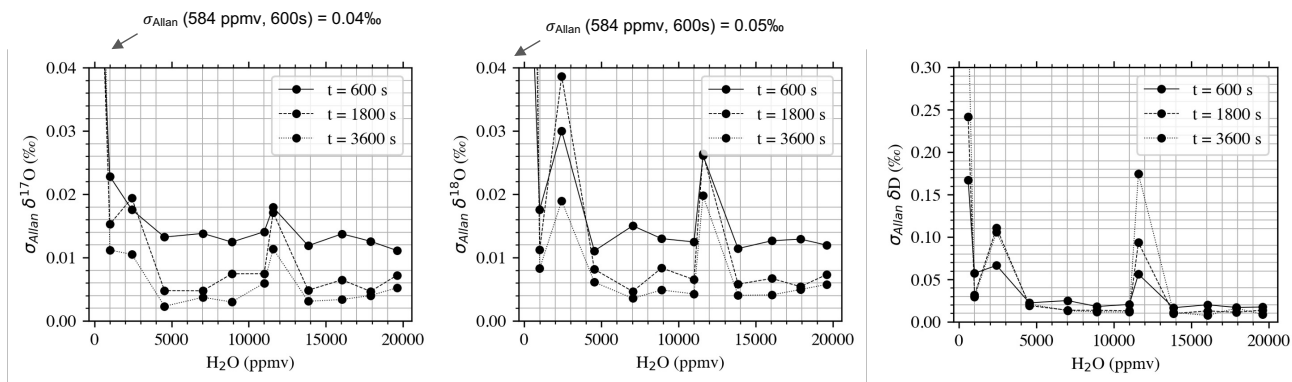

780 **Figure A1:** Allan Deviation for  $\delta^{17}\text{O}$ ,  $\delta^{18}\text{O}$  and  $\delta\text{D}$  at 600, 1800, and 3600 second integration time as function of humidity level.

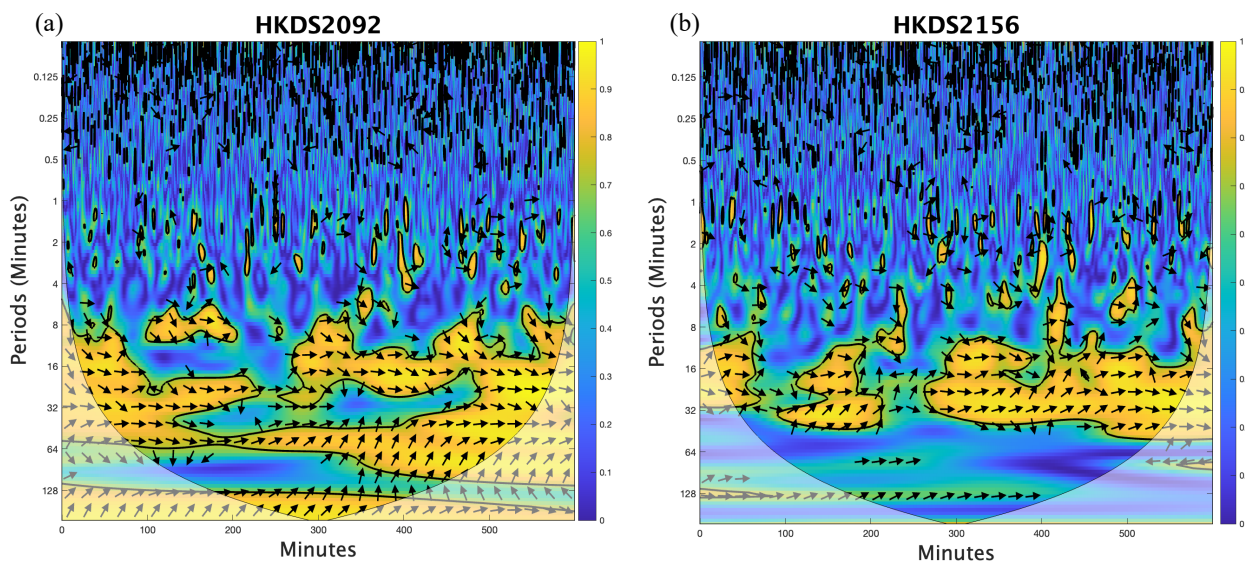

**Figure B1:** Squared Wavelet Coherence analysis between the measured  $\delta^{18}\text{O}$  and recorded cavity temperature of the two Picarro analyzers HKDS2091 (Panel a) and HKDS2156 (Panel b) using procedure by Grinsted et al. (2004). The 5% significance level against red noise is shown as a thick contour. Arrows indicate phasing (angle corresponds to phase behaviour). In-phase behaviour of  $\delta^{18}\text{O}$  and recorded cavity temperature is observed for periods between  $\sim 12$  minutes and  $\sim 30$  to 60 minutes for respectively HKDS2156 and HKDS2092 analysers.

785