

A new portable sampler of atmospheric methane for radiocarbon measurements

Giulia Zazzeri^{1*}, Lukas Wacker¹, Negar Haghypour², Philip Gautschi¹, Thomas Laemmel³, Sönke Szidat³, Heather Graven⁴

5

¹ Laboratory of Ion Beam Physics, ETH, Zurich, Switzerland.

*Now at: RSE, Sviluppo Sostenibile e Fonti Energetiche, Milano, Italy

² Geological Institute, ETH, Zurich, Switzerland

³ Department of Chemistry, Biochemistry and Pharmaceutical Sciences, University of Bern, Bern, Switzerland & Oeschger

10 Centre for Climate Change Research, University of Bern, Bern, Switzerland

⁴ Department of Physics, Imperial College London, London

Correspondence to: Giulia Zazzeri (giulia.zazzeri@rse-web.it)

Radiocarbon (¹⁴C) is an optimal tracer of methane emissions, as ¹⁴C measurements enable distinguishing fossil from biogenic
15 methane (CH₄). However, ¹⁴C measurements in atmospheric methane are still rare, mainly because of the technical challenge
of collecting enough carbon for ¹⁴C analysis from ambient air samples. In this study we address this challenge by advancing
the system in Zazzeri et al. (2021) into a much more compact and portable sampler, and by coupling the sampler with the
MICADAS AMS system at ETH, Zurich, using a gas interface.

Here we present the new sampler setup, the assessment of the system contamination and a first inter-laboratory comparison
20 with the LARA AMS laboratory at the University of Bern.

With our sampling line we achieved a very low blank, 0.7 µgC compared to 5.5 µgC in Zazzeri et al. (2021), and a sample
precision of 0.9 %, comparable with other measurements techniques for ¹⁴CH₄, while reducing the sample size to 60 liters of
air. We show that this technique, with further improvements, will enable routine ¹⁴CH₄ measurements in the field for an
improved understanding of CH₄ sources.

25 1 1 Introduction

Understanding the methane (CH₄) budget and identifying methane sources have become priority to tackle global warming, as
methane is the second most important anthropogenic greenhouse gas after carbon dioxide (CO₂) and because the dynamics
that led to the CH₄ increase in the last decade have not been fully unraveled. Tracing CH₄ sources and monitoring mitigation
strategies are urgently needed.

30 ¹⁴C measurements of atmospheric methane can advance our knowledge on methane production processes by differentiating
fossil vs biogenic sources. This is because fossil CH₄ is depleted in ¹⁴C, and when emitted into the atmosphere, exerts a

dilution of the ^{14}C in atmosphere that can be quantified. However, this research field is still under-explored, as ^{14}C measurements of atmospheric methane are challenging.

35 One of the main challenges is sampling enough air for ^{14}C analysis via accelerator mass spectrometry (AMS), as the atmospheric methane concentration is low (~ 2 ppm). Here we build on recent advances that have been made in the analysis of ^{14}C in atmospheric methane. Traditionally, air was collected in pressurized cylinders using high-pressure pumps, followed by an extraction procedure in the laboratory (Eisma 1994, Townsend-Small 2012). Zazzeri et al. (2021) developed a new technique that separates methane carbon from ambient air while sampling, simplifying the transportation of collected samples in a small trap and minimizing the laboratory processing needed. The F^{14}C measurement precision achieved is 40 between 0.5 and 1.2 %, comparable to the best precisions of alternative but more lab intensive techniques. The laboratory-based system developed by Zazzeri et al. (2021) was applied in the quantification of fossil and biogenic proportions of CH_4 in London (Zazzeri et al. 2023). A portable system using a similar technique was demonstrated by Palonen et al. (2017), but in this study they used only samples with enriched methane concentrations of >100 ppm, e.g. for CH_4 emissions from wetlands. Another promising recently developed technique applies chromatographic separation of CH_4 from air as it requires 45 only 60 l of atmospheric air to be sampled in a bag (Espic et al. 2019), still achieving precisions of 1.2 %.

In this study we advance the sensitive though simple methane sampling system in Zazzeri et al. (2021) with the portability of the system of Palonen et al. (2017), requiring as little air as demonstrated by Espic et al. (2019). The result is a compact and portable system to be deployed in field campaigns. We present the technology advancement and the assessment of the system efficiency, by quantifying the amount of extraneous carbon introduced during sample preparation and ultimately the 50 measurement precision to be achieved. We demonstrate the method by comparing ^{14}C measurements made by the new portable system at the Laboratory of Ion beam Physics (LIP) at ETH Zurich and by the system using bag sampling and chromatographic separation at the Laboratory for the Analysis of Radiocarbon with AMS (LARA) at the University of Bern.

2 Method

1.1 The sampling setup

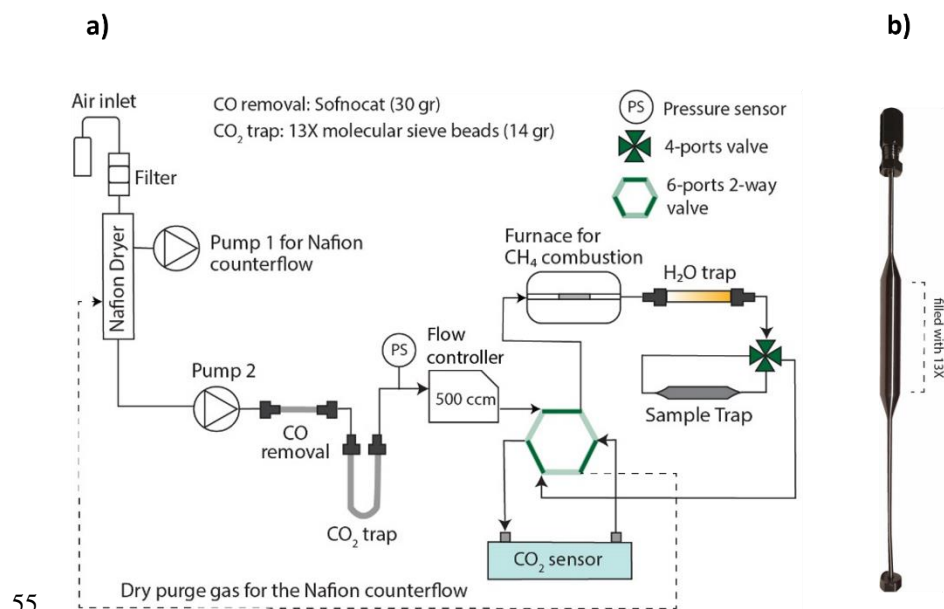


Figure 1: a) Schematic of the sampling system. First, the filtered air is dried with a Nafion dryer; then, any CO₂ from ambient air and from oxidation of CO is removed on a trap. The CO₂ derived from the combustion of CH₄ is collected onto a final sample trap. Dark green lines in the 6-ports valve indicate active flow direction. In the indicated configuration, the CO₂ sensor measures the CO₂ level after the sample trap, enabling to check for the trap breakthrough. In the alternative configuration, complete CO₂ removal prior to CH₄ oxidation can be checked. b) Sample trap filled with 0.250 g of 13X.

The sampling system is based on four main steps as in Zazzeri et al. (2021): 1) H₂O removal with a Nafion dryer; 2) CO and CO₂ removal; 3) combustion of CH₄ to CO₂; 4) adsorption of the combustion-derived CO₂ onto a molecular sieve sample trap. Figure 1 shows the system schematic. Ambient air is sampled through a Nafion dryer (Perma Pure gas dryer, PD-50-24) at up to 500 cc/min of air with a KNF membrane pump (pump 2 in Fig 1) controlled by a mass flow controller. The Nafion enables reduction of the water content to levels of 0.01% (Zazzeri et al. 2021). Downstream of the pump, CO is oxidized to CO₂ using Sofnocat® catalyst before all CO₂ (from ambient and from oxidation of CO) is removed on a trap containing 14 g of 13X molecular sieve in 1 mm pellets. This amount of molecular sieve has been found sufficient to trap atmospheric CO₂ in ~300 L of air (see Figure A1). After collection of three samples, this trap is disconnected from the system via two Swagelok ball valves, then removed and regenerated by heating at 500°C with high purity nitrogen back flush for at least three hours, in a similar manner as in Zazzeri et al (2021).

65

70

After the sample air passes through the CO₂ trap, CH₄ is combusted at 800 °C in a small furnace comprising a 22 cm long quartz tube with 1 g of platinumized quartz wool (Sigma Aldrich) acting as catalyst (Petrenko et al. 2008). The H₂O derived from the CH₄ oxidation is trapped onto a magnesium perchlorate trap (H₂O trap in Figure 1), while the CO₂ derived from combustion of CH₄ is collected on the sample trap (13X, 45-60 mesh) for subsequent ¹⁴C measurement. A non-dispersive

- 75 infrared CO₂ sensor (NDIR FLOW^{EVO} from SmartGas) monitors both completeness of CO₂ removal from air prior to methane combustion and completeness of CO₂ collection on the sample trap. If regularly calibrated and run at constant temperature and pressure, the sensor can measure CO₂ concentrations in a range of 0 to 100 ppm with a precision of ± 1 ppm. The sample trap, minimized in size for low cross contamination, can be cooled with Peltier coolers to maximize trapping efficiency and avoid sample loss.
- 80 The whole system runs either on 115/230 V AC or 48 V DC provided by a battery pack. Two 72V 30Ah 2160Wh Lithium batteries are sufficient to run the sampling system for 10 hours.



85 **Figure 2: Setup of the atmospheric methane sampling device. The whole system fits well into a box of 80 x 40 x 30 cm. It runs either on 115/230 V AC or 48 V DC provided by a battery pack. Major parts of the system are: 1) Nafion dryer (mostly hidden underneath); 2) Pumps (partially hidden); 3) CO₂ trap; 4) Flow controller; 5) Furnace for CH₄ combustion; 6) Sample trap with Peltier coolers; 7) CO₂ sensor**

1.2 Sample trap and cooling system

The sample trap consists of 0.250 g 13X 45-60 mesh molecular sieve packed in a 4 cm long ¼” OD stainless steel tube. The trap tube is welded to stainless steel capillary tubing and attached to a VICI 4 port valve which can be disconnected from the sampling system (Fig 1 b) in order to release the sample for ^{14}C analysis in the AMS. Before its first use, the sample trap is heated gradually to 650 °C in a customized oven, while flushing with high purity nitrogen. The NDIR FLOW^{EVO} CO₂ sensor is used to check when the trap is not releasing CO₂ anymore and does not contain any residual carbon, typically after 1 hour. During sampling, the sample trap is cooled down to -10 °C using two Peltier elements, part 6 in Fig 2. This maximizes the trapping efficiency such that 0.250 g 13X can adsorb ~60 µgC (methane carbon from ~60 L of ambient air at 2 ppm), before the CO₂ breakthrough happens. The adsorption capacity can be enhanced by lowering the temperature even further. After sampling, the sample trap is disconnected from the system and heated at 450 °C for 10 minutes for sample desorption using the TSE (Tube Sealing Equipment) system (<https://www.ionplus.ch/tse>), which enables to measure the pressure of the desorbed gases and to quantify the amount of the CO₂ released. The desorbed CO₂ is cryogenically sealed into a glass ampule to be used in the gas interface system of the Mini Carbon Dating AMS system (MICADAS) (Wacker et al. 2013). Before the next sample is collected, the sample trap is cleaned of remaining CO₂ by flushing with high purity nitrogen while heating at 550 °C for 30 minutes. Such a long procedure compared to other cleaning processes for other applications is only precautionary, a shorter procedure might be sufficient to remove any residual carbon from previous sampling.

1.3 AMS analysis

The sample is measured with the MICADAS accelerator mass spectrometry facilities for radiocarbon measurements in the Laboratory of Ion Beam Physics ETH (Wacker et al. 2010). The ^{14}C analysis using the gas interface of the MICADAS takes about 20 minutes and achieves a measurement precision of less than 1% for modern samples (Wacker et al. 2013) for a sample containing 20 µg carbon. Precisions down to 0.5% can be achieved, when measurements are repeated on ≥ 50 µg of carbon (Fahrni et al. 2010). The combusted NOX standard (SRM-4990C, Man 1983, Wacker et al. 2019) and ^{14}C -free CO₂ pre-mixed with helium in gas bottles were measured for standard normalization respectively or blank correction. Measured data were evaluated with the BATS program, where the samples were fractionation corrected, blank subtracted and normalized with the NOX standard (Wacker et al. 2010) to obtain $F^{14}\text{C}$ values (Reimer et al. 2004).

1.4 Characterization of the extraneous contaminant carbon within the sampler

Extraneous contaminant carbon in the sample trap after a sample collection might derive from intrusion of lab air into the system, from incomplete removal of atmospheric CO₂, from residual carbon on the sample trap prior to sampling, or from impurities within the combustion column.

To check for and quantify the contaminant carbon, we collected CH₄ samples of different sizes, and we follow the relationship between the measured fraction Modern (F¹⁴C) versus the sample masses given by the mass balance in Eq 1:

$$F^{14}C_{meas} = F^{14}C_{true} + \frac{1}{\mu g C_{meas}} [\mu g C_{add} * (F^{14}C_{add} - F^{14}C_{true})] \quad (1)$$

120

where “*meas*” indicates the measured value, $F^{14}C_{true}$ the F¹⁴C value of the sampled air, $\mu g C_{add}$ the carbon added into the system and $F^{14}C_{add}$ its F¹⁴C value. If assuming a constant contamination, the contaminant carbon added to the system is given by the $\mu g C_{add}$ value that produces the best fitting curve through the $F^{14}C_{meas}$ values plotted against the measured sample masses ($\mu g C_{meas}$). We assess the goodness of fit using reduced chi-squared statistics (i.e. “*curve_fit*” function from the “*scipy.optimize*” Python package).

125

To quantify the modern contaminant carbon, we collected seven samples from 10 to 70 $\mu g C$ from a 2 ppm mixture of fossil methane and synthetic air with no CO₂, CO or hydrocarbons (Fossil Ref).

To check for any fossil contaminant, we collected seven samples, from 10 to 75 $\mu g C$, from a cylinder of pressurized ambient air (Ref 1), with a CH₄ mole fraction of 2040 ppb. Note that in this case, the F¹⁴C of the reference gas ($F^{14}C_{true}$) is unknown.

130

The amount of fossil contaminant carbon and the F¹⁴C value of the reference gas are calculated by tweaking $\mu g C_{add}$ and $F^{14}C_{true}$ in Eq 1 to produce the best fitting curve.

In order to verify the source of the contaminant carbon, we collected five blanks. Three blanks were collected by running the system with lab air and without combustion, for three hours. This enabled verification of any contaminant carbon deriving from atmospheric CO₂ that was not trapped in the CO₂ trap and from residual carbon in the sample trap. Two samples were collected by flushing the system with nitrogen and with the combustion furnace at 800 °C to verify that additional carbon was not produced within the combustion process. No carbon was extracted from these five blanks.

135

1.5 Comparison with chromatographic extraction procedure

Three samples transferred in sampling bags from the cylinder of pressurized ambient air Ref 1 were extracted at the LARA laboratory, University of Bern, using 60 L of air and following the chromatographic extraction procedure in Espic et al. (2019). CO₂ derived from the sample extraction in Bern was measured using the gas interface system of the MICADAS AMS system at ETH, in the same manner as the samples collected with our portable sampler.

140

2 Results

Table 1 shows the F¹⁴C values and masses of the samples collected.

ETH nr.	Mass ugC	F ¹⁴ C	+ - (%)
<i>Modern Samples</i>			
133113.15.1	6	1.2903	2.27

133113.16.1	15	1.3570	1.03
133113.17.1	40	1.3610	0.76
133113.18.1	12	1.3293	1.10
133113.19.1	28	1.3577	0.85
133113.20.1	48	1.3604	0.85
133113.22.1	75	1.3816	0.82
<i>Fossil samples</i>			
136294.7.1	56	0.020612	6.81
136294.8.1	66	0.019753	5.90
136294.10.1	20	0.033567	5.03
136294.11.1	18	0.036063	5.09
136294.12.1	30	0.02058	5.60
136294.13.1	47	0.01954	5.48
136294.17.1	15	0.040006	4.50
<i>Bern</i>			
133991.1.1	66	1.3715	0.89
133991.2.1	64	1.3743	0.96
133991.3.1	66	1.3616	0.96

145 **Table 1: Mass, $F^{14}C$ values and uncertainty of samples collected. Modern samples are collected from Ref 1, fossil samples from Fossil Ref and “Bern” are samples extracted following the chromatographic procedure at LARA.**


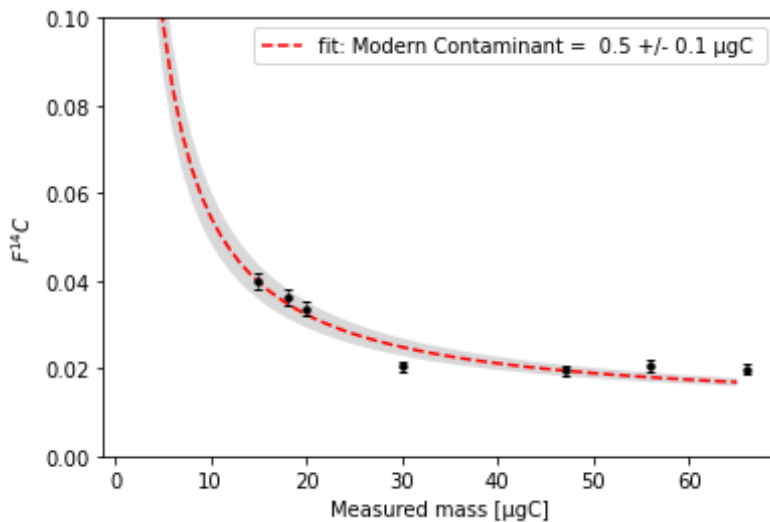


Figure 3: $F^{14}C$ values against the measured mass of the samples collected from the Fossil Ref. The grey bands represent one sigma uncertainty bar on the curve fit.

150 Assuming a $F^{14}C_{true}$ value for Fossil Ref of 0.01 and a $F^{14}C$ value of the modern contaminant ($F^{14}C_{add}$) of 1, the best fitting curve through the Fossil Ref samples indicates a constant level of modern contamination (μgC_{add}) of $0.5 \pm 0.1 \mu gC$. Larger

samples ($>50 \mu\text{gC}$) show an offset that can be explained with a size dependent contamination, an additional $0.1 \mu\text{gC}$ every $10 \mu\text{gC}$ collected, which we can correct for.

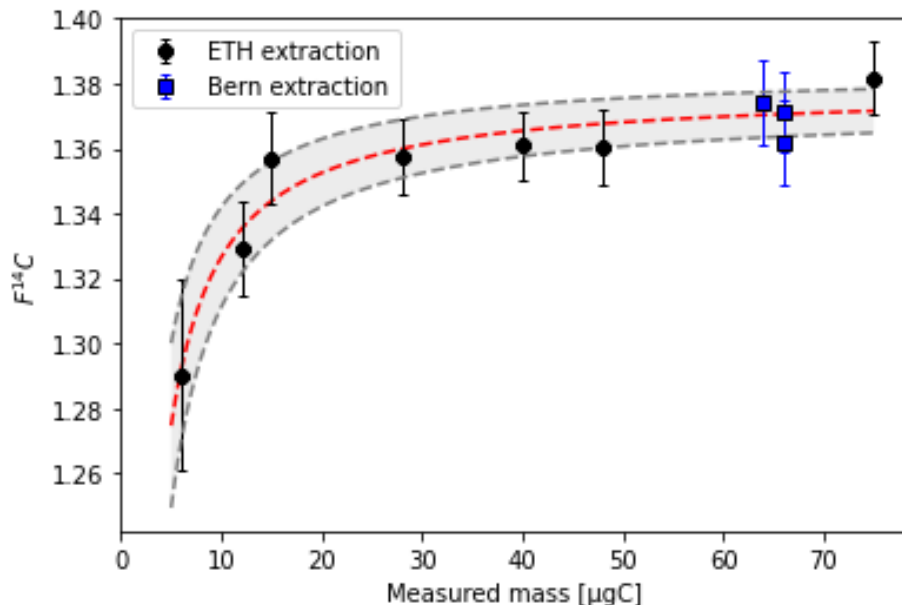

155

Figure 4: Measured $F^{14}\text{C}$ values against the measured mass of the samples collected from Ref 1. Symbols in blue are the Ref 1 samples extracted in Bern and are not included for the curve fitting. The grey bands represent one sigma uncertainty bar on the curve fit.

The data collected from Ref 1 best fit onto a curve with an $F^{14}\text{C}$ value of 1.38 ± 0.01 for the reference gas. However, by
160 considering only the quantified modern contamination of $0.5 \mu\text{gC}$, we do not achieve the best fitting curve, and we need to
add approximately $0.2 \pm 0.1 \mu\text{g}$ of contaminant fossil carbon. Zazzeri et al. (2021) indicated that some fossil carbon might
be produced within the combustion furnace, and therefore it is likely that even with our setup the combustion process led to
the production of some fossil carbon.

Ref 1 samples extracted in Bern, blue markers in Fig 4 (not included for determining the constant contamination), agree well
165 with the $F^{14}\text{C}$ values for Ref 1 samples with the same mass ($60 \mu\text{gC}$) extracted at ETH, indicating that the two extraction
methods are comparable. Samples of $60 \mu\text{gC}$ are equivalent to two/three hours of sampling of ambient air with our portable
system at 500 ccm or 60 liters of ambient air with the extraction line in Bern.

3 Discussion

In order to make the sampler portable we have reduced the size of the sampler components compared to the system in
170 Zazzeri et al. (2021). The main changes include:

- a smaller CO₂ trap placed before the combustion furnace, with 14 g against 60 g of molecular sieve. Its adsorption capacity is demonstrated by the very low modern blank, which indicates that all the ambient CO₂ is captured while sampling;
- a new design of the sample trap, with 0.250 g of molecular sieve against 1 g, accommodated in a 4 cm length tube and connected to a single 4 ports VICI valve. Collection of 60 µgC (two/three hours of sampling at 500 ccm) has been achieved by cooling down the sample trap using two Peltier elements;
- a smaller combustion furnace built at the Laboratory of Ion Beam Physics;
- connections and tubing of 1/8" size instead of 1/4".

175

180 All these modifications led to an important reduction of the level of constant modern contamination, from 5.5 +/- 1.1 µgC in Zazzeri et al. (2021) down to 0.5 +/- 0.1 µgC. According to the F¹⁴C measurements of our modern reference cylinder (Ref 1), we have an extra 0.2 +/- 0.1 µgC of fossil contamination, leading to 0.70 +/- 0.14 µgC total amount of contaminant carbon with an averaged F¹⁴C value of 0.71. We also found a size dependent contamination of 1%, which can be explained either with a tiny leak within the sampler or with some outgassing.

185 To further test the system contamination and demonstrate full separation of CH₄ and CO₂, more gas mixtures could be used for F¹⁴C measurements. For example, the system could be run using a mixture made of 2 ppm of fossil CH₄, 400 ppm of CO₂ from combustion of OXII, diluted in N₂ or He.

The overall uncertainty for individual samples of 60 µgC, calculated by propagating the error from counting statistics and background uncertainty, is 0.9%, comparable with other measurements techniques for ¹⁴CH₄, demonstrating that a larger sample, and therefore a longer sampling time, is not needed.

190

The main benefit of a portable system that needs only 60 liters of air for one sample is the important time saving both in the field and in the laboratory. The sample processing time in the laboratory has been reduced massively, and so the likelihood of contamination and mistakes by the operator. The system, given its small size, could be placed in a vehicle, enabling sampling in a source area, such as a landfill site or an urban environment, or performing a mapping of isotopic signatures in a region.

195

4 Conclusions

We have advanced the CH₄ sampling system from Zazzeri et al. (2021) into a portable system that can be used in field campaigns, while also reducing the contamination in the system. Further improvements could be made to automate the system, so that the valves and pumps switching, and the flow rate are computer-controlled, making the whole sampling procedure more consistent. More samples could be collected in parallel at the same time. In addition, the CO₂ desorbed from the sample trap is presently cryogenically trapped in glass ampules sealed for offline ¹⁴C measurements, but a direct coupling


200

of the zeolite trap to the gas interface (Wacker et al., 2013) connected to the MICADAS AMS system could be implemented, avoiding the additional step using glass ampules.

205 Full assessment of the fossil carbon contamination in $^{14}\text{CH}_4$ measurements is still challenging because there is no modern reference material available for CH_4 . The production of a modern CH_4 standard for ^{14}C analysis, followed by an inter-laboratory comparison, should be pursued.

Overall, the combination of a selective and field deployable CH_4 sampler and sensitive AMS analysis provides a unique technology, that can expand the use of $^{14}\text{CH}_4$ measurements.

Appendix A

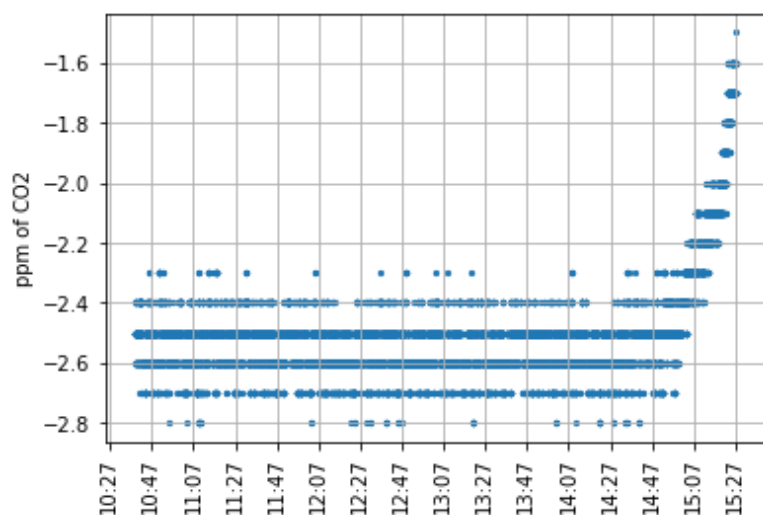

210

Figure A1: CO_2 concentrations in ppm measured with the NDIR sensor downstream the CO_2 trap, while flushing the trap with lab air. The trap starts saturating after 4 hours and 30 minutes of flushing at 1 lpm flow rate. Note that the NDIR sensor measures negative values for a gas stream with no CO_2 .

5 References

215 Eisma, R., Vermeulen, A.T. and Van Der Borg, K.: $^{14}\text{CH}_4$ emissions from nuclear power plants in northwestern Europe. Radiocarbon, 37(2), pp.475-483, doi: 10.1017/S0033822200030952, 1995.

Espic, C., Liechti, M., Battaglia, M., Paul, D., Röckmann, T. and Szidat, S.: Compound-specific radiocarbon analysis of atmospheric methane: a new preconcentration and purification setup. Radiocarbon, 61(5), pp.1461-1476, doi: 10.1017/RDC.2019.76, 2019

220 Fahrni, S.M., Wacker, L., Synal, H.A. and Szidat, S.: Improving a gas ion source for ^{14}C AMS. Nuclear Instruments and Methods in Physics Research Section B: Beam Interactions with Materials and Atoms, 294, pp.320-327, 2013

- Palonen, V., Uusitalo, J., Seppälä, E. and Oinonen, M.: A portable methane sampling system for radiocarbon-based bioportion measurements and environmental CH₄ sourcing studies. *Review of Scientific Instruments*, 88(7), doi: 10.1063/1.4993920, 2017.
- 225 Petrenko, V. V.; Smith, A. M.; Brailsford, G.; Riedel, K.; Hua, Q.; Lowe, D.; Severinghaus, J. P.; Levchenko, V.; Bromley, T.; Moss, R.; Mühle, J.; Brook, E. J.: A New Method for Analyzing ¹⁴C of Methane in Ancient Air Extracted from Glacial Ice. *Radiocarbon*, 50, 53– 73, DOI: 10.1017/s003382220004336, 2008
- Reimer, P.J., Brown, T.A. and Reimer, R.W.: Discussion: reporting and calibration of post-bomb ¹⁴C data. *Radiocarbon*, 46(3), pp.1299-1304, 2004
- 230 Townsend-Small, A., Tyler, S.C., Pataki, D.E., Xu, X. and Christensen, L.E.: Isotopic measurements of atmospheric methane in Los Angeles, California, USA: Influence of “fugitive” fossil fuel emissions. *Journal of Geophysical Research: Atmospheres*, 117(D7), doi: 10.1029/2011JD016826, 2012
- Wacker, L., Bonani, G., Friedrich, M., Hajdas, I., Kromer, B., Němec, M., Ruff, M., Suter, M., Synal, H.A. and Vockenhuber, C.: MICADAS: routine and high-precision radiocarbon dating. *Radiocarbon*, 52(2), pp.252-262, 2010
- 235 Wacker, L., Lippold, J., Molnár, M. and Schulz, H.: Towards radiocarbon dating of single foraminifera with a gas ion source. *Nuclear Instruments and Methods in Physics Research Section B: Beam Interactions with Materials and Atoms*, 294, pp.307-310, doi: 10.1016/j.nimb.2012.08.038, 2013
- Wacker, L., Bollhalder, S., Sookdeo, A. and Synal, H.A.: Re-evaluation of the New Oxalic Acid standard with AMS. *Nuclear Instruments and Methods in Physics Research Section B: Beam Interactions with Materials and Atoms*, 455, pp.178-240 180, 2019
- Zazzeri, G., Graven, H., Xu, X., Saboya, E., Blyth, L., Manning, A.J., Chawner, H., Wu, D. and Hammer, S.: Radiocarbon measurements reveal underestimated fossil CH₄ and CO₂ emissions in London. *Geophysical Research Letters*, 50(15), p.e2023GL103834, doi: 10.1029/2023GL103834, 2023
- Zazzeri, G., Xu, X. and Graven, H.: Efficient sampling of atmospheric methane for radiocarbon analysis and quantification of fossil methane. *Environmental Science & Technology*, 55(13), pp.8535-8541, doi: 10.1021/acs.est.0c03300, 2021
- 245

6 Competing interests

The contact author has declared that none of the authors has any competing interests.

7 Acknowledgement

This work has been funded by the Horizon 2020 Framework Programme (Call: H2020-MSCA-IF-2020, Project: 101026926
250 — FORM) and by the Laboratory of Ion Beam Physics.