



# The Far INfrarEd Spectrometer for Surface Emissivity (FINESSE). Part 1: Instrument description and level 1 radiances

Jonathan E. Murray<sup>1,2</sup>, Laura Warwick<sup>3</sup>, Helen Brindley<sup>1,2</sup>, Alan Last<sup>1</sup>, Patrick Quigley<sup>1</sup>, Andy Rochester<sup>1</sup>, Alexander. Dewar<sup>1</sup>, Daniel. Cummins<sup>1</sup>

5 <sup>1</sup>Department of Physics, Imperial College London, SW7 2BX, UK

<sup>2</sup>National Centre for Earth Observation, UK

<sup>3</sup>ESA-ESTEC, Noordwijk, Netherlands

*Correspondence to:* Jonathan E. Murray (j.murray@imperial.ac.uk)

**Abstract.** The Far INfrarEd Spectrometer for Surface Emissivity (FINESSE) instrument combines a commercial Bruker EM27  
10 spectrometer with a front end viewing and calibration rig developed at Imperial College London. FINESSE is specifically  
designed to enable accurate measurements of surface emissivity covering the range 400-1600 cm<sup>-1</sup> and as part of this remit,  
can obtain views over the full 360° angular range.

In this Part (I) we describe the system configuration, outlining the instrument spectral characteristics, our data acquisition  
methodology and the calibration strategy. As part of the process, we evaluate the stability of the system, including the impact  
15 of knowledge of blackbody target emissivity and temperature. We also establish a numerical description of the instrument  
line shape which shows strong, frequency dependent, asymmetry. We demonstrate why it is important to account for these  
effects by assessing their impact on the overall uncertainty budget on the level 1 radiance products from FINESSE. Initial  
comparisons of observed spectra with simulations show encouraging performance given the uncertainty budget.

## 1 Introduction

20 The infrared spectral emissivity of the Earth's varying surface types plays a fundamental role in determining their radiative  
emission, influencing the surface energy budget and the efficiency with which the Earth cools to space. Knowledge of infrared  
surface emissivity, including any angular dependence, is also a pre-requisite for satellite instruments exploiting these  
wavelengths to retrieve surface and lower tropospheric temperature and/or profiles of certain atmospheric constituents.

Recent modelling work has also indicated that surface emissivity in the far-infrared (wavelengths longer than 15 mm) may  
25 play a more important role than previously thought in influencing, in particular, high latitude surface temperature and its  
evolution (Feldman et al., 2014, Huang et al., 2018). Typically, surface emission at these wavelengths is attenuated by strong  
water vapour absorption. However, under clear-skies at low water vapour concentrations micro-windows within the far-  
infrared can open, allowing the surface emission to propagate further through the atmosphere, and, in some cases, escape to  
space.



30 To date, very few retrievals of far-infrared emissivity exist. Those that do tend to have been obtained over a limited area or  
for a limited time (e.g. Bellisario et al., 2017, Palchetti et al., 2021, Borbas et al., 2021). This will change with the launch of  
two new satellite missions, the Polar Radiant Energy in the Far InfraRed Experiment (PREFIRE) (L'Ecuyer et al., 2022) and  
the Far-infrared Outgoing Radiation Understanding and Monitoring (FORUM) mission (Palchetti et al., 2020). Looking  
further ahead, there are also plans to fly a far-infrared instrument as part of NASA's Atmosphere Observing System mission  
35 (Blanchet et al., 2011).

Theoretical studies suggest that both PREFIRE and FORUM will be capable of retrieving surface emissivity across both the  
mid- and far-infrared under certain conditions (Ben Yami et al., 2022, Xie et al., 2022). These findings reinforce results  
obtained from high-altitude aircraft flights over the Greenland plateau (Murray et al., 2020) and, combined with the  
proliferation of far-infrared focused missions, imply a need for the development of ground-truthing capability to verify  
40 retrievals made across the infrared.

This need has motivated the development of the Far-INfrarEd Spectrometer for Surface Emissivity (FINESSE). Combining a  
commercial Bruker EM27 spectrometer with a custom-built front-end pointing and calibration system, the instrument is  
portable and can be deployed to different locations as0 required. Its particular innovation is the ability to point through a full  
360°, negating the need to tilt the instrument to avoid its own footprint and allowing the angular dependence of emissivity to  
45 be easily assessed.

In the following sections we describe the various components of FINESSE and discuss how it has been  
characterised. Particular attention is paid to the calibration procedure and assessment of the instrument line shape, and we  
show how knowledge of these parameters flows through to the ultimate uncertainty budget associated with the level 1 radiance  
products. Characterisation of this uncertainty budget is particularly important when using the FINESSE measurements to infer  
50 surface emissivity, a process which we describe in full in the accompanying Part (II).

## 2 System Description

### 2.1 EM27 Spectrometer

The EM27 is a relatively inexpensive ruggedised spectrometer, using a RockSolid™ pendulum interferometer, with low  
sensitivity to mechanical shocks and vibrations which has been hardened for operation in temperatures as low as 253 K. EM27  
55 spectrometers are primarily designed for real-time remote monitoring of atmospheric chemical concentrations but have also  
been used to undertake surface emissivity measurements in the mid-IR from  $700\text{ cm}^{-1}$  -  $2200\text{ cm}^{-1}$  (e.g. Langsdale et al., 2020).  
The EM27 series is configurable, with the choice of beam-splitter and detector determining the spectral range that can be  
covered. It can be used in either active mode, utilising a background source, or in passive mode, observing ambient atmospheric  
or target radiance. To extend measurements into the Far-IR FINESSE uses a combination of a potassium bromide (KBr) beam-  
60 splitter, an extended Mercury Cadmium Telluride (MCT) detector cooled to 77 K using liquid nitrogen, and a diamond input  
window for the interferometer housing. Combined, these components give spectral coverage from  $400$  -  $1600\text{ cm}^{-1}$ . As KBr




is hygroscopic the interferometer housing is hermetically isolated from ambient conditions by the diamond input window and kept dry using desiccant, with typical enclosure humidity kept below 3%. The use of an extended MCT detector gives greater sensitivity than uncooled DLaTGS detectors at wavenumbers greater than  $450\text{ cm}^{-1}$  and facilitates a more rapid measurement cycle. This latter advantage is important if ambient conditions are fluctuating rapidly with time. The disadvantage is the need to source and perform repeat fills of liquid  $\text{N}_2$  during extended operations. The resolution of the instrument can be set using the control software supplied with the EM27 at values between  $0.5\text{ cm}^{-1}$  and  $4\text{ cm}^{-1}$ .

As built, the EM27 has a single, variable temperature, blackbody calibration target which is internal to the interferometer enclosure. During typical operation this blackbody is used on a periodic basis, approximately every 2 hours, to provide a nominal radiance calibration for the observations. When in calibration mode an internal mirror is rotated into the beam path bringing the blackbody into the instrument field of view. During the internal calibration the blackbody is first cooled, and a user selectable number of scans are acquired, after which the blackbody is heated, and a similar number of scans are acquired. These two sets of observations can then be applied to external observations to yield radiance estimates. For our scientific goals we desire a verifiable accuracy assessment so use purpose built external blackbody targets (section 2.2) to provide calibration for FINESSE. However, we find it helpful to initiate an internal calibration at the start of the day: this sets the internal calibration target at 343 K providing a thermal heat source for the system in cold environments. Additionally, as described in section 3.5, a comparison of the spectral response functions derived from the external and internal calibration targets is used to derive the frequency dependent instrument line shape.

## 2.2 FINESSE front end scene selection and calibration system


As described above, the standard calibration process of the EM27 does not fully account for the mirror reflectivity and the transmission of any window to the exterior. To account for this and allow more versatility in scene selection we employ a purpose-built external targeting system, with scene selectable view mirror and external blackbody sources.

Figure 1 shows the EM27 and external calibration system during assembly. The steerable mirror at the front of the EM27 input aperture can be rotated through  $360^\circ$ . This allows us to steer the EM27 view towards the hot or ambient temperature blackbody for calibration purposes or towards a target scene at any given angle from zenith through to nadir.

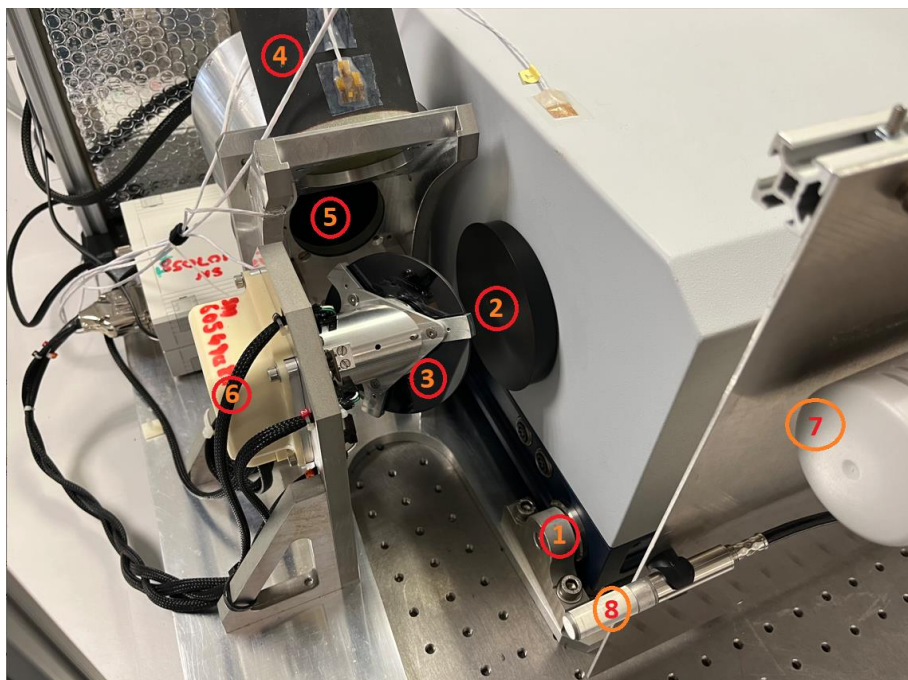

**Figure 1.** Close-up of the front-end pointing and calibration system attached to the EM27. 1: Dowel locator and receptacle. 2: EM27 input window. 3: Steering mirror. 4: Ambient temperature black body. 5: Hot black body. 6: Stepper motor. 7: Vaisala CO<sub>2</sub> monitor and 8: Vaisala Pressure/humidity and temperature sensor.

- 90 The blackbody cavities are fabricated using 80 mm outer diameter copper rod, (Figure 2(A)). The cavities themselves are 80 mm in depth with high emissivity target backplates. The inner cavity is machined to form a cone tapering towards the input aperture so that the wall thickness is 7 mm at the back of the cavity to 9 mm at the front. This design is based on heritage from the Tropospheric Airborne Fourier Transform Spectrometer, which was developed in-house at Imperial College (Canas et al., 1997).

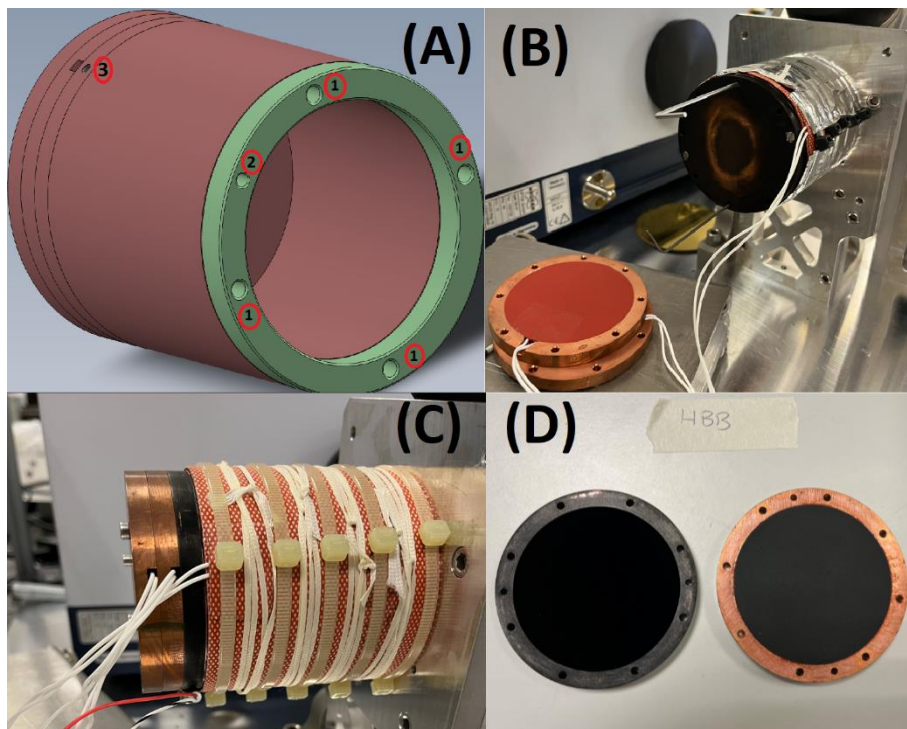

95

100

**Figure 2:** Panel A: Schematic layout of the hot blackbody. The cavity and backplates are machined from 80 mm diameter solid copper rod. The copper cavity is thermally isolated from the mounting frame using a Tufnol isolating ring (green). Holes marked 1 indicate the locations of fixing bolts and the through hole 2 allows a PRT100 temperature sensor to be inserted into the front of the copper cavity, an additional PRT100 is inserted into the backplate, hole 3 and sits central to the backplate disk, 1.5 mm from the disc surface. Panel B: Cavity fixed to the mounting frame. To the lower left are two additional plates which are seen bolted to the target plate in Panel C. Each plate includes a 5 W rubber heater pad whose diameter matches the diameter of the inner target plate emission surface. A 25 W heater is wrapped around the circumference of the cavity wall. Panel D: Target backplates, to the left is a plate coated in Vanta black and to the right a plate coated in Aeroglaze Z306.

105

110

115

To obtain a high effective emissivity the cavity emission surfaces are coated in Aeroglaze Z306 paint (Adibekyan et al., 2017). The backplates sealing the blackbodies are copper discs 7 mm in thickness: in initial testing and for the measurements of de-ionised water described in Part (II) these were also coated in Z306. For the purposes of establishing their performance and also for future use, we acquired a second set of backplates coated with Vanta Black S-IR (Adams et al., 2019). To monitor the blackbody temperature and obtain information regarding any temperature gradient, we use class-A 25 mm x 2.8 mm diameter PRT100 sensors: one is embedded centrally within the backplate disk 1.5 mm from the emission surface and a second is embedded at the front end of the cavity wall (Figure 2(A)). The hot blackbody cavity has an external heater pad mounted around the circumference while the backplates use two compressible circular rubber heater pads, matching the inner surface diameter. These pads are mounted on the far side of the disc and are each gently compressed between successive copper discs to give good thermal contact (Figure 2(C)). The hot blackbody and heaters are insulated and housed in an aluminium case isolating them from ambient conditions. Power to the heater pads is controlled using a TE technology TC-48-20 controller with thermistor feedback, providing a nominal set point for the hot black body temperature of about 343 K. As will be





demonstrated in section 3.2.1, shortly after the set point temperature is reached the stability of this hot black body is better than 0.1 K over periods of hours.

The ambient temperature blackbody is not temperature stabilised and is left exposed to the ambient atmospheric conditions. PRT100 sensors are embedded within the backplate and front of the cavity wall to monitor the emission and cavity wall temperatures. When using FINESSE, we have measurement periods that typically last of the order a few hours. Once the system has stabilised after initial power up, we find that there is a warming trend in the ambient blackbody temperature due to its position relative to the hot blackbody. The magnitude of this trend is dependent on ambient conditions. In the laboratory it is of the order 0.03 K min<sup>-1</sup> increasing to order 0.1 K min<sup>-1</sup> in some deployment environments. These drifts can be accurately accounted for by extrapolation between calibration measurements as needed. Overall, the high thermal mass of the copper body helps to temporally smooth the effects of fluctuations in external conditions.

We typically operate FINESSE at a spectral resolution of 0.5 cm<sup>-1</sup> which translates to a scan time of about 1.5 seconds to acquire a single interferogram. To achieve adequate signal-to-noise while ensuring low impact on the calibration response from changing ambient atmospheric conditions we set the Bruker OPUS instrument control software to acquire 40 individual interferograms for a given target view. The control of all data acquisition, target views and system logging are via a custom-built FINESSE Graphical User Interface (GUI). This GUI connects to the EM27 through the EM27 internal PC web-interface and is used to issue start/stop scan commands. To automate data acquisition, we have created script files which are loaded into the GUI interface and define an observation sequence which is run repetitively for a given number of cycles. Typically, a calibration-observation cycle consists of three target views: a hot blackbody view, an ambient blackbody view and a scene measurement, taking a little over 3 minutes to complete before the cycle is repeated.

### 2.3 Ancillary atmospheric measurements

In order to retrieve emissivity, the influence of the atmospheric path between the detector and the surface needs to be accounted for. To help to constrain conditions along the path ancillary measurements of atmospheric temperature, pressure and relative humidity are provided by a Vaisala PTU300 transmitter (Figure 1). These can also be used to provide context when characterising the instrument spectral response and assessing its stability. Quoted calibration uncertainties are within 0.05 hPa, 1% and 0.1 K, over the ambient ranges typically observed during these observations. A separate Vaisala GMP343 probe is used to monitor CO<sub>2</sub> concentrations (Figure 1).

## 3 FINESSE instrument characteristics and performance

To optimise the retrieval of emissivity from the FINESSE radiance measurements we require the instrument spectral response to either be stable or that any drift in response be slow and measurable over the period of the radiance measurements. We also require knowledge of the FINESSE instrument line shape so that this can be accounted for in the forward modelling of the observed radiances.



The following sections outline our data processing strategy. These steps include the application of spectral phase corrections required to remove instrument self-emission terms that might compromise the radiance calibration. The stability of the spectral response function is evaluated, including the impact of assumptions concerning the calibration blackbody emissivity and temperature. We also look closely at the instrument spectral line shape of the Bruker EM27 which appears to have significant, frequency dependent, line broadening and line asymmetry.

### 3.1 Phase Correction

A thorough explanation of Fourier transforms spectrometry can be found in many textbooks (e.g. Griffiths and De Hasseth 2007). In this paper we limit detail of the application of the Fourier Transform to a simple formulation of the phase function and phase correction of the complex spectra in order to highlight a phase anomaly that impacts the spectra observed by the EM27.

After acquisition of the interferogram the complex Fourier transform (eq. 1),

$$B(\sigma) = \int_{-\infty}^{+\infty} I(x)e^{-2\pi i\sigma x} dx, \quad (1)$$

is used to yield the complex spectrum (eq. 2),

$$B(\sigma) = Re(\sigma) \cos(\theta_\sigma) + Im(\sigma) \sin(\theta_\sigma). \quad (2)$$

Here  $\sigma$  is wavenumber in  $\text{cm}^{-1}$ ,  $x$  optical path difference in cm,  $Re$  and  $Im$  denote the real and imaginary spectral components and  $\theta_\sigma$  the wavenumber dependent phase function.

The phase function is retrieved from a low-resolution complex spectra thus,

$$\theta_\sigma = \arctan \frac{Im(\sigma)}{Re(\sigma)}. \quad (3)$$

This phase function is applied to the full resolution complex spectra, using the method described by Mertz (Mertz, 1965). In routine operations of the EM27 the OPUS control software acquires and stores, amongst additional house-keeping information, individual raw interferograms for each 1.5 second scan, from which the complex spectra are obtained. When deriving the phase functions for individual spectra we found that these phase functions exhibited features consistent with significant self-emission from the EM27. To address this, we follow an approach which properly corrects for an anomalous phase associated with instrument self-emission. To remove the influence of this anomalous phase on the phase function for individual spectra Revercomb et al. (1988) take the difference between two complex spectra, for example the complex spectra associated with the hot and ambient targets, before the phase function is derived and applied. The same authors note that if the instrument interferogram acquisition system is stable between different scene views, differencing the interferograms before applying the phase correction will also correct for the anomalous phase. For the EM27 we find the reproducibility of the sampled interferograms between calibration cycles to be very stable and hence choose to difference the interferograms, thus removing the self-emission term, before transforming and phase correcting.



### 3.2 FINESSE spectral response and spectral response stability

The instrument spectral response converts raw spectral signals to radiance and for FINESSE is derived from measurements of the external calibration targets, thus:


$$180 \quad R(\sigma)_{FIN} = \frac{FFT\{I(x)_{hot} - I(x)_{amb}\}}{[\varepsilon_{eff}(\sigma)B(\sigma, T)_{hot} + (1 - \varepsilon_{eff})L(\sigma)_{hot}^{ext}] - [\varepsilon_{eff}(\sigma)B(\sigma, T)_{amb} + (1 - \varepsilon_{eff})L(\sigma)_{amb}^{ext}]} \quad (4)$$

The numerator is the phase corrected complex spectrum derived from the difference in sequentially measured interferograms for the hot and ambient blackbodies. The denominator is the difference in the radiance signal from the two blackbodies, which comprises their Planckian emission,  $B(\sigma, T)$ , modulated by the cavity effective emissivity,  $\varepsilon_{eff}$ , and the reflected external radiance incident on each cavity,  $L(\sigma)^{ext}$ . If the effective emissivity of the blackbody cavities is assumed to be unity, then the reflected terms disappear, and the denominator relaxes to the difference of two Planck functions.

185 We initially make this simplifying assumption in order to investigate the stability of the FINESSE response function under laboratory conditions. The system was configured to run a series of alternating views between the hot and ambient temperature calibration targets with a 96 second integration time for each target. After powering up, the system was given 60 minutes to stabilise before measurements were initiated and left to run for about 6.5 hours.

190 Figure 3(A) shows the 119 spectral response functions acquired during this period as a function of wavenumber. To provide greater detail, figure 3(B) shows the spectral response in four wavenumber channels, expressed as the percentage difference relative to the channel average spectral response over the entire period. During the first 30 minutes we see that the system is still stabilising, slowly dropping to a stable behaviour from about 2 % above the average. After this initial 30 minutes the stability at  $500 \text{ cm}^{-1}$ ,  $900 \text{ cm}^{-1}$  and  $1200 \text{ cm}^{-1}$ , is within 0.2 % of the mean response after stabilisation. It is even possible to see when the detector dewar, housing the liquid nitrogen coolant, was topped up at 15:30 UTC. Given its proximity to the detector band edge the  $410 \text{ cm}^{-1}$  channel is noisier as expected. This channel also has a discernible trend after the initial stabilisation period, with a decrease in spectral response, from 1 % above the mean to 1% below. This may reflect changing atmospheric conditions (Figure 3(C)) to which the  $410 \text{ cm}^{-1}$  channel will be more susceptible. However, away from the detector band edges the stability of the FINESSE system spectral response appears excellent.



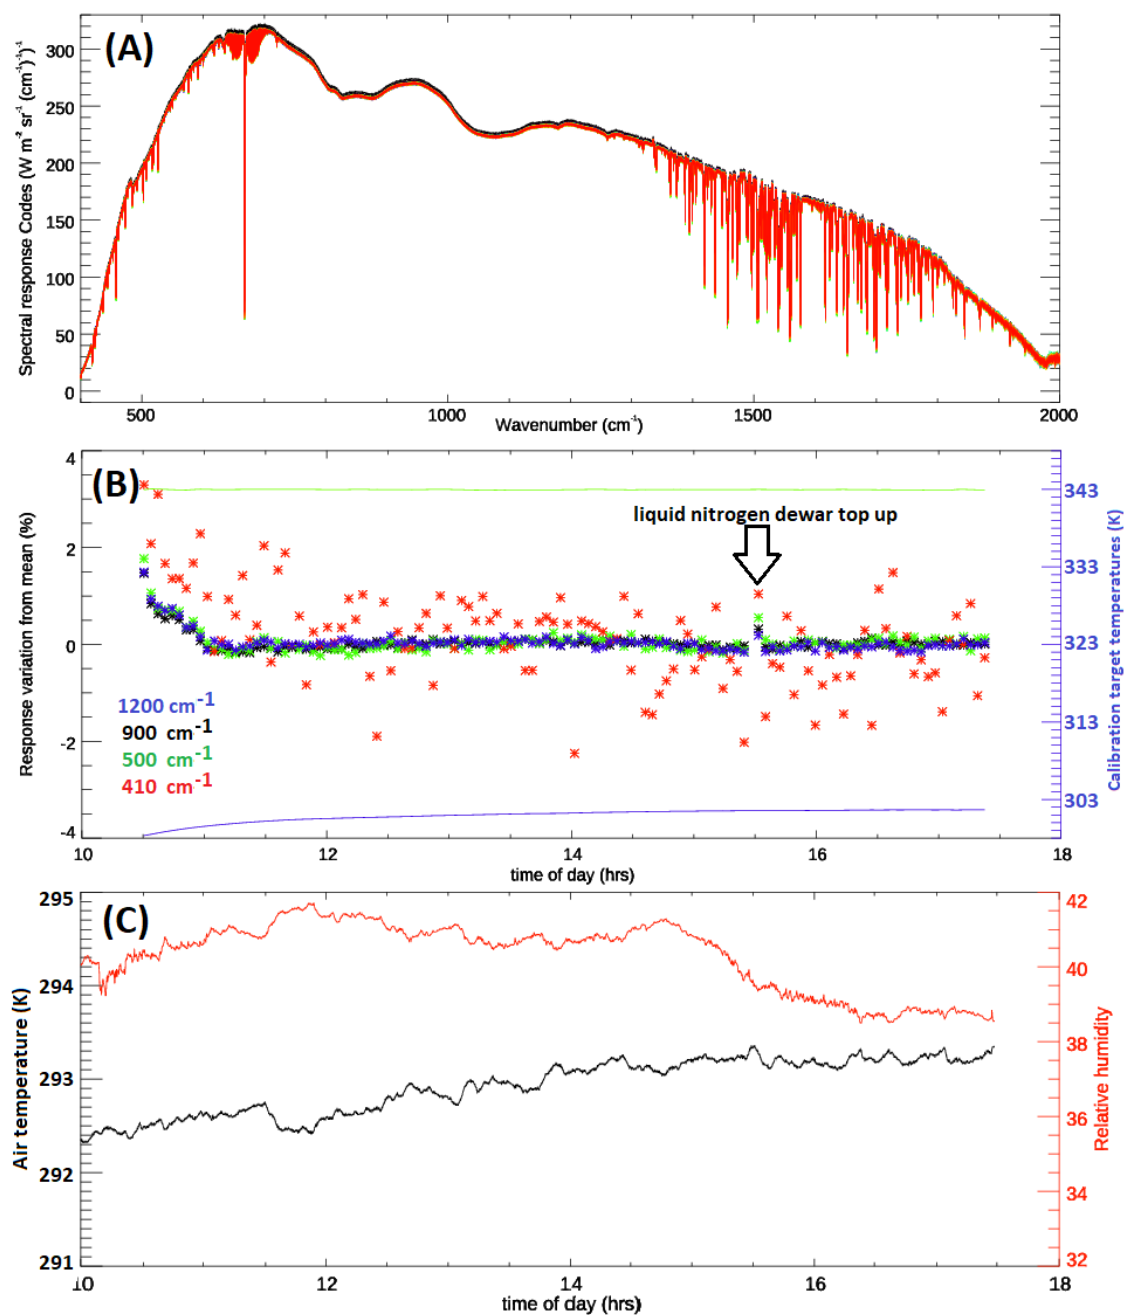

200

Figure 3. Panel A: FINESSE spectral gain function, 119 measurements, from black to red over 6.5 hours. Panel B: Gain variance with time for four spectral channels. These channels have width 4  $\text{cm}^{-1}$  and are centred on 1200  $\text{cm}^{-1}$ , 900  $\text{cm}^{-1}$ , 500  $\text{cm}^{-1}$  and 410  $\text{cm}^{-1}$ . The green and purple solid lines show the hot and ambient blackbody temperatures. Panel C shows the ambient atmospheric conditions in the laboratory during the extended measurements period.



### 205 3.3 Blackbody emissivity estimates


The FINESSE blackbodies use a simple cavity geometry with a relatively low aperture-to-length aspect ratio to isolate the target backplate emission in the field-of-view of the instrument from the external radiance field beyond the blackbody aperture. Typically, cavities are held at the same temperature as the backplate and are designed such that rays entering the cavity undergo multiple internal reflections before being reflected into the field-of-view of the spectrometer. These multiple reflections  
 210 compensate for coatings with relatively low emissivity and enhance the effective emissivity of the BB target.

As noted earlier, in our first iteration of blackbody design, both the cavity walls and the backplates of the FINESSE blackbodies are coated in Aeroglaze Z306, which has a measured emissivity of between 0.9 and 0.97 dependent on wavenumber and temperature. The emissivity temperature dependence shown in previously published data suggests an increase in emissivity of about 5 % between 298 K and 423 K for a surface coated in Z306 (Adibekyan et al., 2017). Linearly interpolating these  
 215 published emissivity curves for Z306 with temperature to the FINESSE blackbody temperatures of 300 and 343 K gives an anticipated difference in spectral emissivity between the blackbodies of less than 2 % (Figure 4(E)).

Vantablack S-IR coatings have measured emissivities in excess of 0.997 at wavenumbers greater than 700 cm<sup>-1</sup> (Adams et al., 2019) with no known emissivity temperature dependence. The choice of a Vantablack coated blackbody is therefore theoretically preferable over one coated in Z306 and so, in a second iteration of the blackbodies, we coated both backplates  
 220 with Vantablack S-IR. However due to the fragility of Vantablack and the difficulty in coating the inner surface of the cavity it was decided to retain the Z306 cavity coating. We make the assumption that the high emissivity of the Vantablack coated backplate within the cavity housing will provide an effective emissivity not measurably discernible from unity for the FINESSE setup.

The measurements described in Part (II) use the fully Z306 coated blackbodies. To derive an upper limit for the effective  
 225 emissivity of the blackbodies coated wholly in Z306 we compare the spectral response of the two blackbody configurations. Specifically, we measure the instrument spectral response over 2-hour periods for each backplate type and undertake a comparison through the ratio of these responses, as shown in equation 5. We note that as the geometries of the hot and ambient blackbodies are the same, the reflected components, included in equation 4, will effectively cancel. For the full Z306 case, this assumes that the temperature induced emissivity difference of 2% will be adequately mitigated by the cavity  
 230 effect.

$$\frac{R(\sigma)_{FIN}^{Z306}}{R(\sigma)_{FIN}^{Vanta}} = \frac{FFT\{I(x)_{hot}^{Z306} - I(x)_{amb}^{Z306}\} e_{eff}^{Vanta}(L(\sigma, T)_{hot}^{Vanta} - L(\sigma, T)_{amb}^{Vanta})}{FFT\{I(x)_{hot}^{Vanta} - I(x)_{amb}^{Vanta}\} e_{eff}^{Z306}(L(\sigma, T)_{hot}^{Z306} - L(\sigma, T)_{amb}^{Z306})}. \quad (5)$$

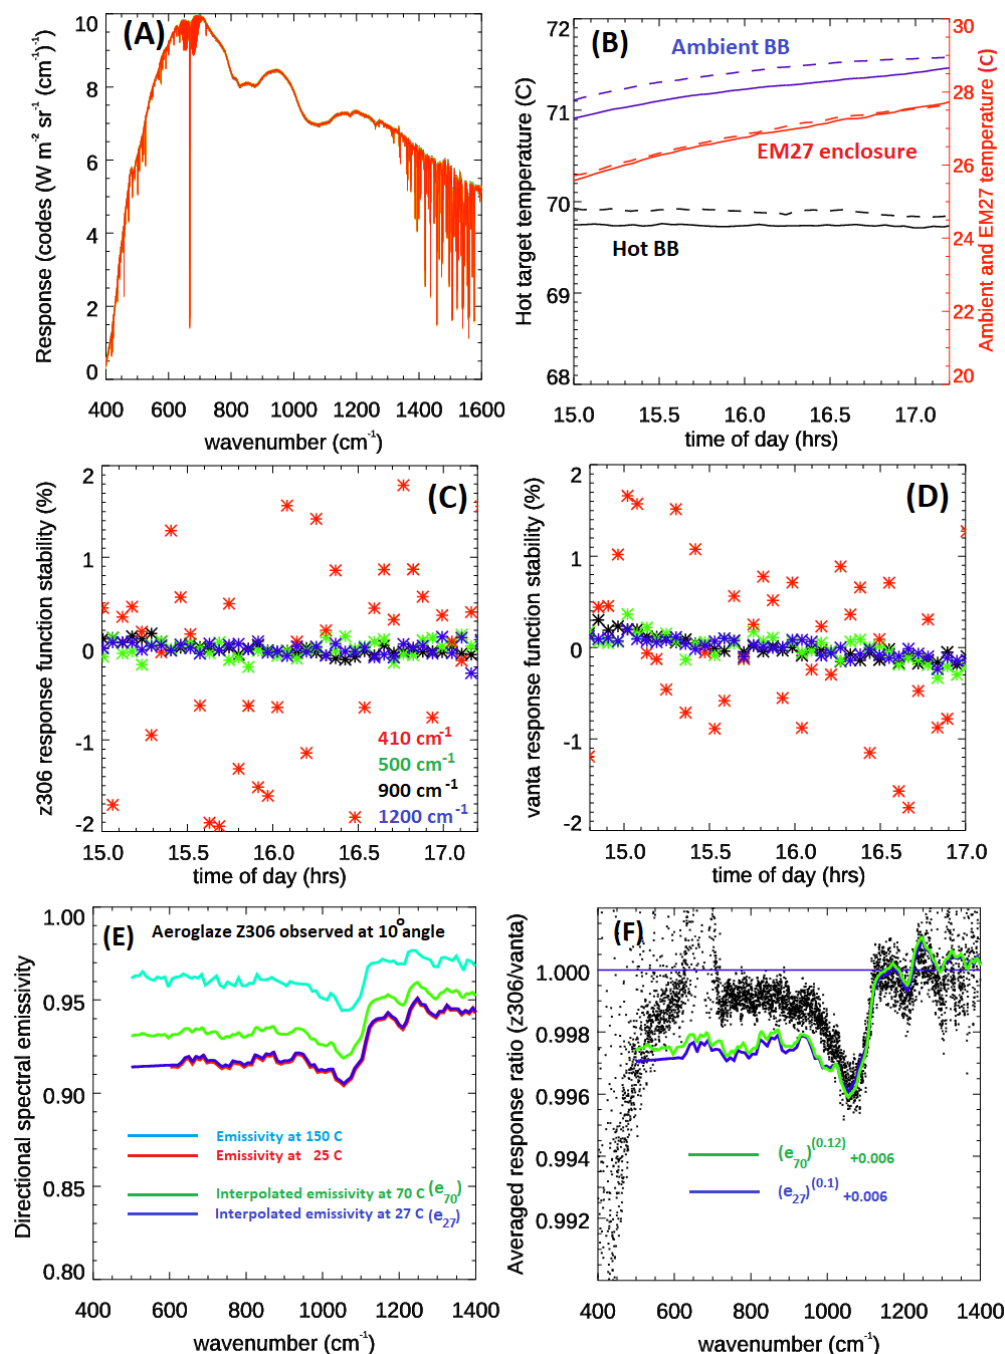

235

Figure 4(A) 40 spectral response functions obtained using the full Z306 blackbodies (Z306 case). (B) Temperatures of the blackbodies and EM27 enclosure during the response function measurements: solid lines correspond to Z306 case, dashed lines: Vanta case. (C) Response function as a function of time in 4 selected wavenumber channels for the Z306 case. (D) As (C) for Vanta case. (E) Emissivity measurements at 10° view angle for Z306 for surface temperatures of 298 and 423 K (Adibekyan et al., 2017) and interpolated emissivities for temperatures associated with the FINESSE blackbodies. (F) Ratio of Z306 to Vanta spectral response. Fitted lines show the power relationships required to best match the interpolated emissivities shown in (E) to the step in the ratio between 1050  $\text{cm}^{-1}$  and 1150  $\text{cm}^{-1}$ .



240 For both sets of observations FINESSE was allowed to stabilise for the same time and the measurements were started with both hot and ambient blackbodies at similar temperatures (Figure 4(B)). In both cases FINESSE was configured to run a series of alternating views of 96 s duration between the hot and ambient temperature calibration targets. Figure 4(A) displays the 40 spectral responses using the wholly Z306 set-up acquired over this time. Panels C and D show the stability of the spectral response function in 4 selected narrow band channels of  $4\text{ cm}^{-1}$  width centred on  $410\text{ cm}^{-1}$ ,  $500\text{ cm}^{-1}$ ,  $900\text{ cm}^{-1}$  and  $1200\text{ cm}^{-1}$ .  
245 The stability of the response function during the Z306 backplate measurements is compatible with that shown in Figure 3, within 0.2% of the mean for the  $500\text{ cm}^{-1}$ ,  $900\text{ cm}^{-1}$  and  $1200\text{ cm}^{-1}$  channels, with a small negative trend over the measurement period of about 0.1% (Fig. 4(C)). Similar to Fig. 3(B) the  $410\text{ cm}^{-1}$  band shows a much higher scatter associated with higher noise at the edges of the detector response, accompanied by a slight increase over the 2-hour period. For the Vanta backplate case, similar behaviour is seen in the  $500\text{ cm}^{-1}$ ,  $900\text{ cm}^{-1}$  and  $1200\text{ cm}^{-1}$  channels, with all showing a small negative drift in the  
250 response function of about 0.4 % over the 2-hour period. The scatter in the  $410\text{ cm}^{-1}$  channel for the Vanta case is significantly less than that seen for the Z306 measurement but there is a decrease in the relative response with time. Overall, the stability of the system is demonstrably excellent across much of the FINESSE spectral range allowing us to estimate the effectiveness of the cavity using the known spectral structure of Z306.

Our comparison of the Z306 and Vanta spectral response functions is shown in Figure 4(F). The spectral behaviour outside of  
255 regions of strong atmospheric absorption from water vapour and  $\text{CO}_2$  shows a clear signature related to the spectral emissivity of Z306. To highlight this, we have applied a power relationship and offset to the interpolated Z306 emissivities shown in panel 4(E), to match the step seen between  $1050\text{ cm}^{-1}$  and  $1150\text{ cm}^{-1}$  in the spectral response ratio. The step in our interpolated emissivity is 0.04 at 300 K and 0.03 at 343 K while the equivalent step in the FINESSE spectral response ratio is 0.004 (Fig. 4(F)), a significant improvement suggesting a cavity enhancement of order 8.

260 Direct comparison of the ratio between the Z306 and Vantablack cases shown in figure 4(F) would suggest an effective emissivity for the cavities with Z306 coated backplates of better than 0.998 across the majority of the FINESSE spectral range, excluding the band between  $1050\text{ cm}^{-1}$  and  $1150\text{ cm}^{-1}$  where the values drop to a minimum of 0.996. Between  $400\text{ cm}^{-1}$  and  $500\text{ cm}^{-1}$ , we see a large divergence in the response function ratio. This is most likely due to the proximity of these wavelengths to the detector band edge combined with the effect of drifts in the ambient atmospheric state. For our analysis and calibration  
265 purposes we use the inferred emissivity of 0.998 at  $500\text{ cm}^{-1}$  at lower wavenumbers.

We expect that the 0.4 % drift we see in spectral response for the Vanta case (Fig. 4(D)) coupled with our assumption that, for the Z306 case, the reflected radiance signal from the ambient and hot blackbodies cancels, will introduce some uncertainty on our effective emissivity estimate. Treating the 0.4 % drift as an uncertainty and adding, in quadrature, a 0.25 % uncertainty to account for the 2 % emissivity off-set for the Z306 targets at 300 K and 343 K, we estimate an overall uncertainty in the  
270 effective emissivity of 0.005.



### 3.4 Knowledge of BB emission temperature

275 There are three sources of temperature uncertainty associated with the knowledge of the backplate surface emission temperature. These are the absolute uncertainty of the PRT100 sensors embedded in the backplate and cavity wall, the temperature gradient between the PRT100 backplate sensor and the surface emission temperature, and the spatial uniformity of temperature across the emission surface.

#### 3.4.1 PRT100 sensor uncertainty

The PRT100 sensors used to monitor the blackbody temperatures, as shown in figure 2, are 4-wire Din Class A PRT100 sensors, from Omega, with tolerances of  $\pm 0.15^\circ\text{C}$  (at  $0^\circ\text{C} + 0.002|T|$ ) where T is the temperature of the body being measured. For ambient and hot blackbody temperatures of 300 K and 343 K these tolerances equate to  $\pm 0.20$  K and  $\pm 0.29$  K respectively.


#### 280 3.4.2 Blackbody temperature uniformity across the aperture plane

To evaluate the uniformity of the hot blackbody temperature in the field of view of FINESSE we used a FLIR E8-XT thermal imaging camera. These cameras employ a 320 x 240 vanadium oxide microbolometer sensor array covering a field of view of  $45^\circ \times 34^\circ$ , with a sensitivity of 0.05 K over the thermal range 253 to 823 K and a quoted absolute uncertainty of  $\pm 0.7$  K. The camera band pass covers the spectral range 7.5  $\mu\text{m}$  to 13  $\mu\text{m}$  minimising the impact on measured temperature of the intervening atmosphere between sensor and source. Although the camera temperature uncertainty is relatively poor, its sensitivity allows us to obtain measurements of the temperature spatial uniformity across the FINESSE blackbody aperture.

285 We note that the E8-XT sensor is un-cooled and that variations in sensor temperature will impact the pixel sensitivity, so we undertake all uniformity measurements within a short period of time with the camera temperature stable to within 0.1 K. After start-up the camera takes some time to stabilise and while doing so performs automated non-uniform-corrections (NUCs) (Wan, 2021) at irregular intervals, placing a shutter in the field of view and applying individual pixel corrections to the image assuming the shutter thermal signal is uniform. The frequency of the NUCs decreases with time so we allowed a minimum of 60 minutes stabilisation after powering up the camera before taking measurements to minimise their impact.

To allow for residual non-uniformity in the camera response and/or non-uniformity introduced by the internal shutter itself, we took measurements of the blackbodies with the camera initially in an inverted and then an upright orientation (Fig. 295 5(A),(B)). For each orientation the centre of the image array was aligned normal to, and centred on, the blackbody aperture. After the initial stabilisation period, 100 consecutive images of the FINESSE hot black body were taken, with roughly 4 seconds between images. The camera records JPEG files containing the measured thermogram, proportional to the detected radiance signal, visible image data and associated metadata. We extracted the thermogram as an array of pixel values, accessing the metadata to convert these to an array of temperature values. The thermogram to temperature conversion routine allows for in-camera correction factors associated with the ambient atmospheric conditions and target emissivity. As the camera was 300 placed within 150 mm of the cavity aperture atmospheric corrections were switched off and the target emissivity was set to 1.



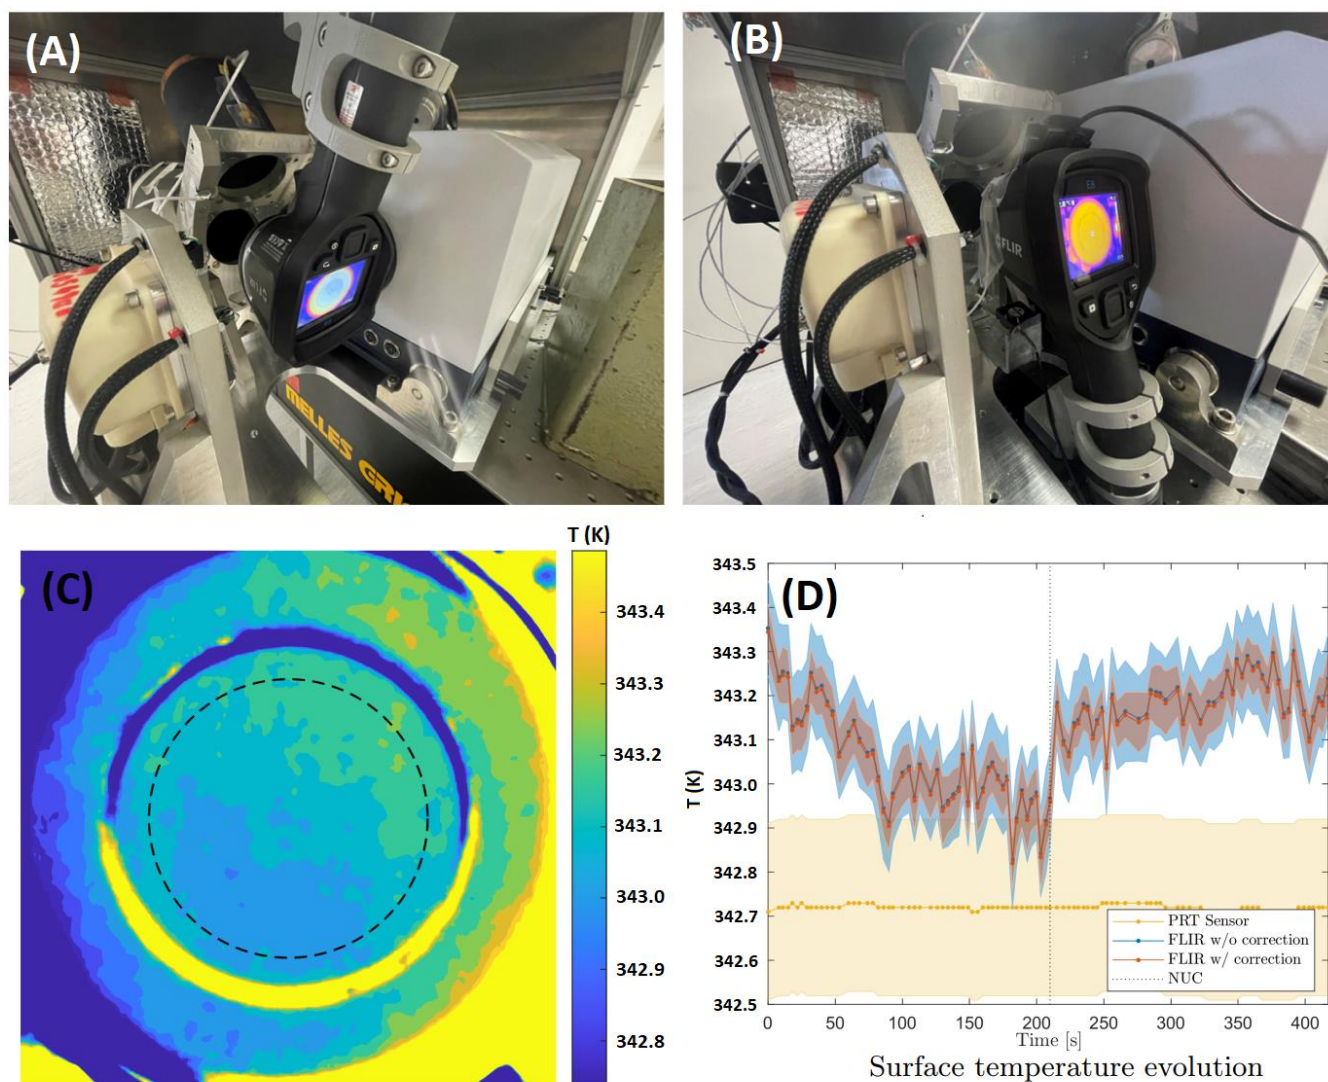

305

**Figure 5: Inverted (A) and Upright (B) orientation for the FLIR E8 XT camera measurements used to estimate the spatial uniformity of the hot blackbody. (C) Temperature spatial uniformity measured from camera orientation (B) after correction for camera non-uniformity derived from measurements using camera orientation (A). The circle indicated by the dashed line represents the spatial extent of the FINESSSE field of view in the plane of the blackbody backplate. (D) Camera mean temperature and rms spread for the 100 thermograms obtained over a period of 420 seconds. PRT values are from the sensor embedded within the hot blackbody backplate, 1.5 mm from the emission surface.**

310

Temperature observations for each individual pixel were averaged over the 100 thermograms taken in the inverted orientation when viewing the hot blackbody at 343 K. The average of all pixels within the field of view of FINESSSE, defined by the dashed circle in Figure 5(C), was then calculated to obtain a reference ‘field of view integrated’ or ‘camera mean’ temperature. This reference temperature was subtracted from the temporally averaged temperature array to derive a pixel dependent correction off-set. The off-set was then applied to the temperature measurements of the blackbody with the camera in the upright orientation. Fig. 5(C) shows a temperature corrected thermal image of the hot blackbody with the camera in the upright





315 position. The maximum temperature range within the FINESSE field of view is about 0.3 K. We assess the effectiveness of  
the correction factor by plotting the camera mean temperature and associated rms for each temperature array, with and without  
correction. These values are plotted in Figure 5(D). The camera mean temperature shows no significant change but the rms  
has reduced from about 0.1 K to 0.05 K.

### 3.4.3 Blackbody surface emission temperature

320 Uncertainty in the knowledge of the blackbody surface emission temperature makes the largest contribution to the radiance  
uncertainty in our calibration. Both the hot and ambient blackbody emission temperatures are derived using the temperature  
measurement of the PRT100 sensors embedded within the backplate, 1.5 mm from the emission surface. In the case of the  
ambient blackbody, which has no associated heating, the PRT sensor measurement is used as our surface emission temperature  
with an uncertainty as defined by the tolerance described in section 3.4.1. For reference, with the hot blackbody at an ambient  
325 room temperature of 305.4 K we see an offset between the mean E8-XT camera temperature and backplate PRT100  
temperature measurement of about -0.2 K, the PRT sensor indicating a higher temperature. Fig.5(D) indicates a +0.5 K offset  
for the blackbody at 343 K, with the E8-XT camera now indicating a higher temperature. Using similar observations between  
known blackbody temperatures against an E8-XT camera (Wan et al., 2021) report E8-XT offsets of +1 K and +2 K for target  
temperatures of 308 K and 328 K, respectively, suggesting a rate of change in temperature off-set of  $0.05 \text{ K K}^{-1}$  over this range.  
330 This temperature dependent off-set is also likely to be camera dependent and means we cannot use the E8-XT camera to  
directly evaluate the emission temperature of our hot black body.

We note that, given the position of the backplate PRT100 between heaters and emission surface, we expect the PRT100  
temperature reading to be higher than the surface emission temperature. Typically, we observe temperature gradients of  
between +1.2 K and +1.6 K between the PRT100s embedded in the front cavity wall and the backplate. The latter is always  
335 higher in temperature and this temperature difference is dependent on the ambient atmospheric conditions. We currently use  
the mean temperature between the front and rear PRT100 readings for our surface emission temperature. This approach to  
establishing the surface emission temperature will be further refined in future: our PRT measurements imply that the current  
methodology introduces an additional uncertainty of 0.3 K in emission temperature, giving an overall uncertainty of 0.43 K.

### 3.5 Instrument Line shape

340 The instrument line shape (ILS) is an important parameter required for the simulation, analysis and interpretation of  
atmospheric radiative measurements. Previous efforts to determine the ILS of instruments in the EM27 family have indicated  
that the line-shape can be broadened due to self-apodisation and can also have a notable asymmetry (e.g. Frey et al., 2015,  
Alberti et al., 2022). Initial inspection of the radiance spectra also suggests that this is the case for FINESSE, so we use the  
approaches described by Bianchini et al. (2019) and Genest and Trembley (1999) to model the self-apodisation and asymmetric  
345 components, respectively.



To assess self-apodisation, we concentrate on the impact of the finite solid angle of the radiation propagating through the interferometer broadening the ILS. As described by Bianchini et al. (2019) the impact of the finite solid angle is to broaden and shift spectral lines by convolving the ideal ILS, given by  $\text{sinc}(2\pi\sigma z_{max})$ , by a wavenumber dependent box function extending from 0 to  $\sigma_0\Omega/2\pi$  in the wavenumber domain. Here  $z_{max}$  is the maximum optical path,  $\sigma_0$  is the spectral line centre and  $\Omega$  is the finite solid angle.

In the spatial domain this equates to an additional apodisation function which multiplies the boxcar apodisation imposed by the finite scan length of  $\pm z_{max}$ . What confounds the application of this additional apodisation over an extended spectrum is its frequency dependence. This makes an exact treatment problematic. Bianchini et al. (2019) indicate that if the solid angle contribution to the ILS is small, ( $\pi/\sigma_0\Omega \gg z_{max}$ ), the apodisation can be treated as a linear combination of a boxcar and a triangle function with coefficients  $\alpha$  and  $(1 - \alpha)$  respectively, where  $\alpha = \text{sinc}(z_{max}\sigma_0\Omega/2)$ . Using this approach, the self-apodisation ILS,  $ILS(\sigma)_{sa}$ , applied to FINESSE is then determined by the following equation:

$$ILS(\sigma)_{sa} = \alpha \text{sinc}(2\pi(\Delta\sigma)\sigma) + (1 - \alpha)\text{sinc}^2(\pi(\Delta\sigma)\sigma), \quad (6)$$

where  $\Delta\sigma$  is the instrument resolution, which we set to  $0.5 \text{ cm}^{-1}$ .

To simulate the wavenumber dependent asymmetric line shape observed in the FINESSE spectra, ( $ILS_{asy}(\sigma)$ ), we make use of the geometric description of line asymmetry by Genest and Trembley (1999) for an off-axis circular detector:


$$ILS_{asy}(\sigma) = \frac{1}{\pi} \arccos \left( \frac{r_c^2 + f^2 \left[ \left( \frac{\sigma_0}{\sigma} \right)^2 - 1 \right] - R^2}{2r_c f \left[ \left( \frac{\sigma_0}{\sigma} \right)^2 - 1 \right]^{\frac{1}{2}}} \right). \quad (7)$$

Here  $R$  is the detector element radius,  $f$  the detector optics focal length (3.3 cm) and  $r_c$  the detector spatial offset from the optical axis. We define the ILS using a normalised wavenumber scale from 0 to  $100 \text{ cm}^{-1}$  on a sampling grid of  $0.001 \text{ cm}^{-1}$  and centred on a nominal frequency,  $\sigma_0$  of  $50 \text{ cm}^{-1}$ . Although this is not a true representation of the EM27 optical system, which employs a square detector of area  $1 \text{ mm}^2$ , it does allow us to simulate the observed frequency dependent asymmetry using equation 7 by increasing  $r_c$ , the optical axis-to-detector element offset. We reference all dimensions relative to  $f$ . With  $R$  set to  $0.005f$ , which suggests the source is underfilling the detector, we find that varying  $r_c$  between  $0.005f$  to  $0.012f$  over the spectral range  $400 \text{ cm}^{-1}$  to  $1600 \text{ cm}^{-1}$  gives a reasonable fit to the observed asymmetry. This manifests in the spectra as a slight shift of the line centre towards lower wavenumbers and a low wavenumber foot evident at the base of the line, as one might expect from the asymmetry components shown in figure 9A. The wavenumber dependent shift in  $r_c$  indicates that there may be some optical induced dispersion of the beam, possibly in the beam-splitter or the window of the detector housing.

We determine the ILS for FINESSE using water vapour absorption lines in the region  $400 \text{ cm}^{-1} - 500 \text{ cm}^{-1}$  and  $1300 \text{ cm}^{-1} - 1600 \text{ cm}^{-1}$ . Specifically, we compare the measured to simulated transmittance of the air-path between the FINESSE diamond window and blackbodies. Measured transmittances are derived from the set of external calibration measurements described earlier and shown in figure 3, which are compared to equivalent measurements of the internal calibration target, obtained under similar instrument environmental conditions. The average instrument spectral responses for both these sets of measurements



are shown in figure 6(A). The spectral response derived from the internal target is considerably higher than that derived from the external targets due to reflection and transmission losses of the diamond window. We ratio the two responses, allowing for these losses, to obtain an ‘apparent’ transmission spectrum for the path between the diamond window and external black bodies (Figure 6(B)). The relative humidity within the spectrometer was approximately 2% for both sets of measurements and the associated absorption is assumed to cancel in the ratio.

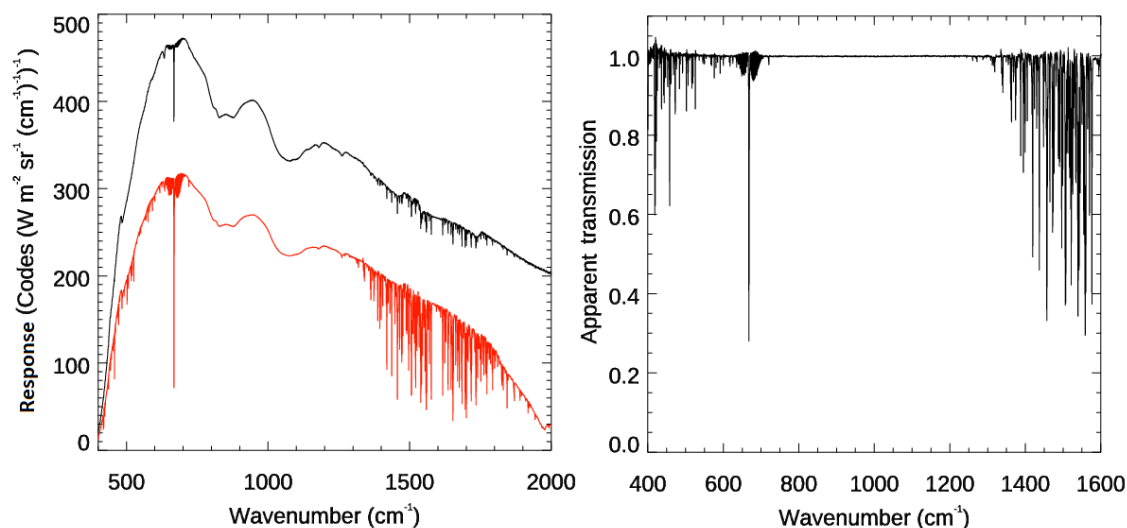


385 **Figure 6. A: The instrument spectral responses derived using the internal blackbody (black) and external FINESSE calibration targets (red). B: “Apparent” external air-path transmission between the FINESSE calibration targets and EM27 input window derived by taking the ratio of the spectral response curves allowing for the transmission losses in the diamond window transmission (0.675) and an estimate of absorption due to the diamond phonon absorption (Bennet, 2014) towards 1600  $\text{cm}^{-1}$ .**

Simulated transmittances are obtained from radiative transfer modelling, using the average humidity, temperature and pressure observed over the measurement period (Figures 3(C) and (D)) as input to LBLRTM V12.13 (Clough et al., 2005). These ‘ideal’ values then need to be modified by the FINESSE ILS: this modification is performed iteratively for different values of  $\text{ILS}_{\text{sa}}$  and  $\text{ILS}_{\text{asy}}$ , with the optimal ILS chosen as that which minimises the residual between the measured and simulated transmittances in the vicinity of spectral absorption features.

To deduce the optimal ILS we consider thirteen frequency bins, of varying width, starting from  $400 \text{ cm}^{-1}$  and extending to  $1600 \text{ cm}^{-1}$ . For increasing wavenumber (increasing bin number) a series of asymmetric ILS components are calculated using equation 7 by increasing the initial  $r_c$  offset chosen for the  $400 \text{ cm}^{-1}$  bin in equal steps up to the  $1600 \text{ cm}^{-1}$  bin. This is equivalent to a frequency dependent misalignment between the detector and optical axis which, if it is the cause of the asymmetry, suggests an optical component is causing dispersion. This results in an increasing asymmetry with wavenumber. A set of asymmetry arrays, consisting of an asymmetric component, can then be calculated for each wavenumber bin by modifying the initial  $r_c$  offset and rate of change of  $r_c$ .



400 Separately to this we generate an equivalent set of arrays which consist of the self apodisation ILS components for each wavenumber bin. Each array is obtained by fixing the solid angle, calculating the equivalent alpha terms and generating  $ILS(s)_{sa}$  according to equation 6. A set of these self-broadened ILS arrays is generated by adjusting the solid angle between arrays. The asymmetric and self-apodised ILS arrays are then convolved for each wavenumber bin and applied to the simulated transmission. When optimising the ILS convolved simulation with the observations we also need to adjust the observations for  
405 slight optical alignment offsets between the metrology sampling laser and the mid-infrared optical axis. An optical misalignment results in a scaling of the sampling interval which to first order is constant in  $d\sigma/\sigma$ , where  $d\sigma$  is the wavenumber offset at a given wavenumber. We find a frequency scaling of 1.00016 adequately corrects the FINESSE observations. The entire ILS determination process is summarised in Figure 7.

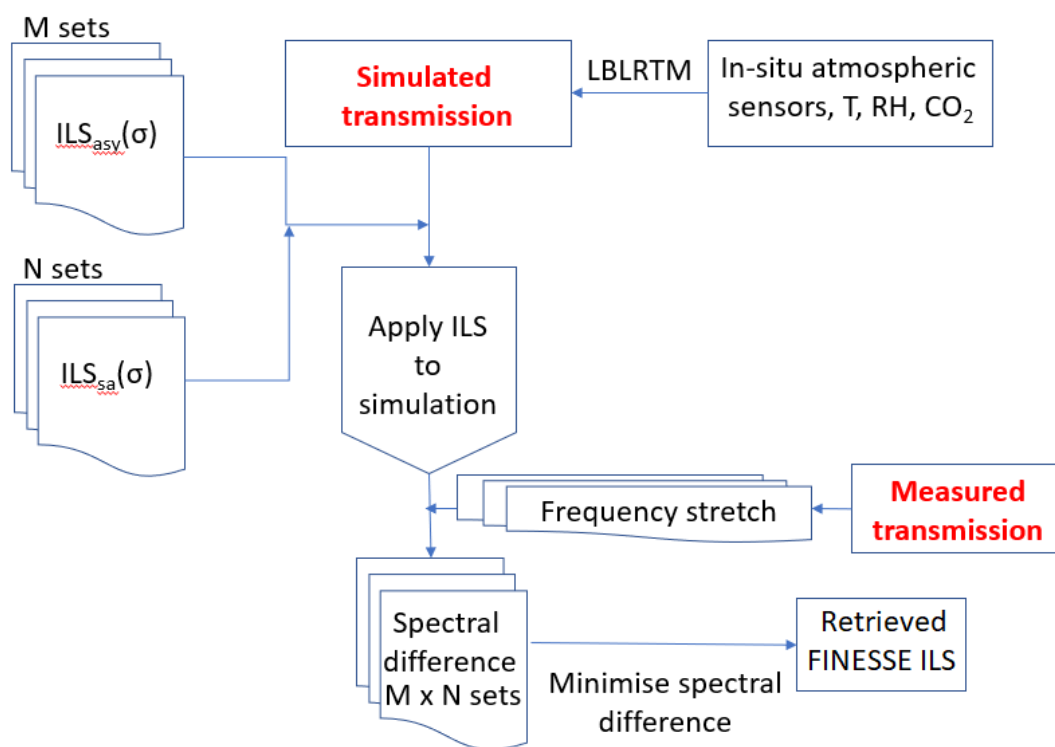

410 **Figure 7: Flowchart showing the retrieval method for the FINESSE ILS**

Figure 8(A) shows the apparent transmission over-plotted by the simulated transmission after the optimal ILS has been applied. Differences, in blue, are less than 1% below  $500\text{ cm}^{-1}$  and of order 2% towards  $1600\text{ cm}^{-1}$ . Panels B and C highlight regions of strong water vapour absorption where the largest residuals are seen. Figures 9(A) and 9(B) show the  $ILS_{asy}$  (equation 7) and alpha values (equation 6) that lead to the optimal ILS. This optimal ILS (Fig. 9(C)) clearly has a strong frequency  
415 dependent asymmetry and a self-apodisation component which also depends on wavenumber.

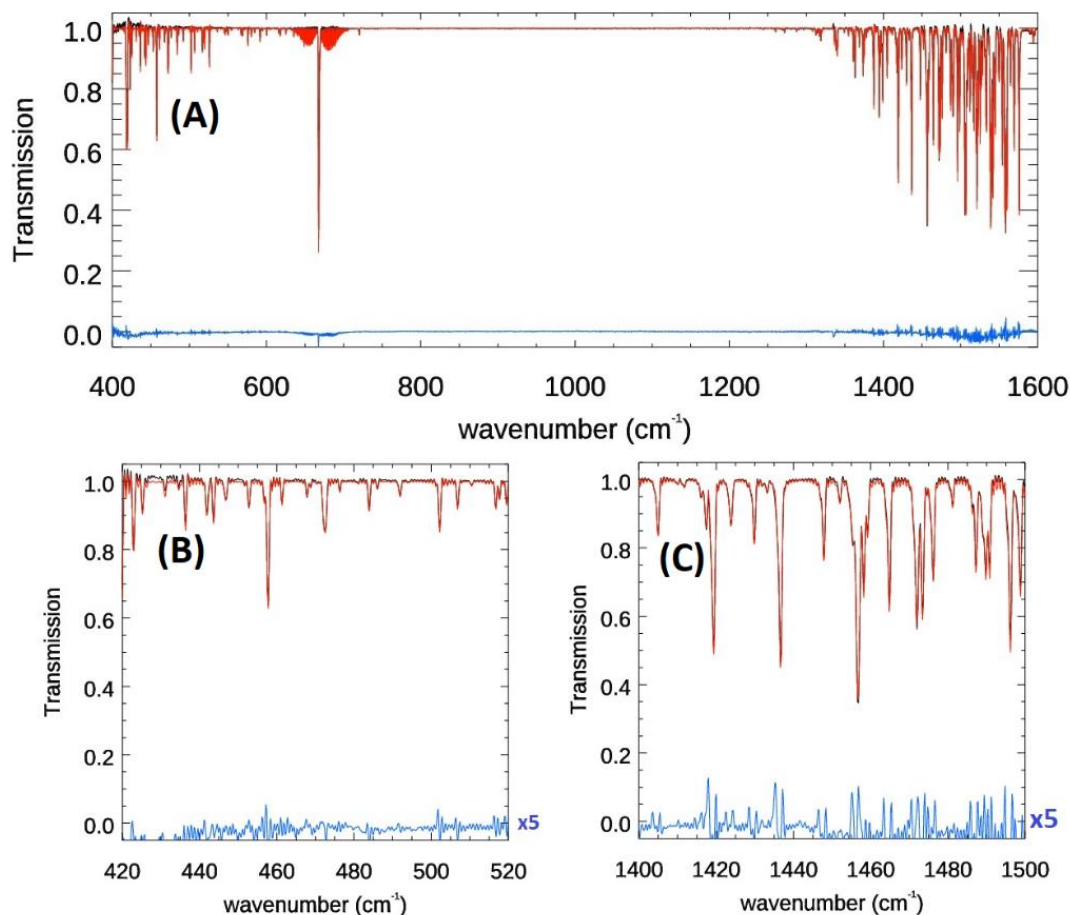


Figure 8(A): Observed atmospheric transmission (black), simulated transmission (red) and residual between the two (blue) for the optimal FINESSE ILS. Panels (B) and (C) highlight the two water vapour absorption regions used to minimise the residuals. The residuals have been scaled by a factor of 5 to allow them to be distinguished.

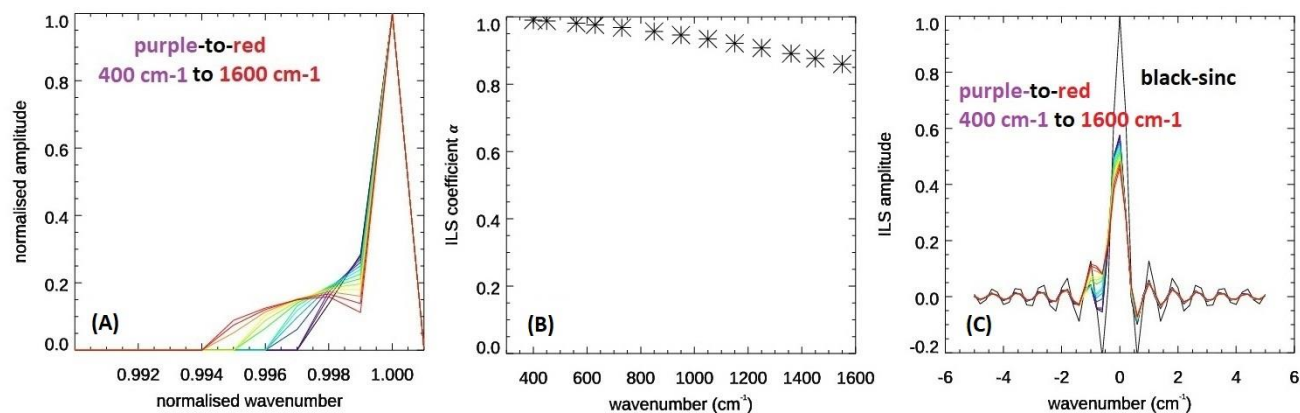


Figure 9(A): The asymmetric component of the ILS defined by equation 7, plotted as an ILS for increasing frequency. (B): The FINESSE alpha scaling value, used in equation 6, that best represents the observed ILS self-apodisation and is equivalent to a solid angle of 0.001 sr. (C): the best fit ILS, derived from a combination of asymmetry and self-broadening terms.

420



#### 4 Calibration and radiance uncertainties: application to clear-sky observations

425 To illustrate FINESSE performance, we highlight zenith view observations made from Imperial College London on 23<sup>rd</sup> March  
2022 from 0900-1300 UTC. Examples of calibrated radiances,  $L(\sigma)_{scene}$ , are shown in figure 10. These radiances are derived  
using equation 8, where the variables are as defined in equation 4 and  $I(x)_{scene}$  is the acquired interferogram for the given  
scene.

$$L(\sigma)_{scene} = [\varepsilon_{eff}(\sigma)B(\sigma, T)_{hot} + (1 - \varepsilon_{eff})L(\sigma)_{hot}^{ext}] - \frac{FFT\{I(x)_{hot} - I(x)_{scene}\}}{R(\sigma)_{FIN}}. \quad (8)$$


430  $R(\sigma)_{FIN}$  is derived from calibration observations taken before and after the scene views. Typically, we set the observation  
cycle to undertake 1 minute of measurements of the hot BB followed by 1 minute of ambient blackbody views. Dependent on  
the instrument stability and requirements for the experiment we can vary the scene view measurement period from 1 minute  
to 4 minutes. During this scene view period, we may repeat a given view angle or vary the view angle to undertake surface  
and sky view measurements: regardless these data are acquired in sets of 1-minute periods.

435 When deriving the uncertainties on the FINESSE calibrated radiances we differentiate between spectrally correlated and  
uncorrelated components. This is important as spectrally uncorrelated detector noise, which we refer to as noise equivalent  
spectral radiance (NESR), can be reduced through spectral or temporal averaging, whereas, for instance, the uncertainty on the  
calibrated radiances, due to knowledge of the absolute temperature of the PRT100 sensors, is fixed for a given observational  
setup and will yield a spectrally correlated shift in the calibrated radiance which cannot be reduced through averaging.

440 It should be noted that if the temperature of the hot calibration target,  $T_{hot}$ , which appears in the first term on the right-hand  
side of Eq. 8, is greater than the “true” emission temperature,  $\Delta T_{hot} > 0$ , then this term will introduce a positive radiance offset.  
However, the response function,  $R(\sigma)_{FIN}$ , also uses  $T_{hot}$  and decreases for  $\Delta T_{hot} > 0$  (Eq. 4). The last term in Eq. 8 will  
therefore, also increase with increasing  $\Delta T_{hot}$  and acts to help compensate for the first term. Similarly, any offset in the effective  
emissivity relative to the ‘true’ emissivity will see some compensation between the first and third terms of Eq. 8. Uncertainty  
445 on the ambient blackbody temperature,  $T_{amb}$ , impacts the spectral response function only so, for this variable, there are no  
compensating terms. However, as this ambient blackbody has high thermal mass and no heating sources, we expect no  
significant thermal gradients between the PRT100 and emission surface. We therefore combine the uncertainty associated  
with the PRT100 itself with knowledge of the small thermal drift observed during the calibration scans, to estimate the  
uncertainty in  $T_{amb}$ .

450 Any observed external radiance seen in reflection from the hot blackbody, which is included as the second term on the right-  
hand side of Eq. 8, can be mitigated for by increasing the effective emissivity of the calibration target as discussed in section  
3.3.



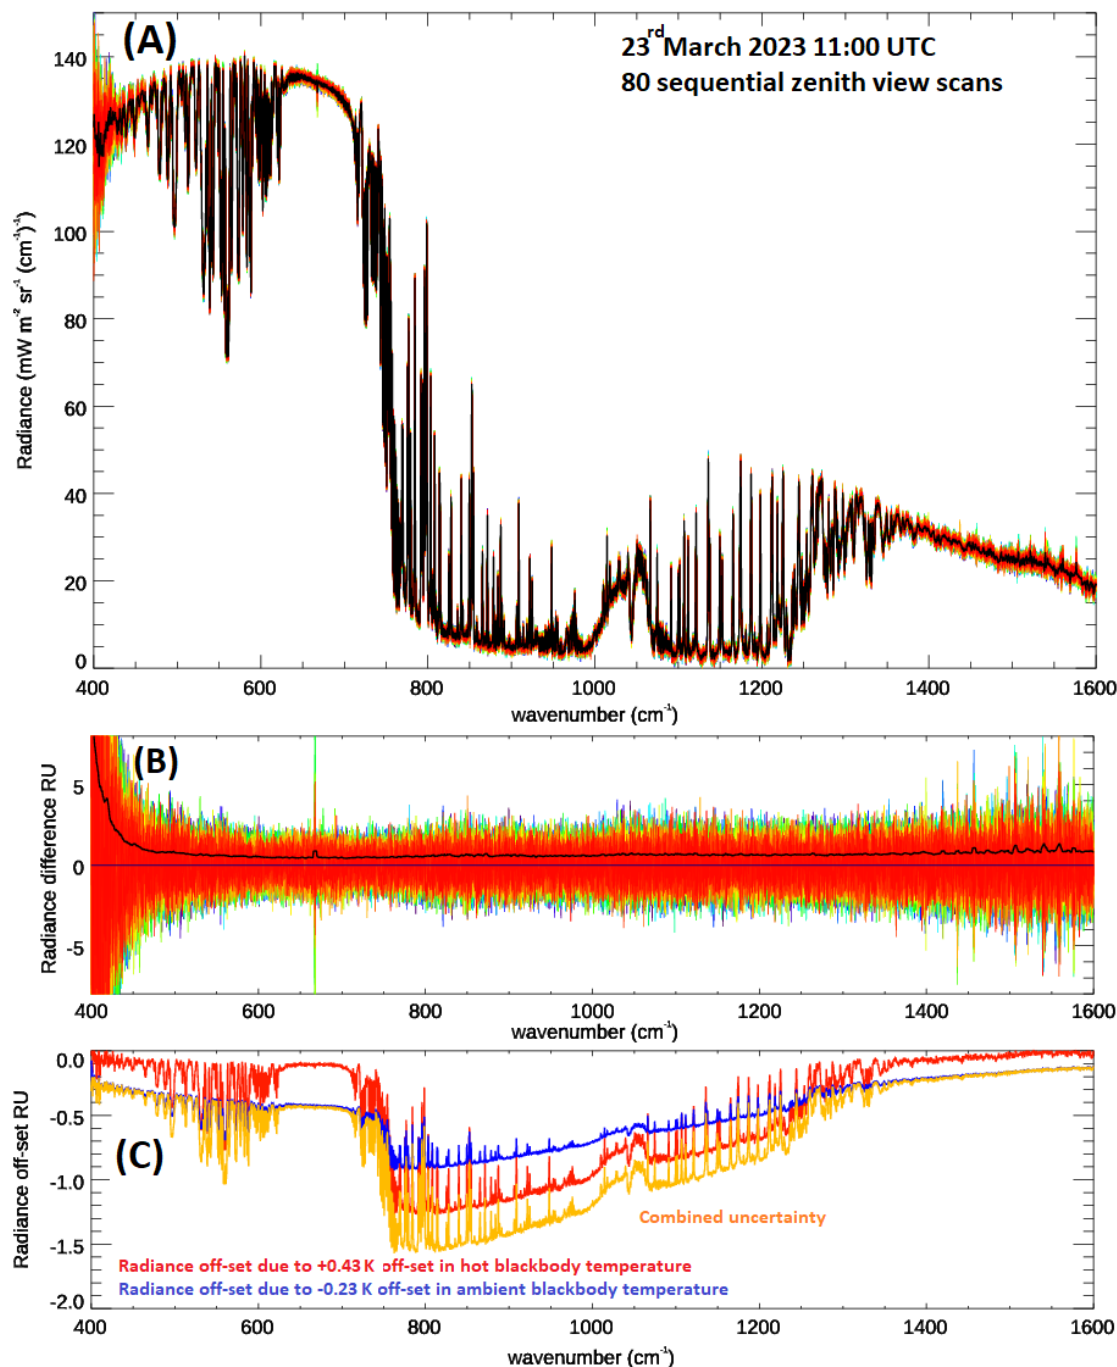

455 **Figure 10:** (A) Individual calibrated radiances obtained over a 2-minute view period colour coded from blue to red in time. Overplotted in black is the average of these scans. (B) Radiance differences between successive scans with NESR for a single scan overplotted in black. (C) Calibrated radiance offset introduced when applying a +0.43 K offset to the hot blackbody temperature (red) or a -0.23 K offset to the ambient blackbody temperature relative to their estimated emission temperatures ( $1 \text{ RU} = 1 \text{ mW m}^{-2} \text{sr}^{-1} (\text{cm}^{-1})^{-1}$ ).



## 4.1 Evaluating radiance uncertainties

### 460 4.1.1 Detector noise (NESR)

The calibrated radiances shown in Figure 10(A) are for a set of 80 sequential scans. The raw spectra were calibrated using the mean spectral response function of the calibration scans before and after the zenith view. The hot blackbody observations used in Eq. 8 were also an average of the hot blackbody measurements from before and after these zenith view measurements. Assuming negligible change between successive scans we estimate the NESR for a single scan from the set of 79 differences

465 between the 80 successive calibrated scans: these differences are shown in Fig. 10(B).

For each of these 79 difference spectra shown in Fig. 10(B), blue-to-red, we calculate the spectrally resolved NESR from the rms value derived from a rolling bin  $5 \text{ cm}^{-1}$  in width centred on sequential wavenumbers covering the full spectral range. To improve the overall signal-to-noise of these NESR estimates we take the average of the 79 NESR estimates. As the calibration scans are averages of 80 hot and ambient target measurements the dominant noise on the calibrated radiance difference will

470 be a combination of the two successive zenith measurements. Assuming the detector noise is incoherent we take the square root of the spectrally resolved NESR described above as the resultant single scan NESR, this is shown in figure 10 panel B as the overlying black line.

### 4.1.2 Correlated uncertainty

We have discussed the impact of offsets between the estimated emission temperature and the true surface emission temperature.

475 As well as the PRT100 accuracy of 0.2 K and 0.29 K for the ambient and hot targets (Section 3.4.1) there is also a temperature drift over the 1-minute observation period for each target view, seen both in our laboratory and outdoor measurements. For the ambient target we observe an upwards drift of about 0.1 K per minute, indoors while the hot target temperature is controlled to within 0.1 K over the same period, as shown in Fig. 4(B). Outdoors the drift in the ambient blackbody temperature generally follows the ambient air temperature but we have seen variations associated with changes in wind direction or gustiness. For

480 the outdoor measurements shown here the ambient blackbody temperature variation was similar to the 0.1 K per minute seen in the laboratory. Our measurements in section 3.4.2 indicate a spatial variation of 0.05 K across the blackbody target apertures. In addition, for the hot blackbody, following the discussion in section 3.4.3 we factor in an additional 0.3 K uncertainty due to along axis thermal gradients. Combining all of these uncertainties results in final uncertainties of 0.23 K and 0.43 K for the ambient and hot blackbody emission temperature, respectively.


485 Figure 10(C) shows the impact on the calibrated radiance if a recalibration is performed using blackbody emission temperature offsets of +0.43 K for the hot, and -0.23 K for the ambient blackbodies. Over wavenumber ranges sampling warmer atmospheric levels ( $400 < s < 700 \text{ cm}^{-1}$ ,  $1250 < s < 1600 \text{ cm}^{-1}$ ) the calibrated radiance is more sensitive to offsets in the ambient blackbody temperature than to offsets in the hot blackbody temperature. This lower sensitivity to offsets in the hot target is due to the self-compensation effects discussed earlier. At wavenumbers sounding a colder scene temperature ( $700 < s < 1250$



490  $\text{cm}^{-1}$ ) the effectiveness of this compensation reduces and the calibrated radiance becomes more sensitive to offsets in the hot  
blackbody than those associated with the ambient blackbody.

#### 4.2 Observation-simulation comparison

We have not yet had the opportunity to undertake a full radiative closure study using FINESSE and co-located atmospheric  
soundings so for the purpose of demonstrating performance we undertake a comparison of the observed zenith view spectra  
495 against a simulation from LBLRTM using profiles taken from ERA-5 37 level,  $0.25^\circ \times 0.25^\circ$  gridded array (Hersbach et al.,  
2020). Figure 11 shows the temperature and humidity profile from 1100 UTC on the 23<sup>rd</sup> March 2022 as recorded by ERA-5  
at the nearest grid-point to the observations. The balcony from which the observations were made is at an altitude of 30 m.  
The ambient pressure, temperature, humidity and  $\text{CO}_2$  concentrations obtained from the Vaisala sensors described in section  
2.3 were used to set conditions at the surface, with the ERA-5 pressure, temperature, humidity and ozone values superposed  
500 above. Above the surface,  $\text{CO}_2$  concentrations were set at 420 ppmv.

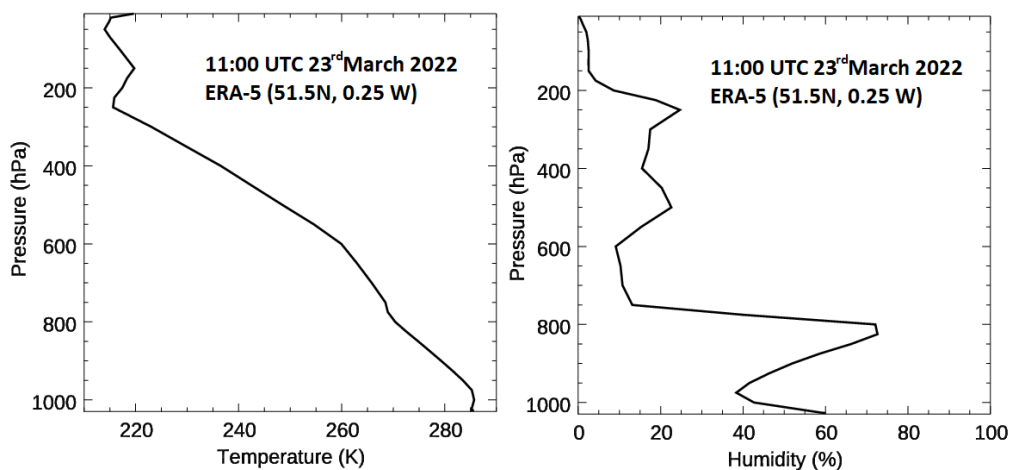


**Figure 11: ERA-5 profiles of (A) temperature and (B) relative humidity from 1100 UTC on March 23<sup>rd</sup> 2022 at for the closest grid-box to the FINESSE measurements.**

Figure 12(A) shows the 2-minute averaged observed spectrum closest to 11:00 UTC with the corresponding apodised  
505 LBLRTM simulation overplotted. Figure 12(B) shows the difference between observation and simulation with the NESR and  
calibration radiance offset envelope associated with uncertainty of the surface emission temperature overplotted for  
comparison. We expect strongly absorbing spectral regions to give good agreement with the simulation as the near surface  
temperature, humidity,  $\text{CO}_2$  and pressure is strongly influenced by the Vaisala measurements and indeed we see good  
agreement between the simulations and observations within the centre of the 15 mm  $\text{CO}_2$  band ( $620\text{-}710 \text{ cm}^{-1}$ ) and within the  
510 band wings of the 6.3 mm water-vapour vibration-rotation band ( $1350\text{-}1450 \text{ cm}^{-1}$ ). Agreement is also very good within the  
atmospheric window ( $800\text{-}1250 \text{ cm}^{-1}$ ) outside of the 9.6 mm ozone band and isolated line features. This general agreement is  
very encouraging given the fact that the ERA5 profile is representative of a much larger spatial scale than the narrow vertical



515 profile from FINESSE, with radiance differences generally falling within the range of the measured radiance uncertainty. The obvious exception occurs at wavenumbers above  $1450\text{ cm}^{-1}$  where we see an increase in observed radiance. We believe that this is likely due to uncorrected emission/absorption from the diamond phonon band, occurring within the EM27 entrance window.

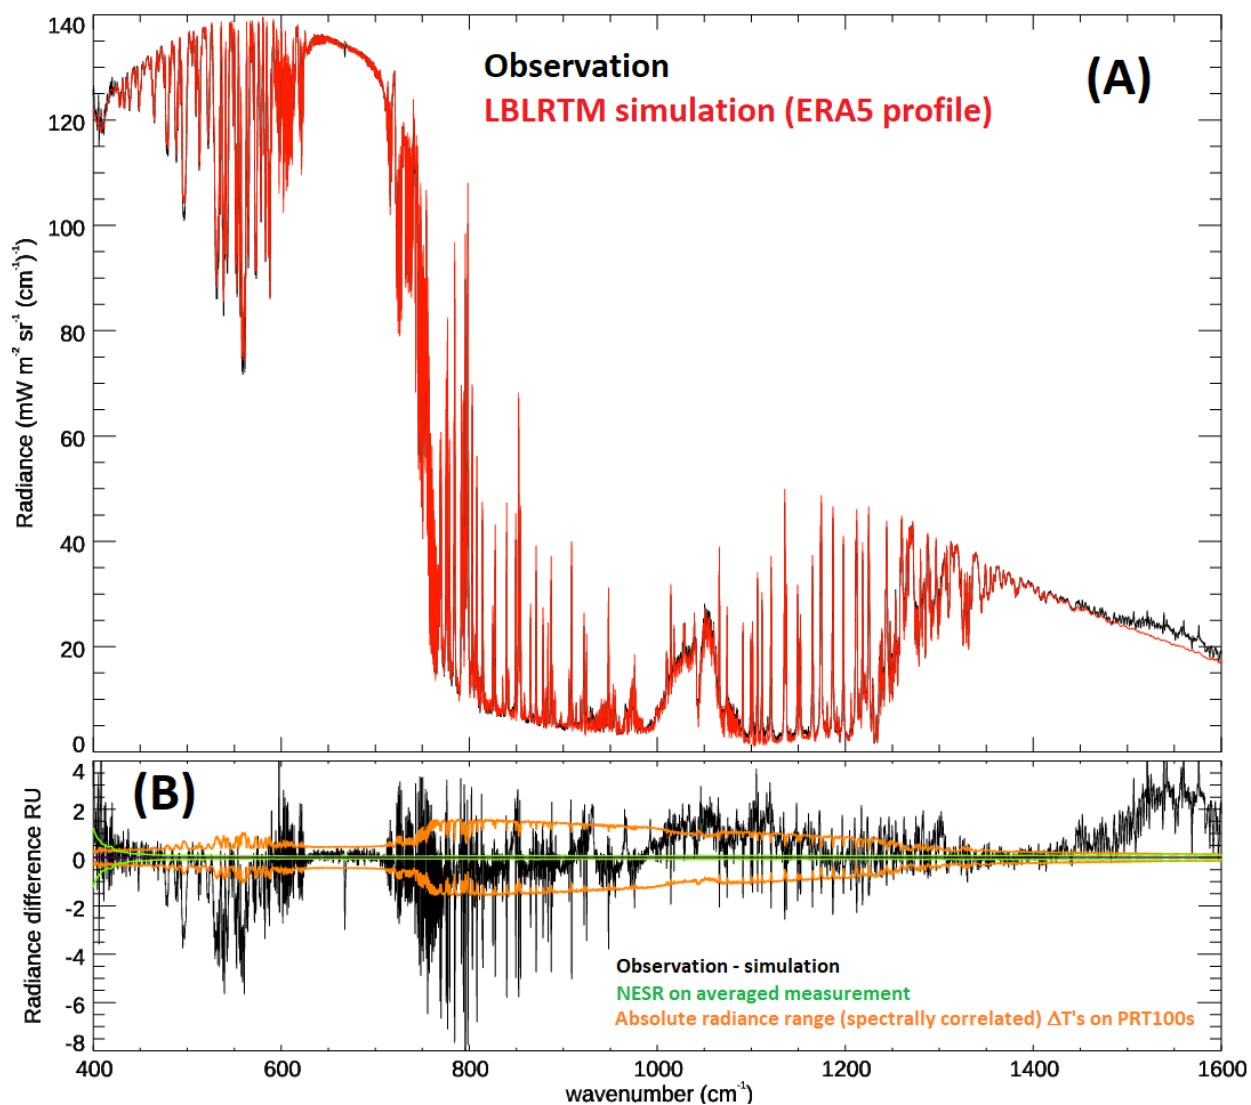

520 **Figure 12:** (A) Two-minute averaged calibrated radiance spectrum for the zenith scan cycle around 11:00 UTC with corresponding LBLRTM simulation. (B) Radiance difference between measurement and simulation. The radiance offsets associated with the uncertainty in surface emission temperature and the NESR for the 2-minute average spectrum are also shown.

To probe the comparison in more detail, Figure 13 shows the simulation and observation across expanded frequency ranges along with the radiance differences. Panels (A) and (C) suggest that the ERA5 profile is too wet with simulated radiances in far-infrared micro-windows appearing slightly too opaque relative to the measurements. Over these wavenumbers we see no



525 significant evidence of line wing dependent residuals implying that the estimated FINESSE ILS is a good fit. For the spectral  
range  $900\text{ cm}^{-1}$  –  $1000\text{ cm}^{-1}$  (panels (B) and (D)) we see some evidence at  $910\text{ cm}^{-1}$  (and  $920$  and  $948\text{ cm}^{-1}$ ) of an asymmetric  
difference around zero that is likely due to the veracity of our estimate of the ILS. Interestingly the broader spectroscopic  
features at  $930\text{ cm}^{-1}$  and  $965\text{ cm}^{-1}$  look real and are likely due to  $\text{NH}_3$  whose absorption was not included in the LBLRTM  
simulation. From  $1200\text{ cm}^{-1}$  to  $1250\text{ cm}^{-1}$  (panels (E) and (G)) we do see residuals around zero that suggest the retrieved ILS  
may not be sufficiently modelling the true line profile, this is in keeping with the residuals seen in figure 8, panels (B) and (C).  
530 Over the range  $1280\text{ cm}^{-1}$  to  $1320\text{ cm}^{-1}$ , outside of  $\text{CH}_4$  absorption centred at around  $1300\text{ cm}^{-1}$ , which is not included in our  
simulation, panels (F) and (H) the differences fall within the uncertainties.

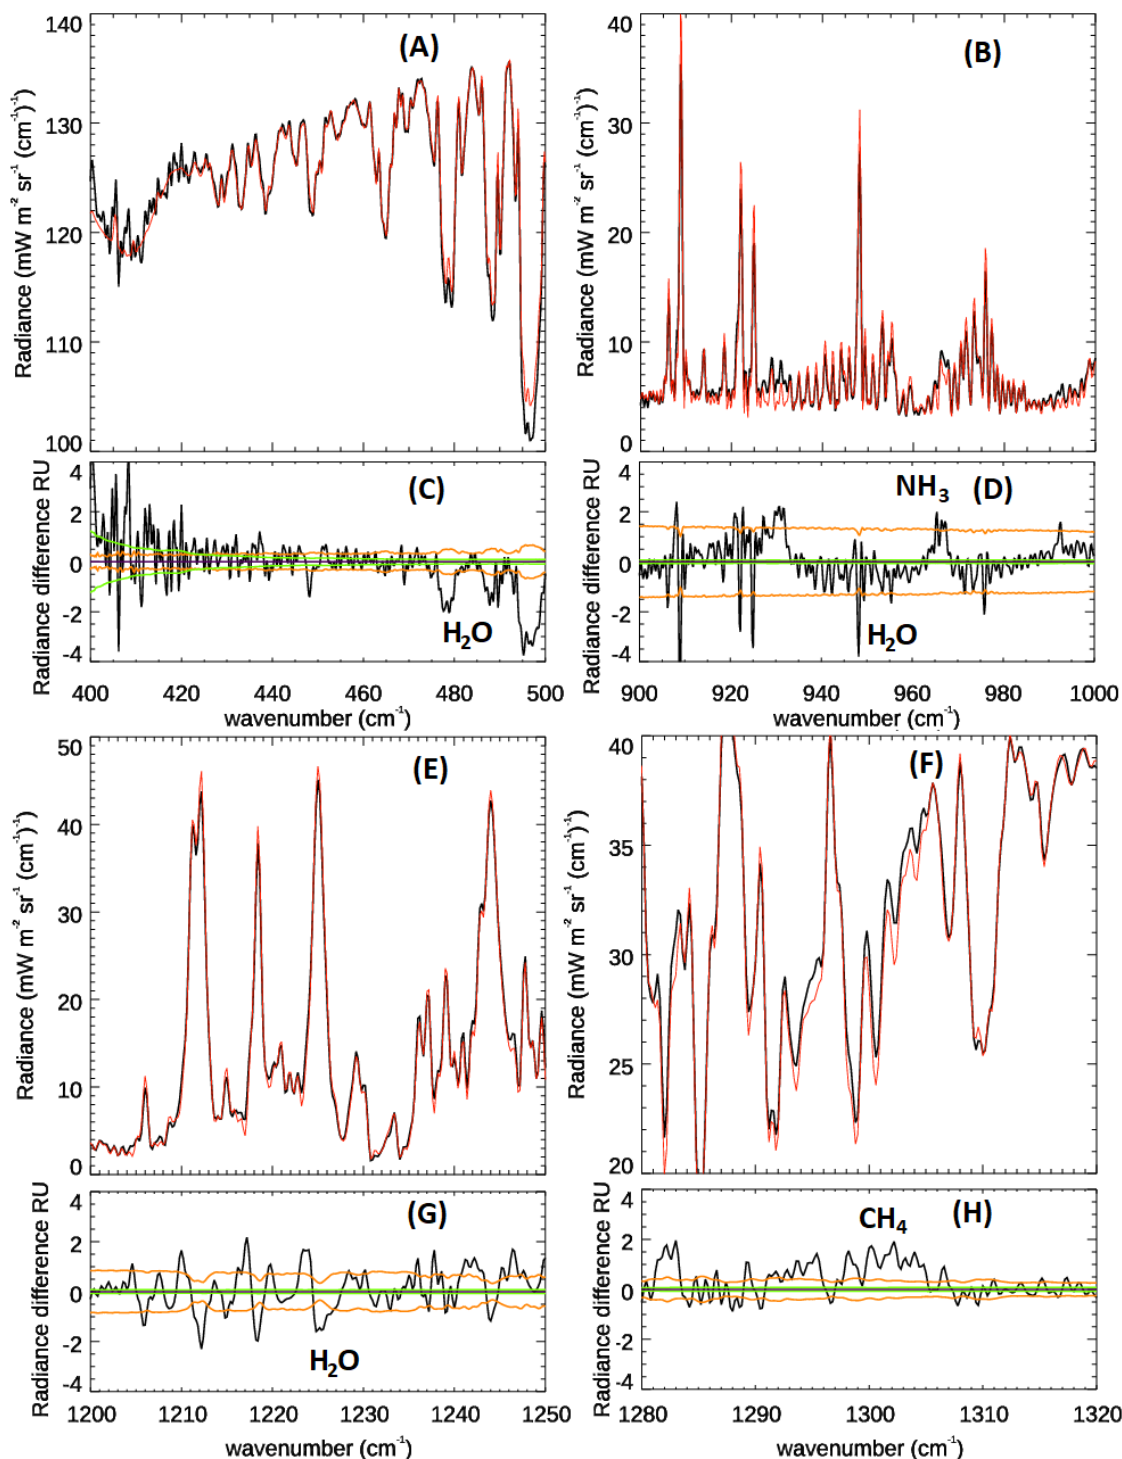


Figure 13: Expanded views of the radiance observation and simulation (Panels (A), (C), (E) and (G)) and associated differences (Panels (B), (D), (F) and (H)) shown in Fig. 12 for selected wavenumber ranges.





## 535 5 Discussion and conclusions

This paper has provided an outline of the Far INfrarEd Spectrometer for Surface Emissivity (FINESSE), which combines a commercial Bruker EM27 spectrometer with a front-end calibration and scene selection rig designed at Imperial College London in order to facilitate emissivity retrievals extending into the far-infrared. We have discussed the two-point calibration procedure and shown that the instrument spectral response is stable to within  $\pm 0.2\%$  over several hours over the majority of its spectral range (400-1600  $\text{cm}^{-1}$ ).

An important aspect of any new instrumental development is the characterisation of uncertainty. We have taken great care to provide realistic assessments of the contribution of different error sources, particularly focusing on our knowledge of the blackbody targets effective emissivity and emission temperature. Using these estimates, we have established an initial overall budget on the blackbody emission uncertainty, providing a baseline for FINESSE's calibration uncertainties. Additionally, we have used laboratory measurements to establish an initial estimate of the spectrally varying ILS which is a requirement for future emissivity and atmospheric profile retrieval efforts. In common with previous work which investigated non-ideal instrument line shapes within their EM27/Sun spectrometers (Frey et al 2015, Frey et al 2019) our estimate shows that the FINESSE ILS is highly asymmetric, and that this asymmetry is frequency dependent.

Clear-sky zenith measurements from FINESSE have been used to derive the radiance sensitivity, in the form of a single scan NESR. Comparison to radiative transfer simulations driven by temporally and spatially co-incident ERA5 profiles shows encouraging agreement given the limitations of the ERA-5 spatial scale relative to the point view of FINESSE. By removing specific gaseous species, the simulations also hint at the sensitivity that the instrument will have to specific absorbers such as  $\text{NH}_3$  and  $\text{CH}_4$ .

One feature that does need further investigation is the anomalous emission between 1450-1600  $\text{cm}^{-1}$  which we attribute to unaccounted for emission from the instrument diamond window (Shi et al 2021). Although this currently precludes the use of the FINESSE observations in this part of the spectrum it is not an issue for emissivity retrievals, which primarily use measurements from the main atmospheric window and the so-called dirty window in the far-infrared. Part II of this paper validates the operational capability of FINESSE by undertaking emissivity retrievals of de-ionised water in the spectral range 400- 1400  $\text{cm}^{-1}$ . The emissivity of deionised water has been well studied in the mid-IR and offers the opportunity for cross-comparison/validation of the FINESSE retrieved emissivities with literature values as well as extending emissivity measurements into the far-infrared.

Finally, we note that, despite its name, FINESSE is not limited to emissivity retrievals. Recently the instrument was deployed to Andoya, Norway to undertake measurements in support of the FORUM mission. The observations obtained during the campaign encompass both clear-sky and cloudy sky zenith radiances as well as down-looking views of snow and ice. These radiances have been calibrated using the approach outlined in this paper and are currently being evaluated both at Imperial, ESA and by colleagues at CNR Italy. We anticipate that these collaborative studies will help refine our knowledge of the uncertainty budget and ILS estimates described here, enhancing the utility of FINESSE for future deployments.



*Data availability.*

570 We aim to upload all applicable data sets on CERNs Zenodo data repository.

*Author contributions.*

The experimental methodology was conceptualised by JM, HB and LW. The design of the EM27 instrument interface with the external calibration system was undertaken by JM, AR and AL. The system control and data acquisition software were  
575 written by AL, AD and DC. JM and LW developed the data analysis methods. Experimental characterisation of the system was undertaken by JM, LW and PQ. HB was responsible for supervision and funding acquisition. This manuscript was written by JM and HB with input from LW.

*Competing interests.*

580 The authors declare that they have no conflict of interest.

*Acknowledgements.*

HB and JM were funded as part of NERC's support of the National Centre for Earth Observation under Grant No. NE/R016518/1. LW was funded by a Cooperative Awards in Science and Technology (CASE) partnership between EPSRC  
585 and the National Physical Laboratory, Grant No.EP/R513052/1.

We would like to thank Chris Stapleton at Bruker for his help answering numerous queries concerning the operation and capabilities of the EM27 during our acquisition of the system. The fabrication of the front-end calibration system was through the effort of Imperial College's Physics workshop personnel, particularly Paul Brown and David Williams. Additional support for the FINESSE control system software was provided by Imperial College London's Research Software Engineering team,  
590 specifically Diego Alonso Alvarez and Callum West. We make use of ERA5 re-analysis data and acknowledge the Copernicus Climate Change Service (C3S) (2017). ERA5: Fifth generation of ECMWF atmospheric reanalyses of the global climate. Copernicus Climate Change Service Climate Data Store (CDS). <https://cds.climate.copernicus.eu/cdsapp#!/home>. We employed Adibekyan's Aeroglaze Z306 emissivity data available as supplementary material under the terms of the Creative Commons Attribution 4.0 International License ([CC BY 4.0 Deed | Attribution 4.0 International | Creative Commons](#)).

595 **References**

Adams A, Nicol F, McHugh S, Moore J, Matis G and Amparan G, 2019. Vantablack properties in commercial thermal infrared imaging systems. *Infrared Imaging Syst.* 2019 XXX. 11001 (2019/05/14) 110010W.



Adibekyan, A., Kononogova, E., Monte, C. et al., 2017, High-Accuracy Emissivity Data on the Coatings Nextel 811-21,  
600 Herberts 1534, Aeroglaze Z306 and Acktar Fractal Black, *Int. J. Thermophys.*, 38, doi:10.1007/s10765-017-2212-z

Alberti, C., Hase, F., Frey, M., Dubravica, D., Blumenstock, T., Dehn, A., Castracane, P., Surawicz, G., Harig, R., Baier, B.  
C., Bès, C., Bi, J., Boesch, H., Butz, A., Cai, Z., Chen, J., Crowell, S. M., Deutscher, N. M., Ene, D., Franklin, J. E., García,  
O., Griffith, D., Grouiez, B., Grutter, M., Hamdouni, A., Houweling, S., Humpage, N., Jacobs, N., Jeong, S., Joly, L., Jones,  
605 N. B., Jouglet, D., Kivi, R., Kleinschek, R., Lopez, M., Medeiros, D. J., Morino, I., Mostafavipak, N., Müller, A., Ohyama,  
H., Palmer, P. I., Pathakoti, M., Pollard, D. F., Raffalski, U., Ramonet, M., Ramsay, R., Sha, M. K., Shiomi, K., Simpson, W.,  
Stremme, W., Sun, Y., Tanimoto, H., Té, Y., Tsidu, G. M., Velazco, V. A., Vogel, F., Watanabe, M., Wei, C., Wunch, D.,  
Yamasoe, M., Zhang, L., and Orphal, J. (2022): Improved calibration procedures for the EM27/SUN spectrometers of the  
COLlaborative Carbon Column Observing Network (COCCON), *Atmos. Meas. Tech.*, 15, 2433–2463,  
610 <https://doi.org/10.5194/amt-15-2433-2022>

Bellisario, C., H. Brindley, J. Murray, A. Last, J. Pickering, C. Harlow, S. Fox, C. Fox, S. Newman, M. Smith, D. Anderson,  
X. Huang and X. Chen, 2017. Retrievals of the Far Infrared surface emissivity over the Greenland Plateau using the  
Tropospheric Airborne Fourier Transform Spectrometer (TAFTS)., *J. Geophys. Res.*, 122, doi: 10.1002/2017JD027328  
615

Ben-Yami, M., H. Oetjen, H. Brindley et al., 2022. Emissivity retrievals with FORUM's end-to-end simulator: challenges and  
recommendations, *Atmospheric Measurement Techniques*, 15, 1755-1777, doi: 10.5194/amt-15-1755-2022

Bennett, A.M, Wickham, B.J, Dhillon, H.K Chen, Y, Webster, S, Turri, G. Bass, M. Development of high-purity optical grade  
620 single-crystal CVD diamond for intracavity cooling. In *Solid State Lasers XXIII: Technology and Devices*; Clarkson, W.A.,  
Shori, R.K., Eds.; SPIE: Bellingham, WA, USA, 2014. doi:10.1117/12.2037811.

Bianchini, G., F. Castagnoli, G. Di Natale et al., 2019. A Fourier transform spectroradiometer for ground-based remote sensing  
of the atmospheric downwelling long-wave radiance. *Atmos. Meas. Tech.*, 12, 619-635, doi: 10.5194/amt-12-619-2019  
625

Blanchet, J-P, A. Royer, F. Châteauneuf et al., 2011. TICFIRE: a far infrared payload to monitor the evolution of thin ice  
clouds, *SPIE Proceedings*, 8176, doi: 10.1117/12.898577

Borbas, E., D. Adler, F. Best et al., 2021, Ground-based far-infrared emissivity measurements with the University of Wisconsin  
630 absolute radiance interferometer (ARI). *SPIE Proceedings*, 11830, *Infrared remote sensing and instrumentation*,  
doi:10.1117/12.2594834



- 635 Canas, T., J. Murray and J. Harries, 1997. Tropospheric Airborne Fourier Transform Spectrometer (TAFTS). Proc. SPIE 3220, Satellite Remote Sensing of Clouds and the Atmosphere II, doi:10.1117/12.301139
- Clough, S., Shephard, M., Mlawer, E., Delamere, J., Iacono, M., and K. Cady-Pereira, 2005. Atmospheric radiative transfer modelling: A summary of the AER codes. *J. Quant. Spectrosc. Radiat. Trans.*, **91**, 233-244. doi:10.1016/j.jqsrt.2004.05.058
- Feldman, D., W. Collins, R. Pincus, X. Huang and X. Chen, 2014. Far-infrared surface emissivity and climate. Proc. Natl. Acad. Sci. USA, 111, 16 297–16 302, doi:10.1073/pnas.1413640111
- 640 Frey, M., Hase, F., Blumenstock, T., Groß, J., Kiel, M., Mengistu Tsidu, G., Schäfer, K., Sha, M. K., and Orphal, J. (2015): Calibration and instrumental line shape characterization of a set of portable FTIR spectrometers for detecting greenhouse gas emissions, *Atmos. Meas. Tech.*, 8, 3047–3057, <https://doi.org/10.5194/amt-8-3047-2015>
- 645 Frey, M., Sha, M. K., Hase, F., Kiel, M., Blumenstock, T., Harig, R., Surawicz, G., Deutscher, N. M., Shiomi, K., Franklin, J. E., Bösch, H., Chen, J., Grutter, M., Ohyama, H., Sun, Y., Butz, A., Mengistu Tsidu, G., Ene, D., Wunch, D., Cao, Z., Garcia, O., Ramonet, M., Vogel, F., and Orphal, J.: Building the COllaborative Carbon Column Observing Network (COCCON): long-term stability and ensemble performance of the EM27/SUN Fourier transform spectrometer, *Atmos. Meas. Tech.*, 12, 1513–1530, <https://doi.org/10.5194/amt-12-1513-2019>, 2019
- 650 Genest, J. and P. Tremblay, 1999. Instrument line shape of Fourier transform spectrometers: analytic solutions for nonuniformly illuminated off-axis detectors, *Appl. Opt.*, 38, 5438-5446, doi:10.1364/AO.38.005438
- Griffiths, P R and De Hasseth J A, 2008. *Fourier Transform Infrared Spectrometry 2<sup>nd</sup> addition*. John Wiley and Sons, ISBN 978-0-471-19404-0.
- 655 Hersbach, H., Bell, B., Berrisford, P., Hirahara, S., Horányi, A., Muñoz-Sabater, J., Nicolas, J., Peubey, C., Radu, R., Schepers, D., Simmons, A., Soci, C., Abdalla, S., Abellan, X., Balsamo, G., Bechtold, P., Biavati, G., Bidlot, J., Bonavita, M., De Chiara, G., Dahlgren, P., Dee, D., Diamantakis, M., Dragani, R., Flemming, J., Forbes, R., Fuentes, M., Geer, A., Haimberger, L., Healy, S., Hogan, R. J., Hólm, E., Janisková, M., Keeley, S., Laloyaux, P., Lopez, P., Lupu, C., Radnoti, G., de Rosnay, P.,
- 660 Rozum, I., Vamborg, F., Villaume, S., and Thépaut, J.-N.: The ERA5 global reanalysis, *Q. J. Roy. Meteor. Soc.*, 146, 1999–2049, <https://doi.org/10.1002/qj.3803>, 2020.
- Huang, X., X. Chen, M. Flanner, P. Yang, D. Feldman and C. Kuo, 2018. Improved representation of surface spectral emissivity in a global climate model and its impact on simulated climate, *J. Climate*, 31, 3711-3727, doi:10.1175/JCLI-D-17-0125.
- 665



- Langsdale, M., T. Dowling, M. Wooster et al., 2020. Inter-Comparison of Field- and Laboratory-Derived Surface Emissivities of Natural and Manmade Materials in Support of Land Surface Temperature (LST), *Remote Sensing*, 12, doi: 10.3390/rs12244127
- 670
- L'Ecuyer, T. and the entire PREFIRE science team, 2021. The Polar Radiant Energy in the Far InfraRed Experiment: A New Perspective on Polar Longwave Energy Exchanges, *Bull. Amer. Met. Soc.*, 102, doi:10.1175/BAMS-D-20-0155.1, 2021
- Mertz L, Transformation in Optics (John Wiley and Son, New York, 1965)
- 675
- Murray J., H. Brindley, S. Fox, C. Bellisario, J. Pickering, C. Fox, C. Harlow, M. Smith, D. Anderson, X. Huang, X. Chen, A. Last and R. Bantges, 2020, Retrievals of high latitude surface emissivity across the infrared from high altitude aircraft flights, *J. Geophys. Res.*, 125, doi: 10.1029/2020jd033672
- 680
- Palchetti, L., H. Brindley, R. Bantges, S. Buehler, C. Camy-Peyret, B. Carli, U. Cortesi, S. Del Bianco, G. Di Natale, B. Dinelli, D. Feldman, X. Huang, L. Labonnote, Q. Libois, T. Maestri, M. Mlynczak, J. Murray, H. Oetjen, M. Ridolfi, M. Riese, J. Russell, R. Saunders and C. Serio, 2020. FORUM: unique far-infrared satellite observations to better understand how Earth radiates energy to space. *Bull. Amer. Meteor. Soc.*, 101, doi: 10.1175/BAMS-D-19-0322.1
- 685
- Palchetti, L., M. Barucci, C. Belotti et al., 2021. Observations of the downwelling far-infrared atmospheric emission at the Zugspitze observatory, *Earth Sys. Sci. Data*, 13, 4303-4312, doi: 10.5194/essd-13-4303-2021
- Revercomb, H. E., Buijs, H., Howell, H. B., LaPorte, D. D., Smith, W. L., and Sromovsky, L. A.: Radiometric calibration of IR Fourier transform spectrometers: solution to a problem with the High-Resolution Interferometer Sounder, *Appl. Optics*, 27, 3210–3218, <https://doi.org/10.1364/AO.27.003210>, 1988.
- 690
- Shi, Z.; Yuan, Q.; Wang, Y.; Nishimura, K.; Yang, G.; Zhang, B.; Jiang, N.; Li, H. Optical Properties of Bulk Single-Crystal Diamonds at 80–1200 K by Vibrational Spectroscopic Methods. *Materials* 2021, 14, 7435. <https://doi.org/10.3390/ma14237435>
- 695
- Wan Q, B. Brede, M. Smigaj and L. Kooistra, 2021. Factors influencing temperature measurements from miniaturised thermal infrared (TIR) cameras: A laboratory-based approach, *Sensors* 2021, 21(24), 8466; <https://doi.org/10.3390/s21248466>



700 Wilson, S. H. S., Atkinson, N. C., & Smith, J. A. (1999). The development of an airborne infrared interferometer for  
meteorological sounding studies. *Journal of Atmospheric and Oceanic Technology*, **16**(12), 1912–  
1927. [https://doi.org/10.1175/1520-0426\(1999\)016%3C1912:TDOAAI%3E2.0.CO;2](https://doi.org/10.1175/1520-0426(1999)016%3C1912:TDOAAI%3E2.0.CO;2)

705 Xie, Y., X. Huang, X. Chen, T. L'Ecuyer, B. Drouin and J. Wang, 2022. Retrieval of Surface Spectral Emissivity in Polar  
Regions based on the Optimal Estimation Method, *J. Geophys. Res.*, 127, doi: 10.1029/2021JD035677