

Supplement of

Spatial analysis of PM_{2.5} using a Concentration Similarity Index applied to air quality sensor networks

Byrne et al.

Table of Contents

Table S1	Page S3
Table S2	Page S4
Table S3	Page S5
Table S4	Page S6
Table S5	Page S7
Table S6	Page S8
Table S7	Page S9
Figure S1	Page S10
Figure S2	Page S11
Figure S3	Page S12
Figure S4	Page S13
Figure S5	Page S14
Figure S6	Page S15
Figure S7	Page S16

Table S1: Co-location periods for Clarity Node-S devices used in the Dungarvan sensor network. Grey cells indicate a device was not present for the co-location, blue cells indicate a device was present for part of the co-location period, and green cells indicate a device was present for the entire co-location period.

Co-location deployment period	Devices present for co-location																
	A3	A4	A8H	A8Z	A9	AQ	AZ	A7	A6P	AJ3	AP7	AQV	ARF	AW6	AWF	AY9N	AY93
19/01/2022 – 28/01/2022	Grey	Green	Green	Green	Green	Green	Green	Grey									
29/10/2022 – 22/11/2022	Grey	Grey	Green	Grey	Green	Grey	Grey	Green									
16/06/2023 – 17/07/2023	Green	Green	Green	Green	Green	Green	Green	Green	Blue	Blue	Green	Green	Blue	Green	Blue	Blue	Blue

Table S2: Linear regression results for co-located Clarity Node-S devices when compared to the mean values of all co-located data, before and after data harmonisation procedures were carried out.

Device ID	Pre-harmonisation			Post-harmonisation		
	Slope	Intercept	R ²	Slope	Intercept	R ²
	$\mu\text{g m}^{-3}$			$\mu\text{g m}^{-3}$		
A3	1.036	0.933	0.992	1	0	0.992
A4	1.012	-0.278	0.996	1	0	0.996
A8H	0.905	0.979	0.995	1	0	0.995
A8Z	1.003	-0.302	0.997	1	0	0.997
A9	1.06	-0.535	0.979	1	0	0.979
AQ	0.989	0.859	0.997	1	0	0.997
AZ	0.979	0.079	0.997	1	0	0.997
A7	0.947	0.047	0.992	1	0	0.992
A6P	1.027	0.632	0.995	1	0	0.995
AJ3	0.989	-0.415	0.993	1	0	0.993
AP7	0.964	-0.477	0.992	1	0	0.992
AQV	1.042	0.797	0.997	1	0	0.997
ARF	1.016	-0.276	0.996	1	0	0.996
AW6	0.958	0.291	0.984	1	0	0.984
AWF	0.965	-0.554	0.989	1	0	0.989
AY9N	1.065	-0.364	0.988	1	0	0.988
AY93	0.955	0.298	0.995	1	0	0.995
AYG	0.976	-0.168	0.994	1	0	0.994

Table S3: Concentration Similarity Indices for hourly averaged PM_{2.5} measured by a range of co-located PurpleAir devices.
 $\text{PM}_{\text{lim}} = 15 \mu\text{g m}^{-3}$, $C_{\text{lim, upper}} = 0.2$, $C_{\text{lim, lower}} = 0.7$.

	UNIT 2	UNIT 3	UNIT 4	UNIT 5
UNIT 2	1	0.98	0.99	1.0
UNIT 3		1	0.99	0.99
UNIT 4			1	0.99
UNIT 5				1

Table S4: Concentration Similarity Indices for the hourly averaged PM_{2.5} measured by Clarity Node-S devices in the Dungarvan AQS network for January 2023.

	A3	A4	A8H	A8Z	A9	AQ	AZ	A7	A6P	AJ3	AP7	AQV	ARF	AW6	AWF	AY9N	AY93	AYG
A3	1	0.48	0.6	0.46	0.5	0.63	0.45	0.51	0.5	0.46	0.26	0.46	0.4	0.58	0.42	0.41	0.38	0.46
A4		1	0.47	0.46	0.55	0.48	0.52	0.51	0.43	0.54	0.38	0.51	0.45	0.51	0.51	0.5	0.45	0.49
A8H			1	0.49	0.53	0.54	0.46	0.56	0.49	0.53	0.37	0.55	0.44	0.59	0.47	0.57	0.41	0.5
A8Z				1	0.58	0.42	0.62	0.46	0.49	0.57	0.57	0.57	0.52	0.52	0.55	0.61	0.49	0.6
A9					1	0.48	0.57	0.53	0.46	0.54	0.47	0.56	0.45	0.54	0.5	0.51	0.44	0.56
AQ						1	0.43	0.5	0.47	0.45	0.26	0.45	0.39	0.56	0.37	0.45	0.35	0.42
AZ							1	0.52	0.52	0.61	0.52	0.61	0.51	0.53	0.56	0.53	0.44	0.67
A7								1	0.46	0.51	0.34	0.53	0.41	0.56	0.47	0.46	0.37	0.48
A6P									1	0.61	0.42	0.5	0.49	0.57	0.55	0.51	0.49	0.61
AJ3										1	0.49	0.67	0.54	0.59	0.72	0.53	0.63	0.71
AP7											1	0.45	0.5	0.37	0.49	0.51	0.44	0.54
AQV												1	0.5	0.58	0.63	0.55	0.52	0.66
ARF													1	0.52	0.54	0.59	0.46	0.58
AW6														1	0.54	0.59	0.49	0.58
AWF															1	0.49	0.64	0.73
AY9N																1	0.5	0.54
AY93																	1	0.63
AYG																		1

Table S5: Concentration Similarity Indices for the hourly averaged PM_{2.5} measured by Clarity Node-S devices in the Dungarvan AQS network for May 2023.

	A3	A4	A8H	A8Z	A9	AQ	AZ	A7	A6P	AJ3	AP7	AQV	ARF	AW6	AWF	AY9N	AY93	AYG
A3	1	0.85	0.9	0.83	0.84	0.89	0.87	0.88	0.9	0.88	0.8	0.9	0.81	0.88	0.82	0.81	0.86	0.86
A4		1	0.84	0.82	0.87	0.8	0.82	0.89	0.82	0.87	0.81	0.85	0.75	0.81	0.81	0.79	0.79	0.81
A8H			1	0.83	0.84	0.86	0.83	0.87	0.88	0.86	0.79	0.86	0.75	0.82	0.79	0.8	0.85	0.83
A8Z				1	0.87	0.84	0.91	0.85	0.85	0.87	0.89	0.88	0.78	0.76	0.82	0.82	0.82	0.9
A9					1	0.79	0.86	0.89	0.84	0.91	0.85	0.88	0.78	0.81	0.89	0.85	0.78	0.84
AQ						1	0.82	0.83	0.84	0.83	0.76	0.87	0.74	0.8	0.73	0.77	0.83	0.84
AZ							1	0.82	0.88	0.9	0.83	0.93	0.84	0.84	0.86	0.8	0.81	0.94
A7								1	0.86	0.88	0.83	0.86	0.77	0.86	0.82	0.8	0.82	0.82
A6P									1	0.92	0.84	0.93	0.84	0.9	0.9	0.87	0.86	0.93
AJ3										1	0.86	0.93	0.85	0.89	0.94	0.91	0.84	0.94
AP7											1	0.82	0.81	0.72	0.87	0.79	0.8	0.82
AQV												1	0.84	0.89	0.9	0.86	0.84	0.94
ARF													1	0.77	0.84	0.72	0.76	0.87
AW6														1	0.83	0.76	0.81	0.84
AWF															1	0.91	0.76	0.92
AY9N																1	0.77	0.88
AY93																	1	0.83
AYG																		1

Table S6: Concentration Similarity Indices for hourly averaged PM_{2.5} measured by PurpleAir devices in the Cork City AQS network for January 2021.

	CCC1	CCC2	CCC3	CCC4	CCC5	CCC7	CCC8	CCC9	CCC11	CCC12	MTU	UCC
CCC1	1	0.55	0.63	0.52	0.72	0.61	0.6	0.42	0.7	0.54	0.55	0.59
CCC2		1	0.54	0.58	0.63	0.48	0.59	0.56	0.69	0.6	0.4	0.59
CCC3			1	0.48	0.58	0.67	0.65	0.35	0.67	0.49	0.63	0.56
CCC4				1	0.59	0.45	0.51	0.54	0.6	0.58	0.42	0.5
CCC5					1	0.54	0.62	0.65	0.7	0.6	0.4	0.66
CCC7						1	0.54	0.33	0.59	0.42	0.6	0.46
CCC8							1	0.65	0.66	0.57	0.4	0.75
CCC9								1	0.5	0.57	0.18	0.7
CCC11									1	0.59	0.46	0.65
CCC12										1	0.33	0.55
MTU											1	0.31
UCC												1

Table S7: Concentration Similarity Indices for hourly averaged PM_{2.5} measured by PurpleAir devices in the Cork City AQS network for May 2021.

	CCC1	CCC2	CCC3	CCC4	CCC5	CCC7	CCC8	CCC9	CCC11	CCC12	MTU	UCC
CCC1	1	0.58	0.7	0.51	0.63	0.63	0.58	0.45	0.5	0.39	0.74	0.58
CCC2		1	0.91	0.94	0.93	0.92	0.94	0.89	0.95	0.91	0.81	0.95
CCC3			1	0.85	0.93	0.95	0.92	0.84	0.88	0.79	0.9	0.92
CCC4				1	0.91	0.86	0.9	0.94	0.93	0.91	0.74	0.92
CCC5					1	0.92	0.9	0.83	0.94	0.83	0.86	0.96
CCC7						1	0.93	0.86	0.9	0.8	0.86	0.91
CCC8							1	0.89	0.92	0.84	0.79	0.9
CCC9								1	0.92	0.91	0.63	0.91
CCC11									1	0.91	0.75	0.96
CCC12										1	0.6	0.87
MTU											1	0.79
UCC												1



Figure S1: Map of Dungarvan with Clarity Node-S sensor locations and labels. (Map obtained from Esri, DigitalGlobe, GeoEye, i-cubed, USDA FSA, USGS, AEX, Getmapping, Aerogrid, IGN, IGP, swisstopo, and the GIS User Community)

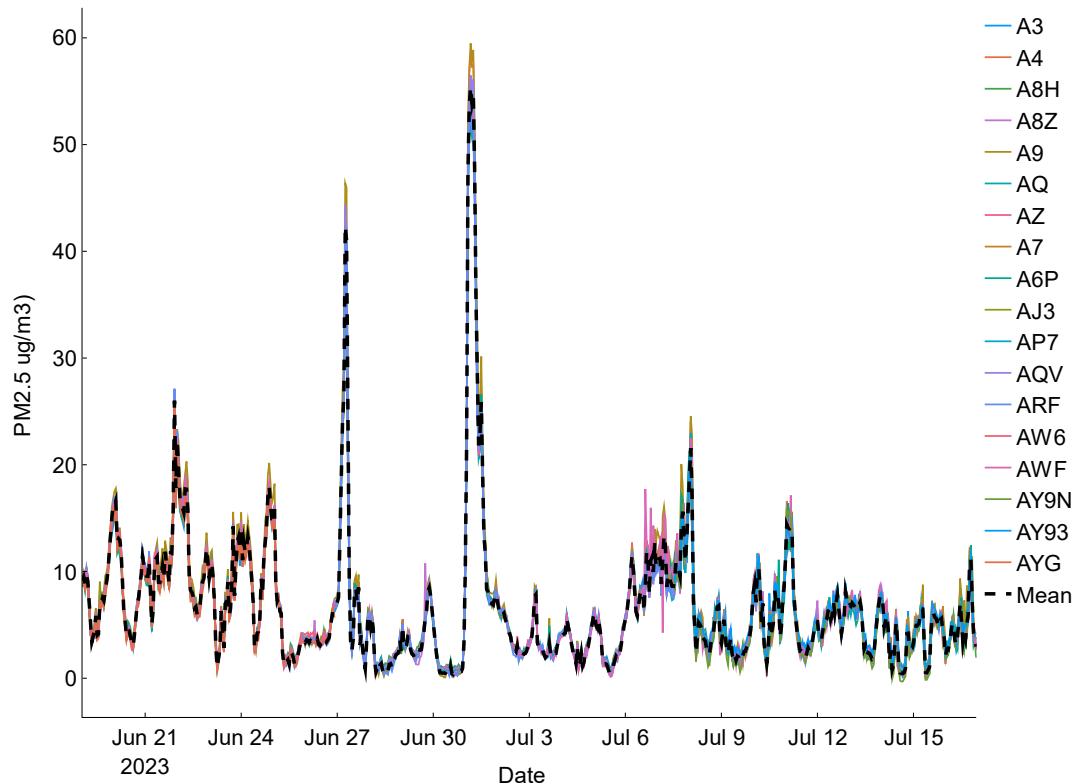


Figure S2: Hourly averaged PM_{2.5} from co-located and harmonised Clarity Node-S devices including the mean PM_{2.5} data series used for the harmonisation (19 June 2023–18 July 2023).

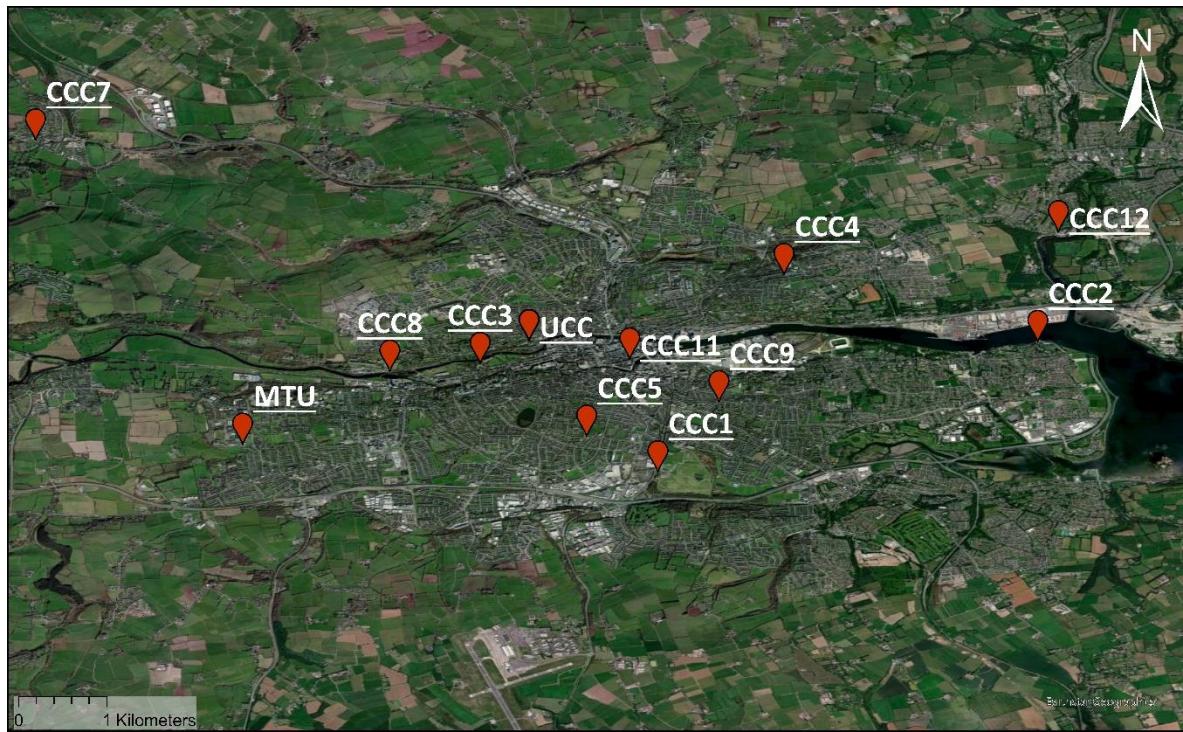


Figure S3: Map of Cork city with PurpleAir PA-II-SD sensor locations and labels. (Map obtained from Esri, DigitalGlobe, GeoEye, i-cubed, USDA FSA, USGS, AEX, Getmapping, Aerogrid, IGN, IGP, swisstopo, and the GIS User Community)

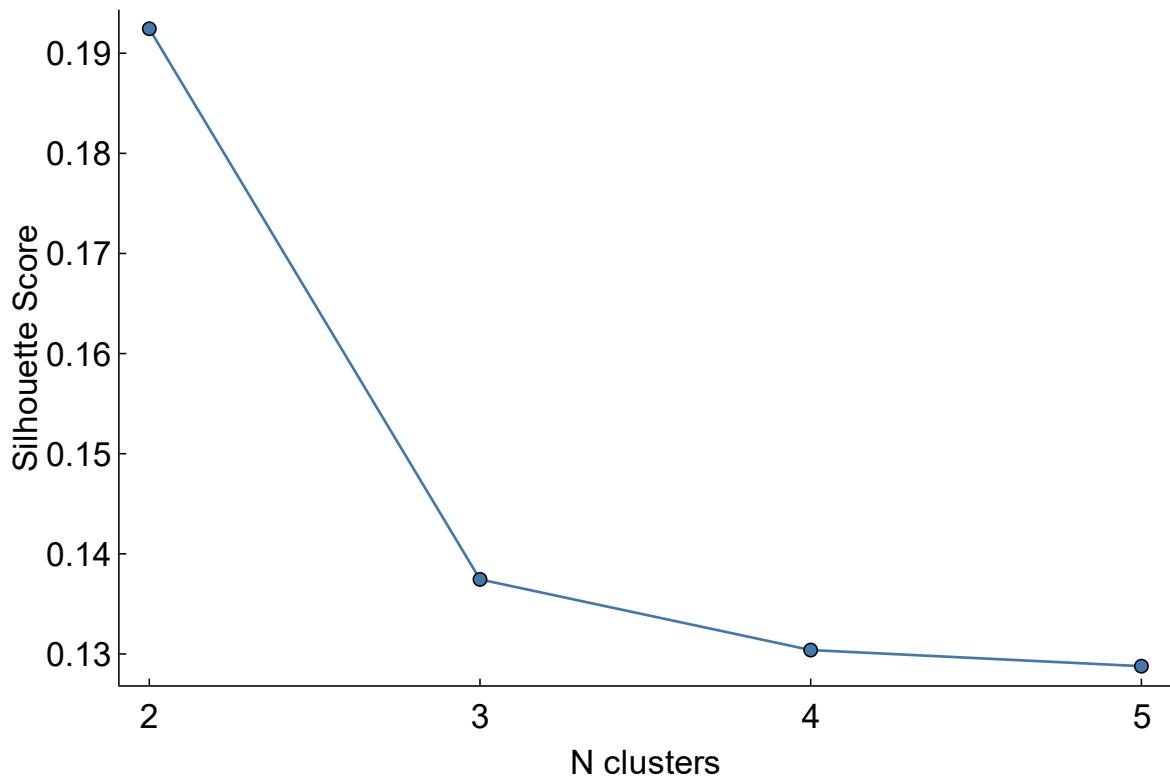


Figure S4: Silhouette scores for Hierarchical clustering on the Dungarvan sensor network CSI results.

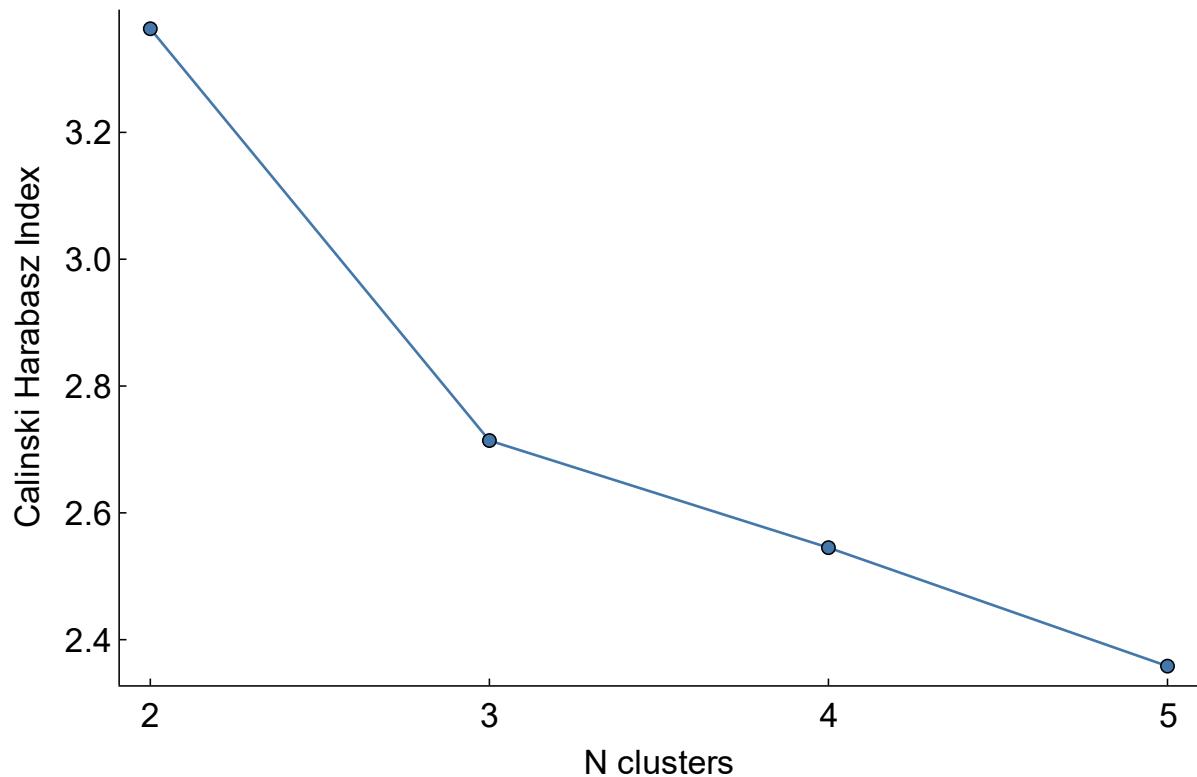


Figure S5: Calinski-Harabasz Indices for FCM clustering on the Dungarvan sensor network CSI results.

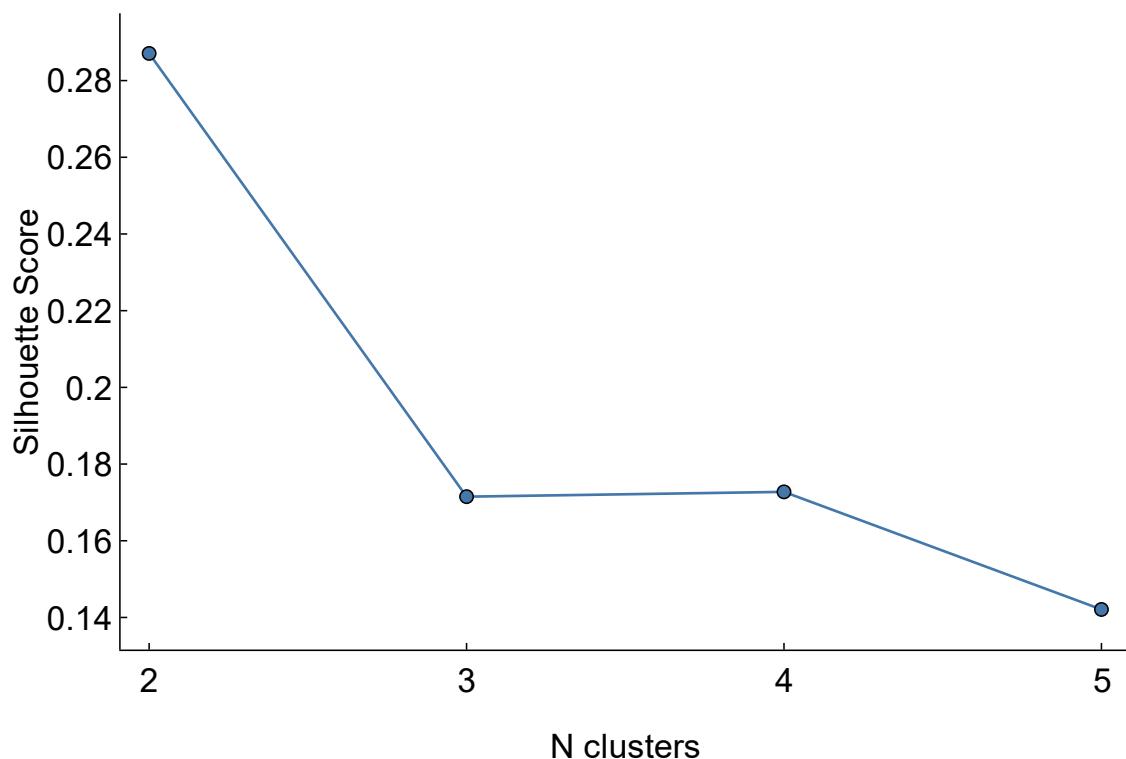


Figure S6: Silhouette scores for Hierarchical clustering on the Cork sensor network CSI results.

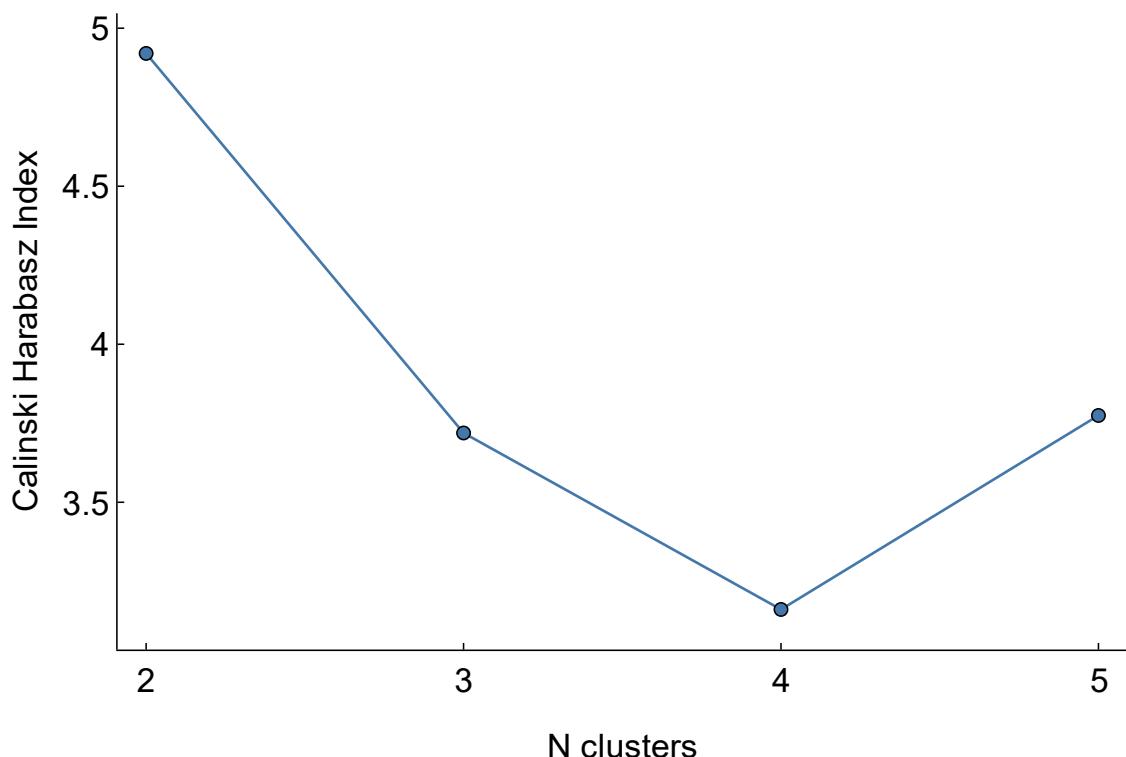


Figure S7: Calinski-Harabasz Indices for FCM clustering on the Cork sensor network CSI results.